

This is the author's final, peer-reviewed manuscript as accepted for publication. The publisher-formatted version may be available through the publisher's web site or your institution's library.

## Standardization of a method to detect bovine sperm-bound anti-sperm antibodies by flow cytometry

M. C. Sardoy, D. E. Anderson, A. George, M. J. Wilkerson, S. Skinner, M. S. Ferrer

### How to cite this manuscript

If you make reference to this version of the manuscript, use the following information:

Sardoy, M. C., Anderson, D. E., George, A., Wilkerson, M. J., Skinner, S., & Ferrer, M. S. (2012). Standardization of a method to detect bovine sperm-bound anti-sperm antibodies by flow cytometry. Retrieved from <http://krex.ksu.edu>

### Published Version Information

**Citation:** Sardoy, M. C., Anderson, D. E., George, A., Wilkerson, M. J., Skinner, S., & Ferrer, M. S. (2012). Standardization of a method to detect bovine sperm-bound anti-sperm antibodies by flow cytometry. *Theriogenology*, 78(7), 1570-1577.

**Copyright:** © 2012 Elsevier Inc.

**Digital Object Identifier (DOI):** doi:10.1016/j.theriogenology.2012.06.026

### Publisher's Link:

<http://www.sciencedirect.com/science/article/pii/S0093691X12003962>

This item was retrieved from the K-State Research Exchange (K-REx), the institutional repository of Kansas State University. K-REx is available at <http://krex.ksu.edu>

1 Standardization of a method to detect bovine sperm-bound anti-sperm antibodies by flow  
2 cytometry

3  
4 Sardoy MC<sup>a1</sup>, Anderson DE<sup>a</sup>, George A<sup>b</sup>, Wilkerson ME<sup>b</sup>, Skinner S<sup>c</sup>, Ferrer MS<sup>a\*</sup>

5  
6 <sup>a</sup>Department of Clinical Sciences, College of Veterinary Medicine, Kansas State University,  
7 Manhattan, KS 66506, <sup>b</sup>Department of Diagnostic Medicine and Pathobiology, College of  
8 Veterinary Medicine, Kansas State University, Manhattan, KS 66506, <sup>c</sup>Developing Scholars  
9 Program, Kansas State University, Manhattan, KS 66506.

10  
11 \* Corresponding author: Department of Clinical Sciences, College of Veterinary Medicine,  
12 Kansas State University, Manhattan, KS 66506, USA. Tel.: +1-785-532-5700. Fax: +1-785-532-  
13 4989. Email address: [mferrer@vet.k-state.edu](mailto:mferrer@vet.k-state.edu)

14 <sup>1</sup>Present address at: Milton Equine Hospital, Campbellsville, Ontario, Canada

15  
16 Abstract

17  
18 The objectives of this study were to standardize some methodological and analytical  
19 aspects of a direct technique to detect sperm-bound anti-sperm antibodies (ASAs) in bovine  
20 semen using flow cytometry. Four ASA-positive bulls with experimentally induced ASAs and 10  
21 reproductively normal ASA-negative bulls were included in the study. The effect of pre-fixation  
22 of sperm membranes with formalin buffer solution and inclusion of dead cells in the analysis was  
23 evaluated. Fixation of sperm membranes had no significant effect on the percentage of IgG- or

24 IgA-bound spermatozoa detected by flow cytometry. Including dead cells in the analysis  
25 increased the percentage of IgG-bound spermatozoa in fixed (live and dead  $18.6 \pm 9.7$  % and live  
26  $1.3 \pm 0.5$  %) and non-fixed samples (live and dead  $18.8 \pm 9.2$  %, live  $1.5 \pm 0.6$  %) ( $P = 0.0029$ ),  
27 as well as IgA-bound spermatozoa in fixed (live and dead  $16.3 \pm 6.4$  %, live  $0.3 \pm 0.5$  %) and  
28 non-fixed samples (live and dead  $21.4 \pm 4.6$  %, live  $1.0 \pm 0.5$  %) ( $P = 0.0041$ ) (median  $\pm$  SE) in  
29 semen from ASA-negative bulls. Intra-sample, intra-assay and inter-assay coefficients of  
30 variation (CV) for determination of sperm-bound IgG were 0.8 %, 4.6 % and 5.3 %, respectively.  
31 For determination of sperm-bound IgA, intra-sample, intra-assay and inter-assay CV were 2.8 %,  
32 8.4 % and 40.3 %, respectively. In spite of the high inter-assay CV for IgA determination, all  
33 ASA-positive bulls had high percentages of IgA-bound spermatozoa at all times. Flow cytometry  
34 correctly identified ASA-positive bulls. Confocal laser microscopy confirmed the binding of  
35 ASAs to the sperm head and cytoplasmic droplets, and less frequently to the mid and principal  
36 piece. It was concluded that fixation was not necessary. Dead cells should be excluded from the  
37 analysis since ejaculates with large numbers of dead cells can yield false-positive results. Flow  
38 cytometry was accurate and reliable for detection of sperm-bound IgG and IgA and  
39 discrimination between ASA-positive and ASA-negative bulls.

40

41 Keywords: Flow cytometry; anti-sperm antibodies; sperm-bound antibodies; immunoinfertility;  
42 bovine

43

44 1. Introduction

45

46           During spermatogenesis, developing germ cells express new surface antigens that are not  
47 recognized as self. Sperm-specific surface antigens first appear on pachytene primary  
48 spermatocytes [1]. The blood-testis barrier (BTB), removal of antigenic apoptotic cells by  
49 phagocytosis and immunosuppressive factors released by Sertoli cells confer the testes an  
50 immune privileged status. Disruption of the BTB induced by infectious, inflammatory or  
51 degenerative conditions exposes sperm antigens to the immune system and results in formation  
52 of anti-sperm antibodies (ASAs) [2]. In bulls, genital infection with *Chlamydia sp.*, *Brucella*  
53 *abortus* and Infectious Bovine Rhinotracheitis Virus was associated with concomitant presence  
54 of ASAs [3,4]. Antisperm antibodies were also detected in bulls with seminal vesiculitis [5] and  
55 orchitis [6]. The ASAs persisted in a bull with orchitis for 18 m after initial presentation [6].  
56 Persistence of ASAs can account, at least in part, for the long-term effects of genital infection on  
57 fertility. Exposure to electromagnetic pulses was also shown to alter the BTB and result in  
58 formation of ASAs in mice [7]. Exposure to electromagnetic pulses from electric transmission  
59 lines, generators and fences could represent an unidentified risk factor for immune-mediated  
60 infertility in bulls.

61           Bovine ASAs can reduce penetration and fertilization of oocytes *in vivo* and *in vitro*,  
62 sperm-zona pellucida secondary binding, the ability of capacitated spermatozoa to complete the  
63 acrosome reaction and the motility of capacitated and non-capacitated spermatozoa [8-10].  
64 Antisperm antibodies can impair fertility by contributing one more factor to an already  
65 compromised semen sample, or by being the primary cause of idiopathic infertility. Their effect  
66 on fertility depends on the location of the ASAs, their regional specificity, the antibody class,  
67 isotype and load, and the antigen specificity [11-13]. Antibodies directed against sperm antigens  
68 can be detected free in seminal plasma or serum. However, only those bound to the surface of

69 spermatozoa are of significance for fertility [13]. Both IgA and IgG, but not IgM, have a proven  
70 negative effect on fertility [11,14]. Therefore, an ideal diagnostic test should be able to identify  
71 sperm-bound ASAs and provide information about the proportion of ASA-bound spermatozoa in  
72 an ejaculate, the antibody class and load, and the regional specificity [15].

73         To date, most reports in veterinary medicine have involved the use of indirect techniques  
74 to detect ASAs in serum or seminal plasma. Sperm agglutination [16,17] and immobilization  
75 tests [18] have been used to detect ASAs in bulls. However, these tests are insensitive and  
76 nonspecific [15]. Immunofluorescence [17], immunocytochemistry [3,19] and enzyme-linked  
77 immunosorbent assay [8,20] have also been used in bulls. These techniques require fixation of  
78 the cell membranes. Fixation can result in non-specific binding of antibodies, exposure of  
79 intracellular antigens, denaturation of sperm antigens or membrane damage, resulting in false-  
80 positive or false-negative results [15,21]. The mixed antiglobulin reaction and immunobead-  
81 binding tests are most commonly used in human medicine [22]. These tests provide a semi-  
82 quantitative estimation of the proportion of ASA-positive spermatozoa, and information on the  
83 antibody class and its location on the spermatozoa. However, both tests are based on counting  
84 motile spermatozoa bound to beads or latex particles. Therefore, the estimation is subjective. The  
85 tests require good sperm motility in the samples from the infertile patients if a direct test is used,  
86 or availability of a semen donor with good sperm motility if the indirect test is used [15]. Instead,  
87 flow cytometry allows objective and quantitative estimation of ASAs on the surface of living  
88 spermatozoa and is a sensitive, specific and repeatable test [15]. Flow cytometry also allows  
89 identification of the antibody class, isotype and load [15].

90         The use of flow cytometry to detect ASAs in bulls was only recently reported [6].  
91 Moreover, a standardized direct technique to detect sperm-bound ASAs has not been developed

92 in veterinary medicine. How the samples are processed and analyzed can have a significant  
93 impact on the reliability of the results. When analyzing live cells, cross-linking of surface  
94 antigens by multivalent antibodies, or of antigen-antibody (ag-ab) complexes by secondary  
95 antibodies can cause aggregation of ag-ab complexes into patches and caps [21,23]. Patching  
96 and capping is followed by shedding of the ag-ab complexes. Patching and capping can be  
97 prevented by fixing the cell membranes prior to incubation with antibodies [21,23]. However,  
98 as mentioned before, fixation can alter the membranes or antigens also giving misleading  
99 results [15,21]. Another source of error is nonspecific uptake of antibody by dead spermatozoa.  
100 Nonspecific binding can yield false-positive results if the proportion of dead cells in the  
101 ejaculate is high [15].

102 The objectives of this study were to standardize some methodological and analytical  
103 aspects of a direct technique to detect sperm-bound ASAs in bovine semen using flow  
104 cytometry. The effect of fixation and inclusion of dead cells in the analysis were evaluated,  
105 coefficients of variation for the standardized protocol were calculated and binding of ASAs to  
106 bovine spermatozoa was confirmed with confocal laser scanning microscopy.

107

## 108 2. Materials and Methods

109

### 110 2.1. Animals

111

112 Four 1-year old *Bos Taurus* bulls of Angus breed were purchased from local producers. The  
113 bulls were housed individually or in pairs in pens, and fed brome hay and water *ad libitum*, and 2  
114 lb of sweet feed twice daily. Bulls were allowed to acclimate for one week prior to starting the

115 experiments. To provide a known ASA-positive control, the bulls were immunized with  
116 autologous spermatozoa as described below. When the percentage of ASA-bound spermatozoa  
117 was  $\geq 20\%$ , bulls were considered to have a positive response [24] and experiments were  
118 initiated. Additionally, ten privately owned Angus bulls (standardization of the technique,  $n = 5$ ;  
119 calculation of coefficients of variation,  $n = 5$ ) classified as satisfactory breeders during routine  
120 breeding soundness examination [25] were included as ASA-negative control bulls. Bulls were  
121 considered satisfactory breeders if they had no gross abnormalities of their internal and external  
122 genitalia, a scrotal circumference above the minimum recommended value for the age,  $\geq 30\%$   
123 individual sperm motility and  $\geq 70\%$  morphologically normal spermatozoa [25]. The study was  
124 performed following Kansas State University's Institutional Animal Care and Use Committee's  
125 guidelines. The bulls with experimentally-induced antibodies were euthanized at the end of the  
126 study.

127

## 128 2.2. Semen collection and evaluation

129

130 Semen was collected using electroejaculation (SireMaster Original, ICE Corporation,  
131 Manhattan, KS, USA). The accessory sex glands were massaged transrectally with a gloved hand  
132 for 30 to 60 sec. A 6.5-cm in diameter lubricated rectal probe was inserted into the rectum with  
133 the electrodes facing ventrally. Electrical stimulation was applied with increasing intensity until  
134 ejaculation [25]. A complete semen evaluation [25] was performed immediately after collection.  
135 Semen was then used for immunization or for the experiments.

136

## 137 2.3. Immunization of bulls

138

139        Immunizations were performed as described before with some modifications [18]. Ejaculated  
140 spermatozoa were washed three times by centrifugation at 900 x g for 10 min diluted in warm  
141 Dulbecco's phosphate buffered saline (DPBS, Invitrogen, Grand Island, NY, USA). Washed  
142 spermatozoa,  $1 \times 10^9$ , were re-suspended to 1 mL in DPBS. One milliliter of Freund's complete  
143 adjuvant (Sigma-Aldrich, St. Louis, MO, USA) was then added. Each bull was immunized with  
144 2 mL of inoculum containing  $1 \times 10^9$  autologous spermatozoa. The inoculum was administered  
145 intramuscularly in the neck in four different aliquots of 0.5 mL each. Booster immunizations  
146 were administered to three bulls 22 d after the primary immunization. Semen was processed in the  
147 same way as for primary immunizations but Freund's Incomplete Adjuvant (Sigma-Aldrich) was  
148 used instead of Freund's Complete Adjuvant. One bull did not receive a booster immunization  
149 since the response to the primary immunization was satisfactory.

150

#### 151 2.4. Standardization of flow cytometry for detection of ASAs

152

153        The effect of fixing spermatozoa with formalin buffer solution prior to labeling on the ability  
154 to detect sperm-bound ASAs was evaluated. One ejaculate was collected from each bull with  
155 experimentally-induced ASAs ( $n = 4$ ) and each ASA-negative bull ( $n = 5$ ). Each ejaculate was  
156 initially divided into two aliquots. Semen was diluted to  $50 \times 10^6$  spermatozoa /mL in DPBS  
157 (non-fixed samples) or formalin buffer solution (FBS, Animal Reproduction Systems, Chino,  
158 CA, USA) (fixed samples). Formalin buffer solution had been previously diluted 1:10 in DPBS.  
159 After 10 min at room temperature, samples were washed three times by centrifugation and  
160 labeled with fluorescein isothiocyanate (FITC)-labeled anti-bovine IgG or IgA, or their



161 respective isotype control antibodies as described below. Samples were analyzed by flow  
162 cytometry. The percentage of IgG- and IgA-bound spermatozoa was calculated including the  
163 entire cell population (live and dead cells) or live cells only. Comparisons were made among  
164 treatment groups: non-fixed samples including live cells only in the analysis, non-fixed samples  
165 including both live and dead cells in the analysis, fixed samples including live cells only in the  
166 analysis, and fixed samples including live and dead cells in the analysis.

167

## 168 2.5. Calculation of coefficients of variation

169

170 It was determined in the previous experiment that fixation was not necessary and that  
171 including dead cells in the analysis yielded false-positive results. Therefore, non-fixed samples  
172 were used and only live cells were included in the analysis for calculation of coefficients of  
173 variation (CV). One ejaculate from each ASA-negative (n = 5) and ASA-positive bull (n = 4)  
174 was divided into five aliquots and processed in five replicates to calculate intra-assay CV. One of  
175 the aliquots was evaluated five times to assess intra-sample CV. Only semen from ASA-positive  
176 bulls was available for assessment of the inter-assay CV. Inter-assay CV was calculated  
177 retrospectively from two ejaculates collected from each bull 6 to 20 d apart. The CVs were  
178 calculated with the following formula:  $CV (\%) = \text{mean of standard deviations} / \text{mean} \times 100$ .

179

## 180 2.6. Antibody labeling

181

182 Semen was diluted to a concentration of  $50 \times 10^6$  spermatozoa /mL in warm DPBS, and was  
183 washed three times by centrifugation at  $900 \times g$  for 10 min in DPBS. Then,  $2.5 \times 10^6$  of washed

184 spermatozoa were added to each of four tubes containing 320  $\mu$ L of DPBS. The corresponding  
185 antibodies were added to each tube: IgG = 30  $\mu$ L of FITC-labeled polyclonal goat anti-bovine  
186 IgG F(ab')<sub>2</sub> (12.5  $\mu$ g/mL; Cat. No. 101-096-003, Jackson Immunoresearch Laboratories Inc.,  
187 West Grove, PA, USA); IgG isotype control = 30  $\mu$ L of FITC-labeled polyclonal rabbit anti-goat  
188 IgG F(ab')<sub>2</sub> (12.5  $\mu$ g/mL; Cat. No. 305-096-003; Jackson Immunoresearch Laboratories Inc.);  
189 IgA = 20  $\mu$ L of FITC-labeled polyclonal rabbit anti-bovine IgA (12.5  $\mu$ g/mL; Cat. No. A10-  
190 108F; Bethyl Laboratories, Montgomery, TX, USA); or IgA isotype control = 20  $\mu$ L of FITC-  
191 labeled polyclonal goat anti-mouse IgA (12.5  $\mu$ g/mL; Cat. No. A90-103F; Bethyl laboratories).  
192 A preliminary study was performed to evaluate saturating concentrations and select the  
193 appropriate concentration of each antibody (data not shown). The samples were incubated for 30  
194 min at room temperature in the dark, followed by three washes by centrifugation at 900 x g for  
195 10 min in DPBS. Propidium iodide (PI, viability stain), 5  $\mu$ L, was then added for simultaneous  
196 staining of dead cells.

197

## 198 2.7. Flow Cytometry

199

200 The percentage of IgG- and IgA-bound spermatozoa was assessed by flow cytometry  
201 (FACSCalibur, Becton Dickinson, San Jose CA, USA). From each sample, 10 000 cells were  
202 analyzed at a rate of 1 to 2 x 10<sup>3</sup> cells /sec using DPBS as the sheath fluid. Data from these cells  
203 were collected using forward scatter as the size parameter. A gate containing spermatozoa was  
204 selected based on dot plot distribution of forward (size) versus side scatter (complexity  
205 parameter) to eliminate debris and epithelial cells from the analysis (Fig. 1). The FITC and PI  
206 signals were detected using a standard argon laser (488 nm) and emission filters (535  $\pm$  30 nm

207 for FITC and  $585 \pm 30$  nm for PI). The instrument was calibrated daily with standard beads so  
208 that the CV of the forward scatter and fluorescence channels were  $< 5\%$  on a daily basis.  
209 Compensation for FITC emission into the PI detector or vice versa was done by establishing  
210 quadrants on spermatozoa labeled only with PI or FITC-conjugated antibodies, followed by  
211 electronic subtraction of the FITC emission into the PI detector and PI emission into the FITC  
212 detector. After color compensation, fluorescence emission data were collected with logarithmic  
213 amplification for green fluorescence (FITC using FL1 detector) and orange-red fluorescence (PI  
214 using FL2 detector). Quadrant settings were adjusted for each sample. The control quadrant  
215 (lower left, LL) was marked on samples labeled with the isotype control to include  $< 1\%$  of cells  
216 as positive in the upper left (UL), upper right (UR) and lower right (LR) quadrants (Fig. 1). The  
217 ASA-negative dead cells (PI stained) appeared in the UL quadrant, ASA-negative live cells (no  
218 stain) in the LL quadrant, ASA-positive dead cells (dual stained) in the UR quadrant, ASA-  
219 positive live cells (FITC stained) in the LR quadrant (Fig. 1). The percentage of ASA-positive  
220 live spermatozoa (LR quadrant) was calculated considering only live cells (PI negative cells in  
221 LL and LR quadrants) in the analysis. When including dead cells (PI positive cells), the  
222 percentage of ASA-positive spermatozoa (LR and UR quadrants) was calculated considering all  
223 quadrants.

224

## 225 2.8. Confocal laser scanning microscopy

226

227 Labeled spermatozoa from bulls with experimentally-induced antibodies were evaluated  
228 under confocal laser scanning microscopy to confirm binding of the antibodies to the sperm  
229 surface. No attempts were made to quantitatively evaluate the percentage of ASA-bound

230 spermatozoa or the relative distribution of the binding sites. Spermatozoa were labeled with  
231 FITC-labeled anti-bovine IgG or IgA as described above. After labeling, 10  $\mu$ L of FBS was  
232 added to inhibit sperm motility and facilitate visual evaluation. A drop of sperm suspension was  
233 evaluated on a microscope slide under a cover slide. The FITC signal was excited at 488 nm and  
234 was collected with a band pass filter at a wavelength of 505-550 nm. Samples were assessed at  
235 X20 and X40 and optical sections were collected (LSM 710 META, Carl Zeiss MicroImaging,  
236 Thornwood, NY).

237

## 238 2.9. Statistical analysis

239

240 Statistical analysis was performed using SAS package (SAS Institute, Cary, NC, USA).  
241 Distribution of the data was tested for normality using a Shapiro Wilk test. Data were not  
242 normally distributed. To determine response to immunization, percentages of IgG- and IgA-  
243 bound spermatozoa before and after the last immunization were compared using a Wilcoxon  
244 signed test. Only non-fixed live spermatozoa were included in this analysis. To assess the effect  
245 of fixation and inclusion of dead cells in the analysis, differences in median percentages of IgG-  
246 and IgA-bound spermatozoa among treatment groups were compared using a Friedman test. The  
247 Friedman test is a non-parametric test that compares median values across treatments controlling  
248 for bull. Since non-parametric tests were used, data were reported as median  $\pm$  SE. Differences  
249 were considered significant at  $P < 0.05$ .

250

## 251 3. Results

252

253 Immunization with autologous spermatozoa induced a significant increase in the  
254 percentage of both IgG-bound spermatozoa and IgA-bound spermatozoa. The percentage of IgG-  
255 bound spermatozoa was  $2.9 \pm 2.1$  % and  $89.8 \pm 4.6$  % before and after immunization,  
256 respectively ( $P = 0.0209$ ). The percentage of IgA-bound spermatozoa was  $7.7 \pm 2.2$  % and  $75.7 \pm$   
257  $18.9$  % before and after immunization, respectively ( $P = 0.0433$ ) (median  $\pm$  SE).

258 There was no significant difference in the percentage of IgG- or IgA-bound spermatozoa  
259 between samples fixed with FBS and non-fixed samples (Fig. 2). Including dead cells in the  
260 analysis increased the percentage of IgG- ( $P = 0.0029$ ) and IgA-bound spermatozoa ( $P = 0.0041$ )  
261 detected in semen samples from ASA-negative bulls (Fig. 2). However, median percentages of  
262 ASA-bound spermatozoa did not differ among semen samples from ASA-positive bulls when  
263 dead cells were included in the analysis (Fig. 2).

264 Intra-sample CV for determination of sperm-bound IgG was 0.8 %, intra-assay CV was  
265 4.6 % and inter-assay CV was 5.3 %. For determination of sperm-bound IgA, intra-sample CV  
266 was 2.8 %, intra-assay CV was 8.4 % and inter-assay CV was 40.3 %. Both antibody classes  
267 bound to the acrosomal, equatorial and post-acrosomal areas of the sperm head, and to  
268 cytoplasmic droplets (Fig.3). Least frequently, ASAs bound to the sperm midpiece and principal  
269 piece.

270

#### 271 4. Discussion

272

273 Systemic immunization with autologous spermatozoa induced an immune response in all  
274 bulls characterized by an increase in sperm-bound IgG and IgA. Immunoglobulin G in genital  
275 secretions is mostly derived from systemic circulation [26]. In the presence of an intact blood-

276 testis or blood-epididymis barrier, IgG reaches the genital tract and binds to spermatozoa at the  
277 rete testis or at ejaculation when spermatozoa contact the secretions of the accessory sex glands  
278 [27-29]. On the other hand, IgA is produced locally [26]. Systemic immunization can result in  
279 increased production of IgA within the genital tract, and increases in antigen-specific B cells in  
280 the testis [29]. It is possible that systemic immunization of bulls with spermatozoa induced both  
281 a systemic and mucosal immune response here. It is also possible that migration of activated  
282 IgA-committed B cells from lymph nodes draining the injection site to the genital mucosa  
283 contributed to the increase in sperm-bound IgA after immunization, as described in humans [30].

284         Recommendations for processing and evaluating bovine semen samples for detection of  
285 sperm-bound ASAs by flow cytometry can be made based on the results of this study. Polyclonal  
286 antibodies and F(ab')<sub>2</sub> fragments were used here. Since they are expected to react with all  
287 subclasses, use of polyclonal antibodies may decrease the likelihood of obtaining false-negative  
288 results [15]. Use of F(ab')<sub>2</sub> fragments is also preferred to prevent non-immune binding of the Fc  
289 portion of the IgG molecule to the sperm membrane [15], which occurs via disulfide  
290 rearrangement at the cell surface in bulls [31]. Fixation of sperm membranes with formalin  
291 buffer solution prior to labeling did not affect the ability to detect sperm-bound ASAs. Fixation  
292 was performed to potentially prevent patching or capping of ag-ab complexes, which would have  
293 yielded false-negative results. Mature spermatozoa have both mobile and non-mobile surface  
294 antigens [32,33]. Patching and capping involve redistribution of mobile antigens in response to  
295 multivalent ligands. Patching is a local clustering of molecules, while capping is the aggregation  
296 of the clusters to a single area of the membrane. Following capping, molecules are shed from the  
297 cell membrane [23]. While these phenomena were demonstrated in early spermatogenic cells [1],  
298 patching and capping were not observed in late spermatids [1] or mature spermatozoa [34]. It

309 was speculated that non-mobile antigens are inserted later in germ cell development, and that  
300 cross-linking between mobile and non-mobile antigens results in loss of capping in late  
301 spermatids [1] and spermatozoa. While fixation may be necessary to prevent lateral mobility of  
302 antigens, it can also alter the results by causing non-specific binding of antibodies, exposure of  
303 intracellular antigens, denaturation of sperm antigens and membrane damage [15,21]. It was  
304 concluded that since fixation of sperm membranes prior to labeling did not affect the results but  
305 increased processing times, this procedure could be avoided.

306 When dead cells were included in the analysis, false-positive results were obtained in  
307 samples from ASA-negative bulls. It is likely that non-specific binding of antibodies to dead  
308 cells or increased autofluorescence displayed by dead cells accounted for the increase in the  
309 percentage of fluorescently-labeled spermatozoa among ASA-negative bulls [15,35]. In ASA-  
310 positive bulls, the percentage of ASA-bound spermatozoa was already high. Even when non-  
311 specific binding to dead cells may have occurred, the difference may not have been large enough  
312 to be significant. It was concluded that dead cells should be excluded from the analysis to  
313 prevent false-positive results in ASA-negative bulls. This limits the use of flow cytometry to  
314 detect ASAs in bulls with necrozoospermia.

315 Coefficients of variation were all  $< 10\%$ , except for inter-assay CV for IgA-bound  
316 spermatozoa. It is not known if this high CV resulted from the low number of samples available,  
317 or from different frequencies of ejaculation that resulted in varying storage times and contact  
318 with ASA-loaded genital secretions. It is also possible that the variation reflected changes in  
319 antibody titers at different times post-immunization and was inherent to the model used rather  
320 than the test itself. The reason for the high inter-assay CV of the IgA test requires further  
321 investigation with more standardized sampling times. Nonetheless, the percentage of IgA-bound

322 spermatozoa was  $\geq 20\%$  in all samples from all ASA-positive bulls. In spite of the high inter-  
323 assay CV, the test was able to correctly identify IgA-positive bulls. With this exception, CVs in  
324 this study were similar to those reported in the human literature [15]. It was concluded that flow  
325 cytometry was accurate and reliable for detection of sperm-bound ASAs and discrimination  
326 between ASA-positive and ASA-negative bulls.

327         Confocal laser microscopy confirmed binding of ASAs to the sperm surface. The  
328 combination of flow cytometry and fluorescence microscopy provided an ideal diagnostic  
329 approach. Flow cytometry allowed identification of sperm-bound ASAs and provided objective  
330 and quantitative information about the antibody class and load. Additional use of fluorescence  
331 microscopy provided information about the regional specificity of the ASAs. Due the lack of  
332 reports on presence and behavior of naturally-occurring sperm-bound antibodies in bulls, it is  
333 difficult to determine how detection of experimentally-induced antibodies compares with  
334 detection of sperm-bound ASAs produced during bacterial infection or trauma. Studies are under  
335 way to determine the reference ranges and prevalence of naturally-occurring sperm-bound ASAs  
336 in satisfactory breeder beef bulls and bulls with reproductive pathology.

337         In conclusion, a direct technique to detect sperm-bound ASAs in bull semen was  
338 developed. Flow cytometry was accurate and reliable for detection of sperm-bound ASAs and  
339 discrimination between ASA-positive and ASA-negative bulls. When combined with  
340 fluorescence microscopy, this method provided an ideal diagnostic approach for objective and  
341 quantitative evaluation of sperm-bound ASAs in bulls.

342

343 Disclosure statement

344



345 The authors declare that there is no conflict of interest that could be perceived as prejudicing the  
346 impartiality of the research reported.

347

#### 348 Funding

349

350 This work was supported by Kansas State University, College of Veterinary Medicine, Mentored  
351 Clinical and Applied Translational Research, and NIH-P20-RR017686, COBRE Core B.

352

#### 353 Acknowledgements

354

355 The authors thank Tammy Koopman for providing guidance and assay troubleshooting with flow  
356 cytometry, and Joel Sannemann for his assistance on the use of the confocal laser microscope.

357 Thanks to Shelie Laflin, Meredyth Jones, Matt Miesner and Andrea Meyer for providing semen  
358 samples from ASA-negative bulls. Robert Larson provided guidance with the statistical analysis.

359

#### 360 References

361

362 [1] Romrell LJ, O’Rand MG. Capping and ultrastructural localization of sperm surface  
363 isoantigens during spermatogenesis. *Dev Biol* 1978;63:76-3.

364 [2] Comhaire FH, Mahmoud AMA, Depuydt CE, Zalata AA, Christophe AB. Mechanisms and  
365 effects of male genital tract infection on sperm quality and fertilizing potential: the andrologist’s  
366 point of view. *Human Reprod Update* 1999;5:939-98.

367 [3] Zralý Z, Benová J, Šišák M, Diblíková I, Švecová D, Zajícová A, Věžník Z. Occurrence of  
368 antibodies to sperms in blood sera of bulls and boars. *Vet Med – Czech* 1998;43:197-204.

369 [4] Hegazi AG, Ezzo O. Serum auto antibodies in buffaloes and cattle naturally infected with  
370 IBRV and brucella. *Buffalo J* 1995;3:325-30.

371 [5] Perez T, Carrasco LW. Autoimmunizacion espermatica en sementales bovinos como causa de  
372 subfertilidad. *IVth Int Congr Anim Reprod Artif Insem* 1964; 5:527.

373 [6] Vlok I, Ferrer M, Sardoy M, Anderson D. Serum anti-sperm antibodies associated with  
374 orchitis in a bull. *Clinical Theriogenology* 2009;1:251.

375 [7] Wang XW, Ding GR, Shi CH, Zeng LH, Liu JY, Li J, Zhao T, Chen YB, Guo GZ.  
376 Mechanisms involved in the blood-testis barrier increased permeability induced by EMP.  
377 *Toxicology* 2010;276:58-63.

378 [8] Kim CA, Parrish JJ, Momont HW, Lunn DP. Effects of experimentally generated bull  
379 antisperm antibodies on in vitro fertilization. *Biol Reprod* 1999; Jun;60(6):1285-91.

380 [9] Coonrod SA, Westhusin ME, Naz RK. Monoclonal antibody to human fertilization antigen-1  
381 (FA-1) inhibits bovine fertilization in vitro: application in immunocontraception. *Biol Reprod*  
382 1994;51:14-23.

383 [10] Coonrod SA, Herr JC, Westhusin ME. Inhibition of bovine fertilization in vitro by  
384 antibodies to SP-10. *J Reprod Fertil* 1996;107:287-97.

385 [11] Yeh WR, Acosta AA, Seltman HJ, Doncel G. Impact of immunoglobulin isotype and sperm  
386 surface location of antisperm antibodies on fertilization in vitro in the human. *Fertil Steril*  
387 1995;63:1287-92.

- 388 [12] Krause WKH. Sperm functions influenced by immune reactions. In: Immune Infertility,  
389 Krause WKH and Naz RK, Eds., Springer Verlag Berlin Heidelberg, Berlin, Germany. 2009, p.  
390 49-65.
- 391 [13] Eggert-Kruse W, Christmann M, Gerhard I, Pohl S, Klinga K, Runnenbaum B. Circulating  
392 antisperm antibodies and fertility prognosis: a prospective study. *Hum Reprod* 1989;4:513-20.
- 393 [14] Chamley LW, Clarke GN. Antisperm antibodies and conception. *Semin Immunopathol*  
394 2007; 29:169–84.
- 395 [15] Räsänen ML, Hovatta OL, Penttilä IM, Agrawal YP. Detection and quantitation of sperm-  
396 bound antibodies by flow cytometry of human semen. *J Androl*. 1992;13:55-64.
- 397 [16] Wright PJ. Serum spermagglutinins and semen quality in the bull. *Australian Vet J*  
398 1980;56:10-13.
- 399 [17] Purswell BJ, Dawe DL, Caudle AB, Williams DJ, Brown J. Spermagglutinins in serum and  
400 seminal plasma of bulls and their relationship to fertility classification. *Theriogenology*  
401 1983;20:375-81.
- 402 [18] Menge AC, Christian JJ Jr. Effects of auto- and iso-immunization of bulls with semen and  
403 testis. *Int J Fertil* 1971; 16:130-8.
- 404 [19] Fayemi O. Sperm antibodies and reproductive efficiency in the zebu cattle in south-western  
405 Nigeria. *Pakistan Vet J* 2005; 25:111-4.
- 406 [20] Zralý Z, Benová J, Diblíková I, Švecová D, Kummer V, Mašková J, Věžník Z. Antisperm  
407 antibodies in blood sera of bulls and correlations with age, breed and ejaculate quality. *Acta Vet*  
408 Brno 2002;71:303-8.

409 [21] Nikolaeva MA, Kulakov VI, Korotkova IV, Gulobeva EL, Kuyavskaya DV, Sukhikh GT.  
410 Antisperm antibodies detection by flow cytometry is affected by aggregation of antigen-antibody  
411 complexes on the surface of spermatozoa. *Human Reprod* 2000;15:2545-53.

412 [22] Krapez JA, Hayden CJ, Rutherford AJ, Balen H. Survey of the diagnosis and management  
413 of antisperm antibodies. *Hum Reprod* 1998;13:3363-7.

414 [23] Santoso S, Zimmerman U, Neppert J, Mueller-Eckhardt C. Receptor patching and capping  
415 of platelet membranes induced by monoclonal antibodies. *Blood* 1986;67:343-9.

416 [24] Nicholson SC, Robinson JN, Sargent IL, Barlow DH. Detection of antisperm antibodies in  
417 seminal plasma by flow cytometry: comparison with the indirect immunobead binding test. *Fertil*  
418 *Steril* 1997;68:1114-9.

419 [25] Chenoweth PJ, Hopkins FM, Spitzer JC, Larsen RE. Guidelines for using the bull breeding  
420 soundness evaluation form. *Clin Theriogenology* 2010;2:43-9.

421 [26] Mestecky J, Fultz PN. Mucosal immune system of the human genital tract. *J Infect Dis*  
422 1999;179(suppl 3):S470-4.

423 [27] Knee RA, Hickey DK, Beagley KW, Jones RC. Transport of IgG across the blood-luminal  
424 barrier of the male reproductive tract of the rat and the effect of estradiol administration on  
425 reabsorption of fluid and IgG by the epididymal ducts. *Biol Reprod* 2005;73:688-94.

426 [28] Wang Y, Ben K, Cao X, Wang Y. Transport of anti-sperm monoclonal IgA and IgG into  
427 murine male and female genital tracts from blood. Effect of Sex Hormones. *J Immunol*  
428 1996;156:1014-9.

429 [29] Cunningham KA, Carey AJ, Finnie JM, Bao S, Coon C, Jones R, Wijburg O, Strugnell RA,  
430 Timms P, Beagley KW. Poly-immunoglobulin receptor-mediated transport of IgA into the male

431 genital tract is important for clearance of Chlamydia muridarum infection. Am J Reprod  
432 Immunol 2008; 60:405–14.

433 [30] Brokstad KA, Cox RJ, Olofsson J, Jonsson R, Haaheim LR. Parenteral influenza  
434 vaccination induces a rapid systemic and local immune response. J Infect Dis 1995;171:198-203.

435 [31] Richards JM, Witkin SS. Non-immune IgG binding to the surface of spermatozoa by  
436 disulphide arrangement. Clin Exp Immunol 1984;58:493-501.

437 [32] O’Rand MG, Metz CB. Immunofluorescence of rabbit spermatozoa treated with anti-sera to  
438 a single sperm surface membrane glycoprotein and wheat germ agglutinin. J Cell Biol  
439 1975;67:317a.

440 [33] Gaunt SJ, Brown CR, Jones R. Identification of mobile and fixed antigens on the plasma  
441 membrane of rat spermatozoa using monoclonal antibodies. Exp Cell Res 1983;144:275-284.

442 [34] Koehler JK. Studies on the distribution of antigenic sites on the surface of rabbit  
443 spermatozoa. J Cell Biol 1975;67:647-59.

444 [35] Schmid I, Ferbas J, Uittenbogaart CH, Giorgi JV. Flow cytometric analysis of live cell  
445 proliferation and phenotype in populations with low viability. Cytometry 1999;35:64-74.

446

447

448


449

450

451

452

453



454  
 455  
 456  
 457  
 458  
 459

460 Fig. 1. Example of dot plot distribution of forward (FSC-H) and side scatter (SSC-H) of a  
 461 washed sperm sample (left panel). The cells within gate 1 (R1) represent the population of  
 462 spermatozoa. Example of dot plot distribution of two-color analysis of a sperm sample from a  
 463 bull with experimentally-induced anti-sperm antibodies stained with FITC-labeled anti-mouse  
 464 IgA (isotype control) (central panel) or FITC-labeled anti-bovine IgA (right panel). Fluorescence  
 465 data was collected with logarithmic amplification for green (FITC; FL1-H) and red (PI; FL2-H)  
 466 fluorescence. The anti-sperm antibody (ASA)-negative dead sperm appeared in the upper left  
 467 (UL) quadrant, ASA-negative live sperm in the lower left (LL) quadrant, ASA-positive dead  
 468 sperm in the upper right (UR) quadrant, and ASA-positive live sperm in the lower left (LR)  
 469 quadrant.

470  
 471  
 472  
 473  
 474  
 475  
 476

477  
478  
479  
480  
481  
482  
483  
484  
485  
486  
487  
488  
489  
490  
491  
492  
493  
494

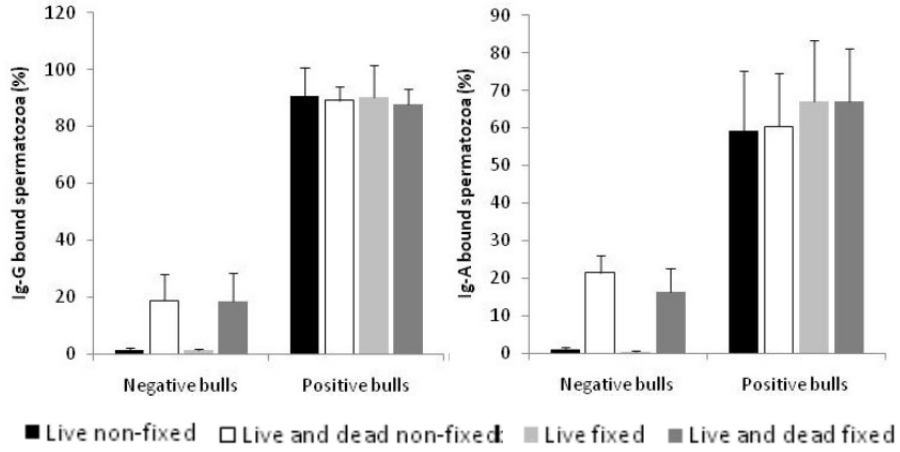


Fig. 2. Percentage of anti-sperm antibody (ASA)-bound spermatozoa in samples fixed with formalin buffer solution and non-fixed samples, and including live only or live and dead cells in the analysis. <sup>a,b</sup>Values with different superscript differ significantly among treatments within ASA-negative bulls (Median  $\pm$  SE).




Fig. 3. Antibody-negative spermatozoa (left) and spermatozoa with IgG binding to the equatorial area and the junction between the sperm head and midpiece (right).