

CALIBRATION OF A FAST FIELD CYCLING RELAXOMETER FOR ULTRA-LOW FIELD MEASUREMENTS OF T_1 -DISPERSION

Vasileios Zampetoulas, Lionel M. Broche and David J. Lurie

Aberdeen Biomedical Imaging Centre, University of Aberdeen,
Foresterhill, Aberdeen, AB25 2ZD, Scotland, United Kingdom

www.ffc-mri.org

In Fast-Field Cycling (FFC) MRI the field switches to different levels, allowing for the measurement of NMR parameters such as T_1 over a range of fields [1].

For the successful implementation of the ultra-low field FFC techniques on a commercial bench-top FFC relaxometer (Stelar S.r.l., Italy) the stray magnetic fields need to be compensated. These are determined with the application of FFC measurements in a range of fields close to zero. During this process correction fields of varying magnitude and orientation are applied by the relaxometer while the magnetisation precesses around a stray component of unknown direction with the frequency of precession determined by the magnitude of the transverse and longitudinal fields. The successful compensation of the stray fields is shown as a minimum in the frequency of precession (Figure 1a) [2].

After the successful calibration of the relaxometer FC methods at ultra-low fields can be applied, including extension of the T_1 -dispersion curve acquired to the region of μT (Figure 1b).

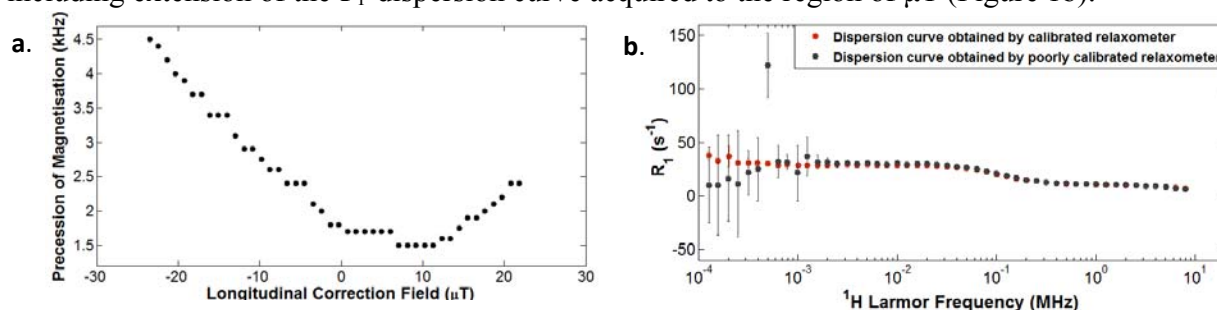


FIGURE 1. (a) Precession frequency against the longitudinal correction field applied. The minimum is observed in the range of 6 to 12 μT . For values larger than 22 μT magnetisation decays exponentially as in conventional FFC experiments thus no precession is observed (b) R_1 -dispersion curve (where $R_1=1/T_1$) of a sample of MnCl_2 acquired before and after the calibration, with the range of minimum ^1H Larmor frequencies extending to 100 Hz (corresponding to a field of 2.3 μT).

Acknowledgements

The author acknowledges funding from the EPSRC through the Centre for Doctoral Training in Integrated Magnetic Resonance.

References

- [1] Kimmich R, Anoardo E., Prog. NMR Spectrosc., **44**, 257-320 (2004).
- [2] Anoardo E, Ferrante GM, Appl. Magn. Reson., **24**, 85-96 (2003).