



Contents lists available at ScienceDirect

Electrochemistry Communications

journal homepage: www.elsevier.com/locate/elecom

Detection of hydrogen peroxide produced at a liquid/liquid interface using scanning electrochemical microscopy

Fei Li, Bin Su, Fernando Cortes Salazar, Raheleh Partovi Nia, Hubert H. Girault *

Laboratoire d'Electrochimie Physique et Analytique, Ecole Polytechnique Fédérale de Lausanne (EPFL), Station 6, CH-1015 Lausanne, Switzerland

ARTICLE INFO

Article history:

Received 14 November 2008
Received in revised form 8 December 2008
Accepted 9 December 2008
Available online 16 December 2008

Keywords:

Scanning electrochemical microscopy
Liquid/liquid interface
Oxygen reduction reaction
H₂O₂ production
Substrate generation/tip collection

ABSTRACT

Scanning electrochemical microscopy (SECM) was used to monitor *in situ* hydrogen peroxide (H₂O₂) produced at a polarized water/1,2-dichloroethane (DCE) interface. The water/DCE interface was formed between a DCE droplet containing decamethylferrocene (DMFc) supported on a solid electrode and an acidic aqueous solution. H₂O₂ was generated by reducing oxygen with DMFc at the water/DCE interface, and was detected with a SECM tip positioned in the vicinity of the interface using a substrate generation/tip collection mode. This work shows unambiguously how the H₂O₂ generation depends on the polarization of the liquid/liquid interface, and how proton-coupled electron transfer reactions can be controlled at liquid/liquid interfaces.

© 2008 Elsevier B.V. All rights reserved.

1. Introduction

The interface between two immiscible electrolyte solutions (ITIES), is well-suited to carry out proton-coupled electron transfer reactions [1–3], i.e., protons can be provided from the aqueous side, and lipophilic electron donors or acceptors can be located in the organic side. Furthermore, by controlling the polarization of the interface, it is possible to control the rate of either proton or electron transfer across the interface. Recently, we have investigated oxygen reduction by lipophilic donors in 1,2-dichloroethane (DCE) in contact with aqueous acid solutions and shown that the final product of this biphasic reaction was hydrogen peroxide (H₂O₂) in water [4].

Herein, scanning electrochemical microscopy (SECM) was employed for the detection of H₂O₂ generated at a water/DCE interface. SECM is a well-established technique with a key advantage of localizing and detecting interfacial electrochemical reactions [5] and has been widely employed to detect H₂O₂ produced by the oxygen reduction reaction (ORR) on various solid substrates [6–8]. In this work, the water/DCE interface was formed between a DCE droplet containing DMFc supported on a solid electrode and immersed in an acidic aqueous solution. The SECM tip was positioned close to the water/DCE droplet interface in the top aqueous solution. With this configuration, the polarization of the water/DCE interface to drive the proton transfer to allow oxygen

reduction with DMFc on the organic side of the interface was found to be concomitant with the amperometric detection H₂O₂ by the SECM tip biased at a potential for the oxidation of H₂O₂. The different SECM parameters, including the tip-interface distance and interfacial Galvani potential difference, have been optimized for an efficient H₂O₂ detection.

2. Experimental

All chemicals were used as received. The organic supporting electrolyte was bis(triphenylphosphoranylidene) ammonium tetrakis(pentafluorophenyl)borate (BTTPATPFB) [9]. All aqueous solutions were prepared with Milli-Q reagent water (Millipore, > 18.2 MΩ/cm) and the DCE (Synthesis Grade, SDS) was saturated with water prior to use.

All the electrochemical measurements were carried out on a CHI 900 SECM (CH Instruments, Austin, TX) at room temperature with air-saturated solutions. A 5 μL DCE droplet was deposited on the surface of a 2 mm-diameter silver/silver tetrakis-(pentafluorophenyl)borate (Ag/AgTPFB) electrode [10], which was inserted into a Teflon cell and 1.5 mL aqueous solution was added on the top of it to overlap the droplet, a water/DCE interface was thus formed. The voltammograms at this interface were obtained in a three-electrode configuration (Fig. 1a) with the DCE droplet-covered Ag/AgTPFB electrode as the working electrode (WE), a Ag/AgCl wire and a Pt wire positioned in the aqueous solution as the reference electrode (RE) and counter electrode (CE), respectively. The electrochemical cell is depicted as follows:

* Corresponding author. Tel.: +41 0 21 6933151; fax: +41 0 21 6933667.
E-mail address: hubert.girault@epfl.ch (H.H. Girault).


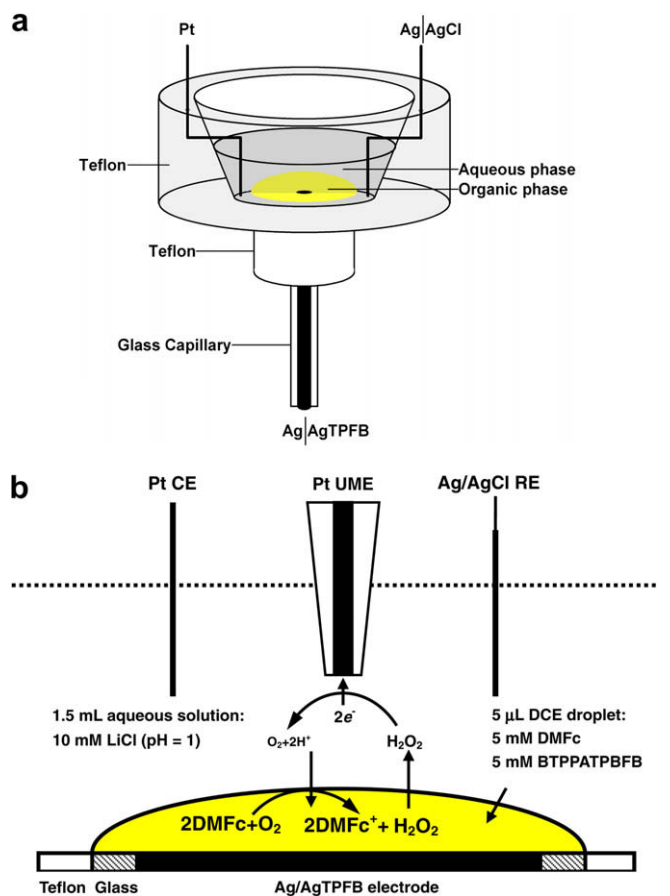


Fig. 1. Schematic diagrams of (a) a three-electrode cell and (b) its combination with SECM in a SG/TC mode.



The Galvani potential difference across the water/DCE interface ($\Delta\phi^w$) was calibrated by the ion transfer of tetraethylammonium (TEA^+) [11]. The ionic current resulting from the transfer of cation from the aqueous to DCE phase is defined as a positive current.

The combination of SECM with the droplet was achieved by positioning a 25 μm -diameter Pt microelectrode tip [12] ($\text{RG} = r_g/a$ was about 3, where r_g is the radius of the glass insulator plus the radius a of the disk-shape microelectrode) on the top of the droplet, as illustrated in Fig. 1b. The Pt microelectrode was first brought to a known distance from the droplet on the basis of feedback current measurements. The tip current due to H_2O_2 oxidation was then monitored using the substrate generation/tip collection (SG/TC) mode [5], whereby the Galvani potential difference across the water/DCE interface was scanned or biased at a constant value through applying a potential at the substrate electrode and the tip potential was simultaneously scanned or fixed at a H_2O_2 oxidation potential. The tip and substrate potentials were independently controlled by the SECM bipotentiostat.

3. Results and discussion

Fig. 2a shows the cyclic voltammograms obtained at the water/DCE droplet interface supported on an Ag/AgTPFB electrode. The dotted curve represents the cyclic voltammogram in the absence

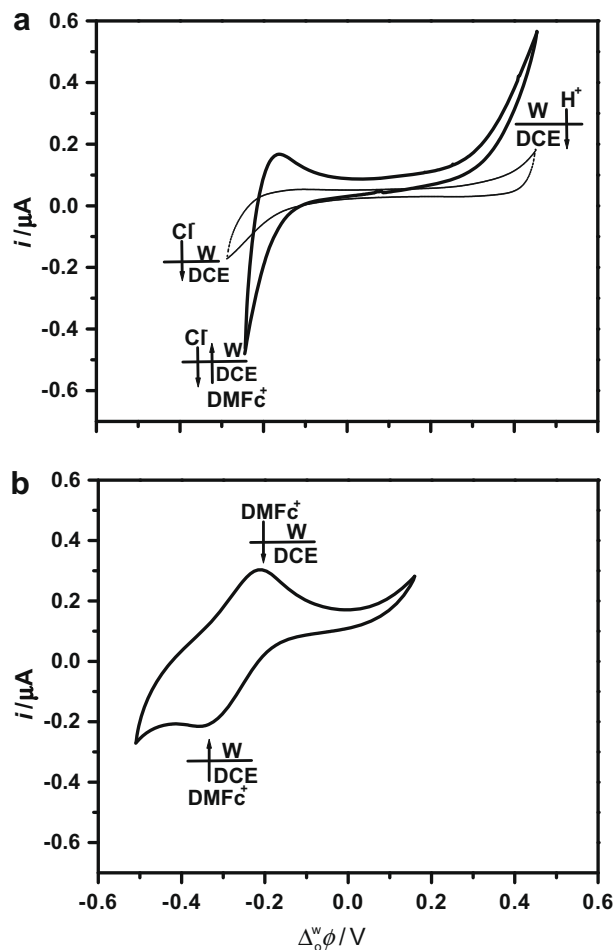


Fig. 2. Cyclic voltammograms measured with: (a) Cell 1 in the absence (dotted curve) and presence (solid curve) of 5 mM DMFc in DCE and (b) Cell 1 but using Li_2SO_4 (10 mM) and H_2SO_4 (pH 3) instead of LiCl and HCl in the aqueous phase. Scan rates 20 mV s^{-1} .

of DMFc, which shows a potential window limited by the transfers of Cl^- and H^+ from aqueous to DCE phases on the negative and positive sides, respectively [11]. In Cell 1 including 5 mM DMFc in the DCE droplet, a current increase was observed at positive potentials (solid curve), which is similar to that observed at a water/DCE interface using a four-electrode setup [4] and the current increase stems from a proton transfer followed by O_2 reduction with DMFc to produce H_2O_2 (Fig. 1b). Moreover, an ion transfer voltammetric wave of decamethylferrocenium (DMFc^+) produced by O_2 reduction can be visualized in Fig. 2b, if extending the negative side of the potential window by replacing the aqueous supporting electrolyte anion Cl^- with more hydrophilic SO_4^{2-} . These facts prove that the oxygen reduction by DMFc can be realized with the present droplet methodology using a three-electrode setup, which also suggests a potential polarization range, namely 0.25 ~ 0.45 V, for the following SECM detection of H_2O_2 .

To perform the SG/TC measurement to detect H_2O_2 generated at the water/DCE interface, the tip potential and tip-interface distance must be optimized. First, the tip potential was determined as 0.6 V (oxidation potential of H_2O_2) by recording a linear sweep voltammogram (LSV) with the Pt microelectrode in an acid aqueous solution containing 0.1 mM H_2O_2 (figure not shown here). The tip-interface distance was determined by moving the Pt microelectrode slowly to the water/DCE interface with a tip potential (E_{tip}) of 0.6 V and the Galvani potential difference across the

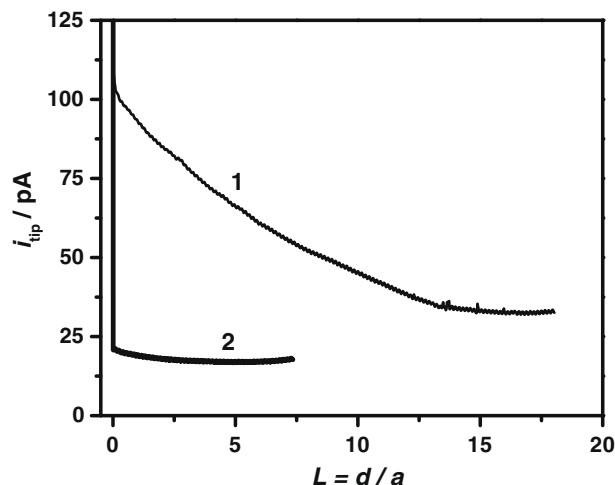


Fig. 3. Experimental approach curves with (Curve 1) and without (Curve 2) applying 0.45 V at the water/DCE interface: the tip potential 0.6 V and the approach rate $0.5 \mu\text{m s}^{-1}$.

water/DCE interface of 0.45 V. A gradual increase in the tip current due to the oxidation of H_2O_2 was observed as the tip approaches the water/DCE interface (Curve 1 in Fig. 3). The sharp increase of the tip current indicates a contact of the tip with the interface (due to oxidation of DMFc in DCE), which is taken as the zero tip-interface distance. Note that a control approach curve (Curve 2 in Fig. 3) was also measured by keeping the substrate Ag/AgTPFB electrode open circuited, in which no tip current increase was observed as no H_2O_2 was produced. Based on this feedback operation, the Pt microelectrode can be positioned about $15 \sim 20 \mu\text{m}$ above the water/DCE interface.

The final detection of H_2O_2 generated at the interface was based on the SG/TC operation mode in two ways. First, a LSV was measured at the tip when a constant potential of 0.45 V was applied at the water/DCE interface. As shown in Fig. 4a, instead of a conventional steady-state behavior at a microdisk electrode, a peak-shaped wave is observed at about 0.6 V, which is due to the H_2O_2 oxidation at the Pt microelectrode is not diffusion-controlled as it involves some surface reactions with platinum oxide [13,14].

Alternatively, the detection of H_2O_2 by SECM was performed using the method described by Zhou et al. [15], where the tip potential was held at 0.6 V and the Galvani potential difference across the water/DCE interface was cycled between -0.25 and 0.45 V. In this case, the cyclic voltammograms of the water/DCE interface and the tip current can be recorded simultaneously, as shown in Fig. 4b and c. The cyclic voltammogram of the water/DCE interface (Fig. 4b) is similar to the one observed in Fig. 2a with an irreversible current rising at positive potentials ($0.25\text{--}0.45$ V). Accordingly, in this potential range, the tip current on the forward scan (solid curve in Fig. 4c) for the oxidation of H_2O_2 increases as the Galvani potential difference becomes more positive (solid curve in Fig. 4b). When sweeping the Galvani potential difference across the water/DCE interface backward from 0.45 V to a lower value (dotted curve in Fig. 4b), the tip current (dotted curve in Fig. 4c) continues to increase and then falls following the decrease of the current at the water/DCE interface. At potentials below 0.25 V on the forward scan, the tip current is constant at a residual plateau value indicating that the production of H_2O_2 at the water/DCE interface does not occur. The synchronicity between the tip and interface current proves that the generation of H_2O_2 at the water/DCE interface is an interface potential-dependent process. The interface functions as a proton pump driven by the Galvani potential difference and the reaction pathway can be expressed as:





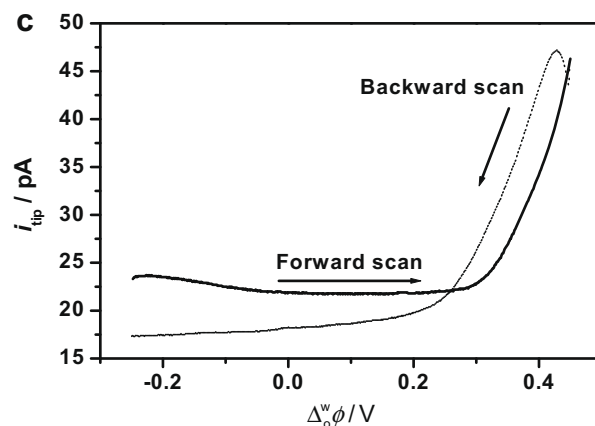


Fig. 4. (a) LSV at the Pt microelectrode obtained by applying 0.45 V at the water/DCE interface. The tip-interface distance $20 \mu\text{m}$ and the scan rate 10 mV s^{-1} , (b) Substrate and (c) tip voltammograms obtained with the tip potential held at 0.6 V and the Galvani potential difference across the water/DCE interface was scanned from -0.25 to 0.45 V at a scan rate of 10 mV s^{-1} . The tip-interface distance was $15 \mu\text{m}$.

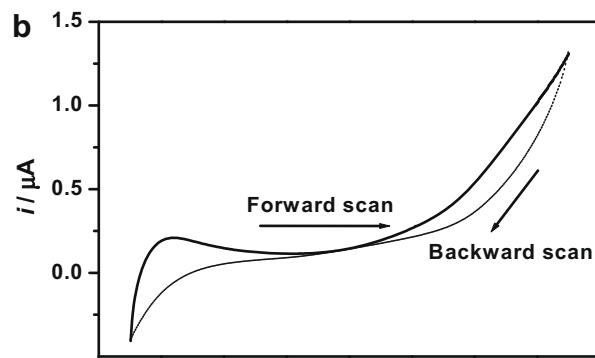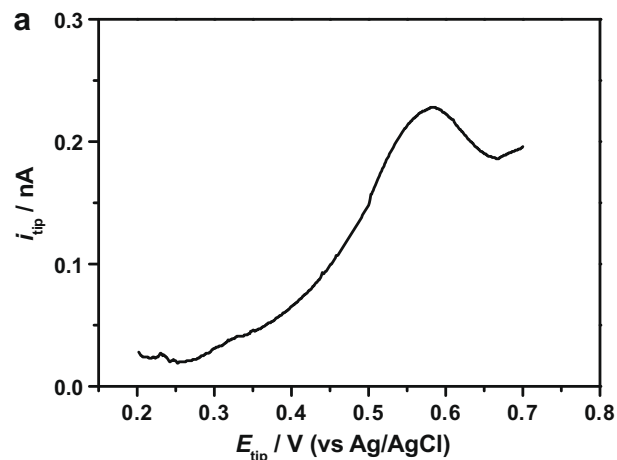

Density functional theory (DFT) calculations (details not shown here) have shown that DMFc preferentially complexes with O_2 to form a superoxide adduct, which can further bind a proton from water. This protonated superoxide species can be reduced by a second DMFc to produce H_2O_2 . Considering that H_2O_2 is very hydrophilic, any H_2O_2 produced on the organic side of the interface is extracted to water [4], and can therefore be detected at the SECM tip.

4. Conclusions

The produced H_2O_2 at the water/DCE interface was successfully detected by SECM combined with a droplet method in a substrate generation/tip collection mode on the basis of monitoring the tip current. The resulting tip current for the H_2O_2 oxidation is concomitant with the substrate current due to the H_2O_2 production, which was found to be dependent on the Galvani potential difference across the water/DCE interface. Further work is required to unravel the kinetic aspects of this mechanism.

Acknowledgements

This work was supported by EPFL, the Swiss Natural Science Foundation (FNRS 200020-116588) and European COST Action (D36/007/06).

References

- [1] H.H. Girault, D.J. Schiffrin, *Electrochemistry of liquid/liquid interfaces*, in: A.J. Bard (Ed.), *Electroanalytical Chemistry*, vol. 15, Marcel Dekker, New York, 1989, pp. 1–48.
- [2] A.G. Volkov, D.W. Deamer, *Liquid/Liquid Interface: Theory and Methods*, Boca Raton FL, CRC Press, 1995.
- [3] H. Ohde, K. Maeda, Y. Yoshida, S. Kihara, *J. Electroanal. Chem.* 483 (2000) 108–116.
- [4] B. Su, R. NiaPartovi, F. Li, M. Hojeij, M. Prudent, Z. Samec, H.H. Girault, *Angew. Chem. Int. Ed.* 47 (2008) 4675–4678.
- [5] A.J. Bard, M.V. Mirkin (Eds.), *Scanning Electrochemical Microscopy*, Marcel Dekker, Inc., New York, 2001.
- [6] S. Kasai, Y. Hirano, N. Motochi, H. Shiku, M. Nishizawa, T. Matsue, *Anal. Chim. Acta* 458 (2002) 263–270.
- [7] Y. Shen, M. Trauble, G. Wittstock, *Anal. Chem.* 80 (2008) 750–759.
- [8] Y.Y. Song, W.Z. Jia, Y. Li, X.H. Xia, Q.J. Wang, J.W. Zhao, Y.D. Yan, *Adv. Funct. Mater.* 17 (2007) 2808–2814.
- [9] B. Su, J.P. Abid, D.J. Fermin, H.H. Girault, H. Hoffmannova, P. Krtil, Z. Samec, *J. Am. Chem. Soc.* 126 (2004) 915–919.
- [10] M.Q. Zhang, P. Sun, Y. Chen, F. Li, Z. Gao, Y.H. Shao, *Anal. Chem.* 75 (2003) 4341–4345.
- [11] T. Wandlowski, V. Marecek, Z. Samec, *Electrochim. Acta* 35 (1990) 1173–1175.
- [12] Z. Ding, B. Quinn, A.J. Bard, *J. Phys. Chem. B* 105 (2001) 6367–6374.
- [13] S.A.G. Evans, J.M. Elliott, L.M. Andrews, P.N. Bartlett, P.J. Doyle, G. Denuault, *Anal. Chem.* 74 (2002) 1322–1326.
- [14] S.B. Hall, E.A. Khudaish, A.L. Hart, *Electrochim. Acta* 43 (1998) 579–588.
- [15] J.F. Zhou, Y.B. Zu, A.L. Bard, *J. Electroanal. Chem.* 491 (2000) 22–29.