

## POSTER PRESENTATION

## Open Access

# The optimization of a rapid low-cost alternative of large-scale medium sterilization

Dominique T Monteil<sup>1</sup>, Cédric A Bürki<sup>2</sup>, Lucia Baldi<sup>1,2</sup>, David L Hacker<sup>1</sup>, Maria de Jesus<sup>2</sup>, Florian M Wurm<sup>1,2\*</sup>*From* 23rd European Society for Animal Cell Technology (ESACT) Meeting: Better Cells for Better Health Lille, France. 23-26 June 2013

## Background

One of the most important unit operations in upstream animal cell bioprocesses at scales over 100 L is the preparation and sterilization of the medium. This complex, sensitive, and expensive process requires a considerable investment in both material and time [1]. Traditionally, large-scale medium sterilization is performed with costly single-use dead-end filters. To optimize and reduce the cost of this unit operation, we investigated the sterilization of mammalian cell culture medium at volumes larger than 100 L.

## Materials and methods

In this study, an optimization of the cost and time for the sterilization of cell culture medium at volumes larger than 100 L was investigated. Pressure-volume diagrams were completed for both a positive displacement pump (Watson-Marlow 620, Cornwall, England) and a bearingless centrifugal pump (Levitronix PuraLev 600 MU, Zurich, Switzerland) to determine optimal pumping speeds and pressures. The study was completed using 0.25" ID tubing with a gate valve downstream of the pump. The pressure (SciLog SciPres, Madison, WI, USA) and flow rate (Equflow flowsensor, Ravenstein, Netherlands) were measured at different closures of the valve. Independently, a range of different size glass microfiber (GF) pre-filters were tested in combination with and without the dead-end filters by measuring the turbidity (TN100, Eutech Instruments, Singapore). A range of different 0.2 µm dead-end membrane filter materials including polyethersulfone (PES), polyvinylidene fluoride (PVDF), and mixed cellulose ester (ME) were tested using a positive displacement pump. In addition,

tangential flow filtration (TFF) was examined with both PES and ME 0.2 µm membranes in comparison to the dead-end filters. A mammalian cell culture medium was filter sterilized at a starting pressure of 500 mbar. The pressure and flow rate were recorded during the filtration until the transmembrane pressure increased to 1200 mbar. The filtration was then stopped at the pressure limit of the tubing connections. Specific filtered medium volume, filter liquid flux rate, and filtrate turbidity were determined for each membrane type.


## Results

The pressure-volume diagram displayed a higher flow rate for the bearingless centrifugal pump (6 to 7 Lpm) in comparison to the peristaltic pump (2.5 Lpm) at the desired pressure of 1000 mbar (data not shown). The turbidity for unfiltered, pre-filtered, and filtered medium was 2.5, 0.75, and 0.2 NTU, respectively, demonstrating the possible benefits of using a pre-filter (data not shown). The filter liquid flux rates ranged from 3 to 25 L/min/m<sup>2</sup> for the range of different filters. The PES hollow fiber TFF filters (Spectrum Labs, Breda, Netherlands) displayed a flux rate of 10 L/min/m<sup>2</sup> (Figure 1B). The specific filtered volume for the dead-end filters was up to 300 L per m<sup>2</sup> of filter surface, while the TFF filter was able to achieve over 1000 L of sterilely filtered medium per m<sup>2</sup> of filter surface (Figure 1A).

## Conclusions

The optimization of pumps for the sterile filtration of mammalian cell culture was completed. Our results indicate that a bearingless centrifugal pump could provide twice the flow rate at the desired filtration pressure in comparison to a peristaltic pump. In addition, the bearingless centrifugal pump was able to provide a constant flow in comparison to the peristaltic pump. Pre-filters were found to clarify the medium and thus could further

\* Correspondence: [florian.wurm@epfl.ch](mailto:florian.wurm@epfl.ch)<sup>1</sup>Laboratory of Cellular Biotechnology, Faculty of Life Sciences, Ecole Polytechnique Fédérale de Lausanne, 1015 Lausanne, Switzerland  
Full list of author information is available at the end of the article

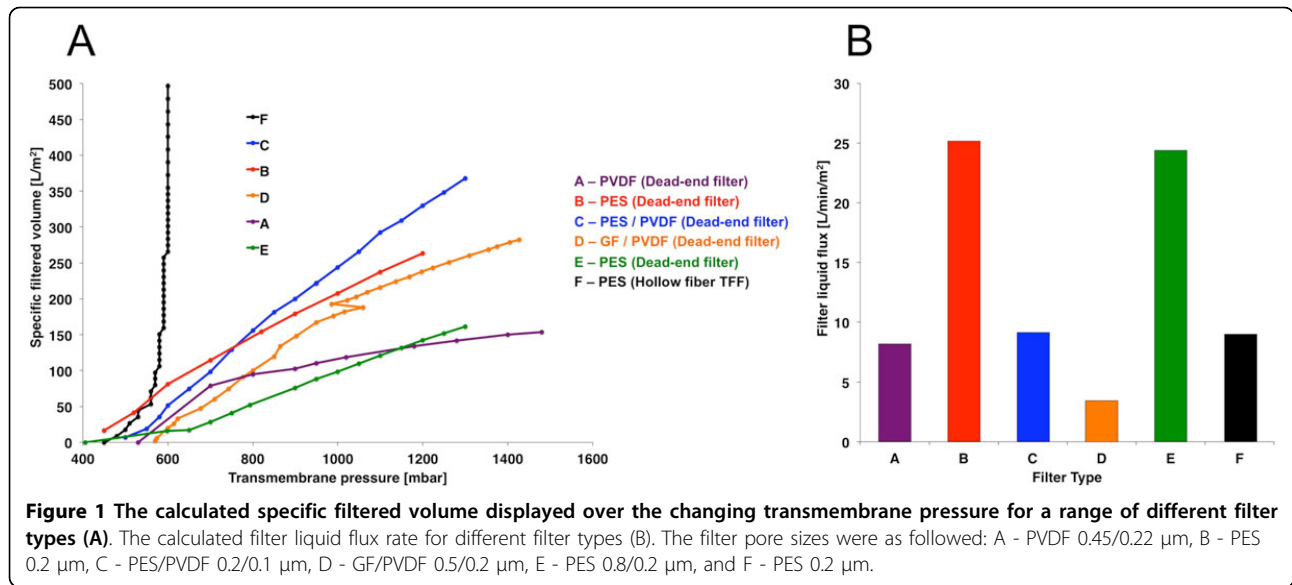

reduce the cost of the filtration. The PES hollow fiber TFF filter was able to filter over three times the sterile medium volume in comparison to the dead-end filters. The TFF filters displayed a similar range of filter liquid flux rates in comparison to the different filters types. This study showed that a hollow fiber TFF coupled with the use of a bearingless centrifugal pump provides a low-cost technology for the rapid large-scale 0.2  $\mu\text{m}$  sterilization of mammalian cell culture medium.

#### Acknowledgements

We gratefully acknowledge Stéphane Itart-Longueville from Spectrum labs and Juerg Burkart from Levitronic GmbH for their considerable support of equipment and material. This work has been supported by the KTI-Program of the Swiss Economic Ministry and by the Swiss National Science Foundation (SNSF).

#### Authors' details

<sup>1</sup>Laboratory of Cellular Biotechnology, Faculty of Life Sciences, Ecole Polytechnique Fédérale de Lausanne, 1015 Lausanne, Switzerland.

<sup>2</sup>ExcellGene SA, 1870 Monthey, Switzerland.

Published: 4 December 2013

#### Reference

1. Zhang X, Stettler M, De Sanctis D, Perrone M, Parolini N, Discacciati M, De Jesus M, Hacker D, Quarteroni A, Wurm F: Use of orbital shaken disposable bioreactors for Mammalian cell cultures from the milliliter-scale to the 1,000-liter scale. *Adv Biochem Eng Biotechnol* 2010, 115:33-53.

doi:10.1186/1753-6561-7-S6-P45

Cite this article as: Monteil et al.: The optimization of a rapid low-cost alternative of large-scale medium sterilization. *BMC Proceedings* 2013 7 (Suppl 6):P45.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at  
www.biomedcentral.com/submit

 BioMed Central