

Easily Constructed Microscale Spectroelectrochemical Cell

published in Spectroscopy Letters, 2010, 43(7/8), 528-533

Paul A. Flowers* and **Jordan C. Strickland[†]**, Chemistry and Physics Department, The University of North Carolina at Pembroke, Pembroke, North Carolina, USA

*corresponding author

[†]undergraduate author

shortened title for running head: **Microscale SEC Cell**

ABSTRACT The design and performance of an easily constructed cell for microscale spectroelectrochemical analysis is described. A cation exchange polymer film, Nafion, was used as a salt bridge to provide ionic contact between a small sample well containing a coiled wire working electrode and separate, larger wells housing reference and auxiliary electrodes. The cell was evaluated using aqueous ferri/ferrocyanide as a test system and shown to be capable of relatively sensitive visible absorption measurements (path lengths on the order of millimeters) and reasonably rapid bulk electrolysis (~ 5 min) of samples in the 1 to 5 μL volume range. Minor alterations to the cell design are cited that could allow for analysis of sub-microliter volumes, rapid multi-sample analysis, and measurements in the ultraviolet spectral region.

KEYWORDS spectroelectrochemistry, microscale analysis, electrochemical cell

INTRODUCTION

Microchemical analysis techniques are beneficial to many applications in which the sample is either inherently small, of limited availability due to scarcity or expense, or hazardous enough to pose problems in personnel exposure and safe disposal. The development of spectral apparatus for microscale measurements has progressed significantly in the recent past, and several vendors presently offer sampling accessories and dedicated instruments for ultraviolet/visible/near infrared analysis of sample volumes as low as $\sim 1 \mu\text{L}$. And though only a few commercially available electrochemical cells can accommodate microscale sample volumes (on the order of a few hundred microliters), there is considerable ongoing research directed towards the development and application of electrochemical cells and sensors, particularly biosensors, that accommodate very small sample volumes.^{1,2}

There have been comparably fewer reports of microscale apparatus permitting simultaneous electrochemical and spectral measurements, so-called spectroelectrochemical (SEC) techniques.³ The most common approach to realizing small cell volumes is by entrapment of sample between two closely spaced, parallel planar surfaces, i.e., the “thin-layer” electrochemical geometry. A variety of optical sampling modes is possible depending upon the identities of the planar substrates, i.e., solid electrodes, optically transparent electrodes (OTE), windows, internal reflection crystals. Cells of this sort have been designed for batch analysis of sample volumes ranging from hundreds^{4,5,6} to tens of microliters.^{7,8,9,10}

Various applications of a versatile SEC sensor design employing film-coated internal reflection OTEs have been described by Heineman et al. in an extensive series of articles published from 1997 to 2007. In one application, the sensor was integrated with a commercially

available electrochemical flow cell to permit visible fluorescence measurements on sample volumes as small as $\sim 4 \mu\text{L}$.¹¹ As the authors note, however, this corresponds to the “sensing volume” of the flow cell, and all the results presented were for operation of the cell in flow-mode. The calibration data reported were for fluorescence measurements made after 45 min of sample flow at $100 \mu\text{L}/\text{min}$, corresponding to a total sample requirement of 4.5 mL. Although this cell could be used in static or “batch” mode with a much lesser volume requirement (but still greater than $4 \mu\text{L}$ due to the dead volume of the cell’s sample introduction plumbing), such use would severely decrease sensitivity due to a greatly diminished preconcentration of analyte into the OTE’s permselective film. Furthermore, if used for absorption measurements, the extremely short path length associated with attenuated total reflectance sampling would likewise result in a very low sensitivity.

Work in our laboratory is concerned with the development of SEC assays for species of biomedical and clinical interest. Towards this goal, we have sought to design a small-volume SEC cell that would permit the rapid analysis of large numbers of samples. Flow injection analysis is a useful approach to these objectives, and we previously developed an SEC flow cell for such purposes.¹² Despite the easy analysis of small volumes via the loop injectors common to flow methods, the unavoidable sample dispersion associated with these methods¹³ serves to decrease sensitivity. In particular for SEC flow cells, the tradeoff between dispersion and electrolysis efficiency¹¹ makes batch analysis the more attractive option from the perspective of sensitivity.

In this paper, an SEC cell for batch analysis of microliter-scale samples is described. Unlike the more common thin-layer designs, this cell employs a small cylindrical cavity and a coaxial coiled wire working electrode to achieve microscale sample volumes, yielding improved

sensitivity due to the much greater optical path length. Additional benefits include the ease of initial construction and assembly/disassembly, and the possibility of modifying the design to accommodate sub-microliter volumes, multiple sample wells, and measurements in the ultraviolet spectral region.

MATERIALS AND METHODS

Reagents. Reagent grade potassium ferricyanide, $K_3Fe(CN)_6$ (13746-66-2) and potassium nitrate, KNO_3 (7757-79-1) were used as received from Fisher Scientific (Pittsburgh, PA, USA). Solutions were typically prepared using distilled / deionized water, stored under refrigeration in tightly capped polyethylene or polycarbonate bottles, and used within a few days of preparation.

SEC Cell Construction. Illustrations of the SEC cell are shown in Figure 1. Base and well plates, approximately 3x7 cm and 3x5 cm, respectively, were cut from polymethylmethacrylate sheet (3 mm thick, United States Plastic Corp., Lima, OH, USA) using a small hacksaw. Holes for the sample well (1.6 mm dia.), reference and auxiliary electrode wells (6.4 mm dia.), and connecting bolt feed-throughs (3.2 mm dia.) were drilled in the well plate using a bench top drill press and standard bits. Matching bolt feed-through holes were drilled in the base plate using the well plate holes as a guide. Ionic contact between the electrode wells was provided by a 1x5 cm sheet of 0.007" thick Nafion 117 perfluorinated membrane (31175-20-9, Sigma-Aldrich, St. Louis, MO, USA). A 1x5 cm gasket was cut from Parafilm M film (Alcan Packaging, Neenah, WI, USA) and hole-punched to match the sample well and electrode reservoirs drilled in the well plate. The volume of the empty sample well after cell assembly was

estimated geometrically to be $\sim 6 \mu\text{L}$ (after insertion of the Pt coil electrode, the well's void volume was $\sim 5 \mu\text{L}$, see below).

A coiled Pt wire working electrode (WE) was fashioned by tightly wrapping 0.25 mm dia. Pt wire (Alfa-Aesar, Ward Hill, MA, USA) around a 1 mm dia. glass capillary tube to yield a coil length of $\sim 3 \text{ mm}$. The capillary tube was then removed, leaving an adequately rigid Pt coil that could be handled without significant deformation. The volume of the Pt coil was estimated to be $\sim 1 \mu\text{L}$. Newly formed electrodes were typically cleaned by heating to incandescence in a butane lighter flame prior to use. A Pt or nichrome wire coil was used as the auxiliary electrode (AE), and a miniature AgCl/Ag electrode prepared from 0.5 mm dia. Ag wire (Alfa-Aesar) according to the procedure reported by Nolan et al.¹⁴ was used as the reference electrode (RE). All potentials are reported relative to this quasireference electrode.

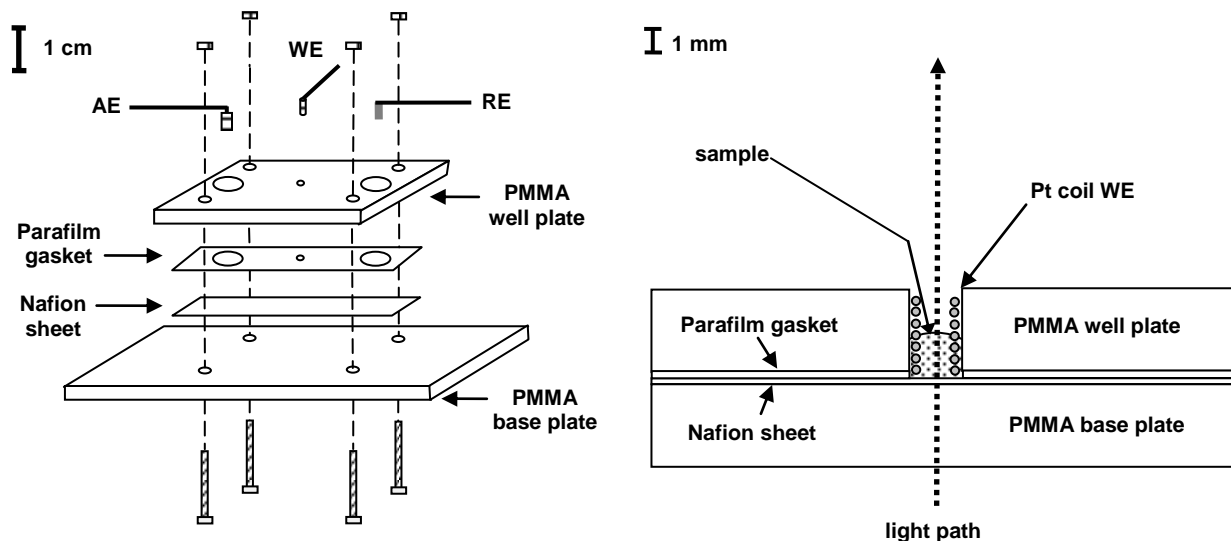


Figure 1. Illustrations of the spectroelectrochemical cell showing an exploded view of the cell assembly (left) and a zoomed cross sectional side view of the sample well region (right).

Prior to assembling the cell, the Nafion sheet was fully hydrated and cation-exchanged to the potassium form by soaking overnight in 1 M KNO₃ (the supporting electrolyte used in all measurements). The cell components were then stacked as shown in Figure 1 and clamped together by tightening the four connecting bolts. Leak-free seals were typically easily achieved as confirmed by monitoring the volume of water added to the well and reservoirs (after capping with Parafilm) over a period of several hours. The assembled cell was stored, with all its wells filled with water, in a sealed container along with a small beaker of water to maintain the Nafion sheet in a fully hydrated state.

Instrumentation. The experimental arrangement is illustrated in Figure 2. A BAS model CV-50W voltammograph (Bioanalytical Systems, Inc., Layfayette, IN, USA) was used for electrochemical control and measurement. Absorbance measurements were made with a model USB2000-FLG CCD spectrometer and model HL450 tungsten-halogen light source (Ocean Optics, Inc., Dunedin, FL, USA). The

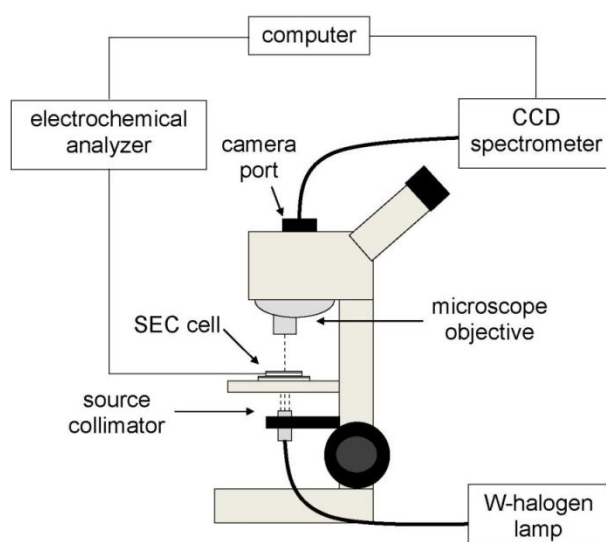


Figure 2. Schematic diagram of the experimental setup depicting the electrical connections (light lines), fiber optic cables (heavy lines), and light path (dashed lines).

output of the light source was directed to the cell via a 0.6 mm single-fiber patch cable terminated with a collimator assembly (Multimode Fiber Optics, Inc., Hackettstown, NJ, USA) and affixed to the condenser mount of a compound, upright optical microscope (Micromaster II series, 12-561-4D, Fisher Scientific). After passing through the SEC cell's sample well as shown in Figure 1, the light was collected by the microscope's objective and directed finally to the spectrometer via another single-fiber patch cable connected to the microscope's camera port via a model C-Mount-MIC adapter (Ocean Optics).

Procedure. The SEC cell was placed on the microscope's X-Y translational stage and secured to its mounting clips with adhesive tape. The reference and auxiliary electrode wells were filled with 1 M KNO₃ using a disposable Pasteur pipet, and all three electrodes were then inserted into their respective wells and secured in place by taping their protruding ends to the top of the well plate. Small squares of Parafilm were used to cover the reference and auxiliary wells in order to minimize solvent evaporation during extended experimentation. A measured volume of sample solution (1 – 5 μ L) was next added to the sample well using a Hamilton model 7105KH zero dead volume 5 μ L syringe (Hamilton Company, Reno, NV, USA). Though any microliter syringe or digital pipet can be used to fill the sample well, a blunt, plunger-in-needle syringe is recommended as it most easily allows the introduction of the small sample volume to the bottom of the well with minimal risk of introducing air bubbles or damaging the surface of the Nafion film. During lengthy experiments, a small square of transparent polyethylene film wrap was used to cover the sample well to slow solvent evaporation and avoid dust contamination. The electrochemical analyzer leads were then connected to the SEC cell electrodes, and microscope stage translation controls were used to align the cell for optimal light throughput. This alignment procedure entailed an initial, rough visual positioning using the

microscope's eyepiece to bring the sample well into the field of view with focus on the top of the Pt coil WE, followed by a fine adjustment of the cell's XY position (in the plane perpendicular to the light beam, via the stage translation controls) and its Z position (along the axis of the light beam, via the microscope focus controls) to maximize signal at the spectrometer. Unless otherwise specified, the microscope's 4X objective was used. The sample was then subjected to the desired electrochemical and/or spectral measurements as detailed in the "Results and Discussion" section. Samples were removed from the well via capillary action using a wick fashioned by tightly twisting a small piece of lint free tissue.

RESULTS AND DISCUSSION

Electrochemistry. Cyclic voltammograms measured at several scan rates, v , for a 3 μL sample of 1 mM potassium ferricyanide in 1 M potassium nitrate measured are shown in Figure 3. The voltammetric peak currents display the expected linear dependence on $v^{1/2}$ ($r > 0.99$) over the examined scan rate range of 1 – 200 mV/s , and the increase in potential difference between the anodic and cathodic peaks with increasing scan rate is moderate, indicating the cell functions essentially in bulk diffusion mode and that the Nafion salt bridge is adequately conductive. Repeating these measurements on the same sample more than an hour after its initial loading showed no significant difference in the voltammograms, indicating that any leakage or other means of sample loss is negligible.

Spectrometry. The cell was used to measure visible spectra of various volumes of aqueous ferricyanide in order to assess its utility as an optical cuvet. In these measurements, a

reference spectrum was first acquired with the cell's sample well containing a volume of electrolyte blank equal to the volume of sample to be used. The alignment procedure described

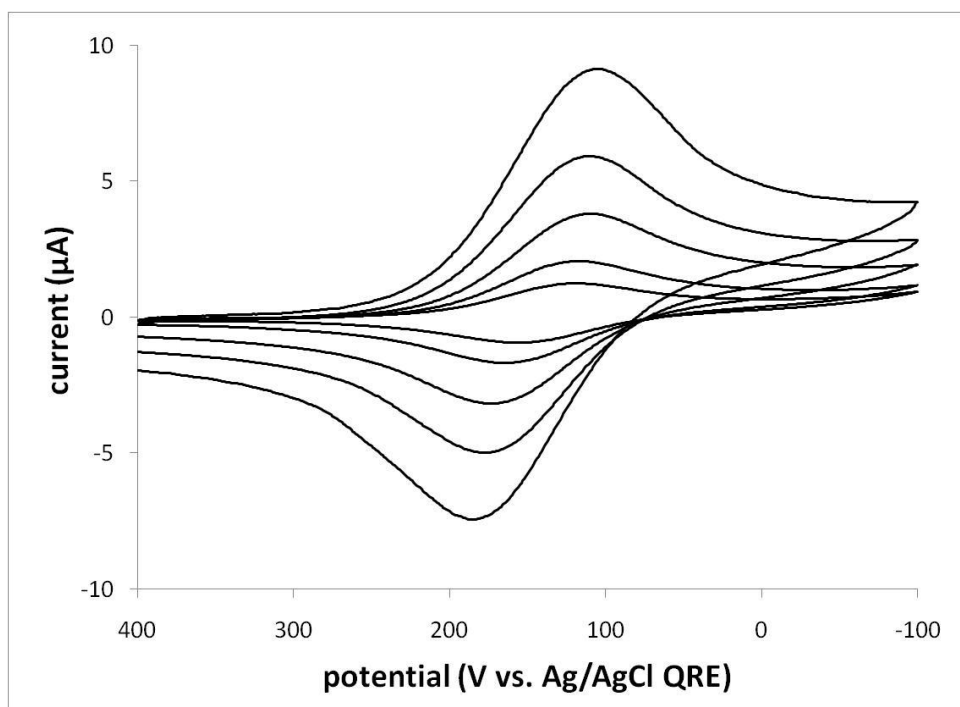


Figure 3. Cyclic voltammograms for 1 mM potassium ferrocyanide in 1 M potassium nitrate measured at scan rates of 1, 2, 5, 10 and 20 mV/s.

in the “Materials and Methods” section was followed for each reference and sample spectrum measured. Spectra were obtained in this fashion for sample volumes of 1, 2, 3, 4 and 5 μL (the effective capacity of the sample well). A plot of peak absorbance for the ferricyanide ion at 420 nm versus sample volume was linear ($r > 0.99$) as expected from Beer’s law and the geometric relation between volume and height (in this case, optical path length) for a cylinder.

Spectroelectrochemistry. The SEC performance of the cell was evaluated by monitoring sample absorbance while performing a double-potential step

chronoabsorptometric experiment. This measurement entails abruptly changing the working electrode potential from a value where one member of a redox couple is predominant to a value where the other member is predominant, the electrode potentials being sufficiently beyond the couple's standard potential, E° , to result in diffusion-limited electrolysis.¹⁵ In this case, the electrode potential was held constant at each value until the sample was exhaustively electrolyzed as evidenced by the attainment of a constant absorbance and a near-zero current. A plot of absorbance at 420 nm versus time for such a measurement using a 3 μ L sample of 1 mM potassium ferricyanide is presented in Figure 4 (see figure caption for experimental details). These data show that electrolysis of the sample is essentially complete in approximately five minutes, a reasonable result

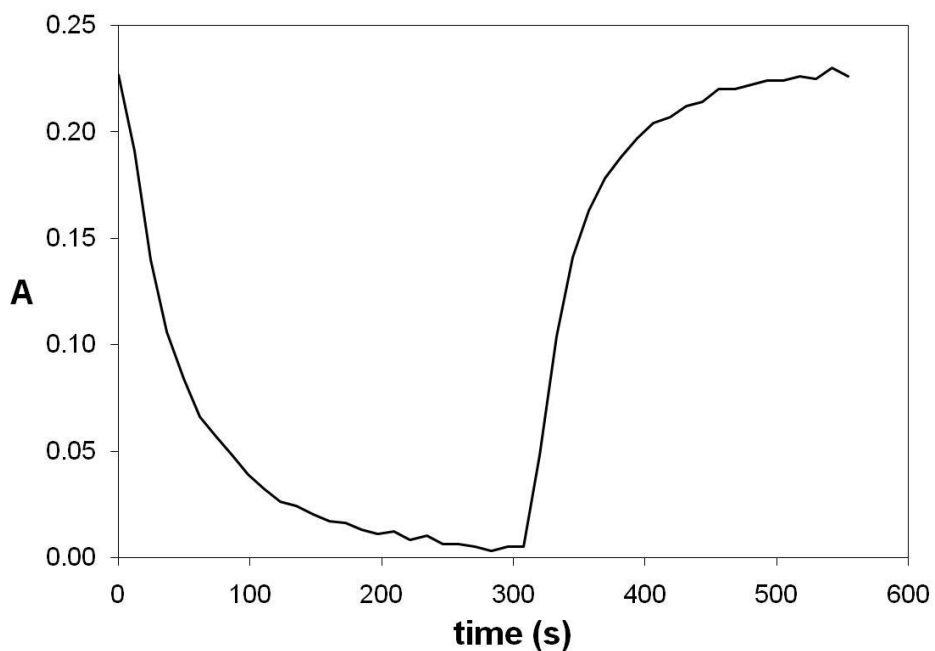


Figure 4. Plot of absorbance at 420 nm versus time for the double-potential step electrolysis of a 3 μ L sample of 1 mM potassium ferrocyanide in 1 M potassium nitrate. WE potential was stepped from 400 mV to -100 mV at $t = 0$ s, and from -100 mV to 400 mV at $t = \sim 300$ s. Reference spectrum measured after exhaustive electrolysis at -100 mV (only ferrocyanide present). Spectra acquired using 47 ms integration, 256 scan average, 19 point smoothing (acquisition time ~ 12 s/spectrum).

considering the diffusion times estimated by the Einstein equation, $t = x^2/2D$, where x is distance and D is diffusion coefficient. Using a value of $7.26 \times 10^{-6} \text{ cm}^2\text{s}^{-1}$ for ferricyanide's diffusion coefficient,¹⁶ and defining d as the diameter of cylindrical volume within the Pt coil electrode ($\sim 0.11 \text{ cm}$), times of ~ 200 and $\sim 400 \text{ s}$ are estimated for species diffusing to the Pt coil's inner wall from the center ($x = d/2$) and the opposite side ($x = d$) of the sample solution.

Full-range visible spectra measured at selected times during the second step of a double-potential step experiment like the one described above are shown in Figure 5. The quality of these spectra is very good, particularly considering the small volume of sample, $3 \mu\text{L}$, and the modest signal acquisition time, 12 s .

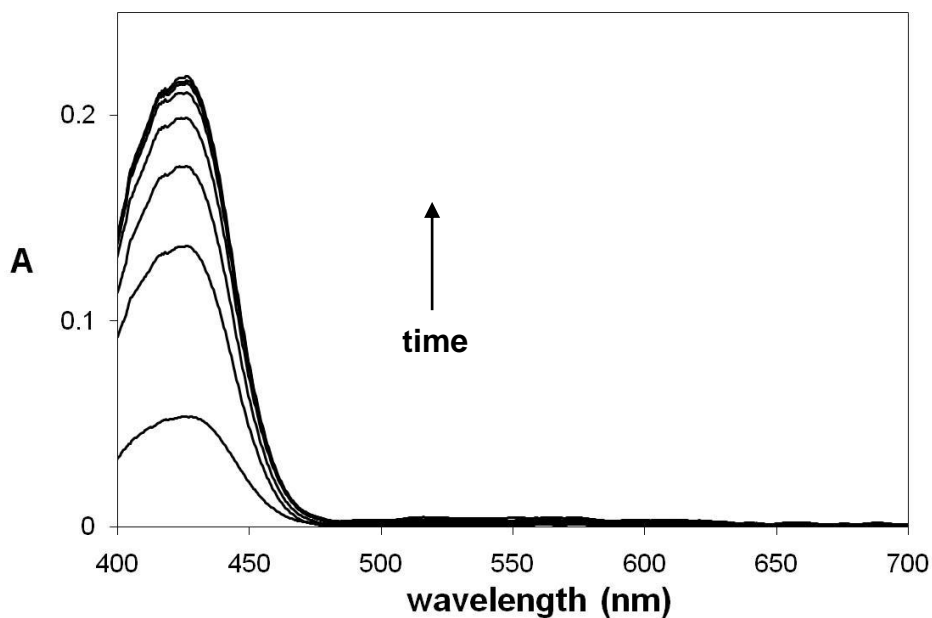


Figure 5. Absorbance spectra measured at various times after the second step (-100 mV to 400 mV) of a double-potential step experiment (conditions as described in Figure 4).

CONCLUSIONS

The cell described in this manuscript has been shown useful for electrochemical, spectral, and SEC measurements on sample volumes in the range of 1 – 5 μL . Several advantages relative to most of the comparable designs previously published have been demonstrated, including

- simple construction, requiring no specialized machine or glass shop services;
- easy assembly/disassembly and sample loading; and,
- greater sensitivity due to longer optical paths (one- or two-orders of magnitude greater than transversely sampled thin-layer cells).

Additionally, some relatively minor alterations to the cell design are envisioned that could expand the scope of its application, for example,

- use of an anion exchange polymer film as the salt bridge to permit the analysis of cationic species;
- incorporation of multiple sample wells in a single device (similar to standard multi-well plates) to increase sample throughput;
- use of smaller diameter sample wells to accommodate sub-microliter sample volumes (with accompanying decreases in bulk electrolysis times); and,
- addition of a matched hole in the base plate beneath the sample well to avoid ultraviolet absorption by the PMMA and thus allow measurements in this spectral region (or, alternatively, use of an ultraviolet-transparent base plate material).

ACKNOWLEDGMENTS

Support of this research by the UNCP RISE Program, funded by the National Institutes of Health, and the UNCP Chemistry & Physics Department is gratefully acknowledged. The authors also acknowledge technical assistance provided by Cilia M. Iluku and Josie R. Torrence.

REFERENCES

-
1. Privett, B.J.; Shin, J.H.; Schoenfish, M.H. *Electrochemical Sensors*, *Anal. Chem.*, **2008**, *80*, 4499-4517.
 2. Zhang, X.; Ju, H.; Wang, J. (Eds.) *Electrochemical Sensors, Biosensors and Their Biomedical Applications*, Elsevier Science: St. Louis, MO, USA, 2007.
 3. Zoski, C.G. *Handbook of Electrochemistry*, Elsevier Science: St. Louis, MO, USA, 2007; Chapter 14.
 4. Hawkrige, F.M.; Pemberton, J.E.; Blount, H.N. Small Volume, High Performance Cell for Nonaqueous Spectroelectrochemistry. *Anal. Chem.* **1977**, *49*, 1646-1647.
 5. Anderson, J.L. Circulating, Long-Optical-Path, Thin-Layer Electrochemical Cell for Spectroelectrochemical Characterization of Redox Enzymes. *Anal. Chem.* **1979**, *51*, 2312-2315.
 6. Rubinson, K.A.; Mark, H.B. Jr. Long-Path, Small Volume Spectroelectrochemistry Cell. *Anal. Chem.* **1982**, *54*, 1204-1206.
 7. Porter, M.D.; Dong, S.; Gui, Y.-P.; Kuwana, T. Spectroelectrochemical Cell with Adjustable Solution Layer Thickness. *Anal. Chem.* **1984**, *56*, 2263-2265.
 8. Luo, H.; Weaver, M.J. A Versatile Surface Raman Spectroelectrochemical Flow Cell: Applications to Chemisorbate Kinetics. *Electroanal. Chem.* **2001**, *501*, 141-150.
 9. Ren, B.; Lin, X.; Jiang, Y.; Cao, P.; Xie, Y.; Huang, Q.; Tian, Z. Optimizing Detection Sensitivity on Surface-Enhanced Raman Scattering of Transition Metal Electrodes With Confocal Raman Microscopy. *Appl. Spectrosc.* **2003**, *57*, 419-427.

-
10. Bonifacio, A.; Millo, D.; Gooijer, C.; Boegschoten, R.; van der Zwan, G. Linearly Moving Low-Volume Spectroelectrochemical Cell for Microliter-Scale Surface-Enhanced Resonance Raman Spectroscopy of Heme Proteins, *Anal. Chem.* **2004**, *76*, 1529-1531.
 11. Kaval, N.; Seliskar, C.J.; Heineman, W.R. Spectroelectrochemical Sensing Based on Multimode Selectivity Simultaneously Achievable in a Single Device. 16. Sensing by Fluorescence. *Anal. Chem.* **2003**, *75*, 6334-6340.
 12. Flowers, P.A.; Maynor, M.A. Easily Constructed Spectroelectrochemical Cell for Batch and Flow Injection Analyses. *Anal. Chem.* **2002**, *74*, 720-723.
 13. Cazes, J.; Ewing, G.W. (Eds.) *Ewing's Analytical Instrumentation Handbook*, 3rd ed., CRC Press: Boca Raton, FL, USA: 2005; p 24.
 14. Nolan, M.; Tan, S.; Kounaves, S. Fabrication and Characterization of a Solid State Reference Electrode for Electroanalysis of Natural Waters with Ultramicroelectrodes. *Anal. Chem.* **1997**, *69*, 1244-1247.
 15. Zoski, C.G. *Handbook of Electrochemistry*, Elsevier Science: St. Louis, MO, USA, 2007; p 600.
 16. Konopka, S. J.; McDuffie, B. Diffusion Coefficient of Ferri- and Ferrocyanide Ions in Aqueous Media, Using Twin-Electrode Thin-Layer Electrochemistry. *Anal. Chem.* **1970**, *42*, 1741-1746.