



**UNIVERSITI PUTRA MALAYSIA**

**DEVELOPMENT OF ELECTROCHEMICAL BIOSENSOR SYSTEMS  
FOR CHLORPYRIFOS PESTICIDE DETECTION**

**ABDU IDRIS OMER**

**FK 2002 78**

**DEVELOPMENT OF ELECTROCHEMICAL BIOSENSOR SYSTEMS FOR  
CHLORPYRIFOS PESTICIDE DETECTION**

**By**

**ABDU IDRIS OMER**

**Thesis Submitted to the School of Graduate Studies, Universiti Putra Malaysia,  
in Fulfilment of the Requirements for the Degree of Doctor of Philosophy**

**April 2002**



Abstract of thesis presented to the senate of Universiti Putra Malaysia in fulfilment  
of the requirements for the degree of Doctor of Philosophy

**DEVELOPMENT OF ELECTROCHEMICAL BIOSENSOR SYSTEMS FOR  
CHLORPYRIFOS PESTICIDE DETECTION**

By

**ABDU IDRIS OMER**

**APRIL 2002**

**Chairman: Bambang Sunaryo Suparjo, Ph.D.**

**Faculty : Engineering**

Environmental monitoring systems are of great interest and highly significant in our life since every day we are exposed to many and various dangerous and fatal contaminants. Organophosphate pesticides such as Chlorpyrifos are widely used in agriculture to eliminate plant destroying pests. However, these pesticides may affect the environmental equilibrium unless continuous monitoring on their presence in water, soil, and agricultural products is carried out to protect human health and other living organisms.

One of the approaches that can be adopted is to develop an on-line monitoring system. The widely used electronic and computer technology can simplify the development process of acquiring and monitoring system. In addition, the invention of biosensors to detect biologically-based materials such as Chlorpyrifos pesticide in the agricultural sector, glucose level in blood, heavy elements in the drinking water etc., have attracted interest.

This research is divided into two parts: development of computer-based instrument and development of biosensor. Both systems are integrated to form a real monitoring device for the detection of Chlorpyrifos pesticide concentration. In the development of computer-based instrument, a serial interfacing board that can be linked to the computer to acquire data from the various developed biosensors was developed. The developed board includes signal conditioning, analog-to-digital (A/D) and universal asynchronous receiver and transmitter (UART) circuits. Visual Designer software was used to control the data flow process and at the same time displaying the biosensor responses in real time, and the data can be stored in hard disk.

For the biosensor development, two amperometric based biosensor electrodes and capacitance-based biosensor were developed. In the amperometric based biosensor electrodes, two different patterns and substrate electrodes (copper and gold) were developed. Both structures can produce similar responses where the electrical signal (in this case voltage) variation is proportional to the pesticide concentration. Also, they can be linked to the computer via the PC-based serial interfacing board. For the capacitance-based biosensor, detection of Chlorpyrifos pesticide was carried out by monitoring the variation of dielectric (mixed pesticide and antibody) between two parallel plates. An oscillator circuit was used to detect the response by measuring the generated signal frequency. It has been shown that the measured frequency is inversely proportional to the pesticide concentration. Therefore, from the results, the developed biosensors are able to detect the presence of the pesticide. Also, the evaluation and comparison between the results of these systems show that the capacitance-based biosensor is the most effective structure. The construction of that structure is relatively simple.

Analysis of previously developed biosensors has been carried out as references. They are a pH glass electrode and a fibre optical biosensor.

The remarkable significant findings and contribution of the author in this research. can be represented in the design of a potentiostat electronic circuit that provides a bias voltage to the electrode systems inserted in a sample of the Chlorpyrifos pesticide. This generates an electrochemical reaction where an electric current proportional to the concentration of the Chlorpyrifos pesticide sample is provided, Secondly, the design of capacitance-based biosensor that relates frequency readings with Chlorpyrifos pesticide concentrations. Finally, the integration of both the various biosensor systems and the PC-based serial board where a real data acquisition system was established to detect the Chlorpyrifos pesticide

Abstrak tesis yang dikemukakan kepada Senat Universiti Putra Malaysia sebagai memenuhi keperluan untuk ijazah Doktor Falsafah

**PEMBANGUNAN SISTEM BERASASKAN BIOSENSOR UNTUK  
PENGESANAN PESTISID CHLORPYRIFOS**

**Oleh**

**ABDU IDRIS OMER**

**APRIL 2002**

**Pengerusi: Bambang Sunaryo Suparjo, Ph.D.**

**Fakulti : Kejuruteraan**

Pestisid organofosfat seperti chlorpyrifos digunakan secara meluas dalam sektor pertanian untuk menghapuskan perosak tanaman. Namun pestisid ini boleh menyebabkan ketidakseimbangan persekitaran kecuali jika pemantauan berterusan dibuat bagi memastikan kandungan pestisid di dalam air, tanah dan penghasilan pertanian tidak memudaratkan manusia dan kehidupan lain. Satu cara yang boleh digunakan ialah dengan membangunkan sistem pemantauan. Sistem pengawasan persekitaran adalah sangat penting dan berkait rapat dengan kehidupan kita yang sentiasa terdedah kepada berbagai bahan cemar dan berbahaya.

Penggunaan teknologi komputer dan elektronik dapat membantu memudahkan proses pemantauan. Tambahan pula, rekaan biosensor untuk mengesan bahan berasaskan biologiikal seperti pestisid chlorpyrifos dalam sektor pertanian, kandungan glukosa dalam darah, bahan kimia dalam air minuman dan seumpamanya amat menarik minat. Penyelidikan ini dibahagikan kepada dua bahagian: pembangunan instrumentasi berasaskan komputer dan pembangunan struktur biosensor khusus untuk mengesan pestisid chlorpyrifos.

Dalam pembangunan instrumentasi berasaskan komputer, litar antaramuka yang boleh disambungkan kepada komputer untuk mendapatkan data dari berbagai jenis biosensor telah dibangunkan. Litar yang dibangunkan termasuk keadaan isyarat, penukar analog kepada digital dan litar penerima dan penghantar. Perisian “Visual Designer” telah digunakan untuk mengawal pengaliran data dan pada masa yang sama mempamerkan isyarat biosensor yang diperolehi. Data yang diperolehi boleh juga disimpan dalam cakera keras. Bagi struktur biosensor, elektrod biosensor amperometrik dan biosensor berasaskan kapasitan telah dibangunkan. Dalam biosensor elektrod amperometrik, dua jenis corak dan substrat elektrod (kuprum dan emas) berbeza telah dibangunkan. Kedua-dua struktur boleh menghasilkan tindakbalas yang hampir sama di mana perbezaan isyarat elektrik (voltan) adalah berkadaran dengan kandungan pestisid. Ia juga boleh disambungkan kepada komputer melalui kad antara muka. Bagi biosensor berasaskan kapasitans pengesanan pestisid chlorpyrifos telah dijalankan dengan memerhatikan perbezaan nilai dwielektrik (campuran pestisid dan antibodi) antara dua plat selari. Litar pengayun digunakan untuk mengesan tindakbalas dengan mengukur isyarat frekuensi yang dihasilkan. Didapati isyarat frekuensi adalah berkadar songsang dengan kandungan pestisid. Oleh itu, dari keputusan yang diperolehi, biosensor yang telah direka boleh mengesan kehadiran pestisid. Dari keputusan yang diperolehi, didapati biosensor berasaskan kapasitans adalah struktur lebih efektif dan pembinaannya adalah sangat mudah. Analisis biosensor terdahulu telah dijadikan sebagai rujukan. Ia adalah elektrod kaca pH dan biosensor optik fibre. Akhir kata, instrumentasi berasaskan komputer dan biosensor telah digabungkan untuk membentuk sistem pemantauan secara langsung. Isyarat biosensor didapati boleh dipaparkan pada skrin

komputer menandakan litar antaramuka dan perisian kawalan telah berjaya  
dibangunkan.



## ACKNOWLEDGEMENTS

I would like to thank the chairman of my supervisory committee Dr. Bambang Sunaryo Suparjo for the unlimited assistance and great effort he exerted to complete this study. A special thank to Dr. Abd Rahman Ramli for his unlimited valuable comments and recommendations. I was also indebted to Dr. Zamri Ishak the co-supervisor head of the program who helped me technically and financially. The fruitful advice he shared yielded a good environment that resulted in a high confidence to go a head in pursuing the study. My thanks and appreciation are extended to Mr. Massnizar Mustapha and Miss Noorshina Hussin for their valuable technical assistance who have helped me in preparing most of the bioreceptors and chemical compounds and other relevant things which have been used throughout the experiments.

I certify that an Examination Committee met on 8<sup>th</sup> April 2002 to conduct the final examination of Abdu Idris Omer on his Doctor of Philosophy thesis entitled "Development of Electrochemical Biosensor Systems for Chlorpyrifos Pesticide Detection" in accordance with Universiti Pertanian Malaysia (Higher Degree) Act 1980 and Universiti Pertanian Malaysia (Higher degree) Regulations 1981. The committee recommends that the candidate be awarded the relevant degree. Members of the Examination Committee are as follows:

**NORMAN MARIUN, Ph.D.**

Faculty of Engineering  
Universiti Putra Malaysia  
(Chairman)

**Bambang Sunaryo Suparjo, Ph.D.**

Faculty of Engineering  
Universiti Putra Malaysia  
(Member)

**ABDUL RAHMAN RAMLI, Ph.D.**

Faculty of Engineering  
Universiti Putra Malaysia  
(Member)

**ZAMRI BIN ISHAK, Ph.D.**

Biodiagnostic and Biosafety Program,  
Biotechnology Research Center, MARDI.  
(Member)

**BURHANUDDIN YEOP MAJLIS, Ph.D.**

Professor  
Faculty of Engineering  
Universiti Kebangsaan Malaysia  
(Independent Examiner)

  
**SHAMSHER MOHAMAD RAMADILI, Ph.D.**

Professor/Deputy Dean  
School of Graduate Studies  
Universiti Putra Malaysia

Date: 10 JUN 2002

The thesis submitted to the Senate of Universiti Putra Malaysia has been accepted as fulfillment of the requirement for the degree of Doctor of Philosophy.



---

**AINI IDERIS, Ph.D.**  
Professor/Dean  
School of Graduate Studies  
Universiti Putra Malaysia

Date 08 AUG 2002

## DECLARATION FORM

I hereby declare that the thesis is based on my original work except for quotations and citations which, have been acknowledged. I also declare that it has not been previously or currently submitted for any other degree at UPM or other institutions.



**ABDU IDRIS OMER**

Date: 10/6/2002

## TABLE OF CONTENTS

	<b>Page</b>
ABSTRACT	ii
ABSTRAK	v
ACKNOWLEDGMENTS	viii
APPROVAL	x
DECLARATION	xi
LIST OF TABLES	xvi
LIST OF FIGURES	xvii
LIST OF ABBREVIATIONS/NOTATIONS/GLOSSARY OF TERMS	xxi
<b>CHAPTER</b>	
1 INTRODUCTION	1
1.1 Overview of the Environment Monitoring Approaches	1
1.2 Organophosphate Pesticides	2
1.3 Definition of Electrochemical Biosensors	3
1.4 Problem Statement and Project Aims	4
1.5 Benefits and Significance Findings	6
1.6 Limitations of the Detecting systems	7
1.7 Computer-Based Instrument	8
1.8 Amperometric Biosensors	9
1.9 Potentiometric Biosensors	10
1.10 Optical Biosensor	11
1.11 Conductance Measurements	12
1.12 Thesis Organisation	12
2 LITERATURE REVIEW	14
2.1 Methods of Analysis Based on Biosensors for Environmental Monitoring	14
2.2 The History of Biosensors	16
2.3 Biosensors Technology	18
2.3.1 Bioreceptor Molecules	18
2.3.2 Electrodes Types and Configurations	20
2.3.3 Recognition and Transduction Methods of Biosensors	23
2.3.4 Biocatalysis-Based Biosensors	24
2.3.5 Bioaffinity-Based Biosensors	27
2.3.6 Microorganism-Based Biosensors	30
2.3.7 Choice of Bioreceptor and Immobilization Techniques	32
2.4 Signal Transduction Techniques	34
2.4.1 Potentiometric Transducers	34
2.4.2 Amperometric Transducers	36
2.4.3 Optical Measurements	39
2.4.4 Conductance Measurements	41

2.5	Biosensors for Environmental Monitoring	41
2.6	PC-based Measurement and Control Systems	44
	2.6.1 Data Acquisition Systems Developments	46
	2.6.2 Real Time Analysis vs. Post-processing	48
2.7	Future Trends of Electrochemical Biosensors for Environmental Monitoring	50
3	AMPEROMETRIC BIOSENSORS (THEORY OF OPERATION)	52
3.1	Overview	52
3.2	Electrochemical Terms and Concepts	52
	3.2.1 Oxidation reaction	52
	3.2.2 Reduction Reaction	54
	3.2.3 Redox Reaction	54
3.3	The measured parameter in the amperometric biosensor	55
3.4	Electrode Set Up and Current Generated	55
	3.4.1 Working Electrode	56
	3.4.2 Reference Electrode	57
3.5	The Faradaic and Nonfaradaic Currents	58
	3.5.1 Faradaic Currents and Diffusion Controlled Reactions	60
3.6	Electrode Configurations	63
	3.6.1 Two Electrode Configuration	64
	3.6.2 Three Electrode Configuration	66
3.7	Equations Governing the Electrode Reactions	69
3.8	Faradaic Vs and Applied Potential Curves ( $i-V$ )	72
	3.8.1 The Cottrell Equation	73
3.9	Examples of Modern Microelectrodes	75
3.10	Conclusion	76
4	DEVELOPMENT OF COMPUTER-BASED INSTRUMENTS	77
4.1	Development of Controlling and Monitoring Software Using Visual Designer	77
	4.1.1 Visual Designer Blocks	80
4.2	Development of PC-Based Serial Interfacing Boards	84
	4.2.1 Overview	84
	4.2.2 Principles of Data Acquisition System	86
	4.2.3 PC-Based Serial Communications	86
	4.2.4 Analogue Signal Conditioning	88
	4.2.5 Digital Signal Processing	92
	4.2.6 Circuit Diagram Description	94
	4.2.7 Printed Circuit Board PCB	95
	4.2.8 Flow Chart of the System	100
	4.2.9 Sequence vs. Software Selectable Ranges	101
	4.2.10 Channel Activation Process of an Input Device	103
4.3	Conclusion	108
5	DEVELOPMENT OF AMPEROMETRIC BIOSENSOR-BASED ELECTRODES AND CAPACITANCE BASED BIOSENSOR	110
5.1	Overview of the Amperometric Biosensor Based Electrodes	110
5.2	Development of the Amperometric Biosensor Based Electrodes	111

5.2.1	Development of Copper Electrode	111
5.2.2	Development of Gold Electrode	114
5.3	Capacitance Based Biosensor	118
5.3.1	Overview	118
5.3.2	Development of Capacitance Based Biosensor	118
5.4	Conclusion	123
6	EXPERIMENTAL RESULTS AND DISCUSSION	124
6.1	Introduction	124
6.2	Detection of Chlorpyrifos Pesticide Using Amperometric Biosensor	125
6.2.1	Amperometric Biosensor Principles	125
6.2.2	Electrical Current Vs. Species Concentration	126
6.2.3	Faradaic Current	126
6.2.4	Electrode Configurations	127
6.2.5	Measurement Technique of Pesticide Concentration	127
6.2.6	Setting up the Amperometric Biosensor System	129
6.2.7	Calibration of the Measurement System	129
6.2.8	PC-Based Interfacing Board and a Digital Meter in Monitoring Pesticide Concentration	133
6.2.9	Analysis Based on Calibration	137
6.2.10	Detecting Chlorpyrifos Pesticide Using Copper Electrodes	138
6.2.11	Detecting Chlorpyrifos Pesticide Based on the Activation of Immobilised Enzyme on Gold Working Electrode	139
6.2.12	Performance of Copper and Gold Electrode in Detecting Chlorpyrifos Pesticide	142
6.3	Detecting Chlorpyrifos Pesticide Using Capacitance-Based Biosensor	144
6.3.1	Theory	144
6.3.2	Preparation of the Rabbit Antibody Dilutions	147
6.3.3	Preparation of the Pesticide Concentration	147
6.3.4	Results	148
6.3.5	Conclusion	154
6.4	Detection of Organochlorine Pesticide Using Capacitance Based-Biosensor	155
6.4.1	Overview	155
6.4.2	Results and Discussion	157
6.4.3	Conclusion	160
6.5	Detection of Chlorpyrifos Pesticide Using pH glass Electrode	160
6.5.1	Chemicals Required for Detecting the Chlorpyrifos Pesticide	161
6.5.2	Results and Discussion	163
6.5.3	Conclusion	165
6.6	Detection of Chlorpyrifos Pesticide Using Fibre Optical Biosensor	165
6.6.1	Background of the Fibre Optical Biosensor	166
6.6.2	Objective of the Fibre Optical Biosensor	167
6.6.3	Operation of Fibre Optical	168

6.6.4 Testing of Fibre Optical Biosensor	169
6.6.5 AchE Enzyme to Detect Chlorpyrifos Pesticide	170
6.6.6 Results and Discussion	170
6.7 Conclusion	175
7 CONCLUSION	177
7.1 Conclusion and Comments Based on the Experimental Results	178
7.2 Computer Based Instruments	179
7.3 Amperometric and Capacitance Biosensors Limitations	180
7.4 Optical Fibre Biosensor Limitations	181
7.5 Serial Interfacing Technique Advantages	181
7.6 Computer Based Instruments Limitations	182
7.7 Suggestions for Future Development and Applications	183
REFERENCES/BIBLIOGRAPHY	184
APPENDICES	194
BIODATA OF THE AUTHOR	231



## LIST OF TABLES

<b>Table</b>	<b>Page</b>
4.1 TTL (Transistor -Transistor logic) and RS logic data	95
6.1 Frequency response vs. parallel plate gap distances	154
A.1 D Type 9 Pin and D Type 25 Pin Connectors	194
A.2 The pin functions of the serial port	195
A.3 Port Addresses & IRQ's	199
A.4 COM Port Addresses in the BIOS Data Area	199
A.5 Pin Description for CDP6402, AY-5-1015 / D36402R-9 and compatible UART's	200
A.6 Possible Baud Rates using a 74HC4060	202
E.1 DC signal captured by digital meter and PC based board	225
E.2a Pesticide concentration measurement using PC and digital meter	225
E.2b Pesticide concentration measurement using PC and digital meter	226
E.2c Pesticide concentration measurement using PC and digital meter	226
E.3 Frequency readings by maintaining the pesticide concentration at 0.01 ppm added to five antibody dilutions separately	226
E.4 Frequency readings by maintaining the pesticide concentration at 0.1 ppm added to five antibody dilutions separately	227
E.5 Frequency readings by maintaining the pesticide concentration at 1.0 ppm added to five antibody dilutions separately	227
E.6 Frequency readings by maintaining the pesticide concentration at 10.0 ppm added to five antibody dilutions separately	227
E.7 Frequency readings by maintaining the antibody dilution at 200x added to four pesticide concentrations separately	227
E.8 Frequency readings by maintaining the antibody dilution at 400x added to four pesticide concentrations separately	228
E.9 Frequency readings by maintaining the antibody dilution at 800x added to four pesticide concentrations separately	228
E.10 Frequency readings by maintaining the antibody dilution at 1600x added to four pesticide concentrations separately	228
E.11 Frequency readings by maintaining the antibody dilution at 3200x added to four pesticide concentrations separately	228
E.12 Interaction of Chlorpyrifos (pesticide) with the enzyme membrane on pH electrode	229
E.13 Results based on the pH electrode without attachment to membrane	229
E.14 Results based on the pH electrode attach to membrane	229
E.15 pH values Vs pesticide concentrations with and without membrane attached to the electrode	229

## LIST OF FIGURES

<b>Figure</b>	<b>Page</b>
1.1 Basic Operation of the Biosensor Principle	3
1.2 Coupling enzymes and electrode reactions	4
1.3 Linking an amperometric biosensor, optical biosensor and pH electrode to the PC via the PC based interfacing board. Based on the Visual Designer software, each system can be selected and monitored independently	7
1.4 Amperometric biosensor principle	10
1.5 Amperometric biosensor for phenolic compounds detection	10
1.6 Principles of Potentiometric Biosensor	11
3.1 Electrical circuit representing current flow through an electrochemical cell	59
3.2 Different processes affecting electrode reaction rates	61
3.3 Two-electrode cell	65
3.4 Two-electrode equivalent circuit, showing potential changes at the reference and working electrodes	65
3.5 Three-electrode cell	67
3.6 Three-electrode equivalent circuit	68
3.7 Nerve regeneration electrodes	75
3.8 Arrays of sensors: 200 nm gold ring electrodes on a silicon substrate	76
4.1 Flow chart of simulation process based on Visual Designer software	78
4.2 Real data acquiring process using Visual Designer Software	80
4.3 Setting Run Controller parameters of the Visual Designer Software	83
4.4 Control and output section of the Visual Designer used to select and activate the particular hardware input channel	83
4.5 Visual Designer software blocks of the input section of the data acquiring process	84
4.6 TTL/CMOS Serial Logic Waveform	87
4.7 The potentiostat circuit	91
4.8 Circuit of ADC0804 Analogue to Digital Converter	93
4.9 Block diagram of the PC-based serial interfacing board	95
4.10 Silkscreen Overlay layer of the Printed Circuit board (PCB)	99
4.11 Operating the Drill Machine as the final stage of PCB design	99
4.12 Flow chart of the PC based interfacing board	101
4.13 Processes of current to voltage converter and PC based gain factor selection	102
4.14 Process of activating an input device based on the PC	106
4.15 Linking PC-based interfacing board to Digital multimeter and Oscilloscope for testing	107
4.16 PCB Testing using digital multimeter and an oscilloscope	107

5.1	Flow chart of the Amperometric based biosensor electrode development	112
5.2	Steps of designing copper electrodes	114
5.3	Steps of designing gold electrode	116
5.4	Investigating the electrodes for connectivity	117
5.5	Photograph of designed Copper and gold electrodes with the external connectors ready for use	117
5.6	Flow chart of capacitance based biosensor system development	120
5.7	Three capacitance-based biosensor electrodes with identical dimension	121
5.8	Block diagram of the 555 timer to provide the functions of control, triggering, level sensing or comparison, discharge, and power output	122
5.9	Pulse generator built around the 555 timer. The parallel copper plate is connected in series with the known capacitance C1	123
6.1	Electrochemical cell	126
6.2	Faradaic current vs. species concentration	127
6.3	Setting up the amperometric biosensor	129
6.4	Calibrating process to the PC-based serial board	131
6.5	DC signal source connected to digital meter and to PC based interfacing board in a way to show the deviation between the two readings	131
6.6	Data Analysis Software Screen Output of sinusoidal signal by a direct connection the PC based interfacing board to the signal generator that provides the signal	132
6.7	Data analysis software screen output: On-line response by dipping gold electrode into distilled and adding tap water	133
6.8a	Typical responses of pesticide concentration using PC and a digital meter. (Table E.2a)	134
6.8b	Typical responses of pesticide concentration using PC and a digital meter. (Table E.2b)	134
6.8c	Typical responses of pesticide concentration using PC and a digital meter. (Table E.2c)	135
6.9a	Visual Designer screen of pesticide concentration measurement on line	135
6.9b	Visual Designer screen of pesticide concentration measurement on line	136
6.9c	Visual Designer screen of pesticide concentration measurement on line	136
6.10	Pico technology software output screen	137
6.11	Chloropyrifos pesticide Detection using copper electrode	139
6.12	Data analysis software screen output: current and voltage plots by applying $-0.6$ Voltage to gold electrode	141
6.13	Typical voltage responses of an immobilized AchE enzyme on gold electrode and non-immobilized when variable voltages are applied	142
6.14	Thevenin equivalent of a discrete circuit	146
6.15	Frequency readings by maintaining the pesticide concentration at 0.01 ppm (Table E.3)	149

6.16	Frequency readings by maintaining the pesticide concentration at 0.1 ppm (Table E.4)	150
6.17	Frequency readings by maintaining the pesticide concentration at 1.0 ppm (Table E.5)	150
6.18	Frequency readings by maintaining the pesticide concentration at 10.0 ppm (Table E.6)	151
6.19	Frequency readings by maintaining the antibody dilution at 200x (Table E.7)	152
6.20	Frequency readings by maintaining the antibody dilution at 400x (Table E.8)	152
6.21	Frequency readings by maintaining the antibody dilution at 800x (Table E.9)	153
6.22	Frequency readings by maintaining the antibody dilution at 1600x (Table E.10)	153
6.23	Frequency readings by maintaining the antibody dilution at 3200x (Table E.11)	154
6.24	Maintaining the antibody at 200x dilution and varying the organochlorine pesticide concentrations	158
6.25	Maintaining the antibody at 400x dilution and varying the organochlorine pesticide concentrations	158
6.26	Maintaining the antibody at 800x dilution and varying the organochlorine pesticide concentrations	159
6.27	Maintaining the antibody at 1600x dilution and varying the organochlorine pesticide concentrations	159
6.28	The experiment set up to connect the Expandable ion Analyzer EA940 to the PC	162
6.29	Plotting pesticide concentrations vs voltage reading with and without membrane	164
6.30	Plotting pesticide concentrations vs pH values with and without membrane	165
6.31	Relative spectral response	167
6.32	The block diagram of fibre optic biosensor system	168
6.33	Subjecting the optical sensor to different coloured papers for testing	169
6.34	optical fiber probe dipped into a sample of Chlorpyrifos Pesticide	171
6.35	Chlorpyrifos pesticide samples to be detected using optical fibre biosensor	172
6.36	optical fibre probe is dipped into a bottle containing a sample of the Chlorpyrifos pesticide	172
6.37a	Standard inhibition curve of AchE by Dynatech plate reader	174
6.37b	Standard inhibition curve of AchE by fibre optic biosensor	174
6.38	Linking the fibre optical biosensor to panel meter	175
A.1	pinout of MAX 232	196
A.2	RS-232 Logic Waveform	197

A.3	External connection of the MAX232	198
A.4	Pin out of the CDP6402 (UART)	200
A.5	Layout of 74HC4060 Binary Counter	202
A.6	Figure A.7: Data shifting process	203
A.7	Complete design of single channel PC based interfacing board	204
A.8	Complete design of 8-channels PC based interfacing board	205
B.1	A transducer that provides a single voltage output	206
B.2	The inputs to amplifier stages can also be modeled as Thevanin-equivalent circuits	207
B.3	The differential output temperature sensing bridge	208
B.4	Remote sensing to avoid offset errors	209
B.5	An isolator allows communication of signal values between two circuits with no electrical connection	210
B.6	An amplifier model to estimate input noise	211
B.7	Bimetallic connections in a sensor circuit form parasitic thermocouple junctions	212
B.8	Open loops in the signal and return paths are an invitation to pick up magnetic interference	213
C.1	I/O read parameters, only the address of the selected Board is inserted	214
C.2	mX+b parameters block, the value of 0.019607 is inserted For the slope (m)	214
C.3	Serial port setting	214
C.4	Timer block parameters	214
C.5	Numeric edit parameter	215
C.6	Chart parameters configuration	215
C.7	Setting Up Switch Bar Parameters	216
C.8	Setting Up PanelMeter parameters	216
C.9	Setting Up Multiplexer Parameters	217
C.10	Setting Alphanumeric Input Block Parameters	218
C.11	Setting Increment Counter Parameters	218
D.1	The basic RC charging circuit in the 555 timer	220
D.2	(a) The capacitor slowing up when it charges (b) The capacitor slowing down when it discharges	221
D.3	555 timer connected as an astable multivibrator	221
D.4	The capacitor charging and discharging operation in the 555 timer	221
D.5	Circuit diagram of 555 timer	223

## LIST OF ABBREVIATIONS/NOTATIONS/GLOSSARY OF TERMS

AC	Alternating current
ADC	Analogue-to-Digital Converter
AP	Alkaline Phosphatase
ASV	anodic stripping voltammetry
BOD	Biological Oxygen Demand
CPU	Central Processing Unit
DA	Data Acquisition
DAC	Digital-to-Analogue Converter
DC	Direct Current
DCE	Data Communication Equipment
DTE	Data Terminal Equipment
DTNB	DITHIO-bis(2-NITROBENZOIC ACID)
ELISA	Enzyme Linked Immunosorbant Assay
EPROM	Erasable Programmable Read Only Memory
FET	Field Effect Transistors
FPXRF	Field Portable X-ray Fluorescence
GEMs	Genetically Engineered Microorganisms
HRP	Horse Radish Peroxidase
IC	integrated circuit
INTR	Interrupt
I/O	Input/Output
ISFET	ion-selective field effective transistor
LED	light emitting diode
MARDI	Malaysia Agricultural Research and Development Institute
ODAM	OZO Diversified Automation Machine
OPCs	Organophosphorus Compounds
OPH	Organophosphate Hydrolase
PCB	Printed Circuit Board
PC	Personal Computer
PLC	Programmable Logic Controller
ppb	part per billion
ppm	part per million
REDOX	Reduction and Oxidation
RTD	Resistance-Temperature Detector
RxD	Receiving
SAMs	Self Assembled Monolayers
SHE	Standard Hydrogen Electrode
SPR	Surface Plasmon Resonance
TBR	Transmitter Buffer Register
TIRF	Total Internal Reflection Fluorescence
TTL	Transistor-Transistor logic
TxD	Transmission
UART	Universal Asynchronous Receiver-Transmitter
UiTM	Universiti Teknologi Mara Malaysia

## CHAPTER ONE

### INTRODUCTION

#### 1.1 Overview of the Environment Monitoring Approaches

During the three decades ago, there was a strong demand to monitor hazardous compounds in life environment as well as to determine thousands of compounds in various areas like clinical chemistry (determining of disease markers and drugs, etc.), food contaminant assessment quality control, and others [1]. The sensitive and selective determination of a large number of compounds is of great relevance for scientific research as well as for several branches of industry, e.g., for process control in the chemical and food industries [2]. Also in the field of health care it is indispensable for the diagnosis of diseases [1]. The frequent outbreaks of food poisoning serve to underline the need for enhanced monitoring of the food processing industry through disposable, operator friendly microbial contamination detection systems [2]. Such thing has given rise to increased effort in science and technology all over the world to develop simple, rapid, sensitive and inexpensive methods of monitoring and analysis. For instance, during the last decade, the breakout of the industrial revolution in Malaysia has resulted in very dangerous various contaminated environments. As the case in the developed countries, Malaysia shows a growing need and a major concern about safety and quality of food supply. For this purpose, in all over the Malaysian peninsula states different specialised institutions have grown to meet the requirements of creating free pollutants environment.

High selectivity, in trace analysis, has been gained by considerable progress in analytical instrumentation, as is reflected by modern gas chromatography, high-pressure liquid chromatography, mass spectrometry, and atomic absorption spectroscopy. However, these powerful instrumental techniques are only used in specialized laboratories. They are not suited to on-line operation. One of the approaches that can be adopted is to develop on-line monitoring system. The wide use of electronic and computer technology can simplify the development process of the system. As an addition, the invention of an electrochemical biosensor to detect biological based materials such as Chlorpyrifos pesticide in the agricultural sector, glucose level in blood, heavy elements in the drinking water etc., have attracted many interests. Moreover, the simplicity of electrochemical biosensor construction and not being limited to the laboratory based systems, proved to replace these heavy and expensive systems. Therefore, the development of electrochemical biosensors, which are highly selective and easy to handle, is thus a key solution in analysis.

## **1.2 Organophosphate Pesticides**

Although Organophosphate pesticides such as Chlorpyrifos pesticide presents a high toxicity that may represent a serious risk for the equilibrium to the environment including the industrial production, agricultural and domestic use, they are considered to be the most important chemicals being utilized extensively in agricultural sectors. Consequently, monitoring these chemicals in water, soil, and food products is highly needed to protect human health and living organisms. A lot of efforts and researches have been oriented and exerted to monitor these pesticides based on the principle of enzyme inactivation [3].



### 1.3 Definition of Electrochemical Biosensors

Electrochemical biosensors are analytical tools combining biochemical reaction component with a physical transducer (Figure 1.1); the biological sensing element can be an enzyme, antibody, DNA sequence, or event microorganism. The biochemical component serves to selectively catalyse a reaction or facilitates a binding event. The selectivity of the biochemical recognition event allows for the operation of biosensors in a complex sample matrix. The transducer converts the biochemical event into a measurable signal, thus providing the means for detecting it [5]. Measurable events range from spectral changes, which are due to production or consumption of an enzymatic reaction's product/substrate, to mass change upon biochemical complexity.

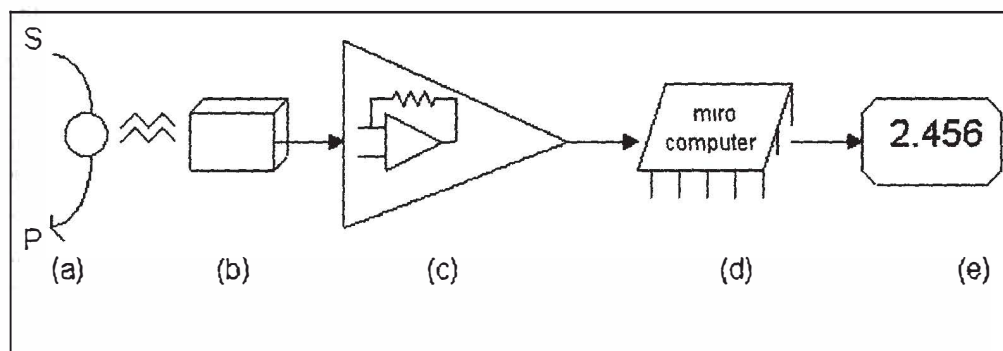


Figure 1.1: Basic Operation of the Electrochemical Biosensor Principle

In Figure 1.1, (S) a sample illustrates any substance such as pesticides, blood etc., that needed to be detected. (a) Biocatalyst - converts the analyte into product. See Figure 1.2. (b) Transducer - detects the occurrence of the reaction and converts it into an electrical signal. (c) Amplifier - amplifies the usually small signal to a useable level. (d) Microcomputer - signal is digitized and stored for further