

Arch Gynecol Obstet (2009) 279:533–537
DOI 10.1007/s00404-008-0774-5

ORIGINAL ARTICLE

High throughput non-invasive determination of foetal Rhesus D status using automated extraction of cell-free foetal DNA in maternal plasma and mass spectrometry

Simon Grill · Irina Banzola · Ying Li · Tea Rekhviashvili · Tobias J. Legler · Sina P. Müller · Xiao Yan Zhong · Sinuhe Hahn · Wolfgang Holzgreve

Received: 14 July 2008 / Accepted: 14 August 2008 / Published online: 28 August 2008
© Springer-Verlag 2008

Abstract

Purpose To examine the potential high throughput capability and efficiency of an automated DNA extraction system in combination with mass spectrometry for the non-invasive determination of the foetal Rhesus D status.

Methods A total of 178 maternal plasma samples from *RHD*-negative pregnant women were examined, from which DNA was extracted using the automated Roche MagNA Pure™ system. Presence of the foetal *RHD* gene was detected by PCR for *RHD* exon 7 and subsequent analysis using the Sequenom MassArray™ mass spectrometric system.

Results We determined that as little as 15 pg of *RHD*-positive genomic DNA could be detected in a background of 585 pg of *RHD*-negative genomic DNA. The analysis of the clinical samples yielded a sensitivity and specificity of 96.1 and 96.1%, respectively.

Conclusion Our study indicated that automated DNA extraction in combination with mass spectrometry permits the determination of foetal Rhesus D genotype with an

accuracy comparable to the current approaches using real-time PCR.

Keywords Rhesus D · *RHD* · MALDI-TOF · Non-invasive · Saber assay

Introduction

The non-invasive determination of the foetal *RHD* status via the analysis of cell-free foetal DNA in maternal plasma or serum by real-time PCR is well established and already offered as a clinical service in a number of countries [2, 6]. This development can greatly assist with the screening and monitoring of pregnancies at risk for haemolytic disease of the foetus and newborn (HDN), and also reduce the health care costs by avoiding unnecessary prophylactic treatment in those cases where the foetus is *RHD* negative [7].

It has recently been shown that MALDI-TOF (matrix assisted laser desorption ionization-time of flight) mass spectrometric devices, such as the Sequenom MassArray™ system, can be used for the detection of foetal genetic loci by the analysis of cell-free foetal DNA in maternal plasma or serum [11, 12]. The main advantage of this approach over conventional real-time PCR is that it permits the ready detection of foetal genetic loci which only differ slightly from the maternal counterpart, such as point mutations. Furthermore, it is possible to examine a large number of multiplex PCR products by mass spectrometry, implying that a large number of mutations or different loci can be examined in a single analysis [18]. A further attribute of the MassArray™ system is that it is highly amenable to high throughput analysis of several thousand samples per day. Consequently, it has been proposed that this system may be

S. Grill · I. Banzola · Y. Li · T. Rekhviashvili · X. Y. Zhong · S. Hahn · W. Holzgreve
Department Biomedicine, University Women's Hospital,
Basel, Switzerland

T. J. Legler · S. P. Müller
Department of Transfusion Medicine,
University of Göttingen, Göttingen, Germany

W. Holzgreve (✉)
Laboratory for Prenatal Medicine and Gynaecological Oncology,
Women's Hospital, University of Basel, Hebelstrasse 20,
4031 Basel, Switzerland
e-mail: hahns@uhbs.ch; wolfgang.holzgreve@unibas.ch

suitable for the analysis of cell-free foetal DNA in routine clinical diagnostic labs [5, 11, 12].

As to date few large-scale studies have examined the suitability of such a system for this purpose, we have now performed a study in which 178 clinical samples were analysed in a blinded manner for the presence or absence of the foetal *RHD* gene.

Materials and methods

Plasma sample collection and processing

The study was approved by the review boards from both the institutions. After written informed consent, 15 mL EDTA blood samples were obtained from pregnant women at risk for HDN caused by alloimmunization. The samples were processed on site at the University of Göttingen, Germany, by twofold centrifugation (1: 10 min, 2,700×g; 2: 45 min 12,500×g). The plasma was divided into 1 mL aliquots and stored at −80°C. One aliquot of each sample was frozen and sent to Basel for analysis.

DNA isolation from maternal plasma

The automatic DNA isolation system MagNA Pure™ instrument (Roche Applied Science, Switzerland) was used for plasma DNA extraction. Following the “DNA LV Blood_1000.blk” protocol, DNA was extracted from 1 mL of *RHD*-negative maternal plasma with the Roche MagNA Pure™ Pure LC DNA Isolation Kit-Large Volume. The DNA was eluted into 200 µL of elution buffer and stored at −20°C for later use. A sample volume of 50 µL was available for analysis.

Assay design

The assay design was kindly provided by Sequenom Inc., USA. As only the foetal *RHD* gene is detected, and no corresponding maternal allele, a SABER (single allele base extension reaction) assay was used which exclusively detects the presence of the *RHD* 7 exon (see below). All oligonucleotides were synthesised and HPLC purified by Microsynth (Switzerland). Amplification primers contained

a 5′–10 mer tag to keep them out of the analytical mass range.

PCR amplification

PCR reactions were performed in a total volume of 12.5 µL containing 8 µL of eluted cfDNA, 400 nM of each primer (PCR-*RHD7*-fw and PCR-*RHD7*-rev, Table 1), 3 mM Mg²⁺, 0.5 U HotStart *Taq* DNA Polymerase (Qiagen, Switzerland), 50 µM dNTPs and 1× PCR buffer. Thermal cycling was performed as follows: 15 min at 95°C followed by 50 cycles of 95°C for 45 s, 57°C for 45 s and 72°C for 1 min. The reaction was completed with a final extension at 72°C for 7 min.

Shrimp alkaline phosphatase (SAP) treatment

For the dephosphorylation of excess dNTPs, 4 µL of a solution containing 3.06 µL ddH₂O, 0.34 µL hME buffer (Sequenom Inc.) and 0.6 µL shrimp alkaline phosphatase (Sequenom Inc.) were added to 12.5 µL of PCR product. After incubation at 37°C for 60 min, the enzyme was inactivated at 85°C for 5 min.

Single allele base extension reaction

Four microliters of a solution containing 3.12 µL ddH₂O, 0.4 µL Termination Mix C (containing 2′,3′-dideoxycytosintriphosphate (ddCTP), Sequenom Inc.), 0.4 µL 25 µM *RHD7* extension primer (Table 1) and 0.08 µL (2.56 U) Thermo Sequenase (Sequenom Inc.) were added to 18.5 µL SAP treated PCR product. Thermal cycling was performed as follows: 2 min at 94°C followed by 99 cycles of 94°C for 5 s, 51°C for 5 s and 52°C for 5 s.

Desalting and mass spectrometric analysis

A total of 29.5 µL H₂O and 6 mg of SpectroCLEAN resin (Sequenom Inc.) were added to 20.5 µL extension product. The plate was rotated for 10 min at room temperature followed by centrifugation at 3,000×g for 3 min to pellet the resin.

A total of 15 nL of each desalted sample were dispensed onto a 384-format SpectroCHIP using a MassARRAY

Table 1 Oligonucleotides for PCR and extension reaction and corresponding masses used for the *RHD* exon 7 mass spectrometry assay

PCR- <i>RHD7</i> -fw	5′-ACGTTGGATGGGGTGTGTGAACCGAGTGCTG-3′
PCR- <i>RHD7</i> -rev	5′-ACGTTGGATGCCGGCTCCGACGGTATC-3′
<i>RHD7</i> extension primer	5′-ATTCCCCACAGCTCCAT-3′
SABER-assay terminator	2′,3′-dideoxycytosintriphosphate (ddCTP)
Mass of extension primer	5050.3 Da
Mass of extension product (Call: G)	5323.5 Da

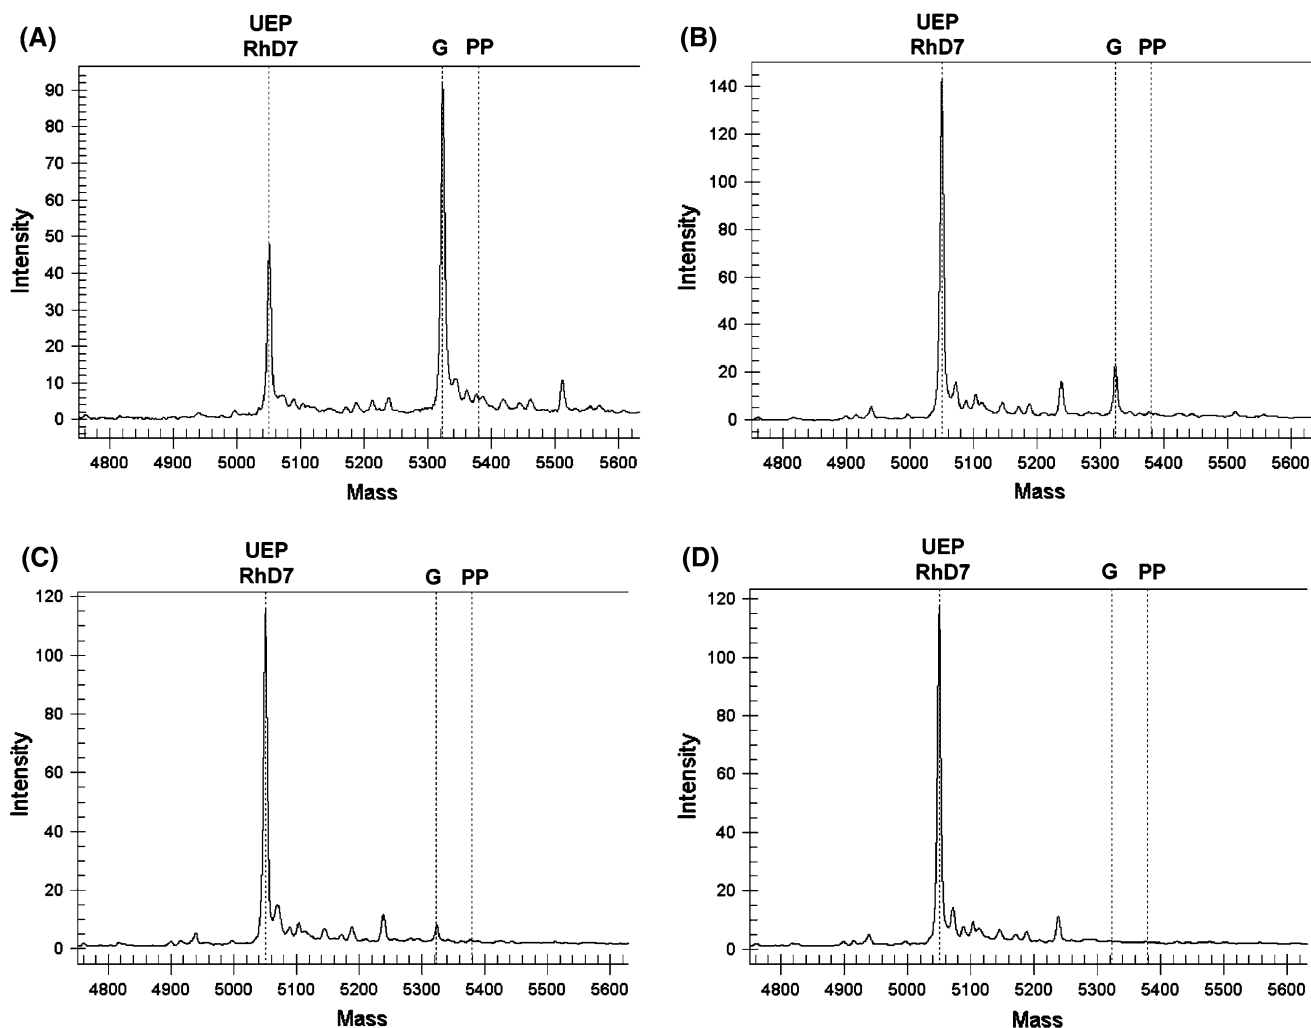


Fig. 1 Sensitivity and specificity of the *RHD* assay using the MALDI-TOF MS based SABER approach. *RHD*-positive genomic DNA was diluted into *RHD*-negative genomic DNA. The total DNA amount per reaction was 600 pg. **a** 600 pg *RHD*-positive genomic DNA. **b** 30 pg

RHD-positive DNA in 570 pg *RHD*-negative background. **c** 15 pg *RHD*-positive DNA in 585 pg *RHD*-negative background. **d** 600 pg *RHD* negative genomic DNA. UEP unextended primer, G *RHD* allele, PP pausing peak

nanodispenser (Sequenom Inc.) and subsequently analysed by MassARRAY Analyzer Compact. The data were recorded and interpreted by MassARRAY TYPER (Sequenom Inc.) software.

Results

Validation of the mass spectrometry Assay for *RHD* exon 7

To evaluate the sensitivity of the SABER assay, we serially diluted *RHD*-positive genomic DNA into *RHD*-negative genomic DNA, such that the overall quantity of DNA was 600 pg per reaction. This is the equivalent amount to that normally present in cell-free DNA preparations. Under these conditions, we were able to detect 15 pg of *RHD*-positive

genomic DNA in a background of 585 pg of *RHD*-negative genomic DNA (Fig. 1). This is almost equal to the three copies of the *RHD* gene in a single reaction, indicating that the *RHD* assay exhibits a degree of sensitivity and specificity suitable for the analysis of cell-free foetal DNA.

Detection of the foetal *RHD* exon 7 in maternal plasma

A total of 178 samples were analysed in a blinded manner. The results were confirmed by those obtained from serological analysis using cord blood in Göttingen. The presence or absence of the foetal *RHD* exon 7 was determined following the analysis of the samples in duplicates. If the result was unambiguously positive or negative, the samples were scored accordingly. If the result was equivocal, the sample was re-analysed in duplicate. The sample was only

Table 2 The results of foetal *RHD* genotyping in maternal plasma using the MALDI-TOF based SABER assay

Gestational age	No. of cases	<i>RHD</i> positive	<i>RHD</i> negative	Sensitivity/specificity (%)
First trimester	5	4/4	1/1	100/100
Second trimester	127	91/93	33/34	97.8/97.1
Third trimester	32	18/21	10/11	85.7/90.1
Unknown	15	10/10	5/5	100/100
Total	178	122/127	49/51	96.1/96.1

scored as *RHD* positive if at least two positive signals were detected amongst the two sets of duplicates, else it was scored as *RHD* negative.

Following a comparison of our results with those obtained by classical serology of the cord blood, we ascertained that out of 178 samples we had examined, five samples had been incorrectly scored as *RHD* negative and two samples incorrectly determined as being *RHD* positive (Table 2). This equates to a sensitivity of 96.1% and a specificity of 96.1%. Our data show 96.1% concordance to those obtained by quantitative real-time PCR.

Discussion

Non-invasive prenatal *RHD* analysis is currently most frequently performed using real-time PCR, either in conjunction with manual or automated procedures for the extraction of cell-free DNA from the maternal plasma/serum samples [4, 9, 13, 15, 16, 19]. In this study, we analysed the foetal *RHD* status by mass spectrometry, in combination with automated system for the extraction of cell-free DNA from maternal plasma.

The validation of the assay showed that we were able to detect as little as 2.5% of *RHD*-positive genomic DNA in a background of *RHD*-negative genomic DNA, indicating that the assay is very sensitive. A similar sensitivity (20 pg mutant DNA in 580 pg wildtype DNA) has recently been reported by our group for the mass spectrometry based genotyping of the foetal KEL1 blood group from cell-free DNA in maternal plasma [11].

Out of 178 samples, five cases were incorrectly scored as *RHD* negative and two were incorrectly scored as *RHD* positive. Of those five false negative samples, three were obtained during the third trimester, while the remaining two were from the second trimester of pregnancy. The two samples that were scored false positive were from the second and third trimester or pregnancy. These remained to be assessed incorrectly, even after several rounds of re-analysis, indicating that the sample may have been contaminated. As the samples stem from a Caucasian population, a false positive result caused by the inactive allele *RHD* Ψ [10, 16]

is unlikely, but can only be excluded convincingly by examining for the presence of this allele.

In those cases where the foetal *RHD* gene cannot be detected, it is unclear, whether the foetus is Rhesus-negative or if the amount of foetal DNA in the sample is below the detection limit of the system. For the exclusion of the latter case, the detection of paternally inherited single nucleotide polymorphisms [12], the detection of a Y-chromosome specific sequence [8], or the detection of an epigenetic marker such as the foetal hypermethylated RASSF1A sequence [3] can be performed. In our current study, we were unable to perform such additional analyses due to very limited amount of sample available.

A recent review of large-scale studies reporting on the non-invasive determination of foetal *RHD* status by the real-time PCR analysis of cell-free DNA indicated that accuracies between 95 and 99% could be attained [14]. As such, our data yielding an overall accuracy of 96.1% concur favourably with those obtained by real-time PCR.

In future studies we aim to make better use of the Sequenom MassArrayTM mass spectrometric system, by performing multiplex analyses. In this manner it will be possible to detect variant *RHD* alleles such as the *RHD* Ψ gene [1, 17], as well as polymorphic markers indicating whether cell-free foetal DNA was present in the sample or not. This added information will increase the value of the analysis, and by being able to perform these numerous examinations in a single analytic run, help to reduce costs.

In this manner, the combination of an automated DNA extraction system and mass spectrometry may emerge as a competitive alternative to the current commonly used real-time PCR approaches used to determine non-invasively the foetal *RHD* status.

Acknowledgments Funding from the European Commission for the Special Non-invasive Advances in Fetal and Neonatal Evaluation (SAFE) Network of Excellence (LSHB-CT-2004-503243) and the Swiss National Science Foundation (SNSF 3200B0-107697/1), from which this study was partially funded, is gratefully acknowledged.

References

1. Avent ND (2008) RHD genotyping from maternal plasma: guidelines and technical challenges. *Methods Mol Biol* 444:185–201. doi:10.1007/978-1-59745-066-9_14
2. Bianchi DW, Avent ND, Costa JM, van der Schoot CE (2005) Noninvasive prenatal diagnosis of fetal Rhesus D: ready for prime(r) time. *Obstet Gynecol* 106:841–844
3. Chan KC, Ding C, Gerovassili A, Yeung SW, Chiu RW, Leung TN et al (2006) Hypermethylated RASSF1A in maternal plasma: a universal fetal DNA marker that improves the reliability of non-invasive prenatal diagnosis. *Clin Chem* 52:2211–2218. doi:10.1373/clinchem.2006.074997
4. Costa JM, Giovangrandi Y, Ernault P, Lohmann L, Nataf V, El HN et al (2002) Fetal RHD genotyping in maternal serum during the

- first trimester of pregnancy. *Br J Haematol* 119:255–260. doi:[10.1046/j.1365-2141.2002.03780.x](https://doi.org/10.1046/j.1365-2141.2002.03780.x)
5. Ding C (2008) Maldi-TOF mass spectrometry for analyzing cell-free fetal DNA in maternal plasma. *Methods Mol Biol* 444:253–267. doi:[10.1007/978-1-59745-066-9_20](https://doi.org/10.1007/978-1-59745-066-9_20)
 6. Finning K, Martin P, Daniels G (2004) A clinical service in the UK to predict fetal Rh (Rhesus) D blood group using free fetal DNA in maternal plasma. *Ann N Y Acad Sci* 1022:119–123. doi:[10.1196/annals.1318.019](https://doi.org/10.1196/annals.1318.019)
 7. Finning K, Martin P, Summers J, Massey E, Poole G, Daniels G (2008) Effect of high throughput RHD typing of fetal DNA in maternal plasma on use of anti-RhD immunoglobulin in RhD negative pregnant women: prospective feasibility study. *BMJ* 336:816–818. doi:[10.1136/bmj.39518.463206.25](https://doi.org/10.1136/bmj.39518.463206.25)
 8. Finning KM, Chitty LS (2008) Non-invasive fetal sex determination: impact on clinical practice. *Semin Fetal Neonatal Med* 13:69–75. doi:[10.1016/j.siny.2007.12.007](https://doi.org/10.1016/j.siny.2007.12.007)
 9. Harper TC, Finning KM, Martin P, Moise KJ Jr (2004) Use of maternal plasma for noninvasive determination of fetal RhD status. *Am J Obstet Gynecol* 191:1730–1732. doi:[10.1016/j.ajog.2004.06.098](https://doi.org/10.1016/j.ajog.2004.06.098)
 10. Legler TJ, Lynen R, Maas JH, Pindur G, Kulenkampff D, Suren A et al (2002) Prediction of fetal Rh D and Rh CcEe phenotype from maternal plasma with real-time polymerase chain reaction. *Transfus Apher Sci* 27:217–223. doi:[10.1016/S1473-0502\(02\)00068-X](https://doi.org/10.1016/S1473-0502(02)00068-X)
 11. Li Y, Finning K, Daniels G, Hahn S, Zhong X, Holzgreve W (2008) Noninvasive genotyping fetal Kell blood group (KEL1) using cell-free fetal DNA in maternal plasma by MALDI-TOF mass spectrometry. *Prenat Diagn* 28:203–208. doi:[10.1002/pd.1936](https://doi.org/10.1002/pd.1936)
 12. Li Y, Wenzel F, Holzgreve W, Hahn S (2006) Genotyping fetal paternally inherited SNPs by MALDI-TOF MS using cell-free fetal DNA in maternal plasma: influence of size fractionation. *Electrophoresis* 27:3889–3896. doi:[10.1002/elps.200600084](https://doi.org/10.1002/elps.200600084)
 13. Lo YM, Hjelm NM, Fidler C, Sargent IL, Murphy MF, Chamberlain PF et al (1998) Prenatal diagnosis of fetal RhD status by molecular analysis of maternal plasma. *N Engl J Med* 339:1734–1738. doi:[10.1056/NEJM199812103392402](https://doi.org/10.1056/NEJM199812103392402)
 14. Maron JL, Bianchi DW (2007) Prenatal diagnosis using cell-free nucleic acids in maternal body fluids: a decade of progress. *Am J Med Genet C Semin Med Genet* 145:5–17. doi:[10.1002/ajmg.c.30115](https://doi.org/10.1002/ajmg.c.30115)
 15. Rouillac-Le SC, Puillandre P, Gillot R, Baulard C, Metral S, Le Van KC et al (2004) Large-scale pre-diagnosis study of fetal RHD genotyping by PCR on plasma DNA from RhD-negative pregnant women. *Mol Diagn* 8:23–31. doi:[10.2165/00066982-200408010-00004](https://doi.org/10.2165/00066982-200408010-00004)
 16. van der Schoot CE, Hahn S, Chitty LS (2008) Non-invasive prenatal diagnosis and determination of fetal Rh status. *Semin Fetal Neonatal Med* 13:63–68. doi:[10.1016/j.siny.2007.12.012](https://doi.org/10.1016/j.siny.2007.12.012)
 17. van der Schoot CE, Soussan AA, Koelewijn J, Bonsel G, Paget-Christiaens LG, de HM (2006) Non-invasive antenatal RHD typing. *Transfus Clin Biol* 13:53–57. doi:[10.1016/j.tracli.2006.02.021](https://doi.org/10.1016/j.tracli.2006.02.021)
 18. Xiu-Cheng FA, Garritsen HS, Tarhouny SE, Morris M, Hahn S, Holzgreve W et al (2008) A rapid and accurate approach to identify single nucleotide polymorphisms of mitochondrial DNA using MALDI-TOF mass spectrometry. *Clin Chem Lab Med* 46:299–305. doi:[10.1515/CCLM.2008.071](https://doi.org/10.1515/CCLM.2008.071)
 19. Zhong XY, Holzgreve W, Hahn S (2001) Risk free simultaneous prenatal identification of fetal Rhesus D status and sex by multiplex real-time PCR using cell free fetal DNA in maternal plasma. *Swiss Med Wkly* 131:70–74