



*Citation for published version:*

Jolly, P, Formisano, N & Estrela, P 2015, 'DNA Aptamer-based detection of prostate cancer', *Chemical Papers*, vol. 69, no. 1, pp. 77-89. <https://doi.org/10.1515/chempap-2015-0025>

*DOI:*

[10.1515/chempap-2015-0025](https://doi.org/10.1515/chempap-2015-0025)

*Publication date:*

2015

*Document Version*

Early version, also known as pre-print

[Link to publication](#)

## University of Bath

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

### Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

# DNA aptamer-based detection of prostate cancer

Pawan Jolly, Nello Formisano, Pedro Estrela

*Department of Electronic & Electrical Engineering, University of Bath, Bath BA2 7AY,  
United Kingdom*

Corresponding author: Dr Pedro Estrela; P.Estrela@bath.ac.uk; Department of Electronic and Electrical Engineering, University of Bath, Claverton Down, Bath, BA2 7AY, United Kingdom

Received [Dates will be filled in by the Editorial office]

The use of aptamers in biosensing have gained considerable attention as an attractive alternative to antibodies because of their unique properties such as long term stability, cost effectiveness and tunability to various applications. Among various cancers, early diagnosis of prostate cancer (PCa) is one of the biggest concerns for ageing men worldwide. One of the most commonly used biomarker for PCa is prostate specific antigen (PSA), which can be found in elevated levels in patients with cancer. In this review, a presentation on the gradual transition of research from antibody-based to aptamer-based biosensors is presented specifically for PSA. A brief description on aptamer-based biosensing for other PCa biomarkers is also presented. Special attention is given to electrochemical methods as analytical techniques for development of simple, sensitive and cost effective biosensors. The review also focuses on different surface chemistries exploited for fabrication and their application with clinical samples. Utilization of aptamers provides a promising tool for development of point-of-care biosensors for early detection of prostate cancer. In the view of the unmatched upper hand of aptamers, future perspectives are also discussed, not only in the point of care format but also in other novel applications.

**Keywords:** DNA aptamer, biosensor, electrochemical detection, prostate specific antigen, prostate cancer, surface chemistry

34

35

36

## Introduction

37

38 Prostate cancer (PCa) is a type of cancer that develops in the prostate gland, which is a  
39 part of a male reproductive system. PCa is the most commonly diagnosed cancer amongst  
40 men in Europe and the United States and is the second worldwide leading cause of morbidity.  
41 It has been reported that PCa is predominant in older men above the age of 50 (Kirk, 1997;  
42 Hoffman, 2011) and among black men (Stanford et al., 1999; Greenlee et al., 2000). It has  
43 been also projected that PCa will be the most common cancer by 2030 in the UK (Greenlee et  
44 al., 2000; Jeong et al., 2010).

45 Most of the PCa generate in the epithelium cells (Bostwick, 1989). As androgens  
46 regulate cell division of the gland epithelium (Ross et al., 1998), these hormones are believed  
47 to be the main cause of PCa. However, a study demonstrating a consistent correlation between  
48 androgens and prostatic carcinogenesis has not yet been reported to date and the precise  
49 causes that lead to PCa are still not well understood (Kufe et al., 2003).

50 PCa often develops very slowly and the lack of symptoms during the early stages of  
51 the disease leads to a late diagnosis of the tumour. Moreover, if diagnosed at a late stage, no  
52 effective treatments are currently available for its cure. In many cases PCa does not show any  
53 clinical manifestation during the lifetime of a patient, who might die for non-related PCa  
54 causes. However, for those patients that develop a more aggressive cancer form, PCa cells can  
55 break away from a prostate tumour and metastasise. Since the prostate is well connected to  
56 numerous lymph nodes, the spread is easy and some of the most common sites of PCa  
57 metastatic process are bones (Chou & Simons, 1997).

58

59

60

## Current detection methods

61

62 There is no solitary test for the diagnosis of PCa. Moreover, all the tests which are  
63 used to diagnose have pros and cons which are usually discussed by the doctors with their  
64 patients. The most commonly used methods for PCa detection are: digital rectal examination  
65 (DRE), transrectal ultrasound (TRUS), biopsy and PSA blood test.

66 In DRE, a doctor inserts a gloved finger into the rectum and examines for bumps or  
67 swelling of the prostate gland. It is an inexpensive method and can also detect PCa

68 irrespective of changes in the level of prostate specific antigen (PSA) in blood. Accuracy of  
69 diagnosis can be increased when DRE is combined with PSA tests and biopsy results (Uzzo et  
70 al., 1995; Basler & Thompson, 1998; Jeong et al., 2010). In comparison to DRE, in the TRUS  
71 method an ultrasound probe is inserted into the rectum, emitting energy sound waves to image  
72 the prostate gland. It is a very useful tool to understand pathology of tumours and in guiding  
73 needle biopsies for sampling of tissue (Aus et al., 1996; Irani et al., 1997). For a biopsy, a  
74 small section of the tissue is removed through the rectum using a needle and is  
75 microscopically examined by pathologists. It requires a high number of samples from the  
76 prostate making it a painful protocol. Not only the results from biopsies are controversial,  
77 there is also a high risk of severe infections with subsequent biopsies (Jeong et al., 2010; Loeb  
78 et al., 2013).

79 The most frequently used test for PCa screening is the quantification of levels of PSA  
80 in blood. If PSA levels are higher than the cut off levels of 4 ng/ml, biopsy procedures are  
81 considered (Catalona et al., 1991, Jeong et al., 2010; Savory et al., 2010). However, the levels  
82 of PSA in blood in ageing men can also be raised due to other factors like benign prostatic  
83 hyperplasia (BPH) and prostatitis, which could lead to an over-diagnosis in men (Carter et al.,  
84 1992). Consequently, due to faulty diagnosis, patients undergo biopsy surgery making PSA  
85 testing a controversial diagnostic tool. Due to these controversies with PSA testing, in May  
86 2012 the US Preventative Services Task Force recommended against PSA screening in all  
87 men. This emphasized the need for more reliable biomarkers for diagnosis of the disease  
88 (Moyer, 2012).

89

90

91

### **Prostate specific antigen (PSA): a PCa biomarker**

92

93 PSA belongs to the family of kallikrein proteins which are defined as serine proteases.  
94 There are about 15 kallikrein family members that have been identified in humans. PSA is the  
95 only kallikrein specific to prostate (hK3). Pancreatic renal kallikrein (hK1) and human  
96 glandular kallikrein (hK2), which are androgen regulated, are also expressed in the prostate  
97 (Balk et al., 2003).

98

99 PSA is synthesised in its inactive form: a 244 amino acid long protein called pro-PSA.  
100 Pro-PSA is cleaved from the N terminus in the prostate by the hK2 enzyme leading to active  
101 PSA which is a 237 amino acid long protein (Takayama et al., 1997). The active PSA is a  
101 30 kDa protein which can be found in both serum and semen of men. PSA is present in semen

102 in the range of 0.5 - 2 mg/ml and its physiological role is to de-coagulate semen by breaking  
103 down the proteins semenogelin I and II (Lilja et al., 1987; Lövgren et al., 1999). In prostate  
104 cancer there is release of both active PSA and pro-PSA due to rupture of the basal membrane.  
105 Moreover, internally cleaved forms of PSA (with no enzymatic activity) also enter the blood  
106 stream but remain un-complexed and are taken into the free PSA (fPSA) count. However,  
107 when active PSA enters the blood stream it becomes immediately complexed with protein  
108 inhibitors. Most of the assays employing antibodies measure the total amount of PSA (tPSA)  
109 (Takayama et al., 1997).

110 Many studies reported that PSA levels are directly proportional to the stage of the  
111 cancer and to the volume of the tumour (Stamey et al., 1987; Grossklau et al., 2002; Pinsky  
112 et al., 2007; Lilja et al., 2008). PSA detection results are nowadays highly sensitive (Madu &  
113 Lu, 2010) and reasonably inexpensive. Moreover PSA testing is a more accepted procedure  
114 by patients compared to DRE and this has augmented the early detection of PCa (Balducci et  
115 al., 1997). However, even though PSA testing induced a decrease in PCa mortality of 20% its  
116 screening led to over-diagnosis and over-treatment (Andriole et al., 2009) of patients that  
117 would have not been clinically affected by the tumour during their lifetime. Over diagnosis  
118 can, in fact, lead to unnecessary treatments and increase the state of anxiety in patients.  
119 Conversely, clinicians are not able nowadays to discriminate between a harmless or lethal  
120 form of prostate cancer and so to decide whether the patient needs a treatment. Once a  
121 prostate cancer has been definitively treated, PSA screening is the most reliable and fast  
122 means that enable to detect a contingent recurrence of the tumour (Lilja et al., 2008).

123 With the shortcomings of the current tests for PCa, including PSA testing, there is a  
124 concerted effort to look for alternatives. However, it would be a challenge to replace PSA  
125 entirely due to its minimally invasive nature and low cost. Instead, there is a pressing need to  
126 look for other biomarkers to complement PSA that can increase the specificity and sensitivity  
127 of PCa screening and inform prognosis and treatment courses.

128 One path currently being looked at when a high level of PSA is detected in patients  
129 with cancer, is to differentiate PSA into different forms namely free PSA (fPSA) and total  
130 PSA (tPSA) and quantify them independently. One of the approaches is to measure the ratio  
131 of free PSA to total PSA in the blood. It has been proven, in fact, that the levels of fPSA are  
132 lower in patients with PCa than in patients with BPH (Christensson et al., 1993), which can  
133 thus be an indication of the aggressiveness of the cancer. However, the method can cause  
134 false negative results as the amount of fPSA can be higher in patients with larger prostate  
135 volume (Stephan et al., 1997; Catalona et al., 1998). Nevertheless, the ratio of free to total

136 PSA when combined with the total PSA levels increases the confidence of the diagnosis  
137 (Velonas et al., 2013).

138

### 139 ***Pro-PSA***

140 Several studies are also focused on the detection of a distinct form of free PSA, called  
141 proenzyme PSA (pro-PSA). Pro-PSA is an enzymatically inactive precursor of PSA obtained  
142 by co-translational removal of an amino-terminal leader. The N-terminal of pro-PSA can be  
143 cleaved at various positions resulting in different forms of pro-PSA. Pro-PSA truncated  
144 between the third and second amino acid is called [-2]pro-PSA and is believed to provide a  
145 better discrimination between cancerous and benign form of prostate disorders (Mikolajczyk  
146 et al., 2001; Mikolajczyk et al., 2004). Increased values of other forms of pro-PSA ([-5] and  
147 [-7]) have also been associated to PCa. A truncated precursor form of prostate-specific  
148 antigen is therefore a more specific serum marker of prostate cancer.

149

### 150 ***PSA density***

151 A better discrimination of BPH from PCa might be achieved by measuring the ratio of  
152 PSA to prostate volume. However, this parameter called PSA density showed contradictory  
153 evidence on the tumour aggressiveness and malignity (Stamey et al., 1987; Ohori et al.,  
154 1995). Furthermore, in order to obtain prostate volume values, TRUS is required in addition  
155 to the standard PSA test with a consequent discomfort for patients as well as an increase in  
156 the cost and time required to perform the test. For these reasons PSA density has not been  
157 extensively employed as a routine test for PCa.

158

### 159 ***PSA velocity and PSA doubling time***

160 PSA velocity refers to the rate of serum PSA increase over time while PSA double  
161 time refers to the time required for a given PSA level to be doubled. As the previous PSA  
162 derivatives, also PSA velocity can be used to distinguish a prostate cancer from a BPH (Carter  
163 et al., 1992). Both PSA velocity and PSA double time are used to monitor the recurrence of  
164 the tumour after treatment (D'Amico et al., 2004; D'Amico et al., 2005). Again, some studies  
165 compared the responses from PSA velocity and PSA double time with biopsy results  
166 demonstrating how these two PSA derivatives can fail the diagnosis (Melichar, 2012)

167

### 168 *Age-specific PSA reference ranges*

169           Since the level of PSA increases with the age of men, scientists studied this correlation  
170 in order to obtain a median value of PSA for given ranges of age. By comparing the PSA  
171 level with the median PSA for that patient's age (age-specific PSA) a better choice might  
172 been taken before ordering biopsies (Loeb & Catalona, 2007).

173

174

175

### **Oligonucleotide Aptamers**

176

177           In recent years, a range of assays for PSA detection such as electrochemical assays  
178 (Okuno et al., 2007; Panini et al., 2008), enzyme linked immunosorbent assays (Acevedo et  
179 al., 2002), cantilever assays (Wee et al., 2005), and chemiluminescent immunoassays  
180 (Albrecht et al., 1994; Seto et al., 2001) have been developed. These assays are mostly based  
181 on antibodies as recognition elements. One of the alternatives to antibodies is aptamers which  
182 can offer several advantages with respect to the former. However, an enormous research is  
183 being carried out to prove if antibodies can be replaced by aptamers to develop a real  
184 biosensor for clinical applications. The scope of this review is to highlight the major  
185 developments on PSA aptasensors and their potential to be used with real clinical blood  
186 samples.

187


188           Oligonucleotide aptamers are single stranded DNA or RNA sequences that can bind to  
189 a target molecule with high specificity and affinity. Aptamers had already been widely used in  
190 drug delivery applications and are now being extensively studied as new emerging  
191 bioreceptors for biosensors (termed aptasensors) (Hianik & Wang, 2009; Iliuk et al., 2011).  
192 Aptamers have shown comparable or even stronger binding than antibodies towards a broad  
193 range of targets (e.g. proteins, peptides, amino acids, drugs, whole cells, etc.), especially with  
194 the development of novel selection technologies (Xiao et al., 2005). The high affinity of the  
195 aptamers towards the target molecule is defined by their capability of undergoing  
196 conformation changes upon the binding event (Hermann & Patel, 2000; Song et al., 2008;  
197 Hianik & Wang, 2009). Although using aptamers have many added advantages over  
198 antibodies, they still need careful consideration while fabricating a biosensor. For instance,  
199 binding of an aptamer to protein might be affected by changing buffer conditions. Also, as  
apptamers are oligonucleotide sequences, special care is needed as they are sensitive to DNase

200 and RNase activity. Furthermore, the  $k_d$  value of aptamers is often not as good as that for  
 201 antibodies.

202 Aptamers are developed using an *in vitro* selection process based on Systematic  
 203 Evolution of Ligands by EXponential enrichment (SELEX) (see fig. 1). Briefly, it consists of  
 204 three steps that are repeated systematically in order to identify the oligonucleotide sequence  
 205 that binds better to the target. The first step is called library generation, where a library  
 206 consisting of random DNA or RNA sequences (usually 30-40 base-pairs long) flanked by the  
 207 primer binding site are used. The library is then incubated with the target molecule.  
 208 Thereafter, the target bound library is separated from unbound library. Finally, the target-  
 209 bound library is amplified using polymerase chain reaction (PCR) to create a new library to be  
 210 used in the next round. Aptamers binding and conformation characteristics are identified  
 211 using various biological assays (Syed & Pervaiz, 2010; Liu et al., 2012).

212

213

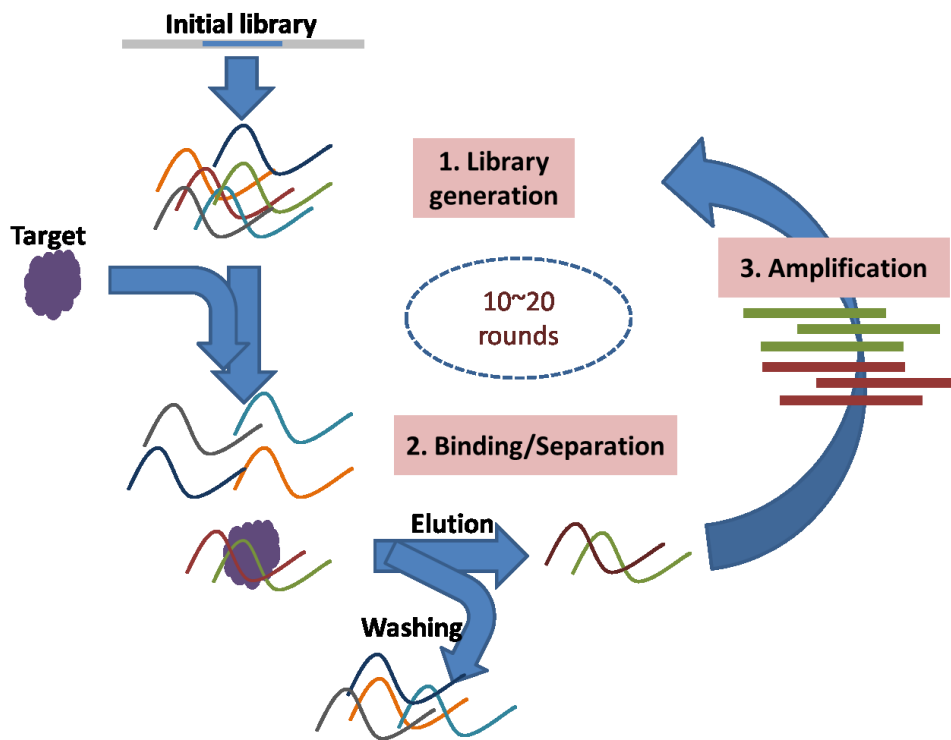

214

215

216 **Fig. 1.** The general SELEX protocol. Starting with a random library followed by incubation  
 217 with the target. Later the bound sequences are separated and further amplified for the  
 218 next round of selection. Adapted from Song et al. (2008).

219

220



221 There has been an intense interest in understanding the in-depth of ligand-binding and  
222 conformational properties of aptamers. Aptamers have many advantages over antibodies,  
223 making them very important molecular tools for both diagnostics and therapeutics. For  
224 instance, selection of aptamers is an *in vitro* process and they can be raised to a wide variety  
225 of targets ranging from small molecules and toxins to large proteins and even whole cells.  
226 Secondly, aptamers, once selected, can be synthesised with high purity and reproducibility.  
227 Also, as compared to antibodies, aptamers are usually highly chemically stable. Furthermore,  
228 they can undergo significant conformational changes in their structure upon binding with the  
229 target – a feature which can be exploited for biosensing applications. This offers great  
230 flexibility to design novel biosensors (Clark & Remcho, 2002; Tombelli et al., 2005; Willner  
231 & Zayats, 2007; Mairal et al., 2008; Song et al., 2008; Liu et al., 2012).

232

233

234

### PSA detection

235

236 PSA is currently detected in dedicated laboratory settings using automated analysers  
237 running antibody-based assays which are generally expensive and time consuming (Lin & Ju,  
238 2005; Healy et al., 2007). Cost effective, easy to use and possibly portable devices are  
239 required in order to allow more powerful tools for early detection of prostate cancer. To date,  
240 researchers have exploited several techniques for PSA detection such as optical (Besselink et  
241 al., 2004; Huang et al., 2005; Cao & Sim, 2007), piezoelectric (Weeks et al., 2003; Wee et al.,  
242 2005) and electrochemical (Sarkar et al., 2002; Fernández-Sánchez et al., 2004; Liu et al.,  
243 2013).

244

245 Although label-free-based biosensors can provide many advantages, label-based  
246 approaches are still intensively studied and can offer interesting features such as low limit of  
247 detection due to amplification strategies. An interesting magnetic bead-based detection system  
248 for PSA detection was developed by Zani et al. (2009): paramagnetic microparticles were  
249 adsorbed on an array of screen-printed electrodes and PSA was sandwiched in between two  
250 antibodies on the beads; the alkaline-phosphatase-labelled secondary antibody could be  
251 detected with differential pulse voltammetry (DPV) to achieve a detection limit of 1.4 ng/ml.  
252 A limit of detection as low as 0.5 pg/ml in undiluted serum samples was obtained by Mani et  
253 al. (2010) by combining a multienzyme-labelled immunoassay with gold nanoparticles  
254 sensing surface: in this case the secondary antibody was bound to micromagnetic HRP-  
labelled beads, which massively amplified the current signals for a very low PSA detection

255 limit. A similar detection technique was improved and integrated in a microfluidic system by  
256 Chikkaveeraiah et al. (2011) reaching an even lower detection limit. A fascinating  
257 electrochemiluminescence-based immunoassay was developed by Sardesai et al. (2011) for  
258 both PSA and interleukin 6 (IL-6) by using single-wall carbon nanotubes (SWCNT) fabricated  
259 on microwells and a sandwich assay where the secondary PSA antibody was functionalized  
260 with RuBYP-Silica particles: the detection limit achieved was of 1 pg/ml for PSA.

261

### 262 ***Label-free electrochemical sensors for PSA detection***

263 Electrochemical techniques are widely employed in biosensing devices as they can be  
264 highly sensitive, simple to perform and cost effective. An electrochemical biosensor involves  
265 an electrode surface that is functionalised with a molecular recognition element for sensing  
266 biomolecules. Binding of an analyte to this element results in an electrical change in current  
267 transfer (amperometric), voltage (potentiometric and field effect transistors), impedance  
268 (impedimetric), conductivity (conductometric) or ion charge across the electrode, which can  
269 be quantified and correlated to the amount of analyte captured. As mentioned in the previous  
270 sections, most biosensors for PSA detection currently available are antibody-based. Amongst  
271 the antibody-based electrochemical sensors, particularly important results are the ones using  
272 label-free systems. Arya & Bhansali (2012) developed a gold biosensor modified with a  
273 cysteamine self-assembled monolayer (SAM) for PSA detection. Li et al. (2005), on the hand,  
274 employed In<sub>2</sub>O<sub>3</sub> nanowires and carbon nanotubes. Electrochemical impedance spectroscopy  
275 (EIS) based sensors have been reported by Chiriaco et al. (2013) and Chornokur et al. (2011).  
276 The former exploits a combined use of two different antibodies for both free and total PSA,  
277 while the latter reported on a miniaturized sensor obtained with photolithographic techniques  
278 using a single monoclonal antibody. Another label-free antibody-based sensor which uses a  
279 polycrystalline silicon field-effect transistor was reported by Huang et al. (2013).

280

281

282

### 282 **Aptasensor for PSA detection**

283

284 An aptasensor biosensor comprises an aptamer as a biorecognition element (Lim et al.,  
285 2009). Aptasensors can be integrated with different sensing techniques such as  
286 electrochemical, optical, and mass sensitive. Among these varied techniques, electrochemical  
287 aptasensors have been fabricated using several detection techniques, namely EIS,  
288 potentiometry and differential pulse voltammetry (DPV) (Cho et al., 2009; Clark & Remcho,

289 2002; Feng et al., 2008; Ikebukuro et al., 2005; Liu et al., 2012; Numnuam et al., 2008; Wang  
 290 et al., 2007; Xu et al., 2005). For detection of PSA, both RNA and DNA aptamers have been  
 291 developed, although there are only a handful of reports on PSA biosensors using aptamers. A  
 292 summary of aptamer-based biosensors for PCa detection is presented in table 1.

293

294

295 **Table 1.** Performance comparison of different aptasensors for PCa detection

296

<i>Method</i>	<i>Material</i>	<i>Biomarker</i>	<i>Detection limit</i>	<i>Reference</i>
QCM-D/EIS	Gold	PSA	-	Formisano et al., 2014
EIS	Gold	PSA	1 ng/ml	Jolly et al., 2014
Optical	AuNPs	PSA	32 pg/ml	Chen et al., 2012
DPV/CV	AuNPs@GMCs	PSA	0.25 ng/ml	Liu et al., 2012
EIS	Gold	PSMA cells	-	Min et al., 2010

297

298

299 The first aptamer developed was a RNA aptamer (Jeong et al., 2010) that has been  
 300 used to demonstrate the recognition of active PSA. Following that, a DNA aptamer was  
 301 developed using a genetic algorithm with post-SELEX screening against PSA (Savory et al.,  
 302 2010). To date, there is no reported literature on the application of RNA aptamers for PSA  
 303 biosensing, which could be due to the long length of the sequence making it difficult to  
 304 synthesise commercially.


305

306 DNA based PSA aptamer has been combined with different sensing techniques with  
 307 sensitivities ranging from pg/ml to ng/ml. Chen et al. (2012) were the first to report the use of  
 308 PSA aptamer to develop an optical based aptasensor. The conjugation of gold nanoparticles  
 309 (AuNPs) with DNA aptamers were used to develop an aptasensor based on resonance light  
 310 scattering (RLS) spectral assay. The novel technique relied on changes in resonance light  
 311 scattering on binding of PSA to the aptamer, with a detection limit of 32 pg/ml. Thiolated  
 312 DNA aptamers were immobilized on AuNPs and then a blocking step with BSA was  
 313 performed prior the use of the complex AuNPs-aptamers with PSA samples. In this  
 314 configuration, the gold surface of the nanoparticles was covered by the flexible aptamer  
 315 structure and as a result no aggregation of particles occurred in absence of PSA. In the  
 316 presence of PSA, aptamer-PSA complexes were formed and the aptamers undergo a  
 conformational change in their structure from flexible to rigid. The changes in aptamer

317 conformation exposed some parts of the AuNPs that were thus available to form AuNPs  
 318 aggregates upon addition of potassium chloride. This resulted in an increase in the RLS  
 319 signal. The assay exhibited good sensitivity and selectivity towards PSA and tests made on  
 320 human blood samples showed results comparable to those obtained with ELISA (relative  
 321 deviation < 7%).

322

323

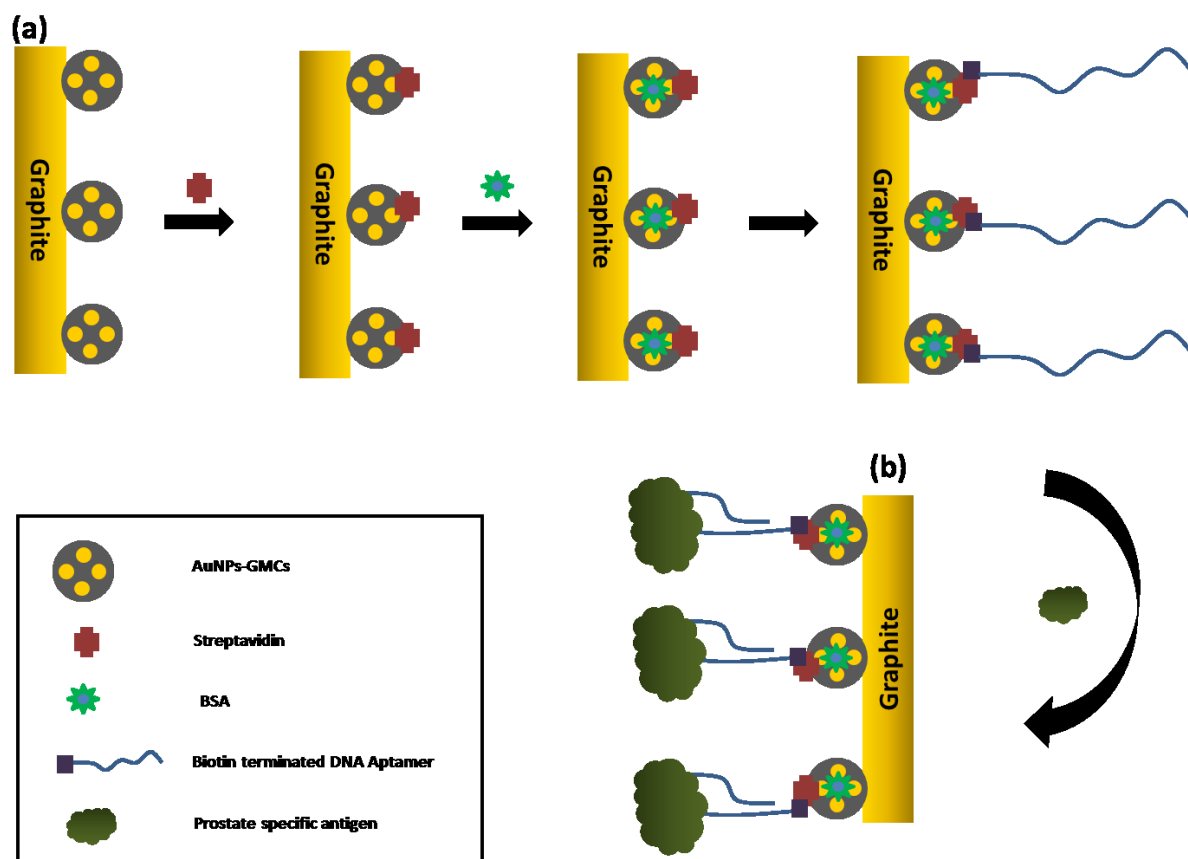

324

325

326 **Fig. 2.** Schematic illustration of fabrication process of the aptasensor based on gold  
 327 nanoparticles encapsulated by graphitized mesoporous carbon (a); PSA detection (b).  
 328 Adapted from Liu et al. (2012).

329

330


331 With regards to electrochemical aptasensor, modification of the electrode surface is  
 332 one of the biggest fields of investigation. Research is typically focused on finding the most  
 333 suitable recognition platform to give a stable organization to the sensor interface leading to  
 334 optimized binding efficiency and signal outcome (Lee et al., 2005; Putzbach & Ronkainen,  
 335 2013). Liu et al. (2012) applied aptasensors based on amplification via AuNPs and

336 graphitized mesoporous carbon (GMCs) combined with streptavidin-biotin system for  
337 electrochemical detection of PSA (see fig. 2). GMCs encapsulated AuNPs formed the first  
338 layer on cleaned pyrolytic graphite electrode followed by coating with streptavidin. All the  
339 non-specific sites were blocked with bovine serum albumin (BSA). Finally, biotinylated DNA  
340 aptamers were allowed to react with streptavidin immobilized on electrode surface. The  
341 fabricated aptasensor was then used to capture PSA which was measured via differential pulse  
342 voltammetry (DPV). The limit of detection of the aptasensor was 0.25 ng/ml with high  
343 specificity to PSA. In spite of high sensitivity and specificity, the fabrication procedure which  
344 is a layer-by-layer development of sensor surface is quite complex, which may be a drawback  
345 in fabricating a cost effective sensor. The group also used Electrochemical Impedance  
346 Spectroscopy (EIS) to characterize the layer-by-layer fabrication of the aptasensor.

347 Electrochemical Impedance Spectroscopy is one of the most promising  
348 electrochemical techniques for DNA-based approaches but requires a careful design in order  
349 to optimize its signal. Particularly important for EIS biosensors is the formation of a well-  
350 organized self-assembled monolayer (SAM) which allows an optimal charge transfer to occur.  
351 For successful EIS measurements, it is necessary to have a good and reliable SAM layer on  
352 the gold electrode surface. One of the most accepted approaches to achieve this goal is by  
353 alkanethiol chemistry. Alkanethiols can be easily adsorbed and form SAMs (Love et al.,  
354 2005) on a clean gold surface through thiol bonds (see fig. 3). It has been reported that longer  
355 alkane chains give a more compact structure with minimal defects (Campuzano et al., 2006).  
356 Among different configuration of SAM, a mixed SAM of 11-Mercaptoundecanoic acid  
357 (MUA),  $\text{HS}(\text{CH}_2)_{10}\text{COOH}$ , and 6-Mercapto-1-hexanol (MCH),  $\text{HS}(\text{CH}_2)_6\text{OH}$ , exhibited  
358 reasonable starting impedance values and improved reliability (Herne & Tarlov, 1997). In  
359 order to gather or to enhance the extent of a measurable signal of the recognition event  
360 occurring on the working electrode, marker molecules such as redox couples, are exploited.  
361 The recognition events that happen on the SAM not only modify the charge transfer processes  
362 between redox couples present in the measurement solution and the sensor surface but also  
363 affect the double layer at the sensor interface. Both these events cause a change in the system  
364 charge transfer resistance ( $R_{ct}$ ) which can then be measured by using an appropriate  
365 equivalent circuit.

366

367

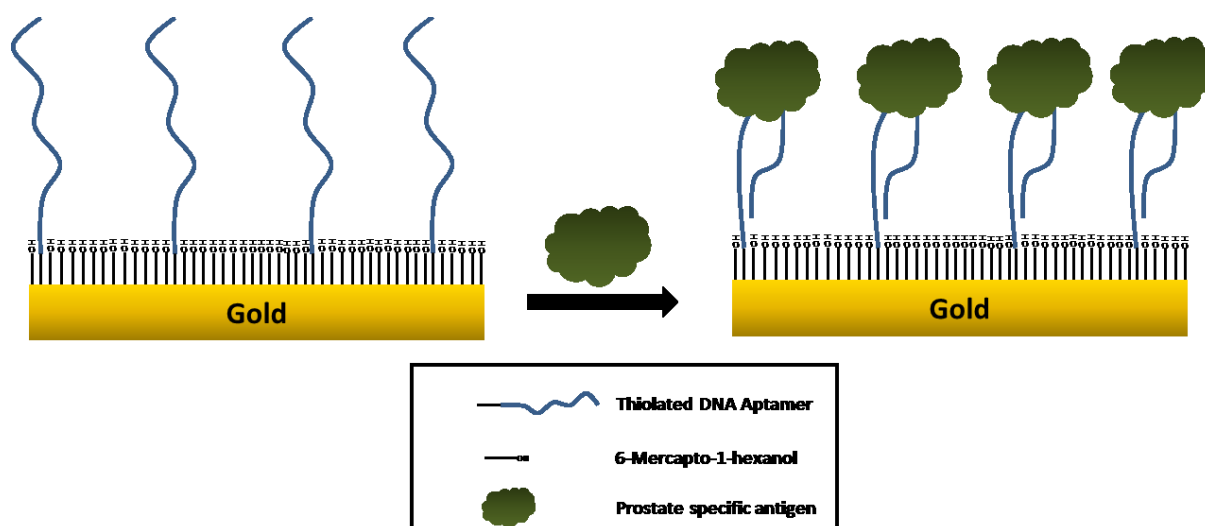

368

369

370 **Fig. 3.** Schematic illustration of fabrication process of the aptasensor with 6-mercaptohexanol  
 371 and thiolated DNA aptamer.

372


373

374 In EIS measurements using PSA aptamers, Jolly et al. (2014) and Formisano et al.  
 375 (2014) reported a reduction in charge transfer resistance ( $R_{ct}$ ) upon binding of PSA to the  
 376 immobilised DNA aptamers. This decrease is contradictory to what has been reported in the  
 377 literature for PSA where an increase of  $R_{ct}$  has been observed (Liu et al., 2012), even though  
 378 these studies used EIS mainly to characterize the bio-recognition layer and not for dose  
 379 response determination. A reduction of  $R_{ct}$  upon aptamer-analyte interaction has also been  
 380 reported for a different aptasensor using a lysozyme aptamer, where the reduction in charge  
 381 transfer resistance upon binding of lysozyme to its specific DNA aptamer was attributed  
 382 mainly due to screening of charges on DNA (Rodriguez et al., 2005). The reduction of  $R_{ct}$   
 383 could arise from two reasons: firstly, upon binding, PSA might screen the charges of the DNA  
 384 aptamer; secondly, as PSA is also a charged protein, it could be that more positive charges are  
 385 exposed because of the protein architecture itself. Consequently, as there is screening of  
 386 charges of DNA, there is a reduction on electrostatic barrier to the ferro/ferricyanide anions  
 387 towards the electrode surface, leading to lowering of the  $R_{ct}$  value of the system.

388 Earlier reports on DNA detection using DNA (Keighley et al., 2008a) and PNA probes  
 389 (Keighley et al., 2008b) have demonstrated the importance of optimization of the  
 390 oligonucleotide probe surface coverage in order to have efficient binding. On the same  
 391 grounds, Formisano et al. (2014) investigated for the first time the importance of optimization  
 392 of surface coverage by DNA aptamer for efficient binding using Quartz Crystal Microbalance

393 with Dissipation mode (QCM-D). The aim of this study was to optimize the conditions of an  
394 EIS aptamer-based sensor for PSA detection. In fact, EIS optimisation for DNA aptamers is  
395 somewhat complex due to the different characteristics that induce a signal change: namely  
396 DNA density, change in charge density close to the electrode upon DNA conformational  
397 changes, size and charge of the analyte, screening of DNA charges upon analyte binding. The  
398 use of QCM-D provided valuable information about conditions for maximum analyte binding  
399 as well as the hydration, folding and behaviour of the aptamer distribution on the electrode.  
400 The system comprised a gold surface functionalized with a mixed SAM made of DNA  
401 aptamer and MCH which was used as spacer molecule. The best conditions in terms of buffer  
402 solution and aptamer mole fraction (concentration of aptamers/total thiols) for the binding of  
403 PSA to the aptamers were obtained by comparing the data from two techniques under similar  
404 conditions. With regards to the buffer conditions, the study demonstrated how the DNA  
405 aptamers' behaviour exhibits a strong dependence on the environment where it interacts with  
406 PSA.


407 In order to investigate an optimum surface chemistry that not only has a good  
408 antifouling effect but is also simple and cost effective, a new molecule has been investigated  
409 by Jolly et al. (2014) as a spacer molecule replacing MCH: a thiol terminated sulfo-betaine  
410 (fig 4). It was the first report on thiol terminated sulfo-betaine application for aptamer-based  
411 sensor. Thiol terminated sulfo-betaine, which has a molecular mass of 398.6 g/mole, is a  
412 zwitter ion due to presence of both positive and negative charges with a flexible chain that  
413 makes it a good antifouling molecule (see Fig 5). It been reported that sulfo-betaine not only  
414 reduces non-specific binding but also increases the sensitivity of the sensor (Bertok et al.,  
415 2013).

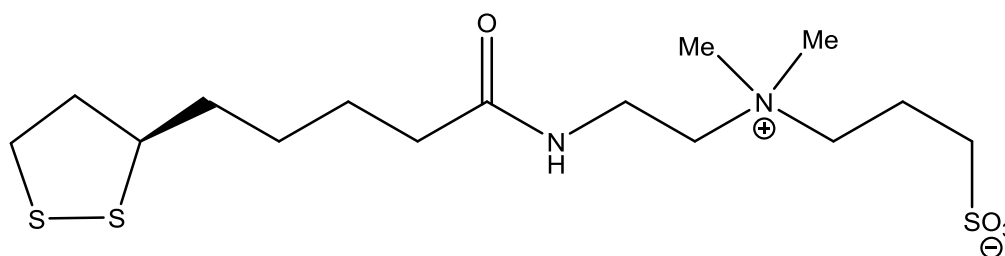

418  
419  
420 **Fig. 4.** Structure of thiol terminated sulfo-betaine. Image adapted from Bertok et al. (2013).

421

422

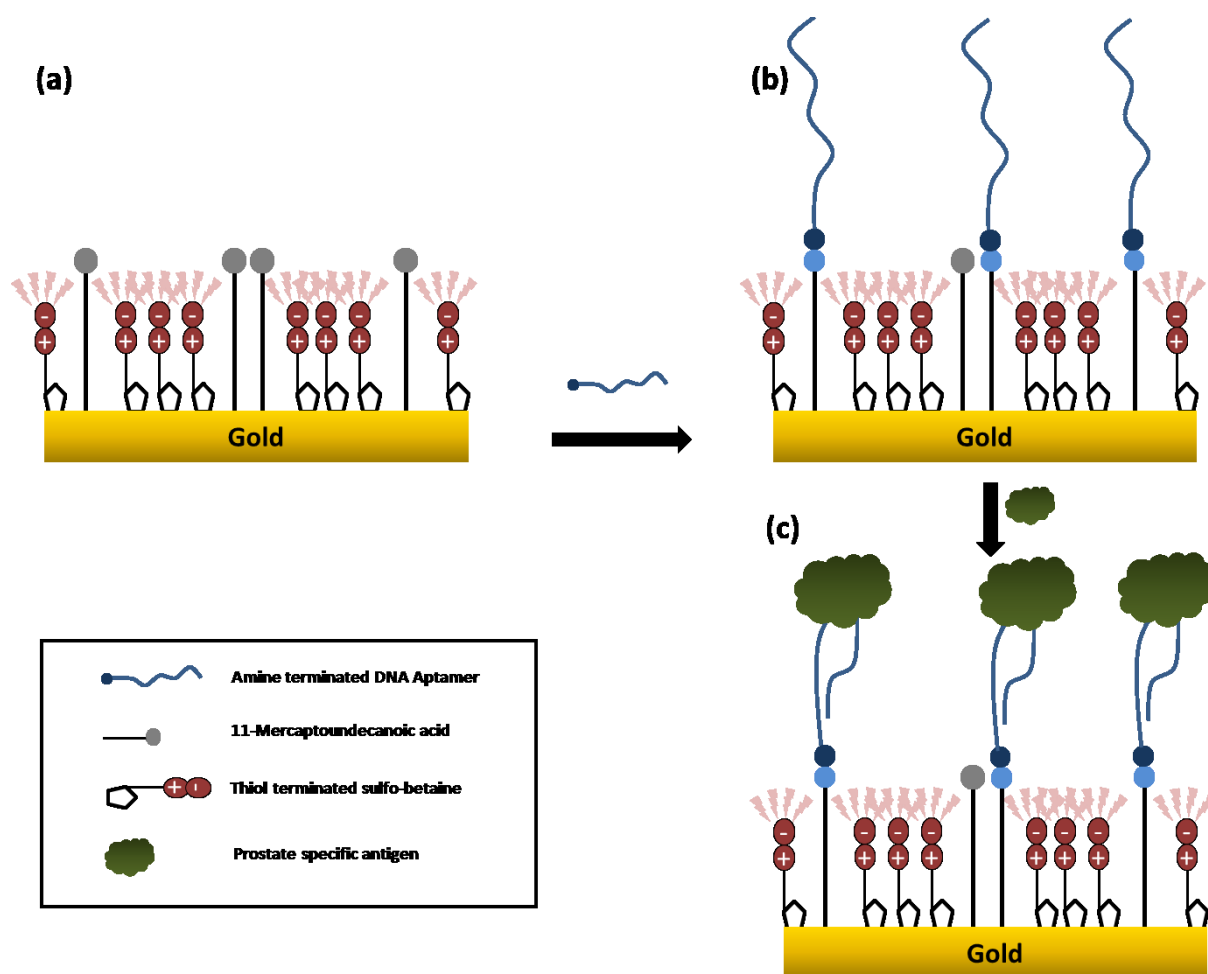

423

424

425 **Fig. 5.** Schematic of fabrication of thiol terminated sulfo-betaine based PSA aptasensor. (a)  
 426 First SAM layer by co-immobilizing 11-mercaptoundecanoic acid with thiol terminated  
 427 sulfo-betaine. Image adapted from Jolly et al. (2014).

428

429

430 A comparison study between MCH and thiol terminated sulfo-betaine thiol chemistry  
 431 was carried out by monitoring non-specific binding using human serum albumin (HSA) as a  
 432 control protein. A schematic of the fabrication protocol for surface chemistry with thiol  
 433 terminated sulfo-betaine is presented in fig 5. Co-immobilization of 11-mercaptoundecanoic  
 434 acid (MUA) and thiol terminated sulfo-betaine formed the first SAM layer on clean gold  
 435 electrodes. The carboxyl group of MUA was then activated with conventional EDC/NHS  
 436 coupling reaction. The activated carboxyl groups were then used to immobilize amine  
 437 terminated DNA aptamers for PSA and finally the electrodes were treated with ethanolamine  
 438 to deactivate all the unreacted groups. The fabricated aptasensor with thiol terminated sulfo-  
 439 betaine surface chemistry can discriminate PSA levels down to 1 ng/ml, which falls in the



440 lower clinical cut-off range of PSA in blood. The fabricated aptasensor with thiol terminated  
441 sulfo-betaine also showed a significant reduction of the non-specific binding with HSA as  
442 compared to the sensor where MCH was used instead as a spacer molecule. However, it has  
443 also been reported the obstacles on the optimization of the amount of DNA aptamers  
444 immobilized on the surface via EDC/NHS coupling. It was assumed that the charged thiol  
445 terminated sulfo-betaine has an influence on the attachment of DNA aptamer to activated  
446 MUA via EDC/NHS coupling leading to difference in amounts of DNA aptamers in different  
447 electrodes fabricated under similar conditions.

448

449

450

### **Aptasensors for other PCa biomarkers**

451

452 Besides PSA, other biomarkers for PCa are currently studied and can potentially be  
453 used for DNA/RNA-based detection systems. One is the prostate-specific membrane antigen  
454 (PSMA), which is a type II integral membrane glycoprotein found in human serum. It is  
455 overexpressed on prostate tumour cells and may play an important role in the progression of  
456 PCa. It can also differentiate between BPH and PCa (Feneley et al., 2000; Ghosh and Heston,  
457 2004; Madu and Lu, 2010; Pircher et al., 2011). Furthermore, by analysing the expression of  
458 PSMA, two cell lines can be distinguished among PCa cells: PSMA (-) and PSMA (+) cells  
459 (Ghosh and Heston, 2004). Min et al. (2010) reported on an RNA/peptide dual-aptamer-based  
460 biosensor able to detect both PSMA (-) and PSMA (+) cells by using EIS. The biosensor  
461 comprises of an anti-PSMA RNA aptamer (Lupold et al., 2002) which can target PSMA (+)  
462 cells and a DUP-1 peptide aptamer (Zitzmann et al., 2005) specific for PSMA (-) cells.

463 Another emerging biomarker is Alpha-methylacyl-CoA Racemase (AMACR), which  
464 is a racemase type of protein found in urine and blood. Its function is to metabolize fatty acids  
465 in the human body. It is also overexpressed in PCa and can be detected with a high sensitivity  
466 and specificity with a cut off value of 10.6 ng/ml. It also has the potential to differentiate  
467 between BPH and PCa. Currently AMACR aptamers have been independently developed by  
468 Base Pair Biotechnologies, Inc. (aptamer AM310\_2) and by Yang et al. (2013). However, no  
469 reports on their application to biosensing have been published so far.

470

471

472

### **Future perspectives and conclusions**

473

474 Recent work on the development of PSA aptasensors has enabled the transition from  
475 using antibody to aptamers as a recognition layer. Surface modification plays an important  
476 role in the development of promising biosensors which would be aided with the ongoing  
477 revolution in fabrication techniques. Easier fabrication would enable these biosensors to be  
478 mass produced and commercially viable. The inclination towards the development of  
479 aptasensors for PSA still needs further investigation for its use as an alternative to antibodies.  
480 Also, the sensitivity of an aptasensor is most likely to be influenced not only by the surface  
481 chemistry but also by the analytical method used for the detection of the target molecule, and  
482 so far no aptasensors have yet been used in complex samples such as blood. Overall, the  
483 development of aptamer based biosensor will see increasing reported literature because of its  
484 ease of synthesis and the possibilities of multiple modifications; it will always be a fresh field  
485 for more scope of adaptation of methodologies that will finally drive their solicitations with  
486 real blood samples. For early diagnosis of PCa, detection of different biomarkers would be  
487 preferred; consequently, more work is expected on development of aptamers for different  
488 isoforms of PSA and other biomarkers of PCa. An ideal biosensor for PCa detection would be  
489 based on a parallel sensing of different biomarkers using an array of sensors for more accurate  
490 diagnosis. In addition to the need for a simple surface chemistry, the scope of biosensor in  
491 future point-of-care devices will majorly depend on the integration of the format into a device  
492 that will enable easy and simple sample handling and an efficient read out system with rapid  
493 and accurate sample analysis of minimal blood sample volumes.

494

495

496 *Acknowledgement(s). This work was funded by the European Commission FP7*  
497 *Programme through the Marie Curie Initial Training Network PROSENSE (grant no.*  
498 *317420, 2012-2016).*

499

500

501

## References

502

503 Acevedo, B., Perera, Y., Ruiz, M., Rojas, G., Benítez, J., Ayala, M., & Gaviñondo, J. (2002).  
504 Development and validation of a quantitative ELISA for the measurement of PSA  
505 concentration. *Clinica Chimica Acta*, 317(1), 55-63. DOI: 10.1016/S0009-8981(01)00749-5.

- 506 Albrecht, S., Brandl, H., Steinke, M., & Freidt, T. (1994). Chemiluminescent enzyme  
507 immunoassay of prostate-specific antigen based on indoxyl phosphate substrate. *Clinical*  
508 *Chemistry*, 40(10), 1970-1971.
- 509 Andriole, G. L., Crawford, E. D., Grubb III, R. L., Buys, S. S., Chia, D., Church, T. R.,  
510 Fouad, M. N., Gelmann, E. P., Kvale, P. A., Reding, D. J., Weissfeld, J. L., Yokochi, L. A.,  
511 O'Brien, B., Clapp, J. D., Rathmell, J.M., Riley, T. L., Hayes, R. B., Kramer, B. S.,  
512 Izmirlan, G., Miller, A. B., Pinsky, P. F., Prorok, P. C., Gohagan, J. K., & Berg, C. D.  
513 (2009). Mortality results from a randomized prostate-cancer screening trial. *New England*  
514 *Journal of Medicine*, 360(13), 1310-1319. DOI: 10.1056/NEJMoa0810696.
- 515 Arya, S. K., & Bhansali, S. (2012). Anti-prostate specific antigen (anti-PSA) modified  
516 interdigitated microelectrode-based impedimetric biosensor for PSA detection. *Biosensors*  
517 *Journal 1*, H110601. DOI: 10.4303/BJ/H110601.
- 518 Aus, G., Ahlgren, G., Bergdahl, S., & Hugosson, J. (1996). Infection after transrectal core  
519 biopsies of the prostate. *British Journal of Urology*, 77(6), 851-855. DOI: 10.1046/j.1464-  
520 410X.1996.01014.x.
- 521 Balducci, L., Pow-Sang, J., Friedland, J., & Diaz, J. I. (1997). Prostate cancer. *Clinics in*  
522 *Geriatric Medicine*, 13(2), 283-306.
- 523 Balk, S. P., Ko, Y. J., & Bublely, G. J. (2003). Biology of prostate-specific antigen. *Journal of*  
524 *Clinical Oncology*, 21(2), 383-391. DOI:10.1200/JCO.2003.02.083.
- 525 Basler, J. W., & Thompson, I. M. (1998). Lest we abandon digital rectal examination as a  
526 screening test for prostate cancer. *Journal of the National Cancer Institute*, 90(23), 1761-  
527 1763. DOI: 10.1093/jnci/90.23.1761.
- 528 Bertok, T., Klukova, L., Sediva, A., Kasák, P., Semak, V., Micusik, M., Omastova, M.,  
529 Chovanová, L., Vlček, M., Imrich, R., Vikartovska, A., & Tkac, J. (2013). Ultrasensitive  
530 impedimetric lectin biosensors with efficient antifouling properties applied in glycoprofiling  
531 of human serum samples. *Analytical Chemistry*, 85(15), 7324-7332. DOI:  
532 10.1021/ac401281t.
- 533 Besselink, G. A. J., Kooyman, R. P. H., van Os, P. J., Engbers, G. H., & Schasfoort, R. B.  
534 (2004). Signal amplification on planar and gel-type sensor surfaces in surface plasmon  
535 resonance-based detection of prostate-specific antigen. *Analytical Biochemistry*, 333(1), 165-  
536 173. DOI: 10.1016/j.ab.2004.05.009.
- 537 Bostwick, D. G. (1989). The pathology of early prostate cancer. *CA: a Cancer Journal for*  
538 *Clinicians*, 39(6), 376-393. DOI: 10.3322/canjclin.39.6.376.

- 539 Campuzano, S., Pedrero, M., Montemayor, C., Fatás, E., & Pingarrón, J. M. (2006).  
540 Characterization of alkanethiol-self-assembled monolayers-modified gold electrodes by  
541 electrochemical impedance spectroscopy. *Journal of Electroanalytical Chemistry*, 586(1),  
542 112-121. DOI: 10.1016/j.jelechem.2005.09.007.
- 543 Cao, C., & Sim, S. J. (2007). Double-enhancement strategy: a practical approach to a femto-  
544 molar level detection of prostate specific antigen-alpha1-antichymotrypsin (PSA/ACT  
545 complex) for SPR immunosensing. *Journal of Microbiology and Biotechnology*, 17(6), 1031-  
546 1035.
- 547 Carter, H. B., Pearson, J. D., Metter, E. J., Brant, L. J., Chan, D. W., Andres, R., Fozard J. L.,  
548 & Walsh, P. C. (1992). Longitudinal evaluation of prostate-specific antigen levels in men  
549 with and without prostate disease. *Journal of the American Medical Association*, 267(16),  
550 2215.-2220. DOI: 10.1001/jama.267.16.2215.
- 551 Catalona, W. J., Smith, D. S., Ratliff, T. L., Dodds, K. M., Coplen, D. E., Yuan, J. J. J.,  
552 Petros, J. A., Andriole, G. L. (1991). Measurement of prostate-specific antigen in serum as a  
553 screening test for prostate cancer. *New England Journal of Medicine*, 324(17), 1156-1161.  
554 DOI: 10.1056/NEJM199104253241702.
- 555 Catalona, W. J., Partin, A. W., Slawin, K. M., Brawer, M. K., Flanigan, R. C., Patel, A.,  
556 Richie, J. P., deKernion J. B., Walsh, P. C., Scardino, P. T., Lange, P. H., Subong, E. N.,  
557 Parson, R. E., Gasior, G. H., Loveland, K. G., Southwick, P. C. (1998). Use of the  
558 percentage of free prostate-specific antigen to enhance differentiation of prostate cancer  
559 from benign prostatic disease: a prospective multicenter clinical trial. *Journal of the*  
560 *American Medical Association*, 279(19), 1542-1547. DOI: 10.1001/jama.279.19.1542.
- 561 Chen, Z., Lei, Y., Chen, X., Wang, Z., & Liu, J. (2012). An aptamer based resonance light  
562 scattering assay of prostate specific antigen. *Biosensors and Bioelectronics*, 36(1), 35-40.  
563 DOI: 10.1016/j.bios.2012.03.041.
- 564 Chikkaveeraiah, B. V.; Mani, V.; Patel, V.; Gutkind, J. S.; & Rusling, J. F. (2011).  
565 Microfluidic electrochemical immunoarray for ultrasensitive detection of two cancer  
566 biomarker proteins in serum. *Biosensors and Bioelectronics*, 26(11), 4477-4483. DOI:  
567 10.1016/j.bios.2011.05.005.
- 568 Chiriaco, M. S., Primiceri, E., Montanaro, A., de Feo, F., Leone, L., Rinaldi, R., & Maruccio,  
569 G. (2013). On-chip screening for prostate cancer: an EIS microfluidic platform for  
570 contemporary detection of free and total PSA. *Analyst*, 138(18), 5404-5410. DOI:  
571 10.1039/c3an00911d.

- 572 Cho, E. J., Lee, J. W., & Ellington, A. D. (2009). Applications of aptamers as sensors. *Annual*  
573 *Review of Analytical Chemistry*, 2, 241-264. DOI:  
574 10.1146/annurev.anchem.1.031207.112851.
- 575 Chornokur, G., Arya, S. K., Phelan, C., Tanner, R., & Bhansali, S. (2011). Impedance-based  
576 miniaturized biosensor for ultrasensitive and fast prostate-specific antigen detection. *Journal*  
577 *of Sensors*, 2011, 983752. DOI: 10.1155/2011/983752.
- 578 Chou, E., & Simons, J. W. (1997). The molecular biology of prostate cancer morbidity and  
579 mortality: accelerated death from ejaculate poisoning? *Urologic Oncology: Seminars and*  
580 *Original Investigations*, 3(3), 79-84. DOI: 10.1016/S1078-1439(97)00041-0.
- 581 Christensson, A. S., Björk, T., Nilsson, O., Dahlén, U., Matikainen, M. T., Cockett, A. T.,  
582 Abrahamsson P. A., Lilja, H. (1993). Serum prostate specific antigen complexed to alpha 1-  
583 antichymotrypsin as an indicator of prostate cancer. *Journal of Urology*, 150(1), 100.
- 584 Clark, S. L., & Remcho, V. T. (2002). Aptamers as analytical reagents. *Electrophoresis*,  
585 23(9), 1335-1340. DOI: 10.1002/1522-2683(200205)23:9<1335::AID-ELPS1335>3.0.CO;2-  
586 E.
- 587 D'Amico, A. V., Chen, M. H., Roehl, K. A., & Catalona, W. J. (2004). Preoperative PSA  
588 velocity and the risk of death from prostate cancer after radical prostatectomy. *New England*  
589 *Journal of Medicine*, 351(2), 125-135. DOI: 10.1056/NEJMoa032975.
- 590 D'Amico, A. V., Renshaw, A. A., Sussman, B., & Chen, M. H. (2005). Pretreatment PSA  
591 velocity and risk of death from prostate cancer following external beam radiation therapy.  
592 *Journal of the American Medical Association*, 294(4), 440-447. DOI:  
593 10.1001/jama.294.4.440.
- 594 Feneley, M. R., Jan, H., Granowska, M., Mather, S. J., Ellison, D., Glass, J., Coptcoat, M.,  
595 Kirby, R. S., Ogden, C., Oliver, R. T. D., Badenoch, D. F., Chinegwundoh, F. I., Nargund,  
596 V. H., Paris, A. M. I., & Britton, K. E. (2000). Imaging with prostate-specific membrane  
597 antigen (PSMA) in prostate cancer. *Prostate Cancer and Prostatic Diseases*, 3(1), 47-52.  
598 DOI: 10.1038/sj.pcan.4500390.
- 599 Feng, K., Sun, C., Kang, Y., Chen, J., Jiang, J. H., Shen, G. L., & Yu, R. Q. (2008). Label-  
600 free electrochemical detection of nanomolar adenosine based on target-induced aptamer  
601 displacement. *Electrochemistry Communications*, 10(4), 531-535.  
602 DOI:10.1016/j.elecom.2008.01.024.
- 603 Fernández-Sánchez, C., McNeil, C. J., Rawson, K., & Nilsson, O. (2004). Disposable  
604 noncompetitive immunosensor for free and total prostate-specific antigen based on

- 605 capacitance measurement. *Analytical Chemistry*, 76(19), 5649-5656. DOI:  
606 10.1021/ac0494937.
- 607 Formisano, N., Jolly, P., Cromhout, M., Fogel, R., Limson, J. L., & Estrela, P. (2014).  
608 Optimisation of an electrochemical impedance spectroscopy aptasensor by exploiting quartz  
609 crystal microbalance with dissipation signals. *Submitted for publication*.
- 610 Ghosh, A., & Heston, W. D. W. (2004). Tumor target prostate specific membrane antigen  
611 (PSMA) and its regulation in prostate cancer. *Journal of Cellular Biochemistry*, 91(3), 528-  
612 539. DOI: 10.1002/jcb.10661.
- 613 Greenlee, R. T., Murray, T., Bolden, S., & Wingo, P. A. (2000). Cancer statistics, 2000. *CA: a*  
614 *Cancer Journal for Clinicians*, 50(1), 7-33. DOI: 10.3322/canjclin.50.1.7.
- 615 Grossklaus, D. J., Smith Jr, J. A., Shappell, S. B., Coffey, C. S., Chang, S. S., & Cookson, M.  
616 S. (2002). The free/total prostate-specific antigen ratio (% fPSA) is the best predictor of  
617 tumor involvement in the radical prostatectomy specimen among men with an elevated PSA.  
618 *Urologic Oncology: Seminars and Original Investigations*, 7(5), 195-198. DOI:  
619 10.1016/S1078-1439(02)00190-4.
- 620 Healy, D. A., Hayes, C. J., Leonard, P., McKenna, L., & O'Kennedy, R. (2007). Biosensor  
621 developments: application to prostate-specific antigen detection. *Trends in Biotechnology*,  
622 25(3), 125-131. DOI: 10.1016/j.tibtech.2007.01.004.
- 623 Hermann, T., & Patel, D. J. (2000). Adaptive recognition by nucleic acid aptamers. *Science*,  
624 287(5454), 820-825. DOI: 10.1126/science.287.5454.
- 625 Herne, T. M., & Tarlov, M. J. (1997). Characterization of DNA probes immobilized on gold  
626 surfaces. *Journal of the American Chemical Society*, 119(38), 8916-8920. DOI:  
627 10.1021/ja9719586.
- 628 Hianik, T., & Wang, J. (2009). Electrochemical aptasensors—recent achievements and  
629 perspectives. *Electroanalysis*, 21(11), 1223-1235. DOI: 10.1002/elan.200904566.
- 630 Hoffman, R. M. (2011). Screening for prostate cancer. *New England Journal of Medicine*,  
631 365(21), 2013-2019. DOI: 10.1056/NEJMcp1103642.
- 632 Huang, L., Reekmans, G., Saerens, D., Friedt, J. M., Frederix, F., Francis, L., Muyldermans,  
633 S., Campitelli, A., & Van Hoof, C. (2005). Prostate-specific antigen immunosensing based  
634 on mixed self-assembled monolayers, camel antibodies and colloidal gold enhanced  
635 sandwich assays. *Biosensors and Bioelectronics*, 21(3), 483-490.  
636 DOI:10.1016/j.bios.2004.11.016.
- 637 Huang, Y. W., Wu, C. S., Chuang, C. K., Pang, S. T., Pan, T. M., Yang, Y. S., & Ko, F. H.  
638 (2013). Real-time and label-free detection of the prostate-specific antigen in human serum

- 639 by a polycrystalline silicon nanowire field-effect transistor biosensor. *Analytical Chemistry*,  
640 85(16), 7912-7918. DOI: 10.1021/ac401610s.
- 641 Ikebukuro, K., Kiyohara, C., & Sode, K. (2005). Novel electrochemical sensor system for  
642 protein using the aptamers in sandwich manner. *Biosensors and Bioelectronics*, 20(10),  
643 2168-2172. DOI: 10.1016/j.bios.2004.09.002.
- 644 Iliuk, A. B., Hu, L., & Tao, W. A. (2011). Aptamer in bioanalytical applications. *Analytical*  
645 *Chemistry*, 83(12), 4440-4452. DOI: 10.1021/ac201057w.
- 646 Irani, J., Fournier, F., Bon, D., Gremmo, E., Dore, B., & Aubert, J. (1997). Patient tolerance  
647 of transrectal ultrasound-guided biopsy of the prostate. *British journal of urology*, 79(4),  
648 608-610. DOI: 10.1046/j.1464-410X.1997.00120.x.
- 649 Jeong, S., Han, S. R., Lee, Y. J., & Lee, S. W. (2010). Selection of RNA aptamers specific to  
650 active prostate-specific antigen. *Biotechnology letters*, 32(3), 379-385. DOI:  
651 10.1007/s10529-009-0168-1.
- 652 Jiang, Z., Fanger, G. R., Woda, B. A., Banner, B. F., Algate, P., Dresser, K., Xu, J., & Chu, P.  
653 G. (2003). Expression of  $\alpha$ -methylacyl-CoA racemase (p504s) in various malignant  
654 neoplasms and normal tissues: a study of 761 cases. *Human Pathology*, 34(8), 792-796.  
655 DOI: 10.1016/S0046-8177(03)00268-5.
- 656 Jolly, P., Formisano, N., Tkáč, J., Kasák, P., Frost, C. G., & Estrela, P. (2014). Label-free  
657 impedimetric prostate cancer aptasensor with antifouling surface chemistry. *Submitted for*  
658 *publication*.
- 659 Keighley, S. D., Li, P., Estrela, P., & Migliorato, P. (2008a). Optimization of DNA  
660 immobilization on gold electrodes for label-free detection by electrochemical impedance  
661 spectroscopy. *Biosensors and Bioelectronics*, 23(8), 1291-1297. DOI:  
662 10.1016/j.bios.2007.11.012.
- 663 Keighley, S. D., Estrela, P., Li, P., & Migliorato, P. (2008b). Optimization of label-free DNA  
664 detection with electrochemical impedance spectroscopy using PNA probes. *Biosensors and*  
665 *Bioelectronics*, 24(4), 906-911. DOI: 10.1016/j.bios.2008.07.041.
- 666 Kirk, D. (1997). MRC study: when to commence treatment in advanced prostate cancer.  
667 *Prostate Cancer & Prostatic Diseases*, 1(1), 11-15.
- 668 Kufe, D. W., Pollock, R. E., Weichselbaum, R. R., Bast, R. C., & Gansler, T. S. (2003).  
669 *Holland-Frei cancer medicine*: BC Decker Hamilton, ON.
- 670 Lee, J. W., Sim, S. J., Cho, S. M., & Lee, J. (2005). Characterization of a self-assembled  
671 monolayer of thiol on a gold surface and the fabrication of a biosensor chip based on surface

- 672 plasmon resonance for detecting anti-GAD antibody. *Biosensors and Bioelectronics*, 20(7),  
673 1422-1427. DOI: 10.1016/j.bios.2004.04.017.
- 674 Leman, E. S., & Getzenberg, R. H. (2009). Biomarkers for prostate cancer. *Journal of*  
675 *Cellular Biochemistry*, 108(1), 3-9. DOI: 10.1002/jcb.22227.
- 676 Li, C., Curreli, M., Lin, H., Lei, B., Ishikawa, F. N., Datar, R., Cote, R. J., Thompson, M. E.,  
677 & Zhou, C. (2005). Complementary detection of prostate-specific antigen using In<sub>2</sub>O<sub>3</sub>  
678 nanowires and carbon nanotubes. *Journal of the American Chemical Society*, 127(36),  
679 12484-12485. DOI: 10.1021/ja053761g.
- 680 Lilja, H., Oldbring, J., Rannevik, G., & Laurell, C. B. (1987). Seminal vesicle-secreted  
681 proteins and their reactions during gelation and liquefaction of human semen. *Journal of*  
682 *Clinical Investigation*, 80(2), 281. DOI: 10.1172/JCI113070.
- 683 Lilja, H., Ulmert, D., & Vickers, A. J. (2008). Prostate-specific antigen and prostate cancer:  
684 prediction, detection and monitoring. *Nature Reviews Cancer*, 8(4), 268-278. DOI:  
685 10.1038/nrc2351.
- 686 Lim, Y. C., Kouzani, A. Z., & Duan, W. (2009). Aptasensors design considerations  
687 *Computational intelligence and intelligent systems* (pp. 118-127): Springer. DOI:  
688 10.1007/978-3-642-04962-0\_14.
- 689 Lin, J., & Ju, H. (2005). Electrochemical and chemiluminescent immunosensors for tumor  
690 markers. *Biosensors and Bioelectronics*, 20(8), 1461-1470. DOI:  
691 10.1016/j.bios.2004.05.008.
- 692 Liu, B., Lu, L., Hua, E., Jiang, S., & Xie, G. (2012). Detection of the human prostate-specific  
693 antigen using an aptasensor with gold nanoparticles encapsulated by graphitized mesoporous  
694 carbon. *Microchimica Acta*, 178(1-2), 163-170. DOI: 10.1007/s00604-012-0822-5.
- 695 Liu, J., Lu, C. Y., Zhou, H., Xu, J. J., Wang, Z. H., & Chen, H. Y. (2013). A dual-functional  
696 electrochemical biosensor for the detection of prostate specific antigen and telomerase  
697 activity. *Chemical Communications*, 49(59), 6602-6604. DOI: 10.1039/C3CC43532F.
- 698 Loeb, S., & Catalona, W. J. (2007). Prostate-specific antigen in clinical practice. *Cancer*  
699 *Letters*, 249(1), 30-39. DOI: 10.1016/j.canlet.2006.12.022.
- 700 Loeb, S., Vellekoop, A., Ahmed, H. U., Catto, J., Emberton, M., Nam, R., Rosario, D. J., &  
701 Lotan, Y. (2013). Systematic review of complications of prostate biopsy. *European Urology*  
702 64(6), 876-92. DOI: 10.1016/j.eururo.2013.05.049.
- 703 Love, J. C., Estroff, L. A., Kriebel, J. K., Nuzzo, R. G., & Whitesides, G. M. (2005). Self-  
704 assembled monolayers of thiolates on metals as a form of nanotechnology. *Chemical*  
705 *Reviews*, 105(4), 1103-1170. DOI:10.1021/cr0300789.



- 706 Lövgren, J., Valtonen-André, C., Marsal, K., Liua, H., & Lundwall, Å. (1999). Measurement  
707 of prostate-specific antigen and human glandular kallikrein 2 in different body fluids.  
708 *Journal of Andrology*, 20(3), 348-355. DOI: 10.1002/j.1939-4640.1999.tb02528.x.
- 709 Lupold, S. E., Hicke, B. J., Lin, Y., & Coffey, D. S. (2002). Identification and characterization  
710 of nuclease-stabilized RNA molecules that bind human prostate cancer cells via the prostate-  
711 specific membrane antigen. *Cancer Research*, 62, 4029-4033.
- 712 Madu, C. O., & Lu, Y. (2010). Novel diagnostic biomarkers for prostate cancer. *Journal of*  
713 *Cancer*, 1, 150-177. DOI: 10.7150/jca.1.150.
- 714 Mairal, T., Özalp, V. C., Lozano Sánchez, P., Mir, M., Katakis, I., & O'Sullivan, C. K.  
715 (2008). Aptamers: molecular tools for analytical applications. *Analytical and Bioanalytical*  
716 *Chemistry*, 390(4), 989-1007. DOI: 10.1007/s00216-007-1346-4.
- 717 Mani, V., Chikkaveeraiah, B. V., Patel, V., Gutkind, J. S., & Rusling, J. F. (2009).  
718 Ultrasensitive immunosensor for cancer biomarker proteins using gold nanoparticle film  
719 electrodes and multienzyme-particle amplification. *ACS Nano*, 3(3), 585-594. DOI:  
720 10.1021/nn800863w.
- 721 Maraldo, D., Garcia, F. U., & Mutharasan, R. (2007). Method for quantification of a prostate  
722 cancer biomarker in urine without sample preparation. *Analytical Chemistry*, 79(20), 7683-  
723 7690. DOI: 10.1021/ac070895z.
- 724 Melichar, B. (2012). Tumor biomarkers: PSA and beyond. *Clinical Chemistry and*  
725 *Laboratory Medicine*, 50(11), 1865-1869. DOI: 10.1515/cclm-2012-0631.
- 726 Mikolajczyk, S. D., Marker, K. M., Millar, L. S., Kumar, A., Saedi, M. S., Payne, J. K.,  
727 Evans, C. L., Gasoir, C. L., Linton, H. J., Carpenter, P., & Rittenhouse, H. G. (2001). A  
728 truncated precursor form of prostate-specific antigen is a more specific serum marker of  
729 prostate cancer. *Cancer Research*, 61(18), 6958-6963.
- 730 Mikolajczyk, S. D., Catalona, W. J., Evans, C. L., Linton, H. J., Millar, L. S., Marker, K. M.,  
731 Katir, D., Amirkhan, A., & Rittenhouse, H. G. (2004). Proenzyme forms of prostate-specific  
732 antigen in serum improve the detection of prostate cancer. *Clinical Chemistry*, 50(6), 1017-  
733 1025. DOI: 10.1373/clinchem.2003.026823.
- 734 Min, K., Song, K. M., Cho, M., Chun, Y. S., Shim, Y. B., Ku, J. K., & Ban, C. (2010).  
735 Simultaneous electrochemical detection of both PSMA (+) and PSMA (-) prostate cancer  
736 cells using an RNA/peptide dual-aptamer probe. *Chemical Communications*, 46, 5566-  
737 5568. DOI: 10.1039/c002524k.

- 738 Moyer, V. A. (2012). Screening for prostate cancer: US Preventive Services Task Force  
739 recommendation statement. *Annals of internal medicine*, *157*(2), 120-134. DOI:  
740 10.7326/0003-4819-157-2-201207170-00459.
- 741 Numnuam, A., Chumbimuni-Torres, K. Y., Xiang, Y., Bash, R., Thavarungkul, P.,  
742 Kanatharana, P., Pretsch, E., Wang, J., & Bakker, E. (2008). Aptamer-based potentiometric  
743 measurements of proteins using ion-selective microelectrodes. *Analytical Chemistry*, *80*(3),  
744 707-712. DOI: 10.1021/ac701910r.
- 745 Ohori, M., Dunn, J. K., & Scardino, P. T. (1995). Is prostate-specific antigen density more  
746 useful than prostate-specific antigen levels in the diagnosis of prostate-cancer? *Urology*,  
747 *46*(5), 666-671. DOI: 10.1016/s0090-4295(99)80298-2.
- 748 Okuno, J., Maehashi, K., Kerman, K., Takamura, Y., Matsumoto, K., & Tamiya, E. (2007).  
749 Label-free immunosensor for prostate-specific antigen based on single-walled carbon  
750 nanotube array-modified microelectrodes. *Biosensors and Bioelectronics*, *22*(9-10), 2377-  
751 2381. DOI: 10.1016/j.bios.2006.09.038.
- 752 Panini, N. V., Messina, G. A., Salinas, E., Fernández, H., & Raba, J. (2008). Integrated  
753 microfluidic systems with an immunosensor modified with carbon nanotubes for detection  
754 of prostate specific antigen (PSA) in human serum samples. *Biosensors and Bioelectronics*,  
755 *23*(7), 1145-1151. DOI: 10.1016/j.bios.2007.11.003.
- 756 Pinsky, P. F., Andriole, G., Crawford, E. D., Chia, D., Kramer, B. S., Grubb, R., Greenlee, R.,  
757 & Gohagan, J. K. (2007). Prostate-specific antigen velocity and prostate cancer gleason  
758 grade and stage. *Cancer*, *109*(8), 1689-1695. DOI: 10.1002/cncr.22558.
- 759 Pircher, A., Hilbe, W., Heidegger, I., Drevs, J., Tichelli, A., & Medinger, M. (2011).  
760 Biomarkers in tumor angiogenesis and anti-angiogenic therapy. *International Journal of*  
761 *Molecular Sciences*, *12*(10), 7077-7099. DOI: 10.3390/ijms12107077.
- 762 Putzbach, W., & Ronkainen, N. J. (2013). Immobilization techniques in the fabrication of  
763 nanomaterial-based electrochemical biosensors: a review. *Sensors*, *13*(4), 4811-4840.  
764 DOI:10.3390/s130404811.
- 765 Rodriguez, M. C., Kawde, A. N., & Wang, J. (2005). Aptamer biosensor for label-free  
766 impedance spectroscopy detection of proteins based on recognition-induced switching of the  
767 surface charge. *Chemical Communications*, (34), 4267-4269. DOI: 10.1039/B506571B.
- 768 Ross, R. K., Pike, M. C., Coetzee, G. A., Reichardt, J. K. V., Yu, M. C., Feigelson, H.,  
769 Stanczyk, F. Z., Kolonel, L. N., & Henderson, B. E. (1998). Androgen metabolism and  
770 prostate cancer: establishing a model of genetic susceptibility. *Cancer Research*, *58*(20),  
771 4497-4504.

- 772 Rubin, M. A., Zhou, M., Dhanasekaran, S. M., Varambally, S., Barrette, T. R., Sanda, M. G.,  
773 Pienta, K. J., Ghosh, D., & Chinnaiyan, A. M. (2002).  $\alpha$ -methylacyl coenzyme A racemase  
774 as a tissue biomarker for prostate cancer. *Journal of the American Medical Association*,  
775 287(13), 1662-1670. DOI: 10.1001/jama.287.13.1662.
- 776 Sardesai, N. P., Barron, J. C., & Rusling, J. F. (2011). *Analytical Chemistry*, 83(17), 6698-  
777 6703. DOI: 10.1021/ac201292q.
- 778 Sarkar, P., Pal, P. S., Ghosh, D., Setford, S. J., & Tothill, I. E. (2002). Amperometric  
779 biosensors for detection of the prostate cancer marker (PSA). *International Journal of*  
780 *Pharmaceutics*, 238(1), 1-9. DOI: 10.1016/S0378-5173(02)00015-7.
- 781 Savory, N., Abe, K., Sode, K., & Ikebukuro, K. (2010). Selection of DNA aptamer against  
782 prostate specific antigen using a genetic algorithm and application to sensing. *Biosensors*  
783 *and Bioelectronics*, 26(4), 1386-1391. DOI: 10.1016/j.bios.2010.07.057.
- 784 Seto, Y., Iba, T., & Abe, K. (2001). Development of ultra-high sensitivity bioluminescent  
785 enzyme immunoassay for prostate-specific antigen (PSA) using firefly luciferase.  
786 *Luminescence*, 16(4), 285-290. DOI: 10.1002/bio.654.
- 787 Song, S., Wang, L., Li, J., Fan, C., & Zhao, J. (2008). Aptamer-based biosensors. *Trends in*  
788 *Analytical Chemistry*, 27(2), 108-117. DOI: 10.1016/j.trac.2007.12.004.
- 789 Stamey, T. A., Yang, N., Hay, A. R., McNeal, J. E., Freiha, F. S., & Redwine, E. (1987).  
790 Prostate-specific antigen as a serum marker for adenocarcinoma of the prostate. *New*  
791 *England Journal of Medicine*, 317(15), 909-916. DOI: 10.1056/nejm198710083171501.
- 792 Stanford, J. L., Stephenson, R. A., Coyle, L. M., Cerhan, J., Correa, R., Eley, J. W., Gilliland,  
793 F., Hankey, B., Kolonel, L. N., Kosary, C., Ross, R., Severson, R., & West, D. (1999).  
794 Prostate cancer trends 1973-1995, SEER Program, National Cancer Institute. *NIH pub 99-*  
795 4543.
- 796 Stephan, C., Lein, M., Jung, K., Schnorr, D., & Loening, S. A. (1997). The influence of  
797 prostate volume on the ratio of free to total prostate specific antigen in serum of patients  
798 with prostate carcinoma and benign prostate hyperplasia. *Cancer*, 79(1), 104-109. DOI:  
799 10.1002/(SICI)1097-0142(19970101)79:1<104::AID-CNCR15>3.0.CO;2-8.
- 800 Syed, M. A., & Pervaiz, S. (2010). Advances in aptamers. *Oligonucleotides*, 20(5), 215-224.  
801 DOI: 10.1089/oli.2010.0234.
- 802 Takayama, T. K., Fujikawa, K., & Davie, E. W. (1997). Characterization of the precursor of  
803 prostate-specific antigen Activation by trypsin and by human glandular kallikrein. *Journal of*  
804 *Biological Chemistry*, 272(34), 21582-21588. DOI: 10.1074/jbc.272.34.21582.

- 805 Tombelli, S., Minunni, M., & Mascini, M. (2005). Analytical applications of aptamers.  
806 *Biosensors and Bioelectronics*, 20(12), 2424-2434. DOI: 10.1016/j.bios.2004.11.006.
- 807 Uzzo, R. G., Wei, J. T., Waldbaum, R. S., Perlmutter, A. P., Byrne, J. C., & Vaughan Jr., D.  
808 (1995). The influence of prostate size on cancer detection. *Urology*, 46(6), 831-836. DOI:  
809 10.1016/S0090-4295(99)80353-7.
- 810 Velonas, V. M., Woo, H. H., dos Remedios, C. G., & Assinder, S. J. (2013). Current status of  
811 biomarkers for prostate cancer. *International Journal of Molecular Sciences*, 14(6), 11034-  
812 11060. DOI: 10.3390/ijms140611034.
- 813 Wang, X., Zhou, J., Yun, W., Xiao, S., Chang, Z., He, P., & Fang, Y. (2007). Detection of  
814 thrombin using electrogenerated chemiluminescence based on Ru (bpy)<sub>3</sub><sup>2+</sup>-doped silica  
815 nanoparticle aptasensor via target protein-induced strand displacement. *Analytica Chimica*  
816 *Acta*, 598(2), 242-248. DOI: 10.1016/j.aca.2007.07.050.
- 817 Wee, K. W., Kang, G. Y., Park, J., Kang, J. Y., Yoon, D. S., Park, J. H., & Kim, T. S. (2005).  
818 Novel electrical detection of label-free disease marker proteins using piezoresistive self-  
819 sensing micro-cantilevers. *Biosensors and Bioelectronics*, 20(10), 1932-1938. DOI:  
820 10.1016/j.bios.2004.09.023.
- 821 Weeks, B. L., Camarero, J., Noy, A., Miller, A. E., De Yoreo, J. J., & Stanker, L. (2003). A  
822 microcantilever-based pathogen detector. *Scanning*, 25(6), 297-299. DOI:  
823 10.1002/sca.4950250605.
- 824 Wu, C. L., Yang, X. J., Tretiakova, M., Patton, K. T., Halpern, E. F., Woda, B. A., Young, R.  
825 H., & Jiang, Z. (2004). Analysis of  $\alpha$ -methylacyl-CoA racemase (P504S) expression in high-  
826 grade prostatic intraepithelial neoplasia. *Human Pathology*, 35(8), 1008-1013, 8. DOI:  
827 10.1016/j.humpath.2004.03.019.
- 828 Willner, I., & Zayats, M. (2007). Electronic aptamer-based sensors. *Angewandte Chemie -*  
829 *International Edition*, 46(34), 6408-6418. DOI: 10.1002/anie.200604524.
- 830 Xiao, Y., Lubin, A. A., Heeger, A. J., & Plaxco, K. W. (2005). Label-free electronic detection  
831 of thrombin in blood serum by using an aptamer-based sensor. *Angewandte Chemie*,  
832 117(34), 5592-5595. DOI: 10.1002/ange.200500989.
- 833 Xu, D., Xu, D., Yu, X., Liu, Z., He, W., & Ma, Z. (2005). Label-free electrochemical  
834 detection for aptamer-based array electrodes. *Analytical Chemistry*, 77(16), 5107-5113. DOI:  
835 10.1021/ac050192m.
- 836 Yang, D. K., Chen, C. S., & Chen, L. C. (2013). Screening of functional aptamers against  
837  $\alpha$ -methylacyl-coA racemase. In Abstracts of the 13th American Institute of Chemical

838 Engineers Annual Meeting, November 3–8, 2013. Retrieved May 9, 2014, from  
839 <https://aiche.confex.com/aiche/2013/webprogram/Paper332288.html>.

840 Zani, A.; Laschi, S.; Mascini, M.; & Marrazza, G. (2011). A new electrochemical multiplexed  
841 assay for PSA cancer marker detection. *Electroanalysis*, 23(1), 91-99. DOI:  
842 10.1002/elan.201000486.

843 Zitzmann, S., Mier, W., Schad, A., Kinscherf, R., Askozyllakis, V., Krämer, S., Altmann, A.,  
844 Eisenhut, M., & Haberkorn, U. (2005). A new prostate carcinoma binding peptide (DUP-1)  
845 for tumor imaging and therapy. *Clinical Cancer Research*, 11, 139-146.

846