

Technical University of Denmark



Inorganic arsenic - SPE HG-AAS method for RICE tested in-house and collaboratively

Rasmussen, Rie Romme; Qian, Yiting; Sloth, Jens Jørgen

Publication date:
2013

Document Version
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

Citation (APA):
Rasmussen, R. R., Qian, Y., & Sloth, J. J. (2013). Inorganic arsenic - SPE HG-AAS method for RICE tested in-house and collaboratively. Poster session presented at 67th Annual Meeting of the Nordic Committee on Food Analysis (NMKL), Kalmar, Sweden.

DTU Library
Technical Information Center of Denmark

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

INORGANIC ARSENIC

SPE HG-AAS METHOD FOR RICE TESTED IN-HOUSE AND COLLABORATIVELY



INTRODUCTION

Internationally accepted validated method(s) are needed for establishment of a maximum level (ML) for inorganic arsenic (iAs) in rice as recently emphasised by the European Food Safety Authority (2009), the World Health Organization (2011) and Codex Alimentarius (2012).

Rice contains most often three forms of the trace element arsenic; iAs and the methylated species monomethylarsonic acid (MA^V) and dimethylarsinic acid (DMA^V). Dietary intake of iAs is of special concern due to its carcinogenicity to humans, whereas DMA and MA are generally considered of less toxicological importance.


CONCLUSION

The presented SPE HG-AAS method enables selective determination of inorganic arsenic in rice by use of inexpensive instrumentation (HG-AAS) and is a **candidate method for future control** of the inorganic arsenic content in rice and rice products.

VALIDATION RESULTS

The developed method was subjected to an **in-house validation study**, which gave satisfying figures of merit (Table 1). The LOD (0.02 mg·kg⁻¹) was below the proposed maximum levels (0.2-0.3 mg·kg⁻¹).

The SPE method was furthermore **collaboratively tested** among 10 laboratories on a wholemeal rice meal sample with a satisfactory HorRat value of 1.6.

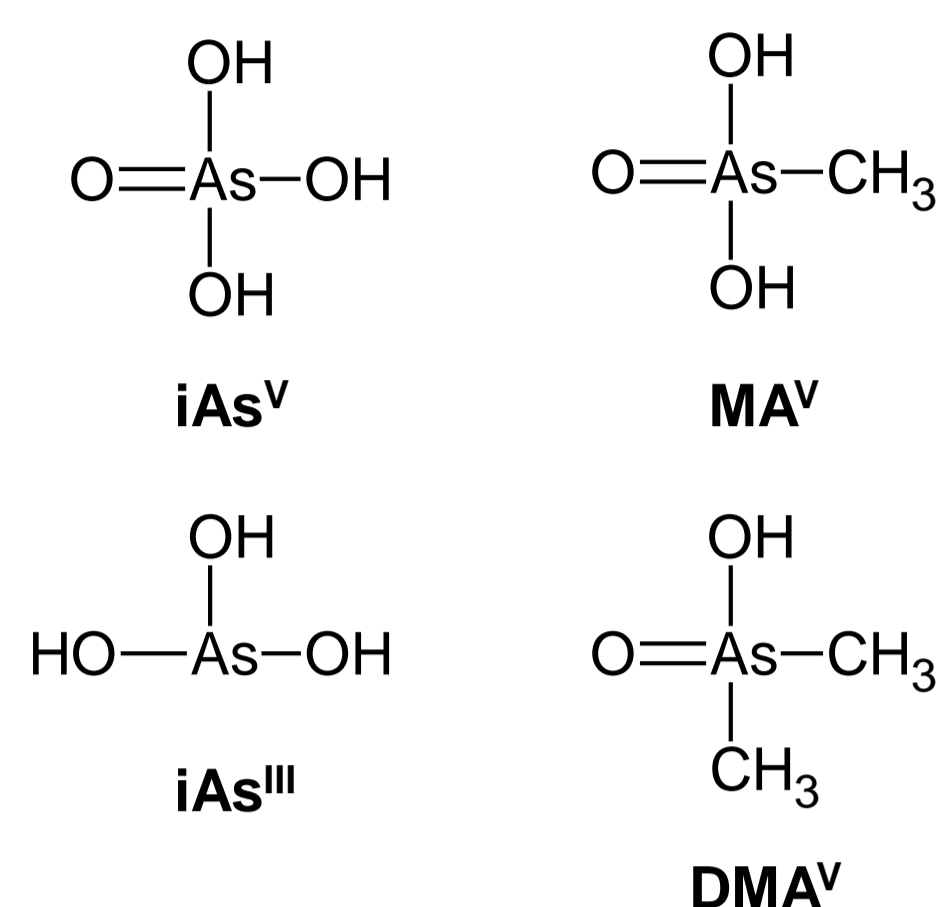

Extraction 0.5 g (dry weight) sample extracted for 60 minutes at 90 °C with 10 ml of a dilute acidic mixture (0.1 M HNO₃ and 3% H₂O₂)

Water bath extraction

SPE separation

HG-AAS detection

SPE SEPARATION

- The charge of the arsenic species depends on pH
- pH 5-7 → iAs^V is negatively charged
- SPE → strong anion exchange
- Sequential elution:
 1. Pre-condition of SPE, MeOH
 2. Equilibrate SPE, 35 mM (NH₄)₂CO₃, 0.05 M HNO₃, 1.5% H₂O₂
 3. Load buffered sample: pH 5.0-7.5
 4. Wash SPE, 0.5 M CH₃COOH
 5. Elute SPE, 0.4 M HNO₃

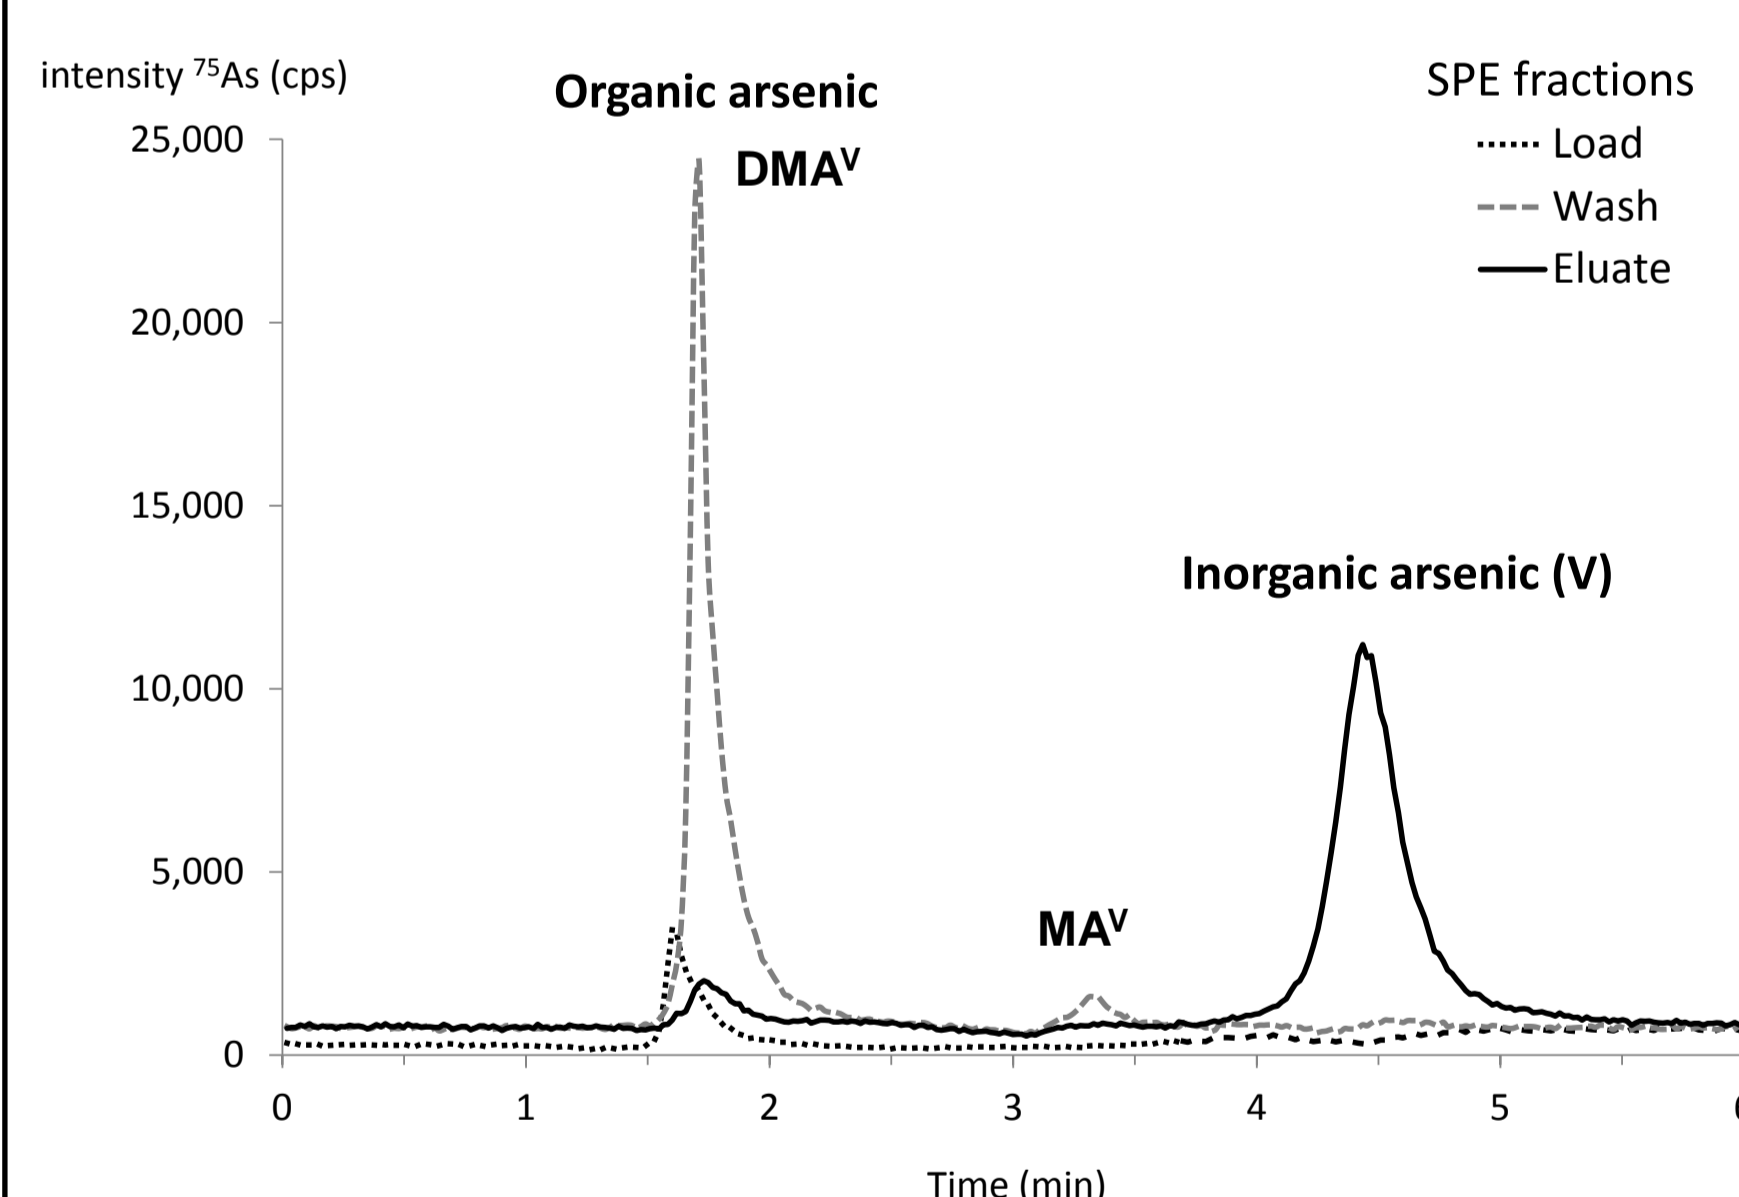


Figure 1. Overlaid HPLC-ICP-MS chromatogram of 3 SPE fractions (load, wash and eluate) of a rice sample (NIST1568a) containing both inorganic and organoarsenic species.

DETECTION

HG-AAS

- Pre-reduction of eluate (As^V → As^{III}) using KI, HCl and ascorbic acid
- Hydride generation using HCl, NaOH and NaBH₄
- HG-AAS settings - heated cell (900°C), As lamp (193.7 nm wave length, 0.5 nm slit width)



Figure 2. The Atomic Absorption Spectrometer (ICE-3300) coupled with a Hydride Generation system (VP100) and an electrically heated quartz cell (all from Thermo Scientific).

SPE HG-AAS versus HPLC-ICP-MS

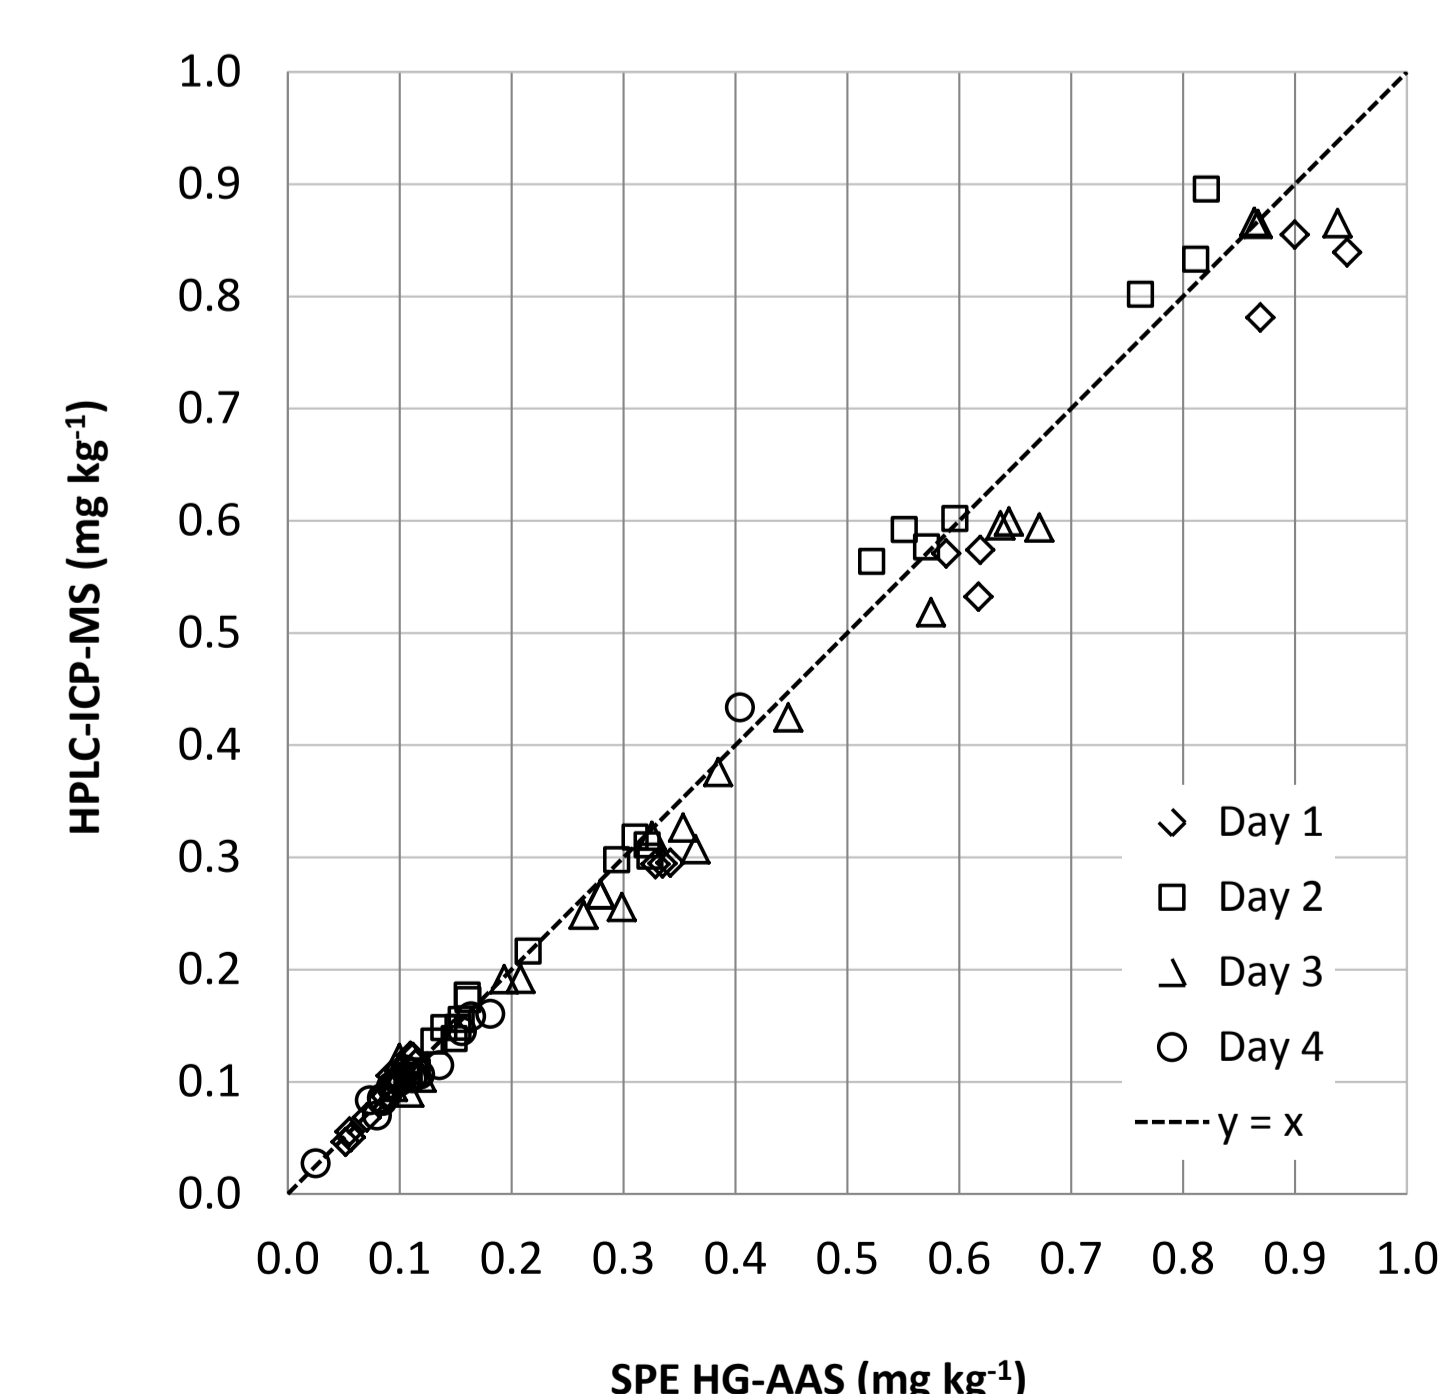


Figure 3. Determination of inorganic arsenic by two different methods; HPLC-ICP-MS and SPE-HG-AAS. In total results for 84 spiked and natural incurred rice samples analysed on four different days. The correlation is $y=x$ (99% confidence interval - regression analysis by Excel 2010).

Table 1. In-house validation results

| | Spiked rice samples | | | Rice reference materials | |
|--------------------------------------|---------------------|--------|------|--------------------------|-----------|
| | Low | Medium | High | IMEP-107 | NIST1568a |
| Target level (mg·kg ⁻¹) | 0.30 | 0.55 | 0.80 | 0.107* | 0.096* |
| Observations (N) | 9 | 9 | 9 | 8 | 7** |
| Mean recovery (%) | 105 | 106 | 106 | 101 | 103 |
| Repeatability RSD _r (%) | 5 | 3 | 4 | 6 | 5 |
| Reproducibility RSD _R (%) | 7 | 9 | 8 | 7 | 7 |

*) Consensus mean values: IMEP-107 (de la Calle MB et al., 2011 TrAC 30:641-651) and NIST1568a (Raab A et al., 2009 J Environ Monit 11:41-44).

**) One outlier result discarded (0.048 mg·kg⁻¹).

References

- Codex (2012) Proposed draft maximum levels for arsenic in rice (at step 3).
- European Food Safety Authority (2009) EFSA Journal 7(10), 1351:1-199
- Rasmussen et al (2013), ABC, doi 10.1007/s00216-013-6936-8
- World Health Organization (2011) WHO Technical Report Series 959