


Accepted Manuscript

Rapid diagnostic tests for determining dengue serostatus: a systematic review and key informant interviews

Robert Luo, Noah Fongwen, Cassandra Kelly-Cirino, Eva Harris, Annelies Wilder-Smith, Rosanna Peeling

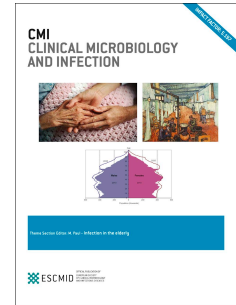

PII: S1198-743X(19)30006-0

DOI: <https://doi.org/10.1016/j.cmi.2019.01.002>

Reference: CMI 1548

To appear in: *Clinical Microbiology and Infection*

Received Date: 18 September 2018

Revised Date: 4 December 2018

Accepted Date: 9 January 2019

Please cite this article as: Luo R, Fongwen N, Kelly-Cirino C, Harris E, Wilder-Smith A, Peeling R, Rapid diagnostic tests for determining dengue serostatus: a systematic review and key informant interviews, *Clinical Microbiology and Infection*, <https://doi.org/10.1016/j.cmi.2019.01.002>.

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

1 Rapid diagnostic tests for determining dengue serostatus:

2 a systematic review and key informant interviews

3
4 Robert Luo^{1*}, Noah Fongwen¹, Cassandra Kelly-Cirino², Eva Harris³,

5 Annelies Wilder-Smith^{4,5}, Rosanna Peeling¹

6
7 ¹ International Diagnostics Centre, London School of Hygiene and Tropical Medicine, London, UK

8 ² Foundation for Innovative New Diagnostics, Geneva, Switzerland

9 ³ Division of Infectious Diseases and Vaccinology, School of Public Health, University of
10 California, Berkeley, USA

11 ⁴ World Health Organization, Geneva, Switzerland

12 ⁵ Department for Disease Control, London School of Hygiene and Tropical Medicine, London, UK

13
14 Intended Category: Systematic Review

15
16 * Corresponding Author:

17 E-mail: rluodx@gmail.com

18 Abstract

19 Objectives: Vaccination for dengue with the live attenuated tetravalent CYD-TDV vaccine
20 (Dengvaxia®) is only recommended in individuals who have had prior dengue virus (DENV)
21 infection. Rapid diagnostic tests (RDT) for past DENV infection would offer a convenient method
22 for pre-vaccination screening at point-of-care. A systematic review was conducted to evaluate
23 the performance of current dengue rapid diagnostic tests (RDTs) for determining dengue
24 serostatus, using IgG antibodies against DENV as a marker of past infection.

25 Methods: PubMed and EMBASE databases were searched from 2000 to 2018 to identify studies
26 evaluating dengue RDTs in individuals with known or possible previous DENV infection. Study
27 quality was evaluated using GRADE and QUADAS-2 criteria. Semi-structured interviews were
28 also performed with available dengue RDT manufacturers.

29 Results: The performance of 4 dengue IgG RDTs was determined in 3137 individuals across 10
30 studies conducted in 13 countries, with serum used in most of the studies. No studies reported
31 data for determining dengue serostatus, and limited data were available regarding cross-
32 reactivity with other viruses. The majority of studies demonstrated sensitivities and specificities
33 between 80-100% for dengue IgG detection in samples from secondary infection or
34 convalescent timepoints after recent infection.

35 Conclusions: Although current dengue IgG RDTs have shown reasonable performance
36 compared to laboratory-based tests in secondary infection, additional research is needed to
37 determine how RDTs would perform in relevant populations targeted for vaccination. New
38 RDTs or modifications to current RDTs are feasible and may optimize the performance of these
39 tests for use in a pre-vaccination screening approach.

40 Introduction

41 Dengue is a flavivirus infection spread by *Aedes aegypti* and *Aedes albopictus* mosquitoes and is
42 estimated to infect up to 400 million people worldwide each year [1]. Four distinct dengue virus
43 serotypes (DENV-1 through DENV-4) cause dengue. After infection with one serotype, an
44 individual develops lifelong immunity to that serotype, but subsequent infection with another
45 serotype increases the risk of severe dengue due to antibody dependent enhancement of
46 infection [2]. The annual incidence of DENV infections has increased exponentially over the past
47 decades, accompanied by continual geographic expansion to new areas [3,4]. International
48 travelers are also increasingly affected [5-8]. Effective vector control strategies are not
49 sustainable [3], community-based approaches have had mixed results [9,10], and compliance
50 with personal protective measures is difficult [11]. Hence, a dengue vaccine would be an
51 important tool to combat the dengue burden.

52
53 Currently, the only commercially available dengue vaccine is a tetravalent live attenuated
54 recombinant vaccine, CYD-TDV (Dengvaxia®), that was developed by Sanofi-Pasteur. Licensed in
55 approximately 20 countries (as of July 2018) for use in individuals between 9 and 45 years of age
56 in most countries, it is given with a 3-dose schedule six months apart [12]. In late 2017, Sanofi-
57 Pasteur released long-term safety data stratified by serostatus [13]. Serostatus refers to
58 whether a person has had a previous DENV infection prior to vaccination: a seropositive person
59 has had at least one past DENV infection, whereas a seronegative person is dengue-naïve [14].
60 Follow-up data of trial participants who were seronegative prior to administration of the vaccine

61 showed a 1.75-fold increased risk of hospitalizations due to dengue and severe dengue from
62 year 3 onwards in comparison with unvaccinated seronegative participants. This unanticipated
63 outcome is thought to be mediated by antibody dependent enhancement of infection, where
64 non-neutralizing antibodies can facilitate greater viral entry into monocytes through Fc receptor
65 binding. This can lead to higher viral load, greater immune activation, and increased risk for
66 severe dengue. In seropositive individuals, the vaccine was efficacious and safe, conferring long-
67 term protection [13]. Consequently, in April 2018, WHO's Strategic Advisory Group of Experts on
68 Immunization (SAGE) revised its recommendations to state a "pre-vaccination screening
69 strategy" would be the preferred option for countries seeking to use Dengvaxia[®], a strategy
70 whereby only dengue-seropositive individuals should be vaccinated [15-17].

71

72 The choice of tests for dengue diagnosis depends on the timing and purpose. For the diagnosis
73 of acute DENV infection, tests are based on DENV isolation, presence of dengue viral antigens,
74 detection of viral nucleic acid in blood through techniques such as RT-PCR, IgM seroconversion,
75 and/or a four-fold or greater rise in IgG antibody titer in paired blood samples collected at least
76 14 days apart [18]. Dengue virus and antigen detection are the most accurate diagnostic tools
77 during the first 5 days of illness, as IgG and IgM antibodies are not produced until 5-7 days after
78 the onset of symptoms in primary infections [19,20]. IgM levels can become undetectable after
79 3-6 months, while IgG levels often persist over an individual's lifetime and can be used to
80 indicate previous DENV infection [19]. Thus, for the detection of past DENV infections, IgG
81 antibodies to DENV serve as a marker of past DENV infection. Enzyme-linked immunosorbent

82 assays (ELISAs) are the most commonly used laboratory-based serology assays to measure DENV
83 IgG. However, ELISAs are time-consuming and require significant laboratory infrastructure,
84 including instrumentation, trained staff, and refrigeration for reagents. Delays in turnaround
85 time would hamper vaccination campaigns as patients would likely be lost to follow-up if
86 required to return several days later for vaccination. The plaque reduction neutralization test
87 (PRNT), which measures the titer of neutralizing antibodies against DENV infection, has also
88 been used to evaluate dengue serostatus, but is even more laborious and expensive than ELISAs,
89 and hence not routinely used [20]. All serological assays can exhibit some degree of cross-
90 reactivity with other flaviviruses such as Zika, Japanese encephalitis and yellow fever [21].

91 Rapid diagnostic tests could enable quick, simple screening in dengue endemic areas, which are
92 often resource-limited and do not have the laboratory capacity to perform ELISA or PRNT
93 testing. RDTs would also provide with results at the point-of-care to ensure safe vaccine
94 administration. However, the disadvantage of currently available RDTs is that they have not yet
95 been validated for screening for past DENV infection and may lack sufficient sensitivity and
96 specificity to ensure effective vaccination strategies. Since RDTs have typically only been
97 evaluated in the context of acute DENV infection and not for the detection of past infection, a
98 systematic review was performed to evaluate the sensitivity and specificity of commercially
99 available RDTs used for detecting IgG antibodies against DENV as a marker of previous DENV
100 infection.

101 **Methods**

102 A systematic review was performed according to the Preferring Reporting Items for Systematic
103 Reviews and Meta-Analyses (PRISMA) [22]. PubMed and EMBASE databases were searched
104 from January 1, 2000, to May 31, 2018 to identify relevant publications in peer-reviewed
105 journals as original scientific research. Search terms were based on a PICO (population,
106 intervention, comparator, and outcome) question format. The population encompassed
107 individuals with known or possible previous DENV infection. The intervention was use of RDTs
108 for detection of DENV IgG antibodies, with the comparator being a validated laboratory-based
109 ELISA or PRNT assay. The primary outcome was previous DENV infection, which was measured
110 in studies by the sensitivity and specificity for IgG detection. The search was performed using
111 the following terms: (dengue OR “dengue virus” OR “dengue fever”) AND (“rapid diagnostic
112 test” OR “rapid test”) AND (IgG OR sensitivity OR specificity OR “commercially available” OR
113 “prior infection” OR “previous infection” OR “convalescent” OR seropositive OR seropositivity).

114
115
116 After all studies were retrieved, two reviewers independently reviewed all potentially relevant
117 studies in full. Disagreements between reviewers were resolved with further discussion
118 between the two primary reviewers. Studies were included if they met the following inclusion
119 criteria: studies evaluating the performance of RDTs that are able to test for DENV IgG, studies
120 comparing RDTs to an established laboratory-based reference standard for determining DENV
121 infection status, and studies involving samples from patients with prior DENV infection. Studies
122 were excluded if they contained one or more of the following exclusion criteria: studies on the
123 use of RDTs for diagnosing acute primary infection only, studies on non-commercially available

124 assays, studies not including an RDT, studies using a reference standard that has not been
125 independently validated, or studies only having a clinical diagnosis as a reference standard.

126

127 Studies were summarized outlining the principal components of each cohort. The summary
128 included the authors, sample size, study location, test characteristics and reference standard.

129 Study results were extracted and summarized for all included studies. Impact on test
130 performance based on variables such as geographic location (if endemic for dengue and other
131 flaviviruses), travel history, previous vaccination status, DENV serotype, and previous infection
132 with other flaviviruses, were also considered. Data from all studies were aggregated, and
133 frequency statistics were run to describe the population tested across all studies. Forest plots
134 were generated to depict the range of sensitivity and specificity results for the RDTs studied.

135 The quality of each study was assessed following QUADAS-2 guidelines, and the complete body
136 of evidence was evaluated using GRADE guidelines [23,24].

137

138 Semi-structured telephone interviews were conducted by the primary author with dengue rapid
139 test product managers from all available dengue RDT manufacturers with commercially-
140 available tests that had published data. Questions were asked regarding the performance,
141 regulatory status, regional availability, intended use, and scientific principles regarding their
142 dengue RDT technology, the availability of data regarding serostatus determination with RDTs,
143 and the feasibility of updating the RDTs for use in determining dengue serostatus. Information
144 was evaluated qualitatively, and common answers regarding the current capabilities of dengue

145 RDTs and the potential for detection of dengue serostatus that were mentioned by a majority of
146 manufacturers were identified.

147


148 **Results**

149 The initial search identified 81 potential published studies for evaluation. Of these, 70 studies
150 did not meet the inclusion and exclusion criteria for the systematic review. Twenty-three studies
151 contained information on the sensitivity and specificity of dengue RDTs compared to
152 conventional laboratory-based ELISA testing. However, 13 of these studies were excluded since
153 they only evaluated RDT performance for acute primary DENV infection and did not provide
154 data on the performance of the IgG component for known or possible previous infection. After
155 filtering studies based on all inclusion and exclusion criteria, 10 studies were included in the
156 final systematic review (Fig 1).

157

158 **Fig 1. PRISMA Diagram**

159

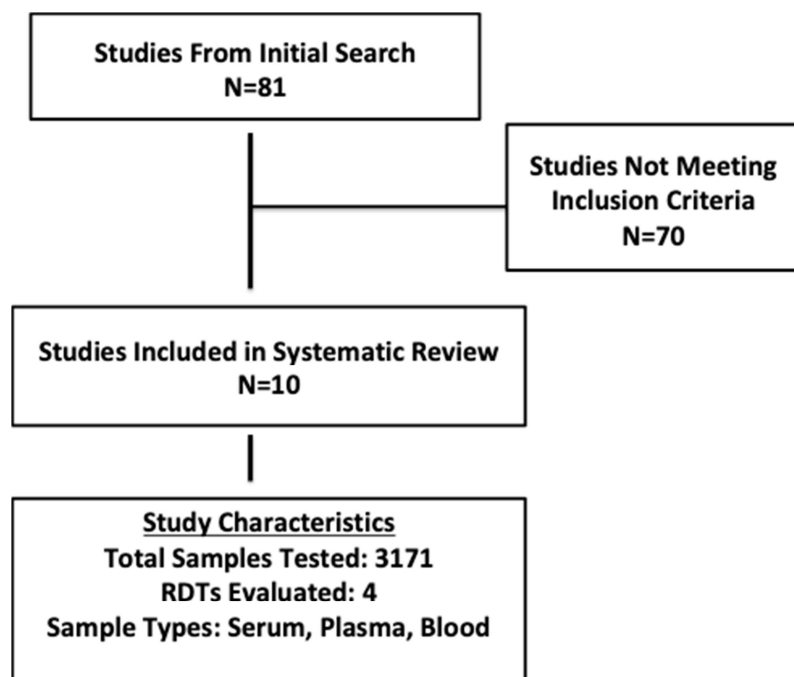

160

161

162 The 10 studies included prospective and retrospective cohort studies [25-34]. Four dengue RDT

163 brands were represented: SD BIOLINE Dengue Duo (Alere/Abbott), Panbio Dengue Duo

164 (Alere/Abbott), OneStep Dengue Fever IgG/IgM RapiCard InstaTest (Cortez), and the GenBody

165 Dengue IgG/IgM test. Table 1 shows a summary of all studies, including information on the

166 types of samples tested and patient characteristics.

167 **Table 1. Study Summary**

Author, year, country	Test(s) Evaluated	Sample Size	Sample Type	Patient Characteristics	Reference Method	IgG Sensitivity (95% CI)	IgG Specificity (95% CI)
Vickers 2017 Jamaica	OneStep Dengue Fever IgG/IgM RapiCard InstaTest	339	Retrospective Serum	Suspected dengue; all ages	ELISA	All Samples: 44.4% (38.2-50.7%)	All Samples: 95.1% (88.0-98.7%)
Piedrahita 2016 Colombia	SD BIOLINE Dengue Duo	41	Prospective Serum	Suspected dengue; ages <18 years	ELISPOT- MNT	All Samples: 26.9% (7.9-41%)	All Samples: 66.7% (39.5-93.9%)
Vickers 2015 Jamaica	SD BIOLINE Dengue Duo	339	Retrospective Serum	Suspected dengue; Secondary infection:	ELISA	All Samples: 39.1% (33.3-45.2%) Secondary	All Samples: N/A Secondary

				IgM/IgG ratio <1.2; all ages		Infection: 52.1% (42-62%)	Infection: 100% (95.6-100%)
Krishnanant- hasivam 2015 Sri Lanka	SD BIOLINE Dengue Duo	143	Prospective Plasma	Suspected dengue	ELISA	All Samples: 38.8% (30.1-48.1%)	All Samples: 95.5% (77.1-99.2%)
Lee 2015 Malaysia	GenBody Dengue IgG/IgM, SD BIOLINE Dengue Duo, Panbio Dengue Duo	311	Prospective Whole Blood	Known dengue IgG positive and negative samples	ELISA	IgG-positive Samples Genbody: 96.7% SD BIOLINE: 82% Panbio: 75.3%	IgG-negative Samples Genbody: 100% SD BIOLINE: 100% Panbio: 100%
Pal	SD BIOLINE	834	Prospective	Suspected	IgG Capture	Convalescent	Convalescent

2015 Peru, USA, Cambodia, Venezuela	Dengue Duo, Panbio Dengue Duo		and Retrospective Serum, Plasma, and Fingerstick Whole Blood	dengue; Convalescent timepoints: 15+ days after symptom onset; All ages	ELISA	Samples SD BIOLINE: 93.9% (90.2-96.6%) Panbio: 98% (95.5-99.4%)	Samples SD BIOLINE: 87.1% (84.1-89.8%) Panbio: 58.3% (54.2-62.4%)
Sanchez- Vargas 2014 Mexico	SD BIOLINE Dengue Duo	397	Prospective Serum	Secondary infection: IgG positive regardless of NS1 or IgM results; Negative samples from other febrile	IgG Capture ELISA	All Samples: 90.1% (85.3-94.8%) Secondary infection: 83.7% (72.3-95.0%)	All Samples: 92.5% (88.8-96.1%)

				illnesses			
Pan-Ngum 2013 Sri Lanka	Panbio Dengue Duo	549	Prospective Serum	Suspected dengue, ages \geq 16 years	ELISA	All Samples: 61.9% (50.7-72.3%)	All Samples: 79.6% (75.6-83.1%)
Moorthy 2009 India	Panbio Dengue Duo	86	Retrospective Serum	Dengue-like illness	IgG Capture ELISA	All Samples: 87.5%	All Samples: 66.6%
Groen 2000 Curacao, Indonesia, Netherlands	Panbio Dengue Duo	132	Retrospective Serum	Suspected dengue; other viral infections	Consensus of multiple immunoas- says	All samples: 52%	All samples: 100%

168

169 Abbreviations: ELISA, enzyme-linked immunoassay. ELISPOT-MNT, enzyme-linked immunospot microneutralization test


170 In total, 3171 samples were tested with RDTs across all the studies. Sample types included
171 whole blood, plasma, and serum. No studies examined the performance of dengue RDTs to
172 detect remote previous infection. Eight of the 10 studies evaluated the ability of the IgG
173 component of the RDT to detect DENV IgG antibodies present in samples from all suspected or
174 known dengue patients being evaluated for DENV infection, compared to a laboratory-based IgG
175 ELISA test. Additionally, four of the 10 studies included samples from individuals described as
176 having secondary DENV infection (defined in studies as documented previous infection or IgG
177 positivity) or convalescent timepoints after recent infection (i.e., defined in one study as 15 days
178 or more after symptom onset), providing some insight into the performance of the IgG
179 component of the RDTs in individuals who had been infected with DENV previously.

180
181 Figure 2 shows the sensitivity of the dengue RDT IgG component from studies evaluating all
182 samples from patients with suspected or known DENV infection as well as studies with separate
183 categories for secondary DENV infection or convalescent timepoints after recent infection.

184

185 **Fig 2. Dengue RDT IgG Sensitivity Results**

186 Figure 2 shows the sensitivity estimates and 95% confidence intervals (when reported) for
187 detection of dengue IgG for each RDT evaluated. Sensitivity in samples from all suspected and
188 known dengue patients is shown in the top half of the figure, followed by sensitivity in samples
189 from secondary infections or convalescent timepoints after recent infection in the bottom half.

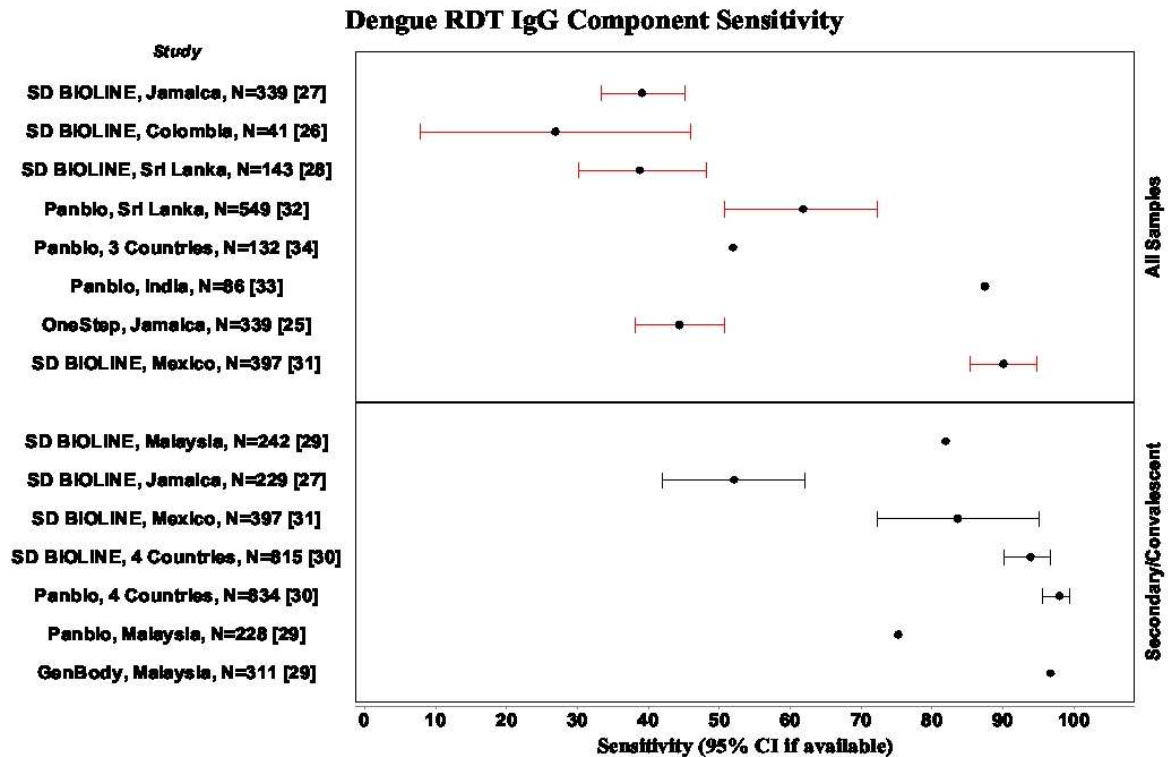

190

191

192 The most commonly studied RDT was the SD BIOLINE Dengue Duo test, followed by the Panbio
 193 Dengue Duo test, and all RDTs in this review could detect both IgG and IgM. When used in the
 194 context of all samples being tested for DENV infection, the sensitivity of the RDT IgG component
 195 typically ranged between 30-60%. However, when evaluated only in secondary infection or
 196 convalescent timepoint samples, the sensitivity of the RDT IgG component was significantly
 197 higher, typically between 75-98% with wide confidence intervals. This is consistent with the fact
 198 that all samples under evaluation for DENV infection included cases of acute primary infection,
 199 which would have had much lower levels or no IgG antibodies present, depending on when in
 200 the course of infection the samples were drawn.

201

202 Figure 3 demonstrates the specificity of the dengue RDT IgG component reported across the
203 studies. In all samples under evaluation for DENV infection, the specificity of the dengue RDTs'
204 IgG component ranged from 65-100%, again with wide confidence intervals. When evaluated
205 only in cases of secondary infection or convalescent timepoints after recent infection, the
206 specificity rose to between 85-100% in most studies.


207

208 **Fig 3. Dengue RDT IgG Specificity Results**

209 Figure 3 shows the specificity estimates and 95% confidence intervals (when reported) for
210 detection of dengue IgG for each RDT evaluated. Specificity in samples from all suspected and
211 known dengue patients is shown in the top half of the figure, followed by specificity in samples
212 from secondary infections or convalescent timepoints after recent infection in the bottom half.

213

214

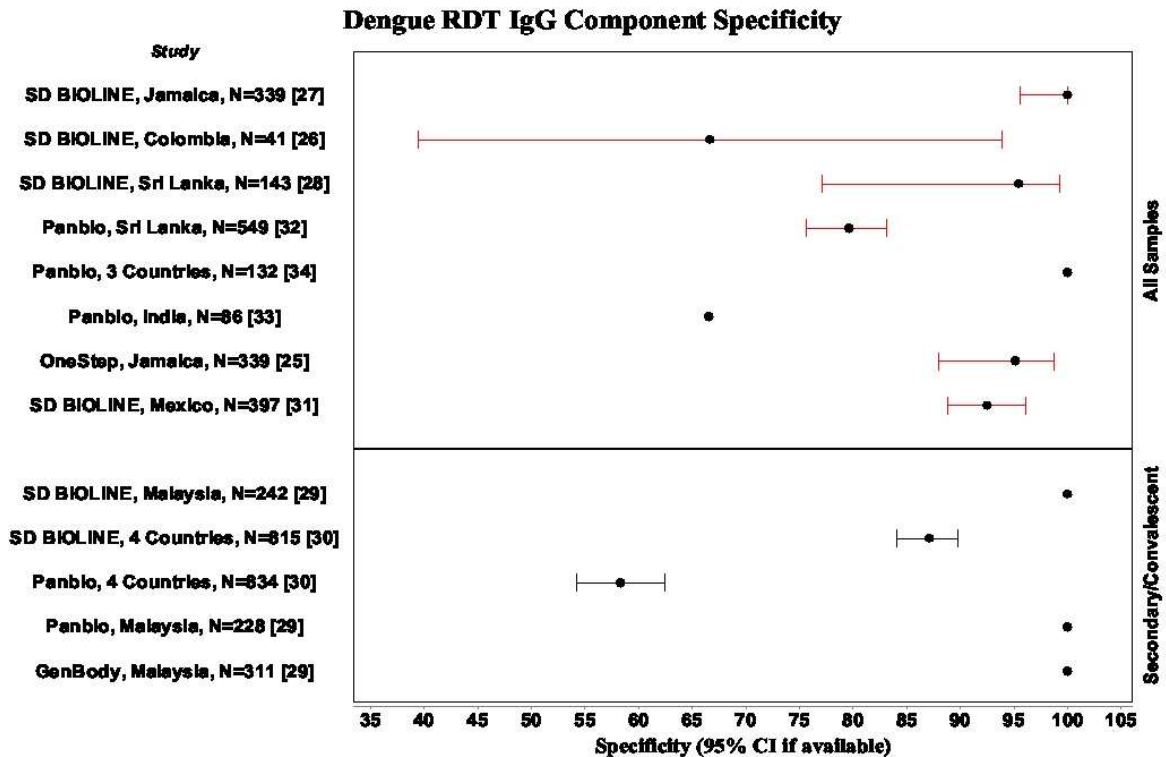

215

216

217 Overall, there were no studies that directly evaluated the use of RDTs for determination of
 218 dengue serostatus, as all studies examined RDT performance in the context of either all samples
 219 from patients with possible DENV infection, and/or a subset from samples of secondary
 220 infection or convalescent timepoints after recent DENV infection. Although all studies included
 221 samples from dengue-endemic areas, none of them provided information on vaccination or
 222 infection status of patients for other flaviviruses, all of which may lead to cross-reactivity with
 223 dengue serological testing. Lack of cross-reactivity data is a major limitation for pre-vaccination
 224 screening, since false-positive results due to cross-reactivity to other co-circulating flaviviruses
 225 could lead to inappropriate vaccination of dengue-naïve individuals. Studies using samples that
 226 have been well-characterized with either ELISA or PRNT for exposure to other flaviviruses,
 227 particularly Zika virus given its genetic similarity to dengue, were absent. Additionally, the

228 majority of studies tested serum samples, and not whole blood samples, which are more
 229 relevant for testing at the point-of-care. There were not enough studies using whole blood to
 230 conclude whether or not the sensitivity and specificity of the test differed compared to serum or
 231 plasma.

232
 233 Table 2 summarizes the QUADAS-2 assessment by study, while Table 3 summarizes the GRADE
 234 assessment of the complete body of evidence, using criteria from published guidelines [23,24].
 235 In the QUADAS-2 assessment, there were high patient selection applicability concerns for all
 236 studies, since none of the RDT tests were exclusively performed on patients with remote
 237 previous DENV infection. This also lead to unclear applicability of the index test, since the
 238 interpretation of an IgG positive result is complicated by the possible detection of IgG in acute
 239 infections and the potential absence of IgG in some cases of previous infection.

240

241 **Table 2. QUADAS-2 Assessment of Studies**

Study	Risk of Bias				Applicability Concerns		
	Patient Selection	Index Test	Reference Standard	Flow & Timing	Patient Selection	Index Test	Reference Standard
Vickers 2017	Low	Low	Low	Low	High	Unclear	Low
Piedrahita 2016	Low	Low	Low	Low	High	Unclear	Low
Vickers 2015	Low	Low	Low	Low	High	Unclear	Low
Krishnananthasivam 2015	Low	Low	Low	Low	High	Unclear	Low
Lee 2015	Unclear	Low	Low	Low	High	Unclear	Low
Pal 2015	Low	Low	Low	Low	High	Unclear	Low

Sanchez-Vargas 2014	Low	Low	Low	Low	High	Unclear	Low
Pan-Ngum 2013	Low	Low	Low	Low	High	Unclear	Low
Moorthy 2009	Low	Low	Low	Low	High	Unclear	Low
Groen 2000	Low	Low	Unclear	Low	High	Unclear	Unclear

242

243 In the GRADE assessment, the overall certainty of evidence for using dengue RDTs for

244 determination of dengue serostatus was low. The indirectness of evidence was serious given the

245 fact that no study evaluated the RDTs for the detection of remote previous DENV infection only.

246 Additionally, the inconsistency of the studies was serious, as studies varied in how they defined

247 secondary infection, the population studied, the laboratory reference standard used, the cutoffs

248 used to define a positive and negative IgG result, and how samples were chosen for inclusion in

249 the evaluations. Due to these differences across studies, a meta-analysis of data was not

250 conducted. Further data analysis and subpopulation analyses were not done due to the absence

251 of data relating to vaccination status, age groups, other flaviviruses, and time since infection, as

252 well as the overall heterogeneity of study designs.

253

254

255 **Table 3. GRADE Evaluation of Evidence Quality**

Number of Studies	Study Design	Risk of bias	Inconsistency	Indirectness	Imprecision	Quality	Importance
-------------------------	-----------------	-----------------	---------------	--------------	-------------	---------	------------

10	Cohort Studies	Not Serious	Serious	Serious	Not Serious	Low	Critical
----	-------------------	----------------	---------	---------	-------------	-----	----------

256

257

258 Semi-structured interviews were conducted with dengue rapid test product managers from 4
259 dengue RDT manufacturers (Abbott/Alere, Bio-Rad, CTK Biotech, and GenBody) who responded
260 to an interview request, along with Sanofi-Pasteur, the manufacturer of Dengvaxia®.

261 Manufacturers noted that dengue RDTs have typically been designed to detect the higher levels
262 of IgG that can be present soon after primary and secondary DENV infections and not low-level
263 IgG, though the specific limit of detection for IgG for each test is not publicly available.

264 Furthermore, current RDTs do not have regulatory approval and were not validated for
265 determination of dengue serostatus. An RDT optimized to detect remote prior infection would
266 benefit from having higher sensitivity for IgG than current RDTs, as IgG levels can wane over the
267 course of time; however, additional testing would be needed to ensure that this does not result
268 in increased cross-reactivity with other flaviviruses. Manufacturers also indicated that this
269 should be technically feasible, given the research already done to develop current RDTs as well
270 as the technical expertise from using and developing laboratory-based ELISA tests, which
271 typically have higher IgG sensitivity. Additional discussions over whether total DENV IgG or IgG
272 specific to particular DENV antigens would be helpful, as well as whether other analytes (e.g.,
273 IgM or other analytes found in current tests) are needed would also be helpful to guide the final
274 design of an RDT.

275

276 **Discussion**

277 In acute secondary DENV infections and convalescent timepoints after recent infection, the
278 sensitivity and specificity of the IgG component of dengue RDTs was typically above 75% and
279 80%, respectively, when compared to IgG detection by laboratory-based ELISA testing.

280 However, a major limitation is the fact that no study evaluated the performance of RDTs for past
281 DENV infection, as studies only used early convalescent samples or samples from presumed
282 acute primary or secondary infection. Therefore, no data are available on RDTs that have tested
283 IgG for DENV infections in the remote past.

284
285 Studies varied depending on the population studied, the types of samples included in each
286 study, how secondary infections were determined, what cutoffs were used to categorized IgG
287 levels as positive or negative, and the reference standard test used. Sensitivity and specificity of
288 the IgG component were lower when the dengue samples tested included acute primary
289 infection samples. This may be due to the lack of IgG or low-levels of IgG present in samples
290 taken soon after infection, where IgM constitutes the primary initial immune response.

291
292 This systematic review did not identify any studies that specifically evaluated dengue RDTs for
293 determining dengue serostatus in the context of remote prior infection only. The review also
294 identified four major challenges of use of dengue RDTs for detecting prior infection:

295 **1) Data challenges**

296 The studies included in this review evaluated the performance of the IgG component of
297 dengue RDTs in the following groups: 1) all samples from individuals with suspected

298 DENV infection and/or 2) samples from individuals described as having secondary DENV
299 infection or convalescent timepoints after recent infection. Although these groups are
300 not equivalent to individuals with more remote previous DENV infection, they do provide
301 some insight into the performance of dengue RDTs for identifying IgG antibodies as
302 compared to a laboratory-based test. However, their performance in these populations
303 should be taken as an overestimate compared to an overall population presenting for
304 vaccination screening, since the groups studied typically have higher IgG levels that are
305 much easier to detect compared to a general population. This will primarily impact the
306 sensitivity of the assays. The extent of specificity will vary depending on the population
307 from which dengue-negative reference samples were drawn (e.g., this ranges from using
308 US adults as dengue-negative controls to samples from dengue-endemic populations).

309

310 **2) Regulatory challenges**

311 Determination of dengue serostatus is not explicitly included as an approved part of the
312 intended use statements of dengue RDTs. This is not surprising, given the fact that the
313 primary intention for these RDTs has been the diagnosis of acute DENV infection in
314 patients with febrile illness. However, the label and intended use for some of these
315 tests, where it is described as an aid to “diagnosis of DENV infection” may be interpreted
316 to include determination of past infection. As an example, the SD Bioline Dengue Duo
317 intended use is to “aid in the presumptive diagnosis between primary and secondary
318 dengue infection.” However, IgG can still be detected during and shortly after acute
319 primary infection, which can complicate the distinction between primary and secondary

320 infection. Regulatory authorities may interpret use of RDTs for determination of past
321 DENV infection as off-label usage, which may lead to procurement and implementation
322 challenges, depending on local policies. Additional research on the use of RDTs for
323 measuring past infection would benefit from following local and regional regulatory
324 requirements, in order to assist RDTs in obtaining an indication for this use.

325

326 **3) Technical challenges**

327 Since IgG antibody levels can be higher during or soon after acute infection, RDTs that
328 have been optimized to diagnose acute infection may not be suitable for detection of
329 lower IgG antibody levels in individuals with more remote prior DENV infection. This may
330 help to explain the lower sensitivity of the IgG component seen in some studies,
331 although the limit of detection for IgG for each test is not publicly available information.
332 Additionally, dengue serological tests can cross-react with antibodies to other
333 flaviviruses, such as West Nile virus and Zika virus, and none of the studies in this review
334 characterized the occurrence of other flaviviruses in their sample sets. Lowering the titer
335 of IgG antibodies that RDTs can detect in order to increase sensitivity for detection of
336 past infection may also lead to lower specificity. More specific antigens could also be
337 explored. Furthermore, specificity may vary depending on the prevalence of other
338 flavivirus infections as well as vaccinations used for other flaviviruses. Therefore, the
339 relatively high sensitivity and specificity of RDTs may show that they match up well with
340 commercial ELISAs designed to diagnose acute infection only. Additional research would

341 be helpful to compare RDTs not only to ELISAs, but also to PRNT assays, which may be a
342 more specific measure of DENV exposure and may be a superior reference standard.

343

344 **4) Impact of Zika virus**

345 Most of the evaluations were conducted before the emergence of Zika virus, which is
346 highly related to DENV. However, recent research on antibody cross-neutralization
347 suggests that ZIKV lies outside the dengue virus serocomplex [35]. In a study on
348 longitudinal serologic specimens from Latin America and Asia, ZIKV neutralizing antibody
349 titers in patients after ZIKV showed low-level cross-reactivity to DENV that was greater in
350 dengue-immune individuals [35]. These antibodies may be able to distinguish ZIKV from
351 DENV infections, although additional research is needed to determine this. Over time it
352 may become harder to distinguish the two viruses, and more specific antigens or tests
353 may be necessary.

354

355 Strengths of this systematic review included over 3000 DENV samples tested, including a
356 smaller subset of secondary infections and convalescent timepoints after recent infection, the
357 geographic diversity of studies, and the inclusion of a number of different commercially-
358 available dengue RDTs and sample types. However, the review was limited by the heterogeneity
359 of data and the inability to evaluate factors such as infection with other flaviviruses and the
360 potential impact of other flavivirus vaccines.

361

362 With such a paucity of data on the use of dengue RDTs for determining serostatus, further
363 research is necessary to inform pre-vaccination screening approaches for dengue, as it is
364 currently difficult to draw distinct conclusions regarding the performance of RDTs for this use.
365 Studies could examine the performance of current RDTs for the direct purpose of determining
366 serostatus, investigate the performance of the test in areas with co-circulating flaviviruses and
367 vaccination, and assess the use of other reference standards such as PRNT. Based on the
368 performance of currently available dengue RDTs in secondary infection and convalescent
369 timepoints after recent infection, the IgG component of these RDTs do have reasonable
370 performance for detection of these infections compared to conventional laboratory-based ELISA
371 testing. However, further discussion within the scientific and public health community is
372 needed to determine if this performance is sufficient for pre-vaccination screening or not. The
373 decision to use RDTs will likely also depend on local factors, such as dengue seroprevalence, the
374 availability of alternative tests, and the public health risk and benefit from vaccination.

375
376 Development of new dengue RDTs or modification of currently available RDTs may be the most
377 beneficial for vaccination screening. Tests with higher sensitivity and specificity, and even new
378 antigen or antibody targets can be investigated and validated by dengue RDT manufacturers,
379 who have the necessary expertise to provide regulatory approved tests suitable for pre-
380 vaccination screening [35]. Alternatively, in settings with sufficient laboratory capacity,
381 laboratory-based testing may also considered, although slower turnaround time of these tests
382 may lead to high rates of individuals not returning for their test results or vaccination [36].
383 Vaccination programs should evaluate all currently available testing options to determine how

384 best to evaluate for dengue serostatus in order to ensure safe and effective vaccination. New
385 tests may be needed with high sensitivity and specificity at the point-of-care to avoid excluding
386 individuals who would benefit from vaccination while at the same time preventing the inclusion
387 of individuals who should not be vaccinated.

ACCEPTED MANUSCRIPT

388 **Acknowledgments**

389 We wish to thank Drs. Leah Katzelnick and Daniela Michlmayr for their thoughtful review and
390 comments on the manuscript and acknowledge funding from the National Institutes of Health
391 grant P01AI106695 (EH).

392

393 **Transparency Declaration**

394 The authors report no conflicts of interest. This systematic review was funded by the World
395 Health Organization.

396 **References**

- 397 1. Bhatt S, Gething PW, Brady OJ, Messina JP, Farlow AW, Moyes CL et al. The global distribution
398 and burden of dengue. *Nature*. 2013;496(7446):504-507.
- 399 2. Katzelnick LC, Gresh L, Halloran ME, Mercado JC, Kuan G, Gordon A, et al. Antibody-
400 dependent enhancement of severe dengue disease in humans. *Science*. 2017;358(6365):929-
401 932.
- 402 3. Wilder-Smith A, Gubler DJ, Weaver SC, Monath TP, Heymann DL, Scott TW. Epidemic arboviral
403 diseases: priorities for research and public health. *Lancet Infect Dis*. 2017;17(3):e101-e106.
- 404 4. Jentes ES, Lash RR, Johansson MA, Sharp TM, Henry R, Brady OJ, et al. Evidence-based risk
405 assessment and communication: a new global dengue-risk map for travellers and clinicians. *J*
406 *Travel Med*. 2016;23(6).
- 407 5. Olivero RM, Hamer DH, MacLeod WB, Benoit CM, Sanchez-Vargas C, Jentes ES, et al. Dengue
408 virus seroconversion in travelers to dengue-endemic areas. *Am J Trop Med Hyg*. 2016.
- 409 6. Neuberger A, Turgeman A, Lustig Y, Schwartz E. Dengue fever among Israeli expatriates in
410 Delhi, 2015: implications for dengue incidence in Delhi, India. *J Travel Med*. 2016;23(3).
- 411 7. Riddell A, Babiker ZO. Imported dengue fever in East London: a 6-year retrospective
412 observational study. *J Travel Med*. 2017;24(3).
- 413 8. Ferguson RW, Henderson SJ, Lee EA, Jung P. Dengue in Peace Corps volunteers, 2000-14. *J*
414 *Travel Med*. 2016;23(3).
- 415 9. Kittayapong P, Olanratmanee P, Maskhao P, Byass P, Logan J, Tozan Y, et al. Mitigating
416 diseases transmitted by *Aedes* mosquitoes: A cluster-randomised trial of permethrin-
417 impregnated school uniforms. *PLoS Negl Trop Dis*. 2017;11(1):e0005197.

- 418 10. Andersson N, Nava-Aguilera E, Arosteguí J, Morales-Perez A, Suazo-Laguna H, Legorreta-
419 Soberanis J, et al. Evidence based community mobilization for dengue prevention in Nicaragua
420 and Mexico (Camino Verde, the Green Way): cluster randomized controlled trial. *BMJ*. 2015 Jul
421 8;351:h3267.
- 422 11. Lalani T, Yun H, Tribble D, Ganesan A, Kunz A, Fairchok M, et al. A comparison of compliance
423 rates with anti-vectorial protective measures during travel to regions with dengue or
424 chikungunya activity, and regions endemic for *Plasmodium falciparum* malaria. *J Travel Med*.
425 2016;23(5).
- 426 12. SAGE Working Group on Dengue Vaccines, WHO Secretariat. Background paper on dengue
427 vaccines. 2016.
- 428 13. Sridhar S, Luedtke A, Langevin E, Zhu M, Bonaparte M, Machabert T, et al. Effect of dengue
429 serostatus on dengue vaccine safety and efficacy. *N Engl J Med*. 2018.
- 430 14. Wilder-Smith A. Serostatus-dependent performance of the first licensed dengue vaccine:
431 implications for travellers. *J Travel Med*. 2018 Aug 1;25(1).
- 432 15. WHO. Updated questions and answers related to the dengue vaccine Dengvaxia® and its
433 use. 22 December 2017.
434 http://www.who.int/immunization/diseases/dengue/q_and_a_dengue_vaccine_dengvaxia_use
- 435 16. WHO. Revised SAGE recommendation on use of dengue vaccine. 19 April 2018.
436 http://www.who.int/immunization/diseases/dengue/revised_SAGE_recommendations_dengue
437 [_vaccines_apr2018/](http://www.who.int/immunization/diseases/dengue/revised_SAGE_recommendations_dengue_vaccines_apr2018/)

- 438 17. Wilder-Smith A, Hombach J, Ferguson N, Selgelid M, O'Brien K, Vannice K, et al.
439 Deliberations of the Strategic Advisory Group of Experts on Immunization on the use of CYD-TDV
440 dengue vaccine. *Lancet Infect Dis*. 2018 Sep 5. pii: S1473-3099(18)30494-8.
- 441 18. Goncalves A, Peeling RW, Chu MC, Gubler DJ, de Silva AM, Harris E, et al. Innovative and new
442 approaches to laboratory diagnosis of Zika and Dengue: A meeting report. *J Infect Dis*.
443 2018;217(7):1060-1068.
- 444 19. WHO. Dengue guidelines for diagnosis, treatment, prevention and control. 2009.
- 445 20. CDC. Laboratory Guidance and Diagnostic Testing: Dengue. 3 August 2017.
- 446 21. Arien KK, Wilder-Smith A. Dengue vaccine: reliably determining previous exposure. *The*
447 *Lancet Global health*. 2018
- 448 22. Moher D, Liberati A, Tetzlaff J, Altman DG, PRISMA Group. Preferred reporting Items for
449 systematic reviews and meta-analyses: the PRISMA statement. *PLoS Med*. 2009;6:e1000097.
- 450 23. Whiting PF, Rutjes AW, Westwood ME, Mallett S, Deeks JJ, Reitsma JB, et al. QUADAS-2: a
451 revised tool for the quality assessment of diagnostic accuracy studies. *Ann Intern Med*.
452 2011;155:529–536.
- 453 24. Schünemann HJ, Oxman AD, Brozek J, Glasziou P, Jaeschke R, Vist GE, et al. Grading quality
454 of evidence and strength of recommendations for diagnostic tests and strategies. *BMJ*.
455 2008;336:1106–1110.
- 456 25. Vickers I, Harvey K, Nelson K, Brown M, Bullock-DuCasse M, Lindo J. Evaluation of OneStep
457 Dengue NS1 RapiDip™ InstaTest and OneStep Dengue Fever IgG/IgM RapiCard™ InstaTest during
458 the course of a dengue type 1 epidemic. *Diagn Microbiol Infect Dis*. 2017 Dec;89(4):271-275.

- 459 26. Piedrahita LD, Agudelo IY, Trujillo AI, Ramírez RE, Osorio JE, Restrepo BN. Evaluation of
460 commercially available assays for diagnosis of acute dengue in schoolchildren during an
461 epidemic period in Medellin, Colombia. *Am J Trop Med Hyg.* 2016 Aug 3;95(2):315-21.
- 462 27. Vickers IE, Harvey KM, Brown MG, Nelson K, DuCasse MB, Lindo JF. The performance of the
463 SD BIOLINE Dengue DUO® rapid immunochromatographic test kit for the detection of NS1
464 antigen, IgM and IgG antibodies during a dengue type 1 epidemic in Jamaica. *J Biomed Sci.* 2015
465 Jul 16;22:55.
- 466 28. Krishnananthasivam S, Fernando AN, Tippalagama R, Tennekoon R, De Man J, Seneviratne D,
467 et al. Evaluation of a commercial rapid test kit for detection of acute dengue infection.
468 *Southeast Asian J Trop Med Public Health.* 2015 Jul;46(4):602-10.
- 469 29. Lee J, Kim YE, Kim HY, Sinniah M, Chong CK, Song HO. Enhanced performance of an
470 innovative dengue IgG/IgM rapid diagnostic test using an anti-dengue EDI monoclonal antibody
471 and dengue virus antigen. *Sci Rep.* 2015 Dec 11;5:18077.
- 472 30. Pal S, Dauner AL, Valks A, Forshey BM, Long KC, Thaisomboonsuk B, et al. Multicountry
473 prospective clinical evaluation of two enzyme-linked immunosorbent assays and two rapid
474 diagnostic tests for diagnosing dengue fever. *J Clin Microbiol.* 2015 Apr;53(4):1092-102.
- 475 31. Sánchez-Vargas LA, Sánchez-Marce EE, Vivanco-Cid H. Evaluation of the SD BIOLINE Dengue
476 Duo rapid test in the course of acute and convalescent dengue infections in a Mexican endemic
477 region. *Diagn Microbiol Infect Dis.* 2014 Apr;78(4):368-72.
- 478 32. Pan-ngum W, Blacksell SD, Lubell Y, Pukrittayakamee S, Bailey MS, Janaka de Silva H, et al.
479 Estimating the true accuracy of diagnostic tests for dengue infection using bayesian latent class
480 models. *PLoS One.* 2013;8(1):e50765.

- 481 33. Moorthy M, Chandy S, Selvaraj K, Abraham AM. Evaluation of a rapid
482 immunochromatographic device for the detection of IgM & IgG antibodies to dengue
483 viruses (DENV) in a tertiary care hospital in south India. *Indian J Med Microbiol.* 2009 Jul-
484 Sep;27(3):254-6.
- 485 34. Groen J, Koraka P, Velzing J, Copra C, Osterhaus AD. Evaluation of six immunoassays for
486 detection of dengue virus-specific immunoglobulin M and G antibodies. *Clin Diagn Lab Immunol.*
487 2000 Nov;7(6):867-71.
- 488 35. Montoya M, Collins M, Dejnirattisai W, Katzelnick LC, Puerta-Guardo H, Jadi R, et al.
489 Longitudinal analysis of antibody cross-neutralization following Zika virus and dengue virus
490 infection in Asia and the Americas. *J Infect Dis.* 2018 Jul 13;218(4):536-545.
- 491 36. Nascimento EJM, George JK, Velasco M, Bonaparte MI, Zheng L, DiazGranados CA, et al.
492 Development of an anti-dengue NS1 IgG ELISA to evaluate exposure to dengue virus. *J Virol*
493 *Methods.* 2018 Jul;257:48-57.