

University of Nebraska - Lincoln

DigitalCommons@University of Nebraska - Lincoln

Mechanical & Materials Engineering Faculty
Publications

Mechanical & Materials Engineering,
Department of

2018

METHODS, SYSTEMS, AND DEVICES FOR SURGICAL ACCESS AND PROCEDURES

Shane M. Farritor

University of Nebraska-Lincoln, sfarritor@unl.edu

Mark Rentschler

Boulder, CO

Amy Lehman

York, NE, alehman2@unl.edu

Stephen R. Platt

Urbana, IL

Jeff Hawks

Lincoln, NE

Follow this and additional works at: <https://digitalcommons.unl.edu/mechengfacpub>



Part of the [Mechanics of Materials Commons](#), [Nanoscience and Nanotechnology Commons](#), [Other Engineering Science and Materials Commons](#), and the [Other Mechanical Engineering Commons](#)

Farritor, Shane M.; Rentschler, Mark; Lehman, Amy; Platt, Stephen R.; and Hawks, Jeff, "METHODS, SYSTEMS, AND DEVICES FOR SURGICAL ACCESS AND PROCEDURES" (2018). *Mechanical & Materials Engineering Faculty Publications*. 330.

<https://digitalcommons.unl.edu/mechengfacpub/330>

This Article is brought to you for free and open access by the Mechanical & Materials Engineering, Department of at DigitalCommons@University of Nebraska - Lincoln. It has been accepted for inclusion in Mechanical & Materials Engineering Faculty Publications by an authorized administrator of DigitalCommons@University of Nebraska - Lincoln.

(12) **United States Patent**
Farritor et al.

(10) **Patent No.:** **US 9,956,043 B2**
(45) **Date of Patent:** ***May 1, 2018**

(54) **METHODS, SYSTEMS, AND DEVICES FOR SURGICAL ACCESS AND PROCEDURES**

(71) Applicant: **Board of Regents of the University of Nebraska**, Lincoln, NE (US)

(72) Inventors: **Shane Michael Farritor**, Lincoln, NE (US); **Mark Rentschler**, Boulder, CO (US); **Amy Lehman**, York, NE (US); **Stephen R. Platt**, Urbana, IL (US); **Jeff Hawks**, Lincoln, NE (US)

(73) Assignee: **Board of Regents of the University of Nebraska**, Lincoln, NE (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 542 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **14/454,035**

(22) Filed: **Aug. 7, 2014**

(65) **Prior Publication Data**

US 2014/0350574 A1 Nov. 27, 2014

Related U.S. Application Data

(63) Continuation of application No. 13/329,705, filed on Dec. 19, 2011, now Pat. No. 8,828,024, which is a (Continued)

(51) **Int. Cl.**
A61B 19/00 (2006.01)
A61B 34/00 (2016.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 19/2203** (2013.01); **A61B 17/00234** (2013.01); **A61B 34/30** (2016.02);
(Continued)

(58) **Field of Classification Search**
CPC ... A61B 17/00234; A61B 34/70; A61B 1/313; A61M 25/0043
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,870,264 A 3/1975 Robinson
3,989,952 A 11/1976 Timberlake et al.
(Continued)

FOREIGN PATENT DOCUMENTS

CN 1082821918 12/2012
DE 102010040405 3/2012
(Continued)

OTHER PUBLICATIONS

Stoianovici et al., "Robotic Tools for Minimally Invasive Urologic Surgery", Jan. 1, 2002, pp. 1-17.

(Continued)


Primary Examiner — Robert N Wieland

(74) *Attorney, Agent, or Firm* — Davis, Brown, Koehn, Shors & Roberts, P.C.; Sean D. Solberg

(57) **ABSTRACT**

The embodiments disclosed herein relate to various medical device components, including components that can be incorporated into robotic and/or in vivo medical devices. Certain embodiments include various actuation system embodiments, including fluid actuation systems, drive train actuation systems, and motorless actuation systems. Additional embodiments include a reversibly lockable tube that can provide access for a medical device to a patient's cavity and further provides a reversible rigidity or stability during operation of the device. Further embodiments include various operational components for medical devices, including medical device arm mechanisms that have both axial and rotational movement while maintaining a relatively compact structure. medical device winch components, medical

(Continued)

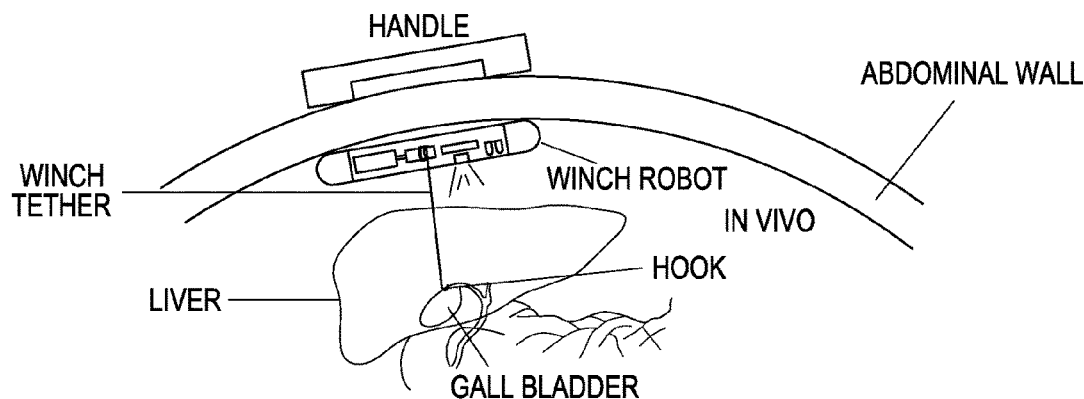

device biopsy/stapler/clamp mechanisms, and medical device adjustable focus mechanisms.

20 Claims, 21 Drawing Sheets

Related U.S. Application Data

continuation of application No. 12/171,413, filed on Jul. 11, 2008, now Pat. No. 8,343,171.

- (60) Provisional application No. 60/949,390, filed on Jul. 12, 2007, provisional application No. 60/949,391, filed on Jul. 12, 2007, provisional application No. 60/990,076, filed on Nov. 26, 2007, provisional application No. 61/025,346, filed on Feb. 1, 2008.

(51) Int. Cl.

A61B 17/00 (2006.01)

A61B 34/30 (2016.01)

(52) U.S. Cl.

CPC *A61B 34/70* (2016.02); *A61B 34/71* (2016.02); *A61B 34/72* (2016.02); *A61B 34/73* (2016.02); *A61B 2017/00278* (2013.01); *A61B 2017/00539* (2013.01); *A61B 2017/00544* (2013.01); *A61B 2034/302* (2016.02); *A61B 2034/306* (2016.02)

(56) References Cited

U.S. PATENT DOCUMENTS

4,246,661	A	1/1981	Pinson	5,515,478	A	5/1996	Wang
4,258,716	A	3/1981	Sutherland	5,524,180	A	6/1996	Wang et al.
4,278,077	A	7/1981	Mizumoto	5,553,198	A	9/1996	Wang et al.
4,538,594	A	9/1985	Boebel et al.	5,562,448	A	10/1996	Mushabac
4,568,311	A	2/1986	Miyaki	5,588,442	A	12/1996	Scovil et al.
4,623,183	A	11/1986	Amori	5,620,417	A	4/1997	Jang et al.
4,736,645	A	4/1988	Zimmer	5,623,582	A	4/1997	Rosenberg
4,771,652	A	9/1988	Zimmer	5,624,380	A	4/1997	Shuichi et al.
4,852,391	A	8/1989	Ruch et al.	5,624,398	A	4/1997	Smith et al.
4,896,015	A	1/1990	Taboada et al.	5,632,761	A	5/1997	Smith et al.
4,897,014	A	1/1990	Tietze	5,645,520	A	7/1997	Nakamura et al.
4,922,755	A	5/1990	Oshiro et al.	5,657,429	A	8/1997	Wang et al.
4,922,782	A	5/1990	Kawai	5,657,584	A	8/1997	Hamlin
4,990,050	A	2/1991	Tsuge et al.	5,672,168	A	9/1997	de la Torre et al.
5,019,968	A	5/1991	Wang et al.	5,674,030	A	10/1997	Sigel
5,108,140	A	4/1992	Bartholet	5,728,599	A	3/1998	Rosteker et al.
5,172,639	A	12/1992	Wiesman et al.	5,736,821	A	4/1998	Suyaman et al.
5,176,649	A	1/1993	Wakabayashi	5,754,741	A	5/1998	Wang et al.
5,178,032	A	1/1993	Zona et al.	5,762,458	A	6/1998	Wang et al.
5,187,032	A	2/1993	Sasaki et al.	5,769,640	A	6/1998	Jacobus et al.
5,187,796	A	2/1993	Wang et al.	5,791,231	A	8/1998	Cohn et al.
5,195,388	A	3/1993	Zona et al.	5,792,135	A	8/1998	Madhani et al.
5,201,325	A	4/1993	McEwen et al.	5,797,538	A	8/1998	Heaton et al.
5,217,003	A	6/1993	Wilk	5,797,900	A	8/1998	Madhani et al.
5,263,382	A	11/1993	Brooks et al.	5,807,377	A	9/1998	Madhani et al.
5,271,384	A	12/1993	McEwen et al.	5,808,665	A	9/1998	Green
5,284,096	A	2/1994	Pelrine et al.	5,815,640	A	9/1998	Wang et al.
5,297,443	A	3/1994	Wentz	5,825,982	A	10/1998	Wright et al.
5,297,536	A	3/1994	Wilk	5,841,950	A	11/1998	Wang et al.
5,304,899	A	4/1994	Sasaki et al.	5,845,646	A	12/1998	Lemelson
5,307,447	A	4/1994	Asano et al.	5,855,583	A	1/1999	Wang et al.
5,353,807	A	10/1994	DeMarco	5,876,325	A	3/1999	Mizuno et al.
5,363,935	A	11/1994	Schempf et al.	5,878,193	A	3/1999	Wang et al.
5,382,885	A	1/1995	Salcudean et al.	5,878,783	A	3/1999	Smart
5,441,494	A	1/1995	Oritz	5,895,417	A	4/1999	Pomeranz et al.
5,388,528	A	2/1995	Pelrine et al.	5,906,591	A	5/1999	Dario et al.
5,436,542	A	7/1995	Petelin et al.	5,907,664	A	5/1999	Wang et al.
5,458,131	A	10/1995	Wilk	5,910,129	A	6/1999	Koblish et al.
5,458,583	A	10/1995	McNeely et al.	5,911,036	A	6/1999	Wright et al.
5,458,598	A	10/1995	Feinberg et al.	5,971,976	A	10/1999	Wang et al.
5,471,515	A	11/1995	Fossum et al.	5,993,467	A	11/1999	Yoon
				6,001,108	A	12/1999	Wang et al.
				6,007,550	A	12/1999	Wang et al.
				6,030,365	A	2/2000	Laufer
				6,031,371	A	2/2000	Smart
				6,058,323	A	5/2000	Lemelson
				6,063,095	A	5/2000	Wang et al.
				6,066,090	A	5/2000	Yoon
				6,102,850	A	8/2000	Wang et al.
				6,107,795	A	8/2000	Smart
				6,132,368	A	10/2000	Cooper
				6,132,441	A	10/2000	Grace
				6,139,563	A	10/2000	Cosgrove, III et al.
				6,156,006	A	12/2000	Brosens et al.
				6,159,146	A	12/2000	El Gazayerli
				6,162,171	A	12/2000	Ng et al.
				D438,617	S	3/2001	Cooper et al.
				6,206,903	B1	3/2001	Ramans
				D441,076	S	4/2001	Cooper et al.
				6,223,100	B1	4/2001	Green
				D441,862	S	5/2001	Cooper et al.
				6,238,415	B1	5/2001	Sepetka et al.
				6,240,312	B1	5/2001	Alfano et al.
				6,241,730	B1	6/2001	Alby
				6,244,809	B1	6/2001	Wang et al.
				6,246,200	B1	6/2001	Blumenkranz et al.
				D444,555	S	7/2001	Cooper et al.
				6,286,514	B1	9/2001	Lemelson
				6,292,678	B1	9/2001	Hall et al.
				6,293,282	B1	9/2001	Lemelson
				6,296,635	B1	10/2001	Smith et al.
				6,309,397	B1	10/2001	Julian et al.
				6,309,403	B1	10/2001	Minoret et al.
				6,312,435	B1	11/2001	Wallace et al.
				6,321,106	B1	11/2001	Lemelson
				6,327,492	B1	12/2001	Lemelson
				6,331,181	B1	12/2001	Tiemey et al.
				6,346,072	B1	2/2002	Cooper
				6,352,503	B1	3/2002	Matsui et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,364,888	B1	4/2002	Niemeyer et al.	6,801,325	B2	10/2004	Farr et al.
6,371,952	B1	4/2002	Madhani et al.	6,804,581	B2	10/2004	Wang et al.
6,394,998	B1	5/2002	Wallace et al.	6,810,281	B2	10/2004	Brock et al.
6,398,726	B1	6/2002	Ramans et al.	6,817,972	B2	11/2004	Snow
6,400,980	B1	6/2002	Lemelson	6,817,974	B2	11/2004	Cooper et al.
6,408,224	B1	6/2002	Lemelson	6,817,975	B1	11/2004	Farr et al.
6,424,885	B1	7/2002	Niemeyer et al.	6,820,653	B1	11/2004	Schempf et al.
6,432,112	B2	8/2002	Brock et al.	6,824,508	B2	11/2004	Kim et al.
6,436,107	B1	8/2002	Wang et al.	6,824,510	B2	11/2004	Kim et al.
6,441,577	B2	8/2002	Blumenkranz et al.	6,832,988	B2	12/2004	Sprout
6,450,104	B1	9/2002	Grant et al.	6,832,996	B2	12/2004	Woloszko et al.
6,451,027	B1	9/2002	Cooper et al.	6,836,703	B2	12/2004	Wang et al.
6,454,758	B1	9/2002	Thompson et al.	6,837,846	B2	1/2005	Jaffe et al.
6,459,926	B1	10/2002	Nowlin et al.	6,837,883	B2	1/2005	Moll et al.
6,463,361	B1	10/2002	Wang et al.	6,839,612	B2	1/2005	Sanchez et al.
6,468,203	B2	10/2002	Belson	6,840,938	B1	1/2005	Morley et al.
6,468,265	B1	10/2002	Evans et al.	6,852,107	B2	2/2005	Wang et al.
6,470,236	B2	10/2002	Ohtsuki	6,858,003	B2	2/2005	Evans et al.
6,491,691	B1	12/2002	Morley et al.	6,860,346	B2	3/2005	Burt et al.
6,491,701	B2	12/2002	Nemeyer et al.	6,860,877	B1	3/2005	Sanchez et al.
6,493,608	B1	12/2002	Niemeyer et al.	6,866,671	B2	3/2005	Tiemey et al.
6,496,099	B2	12/2002	Wang et al.	6,870,343	B2	3/2005	Borenstein et al.
6,508,413	B2	1/2003	Bauer et al.	6,871,117	B2	3/2005	Wang et al.
6,512,345	B2	1/2003	Borenstein	6,871,563	B2	3/2005	Choset et al.
6,522,906	B1	2/2003	Salisbury, Jr. et al.	6,879,880	B2	4/2005	Nowlin et al.
6,544,276	B1	4/2003	Azizi	6,892,112	B2	5/2005	Wang et al.
6,548,982	B1	4/2003	Papanikolopoulos et al.	6,899,705	B2	5/2005	Niemeyer
6,554,790	B1	4/2003	Moll	6,902,560	B1	6/2005	Morley et al.
6,565,554	B1	5/2003	Niemeyer	6,905,460	B2	6/2005	Wang et al.
6,574,355	B2	6/2003	Green	6,905,491	B1	6/2005	Wang et al.
6,587,750	B2	7/2003	Gerbi et al.	6,911,916	B1	6/2005	Wang et al.
6,591,239	B1	7/2003	McCall et al.	6,917,176	B2	7/2005	Schempf et al.
6,594,552	B1	7/2003	Nowlin et al.	6,933,695	B2	8/2005	Blumenkranz
6,610,007	B2	8/2003	Belson et al.	6,936,001	B1	8/2005	Snow
6,620,173	B2	9/2003	Gerbi et al.	6,936,003	B2	8/2005	Iddan
6,642,836	B1	11/2003	Wang et al.	6,936,042	B2	8/2005	Wallace et al.
6,645,196	B1	11/2003	Nixon et al.	6,943,663	B2	9/2005	Wang et al.
6,646,541	B1	11/2003	Wang et al.	6,949,096	B2	9/2005	Davison et al.
6,648,814	B2	11/2003	Kim et al.	6,951,535	B2	10/2005	Ghodoussi et al.
6,659,939	B2	12/2003	Moll et al.	6,965,812	B2	11/2005	Wang et al.
6,661,571	B1	12/2003	Shioda et al.	6,974,411	B2	12/2005	Belson
6,671,581	B2	12/2003	Niemeyer et al.	6,974,449	B2	12/2005	Niemeyer
6,676,684	B1	1/2004	Morley et al.	6,979,423	B2	12/2005	Moll
6,684,129	B2	1/2004	Salisbury, Jr. et al.	6,984,203	B2	1/2006	Tartaglia et al.
6,685,648	B2	2/2004	Flaherty et al.	6,984,205	B2	1/2006	Gazdzinski
6,685,698	B2	2/2004	Morley et al.	6,991,627	B2	1/2006	Madhani et al.
6,687,571	B1	2/2004	Byrne	6,993,413	B2	1/2006	Sunaoshi
6,692,485	B1	2/2004	Brock et al.	6,994,703	B2	2/2006	Wang et al.
6,699,177	B1	3/2004	Wang et al.	6,994,708	B2	2/2006	Manzo
6,699,235	B2	3/2004	Wallace et al.	6,997,908	B2	2/2006	Carrillo, Jr. et al.
6,702,734	B2	3/2004	Kim et al.	7,025,064	B2	4/2006	Wang et al.
6,702,805	B1	3/2004	Stuart	7,027,892	B2	4/2006	Wang et al.
6,714,839	B2	3/2004	Salisbury, Jr. et al.	7,033,344	B2	4/2006	Imran
6,714,841	B1	3/2004	Wright et al.	7,039,453	B2	5/2006	Mullick
6,719,684	B2	4/2004	Kim et al.	7,042,184	B2	5/2006	Oleynikov et al.
6,720,988	B1	4/2004	Gere et al.	7,048,745	B2	5/2006	Tierney et al.
6,726,699	B1	4/2004	Wright et al.	7,053,752	B2	5/2006	Wang et al.
6,728,599	B2	4/2004	Wright et al.	7,063,682	B1	6/2006	Whayne et al.
6,730,021	B2	5/2004	Vassiliades, Jr. et al.	7,066,879	B2	6/2006	Fowler et al.
6,731,988	B1	5/2004	Green	7,066,926	B2	6/2006	Wallace et al.
6,746,443	B1	6/2004	Morley et al.	7,074,179	B2	7/2006	Wang et al.
6,764,441	B2	7/2004	Chiel et al.	7,077,446	B2	7/2006	Kameda et al.
6,764,445	B2	7/2004	Ramans et al.	7,083,571	B2	8/2006	Wang et al.
6,766,204	B2	7/2004	Niemeyer et al.	7,083,615	B2	8/2006	Peterson et al.
6,770,081	B1	8/2004	Cooper et al.	7,087,049	B2	8/2006	Nowlin et al.
6,774,597	B1	8/2004	Borenstein	7,090,683	B2	8/2006	Brock et al.
6,776,165	B2	8/2004	Jin	7,097,640	B2	8/2006	Wang et al.
6,780,184	B2	8/2004	Tanrisever	7,105,000	B2	9/2006	McBrayer
6,783,524	B2	8/2004	Anderson et al.	7,107,090	B2	9/2006	Salisbury, Jr. et al.
6,785,593	B2	8/2004	Wang et al.	7,109,678	B2	9/2006	Kraus et al.
6,788,018	B1	9/2004	Blumenkranz	7,118,582	B1	10/2006	Wang et al.
6,792,663	B2	9/2004	Krzyzanowski	7,121,781	B2	10/2006	Sanchez et al.
6,793,653	B2	9/2004	Sanchez et al.	7,125,403	B2	10/2006	Julian et al.
6,799,065	B1	9/2004	Niemeyer	7,126,303	B2	10/2006	Farritor et al.
6,799,088	B2	9/2004	Wang et al.	7,147,650	B2	12/2006	Lee
				7,155,315	B2	12/2006	Niemeyer et al.
				7,169,141	B2	1/2007	Brock et al.
				7,182,025	B2	2/2007	Ghorbel et al.
				7,182,089	B2	2/2007	Ries

(56)

References Cited

U.S. PATENT DOCUMENTS

7,199,545 B2	4/2007	Oleynikov et al.	2004/0034283 A1	2/2004	Quaid	
7,206,626 B2	4/2007	Quaid, III	2004/0034302 A1	2/2004	Abovitz et al.	
7,206,627 B2	4/2007	Abovitz et al.	2004/0050394 A1	3/2004	Jin	
7,210,364 B2	5/2007	Ghorbel et al.	2004/0070822 A1	4/2004	Shioda et al.	
7,214,230 B2	5/2007	Brock et al.	2004/0099175 A1	5/2004	Perrot et al.	
7,217,240 B2	5/2007	Snow	2004/0102772 A1	5/2004	Baxter et al.	
7,239,940 B2	7/2007	Wang et al.	2004/0106916 A1	6/2004	Quaid et al.	
7,250,028 B2	7/2007	Julian et al.	2004/0111113 A1	6/2004	Nakamura et al.	
7,259,652 B2	8/2007	Wang et al.	2004/0138525 A1*	7/2004	Saadat	A61B 1/0055 600/104
7,273,488 B2	9/2007	Nakamura et al.	2004/0138552 A1	7/2004	Harel et al.	
7,311,107 B2	12/2007	Harel et al.	2004/0140786 A1	7/2004	Borenstein	
7,339,341 B2	3/2008	Oleynikov et al.	2004/0153057 A1	8/2004	Davison	
7,372,229 B2	5/2008	Farritor et al.	2004/0173116 A1	9/2004	Ghorbel et al.	
7,447,537 B1	11/2008	Funda et al.	2004/0176664 A1	9/2004	Iddan	
7,492,116 B2	2/2009	Oleynikov et al.	2004/0215331 A1	10/2004	Chew et al.	
7,566,300 B2	7/2009	Devierre et al.	2004/0225229 A1	11/2004	Viola	
7,574,250 B2	8/2009	Niemeyer	2004/0254680 A1	12/2004	Sunaoshi	
7,637,905 B2	12/2009	Saadat et al.	2004/0267326 A1	12/2004	Ocel et al.	
7,645,230 B2	1/2010	Mikkaichi et al.	2005/0014994 A1	1/2005	Fowler et al.	
7,655,004 B2	2/2010	Long	2005/0021069 A1	1/2005	Feuer et al.	
7,670,329 B2	3/2010	Flaherty et al.	2005/0029978 A1	2/2005	Oleynikov et al.	
7,678,043 B2	3/2010	Gilad	2005/0043583 A1	2/2005	Killmann et al.	
7,731,727 B2	6/2010	Sauer	2005/0049462 A1	3/2005	Kanazawa	
7,762,825 B2	7/2010	Burbank et al.	2005/0054901 A1	3/2005	Yoshino	
7,772,796 B2	8/2010	Farritor et al.	2005/0054902 A1	3/2005	Konno	
7,785,251 B2	8/2010	Wilk	2005/0064378 A1	3/2005	Toly	
7,785,333 B2	8/2010	Miyamoto et al.	2005/0065400 A1	3/2005	Banik et al.	
7,789,825 B2	9/2010	Nobis et al.	2005/0083460 A1	4/2005	Hattori et al.	
7,794,494 B2	9/2010	Sahatjian et al.	2005/0095650 A1	5/2005	Khalili et al.	
7,865,266 B2	1/2011	Moll et al.	2005/0096502 A1*	5/2005	Khalili	A61B 1/018 600/106
7,960,935 B2	6/2011	Farritor et al.	2005/0143644 A1	6/2005	Gilad et al.	
8,021,358 B2	9/2011	Doyle et al.	2005/0154376 A1	7/2005	Riviere et al.	
8,179,073 B2	5/2012	Farritor et al.	2005/0165449 A1	7/2005	Cadeddu et al.	
8,353,897 B2	1/2013	Doyle et al.	2005/0283137 A1	12/2005	Doyle et al.	
8,604,742 B2	12/2013	Farritor et al.	2005/0288555 A1	12/2005	Binmoeller	
9,089,353 B2	7/2015	Farritor	2005/0288665 A1	12/2005	Woloszko	
2001/0018591 A1	8/2001	Brock et al.	2006/0020272 A1	1/2006	Gildenberg	
2001/0049497 A1	12/2001	Kaloo et al.	2006/0046226 A1	3/2006	Bergler et al.	
2002/0003173 A1	1/2002	Bauer et al.	2006/0119304 A1	6/2006	Farritor et al.	
2002/0013601 A1	1/2002	Nobles et al.	2006/0149135 A1	7/2006	Paz	
2002/0026186 A1	2/2002	Woloszka et al.	2006/0152591 A1	7/2006	Lin	
2002/0038077 A1	3/2002	de la Torre et al.	2006/0155263 A1	7/2006	Lipow	
2002/0065507 A1	5/2002	Azizi	2006/0195015 A1	8/2006	Mullick et al.	
2002/0091374 A1	7/2002	Cooper	2006/0196301 A1	9/2006	Oleynikov et al.	
2002/0103417 A1	8/2002	Gazdzinski	2006/0198619 A1	9/2006	Oleynikov et al.	
2002/0111535 A1	8/2002	Kim et al.	2006/0241570 A1	10/2006	Wilk	
2002/0120254 A1	8/2002	Julien et al.	2006/0241732 A1	10/2006	Denker	
2002/0128552 A1	9/2002	Nowlin et al.	2006/0253109 A1	11/2006	Chu	
2002/0140392 A1	10/2002	Borenstein et al.	2006/0258954 A1	11/2006	Timberlake et al.	
2002/0147487 A1	10/2002	Sundquist et al.	2007/0032701 A1	2/2007	Fowler et al.	
2002/0151906 A1	10/2002	Demarais et al.	2007/0043397 A1	2/2007	Ocel et al.	
2002/0156347 A1	10/2002	Kim et al.	2007/0055342 A1	3/2007	Wu et al.	
2002/0171385 A1	11/2002	Kim et al.	2007/0080658 A1	4/2007	Farritor et al.	
2002/0173700 A1	11/2002	Kim et al.	2007/0106113 A1	5/2007	Ravo	
2002/0190682 A1	12/2002	Schempf et al.	2007/0123748 A1	5/2007	Meglan	
2003/0020810 A1	1/2003	Takizawa et al.	2007/0142725 A1	6/2007	Hardin et al.	
2003/0045888 A1	3/2003	Brock et al.	2007/0156019 A1	7/2007	Larkin et al.	
2003/0065250 A1	4/2003	Chiel et al.	2007/0156211 A1	7/2007	Ferren et al.	
2003/0089267 A1	5/2003	Ghorbel et al.	2007/0167955 A1	7/2007	De La Menardiere et al.	
2003/0092964 A1	5/2003	Kim et al.	2007/0225633 A1	9/2007	Ferren et al.	
2003/0097129 A1	5/2003	Davison et al.	2007/0225634 A1	9/2007	Ferren et al.	
2003/0100817 A1	5/2003	Wang et al.	2007/0241714 A1	10/2007	Oleynikov et al.	
2003/0114731 A1	6/2003	Cadeddu et al.	2007/0244520 A1	10/2007	Ferren et al.	
2003/0135203 A1	7/2003	Wang et al.	2007/0250064 A1	10/2007	Darois et al.	
2003/0139742 A1	7/2003	Wampler et al.	2007/0255273 A1	11/2007	Fernandez et al.	
2003/0144656 A1	7/2003	Ocel et al.	2008/0004634 A1	1/2008	Farritor et al.	
2003/0167000 A1	9/2003	Mullick	2008/0015565 A1	1/2008	Davison	
2003/0172871 A1	9/2003	Scherer	2008/0015566 A1	1/2008	Livneh	
2003/0179308 A1	9/2003	Zamorano et al.	2008/0033569 A1	2/2008	Ferren et al.	
2003/0181788 A1	9/2003	Yokoi et al.	2008/0045803 A1	2/2008	Williams	
2003/0229268 A1	12/2003	Uchiyama et al.	2008/0058835 A1	3/2008	Farritor et al.	
2003/0230372 A1	12/2003	Schmidt	2008/0058989 A1	3/2008	Oleynikov et al.	
2004/0117032 A1	1/2004	Roth et al.	2008/0103440 A1	5/2008	Ferren et al.	
2004/0024311 A1	2/2004	Quaid	2008/0109014 A1	5/2008	de la Pena	
2004/0034282 A1	2/2004	Quaid	2008/0111513 A1	5/2008	Farritor et al.	
			2008/0119870 A1	5/2008	Williams et al.	
			2008/0132890 A1	6/2008	Woloszko et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0161804	A1	7/2008	Rioux et al.
2008/0164079	A1	7/2008	Ferren et al.
2008/0183033	A1	7/2008	Bern et al.
2008/0221591	A1	9/2008	Farritor et al.
2008/0269557	A1	10/2008	Marescaux et al.
2008/0269562	A1	10/2008	Marescaux et al.
2009/0020724	A1	1/2009	Paffrath
2009/0024142	A1	1/2009	Ruiz Morales
2009/0048612	A1	2/2009	Farritor et al.
2009/0054909	A1	2/2009	Farritor et al.
2009/0069821	A1	3/2009	Farritor et al.
2009/0076536	A1	3/2009	Rentschler et al.
2009/0137952	A1	5/2009	Ramamurthy et al.
2009/0143787	A9	6/2009	De La Pena
2009/0163929	A1	6/2009	Yeung et al.
2009/0171373	A1	7/2009	Farritor et al.
2009/0234369	A1	9/2009	Bax et al.
2009/0236400	A1	9/2009	Cole et al.
2009/0240246	A1	9/2009	Devill et al.
2009/0247821	A1	10/2009	Rogers
2009/0248038	A1	10/2009	Blumenkranz et al.
2009/0281377	A1	11/2009	Newell et al.
2009/0305210	A1	12/2009	Guru et al.
2010/0010294	A1	1/2010	Conlon et al.
2010/0016659	A1	1/2010	Weitzner et al.
2010/0016853	A1	1/2010	Burbank
2010/0042097	A1	2/2010	Newton et al.
2010/0056863	A1	3/2010	Dejima et al.
2010/0069710	A1	3/2010	Yamatani et al.
2010/0069940	A1	3/2010	Miller et al.
2010/0081875	A1	4/2010	Fowler et al.
2010/0139436	A1	6/2010	Kawashima et al.
2010/0198231	A1	8/2010	Manzo et al.
2010/0204713	A1	8/2010	Ruiz
2010/0245549	A1	9/2010	Allen et al.
2010/0262162	A1	10/2010	Omori
2010/0292691	A1	11/2010	Brogna
2010/0318059	A1	12/2010	Farritor et al.
2011/0015569	A1	1/2011	Kirschenman et al.
2011/0020779	A1	1/2011	Hannaford et al.
2011/0071347	A1	3/2011	Rogers et al.
2011/0071544	A1	3/2011	Steger et al.
2011/0077478	A1	3/2011	Freeman et al.
2011/0082365	A1	4/2011	McGrogan et al.
2011/0098529	A1	4/2011	Ostrovsky et al.
2011/0152615	A1	6/2011	Schostek et al.
2011/0224605	A1	9/2011	Farritor et al.
2011/0230894	A1	9/2011	Simaan et al.
2011/0237890	A1	9/2011	Farritor et al.
2011/0238080	A1	9/2011	Ranjit et al.
2011/0264078	A1	10/2011	Lipow
2011/0270443	A1	11/2011	Kamiya et al.
2012/0035582	A1	2/2012	Nelson et al.
2012/0109150	A1	5/2012	Quaid et al.
2012/0116362	A1	5/2012	Kieturakis
2012/0179168	A1	7/2012	Farritor
2012/0253515	A1	10/2012	Coste-Maniere et al.
2013/0041360	A1	2/2013	Farritor
2013/0131695	A1	5/2013	Scarfogliero et al.
2013/0345717	A1	5/2013	Scarfogliero et al.
2014/0039515	A1	2/2014	Mondry et al.
2014/0046340	A1	2/2014	Wilson et al.
2014/0058205	A1	2/2014	Frederick et al.
2014/0303434	A1	10/2014	Farritor et al.
2015/0051446	A1	2/2015	Farritor et al.

FOREIGN PATENT DOCUMENTS

EP	1354670	10/2003
EP	2286756	2/2011
EP	2286756 A1	2/2011
EP	2329787	8/2011
EP	2563261	3/2013
JP	2004144533	5/1990
JP	5115425	5/1993

JP	200716235	6/1993
JP	2006507809	9/1994
JP	07 136173	5/1995
JP	7306155	11/1995
JP	08-224248	9/1996
JP	201505810 A	5/2001
JP	2001505810	5/2001
JP	2003220065	8/2003
JP	2004322310	6/2004
JP	2004180781	7/2004
JP	2004329292	11/2004
JP	2006508049	3/2006
JP	2009-106606	5/2009
JP	2010-533045	10/2010
JP	2010-536436	12/2010
JP	2011-504794	2/2011
JP	2011-045500	3/2011
JP	2011-115591	6/2011
WO	WO 1992/21291	5/1991
WO	WO 0189405	11/2001
WO	WO 2002/082979	10/2002
WO	WO 2002/100256	12/2002
WO	WO 2005/009211	7/2004
WO	WO 2005009211	2/2005
WO	WO 2005044095	5/2005
WO	WO 2006/052927	8/2005
WO	WO 2006 005075	1/2006
WO	WO 2006/079108	1/2006
WO	WO2006079108	7/2006
WO	WO 2007011654	1/2007
WO	WO 2007/111571	10/2007
WO	WO 2007/149559	12/2007
WO	WO 2009023851 A1	8/2008
WO	WO 2009/144729	12/2009
WO	WO2010/042611	4/2010
WO	WO2010/046823	4/2010
WO	WO201050771 A2	5/2010
WO	WO2011118646 A1	9/2011
WO	WO 2011/135503 A1	11/2011
WO	WO 2011135503	11/2011
WO	WO 2011075693	7/2012
WO	WO 2013009887	1/2013
WO	WO 2014011238	1/2014

OTHER PUBLICATIONS

Cleary et al., "State of the Art in Surgical Robotics: Clinical Applications and Technology Challenges", "Computer Aided Surgery", Jan. 1, 2002, pp. 312-328, vol. 6.

Green, "Telepresence Surgery", Jan. 1, 1995, Publisher: IEEE Engineering in Medicine and Biology.

International Preliminary Report on Patentability from related case PCT/US2007/014567, dated Jan. 8, 2009, 11 pp.

International Search report and Written Opinion from international application No. PCT/US2012/41911, dated Mar. 13, 2013.

International Search Report and Written Opinion from international application No. PCT/US12/46274, dated Sep. 25, 2012.

International Search Report and Written Opinion from international application No. PCT/US2007/089191, dated Nov. 10, 2008, 20 pp.

"International Search Report and Written Opinion from international application No. PCT/US07/14567, dated Apr. 28, 2008, 19 pp."

International Search Report and Written Opinion of international application No. PCT/US2008/069822, dated Aug. 5, 2009, 12 pp.

International Search Report and Written Opinion of international application No. PCT/US2008/073334, dated Jan. 12, 2009, 11 pp.

International Search Report and Written Opinion of international application No. PCT/US2008/073369, dated Nov. 12, 2008, 12 pp.

International Search Report and Written Opinion issued in PCT/US11/46809, dated Dec. 8, 2011.

Ishiyama et al., "Spiral-type Micro-machine for Medical Applications," 2000 International Symposium on Micromechatronics and Human Science, 2000: 65-69.

Jagannath et al., "Peroral transgastric endoscopic ligation of fallopian tubes with long-term survival in a porcine model," Gastrointestinal Endoscopy, 2005; 61(3): 449-453.

(56)

References Cited**OTHER PUBLICATIONS**

- Kalloor et al., "Flexible transgastric peritoneoscopy: a novel approach to diagnostic and therapeutic interventions in the peritoneal cavity," *Gastrointestinal Endoscopy*, 2004; 60(1): 114-117.
- Kang et al., "Robotic Assistants Aid Surgeons During Minimally Invasive Procedures," *IEEE Engineering in Medicine and Biology*, Jan.-Feb. 2001; pp. 94-104.
- Kantsevoy et al., "Endoscopic gastrojejunostomy with survival in a porcine model," *Gastrointestinal Endoscopy*, 2005; 62(2): 287-292.
- Kantsevoy et al., "Transgastric endoscopic splenectomy," *Surgical Endoscopy*, 2006; 20: 522-525.
- Kazemier et al. (1998), "Vascular Injuries During Laparoscopy," *J. Am. Coli. Surg.* 186(5): 604-5.
- Kim, "Early Experience with Telemicroscopic Robot-Assisted Laparoscopic Cholecystectomy Using da Vinci," *Surgical Laparoscopy, Endoscopy & Percutaneous Techniques*, 2002; 12(1):33-40.
- Ko et al., "Per-Oral transgastric abdominal surgery," *Chinese Journal of Digestive Diseases*, 2006; 7: 67-70.
- Lafullarde et al., "Laparoscopic Nissen Fundoplication: Five-year Results and Beyond," *Arch/Surg*, Feb. 2001; 136:180-184.
- Leggett et al. (2002), "Aortic injury during laparoscopic fundoplication," *Surg. Endoscopy* 16(2): 362.
- Li et al. (2000), "Microvascular Anastomoses Performed in Rats Using a Microsurgical Telemicroscop," *Comp. Aid. Surg.* 5: 326-332.
- Liem et al., "Comparison of Conventional Anterior Surgery and Laparoscopic Surgery for Inguinal-hernia Repair," *New England Journal of Medicine*, 1997; 336(22): 1541-1547.
- MacFarlane et al., "Force-Feedback Grasper Helps Restore the Sense of Touch in Minimally Invasive Surgery," *Journal of Gastrointestinal Surgery*, 1999; 3: 278-285.
- Mack et al., "Present Role of Thoracoscopy in the Diagnosis and Treatment of Diseases of the Chest," *Ann Thorac Surgery*, 1992; 54: 403-409.
- Mack, "Minimally Invasive and Robotic Surgery," *JAMA*, Feb. 2001; 285(5): 568-572.
- Mei et al., "Wireless Drive and Control of a Swimming Microrobot," *Proceedings of the 2002 IEEE International Conference on Robotics & Automation*, May 2002: 1131-1136.
- Melvin et al., "Computer-Enhanced vs. Standard Laparoscopic Antireflux Surgery," *J Gastrointest Surg* 2002; 6: 11-16.
- Menciassi et al., "Locomotion of a Leffed Capsule in the Gastrointestinal Tract: Theoretical Study and Preliminary Technological Results," *IEEE Int. Conf. on Engineering in Medicine and Biology*, San Francisco, CA, pp. 2767-2770, Sep. 2004.
- Menciassi et al., "Robotic Solutions and Mechanisms for a Semi-Autonomous Endoscope," *Proceedings of the 2002 IEEE/RSJ Intl. Conference on Intelligent Robots and Systems*, Oct. 2002; 1379-1384.
- Menciassi et al., "Shape memory alloy clamping devices of a capsule for monitoring tasks in the gastrointestinal tract," *J. Micromech. Microeng.* 2005, 15: 2045-2055.
- Meron, "The development of the swallowable video capsule (M2A)," *Gastrointestinal Endoscopy* 2000; 52 6: 817-819.
- Micron, <http://www.micron.com>, 2006, 1/4-inch VGA NTSC/PAL CMOS Digital Image Sensor, 98 pp.
- Midday Jeff et al., "Material Handling System for Robotic natural Orifice Surgery", *Proceedings of the 2011 Design of medical Devices Conference*, Apr. 12-14, 2011, Minneapolis, MN, 4 pages.
- Miller, Ph.D., et al., "In-Vivo Stereoscopic Imaging System with 5 Degrees-of-Freedom for Minimal Access Surgery," *Dept. of Computer Science and Dept. of Surgery, Columbia University*, New York, NY, 7 pp.
- Munro (2002), "Laparoscopic access: complications, technologies, and techniques," *Curro Opin. Obstet. Gynecol.*, 14(4): 365-74.
- Nio et al., "Efficiency of manual vs robotical (Zeus) assisted laparoscopic surgery in the performance of standardized tasks," *Surg Endosc*, 2002; 16: 412-415.
- Office Action dated Apr. 17, 2007, received in related U.S. Appl. No. 11/552,379, 5 pp.
- Office Action dated Apr. 3, 2009, received in related U.S. Appl. No. 11/932,516, 43 pp.
- Office Action dated Aug. 18, 2006, received in related U.S. Appl. No. 11/398,174, 6 pp.
- Office Action dated Aug. 21, 2006, received in related U.S. Appl. No. 11/403,756, 6 pp.
- Office Action dated Oct. 29, 2007, received in related U.S. Appl. No. 11/695,944, 6 pp.
- Office Action dated Oct. 9, 2008, received in related U.S. Appl. No. 11/932,441, 4 pp.
- Oleynikov et al., "In Vivo Camera Robots Provide Improved Vision for Laparoscopic Surgery," *Computer Assisted Radiology and Surgery (CARS)*, Chicago, IL, Jun. 23-26, 2004b.
- Oleynikov et al., "In Vivo Robotic Laparoscopy," *Surgical Innovation*, Jun. 2005, 12(2): 177-181.
- Oleynikov et al., "Miniature Robots Can Assist in Laparoscopic Cholecystectomy," *Journal of Surgical Endoscopy*, 19-4: 473-476, 2005.
- O'Neill, "Surgeon takes new route to gallbladder," *The Oregonian*, Jun. 2007, 2 pp.
- Orlando et al., (2003), "Needle and Trocar Injuries in Diagnostic Laparoscopy under Local Anesthesia: What Is the True Incidence of These Complications?" *Journal of Laparoendoscopic & Advanced Surgical Techniques* 13(3): 181-184.
- Park et al., "Trocar-less Instrumentation for Laparoscopy: Magnetic Positioning of Intra-abdominal Camera and Retractor," *Ann Surg*, Mar. 2007; 245(3): 379-384.
- Park et al., "Experimental studies of transgastric gallbladder surgery: cholecystectomy and cholecystogastric anastomosis (videos)," *Gastrointestinal Endoscopy*, 2005; 61(4): 601-606.
- Patronik et al., "Development of a Tethered Epicardial Crawler for Minimally Invasive Cardiac Therapies," *IEEE*, pp. 239-240.
- Patronik et al., "Crawling on the Heart: A Mobile Robotic Device for Minimally Invasive Cardiac Interventions," *MICCAI*, 2004, pp. 9-16.
- Patronik et al., "Preliminary evaluation of a mobile robotic device for navigation and intervention on the beating heart," *Computer Aided Surgery*, 10(4): 225-232, Jul. 2005.
- Peirs et al., "A miniature manipulator for integration in a self-propelling endoscope," *Sensors and Actuators A*, 2001, 92: 343-349.
- Peters, "Minimally Invasive Colectomy: Are the Potential Benefits Realized?" *Dis Colon Rectum* 1993; 36: 751-756.
- Phoe et al., "Analysis and Development of Locomotion Devices for the Gastrointestinal Tract," *IEEE Transaction on Biomedical Engineering*, vol. 49, No. 6, Jun. 2002, pp. 613-616.
- Phoe et al., "Development of Microrobotic Devices for Locomotion in the Human Gastrointestinal Tract," *International Conference on Computational Intelligence, Robotics and Autonomous Systems (CIRAS 2001)*, Nov. 28-30, (2001), Singapore.
- Platt et al., "In Vivo Robotic Cameras can Enhance Imaging Capability During Laparoscopic Surgery," in the *Proceedings of the Society of American Gastrointestinal Endoscopic Surgeons (SAGES) Scientific Conference*, Ft. Lauderdale, FL, Apr. 13-16, 2005, 1 pg.
- Preliminary Amendment filed Apr. 11, 2007, in related U.S. Appl. No. 11/403,756, 7 pp.
- Preliminary Amendment filed Jul. 30, 2008, in related U.S. Appl. No. 12/171,413, 4 pp.
- RCE and Amendment filed Jun. 13, 2007, in related U.S. Appl. No. 11/403,756, 8 pp.
- Rentschler et al., "Mobile In Vivo Biopsy and Camera Robot," *Studies in Health and Infonnatics Medicine Meets Virtual Reality*, vol. 119., pp. 449-454, IOS Press, Long Beach, CA, 2006e.
- Rentschler et al., *Mobile In Vivo Biopsy Robot*, *IEEE International Conference on Robotics and Automation*, Orlando, Florida, May 2006, pp. 4155-4160.
- Rentschler et al., "Miniature in vivo Robots for Remote and Harsh Environments," *IEEE Transactions on Information Technology in Biomedicine*, Jan. 2006; 12(1): 66-75.
- Rentschler et al., "An In Vivo Mobile Robot for Surgical Vision and Task Assistance," *Journal of Medical Devices*, Mar. 2007, vol. 1: 23-29.

(56)

References Cited**OTHER PUBLICATIONS**

- Rentschler et al., "In vivo Mobile Surgical Robotic Task Assistance," 1 pg.
- Rentschler et al., "In vivo Robotics during the NEEMO 9 Mission," *Medicine Meets Virtual Reality*, Feb. 2007, 1 pg.
- Rentschler et al., "In Vivo Robots for Laparoscopic Surgery," *Studies in Health Technology and Informatics—Medicine Meets Virtual Reality*, ISO Press, Newport Beach, CA, 2004a, 98: 316-322.
- Rentschler et al., "Mechanical Design of Robotic In Vivo Wheeled Mobility," *ASME Journal of Mechanical Design*, 2006a, pp. I-II.
- Rentschler et al., "Mobile In Vivo Camera Robots Provide Sole Visual Feedback for Abdominal Exploration and Cholecystectomy," *Journal of Surgical Endoscopy*, 20-I: 135-138, 2006b.
- Rentschler et al., "Mobile In Vivo Robots Can Assist in Abdominal Exploration," from the Proceedings of the Society of American Gastrointestinal Endoscopic Surgeons (SAGES) Scientific Conference, Ft. Lauderdale, FL, Apr. 13-16, 2005b.
- Rentschler et al., "Modeling, Analysis, and Experimental Study of In Vivo Wheeled Robotic Mobility," *IEEE Transactions on Robotics*, 22(2): 308-321, 2005c.
- Rentschler et al., "Natural Orifice Surgery with an Endoluminal Mobile Robot," *The Society of American Gastrointestinal Endoscopic Surgeons*, Dallas, TX, Apr. 2006d, 14 pp.
- Rentschler et al., "Theoretical and Experimental Analysis of In Vivo Wheeled Mobility," *ASME Design Engineering Technical Conferences: 28th Biennial Mechanisms and Robotics Conference*, Salt Lake City, Utah, Sep. 28-Oct. 2, 2004, pp. 1-9.
- Rentschler et al., "Toward In Vivo Mobility," *Studies in Health Technology and Informatics—Medicine Meets Virtual Reality*, ISO Press, Long Beach, CA, 2005a, III: 397-403.
- Response to Rule 312 Amendment in related U.S. Appl. No. 11/695,944, dated Jan. 12, 2009, 2 pp.
- Riviere et al., "Toward Active Tremor Canceling in Handheld Microsurgical Instruments," *IEEE Transactions on Robotics and Automation*, Oct. 2003, 19(5): 793-800.
- Rosen et al., "Force Controlled and Teleoperated Endoscopic, Grasper for Minimally Invasive Surgery—Experimental Performance Evaluation," *IEEE Transactions of Biomedical Engineering*, Oct. 1999; 46(10): 1212-1221.
- Rosen et al., "Objective Laparoscopic Skills Assessments of Surgical Residents Using Hidden Markov Models Based on Haptic Information and Tool/Tissue Interactions," *Studies in Health Technology and Informatics—Medicine Meets Virtual Reality*, Jan. 2001, 7 pp.
- Rosen et al., "Spherical Mechanism Analysis of a Surgical Robot for Minimally Invasive Surgery—Analytical and Experimental Approaches," *Studies in Health Technology and Informatics—Medicine Meets Virtual Reality*, pp. 442-448, Jan. 2005.
- Rosen et al., "Task Decomposition of Laparoscopic Surgery for Objective Evaluation of Surgical Residents' Learning Curve Using Hidden Markov Model," *Computer Aided Surgery*, vol. 7, pp. 49-61, 2002.
- Rosen et al., "The Blue Dragon—A System of Measuring the Kinematics and the Dynamics of Minimally Invasive Surgical Tools In-Vivo," *Proc. of the 2002 IEEE International Conference on Robotics and Automation*, Washington, DC, pp. 1876-1881, May 2002.
- Ruurda et al., "Robot-Assisted surgical systems: a new era in laparoscopic surgery," *Ann R. Coll Surg Engl.*, 2002; 84: 223-226.
- Ruurda et al., "Feasibility of Robot-Assisted Laparoscopic Surgery," *Surgical Laparoscopy, Endoscopy & Percutaneous Techniques*, 2002; 12(1):41-45.
- Sackier et al., "Robotically assisted laparoscopic surgery," *Surgical Endoscopy*, 1994; 8: 63-66.
- Salky, "What is the Penetration of Endoscopic Techniques into Surgical Practice?" *Digestive Surgery*, 2000; 17:422-426.
- Satava, "Surgical Robotics: The Early Chronicles," *Surgical Laparoscopy, Endoscopy & Percutaneous Techniques*, 2002; 12(1): 6-16.
- Schippers et al., (1996) "Requirements and Possibilities of Computer-Assisted Endoscopic Surgery," In: *Computer Integrated Surgery: Technology and Clinical Applications*, pp. 561-565.
- Schurr et al., "Robotics and Telem Manipulation Technologies for Endoscopic Surgery," *Surgical Endoscopy*, 2000; 14: 375-381.
- Schwartz, "In the Lab: Robots that Slink and Squirm," *The New York Times*, Mar. 27, 2007, 4 pp.
- Sharp LL-151-3D, <http://www.sharp3d.com>, 2006, 2 pp.
- Slatkin et al., "The Development of a Robotic Endoscope," *Proceedings of the 1995 IEEE International Conference on Robotics and Automation*, pp. 162-171, 1995.
- Smart Pill "Fantastic Voyage: Smart Pill to Expand Testing," <http://www.smartpilldiagnostics.com>, Apr. 13, 2005, 1 pg.
- Southern Surgeons Club (1991), "A prospective analysis of 1518 laparoscopic cholecystectomies," *N. Eng. J. Med.* 324(16): 1073-1078.
- Stefanini et al., "Modeling and Experiments on a Legged Microrobot Locomoting in a Tubular Compliant and Slippery Environment," *Int. Journal of Robotics Research*, vol. 25, No. 5-6, pp. 551-560, May-Jun. 2006.
- Stiff et al., "Long-term Pain: Less Common After Laparoscopic than Open Cholecystectomy," *British Journal of Surgery*, 1994; 81: 1368-1370.
- Strong, et al., "Efficacy of Novel Robotic Camera vs. a Standard Laparoscopic Camera," *Surgical Innovation* vol. 12, No. 4, Dec. 2005, Westminster Publications, Inc., pp. 315-318.
- Suzumori et al., "Development of Flexible Microactuator and its Applications to Robotics Mechanisms," *Proceedings of the IEEE International Conference on Robotics and Automation*, 1991: 1622-1627.
- Taylor et al., "A Telerobotic Assistant for Laparoscopic Surgery," *IEEE Eng Med Biol*, 1995; 279-287.
- Tendick et al. (1993), "Sensing and Manipulation Problems in Endoscopic Surgery: Experiment, Analysis, and Observation," *Presence* 2(1): 66-81.
- Tendick et al., "Applications of Micromechanics in Minimally Invasive Surgery," *IEEE/ASME Transactions on Mechatronics*, 1998; 3(1): 34-42.
- Thomann et al., "The Design of a new type of Micro Robot for the Intestinal Inspection," *Proceedings of the 2002 IEEE Intl. Conference on Intelligent Robots and Systems*, Oct. 2002: 1385-1390.
- U.S. Appl. No. 60/180,960, filed Feb. 2000.
- U.S. Appl. No. 60/956,032, filed Aug. 15, 2007.
- U.S. Appl. No. 60/983,445, filed Oct. 29, 2007.
- U.S. Appl. No. 60/990,062, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,076, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,086, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,106, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,470, filed Nov. 27, 2007.
- U.S. Appl. No. 61/025,346, filed Feb. 1, 2008.
- U.S. Appl. No. 61/030,588, filed Feb. 22, 2008.
- U.S. Appl. No. 61/030,617, filed Feb. 22, 2008.
- Way et al., (editors), "Fundamentals of Laparoscopic Surgery," Churchill Livingstone Inc., 1995, 14 pp.
- Wolfe et al., "Endoscopic Cholecystectomy: An analysis of Complications," *Arch. Surg.* Oct. 1991; 126: 1192-1196.
- Worn et al., "Espirit Project No. 33915: Miniaturised Robot for Micro Manipulation (MINIMAN)", Nov. 1998; <http://www.ipr.ira.ujka.de/~microbot/miniman>.
- Yu et al., "Microrobotic Cell Injection," *Proceedings of the 2001 IEEE International Conference on Robotics and Automation*, May 2001; 620-625.
- Yu, BSN, RN, "M2ATM Capsule Endoscopy A Breakthrough Diagnostic Tool for Small Intestine Imaging," vol. 25, No. 1, *Gastroenterology Nursing*, pp. 24-27.
- International Search Report and Written Opinion of international application No. PCT/US2010/061137, dated Feb. 11, 2011, 10 pp.
- Abbou et al., "Laparoscopic Radical Prostatectomy with a Remote Controlled Robot," *The Journal of Urology*, Jun. 2001, 165: 1964-1966.
- Glukhovskiy et al., "The development and application of wireless capsule endoscopy," *Int. J. Med. Robot. Comput. Assist. Surgery*, 2004; 1 (1): 114-123.

(56)

References Cited**OTHER PUBLICATIONS**

- Gong et al., Wireless endoscopy, *Gastrointestinal Endoscopy* 2000; 51(6): 725-729.
- Hanly et al., "Value of the SAGES Learning Center in introducing new technology," *Surgical Endoscopy*, 2004; 19(4): 477-483.
- Hanly et al., "Robotic Abdominal Surgery," *The American Journal of Surgery* 188 (Suppl. to Oct. 1994): 19S-26S, 2004.
- Heikkinen et al., "Comparison of laparoscopic and open Nissen fundoplication two years after operation: A prospective randomized trial," *Surgical Endoscopy*, 2000; 14: 1019-1023.
- Hissink, "Olympus Medical develops capsule camera technology," Dec. 2004, accessed Aug. 29, 2007, <http://www.letsdigital.org>, 3 pp.
- Horgan et al., "Technical Report: Robots in Laparoscopic Surgery," *Journal of Laparoendoscopic & Advanced Surgical Techniques*, 2001; 11(6): 415-419.
- Palm, William, "Rapid Prototyping Primer" May 1998 (revised Jul. 30, 2002) (<http://www.me.psu.edu/lamancusa/rapidpro/primer/chapter2.htm>).
- Guo et al., "Micro Active Guide Wire Catheter System—Characteristic Evaluation, Electrical Model and Operability Evaluation of Micro Active Catheter," *Proceedings of the 1996 IEEE International Conference on Robotics and Automation*, Apr. 1996: 2226-2231.
- Guo et al., "Fish-like Underwater Microrobot with 3 DOF," *Proceedings of the 2002 IEEE International Conference on Robotics & Automation*, May 2002: 738-743.
- Abbott et al., "Design of an Endoluminal Notes Robotic System," from the *Proceedings of the 2007 IEEE/RSJ Int'l Conf. on Intelligent Robot Systems*, San Diego, CA, Oct. 29-Nov. 2, 2007, pp. 410-416.
- Allendorf et al., "Postoperative Immune Function Varies Inversely with the Degree of Surgical Trauma in a Murine Model," *Surgical Endoscopy* 1997; 11:427-430.
- Ang, "Active Tremor Compensation in Handheld Instrument for Microsurgery," *Doctoral Dissertation*, tech report CMU-RI-TR-04-28, Robotics Institute, Carnegie Mellon University, May 2004, 167pp.
- Applicant Amendment after Notice of Allowance under Rule 312, filed Aug. 25, 2008, in related case U.S. Appl. No. 11/695,944, 6pp.
- Applicant Response to Office Action dated Apr. 17, 2007, in related case U.S. Appl. No. 11/552,379, filed Aug. 8, 2007, 7 pp.
- Applicant Response to Office Action dated Aug. 18, 2006, in related case U.S. Appl. No. 11/398,174, filed Nov. 7, 2006, 8pp.
- Applicant Response to Office Action dated Aug. 21, 2006, in related case U.S. Appl. No. 11/403,756, filed Nov. 21, 2006, 52pp.
- Applicant Response to Office Action dated Oct. 29, 2007, in related case U.S. Appl. No. 11/695,944, filed Jan. 22, 2008, 6pp.
- Atmel 80C5X2 Core, <http://www.atmel.com>, 2006, 186pp.
- Bailey et al., "Complications of Laparoscopic Surgery," *Quality Medical Publishers, Inc.*, 1995, 25pp.
- Ballantyne, "Robotic Surgery, Telerobotic Surgery, Telepresence, and Telementoring," *Surgical Endoscopy*, 2002; 16: 1389-1402.
- Bauer et al., "Case Report: Remote Percutaneous Renal Percutaneous Renal Access Using a New Automated Telesurgical Robotic System," *Telemedicine Journal and e-Health* 2001; (4): 341-347.
- Begos et al., "Laparoscopic Cholecystectomy: From Gimmick to Gold Standard," *J Clin Gastroenterol*, 1994; 19(4): 325-330.
- Berg et al., "Surgery with Cooperative Robots," *Medicine Meets Virtual Reality*, Feb. 2007, 1 pg.
- Breda et al., "Future developments and perspectives in laparoscopy," *Eur. Urology* 2001; 40(1): 84-91.
- Breedveld et al., "Design of Steerable Endoscopes to Improve the Visual Perception of Depth During Laparoscopic Surgery," *ASME*, Jan. 2004; vol. 126, pp. 1-5.
- Breedveld et al., "Locomotion through the Intestine by means of Rolling Stents," *Proceedings of the ASME Design Engineering Technical Conferences*, 2004, pp. 1-7.
- Calafiore et al., Multiple Arterial Conduits Without Cardiopulmonary Bypass: Early Angiographic Results, *Ann Thorac Surg*, 1999; 67: 450-456.
- Camarillo et al., "Robotic Technology in Surgery: Past, Present and Future," *The American Journal of Surgery*, 2004; 188: 2S-15.
- Cavusoglu et al., "Telesurgery and Surgical Simulation: Haptic Interfaces to Real and Virtual Surgical Environments," In McLaughlin, M.L., Hespanha, J.P., and Sukhatme, G., editors. *Touch in virtual environments*, IMSC Series in Multimedia 2001, 28pp.
- Cavusoglu et al., "Robotics for Telesurgery: Second Generation Berkeley/UCSF Laparoscopic Telesurgical Workstation and Looking Towards the Future Applications," *Industrial Robot: An International Journal*, 2003; 30(1): 22-29.
- Chanthasopeephan et al., (2003), "Measuring Forces in Liver Cutting: New Equipment and Experimental Results," *Annals of Biomedical Engineering* 31: 1372-1382.
- Choi et al., "Flexure-based Manipulator for Active Handheld Microsurgical Instrument," *Proceedings of the 27th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBS)*, Sep. 2005, 4pp.
- Cuschieri, "Technology for Minimal Access Surgery," *BMJ*, 1999, 319: 1-6.
- Dakin et al., "Comparison of laparoscopic skills performance between standard instruments and two surgical robotic systems," *Surg Endosc.*, 2003; 17: 574-579.
- Dumpe et al., "Improving in Vivo Robot Vision Quality," from the *Proceedings of Medicine Meets Virtual Reality*, Long Beach, CA, Jan. 26-29, 2005. 1 pg.
- Dumpe et al., "Stereoscopic In Vivo Surgical Robots," *IEEE Sensors Special Issue on In Vivo Sensors for Medicine*, Jan. 2007, 10 pp.
- Examiner Interview Summary dated Aug. 6 and Aug. 12, 2008, in related U.S. Appl. No. 11/695,944, 1 pg.
- Examiner Interview Summary dated May 9, 2008, in related U.S. Appl. No. 11/695,944, 1 pg.
- Examiner Interview Summary dated Nov. 30, 2006, in related U.S. Appl. No. 11/398,174, 2pp.
- Falcone et al., "Robotic Surgery," *Clin. Obstet. Gynecol.* 2003, 46(1): 37-43.
- Faraz et al., "Engineering Approaches to Mechanical and Robotic Design for Minimally Invasive Surgery (MIS)," *Kluwer Academic Publishers (Boston)*, 2000, 13pp.
- Fearing et al., "Wing Transmission for a Micromechanical Flying Insect," *Proceedings of the 2000 IEEE International Conference on Robotics & Automation*, Apr. 2000; 1509-1516.
- Fireman et al., "Diagnosing small bowel Crohn's disease with wireless capsule endoscopy," *Gut* 2003; 52: 390-392.
- Flynn et al., "Tomorrow's Surgery: micromotors and microbots for minimally invasive procedures," *Minimally Invasive Surgery & Allied Technologies*.
- Franklin et al., "Prospective Comparison of Open vs. Laparoscopic Colon Surgery for Carcinoma: Five-Year Results," *Dis Colon Rectum*, 1996; 39: S35-S46.
- Franzino, "The Laprotek Surgical System and the Next Generation of Robotics," *Surg Clin North Am*, 2003 83(6).
- Fraulob et al., "Miniature assistance module for robot-assisted heart surgery," *Biomed. Tech.* 2002, 47 Suppl. 1, Pt. 1: 12-15.
- Fukuda et al., "Mechanism and Swimming Experiment of Micro Mobile Robot in Water," *Proceedings of the 1994 IEEE International Conference on Robotics and Automation*, 1994: 814-819.
- Fukuda et al., "Micro Active Catheter System with Multi Degrees of Freedom," *Proceedings of the IEEE International Conference on Robotics and Automation*, May 1994, pp. 2290-2295.
- Fuller et al., "Laparoscopic Trocar Injuries: A Report from a U.S. Food and Drug Administration (FDA) Center for Devices and Radiological Health (CDRH) Systematic Technology Assessment of Medical Products (STAMP) Committee," *U.S. Food and Drug Administration*, available at <http://www.fda.gov/ov>, Finalized: Nov. 7, 2003; Updated: Jun. 24, 2005, 11 pp.
- Grady, "Doctors Try New Surgery for Gallbladder Removal," *The New York Times*, Apr. 20, 2007, 3 pp.



(56)



References Cited

OTHER PUBLICATIONS

Guber et al., "Miniaturized Instrument Systems for Minimally Invasive Diagnosis and Therapy," Biomedizinische Technik. 2002, Band 47, Ergänzungsband 1.

* cited by examiner

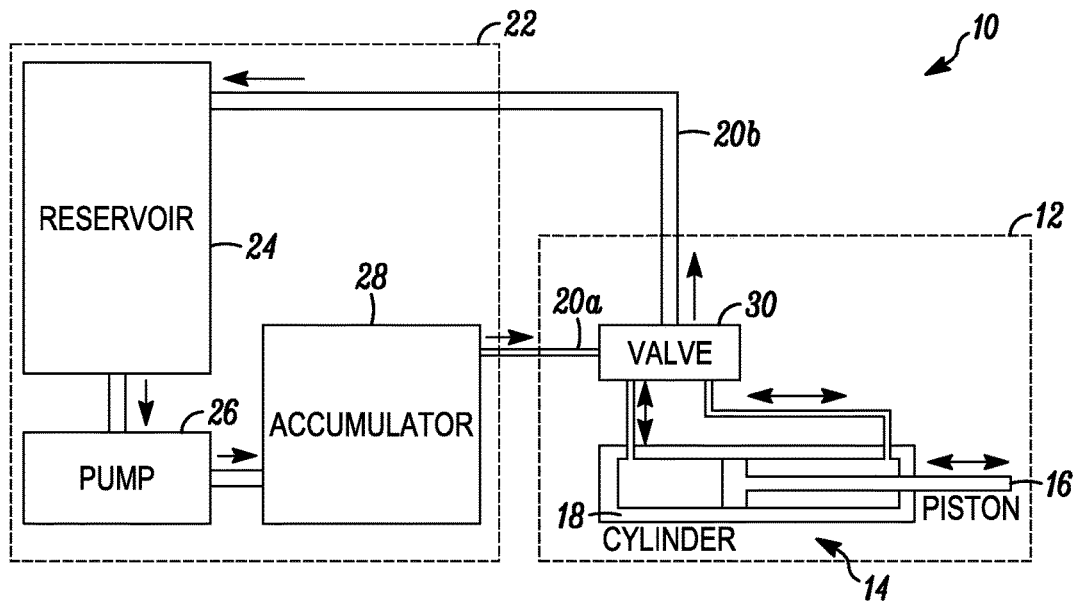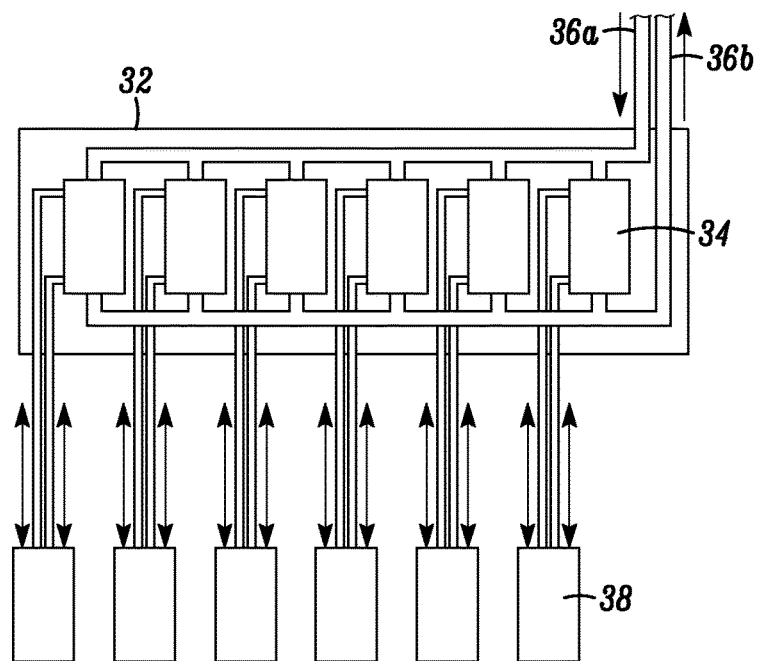*FIG. 1A**FIG. 1B*

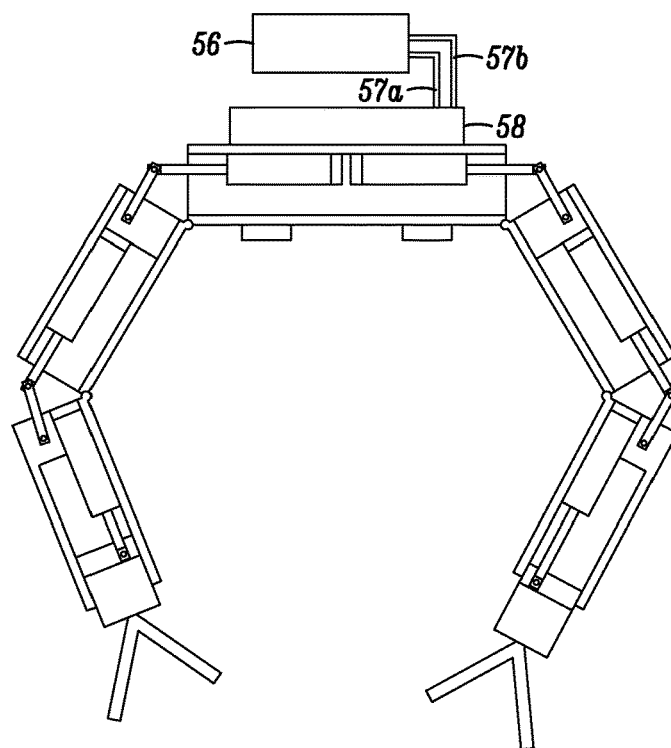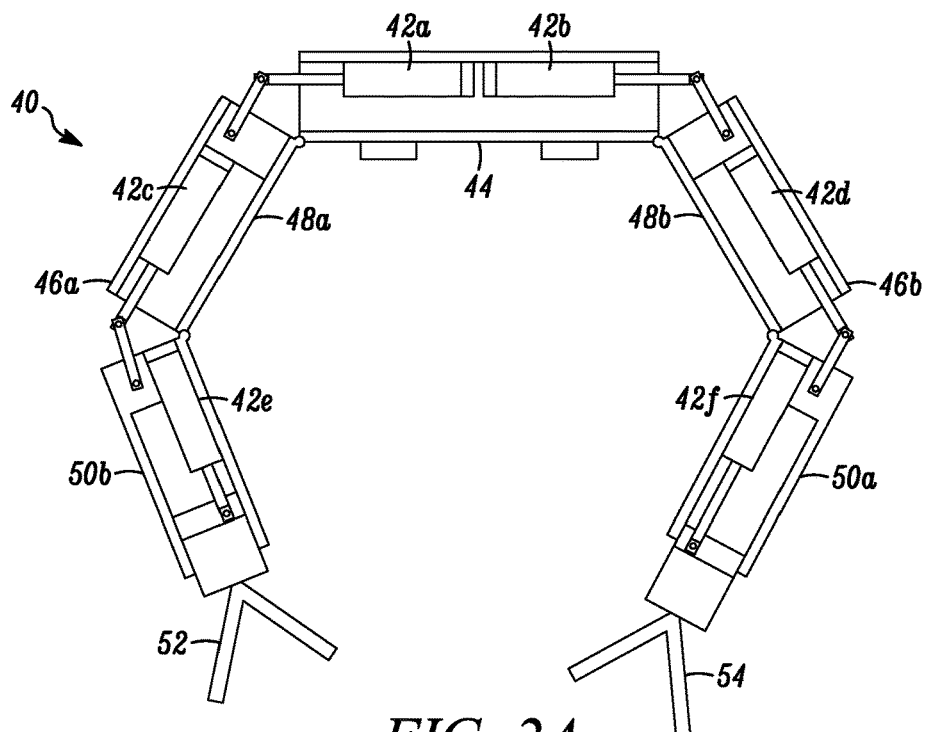

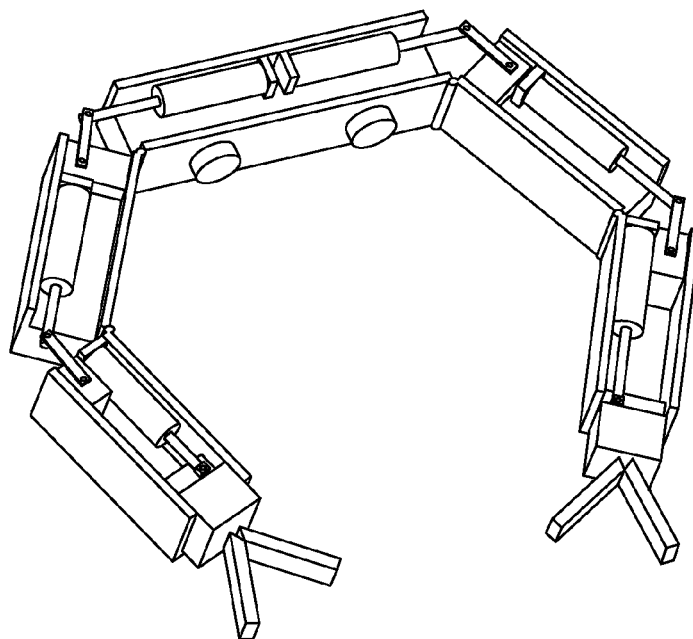


FIG. 3

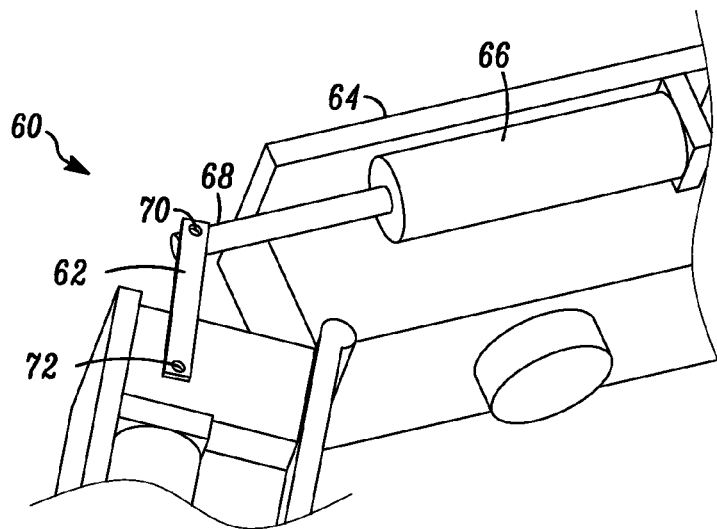


FIG. 4

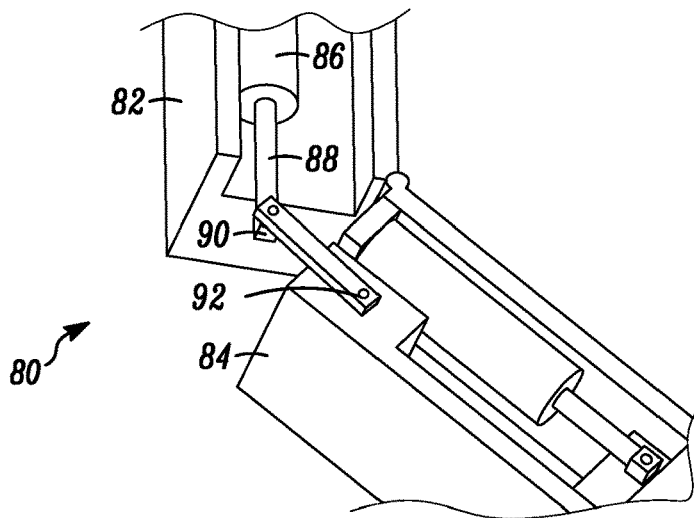


FIG. 5

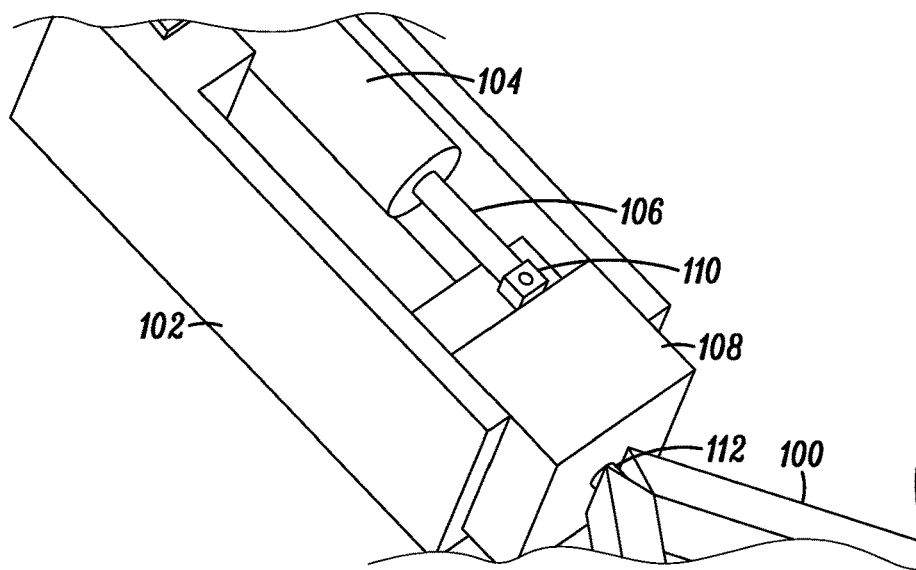


FIG. 6

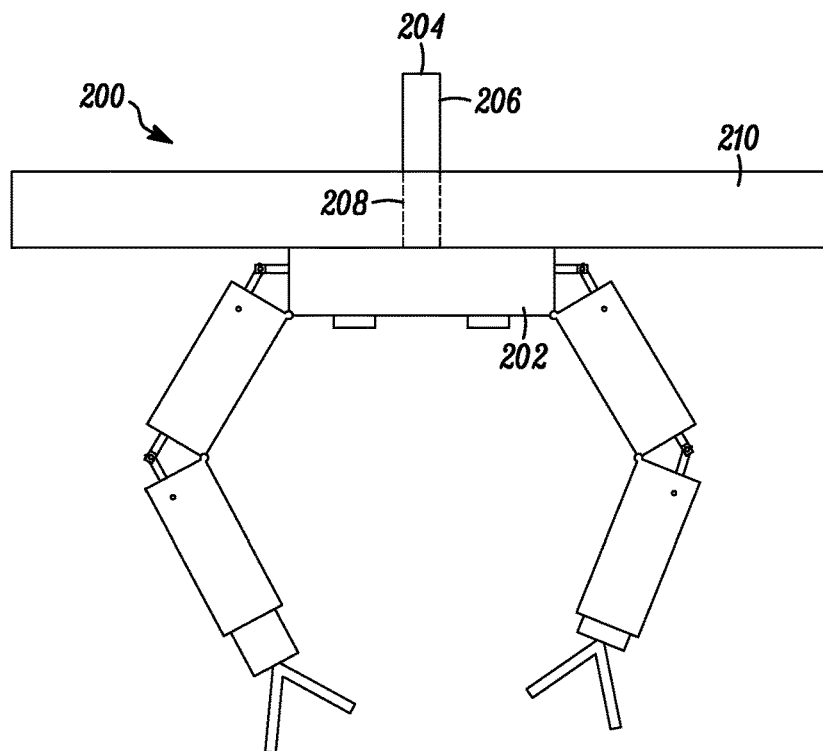


FIG. 7A

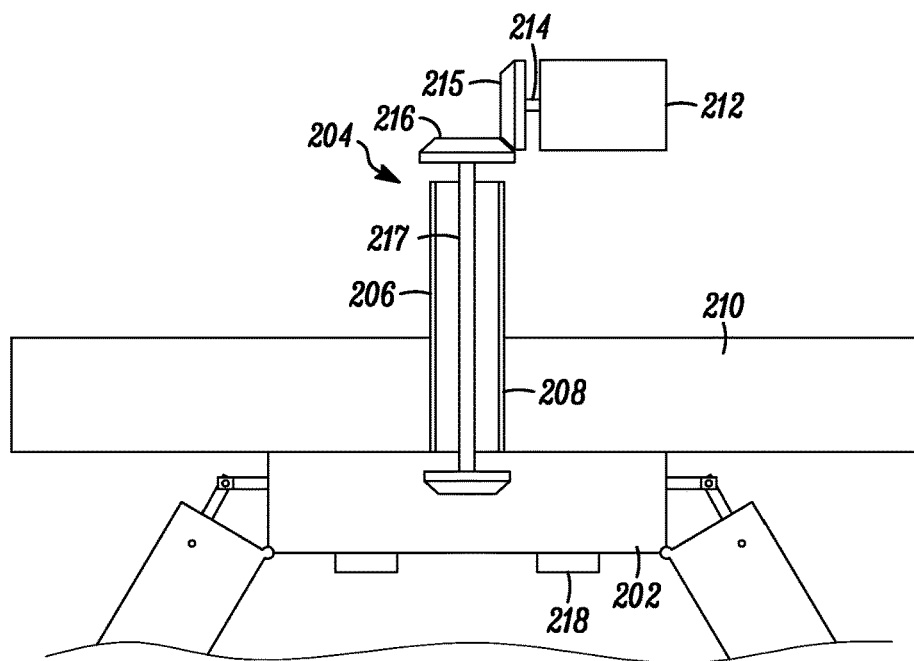
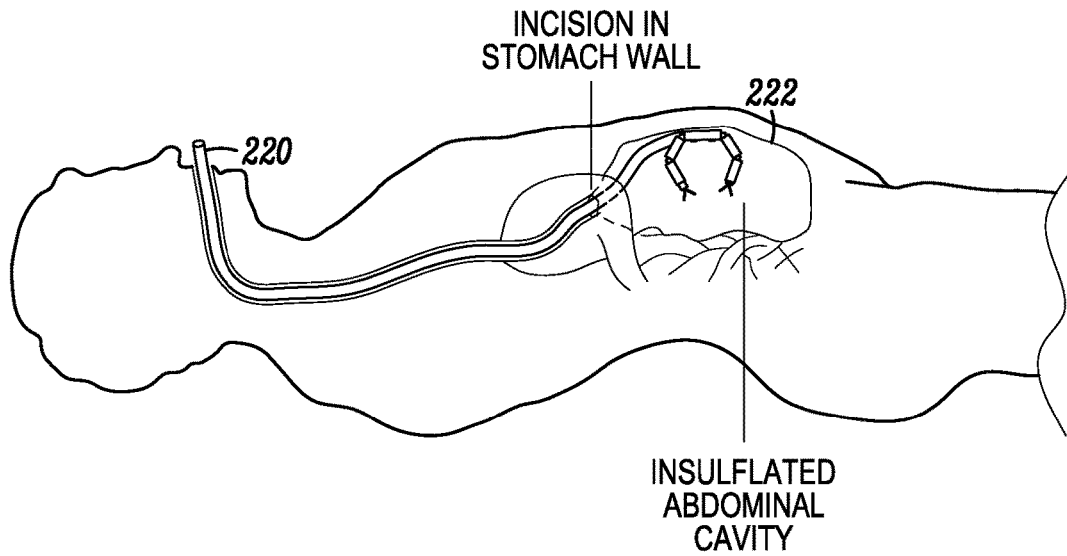
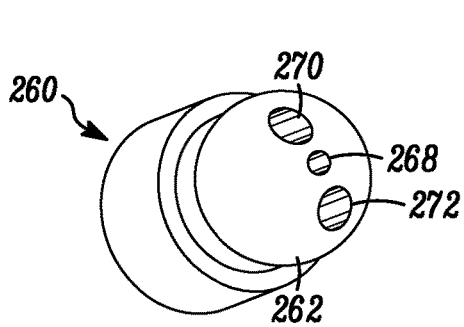
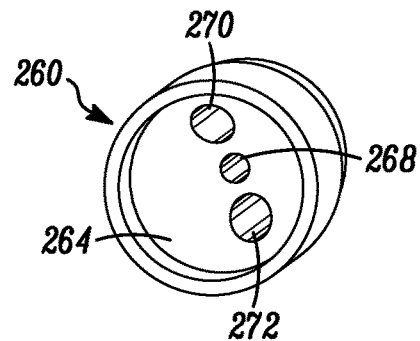


FIG. 7B

*FIG. 8**FIG. 9A**FIG. 9B*

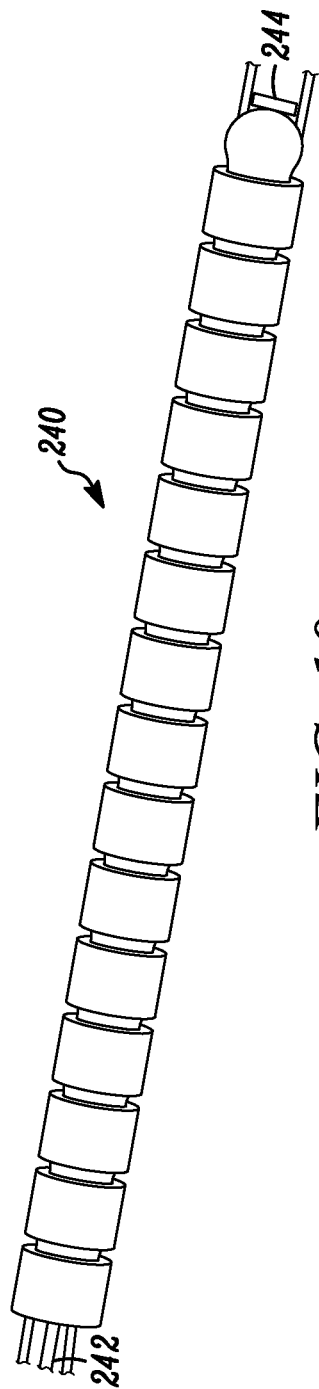


FIG. 10

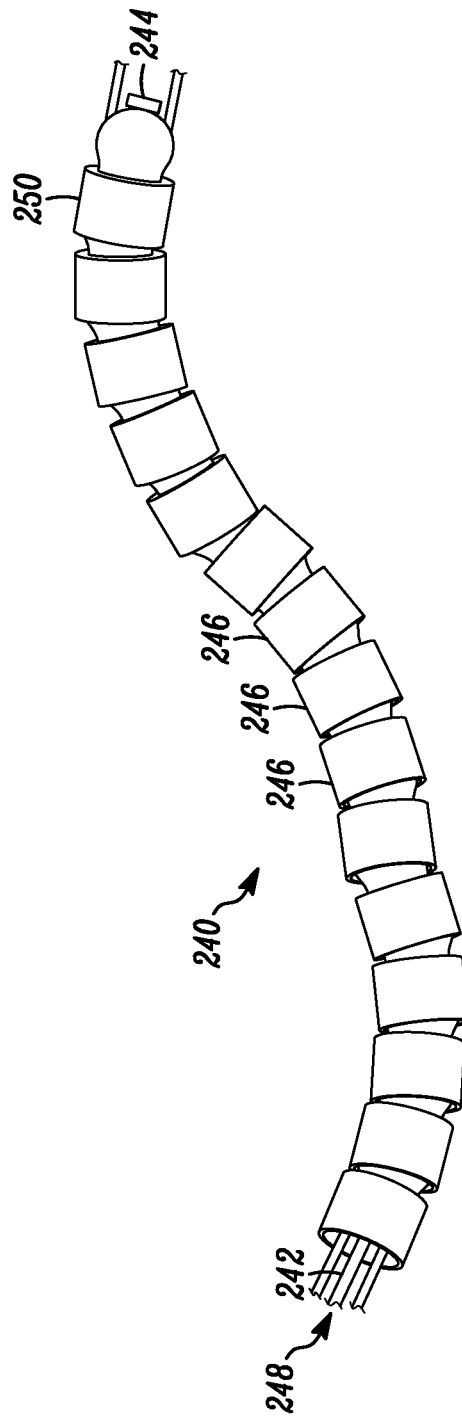


FIG. 11

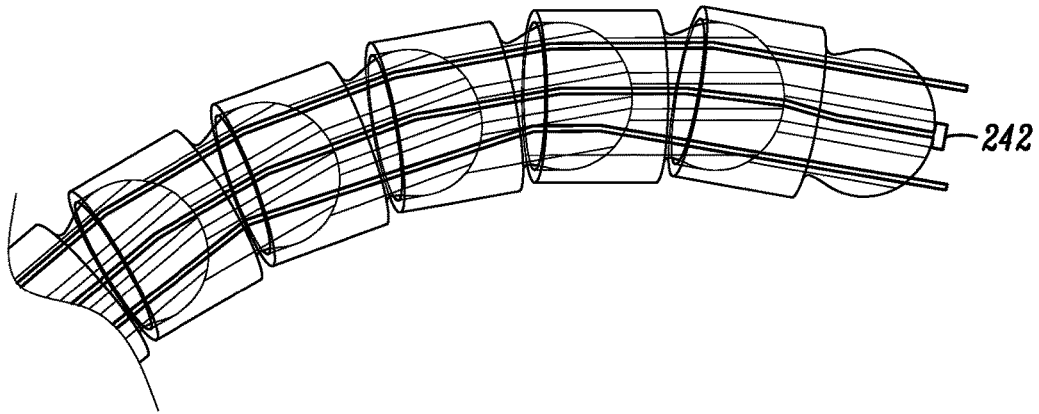


FIG. 12

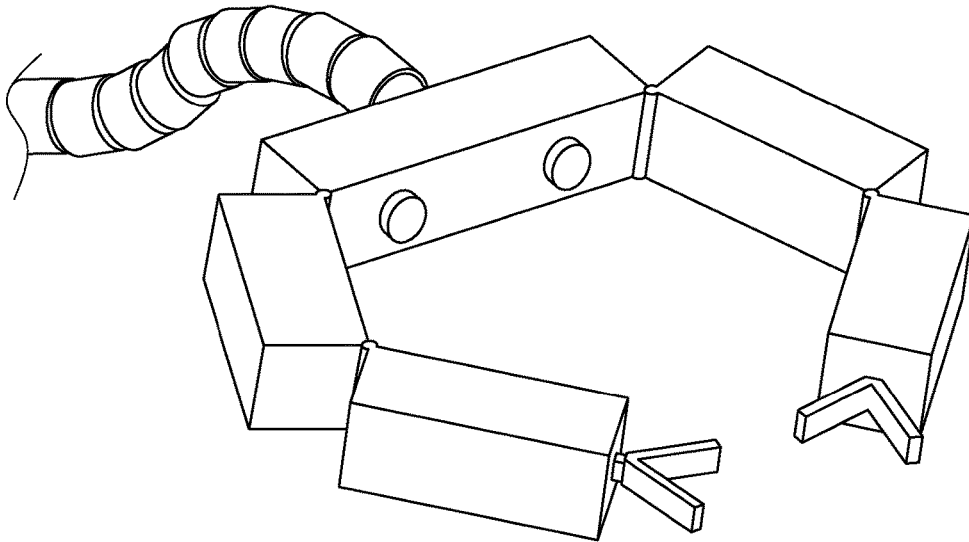


FIG. 13

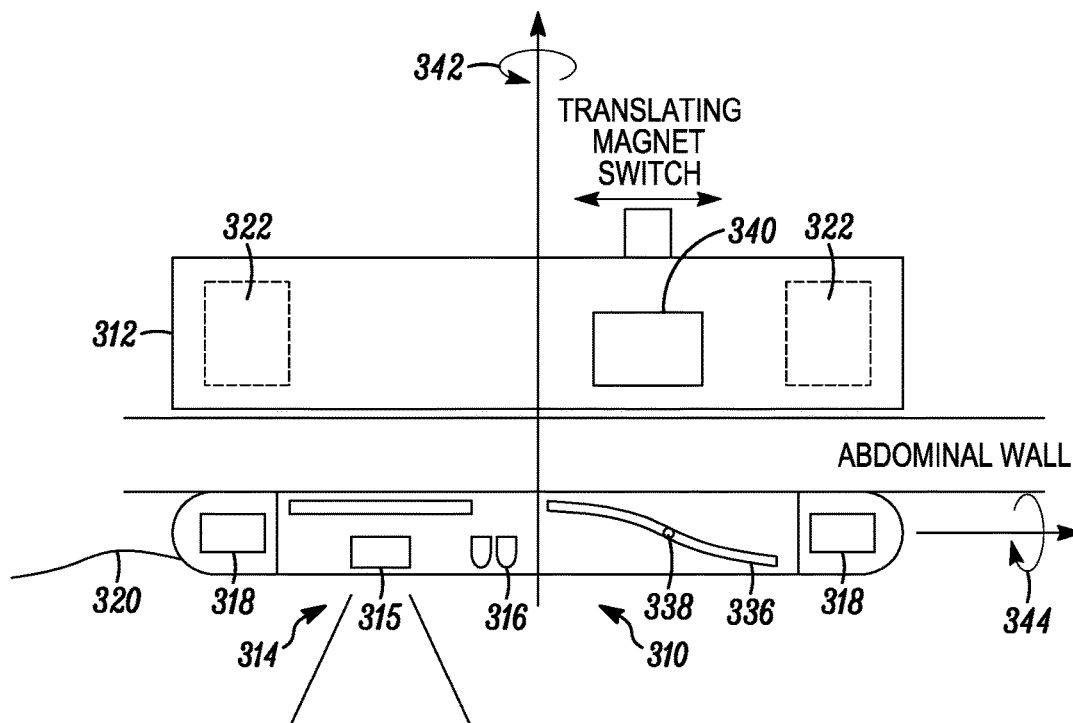


FIG. 14A

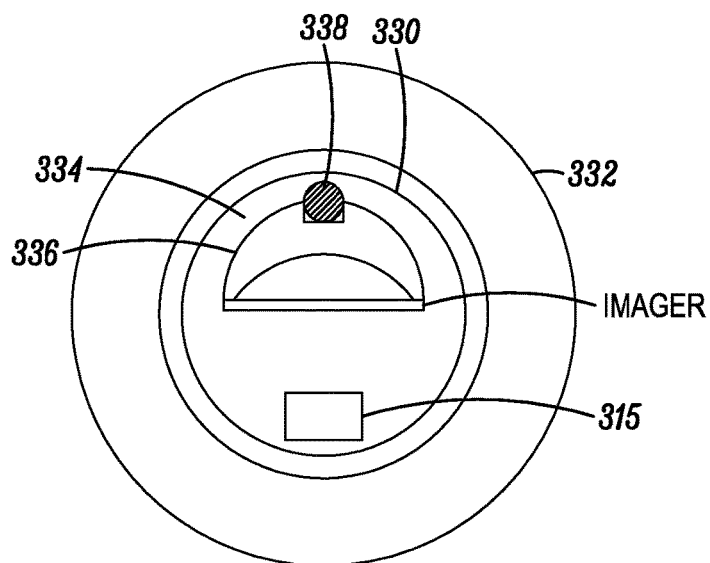


FIG. 14B

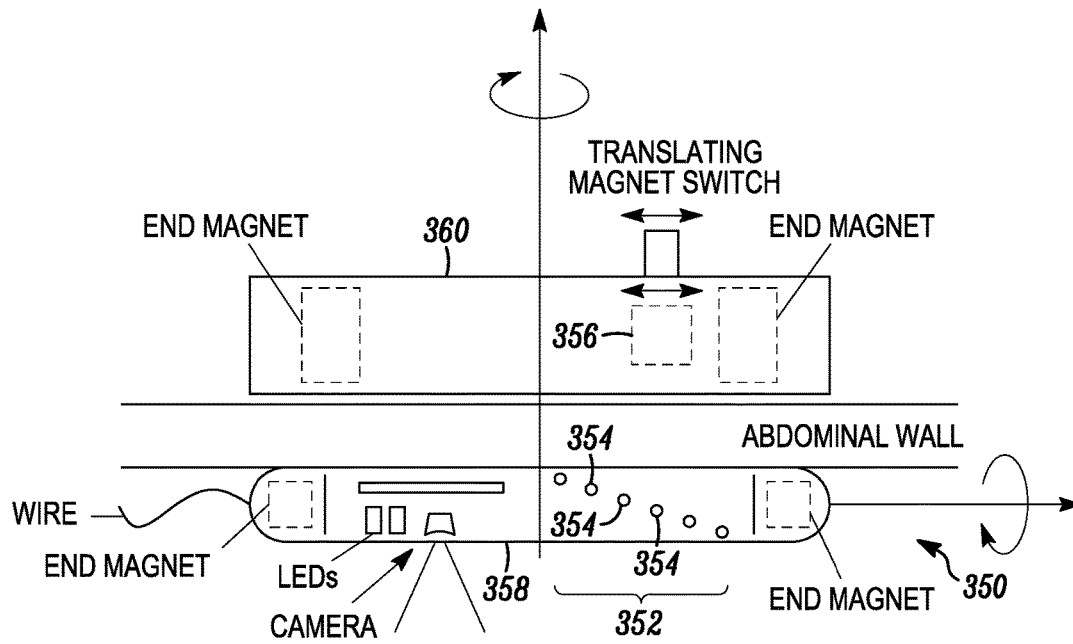


FIG. 15

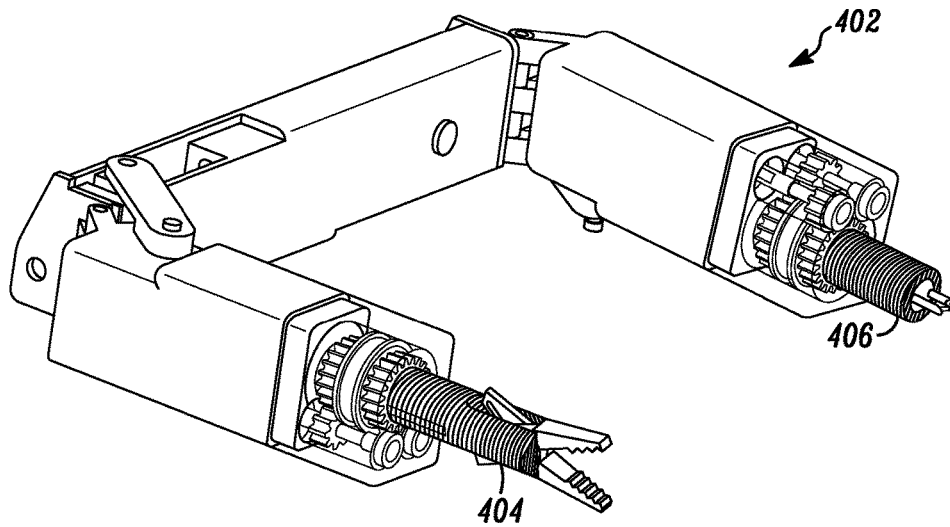


FIG. 16

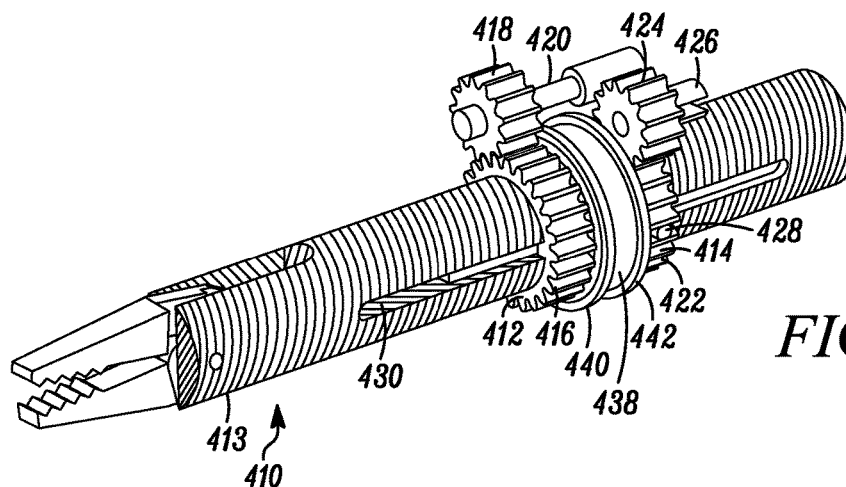


FIG. 17A

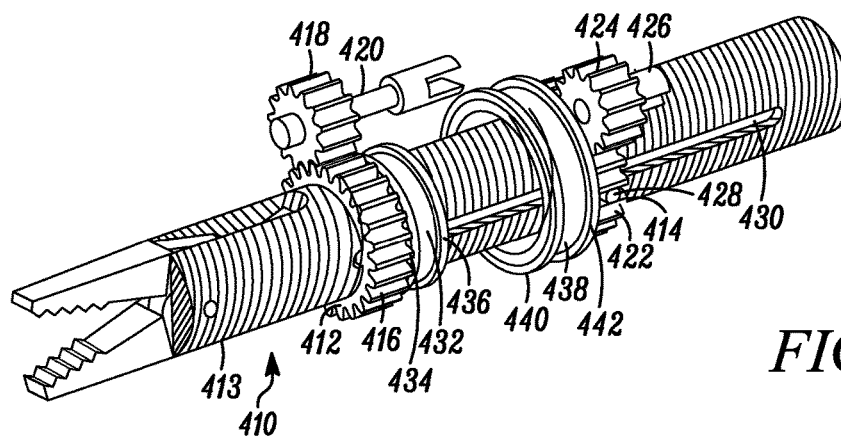


FIG. 17B

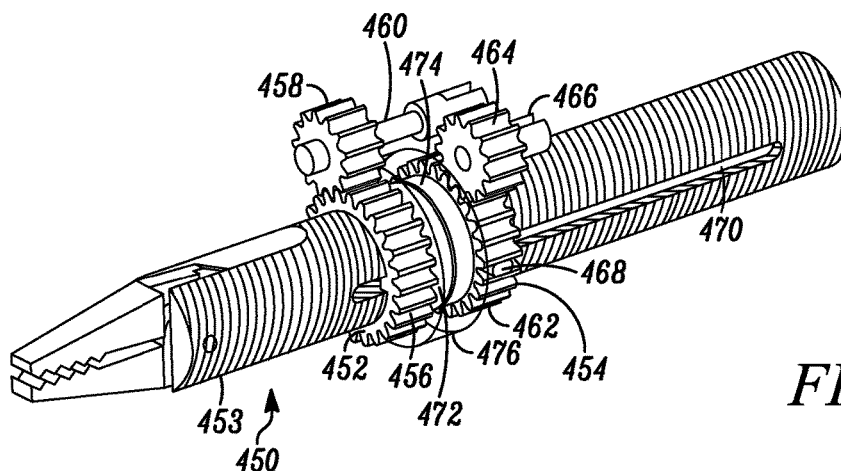
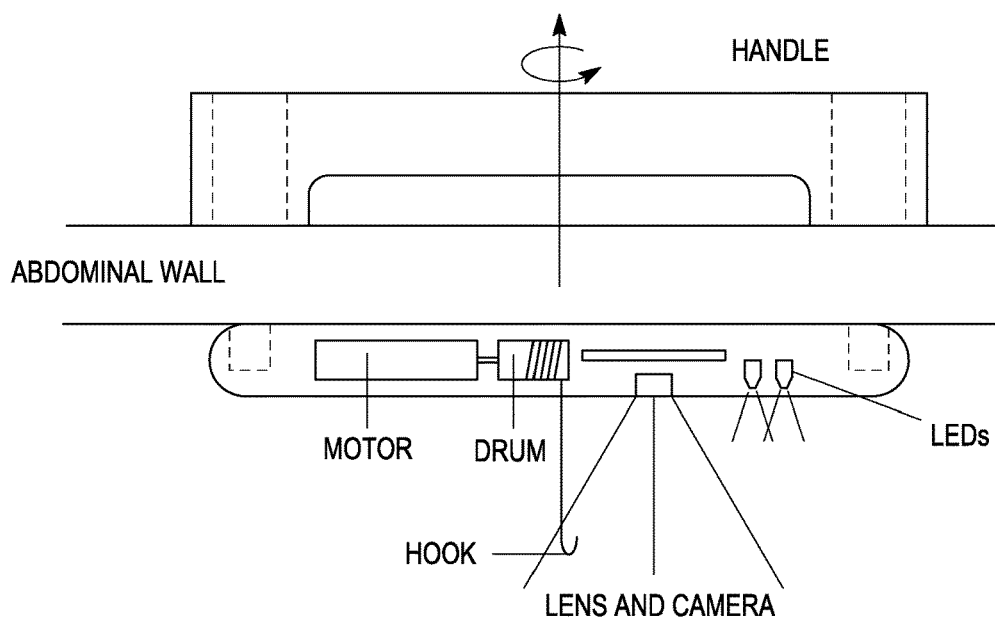
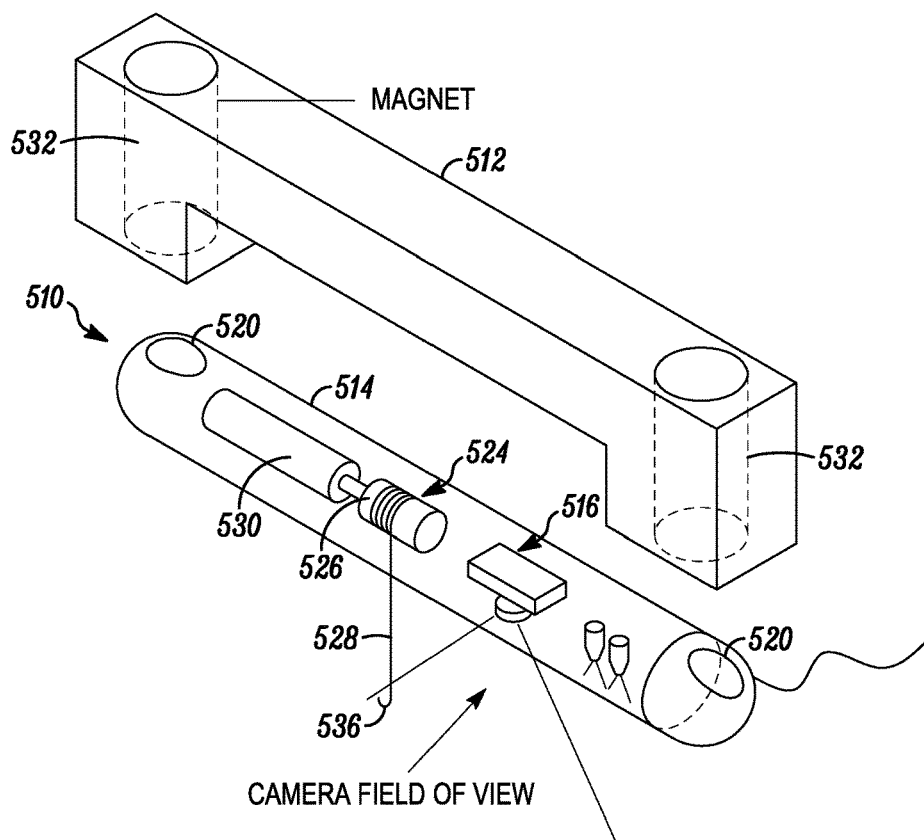


FIG. 18



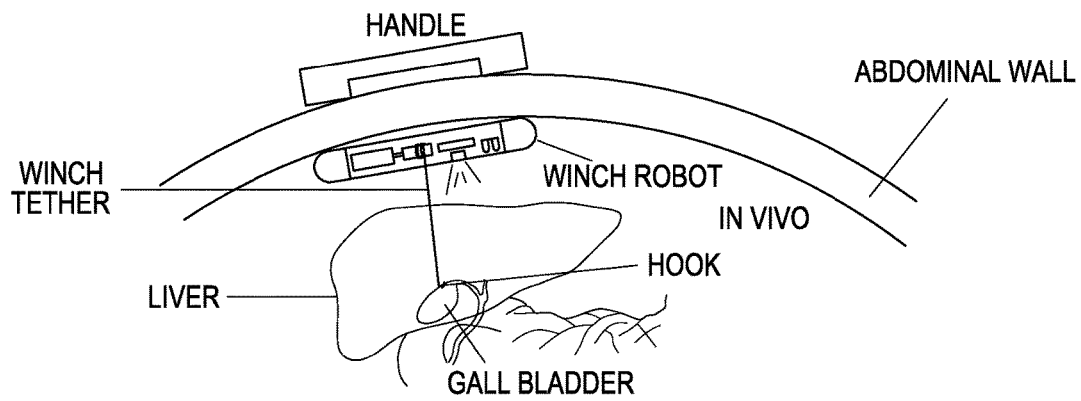


FIG. 20

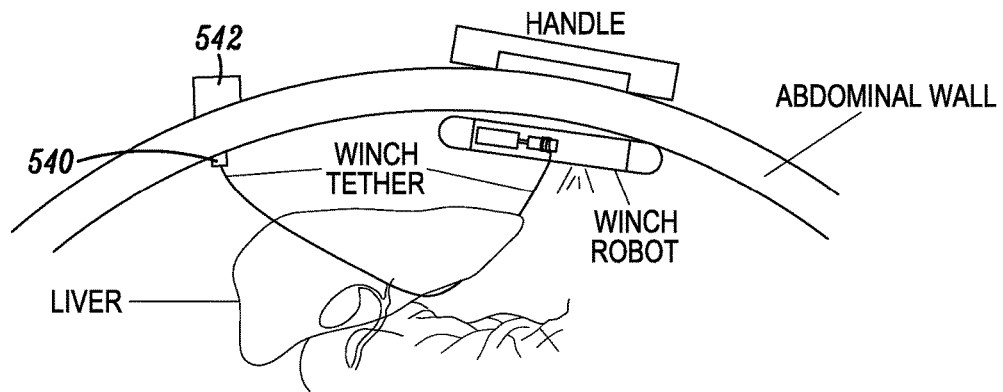


FIG. 21

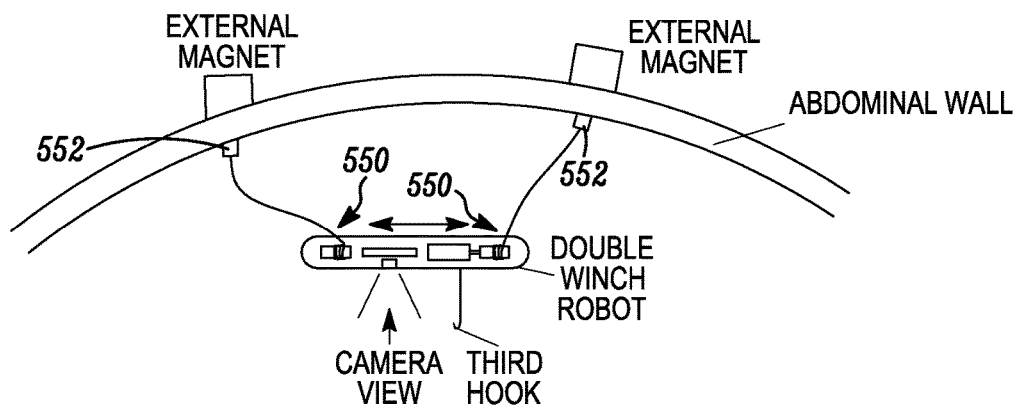


FIG. 22

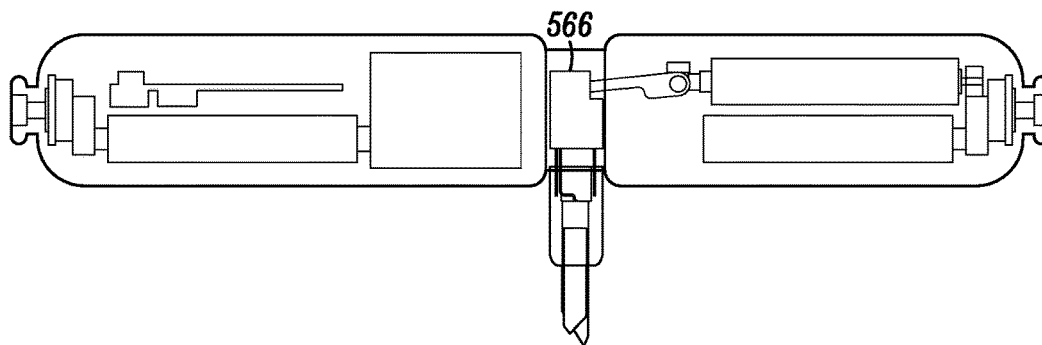


FIG. 23A

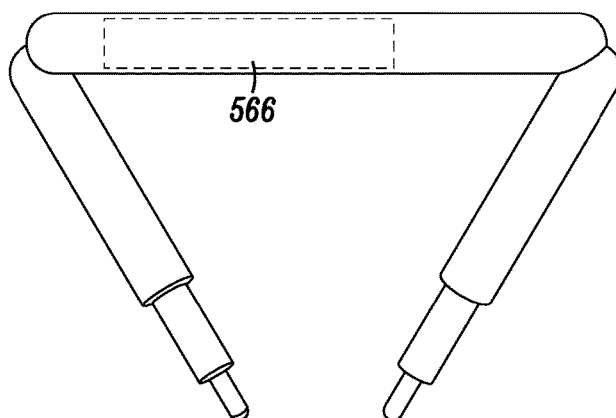
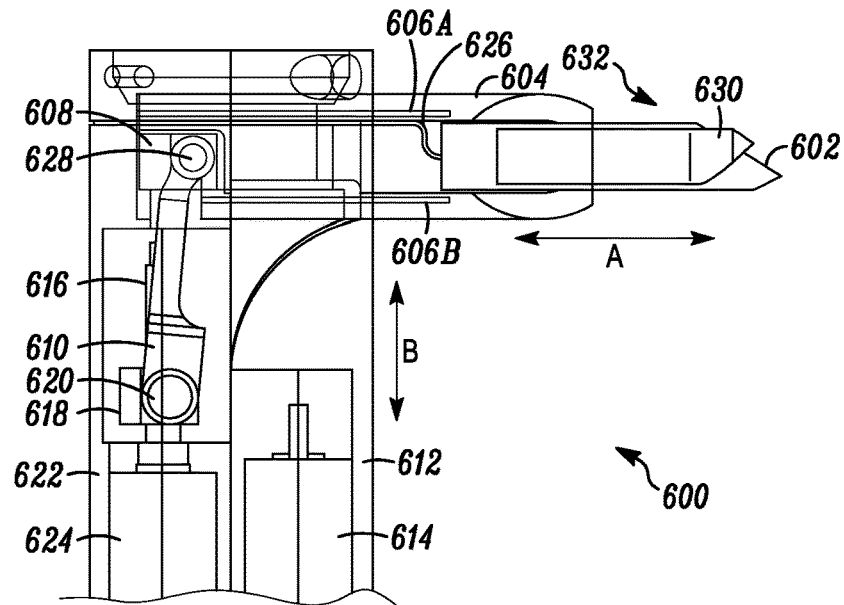
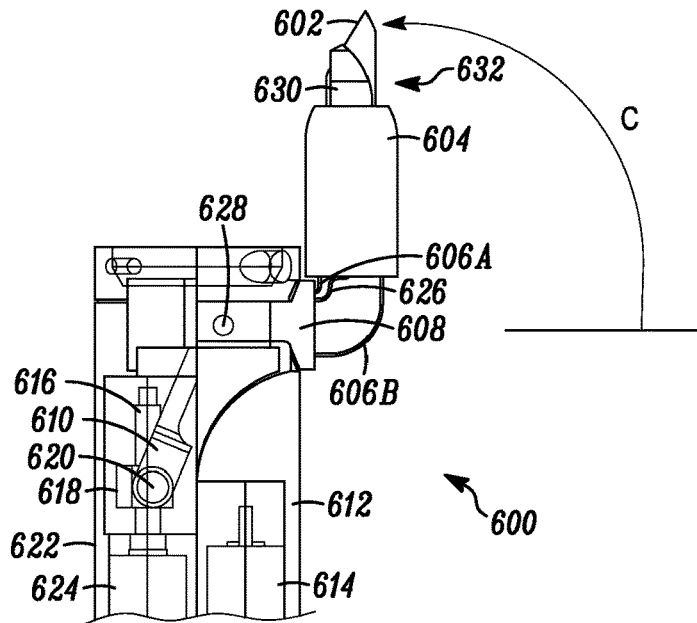


FIG. 23B

*FIG. 24A**FIG. 24B*

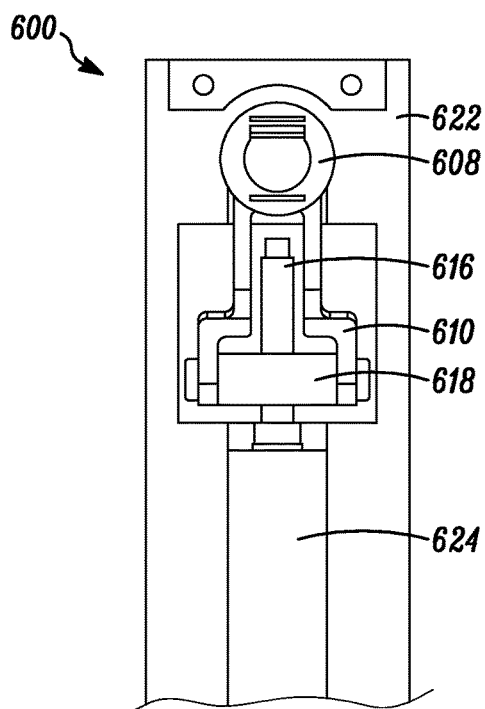


FIG. 24C

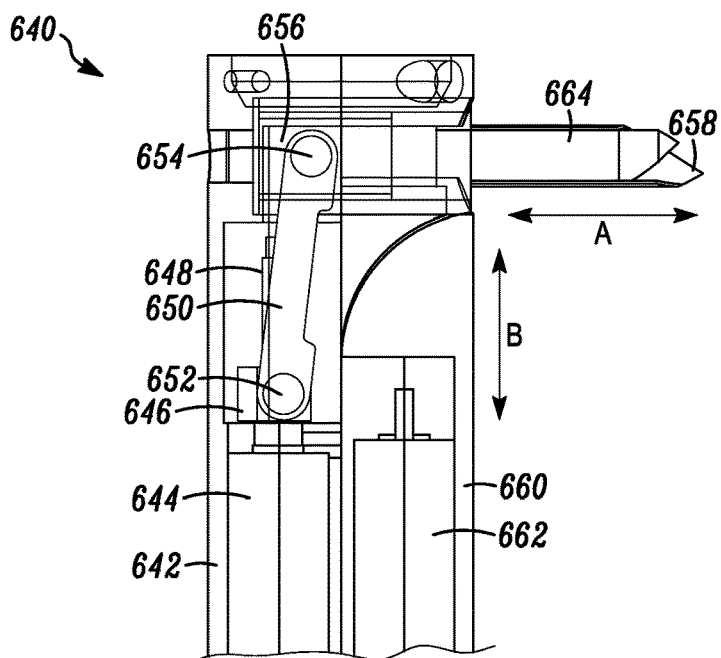


FIG. 25A

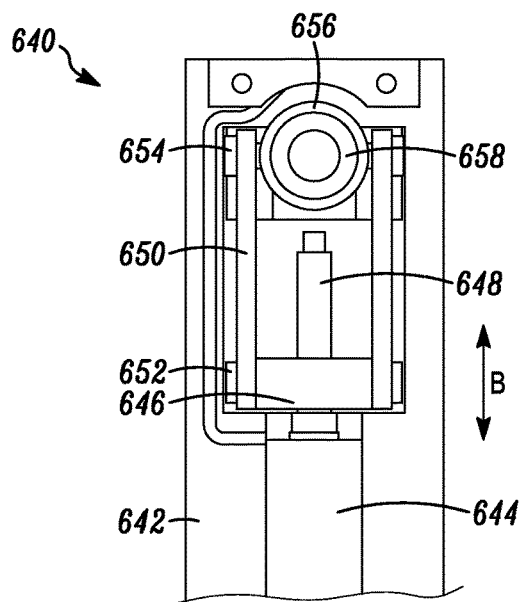


FIG. 25B

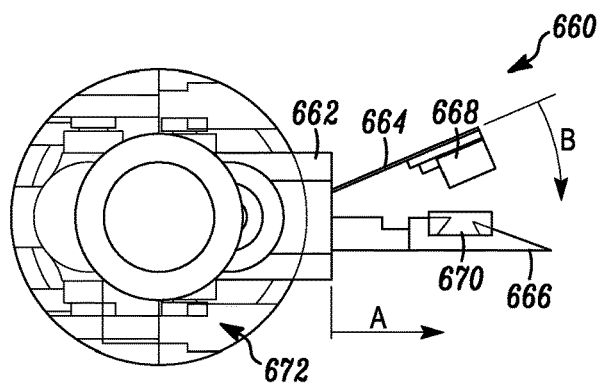


FIG. 26

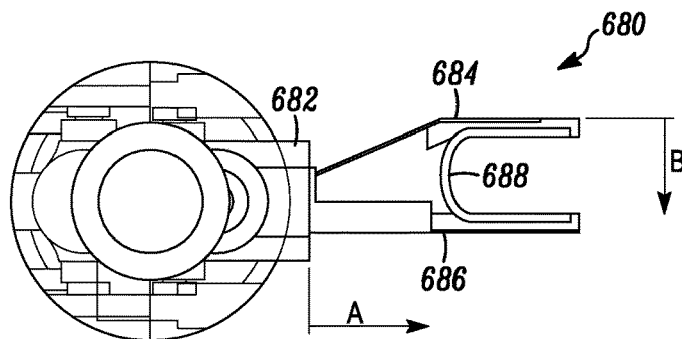


FIG. 27

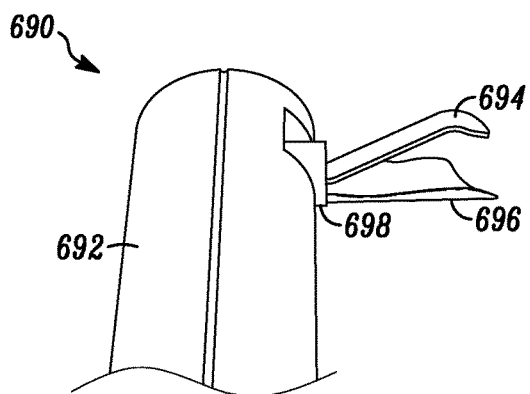


FIG. 28A

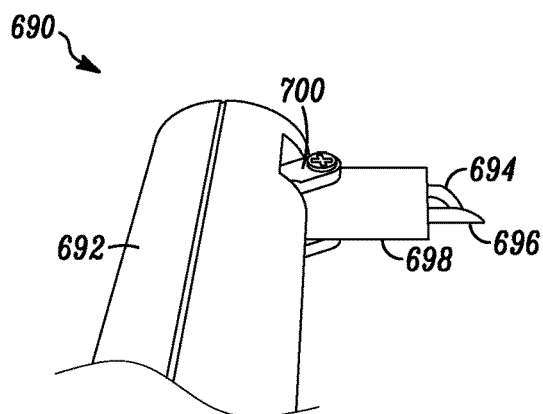


FIG. 28B

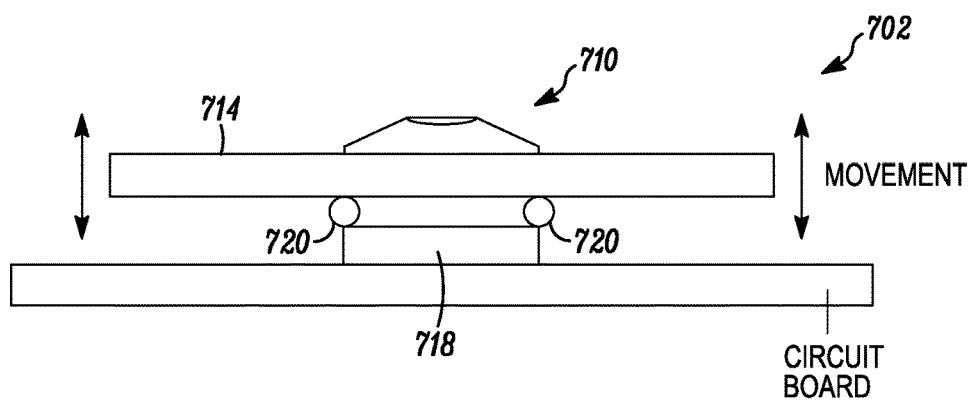


FIG. 29A

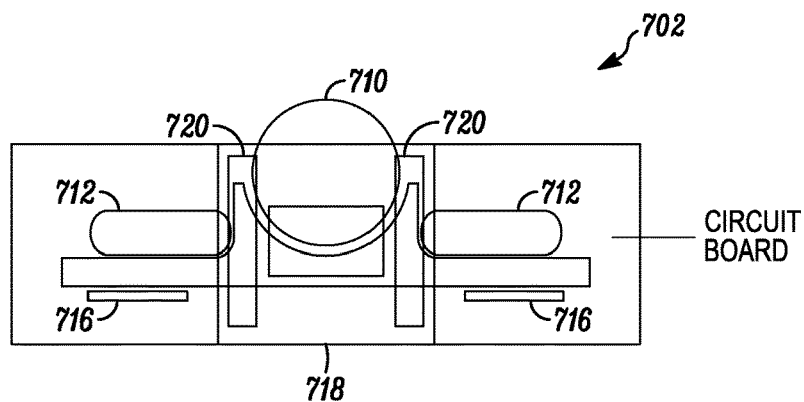


FIG. 29B

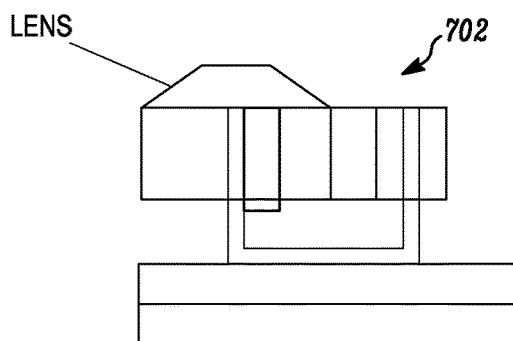


FIG. 29C

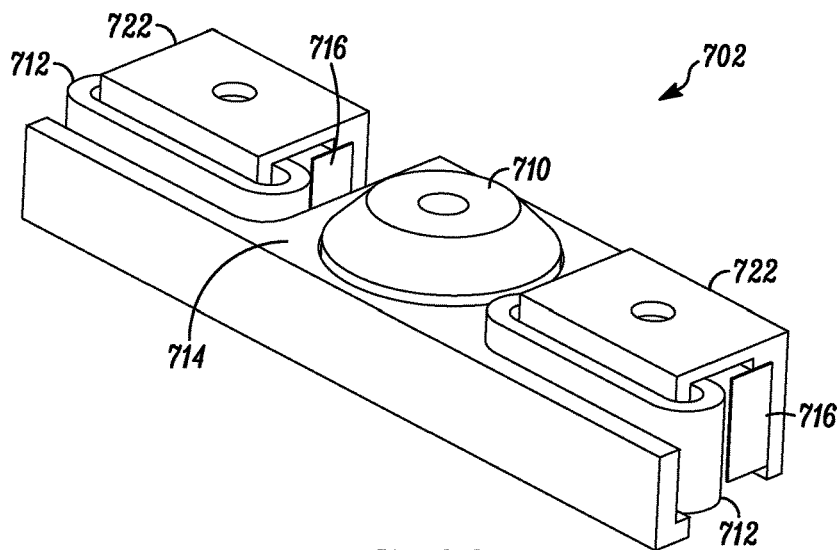


FIG. 29D

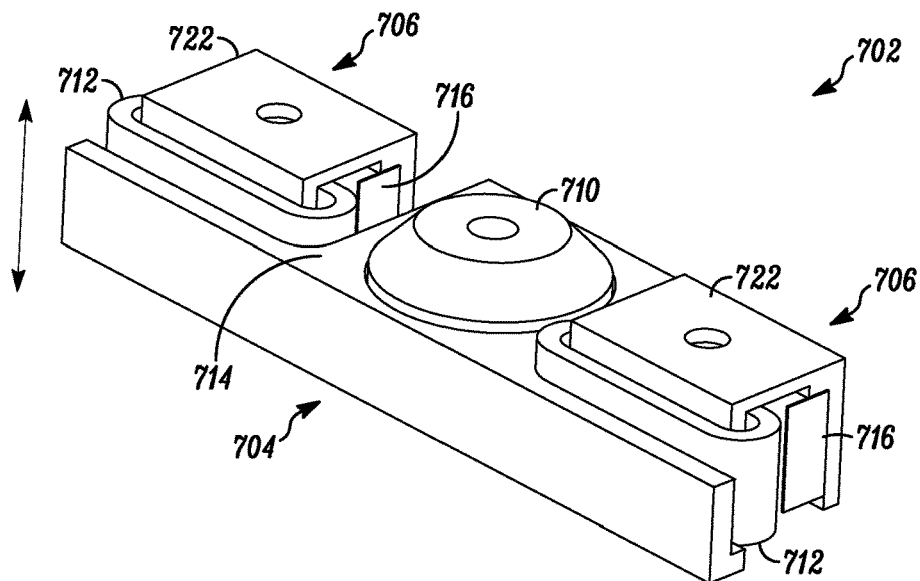


FIG. 29E

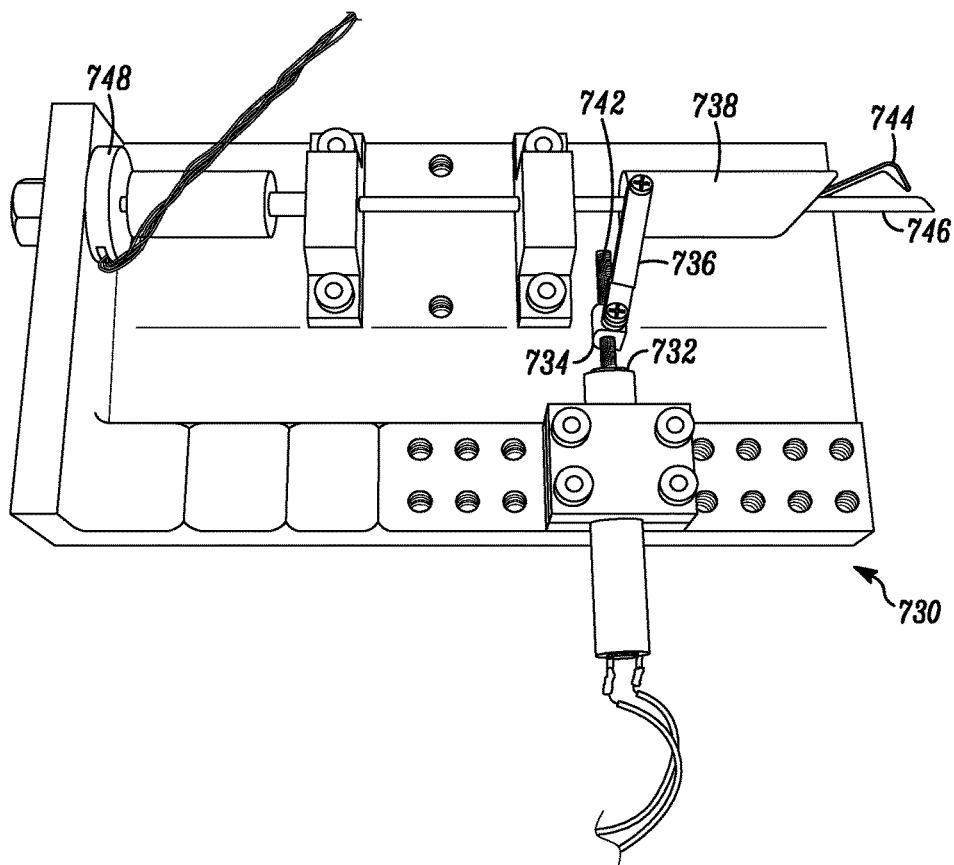


FIG. 30A

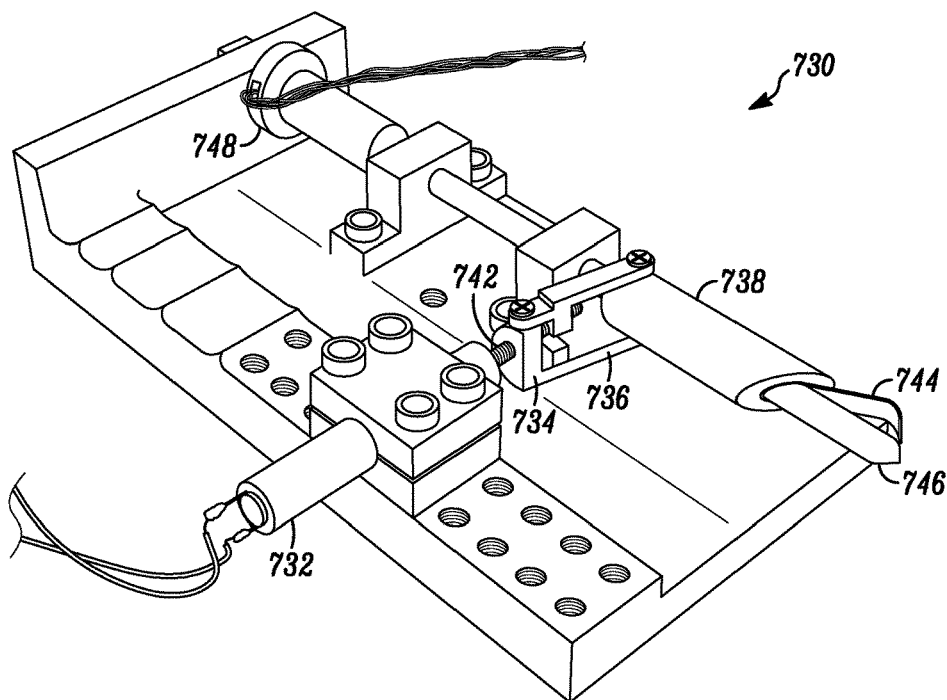


FIG. 30B

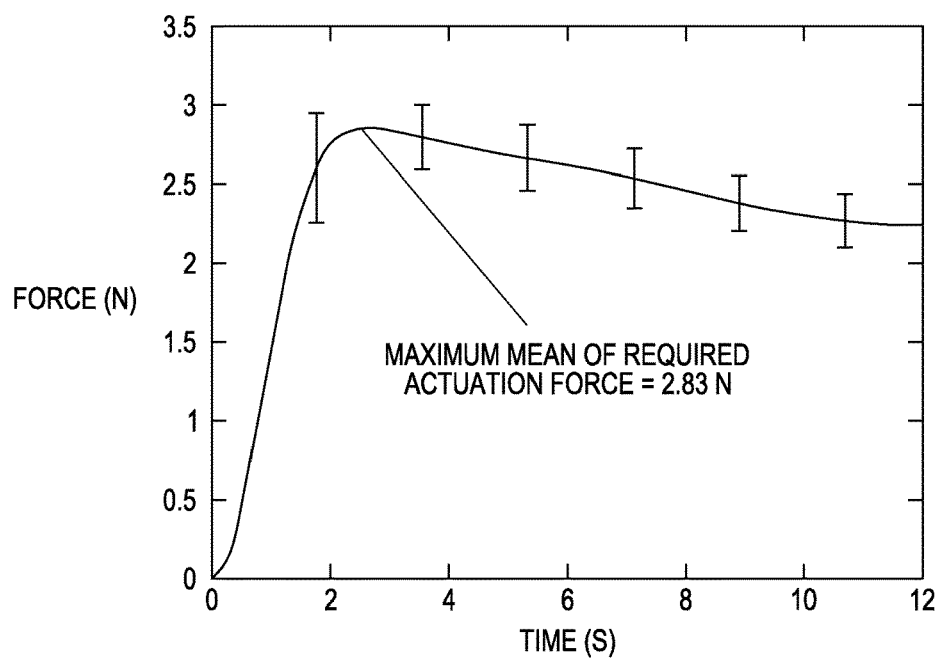


FIG. 31

1

METHODS, SYSTEMS, AND DEVICES FOR SURGICAL ACCESS AND PROCEDURES

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation application of U.S. application Ser. No. 13/329,705, filed on Dec. 9, 2011 and entitled "Methods, Systems, and Devices for Surgical Access and Procedures," now issued as U.S. Pat. No. 8,828,024, which is a continuation application of U.S. Pat. No. 8,343,171, filed on Jul. 11, 2008 and entitled "Methods and Systems of Actuation in Robotic Devices," both of which are hereby incorporated by reference in their entireties. Further, U.S. Pat. No. 8,343,171 claims priority to Provisional Application No. 60/949,390, filed Jul. 12, 2007; Provisional Application No. 60/949,391, filed Jul. 12, 2007; Provisional Application No. 60/990,076, filed Nov. 26, 2007; and Provisional Application No. 61/025,346, filed Feb. 1, 2008, all of which are hereby incorporated herein by reference in their entireties.

GOVERNMENT SUPPORT

This invention was made with government support under grant number R21 EB056632 awarded by the National Institutes of Health. The government has certain rights in the invention.

TECHNICAL FIELD

The embodiments disclosed herein relate to various medical device components, including components that can be incorporated into robotic and/or in vivo medical devices. Certain embodiments include various actuation system embodiments, including fluid actuation systems, drive train actuation systems, and motorless actuation systems. Further embodiments include various operational components for medical devices, including medical device arm mechanisms, medical device winch mechanisms, medical device biopsy/stapler/clamp mechanisms, and medical device adjustable focus mechanisms. Other embodiments relate to reversibly lockable tube mechanisms.

BACKGROUND

Invasive surgical procedures are essential for addressing various medical conditions. When possible, minimally invasive procedures such as laparoscopy are preferred.

However, known minimally invasive technologies such as laparoscopy are limited in scope and complexity due in part to 1) mobility restrictions resulting from using rigid tools inserted through access ports, and 2) limited visual feedback. Known robotic systems such as the da Vinci® Surgical System (available from Intuitive Surgical, Inc., located in Sunnyvale, Calif.) are also restricted by the access ports, as well as having the additional disadvantages of being very large, very expensive, unavailable in most hospitals, and having limited sensory and mobility capabilities.

There is a need in the art for improved surgical methods, systems, and devices.

SUMMARY

One embodiment disclosed herein relates to a biopsy component having a substantially fixed jaw component, a mobile jaw component adjacent to the substantially fixed

2

jaw component, and a sliding component configured to move between a first position and a second position. The mobile jaw component is predisposed to a position in which a distal end of the component is not in contact with the substantially fixed jaw component. Further, the sliding component in the second position is in contact with the mobile jaw component such that the sliding component urges the distal end of the mobile jaw component toward the substantially fixed jaw component.

Another embodiment disclosed herein relates to an arm device having an extendable rotational arm, a first drive component, a second drive component, a first driven component, a second driven component, and a pin. The extendable rotational arm has an exterior portion having a first coupling component and further has a first aperture defined within the arm. The first drive component is coupled with the first driven component, and the first driven component has an inner surface having a second coupling component that is configured to be coupled with the first coupling component. The second drive component is coupled with the second driven component, and the second driven component has a second aperture defined within it. The pin is disposed within the first and second apertures. According to one embodiment, the first and second coupling components are threads. In a further embodiment, the first and second drive components and first and second driven components are gears. Alternatively, the first and second drive components and the first and second driven components are a pulley system or a friction drive system.

Yet another embodiment disclosed herein relates to a medical device having a body, a first winch component and an actuation component. The first winch component has a first drum and a first tether operably coupled to the first drum. In one embodiment, the actuation component is operably coupled to the first drum. In an additional embodiment, the device further has an end effector operably coupled to the distal end of the tether. In yet another implementation, the device also has a second winch component having a second drum and a second tether operably coupled to the second drum. According to a further embodiment, the device also has a third winch component having a third drum and third tether operably coupled to the third drum.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1A is a schematic depicting a fluid actuation system, according to one embodiment.

FIG. 1B is a schematic depicting a valve component, according to one embodiment.

FIG. 2A shows a front view of a medical device having a fluid actuation system, according to one embodiment.

FIG. 2B depicts a front view of a medical device having a fluid actuation system, according to another embodiment.

FIG. 3 is a perspective view of a medical device, according to another embodiment.

FIG. 4 depicts a perspective view of a medical device joint, according to one embodiment.

FIG. 5 shows a perspective view of a medical device joint, according to another embodiment.

FIG. 6 is a perspective view of an operational component, according to one embodiment.

FIG. 7A depicts a front view of a medical device having a drive train system, according to one embodiment.

FIG. 7B shows a front view of a medical device having a drive train system, according to another embodiment.

3

FIG. 8 is a cutaway view of a reversibly lockable tube positioned in a target body cavity of a patient, according to one embodiment.

FIG. 9A depicts a perspective view of a modular tube component, according to one embodiment.

FIG. 9B shows another perspective view of the modular tube component of FIG. 9A.

FIG. 10 is a front view of a reversibly lockable tube, according to one embodiment.

FIG. 11 depicts a perspective view of the reversibly lockable tube of FIG. 10.

FIG. 12 shows a perspective view of a reversibly lockable tube, according to another embodiment.

FIG. 13 is a perspective view of a reversibly lockable tube, according to yet another embodiment.

FIG. 14A depicts a front view of a medical device having a motorless actuation component, according to one embodiment.

FIG. 14B shows a side view of the medical device of FIG. 14A.

FIG. 15 is a front view of a medical device having a motorless actuation component, according to another embodiment.

FIG. 16 depicts a perspective view of a medical device having an arm component, according to one embodiment.

FIG. 17A shows a perspective view of an arm component, according to one embodiment.

FIG. 17B is a perspective exploded view of the arm component of FIG. 17A.

FIG. 18 depicts a perspective view of an arm component, according to another embodiment.

FIG. 19A shows a perspective view of a medical device having a winch component, according to one embodiment.

FIG. 19B is a front view of the medical device having the winch component of FIG. 19A.

FIG. 20 depicts a cutaway view of a medical device utilizing a winch component during a procedure in a patient, according to one embodiment.

FIG. 21 shows a cutaway view of a medical device utilizing a winch component during a procedure in a patient, according to another embodiment.

FIG. 22 is a cutaway view of a medical device utilizing two winch components during a procedure in a patient, according to yet another embodiment.

FIG. 23A depicts a front view of a medical device having a payload area that is a biopsy mechanism, according to one embodiment.

FIG. 23B shows a front view of a medical device having a payload area, according to another embodiment.

FIG. 24A is a side view of a modular biopsy mechanism, according to one embodiment.

FIG. 24B depicts another side view of the modular biopsy component of FIG. 24A.

FIG. 24C shows a front view of the modular biopsy mechanism of FIGS. 24A and 24B.

FIG. 25A is a side view of a modular biopsy mechanism, according to another embodiment.

FIG. 25B depicts a front view of the modular biopsy mechanism of FIG. 25A.

FIG. 26 shows a top view of a biopsy mechanism, according to another embodiment.

FIG. 27 is a top view of another biopsy mechanism, according to yet another embodiment.

FIG. 28A depicts a perspective view of another biopsy mechanism, according to a further embodiment.

FIG. 28B shows a perspective view of the biopsy mechanism of FIG. 28A.

4

FIG. 29A is a side view of an adjustable focus component, according to one embodiment.

FIG. 29B depicts a top view of the adjustable focus component of FIG. 29A.

FIG. 29C shows an end view of the adjustable focus component of FIGS. 29A and 29B.

FIG. 29D is a perspective view of the adjustable focus component of FIGS. 29A, 29B, and 29C.

FIG. 29E depicts a perspective view of the adjustable focus component of FIGS. 29A, 29B, 29C, and 29D.

FIG. 30A shows a top view of a laboratory test jig used to measure forces applied by a biopsy mechanism, according to one embodiment.

FIG. 30B is a perspective view of the test jig and biopsy mechanism of FIG. 30A.

FIG. 31 depicts a line graph relating to data collected from the operation of the test jig depicted in FIGS. 30A and 30B.

DETAILED DESCRIPTION

The various systems and devices disclosed herein relate to devices for use in medical procedures and systems. More specifically, the various embodiments relate to various actuation or end effector components or systems that can be used in various procedural devices and systems.

It is understood that the various embodiments of actuation, end effector, and other types of device components disclosed herein can be incorporated into or used with any known medical devices, including, but not limited to, robotic or in vivo devices as defined herein.

For example, the various embodiments disclosed herein can be incorporated into or used with any of the medical devices disclosed in copending U.S. application Ser. No. 11/932,441 (filed on Oct. 31, 2007 and entitled "Robot for Surgical Applications"), Ser. No. 11/695,944 (filed on Apr. 3, 2007 and entitled "Robot for Surgical Applications"), Ser. No. 11/947,097 (filed on Nov. 27, 2007 and entitled "Robotic Devices with Agent Delivery Components and Related Methods"), Ser. No. 11/932,516 (filed on Oct. 31, 2007 and entitled "Robot for Surgical Applications"), Ser. No. 11/766,683 (filed on Jun. 21, 2007 and entitled "Magnetically Coupleable Robotic Devices and Related Methods"), Ser. No. 11/766,720 (filed on Jun. 21, 2007 and entitled "Magnetically Coupleable Surgical Robotic Devices and Related Methods"), Ser. No. 11/966,741 (filed on Dec. 28, 2007 and entitled "Methods, Systems, and Devices for Surgical Visualization and Device Manipulation"), 60/949,391 (filed on Jul. 12, 2007), 60/949,390 (filed on Jul. 12, 2007), 60/990,062 (filed on Nov. 26, 2007), 60/990,076 (filed on Nov. 26, 2007), 60/990,086 (filed on Nov. 26, 2007), 60/990,106 (filed on Nov. 26, 2007), 60/990,470 (filed on Nov. 27, 2007), 61/025,346 (filed on Feb. 1, 2008), 61/030,588 (filed on Feb. 22, 2008), and 61/030,617 (filed on Feb. 22, 2008), all of which are hereby incorporated herein by reference in their entireties.

In an exemplary embodiment, any of the various embodiments disclosed herein can be incorporated into or used with a natural orifice transluminal endoscopic surgical device, such as a NOTES device. Those skilled in the art will appreciate and understand that various combinations of features are available including the features disclosed herein together with features known in the art.

Certain device implementations disclosed in the applications listed above can be positioned within a body cavity of a patient, including certain devices that can be positioned against or substantially adjacent to an interior cavity wall, and related systems. An "in vivo device" as used herein

means any device that can be positioned, operated, or controlled at least in part by a user while being positioned within a body cavity of a patient, including any device that is positioned substantially against or adjacent to a wall of a body cavity of a patient, further including any such device that is internally actuated (having no external source of motive force), and additionally including any device that may be used laparoscopically or endoscopically during a surgical procedure. As used herein, the terms “robot,” and “robotic device” shall refer to any device that can perform a task either automatically or in response to a command.

Certain embodiments disclosed herein relate to actuation components or systems that are configured to provide motive force to any of the various procedural device embodiments described above. One such embodiment is a fluid actuation system. FIG. 1A schematically depicts one embodiment of a fluid actuation system 10 for a procedural device. According to one implementation, the fluid actuation system 10 is a hydraulic system. Alternatively, the fluid actuation system 10 is a pneumatic system. In a further alternative, the fluid actuation system can be any known such system. Hydraulic systems are generally preferred for higher power transmission, while pneumatic systems can be a good actuation system for binary actuation, such as actuation required for a grasper. In the hydraulic embodiment depicted in FIG. 1A, the system 10 includes a medical device 12 that is connected via a hydraulic connection line 20 to external hydraulic components 22. The device 12 as shown has a hydraulic piston assembly 14 having a piston 16 positioned within a cylinder 18. The piston assembly 14 can be used for any actuation associated with the device 12, such as powering movement of the device 12 in relation to the patient's body, actuating a component of the device to perform an action, or any other desired actuation.

As further shown in FIG. 1A, the piston assembly 14 is connected via a hydraulic connection line 20 to the external hydraulic components 22, which include a reservoir 24, a pump 26, and an accumulator 28. The external hydraulic components 22 are positioned at a location external to the patient's body. Thus, the hydraulic connection line 20 is connected to the piston assembly 14 in the device 12 through the valve component 30 and to the external hydraulic components 22 such that the line 20 extends from the interior of the patient's body to the exterior when the device 12 is positioned in the patient's body. According to one embodiment, the line 20a that couples the accumulator 28 to the valve component 30 is a high pressure supply line 20a that provides fluid to the valve component 30 under high pressure. In accordance with a further implementation, the line 20b that couples the valve component 30 to the reservoir 24 is a low pressure supply line 20b that allows fluid to move from the valve component 30 to the reservoir 24 under low pressure.

In one embodiment, the hydraulic fluid used in the hydraulic system 10 is saline solution. Alternatively, the fluid is water-based. In a further alternative, the hydraulic fluid can be any fluid that is non-toxic, biocompatible, and less compressible as required to provide sufficient precise control.

In one implementation, the external hydraulic components 22 are the reservoir 24, pump 26, and accumulator 28 as discussed above, which operate in known fashion to hydraulically power the piston assembly 14. In one example, the pump 26 used in this system is a commercially-available surgical irrigation pump, while the accumulator 28 and reservoir 24 are commercially available from Parker Hannifin, which is located in Cleveland, Ohio. Alternatively, the

external hydraulic components 22 can be any known configuration of any hydraulic components capable of hydraulically powering the piston 16.

According to one implementation of a fluid actuation system, the piston 16 is a standard syringe handle and the cylinder 18 is the syringe body. Alternatively, the piston assembly 14 can be a small commercially available system used for model airplane landing gear. In a further embodiment, the piston 16 is custom machined with an o-ring around the piston head, while the cylinder 18 is a machined or molded cavity within the robot's base or arms.

The valve component 30 has a valve for each piston assembly 14. Thus, the valve component 30 may have anywhere from one valve to any number equal to the maximum number of valves provided in the system.

Another example of a valve component 32 is provided in FIG. 1B. In this embodiment, the component 32 has six valves 34. The fluid is provided at high pressure through the high pressure supply line 36a and exits the valve component 32 at a low pressure through the low pressure line 36b. In addition, the valves 34 are each coupled to a respective piston assembly 38 as shown. According to one embodiment, such a valve component 30 (also referred to as a “valve system”) is sold by Parker Hannifin.

As mentioned above, the fluid actuation systems depicted in FIGS. 1A and 1B can alternatively be a pneumatic system. Returning to FIG. 1A, in this embodiment of a pneumatic system 10, the external pneumatic components 22 are disposed externally to the patient's body. Thus, the pneumatic connection line 20 is connected to the valve component 30 in the medical device 12 and to the external pneumatic components 22 such that the line 20 extends from the interior of the patient's body to the exterior when the device 12 is positioned in the patient's body.

According to one embodiment of a pneumatic system, in place of the pump 26, accumulator 28, and reservoir 24, the external pneumatic component 22 is a pressurized cylinder (not shown). In this embodiment, the return air is emitted into the external environment of the system. One example of a pressurized cylinder is a canister of readily-available carbon dioxide, which is commonly used to insufflate the abdominal cavity during laparoscopic surgery. Alternatively, the external pneumatic components 22 can be any known configuration of any pneumatic components capable of pneumatically powering the piston 16.

FIGS. 2A and 3 depict a robotic device 40 with a hydraulic system, according to one embodiment. The device 40 has six piston assemblies 42a, 42b, 42c, 42d, 42e, 42f. Piston assemblies 42a and 42b are disposed within the body 44 of the device 40 and actuate the first links 48a, 48b of the robotic arms 46a, 46b. Piston assemblies 42c, 42d are disposed within the first links 48a, 48b and actuate the second links 50a, 50b. In addition, piston assemblies 42e, 42f are disposed within the second links 50a, 50b and actuate the operational components 52, 54.

Alternatively, the device 40 can have from one to any number of piston assemblies that can be integrated into the robotic device as actuation components. According to one embodiment, a piston is provided for each degree of freedom.

According to one embodiment as shown in FIG. 2B, the external components of the hydraulic system 56 provide a high pressure supply line 57a to the robotic device and receive a low pressure return line 57b from the device. In a further embodiment, the robotic device has a system of valves or a master valve system 58 that controls the hydrau-

lic fluid flow and directs the fluid as needed to the piston assemblies, such as the assemblies depicted in FIGS. 2A and 3.

FIG. 4 depicts a robotic device joint 60 connecting a link 62 to the robotic body 64, according to one embodiment. The body 64 has a piston assembly 66 in which the piston 68 is coupled to a pin 70 that is coupled in turn to the link 62 at the connection point 72. In one implementation, the link 62 is a first link 62 such that the joint 60 is a joint 60 between a robotic body 64 and a first link 62 (also referred to as a “shoulder joint”).

FIG. 5 depicts a robotic device joint 80 connecting a first link 82 to a second link 84, according to one embodiment. The first link 82 has a piston assembly 86 in which the piston 88 is coupled to a pin 90 that is coupled in turn to the second link 84 at the connection point 92. In one implementation, the joint 80 between the two links 82, 84 is referred to as an “elbow joint.”

FIG. 6 depicts an operational component 100 coupled to a robotic arm 102, according to one embodiment. The robotic arm 102 has a piston assembly 104 in which the piston 106 is coupled to a portion of the operational component 100. More specifically, the piston 106 is coupled to a sliding component 108 at a connection point 110, wherein the sliding component is slidably positioned in the arm 102 such that the force created by the piston assembly 104 is translated to the sliding component 110, causing the sliding component 110 to slide back and forth in the arm 102.

The operational component 100 is coupled to the sliding component 110 at joint 112 such that the sliding back and forth of the sliding component 110 causes the operational component 100 to extend and retract relative to the arm 102. This allows for the lengthening and shortening of the reach of the operational component 100 with respect to the arm 102 and the procedural space in which the operational component 100 is operating. Stated in another way, according to one embodiment, this slidable coupling of the sliding component 110 and the arm 102 is considered to be the “wrist” of the arm 102, wherein the sliding of the sliding component 110 back and forth operates to lengthen and shorten the “wrist” in relation to the rest of the arm 102.

In one embodiment, an actuator (not shown) disposed in the sliding component 108 actuates the operational component 100. For example, in the embodiment depicted in FIG. 6 in which the operational component 100 is a set of graspers 100, the actuator actuates the graspers to move between the open and closed positions.

It is understood that a pneumatic system could be incorporated into any of the embodiments and components depicted in FIGS. 2A, 2B, and 3-6 and could operate in generally the same fashion as discussed above. It is further understood that any other type of fluid actuation system could also be implemented in any of these embodiments in generally the same fashion.

In accordance with one implementation, a device having a fluid actuation system such as the various systems disclosed herein could reduce costs associated with the device. That is, the components of the system associated with the device can be integrated into the device at a low cost (in comparison to devices having costly onboard motors, etc.), while the more expensive components can be incorporated into the external components of the system and thus can be re-used for extended periods of time. In another embodiment, the use of a fluid actuation system in a device can provide increased force and/or speed in comparison to internal motors.

In a further alternative embodiment, the device is a “hybrid” that has at least one piston and at least one motor, thereby providing for further flexibility in the configuration of the device and the capability of accomplishing very precise motions. For example, the precise motions could include motions of the wrist such as rotation or extension that might require very precise control for delicate tissue dissection. In such an embodiment, the fluid actuation piston assemblies could be used for purposes of gross and/or quick actuations that require greater power, such as actuation of the shoulder and/or elbow joints, while the motor assemblies could be used for purposes of precise, slower actuations, such as actuation of the wrist or operational component for precise tasks such as dissection. In this context, the fluid actuation assemblies of the shoulder and elbow joints could then subsequently be used for the pulling or cutting motions that require greater power.

In addition to the fluid actuation systems described above, yet another actuation system that can be implemented with the various medical devices disclosed or incorporated herein is a drive train system. One exemplary implementation of a drive train system is shown in FIG. 7A, which depicts a robotic device 202 mechanically powered or actuated with a drive train system 200. The system 200 has a drive component 204 that is coupled to the robotic device 202 and thereby provides mechanical force to the device 202.

In one embodiment as shown in FIG. 7B, the drive component 204 includes a series of axles and couplers that are connected to each other and to an actuation component 212 (which, according to one implementation, can be a drive motor 212) and ultimately are connected to the device 202. More specifically, the drive component 204 includes the drive shaft 214, the first coupling component 215, the second coupling component 216, the connecting shaft 217, and the third coupling component 218. According to one embodiment, the first, second, and third coupling components 215, 216, 218 are coupleable gears. In operation, the actuation component 212 depicted in FIG. 7B powers the drive component 204 by actuating the drive shaft 214. The rotation of drive shaft 214 powers the rotation of the connecting shaft 217 via the first and second coupleable gears 215, 216. The power is then transferred to the medical device 202 via the third gear 218.

Alternatively, the drive component 204 is a flexible rod that is capable of transferring rotational power to the device 202. In a further embodiment, the drive component 204 is any known drive component capable of transferring power to a robotic device 202.

As shown in FIGS. 7A and 7B, this particular embodiment relates to a drive component 204 that is positioned inside a needle, port, or other kind of insertion component 206 that is connected to a device 202 positioned inside the patient’s body. Alternatively, the insertion component 206 is an opening or channel that provides for access or connection to the device 202 inside the patient’s body. More specifically, in the embodiment depicted in FIG. 7, the insertion component 206 is a trocar-like port 206 that is inserted through an incision 208 in the patient, such as an incision 208 through the abdominal wall 210. The drive component 204 is then positioned within the port 206 and coupled to the device 202 positioned in the patient’s body cavity.

As described above, the drive component 204 can be a rotary shaft 204 that supplies rotational actuation to the device 202. In one exemplary implementation, the shaft 204 has a series of clutches (not shown) that transfer the actuation to the piston assemblies or other translation assemblies for actuation of the joints and other actuable components.

The miniature clutches are common components that are available commercially from Small Parts, Inc., located in Miami Lakes, Fla. In one embodiment, the clutches are operated hydraulically. Alternatively, the clutches are operated electrically or by any other known method.

In a further alternative implementation, the drive component **204** winds one or more onboard tensionable springs that can then be used to provide power to the end effectors or other drivable/driven components in the device through a clutch system.

Alternatively, the rotary shaft **204** is a flexible rod **204**. In this embodiment, the insertion component **206** does not necessarily need to be straight. In one example, the insertion component **206** is inserted through the esophagus of the patient and into the abdominal cavity through an incision in the stomach wall. The inner flexible rod **204** is positioned within the insertion component **206** and coupled to the robotic device **202**. In this example, the flexible rod **204** is rotated to provide rotational actuation to the robotic device **202**.

One component that can be used in conjunction with any fluid actuation or drive train actuation system such as those systems described above is a reversibly lockable tube. As used herein, “reversibly lockable tube” is intended to mean any tubular component that can be switched, adjusted, or otherwise changed between a flexible configuration and a locked configuration (in which “locked” is intended to encompass any level of substantial rigidity). This adjustability between flexible and rigid configurations shall also be referred to herein as the “reversibly lockable” feature. Please note that the term “tube” as used herein is intended to encompass any tubular or hose-like component that provides access to various cavities of a patient’s body for medical procedure devices and/or connection to such devices positioned in the patient’s body.

FIG. **8** provides one exemplary depiction of an embodiment of a reversibly lockable tube **220** coupled to a robotic device **222** that is positioned in the target body cavity of the patient. As discussed above, one embodiment of the tube **220** can be adjusted between a flexible configuration and a rigid or “locked” configuration. In use, such components as a hydraulic or pneumatic actuation system as described above can be disposed within the tube **220**, along with any other components that connect a robotic device disposed within the patient’s body with components positioned externally to the patient’s body. More specifically, the tube **220** is maintained in its flexible configuration while the tube **220** is being positioned through an orifice into a patient’s body such as through the mouth and esophagus of the patient as depicted in FIG. **8**. Once the tube **220** has been positioned, the tube **220** can be adjusted into the locked configuration during operation of the device **222**. The operation of the various lockable tube embodiments disclosed herein will be described in further detail below.

FIGS. **10** and **11** depict a reversibly lockable tube **240** according to one embodiment that is made up of multiple modular tube components (also referred to herein as “links”).

One example of modular tube components **260** (such as those used in the tube **240** shown in FIGS. **10** and **11**) is depicted in FIGS. **9A** and **9B**. FIG. **9A** depicts the male end **262** (or “protrusion”), while FIG. **9B** depicts the female end **264**. As shown in FIG. **9A**, the male end **262** is a convex protrusion. Alternatively, the male end **262** can be any form of protrusion that mates with the female end **264**. As shown in FIG. **9B**, the female end **264** is a concave formation.

Alternatively, the female end **264** can take any form or configuration that mates with the male end **262**.

As shown in FIGS. **9A** and **9B**, each modular component **260** has at least one hole **268** (also referred to herein as a “channel”) defined through the component **260**. As depicted, the component **260** has three channels **268**, **270**, **272**. According to one embodiment, the channels **268**, **270**, **272** are configured to receive and/or allow the passage of any cables or tubes that are to be inserted through or positioned within the reversibly lockable tube **240**, such as those shown in FIGS. **10** and **11**. In accordance with one implementation, the center channel **268** is configured to receive a rigidity cable **242**, best shown in FIGS. **10** and **11**. The rigidity cable **242** is used to convert or adjust the tube **240** into the rigid configuration or phase. Any additional channels, such as channels **270**, **272**, are configured to receive electrical connection components, hydraulic or pneumatic tubes, or any other elongate members that require insertion into the target cavity or connection to a robotic device positioned in the target cavity.

According to one embodiment as best shown in FIGS. **10**, **11**, and **12**, the rigidity cable **242** operates in the following manner to adjust or convert the tube **240** from the flexible configuration to the rigid configuration. In the flexible state as shown in FIG. **11**, the cable **242** is allowed to be loose and thus the modular components **246** are not being urged against each other into a tight configuration. According to one embodiment, each modular component **246** can move about 20 degrees relative to the adjacent components **246** in the flexible state. When it is desirable to adjust or transform the tube **240** from the flexible state to the rigid state, the cable **242** is pulled or otherwise urged at its proximal end **248** in a direction away from the tube **240**. This causes the cable end **244** to contact the distal modular component **250** and begin urging that component **250** toward the other components of the tube **240**. Ultimately, this urges the modular components **246** into a tight configuration of the components **246** in which each of the components **246** is stacked tightly, or is otherwise urged in close contact, with the other components **246**, thereby resulting in a substantially rigid configuration of the tube **240**.

In use, the tube (such as tubes **220** or **240**, for example) is placed in its flexible configuration or state for insertion of the robotic device into the patient’s body. Once the device has been positioned as desired by the user (such as the positioning of the device **222** and tube **220** depicted in FIG. **8** or alternatively as shown in FIG. **13**), the tube is then adjusted or converted or otherwise placed into its rigid configuration or phase. This rigidity can assist in maintaining the geometric or physical shape and/or positioning of the tube in relation to the patient and resist against the straightening force of the hydraulic, pneumatic, or physical force being applied through the connections between the device and the external components of the hydraulic, pneumatic, or drive train systems, respectively, as known in the art or as described above. Thus, the tube can assist in maintaining the stability of the robotic device during use. Alternatively, the rigidity can assist with maintaining the geometric or physical shape and/or positioning of the tube for any reason that may benefit the operation of the medical device or the medical procedure generally.

In addition to the fluid actuation system and drive train embodiments discussed above, yet another actuation component that can be incorporated into or used with any of the medical devices disclosed or otherwise described herein is a motorless actuation system or component.

11

FIGS. 14A and 14B depict one embodiment of a motorless actuation component. More specifically, FIGS. 14A and 14B depict a robotic camera device 310, according to one embodiment, in which the robotic device 310 is disposed within the abdominal cavity of a patient, and a magnetic handle 312 is disposed at a location external to the patient. The handle 312 operates to hold the device 310 inside the abdominal cavity against the peritoneum (abdominal wall) via magnetic forces.

It is understood that this embodiment is similar to the embodiments disclosed in U.S. patent application Ser. No. 11/766,720, filed on Jun. 21, 2007, and U.S. patent application Ser. No. 11/766,683, filed on Jun. 21, 2007, both of which were incorporated herein above. It is further understood that any of the instant motorless actuation component embodiments can be incorporated into any of the embodiments disclosed in those co-pending applications.

In the implementation shown in FIGS. 14A and 14B, the device 310 is cylindrical and includes an imaging component 314, a lighting component 316, magnets 318 at each end of the device, and a wired connection component 320 (also referred to herein as a “wire tether”). The magnets 318 are magnetically coupleable with magnets 322 on the handle 312 such that the device 310 is urged toward and held against the body cavity wall. In one embodiment, the magnets 318 are configured to ensure that the imaging component 314 is positioned to capture a view of the body cavity or the target area of interest.

It is understood that the magnets 318 in the device 310 and those magnets 322 in the handle 312 can be positioned in any configuration and include any number of magnets as disclosed in the U.S. patent application Ser. Nos. 11/766,720 and 11/766,683, incorporated herein.

It is further understood that, in one embodiment, the magnetic handle 312, also referred to herein as an “external magnet,” is in the shape of a handle. Alternatively, the handle 312 is intended to encompass any magnetic component that is magnetically coupleable with any robotic device as described herein such that the magnetic component can be used to position, operate, or control the device.

In one embodiment as described in the incorporated references above, the handle 312 can be rotated as shown by arrow 342 to allow a tilting functionality for the imaging component. Further, the device can also provide for a panning functionality via rotation of the imaging component as shown by arrow 344, as described in further detail below.

In use, the device 310 can be moved within the patient's body to any desired position by moving the handle 312 outside the body. Alternatively, the device 310 can be positioned, operated, or controlled anywhere in a patient's body at least in part by the magnetic handle 312 positioned outside the body in any fashion described in the references incorporated above.

According to one implementation, the robotic device 310 shown in FIGS. 14A and 14B has two portions: an inner portion 330 and an outer portion 332, as best shown in FIG. 14B. The inner portion 330, according to one embodiment, is a cylindrically shaped inner body 330, and the outer portion 332 is an outer sleeve 332 configured to be rotatably disposed over the inner body 330. In such an embodiment, the imaging component 314 and lens 315 can be panned by rotating the inner body 330 with respect to the sleeve 332, causing the lens 315 to rotate in a fashion similar to that depicted by the arrow 344. In accordance with one implementation, the inner body 330 is coupled to the outer sleeve 332 with a set of bearings (not shown).

12

In one implementation, the actuation component 334 that rotates the inner portion 330 relative to the outer portion 332 is a motorless actuation component. That is, the actuation component is not a motor or a motorized component of any kind. For example, the actuation component 334 as shown in FIGS. 14A and 14B includes a race 336 and ball 338. In this embodiment, a magnet 340 external to the patient is used to urge the ball 338 along the race 336. In such an embodiment, the magnet 340 can be coupled with the magnetic handle 312 described here as shown in FIG. 14A. In one embodiment, the race 336 is helical and the ball 338 is steel. In a race and ball implementation, as the ball 338 moves along the race channel 336, the inner body 330 rotates relative to the outer sleeve 332. In another embodiment, the ball 338 is magnetic and moves along a race 336.

FIG. 15 depicts an alternative embodiment of a motorless actuation component in which the actuation component 352 has multiple magnets 354 that are disposed in or on the robotic device 350. In this embodiment, the magnets 354 are placed in a helical pattern in the inner cylinder (not shown) so that as the external magnet 356 is translated, the inner body rotates relative to the outer sleeve 358 as the inner body magnet 354 in closest proximity to the external magnet 356 is urged toward the external magnet 356. In another embodiment, a series of electromagnets in the handle 360 can be actuated in order to move the effective magnetic field along the handle 360.

In yet another alternative embodiment, the ball can be urged along the race by other means. For example, the device can have a cable or wire connected to it and also connected to an external handle. Actuation of this cable urges the ball along the race, thereby resulting in a panning motion of the inner body relative to the outer sleeve. In one embodiment, the cable is attached or operably coupled in some fashion to the ball so that actuation of the cable urges the ball along the race.

In a further alternative, the motorless actuation component does not include a ball and race, but instead has a drum. In this embodiment, a cable such as that described above is attached to the drum so that actuation of the cable urges the drum to rotate. This rotation of the drum causes rotational actuation in the medical device. Alternatively, any known method of transitioning translation motion into rotary motion could be used. Further, it is understood that any known motorless actuation component can be incorporated into any of the medical devices described herein or incorporated by reference herein.

Various mechanical arm embodiments are provided herein that can be incorporated into any number of different kinds of medical devices. The medical device arm configurations disclosed herein provide for various arm embodiments having two degrees of freedom—both (1) axial movement (extension and retraction of a portion of the arm along the longitudinal axis of the arm), and (2) rotational movement around the axis of the arm. These configurations provide for the two degrees of freedom while maintaining a relatively small or compact structure in comparison to prior art configurations.

It is understood that the arm embodiments disclosed herein can be utilized in any type of medical device, including those devices in which a compact or smaller size is desirable, such as devices for procedures to be performed within a patient. For example, the arm embodiments could be incorporated into various robotic medical devices, including in vivo robotic devices such as robotic devices positionable on or near an interior cavity wall of a patient, mobile robotic devices, or robotic visualization and control systems.

13

An “in vivo device” as used herein is any device that can be positioned, operated, or controlled at least in part by a user while being positioned within a body cavity of a patient, including any device that is positioned substantially against or adjacent to a wall of a body cavity of a patient, and further including any such device that is internally actuated (having no external source of motive force). As used herein, the terms “robot,” and “robotic device” shall refer to any device that can perform a task either in response to a command or automatically. Further, the arm embodiments could be incorporated into various robotic medical device systems that are actuated externally, such as those available from Apollo Endosurgery, Inc., Hansen Medical, Inc., Intuitive Surgical, Inc., and other similar systems.

According to one embodiment as depicted in FIG. 16, one arm embodiment is incorporated into an in vivo medical device 402 as shown. The device 402 has two robotic arms 404, 406 that can be configured according to any embodiment described herein.

FIGS. 17a and 17b depict a device arm 410, according to one embodiment. The arm 410 has two gears: (1) a distal gear 412 that provides for extension and retraction of the arm 410, and (2) a proximal gear 414 that provides for rotation of the arm 410.

The distal gear 412 has gear teeth 416 on its outer surface and further is threaded on its inner surface (not shown). The gear teeth 416 mate or couple with gear teeth 418 on a drive gear 420, which is coupled to an actuator (not shown). In one embodiment, the actuator is a Permanent Magnet Direct Current (“PMDC”) motor. Thus, the distal gear 412 is driven by the actuator.

The threading on the inner surface of the distal gear 412 mates or couples with the threading 413 on the outer surface of the arm 410 such that when the distal gear 412 is driven by the actuator, the gear 412 rotates and the coupling of the threads on the inner surface of the gear 412 with the threads 413 on the arm 410 causes the arm 410 to extend or retract depending on which direction the gear 412 turns.

The proximal gear 414 has gear teeth 422 on its outer surface that mate or couple with gear teeth 424 on a drive gear 426, which is coupled to an actuator (not shown). The gear 414 also has a pin 428 disposed within the gear 414 that extends through the gear 414 and further through a slot 430 in the arm 410. Thus, when the proximal gear 414 turns, the pin 428 causes the arm 410 to turn as well.

The distal 412 and proximal 414 gears interface or interact at the bearing surfaces. More specifically, the distal gear 412 has a bearing surface 432 (best shown in FIG. 17b) having two bushings 434, 436 disposed or positioned on the outer surface of the bearing surface 432. Similarly, the proximal gear 414 has a bearing surface 438 having two bushings 440, 442. The bearing surface 432 has a smaller diameter than, and is disposed within, the bearing surface 438 such that the inner surface of bearing surface 438 is in contact with the two bushings 434, 436. As such, the bearing surfaces 432, 438 contact each other and rotate in relation to one another at the two bushings 434, 436. Further, the two bushings 440, 442 disposed on the outer surface of the bearing surface 438 typically contact the external gear housing or other type of housing (not shown).

In an alternative embodiment, gear pairs 418, 412 and 424, 422 as depicted in FIGS. 17A and 17B are replaced with round wheel pairs in which each wheel is configured to be in contact with the other wheel in the pair. In such an embodiment, each wheel has a coating or other surface component that provides for sufficient friction when the wheels are in contact to transmit rotational energy between

14

the two wheels. According to one embodiment, the coating is a thin rubber coating. Alternatively, the coating or surface can be any known coating or surface that provide sufficient friction to allow transmission of rotational energy. This friction drive system allows the gearing components to be reduced in size because of the elimination of the gear teeth.

In a further embodiment, the gears can also be replaced with a series of cables and drums that are used to actuate the arm. In this pulley system embodiment, the actuator that drives the cables can be located in another portion of the robot, while a series of drums are disposed on the arms. The cabling connects the drums with the actuator (such as a motor). This embodiment allows the actuators, drums, and arm components to be configured in a variety of different orientations while still providing sufficient actuation forces and speed to the arm end effectors.

FIG. 18 depicts another device arm 450, according to an alternative embodiment. The arm 450 has a distal gear 452 and a proximal gear 454.

The distal gear 452 has gear teeth 456 and is threaded on its inner surface (not shown). The gear teeth 456 mate or couple with gear teeth 458 on a drive gear 460, which is coupled to an actuator (not shown). As with the previous embodiment, the threading on the inner surface of the distal gear 452 mates or couples with the threading (453) on the outer surface of the arm 450 such that when the distal gear 452 is driven by the actuator, the gear 452 rotates and the coupling of the threads on the inner surface of the gear 452 with the threads 453 on the arm 450 causes the arm 450 to extend or retract depending on which direction the gear 452 turns.

Similarly, the proximal gear 454 has gear teeth 462 on its outer surface that mate or couple with gear teeth 464 on a drive gear 466, which is coupled to an actuator (not shown). The gear 454 also has a pin 468 disposed within the gear 454 that extends through the gear 454 and further through a slot 470 in the arm 450. Thus, when the proximal gear 454 turns, the pin 468 causes the arm 450 to turn as well.

The bearing surfaces in this embodiment depicted in FIG. 18 differ from those in the prior embodiment. That is, the distal gear 452 has a bearing surface 472 that is adjacent to and in contact with a bearing surface 474 of the proximal gear 454. Thus, the gears 452, 454 rotate in relation to each other at the bearing surfaces 472, 474. In addition, the two bearing surfaces 472, 474 typically contact or are disposed within an external gear housing 476.

Although the present invention has been described with reference to preferred embodiments, persons skilled in the art will recognize that changes may be made in form and detail without departing from the spirit and scope of the invention.

One end effector or operational component that can be used with any of the procedural devices disclosed herein is a winch system. Generally, the devices or systems discussed herein are configured to be inserted into or positioned in a patient’s body, such as a body cavity, for example. Alternatively, the winch systems and devices disclosed herein can be used with any medical or procedural device.

One embodiment of a medical device having a winch component is set forth in FIGS. 19A and 19B. The medical device 510 is an in vivo robotic device 510 that can be positioned within a cavity of a patient, and further has a magnetic handle 512 that can be disposed at a location external to the patient. In this embodiment, the handle 512 operates to hold the device 510 inside the abdominal cavity against the peritoneum (abdominal wall) via magnetic forces. Alternatively, any known method or component for

15

holding the device **510** against the wall could be used. For example, in one embodiment, the robot **510** could be held against the wall using hooks or clamps. In a further alternative, the winch systems disclosed herein can be used with any known medical devices, including—but not limited to—in vivo devices with arms or wheels.

In the implementation depicted in FIGS. **19A** and **19B**, the device **510** has a winch component **524** and a motor **530** to actuate the winch **524**. In this embodiment, the winch component **524** includes a drum **526** and a winch tether **528**. The drum **526** operates to wind and unwind the winch tether **528**.

In accordance with the depicted embodiment, the device **510** has magnets **520** that are magnetically coupleable with magnets **532** on the handle **512** such that the device **510** is urged toward and held against the body cavity wall. The device **510**, the handle **512**, and the magnets **520**, **532** can be configured and/or operated in the same fashion as described in U.S. application Ser. No. 11/766,720, filed on Jun. 21, 2007 and entitled “Magnetically Coupleable Robotic Devices and Related Methods,” which is incorporated by reference above. In one embodiment, it is understood that the magnets **520** are configured not only to ensure that the imaging component **516** is positioned to capture a view of the body cavity or the target area of interest for securing the winch **524**, but are also configured to provide a magnetic coupling that is strong enough to maintain the device **510** in a stable and substantially fixed position such that the winch component **524** can be operated as desired and as described herein.

According to the exemplary embodiment in FIGS. **19A** and **19B**, the actuation component **530** is a motor **530** that provides force for rotating the drum **526**. In this embodiment, the motor **530** is a 6 mm brushed motor that turns a planetary gear, which revolves around a stationary sun gear, thereby causing the drum **526** to rotate inside the body **514**. Alternatively, a clutch (not shown) can be used to provide both (1) panning motion of a camera **516** along the axis of the body **514**, and (2) winch actuation using a single motor. In a further alternative, an exterior drive train can be used to actuate the winch **524**. It is understood that any known actuation component that can be used with medical devices can be used with the winch components or systems disclosed herein.

In one embodiment, the winch tether **528** is made from suture material. In another embodiment, it is metallic cabling. Alternatively, any known material for use in a medical winch tether can be used.

In one embodiment, various operational components or end effectors can be attached to the end of the winch tether. In one embodiment, the end of the winch tether **528** is attached to a hook **536**, as depicted in the embodiment of FIGS. **19A** and **19B**. Such a hook is depicted in use in FIG. **20**. Alternatively, the end effector (also referred to as an “operational component”) of the tether can be a clamp or loop. In a further alternative, any known operational component, including any known component for attaching to tissue, can be used.

In another embodiment, the operational component can be a magnet **540** that can be held against the wall with a second handle **542** as depicted in FIG. **21**. In a further embodiment, the device could have two winch components **550** with magnet operational components **552** that attach to two points in vivo as depicted in FIG. **22**. Such a device could have two separate drums and motors, or alternatively, a single motor and drum.

16

The winch components and systems can be used to accomplish a variety of procedural tasks. In one embodiment, a device having a winch component could be used to retract an organ, such as the gallbladder, as depicted for example in FIG. **20**. In another embodiment, a device having a winch component and a magnet operational component could be used as a sling to retract or move a very large organ such as the liver as depicted in FIG. **21**. In yet another embodiment, the device is used as a “gantry crane” with two winch tethers attached to the abdominal wall, as depicted in FIG. **22**, or to other organs. In this embodiment, the device is guided along the winch tethers to change the camera or illumination location. In another embodiment, the device could be guided along the winch tether, with a third winch hook (or grasper) below the device as shown in FIG. **22**. This would allow the robot to reposition itself along the line of the first two tethers while the third winch could be used to grasp a tissue of interest for retraction or other manipulation. In yet another embodiment, the guide tethers are not suspended but lying on the organs.

In yet another alternative embodiment, the winch component can be any known configuration or be made up of any known components for use in a winch. Further, while certain device embodiments are described for exemplary purposes herein, it is understood that a winch component can be incorporated into any known robotic device for use inside a patient. For example, such a component can be incorporated into any of the devices disclosed in the applications that are incorporated herein elsewhere in this application.

Various additional embodiments disclosed herein relate to procedural devices with modular mechanical and electrical packages that can be used together in various combinations to provide capabilities such as obtaining multiple tissue samples, monitoring physiological parameters, and wireless command, control and data telemetry. This modular technology provides a flexible device into which one or more of various different components or systems can be integrated.

Current known minimally-invasive surgical technologies require two to three ports to accommodate the laparoscopic tools to explore the abdominal cavity and biopsy tissue of interest. The various embodiments of the devices and modular components disclosed herein require only one port for any medical procedure, thereby reducing patient trauma (1 incision rather than 2 or 3).

FIG. **23A** depicts one exemplary implementation of a modular device having a payload area **566**. The payload area **566** is configured to receive any one of several modular components, including such components as the sensor, controller, and biopsy components discussed herein. It is understood that in addition to the specific modular components disclosed herein, the payload areas of the various embodiments could receive any known component to be added to a medical procedural device.

The modular technology disclosed herein can be incorporated into any type of medical procedural device and is not limited to the robotic devices described in detail herein. Certain device embodiments can be in vivo or robotic devices as defined herein, including devices configured to be positioned within a body cavity of a patient, including certain devices that can be positioned against or substantially adjacent to an interior cavity wall, and related systems. For example, FIG. **23B** depicts a different device embodiment having a payload area **566**. Thus, while the robotic device embodiments depicted in FIG. **23A** is a mobile device having wheels, the various modular components described herein could just as readily be positioned or associated with a payload area in any other kind of robotic device or in vivo

device such as the device depicted in FIG. 23B or can further be used in other medical devices and applications that don't relate to robotic devices.

FIGS. 24A, 24B, and 24C depict a biopsy component 600 according to one embodiment that can be used with any robotic device disclosed herein, including as shown for exemplary purposes in FIG. 23A or FIG. 23B. The mechanism 600 has a biopsy grasper 632 that in this implementation has a piercing or lower jaw component 602 and an upper jaw component 630. The piercing component 602 and jaw component 630 are structured like a pair of jaws, with the piercing component 602 being configured to remain stationary during the sampling process, providing a substantially rigid and stable base against which the upper jaw component 630 can move in a jaw-like fashion in relation to the piercing component 602 such that the jaw component 630 can ultimately make contact with the piercing component 602 and thereby cut the target tissue. Unlike standard laparoscopic biopsy tools that are generally designed to grasp tissue so that the surgeon can then tear the sample free, this grasper is designed to completely sever the sample from the tissue of interest without manual manipulation required by the surgeon or user.

In this embodiment, the upper jaw component 630 is moved in relation to the piercing component 602 via the collar 604. More specifically, the collar 604 is movably disposed over the piercing component 602 such that it can move back and forth in the direction indicated by arrow A. A proximal portion of the upper jaw component 630 is disposed between the piercing component 602 and the collar 604 and is configured to be positioned such that the distal end of the upper jaw 630 is not in contact with the piercing component 602 and remains in that position when no force is applied to the jaw 630. Thus, when the collar 604 is urged toward the distal end of the piercing component 602, the distal end of the upper jaw component 630 is urged toward the piercing component 602 such that the component 630 is capable of incising or cutting any tissue disposed between the upper jaw 630 and the piercing component 602 as the upper jaw 630 makes contact with the component 602. And when the collar 604 is urged away from the distal end of the piercing component 602, the distal end of the upper jaw 630 moves away from the piercing component 602 and toward its unrestrained position. Alternatively, it is understood that any known component that can operate in the same fashion as the collar to urge the upper jaw 630 into contact with the piercing component 602 can be incorporated herein.

The collar 604 is urged back and forth by the motor 624. It is understood that this embodiment is intended to encompass any actuation structure that urges the collar 634 to move back and forth such that the upper jaw component 630 is urged to move in relation to the piercing component 602 and thereby cut target tissue.

In this particular embodiment as shown in FIG. 24A, the grasper 632 is powered by the motor 624. Motor 624 is coupled to a nut 618 that is driven by the motor 624 along the axis of a lead screw 616 parallel to arrow B. The nut 618 is coupled to a slider 608 via a linkage 610 that is pivotally coupled to the nut at pin 620 and to the slider 618 at pin 628. The nut 618, linkage 610, and slider 608 convert the actuation direction from the direction of arrow B to the direction of arrow A and, according to one embodiment, increase the amount of force applied by the motor 624 to the slider 608.

The slider 608 is coupled to the collar 604 at two flexible components 606A, 606B, which can be shape-memory components 606A, 606B according to one embodiment. In

one example, the flexible components 606A, 606B are comprised of nitinol. Further, the piercing component 602 is coupled to the housing 622 via a flexible component 626. According to one embodiment, the flexible component 626 is a shape-memory component 626 such as nitinol. These flexible components 606A, 606B, and 626 allow for the grasper 632 to be repositioned in relation to the rest of the robotic device to which it is coupled, as will be discussed in further detail below.

Alternatively, the actuation component and the connection of the actuation component to the collar 634 can be any known structure or component or combination thereof that provides motive force to actuate the grasper 632.

In one alternative implementation, the piercing component 602 has an internal reservoir (not shown) for storing one or more acquired samples. Unlike most standard laparoscopic biopsy tools that include space for only a single sample, this reservoir can be generally large enough or long enough (or otherwise has sufficient volume) to house multiple samples during a biopsy procedure.

In use, the biopsy component 600 is positioned next to the target tissue using a method such as the mobile robot wheel, or articulating robot arm. Next, the biopsy component 600 operates in the following manner to obtain a tissue sample. The motor 624 actuates the collar 604 to move toward the distal end of the piercing component 602 and thus actuates the upper jaw 630 to close and contact the piercing component 602. The tissue is cut as the upper jaw 630 is actuated towards the piercing component 602 in a slicing motion. In one embodiment the tissue sample is then stored in the piercing component 602 while additional samples are taken.

It is understood that the device containing the biopsy component 600 may also have other actuable components such as wheels, arms, etc. FIG. 24A further depicts a motor 614 disposed within a second housing 612 that is configured to actuate one or more additional actuable components of the device. In one example, the motor 614 can actuate a wheel (not shown) operably coupled with the device. In another example, this motor 614 actuates an arm (not shown) connected to the device.

In one aspect, the biopsy component 600 can also be configured to make it easier for the medical device to be inserted through incisions, transported, and stored. FIG. 24B depicts the grasper 632 of the biopsy component 600 positioned at a ninety degree angle in relation to its position in FIG. 24A. This re-positioning of the grasper 632 is accomplished due to the flexibility of the flexible components 606A, 606B, 626 as discussed above. According to one embodiment, this second position of the grasper 632 allows for easier insertion and retraction of the device to which the grasper is coupled. That is, the second position of the grasper 632 allows for the entire device to fit more easily through an incision, a port, or any other opening or device for use in medical procedures. In its operating position as depicted in FIG. 24A, the grasper 632 is positioned perpendicularly to the body of the robotic device to which it is coupled. The overall length of the robot body and grasper 632 is greater than the diameter of most laparoscopic trocars. Thus, to allow the robot/grasper 632 to be inserted through a trocar, the grasper 632 can be moved into a position that is parallel to the length of the robotic device using the support mechanism provided by the three flexible components 606A, 606B, 626 that provide both rigidity and the ability to flex the arm 640 degrees during insertion and retraction through a trocar or through any type of orifice, incision, or tool as necessary. This support mechanism provides the rigidity and

forces required during biopsy sampling, with the flexibility required for insertion and retraction before and after the biopsy occurs.

Alternatively, a variety of alternative support mechanisms using this concept can be envisioned.

FIG. 25A depicts an alternative embodiment of a biopsy component 640 that can be used with any robotic device disclosed herein. The component 640 has actuation components similar to those in the embodiment depicted in FIGS. 24A, 24B, and 24C, including a nut 646 driven along the axis of a lead screw 648 in the direction indicated by arrow B by a motor 644. The nut 646 is attached to a slider 656 via a linkage 650 that is coupled to the nut 646 at pin 652 and to the slider 656 at pin 650.

In this embodiment, the slider 656 performs generally the same function as the collar described in FIG. 24. That is, the slider 656 can move in the direction indicated by arrow A in relation to the piercing component 658. Thus, similarly to the collar as described above, as the slider 656 moves over the upper jaw 664, the upper jaw 664 is closed relative to the lower piercing jaw 658.

FIG. 26 depicts an alternative embodiment of the biopsy component 660 that can be used with any robotic device disclosed herein. The component 660 has actuation components similar to those in the embodiment depicted in FIGS. 24A, 24B, and 24C. In this embodiment the collar 662 is urged in the direction A. As the collar 662 moves forward it pushes the top jaw 664 downwards toward the bottom jaw 666 in direction B. The collar is held in place by the housing 672 in the same manner as described for FIG. 24.

Unlike other laparoscopic biopsy forceps in which both jaws are hinged about a pivot point, only one jaw, the top jaw 664, of the robotic grasper moves during sampling. The lower half of the grasper, bottom jaw 666, remains stationary and provides a rigid and stable base against which the top jaw 664 can cut. The fixed bottom jaw 666 is constructed from a hypodermic medical stainless steel tube and it forms a reservoir for storing multiple samples.

In one embodiment the profile of the top jaw 664 is constructed out of a super-elastic shape-memory nickel titanium alloy (Nitinol) ribbon (Memry Corporation) 0.25 mm thick and 3 mm wide. It is profiled such that the grasper is normally open. A wide variety of profiles can be achieved by heat-treating the ribbon for approximately 10 min at 500° C., followed by quenching in water. The Nitinol ribbon is glued to a fixed nylon rod insert that fits inside the bottom jaw 666.

The blades of the grasper are titanium nitrate coated stainless steel approximately 1.5 mm long. Small plastic inserts are fixed to the top and bottom jaws, and the blades 668 and 670 are glued to these inserts. The round blade 670 fixed to the bottom jaw has a diameter of 3 mm. The top blade 668 has a semi-circular profile with a diameter of 3.8 mm and overlaps the bottom blade when the jaw is closed. The sample is held within the bottom blade as the trailing edges of the top blade help sever the sample from the tissue.

FIG. 27 depicts an alternative embodiment of the biopsy component 680 that can be used with any robotic device disclosed herein to staple or clamp tissue. The component 680 has actuation components similar to those in the embodiment depicted in FIGS. 24A, 24B, and 24C. In this embodiment the collar 682 is urged in the direction A. As the collar 682 moves forward it pushes the top jaw 684 downwards toward the bottom jaw 686 in direction B. As the top jaw 684 is pressed downwards against the bottom jaw 686, a small surgical staple 688 can be compressed to staple tissue of interest or to clamp an artery or other vessel.

This stapling arm 680 was designed to hold and close a common laparoscopic surgical staple. In addition to stapling, this end effector can also be used for applications requiring clamping and holding, such as applying pressure to a bleeding blood vessel or manipulating other tissues of interest.

FIGS. 28A and 28B depict a further embodiment of a biopsy mechanism 690, according to one implementation. These two figures provide a detailed depiction of the opening and closing of grasper jaws 694, 696 according to one embodiment. More specifically, FIG. 28A depicts the mechanism 690 with the grasper jaws 694, 696 in their open configuration. In this configuration, the upper jaw 694 is in a position in which the distal end is not in contact with the distal end of the lower jaw 696.

FIG. 28B depicts the mechanism 690 with the grasper jaws 694, 696 in their closed configuration. That is, the collar 698 has moved from its retracted position in FIG. 28A to its extended position in FIG. 28B such that it has urged the upper jaw 694 down toward the lower jaw 696 such that the jaws 694, 696 ultimately reach the closed configuration.

According to one embodiment, an imaging component in any medical device disclosed or incorporated herein having an imaging component can have an adjustable focus mechanism incorporated into or used with the imaging component. One exemplary implementation of such an adjustable focus mechanism 702 is depicted in FIGS. 29A, 29B, 29C, 29D, and 29E. As best shown in FIG. 29E, the mechanism 702 includes a lens subassembly 704 and two magnetic subassemblies 706. The lens subassembly 704 comprises a lens 710, two coils of wire 712 (as best shown in FIGS. 29B, 29D, and 29E), and a lens holding component 714 (as best shown in FIGS. 29A, 29D, and 29E) to hold the lenses 710 and coils 712 together in one subassembly. As best shown in FIGS. 29D and 29E, each magnetic subassembly 706 includes a small magnet 716 attached to one side of a U-channel 722 made from ferrous metal. The lens subassembly 704 is positioned between the two magnetic subassemblies 706. The coils 712 pass over the U-channels 722 and are positioned in the magnetic field that is generated between the small magnet 716 and the open side of the U-channel 722 where the coil 712 sits. As current is passed through the coiled wire 712 that is positioned in the magnetic field, an electromagnetic force is created that is parallel to the axis of the lens 710 and imager 718. This electromagnetic force is created by the magnetic field being perpendicular to the direction of the current.

In one embodiment, the small magnets 716 are Neodymium Magnets manufactured by K and J Magnetics of Jamison, Pa., the coils 712 are manufactured by Precision Econowind of North Fort Myers, Fla., and the lens 710 is manufactured by Sunex of Carlsbad, Calif. In this embodiment the magnets have a pull force of 2.17 lbs and a surface field of 2505 Gauss, while the coils are made of 120 turns of 36 AWG coated copper wire with a DSL758 lens. Alternatively, the above components can be any commercially available components.

According to one implementation, the lens holding component 714 is manufactured of polycarbonate plastic to minimize weight. In the embodiment shown in FIGS. 29D and 29E, the magnets 716 are $\frac{1}{16}'' \times \frac{1}{8}'' \times \frac{1}{4}''$ and the lens subassembly has a vertical stroke of 1 mm.

In one embodiment, a restoring force is provided that urges the lens 710 back to its resting position when the current from the coiled wire 712 is removed. This allows for consistent lens subassembly travel and can be used to maintain the lens in an optimum middle range of focus. According to one implementation, the restoring force com-

21

ponent **720** as best shown in FIGS. **29A** and **29B** is a foam component **720**. Alternatively, any known component for providing a restoring force can be used.

In accordance with one embodiment, the adjustable focus mechanism **702** is coupled with an auto focus algorithm to automatically command the mechanism **702** to focus the lens to a commanded depth. In a further embodiment, additional lens subassemblies **704** and magnetic subassemblies **706** can be combined to provide additional points of depth adjustment around the lens. These additional adjustment points allow a higher range of orientation angles of the lens to correct for any imperfections in manufacturing assembly. In this embodiment, the coils can be commanded separately to tilt the lens to correct for manufacturing error.

EXAMPLE

In this example, different biopsy grasper profiles and lengths were examined, including the effects of those profiles and lengths on the forces required to actuate the biopsy mechanism and further the maximum forces that could actually be applied by the mechanism.

FIGS. **30A** and **30B** depict a test jig **730** having a biopsy mechanism according to one embodiment. The test jig **730** as shown included a load cell **748** that was used to measure the tensile force in the nylon supporting rod when the collar **738** was actuated. Further, the biopsy mechanism of the jig **730** had a motor **732**, linkage **736**, lead nut **734**, collar **738**, lower jaw **746** and upper jaw **744**.

Various grasper embodiments with a wide range of jaw lengths, opening angles, and jaw profiles were tested for actuation forces. Required actuation forces were determined by using the motor **732** and lead screw linkage **736** to slide the grasper collar **738** over the upper jaw **744** until closed. For each actuation, the required force was recorded starting with the upper jaw **744** completely open and continuing until the upper jaw **744** was closed. Maximum actuation forces were determined by recording the forces applied with the collar **738** held fixed at various positions corresponding to different times during actuation process. Each complete test consisted of 50 actuations of the biopsy grasper. Load cell data were recorded during each actuation at a rate of 20 Hz.

FIG. **31** depicts the mean results from a required force test for a grasper that is approximately 12 mm long, has an opening angle of 25° and has a cutting tip with a length of 4 mm profiled with a closing angle of approximately 40°. The error bars indicate the standard deviation in the measured forces at intervals of approximately 1.8 seconds. The maximum required actuation force of 2.83 N is at the very start of the motion of the collar due to the need to overcome static friction and to begin flexing the top jaw of the grasper. The force decreases with time as the contact point between the collar and the top jaw moves farther away from the anchor point. The test results indicate that approximately a maximum of 3 N of force is required to close the biopsy grasper.

What is claimed is:

1. A robotic surgical system, comprising:

(a) a robotic device sized to be positioned completely within a patient, the device comprising:

(i) a device body;

(ii) a first robotic arm operably coupled with the device body, the first robotic arm comprising:

(1) a first arm first link operably coupled to the device body via a first shoulder joint;

(2) a first arm second link operably coupled to the first arm first link via a first elbow joint; and

22

(3) a first operational component operably coupled to the first arm second link; and

(iii) a second robotic arm operably coupled with the device body;

(1) a second arm first link operably coupled to the device body via a second shoulder joint;

(2) a second arm second link operably coupled to the second arm first link via a second elbow joint; and

(3) a second operational component operably coupled to the second arm second link;

(b) a tubular component comprising a distal end operably coupled to the device body, the tubular component comprising a first lumen; and

(c) at least one connection component disposed through the first lumen of the tubular component, the at least one connection component comprising a distal end operably coupled to the robotic device.

2. The robotic surgical system of claim 1, wherein the tubular component comprises at least one modular tube component.

3. The robotic surgical system of claim 1, wherein the tubular component comprises a plurality of modular tube components.

4. The robotic surgical system of claim 3, wherein the tubular component is a reversibly lockable tube.

5. The robotic surgical system of claim 1, further comprising a power source operably coupled to a proximal end of the at least one connection component.

6. A robotic surgical system, comprising:

(a) a tubular component comprising a first lumen, the tubular component configured to be positioned through an incision formed in a cavity wall of a patient;

(b) a robotic device comprising:

(i) a device body;

(ii) a first robotic arm operably coupled to the device body and sized to be positioned in the cavity of the patient through the tubular component, the first robotic arm comprising:

(1) a first arm first link operably coupled to the device body at a first shoulder joint at a first end of the first arm first link;

(2) a first arm second link operably coupled to a second end of the first arm first link via a first elbow joint; and

(3) a first operational component operably coupled to the first arm second link; and

(iii) a second robotic arm operably coupled to the device body and sized to be positioned in the cavity of the patient through the tubular component, the second robotic arm comprising:

(1) a second arm first link operably coupled to the device body at a second shoulder joint at a first end of the second arm first link;

(2) a second arm second link operably coupled to a second end of the second arm first link via a second elbow joint; and

(3) a second operational component operably coupled to the second arm second link; and

(c) at least one connection component disposed through the first lumen of the tubular component, the at least one connection component comprising a distal end operably coupled to the robotic device.

7. The robotic surgical system of claim 6, further comprising a power source operably coupled to a proximal end of the at least one connection component.

23

8. The robotic surgical system of claim 6, wherein the at least one connection component comprises an electrical connection component.

9. The robotic surgical system of claim 6, wherein the at least one connection component comprises a hydraulic tube or a pneumatic tube.

10. A method of surgery comprising:
providing a robotic device comprising:

- (a) a device body;
- (b) a first robotic arm operably coupled with the device body, the first robotic arm comprising:
 - (i) a first arm first link operably coupled to the device body via a first shoulder joint;
 - (ii) a first arm second link operably coupled to the first arm first link via a first elbow joint; and
 - (iii) a first operational component operably coupled to the first arm second link; and
- (c) a second robotic arm operably coupled with the device body;
 - (i) a second arm first link operably coupled to the device body via a second shoulder joint;
 - (ii) a second arm second link operably coupled to the second arm first link via a second elbow joint; and
 - (iii) a second operational component operably coupled to the second arm second link;

inserting the robotic device into a body cavity through an incision in a wall of the body cavity such that the first and second robotic arms are positioned within the body cavity;

coupling an external controller to the robotic device via a connection component disposed through a tubular component and operably coupled to the robotic device; and

24

actuating the robotic device via the external controller and thereby performing a procedure with the first and second robotic arms within the body cavity.

11. The method of claim 10, further comprising adjusting the tubular component between a flexible configuration and a substantially rigid configuration.

12. The method of claim 10, further comprising placing the tubular component into a flexible configuration prior to inserting the robotic device into the body cavity.

13. The method of claim 10, further comprising placing the tubular component into a substantially rigid configuration when the robotic device is positioned within the body cavity.

14. The robotic surgical system of claim 1, wherein the at least one connection component comprises an electrical connection component.

15. The robotic surgical system of claim 1, wherein the at least one connection component comprises a hydraulic tube or a pneumatic tube.

16. The robotic surgical system of claim 6, wherein the tubular component comprises at least one modular tube component.

17. The robotic surgical system of claim 6, wherein the tubular component comprises a plurality of modular tube components.

18. The robotic surgical system of claim 17, wherein the tubular component is a reversibly lockable tube.

19. The robotic surgical system of claim 1, further comprising an external controller operably coupled to a proximal end of the at least one connection component.

20. The robotic surgical system of claim 6, further comprising an external controller operably coupled to a proximal end of the at least one connection component.

* * * * *