

International Journal of
Technology Assessment in
Health Care

**Participatory Design of Paediatric Upper Limb Prostheses:
qualitative methods and prototyping**

| | |
|-------------------------------|---|
| Journal: | <i>International Journal of Technology Assessment in Health Care</i> |
| Manuscript ID | IJTAHC-16-172.R4 |
| Manuscript Type: | Methods |
| Date Submitted by the Author: | 18-Jul-2017 |
| Complete List of Authors: | Sims, Tara; University of Brighton, School of Health Sciences Cranny, Andy; University of Southampton Metcalf, Cheryl ; University of Southampton Chappell, Paul; University of Southampton Donovan-Hall, Maggie; University of Southampton |
| Keywords: | Prosthesis Design, Printing, Three-Dimensional, Patient Participation, Child, Qualitative Research |
| Abstract: | <p>Objectives: The study aims to develop an understanding of the views of children and adolescents, parents and professionals on upper limb prosthetic devices in order to develop and improve device design. Previous research has found that children are dissatisfied with prostheses but has relied heavily on parent proxy reports and quantitative measures (such as questionnaires) to explore their views.</p> <p>Methods: 34 Participants (eight children aged 8-15 with upper limb difference, nine parents, eight prosthetists and nine occupational therapists) contributed to the development of new devices through the BRIDGE methodology of participatory design, using focus groups and interviews.</p> <p>Results: The study identified areas for improving prostheses from the perspective of children and adolescents, developed prototypes based on these and gained feedback on the prototypes from the children and other stakeholders (parents and professionals) of paediatric upper limb prostheses. Future device development needs to focus on ease of use, versatility, appearance and safety.</p> <p>Conclusions: This study has demonstrated that children and adolescents can and should be involved as equal partners in the development of daily living equipment and that rapid prototyping (3D printing or additive manufacturing), used within a participatory design framework, can be a useful tool for facilitating this.</p> |

For Peer Review

1) Cover Sheet

Title: Participatory Design of Paediatric UL Prostheses: qualitative methods and prototyping.

Short title: Participatory Design of Paediatric UL Prostheses.

Authors:

Tara Sims¹, Andy Cranny², Cheryl Metcalf³, Paul Chappell², Maggie Donovan-Hall³

1. School of Health Sciences, University of Brighton.
2. School of Engineering and Computer Science, University of Southampton
3. Faculty of Health Sciences, University of Southampton

2) Abstract and key words

Abstract

Objectives: The study aims to develop an understanding of the views of children and adolescents, parents and professionals on upper limb prosthetic devices in order to develop and improve device design. Previous research has found that children are dissatisfied with prostheses but has relied heavily on parent proxy reports and quantitative measures (such as questionnaires) to explore their views.

Methods: 34 Participants (eight children aged 8-15 with upper limb difference, nine parents, eight prosthetists and nine occupational therapists) contributed to the development of new devices through the BRIDGE methodology of participatory design, using focus groups and interviews.

Results: The study identified areas for improving prostheses from the perspective of children and adolescents, developed prototypes based on these and gained feedback on the prototypes from the children and other stakeholders (parents and professionals) of paediatric upper limb prostheses. Future device development needs to focus on ease of use, versatility, appearance and safety.

Conclusions: This study has demonstrated that children and adolescents can and should be involved as equal partners in the development of daily living equipment and that rapid prototyping (3D printing or additive manufacturing), used within a participatory design framework, can be a useful tool for facilitating this.

Key words: Prosthesis Design; Printing, Three-Dimensional; Qualitative Research; Child; Patient Participation.

3) Acknowledgments

We would like to extend our thanks and appreciation to the children, parents and professionals who participated in this study. This research was completed as part of the first author's faculty funded PhD studentship study in the Faculty of Health Sciences at the University of Southampton.

For Peer Review

4) Text

Background

Upper limb difference refers to the congenital absence or malformation, or absence due to surgical or traumatic amputation, of any part of the arm or hand (1). Congenital upper limb difference is present at birth and can, in rare instances, involve multiple limbs (1). Acquired amputations can be the result of cancer, trauma or severe infections, such as meningococcal septicaemia (1). Upper limb difference can have both a physical and psychological effect on a child (1). However, non-use rates of upper limb prostheses amongst children can be as high as 50% (2). Studies have found that children feel that prostheses do not help function, are uncomfortable, are unreliable, are too heavy and are not aesthetically acceptable (3, 4, 5, 6,7).

There has been an increasing emphasis on the importance of involving users of devices when designing technology used both within and outside of healthcare settings (8). Furthermore, increasing recognition of children's rights has led to children more frequently being asked for their opinions on the health services and treatment they receive (9).

Nesset and Large (10) argued that involving children in the design of products resulted in software that truly met the children's needs. They suggested that likes and dislikes were revealed which were contrary to the researchers' preconceived ideas about the children and would have remained unknown without their involvement.

Light et al (11) and Rigby et al (12) incorporated the views and preferences of children into the design of assistive equipment and Cooke (13) involved children in the design of a hospital building using play sessions, interviews and focus groups to elicit their views. Weightman et

al (14) involved children with cerebral palsy in the development of devices for upper limb therapy using a range of methods, including the traditional approaches of questionnaires and interviews to explore their views, and peer-tutoring methods to test the usability of the devices. Whilst they found interviews and questionnaires to be useful, the researchers felt that these methods were commensurate with a marginalising power relationship, with the adults being in the position of power when asking the questions. They suggested this could be addressed by giving children some choice and control over how they participate.

Research involving children in prosthesis development has explored the development priorities of prosthesis users of all ages, combining the findings from adult and child populations (15; 16). This approach does not fully appreciate children's needs and views as unique to those of adults. Design priorities can vary substantially between adults and children, suggesting there are distinct requirements for paediatric users (16).

In addition to involving children and adolescents (the users of upper limb prostheses), it is important to consult with other stakeholders (parents/carers and professionals), as they will have different levels of expertise and different goals for using the devices (17).

Comprehensive consideration of the needs of all stakeholders is essential if better devices are to be developed (18).

Many authors have emphasised the impact of involving the parents and providing them with guidance and information, on the child's acceptance of a prosthesis, yet there is a paucity of research that involves parents in the development of prostheses for children (19). Postema et al (20) found that when parents were disappointed with the functional capabilities, appearance and weight of upper limb prostheses, or felt that they were not adequately

involved in decision-making, this increased the likelihood that the child would not use the prosthesis. These findings infer that parental encouragement may positively affect a child's use of prostheses and supports the notion that parents should be involved in the development of prostheses for children and adolescents. Additionally, if professionals find it difficult to prescribe or fit a prosthesis or provide training for use, children are likely to experience greater problems (21; 22; 23).

The field of Human Computer Interaction (HCI) is significantly further ahead than healthcare in involving children in product design (24). The BRIDGE method is a HCI methodology for involving children as equal stakeholders in the design process (25). This approach argues that, providing consideration is given to context, collaboration and cultural sensitivity, children do not need to participate in product design in a fundamentally different way to adults (25). The BRIDGE method views children as experts in their everyday lives, using their experiences as a starting point for the design process (25). It is the responsibility of the researcher to understand the viewpoints of the children participating through using methods which enable them to express their views (25). However, a central driving belief behind the methodology is that designing a new technology requires active participation of all stakeholders, and not just the user of the device (25). In the case of upper limb prostheses for children, this will include the parents and multidisciplinary healthcare professionals working with the child, as well as the child (taking into account the entire context of the technology's use). A multidisciplinary team is important in this approach to ensure that children's novel ideas can be gleaned, whilst being feasible to manufacture, prescribe and use (10). Advances in three-dimensional (3D) printing permit rapid development of new and inexpensive prostheses in response to participants' views. 3D printing facilitates an iterative approach to

device development which is central to the BRIDGE methodology. An iterative approach is fundamental in including participants' views in prosthesis design.

The current study responds to the high non-use rates and dissatisfaction by involving children (and other stakeholders) in the development of new upper limb prosthetic devices.

The aims of the current study were to:

- Understand the views of children and adolescents with upper limb difference, their parents and professionals on the usefulness of upper limb prosthetic devices and how they could be improved;
- Develop and improve devices using qualitative techniques and iterative prototyping (using 3D printing) within the BRIDGE methodology.

Methods

The study applied the BRIDGE methodology to the design of children's upper limb prostheses. Figure 1 outlines the overall research process within the framework of the BRIDGE methodology. Ethical approval for the various stages of this study was granted by the University of Southampton's Faculty of Health Sciences Ethics Committee (FoHS-ETHICS-2011-056; FoHS-ETHICS 2011-075; ID 1224).

Participants

Total sample size was 34, including eight children and adolescents with upper limb difference, nine parents, eight prosthetists and nine OTs. Parents and children were recruited through a charitable organisation (Reach Charity Ltd: <http://reach.org.uk/>). Professionals were recruited via conferences and professional networks, and worked at seven different limb clinics in England.

Design

The study followed a multi-stage design using focus groups and semi-structured interviews (with thematic analysis) to understand children's, parents' and professionals' views on upper limb prostheses, develop devices responding to these views and gain feedback on the devices. Children and adolescents and their parents were offered the choice to participate in a focus group or individual interview. Focus groups were not used with the professionals as the professional world of paediatric upper limb prosthetics in the UK is small and close-knit, which may have resulted in participants being reluctant to answer honestly and openly. Table 1 provides an outline of the demographic characteristics of the children and adolescents who participated and information about the number of participants for each data collection technique in the different stages of the study.

Techniques for developing prototypes

The prototypes were developed using 3D printing (specifically, additive manufacturing), which is a form of Rapid Prototyping Technology (RPT). RPT provides a means of quickly producing solid, 3D prototypes from 3D computer aided design files. Additive manufacturing is a cost effective method of RPT based on ink-jet technology, where a 3D structure is built up, layer by layer, in 2D slices. This enables a complete prototype to be created in one printing process. An Objet Connex350 3D printer was used because of its versatile range of printable engineering plastics and multi-material jetting technology.

Results

In stage one of the research, children and adolescents identified several characteristics of prostheses that they would like to see improved: appearance, comfort, ease of use, functional

use and movement. The second stage of the process involved developing five task-specific terminal devices and an adjustable wrist unit to support each of these devices; these were designed and fabricated by the second author of this paper. See table 2 for information about the different characteristics requested by the participants and the prototype that attempts to provide it. See figure 2 for photographs of the prototypes. Stages three, four and five involved gaining an understanding of all of the stakeholders' feedback on the prototypes. This feedback has been combined and linked to each device with direct quotes (using pseudonyms but with real ages) from the different participants.

Views of the newly developed prototypes:

Adjustable wrist unit (figure 2, photograph a)

Improved wrist rotation was identified by the children and adolescents as a desired development:

"I think if [the wrist] bends any way you want quite easily, that'd be [...] good"

(Gareth, aged 15).

Designing it to work within a modular system provides choice concerning the use of task-specific devices. Modularity also takes into consideration the impact of growth. The adjustable wrist unit, based on the ball and socket joint, comprises a fully rotatable and lockable wrist unit that supports a range of functional devices. The device consists of three parts: the wrist mount, the rotation ball and the friction cup. When the friction cup is screwed down over the wrist mount, the rotation ball becomes sandwiched firmly between the wrist mount and the inner surface of the friction cup, locking it securely in place. Unscrewing the friction cup slightly allows the rotation ball to be freely rotated in all axes. A ridged ring around the perimeter of the friction cup makes it easier to grip with the unaffected hand when loosening and tightening.

When presented to participants for feedback, all stakeholder groups felt that the device provided realistic movement (particularly in angulation [flexion/extension and radial/ulnar deviation] and rotation). Additionally parents felt the device would lock in place securely which they reported was important for safety reasons. However, whilst some participants (across all groups) felt the device would be easy to use, others thought it would be difficult due to its lack of spontaneity. Weight, size and shape were identified as potentially problematic by the professionals but these were not attributes that concerned the children and adolescents or parents.

Adjustable gripper (figure 2, photograph b)

Children and adolescents acknowledged the need for a gripper-type hand for dexterous tasks, but commented that available devices were uncomfortable and cumbersome, with particular reference to the discomfort caused by harnesses:

“I’ve always found those round the shoulder ones too hard to use because [...] it’s really itchy against your skin and it’s horrible.” (Chris, aged 12).

An adjustable gripper was designed and fabricated to incorporate a moveable digit rotating between two fixed digits. The device is operated with the unaffected hand using the ridged thumb wheel. The device provides a locked and secure grip between the adjustable and fixed digits.

All groups felt that the device could be useful in specific activities (playing instruments, woodwork) and that it provided a strong grip. However they also felt it was unattractive, heavy, slow and tiring to operate. The children and adolescents identified that this device

could be useful as a substitute prosthesis if their primary device was being altered or repaired. This demonstrates that being without a device has an impact on the children and adolescents.

Cycling appliance (figure 2, photograph c)

Participants identified it was important to have a device for cycling due to needing to look over both shoulders (and this being made difficult by unilateral upper limb difference), problems with using brakes one-handed and the need to wear a prosthesis in order to cycle at a standard required by the cycling proficiency test:

“I have to get [a prosthesis] for my cycling test [...] I think I’m going to have two brakes on the same side but I’ve got to wear a prosthetic.” (Emma, aged 9).

This motivated the design of a simple cycling appliance, which is a handlebar attachment shaped like a curled hand. The diameter of the inner grip can be redesigned using RPT to match the diameters of a range of handlebars.

All groups agreed that a device for cycling would be very useful as it is an activity that children with upper limb difference commonly have difficulties with. However, all were concerned about the lack of a quick-release mechanism and the risk this could present. OTs felt the device did not look attractive. The children and adolescents, however, were not concerned as, due to its task-specificity, they would not be using it for cosmetic reasons.

Jointed hand (figure 2, photograph d)

A jointed hand was developed based on the comments of children and adolescents that currently available passive prostheses do not have realistic movement. The movement of the prosthesis was identified by the children and adolescents as the reason it is noticeable that it is not a real hand:

“They look like a hand [but] they don’t exactly move like a hand.” (James, aged 8).

The hand was designed based on Snyder et al’s (26) dimensions for an average 8-year old male child, as these were the most recent published dimensions available at the time. The hand includes independent movement of all the fingers and thumb. It was designed as a conceptual piece to promote discussion among the children during follow-up sessions, demonstrating the introduction of technical expertise which may challenge children’s current thoughts about the possibilities for developing prosthetic devices.

Participants also identified that they would like prostheses to have fingers that move individually instead of only having one grip in order to replicate the natural movement of a hand as closely as possible:

“An opposable thumb and a lot more dexterity [...] and I think it would be really good if your fingers could move separately.” (Anna, aged 14).

Through further design it would be possible to automate finger and thumb movement as either a body-powered or myoelectric device.

All groups enjoyed the fluid movement that this device offered but were concerned that it should have softer, rounder edges to improve the appearance. Professionals suggested it could be used for gesturing or even holding objects, combining aesthetics and function.

Smartphone holder (figure 2, photograph e)

Difficulties in using computer and communication technology is an issue that the participants identified as important:

“I play loads of video games that require two hands and I can’t play them which is really annoying.” (David, aged 10).

Additionally, Smartphones were identified as potentially posing a difficulty for young people with unilateral upper limb difference as a prosthetic hand would not be tactile enough to operate a touch screen device. However, neither would it be able to hold a device securely or comfortably over long periods of time. A Smartphone holder was designed to support an iPhone4/4S, but using RPT these dimensions could be quickly changed to produce new versions for any mobile phone, tablet or multimedia device. The phone slots into the holder and is secured by closing the hinged lid at the top.

Some of the children and adolescents felt they would use a device to hold their Smartphone as they currently felt nervous about dropping and breaking it. Others, however, felt that they managed to use their phone without a device, having developed their own strategies (such as, placing their phone on a table to type). It was felt that this device would hold a phone securely whilst looking “cool” or being a gimmick.

Pen holder (figure 2, photograph f)

Children and adolescents identified that a prosthesis should help with the fine motor activities of writing and typing:

“What would be really, really magic would be if it could write.” (Emma, aged 9).

“It would be good if they could make a hand that you’d be able to like touch type with” (Anna, aged 14).

A two-part holder was designed consisting of a tapered tubular body, threaded at each end, and an adjustable clamp. The adjustable clamp has a hole to support a pen or other writing device up to a maximum external diameter of 10mm which, when screwed down onto the body of the holder, clamps the writing implement securely in place.

Whilst professionals could identify potential benefits of this device for their clients, the children and adolescents felt that it would not really be necessary for them. All groups, however, felt it could benefit bilateral amputees and could be adapted for use in a range of activities (such as typing and arts and crafts).

Combining participants' views to develop key themes:

The feedback from participants on the prototypes developed led to the identification of five broad themes relating to prosthesis development: that they should be quick and easy to use; inconspicuous; versatile; have natural movement and be safe and secure.

Theme one: Quick and easy to use

Children and adolescents explained that the device has to be quick and easy to use because it has to make performing the task more convenient than doing it using their residual limb. Professionals echoed this, explaining that anything that is a 'hassle' to use is likely to be unsuccessful for children. Participants felt that the method of screwing devices in and out of the wrist device was too time-consuming and that operating it could be too complicated and tiring.

Theme two: Inconspicuous

Some participants felt the Smartphone holder looked “cool” and would not draw attention as it looks similar to other Smartphone covers. Others, however, felt due to its size it may in fact draw attention. Participants also reported the 3-point grip, writing device and cycling appliance looked unrealistic and felt they could be improved if they looked more like a hand or had the suggestion of fingers. Participants believed this would prevent them from attracting unwanted attention from strangers.

Theme three: Versatile

The interchangeability of the terminal devices in the wrist unit was seen as positive by some participants as it was felt this was an improvement on needing to have more than one prosthesis (for different functions). Some participants (particularly the professionals) reported, however, that having a range of terminal devices may be difficult for a child to manage as they may potentially have several to carry around. Professionals and parents suggested this could be burdensome for children and may result in them forgetting or losing their devices. Terminal devices that were versatile for use in several activities were viewed more favourably by professionals. However the child participants did not reflect this view as they felt the different devices could be kept in different places depending on where they would be used, reducing the necessity to carry a range of devices at all times.

“You wouldn’t always have to carry them around, only if you needed to use them. The iPhone one could just go in a pocket... I guess you could wear one on your hand that was for general things and carry the more specific ones with you. And the writing one you could just keep it in your locker at school or work so you wouldn’t really need to carry it around.” (Anna, aged 14).

Theme four: Moves naturally

Participants liked the natural movement of the jointed hand. They reported that devices that require operation with the unaffected hand are less appealing (such as the wrist device and dial-operated 3-point grip) because it is not natural or instinctive to operate them in this way. They expressed a preference for devices which can be operated with the residuum only. It was reflected by professionals that children tend to prefer devices they can use in an instinctive, spontaneous manner rather than those that require planning and higher cognitive processes for operating. This idea is embodied in the hierarchical control of a myoelectric prosthesis.

Theme five: Safe and secure

Participants reported that it is important that the device they are using can be relied upon to securely hold an item. They felt that the dial-operated 3-point grip and Smartphone holder provided this. All participants were concerned about the safety of the cycling appliance and expressed a need for it to have a quick release mechanism in case the user fell off their bicycle when using it. Parents expressed a concern that children with unilateral upper limb difference have to be particularly careful not to injure their sound limb as that can have a huge impact on their function.

“It’s difficult because one time he got his arm trapped at school, his good arm, and it was in a sling for two days and he couldn’t do anything. So when someone’s got a disability you’re extra careful with what they have.” (Mother of James, aged 8).

Discussion

This study represents the first stage in the development of new prosthetic devices: continual, iterative development will be required to reach the stage at which they can be commercially

manufactured. However, involving users from this early stage ensures that the point of departure for the design is the users' own views, experiences and expertise. The findings support previous work (3; 4; 5; 6; 7) that prostheses for children need to be lighter, more comfortable, more useful and more attractive. Using this methodology has also highlighted that prostheses should be safe, quick and easy to use; and natural (in both appearance and movement). This demonstrates the value of involving children in the development of prostheses and medical technology generally. The participants demonstrated an ability to engage fully in the study and share unique insights which may not have been gleaned through other methods. Children have been enabled to express their views on matters they may not routinely be consulted on, allowing them to exert more control over matters affecting them, as well as recognising them as equally able to impart insightful knowledge and experience.

Iversen and Brodersen (25) used the BRIDGE method to involve children in the design process for information technology applications. The current study is the first to apply the methodology to healthcare technology and has demonstrated how this method can be successfully applied to a range of stakeholders and in a health technology domain. Having an awareness of the issues relevant to all users is important to prosthesis design because they can impact on the use or non-use of the devices. Prosthetists and OTs have expressed the belief that involving children and parents in designing and choosing prostheses leads to feelings of ownership and, subsequently, reduces non-use of devices (27). Taking the views of any of the stakeholders in isolation may lead to a neglect of important influences that impact on prosthesis use.

Appreciating the involvement of children reflects the ethos of the BRIDGE methodology: children are experts in their daily lives and design cannot happen without the involvement of

these experts (25). The current study has demonstrated that this approach to participatory design can produce rich and relevant data in the context of health technology design.

Additionally, a consequence of involving children in the design process is that they will gain experience of these ways of working with adults, which will enable their learning and development for future participation (25).

Using prototype devices and requesting feedback on them is a tangible way of demonstrating to participants that they have been actively listened to through interpreting and constructing meanings from the information shared by participants. 3D printing provides a method of rapidly producing a model for the visualisation of these interpretations and constructions. Being able to validate a new idea or concept at an early stage in the design process using 3D printing also prevents costly mistakes at later stages. The technical advantages of 3D printing were demonstrated in more complex designs, such as the adjustable wrist unit and the gripper hand, where it was possible to assemble fully functioning (moving) parts and test complex mechanical design concepts. This further allows for a quick and cost effective evaluation of whether a manufactured part will function as designed and allows design refinements and adjustments to be made to meet an individual's needs. 3D printing may prove to be a useful manufacturing technology in the development of new prosthetic devices, particularly in the case of bespoke, customisable solutions. Using the BRIDGE methodology with RPT techniques has led to several recommendations for the development of new devices.

Cost-effective task specific devices:

Participants identified that it would be useful to have prosthetic devices for cycling, writing, typing, computer use, self-care and grooming. Devices should also be designed with

durability in mind due to the environments in which children use prostheses and the activities for which they use them.

Modular devices:

The prototypes designed in this study were fabricated to work in a modular system.

Modularity affords a device greater versatility (identified as important by participants) as its use can be altered through changing specific features. Modular devices can also be more adaptable to a child's growth and development, as certain aspects can be altered without the need for an entirely new device.

Comfort:

Comfort was identified as an important feature of prostheses, with the harnesses on body-powered devices described by participants as uncomfortable and itchy. The scope for the current study was to develop terminal devices, but future device development needs also to focus on improving comfort for the wearer: an otherwise highly useful device may go unworn if it causes pain or discomfort. Device development may also benefit from focusing on reducing the weight of particular components to reduce discomfort. However, another way of addressing this concern may be to provide appropriate training that gradually prepares a child for the increased weight of a prostheses.

Reflection on data collection methods:

This study demonstrates that focus groups and interviews are appropriate tools for the collection of qualitative data with children. Qualitative methods enable participants to influence the agenda of the research interview or direction of focus group discussion, ensuring that the factors that are important to them are highlighted to the researcher in the

participants' own words (28). This is especially important when researching such a personal experience as an individual's use of healthcare technology. Triangulation of data by examining the views of a range of stakeholders enhances the credibility of the findings from this study as multiple perspectives were sought, reducing any potential influence of the researcher's own beliefs and philosophies (29).

Although valuable data regarding participants' views on the prototypes was gained through conversational methods, the data gathered could have been enhanced by the use of audio-visual recording. This would have provided additional information on the way participants interacted with the prototypes and how easy they found them to operate in practice.

Conclusion

The study has led to the development of several prototypes of cost-effective task-specific prosthetic devices that are suitable for further development and refinement. Use of RPT in conjunction with stakeholder perspectives can lead to improved design in prostheses and health technologies more broadly. Inclusion of users of devices, and improvements in design, should result in wider use of such technologies. For children with upper limb difference, this could lead to improvements in physical and psychological well-being. The development of upper limb prostheses needs to continue to involve users, and other stakeholders, to ensure future designs consider the needs and wants of users as well as technological advancements.

5) References

1. Smith DJ. Congenital Limb Deficiencies and Acquired Amputations in Childhood Part 3. *In Motion*. 2006;16(3).
2. Shida-Tokeshi J, Bagley A, Molitor F, Tomhave W, Liberatore J, Brasington K and Montpetit K. Predictors of Continued Prosthetic Wear in Children With Upper Extremity Prostheses. *Journal of Prosthetics and Orthotics*. 2005;17(4):119-124.
3. Routhier F, Vincent C, Morissette MJ and Desaulniers L. Clinical results of an investigation of paediatric upper limb myoelectric prosthesis fitting at the Quebec Rehabilitation Institute. *Prosthetics & Orthotics International*. 2001;25(2):119-131.
4. Wagner LV, Bagley AM and James MA. Reasons for Prosthetic Rejection by Children with Unilateral Congenital Transverse Forearm Total Deficiency. *Journal of Prosthetics and Orthotics*. 2007;19(2):51-54.
5. Biddiss EA and Chau TT. Upper-limb prosthetics: critical factors in device abandonment. *American Journal of Physical Medicine and Rehabilitation*. 2007;86(12):977-87.
6. Pylatiuk C, Schulz S and Döderlein L. Results of an Internet survey of myoelectric prosthetic hand users. *Prosthetics and Orthotics International*. 2007;31(4):362-70.
7. Donovan-Hall M. Supporting the positive development and well-being of children and young people with prostheses: the influence of the appearance of the prosthesis and individual choice. *Big Lottery Final Report*. 2010;RG1/010120846.
8. Allsop MJ, Holt RJ, Levesley MC and Bhakta B. The engagement of children with disabilities in health-related technology design processes: identifying methodology. *Disability, Rehabilitation and Assistive Technology*. 2010;5(1):1-13.

9. Sinclair R and Franklin A. Young People's Participation: Quality Protects Research Briefing, No.3. Department of Health, London; 2000.
10. Nasset V and Large A. Children in the information technology design process, A review of theories and their applications. *Library & Information Science Research*. 2004;26:140–161.
11. Light L, Page R, Curran J, Pitkin L. Children's ideas for the design of AAC assistive technologies for young children with complex communication needs. *Augmentative and Alternative Communication*. 2007;23:274 – 287.
12. Rigby P, Ryan S, From W, Walczak E and Jutai J. A client-centred approach to developing assistive technology with children. *Occupational Therapy International*. 1996;3(1):67–7.
13. Cooke GA. Involving children in planning healthcare: The Derby experience. *Current Paediatrics*. 2004;14:246–251.
14. Weightman APH, Preston N, Holt R, Allsop M, Levesley M and Bhakta B. Engaging children in healthcare technology design, developing rehabilitation technology for children with cerebral palsy. *Journal of Engineering Design*. 2010;21(5):579-600.
15. Atkins D, Heard DCY and Donovan WH. Epidemiologic overview of individuals with upper-limb loss and their reported research priorities. *Journal of Prosthetics and Orthotics*. 1996;8(3):2-11.
16. Biddiss EA, Beaton, D Chau TT. Consumer design priorities for upper limb prosthetics. *Disability and Rehabilitation: Assistive Technology*. 2007; 2(6):346-357.
17. Shah SGS and Robinson I. Medical device technologies: who is the user? *International Journal of Healthcare Technology and Management*. 2008;9(2):181-197.


18. Shah SGS and Robinson I. User Involvement in Medical Device Technology Development and Assessment: A Structured Literature Review. *International Journal of Health Care Quality Assurance*. 2006;19(6):500-515.
19. Nichols PJ, Rogers EE, Clark MS and Stamp WG. The Acceptance and Rejection of Prostheses by Children With Multiple Congenital Limb Deformities. *Journal of Artificial Limbs*. 1968;12(1):1-13.
20. Postema K, van der Donk V, van Limbeek J and Rijken RA. Prosthesis rejection in children with a unilateral congenital arm defect. *Clinical Rehabilitation*. 1999;13(3):243-249.
21. Rycroft-Malone J. Formal consensus, the development of a national clinical guideline. *Quality Health Care*. 2001;10(4):238-44.
22. Resnik L. Development and testing of new upper-limb prosthetic devices, Research designs for usability testing. *Journal of Rehabilitation research and development*. 2011;48(6):697-706.
23. Peerdeman B, Boere D, Witteveen H, Huis R, Hermens H, Stramigioli S, Rietman H, Veltink P and Misra S. Myoelectric forearm prostheses, State of the art from a user-centred perspective. *Journal of Rehabilitation Research and Development*. 2011;48(6):719-738.
24. Glushko A. Participatory Design in Healthcare, Patients and doctors can bridge critical information gaps. *UX Magazine*. 2013;1028.
25. Iversen OS and Brodersen C. Bridging the Gap between users and children - A socio-cultural approach to designing with children. *Cognition, Technology and Work: special issue on Child-Computer Interaction Methodological Research*. 2007;9(2).
26. Snyder RG, Spencer ML, Owings CL and Schneider LW. *Anthropometry of U.S. Infants and Children*. Warrendale, Pa: Society of Automotive Engineers, Inc; 1975.

27. Sims T. A Participatory Design Approach to Developing Upper Limb Prostheses for Children and Young People (Unpublished doctoral thesis). University of Southampton, UK; 2014.
28. Crow I. The power of research. In: Burton D, ed. Research training for social scientists: A handbook for postgraduate researchers. London, Sage; 2000:68-80.
29. Knafl K and Breitmaye B. Triangulation in qualitative research, Issues of conceptual clarity and purpose. In: Morse J, ed.. Qualitative nursing research. Rockville, MD: Aspen; 1989:193-203.

6) Figure Captions

Figure 1: Overall research process within the framework of the BRIDGE methodology.

Figure 2: Prototype devices developed (a=adjustable wrist unit; b=adjustable gripper; c=cycling appliance; d=jointed hand; e=Smartphone holder; f=pen holder).

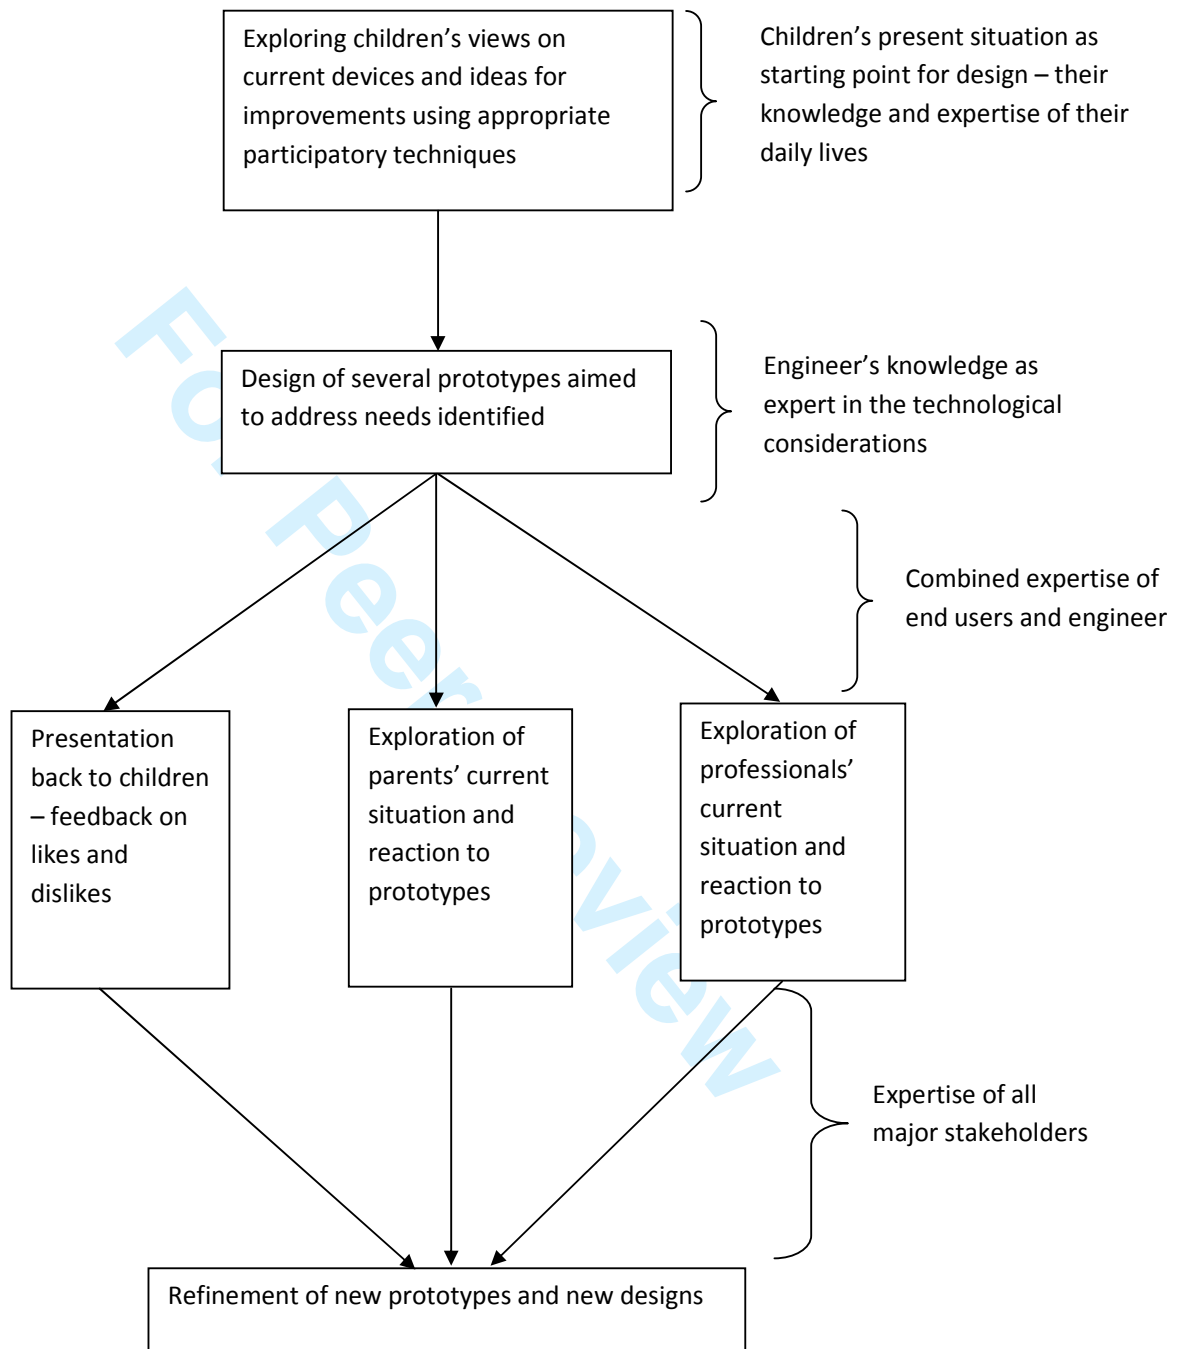




a




b



c

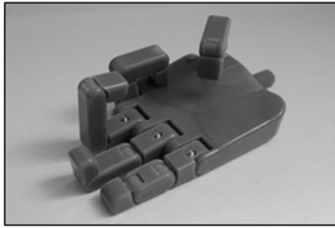

d

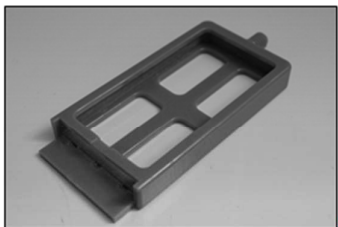

e



f

Review

| Characteristics of child and adolescent participants | | | | | | | | |
|--|-----------------------------------|-----------------------------------|------------------|---|----------------------|------------------------------|------------------------|-----------------|
| Gender | | Limb Difference | | Level/side of limb difference | | Experience of prosthesis use | | |
| Male | Female | Congenital | Acquired | Right arm below elbow | Left arm below elbow | Currently daily | Currently occasionally | Previously used |
| 4 | 4 | 7 | 1 | 5 | 3 | 2 | 4 | 2 |
| Stages of the study, data collection method and number of participants | | | | | | | | |
| | Stage 1: children and adolescents | Stage 2: children and adolescents | Stage 3: parents | Stage 4: prosthetists and occupational therapists | | | | |
| Focus Group | 4 participants | 2 participants | 2 participants | | | | | |
| Interview | 4 participants | 5 participants | 7 participants | 17 participants | | | | |

Table 1: Characteristics of Participants (children and adolescents) and stages of the study, data collection method and number of participants

| Area of improvement | Specific issue identified | Corresponding prototype |
|---------------------|---|---|
| Appearance | Appearance is negatively impacted by unrealistic movement | Jointed hand |
| Comfort | Shoulder harness discomfort | Adjustable gripper (not operated using scapular movements) |
| Ease of use | Lack of wrist rotation Not adaptable to different tasks | Wrist unit – has full rotation and can be used with a range of terminal devices |
| Functional use | Prostheses not suitable for cycling Prostheses not suitable for Smartphone use Prostheses not suitable for writing and typing | Cycling device Smartphone holder Pen holder |
| Movement | Movement provided is limited and not realistic Lack of wrist rotation | Jointed hand Wrist unit |

Table 2: Area of improvement, specific issue and prototype aimed to address it.