

Serveur Académique Lausannois **SERVAL** [serval.unil.ch](https://serval.unil.ch)

## Author Manuscript

Faculty of Biology and Medicine Publication

**This paper has been peer-reviewed but does not include the final publisher proof-corrections or journal pagination.**

Published in final edited form as:

**Title:** Total Blood Carbon Monoxide: Alternative to Carboxyhemoglobin as Biological Marker for Carbon Monoxide Poisoning Determination.

**Authors:** Oliverio S, Varlet V

**Journal:** Journal of analytical toxicology

**Year:** 2018 Oct 29

**DOI:** 10.1093/jat/bky084

In the absence of a copyright statement, users should assume that standard copyright protection applies, unless the article contains an explicit statement to the contrary. In case of doubt, contact the journal publisher to verify the copyright status of an article.

**Total blood carbon monoxide (TBCO): alternative to carboxyhaemoglobin (COHb) as biological marker for carbon monoxide (CO) poisoning determination**

Journal:	<i>Journal of Analytical Toxicology</i>
Manuscript ID	JAT-18-2657.R1
Manuscript Type:	Article
Date Submitted by the Author:	n/a
Complete List of Authors:	Oliverio, Stefania; University Center of Legal Medicine Lausanne-Geneva , Forensic Toxicology and Chemistry Unit; Brunel University London, Department of Environmental Sciences VARLET, Vincent; University Center of Legal Medicine Lausanne- Geneva, Forensic Toxicology and Chemistry Unit
Keywords:	carbon monoxide, carbon monoxide determination, blood analysis, flushing, GC-MS, carbon monoxide exposure, biomarker

SCHOLARONE™  
Manuscripts

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

**Total blood carbon monoxide (TBCO): alternative to  
~~carboxyhaemoglobin~~carboxyhemoglobin (COHb) as biological  
marker for carbon monoxide (CO) poisoning determination**

**Authors: Oliverio S.<sup>1,2</sup>, Varlet V.<sup>1</sup>**

**Author affiliations**

1. Forensic Toxicology and Chemistry Unit, University Centre of Legal Medicine Lausanne-Geneva, Chemin de la Vulliette 4, 1000 Lausanne, Switzerland

2. College of Health and Life Sciences, Department of Environmental Sciences, Brunel University London, Kingston Lane, Uxbridge, Middlesex UB8 3PH, United Kingdom

**Corresponding authors:**

Stefania Oliverio: [stefania.oliverio@chuv.ch](mailto:stefania.oliverio@chuv.ch)

Vincent Varlet: [vincent.varlet@chuv.ch](mailto:vincent.varlet@chuv.ch)

## Abstract

As one of the most abundant toxic contaminants in the atmosphere, carbon monoxide (CO) plays a significant role in toxicology and public health. Every year around half of the accidental non-fire related poisoning deaths are attributed to CO in the US, UK and many other countries. However, due to the non-specificity of the symptoms and often encountered inconsistency of these with the results obtained from measurements of the biomarker for CO poisonings, carboxyhaemoglobin (COHb), there is a high rate of misdiagnoses. The mechanism of toxicity of CO includes not only the reduced transport of oxygen caused by COHb, but also the impairment of cellular respiration and activation of oxidative metabolism by binding to other proteins.

Therefore, in this study we propose the measurement of the total amount of CO in blood (TBCO) by Airtight Gas Syringe-Gas Chromatography-Mass Spectrometry (AGS-GC-MS) as an alternative to COHb for the determination of CO exposures. The method is validated for a clinical range with TBCO concentrations of 1.63-104 nmol/mL of headspace (HS) (0.65-41.6  $\mu\text{mol/mL}$  blood). The limit of quantification (LOQ) was found between 2 and 5 nmol/mL HS (0.8 and 2  $\mu\text{mol/mL}$  blood). The method is applied to a cohort of 13 patients, who were exposed to CO under controlled conditions, and results compared to those obtained by CO-oximetry. Furthermore, samples were compared before and after a "flushing" step to remove excess CO.

Results showed a significant decrease of TBCO when samples were flushed (10-60%), whereas no constant trend was observed for COHb. Therefore, measurement of TBCO by AGS-GC-MS suggests the presence of more dissolved CO than previously known. This constitutes a first step into the acknowledgment of a possibly significant amount of CO present not in form of COHb, but as free CO, which might help explain the incongruences with symptoms and decrease misdiagnoses.

**Keywords:** carbon monoxide exposure; carbon monoxide determination; CO rebreathing; blood analysis; flushing; GC-MS; biomarker;

## 1. Introduction

Carbon monoxide (CO) is a highly toxic gas produced through incomplete combustion of hydrocarbon-based materials and fuels. It is one of the most abundant air pollutants, hence every individual is exposed to it on a daily basis through the innate and essential act of breathing.

However, CO in small amounts is also produced endogenously, mainly through catalysis of heme and heme-containing proteins and through processes such as lipid peroxidation and photooxidation. Therefore, very low levels of CO are present in each individual, even though levels can vary according to physiological as well as pathological conditions [1].

The burden of CO in air varies according to the amount and type of CO sources present in the living or working area of an individual, the season, which determines whether there are higher number of fires and barbecues (summer) or a high use of wood- or fuel-fired stoves and heaters (winter), and whether the individual is a smoker or exposed to passive smoke. Typically, CO concentrations in indoor air are below 30 ppm, they are around double the amount in outdoor air [2]. Even though the World Health Organization (WHO) and the national health and safety institutions of most countries have clear guidelines on the tolerance limits for CO exposure [3-5], carbon monoxide poisoning is the main cause of accidental non-fire related poisoning deaths in western countries [6, 7] and leads to a high number of emergency department (ED) admissions worldwide [6-16]. However, these numbers of fatalities and ED admissions likely underestimate the real burden of CO on the population. This is due to the characteristics of CO and the clinical, non-specific symptoms of CO intoxication. CO is an odorless, tasteless and colorless gas, making it difficult to detect if above normal concentrations and without the appropriate measuring devices [17]. Clinical diagnosis of CO poisoning is difficult due to the non-specific symptoms it presents: dizziness, nausea, fatigue, headaches [18]; often the causes of CO poisonings are misdiagnosed and attributed to other diseases or disturbances [19]. Misdiagnoses can also arise from errors due to the analytical measurement techniques and parameters used (measurement error) and the related incongruence with symptoms reported by patients [19-23].

The current biomarker for CO exposure is ~~earboxyhaemoglobin~~carboxyhemoglobin (COHb). Once CO enters the bloodstream, it binds to hemoglobin (Hb) competitively to oxygen (O<sub>2</sub>) [24, 25]. This very high affinity of CO for Hb (200-250 times higher than O<sub>2</sub>) causes a strong bond

1  
2  
3  
4  
5  
6  
7  
8  
9 between CO and Hb and leads to the inhibition of oxygen transport through Hb and delivery to  
10 tissues, also a suggested mechanism for the resulting hypoxia in brain and heart, primary  
11 consequences of CO exposure [3]. However, the presence of CO in blood only in form of COHb  
12 does not explain the inconsistency repeatedly reported between COHb% results and symptoms  
13 [26]. One hypothesis, suggested in previous studies [23, 27], is that a random and possibly  
14 significant amount of CO in blood is not bound to Hb, but is present in free form and can thus  
15 distribute to other tissues, ~~has~~leading to pathophysiological relevance-effects through direct  
16 cellular toxicity. Around 10-15% of the absorbed CO has been previously documented to bind to  
17 proteins other than Hb [28, 29]. These other proteins include myoglobin, cytochromes and  
18 guanylyl cyclase. Binding to myoglobin reduces the availability of oxygen in the heart and may  
19 lead to arrhythmias and cardiac dysfunctions as well as causing direct toxicity of skeletal muscle  
20 [30]. CO binding to mitochondrial cytochrome oxidase, which was reported for *in vitro* studies  
21 [31, 32], impairs cellular respiration by inactivation of mitochondrial enzymes and also initiates  
22 an oxidative metabolism by generating oxygen free radicals [29, 30, 33]. Even though the  
23 affinity of CO for cytochrome oxidase is relatively low, the dissociation is very slow, leading to  
24 a prolonged impairment of oxidative metabolism, which may help explain the tardive and  
25 sustained effects of CO toxicity even after COHb has been cleared from the system through  
26 hyper- or normobaric oxygen therapy [28, 29]. The loss of consciousness associated with CO  
27 poisoning may be caused by the stimulation of guanylyl cyclase, since increases in cyclic  
28 guanosine monophosphate (cGMP) result in cerebral vasodilation [34, 35].

29  
30  
31  
32  
33  
34  
35  
36  
37 In general, the role of direct cellular CO toxicity seems to be underestimated in the prevailing  
38 CO poisoning literature, given that most studies date back several decades. But given the  
39 numerous pathophysiological mechanisms, it is important to be able to determine the total  
40 amount of CO and not only COHb in CO poisoning cases.

41  
42  
43 However, current measurement methods are based on COHb, either through spectrophotometric  
44 techniques, such as UV-spectrophotometry and CO-oximetry [36-41], or gas chromatographic  
45 techniques, such as Gas Chromatography-mass spectrometry (GC-MS) or GC-Flame Ionization  
46 Detection (GC-FID) [1, 42-48], where the CO measured is backcalculated and correlated to  
47 COHb. The issue with optical methods is the dependency of the technique on the quality of the  
48 sample. Alterations of the sample, which can occur through degradation due to a time-delayed  
49  
50  
51

1  
2  
3  
4  
5  
6  
7  
8  
9 analysis or/and unsatisfactory and uncontrolled storage conditions [39, 45, 49-53], make the  
10 optical analysis difficult to interpret or in some cases infeasible. Gas chromatographic methods  
11 can overcome these problems in most cases. The CO present in blood is released through a  
12 releasing agent and then analysed either directly (GC-MS) [42, 44-46] or after transformation  
13 into methane (GC-FID) [47, 54-57] in its gaseous form. One important step that has been applied  
14 in previous studies includes the “flushing” of the calibrator in order to target only CO bound to  
15 Hb. To achieve that, blood is subjected to a stream of nitrogen gas for an amount of time, to  
16 remove all excess CO [45, 47, 48, 52, 55, 56, 58] and, therefore, this approach does not consider  
17 the amount of excess CO as relevant, but only that bound to Hb. This could lead to mis- or  
18 underestimation of the total load of CO in blood. For this reason, in a previous study an approach  
19 that is based on the measurement of the total amount of CO in blood (TBCO) by airtight gas  
20 syringe(AGS)-GC-MS was developed and validated, however only for a concentration range  
21 with postmortem application [23].  
22  
23  
24  
25  
26

27 With this research, we aim to test the hypothesis of the presence of CO in free form in blood, by  
28 comparing analysis results of flushed and unflushed blood samples obtained at bedside from  
29 patients that were exposed to CO. This represents the first step in expanding the knowledge of  
30 the true CO burden. Furthermore, we want to improve the TBCO measurement technique by  
31 validating it for a concentration range applicable also in clinical settings.  
32  
33  
34  
35

## 36 **2. Materials and Methods**

### 37 2.1 Chemicals and reagents

38  
39  
40  
41  
42  
43  
44 Formic acid (reagent grade, purity  $\geq 95\%$ ) was purchased from Sigma-Aldrich (St Louis, USA)  
45 and CO gas (99%) was from Multigas (Domdidier, Switzerland). To prevent degradation all  
46 formic acid solutions were prepared on a daily basis. The internal standard formic acid (13C,  
47 99%) was ordered from Cambridge Isotope Laboratories (Cambridge, UK). Sulfuric acid  
48 ( $\geq 97.5\%$ ) was purchased from Fluka (Buchs, Switzerland). Human blood samples were obtained  
49  
50  
51

1  
2  
3  
4  
5  
6  
7  
8 from volunteers participating in a study at the Department of Nephrology of the University  
9 Hospital of Geneva (HUG) in Switzerland. Blood of non-smokers before exposure to CO was  
10 used as blank matrix. For the *in vitro* study of CO fortified blood, bovine blood was obtained  
11 from a local butcher.  
12  
13  
14  
15

## 16 2.2 Materials

17  
18  
19  
20  
21 The AVOXimeter 4000 Whole Blood CO-Oximeter and cuvettes were obtained from  
22 International Technidyne Corporation - ITC (Edison, USA). S-Monovettes of following types:  
23 2.6mL K3E (Ethylenediaminetetraaceticacid, EDTA), 3mL 9NC (sodium citrate, NaCit), 2.7mL  
24 FE (sodium fluoride, NaF), 2.6mL KH (lithium heparin, LiH), were obtained from Sarstedt  
25 (Nürnbrecht, Germany). Precision sampling gas syringes equipped with a press button valve and  
26 with capacities of 500 $\mu$ L (for dilution) and 2mL (for injection) were purchased from VICI  
27 (Baton Rouge, LA, USA). Aluminum caps were from Milian (Vernier, Switzerland). All  
28 extractions were carried out in 20mL headspace vials from Agilent Technologies (Santa Clara,  
29 CA, USA).  
30  
31  
32  
33  
34  
35

## 36 2.3 Instruments and GC-MS conditions

37  
38  
39  
40 AVOXimeter 4000 Whole Blood CO-Oximeter from ITC was used for all COHb analyses. The  
41 instrument uses five wavelengths for quantitative analysis, namely 520.1, 562.4, 585.2, 597.5  
42 and 671.7 nm. Following parameters can be measured: total hemoglobin (tHb), oxyhemoglobin  
43 (O<sub>2</sub>Hb), COHb and Methemoglobin (MetHb). In this study, Manufacturer guidelines were  
44 followed to obtain COHb concentrations [59, 60].  
45  
46

47 Agilent 6890 N GC (Palo Alto, USA) equipped with a HP Molecular Sieve 5 Å PLOT capillary  
48 column (30 m x 0.32 mm x 30 $\mu$ m) purchased from Restek (Bellefonte, USA) was used for gas  
49 chromatographic analysis. The temperature program used was as follows: 50°C, held for 4  
50  
51



1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

minutes; injector temperature was set at 180°C, the injector used in splitless mode, and the MS interface at 230°C. Helium was employed as carrier gas, at a flow rate of 40.0 mL/min. A solvent delay of 1.8 minutes was introduced.

An Agilent 5973 mass spectrometer (Palo Alto, USA) was used for detection, operating in electron ionization (EI) mode at 70eV. Selected Ion Monitoring (SIM) mode was used to acquire the signal for CO at m/z 28 and <sup>13</sup>CO at m/z 29, both at the same retention time of 3.5 min.

## 2.4 Sample preparation

### *2.4.1 Calibration standards*

An aliquot of human blood from non-smokers, which was previously controlled by CO-oximetry and found at 0% COHb, is used as matrix for calibration. Calibration standard working solutions of formic acid (43 µmol/mL) and working solutions of the internal standard isotopically labelled formic acid (84 µmol/mL) were prepared daily *de novo* in order to prevent degradation. Calibration points were set in a working range between 0-104 nmol/mL HS, with points at 1.63, 3.25, 6.5, 13, 26, 52 and 104 nmol/mL HS (equivalent to 0.65, 1.3, 2.6, 5.2, 10.4, 20.8 and 41.6 µmol/mL in blood). Matrix effects were evaluated by preparing a blank sample with the matrix without any reagent. 10 µL of the working internal standard solution were added to each calibration sample before extraction, leading to a final concentration of 42 nmol of <sup>13</sup>CO/mL HS. All standards and samples were stored at +4°C when not in use.

### *2.4.2 Quality controls (QC)*

QC were performed with five internal control samples, at concentrations of 2, 5, 10, 30 and 60 nmol/mL HS (0.8, 2, 4, 12 and 24 µmol/mL blood), which were prepared daily with formic acid obtained from a different lot diluted with deionized water.

1  
2  
3  
4  
5  
6  
7  
8  
9 Additionally, validity of the method was tested with external controls, which were prepared by  
10 dilution of pure CO gas at two concentration levels, low and high, respectively 5 and 60  
11 nmol/mL HS.  
12  
13  
14

#### 15 *2.4.3 Extraction procedure*

16  
17 100µL aliquots of blood were introduced in a 20mL HS-vial, followed by 10µL of the internal  
18 standard solution. For calibration points, the respective aliquots of formic acid solution were  
19 added. Aluminum caps of 11mm (i.d.) were first filled with 100µL sulfuric acid and then  
20 carefully introduced into the HS-vial. The vial was immediately hermetically sealed with  
21 PTFE/silicone septum caps of 20 mm (i.d.). In order to ensure complete mixing of the liquids  
22 contained in the vial, the samples were vigorously shaken and vortexed. Extraction was finalized  
23 by heating the vials at 100°C for 60 minutes.  
24  
25  
26  
27  
28  
29

#### 30 2.5 Analysis procedure

##### 31 *2.5.1 CO-oximeter*

32  
33  
34 Approximately 50-100µL of blood were sampled from the sampling tube and placed into an  
35 Avoximeter 4000 Whole Blood CO-oximeter cuvette, which was then introduced in the  
36 Avoximeter 4000 Whole Blood CO-oximeter for analysis.  
37  
38  
39  
40  
41  
42

##### 43 *2.5.2 CO in blood*

44 1mL HS was sampled from the 20mL HS-vial containing the extract and injected in the GC-MS  
45 for analysis.  
46  
47

48 To ensure that no contamination from CO contained in the air affected the measurements  
49 occurred, a 1mL aliquot of air in the analysis-room was additionally analysed prior to sample  
50  
51

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

analyses. Air samples were collected with the AGS and analysed by GC-MS with the same conditions as the blood samples.

## 2.6 Validation procedure

The validation was performed according to the guidelines of the “French Society of Pharmaceutical Sciences and Techniques” (SFSTP) [61] and included following validation parameters: response function (calibration curve), linearity, selectivity, trueness, precision (repeatability and intermediate precision), accuracy, limit of detection (LOD) and limit of quantification (LOQ).

The response function, also defined as the calibration curve, is described as the relationship between the concentration of the analyte in the sample and the corresponding instrument response.

Linearity of the method is assessed by fitting backcalculated concentrations of control samples against the theoretical concentrations through application of the linear regression model and evaluating the resulting regression coefficient.

Trueness, also defined as bias, describes the closeness between the average of the experimental value and the calculated target value. It is expressed as percent deviation from the calculated target value.

Precision is defined as closeness of agreement (degree of scatter) between a measurement series obtained from multiple sampling of the same homogenous sample under the prescribed conditions and is determined by calculating the repeatability (intra-day precision) and intermediate precision (inter-day precision) for each control sample. The repeatability is determined by calculating the intra-day variance ( $S^2_r$ ) and the intermediate precision through the sum of intra- and inter-day variances ( $S^2_{IP}$ ).

1  
2  
3  
4  
5  
6  
7  
8 Accuracy describes the closeness of agreement between the conventional true value or an  
9 accepted reference value and the value experimentally found. It is expressed as the sum of  
10 trueness (systematic error) and precision (random error).  
11  
12

13 Calibrators and QCs were used for the validation experiments performed on three non-  
14 consecutive days ( $p=3$ ) not within the same week. The validation approach is based on the use of  
15 a  $\beta$ -expectation interval tolerance of 80%, indicating that the intervals for each experimental  
16 point include an average of 80% of the total values. The tolerance intervals (TI) were defined as  
17  $TI = X \pm k \times \sqrt{(S_r^2 + S_R^2)}$ , where  $S_r^2$  is the standard deviation of repeatability and  $S_R^2$  is the  
18 standard deviation of reproducibility. In the  $\beta$ -expectation interval tolerance approach,  $k = t_v \times$   
19  $\sqrt{(1 + [1 / (I \times J \times B^2)])}$ , where  $I$  is number of series,  $J$  is the number of repetitions, and  $B^2$  is a  
20 coefficient. This coefficient is given as  $B^2 = (R + 1) / [J \times (R + 1)]$  with  $R = S_r^2 / S_R^2$ .  $t_v$  is  
21 Student's coefficient with degrees of freedom  $v$  defined as  $v = (R + 1)^2 / \{[(R + 1 / J)^2 / (I - 1)] +$   
22  $[(1 - 1/J) / (I \times J)]\}$ .  
23  
24  
25  
26  
27  
28

## 29 2.7 Samples from volunteers

### 30 31 32 33 *2.7.1 CO-rebreathing method*

34  
35 The CO-rebreathing method consists of a closed-circuit breathing system containing oxygen  
36 mixed with a certain amount of carbon monoxide. Patients breathe in and out through a  
37 mouthpiece linked to the circuit. In the study from which we acquired the blood samples,  
38 patients were lying in horizontal position. After insertion of the mouthpiece, an adjustment  
39 period of 2 minutes was used to deliver  $O_2$  only, before starting the delivery of the  $O_2$ -CO  
40 mixture for a period of 10 minutes [62]. The volumes of CO delivered in  $O_2$  were between 57  
41 and 105 mL, calculated according to the body mass index of each volunteer, in order to reach a  
42 target COHb value of approximately 10%.  
43  
44  
45  
46  
47  
48

### 49 *2.7.2 Blood collection and preparation*

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Blood samples were obtained from a cohort of 13 patients (9 men, 4 women) under treatment at the Nephrology Department of the University Hospital in Geneva (HUG), Switzerland.

Three blood samples were taken from volunteers, one before and two directly after exposure to CO. Samples were immediately analysed by CO-oximetry. Half of the samples taken after exposure of the individual to CO were flushed with a nitrogen stream for 2 minutes, with a flow rate below 5 mL/min. Two needles were inserted in the rubber septum of the blood tube. One needle was plunged in blood and provided the nitrogen stream whereas the other was placed in the HS of the blood tube in order to relieve the pressure in the blood tube built with the release of CO and the nitrogen flush. After flushing, the samples were analysed by CO-oximetry. Simultaneously, all samples (before exposure, flushed and not flushed after exposure) were prepared for analysis with AGS-GC-MS and analysed in triplicates. All sampling and testing performed on volunteers was approved by ethical committee under the study number CCER-2017-00421.

### 2.8 *In vitro* study of CO fortified samples

To test the relevance of the validated clinical range of CO concentrations for the blood samples obtained from the volunteers, *in vitro* CO-fortified blood samples were prepared. Bovine blood was obtained freshly from a local butcher and immediately transferred in containers with anticoagulants (EDTA, LiH, NaF, NaCit) to avoid coagulation during transport to the laboratory. After arrival at the laboratory, CO-oximetric analyses of the blood were performed to confirm the baseline CO-content. Fortification with pure CO gas was then carried out by bubbling the gas directly into the blood for varying amounts of time. The COHb saturation levels were checked in 10-minute-intervals with the CO-oximeter until the desired initial COHb% level was reached. To ensure homogenization, the bottles were agitated for 20 minutes after fortification and the final COHb concentration was subsequently measured. After reaching of the designated COHb%-saturation (10-20%, 30-40% and 60-70%), blood was transferred to the sampling tubes and subsequently analysed without any flushing, in order to respect the physiological conditions of blood sampling and analysis when an individual is suspected of a CO poisoning.

## 2.9 Statistical analyses

Mean, standard deviation and interquartile ranges were determined for all measured variables. Paired student *t*-test with a  $\alpha$ -error of 0.05 was performed for comparison of the group means. All data treatment and statistical analyses were performed with R (version 3.3.1, 2016-06-21).

## 3. Results

### 3.1 Validation of the method in a clinical range

Results of the validation for all criteria are summarized in Table 1.

Calibration curves for CO determination were obtained by using CO negative human blood as blank matrix. Calibration curves, which represent the response function, were acquired on three non-consecutive days ( $p = 3$ ), in triplicates ( $n = 3$ ) and at seven concentration levels ( $k = 7$ ): 1.63, 3.25, 6.5, 13, 26, 52 and 104 nmol/mL HS (equivalent to 0.65, 1.3, 2.6, 5.2, 10.4, 20.8 and 41.6  $\mu\text{mol/mL}$  blood). For each calibration point, calculated concentrations were compared to the target values and found to be within  $\pm 20\%$ . The relationship between the CO concentration from samples spiked with formic acid and the measured response was found to be linear. Validation coefficients for the calibration curves are shown in Table 1(I).

On each non-consecutive day ( $p = 3$ ), control samples at five different concentrations ( $k = 5$ ), namely 2, 5, 10, 30 and 60 nmol/mL HS (0.8, 2, 4, 12 and 24  $\mu\text{mol/mL}$  blood), were measured in triplicates ( $n = 3$ ). The concentrations of the control samples were calculated by using the calibration curve determined for each analysis day. As shown in Table 1(II), a satisfactory

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

linearity was obtained, with a slope of 1.05 and a regression coefficient of 0.99 in the range of 2 to 60 nmol/mL HS (0.8-24  $\mu$ mol/mL blood).

Selectivity of the AGS-GC-MS method was previously confirmed in the work by Oliverio *et al.*, hence was not repeated in this study [22].

Trueness was found to be lower than the acceptance criteria (within  $\pm 20\%$  of the accepted reference value and within 20% at the LOQ), as is shown in table **1(III)**, which is satisfactory for [CO determination validation according to SFSTP guidelines \[61\]](#).

Table **1(IV)** shows that the relative standard deviation (RSD) for repeatability and intermediate precision are in a range between 0.50% and 3.55%.

Figure **1** represents the accuracy profile for CO. The mean bias (%) confidence interval limits for the control samples were within the acceptability limits of  $\pm 30\%$ . Taking into consideration the acceptability limits of  $\pm 30\%$ , the limit of quantification within validation criteria was found between 2 and 5 nmol/mL HS (0,8 and 2  $\mu$ mol/mL blood). Thus, the method is confirmed to be accurate within the range of 5 and 60 nmol/mL HS (2-24  $\mu$ mol/mL blood) according to the  $\beta$ -interval tolerance accuracy profile.

In addition, the external controls gave an excellent accuracy, with an RSD below 15% (Table **1(V)**).

### 3.2 Analyses of flushed samples

Blood samples of 13 patients were analysed before and after exposure to CO as well as with and without a flushing step. Triplicates were acquired for analyses with CO-oximetry and AGS-GC-MS. Results of all analyses are found in Table **2** and represented in Figure **2**.

For all samples analysed, a relative increase of both TBCO and COHb can be observed when comparing the values before and after CO exposure (Figure **2** and Table **2**). Increases were confirmed and found to be significant by comparing the means with Student t-Test (Table **3**).

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Important observations can be made when comparing the COHb and TBCO levels before and after a flushing step (Table 2 and 3). For the levels of COHb there is no consistent trend that can be observed, with a COHb increase in some patients and a decrease in others. The 25<sup>th</sup> and 75<sup>th</sup> interquartile range (Table 3) for COHb before and after flushing (range includes 0) as well as the results of the t-Test (p-Value > 0.05) confirm this result. This behavior could be explained by the known analytical variability of CO-oximeters at such low COHb saturations [63, 64].

Conversely, TBCO shows a consistent trend: for all samples analysed, TBCO before flushing is higher than after flushing. Statistical significance was confirmed by performing a paired Student t-Test of the means (p-Value = 8.955e-06). Mean and interquartile range for TBCO differences before and after flushing additionally confirm the positive relationship (Table 3).

#### 4. Discussion

An improved AGS-GC-MS method for CO determination in blood was validated for a clinical concentration range (1.63-104 nmol/mL HS / 0.65-41.6  $\mu$ mol/mL blood) and was successfully applied to the analysis of blood samples coming from individuals with controlled CO exposures. The observed increase of both COHb and TBCO before and after CO exposure was to be expected, since all individuals were breathing in a mixture of O<sub>2</sub> and CO. Patients with a CO burden before exposure, namely patients with ID number 3, 4, 9, 11, 12 and 13, admitted to be smokers. Smokers are known to have a higher baseline CO level, which varies depending on the frequency [65-67], hence it explains the presence of CO in several patients before exposure.

A significant variability of CO burden after exposure is found between individuals. Even though the volumes of CO administered were adapted to the weight and height of the patients, other factors involving the respiratory system and blood circulation, such as ventilation rate, tidal volume, inspiratory and expiratory reserve volume, alveolar ventilation, cardiac rhythm and cardiac output, influence the net amount of CO that enters the circulation [68]. In addition, malfunctioning of the rebreathing system can lead to altered amounts of CO effectively being administered, resulting in the observed inter-patient variations.



1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

The samples were all subject to the same storage and sample treatment conditions (immediately after blood collection) and analysed with the same parameters and measurement method (within 48 hours after blood samplings). It is therefore not very likely that the differences in detected concentrations are due to any error in the measurement technique or used parameters, but mainly to the removal of CO through a constant nitrogen stream. This legitimizes the hypothesis that there is a significant amount of CO present in free form in blood from an individual, who was subject to CO exposure. The amount of free CO on average ranges between 10 and 60% compared to the initial TBCO burden.

Additionally, when plotting the results of the 13 clinical samples with the results obtained from *in vitro* CO-fortified samples (Figure 3), it can be seen that the clinical samples all comply with the *in vitro* measurements, further diminishing the probability of errors in the measurement and strengthening the assumption of CO being eliminated through flushing. This suggests that with the execution of a flushing step a significant amount of CO is removed from the analysed sample. Thus, the result is biased not only from an analytical, but also from a clinical point of view: the excess amount of CO may have a more significant pathophysiological activity than previously suspected. The direct cellular toxicity of molecular CO through impairment of cellular respiration and generation of free radicals, which are known to be tumor-cells promoters, was reported in previous studies [28, 30-35]. Yet, the importance given to its implications in the direct adverse effects in CO poisonings was held to a minimum. Most likely this was because the presence of CO dissolved in blood in free form was never clearly demonstrated before.

Furthermore, the acknowledgment of dissolved CO represents one possible argument for explaining the discrepancy between reported symptoms and measured COHb. Considering only the amount of CO bound to Hb when determining a CO poisoning may lead to underestimation of the true burden CO poses, explaining why in many cases the measurements are inconsistent with the symptoms a patient is showing and also why several patients show symptoms with a certain time-delay. The amount of CO that is dissolved and not bound to Hb may be the missing quantity that gets closer to the true CO concentration in blood and burden on the body of an exposed individual. CO toxicity at cellular level may not only explain some of the symptoms of acute CO poisonings, but, due to the slow dissociation rate from cellular proteins, it may also

1  
2  
3  
4  
5  
6  
7  
8 elucidate the reasons behind the delayed neurological effects reported hours or days after COHb  
9 was removed from the system through oxygen therapy and after low level chronic exposures.  
10  
11  
12

## 13 14 **5. Limitations** 15 16 17

18 This study constitutes a preliminary study that aims to demonstrate the existence of CO dissolved  
19 not bound to Hb. This hypothesis has been tested with a cohort of 13 individuals through bedside  
20 blood collection. However, these findings have to be verified on a higher number of volunteers,  
21 even if the experimental design is complex to perform due to time-dependent analysis.  
22 Moreover, there is no clear evidence about a constant amount of CO dissolved, since in each  
23 patient the difference between TBCO before and after flushing varies. These variations are most  
24 likely due to interindividual variability: several factors such as pre-existing cardiovascular or  
25 respiratory conditions, metabolic rate, ventilation rate and volumes, sex and age can play a role  
26 in the behavior and amount of CO in blood. Additional measurements with more individuals will  
27 lead to higher statistical significance and will reduce the interindividual variability. In addition,  
28 analytical parameters affecting the storage as well as biological phenomena taking place after  
29 sampling of blood are known to potentially alter the measurement results, even if we reduced  
30 them to a minimum in this study. Further investigations into these TBCO pharmacodynamics and  
31 pharmacokinetics are needed to account for this behavior.  
32  
33  
34  
35  
36  
37  
38  
39

## 40 **6. Conclusion** 41 42 43

44 This study presents the validation of an improved carbon monoxide analysis method in human  
45 blood, based on AGS-GC-MS, for a range of 1.63 to 104 nmol/mL HS (0.65-41.6  $\mu\text{mol/mL}$   
46 blood), which is applicable to clinical CO exposure cases. The method was applied to a cohort of  
47 13 patients, who were exposed to controlled amounts of CO, and results compared to  
48 measurements by CO-oximetry. Furthermore, a flushing step was performed on samples after  
49 CO administration. Results seem to support the hypothesis that TBCO may be an alternative to  
50  
51

COHb as biomarker for determination of CO poisoning, since consideration of only CO bound to Hb may underestimate the total burden of CO in blood. By comparing flushed and unflushed samples, it was determined that there is a significant amount of CO present in blood in free form (10-60%) at the sampling time post-exposure.

This represents an important finding for the understanding of the true role played by CO in poisoning cases and for the explanation of the discrepancy often encountered by clinicians between symptoms and results and the onset of delayed neurological sequelae, even after complete removal of COHb from the system after normo- or hyperbaric oxygen therapy, possibly leading to a decrease in the number of misdiagnoses. Nevertheless, before application of the method in clinical settings, this hypothesis needs to be verified by more numerous cohorts and in-depth statistical analyses, to increase statistical power. Additionally, further investigation into the biochemical mechanisms behind the distribution and behavior of dissolved CO in human blood is required.

### **Funding**

This research received funding from the Gas Safety Trust, a UK-based grant giving charity.

### **Acknowledgments**

The authors are grateful to Dr Ariana Zeka from Brunel University London for providing assistance in reviewing the manuscript and Dr Giovanni Leonardi from Public Health England for fruitful discussion on the topic as part of a collaborative project on carbon monoxide measurement error.

The authors would also like to thank Dr Carsten Lundby from the University of Copenhagen and Dr Paul Robach from the National School of Skiing and Mountaineering (ENSA) for their

precious help in controlled CO-delivery, and Dr Belen Ponte and Dr Sophie de Seigneux from the Department of Nephrology of the University Hospital of Geneva (HUG) for their kind hospitality and for granting us access to their study samples.

### Conflict of interest

The authors declare no conflict of interest.

### References

1. Vreman, H., Wong, R., Stevenson, D., Smialek, J., Fowler, D. and Li, L. et al. (2006) Concentration of Carbon Monoxide (CO) in Postmortem Human Tissues: Effect of Environmental CO Exposure. *Journal of Forensic Sciences*, 51, 1182-1190.
2. Fazlzadeh, M., Rostami, R., Hazrati, S. and Rastgu, A. (2015) Concentrations of carbon monoxide in indoor and outdoor air of Ghalyun cafes. *Atmospheric Pollution Research*, 6, 550-555.
3. Penney, D. (2008) Carbon monoxide poisoning. CRC Press, Boca Raton, FL.
4. Bleecker, M. (2015) Carbon monoxide intoxication. *Handbook of Clinical Neurology*, 131, 191-203.
5. WHO guidelines for indoor air quality (2009) WHO Regional Office for Europe, Copenhagen.
6. Gara, E. (2017) Carbon Monoxide Intoxication: Experiences from Hungary. In Poisoning - From Specific Toxic Agents to Novel Rapid and Simplified Techniques for Analysis. <https://www.intechopen.com/books/poisoning-from-specific-toxic-agents-to-novel-rapid-and-simplified-techniques-for-analysis/carbon-monoxide-intoxication-experiences-from-hungary> (7 June 2018).
7. Braubach, M., Algoet, A., Beaton, M., Lauriou, S., Héroux, M. and Krzyzanowski, M. (2012) Mortality associated with exposure to carbon monoxide in WHO European Member States. *Indoor Air*, 23, 115-125.

Formatted: No bullets or numbering

- 1  
2  
3  
4  
5  
6  
7  
8  
9  
10 | ~~7-8.~~ Sedda, A. and Rossi, G. (2006) Death scene evaluation in a case of fatal accidental  
11 carbon monoxide toxicity. *Forensic Science International*, 164, 164-167.
- 12 | ~~8-9.~~ Carbon Monoxide-Related Deaths—United States, 1999-2004 (2007) *Morbidity and*  
13 *mortality weekly report*, 57, 1309-1312.
- 14  
15 | ~~9-10.~~ Salameh, S., Amitai, Y., Antopolsky, M., Rott, D. and Stalnicowicz, R. (2009) Carbon  
16 monoxide poisoning in Jerusalem: epidemiology and risk factors. *Clinical Toxicology*, 47,  
17 137-141.
- 18  
19 | ~~10-11.~~ Nielsen, P., Gheorghe, A. and Lynnerup, N. (2014) Forensic aspects of carbon monoxide  
20 poisoning by charcoal burning in Denmark, 2008–2012: an autopsy based study. *Forensic*  
21 *Science, Medicine, and Pathology*, 10, 390-394.
- 22  
23 | ~~11-12.~~ Fisher, D., Leonardi, G. and Flanagan, R. (2014) Fatal unintentional non-fire-related  
24 carbon monoxide poisoning: England and Wales, 1979–2012. *Clinical Toxicology*, 52, 166-  
25 170.
- 26  
27  
28 | ~~12-13.~~ Sircar, K., Clower, J., Shin, M., Bailey, C., King, M. and Yip, F. (2015) Carbon  
29 monoxide poisoning deaths in the United States, 1999 to 2012. *The American Journal of*  
30 *Emergency Medicine*, 33, 1140-1145.
- 31  
32 | ~~13-14.~~ Ghosh, R., Close, R., McCann, L., Crabbe, H., Garwood, K. and Hansell, A. et al. (2015)  
33 Analysis of hospital admissions due to accidental non-fire-related carbon monoxide  
34 poisoning in England, between 2001 and 2010. *Journal of Public Health*, 38, 76-83.
- 35  
36  
37 | ~~14-15.~~ Janík, M., Ublová, M., Kučerová, Š. and Hejna, P. (2017) Carbon monoxide-related  
38 fatalities: A 60-year single institution experience. *Journal of Forensic and Legal Medicine*,  
39 48, 23-29.
- 40  
41 | ~~15-16.~~ Dueñas-Laita, A., Ruiz-Mambrilla, M., Gandía, F., Cerdá, R., Martín-Escudero, J. and  
42 Pérez-Castrillón, J. et al. (2001) Epidemiology of Acute Carbon Monoxide Poisoning in a  
43 Spanish Region. *Journal of Toxicology: Clinical Toxicology*, 39, 53-57.
- 44  
45  
46 | ~~16-17.~~ Rose, J., Wang, L., Xu, Q., McTiernan, C., Shiva, S. and Tejero, J. et al. (2017) Carbon  
47 Monoxide Poisoning: Pathogenesis, Management, and Future Directions of  
48 Therapy. *American Journal of Respiratory and Critical Care Medicine*, 195, 596-606.
- 49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

- 1  
2  
3  
4  
5  
6  
7  
8  
9 | ~~17-18.~~ Prockop, L. and Chichkova, R. (2007) Carbon monoxide intoxication: An updated  
10 review. *Journal of the Neurological Sciences*, 262, 122-130.
- 11  
12 | ~~18-19.~~ Harper, A. and Croft-Baker, J. (2004) Carbon monoxide poisoning: undetected by both  
13 patients and their doctors. *Age and Ageing*, 33, 105-109.
- 14  
15  
16 | ~~19-20.~~ Youakim, S. (2017) Carbon monoxide toxicity. *British Columbia Medical Journal*, 59,  
17 465.
- 18  
19 | ~~20-21.~~ Raub, J., Mathieu-Nolf, M., Hampson, N. and Thom, S. (2000) Carbon monoxide  
20 poisoning — a public health perspective. *Toxicology*, 145, 1-14.
- 21  
22  
23 | ~~21-22.~~ Chiew, A. and Buckley, N. (2014) Carbon monoxide poisoning in the 21st  
24 century. *Critical Care*, 18, 221.
- 25  
26 | ~~22-23.~~ Oliverio, S. and Varlet, V. (2018) Carbon monoxide analysis method in human blood by  
27 Airtight Gas Syringe – Gas Chromatography – Mass Spectrometry (AGS-GC-MS):  
28 Relevance for postmortem poisoning diagnosis. *Journal of Chromatography B*, 1090, 81-89.
- 29  
30  
31 | ~~23-24.~~ Case, D., Huynh, B. and Karplus, M. (1979) Binding of oxygen and carbon monoxide to  
32 hemoglobin. An analysis of the ground and excited states. *Journal of the American Chemical*  
33 *Society*, 101, 4433-4453.
- 34  
35 | ~~24-25.~~ Eaton, W., Henry, E., Hofrichter, J. and Mozzarelli, A. (2006) Is cooperative oxygen  
36 binding by hemoglobin really understood?. *Rendiconti Lincei*, 17, 147-162.
- 37  
38  
39 | ~~25-26.~~ Townsend, C. and Maynard, R. (2002) Effects on health of prolonged exposure to low  
40 concentrations of carbon monoxide. *Occupational and Environmental Medicine*, 59, 708-  
41 711.
- 42  
43 | ~~26-27.~~ Ouahmane, Y., Mounach, J., Satte, A., Bourazza, A., Soulaymani, A. and Elomari, N.  
44 (2018) Severe poisoning with carbon monoxide (CO) with neurological impairment, study of  
45 19 cases. *Toxicologie Analytique et Clinique*, 30, 50-60.
- 46  
47  
48 | ~~27-28.~~ Hardy, K. and Thom, S. (1994) Pathophysiology and Treatment of Carbon Monoxide  
49 Poisoning. *Journal of Toxicology: Clinical Toxicology*, 32, 613-629.
- 50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

- 1  
2  
3  
4  
5  
6  
7  
8 | ~~28-29~~. Kao, L. and Nañagas, K. (2005) Carbon Monoxide Poisoning. *Medical Clinics of North*  
9 *America*, 89, 1161-1194.  
10  
11  
12 | ~~29-30~~. Olson, K. (1984) Carbon monoxide poisoning: Mechanisms, presentation, and  
13 controversies in management. *The Journal of Emergency Medicine*, 1, 233-243.  
14  
15  
16 | ~~30-31~~. Hill, B. (1994) The pathway of CO binding to cytochromecoxidase Can the gateway be  
17 closed?. *FEBS Letters*, 354, 284-288.  
18  
19 | ~~31-32~~. Chance, B., Erecinska, M. and Wagner, M. (1970) MITOCHONDRIAL RESPONSES  
20 TO CARBON MONOXIDE TOXICITY. *Annals of the New York Academy of Sciences*, 174,  
21 193-204.  
22  
23  
24 | ~~32-33~~. Zhang, J. and Piantadosi, C. (1992) Mitochondrial oxidative stress after carbon monoxide  
25 hypoxia in the rat brain. *Journal of Clinical Investigation*, 90, 1193-1199.  
26  
27 | ~~33-34~~. Verma, A., Hirsch, D., Glatt, C., Ronnett, G. and Snyder, S. (1993) Carbon monoxide: a  
28 putative neural messenger. *Science*, 259, 381-384.  
29  
30  
31 | ~~34-35~~. Barinaga, M. (1993) Carbon monoxide: killer to brain messenger in one step. *Science*,  
32 259, 309-309.  
33  
34 | ~~35-36~~. Ramieri, A., Jatlow, P. and Seligson, D. (1984) New method for rapid determination of  
35 carboxyhemoglobin by use of double-wavelength spectrophotometry. *Journal of Analytical*  
36 *Toxicology*, 8, 277-281.  
37  
38  
39 | ~~36-37~~. Fukui, Y., Matsubara, M., Takahashi, S. and Matsubara, K. (1984) A Study of Derivative  
40 Spectrophotometry for the Determination of Carboxyhemoglobin in Blood. *Journal of*  
41 *Analytical Toxicology*, 8, 277-281.  
42  
43  
44 | ~~37-38~~. Vreman, H., Stevenson, D. and Zwart, A. (1987) Analysis for carboxyhemoglobin by gas  
45 chromatography and multicomponent spectrophotometry compared. *Clinical chemistry*, 33,  
46 694-697.  
47  
48 | ~~38-39~~. Boumba, V. and Vougiouklakis, T. (2005) Evaluation of the Methods Used for  
49 Carboxyhemoglobin Analysis in Postmortem Blood. *International Journal of Toxicology*, 24,  
50 275-281.  
51

- 1  
2  
3  
4  
5  
6  
7  
8 | ~~39-40.~~ Luchini, P., Leyton, J., Strombeck, M., Ponce, J., Jesus, M. and Leyton, V. (2009)  
9 Validation of a Spectrophotometric Method for Quantification of  
10 Carboxyhemoglobin. *Journal of Analytical Toxicology*, 33, 540-544.  
11  
12  
13 | ~~40-41.~~ Droghetti, E., Bartolucci, G., Focardi, C., Bambagiotti-Alberti, M., Nocentini, M. and  
14 Smulevich, G. (2011) Development and validation of a quantitative spectrophotometric  
15 method to detect the amount of carbon monoxide in treated tuna fish. *Food Chemistry*, 128,  
16 1143-1151.  
17  
18 | ~~41-42.~~ Oritani, S., Zhu, B., Ishida, K., Shimotouge, K., Quan, L. and Fujita, M. et al. (2000)  
19 Automated determination of carboxyhemoglobin contents in autopsy materials using head-  
20 space gas chromatography/mass spectrometry. *Forensic Science International*, 113, 375-379.  
21  
22  
23 | ~~42-43.~~ Bartolucci, G., Droghetti, E., Focardi, C., Bambagiotti-Alberti, M., Nocentini, M. and  
24 Smulevich, G. (2010) High throughput headspace GC-MS quantitative method to measure  
25 the amount of carbon monoxide in treated tuna fish. *Journal of Mass Spectrometry*, 45, 1041-  
26 1045.  
27  
28 | ~~43-44.~~ Varlet, V., Lagroy De Croutte, E., Augsburg, M. and Mangin, P. (2012) Accuracy  
29 profile validation of a new method for carbon monoxide measurement in the human blood  
30 using headspace-gas chromatography–mass spectrometry (HS-GC–MS). *Journal of*  
31 *Chromatography B*, 880, 125-131.  
32  
33  
34 | ~~44-45.~~ Hao, H., Zhou, H., Liu, X., Zhang, Z. and Yu, Z. (2013) An accurate method for  
35 microanalysis of carbon monoxide in putrid postmortem blood by head-space gas  
36 chromatography–mass spectrometry (HS/GC/MS). *Forensic Science International*, 229, 116-  
37 121.  
38  
39 | ~~45-46.~~ Varlet, V., De Croutte, E., Augsburg, M. and Mangin, P. (2013) A New Approach for  
40 the Carbon Monoxide (CO) Exposure Diagnosis: Measurement of Total CO in Human Blood  
41 Versus Carboxyhemoglobin (HbCO). *Journal of Forensic Sciences*, 58, 1041-1046.  
42  
43  
44 | ~~46-47.~~ Vreman, H., Kwong, L. and Stevenson, D. (1984) Carbon monoxide in blood: an  
45 improved microliter blood-sample collection system. *Clinical Chemistry*, 30, 1382-1386.  
46  
47 | ~~47-48.~~ Vreman, H., Wong, R., Kadotani, T. and Stevenson, D. (2005) Determination of carbon  
48 monoxide (CO) in rodent tissue: Effect of heme administration and environmental CO  
49 exposure. *Analytical Biochemistry*, 341, 280-289.  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60



- 1  
2  
3  
4  
5  
6  
7  
8  
9 | ~~48-49.~~ Cardeal, Z., Pradeau, D., Hamon, M., Abdoulaye, I., Pailler, F. and Lejeune, B. (1993)  
10 | New Calibration Method for Gas Chromatographic Assay of Carbon Monoxide in  
11 | Blood. *Journal of Analytical Toxicology*, 17, 193-195.
- 12  
13 | ~~49-50.~~ Rodkey, F. and Collison, H. (1970) An artifact in the analysis of oxygenated blood for its  
14 | low carbon monoxide content. *Clinical Chemistry*, 16, 896-899.
- 15  
16 | ~~50-51.~~ Widdop, B. (2002) Analysis of carbon monoxide. *Annals of Clinical Biochemistry*, 39,  
17 | 378-391.
- 18  
19  
20 | ~~51-52.~~ Gore, C., Hopkins, W. and Burge, C. (2005) Errors of measurement for blood volume  
21 | parameters: a meta-analysis. *Journal of Applied Physiology*, 99, 1745-1758.
- 22  
23 | ~~52-53.~~ Popovic, V., Atanasijevic, T., Nikolic, S. and Micic, J. (2009) Concentration of carbon-  
24 | monoxide in carbonized bodies – Forensic aspects. *Legal Medicine*, 11, S318-S320.
- 25  
26 | ~~53-54.~~ Ayres, S., Criscitiello, A. and Giannelli, S. (1966) Determination of blood carbon  
27 | monoxide content by gas chromatography. *Journal of Applied Physiology*, 21, 1368-1370.
- 28  
29 | ~~54-55.~~ Collison, H., Rodkey, F. and O'Neal, J. (1968) Determination of carbon monoxide in  
30 | blood by gas chromatography. *Clinical Chemistry*, 14, 162-171.
- 31  
32 | ~~55-56.~~ Guillot, J., Weber, J. and Savoie, J. (1981) Quantitative Determination of Carbon  
33 | Monoxide in Blood by Head-Space Gas Chromatography. *Journal of Analytical Toxicology*,  
34 | 5, 264-266.
- 35  
36 | ~~56-57.~~ Levine, B., Green, D., Saki, S., Symons, A. and Smialek, J. (1997) Evaluation of the IL-  
37 | 682 Co-Oximeter; Comparison to the IL-482 Co-Oximeter and Gas  
38 | Chromatography. *Canadian Society of Forensic Science Journal*, 30, 75-78.
- 39  
40 | ~~57-58.~~ Walch, S., Lachenmeier, D., Sohnius, E., Madea, B. and Musshoff, F. (2010) Rapid  
41 | determination of carboxyhemoglobin in postmortem blood using fully-automated headspace  
42 | gas chromatography with methaniser and FID. *The Open Toxicology Journal*, 4, 21-25.
- 43  
44  
45  
46  
47  
48 | 59. (2007) Avoximeter 4000 Operator's Manual (ITC)—2007 Version. International Technidyne  
49 | Corporation. [www.accriva.com/uploads/literature/ap4001--1007.pdf](http://www.accriva.com/uploads/literature/ap4001--1007.pdf) (accessed August 20,  
50 | 2018).

Formatted: Pattern: Clear

Formatted: List Paragraph, No bullets or numbering

60. Shepherd, A. P. and Steinke, J. M. (2006). Method and apparatus for direct spectrophotometric measurement in unaltered whole blood. US patent 0.203.225 A1.
61. Hubert, P., Nguyen-Huu, J. J., Boulanger, B., Chapuzet, E., Cohen, N., Compagnon, P. A., ... et al., (2008). Harmonization of strategies for the validation of quantitative analytical procedures: A SFSTP proposal: Part IV. Examples of application. *Journal of pharmaceutical and biomedical analysis*, 48, 760-771.
62. Siebenmann, C., Keiser, S., Robach, P., and Lundby, C. (2017). CORP: The assessment of total hemoglobin mass by carbon monoxide rebreathing. *Journal of Applied Physiology*, 123, 645-654.
63. Brehmer, C. and Iten, P. X. (2003). Rapid determination of carboxyhemoglobin in blood by Oximeter. *Forensic Science International*, 133, 179-181.
64. Mahoney, J. J., Vreman, H. J., Stevenson, D. K. and Van Kessel, A. L. (1993). Measurement of carboxyhemoglobin and total hemoglobin by five specialized spectrophotometers (CO-oximeters) in comparison with reference methods. *Clinical Chemistry*, 39, 1693-1700.
- ~~58-65.~~ Czogala, J. and Goniewicz, M. (2005) The Complex Analytical Method for Assessment of Passive Smokers' Exposure to Carbon Monoxide. *Journal of Analytical Toxicology*, 29, 830-834.
- ~~59-66.~~ Schimmel, J., George, N., Schwarz, J., Yousif, S., Suner, S. and Hack, J. (2017) Carboxyhemoglobin Levels Induced by Cigarette Smoking Outdoors in Smokers. *Journal of Medical Toxicology*, 14, 68-73.
- ~~60-67.~~ Stewart, R. and Baretta, M. (1974) Carboxyhemoglobin levels in American blood donors. *JAMA: The Journal of the American Medical Association*, 229, 1187-1195.
- ~~64-68.~~ Weaver, L. (2009) Carbon Monoxide Poisoning. *New England Journal of Medicine*, 360, 1217-1225.

Formatted: English (U.S.)

Formatted: List Paragraph, No bullets or numbering

Formatted: English (U.S.)

Formatted: Font: Italic, English (U.S.)

Formatted: English (U.S.)

Formatted: Font: Italic, English (U.S.)

Formatted: English (U.S.)

Formatted: Pattern: Clear

Formatted: List Paragraph, No bullets or numbering

Formatted: English (U.S.)

Formatted: German (Germany)

Formatted: Font: Italic

Formatted: English (U.S.), Pattern: Clear

Formatted: List Paragraph, No bullets or numbering

Formatted: English (U.S.)

Formatted: Font: Italic

Formatted: Font: Italic

Formatted: Pattern: Clear

Formatted: List Paragraph, No bullets or numbering

Formatted: Font: Italic

Formatted: Pattern: Clear

Formatted: List Paragraph, No bullets or numbering

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

### Legends for figures

**Figure 1:** Accuracy profile for CO determination using a simple linear regression model within the range of 2-60 nmol/mL HS (0.8-24  $\mu\text{mol/mL}$  blood). The continuous line represents the trueness (bias), the dashed lines represent the acceptance limits set at  $\pm 30\%$  and the dotted lines are the relative lower and upper accuracy limits

**Figure 2:** Results for the total CO concentration in blood (TBCO) in  $\mu\text{mol/mL}$  (bars, left axis) measured by AGS-GC-MS and the COHb saturation in % (dots, right axis) measured through CO-oximetry in blood for 13 patients before (green) and after (blue) CO exposure and after a flushing step (orange).

**Figure 3:** Correlation plot between TBCO in  $\mu\text{mol/mL}$  measured by AGS-GC-MS vs. the COHb saturation in % measured through CO-oximetry for two groups of samples: stored blood samples fortified with CO (squares for high fortification level 60-70%, lines for medium fortification level 30-40% and triangles for low fortification level 10-20%,  $n=54$ ) and real case samples (circles for flushed and diamonds for not flushed samples,  $n=26$ ).

Figure 1

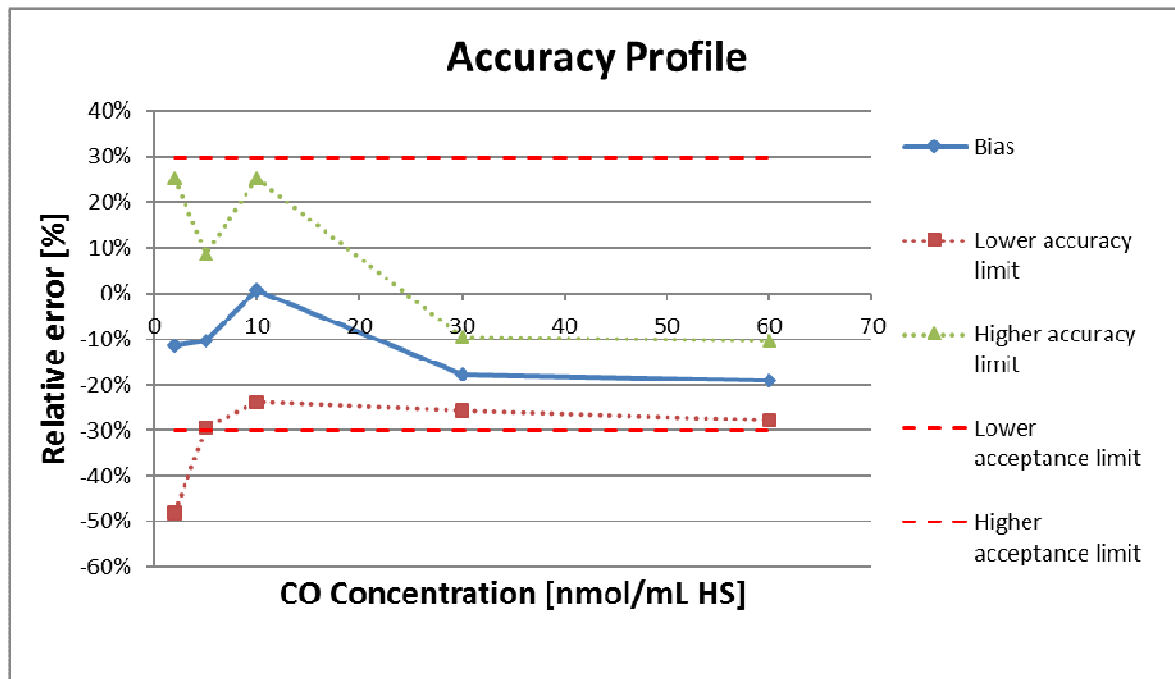


Figure 2

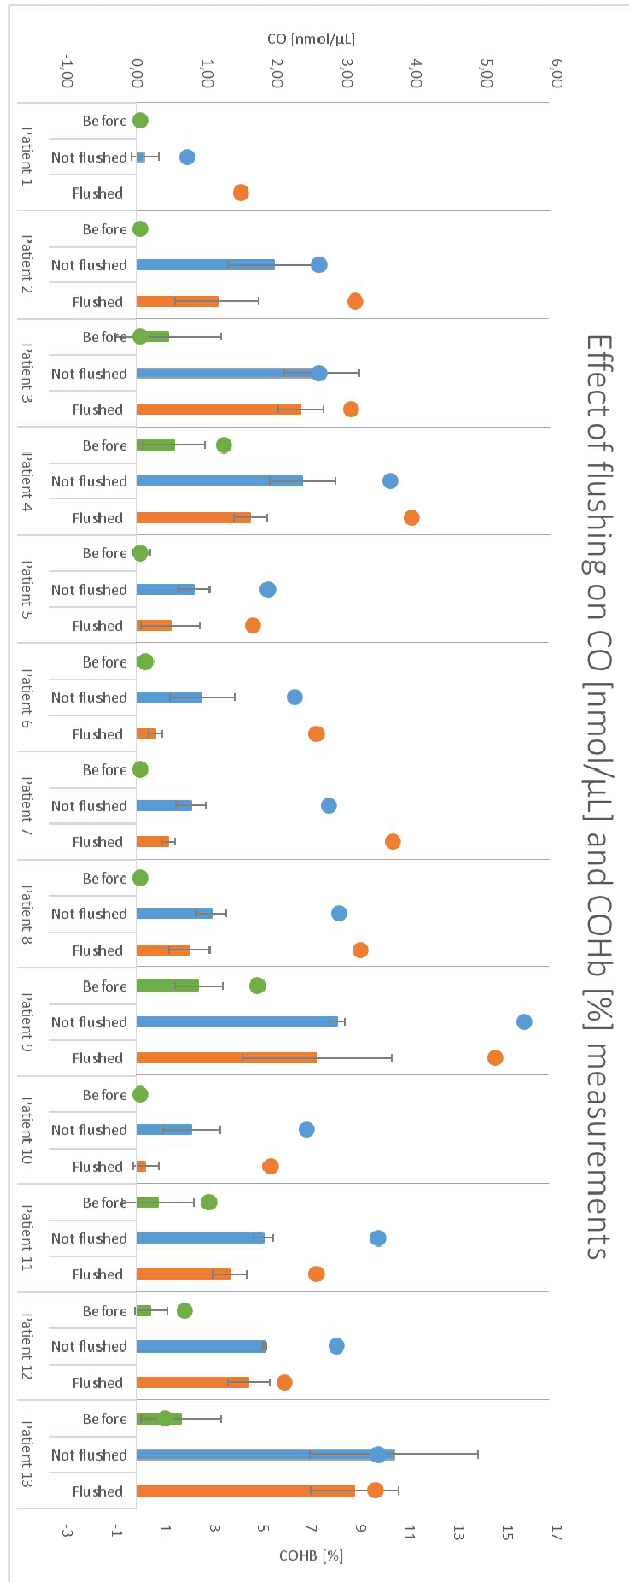
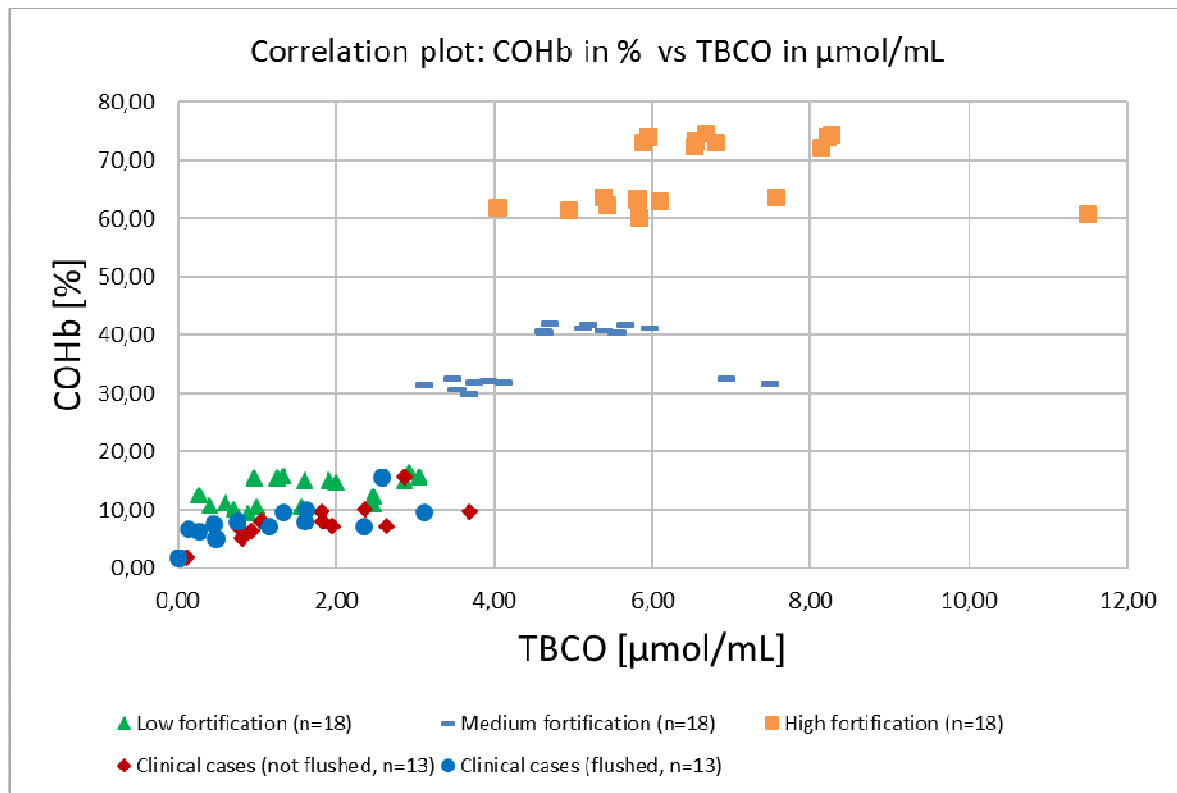


Figure 3



**Table 1:** Validation results for CO determination in blood by AGS-GC-MS – (I) represents the mean coefficients of the calibration functions obtained from analysis of the calibrators; (II) represents the coefficients of the linear regression function obtained from analysis of the QCs against their theoretical value; (III) represents the trueness obtained from the QC analyses expressed in %; (IV) represents the precision obtained from QC analyses expressed in relative standard deviation % (RSD%); (V) shows mean and RSD% of the external controls.

<b>(I) Response function [1.63-104 nmol/mL HS] (<math>k = 7, n = 3, p = 3</math>)</b>			
	<b>Day 1</b>	<b>Day 2</b>	<b>Day 3</b>
<b>Slope</b>	0.03	0.02	0.03
<b>Intercept</b>	0.59	0.63	0.61
<b>r<sup>2</sup></b>	0.98	0.99	0.98

$k$ : number of concentration levels;  $n$ : number of repetitions for each level;  $p$ : number of non-consecutive days

<b>(II) Linearity [2-60 nmol/mL HS] (<math>k = 5, n = 3, p = 3</math>)</b>	
<b>Slope</b>	1.05
<b>Intercept</b>	-0.48
<b>r<sup>2</sup></b>	0.99

<b>(III) Trueness (relative bias) (<math>k = 5, n = 3, p = 3</math>)</b>	
<b>Levels [nmol/mL HS]</b>	<b>Trueness (%)</b>
<b>2.0</b>	-11
<b>5.0</b>	-10
<b>10</b>	1
<b>30</b>	-18
<b>60</b>	-19

<b>(IV) Precision (RSD%) (<math>k = 5, n = 3, p = 3</math>)</b>	
<b>Levels [nmol/mL HS]</b>	<b>Repeatability and Intermediate Precision*</b>
<b>2.0</b>	0.5
<b>5.0</b>	0.6
<b>10</b>	1.7
<b>30</b>	1.6
<b>60</b>	3.6

\*Inter-series variance ( $s^2_g$ ) is negligible for all levels, resulting in same values for repeatability and intermediate precision

<b>(V) External controls (<math>k = 2, n = 3, p = 1</math>)</b>		
<b>Levels [nmol/mL HS]</b>	<b>Mean (Confidence Interval)</b>	<b>RSD [%]</b>
<b>5</b>	4.49 (3.93, 5.06)	12.0
<b>60</b>	65.5 (60.0, 73.9)	6.57

**Table 2:** Differences in measurement results for COHb [%] and TBCO [ $\mu\text{mol/mL}$ ] for before and after CO exposure and before and after flushing; for each individual, sex and volume of CO administered are provided.

Patient ID	Sex	Volume CO [mL]	COHb [%]		TBCO [ $\mu\text{mol/mL}$ ]	
			Difference After-Before CO exposure	Difference Not flushed-flushed	Difference After-Before CO exposure	Difference Not flushed-flushed
1	M	84.3	1.90	-2.20	0.11	0.11
2	M	89.0	7.30	-1.50	1.95	0.81
3	F	87.9	7.30	-1.30	2.20	0.30
4	M	59.3	6.80	-0.90	1.84	0.75
5	F	48.3	5.20	0.60	0.75	0.34
6	M	104	6.10	-0.90	0.93	0.67
7	M	86.7	7.70	-2.60	0.74	0.33
8	M	89.1	8.10	-0.90	1.06	0.31
9	F	71.2	10.90	1.20	1.99	0.30
10	M	57.4	6.80	1.50	0.78	0.66
11	F	99.5	6.90	2.50	1.51	0.49
12	M	60.8	6.20	2.10	1.63	0.23
13	M	65.3	8.70	0.10	3.05	0.57



**Table 3:** Summary statistics and results of paired t-Test with 95% confidence interval (CI) for the differences for COHb and TBCO before (B) and after (A) exposure and before (NF) and after flushing (F); p-Values in **bold** are significant (below 0.05).

	COHb Diff A/B [%]	COHb Diff NF/F [%]	TBCO Diff A/B [ $\mu\text{mol/mL}$ ]	TBCO Diff NF/F [ $\mu\text{mol/mL}$ ]
<b>Mean</b>	6.92	-0.18	1.43	0.45
<b>SD</b>	2.06	1.64	0.79	0.22
<b>1st Quartile</b>	6.20	-1.30	0.78	0.30
<b>3rd Quartile</b>	7.70	1.20	1.95	0.66
<b>p-Value</b>	<b>6.02*e-07</b>	0.71	<b>2.93*e-05</b>	<b>8.96*e-06</b>
<b>95% CI</b>	5.98; 9.53	-1.17; 0.81	0.95; 1.90	0.32; 0.58