



## University of Dundee

### VAMPIRE® fundus image analysis algorithms

Cirla, Alessandro; Drigo, Michele; Ballerini, Lucia; Trucco, Emanuele; Barsotti, Giovanni

*Published in:*  
Veterinary Ophthalmology

*DOI:*  
[10.1111/vop.12657](https://doi.org/10.1111/vop.12657)

*Publication date:*  
2019

*Document Version*  
Peer reviewed version

[Link to publication in Discovery Research Portal](#)

*Citation for published version (APA):*

Cirla, A., Drigo, M., Ballerini, L., Trucco, E., & Barsotti, G. (2019). VAMPIRE® fundus image analysis algorithms: Validation and diagnostic relevance in hypertensive cats. *Veterinary Ophthalmology*, 22(6), 819-827. <https://doi.org/10.1111/vop.12657>

#### General rights

Copyright and moral rights for the publications made accessible in Discovery Research Portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from Discovery Research Portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain.
- You may freely distribute the URL identifying the publication in the public portal.

#### Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

1  
2  
3 1 **VAMPIRE® fundus image analysis algorithms: validation and diagnostic relevance in**  
4  
5 2 **hypertensive cats**  
6  
7  
8 3

9  
10 4 Alessandro Cirila,<sup>\*,†</sup>DVM, PhD Michele Drigo,<sup>‡</sup> DVM, PhD Lucia Ballerini,<sup>§</sup> PhD Emanuele  
11  
12 5 Trucco<sup>§</sup> PhD and Giovanni Barsotti<sup>†</sup> DVM, PhD  
13  
14 6

15  
16  
17 7 <sup>\*</sup>Department of Ophthalmology, San Marco Veterinary Clinic and Laboratory – Veggiano, PD,  
18  
19 8 Italy; <sup>†</sup>Department of Veterinary Science, University of Pisa – S. Piero a Grado, PI, Italy;  
20  
21 9 <sup>‡</sup>Department of Animal Medicine, Production and Health, University of Padova – Legnaro, PD,  
22  
23 10 Italy and <sup>§</sup> School of Computing, University of Dundee – Dundee, Scotland  
24  
25  
26 11

27  
28 12 The authors declare no financial interests with companies that manufacture products that are the  
29  
30 13 subject of the present research or with companies that manufacture competing products.  
31  
32  
33 14

34  
35 15 Corresponding author: Alessandro Cirila

36  
37 16 San Marco Veterinary Clinic and Laboratory

38  
39 17 Via dell'Industria 3, 35030 – Veggiano, PD, Italy

40  
41 18 Tel.: +39-049-856-1098

42  
43 19 Fax: +39-049-796-9254

44  
45 20 e-mail: [alessandro.cirila@sanmarcovet.it](mailto:alessandro.cirila@sanmarcovet.it)  
46  
47 21  
48  
49 22  
50  
51 23  
52  
53 24  
54  
55  
56 25  
57

58 25 This is the peer reviewed version of the following article: "VAMPIRE® fundus image analysis algorithms: Validation  
59 and diagnostic relevance in hypertensive cats", *Veterinary Ophthalmology* (2019) which has been published in final  
60 26 form at <https://doi.org/10.1111/vop.12657>. This article may be used for non-commercial purposes in accordance  
with Wiley Terms and Conditions for Self-Archiving.

## Abstract

**Objectives:** To validate a retinal imaging software named VAMPIRE® (Vascular Assay and Measurement Platform for Images of the Retina) in feline patients and test the clinical utility in hypertensive cats.

**Animals studied:** One hundred and five healthy cats were enrolled. They represented the normal dataset used in the validation (group 1). Forty-three hypertensive cats with no noticeable retinal abnormalities were enrolled for the clinical validity of the software (group 2).

**Procedures:** Eleven points (4 veins, 4 arteries and 3 arterial bifurcations) were measured for each digital image. Repeatability and reproducibility of measurements were assessed using two independent operators. Data were statistically analyzed by the Mann-Whiney and Tukey box-plot. Significance was considered when  $P < 0.05$ .

**Results:** Two hundred and ten retinal images were analyzed for a total of 2310 measurements. Total mean was 9.1 and 6.1 pixels for veins and arteries, respectively. First, second and third arteriolar bifurcations angles were  $73.6^\circ$ ,  $76.9^\circ$  and  $85.4^\circ$ , respectively. A comparison between groups 1 and 2 showed a statistically significant reduction in arteriolar diameter (mean 3.3 pixels) and branch angle ( $55^\circ$ ,  $47.8^\circ$  and  $59.9^\circ$ ) associated with increasing vein diameter (mean 24.15 pixels). **Conclusions:** Current image analysis techniques used in human medicine were investigated in terms of extending their use to veterinary medicine. The VAMPIRE® algorithm proved useful for an objective diagnosis of retinal vasculature changes secondary to systemic hypertension in cats, and could be an additional **diagnostic** test for feline systemic hypertension.

**Key Words:** cat, fundus, image analysis algorithms, software validation, retinal photography, systemic hypertension

## 53 INTRODUCTION

54 Arterial systemic hypertension is a clinical condition in which the blood pressure in the arteries is  
55 higher than its physiological values. Arterial hypertension is often correlated to systemic  
56 pathologies and is increasingly considered a cause of morbidity and, in some cases, death, both in  
57 humans and veterinary patients (1, 2, 3, 4, 5).

58 The eye, like the kidneys, heart and encephalon, is one of the target organs of the persistent  
59 hypertensive state. (6, 7, 8, 9, 10, 11, 12, 13, 14) At the ocular and particularly the retinal level,  
60 damage due to hypertension often causes sudden blindness although, at least in humans, this is  
61 increasingly less frequent thanks to early diagnosis of the disease. (12, 13, 14, 15)

62 Systemic hypertension is commonly found in cats, and often causes secondary ocular lesions. (4, 6,  
63 8, 13, 16, 17, 18) Characteristic ocular lesions are the result of the rupture of the retinal endothelial  
64 barrier, and ischemia of the vascularisation of the choroid. The most common lesions associated with  
65 hypertension include intra/subretinal oedema, retinal hemorrhages and retinal detachment. (1, 2, 3, 4,  
66 6, 8, 11, 12, 13, 14, 16) The literature on the ocular manifestations of feline hypertension is based on  
67 information and data derived from clinical practice. (1, 3, 4, 8, 10, 17) Inevitably the disease is already  
68 in the advanced stages at the time of clinical presentation and diagnosis, and blindness is the most  
69 evident clinical sign.

70 The retina is an excellent window for studying microcirculation both in physiological and  
71 pathological conditions. Retinal vessels, which can easily be seen using non-invasive methods, also  
72 share similar physiological characteristics to encephalic and cardiac microcirculation. (4, 6, 8,  
73 12,16, 17) Therefore, recognizing the early signs of hypertensive retinopathy is key not only in  
74 order to preserve the anatomical and functional integrity of the eye but also to shed light on a  
75 complex system which affects other organs and vital systems.

76 Analysis of the retinal vascular structures provides a unique opportunity in that these are the only  
77 components of the entire circulatory system that can be observed in a non-invasive manner. The  
78 diagnosis of hypertensive retinopathy is qualitative and takes place via direct analysis of the fundus

1  
2  
3 79 using ophthalmoscopes (direct and indirect). However, this diagnosis is subjective and consequently  
4  
5 80 lacking in reliability. This kind of analysis is clinical, whereas a better solution is automatic or  
6  
7  
8 81 semiautomatic retinal image analysis. A fundus camera facilitates the collection of retinal images  
9  
10 82 which can then be analysed objectively. Photographing the fundus makes it possible to obtain high  
11  
12 83 resolution images of large retinal areas, including the microcirculation, and provides objective  
13  
14 84 documentation of the major retinal vessels and their bifurcations. (19) Defining an ideal instrument  
15  
16 85 (objective and non-invasive) for assessing retinal vessels in human medicine has long been linked  
17  
18 86 to using computer aided algorithms for measuring the properties of retinal vessels. (19, 20, 21, 22,  
19  
20 87 23, 24, 25, 26, 27, 28, 29) On the other hand, no such publications are available in recent veterinary  
21  
22 88 literature where the analysis of the retinal vasculature is typically still correlated to the subjectivity  
23  
24 89 of the observer.

25  
26  
27  
28 90 The aim of this study was to verify whether Vascular Assessment and Measurement Platform for  
29  
30 91 Images of the Retina software (VAMPIRE®) can be validated in veterinary medicine, and can help  
31  
32 92 in the early diagnosis of retinal vasculature changes due to systemic hypertension in cats.  
33  
34  
35  
36

## 37 94 **MATERIALS AND METHODS**

38  
39  
40 95 This research was approved by the Agency for Animal Welfare of Pisa University (22/16) and  
41  
42 96 developed with the coordination of the Department of Veterinary Science (Pisa University), in  
43  
44 97 cooperation with the School of Computing (Dundee University, Scotland) and the Department of  
45  
46 98 Animal Medicine, Productions and Health (Padua University). All the patients enrolled were  
47  
48 99 examined in the same clinic (San Marco Veterinary Clinic and Laboratory, Padua).  
49  
50

### 51 100 *Animal enrolment*

52  
53 101 One hundred and five clinically healthy cats (group 1) were enrolled for the validation of  
54  
55 102 VAMPIRE® during a one-year period **and** represented the normality dataset used for the validation.  
56  
57  
58 103 **Out of 159** hypertensive cats **that** underwent a complete ophthalmic examination, **43** cats with no  
59  
60 104 noticeable retinal abnormalities but clinically diagnosed with hypertension (group 2) were enrolled

1  
2  
3 105 for the assessment of the software potential clinical applications. **Overall 116** cats were excluded  
4  
5 106 from the study because of hyphema (12/116), retinal hemorrhages (48/116), bullous (24/116) and  
6  
7  
8 107 complete (32/116) retinal detachment.

9  
10 108 *Clinical examination group 1*

11  
12 109 All cats underwent a physical examination which included measurements of body temperature,  
13  
14  
15 110 pulse, respiratory rate, hydration status, thoracic auscultation, abdominal palpation and palpation of  
16  
17 111 the ventral neck to detect enlarged thyroid gland. Systemic **blood** pressure was assessed using a  
18  
19 112 high-definition oscillometry (petMAP<sup>®</sup>, Ramsey Medical Inc, Tampa, Florida, United States). Each  
20  
21  
22 113 cat was allowed 15 minutes to acclimatize to the clinic environment with the owner present, in a  
23  
24 114 setting with no stimuli, and systemic pressure was measured before performing any clinical  
25  
26 115 procedure. The appropriately sized cuff (size 3.0 cm) was applied at the base of the tail with the cat  
27  
28  
29 116 in a sternal-recumbent position. The same operator carried out three sequential measurements at  
30  
31 117 one-minute intervals. Blood pressure values (systolic and diastolic) were calculated as the  
32  
33 118 mathematical mean of the three measurements. The measurements taken in agitated or moving cats  
34  
35 119 were eliminated, as were those in which the heart rate measured with the instrument differed from  
36  
37  
38 120 the heart rate measured manually by more than 50 beats per minute.

39  
40 121 Anamnestic and clinical information were analysed in order to exclude current or prior systemic  
41  
42 122 diseases.

43  
44 123 *Clinical examination group 2*

45  
46  
47 124 All the cats underwent a clinical examination using the procedure described above for group 1. Cats  
48  
49 125 with a systolic pressure equal to or higher than 160 mmHg and diastolic pressure equal to or higher  
50  
51 126 than 100 mmHg were considered hypertensive.

52  
53  
54 127 All the cats underwent diagnostic procedures including laboratory diagnostics to help reach a  
55  
56 128 diagnosis. All the blood samples were taken from the jugular vein. The urine samples were taken  
57  
58 129 via cystocentesis. All tests were carried out at the same clinic (San Marco Veterinary Clinic and  
59  
60 130 Laboratory) and always included:

- 131 1. **Complete** blood count (CBC);
- 132 2. complete biochemical profile;
- 133 3. coagulation profile;
- 134 4. serum electrophoresis;
- 135 5. thyroid function tests (TSH, TT4 fT4);
- 136 6. urine test (urinary dipstick, specific gravity on refractometer, osmolality, urinary protein  
137 to urinary creatine ratio, microscopic sediment).

138 To formulate a reliable etiological diagnosis, each cat underwent a cardiology consultation and,  
139 where necessary, imaging diagnostic procedures such as thoracic radiographs, electrocardiography,  
140 abdominal and thyroid ultrasound were performed.

141 *Ophthalmic examination and photographic documentation of the fundus (groups 1 and 2)*

142 Each cat underwent an ophthalmic examination, carried out in a dark room where there were no  
143 stimuli, with minimal physical restriction. Complete ophthalmic examination always included  
144 neurophthalmic examination (palpebral reflex, assessment of menace response, pupillary light and  
145 dazzle reflexes), slit-lamp biomicroscopy (SL-15 portable Slit lamp, Kowa Company, Tokyo,  
146 Japan) and indirect ophthalmoscopy (Heine Omega 500 Unplugged and Heine 30D lens; Heine  
147 Instruments, Herrsching, Germany). Retention of corneal sodium fluorescein dye (HS Haag-Streit  
148 International fluorescein, Switzerland) and intraocular pressure estimation (TonoPen Vet, Reichert  
149 Inc, Depew, NY, USA) were performed.

150 For the photographic documentation of the fundus of the cats included in the study, a digital fundus  
151 camera for veterinary use (Clearview, Optibrand LLC, Ft Collins, Columbia, United States) was  
152 employed.

153 To prevent alteration of the anatomic characteristics of the retinal vasculature, both eyes were  
154 always examined without pharmacological dilation. (29)

155 A standard image shot centered on the optic disc was also defined, to allow the correct visualisation  
156 of the retinal vascular tree (arteries, veins and arteriolar bifurcations). The images obtained using

1  
2  
3 157 this technique needed to be free from defects caused by movement. The deliberate absence of all  
4  
5 158 identifying details prevented observers from recognising the images and, therefore, guaranteed a  
6  
7  
8 159 more objective judgement.

### 10 160 *Imagine analysing methods*

12 161 The program used for this project is semi-automatic, modified and adapted for measuring the feline  
13  
14  
15 162 fundus by the developers. The software algorithms are, therefore, able to calculate both vascular  
16  
17 163 and arterial diameters and to measure the angles of the arteriolar bifurcations (Fig. 1).

19 164 With the VAMPIRE<sup>®</sup> platform, the image processing system consists of I) digitalising the retina  
20  
21  
22 165 and II) measuring it.

### 24 166 *Digitalisation of the retina*

26 167 Digitalising the retina entails:

- 28 168 1. Applying a monochrome filter to enhance the contrast and definition of the vascular tree;
- 30  
31 169 2. Automatically defining the four standard measurement areas (SMA) identified with the  
32  
33 170 letters A, B, C and D. Guidelines (GL) for measuring the vessels were automatically  
34  
35 171 outlined within each of these areas (Figure 2.a);
- 37  
38 172 3. Manual cataloguing the vessels as arterial and venous (three arteries and three veins) for the  
39  
40 173 subsequent analysis of their diameters;
- 42 174 4. Selecting measuring points of the vessels for each SMA, defined as localised at the  
43  
44 175 intersection between the GL and the vessel itself (Figure 2.b);
- 46  
47 176 5. Identifying and selecting for the subsequent measurement the first, second and third  
48  
49 177 arteriolar bifurcations (Figure 2.c).

### 51 178 *Measurements*

53  
54 179 Information on the vascular diameters and the inner angle ( $\alpha$ ) of the first, second and third arteriolar  
55  
56 180 bifurcations was obtained as follows:

- 58 181 1. For each vascular measurement point previously identified, the margins of the vessel were  
59  
60 182 selected manually (Figure 3.a,b,c). The vascular diameter was calculated automatically;



- 1  
2  
3 183 2. For each arteriolar branch measurement point previously identified (mother vessel), the  
4  
5 184 anatomical landmarks (daughter vessels) were selected manually for the subsequent  
6  
7  
8 185 automatic calculation of the inner angle  $\alpha$  (Figure 3.d,e,f).  
9

### 10 186 *Assessment of intra- and inter-operator variability*

11  
12 187 **In order to validate the use of VAMPIRE® (semiautomatic) in terms of repeatability and**  
13  
14  
15 188 **reproducibility, 35 healthy cats randomly selected from the 105 healthy cats were evaluated in**  
16  
17 189 **relation to the following parameters: vein and artery for every SMA, first, second and third**  
18  
19 190 **arteriolar bifurcations angle. Two observers (experiments) were used and three repetitions**  
20  
21 191 **(tests) were made of the same measurement.** Research Randomizer ([www.randomizer.org](http://www.randomizer.org)) was  
22  
23 used to randomly organise both the selection and the order of the images to analyse. It seems  
24 192 unlikely that the images were memorized by the operators due to the long interval between the  
25  
26 193 different measuring sessions (three weeks) and the large number of vessels identified.  
27  
28 194

29  
30  
31 195 **Repeatability and reproducibility were assessed in relation to their individual and combined**  
32  
33 196 **effects on the overall variability of the measurements taken.**

### 35 197 *Assessment of the software potential clinical application*

36  
37  
38 198 **To assess the software potential clinical application** the measurements were compared by  
39  
40 199 analysing the photographic images **from group 2 (hypertensive animals) and a subset from**  
41  
42 200 **group 1 (healthy cats). The same parameters considered in the validation of VAMPIRE® were**  
43  
44 201 **used to compare the group of 105 healthy cats and the group of 43 clinically hypertensive cats**  
45  
46 202 **without evident abnormalities of the fundus. For the comparison of healthy and hypertensive**  
47  
48 203 **cats the** measurements were taken on the right eye only.  
49  
50

### 51 204 *Statistical analysis*

52  
53  
54 205 After testing the normality of the data, the non-parametric Mann-Whitney test was used to compare  
55  
56 206 the distribution of the values between healthy and hypertensive cats. Tukey box plot graphs were  
57  
58 207 produced for the graphic visualisation of these distributions.  
59

60  
208 The level of statistical importance was set for values of  $P < 0.05$ .

1  
2  
3 209 **RESULTS**

4  
5 210 The cats belonging to group 1 (clinically healthy cats) represented the normality dataset of the  
6  
7  
8 211 retinal measurements taken. One hundred and five cats of the same breed (domestic short hair)  
9  
10 212 were used: 55 males and 50 females with a mean **and median** of 55 months (minimum 48,  
11  
12 213 maximum 78). A total of 210 retinal images (**right and left eyes**) were analysed. Eleven points  
13  
14 214 (four veins, four arteries and three arterial bifurcations) were recognised and measured for each  
15  
16  
17 215 image, totalling 2310 measurements. **No statistical difference was found for each of the**  
18  
19 216 **comparison assessed. Table 1 summarised the values of the measurements taken only on the**  
20  
21 217 **right eye and represent the reference parameters for cats.**

22  
23  
24 218 **Group 2 was constituted by 43** hypertensive cats (**24 males and 20 females**) that met the criteria  
25  
26 219 for inclusion in the study. Mean **and median** age was 138 months (minimum 120, maximum 185).  
27  
28 220 Twenty-five cats were affected by chronic renal failure, 16 cats were affected by hyperthyroidism,  
29  
30  
31 221 and 2 cats presented both these diseases.

32  
33 222 *Intra- and inter-operator variability (repeatability and reproducibility)*

34  
35 223 Repeatability (r) and reproducibility (R) were blind tested by two independent operators who  
36  
37  
38 224 performed three series of measurements in a set consisting of 35 images at intervals of three weeks  
39  
40 225 (**Figure 4**). As no statistical difference was found between the measurements of the images of the  
41  
42 226 right eye (OD) and the left eye (OS), both observers assessed OD only. Each observer performed a  
43  
44 227 total of 1155 measurements (**i.e. 35 images multiplied by 11 points of evaluation**).

45  
46  
47 228 Lastly, the **coefficient of variation (CV)** was calculated, in terms of R and r, for every  
48  
49 229 measurement area (Table 2).

50  
51 230 *Comparison between the measurements taken in the two groups (healthy-hypertensive animals)*

52  
53 231 To assess the potential clinical applications of VAMPIRE<sup>®</sup>, 43 retinal images belonging to group 1  
54  
55  
56 232 and group 2 were analysed. In hypertensive cats the statistical processing proved the existence of a  
57  
58 233 statistically significant reduction (P<0.001) in arterial vascular diameter (group 1 mean 6.1 +/- 0.8;  
59  
60 234 group 2 mean 3.3 +/- 1.4) and arteriolar branch angles (first arteriolar branch angle: group 1 mean

1  
2  
3 235 73.3° +/- 19°; group 2 mean 54.7° +/- 20.5°. Second arteriolar branch angle: group 1 mean 77.1° +/-  
4  
5 236 17.1°; group 2 mean 54.7° +/- 20.5°. Third arteriolar branch angle: group 1 mean 83.9° +/-15.2°;  
6  
7  
8 237 group 2 mean 59.9° +/- 24.7°) associated with an increase in vein diameter (group 1 9.1 +/- 1; group  
9  
10 238 2 16.1 +/- 4) as shown in Figure 5.

11  
12 239

## 13 14 240 **DISCUSSION**

15  
16  
17 241 The results of the present study provide a validation of the semi-automatic software VAMPIRE® in  
18  
19 242 cats. Our results cannot be compared with the current veterinary literature as no studies have been  
20  
21 243 published in this field. In contrast, in human medicine some softwares for retinal imaging analysis  
22  
23  
24 244 has been validated, and some publications demonstrate their utility in the early diagnosis of retinal  
25  
26 245 vasculature changes during systemic hypertension. (7,19, 20, 21, 23)

27  
28 246 Our results showed that VAMPIRE® is consistent when giving interpretations. The results showed  
29  
30  
31 247 an optimum R for vein measurements (Mean **CV**: 1.1%) and a very good R for artery  
32  
33 248 measurements (Mean **CV**: 3.1%) and bifurcation angles (Mean **CV**: 3.4%). In these last two  
34  
35 249 groups, the Mean Variation Coefficient was higher in the standard measuring area (SMA) B for  
36  
37 250 arterioles (Mean **CV**: 5%) and in the assessment of third arteriolar bifurcations (Mean **CV**: 9.3%).

38  
39  
40 251 In fact, in SMA B, there is a higher overlapping of arteries and veins which could generate possible  
41  
42 252 errors in clearly distinguishing and precisely identifying the arterial walls. The third arteriolar  
43  
44 253 bifurcation angle (Mean **CV**: 9.3%) in the digital image was the least clear and most peripheral  
45  
46  
47 254 one, **prone** to more errors in interpretation.

48  
49 255 Repeatability absorbs most of the total variability in measurements. Nevertheless, R shows that  
50  
51 256 these measurements tend to comprise the same centre of measurement. “Poor” r must be considered  
52  
53  
54 257 in the light of the type of measurements taken, i.e. the possible discrepancy between these  
55  
56 258 measurements and the possible sphere of variation, which is very slight. In the comparison between  
57  
58 259 the two group measurements (clinically healthy and hypertensive cats), in the hypertensive cats  
59  
60 260 there was a statistically significant reduction in the arteriolar diameter (mean total: 3.5 pixels) and

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

261 branch angles ( $55^\circ$ ,  $47.8^\circ$  and  $24.7^\circ$ ), associated with an increase in the vein diameter (mean total:  
262 24.15 pixels).

263 Microvascular dysfunction has been suggested to be a pathogenic factor for the development of  
264 systemic hypertension (5, 6). In human medicine retinal vascular calibre can be assessed non-  
265 invasively from retinal photographs and computer-assisted approaches (20, 21, 22, 25, 27, 28),  
266 while there is currently no data on the application of retinal imaging analysis software in veterinary  
267 medicine.

268 There are intrinsic limitations to the method analysed: the measurements, although taken in  
269 standardised anatomical landmarks, refer to very small anatomical structures; and errors in the  
270 procedure are possible. Consequently, the operator is a variable. The results of our analysis were  
271 based on a single-occasion retinal measurements, and lacks information on serial measurements.  
272 VAMPIRE<sup>®</sup> is semi-automatic, thus the measurements have to be taken manually. To date, also in  
273 human medicine most publications (20, 21, 27) on assessing the change in vascular changes  
274 (vascular calibre and bifurcation angles) in fundus images still rely on a semi-automatic tool. Huang  
275 *et al.* proposed an automatic quantitative width measurement for retinal blood vessels, validating  
276 the technique by comparing the results with VAMPIRE<sup>®</sup>. (28)

277 Based on the observations from this study, the development of future automated algorithms for  
278 medical veterinary imaging essentially entails collecting a larger dataset including both normal and  
279 abnormal cases. An automatic retinal vessel measurement technique will enable fully quantitative  
280 retinal vessel analyses in large-scale screening programs.

## 281 CONCLUSIONS

282 The image processing of color fundus images could potentially play a role in the diagnosis of  
283 hypertensive retinopathy in cats. The findings of the retina image analysis offer a new method for  
284 the early diagnosis of hypertension and objectively reflect the complex, but only partially

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

285 understood, physiopathological mechanisms at the base of the initial stages of this syndrome, both  
286 in cats and humans. The VAMPIRE® algorithm used to measure vascular diameters and angles of  
287 the arteriolar bifurcations contributes to the objective diagnosis of early damage to the ocular  
288 fundus as a result of systemic hypertension. It also facilitates an additional investigation into the  
289 effect of microvascularisation on the physiopathology of this complex syndrome.

290  
291  
292  
293  
294  
295  
296  
297  
298  
299  
300  
301  
302  
303

For Peer Review

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60304 **REFERENCES**

- 305 1. Bijsmans ES, Jepson RE, Chang YM *et al.* Changes in systolic blood pressure over time  
306 in healthy cats and cats with chronic kidney disease. *Journal of Veterinary Internal*  
307 *Medicine* 2015; 29:855-861.
- 308 2. Chetboul V, Lefebvre HP, Pinhas C *et al.* Spontaneous feline hypertension: clinical and  
309 echocardiographic abnormalities, and survival rate. *Journal of Veterinary Internal*  
310 *Medicine* 2003; 17:89-95.
- 311 3. Kobayashi DL, Peterson ME, Graves TK *et al.* Hypertension in cats with chronic renal  
312 failure or hyperthyroidism. *Journal of Veterinary Internal Medicine* 1990; 4:58-62.
- 313 4. Maggio F, De Francesco TC, Atkins CE *et al.* Ocular lesions associated with systemic  
314 hypertension in cats: 69 cases (1985-1998). *Journal of the American Veterinary*  
315 *Medicine Association* 2000; 217:695-702.
- 316 5. Oparil S, Zaman MA, Calhoun DA. Pathogenesis of hypertension. *Annals of Internal*  
317 *Medicine* 2003; 139:761-776.
- 318 6. Attariwale R, Giebs CP, Glucksberg MR. The influence of elevated intraocular pressure  
319 on vascular pressures in the cat retina. *Investigative Ophthalmology and Visual Science*  
320 1994; 35:1019-1025.
- 321 7. Chew SK, Xie J, Wang JJ. Retinal arteriolar diameter and the prevalence and incidence  
322 of hypertension: a systemic review and meta-analysis of their association. *Current*  
323 *Hypertension Reports* 2012; 14:144-151.
- 324 8. Crispin SM, Mould JR. Systemic hypertensive disease and feline fundus. *Veterinary*  
325 *Ophthalmology* 2001; 4(2):31-140.
- 326 9. De Venecia G, Jampol LM. The eye in accelerated hypertension. II. Localized serous  
327 detachment of the retina in patients. *Archives of Ophthalmology* 1984;102(1):68-73.

- 1  
2  
3 328 10. Henik R, Snyder P, Volk L. Treatment of systemic hypertension in cats with amlodipine  
4  
5 329 besylate. *Journal of the American Animal Hospital Association* 1997; 33:226-234.  
6
- 7  
8 330 11. Henik RA. Diagnosis and treatment of feline systemic hypertension. *Compendium on*  
9  
10 331 *Continuing Education for the Practising Veterinarian* 1997; 19:163-179.  
11
- 12 332 12. Morgan GE, Mikhail MS, Murray MJ. Systemic hypertension in four cats: ocular and  
13  
14  
15 333 medical findings. *Journal of the American Animal Hospital Association* 1986; 22:615-  
16  
17 334 621.  
18
- 19 335 13. Sansom J, Barnett KC, Dunn KA *et al.* Ocular disease associated with hypertension in 16  
20  
21 336 cats. *Journal of Small Animal Practice* 1994; 35:604-611.  
22
- 23  
24 337 14. Sansom J, Bodey A. Ocular sign in four dogs with hypertension. *Veterinary Record*  
25  
26 338 1997; 140:593-598.  
27
- 28  
29 339 15. Connell JM, Davies E. The new biology of aldosterone. *Journal of Endocrinology* 2005;  
30  
31 340 186:1-20.  
32
- 33 341 16. Brown S, Atkins C, Bagley R *et al.* Guidelines for the identification, evaluation, and  
34  
35 342 management of systemic hypertension in dogs and cats. *Journal of Veterinary Internal*  
36  
37 343 *Medicine* 2007; 21:542-558.  
38
- 39  
40 344 17. Carter JM, Irving AC, Bridges JP *et al.* The prevalence of ocular lesions associated with  
41  
42 345 hypertension in a population of geriatric cats in Auckland, New Zealand. *New Zealand*  
43  
44 346 *Veterinary Journal* 2014; 62:21-29.  
45
- 46  
47 347 18. Anderson DH, Guerin CJ, Erikson PA *et al.* Morphological recovery in the reattached  
48  
49 348 retina. *Investigative Ophthalmology and Visual Science* 1986; 27:168-183.  
50
- 51 349 19. Hubbard LD, Brothers RJ, King WN *et al.* Methods for evaluation of retinal  
52  
53 350 microvascular abnormalities associated with hypertension/sclerosis in the  
54  
55 351 Atherosclerosis Risk in Communities Study. *Ophthalmology* 1999; 106:2269-2280.  
56  
57 352 20. Abtamooff MD, Garvin MK, Sonka M. Retinal imaging and image analysis. *IEEE Review*  
58  
59 353 *in Biomedical Engineering* 2010; 3:169-208.  
60

- 1  
2  
3 354 21. Abtamoff MD, Garvin MK, Sonka M. Retinal imaging and image analysis. *IEEE Review*  
4  
5 355 *in Biomedical Engeneering* 2010; 3:169-208.  
6  
7  
8 356 22. Bartling H, Wanger P, Martin L. Measurement of optic disc parameters on digital fundus  
9  
10 357 photographs: algorithm development and evaluation. *Acta Ophthalmologica* 2008;  
11  
12 358 86:837-841  
13  
14  
15 359 23. Ikram MK, De Jong FJ, Vingerling JR *et al.* Are retinal arteriolar or venular diametes  
16  
17 360 associated with markers for cardiovascular disorders? The Rotterdam Study.  
18  
19 361 *Investigative Ophthalmology and Visual Science* 2004; 45:2129-2134.  
20  
21  
22 362 24. Ikram MK, Janssen JA, Roos AM *et al.* Retinal vessel diameters and risk of impaired  
23  
24 363 fasting glucose or diabetes: the Rotterdam Study. *Diabetes* 2006; 55:506-510.  
25  
26 364 25. Knudston MD, Klein BE, Klein R *et al.* Variation associated with measurement of  
27  
28 365 retinal vessel diameters at different points in the puls cycle. *British Journal of*  
29  
30 366 *Ophthalmology* 2004; 88:57-61.  
31  
32  
33 367 26. Mansour AM. Measuring fundus landmarks. *Investigative Ophthalmology and Visual*  
34  
35 368 *Science* 1990; 31:41-42.  
36  
37  
38 369 27. Trucco E, Ruggieri A, Karnowski T *et al.* Validating retinal fundus image analysis  
39  
40 370 algorithms: issues and proposal. *Investigative Ophthalmology and Visual Science* 2013;  
41  
42 371 54:3546-3559.  
43  
44  
45 372 28. Hunag F, Dashtbozorg B, Ka Shing Yeung A *et al.* A comparative study towards the  
46  
47 373 establishment of an automatic retinal vessel width measurement technique. In: Cardoso  
48  
49 374 M. *et al.* (eds) *Fetal, Infant and Ophthalmic Medical Image Analysis. OMIA 2017,*  
50  
51 375 *FIFI 2017. Lecture Notes in Computer Science, vol 10554.* Springer, Cham  
52  
53  
54 376 29. Harazny JM, Scmieder RE, Welzenbach J *et al.* Local application of tropicamide 0.5%  
55  
56 377 reduces retinal capillary blood flow. *Blood Pressure* 2013; 22(6):371-376.  
57  
58 378  
59  
60 379



## 380 TABLES

Table 1 – Vascular reference parameters in normal feline fundus (measurements from OD expressed in px)

	Mean	Standard Deviation	Median	Min	Max	Percentile 25	Percentile 75
Vein A	9.0	0.6	8.9	7.7	11.8	8.6	9.1
Vein B	9.1	1.0	9.0	6.9	14.2	8.5	9.4
Vein C	9.1	0.8	9.2	7.1	11.8	8.5	9.4
Vein D	9.3	0.7	9.3	7.3	11.4	8.9	9.7
Artery A	6.3	0.8	6.3	4.6	8.6	5.7	6.8
Artery B	6.2	0.8	6.2	3.7	7.8	5.7	7.0
Artery C	6.1	1.0	6.1	2.9	10.2	5.5	6.6
Artery D	5.8	1.1	5.8	2.4	8.6	5.1	6.5
1 <sup>st</sup> Angle	73.3	17.1	73.6	42.1	102.9	60.0	87.9
2 <sup>nd</sup> Angle	77.1	19.0	76.9	9.5	125.0	65.4	87.6
3 <sup>rd</sup> Angle	83.9	15.2	85.4	44.1	126.7	75.4	92.7

Table 2 – Evaluation of R&r in each SMA (%)

Arteries	A	B	C	D
CV R	2.8	5.0	2.5	2.6
CV r	7.7	5.6	8.9	11.1

Veins	A	B	C	D
CV R	0.4	0	0	0
CV r	4.7	3.8	4.2	3.6

Angles	1 <sup>st</sup> Gen	2 <sup>nd</sup> Gen	3 <sup>rd</sup> Gen
CV R	1.3	3.6	9.3
CV r	9.9	14.1	13.6

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

386 **FIGURES**

387 **Fig. 1. First (yellow square), second (green square) and third (blue square) arteriolar bifurcations (a) defined as**  
388 **the junction between two daughter vessels (d1 and d2) and a mother vessel (M) (b). Fig. 1.b is a magnified image**  
389 **belonging to Fig. 1.a.**

390 **Fig. 2. Definition of standard measurement areas (SMA) identified with letters and identification of**  
391 **measurement guidelines (yellow lines) (a). Selection of the vessel measuring point for each SMA (arteries red**  
392 **dots, veins light blue dots) (b). Identification of the first, second and third arteriolar bifurcations (red dots) (c).**

393 **Fig. 3. Semi-automatic measurement of the vascular diameters (a) and arteriolar bifurcations (d). Manual**  
394 **selection of the vessel margins (b) and of the arteriolar branch (e) before automatic calculation of vascular**  
395 **diameter (c) and the inner angle  $\alpha$  (f).**

396 **Fig. 4. Repeatability and reproducibility summary plot in arterial (a), venous vessels (b) and arteriolar**  
397 **bifurcations (c). The points traced in the graphs represent the deviations of the respective measurements from**  
398 **the average measurement for each individual part. Each operator is represented by a square. The height of the**  
399 **square represents an indication of the variability in measurements between tests. The length of the vertical lines**  
400 **containing the points joins together the various tests carried out by the same operator for each part.**

401  
402 **Fig. 5. Tukey box plots of the comparison of measurements of healthy and hypertensive cats. All these**  
403 **comparisons are statistically significant at level  $P < 0.001$**

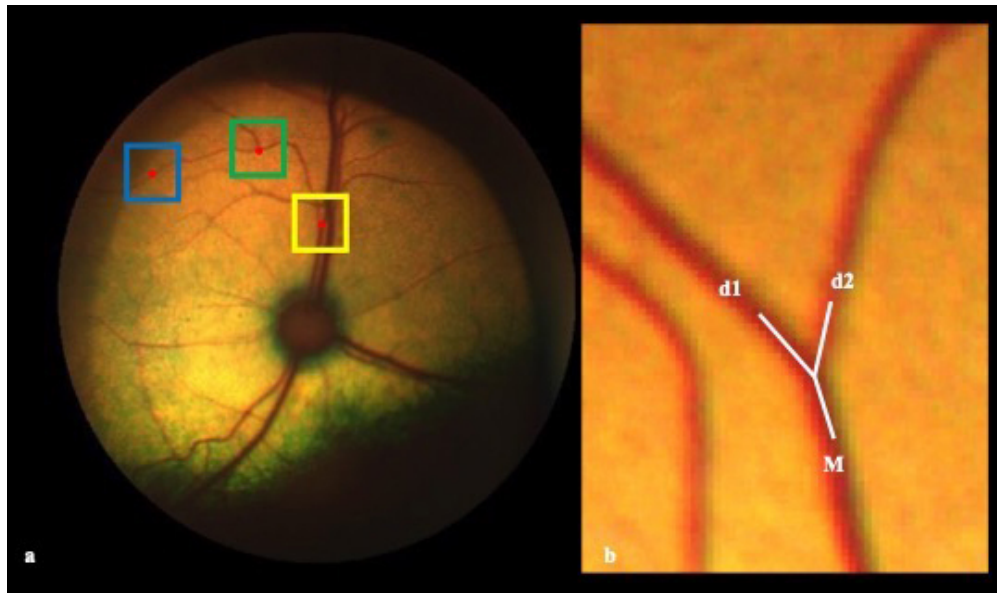


Fig. 1. First (yellow square), second (green square) and third (blue square) arteriolar bifurcations (a) defined as the junction between two daughter vessels (d1 and d2) and a mother vessel (M) (b). Fig. 1.b is a magnified image belonging to Fig. 1.a.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

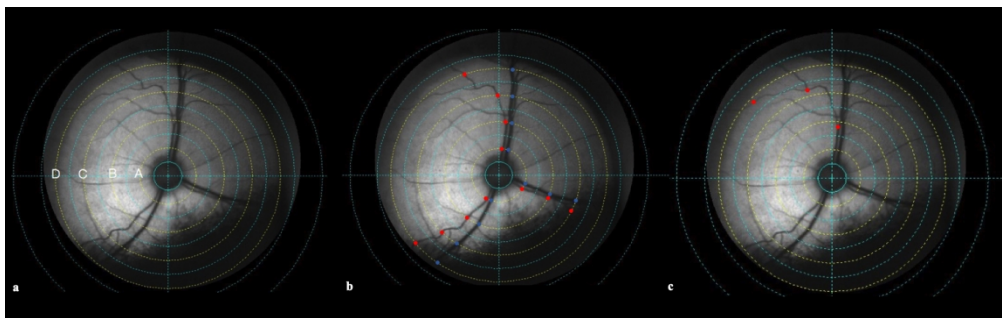


Fig. 2. Definition of standard measurement areas (SMA) identified with letters and identification of measurement guidelines (yellow lines) (a). Selection of the vessel measuring point for each SMA (arteries red dots, veins light blue dots) (b). Identification of the first, second and third arteriolar bifurcations (red dots) (c).

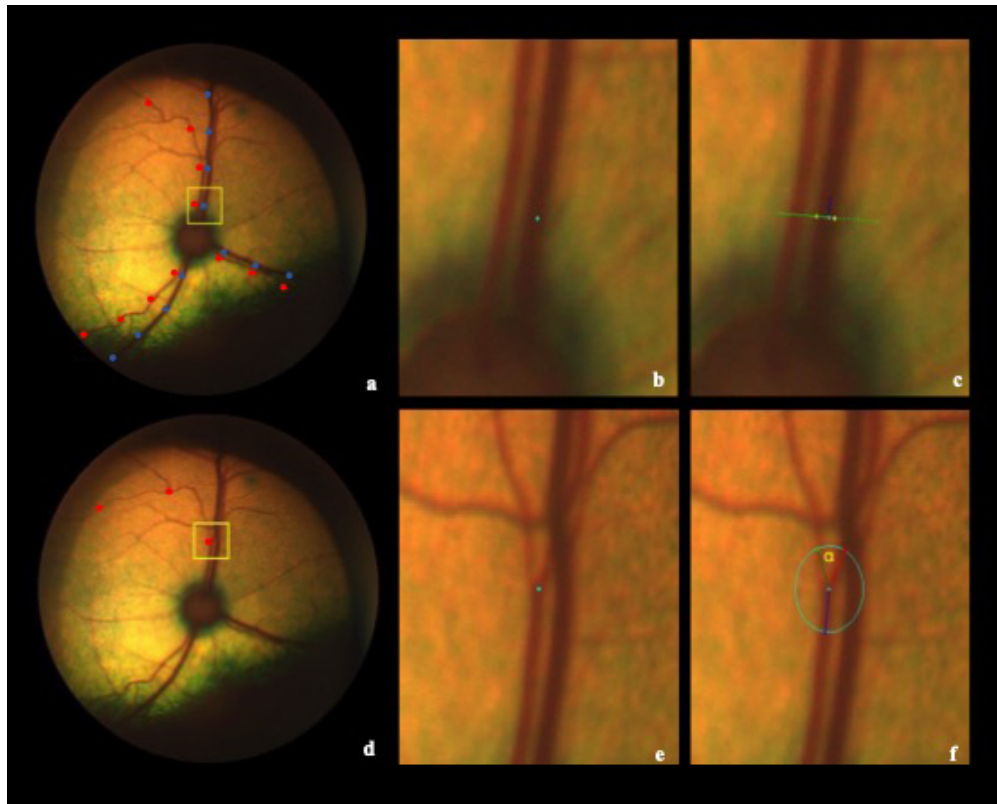


Fig. 3. Semi-automatic measurement of the vascular diameters (a) and arteriolar bifurcations (d). Manual selection of the vessel margins (b) and of the arteriolar branch (e) before automatic calculation of vascular diameter (c) and the inner angle  $\alpha$  (f).

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

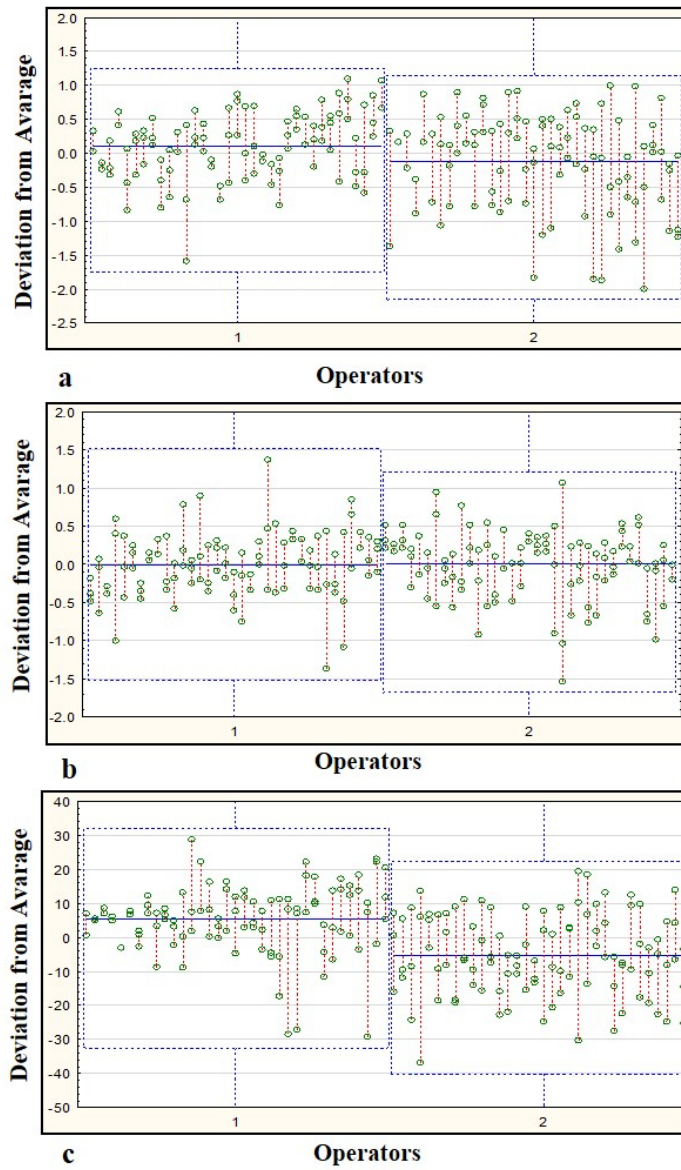


Fig. 4. Repeatability and reproducibility summary plot in arterial (a), venous vessels (b) and arteriolar bifurcations (c). The points traced in the graphs represent the deviations of the respective measurements from the average measurement for each individual part. Each operator is represented by a square. The height of the square represents an indication of the variability in measurements between tests. The length of the vertical lines containing the points joins together the various tests carried out by the same operator for each part.

51x86mm (300 x 300 DPI)

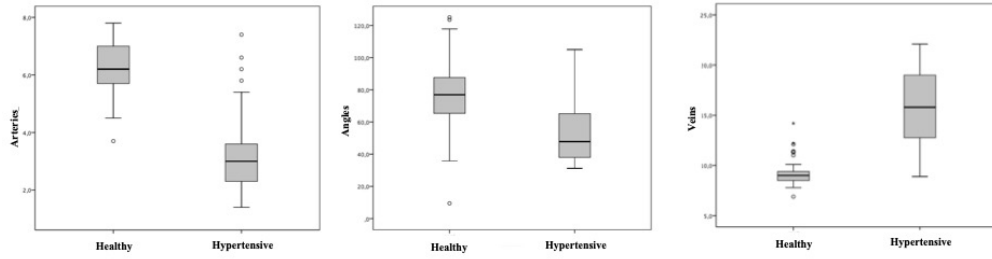


Fig. 5. Tukey box plots of the comparison of measurements of healthy and hypertensive cats. All these comparisons are statistically significant at level  $P < 0.001$

78x20mm (300 x 300 DPI)

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60