



Swansea University
Prifysgol Abertawe



Cronfa - Swansea University Open Access Repository

This is an author produced version of a paper published in:

Electrochimica Acta

Cronfa URL for this paper:

<http://cronfa.swan.ac.uk/Record/cronfa50057>

Paper:

Jones, T., Hernandez-Aldave, S., Kaspar, R., Letterio, M., Yan, Y. & Bertoncello, P. (2019). Tris(2,4,6-trimethoxyphenyl)polysulfone-methylene quaternary phosphonium chloride (TPQPCI) ionomer chemically modified electrodes: An electroanalytical study towards sensing applications. *Electrochimica Acta*

<http://dx.doi.org/10.1016/j.electacta.2019.04.089>

This item is brought to you by Swansea University. Any person downloading material is agreeing to abide by the terms of the repository licence. Copies of full text items may be used or reproduced in any format or medium, without prior permission for personal research or study, educational or non-commercial purposes only. The copyright for any work remains with the original author unless otherwise specified. The full-text must not be sold in any format or medium without the formal permission of the copyright holder.

Permission for multiple reproductions should be obtained from the original author.

Authors are personally responsible for adhering to copyright and publisher restrictions when uploading content to the repository.

<http://www.swansea.ac.uk/library/researchsupport/ris-support/>

Accepted Manuscript

Tris(2,4,6-trimethoxyphenyl)polysulfone-methylene quaternary phosphonium chloride (TPQPCI) ionomer chemically modified electrodes: An electroanalytical study towards sensing applications

Thomas R. Jones, Sandra Hernandez-Aldave, Robert B. Kaspar, Michael Letterio, Yushan Yan, Paolo Bertoncello

PII: S0013-4686(19)30775-3

DOI: <https://doi.org/10.1016/j.electacta.2019.04.089>

Reference: EA 34037

To appear in: *Electrochimica Acta*


Received Date: 13 January 2019

Revised Date: 14 April 2019

Accepted Date: 14 April 2019

Please cite this article as: T.R. Jones, S. Hernandez-Aldave, R.B. Kaspar, M. Letterio, Y. Yan, P. Bertoncello, Tris(2,4,6-trimethoxyphenyl)polysulfone-methylene quaternary phosphonium chloride (TPQPCI) ionomer chemically modified electrodes: An electroanalytical study towards sensing applications, *Electrochimica Acta* (2019), doi: <https://doi.org/10.1016/j.electacta.2019.04.089>.

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

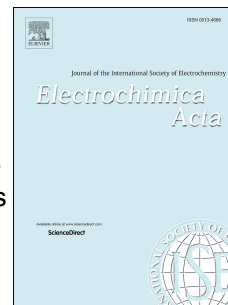

Quaternary Phosphonium Chloride (TPQPCI) Ionomer Chemically Modified Electrodes: an Electroanalytical Study towards Sensing Applications

Thomas R. Jones,^a Sandra Hernandez-Aldave,^a Robert B. Kaspar,^b Michael Letterio,^b
Yushan Yan,^b , and Paolo Bertoncello,^{a,c,*§}

^aSystems and Process Engineering Centre
College of Engineering
Swansea University, Bay Campus, Crymlyn Burrows, Swansea SA1 8EN, United
Kingdom

^bDepartment of Chemical and Biomolecular Engineering
University of Delaware, 150 Academy Street, Newark, DE 19716, USA

^cCentre for NanoHealth, Swansea University, Singleton Park, Swansea SA2 8PP, United
Kingdom

* To whom correspondence should be addressed

§ ISE member

We report for the first time the redox properties of an anion-exchange ionomer membrane, tris(2,4,6-trimethoxyphenyl)polysulfone-methylene quaternary phosphonium chloride (TPQPCl). TPQPCl was solubilized in ethanol/water solutions and films of TPQPCl at different concentrations were drop casted on glassy carbon electrodes. The thickness of TPQPCl films in dry conditions was evaluated using profilometer. The anion-exchange properties and charge transport properties of TPQPCl coated electrodes were investigated using $K_4Fe(CN)_6$ as anionic redox probe. The permselectivity properties of TPQPCl coated electrodes were assessed using hexaammine ruthenium(II) chloride. Cyclic voltammetry performed at low scan rate was utilized to determine the concentration of the redox mediator inside the films, with the apparent diffusion coefficient values of different TPQPCl coating estimated using both the Randles-Sevcik equation and the Anson's method. We found the concentration of the ferro/ferricyanide couple redox within the TPQPCl films in the order of 10^{-2} - 10^{-1} mol dm⁻³, with values of D_{app} in the order of 10^{-9} cm² s⁻¹. TPQPCl drop casted films evidenced good preconcentration capabilities towards incorporation of anions. To ascertain the suitability of the ionomer coated films towards the electroanalytical detection of anions, TPQPCl coated electrodes were utilized for the voltammetric detection of nitrites in tap and river waters. The results showed that TPQPCl coated electrodes are suitable to quantify nitrites in fresh waters with a limit of detection, LoD, of 1.07 μ M, sensitivity as 0.267 μ A μ M⁻¹ cm⁻² and linear range between 1 μ M and 500 μ M.

1. INTRODUCTION

Ionomers are an important class of ion-containing polymers. Specifically, ionomers can be defined as ionized copolymers constituted by a nonionic backbone with a small proportion (up to 15%) of ionized units with associated counterions [1]. As such, ionomers have found utilization in a variety of industrial applications, most significantly as membranes to separate the anode and cathode in fuel cells (proton exchange and alkaline fuel cells) [2-8] water electrolyzers [9-11] water purification [12, 13] and electro-membrane processes for desalination [14, 15]. From the electrochemical point of view, ionomers are an interesting class of material because when they are used as coating of electrode surfaces, the ionized groups can be utilized to preconcentrate, and hence quantify, electroactive species of opposite charge (cationic or anionic) using voltammetric methods [16]. Modification of electrode surfaces with ion selective polymeric materials has led to the development of the ion exchange voltammetry (IEV) with a variety of electroanalytical applications [16-19]. Among ionomers, Nafion[®], a sulfonated tetrafluoroethylene based fluoropolymer-copolymer, has undoubtedly been the most utilized material, since pioneer works from the Bard's [20-23] and Anson's [24-27] groups in the early 80' until today. In these works, Nafion[®] coatings were deposited on electrode surfaces by evaporation from alcoholic solutions. The dissociable proton allowed the incorporation of redox cations via ion-exchange from contacting solutions. Typical redox mediators incorporated in Nafion[®] films include tris(2-2'-

electrochemiluminescence [20, 21, 31, 32] applications. These studies provided also fundamental insights into the mechanisms (physical diffusion and “electron hopping”) of charge transport within ionomers containing redox mediators [22, 23, 33-38]. Other redox mediators incorporated in Nafion[®] films include positively charge ferrocene derivatives for biosensing applications [39-41]. For electroanalytical purposes, ionomers also possess additional advantages such as permselective properties: this means that not only they do preconcentrate cations (if the ionomer is negatively charged) or anions (if the ionomer is positively charged), but at the same time, they help on preventing potential interferences by repelling ions of same charge. While there is an extensive literature for Nafion and other cation-exchanger ionomers for electroanalytical applications, in the case of anion (alkaline)-exchange ionomers, their use as coating membranes for voltammetric detection is more limited and mainly based on quaternary ammonium functionalized membranes [16, 19, 42-52]. In 2009, Gu *et al.* reported for the first time the synthesis and characterization of tris(2,4,6-trimethoxyphenyl)polysulfone-methylene quaternary phosphonium hydroxide (TPQPOH) with ion-exchange capability (IEC) values comparable to Nafion[®] towards use as a membrane in hydroxide fuel cells [53, 54]. Recently, we demonstrated the possibility to use a TPQPOH derivative as composite material with graphite nanoplatelets for simultaneous detection of ascorbic acid and dopamine [55]. However, the evaluation of charge transport and diffusion properties of TPQPCl ionomer has not yet been reported. TPQPOH is the first example of quaternary phosphonium functionalized membrane that showed exceptional thermal stability as well as high solubility in methanol [53, 54]. These properties led us to explore in this study

applications, for instance detection of anions such nitrites. Nitrite ions (NO_2^-) are ubiquitous in nature, and extensively utilized as an additive in the food industry to prevent the formation of microorganisms that causes rancidity, and to maintain the color of red meat. However, nitrites in acidic environments as it is the stomach for example, combined with amines of food, lead to the formation of carcinogenic nitrosamines, which have been linked to various forms of cancer [56-58]. This has led the World Health Organisation (WHO) to set up a daily intake limit of nitrite as $0.07 \text{ mg NO}_2^-/\text{kg}$ body weight. Various electrochemical methods have been developed for the detection of nitrites and these involved either the oxidation or reduction of nitrites at bare or chemically modified electrodes [59-64]. Because the reduction of nitrites is affected by interferences such as oxygen and nitrate reduction, hence oxidation is usually preferred [59, 65, 66]. In this work, with a ligand exchange procedure, we exchanged the hydroxide counterion with the chloride one to obtain TPQPCl, to avoid potential interferences in the electrochemical characterization. Then, we fabricated TPQPCl coatings on glassy carbon electrodes and we investigated the charge transport properties using $\text{K}_4\text{Fe}(\text{CN})_6$ as a model anionic redox probe. The electrochemical characterization allowed us the estimation of the concentration of the redox species inside TPQPCl coating as well as the apparent diffusion coefficients. Finally, we demonstrated the potentiality of TPQPCl coated electrodes for the detection of anions, such as nitrite ions in tap and river waters.


2. EXPERIMENTAL SECTION

2.1. Materials. Potassium ferrocyanide $\text{K}_4\text{Fe}(\text{CN})_6$, NaCl, NaNO_2 and all other reagents were obtained from Sigma Aldrich and used as received.

Chemicals. All electrodes and polishing materials were purchased from IJ Cambria (UK).

All aqueous solutions were made using Milli-Q Ultra-pure water (UWP with a resistivity of $\geq 18.2 \text{ M}\Omega\cdot\text{cm}$ @ $25 \text{ }^\circ\text{C}$) from a Millipore Direct Q3 water purifier.

2.2. Synthesis of TPQPCl. TPQPCl was synthesized using the procedure reported earlier by one of us: the quaternary phosphorization of chloromethylated polysulfone, CMPSf, with tris(2,4,6-trimethoxyphenyl)phosphine [53]. The CMPSf was determined by ^1H NMR to have a degree of chloromethylation (dc) of 165%, leading to the final TPQPCl product containing 1.65 quaternary phosphonium group ion exchange sites per polysulfone unit, or a degree of functionalization (df) of 165%. By knowing the average molecular weight of the Udel-3500 polysulfone precursor (80-86 KDa) [67], and the degree of functionalization of TPQPCl (165%) [53], the average molecular weight of TPQPCl has been calculated as 242-261 KDa. The structure of TPQPCl is reported in Scheme 1.

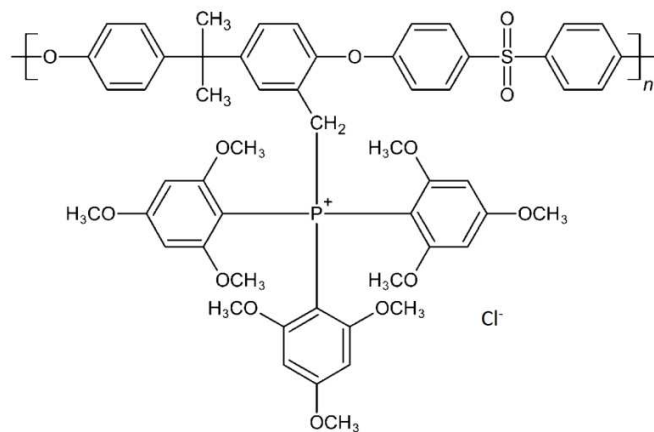

Scheme 1. Structure of Tris(2,4,6-trimethoxyphenyl)polysulfone-methylene quaternary phosphonium chloride (TPQPCl).

Cyclic voltammetry (CV), chronoamperometry (CA), and differential pulse voltammetry (DPV) measurements were performed using a bipotentiostat electrochemical analyzer (CH Instrument, Model CHI760). A conventional three electrode configuration was used, where the working electrode was a glassy carbon electrode (CH Instruments) of 3 mm diameter; a platinum wire as a counter electrode and a Ag/AgCl was used as a reference electrode. The experiments were carried out at room temperature. Glassy carbon electrodes (GCEs) were cleaned by successive polishing to gain a mirror-like appearance using 1 μm and 0.05 μm alumina slurry on micro cloth pads (Buehler), followed by sonication in acetone, ethanol and water, respectively, for 15 minutes. The cleaning procedure was carried out immediately prior to each use or polymer deposition. Film thicknesses were measured using a Taylor Hobson Talysurf stylus profilometer, while pH measurements were recording using a Hanna instruments 2002 Edge pH meter.

2.4. TPQPCl coated electrodes. A 2.5% stock solution of TPQPCl was prepared by dissolving TPQPCl powder in a solvent mix that was 1:1 by weight ethanol and water using sonication. 50 mg of TPQPCl were dissolved in 1.23 ml ethanol and 0.975 ml of DI water to give a 2.5% TPQPCl solution. 1% and 0.5% TPQPCl concentrations were prepared by dilution of the 2.5% TPQPCl solution as appropriate in an ethanol/water mixture. Drop casted TPQPCl films were prepared by casting 10 μl aliquots of the polymer solutions (1% or 0.5%) on a polished GCE surface using an Eppendorf micropipette and then evaporating to dryness under ambient conditions. Typical drying times were 25 minutes. TPQPCl films were loaded in $\text{K}_4\text{Fe}(\text{CN})_6$ redox mediator solutions of varying concentrations with a 0.1 M NaCl supporting electrolyte. All

ensure complete saturation of the TPQPCI. The polymer-coated electrodes loaded with the redox mediator were rinsed briefly with distilled water and placed in the electrochemical cell containing only supporting electrolyte solution, where CVs were carried out at a different range of scan rates. The surface coverage values were experimentally calculated from the charge, Q , associated with the complete oxidation of the film-bound redox species. Q was extracted by graphical integration of the background corrected cyclic voltammograms at scan rate of 1 mV s^{-1} in 0.1 M NaCl supporting electrolyte. The concentration of redox mediator incorporated into TPQPCI films was calculated from thickness measurements and the calculated surface coverage.

2.5. Detection of Nitrite ions. A 50 mM sodium nitrite stock solution was prepared using NaNO_2 (Sigma) and 0.1 M NaCl as supporting electrolyte. All other solutions were obtained by dilution of the 50 mM nitrite solution. For pH experiments the solution was adjusted as appropriate by addition of concentrated HCl or NaOH solutions with stirring. For the analysis of nitrite ions in tap and river waters, the samples were used as received without any pH adjustment. The pH values of these samples were in the range of pH 7-8.1. The investigation on potential interference were carried out by addition of various analytes to the 0.1 M solution of NaCl supporting electrolyte at 25 seconds time intervals, whilst running a chronoamperometry experiment with applied potential of 0.86 V under constant stirring (1000 rpm). Each interference analyte was dissolved in 0.1 M NaCl supporting electrolyte before addition to the electrochemical cell and the final concentration of each analyte in the solution was $5 \text{ }\mu\text{M}$. Tap water samples were taken from the mains water tap in our laboratory, while samples of water from the Llynfi River

any treatment. TPQPCl coated electrodes were conditioned in each nitrite sample for 20 minutes with stirring, whereas DPV scans were carried out under quiet conditions. DPV scans were carried out with increment 0.005 V, amplitude 0.05 V, pulse width 0.05 s, sampling width 0.0334 s, pulse period 0.5, E_{initial} 0.5 V; E_{final} 1.3 V.

3. RESULTS AND DISCUSSION

3.1. General Electrochemical Properties.

In order to ascertain the dynamics of incorporation of the redox mediators, TPQPCl coated electrodes were exposed to a negatively charged redox mediator such as the $\text{K}_4\text{Fe}(\text{CN})_6$ redox couple, and several CVs were recorded during the loading procedure. S1 reports typical CVs (first 100 scans) performed at 1% TPQPCl coated electrode during loading in a solution containing 5 mM $\text{K}_4\text{Fe}(\text{CN})_6$. The incorporation of the redox mediator occurs rapidly with peak currents that increase linearly with the time until CVs revealed time-invariant peak currents at higher loading times (up to 7200 s, see S2). The CVs recorded under loading conditions with the redox mediator in the electrolyte solution (Figure 1, solid line) reveals the typical redox behavior of the $\text{Fe}^{2+/3+}$ couple with peak currents that scale linearly with the square root of the scan rate as in indication of a process diffusion-controlled. When the electrode is transferred into the medium containing only supporting electrolyte (Figure 1, dotted line), the peak currents for the TPQPCl coated electrodes decreased slightly to 70 μA from the initial value of 82 μA recorded in the loading solution, and with ΔE_p values slightly decreased compared to those obtained under loading conditions.

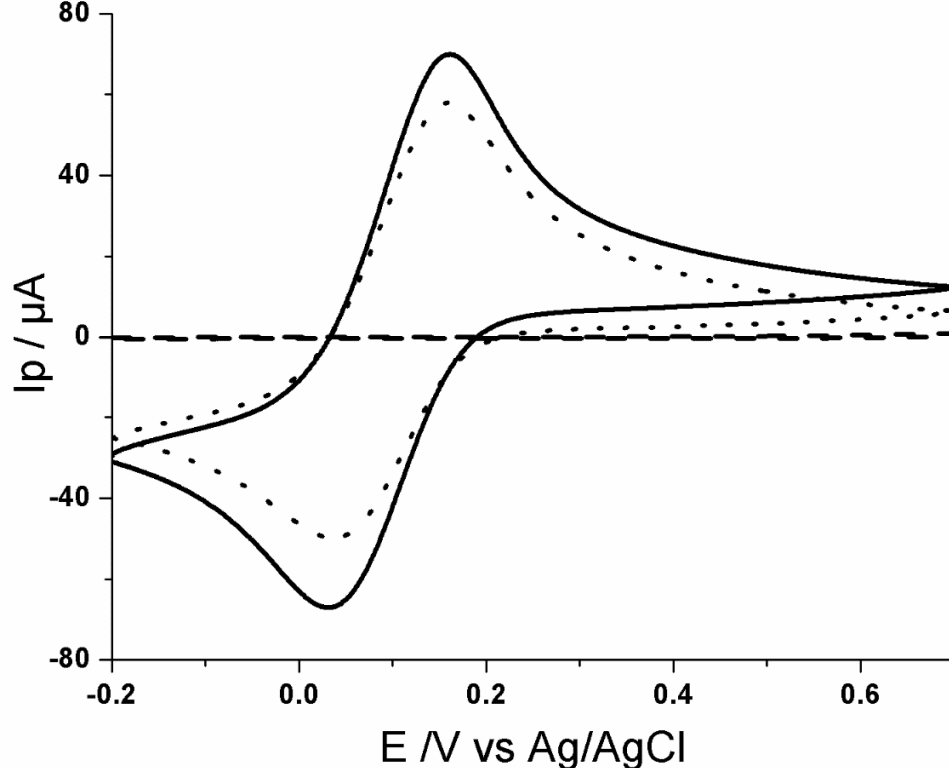


Figure 1. CVs of 1% TPQPCl coated film loaded in 5 mM $K_4Fe(CN)_6$ (solid line) and after transferring to 0.1 M NaCl supporting electrolyte (dotted line). Dashed line: background CV of 1% TPQPCl coated film in 0.1 M NaCl supporting electrolyte prior to loading. Scan rate of 100 mV s^{-1}

Note that the ΔE_p values were found to be larger at a higher scan rate (up to 150 mV at scan rate of 750 mV s^{-1}), whereas they decreased down to 23 mV at a lower scan rate (between $1\text{-}10 \text{ mV s}^{-1}$). In 0.1 M NaCl supporting electrolyte, the peak currents depended linearly on the scan rate at $\nu < 10 \text{ mV s}^{-1}$ as shown in Figure 2(a). This indicates a thin-layer like behavior. However, at high scan rates (from 100 mV s^{-1} to 2000 mV s^{-1}), the current was found to scale linearly with the square root of the scan rate, as an indication of a diffusion-controlled process (Figure 2(b)).

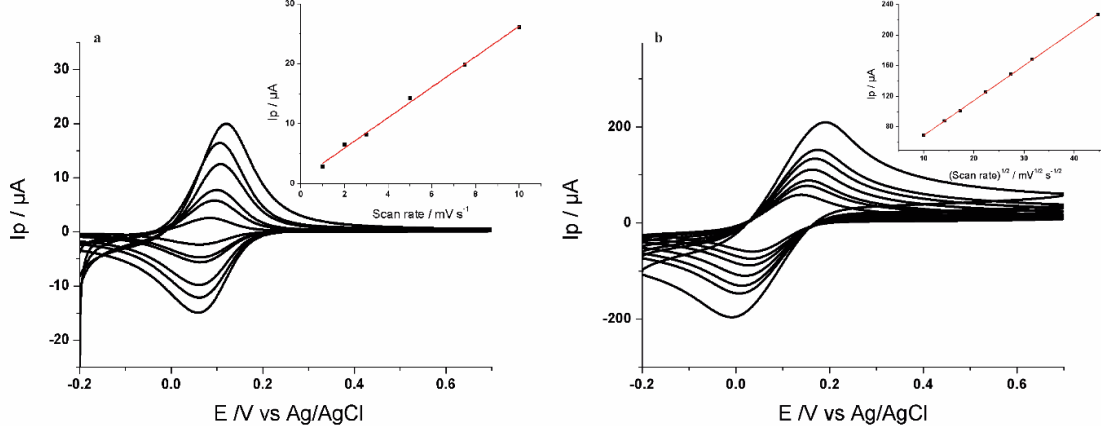


Figure 2. CVs of 1% TPQPCI coated film loaded in 5 mM $\text{K}_4\text{Fe}(\text{CN})_6$ after transferring to 0.1 M NaCl supporting electrolyte. Scan rate: from 1 mV s^{-1} to 10 mV s^{-1} (a) and from 100 mV s^{-1} to 2000 mV s^{-1} (b). The inset shows the plot of the anodic peak current vs the scan rate (a) and square root of the scan rate (b).

A similar behavior was observed also in the case of 0.5% TPQPCI coated electrode (see S3). Diffusion control is operative when the ionomer coating layer is thicker than the concentration gradient of the redox species in the films, hence the transition from thin-layer to diffusion-control is also thickness dependent. Note that the loss of the redox mediator in the time scale of the experiment (20 minutes) recorded at the beginning and the end of the experiments was typically around 15% (see S4). The surface coverage values (Γ , mol cm^{-2}) of the redox probe $\text{K}_4\text{Fe}(\text{CN})_6$ in the loaded TPQPCI coated electrodes were calculated from the CVs recorded in the electrolyte solution without redox species (Figure 2 (a) and (b)), and displaying thin-layer characteristics using the relation [68]

where Q (C) is the charge on the forward or reverse scan, n is the number of electrons transferred, A (cm²) is the geometric area of the electrode, and F is the Faraday constant (96486 C mol⁻¹). These values can be expressed as concentrations, with the knowledge of the thickness of the TPQPCl coated film, Φ (cm), and calculated using the profilometer. To estimate the apparent diffusion coefficients, we utilized two methods, *e.g.* (1) the Randles-Sevcik equation and (2) the Anson's plot method. For the former, we plotted the anodic peak currents, $I_{p,a}$ versus the square root of the scan rate, $v^{1/2}$, and applied the Randles-Sevcik equation [68], with the underlying assumption that the redox process is reversible. Note that the ΔE_p for each recorded CV increased monotonically with the scan rate which will tend to lead to an underestimation of D_{app} . The slope of these plots in the faster scan rate regime, combined with the polymer film thickness (calculated using the profilometer) and the number of electroactive species obtained by coulometric integration of the anodic peak current under thin layer conditions allowed the evaluation of the apparent diffusion coefficient values of TPQPCl coated electrodes. The calculated D_{app} for the Fe^{2+/3+} redox couple using the Randles-Sevcik equation was found to be $7.1 \pm 0.9 \times 10^{-9}$ cm² s⁻¹. For the latter method (Anson's plot), potential-step chronocoulometry was used to determine the values of D_{app} from the slope of the plots of the charge Q vs the square root of time, $t^{1/2}$, using the following relation:

$$D_{app} = \left[\frac{S\Phi\pi^{1/2}}{2F\Gamma} \right]^2 = \left[\frac{S\pi^{1/2}}{2FC} \right]^2 \quad (2)$$

conventional meaning as previously mentioned [33]. The value of D_{app} using the Anson's plot was estimated as $5.4 \pm 1.1 \times 10^{-9} \text{ cm}^2 \text{ s}^{-1}$ and in good agreement with that one calculated using the Randles-Sevcik equation. These values are consistent and of the same order of magnitude of D_{app} of ferrocyanide within cationic perfluoropolymer on basal plane pyrolytic graphite electrodes as reported by Oyama *et al.*[69]. To note that in using these methods to evaluate the apparent diffusion coefficients we made the tacit assumptions that ionomer films do not swell when immersed in solution, as well as that it is uniformly distributed throughout the ionomer coated film. Analysis of topography using AFM (see FigureS5) on TPQPCl recasted films (0.5% and 1%) evidenced the formation of a uniform film with root mean squared roughness (Rq) between 0.6 nm- 0.7 nm. These values are similar to those reported by Paul *et al.* for Nafion self-assembled films [70]. Measurements of the thickness of TPQPCl recasted films using profilometer before and after immersion in 0.1 M NaCl for 15 minutes did not show any variation due to swelling of the ionomer film. However, the values of D_{app} have to be taken as a general estimation, since TPQPCl may swell as a result of ingress and egress of ions during the voltammetric scans. Despite that, the values of D_{app} herein calculated are within the expected range for ionomer coated films, such as Nafion with redox mediators such as $\text{Ru}(\text{bpy})_3^{2+}$ and $\text{Ru}(\text{NH}_3)_6^{3+}$ [22],[24]. Table 1 reports the values of the surface coverage, concentration of redox probe, and apparent diffusion coefficient extracted using these methods for 0.5% and 1% TPQPCl coated electrodes. It is interesting to note that loaded TPQPCl coated films retains the redox species after been transferred in supporting

film in the order of magnitude of 10^{-2} - 10^{-1} mol dm⁻³.

Table 1. Parameters extracted using cyclic voltammetry and chronocoulometry relating to 0.5% and 1% TPQPCI coated electrodes loaded in 5 mM K₄Fe(CN)₆ after transferring to 0.1 M NaCl supporting electrolyte.; S = Anson slope of I_p vs. $t^{1/2}$, Φ = film thickness, C_p = concentration of K₄Fe(CN)₆ in TPQPCI, m = number of moles of K₄Fe(CN)₆ incorporated into the film.

[TPQPCI] %	Φ / (10 ⁻⁴) cm	Γ / (10 ⁻⁸) mol cm ⁻²	C_p / (10 ⁻⁴) mol cm ⁻³	m / (10 ⁻⁹) moles	D_{app}/RS (10 ⁻⁹) cm ² s ⁻¹	S / (10 ⁻⁵) C s ^{-1/2}	$D_{app}/Anson$ (10 ⁻⁹) cm ² s ⁻¹
0.5	1.64 ± 0.28	1.47 ± 0.03	0.9 ± 0.023	1.09 ± 0.03	2.35 ± 0.29	3.88 ± 0.70	3.26 ± 0.90
1	2.57 ± 0.22	3.40 ± 0.14	1.33 ± 0.09	2.44 ± 0.11	7.1 ± 0.43	7.07 ± 0.90	5.40 ± 1.10

The coated TPQPCI film retains a significant portion (*ca.* 70%) of the redox mediator after continuous cycling, and despite the peak current decreasing with the time, a voltammetric peak is still clearly visible even after 24 hour of continuous cycling (see S4). An important characteristic of ionomer membranes is the permselectivity, *e.g.* the ability to incorporate ions of opposite charge, whilst repelling those of the same charge. Figure 3 shows the CVs recorded at 1% TPQPCI coated electrodes fully loaded in 5 mM of K₄Fe(CN)₆ after transferring in supporting electrolyte containing different concentrations (from 0.1 mM to 50 mM) of a positively charge redox probe such as Ru(NH₃)₆³⁺. The TPQPCI coated electrode does not show any voltammetric peak related to the redox behaviour of the Ru(NH₃)₆^{3+/2+} couple for concentration below 1 mM (see S6). At concentrations higher than 1 mM, the typical redox peak of the couple Ru(NH₃)₆^{3+/2+} is noticeable at -0.15 V along with the redox peak current related to the

$\text{Ru}(\text{NH}_3)_6^{3+/2+}$ increase. Note that in order to clearly detect the peak of $\text{Ru}(\text{NH}_3)_6^{3+/2+}$, a

high concentration (up to 50 mM) has to be added to the solution.

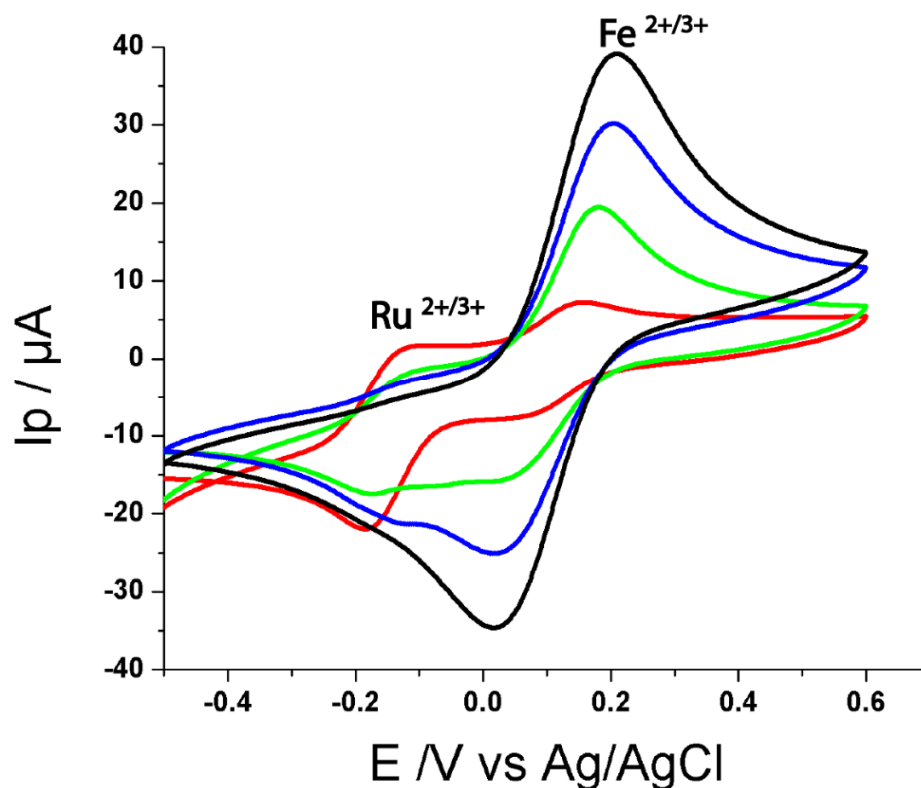


Figure 3. CVs of 1% TPQPCI coated film loaded in 5 mM $\text{K}_4\text{Fe}(\text{CN})_6$ after transferring to 0.1 M NaCl supporting electrolyte, and with addition of different concentration of $\text{Ru}(\text{NH}_3)_6^{3+}$; 0.1 mM (black); 1 mM (blue), 10 mM (green), and 50 mM (red). Scan rate of 100 mV s^{-1} .

3.2. Electrochemical behavior of nitrite at TPQPCI coated electrodes.

The electrochemical behavior of TPQPCI coated electrodes in the presence of nitrite ions were investigated using cyclic voltammetry and differential pulse voltammetry. Figure 4 shows the CV of bare GCE (left) and 1% TPQPCI (right) obtained at different

irreversible oxidation peak at 1.05 V and 0.97 V for bare GCE and TPQPCl coated electrode, respectively. Noticeably, the peak current at the TPQPCl coated electrode is *ca.* 3 times higher than the bare GCE. While for the TPQPCl coated electrode the addition of 2 μM of nitrite ions is sufficient to clearly visualize the related oxidation peak, for the bare GCE a voltammetric peak is only visible at concentrations higher than 20 μM . For the TPQPCl coated electrodes we observed a slight deviation from linearity at concentrations of nitrite higher than 0.5 mM as an indication that at such concentrations the TPQPCl coated films may have reached saturation. In fact, for concentration of nitrite ions higher than 20 mM, the peak current at the pristine GCE is larger than that one observed at TPQPCl coated electrode (see Figure S7). We believe this is an indication that as such high concentrations the fully saturated ionomer film further prevent the diffusion of nitrite ions. We observed also that the background current at the bare GCE to be higher than that one observed for TPQPCl coated electrode (see Figure S8). This fact, along with the ability of TPQPCl to accumulate nitrite ions, implies that lower concentrations of nitrite ions can be detected at TPQPCl coated electrodes. (Figures S8(a-b)). Interestingly, while the full preconcentration of $\text{K}_4\text{Fe}(\text{CN})_6$ within TPQPCl films requires a relatively long time (at least 20 minutes, see S2(b)), in the case of nitrite ions the preconcentration occurs in a matter of a couple of minutes as evidenced in Figure S9. This is due to the fact that nitrite ions are smaller than ferrocyanide ions and therefore penetrate more easily into the ionomer film.

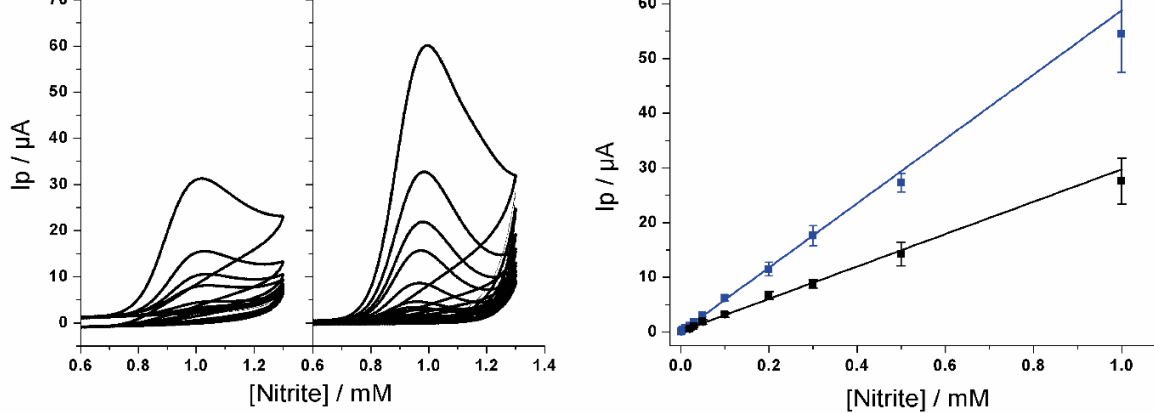


Figure 4. (a) CVs of bare GCE (left) and 1% TPQPCl coated electrode (right) recorded in 0.1 M NaCl supporting electrolyte in the presence of various concentrations of NO_2^- , from 5 μM to 1 mM. Scan rate of 100 mV s^{-1} . (b) Inset: plot of peak currents vs concentration of NO_2^- : bare GCE (black line), TPQPCl coated electrode (blue line). Error bars calculated from 5 repeat measurements.

These data highlight as TPQPCl coated electrodes are able to accumulate the nitrite ions as a result of the exchange properties between the positively charged phosphonium groups of the ionomer and the negatively charged nitrite ions available in solution. The peak current scale linearly with the concentration of nitrite ions until 1 mM concentration, then it increases until 25 mM where it starts to plateau (See Figure S7). It is worth mentioning that typically the nitrite content in water and food are in the order of sub-micromolar concentrations, and therefore it is at such range of concentrations that the sensor will have to operate. The sensitivity of TPQPCl coated electrode is even more pronounced when using DPV. Figure 5 shows the DPV curves recorded at bare GCE and TPQPCl coated electrode at different concentrations of nitrite. In this case the oxidation peak of nitrite at TPQPCl coated electrode occurs at a potential *ca.* 0.2 V less positive

coated electrode is *ca.* 5 times higher than that one recorded at the bare GCE.


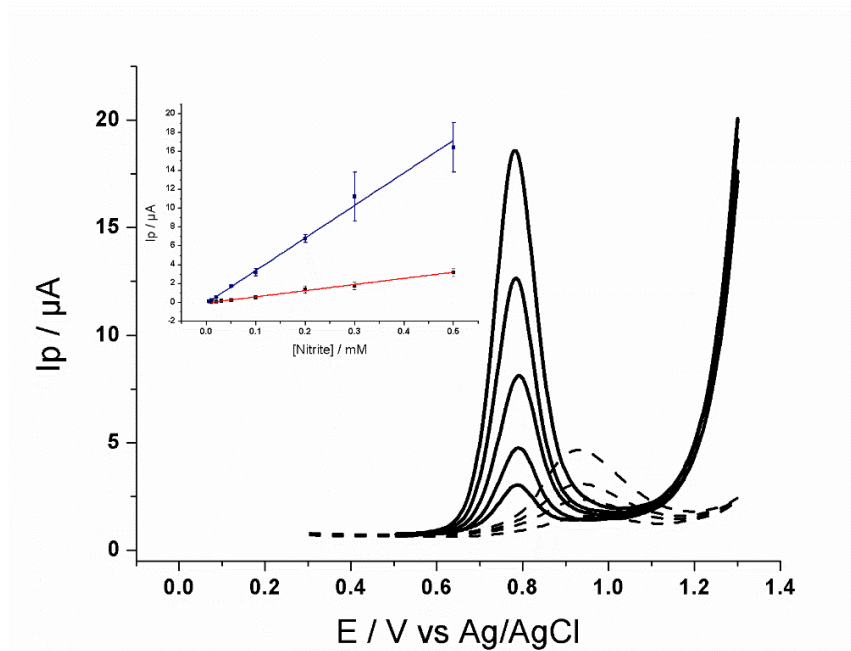



Figure 5. DPVs of bare GCE (dashed line) and 1% TPQPCI coated electrode (solid line) recorded in 0.1 M NaCl supporting electrolyte in the presence of various concentrations of NO_2^- , from 5 μM to 0.5 mM. Scan rate of 10 mV s^{-1} . Inset: plot of peak currents vs concentration of NO_2^- : bare GCE (red line), TPQPCI coated electrode (blue line). Error bars calculated from 5 repeat measurements.

The irreversible oxidation of nitrite to nitrate ions occurs through the following mechanism [71, 72]:



Equation 3 shows that the oxidation of nitrite to nitrate occurs via a two-electron reaction with concomitant formation of protons. This relation suggests that the peak current is pH dependent. For this purpose, we performed several experiments using DPV at different

using DPV after addition of 1 mM of NO_2^- . The peak current shows a maximum for values of pH between 7 and 10, while outside this range (pH <7 and pH >10) the peak current values drop significantly. The fact the peak current decreases at pH <7 shows that nitrite ions are not stable in acidic conditions. It is well established that nitrite ions in acidic environment undergo the following chemical reactions:



In this case NO_2^- ions are converted into NO and NO_3^- ions, with the latter that, of course, can not be further oxidized. Also, the pK_a of HNO_2 is 3.3, hence, at very acidic pH, nitrite ions are protonated forming HNO_2 . Since TPQPCl is effective in exchanging anionic species, if NO_2^- ions are in protonated form they will not be incorporated by the phosphonium groups within TPQPCl. Instead, in the case of pH >10, the decrease of the voltammetric signal can be attributed to the higher concentration of OH^- ions that at this pH range is well in excess and will compete with NO_2^- ions for the phosphonium sites. This is not surprising, taking into account that TPQPCl is originally derived from TPQPOH utilized as a membrane in alkaline fuel cells, hence its affinity for OH^- ions is very high [53]. Based on these results we performed all experiments involving nitrite ions at pH 7 which is also the measured pH of the supporting electrolyte solution.

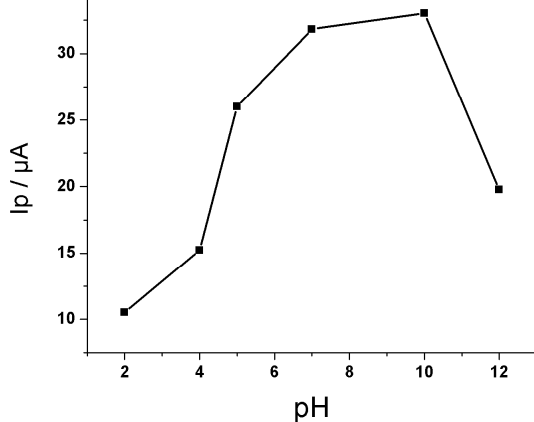


Figure 6. Plot of anodic peak current vs for 1% TPQPCl coated electrode recorded in 1 mM NO_2^- and 0.1 M NaCl supporting electrolyte. Scan rate of 10 mV s^{-1} .

We have also evaluated the response of the TPQPCl coated electrode using chronoamperometry. Figure 7 (a) depicts the amperometric $i-t$ response obtained at 1% TPQPCl coated electrode recorded in 0.1 M NaCl as supporting electrolyte, at various concentration of sodium nitrite and by applying a potential of 0.86 V. The addition of sodium nitrite was performed at regular intervals time of *ca.* 30 seconds and under stirring conditions. The chronoamperometry (CA) $i-t$ curve shows that TPQPCl coated electrode responds rapidly to every addition of nitrite with an increase of the current, and reaching the steady-state after *ca.* 5 seconds. However, the currents measured are *ca.* 3 times smaller than those registered using cyclic voltammetry previously shown in Figure 4. We explain this difference with the fact that in the CA experiment different concentrations of nitrites were added every 30 seconds, instead the CVs were recorded after 20 minutes elapsed time at each nitrite addition. We also observed (Figures not shown) that CVs recorded without elapsing times give consistently lower current than

coated electrodes needs few minutes of recovery time in order to be fully regenerated.

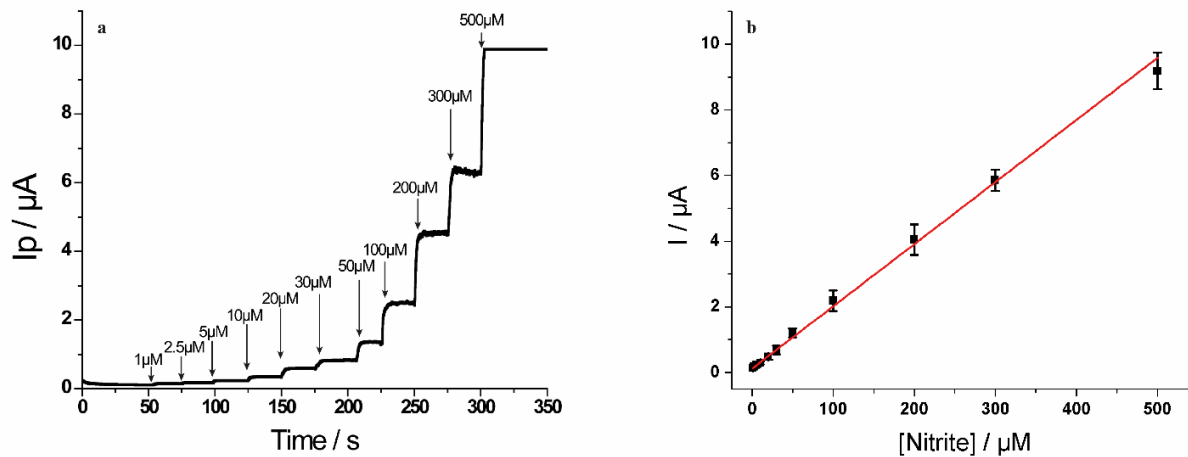


Figure 7. (a) Chronoamperometric (i - t) response of 1% TPQPCl coated electrode obtained with successive concentration of nitrite from 0.001 mM to 0.5 mM recorded in 0.1 M NaCl supporting electrolyte (pH 7), applied potential 0.86 V. (b) Calibration plot as a function of nitrite concentration as in (a). Error bars calculated from 5 repeat measurements.

The corresponding plot of the current vs. nitrite concentrations exhibits a linear response in the range from 1 μM to 0.5 mM with a regression equation expressed as I_p (μA) = 0.0189 [nitrite] (μM) + 0.125 ($R^2=0.9971$). Moreover, the sensitivity of TPQPCl coated electrode is calculated as $0.267 \mu\text{A} \mu\text{M}^{-1} \text{cm}^{-2}$, whereas the limit of detection, LoD, is 1.07 μM , and calculated from the slope of the linear regression plot, S , and the standard deviation, S_b , of 5 repeats of 0.5 μM nitrite addition, using the relation $\text{LoD} = 3S_b/S$. Similarly, the limit of quantification, LoQ, is calculated as 3.45 μM , from the slope of

addition, using the relation $LoQ = 10S_b/S$.

The as-prepared TPQPCl coated electrodes are also very stable up to two weeks when left in aqueous solutions. The performance of TPQPCl coated electrodes herein obtained shows that the as-prepared ionomer-coated electrode is competitive with other systems reported in literature in terms of linear range, sensitivity and limits of detection, despite not being the best, as summarized in Table 2. However, we want to emphasize the simplicity of the as-prepared ionomer coating herein presented compared to the other materials reported in Table 2.

Table 2. Analytical performances of amperometric sensors for the detection of nitrite ions.

<i>Electrode</i>	Linear Range (μM)	Sensitivity ($\mu\text{A } \mu\text{M}^{-1} \text{cm}^{-2}$)	Detection limit (μM)	Technique	Reference
<i>Ag-Fe₃O₄-GO modified GCE</i>	0.5-720	1.996	0.17	Amperometry	Li et al. (2015)
<i>GE/AEBA/DPAN/PtNPs</i>	10-1000	-	5	Amperometry	Miao et al. (2011) [74]
<i>Thionin modified ACNTs</i>	3-500	0.396	1.12	DPV	Zhao et al. (2007) [75]
<i>CaFe₂O₄ modified SPCE</i>	0.016-1928	0.3712	0.066	Amperometry	Balasubramanian et al. (2018) [72]
<i>Cu/MWCNTs modified GCE</i>	5-1260	0.4558	1.8	Amperometry	Manoj et al. (2018) [76]
<i>NiHCF/PDAP hybrid on GCE</i>	0.1-131	7.5	0.0151	Amperometry	Wang et al. (2018) [77]
AgNS /GCE	0.1-8	0.580	0.031	Amperometry	Shivakumar et al. (2017) [78]
Ag-RGO nanocomposite	10-1000	0.373	-	Amperometry	Shaikh et al. (2016) [79]
Pd/Fe ₃ O ₄ /polyDOPA/RGO	2.5-6470	0.01537	0.5	Amperometry	Zhao et al. (2017) [80]
<i>TPQPCl Modified GCE</i>	3-2000	0.488	1.18	DPV	This work
<i>TPQPCl Modified GCE</i>	1-500	0.267	1.07	Amperometry	This work

of the ionomer coated electrode to discriminate analytes that could interfere with the analytical determination of the selected analyte, in our case nitrite ions. Figure 8 illustrates the chronoamperometric response obtained in the presence of several interference species such as sodium sulfite, potassium chloride, glucose, sodium persulfate, and copper nitrate. The concentration of these interference species was as that of sodium nitrite, in our case 5 μM . The results showed that the voltammetric response of TPQPCl coated electrode is not affected by the presence of these interference species at least when their concentration is of the same magnitude of nitrite ions (see Figure 8 (a)). Instead, for the bare GCE, the addition of sodium sulfite is sufficient to generate a noticeable interference (Figure 8 (a)).

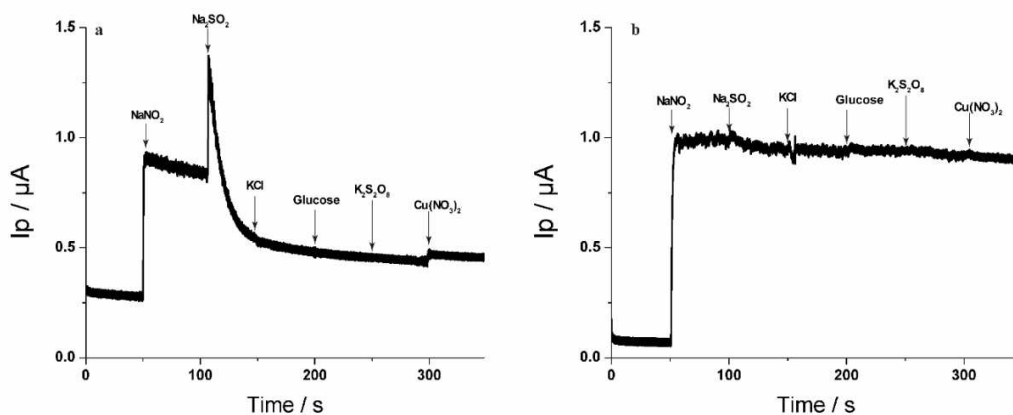


Figure 8. Chronoamperometric (i - t) response of (a) bare GCE and (b) 1% TPQPCl coated electrode obtained with the addition of interference species as highlighted in the figure. The concentration of nitrite and of interference species is 5 μM , supporting electrolyte 0.1 M NaCl (pH 7), applied potential 0.86 V.

as HSO_3^- and SO_3^{2-} and the hydronium ions produced as a result of the electrochemical oxidation of nitrite to nitrate (see Eq. 3) will protonate HSO_3^- to H_2SO_3 and SO_3^{2-} to HSO_3^- . We performed an experiment by recording CVs at bare GCE and 1% TPQPCl at different pH values (pH 7 and pH 10) in the presence of 10 mM sulfite ions where we observed higher oxidation current peaks at basic pH compared to neutral pH (see Figure S10). At pH 10 sulfite ions are present as SO_3^{2-} suggesting that TPQPCl coated electrode have higher affinity for bivalent anions. In this range of pH we expect sulfite to become a potential serious interference species. Additional study of potential interference species was performed using dopamine and ascorbic acid (see Figure S11). Dopamine, which is a positively charged is repelled by TPQPCl and as expected, does not show any interference in the detection of nitrite. In the case of ascorbic acid which is negatively charged, we observed a light interference, however further study using DPV showed that it may become significant at concentrations of ascorbic acid higher than 1 mM, even though the peak separation between the two species could allow the simultaneous detection (see Figure S12). Before proceeding on testing TPQPCl coated electrodes with real samples we have investigated potential issues of memory effects, e.g. accumulation time upon the signal of nitrite. Figure S13 reports the DPVs obtained after addition of 0.1 mM nitrite ions. Immediately after recording the DPV (black curve), we recorded a second DPV curve without recovery time. The DPV showed a substantial decrease in the peak current, however, a recovery time of 3 minutes was sufficient to restore the initial value of the peak current. Also (figure not shown), running a DPV in 0.1M supporting electrolyte allowed to clean the TPQPCl coated electrode for further measurements.

towards the detection of nitrite in samples of tap water and of water taken from the effluent outflow of a paper mill in the Llynfi Valley. The samples were spiked with 0.1 M NaCl supporting electrolyte before use and the pH measured before analysis was equal to 8 and 7.8 for the tap water and effluent river samples, respectively. A known concentration of nitrite was spiked in these samples and the chronoamperometric curves and I_p vs. [nitrite] curves are reported in Figure 9.

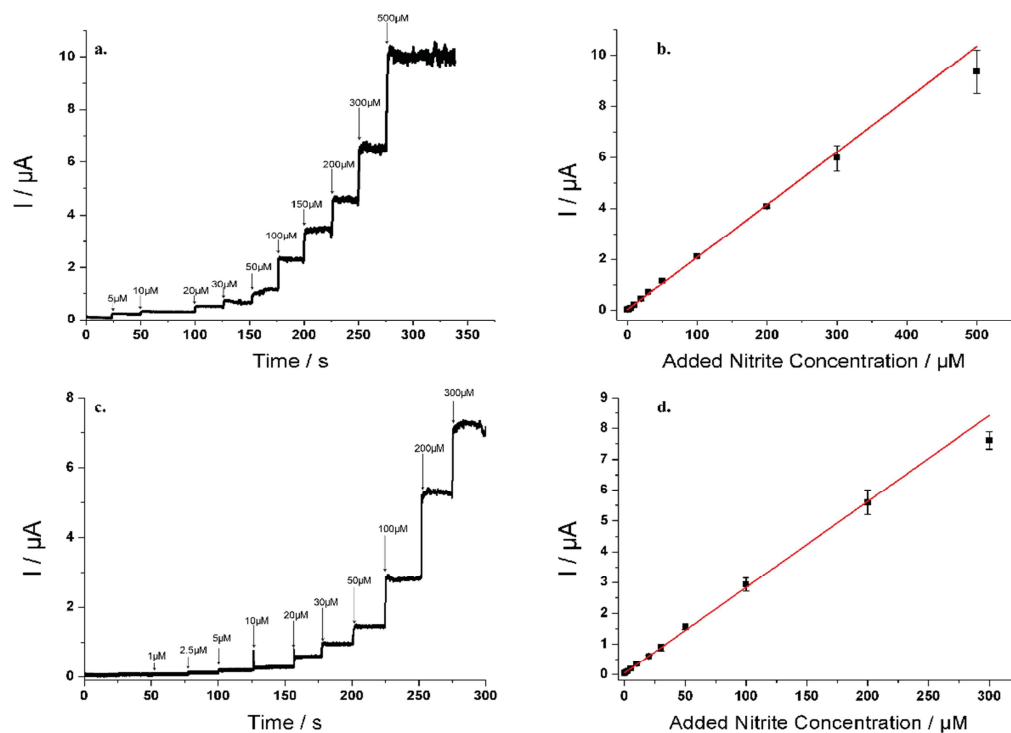


Figure 9. (a) Chronoamperometric (i - t) response of 1% TPQPCl coated electrode obtained in tap water (pH 8.02) and water effluent from a paper mill (pH 7.81) (c), after addition of different concentration of nitrite. Calibration plot (b), (d) as a function of nitrite concentration as in (a), and (c), respectively; Applied potential 0.86 V. Error bars calculated from 3 repeat measurements.

3. The values obtained for the nitrite concentration are 0.0507 mg NO₂⁻/L and 0.0814 mg NO₂⁻/L in tap and river water, respectively. The values found are well below the European standard limits for tap water of 0.5 mg NO₂⁻/L. set up by the European commission [81]. The results showed good reproducibility and RSD values for the nitrite spiked water samples are around 3%. All the results point out as the as-prepared TPQPCl coated electrode as a competitive and simple system compared to other voltammetric systems for the determination of nitrite ions.

Table 3. Analytical performances of TPQPCl coated electrode for the detection of nitrite in tap water and river sample

<i>Sample</i>	Added (μM)	Found (μM)	Recovery %
<i>Tap water</i>	-	1.10 \pm 0.08	-
	20	22.05 \pm 0.65	104.5%
<i>Paper mill Effluent water</i>	-	1.77 \pm 0.19	-
	20	21.56 \pm 0.72	99.1%

4. CONCLUSIONS

We have demonstrated that TPQPCl ionomer can be effectively utilized in electroanalysis for detection of anions. The electrochemical characterization performed using cyclic voltammetry and chronocoulometry allowed the concentration of redox mediator within TPQPCl films, and the apparent diffusion coefficients to be determined. Also, through

the ionomer. TPQPCl coated electrodes were tested for determination of anions such as nitrite ions in tap and river water samples. The results indicated that the as-prepared TPQPCl coated films can detect nitrite ions with a limit of detection (LoD) of 1.07 μM , sensitivity as 0.267 $\mu\text{A } \mu\text{M}^{-1} \text{ cm}^{-2}$, and linearity range between 1 μM -500 μM . The results herein point out that TPQPCl ionomer is an attractive material in electroanalysis for detection of nitrite ions.

ACKNOWLEDGEMENTS. This research was supported by the Engineering and Physical Sciences Research Council (EPSRC), grant EP/L013797/1. We are grateful to Dr. Daniel Johnson (Swansea University) for the AFM images. TRJ and SHA gratefully acknowledge financial support for their PhD scholarship through a Doctoral Training Account funded by the EPSRC (TRJ), and a Knowledge Economy Skills Scholarship (KESS2) under the Welsh Government's European Social Fund (ESF) convergence programme for West Wales and the Valleys (SHA).

Author contributions

T.R.J. performed all electrochemical experiments and analyzed the results. S.H.-A performed some of the electrochemical experiments and the evaluation of ionomer thickness using profilometer. R.B.K. and M.L. synthesized the ionomer membrane. P.B. and Y.Y. cowrote the manuscript.

Notes

The authors declare no competing financial interest.

- [1] C.G. Bazuin, A. Eisenberg, Ion containing polymers: Ionomers, *J. Chem. Educ.*, 58 (1981) 938-943.
- [2] B. Smitha, S. Sridhar, A.A. Khan, Solid polymer electrolyte membranes for fuel cell applications - a review, *J. Membr. Sci.*, 259 (2005) 10-26.
- [3] N.W. Deluca, Y.A. Elabd, Polymer electrolyte membranes for the direct methanol fuel cell: A review, *J. Polym. Sci. Pt. B-Polym. Phys.*, 44 (2006) 2201-2225.
- [4] G. Couture, A. Alaaeddine, F. Boschet, B. Ameduri, Polymeric materials as anion-exchange membranes for alkaline fuel cells, *Prog. Polym. Sci.*, 36 (2011) 1521-1557.
- [5] K.A. Mauritz, R.B. Moore, State of understanding of Nafion, *Chem. Rev.*, 104 (2004) 4535-4585.
- [6] J.R. Varcoe, R.C.T. Slade, Prospects for alkaline anion-exchange membranes in low temperature fuel cells, *Fuel Cells*, 5 (2005) 187-200.
- [7] G. Merle, M. Wessling, K. Nijmeijer, Anion exchange membranes for alkaline fuel cells: A review, *J. Membr. Sci.*, 377 (2011) 1-35.
- [8] Y.J. Wang, J.L. Qiao, R. Baker, J.J. Zhang, Alkaline polymer electrolyte membranes for fuel cell applications, *Chem. Soc. Rev.*, 42 (2013) 5768-5787.
- [9] M. Carmo, D.L. Fritz, J. Merge, D. Stolten, A comprehensive review on PEM water electrolysis, *Int. J. Hydrog. Energy*, 38 (2013) 4901-4934.
- [10] S. Marini, P. Salvi, P. Nelli, R. Pesenti, M. Villa, M. Berrettoni, G. Zangari, Y. Kiros, Advanced alkaline water electrolysis, *Electrochim. Acta*, 82 (2012) 384-391.
- [11] H. Ito, T. Maeda, A. Nakano, H. Takenaka, Properties of Nafion membranes under PEM water electrolysis conditions, *Int. J. Hydrog. Energy*, 36 (2011) 10527-10540.
- [12] G.M. Geise, H.S. Lee, D.J. Miller, B.D. Freeman, J.E. McGrath, D.R. Paul, Water Purification by Membranes: The Role of Polymer Science, *J. Polym. Sci. Pt. B-Polym. Phys.*, 48 (2010) 1685-1718.
- [13] C.L. Liu, H.C. Mao, J.H. Zhu, S.B. Zhang, Ultrafiltration membranes with tunable morphology and performance prepared by blending quaternized cardo poly(arylene ether sulfone)s ionomers with polysulfone, *Sep. Purif. Technol.*, 179 (2017) 215-224.
- [14] C. Vogel, J. Meier-Haack, Preparation of ion-exchange materials and membranes, *Desalination*, 342 (2014) 156-174.
- [15] R.K. Nagarale, G.S. Gohil, V.K. Shahi, Recent developments on ion-exchange membranes and electro-membrane processes, *Adv. Colloid Interface Sci.*, 119 (2006) 97-130.
- [16] P. Ugo, L.M. Moretto, Ion-exchange voltammetry at polymer-coated electrodes: Principles and analytical prospects, *Electroanalysis*, 7 (1995) 1105-1113.
- [17] M. Pesavento, G. Alberti, R. Biesuz, Analytical methods for determination of free metal ion concentration, labile species fraction and metal complexation capacity of environmental waters: A review, *Anal. Chim. Acta*, 631 (2009) 129-141.
- [18] K.Z. Brainina, N.A. Malakhova, N.Y. Stozhko, Stripping voltammetry in environmental and food analysis, *Fresenius J. Anal. Chem.*, 368 (2000) 307-325.
- [19] P. Ugo, L.M. Moretto, F. Vezza, Ionomer-coated electrodes and nanoelectrode ensembles as electrochemical environmental sensors: Recent advances and prospects, *ChemPhysChem*, 3 (2002) 917-925.

- [21] I. Rubinstein, A.J. Bard, Polymer films on electrodes. 4. Nafion-coated electrodes and electrogenerated chemiluminescence of surface-attached tris(2,2'-bipyridine)ruthenium(2+), *J. Am. Chem. Soc.*, 102 (1980) 6641-6642.
- [22] C.R. Martin, I. Rubinstein, A.J. Bard, Polymer films on electrodes. 9. Electron and mass transfer in Nafion films containing tris(2,2'-bipyridine)ruthenium(2+), *J. Am. Chem. Soc.*, 104 (1982) 4817-4824.
- [23] H.S. White, J. Leddy, A.J. Bard, Polymer films on electrodes. 8. Investigation of charge-transport mechanisms in Nafion polymer modified electrodes, *J. Am. Chem. Soc.*, 104 (1982) 4811-4817.
- [24] D.A. Buttry, F.C. Anson, Electron hopping vs. molecular diffusion as charge transfer mechanisms in redox polymer films, *J. Electroanal. Chem.*, 130 (1981) 333-338.
- [25] D.A. Buttry, F.C. Anson, Effects of electron exchange and single-file diffusion on charge propagation in Nafion films containing redox couples, *J. Am. Chem. Soc.*, 105 (1983) 685-689.
- [26] D.A. Buttry, J.M. Saveant, F.C. Anson, Enhancement of charge transport rates by redox cross-reactions between reactants incorporated in Nafion coatings, *J. Phys. Chem.*, 88 (1984) 3086-3091.
- [27] D.A. Buttry, F.C. Anson, Electrochemical control of the luminescent lifetime of Ru(bpy)₃²⁺ incorporated in Nafion films on graphite electrodes, *J. Am. Chem. Soc.*, 104 (1982) 4824-4829.
- [28] M. Kaneko, S. Teratani, K. Harashima, Multiple redox reactions and electrochromism of bilayer membranes of Prussian blue and Ru(bpy)₃²⁺, *J. Electroanal. Chem.*, 325 (1992) 325-332.
- [29] T. Onikubo, R.J. Lin, M. Kaneko, In-situ twin-electrode spectroscopic voltammetry with a cell composed of a pair of Nafion®-coated indium tin oxide electrodes each incorporating Ru(bpy)₃²⁺ and methylviologen, *J. Electroanal. Chem.*, 361 (1993) 143-148.
- [30] R.J. Mortimer, C.P. Warren, Cyclic voltammetric studies of Prussian blue and viologens within a paper matrix for electrochromic printing applications, *J. Electroanal. Chem.*, 460 (1999) 263-266.
- [31] H.N. Choi, S.H. Cho, W.Y. Lee, Electrogenerated chemiluminescence from tris(2,2'-bipyridyl)ruthenium(II) immobilized in titania-perfluorosulfonated ionomer composite films, *Anal. Chem.*, 75 (2003) 4250-4256.
- [32] R.J. Forster, P. Bertoncello, T.E. Keyes, Electrogenerated Chemiluminescence, *Annual Reviews*, Palo Alto, 2009, pp. 359-385.
- [33] D.A. Buttry, F.C. Anson, Effects of electron exchange and single-file diffusion on charge propagation in nafion films containing redox couples, *J. Am. Chem. Soc.*, 105 (1983) 685-689.
- [34] K. Shigehara, N. Oyama, F.C. Anson, Electrochemical responses of electrodes coated with redox polymers. Evidence for control of charge-transfer rates across polymeric layers by electron exchange between incorporated redox sites, *J. Am. Chem. Soc.*, 103 (1981) 2552-2558.

Chem., 87 (1983) 214-219.

[36] F.C. Anson, J.M. Saveant, K. Shigehara, Kinetics of mediated electrochemical reactions at electrodes coated with redox polymer films, *J. Electroanal. Chem.*, 145 (1983) 423-430.

[37] F.C. Anson, D.N. Blauch, J.M. Saveant, C.F. Shu, Ion association and electric field effects on electron hopping in redox polymers. Application to the tris(2,2'-bipyridine)osmium(3+)/tris(2,2'-bipyridine)osmium(2+) couple in Nafion, *J. Am. Chem. Soc.*, 113 (1991) 1922-1932.

[38] P.J. Peerce, A.J. Bard, Polymer films on electrodes : Part III. Digital simulation model for cyclic voltammetry of electroactive polymer film and electrochemistry of poly(vinylferrocene) on platinum, *J. Electroanal. Chem.*, 114 (1980) 89-115.

[39] H.N. Choi, M.A. Kim, W.Y. Lee, Amperometric glucose biosensor based on sol-gel-derived metal oxide/Nafion composite films, *Anal. Chim. Acta*, 537 (2005) 179-187.

[40] M.L. Liu, L.P. Wang, J.H. Deng, Q. Chen, Y.Z. Li, Y.Y. Zhang, H.T. Li, S.Z. Yao, Highly sensitive and selective dopamine biosensor based on a phenylethynyl ferrocene/graphene nanocomposite modified electrode, *Analyst*, 137 (2012) 4577-4583.

[41] Z.H. Fan, D.J. Harrison, Permeability of glucose and other neutral species through recast perfluorosulfonated ionomer films, *Anal. Chem.*, 64 (1992) 1304-1311.

[42] P. Ugo, L.M. Moretto, S. Bellomi, V.P. Menon, C.R. Martin, Ion-exchange voltammetry at polymer film-coated nanoelectrode ensembles, *Anal. Chem.*, 68 (1996) 4160-4165.

[43] P. Ugo, L.M. Moretto, G.A. Mazzocchin, Voltammetric determination of trace mercury in chloride media at glassy-carbon electrodes modified with polycationic ionomers, *Anal. Chim. Acta*, 305 (1995) 74-82.

[44] M.C. Tsai, P.Y. Chen, Electrochemical detection of 2-naphthol at a glassy carbon electrode modified with Tosflex film, *Electroanalysis*, 19 (2007) 1315-1321.

[45] D.M. Tsai, A.S. Kumar, J.M. Zen, A highly stable and sensitive chemically modified screen-printed electrode for sulfide analysis, *Anal. Chim. Acta*, 556 (2006) 145-150.

[46] J.M. Zen, A.S. Kumar, C.R. Chung, A glucose biosensor employing a stable artificial peroxidase based on ruthenium purple anchored cinder, *Anal. Chem.*, 75 (2003) 2703-2709.

[47] T.H. Lu, J.F. Huang, I.W. Sun, Perfluorinated anion-exchange polymer mercury film electrode for anodic stripping voltammetric determination of zinc(II): effect of model organic compounds, *Anal. Chim. Acta*, 454 (2002) 93-100.

[48] J.M. Zen, D.M. Tsai, A.S. Kumar, V. Dharuman, Amperometric determination of ascorbic acid at a ferricyanide-doped Tosflex-modified electrode, *Electrochem. Commun.*, 2 (2000) 782-785.

[49] H.Y. Yang, W.Y. Chen, I.W. Sun, Anodic stripping voltammetric determination of bismuth(III) using a Tosflex-coated mercury film electrode, *Talanta*, 50 (1999) 977-984.

[50] L.M. Moretto, G.A. Mazzocchin, P. Ugo, Electroanalytical study on the ion-exchange voltammetric behaviour of Hg(II) at Tosflex(R)-coated glassy carbon electrodes, *J. Electroanal. Chem.*, 427 (1997) 113-121.

[51] P. Ugo, S. Zampieri, L.M. Moretto, D. Paolucci, Determination of mercury in process and lagoon waters by inductively coupled plasma-mass spectrometric analysis

- [52] E. Castillo, M. Granados, J.L. Cortina, Chemically facilitated chromium(VI) transport throughout an anion-exchange membrane - Application to an optical sensor for chromium(VI) monitoring, *J. Chromatogr. A*, 963 (2002) 205-211.
- [53] S. Gu, R. Cai, T. Luo, Z.W. Chen, M.W. Sun, Y. Liu, G.H. He, Y.S. Yan, A Soluble and Highly Conductive Ionomer for High-Performance Hydroxide Exchange Membrane Fuel Cells, *Angew. Chem.-Int. Edit.*, 48 (2009) 6499-6502.
- [54] S. Gu, R. Cai, T. Luo, K. Jensen, C. Contreras, Y.S. Yan, Quaternary Phosphonium-Based Polymers as Hydroxide Exchange Membranes, *ChemSusChem*, 3 (2010) 555-558.
- [55] S. Hernandez-Aldave, R.B. Kaspar, M.P. Letterio, A. Tarat, Y.S. Yan, P. Bertoncello, Quaternary phosphonium- based (TPQPCl)ionomer/ graphite nanoplatelets composite chemically modified electrodes: a novel platform for sensing applications, *J. Mater. Chem. C*, 6 (2018) 13293-13304.
- [56] N. Kaur, S. Chopra, G. Singh, P. Raj, A. Bhasin, S.K. Sahoo, A. Kuwar, N. Singh, Chemosensors for biogenic amines and biothiols, *J. Mat. Chem. B*, 6 (2018) 4872-4902.
- [57] F. Gassara, A.P. Kouassi, S.K. Brar, K. Belkacemi, Green Alternatives to Nitrates and Nitrites in Meat-based Products-A Review, *Crit. Rev. Food Sci. Nutr.*, 56 (2016) 2133-2148.
- [58] Y.L. Zhao, D.A. Zhao, D.L. Li, Electrochemical and Other Methods for Detection and Determination of Dissolved Nitrite: A Review, *Int. J. Electrochem. Sci.*, 10 (2015) 1144-1168.
- [59] B.R. Kozub, N.V. Rees, R.G. Compton, Electrochemical determination of nitrite at a bare glassy carbon electrode; why chemically modify electrodes?, *Sens. Actuator B-Chem.*, 143 (2010) 539-546.
- [60] J.A. Cox, P.J. Kulesza, A selective electrolytic sensor for nitrite based on a modified platinum-electrode, *Anal. Chim. Acta*, 158 (1984) 335-341.
- [61] J.A. Cox, P.J. Kulesza, Oxidation and determination of nitrite at modified electrodes, *J. Electroanal. Chem.*, 175 (1984) 105-118.
- [62] A. Ourari, B. Ketfi, S.I.R. Malha, A. Amine, Electrocatalytic reduction of nitrite and bromate and their highly sensitive determination on carbon paste electrode modified with new copper Schiff base complex, *J. Electroanal. Chem.*, 797 (2017) 31-36.
- [63] P.K. Rastogi, V. Ganesan, R. Gupta, P. Singh, P.K. Sonkar, D.K. Yadav, Potassium ferricyanide-incorporated branched polyethylenimine as a potential scaffold for electrocatalytic reduction and amperometric sensing of nitrite, *J. Appl. Electrochem.*, 47 (2017) 95-104.
- [64] S.L. Yang, X.D. Zeng, X.Y. Liu, W.Z. Wei, S.L. Luo, Y. Liu, Y.X. Liu, Electrocatalytic reduction and sensitive determination of nitrite at nano-copper coated multi-walled carbon nanotubes modified glassy carbon, *J. Electroanal. Chem.*, 639 (2010) 181-186.
- [65] Y.N. Jiang, H.Q. Luo, N.B. Li, Determination of nitrite with a nano-gold modified glassy carbon electrode by cyclic voltammetry, *Int. J. Environ. Anal. Chem.*, 87 (2007) 295-306.
- [66] P. Kalimuthu, S.A. John, Highly sensitive and selective amperometric determination of nitrite using electropolymerized film of functionalized thiadiazole modified glassy carbon electrode, *Electrochem. Commun.*, 11 (2009) 1065-1068.

Sci., 7 (2014) 354-360.

[68] A.J. Bard, L.R. Faulkner, *Electrochemical methods. Fundamentals and application*, 2 ed.1980.

[69] T. Okajima, T. Ohsaka, N. Oyama, Electrode-kinetics of the $Fe(CN)_6^{4-}$ complex confined in cationic perfluoropolymer films on electrode surfaces, *Bull. Chem. Soc. Jpn.*, 64 (1991) 1305-1312.

[70] D.K. Paul, K. Karan, A. Docoslis, J.B. Giorgi, J. Pearce, Characteristics of Self-Assembled Ultrathin Nafion Films, *Macromolecules*, 46 (2013) 3461-3475.

[71] G. Bharath, R. Madhu, S.M. Chen, V. Veeramani, D. Mangalaraj, N. Ponpandian, Solvent-free mechanochemical synthesis of graphene oxide and Fe_3O_4 -reduced graphene oxide nanocomposites for sensitive detection of nitrite, *J. Mater. Chem. A*, 3 (2015) 15529-15539.

[72] P. Balasubramanian, R. Settu, S.M. Chen, T.W. Chen, G. Sharmila, A new electrochemical sensor for highly sensitive and selective detection of nitrite in food samples based on sonochemical synthesized Calcium Ferrite ($CaFe_2O_4$) clusters modified screen printed carbon electrode, *J. Colloid Interface Sci.*, 524 (2018) 417-426.

[73] B.-Q. Li, F. Nie, Q.-L. Sheng, J.-B. Zheng, An electrochemical sensor for sensitive determination of nitrites based on $Ag-Fe_3O_4$ -graphene oxide magnetic nanocomposites, *Chemical Papers.*, 69 (2015) 911-920.

[74] P. Miao, M. Shen, L. Ning, G. Chen, Y. Yin, Functionalization of platinum nanoparticles for electrochemical detection of nitrite, *Anal Bioanal Chem.*, 399 (2011) 2407-2411.

[75] K. Zhao, H. Song, S. Zhuang, L. Dai, P. He, Y. Fang, Determination of nitrite with the electrocatalytic property to the oxidation of nitrite on thionine modified aligned carbon nanotubes, *Electrochem. Commun.*, 9 (2007) 65-70.

[76] D. Manoj, R. Saravananb, J. Santhanalakshmi, S. Agarwal, V.K. Gupta, R. Boukherrouf, Towards green synthesis of monodisperse Cu nanoparticles: An efficient and high sensitive electrochemical nitrite sensor, *Sens Actuator B*, 266 (2018) 873-882.

[77] X. Wang, W. Tan, H. Ji, F. Liua, D. Wua, J. Maa, Y. Konga, Facile electrosynthesis of nickel hexacyanoferrate/poly(2,6-diaminopyridine) hybrids as highly sensitive nitrite sensor, *Sens Actuator B*, 264 (2018) 240-248.

[78] M. Shivakumar, K.L. Nagashree, S. Manjappa, M.S. Dharmaprakash, Electrochemical Detection of Nitrite Using Glassy Carbon Electrode Modified with Silver Nanospheres ($AgNS$) Obtained by Green Synthesis Using Pre-hydrolysed Liquor, *Electroanalysis*, 29 (2017) 1434-1442.

[79] A. Shaikh, S. Parida, S. Bohm, One step eco-friendly synthesis of Ag -reduced graphene oxide nanocomposite by phyto-reduction for sensitive nitrite determination, *RSC Adv.*, 6 (2016) 100383-100391.

[80] Z.Y. Zhao, Z.H. Xia, C.Y. Liu, H. Huang, W.C. Ye, Green synthesis of Pd/Fe_3O_4 composite based on polyDOPA functionalized reduced graphene oxide for electrochemical detection of nitrite in cured food, *Electrochim. Acta*, 256 (2017) 146-154.

ACCEPTED MANUSCRIPT