

## ORIGINAL

# Effects of FM system fitted into normal hearing ear on speech-in-noise recognition in Japanese school-aged children with unilateral severe-to-profound hearing loss

Aki Shimada<sup>1</sup>, Jiro Udaka<sup>1</sup>, Hinami Nagashima<sup>b</sup>, Izumi Chida<sup>1</sup>, Eiji Kondo<sup>1</sup>, Seiichi Nakano<sup>1</sup>, Hidehiko Okamoto<sup>3</sup>, and Noriaki Takeda<sup>1</sup>

<sup>1</sup>Department of Otolaryngology, Tokushima University Graduate School of Biomedical Sciences, Tokushima, Japan, <sup>2</sup>Department of Speech-Language-Hearing Therapy, Kyushu University of Health and Welfare, School of Health Sciences, Miyazaki, Japan, and <sup>3</sup>Department of Physiology, International University of Health and Welfare School of Medicine, Narita, Japan

**Abstract : Objectives :** We examined speech recognition ability of elementary school-aged Japanese children with unilateral hearing loss under noisy environments and then examined the effects of the FM system fitted into their normal hearing ear on their speech recognition ability. **Methods :** Twelve children with severe-to-profound sensorineural hearing loss and ten age-matched children with bilateral normal hearing received speech recognition test in quiet and noisy environments. Other nine children with severe-to-profound sensorineural hearing loss received speech recognition test with or without the FM receiver fitted to the normal hearing ear in quiet and noisy environments. **Results :** Signal-to-noise ratio (SNR) in Japanese elementary school classrooms was estimated to be -6.9 dB at a preferential seat. In noisy environment of -5 dB SNR similar to working classrooms, the correct rates of speech recognition test in children with unilateral hearing loss were significantly lower, compared with those in children with bilateral normal hearing. In the noisy environment, the correct rates in children aided by the FM system with unilateral hearing loss were significantly better, compared with unaided ones. **Conclusion :** The results suggested that the FM system is recommended as an audiological management for improvement of speech recognition of children with unilateral hearing loss in noisy classrooms. *J. Med. Invest.* 65 : 216-220, August, 2018

**Keywords :** children with unilateral hearing loss, speech recognition, noisy environment, classroom, FM system

## INTRODUCTION

Until recently, it was believed that unilateral hearing loss has little impact on a child's speech-language development. However, there is growing evidence that children with unilateral hearing loss have speech and language delays and impaired speech recognition in noise (1, 2, 3). Recently it was reported that school-aged children with unilateral hearing loss showed worse oral language scores than those of their siblings with normal hearing (4). Since such listening problems could lead to difficulties in following classroom instructions and discussions, unilaterally hearing impaired children may have a risk for academic failure (5, 6). Therefore, it is necessary to clarify speech recognition ability of children with unilateral hearing loss and compare it with that of children with bilateral normal hearing under noisy environments like a classroom setting.

Nowadays, the primary educational recommendation for children with unilateral hearing loss is preferential classroom seating at a minimum distance from the teacher with the normal hearing ear oriented towards the teacher. When audiological management approach is recommended, a contralateral routing of signals (CROS)-type hearing aid is sometimes suggested to offer some benefit for children with unilateral hearing loss. However, a previous study reported that the device might worsen speech recognition in noisy

environments (7).

An alternative audiological approach to classroom management is the "FM system", a personal assistive device that is used as school-based intervention for children with hearing loss. The teacher wears a microphone, and the receiver is applied to the child's normal ear, so that the student can directly hear the teacher's voice. It was reported that regardless of the listening environment, the FM system improved speech recognition in individual children with unilateral hearing loss, compared with CROS (8). However, it is necessary to clarify whether the FM system improves speech recognition ability of children with unilateral hearing loss under noisy environments like a classroom setting.

In the present study, we examined speech recognition ability of elementary school-aged Japanese children with unilateral severe-to-profound sensorineural hearing loss under noisy environments and compared it with that of age-matched children with bilateral normal hearing. Moreover, we examined the effects of the FM system fitted into the normal hearing ear of children with unilateral hearing loss on improvement of their speech recognition ability under noisy environments similar to working elementary school classrooms in Japan.

## PATIENTS AND METHODS

### Patients

Both male and female elementary school-aged Japanese children were enrolled in the present study. Inclusion criteria : children were eligible if they could both pure-tone audiometry and speech recognition test securely. Exclusion criteria : children were excluded

Received for publication April 24, 2018 ; accepted June 4, 2018.

Address correspondence and reprint requests to Noriaki Takeda, M.D., Ph.D. Department of Otolaryngology, University of Tokushima School of Medicine, 3-18-15 Kuramoto, Tokushima 770-8503, Japan and Fax : +81-88-633-7170.

if they had complications other than hearing loss, such as Down syndrome.

The first group was made of twelve children with unilateral severe-to-profound sensorineural hearing loss defined as a pure tone average hearing level of more than 70 dB in one ear and normal hearing defined as a pure tone average hearing level of less than 25 dB in the opposite ear (4 males and 8 females, mean age :  $7.7 \pm 1.2$  years old). The second group was made of ten age-matched children with bilateral normal hearing defined as a pure tone average hearing level of less than 25 dB in both ear as a control (5 males and 5 females, mean age :  $8.1 \pm 1.9$  years old). They received speech recognition test in both quiet and noisy environments.

The third group was made of nine children with unilateral severe-to-profound sensorineural hearing loss, who were fitted with a FM receiver into the normal hearing ear (4 males and 5 females, mean age :  $8.6 \pm 1.8$  years old). They received speech recognition test with or without a FM receiver in both quiet and noisy environments.

The cause of unilateral severe-to-profound sensorineural hearing loss was unknown with the onset in early childhood in both first and third groups of children. No children had a diagnosis of mental retardation in all three groups.

The present study was approved by the Committee for Medical Ethics of Tokushima University Hospital, and a written informed consent was obtained from a parent of each child prior to the study.

#### Speech recognition test in noise

Speech recognition test in a sound field was performed in the audiometric test room of our otolaryngology clinic and correct rates of speech recognition were measured according to the guidelines for the evaluation of hearing aid fitting (2010) published by Japan Audiological Society (9). Japanese monosyllables from the 57-S word list made by Japan Audiological Society was used as the speech material (10). Each monosyllable was presented at 50 dB time-averaged SPL (sound pressure level) from a loudspeaker placed in front of a subject sitting at a distance of 80 cm in quiet environment. It was then presented in noise environments of 0 dB and -5 dB signal-to-noise ratio (SNR), where white noise (WN) was presented at 50 and 55 dB SPL from another loudspeaker placed behind the subject at a distance of 80 cm (Fig. 1A). Children were instructed to look at a soft toy on the front loudspeaker to avoid their head rotation during speech recognition test.

#### Speech recognition test in noise with FM system

The FM system used in the present study consisted of a radio transmitter with a microphone (Inspiro FM transmitter, Phonak Inc., Switzerland) and an open-fit FM receiver (iSense micro FM receiver, Phonak Inc., Switzerland). In the audiometric test room, the radio transmitter was placed at a distance of 20 cm in front of the loudspeaker facing subjects who were fitted with a FM receiver into the normal hearing ear, because in a classroom, the transmitter is hanging on the teacher's neck at a distance of 20 cm from the mouth. Japanese monosyllables from the 57-S word list were presented at 50 dB time-averaged SPL from the front loudspeaker facing a subject sitting at a distance of 80 cm in quiet environment. It was then presented in noisy environments of 0 dB and -5 dB SNR, where WN was presented at 50 and 55 dB SPL from another loudspeaker placed behind the subject at a distance of 80 cm (Fig. 1B). Children were instructed to look at a soft toy on the front loudspeaker to avoid their head rotation during speech recognition test.

#### Noise sound ratio in classroom

Although data logging system in the hearing aid varies considerably across hearing aid manufacturers, it keeps track of the dura-

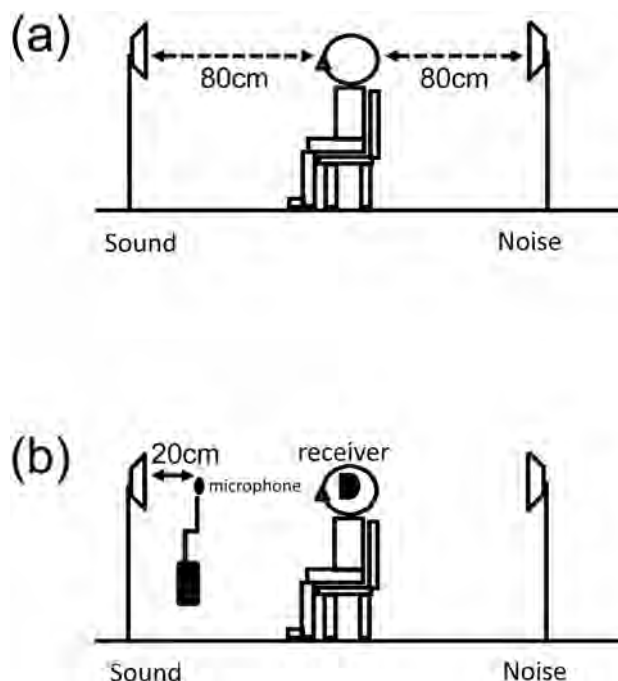


Fig. 1 a, b

Speech recognition test in noise without (a) and with (b) FM system. Japanese monosyllables were presented at 50 dB time-average SPL from the front loudspeaker and a white noise was presented at 50 or 55 dB SPL from the rear loudspeaker.

tion of hearing aid usage and the characteristics listening environments, such as quiet, speech, speech in noise and noise only (11). The data logging system in Oticon's Epoq XW hearing aid (Denmark) can track sound pressure levels of self-speech and ambient noise (12). In a preliminary study, five volunteers wore open-fit Oticon's Epoq XW hearing aid on the auricle without gain, and pronounced like a teacher in a quiet classroom. The sound pressure levels of self-speech obtained by the data logging system of the hearing aid was virtually equivalent to those measured by a sound level meter placed at a distance of 30 cm in front (data not shown). In Japanese elementary school classrooms, a typical preferred seating location for children with unilateral hearing loss is at a distance of 120 cm from the teacher. Theoretically, the sound decay is obtained by the following formula :  $-20 \times \log_{10} (A/B)$ , where A is 0.3 m and B is 1.2 m. Therefore, the sound levels of teacher's talk obtained by the data logging system will be attenuated with  $-20 \times \log_{10} (0.3/1.2) = -12.0$  dB at the preferred seats in Japanese elementary school classrooms. In the present study, averaged ambient noise levels in classrooms of six elementary schools in Tokushima prefecture of Japan and averaged speech levels of a teacher's talk for 50 min in each classroom were measured using the data logging system of open-fit Oticon's Epoq XW hearing aid on teacher's auricle without gain.

#### Statistical analysis

Statistical analysis was done using two-factor factorial analysis of variance and one factor analysis of variance with Scheffe's F post-hoc test (Statcel version 3, OMS Publishing Inc, Saitama, Japan).  $p < 0.05$  was considered statistically significant.

RESULTS

In the children with bilateral normal hearing, the correct rates of speech recognition test were  $89.8 \pm 3.8\%$  (n=10) in quiet,  $78.8 \pm 4.2\%$  (n=10) and  $70.4 \pm 6.4\%$  (n=10) in noisy environments of 50 and 55 dB WN, respectively. Thus, the correct rates of speech recognition test were significantly decreased in noisy environments of 0 and 5 dB SNR, compared with those in quiet environment in normal hearing children ( $p < 0.05$ ). In the children with unilateral severe-to-profound hearing loss, the correct rates of speech recognition test were  $87.3 \pm 5.5\%$  (n=12) in quiet,  $70.7 \pm 6.6\%$  (n=12) and  $57.3 \pm 8.8\%$  (n=9) in noisy environments of 50 and 55 dB WN, respectively. Thus, the correct rates of speech recognition test were also significantly decreased in noisy environments of 0 and -5 dB SNR, compared with those in quiet environment in unilateral hearing deficit children ( $p < 0.05$ ). However, in noisy environment of 55 dB WN (-5 dB SNR), the correct rates of speech recognition test in children with unilateral hearing loss were significantly decreased, compared those in children with bilateral normal hearing ( $p < 0.05$ ) (Fig. 2).

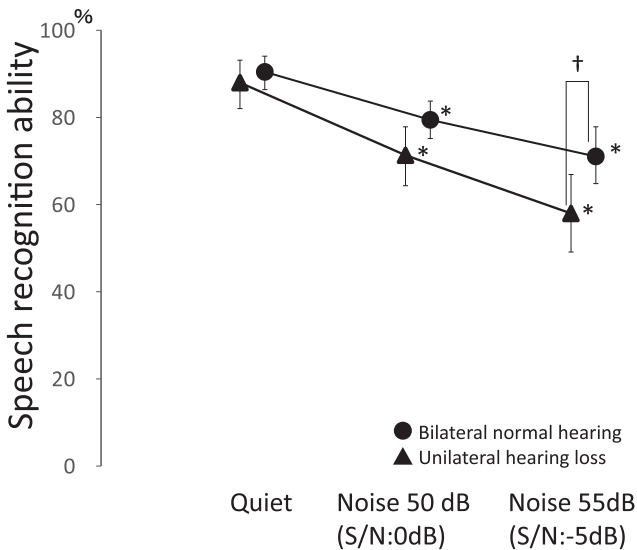


Fig. 2 Effects of noise on speech recognition ability in children with unilateral hearing loss and bilateral normal hearing. Triangles and circles represent children with unilateral hearing loss and with bilateral normal hearing, respectively. \* $p < 0.05$  vs. quiet, † $p < 0.05$  between groups. Data presented as mean  $\pm$  standard deviation.

In other unaided children with unilateral severe-to-profound hearing loss, the correct rates of speech recognition test were  $88.0 \pm 3.0\%$  (n=10) in quiet,  $64.0 \pm 12.3\%$  (n=10) and  $58.4 \pm 11.1\%$  (n=9) in noisy environments of 50 and 55 dB WN, respectively. Thus, the correct rates of speech recognition test were significantly decreased in noisy environments of 0 and -5 dB SNR, compared with those in quiet environment in unaided unilateral hearing deficit children. When they were aided by a FM receiver into the normal hearing ear, the correct rates of speech recognition test were  $89.2 \pm 4.0\%$  (n=10) in quiet,  $84.8 \pm 6.7\%$  (n=10) and  $78.7 \pm 6.4\%$  (n=9) in noisy environments of 50 and 55 dB WN, respectively. Thus, in children with unilateral hearing loss, the correct rates of speech

recognition test when aided were maintained in noisy environments of 50 and 55 dB WN (0 and -5 dB SNR) and significantly increased, compared those when unaided in the noisy environments ( $p < 0.01$ ) (Fig. 3).

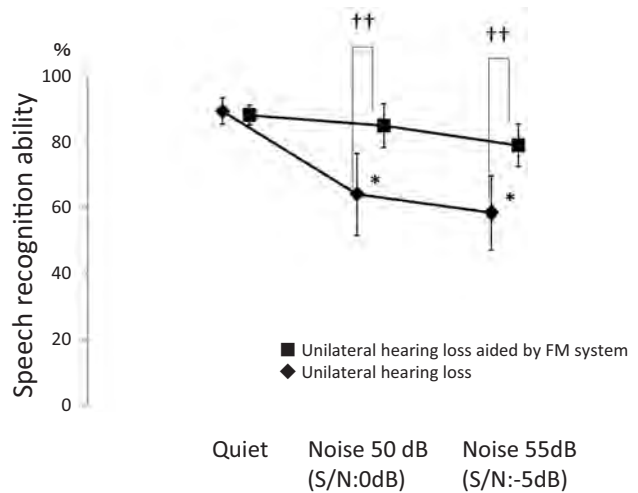


Fig. 3 Effects of FM system on speech recognition ability in noise in children with unilateral hearing loss. Diamonds and squares represent unaided and aided with Open-fit FM system into the normal hearing ear, respectively. \* $p < 0.05$  vs. quiet; †† $p < 0.01$  between unaided and aided with FM system. Data presented as mean  $\pm$  standard deviation.

The averaged noise level in six elementary school classrooms was 68.4 dB SPL, while the averaged speech level of teachers' talk in the classrooms was 73.5 dB SPL. Both levels were obtained by the data logging system of open-fit Oticon's Epoq XW hearing aid on teacher's auricle without gain. Since the sound pressure levels of teacher's talk were attenuated with a decrease of 12.0 dB at a typical preferred seating location (see Methods), an estimated speech level of 61.5 dB SPL would be delivered to students with hearing loss, resulting in -6.9 dB SNR in Japanese elementary school classrooms (Table 1).

DISCUSSION

In the present study, speech recognition ability of Japanese children with unilateral severe-to-profound hearing loss was similar to that of age-matched children with bilateral normal hearing in quiet and slight noisy (50 dB WN) environments. However, in louder noise environment of 55 dB WN, speech recognition ability of children with unilateral hearing loss decreased, compared with that of children with bilateral normal hearing. Since unilateral hearing loss is a disruption of binaural processing of the auditory system including binaural summation, head shadow effect and localization (2), it was reported that children with unilateral hearing loss encounter difficulty understanding speech under noisy environments (13, 14). A recent report also indicated that children with unilateral severe-to-profound hearing loss required at least 2-9 dB better SNR than children with normal hearing for understanding speech in noisy environments (15).

Typical classrooms have been found to have an SNR of +6 dB in USA and an SNR of +11 dB in Canada, which were calculated with

Table 1 Noise level and signal to noise ratio in classrooms

	School A	School B	School C	School D	School E	School F	average
Noise level in classroom	69.5	67.5	73.1	70.8	63.0	66.7	68.4 dB SPL
Level of teacher's talk	74.5	72.1	75.6	74.6	69.3	74.4	73.5 dB SPL
Estimated level of teacher's signal at preferential seat	62.5	60.1	63.6	62.9	57.3	62.4	61.5 dB SPL
Estimated S/N at preferential seat	-7.0	-7.4	-9.5	-7.9	-5.7	-4.3	-6.9 dB

S/N : signal to noise ratio.

background noise level in quiet classrooms (2, 16). However, in the present study, the acoustic condition in Japanese elementary school classrooms was a -6.9 dB SNR, which was calculated from ambient noise in the active classroom measured by the data logging system in Oticon's Epoq XW hearing aid. Since even in normal hearing, younger children require a greater SNR than older children when listening in noise (17), it is suggested that hearing assistive devices are needed for Japanese elementary school children with unilateral hearing loss in noisy environments, particularly in a classroom.

In the present study, a FM receiver fitted into the normal hearing ear improved the speech recognition ability of children with unilateral hearing loss in noisy environment of 55 dB WN like the listening condition in Japanese elementary school classrooms. CROS and bone-anchored hearing aids (BAHA) (18, 19) may be used as another audiological management for children with unilateral hearing loss in noisy classrooms. They can make use of neurophysiological mechanisms of binaural hearing and improve the hearing ability of children with unilateral hearing loss in noisy environments (20). On the other hand, the FM system picks up relevant teacher's voice in a short distance and delivers it to the listener's ear through radio waves that do not interfere with surrounding ambient noises. The FM system can directly improve the SNR of auditory signals. Moreover, it has no side effect contrary to the BAHA implantation that needs an invasive procedure and occasionally causes post-operative complications such as skin irritation and failure of osseointegration (21). In fact, a previous study reported that the FM system improved the word recognition of children with unilateral hearing loss in the typical classroom acoustic condition of +6 dB SNR in USA, compared with CROS and conventional hearing aids (8). Taken together, the findings of the present study also suggest that the FM system is recommended as an audiological management for improvement of speech recognition in noisy elementary school classrooms for Japanese children with unilateral hearing loss. But, children with unilateral hearing loss may encounter difficulty in hearing classmate's talk during they are hearing teacher's talk using FM system, although inactive open-fit FM receiver on the normal hearing ear does not interfere in listening classroom discussion.

## CONCLUSION

The present study demonstrated that the FM system that consists of a microphone worn by the teacher and a receiver applied to the student's normal ear overcomes the listening difficulties of children with unilateral severe-to-profound hearing loss in noisy elementary school classrooms in Japan. In Tokushima prefecture of Japan, about 75% of children with unilateral hearing loss pre-

ferred to use the FM system in classrooms, probably because they felt some benefit for classroom instructions and discussions. The beneficial effects of the FM system need to be examined in children with varying degrees and types of unilateral hearing loss and in various noise conditions. Further research should also include a comparison between the FM system and BAHA as an audiological management for children with unilateral severe-to-profound hearing loss.

## CONFLICT OF INTEREST

The authors declare no conflicts of interest.

## ACKNOWLEDGEMENTS

The authors thank Professor Bukasa Kalubi for his critical reading of the manuscript.

## REFERENCES

1. Bess FH, Tharpe AM : An introduction to unilateral sensorineural hearing loss in children. *Ear Hear* 7 : 3-13, 1986
2. Bess FH, Tharpe AM, Gibler AM : Auditory performance of children with unilateral sensorineural hearing loss. *Ear Hear* 7 : 20-26, 1986
3. Bess FH, Klee T, Culbertson JL : Identification, assessment, and management of children with unilateral sensorineural hearing loss. *Ear Hear* 7 : 43-51, 1986
4. Lieu JE, Tye-Murray N, Karzon RK, Piccirillo JF : Unilateral hearing loss is associated with worse speech-language scores in children. *Pediatrics* 125 : e1348-1355, 2010
5. Bess FH, Tharpe AM : Unilateral hearing impairment in children. *Pediatrics* 74 : 206-216, 1984
6. Lieu JE : Speech-language and educational consequences of unilateral hearing loss in children. *Arch Otolaryngol Head Neck Surg* 130 : 524-530, 2004
7. Shapiro I : Children's use of CROS hearing aids. *Arch Otolaryngol* 103 : 712-716, 1977
8. Updike CD : Comparison of FM auditory trainers, CROS aids, and personal amplification in unilaterally hearing impaired children. *J Am Acad Audiol* 5 : 204-209, 1994
9. Kadera K, Hosoi H, Okamoto M, Manabe T, Kanda Y, Shiraishi K, Sugiuchi T, Suzuki K, Tauchi H, Nishimura T, Matsuhira T, Ishikawa K : Guidelines for the evaluation of hearing aid fitting (2010). *Auris Nasus Larynx* 43 : 217-228, 2016
10. Japan Audiological Society : Speech audiometry *Audiol Jpn*

- 46 : 622-637, 2003
11. McCreery R : Data Logging and Hearing Aid Use : Focus on the Forest, Not the Trees. *Hearing J* 66 : 18-19, 2013
  12. <http://www.audiologyonline.com/articles/incorporating-sound-activity-meter-into-987>
  13. Kenworthy OT, Klee T, Tharpe AM : Speech recognition ability of children with unilateral sensorineural hearing loss as a function of amplification, speech stimuli and listening condition. *Ear Hear* 11 : 264-270, 1990
  14. Reeder RM, Cadieux J, Firszt JB : Quantification of speech-in-noise and sound localisation abilities in children with unilateral hearing loss and comparison to normal hearing peers. *Audiol Neurootol* 20 ; Suppl 1 : 31-37, 2015
  15. Ruschetta MN, Arjmand EM, Pratt SR : Speech recognition abilities in noise for children with severe-to-profound unilateral hearing impairment. *Int J Pediatr Otorhinolaryngol* 69 : 771-779, 2005
  16. Sato H, Bradley JS : Evaluation of acoustical conditions for speech communication in working elementary school classrooms. *J Acoust Soc Am* 123 : 2064-2077, 2008
  17. Bradley JS, Sato H : The intelligibility of speech in elementary school classrooms. *J Acoust Soc Am* 123 : 2078-2086, 2008
  18. Stewart CM, Clark JH, Niparko JK : Bone-anchored devices in single-sided deafness. *Adv Otorhinolaryngol* 71 : 92-102, 2011
  19. Dornhoffer JR, Dornhoffer JL : Pediatric unilateral sensorineural hearing loss : implications and management. *Curr Opin Otolaryngol Head Neck Surg* 24 : 522-528, 2016
  20. Christensen L, Richter GT, Dornhoffer JL : Update on bone-anchored hearing aids in pediatric patients with profound unilateral sensorineural hearing loss. *Arch Otolaryngol Head Neck Surg* 136 : 175-177, 2010
  21. Kiringoda R, Lustig LR : A meta-analysis of the complications associated with osseointegrated hearing aids. *Otol Neurotol* 34 : 790-794, 2013