

## Evaluation of Chirp and Binary Codes based Excitation Pulses for 3D USCT

M. Zapf, B.F. Derouiche, N.V. Rüter

Forschungszentrum Karlsruhe GmbH, Institute for Data Processing and Electronics, Karlsruhe, Germany

### Background

at Forschungszentrum Karlsruhe we are developing a new imaging method for early breast cancer detection: 3D ultrasound computer tomography (3D USCT)

### USCT concept

- 3D SAFT with unfocused spherical waves emitted and received by single transducers.
- multistatic ellipsoid aperture 17cm x 12cm x 12cm, lift- and rotatable
- aperture walls lined with hundreds of transducers
- transducers with resonance frequency of 2.8 MHz and an opening angle of  $\pm 23^\circ$  at -6dB




Figure 2: Emitter excitation pulse damped sine pulse




Figure 1: Current status of the aperture of the 3D USCT demonstrator of 2nd generation, right-bottom: 2nd generation prototype transducer

### Challenge: low signal SNR

- unfocused emission and reception
- long traveling distances in 3D aperture
- for wide opening angle of transducers small active transducer area
- in designated medical application strong frequency damping

### Approach

- advanced coded excitation techniques known from radar
- basic idea: prolonging the excitation pulse for higher energy, followed by pulse compression
- matched filtering (optimal filter) for pulse compression
- usage of frequency modulated chirps
- usage of phase encoded binary codes: Barker codes
- usage of complementary binary codes: Golay codes




Figure 3: Chirp: top: linear frequency modulated chirp pulse, bottom: the time compressed matched filtered pulse

Length	Code	PSL [dB]
2	+-	-6.0
3	++-	-9.0
4	+++-	-12.0
5	++++-	-14.0
7	+++++-	-16.0
11	+++++--	-20.0
13	+++++--+	-22.5

Table 1: Barker binary codes of various lengths, on the right is given the nominal peak-sidelobe level (PSL)

Length	A (A')	B (B')
2	+-	-+
4	+++-	-+--
8	++++-+	-+----
16	+++++--+	-+-----

Table 2: Golay complementary binary codes of different lengths, A and B as signal sequence and A' and B' as corresponding matched filters




Figure 4: Barker binary code: (a) damped sine base pulse, (b) Barker of length 13, (c) convolved signal, (d) time-compressed by matched filtering




Figure 5: Golay complementary binary codes of different lengths, A and B as signal sequence and A' and B' as corresponding matched filters

## Methods

### Measurement setup

- water filled container (45x30x30cm<sup>3</sup>)
- 3D USCT 2nd generation prototype transducer with 2.8 MHz resonance frequency and 2 MHz (-6 dB) bandwidth
- 3D movable hydrophon-arm (Onda HNC-400)
- LabWindows based DAQ and control-software
- PC based Gage digitization card (20MHz)
- Tronix AWG 2021 (arbitrary-wave-generator)




Figure 7: Measurement setup. Left: water container with hydrophone arm movable by three axes. Right: AWG (arbitrary wave generator).



Figure 8: castor oil phantom




Figure 6: Schematic of measurement setup

### Empty measurement

- to simulate the multistatic 3D USCT aperture and evaluate signal processing and transducers
- measurement was done for varying angular position of the hydrophone

### Phantom measurement

- breast tissue mimicking phantom
- consist of a bottle (wall thickness  $< \lambda/4$ ) with dimensions 34cm x 8cm x 8cm filled with castor oil, frequency damping 0.72 dB/(MHz\*cm)

### Evaluated pulses

- simple pulse and linear chirp pulse
- Barker of length 13 and Golay of length 16, both convoluted with the sine pulse

## Results

### Evaluation

application to the USCT setup and designated medical application is evaluated with well-established metrics SNR, GSNR, PSL, and ISL:

Empty measurement	Golay Code 16	Barker Code 13	Chirp Pulse	Sine Pulse
SNR [dB]	56	33	26	12
GSNR [dB]	31	30	16	31
PSL [dB]	-39	-20	-31	-
ISL [dB]	-14	-16	-17	-

Table 3: Scores for different excitation pulses and the empty measurement setup, signal center frequency 1 MHz and bandwidth 0.25 MHz, measurements were averaged 512 times




Figure 9: SNR for empty measurement for varying angular positions, center frequency 2.8 MHz and bandwidth 1.0 MHz, measurements were averaged 512 times

Phantom measurement	Golay Code 16	Barker Code 13	Chirp Pulse	Sine Pulse
SNR [dB]	42	26	19	6
GSNR [dB]	29	27	13	-
PSL [dB]	-28	-13	-21	-
ISL [dB]	-8	-0.5	-6	-

Table 4: Scores for different excitation pulses and phantom measurement setup, signal center frequency 1 MHz and bandwidth 0.25 MHz, measurements were averaged 512 times

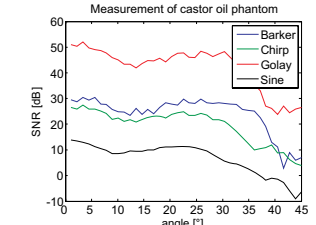


Figure 10: SNR for phantom experiment for varying angular positions, center frequency 1.0 MHz and bandwidth 0.25 MHz, measurements were averaged 512 times

## Discussion

- techniques are suitable to the USCT setup and designated medical application
- Golay complementary code is a promising option for extending SNR, but downside doubled measurement time
- Barker is also a promising option without this downside

### Outlook

- further evaluations are required for analyzing the tissue depended frequency dispersion

KIT – The Consortium of: