

Dichroism-sensitive photoacoustic computed tomography: supplementary material

YUAN QU,^{1†} LEI LI,^{2†} YUECHENG SHEN,² XIAOMING WEI,² TERENCE T.W. WONG,^{1,2} PENG HU,¹ JUNJIE YAO,^{1‡} KONSTANTIN MASLOV,² AND LIHONG V. WANG^{2*}

¹Department of Biomedical Engineering, Washington University in St. Louis, St. Louis, Missouri 63130, USA

²Caltech Optical Imaging Laboratory, Andrew and Peggy Cherng Department of Medical Engineering and Department of Electrical Engineering, California Institute of Technology, Pasadena, California 91125, USA

[‡]Current address: Photoacoustic Imaging Laboratory, Department of Biomedical Engineering, Duke University, Durham, NC 27708, USA

[†]These authors contributed equally to this work.

*Corresponding author: LVW@caltech.edu

Published 18 April 2018

This document provides supplementary information to “Dichroism-sensitive photoacoustic computed tomography,” <https://doi.org/10.1364/OPTICA.5.000495>.

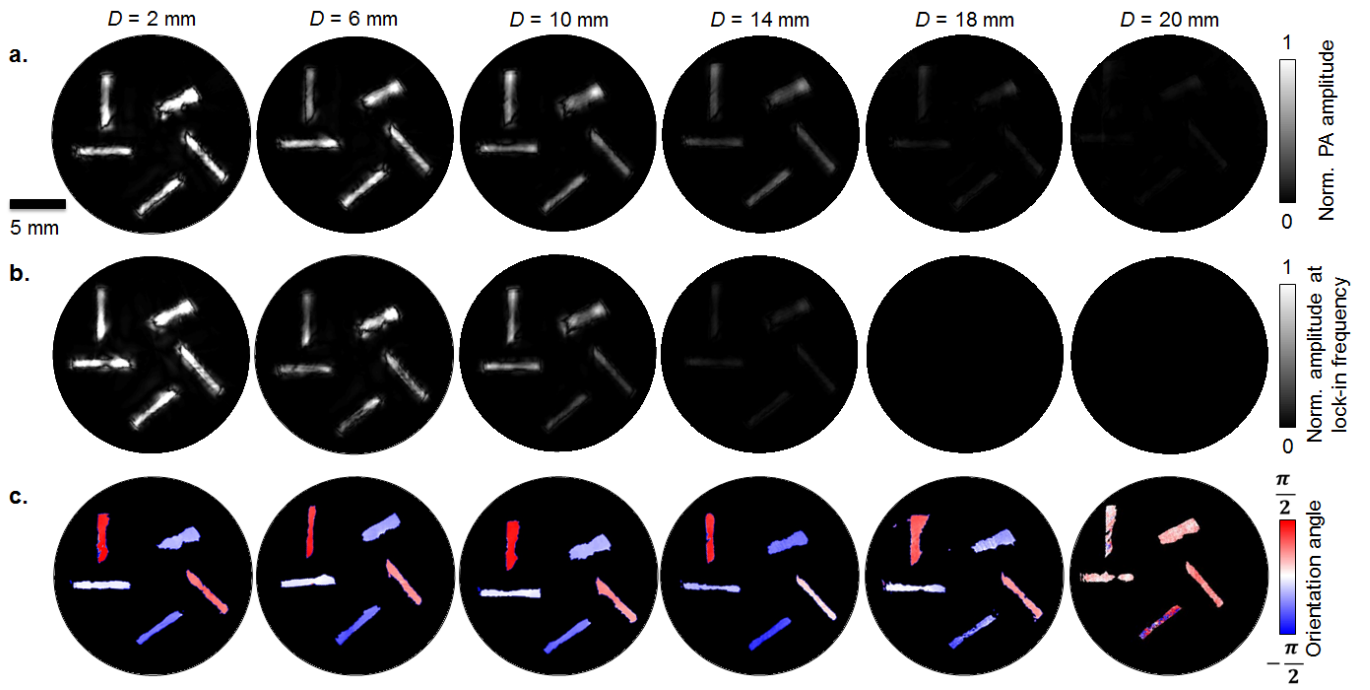


Fig. S1. DS-PACT of the linear polarizers. The sample contains five linear polarizers placed at different orientations. (a) Conventional PACT images, (b) amplitude images using DS-PACT, and (c) orientation angle maps of the linear polarizers at multiple depths.