

SERI/TP--215-4063

SERI/TP-215-4063
UC Categories: 270, 233
DE91002119

DE91 002119

**Photovoltaic Advanced
Research and Development
Project: Solar Radiation
Research Annual Report**

**1 October 1989 - 30 September
1990**

**C. Riordan
R. Hulstrom
T. Cannon
D. Myers
T. Stoffel**

November 1990

Prepared under Task No. PV110201

Solar Energy Research Institute
A Division of Midwest Research Institute

1617 Cole Boulevard
Golden, Colorado 80401-3393

Prepared for the
U.S. Department of Energy
Contract No. DE-AC02-83CH10093

MASTER

DISTRIBUTION OF THIS DOCUMENT IS UNLIMITED

NOTICE

This report was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or any agency thereof.

Printed in the United States of America
Available from:
National Technical Information Service
U.S. Department of Commerce
5285 Port Royal Road
Springfield, VA 22161

Price: Microfiche A01
Printed Copy A03

Codes are used for pricing all publications. The code is determined by the number of pages in the publication. Information pertaining to the pricing codes can be found in the current issue of the following publications which are generally available in most libraries: *Energy Research Abstracts (ERA)*; *Government Reports Announcements and Index (GRA and I)*; *Scientific and Technical Abstract Reports (STAR)*; and publication NTIS-PR-360 available from NTIS at the above address.


PREFACE

This report gives an overview of the fiscal year 1990 research activities and results under the Solar Radiation Research Task of the Photovoltaics Advanced Research and Development Project at the Solar Energy Research Institute. The activities under this task include developing and applying measurement techniques, instrumentation, and data and models to understand and quantify the response of photovoltaic devices to variations in broadband and spectral solar radiation.

The information presented in this report was presented at the SERI Photovoltaic Advanced Research and Development Project 10th Review Meeting, October 1990, and will be published in a special Solar Cells issue dedicated to the meeting.

Approved for the

SOLAR ENERGY RESEARCH INSTITUTE



R.L. Hulstrom, Manager
 Solar Radiation Research and Metrology
 Branch



J.L. Stone, Director
 Solar Electric Research Division

TABLE OF CONTENTS

	<u>Page</u>
1.0 Introduction	1
2.0 Atmospheric Optical Calibration System	2
3.0 Spectroradiometry	5
4.0 Plane-of-Array Solar Irradiance Measurements	8
5.0 Device Spectral Sensitivity and Measurement Techniques	13
6.0 Measurement Support and Technology Transfer	15
7.0 Summary and Future Plans	16
8.0 References	18

LIST OF FIGURES

	<u>Page</u>
2-1. Schematic of the AOCS components and photos of the AOCS direct-beam module	2
2-2. Water vapor absorption for different amounts of water vapor, simulated using a spectral irradiance model	4
3-1. Comparison of SERI's SPIRE 240A pulse simulator with the American Society for Testing and Materials air mass 1.5 global standard spectrum	6
4-1. Cloudiness index (K_t) map for the United States	9
4-2a. Ratios for global POA irradiance for 5 flat-plate collector options, divided by direct-normal POA irradiance	10
4-2b. Ratios for global POA irradiance for 4 flat-plate tracking options, divided by global POA irradiance for a flat plate with a fixed tilt at the latitude	11
4-2c. Ratios for global POA irradiance for a two-axis tracking flat plate, divided by global POA irradiance for three 1-axis tracking options	12
5-1. Total irradiance and the ratio of NIR to total irradiance on a clear day in Golden, Colorado, for direct-normal and global-horizontal cases	14
5-2. Total irradiance and the ratio of NIR to total irradiance on a partly cloudy day in Golden, Colorado, for direct-normal and global-horizontal cases	14

1.0 INTRODUCTION

The purpose of the Solar Radiation Research Task under the Photovoltaic Advanced Research and Development Project at the Solar Energy Research Institute is to support the national photovoltaics (PV) program by helping to develop a fundamental scientific understanding of the relationships between the natural broadband and spectral solar radiation environment and the design, performance, and performance measurements of PV devices. The task addresses the needs expressed by the PV community for instrumentation, data and models, and measurement and analysis techniques to understand the response of PV devices to variations in broadband and spectral solar radiation [1-3].

This report overviews the key activities and results in fiscal year 1990 under the Solar Radiation Research Task. The activities include further developing the Atmospheric Optical Calibration System (AOCS), spectroradiometry, plane-of-array (POA) solar irradiance measurements, PV device spectral sensitivity and measurement techniques, and measurement support and technology transfer.

2.0 ATMOSPHERIC OPTICAL CALIBRATION SYSTEM

The AOCS (shown in Figure 2-1) is an instrument designed to provide real-time information on atmospheric optical conditions, such as haziness (turbidity) and water vapor, and solar radiation conditions that affect PV device performance during outdoor tests [4,5]. A patent, No. 4,779,980, was issued on the system on October 25, 1988. A prototype AOCS working unit (including basic software) was designed and constructed in 1988, followed by extensive laboratory testing in 1989. In 1990, the AOCS working unit was calibrated and tested outdoors, and additional software was also developed. Outdoor calibrations were performed for the narrow-wavelength (10-nm) channels at 368 nm, 500 nm, and 862 nm; data from these channels are used to calculate atmospheric aerosol effects (turbidity). Very repeatable calibration factors were obtained (0.5%



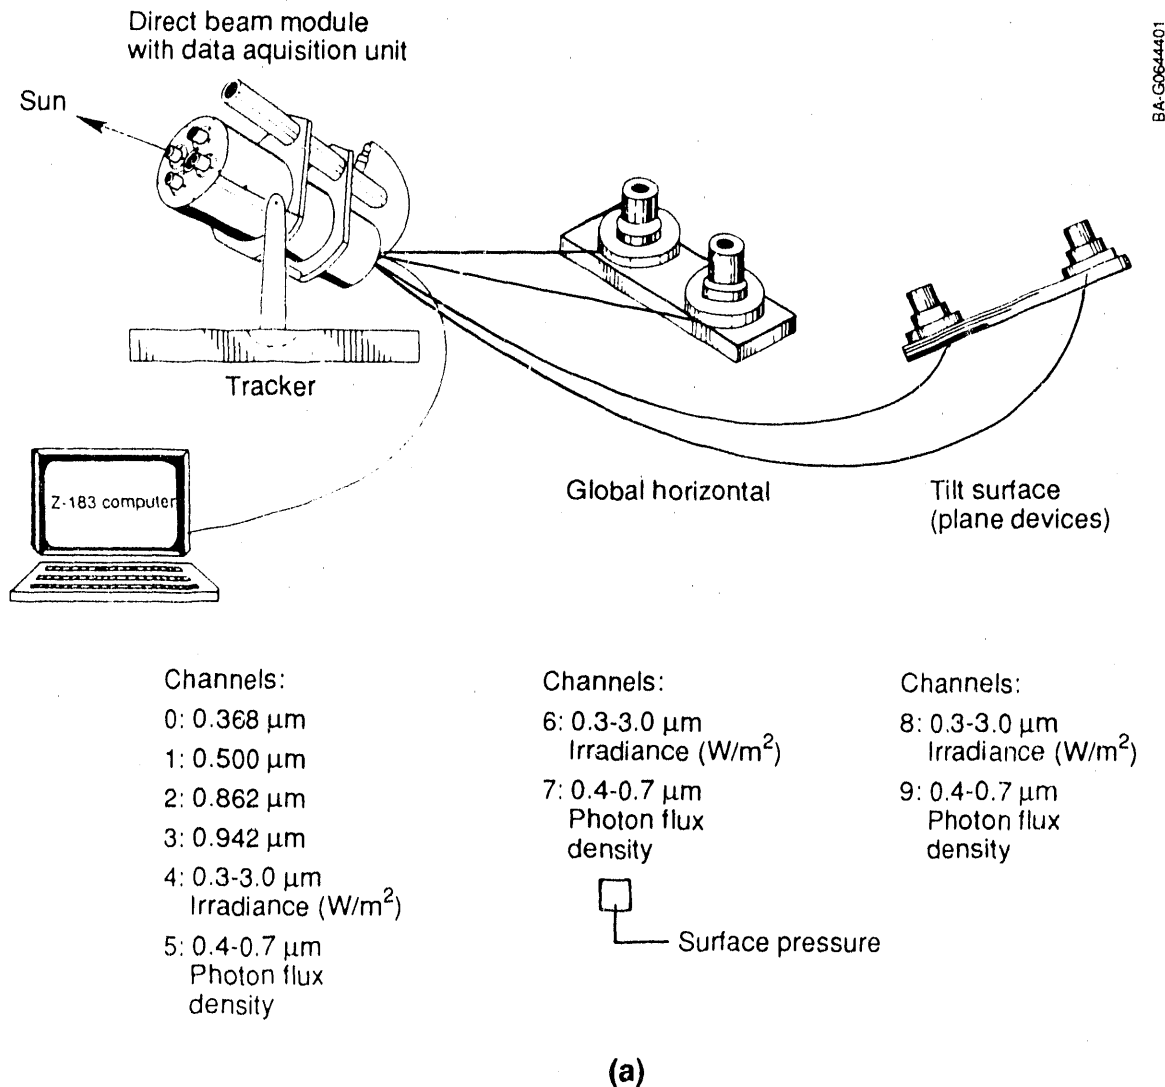


Figure 2-1. Schematic of the AOCS components (a) and photos of the AOCS direct-beam module (b,c)

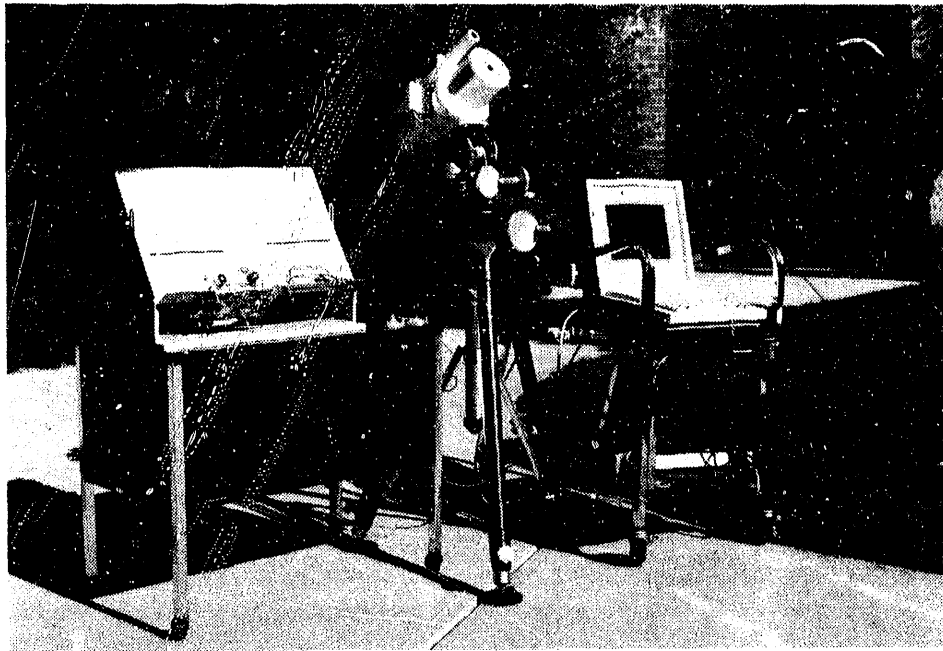

(b)

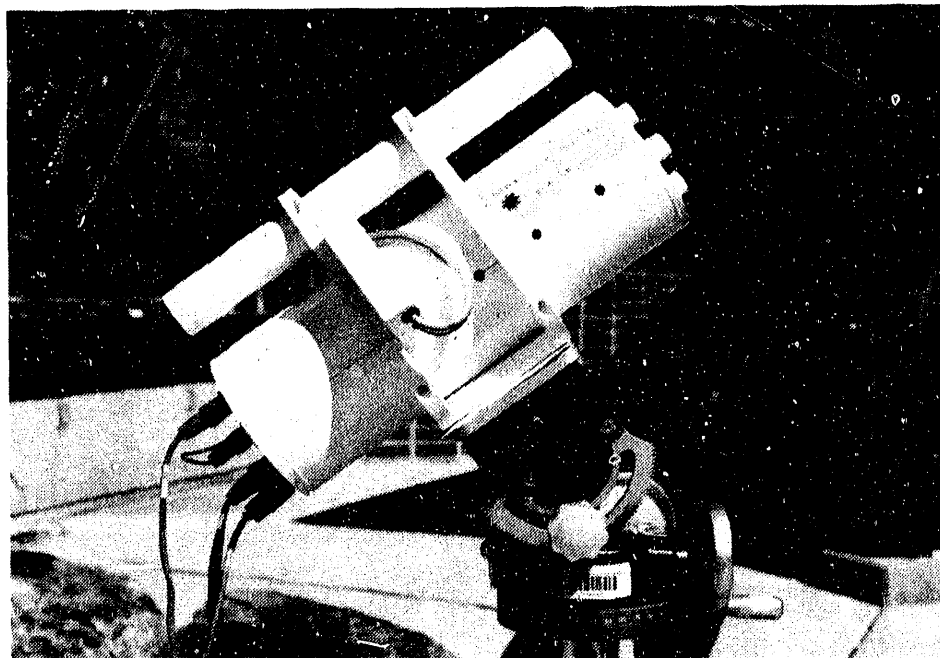

(c)

Figure 2-1. Schematic of the AOCS components (a) and photos of the AOCS direct-beam module (b,c) (concluded)

to 3% standard deviation, depending on the channel), which is important for maximizing the sensitivity of these channels to the atmospheric aerosol effects. Software was written so that the calibration data can be acquired with the AOCS in an unattended mode; this allows the operator to check the calibration frequently when the AOCS is operated routinely. Additional software is being added to temperature correct the AOCS data based on laboratory test data.

A major research activity in the final AOCS software development is modifying an algorithm to calculate precipitable water vapor from AOCS data at 862 nm (outside the absorption bands for atmospheric water vapor) and 942 nm (inside a water-vapor absorption band). A measure of water vapor is important because most atmospheric water vapor absorption occurs in the near-infrared (NIR) region of the spectrum (see Figure 2-2); therefore, it affects the relative spectral irradiance distribution between the visible and NIR regions. The effects of water vapor variations on a PV device depend on the device's spectral response. If the spectral response of a PV device extends into the NIR region, the device's short-circuit current will be affected by water vapor variations. If the spectral response of a PV device does not extend into the NIR region, the calculated device efficiency will be affected by water vapor variations because the total irradiance (the denominator in efficiency calculations) will vary.

In 1990, we obtained balloon sonde data from the National Oceanic and Atmospheric Administration (NOAA). We are using the data to examine how sensitive atmospheric water vapor transmittance is to the vertical profile of water vapor, temperature, and pressure, as well as to surface temperature and pressure. The algorithm in the AOCS software for calculating the transmittance of atmospheric water vapor requires fixed pressure and temperature values, so the results of this study are important for understanding the sensitivity and accuracy of the AOCS water vapor calculation.

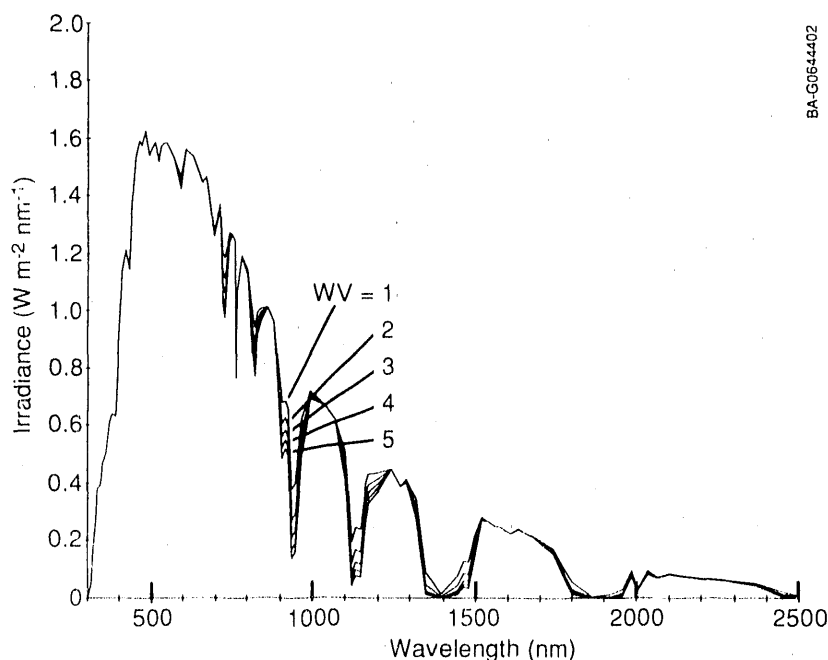


Figure 2-2. Water vapor absorption for different amounts of water vapor, simulated using a spectral irradiance model

3.0 SPECTRORADIOMETRY

PV cell efficiency measurements are usually referenced to a particular spectrum so that results can be compared among various laboratories. Spectral irradiance is measured during the cell performance tests and is used to translate the test results to the reference spectrum. Spectroradiometers with a wavelength range of 290-4000 nm are desirable to cover the wavelength response of all PV devices and to integrate the entire solar spectrum to obtain total irradiance. Otherwise, models must be used to extend the measured spectrum to cover the entire spectral region.


A technical challenge in spectroradiometry for PV applications is to develop an extended wavelength spectroradiometer with a fast time response (a millisecond for measuring flash simulators to less than 1 minute to measure outdoor spectra) with repeatability and accuracy within at least 5% (ideally 1%) over the entire spectral range. In addition, different front-end optics are needed for outdoor solar spectral irradiance measurements of the sun's disk (direct-beam irradiance in a 5° field of view) or the sky hemisphere (global irradiance from the sky hemisphere, with the direct beam at various incidence angles), without compromising the spectral measurement accuracy.

Spectroradiometers with user-friendly operating software are commercially available to measure the range 400-1100 nm with a wavelength-dependent accuracy of approximately 3%-10%. At SERI, we are currently using these spectroradiometers with a view-limiting tube (which restricts the field of view to match that of the absolute cavity radiometer) to measure direct-beam solar spectral irradiance during outdoor PV tests, and we also use a model to extend the measurements beyond 1100 nm [6].


Solar spectral irradiance measurements outside the wavelength range 400-1100 nm are more difficult and require more complex spectroradiometers. We are pursuing two options at SERI. One is to modify a spectroradiometer originally designed for geophysical applications. We are currently using this instrument to measure simulator spectral irradiance between 300 and 3000 nm in a single scan that takes about 3.5 minutes.

The measurement accuracy of this instrument is acceptable (better than 5%), except in the ultraviolet region. An integrating sphere was designed for the unit, but signal levels using the sphere have not been acceptable and therefore more work is needed. Work on this instrument has been temporarily delayed to pursue a second option, which is to develop an EG&G optical multichannel analyzer (OMA III) for solar spectral measurements.

The OMA uses a 1024-element Si (285-1100 nm spectral range) detector array, which allows all wavelengths to be measured simultaneously in less than 1 millisecond. A separate 256-element GaInAs detector array allows the 800-1750 nm spectral range of the pulsed simulators to be measured. This has the advantage over the conventional spectroradiometer of allowing accurate measurements of pulse sources as well as spectrally unstable outdoor conditions. A measurement of SERI's SPIRE 240A pulse simulator is shown together with the American Society for Testing and Materials (ASTM) air mass 1.5 global standard spectrum (E892-87) in Figure 3-1. Integrating the simulator spectrum over the ASTM E927 solar simulation standard band widths

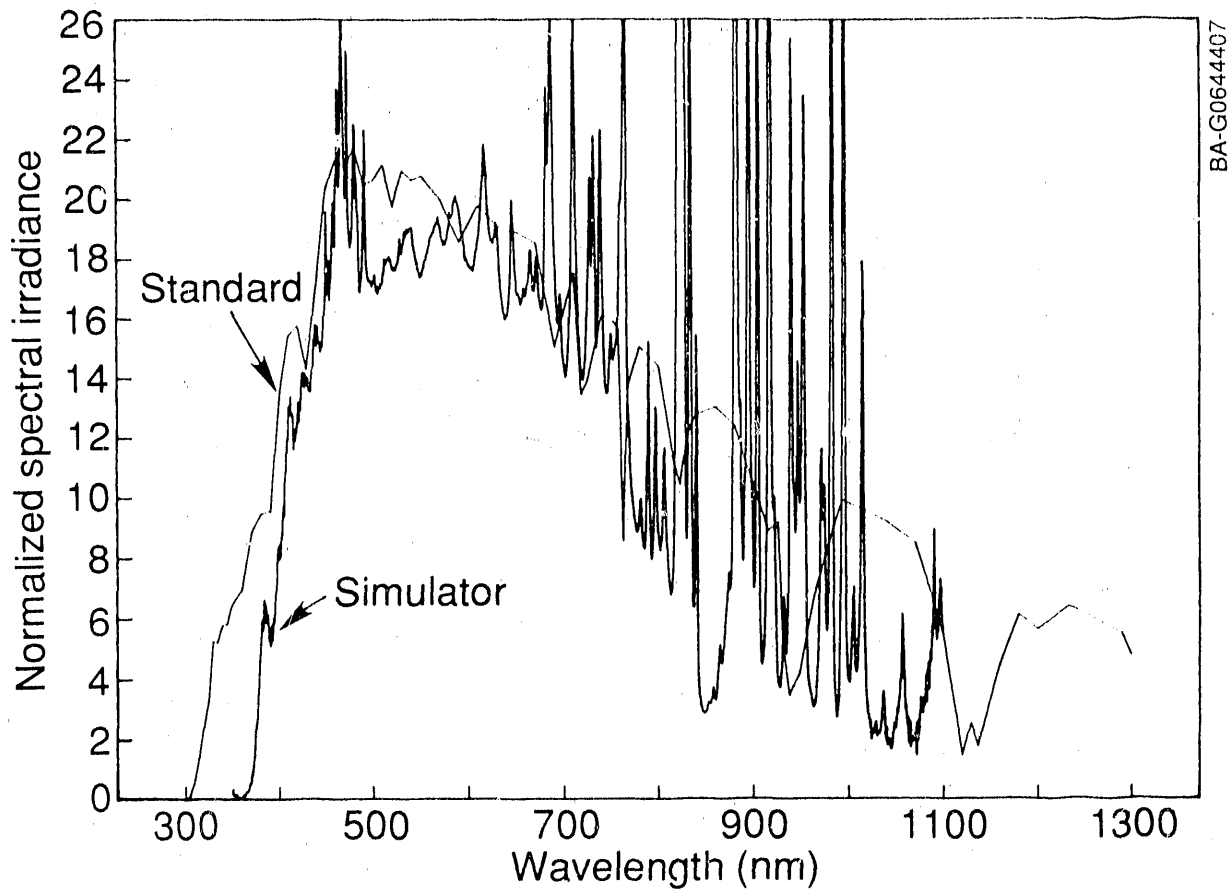

BA-G0644407

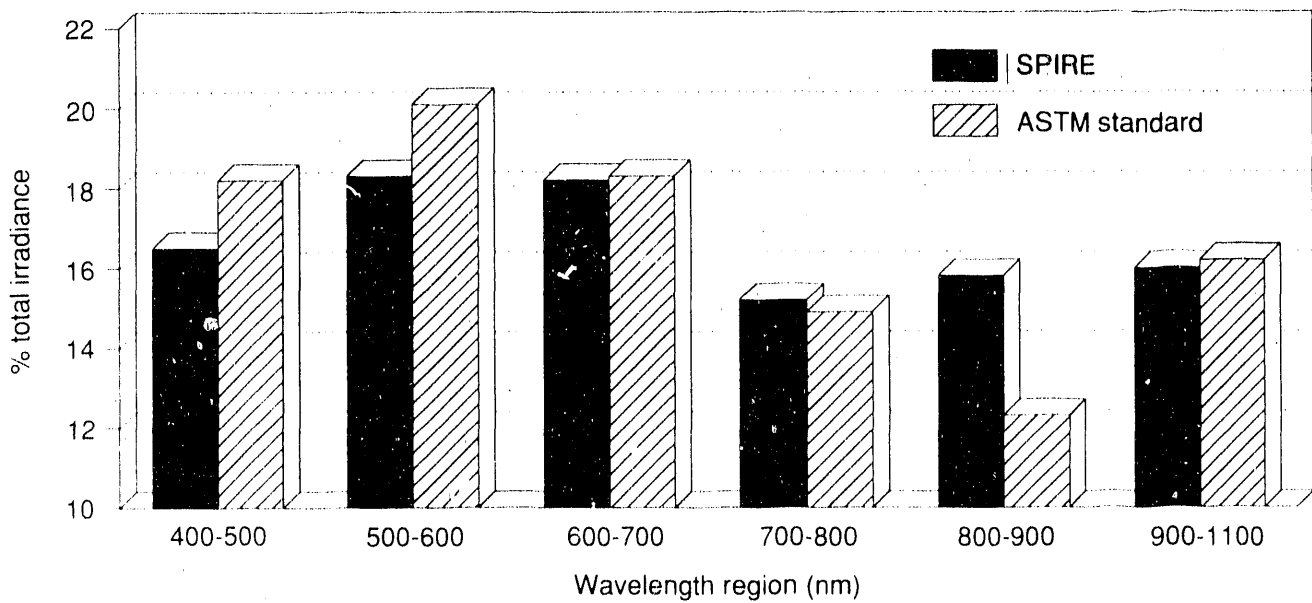

BA-G0657501

Figure 3-1. Comparison of SERI's SPIRE 240A pulse simulator with the American Society for Testing and Materials air mass 1.5 global standard spectrum

shows that the SPIRE simulator meets Class A spectral-content requirements, except in the region 800-900 nm, where the differences are probably within the measurement uncertainty.

Calculating the spectral measurement uncertainty for spectroradiometers is a complex, non-standard procedure [7,8]. To assess the state of the art in spectral measurement uncertainty, we participated in (and helped sponsor) a spectroradiometer intercomparison at DSET Laboratories in Phoenix, Arizona, in April 1990. The participants included experts from four environmental testing laboratories in the United States, as well as from SERI and the National Institute of Standards and Technology. In brief, the objectives of the intercomparison were to compare measurement results from SERI spectroradiometers with results from other laboratories; gather experts together from a few laboratories to improve spectroradiometry information transfer; provide an opportunity to acquire some of the measurements required to begin developing national and international spectroradiometry standards; and improve and document procedures for conducting spectroradiometer intercomparisons.

During the intercomparison, outdoor solar spectral measurements were taken in global and direct-normal modes, and indoor measurements were taken of two ultraviolet enhanced fluorescent sources and three phosphor colors. All results of this intercomparison are confidential at this time; certain results will be released at a later date.

4.0 PLANE-OF-ARRAY SOLAR IRRADIANCE MEASUREMENTS

A key variable in systems analysis of various PV collector options (concentrators, two-axis and one-axis tracking flat plates, and fixed-tilt flat plates) is the POA irradiance. Systems analysis, with irradiance as one of the input variables, is used to compare the cost of more expensive and complex collector options (like two-axis tracking compared to fixed tilt) with the value of increased PV power output resulting from the irradiance enhancement.

In 1990, we examined data, from various published studies and outdoor measurement programs, on POA irradiance or PV energy output (which is dominated by POA irradiance) to show the relationship between potential irradiance enhancements for various collector options and site cloudiness. Ratios of POA irradiance for pairs of collector options indicate potential enhancements [for example, 7.5 kilowatt-hours per square meter per day (kWh/m²/d) divided by 7.0 kWh/m²/d is 1.07, or an enhancement of 7%]. As a measure of site cloudiness, we used a variable called the cloudiness index (K_t), which is global-horizontal irradiance divided by extraterrestrial irradiance on a horizontal surface. This variable is a measure of bulk atmospheric transmittance, which varies with different atmospheric conditions. K_t varies with sun angle (or air mass), but its average annual value is dominated by the site's cloudiness. A map of the average annual K_t for the United States [10] is shown in Figure 4-1.

Annual average daily global POA irradiance values calculated by Sandia National Laboratories [9] for different types of collector options are divided by direct-normal values from the Sandia report, and the ratios are shown in Figure 4-2(a) as a function of average annual K_t . A simple regression of the irradiance ratios and K_t shows the strong inverse relationship. As expected, the ratio of global POA irradiance to direct-normal POA irradiance is a strong function of cloudiness because there is no direct-beam irradiance when the sky is overcast. The ratios of pairs of global POA irradiance values (Figure 4-2 b,c) show less K_t dependence than the ratios for global compared to direct normal. The quadratic fits to the global ratios as a function of K_t do not have high correlation coefficients because there is much scatter in the ratios; however, they do show relative trends in the data and the magnitude of potential irradiance enhancements.

For broad-scale assessments of potential POA irradiance enhancements in various climate regions of the United States, one can use the K_t map (Figure 4-1) with average enhancement factors versus K_t (Figure 4-2). This method is by no means appropriate for site-specific analysis. In all cases of site-specific economic systems analysis, one should obtain local (regional) irradiance data and calculate (or use measured) POA irradiance for each collector option, including flat plates with optimized tilt angles (instead of tilt = latitude) and concentrators with specific apertures and concentration ratios. The POA irradiance data should be combined with other data, such as reflection losses at non-zero incidence angles [12], to obtain the most reliable comparison of collector options. Seasonal variations in the enhancements should be analyzed, especially for evaluating the electric load matching potential of PV.

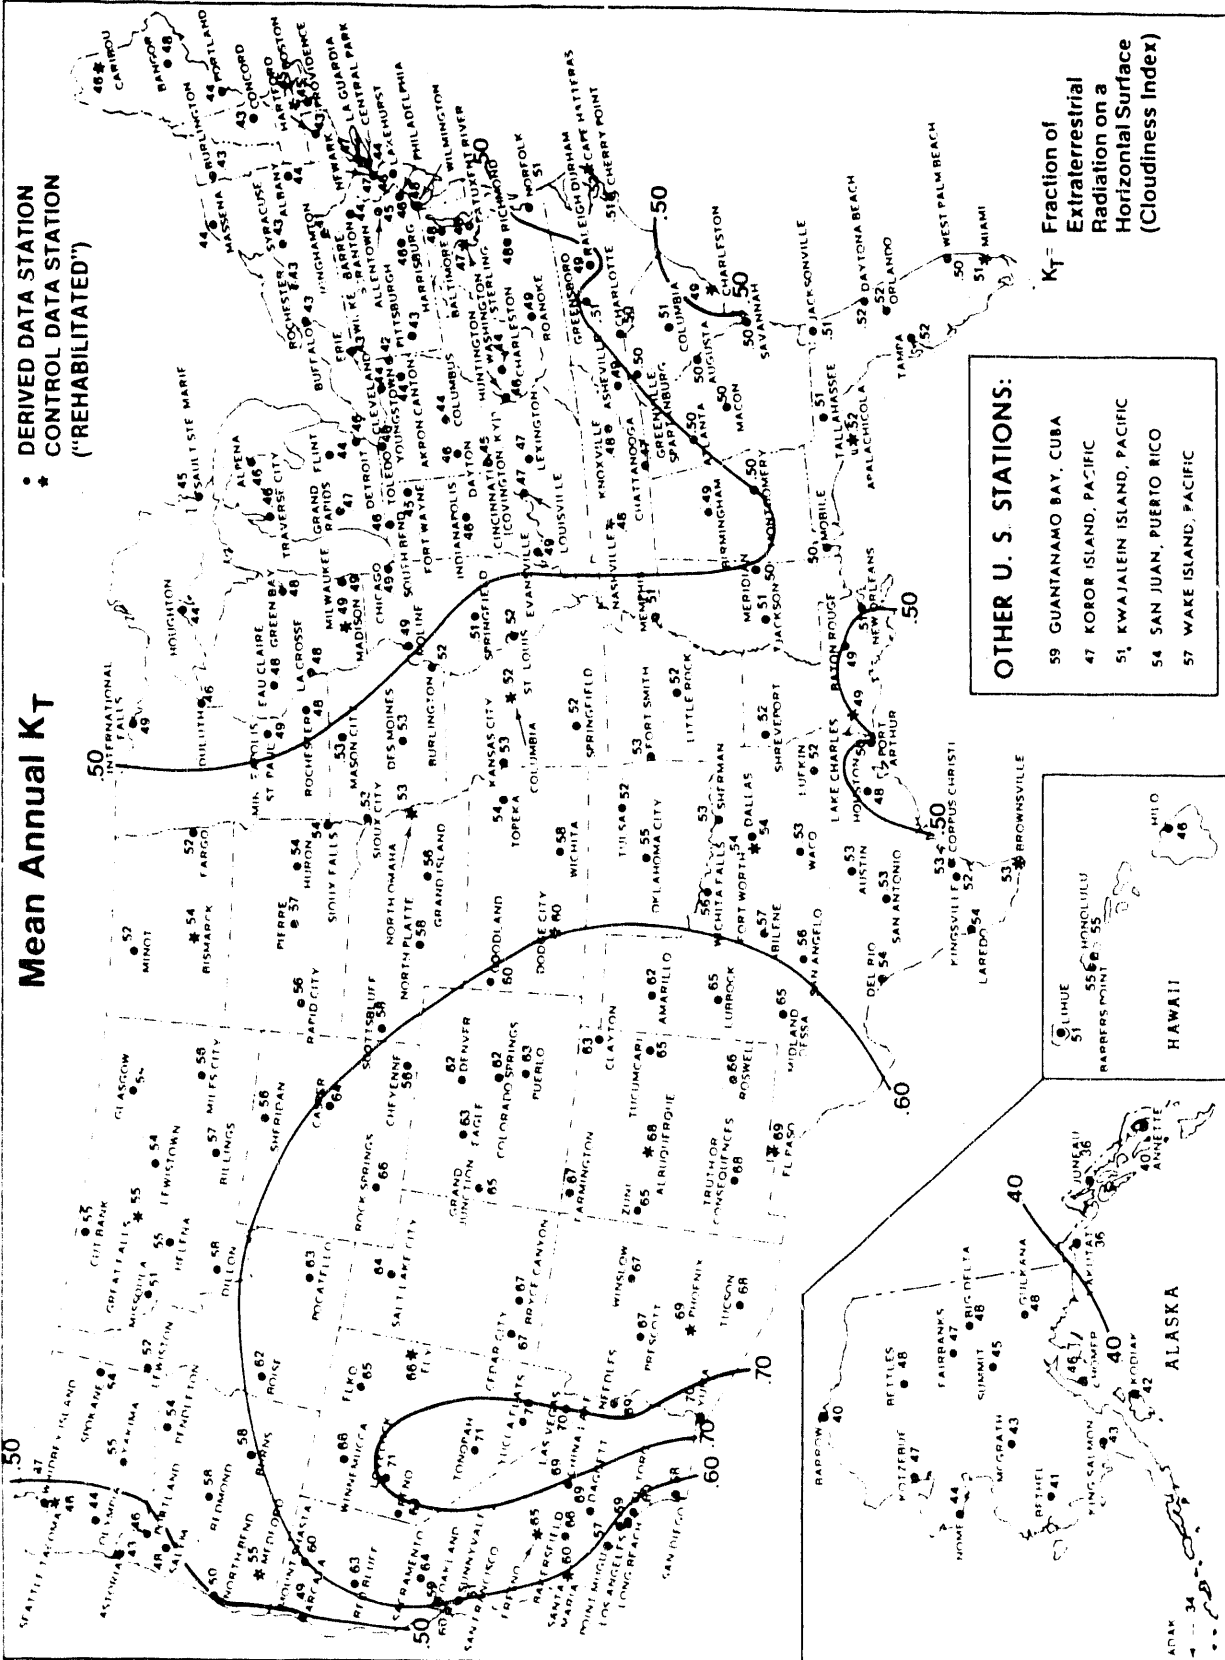


Figure 4-1. Cloudiness index (K_t) map for the United States [10]

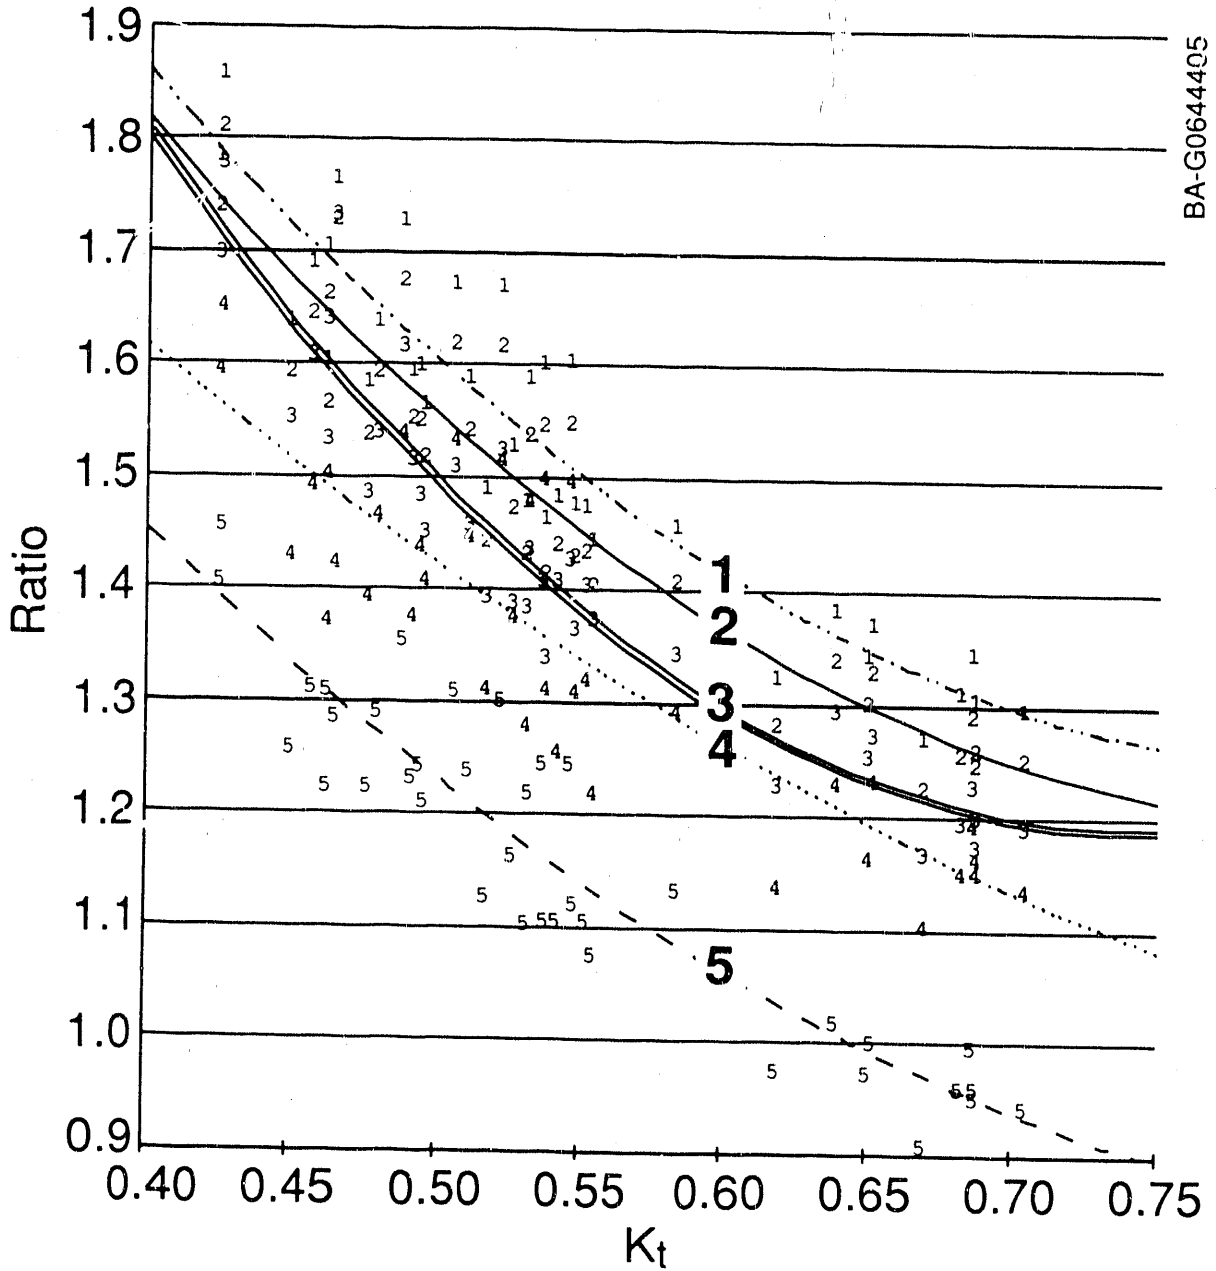


Figure 4-2a. Ratios for global POA irradiance for 5 flat-plate collector options, divided by direct-normal POA irradiance. The numerators in the ratios are as follows:
 1 = 2-axis tracking
 2 = 1-axis tracking, axis oriented north-south, and collectors tilted at the latitude
 3 = 1-axis tracking, vertical axis, and collectors tilted at the latitude
 4 = 1-axis tracking, axis oriented north-south, and collectors horizontal
 5 = fixed tilt at latitude

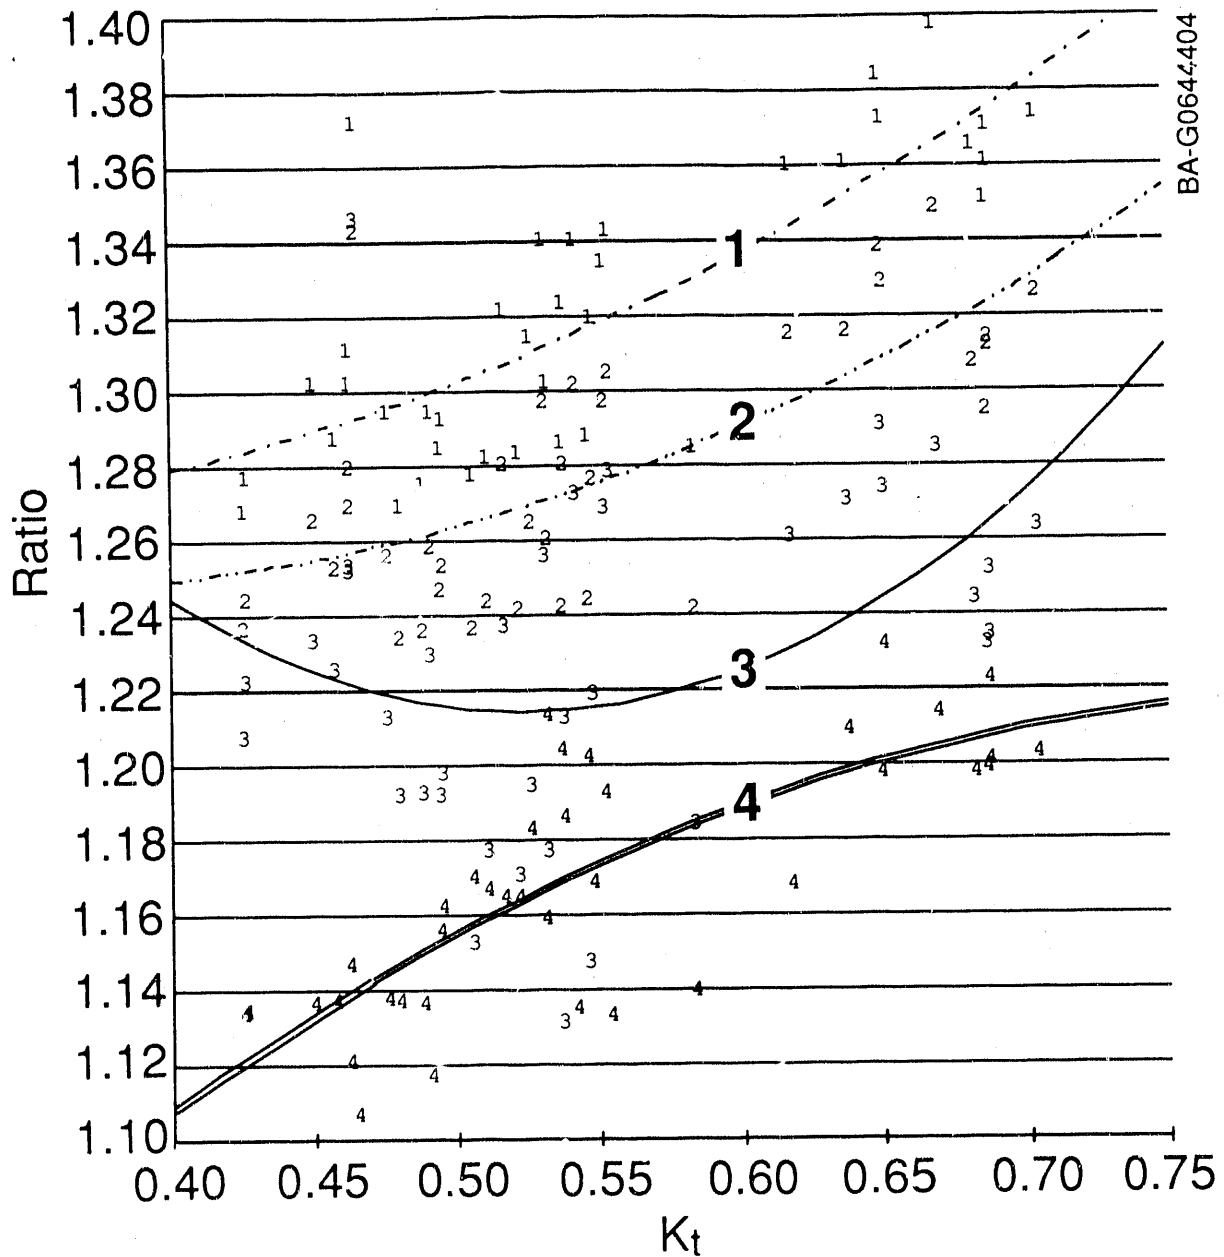


Figure 4-2b. Ratios for global POA irradiance for 4 flat-plate tracking options, divided by global POA irradiance for a flat plate with a fixed tilt at the latitude. The numerators in the ratios are as follows:
 1 = 2-axis tracking
 2 = 1-axis tracking, axis oriented north-south, and collectors tilted at the latitude
 3 = 1-axis tracking, vertical axis, and collectors tilted at the latitude
 4 = 1-axis tracking, axis oriented north-south, and collectors horizontal

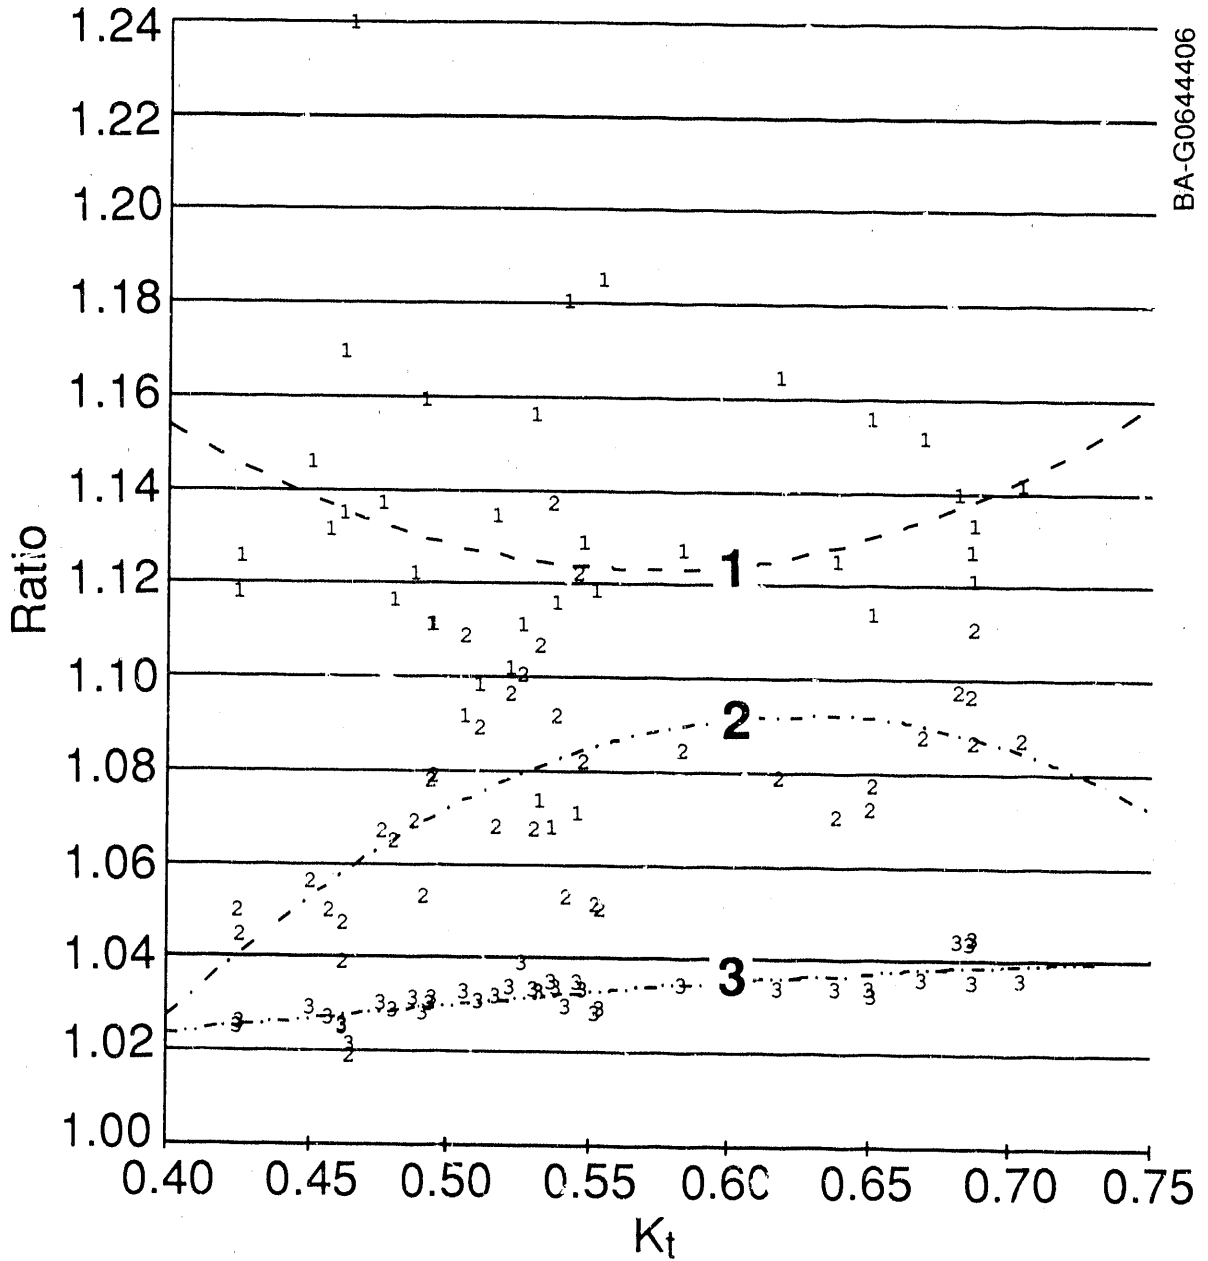


Figure 4-2c. Ratios for global POA irradiance for a two-axis tracking flat plate, divided by global POA irradiance for three 1-axis tracking options. The denominators in the ratios are as follows:
 1 = 1-axis tracking, axis oriented north-south, and collectors horizontal
 2 = 1-axis tracking, vertical axis, and collectors tilted at the latitude
 3 = 1-axis tracking, axis oriented north-south, and collectors tilted at the latitude

5.0 DEVICE SPECTRAL SENSITIVITY AND MEASUREMENT TECHNIQUES

Methods are needed to quantify the sensitivity of PV device performance to natural spectral solar irradiance variations because PV devices are spectrally selective [13]. Although PV device measurements are often corrected to a reference spectrum to compare results among laboratories, the reverse calculations are usually not performed to predict performance for a range of spectral irradiance conditions or to put "error bars" on performance measurements. Measurements or modeling should be performed in the design phase to determine whether or not the PV device performance will be adversely affected by spectral irradiance variations, especially for series-connected multijunction devices that require current matching for optimum performance.

One way to examine spectral sensitivity is to calculate PV device performance using a device model together with a spectral irradiance model or data base for different atmospheric conditions and air masses; a second way is to perform outdoor tests under different spectral irradiance conditions. For the first approach, SERI's spectral irradiance model and data base [14,15] are made available to any user who wants to perform these analyses. The second approach is time consuming if outdoor measurements are made for a full range of atmospheric conditions and air masses.

Although spectroradiometers are available for measuring spectral irradiance during outdoor tests, they are not used routinely to report spectral effects in outdoor PV device performance tests. Simple and economical methods and instruments are needed to measure first-order (coarse) solar spectral irradiance variations (at least until instruments like the AOCS are commercially available).

A simple method for monitoring first-order spectral irradiance variations is to measure irradiance using filtered and unfiltered radiometers, which separate the spectrum into roughly visible (< 780 nm) and NIR (> 780 nm) regions [16]. Such measurements have been taken at SERI since the summer of 1988.

Figures 5-1 and 5-2 give examples of the information on spectral irradiance variations that can be derived from filtered and unfiltered pyrheliometer and pyranometer data. Figure 5-1, for a clear day, shows the total irradiance and the ratio of NIR to total irradiance for direct-normal (left) and global-horizontal (right) cases. In the early morning and late afternoon, the NIR fraction of total irradiance increases for the direct-normal case (from high air mass or low sun elevation effects) while the midday ratio remains relatively constant. The midday ratio may vary from day to day depending on atmospheric water vapor and aerosol effects. For the global-horizontal case, the midday ratio is relatively constant with a slight increase at the ends of the day.

Figure 5-2, for a partly cloudy day, shows patterns similar to those of the clear day. The difference is that the direct-normal ratio is too unstable to be reliable when clouds obscure the sun's disk (because the irradiance values in the ratios are very small), and the global-horizontal ratios decrease slightly when clouds reduce the irradiance (probably because of increased water vapor and liquid water absorption in the clouds [17]).

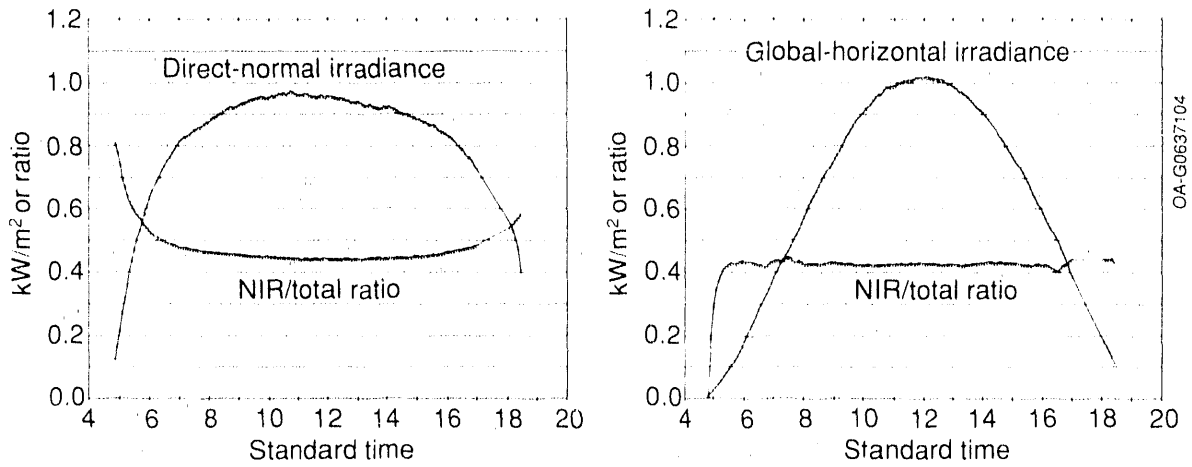


Figure 5-1. Total irradiance and the ratio of NIR to total irradiance on a clear day in Golden, Colorado, for direct-normal (left) and global-horizontal (right) cases

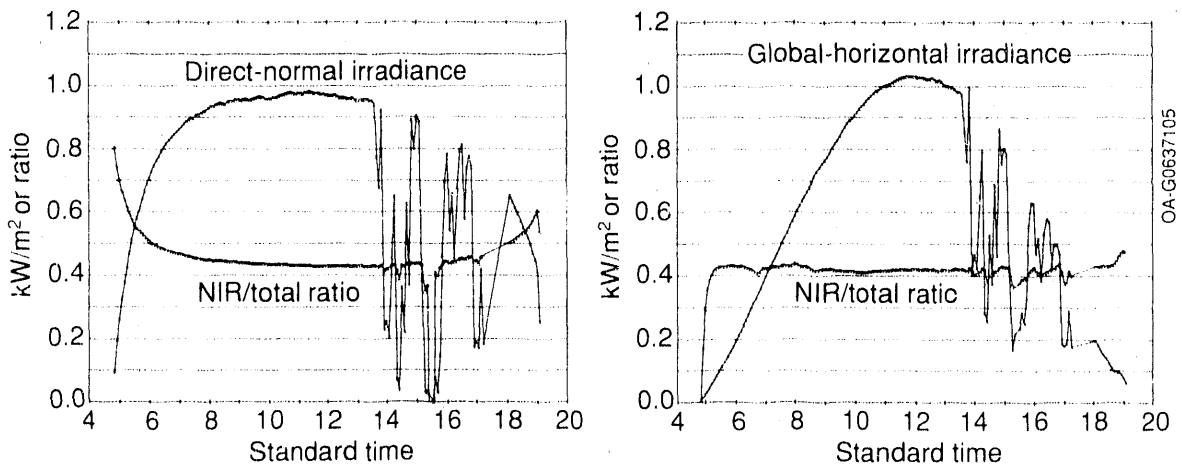


Figure 5-2. Total irradiance and the ratio of NIR to total irradiance on a partly cloudy day in Golden, Colorado, for direct-normal (left) and global-horizontal (right) cases

The extent to which a PV device is affected by changes in the distribution of irradiance between the NIR and visible regions (visible fraction = one minus the NIR fraction) depends on the spectral response (or quantum efficiency) of the PV device, or where it overlaps the visible and NIR regions of the spectrum. If PV device performance and the fraction of visible versus NIR irradiance are monitored simultaneously during outdoor tests, a sensitivity study can be performed to quantify the relationships.

6.0 MEASUREMENT SUPPORT AND TECHNOLOGY TRANSFER

Other activities under the Solar Radiation Research Task include operating the Solar Radiation Research Laboratory, an outdoor laboratory used for radiometer and PV cell calibrations and for performing special experiments; presenting papers at conferences [8,18,19]; and providing expertise, data, and models on spectral solar irradiance as related to PV applications.

7.0 SUMMARY AND FUTURE PLANS

Resources allocated to the Solar Radiation Research Task of the Photovoltaic Advanced Research and Development Project support about two research staff persons at the Solar Energy Research Institute. The research performed under this task is directed toward understanding and quantifying the relationship between PV device performance and spectral and broadband solar irradiance variations. To develop this scientific understanding, the research staff develops instruments (such as the AOCS and spectroradiometers) and solar irradiance measurement and analysis methods (such as simple methods for monitoring first-order spectral irradiance variations and investigating the climate dependence of POA irradiance enhancements for various collector options). The staff also provides analytical and measurement support regarding solar irradiance for PV device design and performance tests.

The major accomplishments in FY 1990 were as follows:

- We incorporated additional software into the AOCS so that calibration of the narrow-band channels can be performed automatically. We obtained outdoor calibration data with very repeatable results, and we acquired and processed NOAA data to refine the algorithm in the AOCS software for calculating precipitable water vapor.
- We maintained several different spectroradiometer systems and used them to measure outdoor and solar simulator spectra. More work is needed to improve the measurement uncertainty, especially in the ultraviolet region. This work was temporarily delayed to help develop a system for measuring the spectral content of SERI's pulse simulator. With the PV Measurements and Performance Branch, we established the capability to measure irradiance from the pulse simulator using an optical multichannel analyzer. This capability is also important for instantaneous measurements of outdoor solar spectra under unstable atmospheric conditions.

To help maintain our expertise in spectroradiometry and assess the state of the art in spectral measurement uncertainty, we participated in (and helped sponsor) a spectroradiometer intercomparison.

- We examined data, from various published studies and outdoor measurement programs, on PV POA irradiance to show the relationship between potential irradiance enhancements for various collector options and a site's cloudiness.
- We examined a simple method for monitoring first-order spectral irradiance using filtered and unfiltered radiometers to separate the spectrum into roughly visible and NIR regions. We analyzed measured data from the Solar Radiation Research Laboratory to show how the NIR (or visible) fraction of total solar radiation can be monitored during outdoor PV tests.

- Other activities included operating the Solar Radiation Research Laboratory to perform outdoor radiometer calibrations and provide solar radiation measurement support for PV cell calibrations and outdoor experiments. We also gave conference presentations and disseminated spectral models and data.

In FY 1991, under the Solar Radiation Research Task, we will continue our multiyear commitment to providing solar radiation models, data bases, instrumentation, and measurement support to analyze and quantify the response of PV devices to solar radiation variations. Activities planned in FY 1991 include the following:

- We will complete a scientific report on the application of sunphotometry to measurements of atmospheric water vapor; we will accomplish this as part of the final software development for the AOCS.
- We will complete the field tests of the AOCS and document this through a final engineering report.
- We will improve spectroradiometric capabilities in the ultraviolet and near-infrared regions of the solar spectrum by modifying and developing the Optronics Laboratories ultraviolet spectroradiometer, the Geophysical Environmental Research extended-wavelength (300-3000 nm) spectroradiometer, and the PV Measurements and Performance Branch's EG&G OMA III spectrometer. The goal is to lower the spectral measurement uncertainties from the ultraviolet through NIR wavelength regions.
- We will operate the Solar Radiation Research Laboratory and the Optics Laboratory to support outdoor PV device calibrations and measurements.
- We will provide spectral solar radiation models and data bases to PV researchers to investigate the spectral sensitivity of selected PV devices, especially multijunction devices.
- Finally, we will provide a variety of support measurements, including high-quality measurements of the irradiance characteristics of simulators and calibrations of spectroradiometers, and we will develop solar radiation measurement techniques to characterize irradiance variations during PV device testing.

8.0 REFERENCES

1. Hulstrom, R.L., T.W. Cannon, and C.J. Riordan, *Photovoltaic Advanced Research and Development Project, Solar Radiation Research, Annual Report for 1 October 1986 - 30 September 1987*, SERI/PR-215-3297, Golden, CO: Solar Energy Research Institute, March 1988.
2. Riordan, C.J., R.L. Hulstrom, T.W. Cannon, T.L. Stoffel, and D.R. Myers, *Photovoltaic Advanced Research and Development Project Solar Radiation Research Task, Annual Report for 1 October 1987 - 30 September 1988*, SERI/TR-215-3445, Golden, CO: Solar Energy Research Institute, February 1989.
3. Riordan, C., R. Hulstrom, T. Cannon, D. Myers, and T. Stoffel, *Photovoltaic Advanced Research and Development Project: Solar Radiation Research Annual Report, 1 October 1988 - 30 September 1989*, SERI/PR-215-3607, Golden, CO: Solar Energy Research Institute, February 1990.
4. Cannon, T.W., and R.L. Hulstrom, "A Multi-channel Radiometer for Measurement of the Optical Properties of the Atmosphere," *SPIE, Vol. 1109 - Optical Radiation Measurements II*, Bellingham, WA: The Society of Photo-Optical Instrumentation Engineers, 1989, pp. 152-159.
5. Cannon, T.W., and R.L. Hulstrom, "Specialized Instrumentation and Techniques for Measurement of Terrestrial Solar Radiation," *Daylight and Solar Radiation Measurement Conference*, October 9-11, 1989, Berlin, Germany, conference proceedings, Institut für Lichttechnik, Technische Universität Berlin, Einsteinufer 19, D-1000 Berlin 10, pp. 312-321.
6. Osterwald, C., K.A. Emery, D.R. Myers, and C. J. Riordan, "Extending the Spectral Range of Silicon-Based Direct-Beam Solar Spectral Radiometric Measurements," *Proceedings of the 20th IEEE PV Specialists Conference*, New York: IEEE, 1988, pp. 1246-1250.
7. Myers, D.R., "Estimates of Uncertainty for Measured Spectra in the SERI Spectral Solar Radiation Data Base," *Solar Energy*, Vol. 43, No. 6, 1989, pp. 87-97.
8. Myers, D., "Principles of Uncertainty Analysis with Examples Drawn from Radiometry," presented at the CORM 90 Annual Meeting, May 9-11, 1990, Rochester, NY (unpublished material, Solar Energy Research Institute).
9. Menicucci, D.F., and J.P. Fernandez, *Estimates of Available Solar Radiation and Photovoltaic Energy Production for Various Tilted and Tracking Surfaces Throughout the U.S. Based on PVFORM, A Computerized Performance Model*, SAND85-2775, Albuquerque, NM: Sandia National Laboratories, March 1986.

10. Solar Technical Information Program, *Insolation Data Manual and Direct Normal Solar Radiation Data Manual*, SERI/TP-220-3880, Golden, CO: Solar Energy Research Institute, July 1990.
11. Riordan, C., and D. Myers, *Solar Radiation Resources Available to Photovoltaic Collectors*, SERI/TP-215-3919, Golden, CO: Solar Energy Research Institute, 1990 (draft).
12. Nann, S., "Potentials for Tracking Photovoltaic Systems and V-Troughs In Moderate Climates," submitted to *Solar Energy*, 1990.
13. Riordan, C.J., and R.L. Hulstrom, *Summary of Studies that Examine the Effects of Spectral Solar Radiation Variations on PV Device Design and Performance*, SERI/TR-215-3437, Golden, CO: Solar Energy Research Institute, March 1989.
14. Bird, R.E., and C. Riordan, "Simple Solar Spectral Model for Direct and Diffuse Irradiance on Horizontal and Tilted Planes at the Earth's Surface for Cloudless Atmospheres," *Journal of Climate and Applied Meteorology*, Vol. 25, No. 1, January 1986, pp. 87-97.
15. Riordan, C., D. Myers, and R. Hulstrom, *Spectral Solar Radiation Data Base Documentation and User's Manual*, Vols. I and II, SERI/TR-215-3513, Golden, CO: Solar Energy Research Institute, January 1990.
16. Riordan, C., and D. Myers, *Using Filtered and Unfiltered Radiometers to Monitor Spectral Solar Radiation Conditions During Outdoor Photovoltaic Tests*, SERI/TP-215-4001, Golden, CO: Solar Energy Research Institute, 1990 (draft).
17. Nann, S., and C. Riordan, "Solar Spectral Irradiance Under Overcast Skies," *SERI Preprints for the 21st IEEE PV Specialists Conference*, SERI/SP-210-3833, Golden, CO: Solar Energy Research Institute, May 1990.
18. Riordan, C., and R. Hulstrom, "What is an Air Mass 1.5 Spectrum?," *SERI Preprints for the 21st IEEE PV Specialists Conference*, SERI/SP-210-3833, Golden, CO: Solar Energy Research Institute, May 1990.
19. Osterwald, C.R., K.A. Emery, D.R. Myers, and R.E. Hart, "Primary Reference Cell Calibrations at SERI: History and Methods," *SERI Preprints for the 21st IEEE Photovoltaic Specialists Conference*, SERI/SP-210-3833, Golden, CO: Solar Energy Research Institute, May 1990.

Document Control Page	1. SERI Report No. SERI/TP-215-4065	2. NTIS Accession No. DE91002119	3. Recipient's Accession No.
4. Title and Subtitle Photovoltaic Advanced Research and Development Project: Solar Radiation Research Annual Report, 1 October 1989 - 30 September 1990		5. Publication Date November 1990	6.
7. Author(s) C. Riordan, R. Hulstrom, T. Cannon, D. Myers, T. Stoffel		8. Performing Organization Rept. No.	
9. Performing Organization Name and Address Solar Energy Research Institute 1617 Cole Blvd. Golden, CO 80401		10. Project/Task/Work Unit No. PV 110201	11. Contract (C) or Grant (G) No. (C) (G)
12. Sponsoring Organization Name and Address		13. Type of Report & Period Covered Annual Report	14.
15. Supplementary Notes			
16. Abstract (Limit: 200 words) This report gives an overview of the fiscal year 1990 research activities and results under the Solar Radiation Research Task of the Photovoltaic Advanced Research and Development Project at the Solar Energy Research Institute. The activities under this task include developing and applying measurement techniques, instrumentation, and data and models to understand and quantify the response of photovoltaic devices to variations in broadband and spectral solar radiation. The information presented in this report was presented at the SERI Photovoltaic Advanced Research and Development Project 10th Review Meeting, October 1990, and will be published in a special issue of <u>Solar Cells</u> dedicated to the meeting.			
17. Document Analysis a. Descriptors photovoltaics ; solar cells ; solar radiation ; resource assessment ; insolation ; solar irradiance b. Identifiers/Open-Ended Terms c. UC Categories 270, 233			
18. Availability Statement National Technical Information Service U.S. Department of Commerce 5285 Port Royal Road Springfield, VA 22161		19. No. of Pages 26	20. Price A03

END

DATE FILMED

02 / 14 / 91