

Visible spectroscopy versus Brewer and satellite instruments


Manuel Gil-Ojeda¹, M. Navarro-Comas¹, A. Redondas², O. Puentedura¹, F. Hendrick³, M. Van Roozendael³, J. Iglesias¹ and E. Cuevas²
 (1) National Institute for Aerospace Technology, (INTA), Madrid, Spain.
 (2) Izaña Atmospheric Research Center, Meteorological State Agency of Spain (AEMET), Izaña, Spain
 (3) Belgian Institute for Space Aeronomy, 3 Ave. Circulaire, B-1180 Brussels, Belgium
 Contact: gilm@inta.es




Abstract

Ozone total columns measured at twilight using a zenith-sky UV-Visible spectrometer installed at the NDACC Izaña Subtropical Observatory (28°N, 16°W) in October 1998 are compared with the RBCC-E reference instrument Brewer #157 at the same location. DOAS retrievals were performed in the visible range (450-535 nm) according to improved settings recommended by the NDACC and using homogenized daily AMFs based on the TOMS V8 (TV8) column-resolved ozone profile climatology. The station is located at 2370 masl well above the Marine Boundary Layer and outside of pollution environment. Comparisons have been performed for the 13-years dataset using daily means to minimize the impact of instruments differences in measurements time. Overall results show an excellent agreement. The UV-Visible to Brewer mean difference is of +1.0% with a standard deviation of 3% and a slight dependence on the amount of ozone. Discrepancies on individual days due to changes in the tropospheric O₃ content and different air masses sampling in fast O₃ changing conditions were identified. The temperature dependence of the UV cross-sections has been found to have a negligible impact at these low latitudes. Seasonal discrepancies are of only few tens of a percent. The station being affected by desert dust from Sahara, cloud filtered data have been split in two sets to examine the potential influence of aerosol scattering and absorption on measurements. Results show a similar behaviour of both techniques also under high aerosol loading conditions. Comparisons with satellite instruments show an average agreement better than 1% for TOMS-V8, OMI and SCIAMACHY and of 1.1% and 1.6% for GOME and GOME-2, respectively with a standard deviation of 3%. However, considering that 2.7 to 3.0 % of the total column resides below the altitude of the station, these values actually point to an underestimation of the satellite instruments in comparison to our ground-based data. Possible causes of these differences are discussed.

Station and Instruments



Technical differences between Brewer, DOAS and satellites

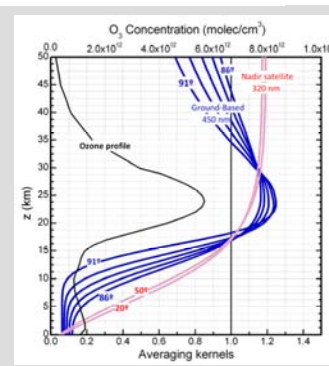


- + Spectral range: Brewer UV DOAS : Visible
- + Sensitivity to atmospheric layers. Zenith measurements at twilight are almost insensitive to tropospheric ozone. Nadir instruments have a limited tropospheric sensitivity, as well (see figure)
- + AMF are sensitive to aerosols content. Both instruments are affected. The effect in diffuse light is larger than at direct sun but is minimum at twilight.
- + Temperature dependence. Negligible in visible but not in the UV.


Algorithm	Ground-Based			Satellites				
	Brewer	RASAS	RASAS-II	TOMS	GOME	SCIA	OMI	GOME-2
Retrieval range (nm)	306-320	430-535	430-520	312,331	326-335	326-334.5	317.5, 331.2	325-334.5
Samples/nm	5 single λ	3.4	8.9	2 single λ	11.1	10.7	2 single λ	11.1
Resolution (nm)	0.6	1.3	0.5	1	0.17	0.25	0.6	0.29
FOV (degrees)	3°	11°	1°					
Scanned area or footprint (approx. km)	Direct Sun	Zenith ¹	Zenith ¹	Nadir (100x100)	Nadir (320x40)	Nadir (30x60)	Nadir (100x100)	Nadir (80x40)

Averaging kernels (AK) describe the sensitivity of total column of a tracer to changes in a given layer. It can be computed as the ratio of the AMF at certain layer to the total AMF. Plot shows AK for a) DOAS at solar zenith angles (sza) of 86° to 91° and wavelength 450 nm. b) Nadir satellite at 20-50 sza and wavelength of 320 nm. Ozone profile used in the calculations is shown as reference. Tropospheric sensitivity is limited and reduces as sza increases. Increasing wavelength results lowering of the maximum of sensitivity.


¹Diffuse light, Effective slant path results from the intensity-weighted integration of all individual paths. At twilight effective location is about 200-300 km toward the sun direction
²OMT03 v8 = O3 below clouds added to results. Clouds taken from TOMS climatology
 v8.5 = RRS used to estimate photons penetration



- + Brewer and satellites measure in the 300-330 nm band (Huggins) where Cross-sections are temperature dependent.
- + Ground-based DOAS measures in the visible band (Chappuis) where differential cross-sections are temperature independent.
- + The effect is minor in tropical/subtropical regions since there is little temperature variability along the year.

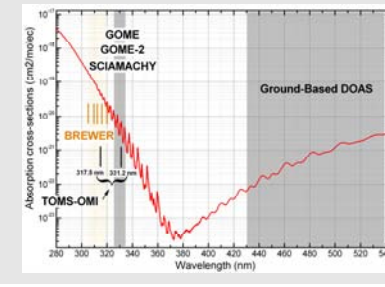


DOAS & Brewer

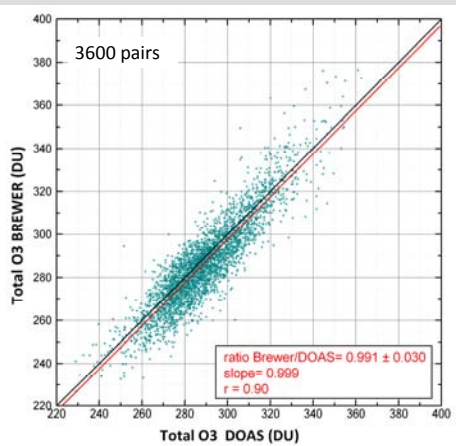

- * Agreement to 0.9 %
- * Departure from diagonal at large values due to occasional pollution events not captured by DOAS (little tropospheric sensitivity)
- * Identified real differences due to a) differences in time b) differences in space (observation geometry makes that DOAS scanned air masses are 200-300 km apart from the station)

The use of a single set of AMF all year round result in a seasonality in the ratio Brewer/DOAS (blue). Seasonality is reduced to less than 1% when using daily AMF as recommended by NDACC (Hendrick et al, 2011)

Blue squares = One single AMF set for all year
 Red open circles = New NDACC AMF
 Blue and red lines = sin fits

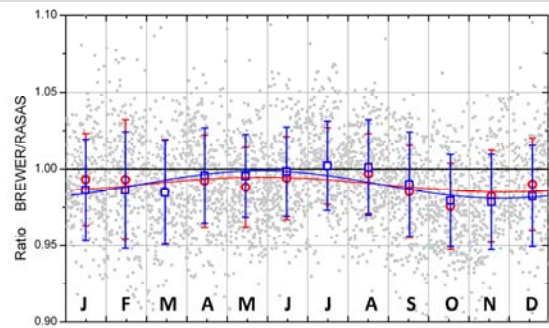

Conclusions


- + O₃ data from DOAS instruments (RASAS and RASAS-2) operating at Izaña Observatory since late 1998 have been compared to the RBCC-E Brewer #157 and nadir satellite overpassing data.
- + Agreement between all instruments intercompared are within 1% with a standard deviation of 3%.
- + Satellite data are 1% lower than ground-based if we consider that 3% of the ozone column resides below the station.
- + No difference in the agreement between UV-direct Sun (Brewer) and Zenith visible (DOAS) has been found under Saharan dust conditions with respect to normal no-dust conditions (AOD < 0.05)
- + The excellent O₃ agreement between instruments (keeping in mind differences in spectral range, cross-sections, geometry, FOV, evaluation procedures, etc) shows that the aim of reaching measurements at the 1% level can be reached at Subtropical latitudes where tropospheric O₃ variability is small.

Future work:
 This work will be completed by including the FTIR instrument on the DOAS intercomparison.


References:

IGACO, ESA SP-1282, 2004 http://www.igaco-o3.fi/linked/en/IGACO_Theme_Report_wmo_gaw159.pdf
 GMES Atmospheric Core Service (GACS), Implementation Plan, Final Report, 2009
 Hendrick, F., J.-P. Pommerehne, F. Goutail, R. D. Evans, D. Ionov, A. Pazmino, E. Kyro, G. Held, P. Eriksen, V. Dorokhov, M. Gil, and M. Van Roozendael, NDACC/SAOZ UV-visible total ozone measurements: improved retrieval and comparison with correlative ground-based and satellite observations, Atmos. Chem. Phys., 11, 5975–5995, 2011
 Schneider, M., A. Redondas, F. Hase, C. Guirado, T. Blumenstock, and E. Cuevas, Comparison of ground-based Brewer and FTIR total column O₃ monitoring techniques, Atmos. Chem. Phys., 8, 5535–5550, 2008
 Lerot, C., M. Van Roozendael, J. van Geffen, J. van Gent, C. Fayt, R. Spurr, G. Lichtenberg, and A. von Bargaen, Six years of total ozone column measurements from SCIAMACHY nadir observations, Atmos. Meas. Tech., 2, 87–98, 2009
 Viatte, C., M. Schneider, A. Redondas, F. Hase, M. Eremenko, P. Chelin, J.-M. Flaud, T. Blumenstock, and J. Orphal, Comparison of ground-based FTIR and Brewer O₃ total column, with data from two different IASI algorithms and from OMI and GOME-2 satellite instruments Atmos. Meas. Tech., 4, 535–546, 2011


DOAS & Nadir-looking Satellite Instruments

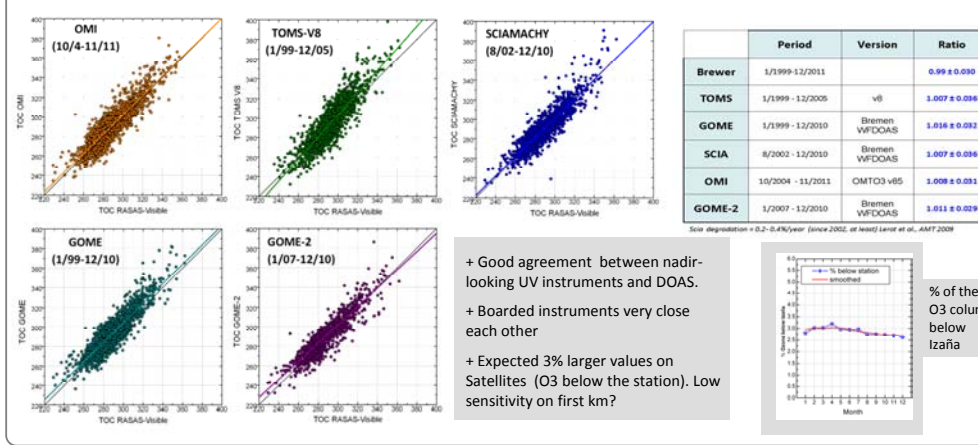

- + Good agreement between nadir-looking UV instruments and DOAS.
- + Boarded instruments very close each other
- + Expected 3% larger values on Satellites (O₃ below the station). Low sensitivity on first km?



Effect of Saharan dust on ozone retrievals: Differences Brewer & DOAS

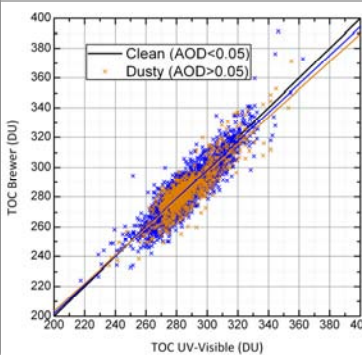

Saharan dust absorbs UV radiation and strongly enhance radiation scattering. Episodes of heavy outbreaks up to 1 AOD for few days are common.

We have explored the potential influence of Saharan dusts events on retrieved ozone amounts by analyzing separately clear non-dusty days and clear dusty days (cloudy days were removed).

No significant differences have been found for Brewer and DOAS spectrometers.

Acknowledgements:

We acknowledge IUPB for providing GOME, GOME- and SCIAMACHY overpassing data. Uri: <http://www.iup.uni-bremen.de/gome/wfdoas/merged/>
 OMI and TOMS data are from overpassing as well. Uri: <http://avdc.gsfc.nasa.gov/index.php?site=830165109>
 This work has been partially funded by NORIS, UE FP7 Project under grant agreement n°284421 and AMISOC, CGL2011-24891, from the Spanish Plan for Research, Development and Innovation.
 Operation of DOAS instrument at Izaña is possible thanks to the technical support from AEMET and SIELTEC teams