



## 20 GHz instantaneous bandwidth RF spectrum analyzer with high time-resolution

Perrine Berger, Muriel Schwarz, Stéphanie Molin, Daniel Dolfi, Loïc Morvan,  
Anne Louchet-Chauvet, Thierry Chanelière, Jean-Louis Le Gouët

### ► To cite this version:

Perrine Berger, Muriel Schwarz, Stéphanie Molin, Daniel Dolfi, Loïc Morvan, et al.. 20 GHz instantaneous bandwidth RF spectrum analyzer with high time-resolution. 2014 International Topical Meeting on Microwave Photonics (MWP) jointly held with the 2014 9th Asia-Pacific Microwave Photonics Conference (APMP), Oct 2014, Hokkaido, France. pp.331-334. hal-02108553

HAL Id: hal-02108553

<https://hal.archives-ouvertes.fr/hal-02108553>

Submitted on 24 Apr 2019

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# 20 GHz instantaneous bandwidth RF spectrum analyzer with high time-resolution

Perrine Berger, Muriel Schwarz, Stéphanie Molin,  
Daniel Dolfi, Loïc Morvan  
Thales Research and Technology  
1 av. Augustin Fresnel, 91767 Palaiseau, FRANCE

Anne Louchet-Chauvet, Thierry Chanelière, Jean-  
Louis Le Gouët  
Laboratoire Aimé Cotton, CNRS-UPR3321  
bât. 505, 91405 Orsay, FRANCE

**Abstract**—We report on the experimental demonstration of a multi-gigahertz bandwidth RF spectrum analyzer exhibiting a resolution below 20 MHz, based on spectral hole burning in a rare-earth ion-doped crystal. To be compatible with demanding real-time spectrum monitoring applications, our demonstrator is designed to reach a high time resolution. For this purpose, we implemented the so-called “rainbow” architecture in which the spectral components of the incoming signal are angularly separated by the crystal, and are then acquired with a pixelated photodetector. The  $\text{Tm}^{3+}$ :YAG crystal is programmed with a semiconductor DFB laser which frequency scan is servo-controlled and synchronized with the angular scan of a resonant galvanometric mirror, while a high-speed camera is used to acquire the spectra. In the perspective of future implementation within a system, the crystal is cooled below 4 K with a closed-cycle cryostat. With this setup, we have been able to monitor and record the spectrum of complex microwave signals over an instantaneous bandwidth above 20 GHz, with a time resolution below 100  $\mu\text{s}$ , 400 resolvable frequency components and a probability of intercept of 100 %.

**Keywords**—Analog optical signal processing, spectrum analysis, broadband microwave spectrum monitoring, spectral hole burning.

## I. INTRODUCTION

The more and more complex signals emitted by modern RF sensing and communication systems make crucial the availability of broadband and real-time microwave spectrum monitoring tools. Indeed, from few tens of megahertz to few tens of gigahertz, the microwave spectrum is now occupied by frequency-hopping and bursting signals which time-frequency characteristics are almost impossible to analyze with standard swept spectrum analyzers. To ensure a large coverage of the spectrum with 100 % probability of intercept, the most stringent applications need an instantaneous analysis bandwidth of at least several gigahertz, far from the capabilities of most recent digital real-time spectral analyzers offering only few tens of megahertz. The solution consisting in digitizing the full spectrum is highly challenging due to the high data rate to be handled, the large computational resources required to provide the spectra through FFTs, and the performances are limited by the poor characteristics of broadband ADCs in terms of dynamic range [1, 2]. In this context, alternative solutions are welcome.

In the optical domain, Spectral Hole Burning (SHB) in rare-earth ion doped crystals (REIC) are particularly attractive to

process broadband signals with impressive time-bandwidth product, since their inhomogeneously broadened absorption bands can reach 200 GHz bandwidth, while preserving a spectral resolution below 10 kHz at low temperature [3]. Various optical functions have been demonstrated REICs, such as cross-correlation analysis of RADAR return signals [4, 5], true-time delay generation for radar application [6], analog-to-digital conversion [7] and more recently, time reversal of microsecond-long RF signals [8]. For wideband microwave spectrum analysis, two main architectures have been proposed.

In the first approach, the spectrum of the microwave signal of interest is converted into the optical domain and then recorded in the SHB material, which is used as a spectral memory. One then has several milliseconds – the memory lifetime – to retrieve the signal components with a fast sweeping read-out laser. This approach is extensively studied for the spectrum analysis of broadband RF signals over 20 GHz, with sub-MHz resolution and sub-millisecond refresh time [9-13], and has even been upgraded to direction finding [14, 15]. To reach higher time resolution, this architecture faces two limitations. First, the signal remains present in the crystal for few milliseconds. Second, even if a post-detection recovery algorithm [16] greatly reduces the read-out time  $t_{res}$  while preserving the spectral resolution  $\delta\omega_{res}$ , these parameters are fundamentally linked to the detector and digital processing bandwidth  $\delta f_{det}$  and the bandwidth  $\Delta f$  by the relation:

$$\delta\omega_{res} = \frac{\Delta f}{\delta f_{det} \cdot t_{res}}. \quad (1)$$

Assuming a reasonable processing bandwidth of 100 MHz, time resolution in the few  $\mu\text{s}$  range would lead, to a resolution in the range of tens of MHz over a 20 GHz bandwidth, while leading to severe constraints on the chirp rate of the read-out laser.

In the second approach, the so-called “rainbow” architecture, the signal is no more recorded in the crystal. Spectral hole burning process is used to store, over the desired bandwidth, a processing function that is designed to angularly separate the spectral components of the signal. These components are then easily acquired with a pixelated photodetector [17-19]. Up to the standard Fourier limit, the time and frequency resolutions are then linked by independent parameters, as it will be further detailed in this paper.

---

This work was funded by the Direction Générale de l'Armement (DGA) within PEA ORGE project.

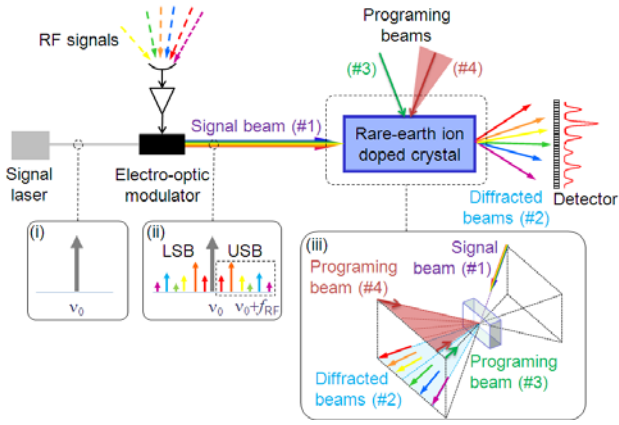


Fig. 1. Principle of the rainbow architecture. The crystal diffracts the spectral components of the microwave signals in different directions thanks to the programmed processing function stored in the crystal. The inserts (i) and (ii) respectively depict the spectra of the cw laser and the modulated laser with the lower sideband (LSB) and upper sideband (USB). (iii) shows the counter propagating box geometry of the four beams which simultaneously enables to program the crystal and to diffract a third polychromatic beam.

The last reported demonstration of the rainbow architecture was limited to a bandwidth of 3.3 GHz with a 33 MHz resolution (100 independent frequency channels), and a time resolution of 10 ms, limited by the photodetector [20]. Moreover, due to the use of a single laser for crystal programming and signal analysis, the probability of intercept was only 50%.

The objective of the present work was then to demonstrate that this architecture is able to operate over a 20 GHz bandwidth with a probability of intercept of 100 %, an improved frequency resolution and a much shorter time resolution. Another requirement was the use of a closed-cycle cryostat for crystal cooling, and only off-the-shelf optoelectronic components, in the perspective of integration in a real system. In the following, after recalling briefly the operating principle of the rainbow analyzer, we detail how we implemented this architecture to reach the above mentioned performances. The results of the analysis of wideband microwave signals is then presented and discussed.

## II. DESCRIPTION OF THE EXPERIMENT

### A. Principle of the rainbow architecture

The principle of the rainbow architecture is depicted in Fig. 1. The investigated microwave signals are transposed on a cw optical carrier thanks to a Mach-Zehnder electro-optics modulator. The sidebands of this polychromatic beam (#1) is then composed of the spectral components of the RF signals (see insert (ii) of Fig. 1). SHB material, once programmed, enables to convert spectral content to spatial angle information over a specified spectral region, which matches the upper (or lower) sideband. The spectral components of the microwave signal are then diffracted and simultaneously retrieved in different directions. An array photodetector detects the diffracted beams (#2) and records the spectrum of the microwave signals.

The physical principle of the SHB material programming is well described in [18]. It relies on spectral holes burning and simultaneous engraving of monochromatic gratings in a rare-earth ion-doped crystal (REIC) cooled at low temperature ( $<5$  K). The REIC is illuminated by two programming beams (#3 and #4) issued from the same laser whose frequency is scanned over the required bandwidth of analysis  $\Delta f$  of the spectrum analyzer. The beam #3 is also angularly scanned in synchrony with the frequency scanning. Consequently, the beams #3 and #4 engrave a set of monochromatic Bragg gratings, and burn associated spectral holes in the absorption profile of the REIC: each diffraction angle is then associated with a specific spectral component. A large number of gratings can coexist within the inhomogeneous width of the absorption line of the REIC, which may reach tens of GHz. The spectral selectivity of these gratings is defined by the width of the associated spectral holes, which ultimately match the homogenous width of the REIC (which may reach 10 kHz at low temperature in some REIC [3]). The programming has to be refreshed at least every 10 ms, corresponding to the lifetime of the populations. The insert (iii) of Fig. 1 shows the counter propagating box geometry which simultaneously enables to program the crystal and to continuously diffract the signal beam (#1). This geometry is necessary to a continuous spectral analysis of the investigated microwave signals.

### B. Hardware overview

The building blocks of the experimental set-up are presented in Fig. 2. The REIC is a 0.5% thulium-doped YAG crystal, cooled at 3 K by a closed-cycle cryostat. The absorption line of the cooled crystal, centered at 793 nm, exhibits an inhomogeneous width larger than 20 GHz. The signal block is composed of an external cavity laser and a 20-GHz bandwidth intensity modulator. The main component of the detection block is a CMOS line camera with a high frame rate (up to 10 kHz). This frame rate will correspond to the refresh time of the spectral analyzer.

The programming of the crystal is one of the major issues of this experiment. The angular scan of the programming beam #3 is performed by a resonant scanning mirror, operating at 2 kHz, whose stability was previously checked in [21].

The programming laser, operating at 793nm, has to scan over 20 GHz within 250  $\mu$ s in synchrony with the sinusoidal angular scan, with a linewidth smaller than the required spectral resolution of the analyzer, and its centered wavelength has to be stabilized on the signal laser. Consequently, the sweeps of the programming laser, which exhibits rapid and abrupt

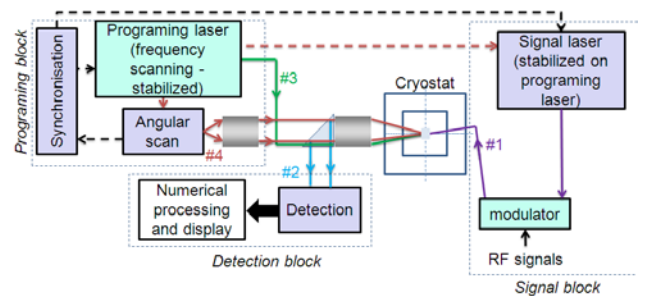


Fig. 2. Building blocks of the experimental set-up.

variations of the optical frequency, has to be precisely controlled. We used a self-referenced laser frequency stabilization scheme, compatible with high frequency agility. This technique has been proposed and demonstrated for high linear chirp by several research groups [22-24]. This scheme is based on phase-locked loop detection of a fiber-interferometer-derived heterodyne beat signal. An example of implementation is illustrated in Fig. 3. The output of the tunable laser is split using an acousto-optic modulator (AO). The first order beam travels through a fiber delay line (introducing a delay  $\tau$ ) and is shifted in frequency by  $f_{AO} = 80$  MHz. The zeroth-order beam is not delayed and is split into two unequal portions by a fiber splitter: 10% is used for the control of the sweep and 90% corresponds to the output of the laser, used for out-of-loop measurement or for the dedicated application. The zeroth-order and the delayed and shifted first-order beams are recombined interferometrically using a fiber combiner and detected by a photodiode (PD). The output of the PD is mixed down using a reference signal. The measured error is then amplified and integrated with a proportional-integrator (PI) filter and injected into the tunable laser. A control voltage is added to the laser input in order to set the nominal optical frequency sweep.

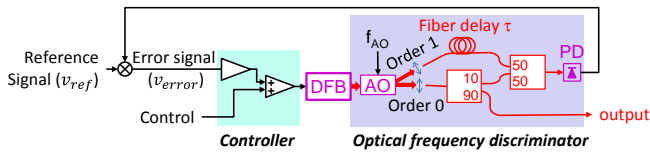


Fig. 3. Set-up for precise control and stabilization of broadband arbitrary frequency sweeps by fibered self-heterodyne technique. Abbreviations are defined in the text.

If the frequency sweep is a linear chirp, the frequency of the reference signal is then fixed. In our experiment, as the programming laser requires arbitrary sweeps with rapid and abrupt variations of the optical frequency, the fixed reference oscillator is replaced by an arbitrary waveform generator, in order to create the appropriate reference signal. The laser is a DFB operating at 793.4 nm. The control and the corrected error signals are applied to the FET-current input of the laser. The systematic chirp nonlinearities are suppressed as much as possible by an open-loop pre-distortion technique [22, 25]. The nominal frequency is swept over 20 GHz within 250  $\mu$ s, with a local slope varying from 25 GHz/ms to 400 GHz/ms. When the optical frequency sweep is locked to a reference electronic signal thanks to the opto-electronic feedback loop previously described, the error is reduced down to less than 1 MHz.

### III. EXPERIMENTAL RESULTS OF THE ANALYSER

In order to test the performances of the spectral analyzer, several RF generators and arbitrary waveforms generators have been used to simulate broadband and complex RF spectra. Two examples of spectrograms are presented in Fig. 4 and Fig. 5.

In Fig. 4, the crystal was programmed over 20 GHz and the frame rate of the photodetector was set to 10 kHz, while the integration time was 98  $\mu$ s (the maximum possible for the camera at this frame rate), leading to a probability of intercept of 98 %. A generator created a cw signal whose frequency was swept over 3.2 GHz within 30 ms, around 18.3 GHz. A second

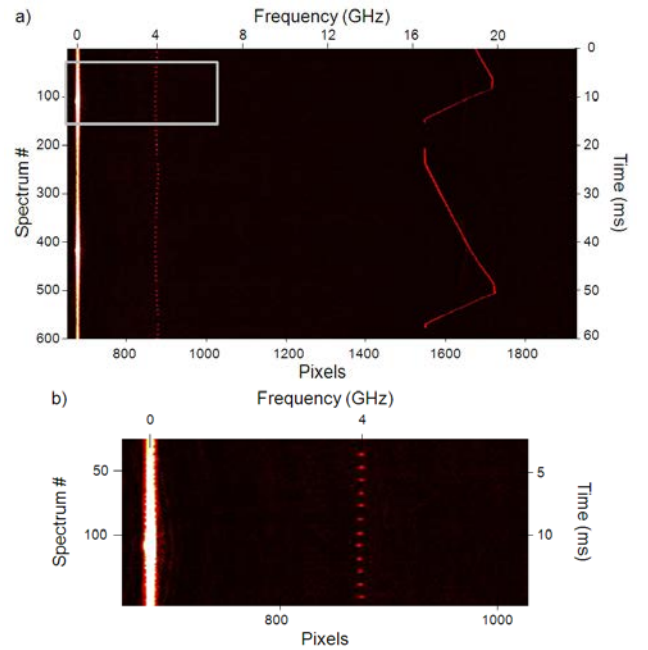


Fig. 4. Spectrogram over 20 GHz with a frame rate of 2 kHz, recorded over 60 ms. The experimental parameters are detailed in the text. (a) Whole spectrogram. (b) zoom of the previous spectrogram.

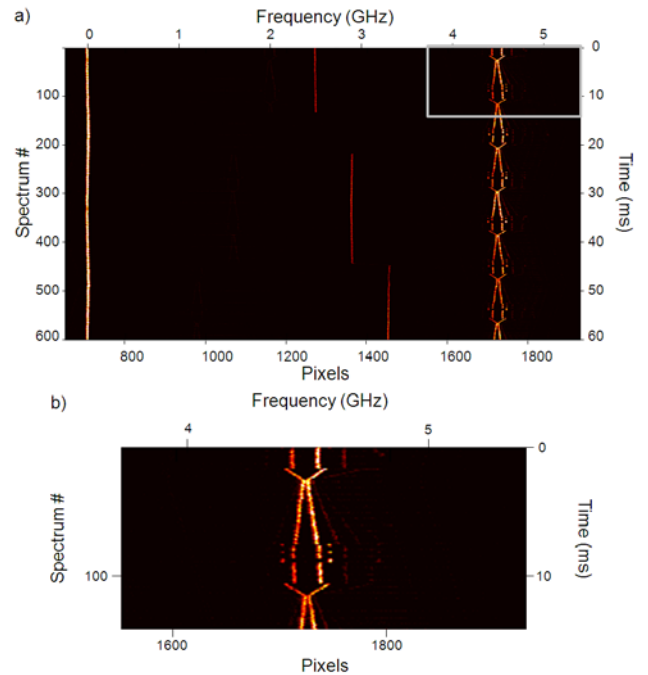


Fig. 5. Spectrogram over 5 GHz with a frame rate of 2 kHz, recorded over 60 ms. The experimental parameters are detailed in the text. (a) Whole spectrogram. (b) zoom of the previous spectrogram.

generator produced pulses at 4 GHz with a repetition rate of 2 kHz. As it can be seen on the spectrograms, the two signals are simultaneously analyzed with all their time-frequency features, with a spectral resolution of 50 MHz.

To illustrate the flexibility of the architecture, the crystal was then programmed for an analysis from 0 to 5 GHz, the frame rate of the photo-detector being kept to 10 kHz. A first

generator produced a cw signal with frequency steps every 20 ms. A complex signal was created by an arbitrary waveform generator (bandwidth 125 MHz) and up-converted at 4.5 GHz. The programmed temporal sequence was the following: i) chirp from 0 to 50 MHz within 5 ms; ii) frequency hopping at 60 MHz and at 110MHz; (iii) chirp from 100 to 50 MHz within 1 ms. The spectrograms of Fig 5 illustrates the correct analysis of these signal by our set-up, with a spectral resolution being now below 20 MHz.

By using an all-optical compensation scheme on the signal beam, we have been able to extend the probability of intercept to 100 %. We also preliminary estimated the dynamic range of our architecture to be above 35 dB.

#### IV. CONCLUSION

We experimentally demonstrated a RF spectrum analyzer based on the so called “rainbow architecture” which enables to monitor and record the spectrum of complex microwave signals over an instantaneous bandwidth of 20 GHz, with a time resolution below 100  $\mu$ s, 400 resolvable frequency components and a probability of intercept of 100 %. This architecture allows easy further improvements: the time resolution can be improved by using higher frame rate photo-detector, and the number of spectral channels can be increased by implementing for example the 2D geometry proposed in [20].

#### REFERENCES

- [1] K. D. Merkel, W. R. Babbitt, Z. W. Barber, and S. H. Bekker, “Extreme wideband photonic cueing receiver for electronic support: Cswap and fidelity comparisons to an all-digital alternative.” in *GOMACTech 2013 conference*, 2013, pp. 11–14.
- [2] S. Gupta, S. Abielmona, and C. Caloz, *Microwave Theory and Techniques, IEEE Transactions on*, no. 12, pp. 2989–2999, Dec 2009.
- [3] Y. Sun, C. Thiel, R. Cone, R. Equall, and R. Hutcheson, “Recent progress in developing new rare earth materials for hole burning and coherent transient applications,” *Journal of Luminescence*, vol. 98, no. 1–4, pp. 281 – 287, 2002.
- [4] K. Merkel, R. K. Mohan, Z. Cole, T. Chang, A. Olson, and W. Babbitt, “Multi-gigahertz radar range processing of baseband and {RF} carrier modulated signals in tm:yag,” *Journal of Luminescence*, vol. 107, no. 1–4, pp. 62 – 74, 2004.
- [5] T. L. Harris, K. D. Merkel, R. K. Mohan, T. Chang, Z. Cole, A. Olson, and W. R. Babbitt, “Multigigahertz range-doppler correlative signal processing in optical memory crystals,” *Appl. Opt.*, vol. 45, no. 2, pp. 343–352, Jan 2006.
- [6] R. Reibel, Z. Barber, J. Fischer, M. Tian, and W. Babbitt, “Broadband demonstrations of true-time delay using linear sideband chirped programming and optical coherent transients,” *Journal of Luminescence*, vol. 107, no. 1–4, pp. 103 – 113, 2004, proceedings of the 8th International Meeting on Hole Burning, Single Molecule, and Related Spectroscopies: Science and Applications.
- [7] R. R. Reibel, C. Harrington, J. Dahl, C. Ostrander, P. A. Roos, T. Berg, R. K. Mohan, M. A. Neifeld, and W. R. Babbitt, “Demonstrations of analog-to-digital conversion using a frequency domain stretched processor,” *Opt. Express*, vol. 17, no. 14, pp. 11281–11286, Jul 2009.
- [8] H. Linget, L. Morvan, J.-L. L. Gouët, and A. Louchet-Chauvet, “Time reversal of optically carried radiofrequency signals in the microsecond range,” *Opt. Lett.*, vol. 38, no. 5, pp. 643–645, Mar 2013.
- [9] R. Mohan, Z. Cole, R. Reibel, T. Chang, K. Merkel, W. Babbitt, M. Colice, F. Schlottau, and K. H. Wagner, “Microwave spectral analysis using optical spectral hole burning,” in *Microwave Photonics, 2004. MWP'04. 2004 IEEE International Topical Meeting on*, Oct 2004, pp. 24–27.
- [10] G. Gorju, V. Crozatier, I. Lorgere, J.-L. Le Gouet, and F. Bretenaker, “10-ghz bandwidth rf spectral analyzer with mhz resolution based on spectral hole burning in tm3+:yag,” *Photonics Technology Letters, IEEE*, vol. 17, no. 11, pp. 2385–2387, Nov 2005.
- [11] R. K. Mohan, T. Chang, M. Tian, S. Bekker, A. Olson, C. Ostrander, A. Khallaayoun, C. Dollinger, W. Babbitt, Z. Cole, R. Reibel, K. Merkel, Y. Sun, R. Cone, F. Schlottau, and K. Wagner, “Ultra-wideband spectral analysis using {S2} technology,” *Journal of Luminescence*, vol. 127, no. 1, pp. 116 – 128, 2007.
- [12] G. Gorju, A. Chauve, V. Crozatier, I. Lorgere, J.-L. L. Gouët, and F. Bretenaker, “10ghz bandwidth rf spectral analyzer with megahertz resolution based on spectral-spatial holography in tm3+:yag: experimental and theoretical study,” *J. Opt. Soc. Am. B*, vol. 24, no. 3, pp. 457–470, Mar 2007.
- [13] K. Merkel, S. Bekker, C. Stiffler, A. Traxinger, A. Woidtke, P. Sellin, M. Chase, W. Babbitt, Z. Barber, and C. Harrington, “Continuous wideband spectrum analysis over 10 ghz bandwidth with 61 dbc spur-free dynamic range,” in *Microwave Photonics (MWP), 2013 International Topical Meeting on*, Oct 2013, pp. 297–300.
- [14] Z. Barber, C. Harrington, C. Thiel, W. Babbitt, and R. K. Mohan, “Angle of arrival estimation using spectral interferometry,” *Journal of Luminescence*, vol. 130, no. 9, pp. 1614 – 1618, 2010.
- [15] R. Mohan, C. Harrington, T. Sharpe, Z. Barber, and W. Babbitt, “Broadband multi-emitter signal analysis and direction finding using a dual-port interferometric photonic spectrum analyzer based on spatial-spectral materials,” in *Microwave Photonics (MWP), 2013 International Topical Meeting on*, Oct 2013, pp. 241–244.
- [16] T. Chang, M. Tian, R. K. Mohan, C. Renner, K. D. Merkel, and W. R. Babbitt, “Recovery of spectral features readout with frequency-chirped laser fields,” *Opt. Lett.*, vol. 30, no. 10, pp. 1129–1131, May 2005.
- [17] L. Ménager, I. Lorgere, J.-L. L. Gouët, D. Dolfi, and J.-P. Huignard, “Demonstration of a radio-frequency spectrum analyzer based on spectral hole burning,” *Opt. Lett.*, vol. 26, no. 16, pp. 1245–1247, Aug 2001.
- [18] I. Lorgere, L. Ménager, V. Lavielle, J.-L. L. Gouët, D. Dolfi, S. Tonda, and J.-P. Huignard, “Demonstration of a radio-frequency spectrum analyser based on spectral hole burning,” *Journal of Modern Optics*, vol. 49, no. 14-15, pp. 2459–2475, 2002.
- [19] V. Lavielle, I. Lorgere, J.-L. L. Gouët, S. Tonda, and D. Dolfi, “Wideband versatile radio-frequency spectrum analyzer,” *Opt. Lett.*, vol. 28, no. 6, pp. 384–386, Mar 2003.
- [20] V. Lavielle, F. D. Seze, I. Lorgere, and J.-L. L. Gouët, “Wideband radio frequency spectrum analyzer: improved design and experimental results,” *Journal of Luminescence*, vol. 107, no. 1–4, pp. 75 – 89, 2004.
- [21] I. Lorgere, G. Gorju, L. Menager, V. Lavielle, F. Bretenaker, J.-L. Le Gouet, S. Molin, L. Morvan, S. Tonda-Goldstein, D. Dolfi, and J. P. Huignard, “Broadband rf spectrum analyzer based on spectral hole burning,” in *Microwave Photonics, 2009. MWP '09. International Topical Meeting on*, Oct 2009, pp. 1–4.
- [22] Y. T. Chen, “Use of single-mode optical fiber in the stabilization of laser frequency,” *Appl. Opt.*, vol. 28, no. 11, pp. 2017–2021, Jun 1989.
- [23] V. Crozatier, G. Gorju, F. Bretenaker, J.-L. Le Gouet, I. Lorgere, C. Gagnol, and E. Ducloux, “Phase locking of a frequency agile laser,” *Applied Physics Letters*, vol. 89, no. 26, pp. 261115–261115–3, 2006.
- [24] N. Satyan, A. Vasilyev, G. Rakuljic, V. Leyva, and A. Yariv, “Precise control of broadband frequency chirps using optoelectronic feedback,” *Opt. Express*, vol. 17, no. 18, pp. 15991–15999, Aug 2009.
- [25] H. Jiang, F. Kéfélian, P. Lemonde, A. Clairon, and G. Santarelli, “An agile laser with ultra-low frequency noise and high sweep linearity,” *Opt. Express*, vol. 18, no. 4, pp. 3284–3297, Feb 2010.