



Contents lists available at ScienceDirect

Chemical Data Collections

journal homepage: www.elsevier.com/locate/cdc

Data Article

Data on physicochemical properties of borehole water and surface water treated using reverse osmosis [RO] and ultra-violet [UV] radiation water treatment techniques

I.P. Okokpujie ^{a,*}, U.C. Okonkwo ^b, O.S.I. Fayomi ^{a,c}, G.B. Dirusu ^b^a Department of Mechanical Engineering, College of Engineering, Covenant University Ota, Lagos state, Nigeria^b Department of Mechanical Engineering, Nnamdi Azikiwe University, Awka, Nigeria^c Department of Chemical, Metallurgical and Materials Engineering, Faculty of Engineering and the Built Environment, Tshwane University of Technology, Pretoria, South Africa

ARTICLE INFO

Article history:

Received 10 October 2018

Revised 18 February 2019

Accepted 27 February 2019

Available online 28 February 2019

Keywords:

Water

Physicochemical properties

Reverse osmosis

Ultra-violet radiation

ABSTRACT

This article present data on reverse osmosis (RO) and ultra-violet (UV) Radiation Water Treatment Techniques effects on the physicochemical properties of a treated surface water (SW) and borehole water (BHW). The water treatment study which was carried out in Omoku community in River State, lies with latitude 5°13'N and 5°22'N and longitude 6°33'E and 6°42' North West of the Niger Delta region of Nigeria, an area with over Nine hundred oil wells with over thirteen active oil fields and playing host to three multinational companies, due to these activities the water is highly contaminated and causing serious health challenges to the water consumer. Therefore, this research work focus on RO and UV water techniques by applying the physicochemical characteristics method and total Coliform count, with the mechanism to check the influence of both techniques on the pH, temperature, Turbidity, conductivity, Total suspended solids Total dissolved solids of the water for three different samples within the Omoku community. The experiment shows that RO treatment technique produces potable water with reduced mineral content in comparison to the UV treatment.

© 2019 The Authors. Published by Elsevier B.V.
This is an open access article under the CC BY license.
(<http://creativecommons.org/licenses/by/4.0/>)

* Corresponding author.
E-mail address: imhade.okokpujie@covenantuniversity.edu.ng (I.P. Okokpujie).

Specifications Table

Subject area	Engineering, environmental Engineering, Chemical Engineering
Compounds	Water; Dihydrogen oxide
Data category	Absorbance data of Physicochemical Properties and the numerical data analyzed by ANOVA
Data acquisition format	Statistical data of absorbance monitoring from an Industrial 500 L/H Ss reverse osmosis system mineral water treatment machine and 60T–500T Ultraviolet Radiation System water treatment instrument.
Data type	Raw from experimental analysis
Procedure	A sterile sampling bottle was used to collect contaminated water samples from three boreholes at different locations of about 3 km apart and from Orashi flowing River at three (3) different points of at least 7 km apart, using the method of sweeping against the flowing river and all the samples were treated using reverse osmosis (RO) and Ultraviolet radiation (UV) techniques instrument. The treated samples were tested and analyzed for both RO and UV, using physicochemical characteristics method and total Coliform count.
Data accessibility	A complete dataset of Physicochemical Properties of the contaminated water after treatment using the physicochemical characteristics method and total Coliform count is provided in this article

1. Rationale

Water is one of the most significant resources for animal, plant, power generation and also for human comfort [1,2]. Access to good and potable drinking water is a basic need. Water, due to its nature and source often exposes to impurities, which makes such water unfit for human consumption [3,4]. Consumption of contaminated water can lead to loss of human life and animal [5,6]. To improve public health, especially in developing countries, there is need to provide communities with safe and clean water, in order to meet the United Nation Sustainable Developmental Goal of access to water [7–11]. Therefore, constant water treatment is needed.

However, this research data will assist the consumers and water production industry the opportunity to make use of any of the methods in treating water before consumption, such as reverse osmosis (RO) and Ultraviolet radiation (UV) treatment techniques, which will help improving the production output of water industries [12–16]. Table 1 shows some likely effects of chemical pollutant in water.

2. Procedure

The experimental analysis was carried out in Omoku community, River State which is one of the highest onshore oil and gas production communities of Niger Delta. It has over Nine hundred oil wells with over thirteen active oil fields and it host three multinational companies [19,20]. Fig. 1 shows the map of the study area. A sterile sampling bottle was used to collect the water samples from these boreholes. The boreholes were switched on and discharge pipes to the reservoir tank was disconnected to allow the water to flow out for minimum period of 5 min before the raw water was collected in a 4-liter jerry-can with laboratory sanitized standard, and the samples were collected before getting to reservoir tank (elevated plastic tank). Table 2, shows the samples collected from ground and Surface Water (River Orashi).

The water samples were treated using reverse osmosis (RO) and Ultraviolet radiation (UV) techniques and to determine the effect of the treatment technique. The water samples were taken for laboratory analysis at Nigerian Agip Oil Company (NAOC) chemical industrial laboratory (located in Aya-Gologo, Port Harcourt, the distance between the sample location and the laboratory is 81.3 km and the lagging time between sample collection to the laboratory is 1 h 20 min. via Elele-Isokpo-Umuele Rd/A231 and Ikiri Airport Road from the Omoku community) for various physicochemical characteristics

Table 1

Health effects of selected chemical pollutants [17,18].

Chemical	Source	Health effect
Inorganic salts e.g. Fluoride	Natural occurring	Yellowing of the teeth and damage to the spinal cord and other crippling diseases
Arsenic	Natural-occurring	Arsenic poisoning—cause liver and nervous system damage, vascular diseases and also skin cancers.
Lead	Pipes fittings solder, and the service connections of water pipes	Lead poisoning; damage, brain of children
Mercury	Gold mining from stream deposits	Mercury poisoning
Benzene	Underground petroleum storage tank	Direct toxicity; causes leukemia
Chlorinated Solvents	Laundry agents, e.g. bleaches and stain removers electronic plastic and aircraft manufacture	Direct toxicity; damages reproductive disorders, carcinogenic
Pesticides	Petrochemicals	Damage nervous system, causes
Nitrates	Internal combustion engines, Nitrate fertilizers	Restricts the amount of oxygen that reaches the brain causing the 'blue baby' syndrome. It is also linked to digestive tract cancers
Crude oil	Petroleum refinery	Toxic, some fractions are carcinogenic

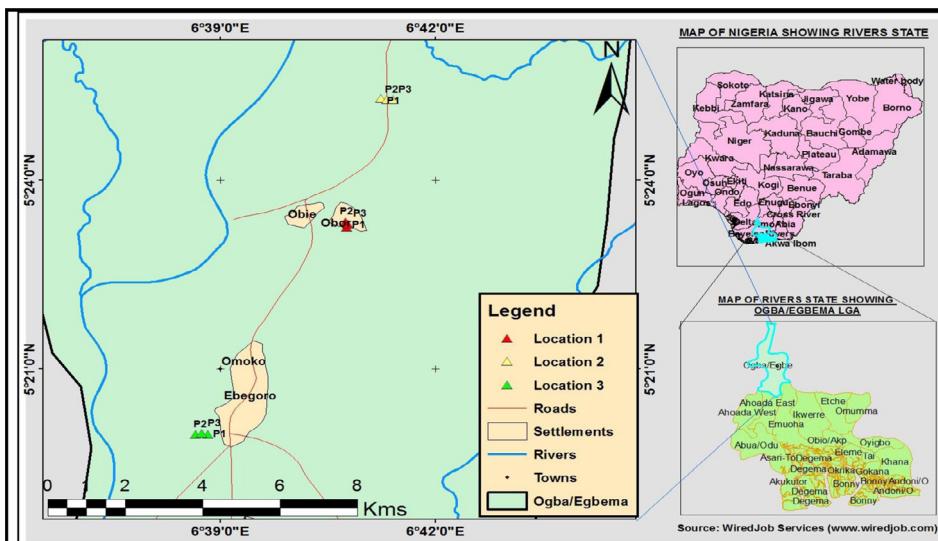


Fig. 1. Map of the study area: source [20].

Table 2
Borehole water and surface water sampling sites.

Borehole Sample	Depth of the borehole (m)	Volume (L)	Surface water sample (Orashi flowing River)
BH1	25	1	7 km apart from each sample
BH2	35	1	7 km apart from each sample
BH3	40	1	7 km apart from each sample

and Coliform count the water was analyzed to determine their physicochemical characteristics. The parameters characterized include pH, electrical conductivity, temperature, total hardness, turbidity, total dissolved solids, total suspended solids, Nutrients such as Nitrate, Sulphate and Chloride, mineral elements such as potassium, sodium and magnesium as well as heavy metals such as Iron, Lead, Chromium and Arsenic and the instrument used to carried out this various tests are ORION 1260, thermometric determination, electrometric method, 2100 T-metre, APHA 2540D, TDS and TDS metre, ASTM D512 titrimetric Method, APHA 4500-NO₃ B method respectively for the parameters. These parameters are indicators of purity levels of water.

3. Data, value and validation

The significance of the raw data acquired from the experiment analysis during the application of RO and UV techniques in water treatment, along with the physicochemical characteristics and Coliform count of the various samples, are stated as follows:

- The data set will give researchers and water production industry, and environmental engineers the optimum parameters to carry out water treatment with both the reverse osmosis (RO) and Ultraviolet radiation (UV) techniques in other to produce safe drinking water at lower cost.
- The data in this study focus on the physicochemical properties of water treated with reverse osmosis and ultraviolet radiation treatment process, to enable author and small scale industry analyse and understand the process of water treatment and make use of the data to eliminate water pollution from the community.
- The data given can be used to study the correlation between physicochemical parameters at different levels of concentrations.
- This data set can also be used in treating the water used to generate power via steam turbine power plant in other to avoid corrosion in the boiler feed drum and in other mechanical components.

The data obtained from all the experimental test analysis for RO and UV are shown in Tables 3–21. The data was subjected to descriptive and two-way analysis of variance (ANOVA) statistics to test the significant difference in the effectiveness of the RO and UV water treatment, in both borehole (BH) and surface water (SW) at 95% confidence limit on the physicochemical properties of the water, as shown in Tables 21–39 respectively. Fig. 2, shows the surface plot of Total Coliform (MPN/100 ml) in BH and SW treated samples with RO (T) and UV (T) and untreated water used as the control.

Table 3
Effect of RO and UV techniques on borehole and surface water to determine the pH.

Source	RO (T)	UV(T)	Control	WHO (pH)
BH ₁	6.50	6.98	6.25	6.5-
BH ₂	6.50	6.70	6.20	7.5
BH ₃	6.55	6.60	6.00	
SW ₁	7.00	6.98	6.98	
SW ₂	5.99	6.00	6.00	
SW ₃	6.00	6.25	6.85	

Table 4
Effect of RO and UV techniques on borehole and surface water to determine the temperature.

Source	R.O (T)	UV (T)	Control	WHO-limit
BH ₁	32.00	320.00	31.00	No limit specified
BH ₂	33.00	30.00	31.00	
BH ₃	33.00	30.00	32.00	
SW ₁	32.00	30.00	31.00	
SW ₂	34.20	32.00	31.00	
SW ₃	35.10	33.00	32.50	

Table 5
Effect of reverse osmosis (RO) and ultra-violet radiation (UV) techniques on borehole and surface water to determine water conductivity.

Source	RO(T)	UV(T)	Control	WHO-limit
BH ₁	43.00	43.00	43.00	<1050.0 μ s/mm
BH ₂	38.00	42.00	42.20	
BH ₃	40.00	40.00	42.00	
SW ₁	405.00	428.10	525.00	
SW ₂	750.00	900.00	1000.00	
SW ₃	120.20	776.70	875.00	

Table 6
Effect of water treatment on turbidity of borehole and surface water.

Source	RO	UV	Control	WHO
BH ₁	0.00001	0.00001	0.00001	<5.00
BH ₂	0.00001	0.00001	0.00001	
BH ₃	0.00001	0.00001	0.00001	
SW ₁	7.00	23.38	23.00	
SW ₂	15.00	33.50	33.50	
SW ₃	14.00	25.34	25.34	

Table 7
Effect of water treatment on total suspended solid (TSS) of borehole and surface water total suspend solid (TSS).

Source	RO (T)	UV	Control	WHO
BH ₁	0.00001	0.00001	0.00001	<5.00 ppm
BH ₂	0.0001	0.00001	0.00001	
BH ₃	0.0001	0.00001	0.00001	
SW ₁	8.50	42.00	45.000	
SW ₂	8.25	50.20	47.20	
SW ₃	10.50	47.10	38.50	

Table 8
Effect of water treatment on total dissolved solid (TDS) of borehole and surface water.

Sources	RO	UV	Control	WHO
BH ₁	0.50	15.00	17.00	00–999 ppm
BH ₂	5.00	15.00	20.00	
BH ₃	5.00	20.00	25.12	
SW ₁	10.00	40.00	500.0	
SW ₂	11.00	45.20	800.00	
SW ₃	20.00	40.99	459.99	

Table 9

Effect of water treatment on salinity (chloride content) of the borehole and surface water.

Sources	RO	UV	Control	WHO
BH ₁	10.00	20.20	39.99	<250 mg/l
BH ₂	10.50	22.00	42.01	
BH ₃	15.00	22.50	40.02	
SW ₁	20.00	15.00	75	
SW ₂	19.90	17.00	100	
SW ₃	20.00	16.00	50	

Table 10

Effect of water treatment on total hardness of borehole and surface water.

Source	RO	UV	Control	WHO
BH ₁	0.09	1.20	2.99	No
BH ₂	1.00	1.22	2.89	limit
BH ₃	0.98	1.25	2.01	
SW ₁	1.00	97.00	207.00	
SW ₂	0.01	100.20	220.20	
SW ₃	0.05	120.87	198.87	

Table 11

Effect of water treatment on nutrients levels (Nitrate and Sulphate) of borehole and surface water.

Source	RO	UV	Control	WHO-limit
BH ₁	0.10	0.11	0.11	<50 mg/l
BH ₂	0.10	0.20	0.21	
BH ₃	0.12	0.30	0.32	
SW ₁	90.00	50.76	150.76	
SW ₂	110.00	20.00	200.00	
SW ₃	180.00	18.50	190.50	

Table 12Concentration of sulphate (SO_4^{2-}) (g/ml) in borehole and surface water samples treated with reverse osmosis (RO (T)) and ultra-violet radiation (RO (T)) and control.

Source	RO	UV	Control	WHO
BH ₁	1.0	1.00	1.00	<500 mg/l
BH ₂	1.10	1.10	1.10	
BH ₃	2.00	2.12	2.12	
SW ₁	50.00	101.01	20.01	
SW ₂	45.00	100.00	15.00	
SW ₃	22.10	180.90	17.90	

Table 13Concentration of Sodium (Na^+) ion in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO
BH ₁	0.01	0.07	0.07	<200 mg/l
BH ₂	0.01	0.08	0.09	
BH ₃	0.01	0.07	0.08	
SW ₁	35.00	20.05	34.45	
SW ₂	37.00	19.00	45.00	
SW ₃	30.50	19.99	29.99	

Table 14

Concentration of Magnesium (Mg) (g/ml) in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO
BH ₁	0.01	0.04	0.06	<0.5 mg/l
BH ₂	0.01	0.45	0.04	
BH ₃	0.01	0.50	0.09	
SW ₁	24.00	20.09	45.09	
SW ₂	35.00	21.15	79.00	
SW ₃	40.00	21.55	78.79	

Table 15

Concentration of Potassium (K) ion (g/ml) in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO-limit
BH ₁	0.01	0.80	3.03	<50.0 mg/l
BH ₂	0.01	1.00	2.98	
BH ₃	0.02	2.00	2.67	
SW ₁	29.50	30.00	50.00	
SW ₂	30.11	35.00	75.00	
SW ₃	32.00	40.00	45.00	

3.1. Effect of RO and UV techniques on concentration of heavy metals of borehole and surface water on Cadmium (Cd), Iron (Fe), Lead (Pb), Arsenic (As) and Chromium (Cr)

Table 16

Concentration of Cadmium (Cd⁻) (g/ml) in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO-limit
BH ₁	0.00001	0.00001	0.00001	<0.003 mg/l
BH ₂	0.00001	0.00001	0.00001	
BH ₃	0.00001	0.00001	0.00001	
SW ₁	0.00001	0.09	1.09	
SW ₂	0.00001	0.02	12.12	
SW ₃	0.00001	0.01	0.99	

Table 17

Concentration of iron (Fe) (g/ml) in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO-limit
BH ₁	0.00001	0.01	0.02	No limit specified
BH ₂	0.00001	0.01	0.01	
BH ₃	0.00001	0.01	0.02	
SW ₁	0.00001	1.20	1.24	
SW ₂	0.00001	1.50	1.55	
SW ₃	0.00001	1.50	1.56	

Table 18

Concentration of Lead (Pb) (g/ml) in borehole and surface water samples treated with RO (T) and ultra- UV (T) and CTRL.

Source	RO	UV	Control	WHO-limit
BH ₁	0.0001	0.0001	0.0001	<0.01 mg/l
BH ₂	0.0001	0.0001	0.0001	
BH ₃	0.0001	0.0001	0.0001	
SW ₁	1.10	4.20	5.00	
SW ₂	1.50	5.10	7.10	
SW ₃	0.50	5.40	6.40	

Table 19

Concentration of Arsenic (As) (g/ml) in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO-limit
BH ₁	0.0001	0.0001	0.0001	<0.01 mg/l
BH ₂	0.0001	0.0001	0.0001	
BH ₃	0.0001	0.0001	0.0001	
SW ₁	0.02	0.09	0.9	
SW ₂	0.99	1.32	1.32	
SW ₃	0.02	0.08	0.08	

Table 20

Concentration of Chromium (Cr) (g/ml) in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO-limit
BH ₁	0.0001	0.001	0.11	0.003 mg/l
BH ₂	0.0001	0.001	0.12	
BH ₃	0.0001	0.001	0.01	
SW ₁	0.01	0.92	0.92	
SW ₂	0.01	1.09	1.09	
SW ₃	0.09	1.01	1.01	

Table 21

Total Coliform (MPN/100 ml) in borehole and surface water samples treated with RO (T) and UV (T) and CTRL.

Source	RO	UV	Control	WHO-limit
BH ₁	0.0001	0.009	1.01	0.005 mg/l
BH ₂	0.0001	0.008	0.09	
BH ₃	0.0001	0.005	0.05	
SW ₁	1.100	2.00	15.00	
SW ₂	1.100	2.50	10.00	
SW ₃	1.500	5.00	50.00	

3.2. Two-way analysis of variance for RO and UV techniques showing the significance in treating surface water and borehole water

Table 22

Anova of two-factor with replication (pH).

Summary	RO(T)	UV(T)	Control	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	19.55	20.28	18.45	58.28
Average	6.52	6.76	6.15	6.48
Variance	0.000833	0.0388	0.0175	0.085003
SD	0.029	0.197	0.132	0.292
<i>SW1</i>				
Count	3	3	3	9
Sum	18.99	19.23	19.83	58.05
Average	6.33	6.41	6.61	6.45
Variance	0.3367	0.2593	0.2833	0.235425
SD	0.580	0.509	0.532	0.485
<i>Total</i>				
Count	6	6	6	
Sum	38.54	39.51	38.28	
Average	6.423333	6.585	6.38	
Variance	0.145467	0.15599	0.1838	
Anova				
<i>Source of Variation</i>	<i>SS</i>	<i>df</i>	<i>MS</i>	<i>F</i>
Sample	0.002939	1	0.002939	0.01883
Trt	0.140078	2	0.070039	0.448759
Interaction	0.550478	2	0.275239	1.763535
Within	1.872867	12	0.156072	0.213084
Total	2.566361	17		3.885294

Table 23

Anova of two-factor with replication temperature.

Summary	RO(T)	UV(T)	Control	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	98	92	94	284
Average	32.67	30.67	31.33	31.56
Variance	0.333333	1.333333	0.333333	1.277778
SD	0.577	1.155	0.577	1.130
<i>SW1</i>				
Count	3	3	3	9
Sum	101.3	95	94.5	290.8
Average	33.77	31.67	31.50	32.31
Variance	2.543333	2.333333	0.75	2.603611
SD	1.595	1.528	0.866	1.614
<i>Total</i>				
Count	6	6	6	
Sum	199.3	187	188.5	
Average	33.21667	31.16667	31.41667	
Variance	1.513667	1.766667	0.441667	
Anova				
Source of Variation	SS	df	MS	F
Sample	2.568889	1	2.568889	2.020979
Trt	15.01	2	7.505	5.904283
Interaction	0.787778	2	0.393889	0.309878
Within	15.25333	12	1.271111	
Total	33.62	17		
P-value				
				0.180605
				4.747225
				0.016394
				3.885294
				0.739234
				3.885294
F crit				

*Sig at $p < 0.05$.**Table 24**

Anova of two-factor with replication for water conductivity.

Summary	RO(T)	UV(T)	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	121	125	127.2	373.2
Average	40.33	41.67	42.40	41.47
Variance	6.333333	2.333333	0.28	3.06
SD	2.517	1.528	0.529	1.749
<i>SW1</i>				
Count	3	3	3	9
Sum	1275.2	2104.8	2400	5780
Average	425.07	701.60	800.00	642.22
Variance	99,464.013	59,902.41	60,625	83,338.9
SD	315.379	244.750	246.221	288.685
<i>Total</i>				
Count	6	6	6	
Sum	1396.2	2229.8	2527.2	
Average	232.7	371.63333	421.2	
Variance	84,194.06	154,615.5	196,437	
Anova				
Source of Variation	SS	Df	MS	F
Sample	1,624,082.6	1	1,624,083	44.2931
Columns	114,583.15	2	57,291.6	1.56249
Interaction	112,151.68	2	56,075.8	1.52934
Within	440,000.74	12	36,666.7	0.256075
Total	2,290,818.1	17		
P-value				
				2.34E-05
				4.74723
				0.249412
				3.88529
				0.256075
				3.88529
F crit				

Table 25

Anova: two-factor with replication for turbidity.

Summary	RO	UV	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	0.00003	0.00003	0.00003	0.00009
Average	0.00001	0.00001	0.00001	0.00001
Variance	0	0	0	0
SD	0.000	0.000	0.000	0.000
<i>SW1</i>				
Count	3	3	3	9
Sum	36	82.22	81.84	200.06
Average	12	27.40667	27.28	22.2289
Variance	19	28.8069333	30.3852	78.40551
SD	4.359	5.367	5.512	8.855
<i>Total</i>				
Count	6	6	6	
Sum	36.00003	82.22003	81.84003	
Average	6.000005	13.7033383	13.640005	
Variance	50.799928	236.860222	235.413436	
Anova				
<i>Source of Variation</i>	<i>SS</i>	<i>df</i>	<i>MS</i>	<i>F</i>
Sample	2223.5538	1	2223.55375	170.6223
trtment	235.42991	2	117.714956	9.032747
Interaction	235.42991	2	117.714956	9.032747
Within	156.38427	12	13.0320222	0.004043
Total	2850.7978	17		3.885294

Table 26

Anova of two-factor with replication for TSS.

Summary	RO(T)	UV(T)	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	0.00021	0.00003	0.00003	0.00027
Average	0.00007	0.00001	0.00001	0.00003
Variance	2.7E-09	0	0	1.575E-09
SD	0.000	0.000	0.000	0.000
<i>SW1</i>				
Count	3	3	3	9
Sum	27.25	139.3	130.7	297.25
Average	9.08	46.43	43.57	33.03
Variance	1.5208333	17.143333	20.4633333	333.82444
SD	1.233	4.140	4.524	18.271
<i>Total</i>				
Count	6	6	6	
Sum	27.25021	139.30003	130.70003	
Average	4.5417017	23.216672	21.7833383	
Variance	25.360035	653.67339	577.601405	
Anova				
<i>Source of Variation</i>	<i>SS</i>	<i>Df</i>	<i>MS</i>	<i>F</i>
Sample	4908.7446	1	4908.74455	752.73062
Columns	1296.166	2	648.082984	99.380178
Interaction	1296.1746	2	648.087294	99.380839
Within	78.255	12	6.52125	3.41E-08
Total	7579.3401	17		3.885294

Table 27

Anova of two-factor with replication TDS.

Summary	RO(T)	UV(T)	CTRL	Total		
<i>BH1</i>						
Count	3	3	3	9		
Sum	10.5	50	62.12	122.62		
Average	3.50	16.67	20.71	13.62		
Variance	6.75	8.333333	16.85813	68.70438		
SD	2.598	2.887	4.106	8.289		
<i>SW1</i>						
Count	3	3	3	9		
Sum	41	126.19	1759.99	1927.18		
Average	13.67	42.06	586.66	214.13		
Variance	30.33333	7.624033	34,534.6	86,858.23		
SD	5.508	2.761	185.835	294.717		
<i>Total</i>						
Count	6	6	6			
Sum	51.5	176.19	1822.11			
Average	8.583333	29.365	303.685			
Variance	45.84167	199.8802	109,912.7			
Anova						
Source of Variation	SS	df	MS	F		
Sample	180,913.2	1	180,913.2	31.36814		
Columns	325,536.7	2	162,768.3	28.22205		
Interaction	300,669.8	2	150,334.9	26.06625		
Within	69,209	12	5767.416	4.29E-05		
Total	876,328.6	17		3.885294		
Source of Variation	SS	df	MS	F	P-value	F crit

Table 28

Anova of two-factor with replication for the water salinity.

Summary	RO(T)	UV(T)	CTRL	Total		
<i>BH1</i>						
Count	3	3	3	9		
Sum	35.5	64.7	122.02	222.22		
Average	11.83	21.57	40.67	24.69		
Variance	7.5833333	1.4633333	1.3402333	164.04024		
SD	2.754	1.210	1.158	12.808		
<i>SW1</i>						
Count	3	3	3	9		
Sum	59.9	48	225	332.9		
Average	19.97	16.00	75.00	36.99		
Variance	0.0033333	1	625	972.17611		
SD	0.058	1.000	25.000	31.180		
<i>Total</i>						
Count	6	6	6			
Sum	95.4	112.7	347.02			
Average	15.9	18.783333	57.836667			
Variance	22.88	10.281667	604.03211			
Anova						
Source of Variation	SS	Df	MS	F		
Sample	680.55902	1	680.55902	6.4164312		
Columns	6584.3209	2	3292.1605	31.039073		
Interaction	1232.6294	2	616.31469	5.8107242		
Within	1272.7805	12	106.06504	0.017189		
Total	9770.2898	17		3.885294		
Source of Variation	SS	Df	MS	F	P-value	F crit

Table 29

Anova of two-factor with replication for total hardness.

Summary	RO(T)	UV(T)	Control	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	2.07	3.67	7.89	13.63
Average	0.69	1.22	2.63	1.51
Variance	0.2701	0.0006333	0.2908	0.8937278
SD	0.520	0.025	0.539	0.945
<i>SW1</i>				
Count	3	3	3	9
Sum	1.06	318.07	626.07	945.2
Average	0.35	106.02	208.69	105.02
Variance	0.314033	167.87763	115.8843	8209.864
SD	0.560	12.957	10.765	90.608
<i>Total</i>				
Count	6	6	6	
Sum	3.13	321.74	633.96	
Average	0.521667	53.623333	105.66	
Variance	0.267657	3362.0633	12,784.687	
Anova				
Source of Variation	SS	Df	F	P-value F crit
Sample	48,212.37	1	48,212.37	1016.2899 5.73E-13 4.747225
Columns	33,163.34	2	16,581.671	349.53239 2.31E-11 3.885294
Interaction	31,953.45	2	15,976.723	336.78042 2.88E-11 3.885294
Within	569.275	12	47,439583	
Total	113,898.4	17		

Table 30

Anova of two-factor with replication for Nitrate.

Summary	RO(T)	UV(T)	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	0.32	0.61	0.64	1.57
Average	0.11	0.20	0.21	0.17
Variance	0.0001333	0.009	0.011033	0.00765
SD	0.012	0.095	0.105	0.087
<i>SW1</i>				
Count	3	3	3	9
Sum	380	89.26	541.26	1010.52
Average	126.67	29.75	180.42	112.28
Variance	2233.3333	331.5	682.3492	5184.56
SD	47.258	18.208	26.122	72.004
<i>Total</i>				
Count	6	6	6	
Sum	380.32	89.87	541.9	
Average	63.386667	14.98	90.31667	
Variance	5698.5635	394.6	10,015.28	
Anova				
Source of Variation	SS	df	MS	F P-value F crit
Sample	56,554.45	1	56,554.45	104.497 2.82E-07 4.747
Columns	17,488.912	2	8744.456	16.1574 0.000394 3.885
Interaction	17,493.168	2	8746.584	16.1613 0.000394 3.885
Within	6494.4505	12	541.2042	
Total	98,030.981	17		

Table 31

Anova of two-factor with replication for Sulphate.

Summary	RO(T)	UV(T)	CTRL	Total	
<i>BH1</i>					
Count	3	3	3	9	
Sum	4.1	4.22	4.22	12.54	
Average	1.37	1.41	1.41	1.39	
Variance	0.303333	0.3841	0.38413	0.2683	
SD	0.551	0.620	0.620	0.518	
<i>SW1</i>					
Count	3	3	3	9	
Sum	117.1	381.91	52.91	551.92	
Average	39.03	127.30	17.64	61.32	
Variance	221.3033	2154.7	6.32703	3130.108	
SD	14.876	46.419	2.515	55.947	
<i>Total</i>					
Count	6	6	6		
Sum	121.2	386.13	57.13		
Average	20.2	64.355	9.52167		
Variance	514.276	5617	81.7083		
Anova					
Source of Variation	SS	df	MS	F	
Sample	16,162.82	1	16,162.8	40.68833	
Columns	10,140.77	2	5070.39	12.7642	
Interaction	10,135.42	2	5067.71	12.75747	
Within	4766.818	12	397.235		
Total	41,205.83	17			
Source of Variation	SS	df	F	P-value	F crit

Table 32

Anova of two-factor with replication for Sodium.

Summary	RO(T)	UV(T)	CTRL	Total	
<i>BH1</i>					
Count	3	3	3	9	
Sum	0.03	0.22	0.24	0.49	
Average	0.010	0.073	0.080	0.054	
Variance	0	3.33E-05	0.0001	0.001153	
SD	0.000	0.006	0.010	0.034	
<i>SW1</i>					
Count	3	3	3	9	
Sum	102.5	59.04	109.44	270.98	
Average	34.167	19.680	36.480	30.109	
Variance	11.08333	0.3477	59.4157	79.89356	
SD	3.329	0.590	7.708	8.938	
<i>Total</i>					
Count	6	6	6		
Sum	102.53	59.26	109.68		
Average	17.08833	9.876667	18.28		
Variance	354.4367	115.4655	421.2543		
Anova					
Source of Variation	SS	df	MS	F	
Sample	4064.713	1	4064.713	344.2394	
Columns	248.0884	2	124.0442	10.50527	
Interaction	249.3755	2	124.6878	10.55977	
Within	141.6937	12	11.80781		
Total	4703.871	17			
Source of Variation	SS	df	F	P-value	F crit

Table 33

Anova of two-factor with replication for Magnesium.

Summary	RO(T)	UV(T)	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	0.03	0.99	0.19	1.21
Average	0.01	0.33	0.06	0.13
Variance	0	0.0637	0.000633	0.038128
SD	0.000	0.252	0.025	0.195
<i>SW1</i>				
Count	3	3	3	9
Sum	99	62.79	202.88	364.67
Average	33.00	20.93	67.63	40.52
Variance	67	0.5692	380.937	552.7853
SD	8.185	0.754	19.518	23.511
<i>Total</i>				
Count	6	6	6	
Sum	99.03	63.78	203.07	
Average	16.505	10.63	33.845	
Variance	353.302	127.5612	1521.816	
Anova				
Source of Variation	SS	df	MS	F
Sample	7339.065	1	7339.065	98.16603
Columns	1748.255	2	874.1275	11.69217
Interaction	1777.191	2	888.5955	11.8857
Within	897.1411	12	74.76176	0.001425
Total	11,761.65	17		
				P-value F crit

Table 34

Anova of two-factor with replication for Potassium.

Summary	RO(T)	UV(T)	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	0.04	3.8	8.68	12.52
Average	0.01	1.27	2.89	1.39
Variance	3.333E-05	0.4133333	0.0380333	1.6767611
SD	0.006	0.643	0.195	1.295
<i>SW1</i>				
Count	3	3	3	9
Sum	91.61	105	170	366.61
Average	30.54	35.00	56.67	40.73
Variance	1.6990333	25	258.33333	217.77593
SD	1.303	5.000	16.073	14.757
<i>Total</i>				
Count	6	6	6	
Sum	91.65	108.8	178.68	
Average	15.275	18.133333	29.78	
Variance	280.18179	351.54667	970.81996	
Anova				
Source of Variation	SS	df	MS	F
Sample	6965.5405	1	6965.5405	146.39446
Columns	708.41988	2	354.20994	7.444415
Interaction	476.2341	2	238.11705	5.0044958
Within	570.96753	12	47.580628	0.026272
Total	8721.162	17		
				P-value F crit

Table 35

Anova of two-factor with replication for Cadmium.

Summary	RO(T)	UV(T)	CTRL	Total		
<i>BH1</i>						
Count	3	3	3	9		
Sum	0.00003	0.00003	0.00003	0.00009		
Average	0.00001	0.00001	0.00001	0.00001		
Variance	0	0	0	0		
SD	0.000	0.000	0.000	0.000		
<i>SW1</i>						
Count	3	3	3	9		
Sum	0.00003	0.12	14.2	14.32003		
Average	0.00001	0.04000	4.73333	1.59111		
Variance	0	0.0019	40.924633	15.785799		
SD	0.000	0.044	6.397	3.973		
<i>Total</i>						
Count	6	6	6			
Sum	0.00006	0.12003	14.20003			
Average	0.00001	0.020005	2.3666717			
Variance	0	0.0012398	23.091158			
Anova						
Source of Variation	SS	df	MS	F		
Sample	11.39226	1	11.39226	1.6701527		
Columns	22.216663	2	11.108332	1.6285276		
Interaction	22.216663	2	11.108332	1.6285276		
Within	81.853067	12	6.8210889	0.236735		
Total	137.67865	17		3.885294		
Source of Variation	SS	df	MS	F	P-value	F crit

Table 36

Anova of two-factor with replication for Iron.

Summary	RO(T)	UV(T)	CTRL	Total		
<i>BH1</i>						
Count	3	3	3	9		
Sum	0.00003	0.03	0.05	0.08003		
Average	0.00001	0.01000	0.01667	0.00889		
Variance	0	0	3.333E-05	6.104E-05		
SD	0.000	0.000	0.006	0.008		
<i>SW1</i>						
Count	3	3	3	9		
Sum	0.00003	4.2	4.35	8.55003		
Average	0.00001	1.40000	1.45000	0.95000		
Variance	0	0.03	0.0331	0.5238929		
SD	0.000	0.173	0.182	0.724		
<i>Total</i>						
Count	6	6	6			
Sum	0.00006	4.23	4.4			
Average	0.00001	0.705	0.7333333			
Variance	0	0.59163	0.6295867			
Anova						
Source of Variation	SS	df	MS	F		
Sample	3.98560556	1	3.9856056	378.77983		
Columns	2.07115358	2	1.0355768	98.418069		
Interaction	1.99421111	2	0.9971056	94.76188		
Within	0.12626667	12	0.0105222	4.46E-08		
Total	8.17723691	17		3.885294		
Source of Variation	SS	df	MS	F	P-value	F crit

Table 37

Anova of two-factor with replication for Lead.

Summary	RO(T)	UV(T)	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	0.0003	0.0003	0.0003	0.0009
Average	0.0001	0.0001	0.0001	0.0001
Variance	0	0	0	2.066E-40
SD	0.000	0.000	0.000	0.000
<i>SW1</i>				
Count	3	3	3	9
Sum	3.1	14.7	18.5	36.3
Average	1.0333	4.9000	6.1667	4.0333
Variance	0.2533333	0.39	1.1433333	5.81
SD	0.503	0.624	1.069	2.410
<i>Total</i>				
Count	6	6	6	
Sum	3.1003	14.7003	18.5003	
Average	0.5167167	2.45005	3.0833833	
Variance	0.4216047	7.358706	11.865297	
Anova				
Source of Variation	SS	df	MS	F
Sample	73.20137	1	73.20137	245.8255
Columns	21.453333	2	10.726667	36.022388
Interaction	21.453333	2	10.726667	36.022388
Within	3.5733333	12	0.2977778	8.47E-06
Total	119.68137	17		3.885294
				P-value F crit

Table 38

Anova of two-factor with replication for Arsenic.

Summary	RO(T)	UV(T)	CTRL	Total
<i>BH1</i>				
Count	3	3	3	9
Sum	0.0003	0.0003	0.0003	0.0009
Average	0.0001	0.0001	0.0001	0.0001
Variance	0	0	0	2.07E-40
SD	0.000	0.000	0.000	0.000
<i>SW1</i>				
Count	3	3	3	9
Sum	1.03	1.49	2.3	4.82
Average	0.3433	0.4967	0.7667	0.5356
Variance	0.313633	0.508433	0.397733	0.339403
SD	0.560	0.713	0.631	0.583
<i>Total</i>				
Count	6	6	6	
Sum	1.0303	1.4903	2.3003	
Average	0.171717	0.248383	0.383383	
Variance	0.160796	0.277347	0.335381	
Anova				
Source of Variation	SS	df	MS	F
Sample	1.290207	1	1.290207	6.34632
Columns	0.137811	2	0.068906	0.338935
Interaction	0.137811	2	0.068906	0.338935
Within	2.4396	12	0.2033	0.719134
Total	4.005429	17		3.885294
				P-value F crit

Table 39

Anova of two-factor with replication for Chromium.

Summary	RO(T)	UV(T)	CTRL	Total		
<i>BH1</i>						
Count	3	3	3	9		
Sum	0.0003	0.003	0.24	0.2433		
Average	0.0001	0.0010	0.0800	0.0270		
Variance	0	0	0.0037	0.002503		
SD	0.000	0.000	0.061	0.050		
<i>SW1</i>						
Count	3	3	3	9		
Sum	0.11	3.02	3.02	6.15		
Average	0.0367	1.0067	1.0067	0.6833		
Variance	0.002133	0.007233	0.007233	0.239375		
SD	0.046	0.085	0.085	0.489		
<i>Total</i>						
Count	6	6	6			
Sum	0.1103	3.023	3.26			
Average	0.018383	0.503833	0.543333			
Variance	0.001254	0.306303	0.261987			
Anova						
Source of Variation	SS	df	MS	F		
Sample	1.938284	1	1.938284	572.8917		
Columns	1.025589	2	0.512794	151.5649		
Interaction	0.868837	2	0.434418	128.3995		
Within	0.0406	12	0.003383	7.92E-09		
Total	3.873309	17		3.885294		
Source of Variation	SS	df	MS	F	P-value	F crit

Table 40

Anova of two-factor with replication for Coliform.

Summary	RO(T)	UV(T)	CTRL	Total		
<i>BH1</i>						
Count	3	3	3	9		
Sum	0.0003	0.022	1.15	1.1723		
Average	0.0001	0.0073	0.3833	0.1303		
Variance	0	4.333E-06	0.29493333	0.1097714		
SD	0.000	0.002	0.543	0.331		
<i>SW1</i>						
Count	3	3	3	9		
Sum	3.7	9.5	75	88.2		
Average	1.2333	3.1667	25.0000	9.8000		
Variance	0.0533333	2.5833333	475	250.07		
SD	0.231	1.607	21.794	15.814		
<i>Total</i>						
Count	6	6	6			
Sum	3.7003	9.522	76.15			
Average	0.6167167	1.587	12.6916667			
Variance	0.4775927	4.0277512	371.912057			
Anova						
Source of variation	SS	df	MS	F		
Sample	420.76781	1	420.767809	5.2823601		
Columns	540.11898	2	270.059489	3.3903532		
Interaction	505.45598	2	252.727992	3.1727719		
Within	955.86321	12	79.6552674	0.078326		
Total	2422.206	17		3.885294		
Source of variation	SS	df	MS	F	P-value	F crit

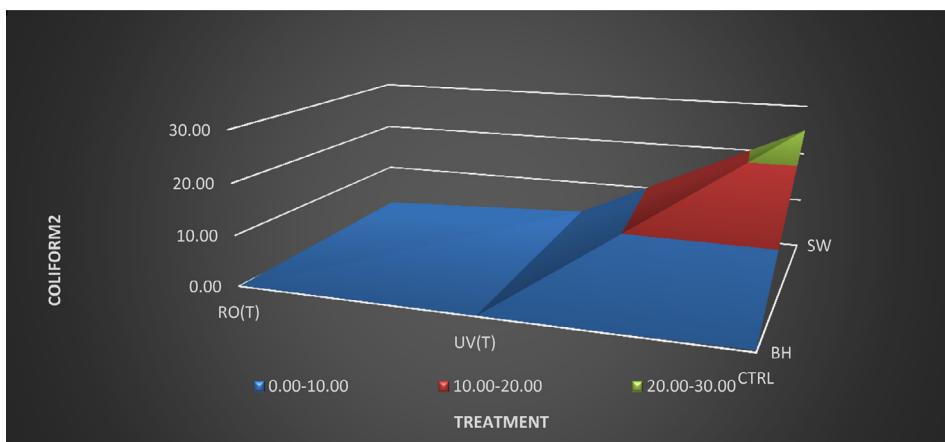


Fig. 2. The surface plot of Total Coliform (MPN/100 ml) in borehole and surface water samples treated with RO (T) and UV (T) and untreated water CTRL.

Acknowledgements

The authors hereby acknowledge the management of Covenant University for their financial support for open access publication.

References

- [1] Y. Jin, H. Lee, M. Zhan, S. Hong, UV radiation pre-treatment for reverse osmosis (RO) process in ultrapure water (UPW) production, *Desalination* 439 (2018 Aug 1) 138–146.
- [2] M.A. Al-Obaidi, C. Kara-Zaitri, I.M. Mujtaba, Performance evaluation of multi-stage and multi-pass reverse osmosis networks for the removal of N-nitrosodimethylamine – D6 (NDMA) from wastewater using model-based techniques, *J. Env. Chem. Eng.*, 6, (2018 Jun 6) 4797–4808.
- [3] H. Biglari, M. Saeidi, K. Karimyan, M.R. Narooie, H. Sharifi, Data for factor analysis of hydro-geochemical characteristics of groundwater resources in Iranshahr, *Data Brief* 19 (2018 Aug 1) 548–563.
- [4] D.O. Omole, A. Ogbiye, E. Longe, I. Adewumi, Water quality checks on River Atuwara, South-West Nigeria, *Water Pollut.* XIV 228 (2018 Aug 21) 165.
- [5] A.A. Badejo, D.O. Omole, J.M. Ndambuki, Municipal wastewater management using *Vetiveria zizanioides* planted in vertical flow constructed wetland, *Appl. Water Sci.* 8 (4) (2018 Jul 1) 110.
- [6] A.S. Ogbiye, D.O. Omole, K.D. Ade-Balogun, O. Onakunle, O.O. Elemile, Treatment of brewery wastewater using electro-Fenton and granulated activated carbon, *Cogent Eng.* 5 (1) (2018 Jan 1) 1447224.
- [7] D.O. Omole, P.C. Emenike, I.T. Tenebe, A.O. Akinde, A.A. Badejo, An assessment of water related diseases in a Nigerian community, *Res. J. Appl. Sci. Eng. Technol.* 10 (7) (2018 Jul 10) 776–781.
- [8] I.T. Tenebe, C.P. Emenike, D.C. Chukwuka, Prevalence of heavy metals and computation of its associated risk in surface water consumed in Ado-Odo Ota, South-West Nigeria, *Hum. Ecol. Risk Assess.* (2018 Apr 10) 1–23.
- [9] M. Weng, J. Pei, Electrochemical oxidation of reverse osmosis concentrate using a novel electrode: parameter optimization and kinetics study, *Desalination* 399 (2016 Dec 1) 21–28.
- [10] C.G. Dirisu, M.O. Maifana, G.B. Dirisu, R. Amodu, Level of pH in drinking water of an oil and gas producing community and perceived biological and health implications, *Eur. J. Basic Appl. Sci.* 3 (3) (2016) 53–60.
- [11] I. Dunmade, M. Udo, T. Akintayo, S. Oyedepo, I.P. Okokpujie, Lifecycle impact assessment of an engineering project management process—a SLCA approach, in: IOP Conference Series: Materials Science and Engineering, 2018 Sep (Vol. 413, No. 1, p. 012061). IOP Publishing.
- [12] O.S. Fayomi, I.P. Okokpujie, M. Udo, The role of research in attaining sustainable development goals, in: IOP Conference Series: Materials Science and Engineering, 2018 Sep (Vol. 413, No. 1, p. 012002). IOP Publishing.
- [13] S.E. Yekini, I.P. Okokpujie, S.A. Afolalu, O.O. Ajayi, J. Azeta, Investigation of production output for improvement, *Int. J. Mech. Prod. Eng. Res. Dev.* 8 (1) (2018) 915–922.
- [14] H. Biglari, M. Tatari, M.R. Narooie, G. Ebrahimzadeh, H. Sharifi, Data for inactivation of free-living nematode Rhabditida from water environment using ultraviolet radiation, *Data Brief* 18 (2018) 30–34.
- [15] B. Keshavarzi, Z. Tazarvi, M.A. Rajabzadeh, A. Najmeddin, Chemical speciation, human health risk assessment and pollution level of selected heavy metals in urban street dust of Shiraz, Iran, *Atmos. Environ.* 119 (2015) 1–10.
- [16] O.T. Kayode, H.I. Okagbue, J.A. Achuka, Water quality assessment for groundwater around a municipal waste dumpsite, *Data Brief* 17 (2018) 579–587.
- [17] T.K. Olusola, P.A. Azegbabor, O.A. Olusegun, S.J. Emmanuel, O. Maxwell, Geochemical analysis of domestic groundwater sources in a suburb of Ota, Southwestern Nigeria, *Indian J. Sci. Technol.* 9 (22) (2016 Jun 29) 1–8.
- [18] O.T. Kayode, A.M. Odukoya, T.A. Adagunodo, Saline water intrusion: its management and control, *J. Inf. Math. Sci.* 9 (2) (2017) 493–499.
- [19] G.B. Dirisu, U.C. Okonkwo, I.P. Okokpujie, OS Fayomi, Comparative analysis of the effectiveness of reverse osmosis and ultraviolet radiation of water treatment, *J. Ecol. Eng.* 20 (1) (2019) 61–75.
- [20] Y. Oruwari, Social Inclusion of the Disadvantaged Groups in development: the Challenges for Civil and Community Based Organizations of the Niger Delta Region, Nigeria, Green Governance Project, Institute of International Studies, University of California, Berkeley, 2007.