

Designing bioactive porous titanium interfaces to balance mechanical properties and in vitro cells behavior towards increased osseointegration

Ana Civantos^{1,2,3}, Cristina Domínguez⁴, Raisa Juliana Pino⁵, Giulia Setti³, Juan José Pavon⁵, Enrique Martínez-Campos^{3,6}, Francisco Jose Garcia Garcia⁷, Jose Antonio Rodríguez⁴, Jean Paul Allain^{1,2,8}, Yadir Torres⁴*

¹Department of Nuclear, Plasma and Radiological Engineering, College of Engineering, University of Illinois at Urbana-Champaign, USA

²Micro and Nanotechnology Laboratory, University of Illinois at Urbana-Champaign, USA

³Tissue Engineering Group, Institute of Biofunctional studies Complutense University of Madrid. Associated Unit to the Institute of Polymer Science and Technology (CSIC), Polymer Functionalization Group, Spain

⁴Department of Engineering and Materials Science and Transportation, University of Seville, Seville, Spain

⁵Group of Advanced Biomaterials and Regenerative Medicine, Bioengineering Program, University of Antioquia, Colombia

⁶Polymer Functionalization Group, Department of Applied Macromolecular Chemistry, Institute of Polymer Science and Technology, CSIC, Madrid, Spain

⁷Department of Inorganic Chemistry and Chemistry engineering, Instituto Universitario de Investigación en Química Fina y Nanoquímica IUIQFN, University of Cordoba, Spain.

⁸Department of Bioengineering, University of Illinois at Urbana-Champaign, USA

* Corresponding author:

Email: ancife@illinois.edu

Address: 1306, Micro and Nanotechnology laboratory, 104 South Wright Street.

Urbana, Illinois 61801. USA

Phone: +1(217) 766-0951

Keywords: Porous titanium, Surface modification, Etching, Biomimetic scaffolds, Trabecular bone, Osseointegration.

ABSTRACT

Titanium implant failures are mainly related to stress shielding phenomenon and the poor cell interaction with host bone tissue. The development of bioactive and biomimetic Ti

scaffolds for bone regeneration remains a challenge which needs the design of Ti implants with enhanced osseointegration. In this context, 4 types of titanium samples were fabricated using conventional powder metallurgy, fully dense, dense etched, porous Ti, and porous etched Ti. Porous samples were manufactured by space holder technique, using ammonium bicarbonate particles as spacer in three different ranges of particle size (100-200 μm , 250-355 μm and 355-500 μm). Substrates were chemically etched by immersion in fluorhydric acid at different times (125 and 625 seconds) and subsequently, were characterized from a micro-structural, topographical and mechanical point of view. Etched surfaces showed an additional roughness preferentially located inside pores. In vitro tests showed that all substrates were biocompatible (80% of cell viability), confirming cell adhesion of preosteoblastic cells. Similarly, osteoblast showed similar cell proliferation rates at 4 days, however, higher cell metabolic activity was observed in fully dense and dense etched surfaces at 7 days. In contrast, a significant increase of Alkaline phosphatase enzyme expression was observed in porous and porous etched samples compared to control surfaces (dense and dense etched), noticing the suitable surface modification parameters (porosity and roughness) to improve cell differentiation. Furthermore, the presence of pores and rough surfaces of porous Ti substrates remarkably decreased macrophage activation reducing the M1 phenotype polarization as well M1 cell marker expression. Thus, a successful surface modification of porous Ti scaffolds has been performed towards a reduction on stress shielding phenomenon and enhancement of bone osseointegration, achieving a biomechanical and biofunctional equilibrium.

1. INTRODUCTION

Titanium (Ti) and some of its alloys are well recognized as the clinical grade metallic biomaterial with the best prognostic for bone replacement. However, the major issues associated with titanium implants failures are related to stress shielding phenomenon and lack of osseointegration. [1–3]. Many research studies have reported the biomechanical mismatch between Ti implants and the surrounding bone tissue, highlighting the higher elastic Young's modulus of Ti as the main cause associated with bone resorption and weakening of implants area. Under these circumstances, the implant may suffer micro-loosening and further combined with poor osseointegration will finally be rejected from the body [4].

Many efforts have been developed to create bioactive scaffolds with similar mechanical properties as bone tissue. Indeed, porous metallic biomaterials have become an interesting approach to reduce the stress shielding effect and to improve long-term fixation of Ti devices [4,5]. The porosity factor has been described before as a strategy to reduce the stress shielding effect due to reproducing similar stiffness and Young's modulus as native bone tissue. Several manufacturing techniques enable porous titanium scaffolds fabrication, such as freeze casting [6,7], rapid prototyping [8,9], laser processing [10,11], electric sintering [12–14], and powder metallurgy [15,16]. Unfortunately, many of those methodologies are complex processes and expensive, leaving toxic residues compromising their use in tissue reconstruction applications. Powder metallurgy technology has been used with space holder (SH) particles offering an easy and scalable method to fabricate highly random interconnected pores with suitable mechanical properties [17,18] older references; The

interconnected pores are key factor in the development of healthy bone tissue since pores allow the required irrigation of blood and nutrients to feed the bone tissue in-growth. This SH technique has shown the advantage to control the space volume fraction which allows tailoring similar pore density and structure as cortical bone [16,19]. Earlier work showed similar Young's modulus values on porous samples (20 -28 GPa) as those of cortical bone (25GPa) using a variation in type and percentage of space holder [20,21] during processing. Although for bone regeneration certain stiffness and mechanical properties are required, according to literature, a pore size between 100 to 500 μm enhances vascularization process promoting tissue bone in-growth [22]. In addition, other studies also demonstrated that the pores generated by this space holder technique yielded intrinsic surface roughness along pore walls, improving the cell adhesion process and inhibiting bacteria attachment [23,24]. However, the increment of porosity may reduce the mechanical properties and compromise the internal stability of the implant which in turn can negatively affect in-vivo tissue reconstruction. In this context, the control of parameters such as pore size, pore volume fraction and pore morphology, as well as surface roughness are key factors to guarantee biomechanical and biofunctional stability with an enhancement in the osseointegration response in living bone tissue [25,26].

On the other hand, the inert biological character of titanium surfaces may lead low levels of cell interactions at the bio interface. This poor integration may delay or even impair the proper reconstruction of the damaged bone tissue, driving to the failure of the implant [27]. For this reason, it is essential to develop bioactive and biomimetic titanium surfaces, to promote the adhesion and differentiation of bone marrow mesenchymal stem cells, osteoblast, macrophages, and osteoclast recovering the required bone homeostasis [28].

Particularly, the implantation of any biomaterial implies an immune host response leading by the action of macrophages which are the first cell line in the immune response process [29]. As any biomaterial, Ti scaffolds triggers an inflammatory response, which usually is resolved in several days once the implant is integrated by the organism. In some scenarios, this initial inflammation may endure several weeks, evolving to a chronic inflammation response by encapsulating the Ti implant [30,31]. This fibrotic capsule isolates the metallic device within a thin layer of fibrous tissue, which reduces cellular interactions with native bone tissue and promotes bacterial infections. This complex and well-orchestrated reaction also referred to as foreign body reaction (FBR) is driven by macrophages, one of the first immune cells which arrive at the implantation area [32–34]. These immune cells are exposed to multiple signals (biophysical and chemical cues from both implant surface and the surrounding tissues). Depending on the integration of these signals, macrophages become activated exhibiting a wide spectrum of polarization states. [35] At either end of such a spectrum, M1 is commonly referred to pro-inflammatory phenotype and M2 to anti-inflammatory. Each M1 and M2 phenotypes show specific features, such as different cell surface markers; expression of particular genes; and secretion of specific cytokines, chemokines, and enzymes, as well as different cell shape [34].

Some reports have shown the importance of surface modification to successfully control macrophages response and enhance osteoblast cell differentiation [33,36,37]. Hence, surface treatments of porous Ti implants have been developed with the aim of controlling the inflammatory reaction and promoting cell differentiation by enhancing the biological interactions at the bio-interface. Chemical surface modification among other treatments such anodic reaction, hydrogen peroxide, sol-gel, chemical vapor deposition, has contributed to

the microtopography by increasing the roughness and the surface free energy, being both essential factors that affect cellular processes such as protein adsorption, cellular adhesion, migration, and differentiation [38]. However, it should be pointed out the great value of nanoscale order in the surface modification role to control cells behavior and develop biomimetic surfaces is still under research by some authors of this group (Civantos and Allain) which are working on the novel nanopatterning of porous titanium scaffolds.

As pointed out above, there is some evidence showing the benefits of porous and rough Ti surfaces in implant fixation and long-term stability [1,36]. Nevertheless, their combined effect has been poorly understood and their interactions with different cellular lineages have not been evaluated before with the aim to reproduce a bone in vitro environment. Under this premise, the hypothesis in this work, based on the controlled chemical etching modification of designed porous Ti disks, will be a biomimetic and bioactive strategy to reestablish bone homeostasis and support faster osseointegration. The mechanical properties and surfaces topography, such as porosity (pore size, shape, and distribution) and roughness profile, were characterized to evaluate their influence on pre-osteoblast, osteoblast and macrophage behavior. This study reveals a porous surface treatment as a successful approach to activate the porous Ti scaffolds which will enhance the osseointegration and fixation in bone tissue.

4. CONCLUSIONS

In this work, it has been developed a chemical treatment of porous c.p.Ti surfaces to modify the roughness in a controlled manner by using an organic inhibitor to generate the observed additional micro-roughness. The etching treatment modified substrates surfaces, as well as porosity in terms of volume fraction and morphology. All this micro-structural and topographical variations involved a decrease of substrates mechanical properties, getting values closed to those of cortical bone, confirming more biomimetic porous ti scaffolds. This study correlates cell viability, adhesion, proliferation, cell morphology and immune response of pre-osteoblastic cells, pre-osteoblastic cells, and macrophages. Cell differentiation was improved, and the immune response was controlled to reduce M1 phenotype. Samples with the time of the attack of 0s and 125s favored the cell biocompatibility, whereas the samples with the chemical attack of 625s enhanced the processes of osteoblast differentiation. In vitro evaluation of porous Ti samples is not sufficient to determine the degree of osseointegration of the samples; making necessary in vivo studies with animal models that allow a better understanding of osseointegration processes in the complex environment.

5. ACKNOWLEDGEMENTS

This article is also dedicated to our dear friend and colleague Prof. Juan Jose Pavón, who prematurely passed away early in 2017, his dedication to his work, his students, his friends and family, will always be remembered. This work was supported by the Ministry of Economy and Competitiveness of Spain under the grant MAT2015-71284-P and of the Junta de Andalucía – FEDER (Spain) through the Project Ref. P12-TEP-1401. The authors would like to thank technician J. Pinto for assistance in micro-mechanical testing.

6. REFERENCES

- [1] M. Takemoto, S. Fujibayashi, M. Neo, J. Suzuki, T. Kokubo, T. Nakamura, Mechanical properties and osteoconductivity of porous bioactive titanium, *Biomaterials*. 26 (2005) 6014–6023. doi:10.1016/j.biomaterials.2005.03.019.
- [2] J.J. Pavón, P. Trueba, J.A. Rodríguez-Ortiz, Y. Torres, Development of new titanium implants with longitudinal gradient porosity by space-holder technique, *J. Mater. Sci.* 50 (2015) 6103–6112. doi:10.1007/s10853-015-9163-1.
- [3] B. Dabrowski, W. Swieszkowski, D. Godlinski, K.J. Kurzydowski, Highly porous titanium scaffolds for orthopaedic applications, *J. Biomed. Mater. Res. B Appl. Biomater.* 95B (2010) 53–61. doi:10.1002/jbm.b.31682.
- [4] A.B. Nover, S.L. Lee, M.S. Georgescu, D.R. Howard, R.A. Saunders, W.T. Yu, R.W. Klein, A.P. Napolitano, G.A. Ateshian, C.T. Hung, Porous titanium bases for osteochondral tissue engineering, *Acta Biomater.* 27 (2015) 286–293. doi:10.1016/j.actbio.2015.08.045.
- [5] E. Rieger, A. Dupret-Bories, L. Salou, M.-H. Metz-Boutigue, P. Layrolle, C. Debry, P. Lavalle, N.E. Vrana, Controlled implant/soft tissue interaction by nanoscale surface modifications of 3D porous titanium implants, *Nanoscale*. 7 (2015) 9908–9918. doi:10.1039/C5NR01237F.
- [6] Y. Chino, D.C. Dunand, Directionally freeze-cast titanium foam with aligned, elongated pores, *Acta Mater.* 56 (2008) 105–113.
- [7] S.-W. Yook, H.-E. Kim, Y.-H. Koh, Fabrication of porous titanium scaffolds with high compressive strength using camphene-based freeze casting, *Mater. Lett.* 63 (2009) 1502–1504. doi:10.1016/j.matlet.2009.03.056.
- [8] G.E. Ryan, A.S. Pandit, D.P. Apatsidis, Porous titanium scaffolds fabricated using a rapid prototyping and powder metallurgy technique, *Biomaterials*. 29 (2008) 3625–3635. doi:10.1016/j.biomaterials.2008.05.032.

- [9] G. Li, L. Wang, W. Pan, F. Yang, W. Jiang, X. Wu, X. Kong, K. Dai, Y. Hao, *In vitro* and *in vivo* study of additive manufactured porous Ti6Al4V scaffolds for repairing bone defects, *Sci. Rep.* 6 (2016) 34072. doi:10.1038/srep34072.
- [10] J. Parthasarathy, B. Starly, S. Raman, A. Christensen, Mechanical evaluation of porous titanium (Ti6Al4V) structures with electron beam melting (EBM), *J. Mech. Behav. Biomed. Mater.* 3 (2010) 249–259. doi:10.1016/j.jmbbm.2009.10.006.
- [11] B.V. Krishna, S. Bose, A. Bandyopadhyay, Low stiffness porous Ti structures for load-bearing implants, *Acta Biomater.* 3 (2007) 997–1006. doi:10.1016/j.actbio.2007.03.008.
- [12] C. Ramskogler, F. Warchomicka, S. Mostofi, A. Weinberg, C. Sommitsch, Innovative surface modification of Ti6Al4V alloy by electron beam technique for biomedical application, *Mater. Sci. Eng. C.* 78 (2017) 105–113. doi:10.1016/j.msec.2017.03.311.
- [13] R. Orru, R. Licheri, A.M. Locci, A. Cincotti, G. Cao, Consolidation/synthesis of materials by electric current activated/assisted sintering, *Mater. Sci. Eng. R Rep.* 63 (2009) 127–287.
- [14] Y.B. An, N.H. Oh, Y.W. Chun, Y.H. Kim, D.K. Kim, J.S. Park, J.-J. Kwon, K.O. Choi, T.G. Eom, T.H. Byun, J.Y. Kim, P.J. Reucroft, K.J. Kim, W.H. Lee, Mechanical properties of environmental-electro-discharge-sintered porous Ti implants, *Mater. Lett.* 59 (2005) 2178–2182. doi:10.1016/j.matlet.2005.02.059.
- [15] I.-H. Oh, N. Nomura, N. Masahashi, S. Hanada, Mechanical properties of porous titanium compacts prepared by powder sintering, *Scr. Mater.* 49 (2003) 1197–1202. doi:10.1016/j.scriptamat.2003.08.018.
- [16] Y. Torres, J. Pavón, P. Trueba, J. Cobos, J.A. Rodriguez-Ortiz, Design, Fabrication and Characterization of Titanium with Graded Porosity by using Space-holder Technique, *Procedia Mater. Sci.* 4 (2014) 115–119. doi:10.1016/j.mspro.2014.07.610.
- [17] M. Bram, C. Stiller, H.P. Buchkremer, D. Stöver, H. Baur, High-Porosity Titanium, Stainless Steel, and Superalloy Parts, *Adv. Eng. Mater.* 2 (2000) 196–199. doi:10.1002/(SICI)1527-2648(200004)2:4<196::AID-ADEM196>3.0.CO;2-K.

- [18] N. Tuncer, G. Arslan, E. Maire, L. Salvo, Investigation of spacer size effect on architecture and mechanical properties of porous titanium, *Mater. Sci. Eng. A.* 530 (2011) 633–642. doi:10.1016/j.msea.2011.10.036.
- [19] S. Muñoz, J. Pavón, J.A. Rodríguez-Ortiz, A. Civantos, J.P. Allain, Y. Torres, On the influence of space holder in the development of porous titanium implants: Mechanical, computational and biological evaluation, *Mater. Charact.* 108 (2015) 68–78. doi:10.1016/j.matchar.2015.08.019.
- [20] Yadir Torres, Sheila Lescano, Jorge Bris, Juan Pavón, José A. Rodriguez, Development of porous titanium for biomedical applications: A comparison between loose sintering and space-holder techniques, (2014). <http://www.sciencedirect.com/recursosbiblioteca.eia.edu.co/science/article/pii/S0928493113006498> (accessed September 1, 2014).
- [21] Y. Torres, J.J. Pavón, I. Nieto, J.A. Rodríguez, Conventional powder metallurgy process and characterization of porous titanium for biomedical applications, *Metall. Mater. Trans. B.* 42 (2011) 891–900.
- [22] C.M. Murphy, F.J. O’Brien, Understanding the effect of mean pore size on cell activity in collagen-glycosaminoglycan scaffolds, *Cell Adhes. Migr.* 4 (2010) 377–381. doi:10.4161/cam.4.3.11747.
- [23] C. Domínguez-Trujillo, F. Ternero, J.A. Rodríguez-Ortiz, J.J. Pavón, I. Montealegre-Meléndez, C. Arévalo, F. García-Moreno, Y. Torres, Improvement of the balance between a reduced stress shielding and bone ingrowth by bioactive coatings onto porous titanium substrates, *Surf. Coat. Technol.* 338 (2018) 32–37.
- [24] C. Domínguez Trujillo, M.D. Garvi Higuera, A. Salazar-Moya, J. Lebrato Martínez, J.A. Rodríguez-Ortiz, C. Lebrato Vázquez, Y. Torres Hernández, A.M. Beltrán Custodio, Bacterial behavior on coated porous titanium substrates for biomedical applications, (2019). doi:10.1016/j.surfcoat.2018.10.098.
- [25] C. Torres-Sanchez, F.R.A. Al Mushref, M. Norrito, K. Yendall, Y. Liu, P.P. Conway, The effect of pore size and porosity on mechanical properties and biological response of porous titanium scaffolds, *Mater. Sci. Eng. C.* 77 (2017) 219–228. doi:10.1016/j.msec.2017.03.249.
- [26] Bungo Otsuki, Mitsuru Takemoto, Shunsuke Fujibayashia, Masashi Neo, Tadashi Kokubo., Takashi Nakamura, Pore throat size and connectivity determine bone and

tissue ingrowth into porous implants: Three-dimensional micro-CT based structural analyses of porous bioactive titanium implants, *Biomater.* 27 2006 5892–5900. (n.d.).

- [27] Y. Chen, J.E. Frith, A. Dehghan- Manshadi, D. Kent, M. Bermingham, M. Dargusch, Biocompatible porous titanium scaffolds produced using a novel space holder technique, *J. Biomed. Mater. Res. B Appl. Biomater.* 106 (2018) 2796–2806. doi:10.1002/jbm.b.34060.
- [28] R.F. do Prado, G.C. Esteves, E.L.D.S. Santos, D.A.G. Bueno, C.A.A. Cairo, L.G.O.D. Vasconcellos, R.S. Sagnori, F.B.P. Tessarin, F.E. Oliveira, L.D.D. Oliveira, M.F.L. Villaça-Carvalho, V.A.R. Henriques, Y.R. Carvalho, L.M.R. De Vasconcellos, In vitro and in vivo biological performance of porous Ti alloys prepared by powder metallurgy, *PLoS ONE.* 13 (2018). doi:10.1371/journal.pone.0196169.
- [29] J.M. Anderson, A. Rodriguez, D.T. Chang, FOREIGN BODY REACTION TO BIOMATERIALS, *Semin. Immunol.* 20 (2008) 86–100. doi:10.1016/j.smim.2007.11.004.
- [30] A.K. Refai, M. Textor, D.M. Brunette, J.D. Waterfield, Effect of titanium surface topography on macrophage activation and secretion of proinflammatory cytokines and chemokines, *J. Biomed. Mater. Res. A.* 70A (2004) 194–205. doi:10.1002/jbm.a.30075.
- [31] A. Civantos, E. Martínez-Campos, V. Ramos, C. Elvira, A. Gallardo, A. Abarrategi, Titanium Coatings and Surface Modifications: Toward Clinically Useful Bioactive Implants, *ACS Biomater. Sci. Eng.* 3 (2017) 1245–1261. doi:10.1021/acsbiomaterials.6b00604.
- [32] J.M. Anderson, A. Rodriguez, D.T. Chang, Foreign body reaction to biomaterials, *Semin. Immunol.* 20 (2008) 86–100. doi:10.1016/j.smim.2007.11.004.
- [33] D. Karazisis, A.M. Ballo, S. Petronis, H. Agheli, L. Emanuelsson, P. Thomsen, O. Omar, The role of well-defined nanotopography of titanium implants on osseointegration: cellular and molecular events in vivo, *Int. J. Nanomedicine.* 11 (2016) 1367–1382. doi:10.2147/IJN.S101294.
- [34] K.M. Hotchkiss, N.B. Ayad, S.L. Hyzy, B.D. Boyan, R. Olivares-Navarrete, Dental implant surface chemistry and energy alter macrophage activation in vitro, *Clin. Oral Implants Res.* 28 (2017) 414–423.

- [35] J. Wang, S. Qian, X. Liu, L. Xu, X. Miao, Z. Xu, L. Cao, H. Wang, X. Jiang, M2 macrophages contribute to osteogenesis and angiogenesis on nanotubular TiO₂ surfaces, *J. Mater. Chem. B*. 5 (2017) 3364–3376. doi:10.1039/C6TB03364D.
- [36] A. Scislowska-Czarnecka, E. Menaszek, B. Szaraniec, E. Kolaczowska, Ceramic modifications of porous titanium: Effects on macrophage activation, *Tissue Cell*. 44 (2012) 391–400. doi:10.1016/j.tice.2012.08.002.
- [37] K.C. Nune, R.D.K. Misra, S.J. Li, Y.L. Hao, R. Yang, Cellular response of osteoblasts to low modulus Ti-24Nb-4Zr-8Sn alloy mesh structure, *J. Biomed. Mater. Res. A*. 105 (2017) 859–870. doi:10.1002/jbm.a.35963.
- [38] K. Subramani, R.T. Mathew, P. Pachauri, Titanium surface modification techniques for dental implants—From microscale to nanoscale, in: *Emerg. Nanotechnologies Dent. Second Ed.*, Elsevier, 2018: pp. 99–124.
- [39] Standard Test Method for Water Absorption, Bulk Density, Apparent Porosity, and Apparent Specific Gravity of Fired Whiteware Products, Ceramic Tiles, and Glass Tiles, 14.
- [40] I. Standard, ISO 13314: 2011 (E)(2011) Mechanical testing of metals—ductility testing—compression test for porous and cellular metals, Ref Number ISO. 13314 (n.d.) 1–7.
- [41] P.C. Potts, L. Ma, S.M. Graham, M.A. Adler, Repeatability and reproducibility of compression strength measurements conducted according to ASTM E9, National Institute of Standards and Technology, 2009. doi:10.6028/NIST.TN.1679.
- [42] W.E. Luecke, L. Ma, S.M. Graham, M.A. Adler, Repeatability and reproducibility of compression strength measurements conducted according to ASTM E9, (2010).
- [43] A. Standard, Standard test methods of compression testing of metallic materials at room temperature, 1990 Annu. Book ASTM Stand. ASTM West Conshohocken PA. (1990) 98–105.
- [44] J.R. Davis, *ASM Handbook: Nondestructive evaluation and quality control*, ASM International, 1989.

- [45] J. Müller-Rochholz, Determination of the elastic properties of lightweight aggregate by ultrasonic pulse velocity measurement, *Int. J. Cem. Compos. Lightweight Concr.* 1 (1979) 87–90.
- [46] T.B. Kim, S. Yue, Z. Zhang, E. Jones, J.R. Jones, P.D. Lee, Additive manufactured porous titanium structures: Through-process quantification of pore and strut networks, *J. Mater. Process. Technol.* 214 (2014) 2706–2715. doi:10.1016/j.jmatprotec.2014.05.006.
- [47] G. Pyka, G. Kerckhofs, I. Papantoniou, M. Speirs, J. Schrooten, M. Wevers, Surface Roughness and Morphology Customization of Additive Manufactured Open Porous Ti6Al4V Structures, *Materials*. 6 (2013) 4737–4757. doi:10.3390/ma6104737.
- [48] C. Aparicio, F.J. Gil, U. Thams, F. Muñoz, A. Padrós, J.A. Planell, Osseointegration of Grit-Blasted and Bioactive Titanium Implants: Histomorphometry in, n.d.
- [49] L.L. Guehenneq, E. Goyenvalle, M.-A. Lopez- Heredia, P. Weiss, Y. Amouriq, P. Layrolle, Histomorphometric analysis of the osseointegration of four different implant surfaces in the femoral epiphyses of rabbits, *Clin. Oral Implants Res.* 19 (2008) 1103–1110. doi:10.1111/j.1600-0501.2008.01547.x.
- [50] C Aparicio, F Gil, J Planell, E Engel, Human-osteoblast proliferation and differentiation on gritblasted and bioactive titanium for dental application, *J Mater Sci Mater Med.* 13 (2003) 1105–1111.
- [51] M. Herrero-Climent, P. Lázaro, J. Vicente Rios, S. Lluch, M. Marqués, J. Guillem-Martí, F.J. Gil, Influence of acid-etching after grit-blasted on osseointegration of titanium dental implants: in vitro and in vivo studies, *J. Mater. Sci. Mater. Med.* 24 (2013) 2047–2055. doi:10.1007/s10856-013-4935-0.
- [52] T.-S. Jang, H.-D. Jung, S. Kim, B.-S. Moon, J. Baek, C. Park, J. Song, H.-E. Kim, Multiscale porous titanium surfaces via a two-step etching process for improved mechanical and biological performance, *Biomed. Mater.* 12 (2017) 025008. doi:10.1088/1748-605X/aa5d74.
- [53] B. Chang, W. Song, T. Han, J. Yan, F. Li, L. Zhao, H. Kou, Y. Zhang, Influence of pore size of porous titanium fabricated by vacuum diffusion bonding of titanium meshes on cell penetration and bone ingrowth, *Acta Biomater.* 33 (2016) 311–321.

- [54] R.F. do Prado, F.S. de Oliveira, R.D. Nascimento, L.M.R. de Vasconcellos, Y.R. Carvalho, C.A.A. Cairo, Osteoblast response to porous titanium and biomimetic surface: In vitro analysis, *Mater. Sci. Eng. C.* 52 (2015) 194–203. doi:10.1016/j.msec.2015.03.028.
- [55] G. Abagnale, M. Steger, V.H. Nguyen, N. Hersch, A. Sechi, S. Jousen, B. Denecke, R. Merkel, B. Hoffmann, A. Dreser, U. Schnakenberg, A. Gillner, W. Wagner, Surface topography enhances differentiation of mesenchymal stem cells towards osteogenic and adipogenic lineages, *Biomaterials.* 61 (2015) 316–326. doi:10.1016/j.biomaterials.2015.05.030.
- [56] F. Romero-Gavilan, A.M. Sánchez-Pérez, N. Araújo-Gomes, M. Azkargorta, I. Iloro, F. Elortza, M. Gurruchaga, I. Goñi, J. Suay, Proteomic analysis of silica hybrid sol-gel coatings: a potential tool for predicting the biocompatibility of implants in vivo, *Biofouling.* 33 (2017) 676–689.
- [57] J.P. Allain, M. Echeverry-Rendón, Surface treatment of metallic biomaterials in contact with blood to enhance hemocompatibility, in: *Hemocompatibility Biomater. Clin. Appl.*, Elsevier, 2018: pp. 279–326.
- [58] A. Ahmad Khalili, M.R. Ahmad, A Review of Cell Adhesion Studies for Biomedical and Biological Applications, *Int. J. Mol. Sci.* 16 (2015) 18149–18184. doi:10.3390/ijms160818149.
- [59] R.A. Gittens, T. McLachlan, R. Olivares-Navarrete, Y. Cai, S. Berner, R. Tannenbaum, Z. Schwartz, K.H. Sandhage, B.D. Boyan, The effects of combined micron-/submicron-scale surface roughness and nanoscale features on cell proliferation and differentiation, *Biomaterials.* 32 (2011) 3395–3403.
- [60] Jean-Philippe St-Pierrea, Louis-Philippe Lefebvre, Maryam Tabrizian, Maxime Gauthierb, Three-dimensional growth of differentiating MC3T3-E1 pre-osteoblasts on porous titanium scaffolds, *Biomater.* 26 2005 7319–7328. (2005).

7. FIGURE CAPTIONS

Figure 1. SEM microphotographs of all c.p.Ti surfaces. Images showed the different surfaces, with and without HF treatment as well the three different pore sizes of space holder (BA). Insets correspond to macroscopic images of the samples revealing the main differences (color and pore size and morphology) of the samples.

Figure 2. Pore's detail of cp. Ti samples by SEM. These microphotographs highlight the pores structure and the HF influence as surface modification treatment. Noticed an increased roughness at the microscale order as well as the presence of geometrical features (upper insets) due to HF treatment and PM process respectively.

Figure 3. Roughness quantification, Sa (μm) of c.p.Ti substrates by the analysis of confocal images using Sensomap software. A, B, C, and D correspond to the Sa values comparing flat and pores surfaces of A, B C and D surfaces at the three times of etching modification (0, 125, and 625). Upper and left insets showed clearly a bigger scale of flat surfaces. Noticed the higher affinity of chemical attack for pore surfaces which reached higher Sa values.

Figure 4. Cell viability of C2C12GFP cells at 1 day. Results were expressed as a percentage of D0 levels. All substrates showed similar metabolic activities with no statistical differences ($P \geq 0.05$).

Figure 5. Fluorescent microphotographs of cell adhesion and proliferation of C2C12-GFP premyoblastic cell line. A) Cell attachment of D, DE, P and PE at 1 day of cell incubation. All samples allowed cell attachment, noticing a slight increase in cell density in D0 which has not rough surface and no pores. Etched Ti scaffolds showed similar cell density as controls revealing the cell biocompatibility of the treatment. B) Cell proliferation of C2C12-GFP

growing on D, DE, P and PE samples at 4 days of cell incubation. Noticed the increase of cell density showing the cytocompatibility character of the treatment.

Figure 6. Cell proliferation of MC3T3E1 preosteoblastic cells expressing cell metabolic activity results as relative fluorescence units at 4 and 7 days of cell culture (A and B respectively). These fluorescence levels showed similar cell proliferation as control and TCP. Noticed a slight reduction trend in porous samples of cell metabolic levels.

Figure 7. Microphotographs of cell morphology of osteoblast MC3T3E1 growing on all c.p. Ti samples at day 7. Actin fibers appeared in red and cell nuclei in blue due to Texas Red Phalloidin and Dapi staining. From these images, Ti samples achieved similar cell density covered the whole surface by preosteoblast showing the cytocompatibility character of the samples.

Figure 8. Evaluation of cell differentiation at 7 days. Detection of Alkaline phosphatase enzyme (ALP), an earlier bone marker, on osteoblast growing on cp. Ti samples. The higher ALP levels were observed in 625 HF treatment and in the pore of bigger size B and C.

Figure 9. Evaluation of cell mineralization at 14 days. Microphotographs of calcium deposits in red color after alizarin test. The higher calcium deposits were increased on B and C samples with 125 HF treatment.

Figure 10. RAW 264.7 seeded on titanium implants with different porosity and roughness. A. Samples of titanium implants (D without porosity and A with porosity; 0s of chemical attack without roughness and 625s of chemical attack with roughness). B. Actin fibers, cell nuclei by Hoechst staining, and M1 cell surface marker (CCR7) staining at 48h. Cells growing on D0 (without porosity and roughness) presented an increased polarization of M1 that was corroborated with the positive signal of CCR7 staining. Moreover, some

multinucleated cells, that could differentiate into FBGC (see yellow arrows), were observed on these samples. In contrast, D625 and A625s, as well as A0, showed less M1 polarization compared to D0 revealing the positive effects of both parameters roughness and porosity on the control of immune response.

Figure 1

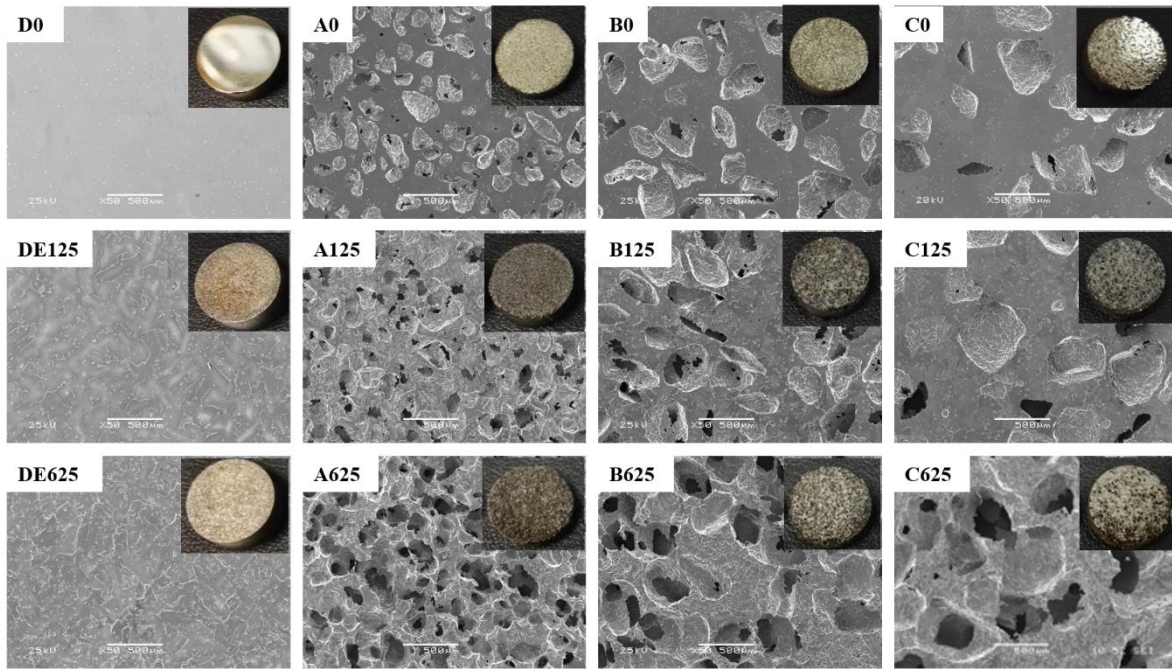


Figure 2

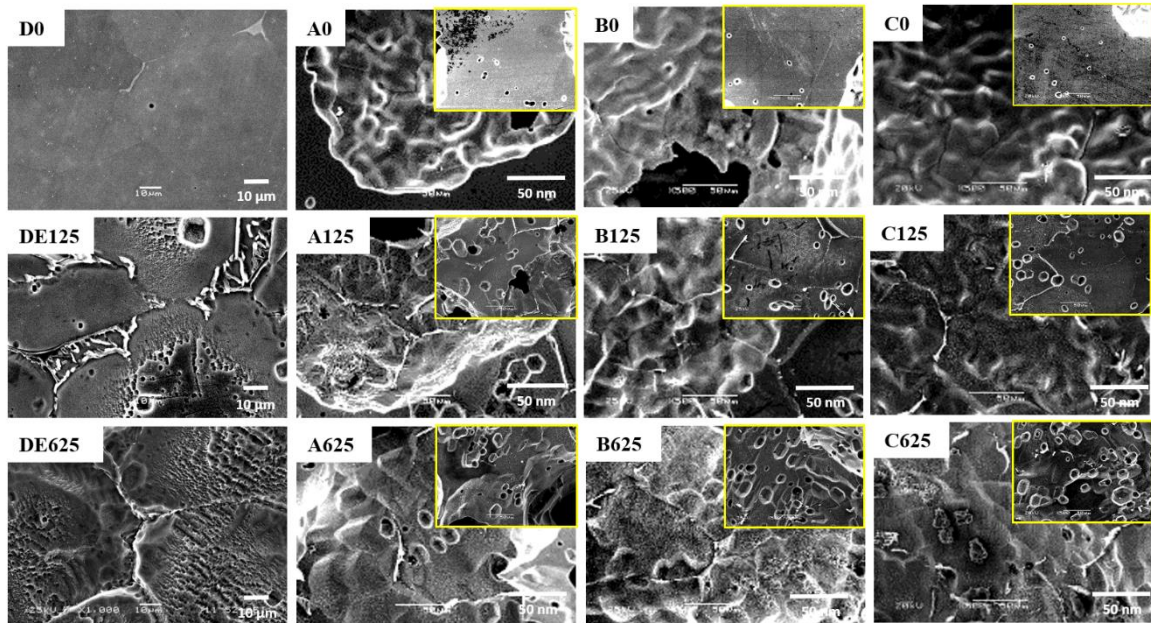


Figure 3

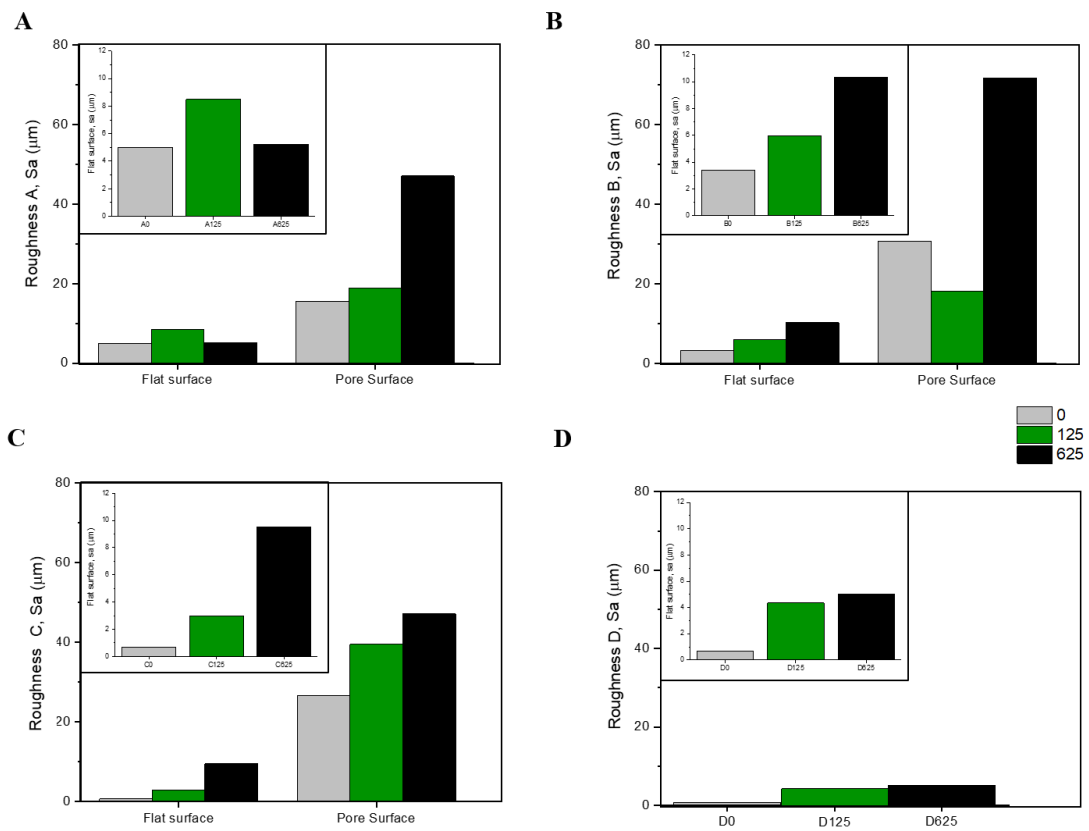


Figure 4

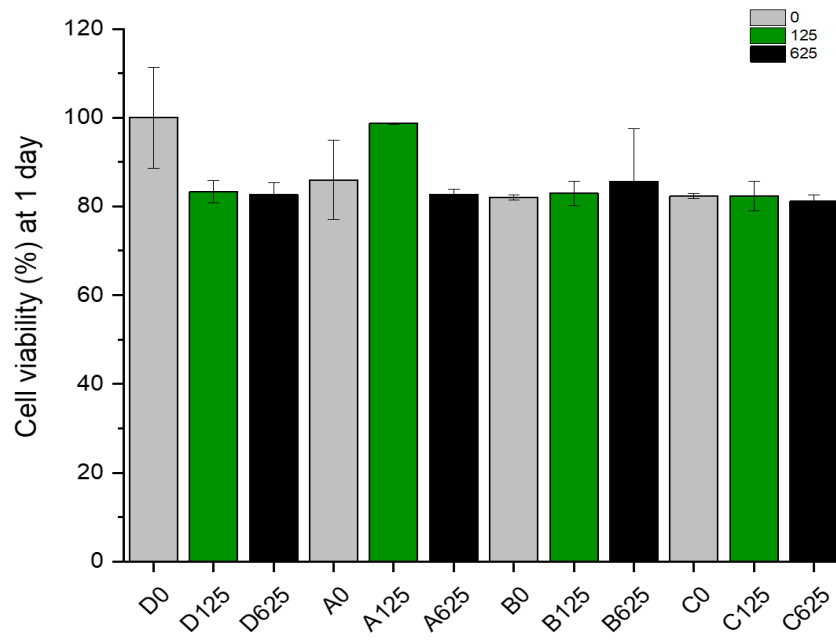


Figure 5

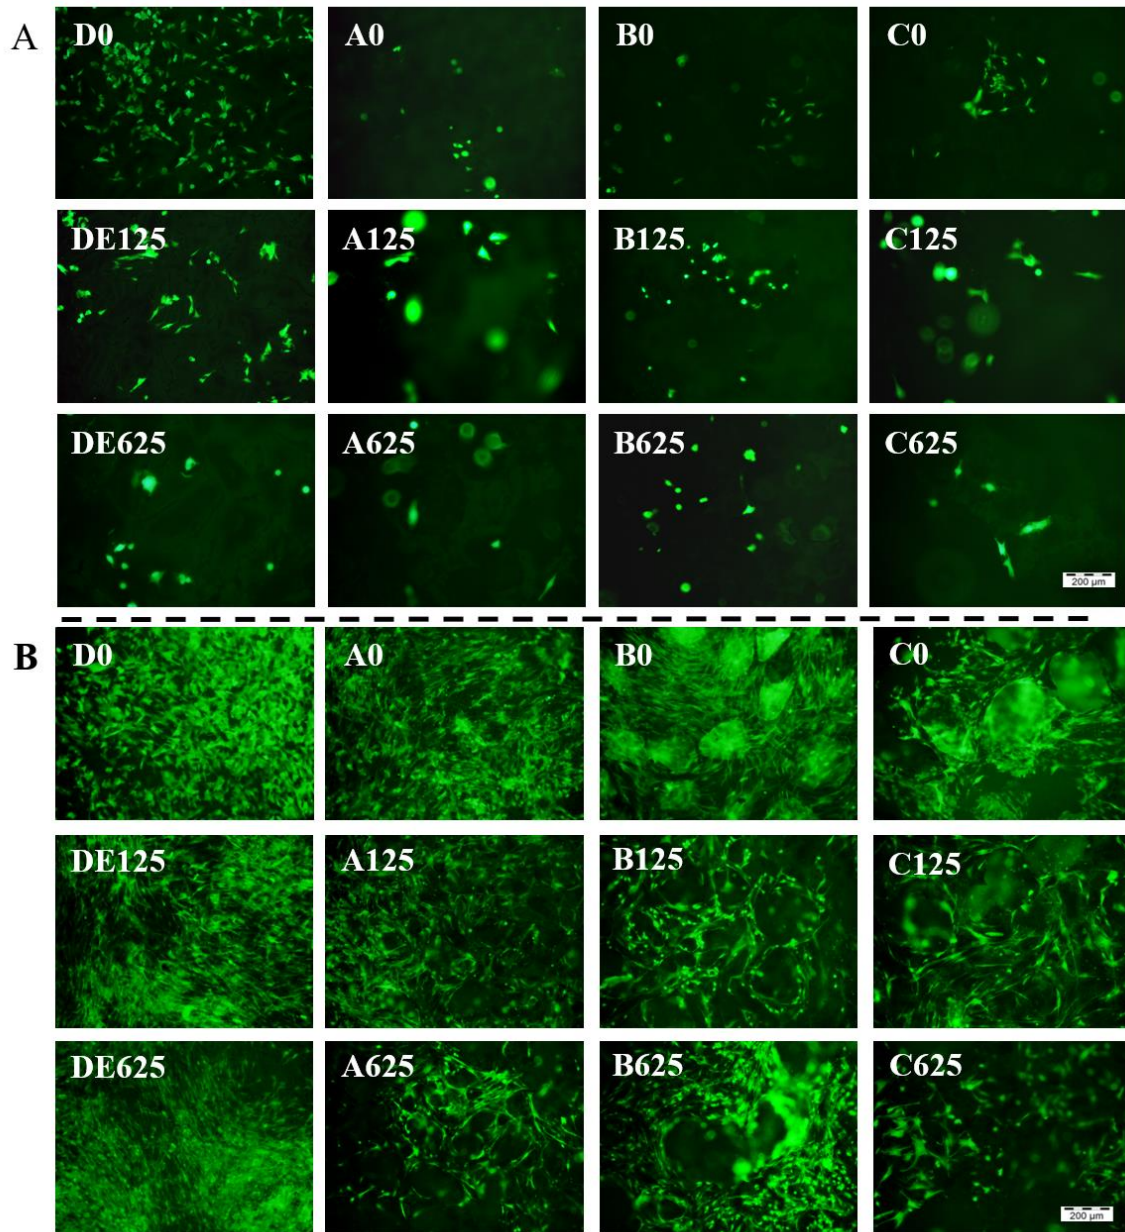


Figure 6

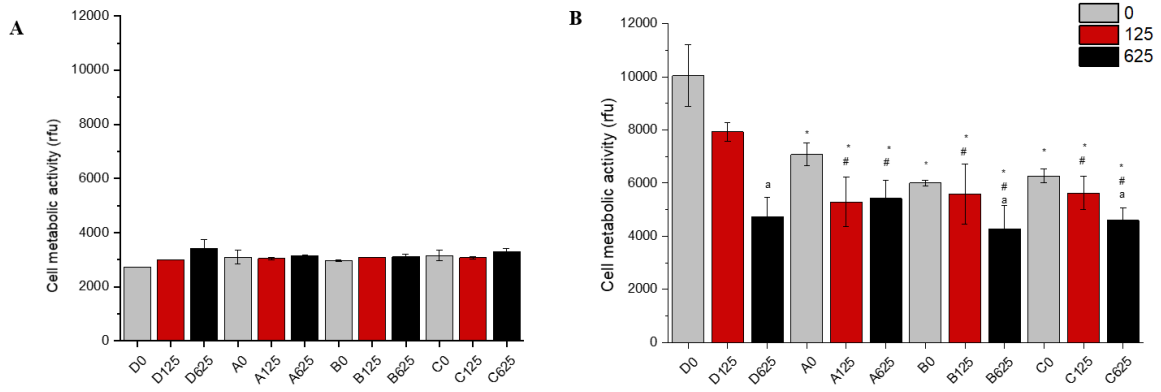


Figure 7

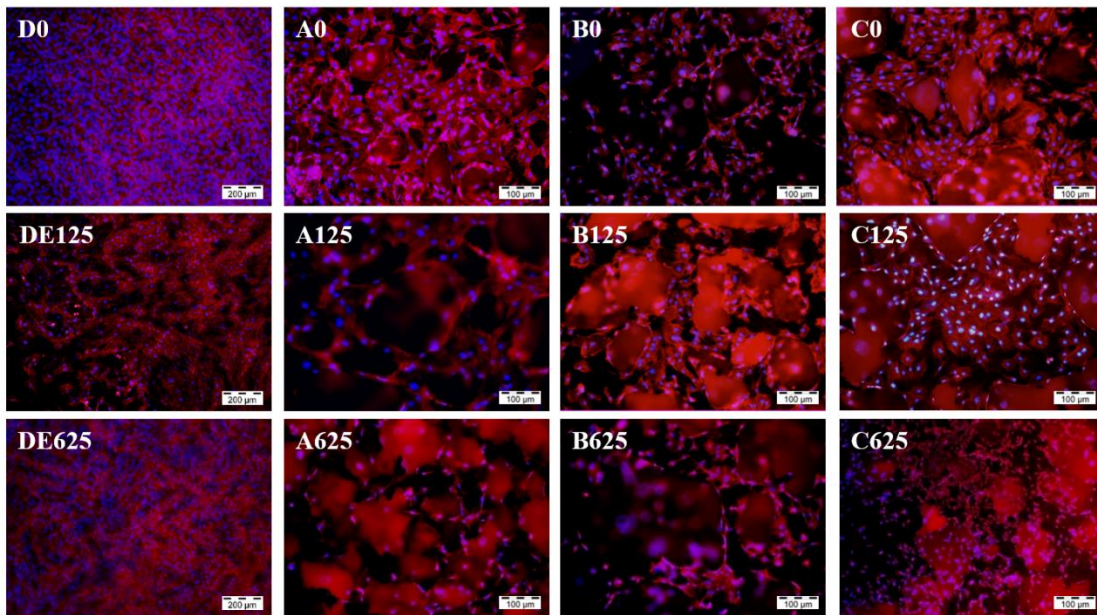


Figure 8

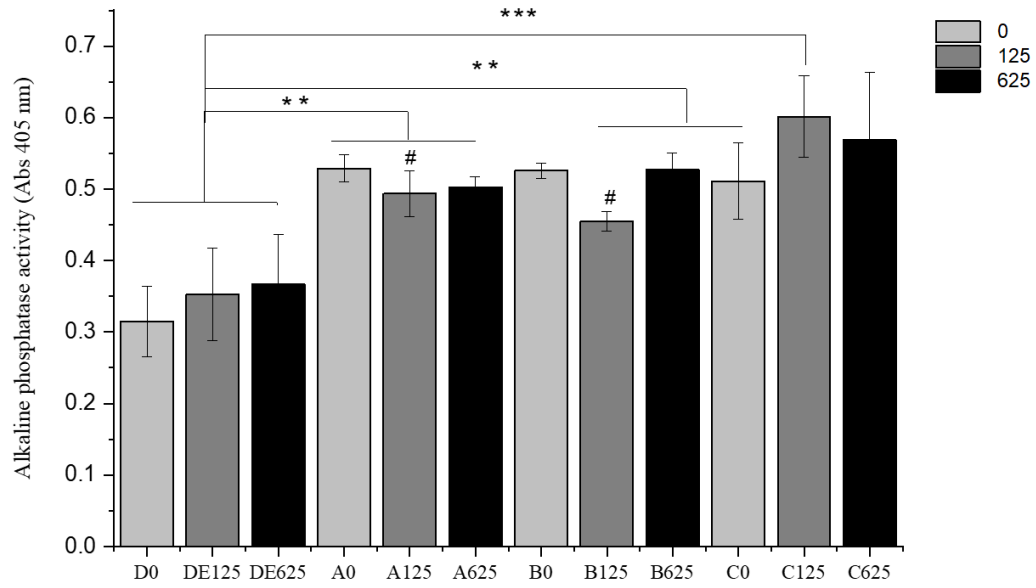


Figure 9

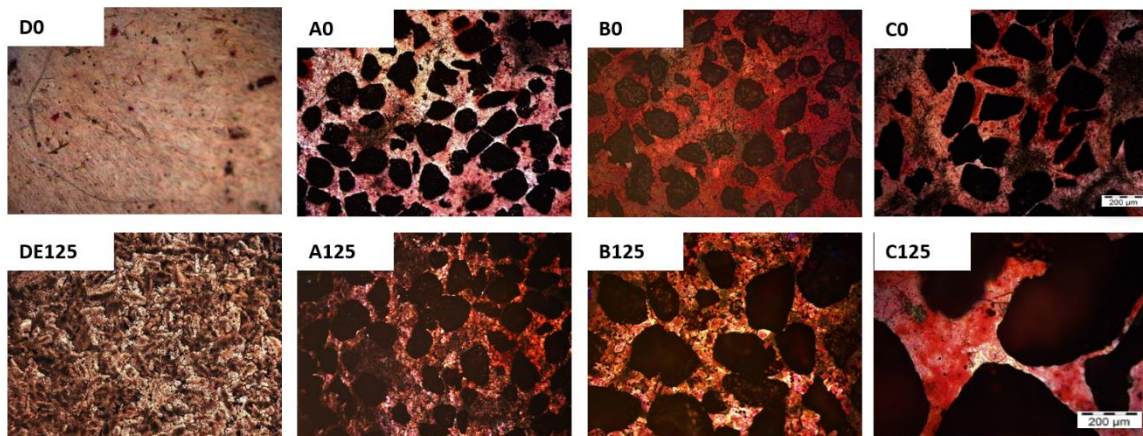


Figure 10

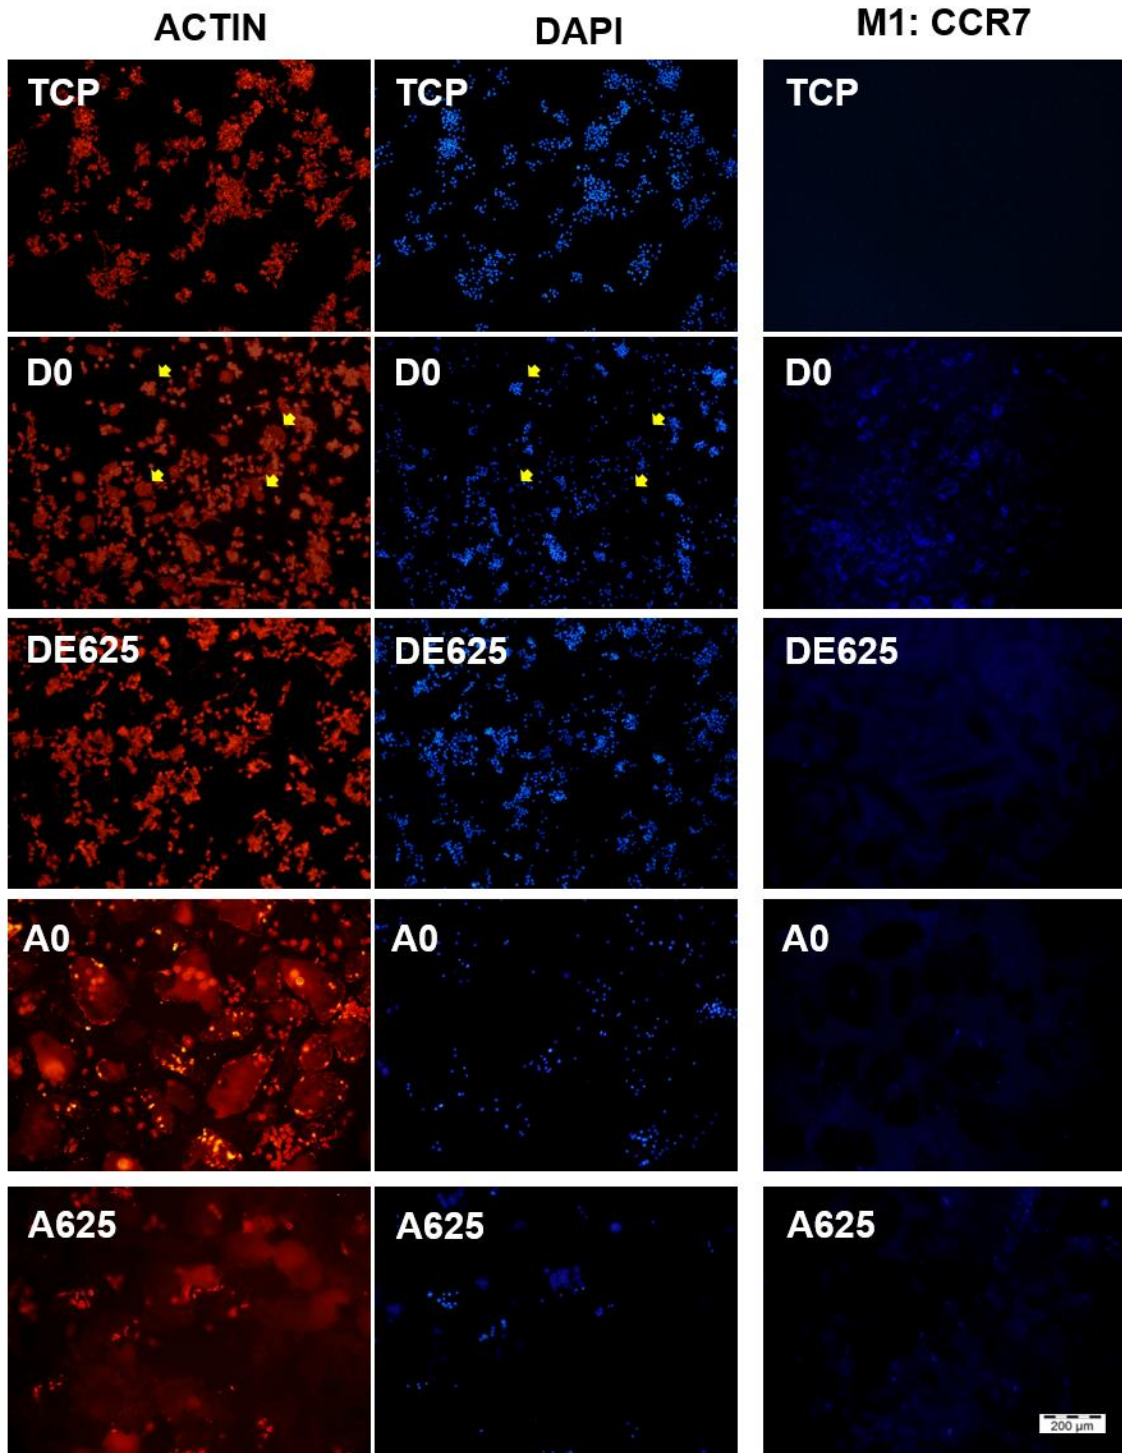


Figure S1

