

Supplementary material for the article:

Jevtić, S.; Stefanović, A.; Stanković, D. M.; Pergal, M. V.; Ivanović, A. T.; Jokić, A.; Petković, B. B. Boron-Doped Diamond Electrode — A Prestigious Unmodified Carbon Electrode for Simple and Fast Determination of Bentazone in River Water Samples. *Diamond and Related Materials* **2018**, *81*, 133–137. <https://doi.org/10.1016/j.diamond.2017.12.009>

Supplementary material for:

**Boron-doped diamond electrode – a prestigious unmodified carbon electrode
for simple and fast determination of bentazone in river water samples**

Sonja Jevtić¹, Anđela Stefanović¹, Dalibor M. Stanković^{2,3}, Marija V. Pergal⁴, Aleksandra T.
Ivanović⁵, Anja Jokić¹, Branka B. Petković^{1*}

*¹Department of Chemistry, Faculty of Natural Science and Mathematics, University of Priština,
Lole Ribara 29, 38220 Kosovska Mitrovica, Serbia*

*²The Vinca Institute of Nuclear Sciences, University of Belgrade, POB 522, 11001 Belgrade,
Serbia*

*³Innovation center of the Faculty of Chemistry, University of Belgrade, POB 51, 118, 11158
Belgrade, Serbia*

*⁴Institute of Chemistry, Technology and Metallurgy, Center of Chemistry, University of
Belgrade, Njegoševa 12, 11000 Belgrade, Serbia*

⁵Mining and Metallurgy Institute, Zeleni bulevar 35, 19210 Bor, Serbia

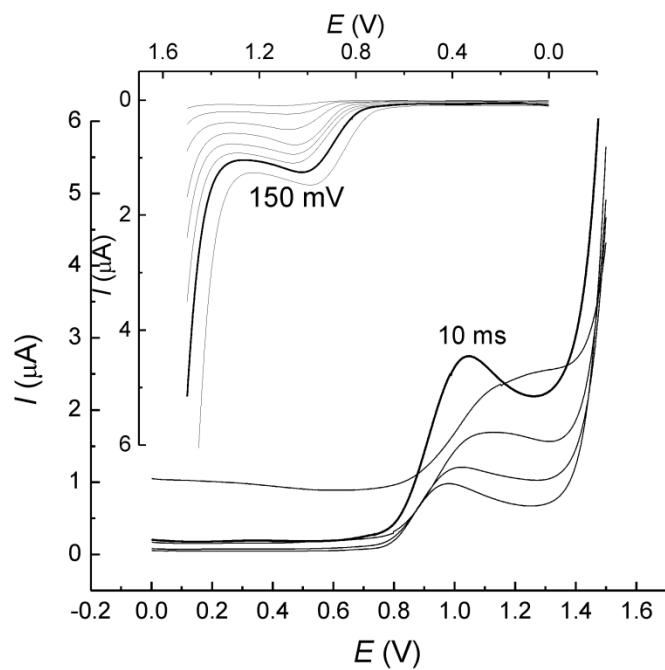


Figure S1. Voltammograms of 100 μM of BZ in BR buffers at pH 4 using BDDE at different working operational parameters for DPV; lower figure – effect of pulse time, upper figure – effect of pulse amplitude

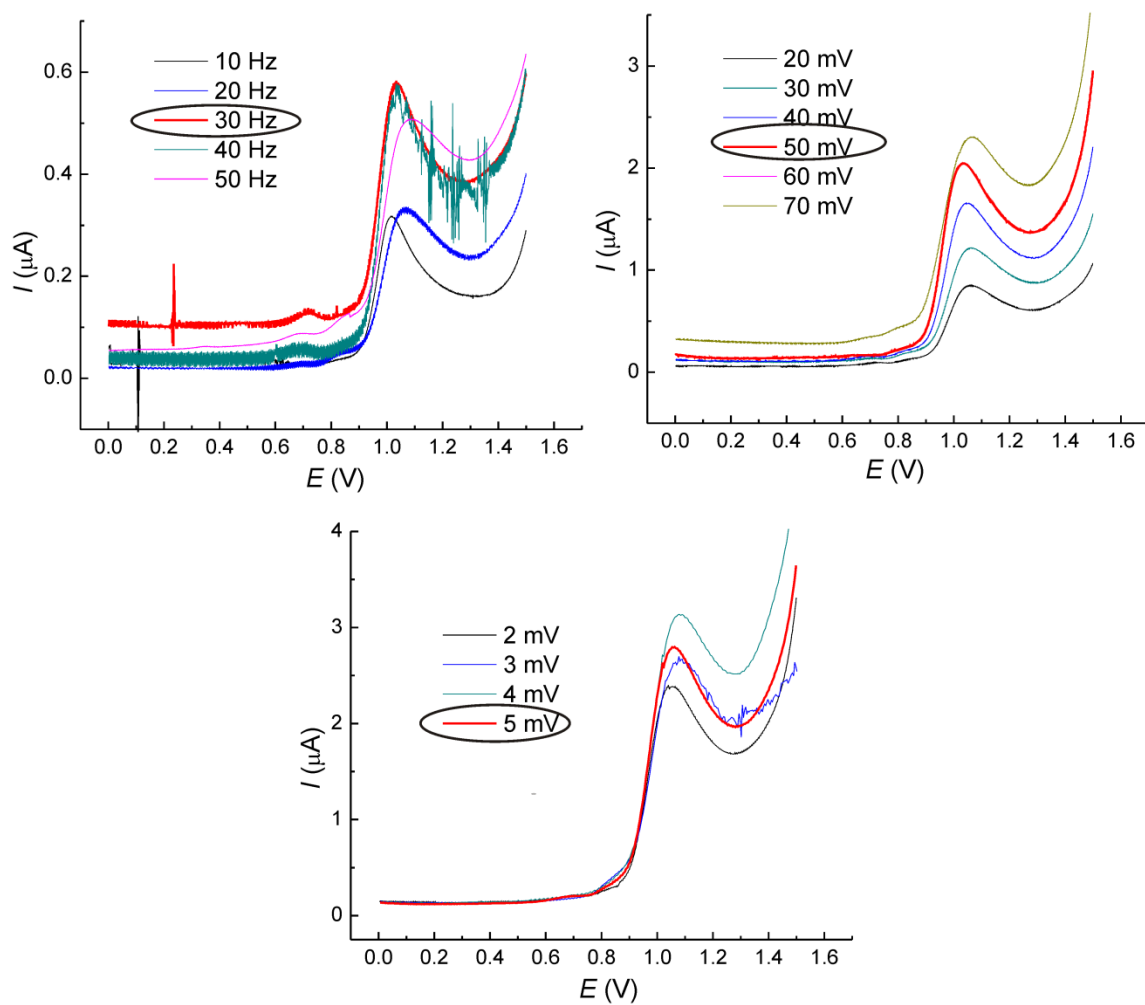


Figure S2. Voltammograms of $100 \mu\text{M}$ of BZ in BR buffers at pH 4 using BDDE at different working operational parameters for SW; above, left figure – effect of frequency; above, right – effect of pulse amplitude; below – effect of potential step

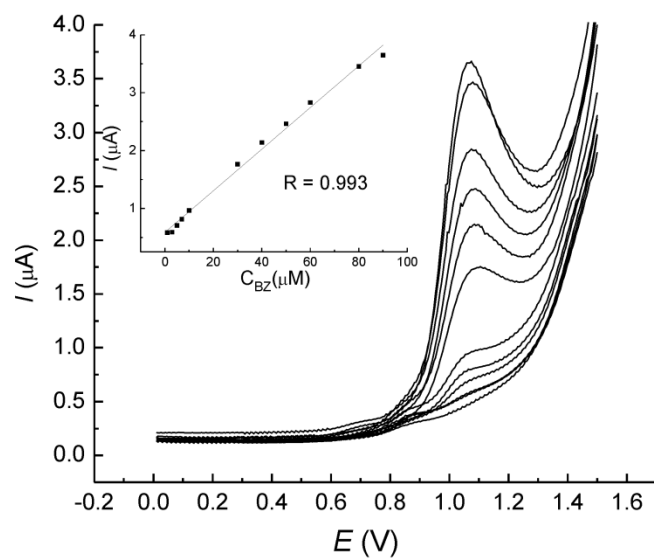


Figure S3. SW voltammograms of various concentrations (0, 1, 3, 5, 7, 10, 30, 40, 50, 60, 80, 90 μM) of bentazone, in BR buffer at pH 4 at BDDE, under optimized experimental conditions; Corresponding calibration curve is in inset.

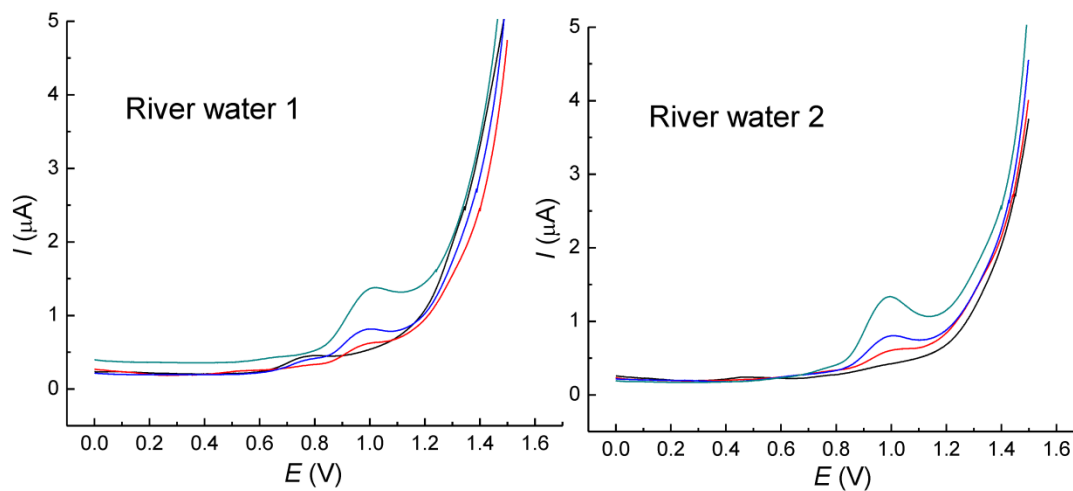


Figure S4. DPVs of BR solutions containing river water samples spiked with various concentrations of bentazone (3, 9 and 24 μM)