

UPPER-LIMB EXOSKELETON FOR HUMAN MUSCLE FATIGUE

S. K. ALI*

*Automatic Control and System Engineering, University of Sheffield,
Sheffield, United Kingdom*

*E-mail: skali1@sheffield.ac.uk

M. O. TOKHI

*School of Engineering, London South Bank University
London, United Kingdom*

Human muscle fatigue is identified as one of the causes to musculoskeletal disorder (MSD). The objective of this paper is to investigate the effect of an exoskeleton in dealing with muscle fatigue in a virtual environment. The focus of this work is, for the exoskeleton to provide support as needed by human joint. A (Proportional, Integration and Derivative) controller is used for both human and exoskeleton. Simmechanics and Simulink are used to evaluate the performance of the exoskeleton. Experiments show that human is able to maintain doing the job by wearing the exoskeleton.

Keywords: Predictive fatigue model; upper-limb exoskeleton; virtual environment.

1. Introduction

Muscle fatigue is a well-known problem to human. Many factors could be contributed to human fatigue such as heavy physical activities, repetitive works, dealing with above-head work and duration of exposure to working environment. Muscle fatigue could effect human's quality of life and performance degradation. In a worse scenario, fatigue could lead to musculoskeletal disorder (MSD). There are two sectors that could lead human to critical fatigue: industry and rehabilitation.

Exoskeleton is one of the solution to solve human fatigue problem. Several works have been done such as in.^{1,2} Most current works related to muscle fatigue and exoskeleton use electromyography (EMG) signal to identify the fatigue. Another ways to measure fatigue is by adding the fatigue model

to the developed muscle model.²⁻⁴ However, a limitation to the second approach is, it is difficult to acquire an accurate force distribution for each individual muscle.^{4,5} Hence,⁵ proposed a new fatigue model which uses an information from joint level. The torque of human joint could be acquired using inverse dynamics. Due to this reason, an investigation is done to see the effect of joint fatigue model developed by Ma et.al (2009) to human joint and to evaluate the performance of an exoskeleton in dealing with human fatigue during movements.

To achieve the investigation, the joint fatigue model developed by⁵ is applied to human joint. Then, an algorithm is developed to activate the exoskeleton using the reading from human joint. In the Section (2), the joint fatigue model is introduced, and an observation is done. Then, in the Section (3), the performance of the exoskeleton with human joint fatigue model is presented.

2. Human Joint Fatigue Model

As mentioned in Section (1), joint fatigue model by⁵ is used. The joint fatigue model is an extension from muscle fatigue model, which was also developed by Ma et. al. Initially, Ma et. al developed fatigue index which is presented as in Eq.(1). The basis new fatigue muscle model is presented in Eq.(2). Further explanation could be referred to.⁴

$$\frac{dU(t)}{dt} = \frac{MVC}{F_{cem}(t)} \frac{F_{load}}{F_{cem}(t)} \quad (1)$$

$$\frac{dF_{cem}(t)}{dt} = -k \frac{F_{cem}(t)}{MVC} F_{load}(t) \quad (2)$$

$$\frac{d\tau_{cem}(t)}{dt} = -k \frac{\tau_{cem}(t)}{\tau_{MVC}} \tau_{joint}(t) \quad (3)$$

Since this paper is applying joint fatigue model, thus Eq. (2) could be rewritten as in Eq. (3). The definition for each term in Eq.(1), (2) and (3) are presented in Table (1). Simulink is used as a platform to apply the joint fatigue model and Simmechanic is used as a platform for human simulation.

Fig. (1) shows human fatigue model system. As shown in Fig. (1)(a), there are three main blocks: fatigue model, human-exoskeleton and performance. The fatigue model block contains Eq.(3). Fig.(1)(b) shows an

Table 1. Parameters in muscle and joint fatigue model.^{4,5}

Muscle-fatigue Model	Unit	Definition
MVC / τ_{max}	Newton(N)	Muscle Maximum voluntary contraction
F_{cem} / τ_{cem}	Newton(N)	Muscle force capacity at time instant t
F_{load} / τ_{load}	Newton(N)	Muscle load at time instant t
Joint-fatigue Model	Unit	Definition
τ_{max}	Newton meter (Nm)	Maximum joint strength
τ_{cem}	Newton meter (Nm)	Joint strength at time instant t
τ_{load}	Newton meter (Nm)	Torque load at time instant t
k	min^{-1}	Fatigue rate
t	min	Time

integration between the joint fatigue to human model. Revolute joint is used to present human joint. Thus, it is essential to have a controller to control the joint. In this paper, conventional PID controller is used for the shoulder joint. A conventional PID controller is chosen because of its easiness in tuning the parameter. The parameters for K_p , K_i and K_d were chosen by a known PID tuning method.

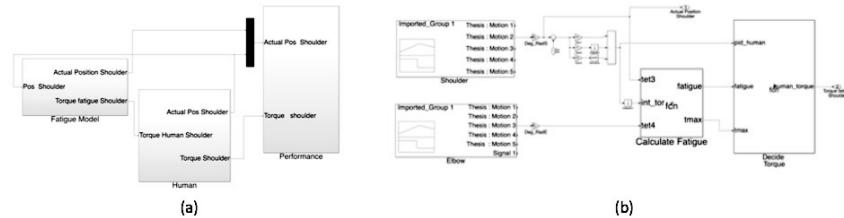


Fig. 1. (a) Human with fatigue model (b) fatigue model.

3. Integration of Human Joint Fatigue and Exoskeleton

Fig.(2)(a) presents the overall system for exoskeleton with human and Fig.(2)(b) presents the integration of the exoskeleton with the human fatigue model. There are three main blocks: PID, human-exoskeleton and performance block. Similar as in Section (2), both human and exoskeleton were controlled by using PID controller, and iterative approach is used to acquire the parameters.

'PID' block contains controller for human and exoskeleton. It also has two important blocks: Calculate Fatigue and Decide Assistive Torque block.

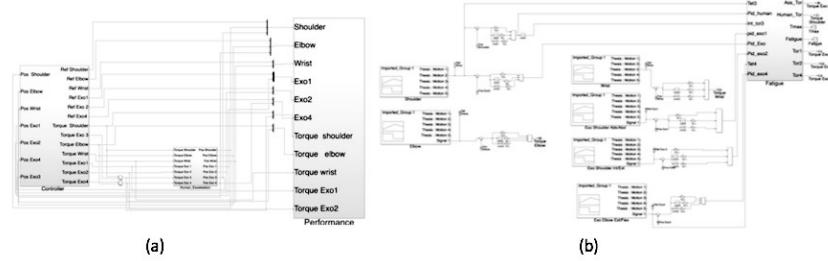


Fig. 2. (a) Human-exoskeleton system (b) Integration of exoskeleton and fatigue model.

Table 2. Parameters for (PID).

Parameter	Shoulder Joint
Proportional	10.0
Integration	1.0
Derivative	0.1

In these two blocks, the algorithm for the activation process is presented. The first algorithm in ‘Calculate Fatigue’ block is presented as follows:

- (i) To measure the human fatigue in joint level, there are three important information: maximum voluntary contraction of joint torque (τ_{MVC}), integrated joint torque ($\int \tau(u, \theta, \dot{\theta}, \ddot{\theta})$) and angle for θ_3 and θ_4 .
- (ii) To calculate (τ_{MVC}), the formula is obtained from [6]. The formula is presented in Eq.(4). This value presents the maximum torque values for shoulder joint at $t = 0$.

$$\tau_{MVC} = (227.338 + 0.525\theta_3 - 0.296\theta_4)0.2854 \quad (4)$$

- (iii) Then, the fatigue could be measured by using Eq. 3. In this work, the value of fatigue rate (k) is set to equal 1. After applying fatigue equation, it is expected that the value of τ_{MVC} is reducing.

The algorithm in ‘Decide Assistive Torque’ block is presented as follows:

- (i) A condition is set up to determine when human is fatigue. In this work, fatigue is identified when the maximum voluntary contraction of the torque is reducing up to 80 %.
- (ii) Once the joint fatigue is identified, an exoskeleton is sent torque support to maintain human in desired position.

```
if fatigue <= 0.8 * τMVC
then
```

```

    asstor = pidexo
    humantorque = asstor - fatigue
else
    asstor = pidexo
    humantorque = pidhuman

```

- (iii) To maintain the position of human shoulder joint, the value of *asstor* is sent to an exoskeleton joint and *humantorque* is sent to human shoulder joint.

In the next section, the results and discussion of the experiment is presented.

Table 3. Parameters for (PID).

Parameter	Shoulder Joint	Exoskeleton Joint (θ_3)
Proportional	10.0	10.0
Integration	1.0	5.0
Derivative	0.1	0.5

4. Result and Discussion

As mentioned in Section (2), the parameters for P, I and D for human shoulder were found by iteratively. The parameters are presented in Table (2). Fig. (3)(a) shows that human is able to maintain at desired position but, small oscillations occur at this joint. By looking at the oscillation in Fig. (3)(a) and Fig.(3)(b), we could said that, the oscillation is actually presenting the fatigue condition. This also could be seen in Fig. 3(c). As mentioned in Algorithm 1 of Section (3), fatigue is identified when the joint strength is reached to 80% of the τ_{MVC} . Hence, the fatigue level is reducing but, when it reached to 80% of the τ_{MVC} , it start to maintain at that value.

As mentioned earlier in Section 3, the parameters for PID controller is obtained with a known tuning PID approach and is presented as in Table (3). For the integration system (Exoskeleton-Human), the PID parameter for shoulder joint use the same values as in Table (2). These values were chosen to ensure that both system (human with joint fatigue model and exoskeleton-human model) are in the same condition. Hence, any changes that occur could be compared.

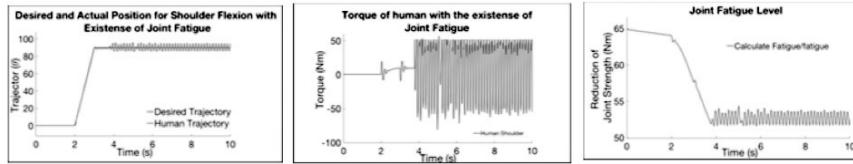


Fig. 3. Results of human with fatigue model: (a) Desired and actual trajectory of human (b) torque of human (c) fatigue level.

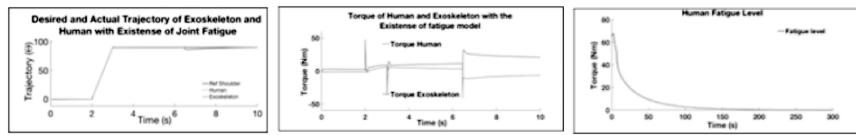


Fig. 4. Results of human fatigue with the existence of an exoskeleton: (a) Desired and actual trajectory of exoskeleton and human (b) torque of exoskeleton and human (c) human fatigue level.

Fig. (4)(a) shows the movement of human and an exoskeleton. The joint fatigue model is included in human model. As shown in Fig. (4)(a) when time reached at approximately to 6.70 s, a small undershoot occur. There are two observations can be found here.

First, after shoulder joint is reached to 90 degree, shoulder joint is able to sustain at this trajectory approximately 3.70 s. A small undershoot occur at 6.70 s. At this point, it can be seen that shoulder joint is approaching at the maximum point of fatigue level and thus, it moves downward. Fig.(4)(a) also shows that the exoskeleton is moving downward following the human joint (the black circle), but eventually, both human and exoskeleton were moving to the desired trajectory back. From here, it shows that, exoskeleton is actually, supporting human to maintain at the desired point. Second observation is, human with an exoskeleton, took time to fatigue. This could be happened due to the support that is given by the exoskeleton from the beginning of the motion.

Fig.(4)(b) shows the torque required by the shoulder joint and exoskeleton joint. As shown here, an exoskeleton has high torque compared to shoulder joint, which shows that the exoskeleton is supporting the human upper limb by providing an assistive torque. This could be seen clearly when the time is extended to 300 s (Fig.(5)). An exoskeleton is providing an assistive torque to ensure human could prolong doing the activities even tough, the strength of human joint has reach to 0 Nm (Fig.(4)(c)).

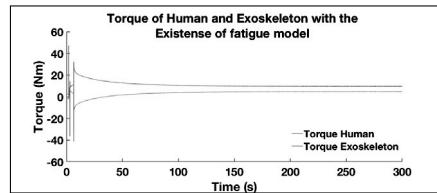


Fig. 5. Torque for exoskeleton and human.

5. Conclusion

Investigation into the impact of deploying an exoskeleton to compensate for human muscle fatigue have been presented using a virtual environment. A mechanism for monitoring and assessment of muscle fatigue has been presented. The information thus gathered allows the exoskeleton control to provide the required level of compensation to counteract the muscle fatigue. Future work will focus on incorporating fatigue compensation into the controller and further assessment of fatigue and corresponding compensation at various levels.

Acknowledgments

S. K. Ali is on study leave and supported financially by the Malaysia of Higher Education (MOHE) and Universiti Putra Malaysia.

References

1. F. P. Bonnet V., Colledani F. and S. N., *J. Industrial Ergonomics* **44**, 475 (2014).
2. C. B. Xu W. and R. E., *J. Control Engineering Practice* **31**, 63 (2014).
3. D. L. M. G. Carmichael and K. J. Waldron, Investigation of reducing fatigue and musculoskeletal disorder with passive actuators, in *Proc. IEEE/RSJ Int. Conference on Intelligent Robots and Systems (MEMS'97)*, (Taipei, Taiwan, 2010).
4. B. F. Ma L., Chablat D. and Z. W., *J. Industrial Ergonomics* **39**, 211 (2009).
5. B. F. Z. W. Ma L., Chablat D. and G. F., *J. Virtual and Physical Prototyping*, 1 (2010).
6. M. R. Sakka S., Chablat D. and B. F., *J. Human Factors Modelling and Simulation*, 1 (2015).