

DVH Analysis of Cobalt-60 treatment plans incorporating a recently developed MLC

Gangarapu Sri Krishna^{1,3}, Roopa Rani Akula^{2,3}, Ayyalasomayajula Anil Kumar¹, Vuppu Srinivas¹, Komanduri Ayyangar², Palreddy Yadagiri Reddy³

¹Department of Radiotherapy, MNJ Institute of Oncology & Regional Cancer Centre, Hyderabad, India

²Department of Physics, International Cancer Centre, Bhimavaram, India

³Department of Physics, Osmania University, Hyderabad, India

Received December 21, 2015; Revised July 13, 2016; Accepted July 14, 2016; Published Online July 16, 2016

Original Article

Abstract

Purpose: The aim of this investigation was to measure the gain in DVH indices when the recently developed MLC was used for Cobalt-60 treatments. **Methods:** A prototype multileaf collimator (MLC) that was retrofitted to telecobalt-60 therapy machine was reported and is currently proposed for clinical trials in our institution. Ten patients' plans that were previously planned through an ECLIPSE[®] treatment planning system and were treated with open beams from Cobalt-60 machine were imported into Radiation Oncology Planning System [ROPS] and the dose calculations and dose volume histogram (DVH) analysis were performed. The plans were re-planned using the Cobalt-MLC, a feature available in the ROPS planning system. The DVH analysis consisted of conformity index (CI), homogeneity index (HI) and conformation number (CN). The results of this study are presented in this paper. The analysis specifically aimed at measuring the gain in these indices when the MLC was compared with open beams. **Results:** DVH Comparison of ten sites using open and Cobalt MLC fields showed that the use of MLC results in reduced normal tissue dose, while maintaining the GTV dose. Lower value of CI for normal structures was observed demonstrating the sparing of critical organs when MLC was used. The index HI was studied to show the significance of hot spots outside the PTV. Hot spots were observed even with MLC beams for some cases due to less number of fields. **Conclusion:** It has been demonstrated through DVH analysis that the use of the recently developed MLC for Cobalt Teletherapy machine results in benefit for the treatment of patients.

Keywords: DVH Analysis, Conformity index, Homogeneity index, Conformation number, MLC Fields, ROPS TPS

1. Introduction

Cobalt-60 treatment machines are still used in developing countries all over the world. In India there are over 200 Co-60 machines are still in operational. Unfortunately, these centers are operating in rural areas with economic disadvantage and hence cannot afford modern treatment planning or custom block fabrication. In a recent review in the red journal, Page *et al.*¹ has cited the benefit of using multileaf collimator (MLC) to make Co-60 treatments on a par with high energy treatment machines. The benefit of using MLC for cobalt-60 was also referred by several investigators²⁻⁸. The overall goal of our MLC project is not only to develop the MLC as a retrofit attachment to the existing

cobalt machines, but also to provide a controller and a low cost treatment planning system (TPS) such as Radiation Oncology Planning System [ROPS] from TJCS (Tirumala Jyothi Computer Systems, Secunderabad, India).

The MLC for Cobalt-60 used in our investigation was previously reported through a Monte Carlo study⁹⁻¹², which had 14 leaf pairs to cover a treatment area of 14 cm × 14 cm field size. Figure 1 shows the Cobalt machine and the attached MLC.

Corresponding author: Gangarapu Sri Krishna; Department of Radiotherapy, MNJ Institute of Oncology & Regional Cancer Centre, Hyderabad, Telangana-500004, Email address: gsrikrishna7@gmail.com

Cite this article as: Sri Krishna G, Akula RR, Kumar AA, Srinivas V, Ayyangar K, Reddy PY. DVH Analysis of Cobalt-60 treatment plans incorporating a recently developed MLC. *Int J Cancer Ther Oncol.* 2016; 4(3):431. DOI: [10.14319/ijcto.43.1](https://doi.org/10.14319/ijcto.43.1)

Subsequently, another prototype with 16 leaves to cover a treatment area of 16 cm × 14 cm field size was fabricated and was used in the current study. The tungsten leaves with dimensions 7 mm wide, 4 cm high and 15 cm long with 2 cm × 2 mm tongue and groove were used. All patient plans reported here were done using dedicated CT scanner with interface to Eclipse TPS from Varian (Varian Medical Systems, Palo Alto, CA). The CT scans and complete plans from Eclipse TPS were available for export through DICOM RT files.

2. Methods and Materials

Ten different cases representing each of the tumor sites like Brain, Head & Neck, Esophagus, Stomach, Abdomen and Pelvis were taken for the study. These cases were originally planned in Eclipse treatment system and treated accordingly with open beams of Cobalt-60 unit. All the cases were re-planned in ROPS treatment planning system with MLC beams fitted to the PTV. For each case, DVH data were obtained for both plans (open and MLC beams).

The ROPS TPS is specially configured for the Cobalt MLC to adjust the MLC leaves around the irregular shape of the target with margin as well as exporting the leaf positions to the MLC controller. Since the controller is indigenously developed with hardware and software, ROPS is the only TPS that can be configured to match the MLC controller. The ROPS TPS was previously tested with TG-53 protocol¹³. This is a part of accepting testing and commissioning of TPS, which verified PDD, profiles, contour corrections, irregular fields and wedge profiles. In addition, the ROPS TPS was compared with Eclipse TPS by using 6 MV and 16 MV plans¹⁴.

For each clinical case the tumor volumes, critical structures and beam parameters were imported from the Eclipse planning system using DICOM_RT transfer. For cobalt treatment, in general 1-1.5 cm margin was used around the clinical target volume (CTV) to make the planning target volume (PTV). If CTV is not defined, then the gross tumor volume (GTV) is chosen as the target of importance. Since there was no asymmetric jaw or MLC available for the cobalt machine, the beam boundaries in Eclipse plans covered the PTV using the collimator jaws only. In the current study, since we have

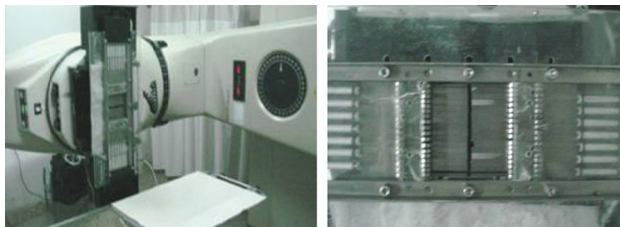


Figure 1: Prototype 1 MLC configured in ROPS TPS (reprinted with permission from Ayyangar *et al.*¹⁰)

the MLC for cobalt machine, the original open beam plans were compared by using the MLC to fit the PTV.

The DVH analysis was carried out by computing three indices viz. conformity index (CI), homogeneity index (HI) and conformation number (CN).

- The conformity index (CI) was determined as the ratio between target volume covered by the 90% or 95% isodose and the target volume (TV). While 95% isodose line is used as a standard isodose line for the definition of the indices, for cobalt-60, we have also considered 90% isodose line since 95% cannot cover the TV in some cases.
- The homogeneity index (HI) was determined as the ratio of maximum dose in the target volume to the prescription dose.
- The conformation number (CN) was defined by Arie van't Riet *et al.*¹⁵ and was calculated using the formula:

$$CN = (TV_{iso}/TV) (TV_{iso}/V_{iso}),$$

where, TV_{iso} is the target volume covered by the isodose line, TV is the target volume and V_{iso} is the total volume covered by the 90% or 95% isodose line. The V_{iso} is calculated from the dose matrix and is not dependent on any structure volume. The advantage of these indices is that ideally the values need to be close to unity for the CTV or GTV while the values should be close to zero for other structures.

The CN shows that the MLC confines the dose to PTV. The value of CI close to unity for the GTV indicates that the dose uniformity of the target is achieved. Since the use of MLC decreases dose to the critical structures, lower values of CI should be expected when compared with open beam. The value of HI close to unity for the GTV indicates that there are no hotspots. However, for certain 3-field plans using Cobalt beams the dose outside the PTV causes $HI > 1$ especially for abdomen and pelvic sites.

3. Results

Figure 2 shows the DVH Comparison of a cervix case using open and Cobalt MLC fields. It can be seen that the use of MLC results in reduced normal tissue dose, while maintaining the GTV dose. Similar comparisons for brain and esophagus sites are shown in Figures 3 and 4 respectively. A typical beam arrangement from the ROPS 3D planning system for a three-field brain case with MLC fields is shown in Figure 5.

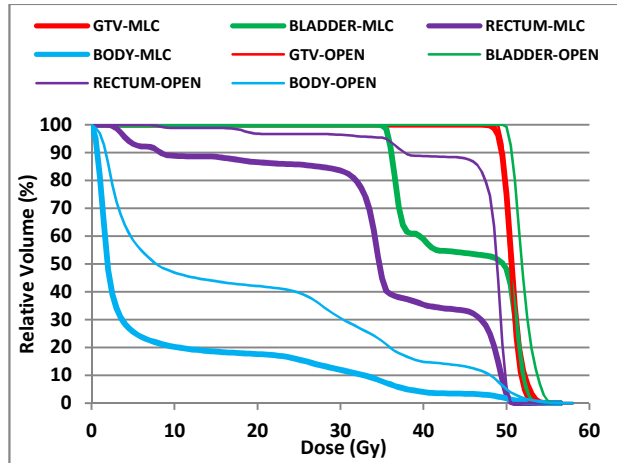


Figure 2: A Case of cervix treatment showing DVH Comparison of MLC vs. OPEN fields. Thick lines are for MLC and thin lines for OPEN beams.

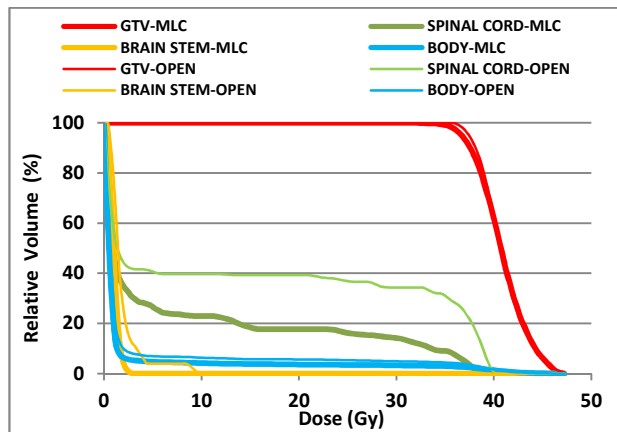


Figure 3: A Case of brain treatment showing DVH Comparison of MLC vs. Open fields. Thick lines are for MLC and thin lines for OPEN beams.

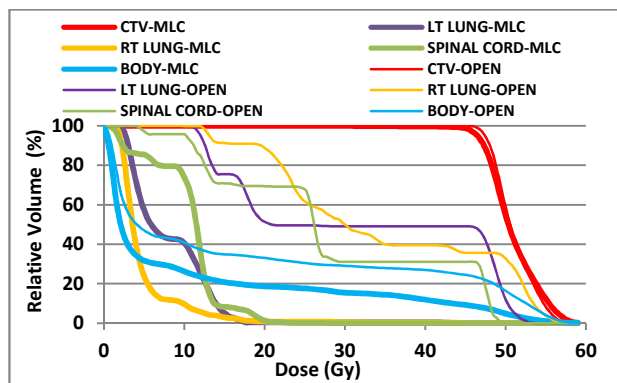


Figure 4: A Case of esophagus treatment showing DVH Comparison of MLC vs. Open fields. Thick lines are for MLC and thin lines for OPEN beams.

Table 1 shows conformity index CI for the GTV. It can be seen that both the open and MLC plans cover the GTV adequately. Due to large or irregular target shape, sometimes the 95% isodose line did not cover even the GTV adequately. In this case, the 90% isodose line

covered adequately. This can be evident in the clinical of case #5 in Table 1.

The CI for critical structure is tabulated in Table 2. It can be seen that the MLC plan showed lower value compared to open beam plan. Once again, a low CI for structures other than the target is desirable.

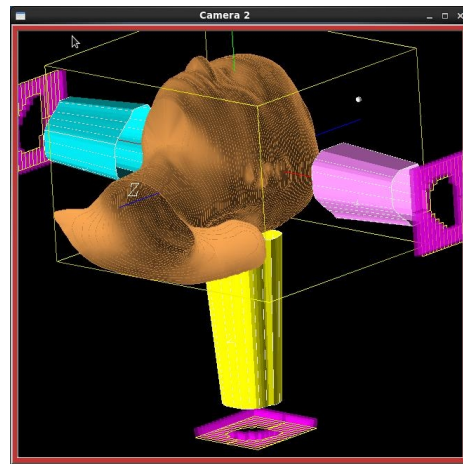


Figure 5: A typical MLC beam arrangement from the ROPS 3D planning system for a three field brain treatment is shown here.

The homogeneity index HI is tabulated in Table 3. The homogeneity index signifies the hot spot in the target volume. A value higher than 1 is undesirable since that signifies the dose outside the GTV is larger than the maximum dose in the target volume. It can be seen from table 3 that for clinical cases 4, 5, 8, 10, the hotspot is larger than in the target volume. This usually happens for three field plans and can be reduced by adding more fields. In this study, our goal was to compare with already treated plans and hence the plans were not modified.

Table 1: Conformity Index for GTV.

Case #	Open	MLC	Open	MLC
	CI 95%	CI 95%	CI 90%	CI 90%
1	1	0.99	1	1
2	1	1	1	1
3	0.96	0.98	1	1
4	1	1	1	1
5	0.8	0.73	0.98	0.94
6	0.99	1	1	1
7	0.93	0.96	1	1
8	0.98	0.96	1	0.99
9	0.91	0.86	1	0.95
10	1	1	1	1

Open means without the use of MLC

Table 2: Conformity Index of critical structures.

Case #	Structure	Open	MLC	Open	MLC
		CI 95%	CI 95%	CI 90%	CI 90%
1	Rectum	0.79	0.48	0.83	0.54
	Bladder	0.41	0.16	0.46	0.2
2	Rectum	0.79	0.25	0.83	0.3
	Bladder	1	0.54	1	0.55
3	Rectum	0.83	0.25	0.91	0.35
	Bladder	0.45	0.04	0.47	0.04
4	Spinal Cord	0.17	0.03	0.21	0.06
	Heart	0.38	0	0.47	0
	Spinal Cord	0	0	0.2	0
5	Lt. Kidney	0.07	0	0.38	0
	Rt. Kidney	0.33	0	0.36	0
6	Spinal Cord	0.02	0	0.05	0
7	Spinal Cord	0.43	0.03	0.54	0.07
8	Optic Nerve	0.99	0.14	0.99	0.14
9	Spinal Cord	0.18	0.05	0.28	0.09
10	Spinal Cord	0.66	0.04	0.83	0.05

Open means without the use of MLC

Table 3: Homogeneity Index for GTV.

Case #	Homogeneity Index	
	Open	MLC
1	1.01	1.01
2	1.01	1.01
3	1.01	1.01
4	1.14	1.20
5	1.12	1.15
6	1.03	1.03
7	1.05	1.07
8	1.11	1.10
9	0.97	0.89
10	1.11	1.20

Open means without the use of MLC

Lastly, Table 4 shows the results of conformation number CN. Even after using 3D plans, the conformation number was not close to unity. This is because isodose cannot conform an irregular shape of the target, unless many beams, 3D dose compensators and non-coplanar beam arrangements are used. However, marked improvement in CN can be noticed by using the MLC compared to open beams. The 90% isodose line resulted in better CN values compared to 95% isodose line.

Table 4: Conformation Number for PTV.

Case #	Open	MLC	Open	MLC
	CN 95	CN 95	CN 90	CN 90
1	0.425	0.590	0.475	0.983
2	0.258	0.669	0.317	0.853
3	0.223	0.526	0.312	0.791
4	0.238	0.543	0.294	0.657
5	0.166	0.346	0.317	0.804
6	0.418	0.521	0.638	0.959
7	0.306	0.592	0.471	0.933
8	0.373	0.555	0.503	0.864
9	0.323	0.359	0.512	0.548
10	0.211	0.670	0.244	0.743

Open means without the use of MLC

4. Discussion

In conventional Telecobalt treatments, patients were treated with open beams, as a consequence of which considerable dose to normal structures are inevitable. It was unavoidable in order to treat the target volumes. Unfortunately, this leads to normal tissue complications for most of organs that were exposed to higher doses. By using shielding blocks, it takes more time to plan a case and for setting up the patient to treat. Also, there is no clear idea about the coverage of PTV and dose to normal structures. Having dedicated treatment planning (ROPS) to control the add-on MLC for existing telecobalt-60 treatment units, it is very easy to plan and treat the required PTV and at the same time, normal organs can be spared. This reduces the normal tissue complications for the patients. This has been shown by adding MLC to existing Telecobalt machines, the same treatments were re-planned in new ROPS treatment planning system. This study showed that a better target coverage and significant dose reduction to OARs could be achieved with the use of MLC.

5. Conclusion

By studying the DVH indices like conformity index, homogeneity index and conformation number, it has been shown that the values of these indices are in favor of MLC beam plans compared to that of open beams. Instead of treating the patients with open beams on old Co-60 units where there is no scope for the modification of the units, it is better to have add-on MLC for the machines. And, it has been demonstrated through DVH analysis that the use of the MLC for Cobalt Teletherapy machine results in benefit for the treatment of patients.

Conflict of interest

The authors declare that they have no conflicts of interest. The authors alone are responsible for the content and writing of the paper.

Funding

This work was done under the financial support of a grant from Board of Research in Nuclear Sciences (BRNS), Mumbai (Project #: 2010/36/65-BRNS).

Acknowledgement

The authors wish to express their sincere thanks to Dr. A.R. Reddy and Dr. M.R. Raju of Mahatma Gandhi Memorial Medical Trust, Bhimavaram for their guidance, support and interest in clinical application of the Cobalt MLC.

References

- Page BR, Hudson AD, Brown DW, *et al.* Cobalt, linac, or other: what is the best solution for radiation therapy in developing countries? *Int J Radiat Oncol Biol Phys.* 2014;89(3):476–80.
- Adams EJ, Warrington AP. A comparison between cobalt and linear accelerator-based treatment plans for conformal and intensity-modulated radiotherapy. *Br J Radiol.* 2008;81:304–10.
- Chandra PJ, Darko J, Vidyasagar PB, *et al.* Dosimetry of interface region near closed air cavities for Co-60, 6 MV and 15 MV photon beams using Monte Carlo simulations. *J Med Phys.* 2010;35(2):73–80.
- Cilla S, Mugambe JK, Digesù C, *et al.* Forward planned intensity modulated radiation therapy using a cobalt source: A dosimetric study in breast cancer. *J Med Phys.* 2013;38(3):125–31.
- Fox C, Romeijn HE, Lynch B, *et al.* Comparative analysis of ⁶⁰Co intensity-modulated radiation therapy. *Phys Med Biol.* 2008;53:3175–88.
- Liu X, Lack D, Rakowski JT, *et al.* Fast Monte Carlo simulation for total body irradiation using a ⁶⁰Co teletherapy unit. *J Appl Clin Med Phys.* 2013;14(3):133–49.
- Schreiner LJ, Joshi CP, Darko J, *et al.* The role of Cobalt 60 in modern radiation therapy: Dose delivery and image guidance. *J Med Phys.* 2009; 34(3):133–36.
- G Sri Krishna, Rani RA, Kumar A, *et al.* Characteristics of the prototype retrofit MLC for telecobalt therapy machine through DVH analysis. Proceedings of National conference on Environmental Radiation and Functional Materials (NCERFM);2015: OP-47.
- Kumar A, Rani RA, Kumar T, *et al.* The use of IMatrix for the measurement of depth dose and profiles of cobalt Teletherapy machine with an automated add-on multi-leaf collimator. Proceedings of 33rd Annual conference of AMPI; 2012:244.
- Ayyangar KM, Rani RA, Kumar A, *et al.* Monte Carlo Study of MLC Fields for Cobalt Therapy Machine. *J Med Phys.* 2014;39(2):71-84.
- Rani RA, Kumar A, Ayyangar KM, *et al.* Experimental verification of MLC fields for cobalt-60 Teletherapy Machine with Monte Carlo simulations. Proceedings of National conference on Environmental Radiation and Functional Materials (NCERFM);2015:OP-45.
- Rani RA, Ayyangar KM, Reddy AR, *et al.* Experimental verification of Monte Carlo simulations of mlc fields for cobalt-60 therapy machine. Proceedings of 35th Annual conference of AMPI (AMPICON);2014:105.
- Kumar A, Rani RA, Ayyangar KM, *et al.* Commissioning and quality assurance of a new Radiation oncology treatment planning system (ROPS). Proceedings of National conference on Environmental Radiation and Functional Materials (NCERFM);2015:OP-46.
- Kumar A, Reddy K, Srinivas V, *et al.* Quantitative comparison of treatment plans using two different planning systems. Proceedings of 35th Annual conference of AMPI (AMPICON); 2014:107.
- Arie van't Riet, Ad C.A. Mak, Marinus A, *et al.* A conformation number to quantify the degree of conformality in brachytherapy and external beam irradiation: application to the prostate. *Int J Radiat Oncol Biol Phys.* 1997;37(3):731-6.