



University of Kentucky  
UKnowledge

---

Surgery Faculty Patents

Surgery

---

10-18-2016

# Compact Heat Exchanger for Venovenous Perfusion-Induced Systemic Hyperthermia Systems

Dongfang Wang

University of Kentucky, [dongfang.wang@uky.edu](mailto:dongfang.wang@uky.edu)

Joseph B. Zwischenberger

University of Kentucky, [joseph.zwischenberger@uky.edu](mailto:joseph.zwischenberger@uky.edu)

**Right click to open a feedback form in a new tab to let us know how this document benefits you.**

Follow this and additional works at: [https://uknowledge.uky.edu/surgery\\_patents](https://uknowledge.uky.edu/surgery_patents)

 Part of the [Surgery Commons](#)

---

## Recommended Citation

Wang, Dongfang and Zwischenberger, Joseph B., "Compact Heat Exchanger for Venovenous Perfusion-Induced Systemic Hyperthermia Systems" (2016). *Surgery Faculty Patents*. 9.  
[https://uknowledge.uky.edu/surgery\\_patents/9](https://uknowledge.uky.edu/surgery_patents/9)

This Patent is brought to you for free and open access by the Surgery at UKnowledge. It has been accepted for inclusion in Surgery Faculty Patents by an authorized administrator of UKnowledge. For more information, please contact [UKnowledge@sv.uky.edu](mailto:UKnowledge@sv.uky.edu).



US009468557B2

(12) **United States Patent**  
**Wang et al.**

(10) **Patent No.:** **US 9,468,557 B2**  
(45) **Date of Patent:** **Oct. 18, 2016**

(54) **COMPACT HEAT EXCHANGER FOR VENO-VENOUS PERFUSION-INDUCED SYSTEMIC HYPERTHERMIA SYSTEMS**

USPC ..... 607/104-106; 600/18; 604/6.13, 4.01  
See application file for complete search history.

(75) Inventors: **Dongfang Wang**, Lexington, KY (US);  
**Joseph B. Zwischenberger**, Lexington, KY (US)

(73) Assignee: **THE UNIVERSITY OF KENTUCKY RESEARCH FOUNDATION**,  
Lexington, KY (US)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 626 days.

(21) Appl. No.: **13/584,696**

(22) Filed: **Aug. 13, 2012**

(65) **Prior Publication Data**

US 2013/0211483 A1 Aug. 15, 2013

**Related U.S. Application Data**

(60) Provisional application No. 61/522,411, filed on Aug. 11, 2011, provisional application No. 61/651,164, filed on May 24, 2012.

(51) **Int. Cl.**

**A61F 7/00** (2006.01)  
**A61M 1/26** (2006.01)  
**A61M 1/16** (2006.01)  
**A61M 1/10** (2006.01)

(52) **U.S. Cl.**

CPC ..... **A61F 7/0085** (2013.01); **A61M 1/1698** (2013.01); **A61M 1/26** (2013.01); **A61M 2001/1006** (2013.01); **A61M 2001/1065** (2013.01); **A61M 2001/267** (2013.01)

(58) **Field of Classification Search**

CPC ..... A61F 2007/126; A61F 2007/0054; A61F 7/12; A61M 1/16; A61M 1/3666

(56) **References Cited**

U.S. PATENT DOCUMENTS

973,868 A	10/1910	Kneuper
2,474,665 A	6/1949	Guarino
2,742,158 A	4/1956	Schuller
3,103,928 A	9/1963	Broman
3,183,908 A	5/1965	Collins et al.
3,410,263 A	11/1968	McGinnis
3,429,443 A	2/1969	Stern

(Continued)

OTHER PUBLICATIONS

United States Patent and Trademark Office, U.S. Appl. No. 13/584,704, Office Action dated Mar. 11, 2014, 9 pages.

(Continued)

*Primary Examiner* — Kaitlyn Smith


*Assistant Examiner* — Yasamin Ekrami

(74) *Attorney, Agent, or Firm* — King & Schickli, PLLC

(57) **ABSTRACT**

A compact heat exchanger for veno-venous perfusion-induced hyperthermia includes an integral pneumatic pump and a hollow tubule heat exchange array. A veno-venous perfusion-induced hyperthermia system incorporating the compact heat exchanger is described. The heat exchanger provides a compact, efficient design allowing a lesser heat exchanging surface area and lesser required pumping power compared to conventional systems. In turn, the system provides a shorter blood circuit compared to conventional systems, allowing maintaining a lower blood temperature than such conventional systems while supplying sufficiently heated blood to patient visceral organs to provide a therapeutic effect, such as in supplementing chemotherapy drugs.

**11 Claims, 7 Drawing Sheets**

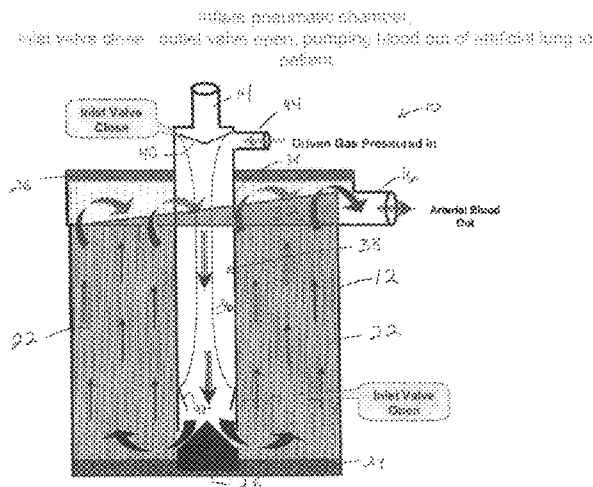

(56)

References Cited

U.S. PATENT DOCUMENTS

3,768,977 A	10/1973	Brumfield et al.	5,817,279 A	10/1998	Eilers et al.	
3,855,995 A	12/1974	Bentley	5,823,987 A *	10/1998	Elgas et al. ....	604/6.13
3,856,475 A	12/1974	Marx	5,858,233 A	1/1999	Elgas et al.	
3,898,045 A	8/1975	Bowley	5,906,741 A	5/1999	Elgas et al.	
3,934,982 A	1/1976	Arp	5,922,202 A	7/1999	Elgas et al.	
3,935,110 A	1/1976	Schmid et al.	5,958,255 A	9/1999	Hobrecht et al.	
3,960,657 A	6/1976	Bowley	6,017,493 A	1/2000	Cambron et al.	
3,989,626 A	11/1976	Bentley et al.	6,224,829 B1	5/2001	Piplani et al.	
4,017,279 A	4/1977	Bowley	6,336,911 B1	1/2002	Westerbeck	
4,094,792 A	6/1978	Bentley	6,368,557 B1	4/2002	Piplani et al.	
4,098,275 A	7/1978	Consalvo	6,379,618 B1	4/2002	Piplani et al.	
4,134,402 A	1/1979	Mahurkar	6,395,226 B1	5/2002	Plunkett	
4,188,360 A	2/1980	Kurata	6,406,452 B1	6/2002	Westerbeck	
4,196,075 A	4/1980	Bentley	6,413,233 B1	7/2002	Sites et al.	
4,205,042 A	5/1980	Lobdell et al.	6,428,747 B1	8/2002	Dueri et al.	
4,268,476 A	5/1981	Raible	6,454,999 B1	9/2002	Farhangnia et al.	
4,297,318 A	10/1981	Raible	6,497,841 B1	12/2002	Plotkin et al.	
4,368,118 A	1/1983	Siposs	6,503,450 B1	1/2003	Afzal et al.	
4,372,914 A	2/1983	Raible	6,508,983 B1	1/2003	McBurney et al.	
4,374,088 A	2/1983	Stenberg et al.	6,572,821 B2	6/2003	Knott	
4,533,516 A	8/1985	Johnsson et al.	6,579,496 B1	6/2003	Fausset et al.	
4,552,552 A	11/1985	Polaschegg et al.	6,607,517 B1 *	8/2003	Dae et al. ....	604/500
4,573,883 A	3/1986	Noon et al.	6,613,008 B2 *	9/2003	Aboul-Hosn et al. ....	604/5.01
4,612,126 A	9/1986	Alt et al.	6,630,107 B1	10/2003	Merce Vives	
4,623,518 A	11/1986	Raible	6,644,320 B2	11/2003	Groth et al.	
4,698,207 A	10/1987	Bringham et al.	6,669,661 B1	12/2003	Yee	
4,770,652 A	9/1988	Mahurkar	6,682,698 B2	1/2004	Chambers et al.	
4,808,155 A	2/1989	Mahurkar	6,689,315 B2	2/2004	Linker et al.	
4,874,581 A	10/1989	Sutherland et al.	6,716,157 B2	4/2004	Goldowsky	
4,906,229 A	3/1990	Wampler	6,716,188 B2	4/2004	Noda et al.	
4,908,014 A	3/1990	Kroyer	6,723,283 B2	4/2004	Ghelli et al.	
4,915,837 A	4/1990	Verity	6,726,653 B2	4/2004	Noda et al.	
4,925,377 A	5/1990	Inacio et al.	6,730,267 B2	5/2004	Stringer et al.	
4,975,247 A	12/1990	Badolato et al.	6,884,360 B2	4/2005	Chang	
5,034,188 A	7/1991	Nakanishi et al.	6,908,446 B2	6/2005	Yokoyama et al.	
5,058,661 A *	10/1991	Oshiyama .....	6,960,322 B2	11/2005	Stringer et al.	
		A61M 5/44	7,022,099 B2	4/2006	Litzie et al.	
		165/11.1	7,022,284 B2	4/2006	Brian et al.	
RE33,932 E	5/1992	Fukasawa et al.	7,135,008 B2	11/2006	O'Mahony et al.	
5,116,308 A	5/1992	Hagiwara	7,238,320 B2	7/2007	Ghelli et al.	
5,120,501 A	6/1992	Mathewson et al.	7,541,000 B2	6/2009	Stringer et al.	
5,139,741 A	8/1992	Hagiwara	7,785,247 B2	8/2010	Tatum et al.	
5,158,533 A	10/1992	Strauss et al.	7,819,835 B2 *	10/2010	Landy et al. ....	604/6.13
5,188,732 A	2/1993	De Niel et al.	2002/0044889 A1 *	4/2002	Aboul-Hosn .....	A61M 1/1698 422/45
5,197,951 A	3/1993	Mahurkar				
5,217,689 A	6/1993	Raible	2004/0226868 A1	11/2004	Shoji et al.	
5,221,255 A	6/1993	Mahurkar et al.	2006/0009728 A1	1/2006	Litzie et al.	
5,225,161 A	7/1993	Mathewson et al.	2006/0177343 A1	8/2006	Brian, III et al.	
5,236,665 A	8/1993	Mathewson et al.	2007/0217948 A1	9/2007	Ghelli et al.	
5,270,004 A	12/1993	Cosentino et al.	2007/0249888 A1	10/2007	Wu et al.	
5,270,005 A	12/1993	Raible	2008/0199357 A1	8/2008	Gellman et al.	
5,282,783 A	2/1994	Lindsay	2008/0234623 A1	9/2008	Strauss et al.	
5,316,724 A	5/1994	Mathewson et al.	2009/0087342 A1 *	4/2009	Maianti .....	A61M 1/1698 422/46
5,338,512 A	8/1994	Mathewson et al.				
5,354,277 A	10/1994	Guzman et al.	2010/0106072 A1	4/2010	Kashefi-Korasaki et al.	
5,358,689 A	10/1994	Jones et al.	2010/0274170 A1 *	10/2010	Carpenter et al. ....	604/6.09
5,374,245 A	12/1994	Mahurkar	2013/0004369 A1	1/2013	Marseille	
5,395,525 A	3/1995	Takano et al.				
5,421,405 A	6/1995	Goodin et al.				
5,476,444 A	12/1995	Keeling et al.				
5,718,871 A	2/1998	Elgas				
5,762,868 A	6/1998	Leonard				
5,762,875 A	6/1998	Gremel et al.				
5,770,149 A	6/1998	Raible				
5,787,729 A	8/1998	Wijaya				
5,788,287 A	8/1998	Gremel				

OTHER PUBLICATIONS

United States Patent and Trademark Office, U.S. Appl. No. 13/584,704, Office Action dated Jun. 25, 2014, 8 pages.  
 United States Patent and Trademark Office, U.S. Appl. No. 13/584,704, Notice of Allowance and Fee(s) Due, dated Aug. 22, 2014, 7 pages.

\* cited by examiner

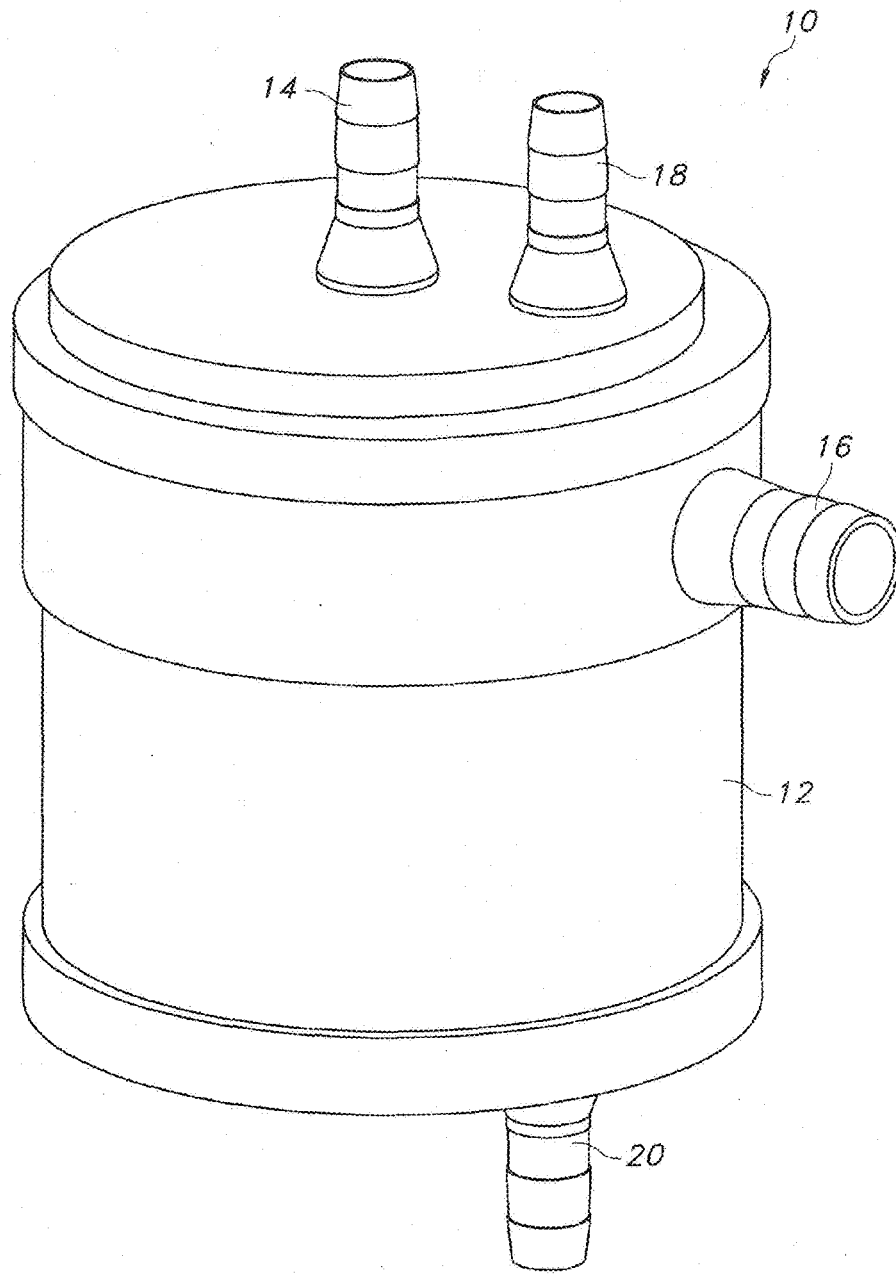
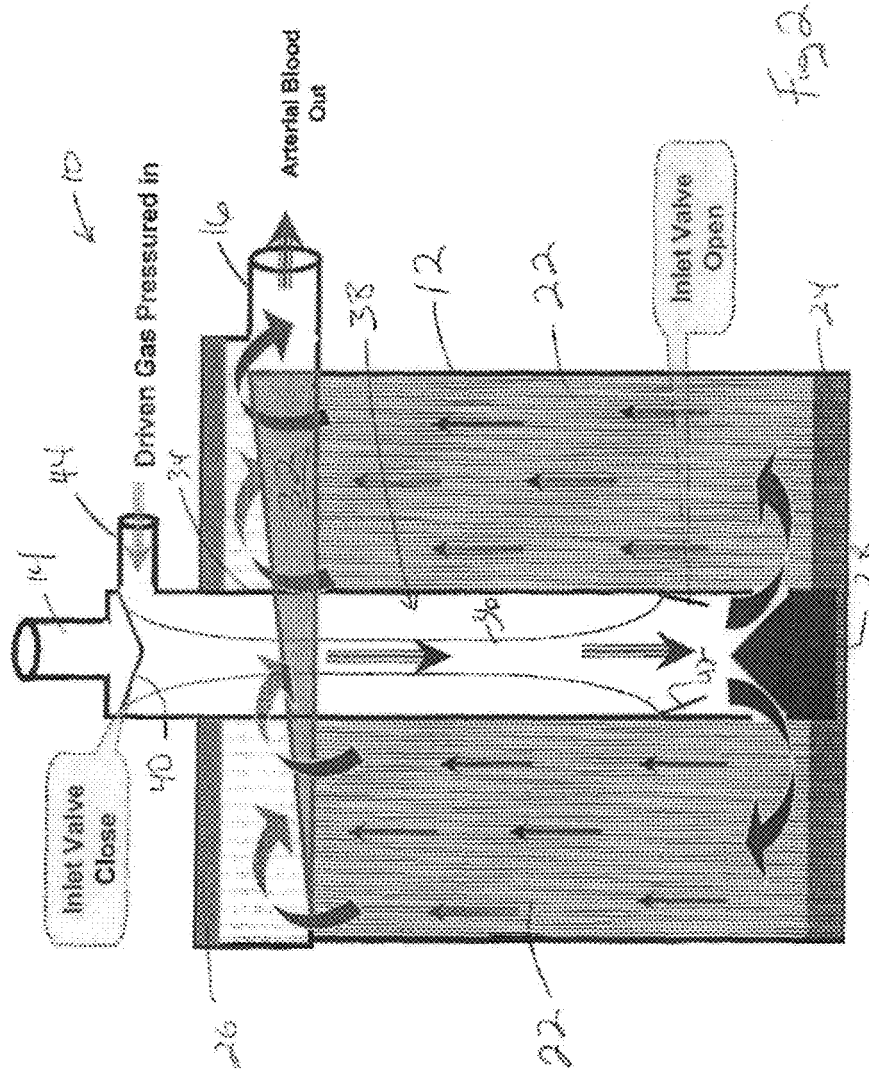


FIG. 1

Inflate pneumatic chamber,  
inlet valve close, outlet valve open, pumping blood out of artificial lung to  
patient



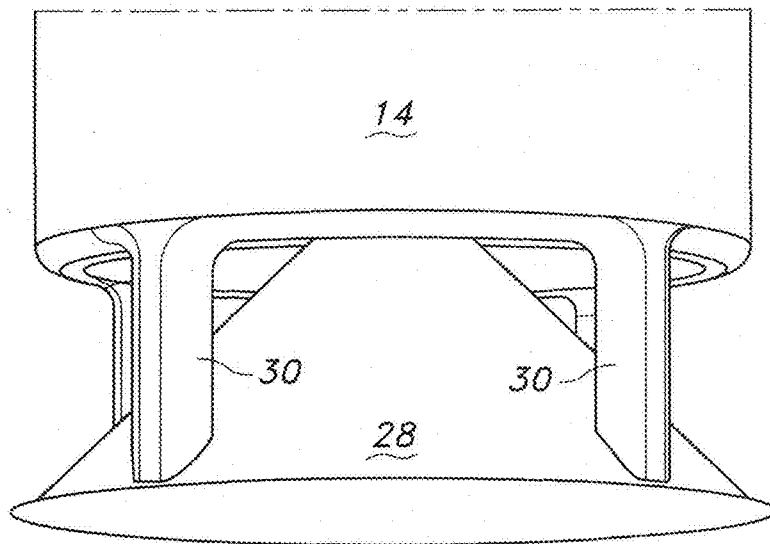


FIG. 3

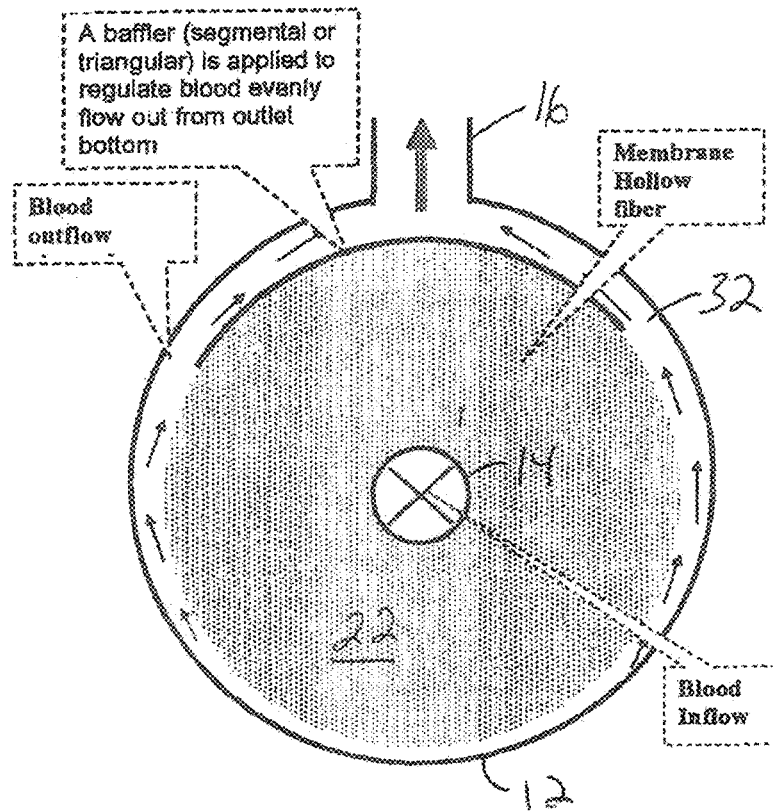


FIG. 4

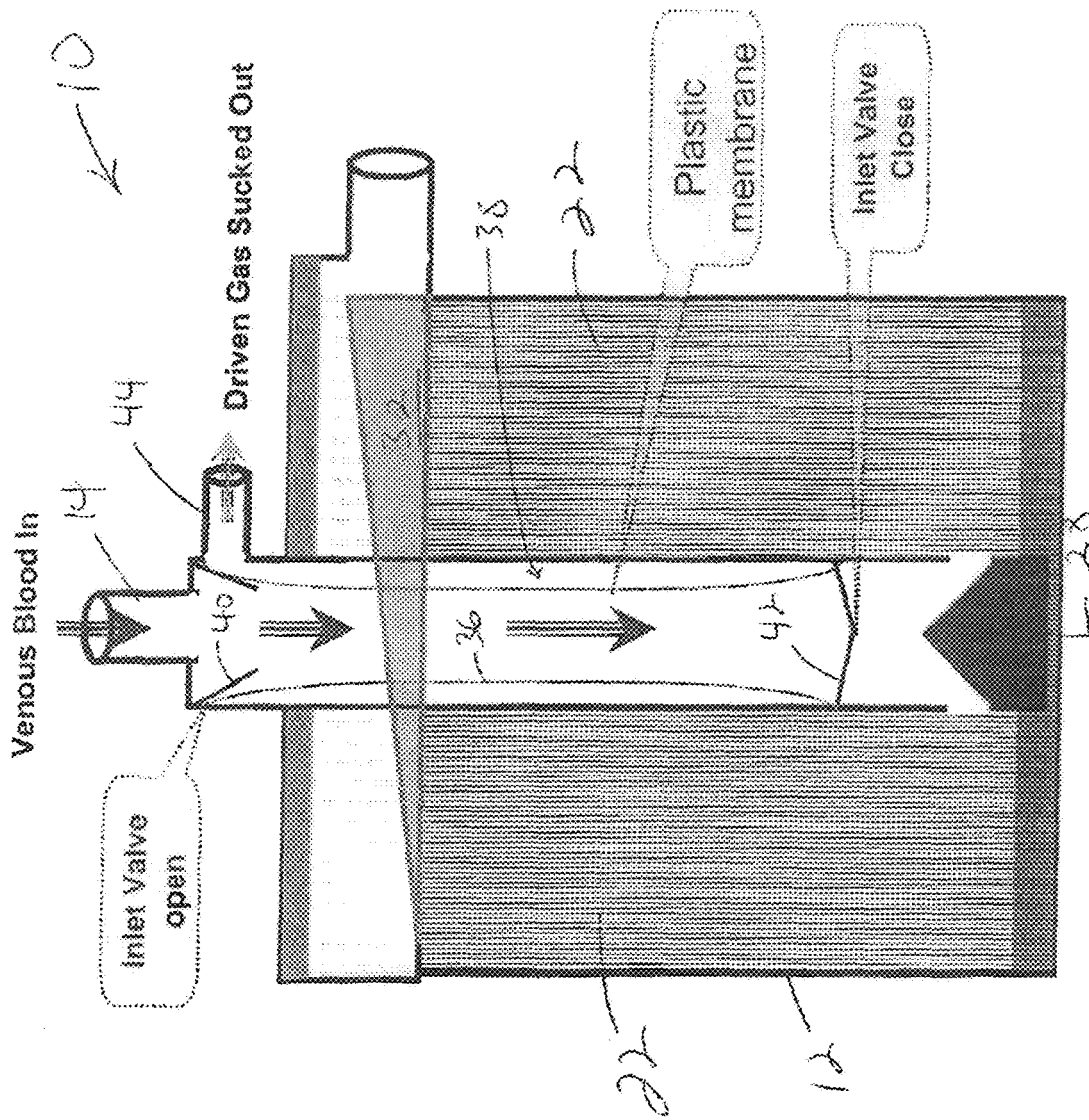


FIG. 5



Diastole

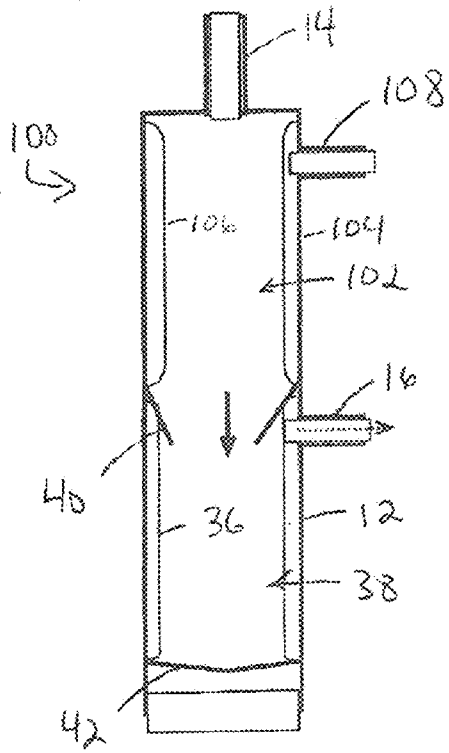


FIG. 6a

Systole

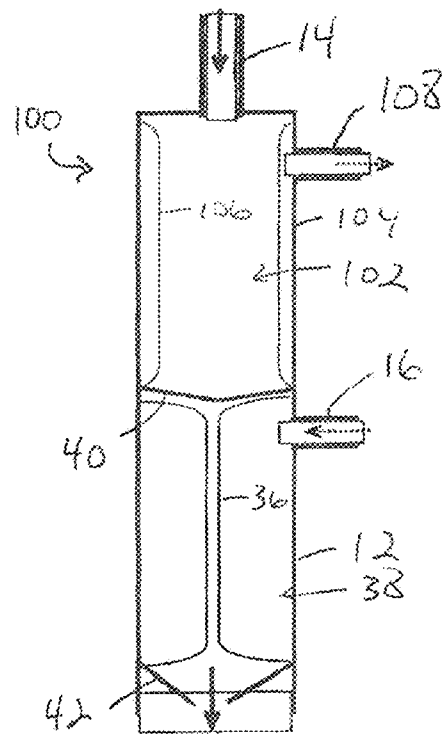


FIG. 6b

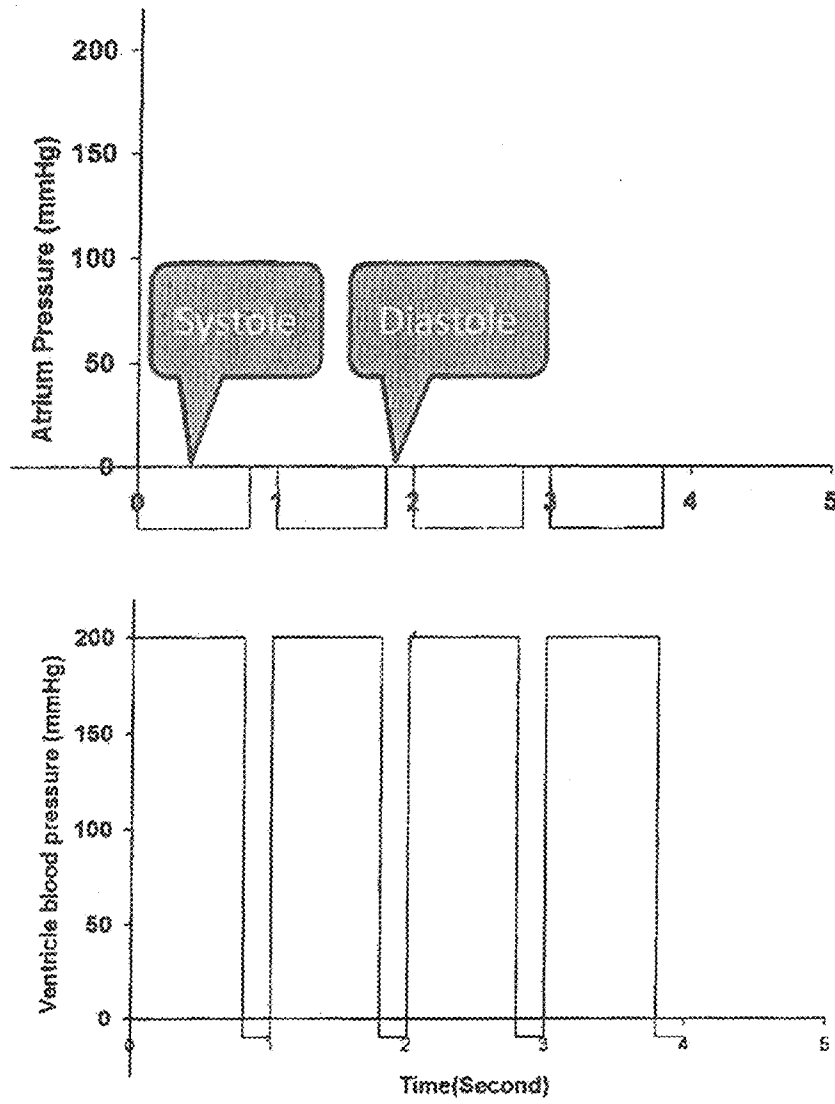


FIG. 7

1

## COMPACT HEAT EXCHANGER FOR VENO-VENOUS PERFUSION-INDUCED SYSTEMIC HYPERTHERMIA SYSTEMS

This application claims the benefit of priority in U.S. Provisional Patent Application Ser. Nos. 61/522,411 filed on Aug. 11, 2011 and 61/651,164 filed on May 24, 2012, the entirety of the disclosures of each of which are incorporated herein by reference.

### TECHNICAL FIELD

The present invention relates generally to the field of medical devices. In particular, the invention relates to a compact heat exchanger for use in veno-venous perfusion induced systemic hyperthermia (vv-PISH) systems.

### BACKGROUND OF THE INVENTION

In 2007 lung cancer was responsible for 31% of all cancer-related deaths. Advanced stage NSCLC present in 75% of all new lung cancer cases provides a median survival rate of only 9-12 months despite maximal combination chemotherapy. Despite improvements in cancer therapies, the long-term prognosis for patients with metastatic lung cancer remains dismal, and indeed chemotherapy provides only a modest improvement in survival over supportive care alone.

It has been shown that regional and local hyperthermia exhibits synergism with various conventional chemotherapy agents. Hyperthermia selectively kills cancer cells and enhances cytotoxicity of certain chemotherapy drugs, increases tumor blood flow and permeability of tumor blood vessels, and thereby increases drug delivery into a tumor. For example, hyperthermia enhances platinum uptake and inhibits platinum-induced DNA adduct repair, an effect that may be important in reversing cisplatin resistance. Thus, concurrent combined hyperthermia and chemotherapy has great potential in advanced NSCLC therapy.

Because advanced stage NSCLC patients often have metastasis to remote sites, it is contemplated that systemic hyperthermia would provide advantages over local hyperthermia. Systemic hyperthermia causes marked physiological changes, but damage to normal tissue occurs when temperatures exceed 44 C. Heat has a selective killing effect on malignant phenotypes (lung, colon, and pancreatic cancers, for example) at temperatures between those exhibited during normal fevers and temperatures that induce tissue destruction (41-45 C). This suggests that a hyperthermia therapeutic window may exist for cancer therapy. However, conventional heat delivery such as radiant heat disadvantageously redistributes blood flow away from visceral organs to skin, and peripheral tissue, resulting in heterogenous heat distribution. This leads to insufficient heat delivery to provide a therapeutic benefit, compromising treatment efficiency, and also induces pain and peripheral nerve damage. In turn, conventional veno-venous perfusion-induced hyperthermia systems, because of their relatively long tubing lengths and requiring multiple cannulations (increased circuit lengths), must heat blood to unacceptable temperatures (46 C and above) to provide the desired hyperthermic effect, risking damage to blood cells and pain to the patient.

To solve this and other problems, the present disclosure provides a veno-venous perfusion-induced hyperthermia system (vv-PISH) which delivers more heat to visceral organs for metastatic cancer treatment while eliminating complications and disadvantages of radiant heat. The system

2

includes, a compact heat exchanger including an integral pneumatic pump and blood flow redirector structures. The device of the present disclosure provides an even blood flow pattern, preventing or reducing incidence of thrombosis. In turn, the presently disclosed design simplifies the blood circuit and also provides a pulsatile blood flow pattern, promoting active blood mixing and thereby improving gas exchange within the pump. The present device finds use at least as a supplemental therapy for conventional chemotherapy regimens.

### SUMMARY OF THE INVENTION

The present disclosure provides a blood heat exchanger for use as a supplement or replacement therapeutic treatment to conventional chemotherapy. The heat exchanger includes an integral pneumatic pump enclosed substantially within a housing thereof, providing a compact and efficient design. Inlet blood redirectors and outlet blood collectors are provided, which in combination with the integral pneumatic pump promote an even perfusion and mixing of blood, eliminating areas of stagnation and improving heat exchange.

In an embodiment, an atrium is provided at an inlet of the blood heat exchanger. The atrium is defined by one or more additional pneumatic pumps for promoting blood flow from a patient body into the heat exchanger. By cyclically maintaining an internal pressure of the atrium pneumatic pump(s) at zero or less, a constant, even supply of blood from the patient is provided at the blood heat exchanger inlet, thereby eliminating the pulsatile inlet blood flow patterns provided by conventional pumping systems.

In turn, a veno-venous perfusion-induced systemic hyperthermia system (vv-PISH) incorporating the heat exchanger of the present disclosure is described, for removing cooler blood from a patient body and returning heated blood to same.

These and other embodiments, aspects, advantages, and features of the present invention will be set forth in the description which follows, and in part will become apparent to those of ordinary skill in the art by reference to the following description of the invention and referenced drawings or by practice of the invention. The aspects, advantages, and features of the invention are realized and attained by means of the instrumentalities, procedures, and combinations particularly pointed out in the appended claims. Unless otherwise indicated, any references discussed herein are specifically incorporated by reference in their entirety into the present disclosure.

### BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings incorporated in and forming a part of the specification, illustrate several aspects of the present invention, and together with the description serve to explain the principles of the invention. In the drawings:

FIG. 1 shows a housing for the heat exchanger of the present disclosure;

FIG. 2 shows a cross-sectional side view of the heat exchanger

FIG. 3 shows an inlet blood flow redirector for the heat exchanger;

FIG. 4 shows a top view of the heat exchanger of the disclosure;

FIG. 5 shows a cross-sectional side view of the heat exchanger, including an integrated pneumatic pump,

FIGS. 6a and 6b show the heat exchanger including an atrium, in diastolic phase (FIG. 6a) and in systolic phase (FIGS. 6b); and

FIG. 7 graphically depicts relative internal pressures of the atrium and heat exchanger in systolic and diastolic phases.

#### DETAILED DESCRIPTION OF THE ILLUSTRATED EMBODIMENTS

In the following detailed description of the illustrated embodiments, reference is made to the accompanying drawings that form a part hereof, and in which is shown by way of illustration, specific embodiments in which the invention may be practiced. These embodiments are described in sufficient detail to enable those skilled in the art to practice the invention. Also, it is to be understood that other embodiments may be utilized and that process, reagent, software, and/or other changes may be made without departing from the scope of the present invention.

In one aspect, the present disclosure provides a compact heat exchanger 10 (see FIG. 1) including a housing 12, at least one blood inlet 14, and at least one blood outlet 16. At least one heated fluid inlet 18 and at least one heated fluid outlet 20 are provided for supplying a heated fluid to and removing same from the heat exchanger 10, typically with the heated fluid being passed through a hollow heat exchanging tubule array 22 of the heat exchanger 10 in a counter-current direction compared to that of the blood flow. The heat exchanging tubule array 22 may be fabricated of any suitable heat exchanging metal. In an embodiment, the tubules of the heat exchanging tubule array 22 are fabricated of 0.2 mm thick stainless steel tubing and provide approximately 0.095-0.113 m<sup>2</sup> of total heat exchanging surface.

As shown in FIG. 2, arrays 22 of heat exchanging tubules may be provided arranged substantially parallel to a longitudinal axis of the heat exchanger 10 housing 12, or alternatively diagonal spirally wound heat exchanging tubule arrays 22 (not shown) may be provided. Inlet potting 24 and outlet potting 26, known in the art, is provided and disposed to prevent entry of blood into the lumens of the hollow heat exchanging tubules of the heat exchanging tubule array 22 and direct mixing with the heated fluid contained therein. The inlet potting 24 may define an inverted dome shape, further assisting in promoting even redistribution of blood passing through the heat exchanger 10. The inlet potting 24 may define an inverted dome shape, further assisting in promoting even redistribution of blood passing through the heat exchanger 10.

The system 10 of the invention further includes blood flow redirector structures, providing an even blood flow pattern as blood passes through the heat exchanger 10. An inlet blood flow redirector 28 is provided at an end of the heat exchanger 10 distal from the blood inlet 14 for evenly redirecting blood flow passing through the blood inlet 14. In an embodiment, a frusto-conical inlet blood flow redirector 28 is provided at a distal end of the blood inlet 14 (see FIG. 3), secured to or molded with the distal end of the blood inlet 14 by one or more columns 30. At least a portion of the conical inlet blood flow redirector 28 is disposed in an interior of the blood inlet 14 distal end. Like structures are described in U.S. Pat. No. 8,906,300, filed concurrently herewith and incorporated herein in its entirety by reference. As shown in FIG. 2, the inlet blood flow redirector 28 promotes even radial perfusion across a surface of the inlet potting 24 at a bottom of the heat exchanger and also even axial blood flow as blood travels through the heat exchanger

10 towards the blood outlet 16 (see arrows), eliminating stagnant blood flow in the heat exchanger 10. In turn, a blood collection channel 32 is provided at a top of the heat exchanger 10, whereby blood exiting the heat exchanging tubule array 22 is collected and redirected to the blood outlet 16 (see FIGS. 2 and 4). A substantially crescent-shaped blood collection channel 32 is shown, although the skilled artisan will appreciate that other cross-sectional shapes are possible and contemplated, such as segmental, triangular, etc. The blood collection channel 32 regulates blood flow evenly at the outlet end of the heat exchanger 10, and further guides blood to the blood outlet 16. That is, blood enters via the blood inlet 14 and is evenly redirected by the inlet blood flow redirector 28 as summarized above to pass over the heat exchanging tubule array 22. On exiting the heat exchanging tubule array 22, blood passes into the blood collection channel 32 and therefrom exits the heat exchanger 10 via the blood outlet 16. In that manner, areas of stagnant blood flow at or near the blood outlet 16 are reduced or eliminated.

In turn, a blood collection channel 32 is provided at a top of the heat exchanger 10, whereby blood exiting the heat exchanging tubule array 22 is collected and redirected to the blood outlet 16 (see FIGS. 2 and 4). A substantially crescent-shaped blood collection channel 32 is shown, although the skilled artisan will appreciate that other cross-sectional shapes are possible and contemplated, such as segmental, triangular, etc. The blood collection channel 32 regulates blood flow evenly at the outlet end of the heat exchanger 10, and further guides blood to the blood outlet 16. That is, blood enters via the blood inlet 14 and is evenly redirected by the inlet blood flow redirector 28 as summarized above to pass over the heat exchanging tubule array 22. On exiting the heat exchanging tubule array 22, blood passes into the blood collection channel 32 and therefrom exits the heat exchanger 10 via the blood outlet 16. In manner, areas of stagnant blood flow at or near the blood outlet 16 are reduced or eliminated.

Rather than utilizing an external pump as is common with conventional heat exchangers, the heat exchanger 10 of the present disclosure includes an integral pneumatic pump to provide pumping action for passing blood from the blood inlet 14, over the heat exchanging tubule array 22, and to the blood outlet 16. As such, a compact, economical and efficient combination of pump and heat exchanger is provided. Providing further advantages, the integral pneumatic pump provides a pulsatile blood flow pattern, promoting active blood mixing as the blood passes through the heat exchanger 10, for improved heat exchange performance and an improved blood flow pattern to reduce thrombogenicity. Because of that improved gas exchange performance, it is possible to provide a lesser heat exchange surface area compared to conventional heat exchangers, allowing a more compact unit.

With reference to FIG. 5, a cylinder 34 is disposed in an interior of the heat exchanging tubule array 22. Within cylinder 34, a flexible membrane 36 is disposed to define a pneumatic pump 38. Pump inlet and outlet valves 40, 42, in an embodiment being duck-bill valves of known configuration, prevent other than a uni-directional blood flow through the pneumatic pump 38 (see arrows).

A pump gas inlet/outlet 44 is connected to a pneumatic console (not shown) for providing gas to operate the pneumatic pump 38. Pump gas is cyclically supplied to and withdrawn from the pump gas inlet/outlet 44, causing the flexible membrane 36 to expand and contract, providing a pumping action to promote blood flow. As shown in FIGS. 2 and 5, when gas is supplied to the pump gas inlet/outlet 44

(systole), the flexible membrane **36** collapses, closing the pump inlet valve **40** and forcing blood out of the pneumatic pump **38** via the now open outlet valve **42** to pass over the heat exchanging tubule array **22**. When gas is withdrawn from the pump gas inlet/outlet **44** (diastole), the flexible

membrane **36** expands, closing the pump outlet valve **42** and opening the pump inlet valve **40**, generating negative pressure and drawing blood into the pneumatic pump **38** from the patient's body through the now-open pump inlet valve **40** (FIG. 5). On the next cycle, the blood is delivered from the pneumatic pump **38** as described above.

In an embodiment, a heat exchanger **10** was fabricated having an integral pneumatic pump **38** with an outer diameter of approximately 20 mm. In bench tests using 37% glycerin in a mock blood flow circuit, this device was shown to provide a pumping rate of from 1.251 L/min at 40 beats per minute to 3.2 L/min at 90 beats per minute against 100 mm Hg afterload, which was more than sufficient to meet a benchmark of 1-1.5 L/min. Heat exchange efficiency for this device was above 70% at a flow rate of 1-1.5 L/min.

By the foregoing design, a heat exchanger **10** is possible which provides a desired circuit blood flow rate of 0.5-2.0 L/min, an therapeutic hyperthermia dose of 42 C for 120 min, a heating period of less than 40 minutes, an infusion blood temperature of 44 C or less, and stable hemodynamics.

In another aspect, an atrium **100** is provided which further improves blood flow through the heat exchanger **10** of the present disclosure (see FIGS. **6a** and **6b**). In an embodiment, the atrium **100** is defined by at least one additional pneumatic pump **102**, disposed at or defining the blood inlet of the heat exchanger **10**. As shown the at least one additional pneumatic pump **102** is configured substantially as described above for the integral pneumatic pump **38** of the heat exchanger **10**, including a pneumatic cylinder **104** and flexible membrane **106**, and a gas inlet/outlet **108**. For convenience and compactness, the atrium outlet valve may define the inlet valve **40** for the heat exchanger **10** integrated pneumatic pump **38**, although of course the valve structures may be entirely separate.

The atrium **100** operates in systolic and diastolic phases as described for the heat exchanger **10** pneumatic pump **38**. That is, cyclically supplying gas to the gas inlet/outlet **108** causes the atrium pneumatic pump **102** flexible membrane **106** to expand and collapse, passing blood through the pneumatic pump **102** and into the heat exchanger **10**.

In use, the atrium **100** is kept primarily in a state of negative internal pressure by withdrawal of gas, with the exception of a time immediately prior to the diastolic phase of the heat exchanger **10** pneumatic pump **38** (see FIG. 7). Typically, the atrium **100** internal pressure is substantially zero at the highest, i.e. during diastole. This is accomplished by intermittently discontinuing withdrawal of gas from the atrium **100** (as distinguished from affirmatively supplying gas to the atrium **100** pneumatic pump **102**). In contrast, the heat exchanger **10** pneumatic pump **38** is provided only a very short phase of negative internal pump pressure (see FIG. 7). In diastole, when an internal pressure of the atrium **100** pneumatic pump **102** is highest, an internal pressure of the heat exchanger **10** pneumatic pump **38** is made slightly negative by withdrawal of gas (see FIG. 7).

By this design, the skilled artisan will appreciate that a consistent flow of blood is established into the inlet of the heat exchanger **10** compared to the pulsatile and irregular entry of blood into heat exchangers established by conventional designs. This is because the internal pressure of the atrium **100** into which blood first flows is almost always

negative and blood is almost always draining from the patient and into the atrium. In turn, very little resistance is imposed to transfer of blood from the atrium **100** into the heat exchanger **10** to fill the pneumatic pump **38**, since when pump gas is withdrawn from the heat exchanger **10** pneumatic pump **38** (diastole, see FIGS. **6a** and **7**), the internal pressure of the atrium **100** is zero at its highest, i.e. slightly higher than the internal pressure of the heat exchanger **10** pneumatic pump **38**. By this mechanism, transfer of blood from the atrium **100** to the heat exchanger **10** pneumatic pump **38** is promoted by that slight pressure differential. These differentials are shown graphically in FIG. 7. Of course, the more even and non-pulsatile blood flow pattern established between the atrium **100** and the heat exchanger **10** achieved by the present mechanism should not be confused with the pulsatile flow established for blood passing through the heat exchanger **10** via the heat exchanger pneumatic pump **38**, for the benefits described above.

The present heat exchanger **10** will typically be supplied with blood from a patient's body by a cannula. A dual lumen cannula such as those described in U.S. Pat. No. 7,473,239 and/or U.S. Published Patent Appl. No. US 2011/0040241 is preferred, which both passes blood from a patient's body via a withdrawal cannula into the oxygenator **10** and passes blood back into the patient's body via a delivery cannula. The dual lumen cannula may be inserted through a small incision into the right jugular vein, via the superior vena cava and traversing the right atrium, with the tip positioned in the inferior vena cava. This has the further advantage of reducing the length of the defined blood flow circuit and thereby the length of the vv-PISH circuit, reducing the length of time blood is exposed to potentially damaging heat and also the amount of heat required to raise the blood temperature to a desired level, and further eliminates multiple and potentially dangerous (to the patient) cannulations. In combination with the pump-integrated heat exchanger **10** of the present disclosure, use of a dual lumen cannula allows shortening the vv-PISH circuit to  $\frac{1}{10}^{th}$  that of prior art systems. Blood contact surface area, circuit resistance, and circuit heat loss are significantly reduced, improving efficiency, reliability, and performance.

An electronically controlled pneumatic console may be provided to drive the above-described pneumatic pump **38**. Because the pump-integrated heat exchanger **10** includes a pneumatic pump **38** of lesser capacity than is needed to drive a conventional heat exchanger, a more compact pneumatic console is possible.

There is accordingly provided by the present disclosure a compact, efficient heat exchanger **10** which provides a pulsatile, evenly dispersed blood flow therethrough, augmenting heat exchange performance and in turn allowing a lessened heat exchange surface area providing a necessary level of heating of blood, to allow a more compact and efficient design. The heat exchanger **10** may include an atrium **100** defined by one or more additional pneumatic pumps **102**, for regulating and providing an even blood supply from a patient's circulatory system into the heat exchanger **10**. The heat exchanger **10** finds use in a variety of procedures, including supplementing conventional cancer chemotherapy regimens. Unlike conventional heat exchanger designs, the present heat exchanger **10** reduces or eliminates regions of stagnant or limited blood flow leading to thrombosis and device occlusion/failure, and further provides a pulsatile flow which also decreases stagnant blood flow and reduces thrombogenicity.

In turn, the integrated pump design of the heat exchanger **10** eliminates connectors and tubing such as are found in

7

conventional heat exchanger/non-integral pump designs, reducing resistance to blood flow and improving pump performance. The combined integrated pump/heat exchanger lung design simplifies and shortens the vv-PISH circuit in that only one component is provided in the circuit, and further increases pump efficiency by eliminating blood flow resistance from connections between the pump and the artificial lung.

One of ordinary skill in the art will recognize that additional embodiments of the invention are also possible without departing from the teachings herein. For example, the above-described vv-PISH system may optionally include a dialysis unit (not shown) for use in patients with compromised kidney function. The dialysis unit may be connected via connectors (not shown) on the heat exchanger **10** blood inlet/outlet. Advantageously, the pressure gradient created by the heat exchanger **10** will drive up to 30% of the circuit blood flow (recirculation) through the dialysis unit, without requiring additional external pumps.

This detailed description, and particularly the specific details of the exemplary embodiments, is given primarily for clarity of understanding, and no unnecessary limitations are to be imported, for modifications will become obvious to those skilled in the art upon reading this disclosure and may be made without departing from the spirit or scope of the invention. Relatively apparent modifications, of course, include combining the various features of one or more figures or examples with the features of one or more of other figures or examples.

What is claimed is:

**1.** A compact heat exchanger for veno-venous perfusion-induced hyperthermia, comprising:

a housing, a blood inlet ending at a distal-most surface of the compact heat exchanger and defining a longitudinal axis, a blood outlet, a heated fluid inlet, and a heated fluid outlet;

a hollow tubule heat exchange array disposed within an interior of the housing for heat exchange to and from blood passing through the compact heat exchanger;

an inlet blood flow redirector disposed at a distal-most end of the blood inlet and configured to redirect a flow of the blood radially to the longitudinal axis across the compact heat exchanger distal-most surface and therefrom to the hollow tubule heat exchange array, the blood perfusing therefrom to the blood outlet; and

a pneumatic pump disposed substantially within the blood inlet and within a perimeter defined by the housing, further wherein the pneumatic pump is disposed in an interior of the hollow tubule heat exchange array.

**2.** The heat exchanger of claim **1**, wherein the pneumatic pump provides a blood flow rate of from about 0.5 to about 2 L/minute.

**3.** The heat exchanger of claim **2**, wherein a heat exchanging surface area of the hollow tubule heat exchange array is optimal for heating the blood passing therethrough at a flow rate of from about 0.5 to about 2 L/minute to a blood temperature of up to 44 C for delivery to a patient body.

**4.** The heat exchanger of claim **1**, wherein the hollow tubule heat exchange array is fabricated of a suitable heat exchanging metal.

**5.** The heat exchanger of claim **4**, wherein the suitable heat exchanging metal is stainless steel.

**6.** A veno-venous perfusion-induced hyperthermia system, comprising:

a compact heat exchanger comprising:

8

a housing, a blood inlet ending at a distal-most surface of the compact heat exchanger and defining a longitudinal axis, a blood outlet, a heated fluid inlet, and a heated fluid outlet;

a hollow tubule heat exchange array disposed within an interior of the housing for heat exchange to and from blood passing through the compact heat exchanger; an inlet blood flow redirector disposed at a distal-most end of the blood inlet and configured to redirect a flow of the blood radially to the longitudinal axis across the compact heat exchanger distal-most surface and therefrom to the hollow tubule heat exchange array, the blood perfusing therefrom to the blood outlet; and

a pneumatic pump disposed substantially within the blood inlet and within a perimeter defined by the housing, further wherein the pneumatic pump is disposed in an interior of the hollow tubule heat exchange array;

a pneumatic console for cyclically supplying and withdrawing gas to and from the compact heat exchanger to operate the pneumatic pump and thereby pass the blood over the compact heat exchanger hollow tubule heat exchange array;

another pump for passing heated fluid through the compact heat exchanger hollow tubule heat exchange array;

and a dual lumen cannula for withdrawing the blood from a patient body, passing the blood through the compact heat exchanger, and returning the blood to the patient body.

**7.** The veno-venous perfusion-induced hyperthermia system of claim **6**, wherein the pneumatic console and pneumatic pump provide a blood flow rate of from about 0.5 to about 2 L/minute.

**8.** The veno-venous perfusion-induced hyperthermia system of claim **7**, wherein a heat exchanging surface area of the hollow tubule heat exchange array is optimal for heating the blood passing therethrough at a flow rate of from about 0.5 to about 2 L/minute to a blood temperature of up to 44 C for delivery to a patient body.

**9.** The veno-venous perfusion-induced hyperthermia system of claim **8**, wherein the hollow tubule heat exchange array is fabricated of a suitable heat exchanging metal.

**10.** The veno-venous perfusion-induced hyperthermia system of claim **9**, wherein the suitable heat exchanging metal is stainless steel.

**11.** A compact heat exchanger for veno-venous perfusion-induced hyperthermia, comprising:

a housing, a blood inlet ending at a distal-most surface of the compact heat exchanger and defining a longitudinal axis, a blood outlet, a heated fluid inlet, and a heated fluid outlet;

a hollow tubule heat exchange array disposed within an interior of the housing for heat exchange to and from blood passing through the compact heat exchanger;

an inlet blood flow redirector disposed at a distal-most end of the blood inlet, the inlet blood flow redirector including a conical tip extending into an interior lumen of the distal-most end of the blood inlet for evenly dispersing the blood radially to the longitudinal axis across the compact heat exchanger distal-most surface and therefrom to the hollow tubule heat exchange array, the blood perfusing therefrom to the blood outlet; and a pneumatic pump disposed substantially within the blood inlet and within a perimeter defined by the housing,

further wherein the pneumatic pump is disposed in an interior of the hollow tubule heat exchange array.

\* \* \* \* \*