

Development Of High Time-Resolution Laser Flash Equipment For Thermal Diffusivity Measurements Using Miniature-Size Specimens Irradiated Heavily In A Reactor

著者	SHIKAMA Tatsuo, NAMBA Chusei
journal or publication title	Science reports of the Research Institutes, Tohoku University. Ser. A, Physics, chemistry and metallurgy
volume	40
number	1
page range	125-129
year	1994-09-16
URL	http://hdl.handle.net/10097/28512

Development Of High Time-Resolution Laser Flash Equipment For Thermal Diffusivity Measurements Using Miniature-Size Specimens Irradiated Heavily In A Reactor*

Tatsuo SHIKAMA¹⁾ and Chusei NAMBA²⁾,

1) the Oarai Branch, Institute for Materials Research, Tohoku University, Oarai, 311-13 Japan

2) National Institute for Fusion Science, Furocho, Chikusa-ku, Nagoya, 464-01 Japan

(Received February 28, 1994)

For measurements of thermal diffusivity of miniature-size specimens heavily irradiated by neutrons, a new Q-switched laser-flash instrument was developed. In the present instrument the time resolution was improved to 0.1 ms by using a laser-pulse width of 25 ns. The realization of high time-resolution made it possible to measure the thermal diffusivity of thin specimens. It is expected that copper of 0.7mm thick, and SUS 304 of 0.1mm could be used for the measurements. In case of ATJ graphite, 0.5mm thick specimen could be used for the reliable measurement in the temperature range of 300-1300K.

KEYWORDS; Experimental Techniques, Thermophysical Properties.

1. Introduction

Thermal property changes due to heavy irradiation should be addressed extensively, for a reliable construction of plasma-facing components in a fusion reactor. Among thermal properties, thermal conductivity is one of the most important and is quite sensitive to radiation effects especially in ceramic materials.¹⁾ Also, we could obtain information concerning size and concentration of radiation induced lattice defects by measuring the thermal diffusivity.

In general, a large specimen is needed to measure the thermal conductivity, especially in so-called steady-state methods, where measuring procedures are complicated and time-consuming.²⁾ The development of the laser-flash method has improved the situations.³⁾ In development of highly thermally-conductive graphite in Japan⁴⁾, introduction of the standardized method of measuring their thermal conductivity with the laser-flash technique has been very effective to evaluate developed materials reliably.⁴⁾

Nowadays, the laser-flash technique is a well-established method for measuring the thermal diffusivity, α , with very simple procedures in a wide temperature range. The thermal conductivity, κ , is evaluated by multiplying measured thermal diffusivity, α with the specific heat, c_p , and the density, ρ , as described in the following.

$$k = \rho c_p \alpha \quad (1).$$

The specific heat above room temperature is thought to be insensitive to small variation of compositions of material constituents and to radiation effects. The density could be measured easily. However, even in the laser-flash technique, the use of medium-size specimens (10mm ϕ and 2-5mm thick) is necessary.

A heavy neutron irradiation is very expensive, thus the irradiation volume is usually limited. Furthermore, to reduce radioactivity of specimens, the specimens has to be as small as possible. Therefore, a miniature-specimen technique is essential for the study of heavy irradiation effects on fusion

reactor materials. In this study, we developed a new laser-flash instrument which enabled us to measure the thermal diffusivity of small specimens. This paper will describe features of the developed instrument and show some preliminary experimental results.

2. Development of Instrument and Experimental Results

Primary target of the present research is to develop a laser flash instrument using a standard miniature specimen, so-called TEM (Transmission Electron Microscopy)-disk for heavy neutron irradiations. Size of the specimen is 3mm ϕ and 0.15-0.5mm thick. In this study, we measured the thermal diffusivity of carbon-material and SUS 304, using specimens of different sizes by the developed instrument. The obtained results were also compared with those obtained by the conventional instrument. These measurements were carried out to clarify that the TEM-disk could be used for the measurement of thermal diffusivity by the present instrument.

One of the main restrictions concerning the geometrical size of the specimens is the finite time pulse effect⁵⁾. A half-width of its laser-pulse is 0.3-0.4ms, and a pulse profile observed through its measuring electric circuits has a time-delay of about 1ms as shown in Fig. 1(a). Here, we measured a time interval between a center of the observed energy deposition profile and the time zero, when a trigger signal which activated the laser-pulse was detected. Also, the half-width of the measured laser pulse was 0.85ms, being about twice of that of the actual laser-pulse. So, phenomena only slower than a few tens milliseconds could be detected reliably in this system.

The response speed will be determined by response speeds of an infra-red temperature monitor and subsequent electric circuits for handling signals from the temperature monitor, and also by various time delays at electric interfaces in the system. In this study, we tried to improve the response speed of the electric circuits. The through rate of operational amplifiers in an amplifier circuit was increased and a time constant of the noise filter was minimized. Also, the isolation amplifiers in the amplifier were removed.

*IMR, Report No. 1974

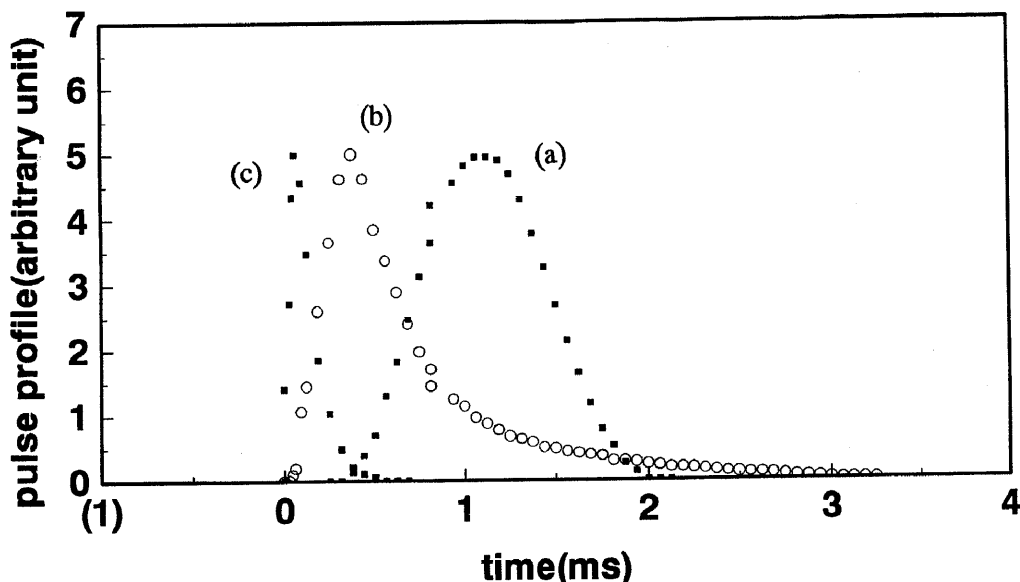


Figure 1 Measured time-profile of laser-pulse, (a)Conventional instrument, (b)Developed instrument with normal laser-pulse, (c) Q-switched laser-pulse.

0.35ms and its half width is 0.45ms, which would be about the same energy-deposition profile of the actual laser-pulse.

Even though we improved the response-time of the electric circuits, we still had a limit of time resolution of about 0.5ms which came from the energy deposition profile of the conventional laser-pulse. Here, we tried to improve it by using a Q-switched laser. The Q-switched laser whose half width of the energy profile was 25ns was adopted as shown in Fig. 2. A energy-deposition profile measured in the present

laser-flash instrument is also shown in Fig 1(c). The peak position was measured to be 0.05ms. So, in the present system, the $t_{1/2}$ value of about 0.25ms could be measured. From the following relation,

$$t_{1/2} = 0.139L^2/a \quad (2),$$

we can estimate the minimum thickness of the specimen, L. Using thermal diffusivities at room temperature, the following thickness was estimated; 0.5mm, 0.1mm, 0.7mm, and 0.6mm for ATJ-graphite, SUS 304, copper, and aluminum, respectively. These values are well near the range of thickness of specimens

irradiated in high flux reactors, up to high neutron doses.⁶⁾

Figure 3 shows measured temperature increase of highly conductive grassy carbon, GC-SS-J developed by Toyo Tanso Co Ltd., whose thickness was 0.535mm. The measured temperature increase had a half time, $t_{1/2}$, of 0.63ms, which was far out of the time-resolution of the conventional laser-flash instrument as described above.

Figure 4 shows data obtained on 0.482mm thick and 8mmφ SUS304 at room temperature. Obtained profile of temperature increase could be approximately described as a general equation (3) expressing temperature increase at the back surface,

$$\theta = \theta_m \{1 + 2 \sum (-1)^n \exp(-n^2 \pi^2 \alpha t / L^2)\} \quad (3).$$

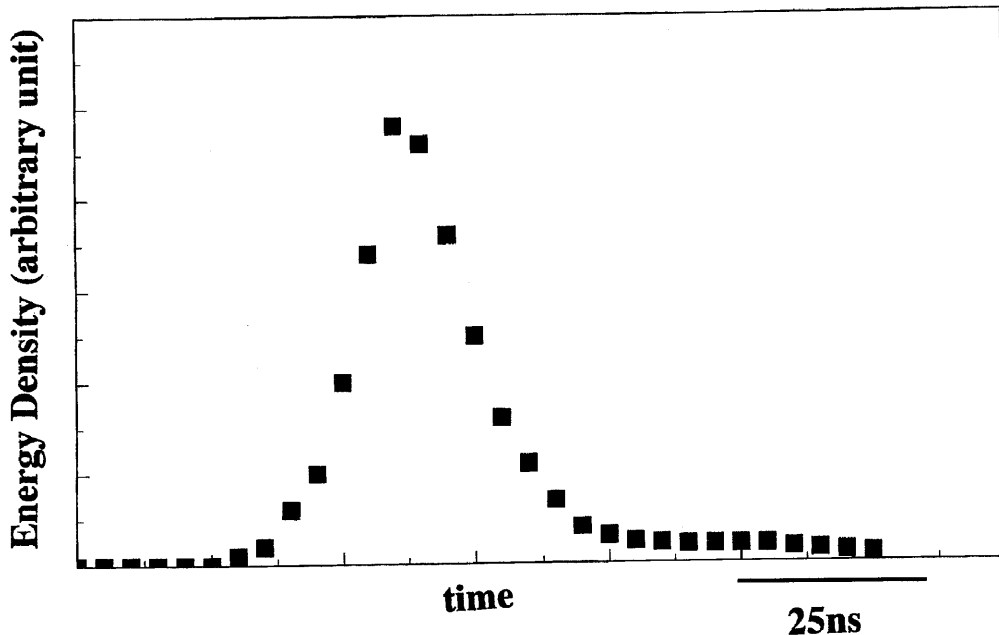


Figure 2 Energy profile of Q-switched laser-pulse.

Figure 1(b) shows the time-delay of the observed laser-pulse through the improved electric circuits. The time-delay was improved to be 0.53ms and the observed peak had a half-width of about 0.5ms, which was comparable with the half-width of actual laser pulse, about 0.4ms.

With increase of the response speed of electric circuits, the measured signals showed an exponential tailing. This tailing made a peak profile asymmetric and made a center of the energy deposition profile shift to a longer-time side. As one can see it clearly in Fig. 1(b), the peak observed in the conventional instrument revealed nearly symmetric, in contrast with that observed in the developed instrument. In the laser-flash technique, the initial response will be the most important and the measured tailing may not be important, although the tailing will affect details of obtained results. Then, we could examine the initial half part of observed peak profile. The observed peak position was

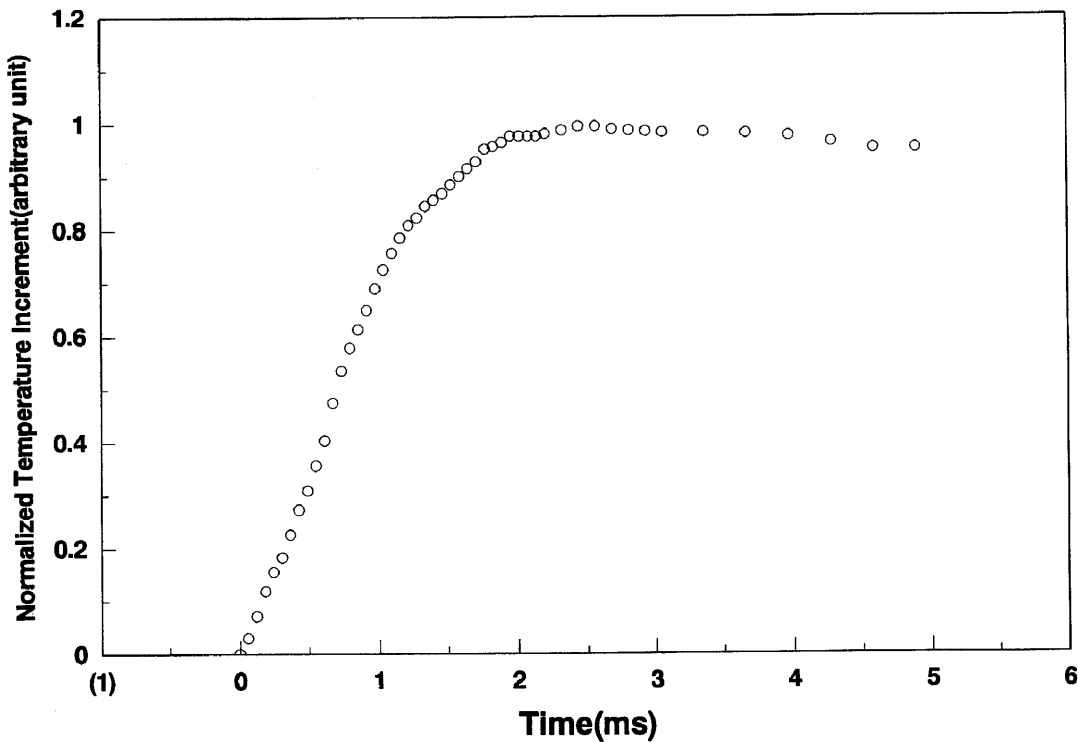


Figure 3 Measured temperature change on GC-SS-J of 0.535mm thick.

Here, θ and θ_m is a temperature increment and its maximum, respectively, and t is time duration after the radiation of laser flash. Here, $t_{1/2}$ is measured to 8.083ms and the obtained thermal diffusivity is about the same as that obtained by a conventional laser-flash instrument for this specimen, $0.0391\text{cm}^2/\text{s}$. The result also confirmed that we can use SUS304 specimen of about 0.9mm thick for the measurement even before the irradiation. Figure 5 shows measured values of thermal diffusivity of SUS 304 at room temperature as a function of specimen thickness. The diameter of the specimens was 3mm. Obtained values are well within + 10% of the recommended value in the range of

thickness of 0.5-1.5mm. These values were obtained from the measured results, using the so-called $t_{1/2}$ method³⁾.

The $t_{1/2}$ method has many advantages but at the same time it has some set-backs caused by deviation of the measuring system from the theoretical descriptions.⁷⁾ The thicker specimens showed the larger thermal diffusivity as shown in Fig. 5. This implies that the heat flow parallel to a specimen surface and the inhomogeneous spatial distribution of energy of laser-flash will be its cause. The present laser flash was found to have inhomogeneous energy deposition profile as a result of attempt to focus the laser beam to a limited area.

This attempt was done to increase spatial-density of the deposition laser energy, because the Q-switching initially caused decrease of the spatial energy density from about 6-10J/pulse to less than 1J/pulse. The specially designed specimen holder to shield the strong noise from the Q-switched laser would have also increased the heat flow parallel to the specimen surface.

More sophisticated analysis than the $t_{1/2}$ method will improve the situation, as the present system has a better time-resolution.⁸⁾

We preliminarily attempted to apply the so-called logarithmic slope method.^{8&9)} The equation (3) can be simplified to

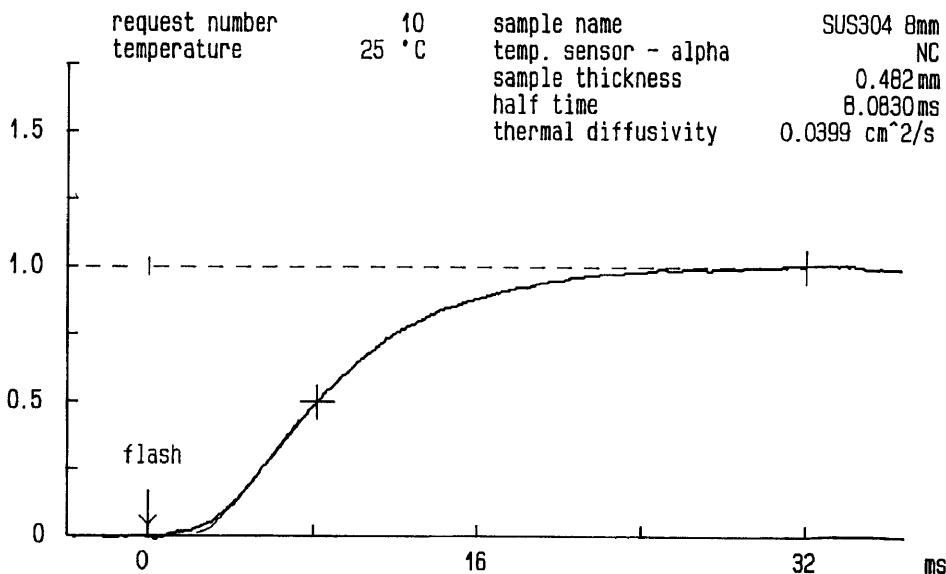


Figure 4 Obtained data on SUS304 of 8mmφ and 0.482mm thick.

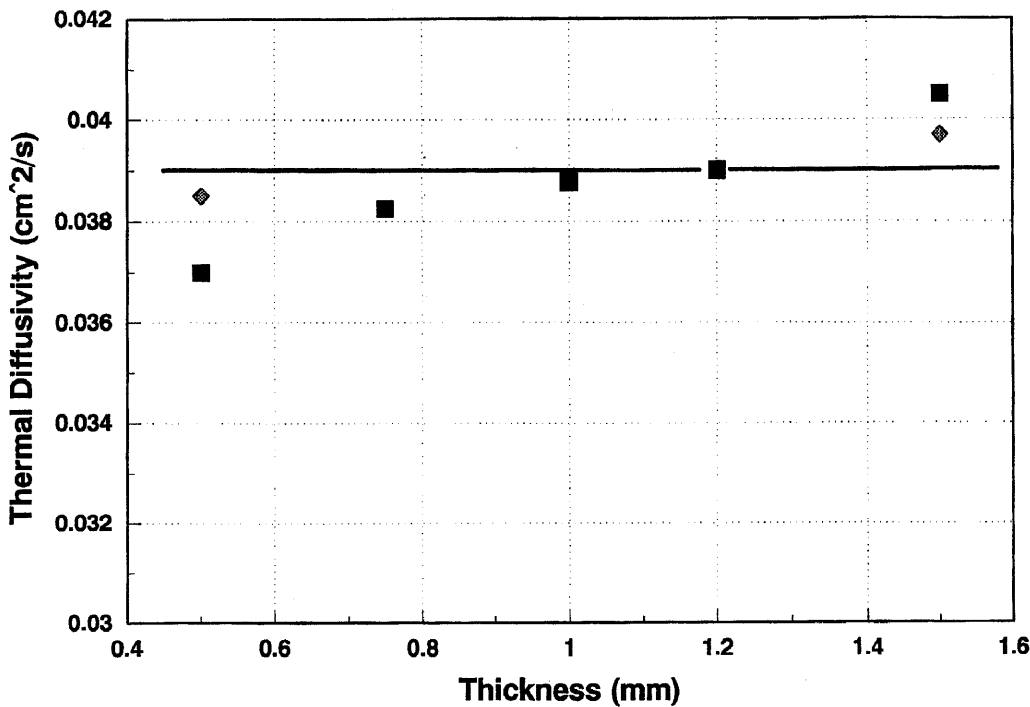


Figure 5 Thickness dependence of measured thermal diffusivity on 3mmf specimens, closed square; obtained by the $t_{1/2}$ method, closed diamond; obtained by the logarithmic slope method.

Temperature dependence of the thermal diffusivity of 1 mm thick SUS 304 was measured on the specimens of 3 and 6mmφ. The results are shown in Fig. 7, which also shows the results obtained on the 0.5mm thick specimen of 6mm. In general, the obtained results fit the recommended value well within + 10% scatters. The trend that the present measurements gave higher thermal diffusivity at elevated temperature may be also due to the heat flow parallel to the specimen surface especially enhanced at elevated temperatures. Results that the 0.5mm thick specimens showed better fitting also support this speculation.

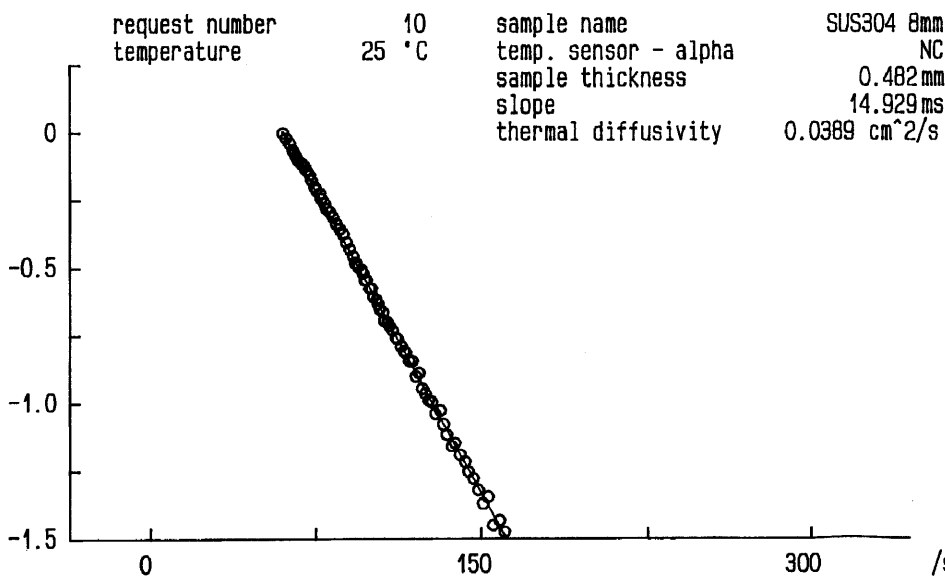


Figure 6 $\text{Log}(\theta t^{1/2})$ as a function of t^{-1} on data obtained with SUS304 of 8mmφ and 0.482mm thick.

In general, the developed instrument could measure the thermal diffusivity of very thin specimens in a wide temperature range. However, we have one serious setback. The present laser has a power of about 1J per one pulse, smaller compared with the value of about 6J of the conventional instrument as shown in Table 1. However, the 25ns pulse means the energy power of $4 \times 10^7 \text{W}$, far larger than the energy density of $2 \times 10^4 \text{W}$ of the conventional laser-flash instrument. The maximum temperature at the laser-irradiated surface could be estimated from the relation⁹⁾,

$$\theta_m^f = 3\theta_m \sqrt{t_{1/2}/\tau} \quad (5).$$

$$\log(\theta \sqrt{t}) = \log(2\theta_m L / \sqrt{\pi \alpha}) - L^2 / 4at \quad (4).$$

Here, logarithm of $\theta t^{1/2}$ will have a linear relationship with $-1/t$. Values of $\log(\theta t^{1/2})$ of SUS304 are plotted as a function of t^{-1} in Fig. 6, where one can see good linear-relationship. Estimated values of thermal diffusivity from the relation (4) are shown as closed diamonds in Fig. 5. Some improvement could be seen. However, further and detailed analyses must be needed to improve the present measurements.

Here, τ is a pulse width of laser. In a typical case of sapphire specimen of 0.3g, the observed temperature increase θ_m is 9.113K with a absorbed laser power of 2.7196J. When we assume $t_{1/2}$, the minimum time resolution, to be 0.25ms, the laser pulse of 25s will yield the value of 2734K for θ_m^f , which means that temperature of the irradiated surface will exceed the melting point.

Actually optical radiation of such a high density laser pulse caused some surface modification, especially on the relatively low-melting point materials. Also, due to the high power pulse, the temperatures involved lead to a non linear behavior of heat transfer, resultantly, the data

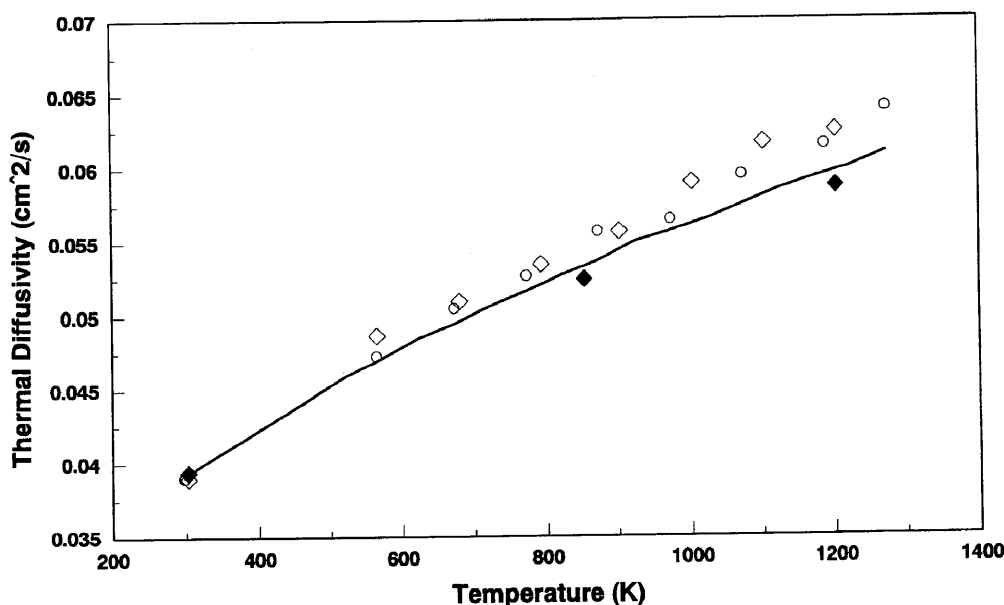


Figure 7 Temperature dependence of thermal diffusivity measured on specimens; open circle; 3mmf and 1mm thick, open diamond; 6mmf and 1mm thick closed diamond; 6mm and 0.5mm thick.

of the ATJ graphite, 0.3mm thick specimen could be used for the reliable measurement. The preliminary measurements confirmed that the developed instrument could measure the thermal diffusivity reliably in the temperature range of 300-1300K, with the miniature specimens.

However, serious surface modification took place due to the deposition of high energy density, 1×10^9 J/s, laser on measured specimen, which disturbed the measurements. Further optimization of the system will be needed.

Table 1. Specifications of conventional and developed laser-flash instrument

	Conventional	Developed
Width of laser pulse	300 - 400 μ s	25 ns
Laser energy per pulse	6 - 10 J	1 - 1.5 J
Diameter of homogeneous energy profile of laser pulse	10 mm	6 mm
Response time of measuring electrical circuits	about 1 ms	about 0.05 ms

reduction method such as $t_{1/2}$ method would not be used. The change of surface conditions sometimes caused serious scatter of measured values. Some carbon-based materials showed increase of scatter with increase of number of measurements. Improvement of sensitivity of a temperature-monitor and optimization of time-width and strength of the laser-pulse will be needed.

3. Conclusion

A new Q-switched laser-flash instrument was developed for the measurement of thermal diffusivity of specimen having miniature-size suitable for neutron irradiation. The present instrument realized the time resolution better than 0.1 ms with a laser-pulse of 25 ns wide. Realization of measurements with a high time-resolution made it possible to measure the thermal diffusivity with thin specimens. It is expected that copper of 0.4mm thick, and SUS 304 of less than 0.1mm could be used for the measurements. In case

- 1) M. Rohde and B. Schulz, STP-1125 (1992) p. 764, ASTM, Philadelphia.
- 2) J.E.Parrot and A.D. Stuckes, Thermal Conductivity of Solids,(Pion, London, 1975) p. 12.
- 3) W.J. Parker, R.J. Jenkins, C.P. Butler and G.L. Abbott, J. Appl. Phys. **32** (1961) 1679.
- 4) T. Yamashina edited, Overall Characterizations of Graphites as Fusion First Wall Material and Evaluation of the Stability Against Plasmas, Interim Report by Fusion First Wall Material Research Group, Nuclear Fusion Research Project, The Ministry of Education, Science and Culture, (Hokkaido University, 1989).
- 5) J.A.Cape and G.W.Lehman, J. Appl. Phys. **34** (1963) 1909.
- 6) A. Kohyama, FFTF CYCLE-11/MOTA-2A, LIST OF JAPANESE SPECIMENS, Research Group of Monbusho-DOE Collaboration in Fundamental Studies of Irradiation Effects in Fusion Materials Utilizing Fission Reactors (Unv. of Tokyo, 1992).
- 7) R.E. Taylor, Rev. Int. Htes. Temp. et. Refrait., **12** (1975) 141.
- 8) T. Baba, Research Report on Innovative Trends of Metrology, Nat. Res. Lab. Metrology of Jpn Report, Tsukuba, (Nat. Res. Lab. Metrology, 1985) p. 119.
- 9) Y. Takahashi, K. Yamamoto, and T. Oosato, Netsusokutei **15** (1988) 103.
- 9) T.Azumi, Doctor Thesis.