

DOI: 10.590/1809-2950/52921032014

Reliability of the measures inter and intra-evaluators with universal goniometer and fleximeter

Confiabilidade das medidas inter e intra-avaliadores com goniômetro universal e flexímetro

Fiabilidad de medidas inter e intra-evaluador con goniómetro universal y flexímetro

Victor Hugo de Oliveira Gouveia¹, Ana Gabriela de Figueiredo Araújo¹, Simone dos Santos Maciel², José Jamacy de Almeida Ferreira², Heleodório Honorato dos Santos²

ORIGINAL RESEARCH

ABSTRACT | The objective of this study was to analyze the reliability of the intra and inter-evaluators measures, with universal goniometer and fleximeter. Eighty university students (45 women and 35 men [average±SD]; age: 20.81±2.63 years, body mass: 68.36±16.31 kg, height: 1.69±0.09 m, BMI: 23.88±4.15 kg/m²) were submitted to goniometry and fleximetry of elbow and knee flexion, ankle dorsiflexion and wrist extension. It was calculated the intraclass correlation coefficient (ICC), considering a significance level of 5%. Overall, the results showed very strong (ICC: 0.91±0.99; P<0.001) and strong (0.75±0.90; P<0.001) correlations in all movements, intra and inter-evaluators. On inter-correlation instruments, there are strong coefficients on all measures (0.75±0.90; P<0.001) for the two instruments. In the studied movements, the evaluator experience did not influence the measurements and both the universal goniometer and the fleximeter showed high reliability.

Keywords | Movement; Measures; Students.

RESUMO | O objetivo deste estudo foi analisar a confiabilidade das medidas intra e inter-avaliadores, com goniômetro universal e flexímetro. Oitenta universitários (45 mulheres e 35 homens [média±DP]; idade: 20,81±2,63 anos, massa corporal: 68,36±16,31 kg, estatura: 1,69±0,09 m e IMC: 23,88±4,15 kg/m²), foram submetidos à goniometria e fleximetria da flexão do cotovelo e joelho, dorsiflexão e extensão de punho. Foi calculado o coeficiente de correlação intraclass (CCI), considerando-se um nível de significância de 5%. De modo geral, os resultados mostraram correlações

muito fortes (CCI: 0,91±0,99; P<0,001) e fortes (0,75±0,90; P<0,001), em todos os movimentos, tanto intra quanto inter-avaliadores. Na correlação inter-instrumentos, constatou-se fortes coeficientes em todas as medidas (0,75±0,90; P<0,001), para os dois instrumentos. Nos movimentos estudados, a experiência do avaliador não influenciou nas medições e tanto o goniômetro universal quanto o flexímetro mostraram alta confiabilidade.

Descritores | Movimento; Medidas; Estudantes.

RESUMEN | El objetivo de este estudio fue analizar la fiabilidad de las medidas inter y intra-evaluadores, con goniómetro universal y flexímetro. Ochenta estudiantes universitarios (45 mujeres y 35 hombres [media±DE]; edad: 20,81±2,63 años; masa corporal: 68,36±16,31 kg; estatura: 1,69±0,09m; IMC: 23,88±4,15 kg/m²) fueron sometidos a goniometría y fleximetry de la flexión del codo y extensión de la rodilla y la flexión dorsal de la muñeca. Se calculó el coeficiente de correlación intraclass (ICC), considerando un nivel de significación del 5%. En general, los resultados mostraron correlaciones muy fuertes (CCI: 0,91±0,99; P<0,001) y fuertes (0,75±0,90; P<0,001) en todos los movimientos, tanto inter como intra-evaluadores. En los instrumentos inter-correlación, encontramos fuertes coeficientes en todas las medidas (0,75±0,90; P<0,001) para ambos los instrumentos. En los movimientos estudiados, la experiencia del evaluador no influye en las mediciones y tanto el goniómetro como flexímetro mostró una alta fiabilidad.

Palabras clave | Movimiento; Medidas; Estudiantes.

Study conducted at the Kinesiology Laboratory at the Physical Therapy Department, Universidade Federal da Paraíba (UFPB) - João Pessoa (PB), Brazil.

¹Physical Therapy Department, UFPB - João Pessoa (PB), Brazil.

²Universidade Federal do Rio Grande do Norte (UFRN) - Natal (RN), Brazil.

Correspondence to: Heleodório Honorato dos Santos - Avenida Monsenhor Odilon Coutinho, 191/402 - Cabo Branco - CEP: 58045-120 - João Pessoa (PB), Brazil - E-mail: dorioufpb@gmail.com

Presentation: July 2013 - Accepted for publication: July 2014 - Financing source: none - Conflict of interests: nothing to declare - Approval at the Ethics Committee n. 436/2010 (CEP/HULW/UFPB).

INTRODUCTION

Measurement of the joint range of motion (ROM) is an important component in the physiotherapeutic evaluation since it not only identifies joint limitations but it also allows following quantitatively the efficiency of therapeutic interventions during rehabilitation¹⁻³.

The ROM measurement depends on three factors:

- instrument being used;
- examiner's skill and experience; and
- characteristics of the assessed subjects⁴⁻⁶.

It should be performed using reliable instruments, preferably noninvasive ones, which may be easily reproduced and should be based on scientific evidence⁷.

Reliability of measures demonstrates its consistence obtained through an instrument or by an examiner in the same evaluation conditions. Intra-evaluator reliability is the consistence of measures performed in the same evaluation conditions in two different moments. On the other hand, the inter-evaluator reliability is associated with consistence of the measures performed by two or more different evaluators⁸.

Among these instruments, both the universal goniometer (UG)^{1,2,8-11} and the fleximeter (electromagnetic goniometer)¹² have showed reliability indices classified from "regular" to "excellent" depending on the joint and movement being analyzed.

Although literature shows that variations between the second and seventh in the ROM are acceptable considering the tested joint¹³, and there has already been evidence of the reliability of UG and fleximeter alone^{2,10}, studies in general restrict the number of instruments when two or more joints^{11,14} are being compared. Or they limit the number of movements to be analyzed when two or more instruments are being correlated^{1,2,8,9,12,15}.

Thus, the hypotheses of this study are:

- the measure would present lower reliability when done by one not very experienced evaluator;
- manual goniometry is an evaluator-dependent measure, therefore it would have lower reliability than fleximetry; and
- there would be a strong reproducibility of inter-instrument measures.

Thus, this study aimed at analyzing the reliability of intra and inter-evaluators measures for elbow and knee flexion movements, ankle dorsiflexion and fist extension, which were performed with the UG and fleximeter.

METHODOLOGY

Sample

In this study, the sample was chosen by convenience and 80 healthy subjects from both sexes were investigated (45 women and 35 men; 20.81±2.63 years old, 68.36±16.31 kg, 1.69±0.09 m and BMI: 23.88±4.15 kg/m²). They had no musculoskeletal alterations, pain or discomfort in the higher and lower limbs or any other disease or dysfunction that could compromise the elbow, fist, knee and ankle ROM.

The study was approved by the Research Ethics Committee in Human Beings of the University Hospital Lauro Wanderley (UFPB), according to protocol CEP/HULW number 436/2010, with the Certificate of Presentation for Ethical Appreciation (CAAE) number 0361.0.126.000-10. Subjects who agreed to participate signed the free informed consent (FIC), according to resolution 196/96 of the Brazilian National Health Counsel (NHC).

Procedures

The following were used as instruments: UG (Carci, Brazil) and fleximeter (Instituto Code de Pesquisa, Brazil). In the UG, the part set apart to read the angles was covered with a poster paper in order to not influence the subsequent measures (Figures 1A, 1C, 1E and 1G), while in the fleximeter, reading was always direct since the evaluator could not have an influence on the results.

The study included two evaluators: one deemed experienced (three years of practice) and another considered unexperienced (only one month of practice), with low familiarization with the goniometer and fleximeter.

Each measure was performed three times in the dominant limb, in only one session, by calculating their mean. Subjects were oriented to wear light clothes in order that the ROMs were not limited, and the evaluator demonstrated all movements before the maximum active ROM measuring. One of the evaluators did measurement, while the second one performed its reading and recording in order to avoid induction of results.

The order to measure movements (elbow and knee flexion; ankle dorsiflexion and fist extension) and use instruments (UG and fleximeter) was randomly performed (<http://www.lee.dante.br/>). After each measure, the subject was requested to return to his/her initial position keeping a 1-minute interval between the three

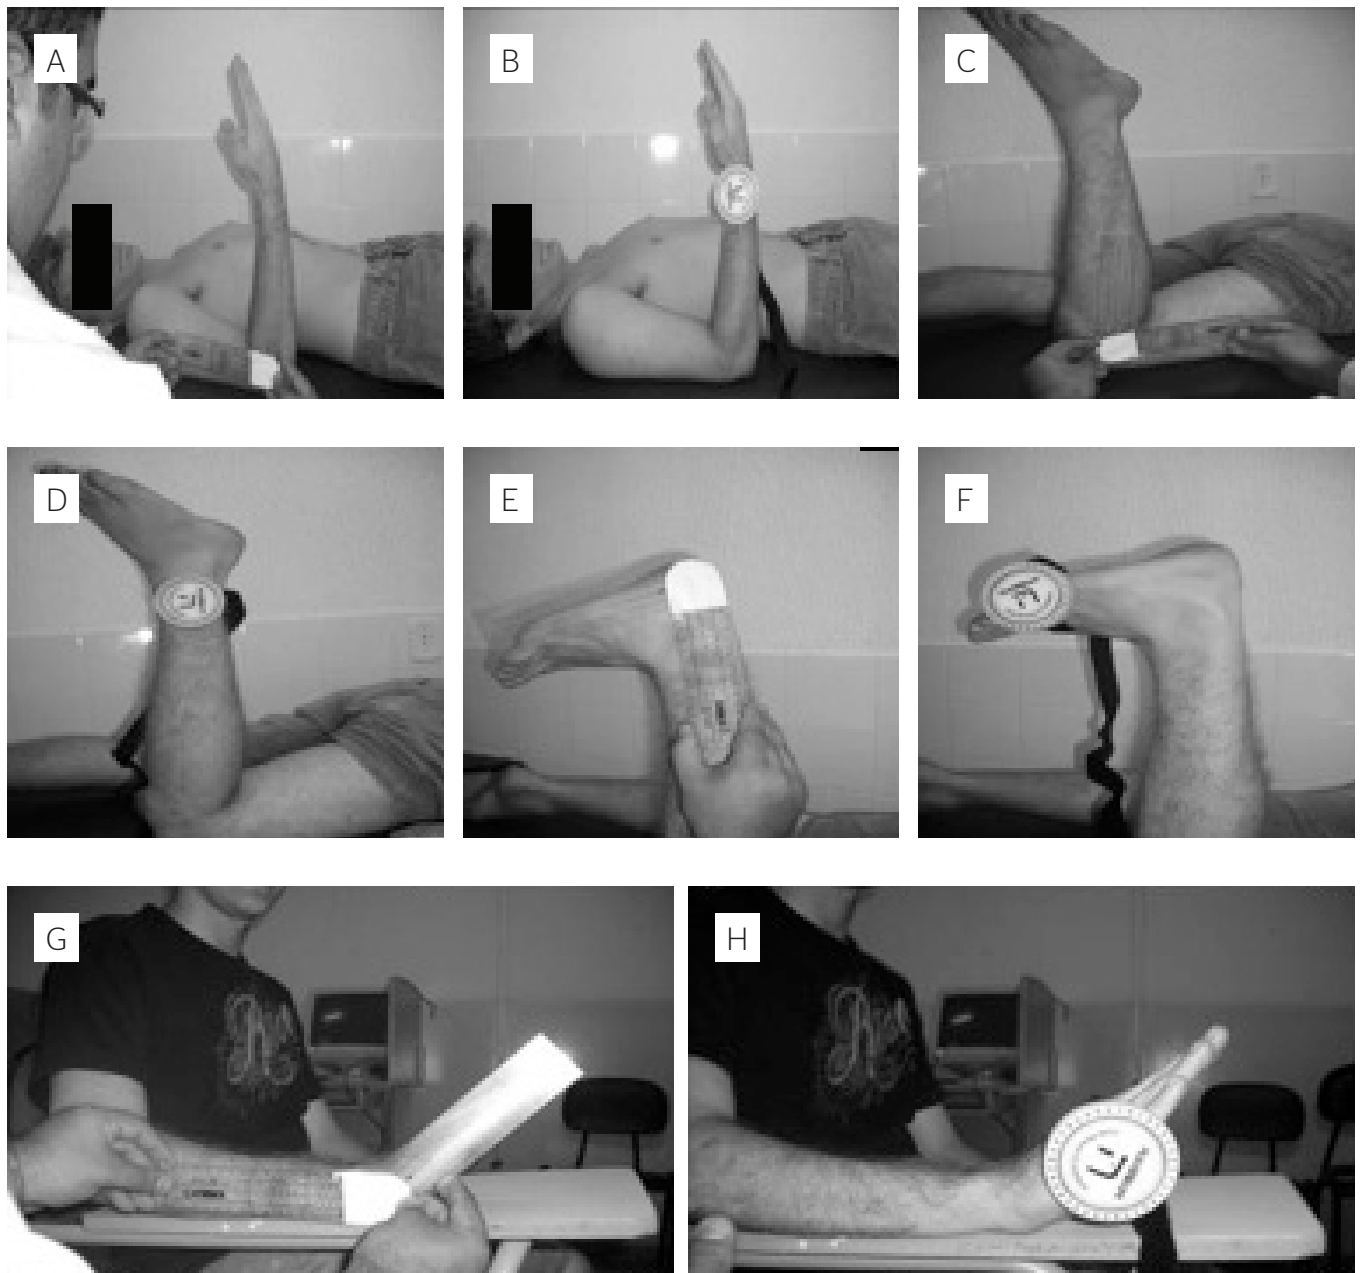


Figure 1. Measure of the movement of elbow (A and B), knee (C and D), ankle (E and F), and fist (G and H) with the universal goniometer and fleximeter, respectively

measures, for each movement (intra-evaluator), and a 5-minute one between evaluators (inter-evaluators) and instruments (inter-instruments).

In order to identify dominance, the subject was questioned on what leg he/she uses to kick a ball and with what hand he/she writes, with the purpose of confirming the dominance of the lower limb (LL)¹⁶ and higher limb (HL)^{17,18} respectively.

When measuring elbow flexion (Figure 1A and 1B), the subject was positioned in the supine position with the HL in supination and extended beside the body with something to support him/her in the distal portion

of the arm dorsal face in order to check a possible elbow hyperextension¹⁹.

Measures of knee flexion (Figure 1C and 1D) and ankle dorsiflexion (Figure 1E and 1F) were performed in the prone position. In the first movement, the subject was positioned with his/her LL extended with something to support it in the distal region of the femur in order to check the existence of a knee hyperextension. For the dorsiflexion, the same position was kept with the addition of flexion (90°) of the knee that was going to be evaluated¹⁹.

For measuring the fist extension (Figure 1G and 1H), subject sat in a chair with his/her shoulder adducted,

inflected elbow ($\cong 90^\circ$), forearm at pronation and fist in neutral position supported on a board¹⁹.

In all measures done with the fleximeter, the same positions of goniometry were adopted. The fleximeter was positioned in the lateral face of the fist (radius styloid process), of the ankle (lateral malleolus), of the foot (head of the fifth metatarsus) and medial face of the hand (fifth metacarpus) to measure elbow and knee flexion, ankle dorsiflexion and fist extension respectively²⁰.

Data analysis

Statistical procedures were carried out in the software Statistical Package for the Social Sciences (SPSS – 15.0). Initially, data normality (Kolmogorov-Smirnov's test) and variance homogeneity (Levene's test) were observed followed by the intraclass correlation coefficient (ICC – reproducibility) in the comparison of ROMs of all intra and inter-evaluators (Av1 X Av2) joints (knee, ankle, elbow and fist) done with UG and fleximeter, using a 5% level of significance.

For the ICC analysis, the following classification was considered: null=0.00; weak=0.01 to 0.30; regular=0.31 to 0.60; strong=0.61 to 0.90; very strong=0.91 to 0.99; and complete=1.00²¹.

RESULTS

ICC tests between the three measures done with UG for each evaluator demonstrated that there was a very strong correlation ($0.91 \leq 0.99$; $P < 0.001$) in all assessed movements, both for the evaluator 1 and evaluator 2, with the exception of the knee flexion movement performed by evaluator 2 (0.83; $P < 0.001$) that had a strong correlation (Table 1).

With regard to comparisons between the three measures of ROMs performed using the fleximeter (Table 2), results also showed a very strong ICC ($0.91 \leq 0.99$; $P < 0.001$) in all analyzed movements, both for evaluator 1 and evaluator 2.

As to comparisons of inter-evaluators measures (Table 3), it was also seen a very strong ICC for elbow and knee flexion movements (0.95 and 0.93; $P < 0.001$, respectively) done using UG, and for movements of knee flexion and fist extension (0.92 and 0.93; $P < 0.001$, respectively) with the fleximeter. All the other results, regardless of the instrument used (UG or fleximeter), achieved a strong ICC ($0.8 \leq 0.9$; $P < 0.001$).

The results of ICC between instruments (UG x fleximeter) found strong correlations (0.76 to 0.90; $P < 0.001$) for all the analyzed movements (Table 4), both for evaluators 1 and 2.

Table 1. Values of the intraclass correlation coefficient (ICC), intra-evaluators, of elbow and knee flexion goniometry, fist dorsiflexion and extension

Movements	Evaluator 1		Evaluator 2	
	ICC (r)	P-value	ICC (r)	P-value
Elbow flexion	0.9823	<0.001	0.9792	<0.001
Knee flexion	0.9836	<0.001	0.8282	<0.001
Dorsiflexion	0.9522	<0.001	0.9508	<0.001
Fist extension	0.9740	<0.001	0.9622	<0.001

Table 2. Values of the intraclass correlation coefficient (ICC), intra-evaluators, of elbow and knee flexion fleximetry, fist dorsiflexion and extension

Movements	Evaluator 1		Evaluator 2	
	ICC (r)	P-value	ICC (r)	P-value
Elbow flexion	0.9819	<0.001	0.9473	<0.001
Knee flexion	0.9776	<0.001	0.9672	<0.001
Dorsiflexion	0.9560	<0.001	0.9428	<0.001
Fist extension	0.9898	<0.001	0.9777	<0.001

Table 3. Values of the intraclass correlation coefficient (ICC), inter-evaluators, of elbow and knee flexion goniometry and fleximetry, fist dorsiflexion and extension

Movements	Universal goniometer		Fleximeter	
	ICC (r)	P-value	ICC (r)	P-value
Elbow flexion	0.9496	<0.001	0.8871	<0.001
Knee flexion	0.9342	<0.001	0.9158	<0.001
Dorsiflexion	0.8825	<0.001	0.8545	<0.001
Fist extension	0.8599	<0.001	0.9341	<0.001

Table 4. Values of the intraclass correlation coefficient (ICC), inter-instruments (universal goniometer x fleximeter), of elbow and knee flexion, fist dorsiflexion and extension measures

Movements	Evaluator 1		Evaluator 2	
	ICC (r)	P-value	ICC (r)	P-value
Elbow flexion	0.7651	<0.001	0.7550	<0.001
Knee flexion	0.7971	<0.001	0.8034	<0.001
Dorsiflexion	0.8287	<0.001	0.7890	<0.001
Fist extension	0.9012	<0.001	0.8506	<0.001

DISCUSSION

In the physiotherapeutic practice, a measure cannot be deemed significant if it is not valid and reliable³. During a physiotherapeutic treatment, the patient usually is assessed more than once to check his/her clinical evolution and sometimes even by different physical therapists. Therefore, reliability of the examiner and of the ROM evaluation instrument is very important to allow the consistence of measures during the clinical evolution and in scientific studies^{3,22}. According to Bonagamba *et al.*³ and Côté *et al.*²³, the most proper statistical test for the reliability analysis is ICC because it analyses data association in a certain time interval.

When comparing data from the present study with literature, it was seen that the ICC indices generally were similar or even higher than in other studies²⁴⁻²⁶, both concerning evaluators and instruments, in most studied movements.

Under *et al.* study²⁷ analyzed the knee flexion of 52 subjects who had undergone total arthroplasty, in three different positions (prone, supine and sat), and they also observed very strong correlations (ICC≥0.91) between inter and intra-evaluators positions.

Similarly to our results, Lustosa *et al.*⁹ and Lessen²⁶ achieved high reliability rates in the measures for both instruments (UG and fleximeter) and between evaluators^{9,28} (0.87 and 0.99) when there was an analysis of knee and elbow flexion movements, therefore despite UG be an instrument of measure considered evaluator-dependent, it also reached similar correlation levels to the fleximeter.

Piriyaprasarth and Morris²⁹, in a systematic revision article, stated that ROM measures are reliable using both the UG and the electromagnetic goniometer (fleximeter), which is in agreement with the findings of this study.

On the other hand, Sacco *et al.*¹⁰ found moderate to weak correlations for the knee and ankle joints, respectively. However, it is believed that these lower correlation levels, if compared to our study, happen because the researchers used a different methodology from the present study.

An investigation developed by Chaves *et al.*² including 106 healthy children, also correlating UG and fleximeter, found contrarily to the results from this study, regular and weak correlations. Nevertheless, although they have used the same instruments, they assessed different movements (cervical spine) that may justify the

results, since some instruments present higher or lower ICC depending on the assessed movement.

With regard to the measure of active ROM of ankle dorsiflexion, Venturini *et al.*⁸, assessing 28 healthy and young (18 to 30 years old) subjects, found a very strong ICC, using both the UG (0.91 and 0.97) and the inclinometer (0.91 and 0.83). In the measures between the two evaluators, the ICC was moderate for the UG (0.72) and strong for the inclinometer (0.83).

When Konor *et al.*³⁰ were analyzing ROM of the elbow dorsiflexion in closed kinetic chain (CKC) of 20 healthy young subjects, through three different instruments (UG, digital inclinometer and metrical tape), with unexperienced evaluators (without previous experience), they also found a very strong ICC, both inter-evaluators (0.85) and inter-instruments (0.99) on both sides (left and right).

On the other hand, when Santos *et al.*³¹ analyzed the dorsiflexion movement in 42 subjects, using a similar methodology to the present study, they found moderate correlations both for inter-evaluators (ICC=0.72) and intra-evaluators (ICC=0.55) measures.

Differently from the results of the present study, Van Trijffel *et al.*³², using UG, reported lower reliability of the LL ROM measures compared to the HL. They stated that it was harder to find bone marks accurately, making it more difficult to get the perfect alignment of the goniometer. However, some studies using UG showed high reliability for the knee flexion (Currier *et al.*³³; ICC=0.87) and ankle dorsiflexion (Diamond *et al.*³⁴; ICC=0.74 to 0.87).

As to the movement of fist extension, only the study performed by LaStayo and Wheeler²⁵ was found, which assessed the UG in three measurement ROM types and, similarly to our results, it was also seen strong reliability indices (ICC=0.80), both for intra and inter-tests.

Another study carried out by Carter *et al.*³⁵ to analyze the ROM of fist flexion and extension, using UG by two different evaluators, also found similar results to the present study, with an ICC between 0.80 (very strong) and 1.00 (complete), both intra and inter-evaluators.

Like other authors^{1,25,31,36}, the present study performed consecutive measures in only one session for all the movements. The first examiner did three consecutive measures, and the same procedure was repeated by the second examiner with the subject in the same position, for each studied movement.

The fact that other studies^{2,8,9,12,24,37,38} used intervals from two to seven days between the first and second measures, with the aim of eliminating effects of viscoelastic adaptation (warming, extensibility, etc.) of the soft

tissues, possibly produced by movement repetition, may be indicated as a limitation of the study. However, like other authors^{1,25,31,36}, the present study performed consecutive measures, in only session, for all movements, which presented high reliability among them.

CONCLUSIONS

Results from this study show that: evaluator's experience did not influence ROM measures of the joints studied; the instruments used (UG and fleximeter) generally present high reliability when performed in the same session of measurements; and use of fleximeter in the physiotherapeutic clinic may be expanded without damage to reliability of measures.

REFERENCES

1. Fernández MG, Escobar JCZ. Fiabilidad y correlación en la evaluación de la movilidad de rodilla mediante goniómetro e inclinómetro. *Fisioter.* 2012;34(2):73-8.
2. Chaves TC, Nagamine HM, Belli JFC, Hannai MCT, Bevilaqua-Grossi D, Oliveira AS. Confiabilidade da fleximetria e goniometria na avaliação da amplitude de movimento cervical em crianças. *Rev Bras Fisioter.* 2008;12(4):283-9.
3. Bonagamba GH, Coelho DM, Oliveira AS. Confiabilidade interavaliadores e intra-avaliador do escoliômetro. *Rev Bras Fisioter.* 2010;14(5):432-7.
4. Dvir Z. *Isocinético: avaliações musculares, interpretações e aplicações clínicas.* São Paulo: Manole; 2002.
5. Georgeu GA, Mayfield S, Logan AM. Lateral digital photography with computer-aided goniometry versus standard goniometry for recording finger joint angles. *J Hand Surg Br.* 2002;27(2):184-6.
6. Tedeschi MA. Goniometria: sua prática e controvérsias. *Fisioter Mov.* 2003;16(2):35-40.
7. Cipriano JJ. *Manual fotográfico de testes ortopédicos e neurológicos.* 4ª ed. São Paulo: Manole; 2005.
8. Venturni C, Ituassú. NT, Teixeira LM, Deus CVO. Confiabilidade de dois métodos de avaliação da amplitude de movimento ativa de dorsiflexão do tornozelo em indivíduos saudáveis. *Acta Fisiatr.* 2006;13(1):41-5.
9. Lustosa LP, Silva CWA, Brito JP, Cordeiro RV, Lemos MS. Goniometria e fleximetria: um estudo de confiabilidade e comparação das medidas nas articulações do cotovelo e joelho. *E-Scient.* 2008;1(1):1-9.
10. Sacco ICN, Alibert S, Queiroz BWC, Pripas D, Kieling I, Kimura AA, *et al.* Confiabilidade da fotogrametria em relação a goniometria para avaliação postural de membros inferiores. *Rev Bras Fisioter.* 2007;11(5):411-7.
11. Carvalho RMF, Mazzer N, Barbieri CH. Análise da confiabilidade e reprodutibilidade da goniometria em relação à fotogrametria na mão. *Acta Ortop Bras.* 2012;20(3):139-49.

12. Florêncio LL, Pereira PA, Silva ERT, Pegoretti KS, Gonçalves MC, Bevilacqua-Grossi, D. Concordância e confiabilidade de dois métodos não-invasivos para a avaliação da amplitude de movimento cervical em adultos jovens. *Rev Bras Fisioter.* 2010;14(2):175-81.
13. Santos CM, Ferreira G, Malacco PL, Sabino GS, Moraes GFS, Felício DC. Confiabilidade intra e interexaminadores e erro da medição no uso do goniômetro e inclinômetro digital. *Rev Bras Med Esporte.* 2012;18(1):38-41.
14. Gerales AAR, Albuquerque RB, Soares RM, Carvalho J, Farinatti PTV. Correlação entre flexibilidade das articulações glenoumerais e coxofemorais e o desempenho funcional de idosas fisicamente ativas. *Rev Bras Fisioter.* 2008;12(4):274-82.
15. Balogh I, Ohlsson K, Nordander C, Skerfving S, Hansson, GA. Precision of measurements of physical workload during standardized manual handling part III: Goniometry of the wrists. *J Electromyogr Kinesiol.* 2009;19(5):1005-12.
16. Teixeira CS, Silva RP, Mota CB. Membro dominante x não dominante durante o chute com o dorso do pé: análise qualitativa com um indivíduo sinistro. *Rev Digital.* Buenos Aires, 2006;95.
17. Hardych C, Petrinovich LF. Left-handedness. *Psychol Bul.* 1977;84(3):385-404.
18. Hervé PY, Crivello F, Perchey G, Mazoyer B, Tzourio-Mazoyer. Handedness and cerebral anatomical asymmetries in young adult males. *Neuroimage.* 2006;29(4):1066-79.
19. Raimundo AKS, Moreira D, Santana LA. Manual fotográfico de goniometria e fleximetria. Brasília: Thesaurus; 2007.
20. Manual de fleximetria: teste de flexibilidade. 2000. [Citado em 28 de março 2011]. Disponível em: <www.institutocode.com> Acesso em: 28/03/2011.
21. Albuquerque PL, Quirino MAB, Santos HH, Alves SB. Interferência da prática de atividade física habitual na postura de jovens. *Rev Ter Man.* 2010;8(37):198-203.
22. Bennell K, Talbot R, Wajswelner H, Techovanich W, Kelly DH, Hall AJ. Intra-rater and inter-rater reliability of a weight-bearing lunge measure of ankle dorsiflexion. *Aust J Physiother.* 1998;44(3):175-80.
23. Côté P, Kreitz BG, Cassidy JD, Dzus AK, Martel J. A study of the diagnostic accuracy and reliability of the Scoliometer and Adam's forward bend test. *Spine.* 1998;23(7):796-802.
24. Boldrini CM, Tomé F, Moesch J, Mallmann JS, Oliveira LU, Roberti NF, et al. Avaliação da confiabilidade intra e interavaliadores e intertécnicas para três instrumentos que mensuram a extensibilidade dos músculos isquiotibiais. *Fit Perf J.* 2009;8(5):342-8.
25. LaStayo PC, Wheeler DL. Reliability of passive wrist flexion and extension goniometric measurements: a multicenter study. *Phys Ther.* 1994;74(2):162-74.
26. Lenssen AF, Van Dam EM, Crijns YH, Verhey M, Geesink RJ, Van Den Brandt PA, et al. Reproducibility of goniometric measurement of the knee in the in-hospital phase following total knee arthroplasty. *BMC Musculoskelet Disord.* 2007;8(83):1-7.
27. Unver B, Karatosun V, Bakirhan S. Reliability of goniometric measurements of flexion in total knee arthroplasty patients: with special reference to the body position. *J Phys Ther Sci.* 2009;21(3):257-62.
28. Gajdosik RL. Passive extensibility of skeletal muscle: review of the literature with clinical implications. *Clin Biomech.* 2001;16(2):87-101.
29. Piriyaprasarth P, Morris ME. Psychometric properties of measurement tools for quantifying knee joint position and movement: a systematic review. *Knee.* 2007;14(1):2-8.
30. Konor MM, Morton S, Eckerson JM, Grindstaff TL. Reliability of three measures of ankle dorsiflexion range of motion. *Int J Sports Phys Ther.* 2012;7(3):279-87.
31. Santos WV, Andrade P, Souza GAB, Ricci NA, Gazzola JM, Ganança FF, et al. Confiabilidade interavaliadores da avaliação goniométrica em vestibulopatas com queixa de tontura. *Fisioter Mov.* 2007;20(2):91-8.
32. Van Trijffel E, Van de Pol RJ, Oostendorp RA, Lucas C. Inter-rater reliability for measurement of passive physiological movements in lower extremity joints is generally low: a systematic review. *J Physiother.* 2010;56(4):223-35.
33. Currier LL, Froehlich PJ, Carow SD, McAndrew RK, Cliborne AV, Boyles RE, et al. Development of a clinical prediction rule to identify patients with knee pain and clinical evidence of knee osteoarthritis who demonstrate a favorable short-term response to hip mobilization. *Phys Ther.* 2007;87(9):1106-19.
34. Diamond JE, Mueller MJ, Delitto A, Sinacore DR. Reliability of a diabetic foot evaluation. *Phys Ther.* 1989;69(10):797-802.
35. Carter TI, Pansy B, Wolff AL, Hillstrom HJ, Backus SI, Lenhoff M, Wolfe SW. Accuracy and reliability of three different techniques for manual goniometry for wrist motion: a cadaveric study. *J Hand Surg Am.* 2009;34(8):1422-8.
36. Paulis WD, Horemans HL, Brouwer BS, Stam HJ. Excellent test-retest and inter-rater reliability for Tardieu Scale measurements with inertial sensors in elbow flexors of stroke patients. *Gait Posture.* 2011;33(2):185-9.
37. Braz RG, Goes FPDC, Carvalho GA. Confiabilidade e validade de medidas angulares por meio do software para avaliação postural. *Fisioter Mov.* 2008;21(3):117-26.
38. De Kraker M, Selles RW, Schreuders TAR, Stam HJ, Hovius SER. Palmar abduction: reliability of 6 measurement methods in healthy adults. *J Hand Surg Am.* 2009;34(3):523-30.