



This is a repository copy of *A critical review of the assessment of medical gloves*.

White Rose Research Online URL for this paper:
<http://eprints.whiterose.ac.uk/157053/>

Version: Accepted Version

Article:

Preece, D., Lewis, R. orcid.org/0000-0002-4300-0540 and Carre, M.J. (2020) A critical review of the assessment of medical gloves. *Tribology: Materials, Surfaces and Interfaces*. ISSN 1751-5831

<https://doi.org/10.1080/17515831.2020.1730619>

This is an Accepted Manuscript of an article published by Taylor & Francis in *Tribology: Materials, Surfaces and Interfaces* on 23 Feb 2020, available online:
<http://www.tandfonline.com/10.1080/17515831.2020.1730619>.

Reuse

Items deposited in White Rose Research Online are protected by copyright, with all rights reserved unless indicated otherwise. They may be downloaded and/or printed for private study, or other acts as permitted by national copyright laws. The publisher or other rights holders may allow further reproduction and re-use of the full text version. This is indicated by the licence information on the White Rose Research Online record for the item.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.



eprints@whiterose.ac.uk
<https://eprints.whiterose.ac.uk/>

A Critical Review of the Assessment of Medical Gloves

D. Preece^{a*}, R. Lewis and M. J. Carré

^a*Department of Mechanical Engineering, University of Sheffield, Sheffield, United Kingdom;*

*dpreece1@sheffield.ac.uk

Abstract

Medical protective gloves must be assessed to adequate standards before becoming available for commercial use. Strength, integrity and contamination are assessed at the manufacturing stage. However, concerns are raised over the standardisation of the testing; should more be done to assess how gloves affect the performance? Over the years, studies have demonstrated how the design of gloves have reduced tactile sensitivity in medical staff, ultimately leading to poor patient care through missed information. Studies have also demonstrated that a loss of grip control and dexterity through glove use are detrimental to medical tasks. However, it remains relatively unexplored as to how wearing medical gloves affects the users and the patients. Gaps in research have been identified around the frictional and grip properties of gloves. Linking the key performance parameters to the manufacturing processes, which affect material properties, will provide more insight into the behaviour of medical gloves and how to properly assess materials.

Keywords: Gloves, Tactile Sensitivity, Dexterity, Perception, Friction, Grip

Funding

This research was fully funded by the Engineering and Physical Science Research Council (EPSRC) through the integrated Tribology Centre for Doctoral Training (iT-CDT) and Synthomer (UK) Ltd.

1. Introduction

Clinical staff, such as doctors and surgeons are required to don medical gloves to protect themselves and patients from contamination. Two types of medical gloves exist. Examination gloves; worn for routine medical examinations and minor procedures and surgical gloves; worn for surgeries by surgical staff. The safety performance of these gloves is relatively undisputed. Their effects on hand performance, however, should not be overlooked. Medical gloves have been investigated for possible reduction in performance capabilities [1]. However, it has yet to be determined as to how gloves should be assessed for quality of purpose. Does placing a membrane over the hand have such an effect on performance that a medical professional cannot perform tasks correctly? This review aims to bring together the knowledge available on how medical glove performance has been assessed within the literature. Firstly, focusing on the varied materials of gloves before discussing how gloves have been assessed in previous studies. The advantages and limitations of such assessments will be discussed, and suggestions will be made on improvements if and where applicable. As the review is focusing on real-world applications, studies focusing on sensitivity, dexterity, friction, grip and performance perception will be evaluated. These studies consider medical glove materials and measuring differences between them or the bare skin condition and have been identified through searching scientific journal databases, specifically for medical examination and surgical glove assessments along with more specific key terms: 'dexterity', 'sensitivity' 'grip' and 'friction'. Databases which included institutional access were used, including PubMed, ScienceDirect, PLOS, JSTOR and the University of Sheffield library database, to bring together research from across 38 journals.

1.1 Glove Materials

The properties of gloves are dependent upon the raw manufacturing materials, manufacturing processes followed, and the chemical treatment gloves receive. Natural rubbers are commonly used, the most prominent being natural rubber latex (NRL), a substance found in the bark of *Hevea* trees [2]. By nature, NRL is a highly deformable elastomer, allowing easy conformation to the shape of the hand [3]. The

Center for Disease Control (CDC) estimates that up to 6% of the worldwide population has a latex allergy [4]. Furthermore, the increasing incidence in NRL allergies means that alternative glove materials must be used where appropriate. Other glove materials include; nitrile (XNBR), polyvinyl chloride (PVC) and polychloroprene [5,6]. The most common alternative material to NRL is nitrile (XNBR), synthetically created using a copolymer of acrylonitrile and butadiene. However, the elastic loading response of XNBR means that the conformability to the hand is perceived to be inferior than that of NRL. The material properties of XNBR gloves is an issue for some, as they report it hinders their ability to carry out tasks [6,7].

Until 2000, powder (e.g. starch) was used to coat the interior surface of gloves, allowing a reduced friction coefficient for donning. However, due to the rise in the incidents of latex allergies, there have been concerns over the proteins in NRL being made airborne upon the removal of the glove [8]. Consequently, in 2010 the Health and Safety Executive (in the UK) released guidelines stating that NRL gloves must be free of powder, prompting the NHS to stop purchasing powdered NRL gloves [9]. As an alternative to powder, chlorination treatment has become a popular choice due to it being a cheap and easy way to treat the glove surface [10]. Gloves can also be treated by chemical coating, such as with hydrogel, amphiphobic acrylic polymer which absorbs water [3,11,12]. Other polymers such as polyurethane can also be used, and new polymers are being developed such as the anti-microbial chlorhexidine-gluconate coating [13]. It is important to note that medical gloves are not just composed of the raw materials, they contain varying degrees of compounding chemicals to aid the glove formation. The difference in manufacturing methods, the compounding chemicals, and the surface treatment method can create different end products which have differing properties [3,10].

1.2 Glove Standards

Medical gloves must conform to the EN455 [14] standards, which covers the material integrity, strength, shelf life and carries the CE mark. These also describe the properties required by glove materials to protect from chemicals and micro-organisms [15]. From manufacture, gloves are tested for durability, tensile strength and force at break. The question of whether these are good enough assessments of medical gloves remains. It can be argued that the glove assessments and standards should also be focusing on the user compatibility, rather than just the protection properties of the materials. Very few areas of literature aim to seek out how medical gloves can be assessed to fully evaluate the extent at which placing a barrier between the fingers and the patient or tools in a surgical setting can, for instance, affect tactile and haptic feedback.

2. Tactile Sensitivity

Tactile sensitivity is defined as the ability to extract information from a foreign object to determine the texture, shape, size and possibly orientation via manual exploration [16]. However, questions concerning the rupture rate and durability of these gloves are being raised [17,18]. Common methods of assessing tactile sensitivity include the use of monofilament tests in conjunction with two-point discrimination tests. In the monofilament test, the subject is blinded, and a microfilament is pressed onto a part of the hand. Once the filament buckles, the examiner ceases pressure application and the subject confirms if contact has been felt. A major limitation of this test is that the thicker filaments buckle at higher loads, thus the pressure at the filament contact will differ between the varying degrees of thickness. The literature regarding these tests is conflicting with Park *et al.* [16], Novak *et al.* [19], Tiefenthaler *et al.* [20], Bucknoer *et al.* [21], Mylon *et al.* [22] Che and Ge [23] and Thompson and Lambert [24] stating that tactility is reduced when gloves are worn when compared to the bare hand. However, Shih *et al.* [25], Nelson and Mital [26] and Johnson *et al.* [27], show that no change in sensitivity is present when donning medical gloves. When comparing glove materials, Kopka [28] found that there was no difference in sensitivity between NRL and 'NRL-free' gloves. It must be noted, that between these studies, many variations are present in the methodology. Some studies use higher thicknesses of monofilaments to assess sensitivity and different glove materials are used throughout. In the two-point discrimination test, two prongs are placed on the skin at varying distances with the aim of identifying at what distance the two prongs feel like one. Fry *et al.* [29] showed that gloves do not hinder the identification of two distinct points. Whereas other studies investigating this found that gloves can reduce the discrimination of two points [19-21,24-25,30-31]. Again, this test has limitations, given that there is no limit on how much pressure is put onto the surface by the subject and the glove

material can spread out the pressure across the finger. It has also been noted by Lundborg and Rosén [32] that it can be tempting for examiners to apply enough pressure to evoke a result, introducing bias into these tests and producing inaccurate results. Whilst Fry *et al.* [29] stated that they did not find any differences in 2-point discrimination tactility between gloves and no gloves, they looked at ulnar and radial surface testing. The radial nerve is less likely to serve purpose in clinical situations, as the back of the thumb or hand is less likely to be used [33] which draws questions on the effect gloves have on tactility. Table 1 shows a breakdown of the available literature regarding tactile tests.

Another commonly use method is a roughness discrimination test. These tests require participants to identify varying bump sizes or roughness/patterns [16,22,36-39]. Of these, only two studies found that detection rates declined when gloves were worn [16,35]. Sandpaper has also been used as a means of measuring tactile discrimination. Mylon *et al.* [40] showed that subjects could perceive roughness differences when moving their gloved fingers across sandpaper, but not when statically pressing. Palpation or surface anomaly detection with patients would require interaction with skin and tissue that is much more viscoelastic and pliable than the materials used in these studies. Thus, it would be preemptive to say that gloves have no effect on the ability to discriminate surface anomalies on or within the body by these test methods. More advanced assessment methods have been produced, such as the Simulated Medical Examination Tactile Tests (SMETT) developed by Mylon *et al.* [34]. In the ‘bumps’ SMETT test, 100-600µm pimples were 3D printed on a soft rubber-like sheet which was fixed onto a board. Participants were asked to run their fingers across the sheet to see if any pimples were identifiable. The ‘Princess and the Pea’ SMETT test required participants to identify pegs of varying heights (2.5-14.5mm) which were submerged in silicone. A similar test was carried out by Ganeswaran *et al.* [35] which utilized 1.25cm dried glue spots covered by sponge. Although the SMETT tests in Mylon *et al.* [34] do appear to be a valid means of in-situ glove assessment, several areas with room for improvement exist in the methodology and design. It was found that the silicone became stiffer over time, making it harder to identify the pegs. Participants also varied placing their fingers flat or perpendicular to the test beds, which could produce different results due to the dispersion of mechanoreceptors. This could provide differing results between people and between the gloving conditions. Although the bumps and roughness discrimination tests are a good measure of identifying tactility loss, it could be argued that the use of more appropriate surfaces that replicate the body and environmental conditions would lead to more accurate results in a clinical context.

An inability to detect a pulse is the most common reported reason for removing or not donning gloves. A study by Mylon *et al.* [41] considered the effects of gloves on pulse detection using a design whereby water was pumped through one of five tubes under a layer of neoprene sponge using a peristaltic pump. They found significant differences in ability to feel the ‘pulse’ in gloved and ungloved conditions. The authors note that this cannot accurately simulate a pulse test due to the pump limitations on the speed and pressure. Also, there was the potential for bias due to the inability to vary the pulse location. Using a pump that will allow the same pressure and speed of blood would be more simulative of the real world. A more quantifiable way of assessing tactility differences is through the use of vibrations. Carré *et al.* [42] used a vibrating platform to measure the sensitivity difference of fingers when a NRL glove was donned. The glove was found to reduce tactility when compared to the no-gloves condition. However, only one participant was used for this. Overall, studies regarding tactile sensation show that gloves have an adverse effect on ability to feel. However, the extent to which this becomes a detriment still remains unknown. Many of these tests aim to quantify tactility loss, but results differ between studies, possibly due to the different methodology. To quantify tactility loss, further studies looking at how the gloves dampen vibration, like in Carré *et al.* [42], could prove vital for future work. Some of the studies discussed here were conducted prior to the banning of powder coated NRL, thus the results may not applicable to gloves used today due to the differences in manufacturing. Ganeswaran *et al.* [35] stated that powdered NRL gloves are better because they have ideal properties. There is a chance that this powder could affect the frictional properties of gloves in any of dynamic tactility tests, which may give different results. Many the studies cited regarding sensitivity are vague in terminology, describing the gloves tested as ‘thick or ‘thin’ without giving any measurements. Due to the issues arising with these assessments, it is unknown as to how much medical gloves affect the tactile sensitivity of a user, but it is clear they are having a negative effect. When comparing glove thickness, studies have found that the thinner gloves provide more sensitivity [28,30]. Surgical gloves are often marketed as

offering better 'tactile sensitivity', however, studies looking at the difference between medical examination and surgical gloves have found no measurable difference in sensitivity [20].

Table 1: Studies relating to the effect glove materials have on tactile sensitivity. Reduced sensitivity is defined as a reduction in ability to discriminate or identify sensations. For a clear representation of the effects on dexterity, only studies looking at the differences between bare hand and gloves are shown here.

<u>Study</u>	<u>No of Participants</u>	<u>Materials</u>	<u>Test</u>	<u>Results</u>
Bruinick <i>et al.</i> [38]	29	NRL and Vinyl	Roughness discrimination	No significant difference observed
Nelson and Mital [26]	20	NRL	Roughness discrimination, needlestick	No significant difference observed
Klatzy and Lederman [39]	12	NRL	Roughness discrimination	Similar results between bare finger and gloved finger
Mylon <i>et al.</i> [40]	30	NRL and XNBR	Roughness discrimination	Reduced roughness perception
Phillips <i>et al.</i> [31]	20	NRL	Two-point discrimination Roughness discrimination	No significant difference observed
Thompson and Lambert [24]	20 and 30	NRL	Two-point discrimination Monofilament Vein location	Tactile sensitivity reduced with gloves.
Han <i>et al.</i> [30]	40	NRL	Two-point discrimination	Tactile sensitivity reduced with glove
Fry <i>et al.</i> [29]	53	Not Stated	Two-point discrimination	No significant difference observed
Shih <i>et al.</i> [25]	10	NRL	Two-point discrimination and monofilament	No significant difference observed
Tiefenthaler <i>et al.</i> [20]	20	NRL	Two-point discrimination and monofilament	Tactile sensitivity reduced with gloves.
Bucknor <i>et al.</i> [21]	52	Not Stated*	Two-point discrimination and monofilament	Tactile sensitivity reduced with gloves
Johnson <i>et al.</i> [27]	42	NRL and XNBR	Monofilament	No significant difference observed between gloves
Mylon <i>et al.</i> [22]	18	NRL and Vinyl	Monofilament	Tactile sensitivity reduced with gloves
Park <i>et al.</i> [16]	12	NRL	Bumps discrimination	Tactile sensitivity reduced with gloves
Mylon <i>et al.</i> [41]	19	NRL and XNBR	Pulse location simulation	Tactile sensitivity reduced with gloves
Mylon <i>et al.</i> [34]	39 and 34	NRL and XNBR	Simulated Medical Examination Tactile Tests (SMETT)	Tactile sensitivity reduced with glove
Carré <i>et al.</i> [42]	1	Latex	Vibration sensitivity	Sensitivity reduced with glove

*Presumed to be NRL as methodology states the participants were asked about NRL allergy.

3. Dexterity

Dexterity is defined as the ability to carry out tasks using motor skill, moving the hands, fingers and arms. The conformity of bending of the hands and fingers, material folding, and thickness are the main areas where gloves affect dexterity [43]. Together these can impact the ability of users to carry out tasks and manipulate objects with fine skill. Numerous dexterity tests have been developed comparing medical glove material performance. Table 2 shows a breakdown of available tests within the literature investigating how medical gloves affect dexterity against the bare hand. Widely used in these studies, are pegboard tests, such as the Purdue Pegboard and the Crawford Small Parts Dexterity Test (CSPDT). Described by Tiffin and Asher [44] the Purdue Pegboard test is designed to assess gross dexterity by measuring how many pegs can be placed into the board in a set time using both hands and each hand separately. Washers can also be placed on the pegs in the test to allow further, finer assessments. The CSPDT test requires the placement of the pins with the use of tweezers, assessing finer dexterity. The results generally show that dexterity is only significantly affected when thicker or double gloves are worn [16, 22, 25-27, 35, 45-51]. Although little difference is observed between glove materials, vinyl showed more of a decrease in dexterity when compared to barehanded, whilst NRL shows a minimal decrease. Drabek *et al.* [52] demonstrated that vinyl gloves do not affect performance when using a grooved pegboard test (similar to the Purdue Pegboard), regardless of the size of the glove used. However, the study did find that the time taken to remove the pegs from the board was significantly increased when best-fit gloves were worn. Whereas Moore *et al.* [45], Pourmoghami [47] and Drabek *et al.* [50] found that dexterity was decreased in the Purdue pegboard test with NRL when the wrong sized glove was worn. Francis *et al.* [53] and Hamstra and Dubrowksi [54] demonstrated the varied skill of professionals is a factor in these assessments. They found students had impaired dexterity and dropped more pins than experienced surgeons in the pegboard tests. This would suggest that in order to accurately interpret results of pegboard tests, recruited participants should all be at the same level of experience. This is an important factor that should be considered in all tests of this manner. Gauvin *et al.* [55] states that these dexterity tests are of a good enough sensitivity to measure performance and discriminate between gloves. However, numerous issues exist when using these tests to assess the effects of glove materials. The primary issue is that the frictional properties of each person's hand is different. Thus, in the 'no gloves' condition, results could be different due to the variation of skin friction, sweat and oils present naturally on the fingers as well as contaminants (such as food residue). No mention of washing the pegs or hands is present in any of the literature, which would standardise this test and avoid contamination. Many of these studies include the NHS first choice gloves: XNBR and NRL as well as gloves that are not commonly used such as butyl and vinyl [56]. Nelson and Mital [26] and Gnaneswaran *et al.* [35] investigated the effect of NRL thickness on dexterity by having subjects cut paper along lines using scissors and found that a glove thickness of 0.83mm did not have an adverse effect on dexterity during the task. Studies oriented at more specific clinical tasks, look at the effect of gloves on suturing and syringing [41, 35]. These studies also did not observe any significant effect on dexterity between materials. The tasks and protocols in most of these studies are very similar throughout and reveal very little to no impact on dexterity when any of the gloves are donned. This would suggest that either the gloves are not having any effect on dexterity or that the tests are not of a good enough sensitivity to pick up the differences. However, dexterity is reported to be affected when thicker gloves are donned. More novel tests need to be designed to simulate the real-world tasks. Work has already been carried out in this area (syringing and suturing [41, 35]), but more studies are needed to create a test that produces repeatable, reliable results and be provide enough resolution to attempt to differentiate between the effects of dexterity with different glove materials.

Table 2: Studies relating to the effect glove materials have on the dexterity. Reduced dexterity defined as a reduction in time taken to carry out tasks/quality of task. For a clear representation of the effects on dexterity, only studies looking at the differences between bare hand and gloves are shown here.

<i>Study</i>	No of Participants	Glove Material	Test	Results
Nelson and Mital [26]	20	NRL	Paper Cutting	No effect on dexterity
Mylon <i>et al.</i> [41]	19	NRL and XNBR	Suturing	No effect on dexterity
Moore <i>et al.</i> [45]	27	NRL	Purdue Pegboard	No effect on dexterity, although dexterity reduced if smaller or larger gloves used
Sawyer and Bennet [48]	24	NRL and XNBR	Purdue Pegboard	XNBR gloves reduced dexterity
Drabek <i>et al.</i> [50]	20	NRL	Purdue Pegboard	No effect on dexterity, although dexterity reduced if smaller or larger gloves used
Fry <i>et al.</i> [29]	53	Not Stated	Purdue Pegboard	No effect on dexterity
Park <i>et al.</i> [16]	12	NRL	Purdue Pegboard	Gloves reduced dexterity
Allahyari <i>et al.</i> [51]	30	NRL and XNBR	Purdue Pegboard	No effect on dexterity
Pourmoghani [47]	10	NRL	Purdue Pegboard and O'Connor	No effect on dexterity, although dexterity reduced if smaller or larger gloves used
Berger <i>et al.</i> [49]	30	XNBR	Purdue Pegboard and O'Connor	Gloves reduced dexterity
Johnson <i>et al.</i> [27]	42	NRL and XNBR	Purdue Pegboard and CSPDT	Manual dexterity reduced when thicker gloves worn
Mylon <i>et al.</i> [22]	18	NRL and Vinyl	Purdue Pegboard and CSPDT	Gloves reduced dexterity in the Pegboard test but not with the CSPDT. Fine dexterity was reduced with the screwing action in CSPDT
Drabek <i>et al.</i> [52]	20	Vinyl	Grooved Pegboard Test	No effect on dexterity regardless of glove size used. Time to remove pegs was significantly quicker with best fit gloves.

4. Grip and Friction

The frictional properties of medical gloves are an important factor which glove manufacturers should consider. It is these properties which allow for the users to ascertain grip and have a sense of force they are applying, which is imperative for the ability to carry out tasks such as holding tools and applying pressure to wounds. Accurate force control for grip precision demands finer detailed information from mechanoreceptors in the skin, thus when these are blocked by a membrane, it would be reasonable to assume that grip force would be impaired [16]. Much of the work regarding grip is oriented at industrial applications and extra vehicular activity gloves for use in space [43], with few looking at medical gloves. Gnanewaran [35] showed that when powder was present on the gloves, more grip force was exerted. This is presumably because the frictional properties of the gloves were lowered due to the presence of the powder. However, similar findings were reported in Shih *et al.* [25], Willms *et al.* [57], and Kinoshita [58] who reported that thicker NRL gloves made participants exert more grip force when picking up a desired load. They conclude that gloves should be thicker in order to retain a greater grip force. However, it has been shown that thicker gloves impair sensitivity [28, 30]. Park *et al.* [16] looked at the role of mechanoreceptors in force control and the effect of gloves on precision grip. The study found that there was a 20% increase in measured grip force when subjects lifted a heavy object after lifting a light object when gloves were not worn. This grip force was not significantly different when the same test was carried out with NRL gloves, suggesting the sensorimotor effects of gripping were not affected by the gloves. Only one study was found where there was a measured decrease in grip force with XNBR and vinyl gloves [59]. Many of these studies appear to see increase in force as beneficial, as grip is imperative for control. Although, these studies do not look at the effects of this. It could be that this increase in grip, however slight, could affect fatigue on the hand and arm, thus affecting dexterity and performance. It should also be noted, that the over-gripping effect could be due to a reduced friction coefficient between the object and the hands when gloves are introduced [59]. As with Willms *et al.* [57] it would be interesting to assess how much pressure is instinctively applied and then how that adjusts over time during a surgical procedure. However, assessing whether the change in load is down to the gloves or the tasks carried out during surgery itself could prove to be a difficult.

Studies looking at the frictional properties focus on surfaces that are impractical to the medical profession, such as glass and sandpaper [25,60-61]. Mylon *et al.* [40] found no significant difference between NRL and bare hand friction with sandpaper but found a significantly lower friction coefficient with XNBR. Carré *et al.* [42] looked at the friction of surgical gloves on steel and found that the friction coefficients of NRL gloves were greater than the bare hand condition. This finding is different from Shih *et al.* [25], who noted that the coefficient of friction decreases when NRL gloves are donned. Laroche *et al.* [62] looked at the static friction of wet NRL and XNBR gloves on a variety of dental tool patterns. Greater friction coefficients for tools with knurled surface patterns were observed. Although this is the first test to incorporate real tool patterns with fluids, this could be greatly improved by having more realistic bodily fluids in contact with the gloves, such as saliva [63]. The study also did not include a control, such as no gloves or dry gloves to compare. However, this is the only study found measuring the performance of medical gloves in the presence of a contaminant. Evermore, paying consideration to the reason why gloves are worn is vital for friction assessments. In medical settings, gloves act as a barrier to protect from bodily fluids. None of the frictional tests incorporate simulative bodily fluids into the systems to assess how frictional properties may change, which will affect sensitivity and dexterity. This is a fundamental consideration, especially in surgical tasks where gloves are more likely to be in contact with bodily fluids (such as blood) and a wide range of tools. Including fluids into assessments would provide a greater significance to the results of any of the friction and grip studies being conducted. Further studies could then look at the effects of vibration on dexterity with fluids, such as replicating the use of a surgical drill. The frictional properties of the inside of the gloves also require consideration. Often a quick change of gloves is needed in fast paced environments which can be made difficult with the presence of moisture [64]. Roberts and Brackley [12] found that coating the glove with hydrogel gives a lower coefficient of friction than chlorination treatment, thus enabling easier donning. Pavlovich *et al.* [64] demonstrated that when hands were wet, the gloves became more difficult to don and greater force was required to pull the glove on, when compared to dry. However, in

this study, the hands were wet, with no drying process involved. This is unrealistic of the real-world scenario of requiring a quick change of gloves. Damp skin has been demonstrated to have higher friction coefficients when compared to dry skin [65]. Many issues occur when donning gloves with damp hands and this should be of consideration when assessing the frictional properties of the inner surface of glove materials [64].

5. Double Gloving

Throughout the literature, it is recommended that where surgery is a high risk due to diseases, such as HIV, two layers of gloves are worn to minimise exposure. Much of the research on double gloving is centred around puncture indication during surgeries (i.e. using different coloured gloves to indicate the outer glove layer has ruptured) [66]. Johnson *et al.* [27] and Kopka *et al.* [28] both show that dexterity decreases when thicker gloves are worn. Thus, it would seem reasonable to assume that dexterity would be affected negatively when multiple layers are worn. However, Webb and Pentlow [67] found that double gloving did not affect dexterity when looking at knot tying. Fry *et al.* [29] also determined that there was no statistically significant difference in performance when subjects wore two glove layers compared to one when completing the Purdue Pegboard test. There are, however, opposing results with regards to the effect of double gloving on tactile sensitivity. Novak *et al.* [19], Shih *et al.* [25] and Han *et al.* [30] show that there is a loss in tactile sensitivity when assessed by monofilament or two-point discrimination. On the other hand, Fry *et al.* [29] and Webb and Pentlow [67] show no statistical difference in two-point discrimination between one and two glove layers. Germaine *et al.* [68] demonstrated that double gloving is not favoured amongst surgeons. Out of the 170-medical staff asked, when practice recommends that they double glove, 78 said that they do not as it decreases their dexterity and 62 said that it was not comfortable. Regardless of the evidence involving the practicality of double gloving during high-risk surgery, there is little discussion in the literature as to how to double glove. Hollaus *et al.* [69] discusses using the same sized gloves as well as whatever makes the user comfortable. However, much of the literature focuses on the method used in Fry *et al.* [29] and recommend double gloving by using a larger inner layer glove and a smaller outer layer glove. The authors suggest this reduces dermatological issues but does not offer any insight into how dexterity and tactile feedback may be affected via this method.

6. Performance Perception

One of the major issues in glove assessment is the material preference of the user. Studies show glove users have a negative perception of performance when un-preferred glove materials are used, despite there being no statistically significant change in measured performance in some of the studies. [7,29,37,38]. Along with Mylon *et al.* [7], Fry *et al.* [29] also showed that surgeons prefer NRL to XNBR because the XNBR appeared to be thicker, although, the materials were in fact, the same thickness. Few studies have demonstrated a correlation between the perceived and actual performance [22,71]. The studies looking at performance perception, such as Mylon *et al.* [7] focus on more experienced medical practitioners rather than junior. In terms of assessing perceptions within a clinical environment, focusing on junior staff could give more accurate feedback as they more inclined to undertake a variety of tasks. Thus, the increase in task variety could induce a broader and more accurate determination of perceived use in different areas and activities. Irrespective of performance, surgeons and clinicians express criticism for glove materials that are different from their preferred choice by claiming the gloves are too thick, slippery and ill fitting. To properly assess medical gloves, this bias against other materials needs to be considered when evaluating the performance, as it is possible the perception of the performance can decrease the actual performance.

7. Paper Grading

To identify gaps where research is required, a paper grading system has been adapted from Harmon and Lewis [72] and Watson *et al.* [73] who found that study design and reporting of key findings was flawed across the field of tribology. The aim of this grading differs from these by the way of trying to identify

areas where research should be focused in the future. The grading is focused on application of research to relevant systems within the clinical environment and categories differ from those used in previous papers in order to reflect the aim and the practices used in this area of research. It is noted that this way of grading papers is subjective, thus the grading has been kept to matter-of-fact as opposed to subjective analysis (*i.e.*, focusing on participant number and statistical analysis as opposed to the experimental design). It is important to note that not all of these criteria will be applicable to the study designs for this grading. This means that a study which scores highly is not essentially a good study, but a study that fulfils more of the criteria. Similarly, a high score may include all criteria, but whether the entire study is fundamentally flawed will not be determined by this grading. The research papers used in this review have been graded according to the following criteria:

1. Repetition of work: does the study repeat tests to obtain an average result?
2. Number of participants/samples: does the study have a respectable number of participants/tests? (The average participant/sample number throughout these tests is 30, thus this has been used as a benchmark. Anything <30 does not meet this criteria).
3. Statistical analysis: has a statistical analysis been conducted?
4. Conclusions: are the conclusions in the paper based on the results presented?
5. Real world simulation: does the work simulate a real world clinical and/or surgical scenario, e.g. suturing, pulse-feel etc.?
6. Glove material: have multiple glove materials been studied?

A grade 'A' constitutes as fulfilling 5-6 of the criteria; grade 'B' constitutes fulfilling 3-4 of the criteria and grade 'C' constitutes 0-2 of the criteria. A graphical representation of the results is displayed in Figure 2. Much of the research is focused on durability; this is most likely to be because the durability of medical gloves is significant to function. Thus, this is an area of primary focus. However, these assessments have focused mainly on obtaining and testing gloves after surgical procedures have been performed. As there are a great number of differing surgical procedures, each with different tasks and different periods of glove wearing, this may result in incomparable data within the literature. Very few studies focus on the grip and frictional properties of medical gloves. It is recommended that further research should be carried out into the frictional properties as well as the performance effects of tactile sensitivity and dexterity of gloves. Although many of the studies here have good grades by these defined criteria, many of the methodologies lack standardisation and do not have a control or a baseline reading of the gloves. Also, as these studies considered a variety of surgeries, there is a tendency to statistically compare the perforation rates. However, in some studies there are orders of magnitude difference between the duration and type of procedure as well as the total number of procedures included, thus making for a unfair comparison between studies, leading to erroneous conclusions [5,12,16,19-32,34-42,45-54,57-62,70,74-92].

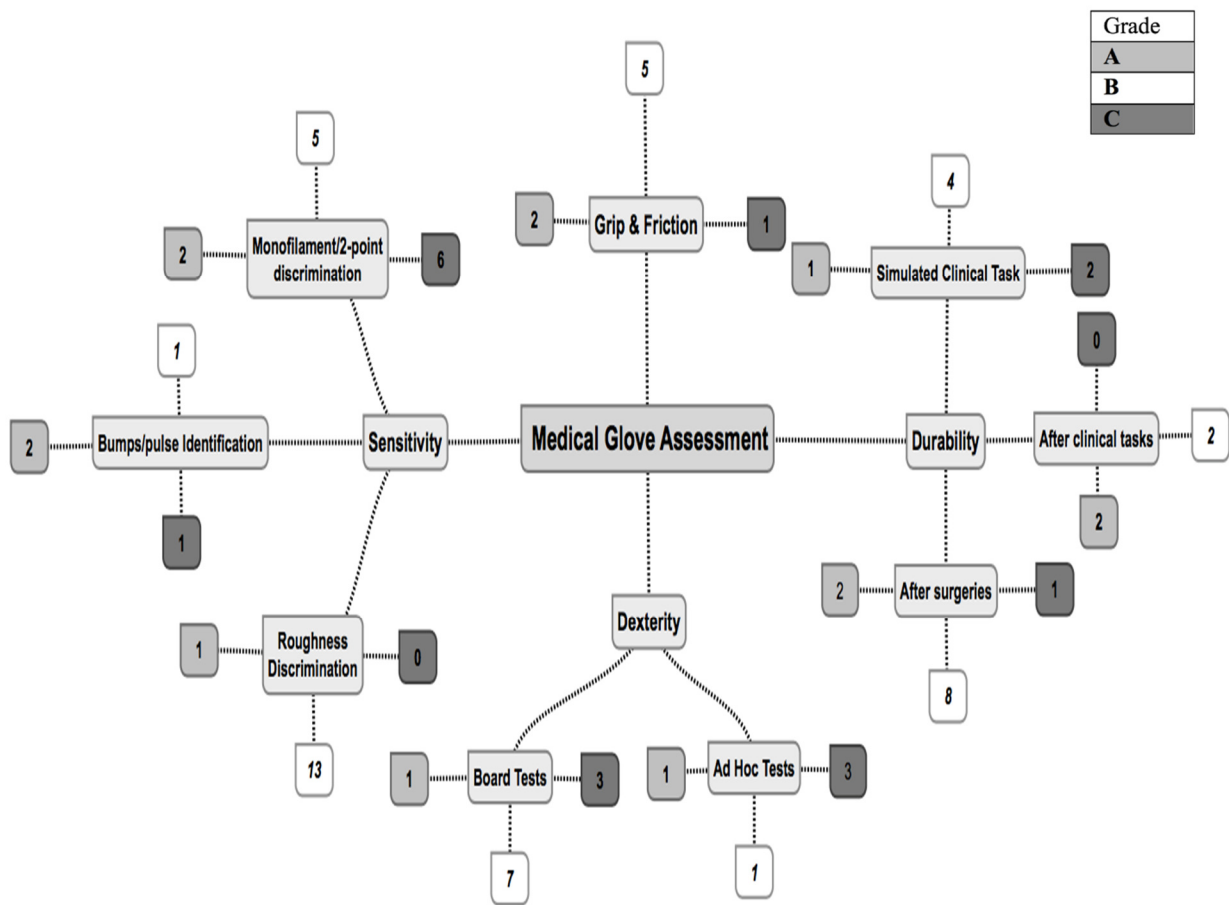


Figure 2: Grading of glove related papers to assess gaps in knowledge.

8. Discussion

The results of most of these studies indicate that medical gloves have a negative effect on tactile sensitivity and user comfort. The research in this field compares different glove materials to determine differentiating performance, rather than assessing the effects gloves have overall. It can be argued that, as no general differences are present between NRL and XNBR gloves there are no major differences in the overall effects on the user. However, research needs to focus on how to assess the gloves effectively to reduce any negative impact they may have on the performance of users. In order to fully evaluate the effects of medical glove materials on user performance, the use of contaminants must be present in the assessments. Similar assessments to existing studies could be developed using different materials and/or simulations that reflect the depth and feel of the skin/tissues to have a more realistic view of the effect of gloves in medical environments. Evaluation of the frictional performance of medical gloves is crucial to understanding how gloves affect grip. This understanding of the principle friction mechanisms can then be applied to key performance issues such as dexterity and sensitivity. Thought should also be given to the fact that the materials surface could be different due to the different processes and treatment methods involved in glove manufacturing. Linking these key manufacturing parameters to performance will give better information about which processes affect the key performance areas. Blinding tests where possible is recommended to limit the psychological 'status-quo' bias that is evident throughout the literature when medical professionals are used as participants.

9. Conclusions

- Overall, studies suggest that sensitivity, friction and grip are affected when medical gloves are worn but dexterity is not. The differences in results between studies of the same tests, could be down to the difference in glove properties, arising from differences in manufacturing
- When assessing medical gloves, the purpose of the barriers should be considered in the tests and contaminants should be incorporated. Understanding how these affect the frictional properties of the gloves will provide vital insight into how medical gloves perform
- Linking the key manufacturing parameters to performance will give better information about which processes affect performance.
- Including the assessment of a desired performance characteristic into the manufacturing process will ensure the production of high-quality gloves that are fit for purpose

10. References

1. Mylon, P, Lewis R, Carré M.J, *et al.* A critical review of glove and hand research with regard to medical glove design. *Ergonomics*. 2014;57:116-129
2. Agrawal AA, Konno K. Latex: a Model for Understanding Mechanisms, Ecology, and Evolution of Plant Defense Against Herbivory. *Annu. Rev. Ecol. Evol. Syst.* 2009;40:311-331
3. Yip E, Cacioli P. The manufacture of gloves from natural rubber latex. *J. Allergy. Clin. Immunol.* 2002;110(2):s3-s14
4. CDC.gov: Latex Allergy [Internet]. Atlanta (GA): Centre for Disease Control and Prevention; 2017 [cited 2017 March 28]. Available from: <https://www.cdc.gov/healthcommunication/toolstemplates/entertainmented/tips/LatexAllergy.html>
5. Rego A, Roley L. In-use barrier integrity of gloves: latex and nitrile superior to vinyl. *Am. J. Infect Control.* 1990;27(5): 405-410
6. Bagg J. (2001). For those of you allergic to latex, nitrile could be the glove material for you. *Br. Dent. J.* 2001;190(7):371
7. Mylon P, Lewis R, Carré M.J, *et al.* A study of clinicians' views on medical gloves and their effect on manual performance. *Am. J. Infect Control.* 2014;42:48-54
8. Edlich RF, Garrison JA, Smith HN. The Food and Drug Administration is Nearing the End of its debate on the life-threatening use of cornstarch powder on medical gloves. *J. Emerg. Med.* 2013;44:193-194
9. Healthy and Safety Executive; Selecting latex gloves [Internet]. United Kingdom. 2010. [cited 16/04/18]. Available at: <http://www.hse.gov.uk/skin/employ/latex-gloves.htm>
10. Akbane T. Production method & market trend of rubber gloves. *Int. Polym. Sci. Technol.* 2015;43(5):45-50
11. Ho CC, Khew MC. Surface Morphology of Pre Vulcanized Natural Rubber Latex Films by Atomic Force Microscopy: New Insight into the Pre Vulcanization mechanism. *Langmuir.* 1999;15(19):6208-6219
12. Roberts AD, Brackley CA (1996). Comfort and frictional properties of dental gloves. *J. Dent.* 1996;24(5):339-343
13. Eng AE, Len KL, Si TL. *et al.* World's First Surgical Glove with Antimicrobial Coating on Inside Surface. *Latex.* 2012;14: 1-6
14. Polyco: EN Standard Tests. [internet]. Polyco; 2017 [cited 17th January]. Available at: <http://www.polyco.co.uk/en-standard-tests/>
15. Kramer A, Assadian, O. Indications and the requirements for single-use medical gloves. *GMS. Hyg. Infect. Control.* 2016;11:1-6
16. Park SB, Davare M, Falla M, *et al.* Fast-adapting mechanoreceptors are important for force control in precision grip but not sensorimotor memory. *J. Neurophysiol.* 2016;115(6):3156-3161
17. Chua KL, Taylor GS, Bagg J. A clinical and laboratory evaluation of three types of operating gloves used in orthodontic practice. *Br. J. Orthod.* 1996;23(2):115-120
18. Said MMD. Fatigue Resistance of Medical Gloves. *J. Rubb. Res.* 2002;5(2):65-83
19. Novak CB, Patterson JM, Mackinnon SE. Evaluation of hand sensibility with single and double latex gloves. *Plast. Reconstr. Surg.* 1996;103:128-129
20. Tiefenthaler W, Gimpl S, Wechselberger G, *et al.* (2006). Touch sensitivity with sterile standard surgical gloves and single-use protective gloves. *Anaesthesia.* 2006;61(10):959-961
21. Bucknor A, Karthikesalingam A, Markar SR, *et al.* A comparison of the effect of different surgical gloves on objective measurement of fingertip cutaneous sensibility. *Ann. R. Coll. Surg. Engl.* 2011;93(2):95-98
22. Mylon P, Carré MJ, Lewis R, *et al.* An Evaluation of dexterity and cutaneous sensibility tests for use with medical gloves. *Proc. Inst. Mech. Eng. C.* 2016;230(16):2896-2912
23. Che S, Ge S. Experimental Research on the tactile perception from fingertip skin friction. *Wear.* 2017;376-377:205-314

24. Thompson PB, Lambert JV. Touch sensitivity through latex examination gloves. *J. Gen. Psychol.* 1995;122:47-58
25. Shih RH, Vasarhelyi EM, Dubrowski A, *et al.* The effects of latex gloves on the kinetics of grasping. *Int. J. Ind. Ergon.* 2001;28(5):265–273
26. Nelson JB, Mital A. An ergonomic evaluation of dexterity and tactility with increase in examination/surgical glove thickness. *Ergonomics.* 1995;38(4):723–733
27. Johnson RL, Smith HM, Duncan CM, *et al.* Factors that Influence the selection of sterile glove brand: a randomized controlled trial evaluating the performance and cost of gloves. *Can. J. Anaesth.* 2013;60(7):700–708
28. Kopka A, Crawford JM, Broome IJ. Anaesthetists should wear gloves – touch sensitivity is improved with a new type of glove. *Acta. Anaesthesiol. Scand.* 2005;49(4):459-462
29. Fry DE, Harris WE, Kohnke EN, *et al.* Influence of double-gloving on manual dexterity and tactile sensation of surgeons. *J. Am. Coll. Surg.* 2010;210(3):325–330
30. Han CD, Kim J, Moon SH, *et al.* A randomized prospective study of glove perforation in orthopedic surgery: is a thick glove more effective? *J. Arthroplasty.* 2013;28(10):1878-1871
31. Phillips AM, Birch NC, Ribbans WJ. Protective gloves for use in high-risk patients: how much do they affect the dexterity of the surgeon? *Ann. R. Coll. Surg. Engl.* 1997;79(2):124–127
32. Lundborg G, Rosén B. The Two-Point Discrimination test—time for re-appraisal. *J. Hand Surg. Br. Vol.* 2004;29(5):418-22
33. Peripheral Nerves of the Upper Extremity [internet]. Toronto: The Orthopaedic Knowledge Network; 2010 Nov 10 [cited 2017 Aug 12]. Available from: <https://www.orthopaedicsone.com/display/Clerkship/Peripheral+Nerves+of+the+Upper+Extremity>
34. Mylon P, Carré MJ, Lewis R, *et al.* How do gloves affect cutaneous sensibility in medical practice? Two new applied tests. *Proc. Inst. Mech. Eng. H.* 2017;231:28-39
35. Gnaneswaran V, Mudhunuri B, Bishu RR. A study of latex and vinyl gloves: Performance versus allergy protection properties. *Int. J. Ind. Ergon.* 2008;38(2):171-181
36. Kennedy WR, Selim MM, Brink TS, *et al.* A new device to quantify tactile sensation in neuropathy. *Neurology.* 2011;76(19):1642-1649
37. Wilson MP, Gound S, Tishk M, *et al.* Gloved versus ungloved dental hygiene clinicians. A comparison of tactile discrimination. *Dent. Hyg. (Chic).* 1986;60(7):310-315
38. Bruinick AL, Burns S, Gross K, *et al.* Comparative study: The effects of latex and vinyl gloves on the tactile discrimination of first year dental hygiene students. *Clin. Prev. Dent.* 1990;12(2):21-25.
39. Klatzy RL, Lederman SJ. Tactile roughness perception with a rigid link interposed between the skin and surface. *Percept. Psychophys.* 1999;61(4):591-607
40. Mylon P, Buckley-Johnstone L, Lewis R, *et al.* Factors influencing the perception of roughness in manual exploration. Do medical gloves reduce cutaneous sensibility? *Proc. Inst. Mech. Eng. J.* 2015;229(3):273-284
41. Mylon P, Carré MJ, Lewis R, *et al.* Evaluation of the effect of medical gloves on dexterity and tactile sensibility using simulated clinical practice tests. *Int. J. Ind. Ergon.* 2016;53:115-123.
42. Carré MJ, Tan SK, Mylon PT, *et al.* Influence of medical gloves on fingerpad friction and feel. *Wear.* 2017;376-377: 324-328
43. Dianat I, Haslegrave CM, Stedmon AW. Methodology for evaluating gloves in relation to the effects on hand performance capabilities: A literature review. *Ergonomics.* 2012;55(11): 1429-1451
44. Tiffin J, Asher EJ. The Purdue Pegboard: Norms and Studies of Reliability and Validity. *J. Appl. Psychol.* 1948;32(2):234-247
45. Moore BJ, Solipuram, SR, Riley MW. The Effects of Latex Examination Gloves on Hand Function: A pilot Study. 39th. Proc. Hum. Factors. Ergon. Soc. Annu. Meet. 1995 Oct 9-13; San Diego CA. p.582–585
46. Chen SC, Tarawneh I, Goodwin B, *et al.* Evaluation of glove liners with objective, subjective and performance measures. 42nd. Proc. Hum. Factors. Ergon. Soc. Annu. Meet. 1998 Oct 5-9; Chicago IL. P.846–850
47. Pourmoghani M. Effects of Gloves and Visual Acuity on Dexterity [dissertation]. Florida: State University of South Florida; 2004

48. Sawyer J, Bennett A. Comparing the level of dexterity offered by latex and nitrile safeskin gloves. *Ann. Occup. Hyg.* 2006;50(3):289-296
49. Berger, MA, Krul AJ, Daanen HA. 2009. Task specificity of finger dexterity tests. *Appl Ergon.* 2009;40:145–147
50. Drabek T, Boucek CD, Buffington CW. Wearing the Wrong Size Latex Surgical Gloves Impairs Manual Dexterity. *J. Occup. Environ. Hyg.* 2010;7:152–155
51. Allahyari T, Khaneshenas F, Khalkhali H. An Investigation of the Impact of Using Latex and Nitrile Gloves on Hand Dexterity. *Int. J. Occup. Hyg.* 2015;7:22-26
52. Drabek T, Boucek, CD, Buffington, CW. Wearing Ambidextrous Vinyl Gloves Does Not Impair Manual Dexterity. *J. Occup. Hyg.* 2013;10(6):307-311
53. Francis NK, Hannah GB, Cresswell AB, *et al.* The performance of Master surgeons on Standards aptitude testing. *Am. J. Surg.* 2001;182:30-33
54. Hamstra SJ, Bubrowska A. Effective training and assessment of surgical skills, and the correlates of performance. *Surg. Innov.* 2005;12(1):71-77
55. Gauvin J, Tellier C, Diagle R, *et al.* Evaluation of the Dexterity Tests for Gloves. *3rd Proc. EU. Conf. Prot. Cloth. Pol.* 2006;330-335
56. Pratt RJ, Pellowe CM, Wilson JA, *et al.* Epic2: National Evidence-Based Guidelines for Preventing Healthcare-Associated Infections in NHS Hospitals in England. *J. Hosp. Infect.* 2007;65:S1-S59.
57. Willms K, Wells R, Carnahan H. Glove attributes and their contribution to force decrement and increased effort in power grip. *Hum Factors.* 2009;51(6):797–812.
58. Kinoshita H. Effect of gloves on prehensile forces during lifting and holding tasks. *Ergonomics.* 1999;42(10):1272-1385
59. Rock KM, Mikat RP, Foster C. The effects of gloves on grip strength and three-point pinch. *J. Hand. Ther.* 2001;14(4):286-290
60. Duvefelt KBK, Olofsson ULO, Johannesson, CMJ. Towards simultaneous measurements of skin friction and contact area: Results and Experiences. *Proc. Inst. Mech. Eng. J.* 2015;229(3):230-242.
61. Mahmoud MM. Frictional Behavior of Different Glove Materials Sliding Against Glass Sheet. *J. Appl. Sci.* 2016;16(10):491-495
62. Laroche C, Barr A, Dong H, *et al.* Effect of dental tool surface texture and material on static friction with a wet gloved fingertip. *J. Biomech.* 2007;40(3):697-701
63. Davies CG, Khan MN, Ghauri ASK, *et al.* Blood and body fluid splashes during surgery --the need for eye protection and masks. *Ann R Coll Surg Engl.* 2007;89(8):770-772
64. Pavlovich LJ, Cox MJ, Thacker JG, *et al.* Ease of donning surgical gloves: an important consideration in glove selection. *J. Emerg. Med.* 1995;13(3): 353-355
65. Persson BBN, Kovalev A, Gorb SN. Contact Mechanics and Friction on Dry and Wet Human Skin. *Tribol Lett.* 2013;50:17-30
66. Tanner J, Parkinson H. Double gloving to reduce surgical cross infection. *Cochrane. Database. Syst. Rev.* 2006;19(3). Art. No. CD003087
67. Webb JM, Pentlow BD. Double gloving and surgical technique. *Ann. Royal Coll. Surg. Engl.* 1993;75(4):291-292
68. Germaine RL, Hanson J, de Gara CJ. Double gloving and practice attitudes among surgeons. *Am J. Surg.* 2003;185(2):141–145
69. Hollaus PH, Lax GF, Janakiev D, *et al.* Glove perforation rate in open lung surgery. *Eur. J. Cardiothorac. Surg.* 1990;15(4):461-464
70. Laine T, Aarnio P. How often does glove perforation occur in surgery? Comparison between single gloves and a double-gloving system. *Am. J. Surg.* 2001;181(6):546-566.
71. Norton L, Hignett S, Hanson SA. Contemporary Ergonomics: Examination gloves for Nurses – A protocol for usability and testability. New York: Taylor & Francis; 2001
72. Harmon M, Lewis R. Review of top of rail friction modifier tribology. *Tribol. Mater. Surf. Interfaces.* 2016;10(3):150-162.
73. Watson M, Christoforou P, Herrera P, *et al.* An analysis of the quality of experimental design and reliability of results in tribology research. *Wear.* 2019;426-427:1712-1718
74. Barbosa MV, Nahas FX, Ferreira LM, *et al.* Risk of glove perforation in minor and major plastic surgery procedures. *Aesthetic. Plast. Surg.* 2003;27(6):481-484

75. Bekele A, Makonnen N, Tesfaye L, *et al.* Incidence and patterns of surgical glove perforations: experience from Addis Ababa, Ethiopia. *BMC Surg.* 2017;17:26
76. Burke FJ, Baggett FJ, Lomax AM. Assessment of the risk of glove puncture during oral surgery procedures. *Oral. Surg. Oral. Med. Oral. Pathol. Oral. Radiol. Endod.* 1996;82:18-21
77. Carré MJ, Tan SK, Mylon PT, *et al.* Influence of Medical Gloves on Fingerpad Friction and Feel. *Wear.* 2017;376-367:324-328
78. Cole RP, Gault DT. Glove perforation during plastic surgery. *Br. J. Plast. Surg.* 1989;42(4):481-483.
79. Douglas A, Simon TR, Goddard M. Barrier durability of latex and vinyl medical gloves in clinical settings. *Am. Ind. Hyg. Assoc. J.* 1997;58(9):672-676.
80. Goldman AH, Haug E, Owen JR, *et al.* High risk of Surgical Glove Perforation from Surgical Rotatory Instruments. *Clin. Orthop. Relat. Res.* 2016;474(11):2513-2517.
81. Hansen KN, Korniewicz DM, Hexter DA, *et al.* Loss of glove integrity during emergency department procedures. *Ann. Emerg. Med.* 1998;31:65-72.
82. Kerr LN, Boivin WS, Chaput MP, *et al.* The Effect of Simulated Clinical Use on Vinyl and Latex Exam Glove Durability. *J. Test. Eval.* 2002;30(5):415-420.
83. Kerr LN, Chaput MP, Cash LD, *et al.* Assessment of the durability of medical examination gloves. *J. Occup. Environ. Hyg.* 2004;1(9):607-612.
84. Korniewicz DM, Kirwin M, Cresci K, *et al.* Leakage of latex and vinyl exam gloves in high and low risk clinical settings. *Am. Ind. Hyg. J.* 1993;51:22-26.
85. Korniewicz DM, Laughon BE, Butz A, *et al.* Integrity of vinyl and latex procedure gloves. *Nurs Res.* 1989;38(3):144-146.
86. Kuroyanagi N, Nagao T, Sakuma H, *et al.* Risk of surgical glove perforation in oral and maxillofacial surgery. *Int. J. Oral. Maxillofac. Surg.* 2012;41(8):1014-1019.
87. Lutsky KF, Jones C, Abboudi J, *et al.* Incidence of Glove Perforation During Hand Surgical Procedures. *Hand Surg.* 2017;42(10):840.e1-840e.5
88. Murray CA, Burke FJ, McHugh S. An assessment of the incidence of punctures in latex and non-latex dental examination gloves in routine clinical practice. *Br. Dent. J.* 2001;190(7):377-380
89. Newsom SW, Smith MO, Shaw P. A randomized trial of the durability of non-allergenic latex-free surgical gloves versus latex gloves. *Ann. R. Coll. Surg. Engl.* 1998;80(4):288-292
90. O'Connell KP, EL-Masri M, Broyles JB, *et al.* Testing for viral penetration of non-latex surgical and examination gloves: a comparison of three methods. *Clin. Microbiol. Infect.* 2004;10(4):322-326
91. Shek KM, Chau JP. Surgical Glove Perforation Among Nurses in Ophthalmic Surgery: A Case-Control Study. *Int. J. Nurs. Pract.* 2014;20(2):179-186
92. Walsh DL, Schwerin MR, Kisielewski RW, *et al.* Abrasion Resistance of Medical Glove Materials. *J. Biomed. Mater. Res. B. Appl. Biomater.* 2004;68:81-87