

CORRIGENDUM: Reliability and consistency of plantarflexor stretch-shortening cycle function using an adapted force sledge apparatus

Laura-Anne M Furlong and Andrew J Harrison

Biomechanics Research Unit, Department of Physical Education and Sport Sciences, University of Limerick, Castletroy, Limerick, Ireland.

In Figure 2 of the original published paper, velocity was incorrectly labelled on the left vertical axis. The correct version of Figure 2 is shown below. We sincerely apologise for any inconvenience caused.

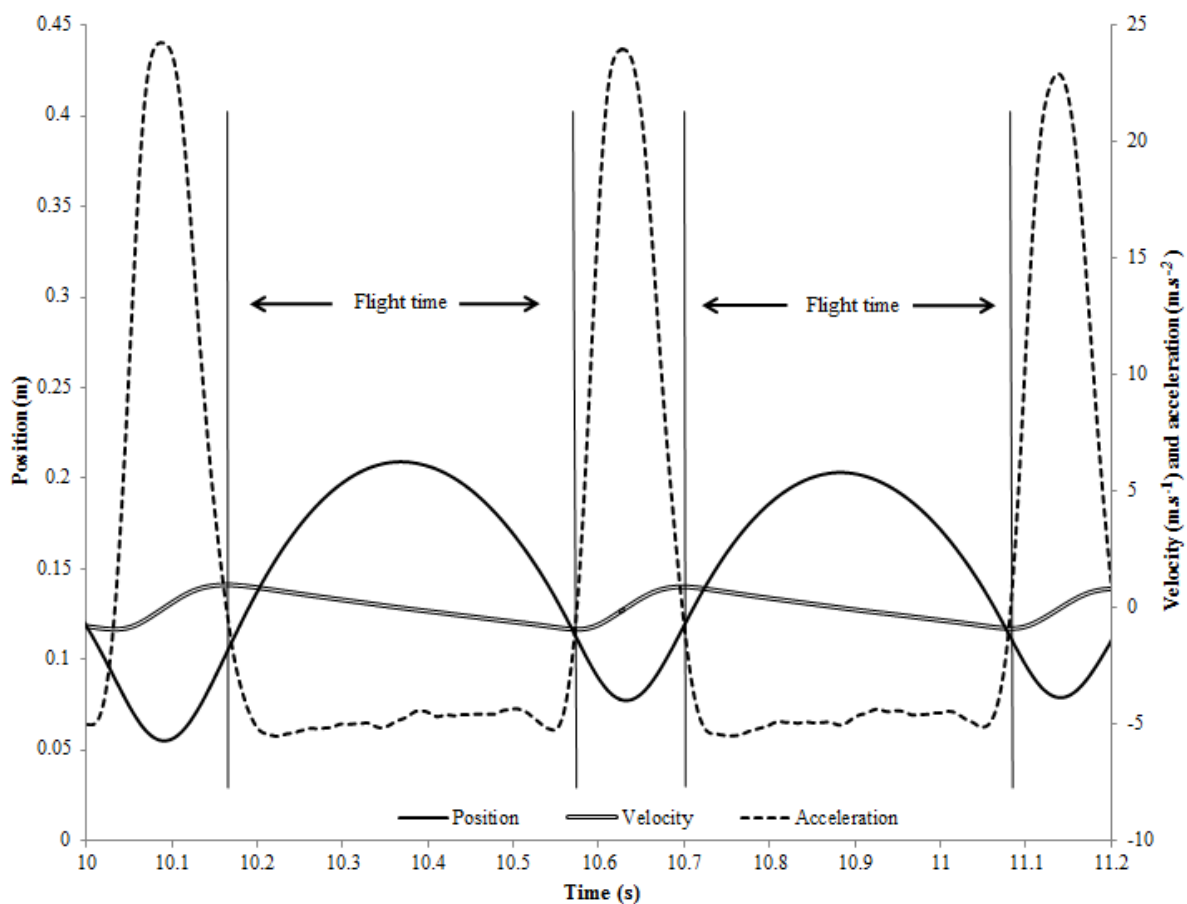


Figure 2. Calculation of CT and FT based on sledge marker kinematics. CT was defined as the time period when acceleration was greater than 0 m.s⁻², and FT as the time between consecutive CT (as shown).