



# DIGITAL ACCESS TO SCHOLARSHIP AT HARVARD

## Myocardial strain imaging with radial acquisitions (SIRA) reduces tag fading compared to Cartesian sampling

The Harvard community has made this article openly available. [Please share](#) how this access benefits you. Your story matters.

<b>Citation</b>	Hulten, Edward, Ravi V Shah, Siddique Abbasi, Tomas Neilan, Jiazuo Feng, John Groarke, Alfonso H Waller, Ron Blankstein, Raymond Y Kwong, and Michael Jerosch-Herold. 2014. "Myocardial strain imaging with radial acquisitions (SIRA) reduces tag fading compared to Cartesian sampling." <i>Journal of Cardiovascular Magnetic Resonance</i> 16 (Suppl 1): P35. doi:10.1186/1532-429X-16-S1-P35. <a href="http://dx.doi.org/10.1186/1532-429X-16-S1-P35">http://dx.doi.org/10.1186/1532-429X-16-S1-P35</a> .
<b>Published Version</b>	<a href="https://doi.org/10.1186/1532-429X-16-S1-P35">doi:10.1186/1532-429X-16-S1-P35</a>
<b>Accessed</b>	February 16, 2015 10:33:46 AM EST
<b>Citable Link</b>	<a href="http://nrs.harvard.edu/urn-3:HUL.InstRepos:12406591">http://nrs.harvard.edu/urn-3:HUL.InstRepos:12406591</a>
<b>Terms of Use</b>	This article was downloaded from Harvard University's DASH repository, and is made available under the terms and conditions applicable to Other Posted Material, as set forth at <a href="http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA">http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA</a>

*(Article begins on next page)*

POSTER PRESENTATION

Open Access

# Myocardial strain imaging with radial acquisitions (SIRA) reduces tag fading compared to Cartesian sampling

Edward Hulten<sup>1,3\*</sup>, Ravi V Shah<sup>1,2</sup>, Siddique Abbasi<sup>1</sup>, Tomas Neilan<sup>1,2</sup>, Jiazuo Feng<sup>1</sup>, John Groarke<sup>1</sup>, Alfonso H Waller<sup>1</sup>, Ron Blankstein<sup>1</sup>, Raymond Y Kwong<sup>1</sup>, Michael Jerosch-Herold<sup>1</sup>

From 17th Annual SCMR Scientific Sessions  
New Orleans, LA, USA. 16-19 January 2014

## Background

Myocardial tagging is considered a gold-standard technique to derive myocardial strain using cardiac magnetic resonance (CMR) in large epidemiologic studies. Nevertheless technical limitations related to tag line fading (via T1 relaxation) limit generalizability and reproducibility of this technique. Our purpose was to test myocardial tagging with radial k-space acquisition against routinely utilized Cartesian k-space sampling techniques, in order to potentially minimize tag-line fading over the cardiac cycle.

## Methods

We compared a new tagging sequence with radial acquisitions for cardiac MRI to a routinely-utilized clinical tagging sequence with Cartesian sampling. Both sequences were added pre-contrast to routine clinical scans of 14 patients. The per phase change in grayscale contrast due to T1 relaxation ("tag fading") of tagged myocardium was modeled using a non-linear fit with maximum likelihood estimation to an exponential decay curve and compared between groups. Peak Eulerian circumferential strain (Ecc) was compared using HARP software.


## Results

14 patients (mean age  $54 \pm 16$  years and 36% were men) and mean left ventricular ejection fraction  $53 \pm 16\%$  (LVEF) were included. Tag fading differed significantly between radial and Cartesian sampling; the exponential decay coefficient was  $-0.045 \pm 0.011$  for the Cartesian and significantly higher than the decay coefficient value of  $0.029 \pm 0.007$  for radial read-outs ( $p < 0.001$ ). Due to

less tag fading myocardial strain could be evaluated for more segments acquired with radial, compared to Cartesian read-outs ( $p < 0.001$ ). The intra-observer reliability for Ecc was higher for radial ( $r = 0.99$ ,  $p < 0.001$ ) than Cartesian ( $r = 0.86$ ,  $p < 0.001$ ) images ( $p = 0.002$  for comparison). The bias was 0.9% and limits of agreement  $-4.1$  to  $6.0\%$  with concordance =  $0.86$  ( $p < 0.001$ ) for Ecc-radial versus Ecc-Cartesian. Both tagging methods correlated with LVEF,  $r = -0.86$  ( $p < 0.001$ ) for Ecc-radial versus  $r = -0.83$  ( $p < 0.001$ ) for Ecc-Cartesian.

## Conclusions

Radial k-space acquisition with very low flip-angle excitations leads to better reliability for myocardial strain relative to standard, widely employed Cartesian readouts, while maintaining good signal-to-noise. Radial k-space

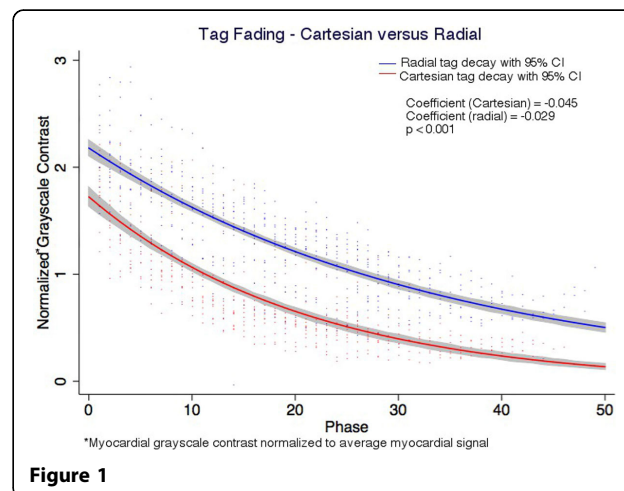

<sup>1</sup>Noninvasive Cardiovascular Imaging, Brigham and Women's Hospital and Harvard Medical School, Boston, Massachusetts, USA  
Full list of author information is available at the end of the article

acquisition is a promising new approach for evaluating myocardial strains using MRI.

## Funding

None.

## Authors' details

<sup>1</sup>Noninvasive Cardiovascular Imaging, Brigham and Women's Hospital and Harvard Medical School, Boston, Massachusetts, USA. <sup>2</sup>Division of Cardiology, Massachusetts General Hospital and Harvard Medical School, Boston, Massachusetts, USA. <sup>3</sup>Cardiology, Walter Reed National Military Medical Center, Bethesda, Maryland, USA.

Published: 16 January 2014

doi:10.1186/1532-429X-16-S1-P35

**Cite this article as:** Hulten *et al.*: Myocardial strain imaging with radial acquisitions (SIRA) reduces tag fading compared to Cartesian sampling. *Journal of Cardiovascular Magnetic Resonance* 2014 **16**(Suppl 1):P35.

**Submit your next manuscript to BioMed Central  
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at  
[www.biomedcentral.com/submit](http://www.biomedcentral.com/submit)

