



# DIGITAL ACCESS TO SCHOLARSHIP AT HARVARD

## MRI-based visual and haptic catheter feedback: simulating a novel system's contribution to efficient and safe MRI-guided cardiac electrophysiology procedures

The Harvard community has made this article openly available.  
[Please share](#) how this access benefits you. Your story matters.

<b>Citation</b>	Kwok, Ka-Wai, Yue Chen, Thomas CP Chau, Wayne Luk, Kent Ronald Nilsson, Ehud J Schmidt, and Zion T Tse. 2014. "MRI-based visual and haptic catheter feedback: simulating a novel system's contribution to efficient and safe MRI-guided cardiac electrophysiology procedures." <i>Journal of Cardiovascular Magnetic Resonance</i> 16 (Suppl 1): O50. doi:10.1186/1532-429X-16-S1-O50. <a href="http://dx.doi.org/10.1186/1532-429X-16-S1-O50">http://dx.doi.org/10.1186/1532-429X-16-S1-O50</a> .
<b>Published Version</b>	<a href="https://doi.org/10.1186/1532-429X-16-S1-O50">doi:10.1186/1532-429X-16-S1-O50</a>
<b>Accessed</b>	February 16, 2015 11:49:57 AM EST
<b>Citable Link</b>	<a href="http://nrs.harvard.edu/urn-3:HUL.InstRepos:12406807">http://nrs.harvard.edu/urn-3:HUL.InstRepos:12406807</a>
<b>Terms of Use</b>	This article was downloaded from Harvard University's DASH repository, and is made available under the terms and conditions applicable to Other Posted Material, as set forth at <a href="http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA">http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA</a>

*(Article begins on next page)*

ORAL PRESENTATION

Open Access

# MRI-based visual and haptic catheter feedback: simulating a novel system's contribution to efficient and safe MRI-guided cardiac electrophysiology procedures

Ka-Wai Kwok<sup>1\*</sup>, Yue Chen<sup>1</sup>, Thomas CP Chau<sup>2</sup>, Wayne Luk<sup>2</sup>, Kent Ronald Nilsson<sup>3</sup>, Ehud J Schmidt<sup>4</sup>, Zion T Tse<sup>1</sup>

From 17th Annual SCMR Scientific Sessions  
New Orleans, LA, USA. 16-19 January 2014

## Background

MRI-guided Electrophysiology (EP) procedures integrate real-time MRI images with catheter position during Radiofrequency Ablation (RFA) of arrhythmias [1]. Using simultaneous MR catheter tracking and imaging [2], this technology can both guide catheter manipulation and provide dynamic assessment of lesion efficacy [3]. Despite advances in MRI-guided EP, maneuvering catheters to the desired location and ensuring appropriate tissue contact is still challenging inside an MRI due to two issues: (1) inconsistent catheter-tissue contact force (CTCF); and (2) visual-motor disorientation arising from differences between manipulation of the catheter's proximal controlling handle and visualization of the catheter-tissue interface. Both issues can increase the risk of cardiac perforation during catheter manipulation. We hypothesized that a technique based on MR imaging to generate force and vibrotactile alarms, as well as the presentation of a reproducible endoscopic view to the catheter operator, could facilitate precise application of RF energy, thereby increasing efficacy and reducing complications.

## Methods

Catheter position and cardiovascular structure were updated from MR images (Figure 1a, upper-right), and the magnitude of CTCF was computed using a graphics processing unit (GPU). A collaborative control strategy, Dynamic Active Constraints (DACs) [4], then rendered CTCF alarms to the catheter operator (Figure 1b-c) in the form of: (i) resistive force against excessive advancement

of catheter into tissue beyond the imaging model; and (ii) catheter handle vibratory feedback indicating tissue proximity to the RFA targets. The CTCF alarm signals were generated using MR-conditional pneumatic catheter braking and vibrotactile units placed on the catheter's handle, and operated with a 30psi pressure. A virtual camera view (Figure 1a, upper-left) was reconstructed at the catheter tip to provide an endoscopic visualization of the 3-dimensional MRI cardiovascular model. An overview of the complete proposed system is included (Figure 2a).



## Results

Ten volunteers without training in EP procedures were recruited to participate in a simulated RFA procedure to evaluate the performance with and without the proposed endoscopic view and haptic interface. RFA targets were pre-defined at the left pulmonary veins inside a left atrium model reconstructed from the preoperative image data from a cardiac patient (Figure 1a). The subjects were allowed to manipulate the catheter so as to locate the virtual catheter tip in the targets, followed by the performance of ablations at multiple locations around the pulmonary vein ostium. Six performance indices with/without the use of the proposed interface are shown in Figure 2b. On average, subjects demonstrated a 61.6% ( $\sigma = 22\%$ ) improvement in terms of RFA accuracy, efficiency and safety.

## Conclusions

The proposed image-based catheter haptic guidance and endoscopic view improved RFA procedural time and accuracy, and reduced the risk of perforation.

<sup>1</sup>College of Engineering, University of Georgia, Athens, Georgia, USA  
Full list of author information is available at the end of the article

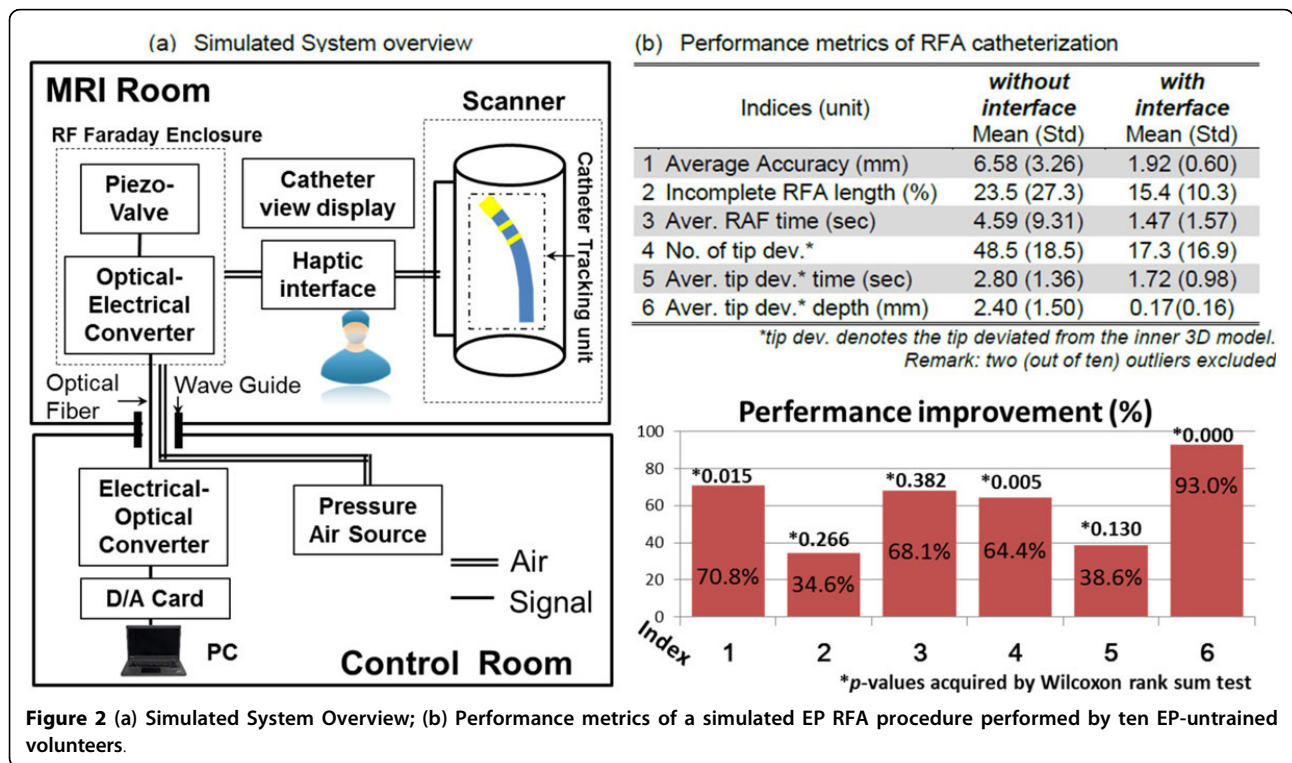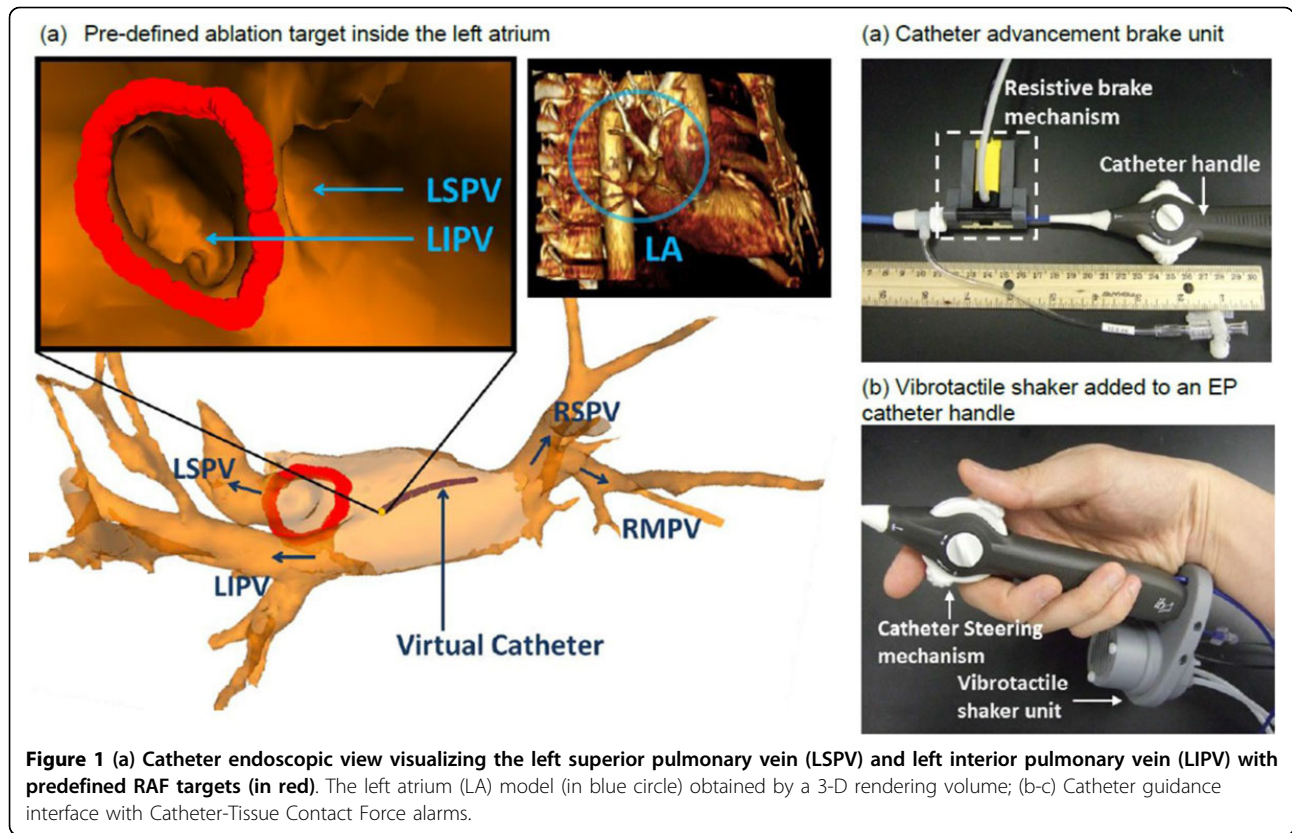

#### Acknowledgements

NIH U41-RR019703, R43 HL110427-01, AHA 10SDG261039, EPSRC and Croucher Foundation Fellowship.

#### Authors' details

<sup>1</sup>College of Engineering, University of Georgia, Athens, Georgia, USA. <sup>2</sup>Computing, Imperial College London, London, UK. <sup>3</sup>Athens Regional Medical Center, University of Georgia, Athens, Georgia, USA. <sup>4</sup>Radiology, Brigham and Women's Hospital, Harvard, Boston, Massachusetts, USA.

Published: 16 January 2014

#### References

1. CE Saikus: *JACC Img.*'09.
2. ZTH Tse: *ISMRM*'12.
3. EJ Schmidt: *Circ.*'09 & *MRM*'13.
4. KW Kwok: *TRO*'13.

doi:10.1186/1532-429X-16-S1-O50

**Cite this article as:** Kwok et al.: MRI-based visual and haptic catheter feedback: simulating a novel system's contribution to efficient and safe MRI-guided cardiac electrophysiology procedures. *Journal of Cardiovascular Magnetic Resonance* 2014 **16**(Suppl 1):O50.

Submit your next manuscript to BioMed Central  
and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at  
[www.biomedcentral.com/submit](http://www.biomedcentral.com/submit)

