



Long-term clinical effects of ventricular pacing reduction with a changeover mode to minimize ventricular pacing in a general pacemaker population

Martin Stockburger^{1,2*}, Serge Boveda³, Javier Moreno^{4,5}, Antoine Da Costa⁶, Robert Hatala⁷, Johannes Brachmann⁸, Christian Butter⁹, Javier Garcia Seara¹⁰, Mara Rolando¹¹, and Pascal Defaye¹²

¹Charité University Hospital, Experimental and Clinical Research Center (ECRC), Berlin, Germany; ²Department of Cardiology, Havelland Kliniken GmbH, Nauen, Germany; ³Arrhythmia Department, Clinique Pasteur, Toulouse, France; ⁴Arrhythmia Department, Cardiovascular Institute, San Carlos University Hospital, Madrid, Spain; ⁵Arrhythmia Department, Hospital Ramón y Cajal, Madrid, Spain; ⁶North Hospital, Saint-Etienne, France; ⁷Narodny Ustav Srdcovych a Cievnych Chorob, Bratislava, Slovak Republic; ⁸Klinikum Coburg, Coburg, Germany; ⁹Herzzentrum Brandenburg, Cardiology, Bernau, Germany; ¹⁰Hospital Clinico Universitario de Santiago, Santiago de Compostela, Spain; ¹¹Sorin Group International SA, Lausanne, Switzerland; and ¹²Arrhythmia Unit, Cardiology Department, University Hospital, Grenoble, France

Received 29 June 2014; revised 24 July 2014; accepted 28 July 2014; online publish-ahead-of-print 1 September 2014

See page 141 for the editorial comment on this article (doi:10.1093/eurheartj/ehu355)

Aim

Right ventricular pacing (VP) has been hypothesized to increase the risk in heart failure (HF) and atrial fibrillation (AF). The ANSWER study evaluated, whether an AAI-DDD changeover mode to minimize VP (SafeR) improves outcome compared with DDD in a general dual-chamber pacemaker population.

Methods and results

ANSWER was a randomized controlled multicentre trial assessing SafeR vs. standard DDD in sinus node disease (SND) or AV block (AVB) patients. After a 1-month run-in period, they were randomized (1:1) and followed for 3 years. Pre-specified co-primary end-points were VP and the composite of hospitalization for HF, AF, or cardioversion. Pre-specified secondary end-points were cardiac death or HF hospitalizations and cardiovascular hospitalizations. ANSWER enrolled 650 patients (52.0% SND, 48% AVB) at 43 European centres and randomized in SafeR ($n = 314$) or DDD ($n = 318$). The SafeR mode showed a significant decrease in VP compared with DDD (11.5 vs. 93.6%, $P < 0.0001$ at 3 years). Deaths and syncope did not differ between randomization arms. No significant difference between groups [HR = 0.78; 95% CI (0.48–1.25); $P = 0.30$] was found in the time to event of the co-primary composite of hospitalization for HF, AF, or cardioversion, nor in the individual components. SafeR showed a 51% risk reduction (RR) in experiencing cardiac death or HF hospitalization [HR = 0.49; 95% CI (0.27–0.90); $P = 0.02$] and 30% RR in experiencing cardiovascular hospitalizations [HR = 0.70; 95% CI (0.49–1.00); $P = 0.05$].

Conclusion

SafeR safely and significantly reduced VP in a general pacemaker population though had no effect on hospitalization for HF, AF, or cardioversion, when compared with DDD.

Keywords

Dual-chamber pacing • Minimization of ventricular pacing • Heart failure • Atrial fibrillation • Randomized controlled trial • SafeR

* Corresponding author. Tel: +49 3321421100, Fax: +49 332142151092, Email: martin.stockburger@charite.de

© The Author 2014. Published by Oxford University Press on behalf of the European Society of Cardiology.

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/4.0/>), which permits non-commercial re-use, distribution, and reproduction in any medium, provided the original work is properly cited. For commercial re-use, please contact journals.permissions@oup.com

Introduction

The risk in experiencing adverse cardiac outcomes due to ventricular pacing (VP) with dual-chamber pacemakers is well established. Ventricular pacing modifies left ventricular (LV) contraction by generating an electrical activation sequence resembling a left bundle branch block. The resulting dyssynchrony is associated with LV remodelling,¹ reduced ejection fraction (EF),^{2,3} and increased risk in heart failure (HF) and death in patients with already depressed LVEF.⁴ A secondary analysis from the mode selection trial (MOST) established the hypothesis that also pacemaker patients with preserved LVEF may develop HF depending on the prevalence of right VP.⁵ Accordingly, a number of different pacing algorithms have been developed that reduce the degree of VP in the atrio-ventricular (AV) sequential pacing mode (DDD). Such systems have been shown in clinical studies to reduce the risk in developing atrial fibrillation (AF), mainly in patients with sinus node disease (SND).^{6,7}

The SafeR algorithm (Sorin CRM, Clamart, France) was developed to individually adapt to a patient's varying AV conduction and to combine the benefits of single-chamber atrial pacing (AAI) with the safety of DDD pacing. Several randomized trials have previously confirmed the efficient VP prevention and safety of the algorithm in selected populations.^{8–10} In the SaveR study, SafeR reduced VP over 1 year in selected patients with preserved or minimally impaired AV conduction compared with DDD.¹¹ However, in patients with conventional indication to pacemaker, including AV block (AVB), long-term data on the impact of SafeR on the risk in developing adverse cardiac outcomes, including developing HF or AF, is undetermined.

The evaluation of the SafeR mode in patients with a dual-chamber pacemaker indication (ANSWER, ClinicalTrials.gov Identifier: NCT00562107) has been designed to assess the efficacy, safety, and benefits of the use of the SafeR mode, in unselected patients with an indication for a dual-chamber pacemaker compared with standard DDD pacing, without minimized VP.

Methods

Study design

The ANSWER study was an investigator-initiated, prospective, randomized, single-blind, controlled, parallel-design, European, multicentre (43 centres) trial. Patients aged ≥ 18 years were included if they had a pacemaker indication and had received a dual-chamber pacemaker equipped with the SafeR mode less than a month prior to enrolment. The pacemaker indication was based on the diagnosis of SND, second degree intermittent AVB, or third degree intermittent or permanent AVB.¹² Patients were excluded if they had permanent AF, sustained ventricular arrhythmias, congenital complete heart block, or vasovagal syncope. The study was conducted in accordance with the declaration of Helsinki¹³ and Good Clinical Practice. The protocol was approved by the local ethics committees.

Devices implanted and randomization

SafeR-enabled pacemakers were used (Symphony 2550 device or REPLY DR, Sorin CRM SAS). The SafeR dual-chamber pacemaker mode has been designed to privilege intrinsic AV activation, while continuously monitoring spontaneous AV conduction and delivering right VP only temporarily, and only in case of demonstrated lasting long PR or repetitively

lacking intrinsic ventricular activation. This changeover pacing mode commutes between single-chamber atrial (AAI) pacing and dual-chamber pacing (DDD) and has previously been described in detail.^{8–10} The selection of atrial (bipolar configuration required) and right VP leads was left to the implanters' discretion. All devices implanted were CE marked at the beginning of the study.

At implant, all pacemakers were programmed to SafeR for 1 month. Subsequently, patients were randomized in a 1 : 1 fashion to the SafeR mode (SafeR group) or to a conventional dual-chamber pacing mode (DDD) with a nominal AV delay (155 ms after a sensed atrial event, 220 ms after a paced atrial event, dynamic shortening with increasing heart rate) as preferred settings (control group).

Follow-up and study end-points

Follow-up visits were scheduled after enrolment before hospital discharge, at 1 month (randomization visit), at 6, 12, 18, 24, and 36 months (termination visit). At each visit, the device memory was interrogated.

ANSWER had a co-primary technical end-point, the percentage of VP at 1 year, and a co-primary clinical end-point, a composite of hospitalization for HF, AF, or cardioversion at 3 years. Pre-specified secondary end-points comprised the percentage of VP at 3 years, the individual components of the co-primary composite end-point, hospitalization for HF or cardiac death, and CV hospitalization (defined as hospitalization for major cardiovascular event, HF, AF, cardioversion, ventricular tachycardia, and cardiac death, occurring at hospital). The comparison of the hospital stay during these cardiovascular hospitalizations was performed as an ancillary analysis.

Collection and adjudication of adverse events

The assessment relied on the site investigators notification of any serious adverse event (AE) and all device-related AE. The site investigators were supported in the detection of events by study monitors. All these events were reported on specific AE forms and had to be transferred to the study manager as soon as possible and no later than five working days after detection. The AE forms included information on the time course, symptoms, treatment modalities, and diagnosis. All events were blindly reviewed and categorized by the Study Steering Committee during regular meetings. The events, including deaths, were adjudicated and classified as serious (Y/N), protocol-related (Y/N), device-related (Y/N), procedure-related (Y/N), hospitalization (Y/N), AF-related (Y/N), HF-related (Y/N), cardioversion (Y/N), other cardiovascular event (Y/N), clinical (non-cardiovascular) event (Y/N), syncope (Y/N). In syncope patients with unclear clinical presentation, the device memory was also reviewed with the aim to identify a correlation with asystolic pauses during AAI-DDD commutations, and to check for possible ventricular tachyarrhythmias induced by changeover episodes. If deemed necessary, additional information was requested from the study sites.

Data on percentage of VP were ascertained from device memories. Changes of the programming mode, retrieved from case report forms and implant files, were also reviewed by the Steering Committee.

Sample size and statistical methods

The trial was designed to detect the effects for both co-primary end-points. The sample size calculation was thus based on the 1-year assumed rate of VP and the 3-years expected incidence of the composite of hospitalization for HF, AF, or cardioversion. Under the assumption of (i) per cent of VP of 30.7% in the control group and 7.1% in the SafeR group, with a common standard deviation of 34%; (ii) frequency of the composite end-point of 20% in the control group and 10% in the SafeR group, corresponding to a difference of 10%; With a statistical power

of 90% and a type 1 error of 0.025 (two-sided), we estimated the sample size to 45 and 532 patients in total, respectively, for the cumulative per cent of VP (co-primary technical end-point at 1 year) and for hospitalization for HF, AF, or cardioversion (co-primary composite end-point at 3 year). Therefore, the sizing was based on the sample size of 532 patients. The rate of loss to follow-up was estimated at 20%, and we therefore planned to enroll 640 patients in total.

The co-primary technical end-point on the percentage of VP was calculated on the intention-to-treat (ITT) population with at least one implant file; and analysed using the Last Observation Carried Forward imputation method. The number of patients with missing data for whom the last observation needed to be carried forward is reported. The co-primary composite end-point was analysed based on a Kaplan–Meier analysis, with patients dropping out censored at the time of their last observation. A Bonferroni correction was applied to both co-primary end-points and a P -value of 0.025 was set as the significance limit for both co-primary end-points. Each of the co-primary end-points had to be significant at the 0.025 level in order to reach the primary end-point. All secondary end-points were carried out on the ITT population and considered statistically significant at a P -value of 0.05. All of them though were considered exploratory.

The co-primary technical end-point on the percentage of VP was analysed by the Mann–Whitney U -test. The co-primary composite end-point (hospitalization for HF, AF, and cardioversion) was analysed by Kaplan–Meier curves and rates per 100 person/year for description, log-rank test for comparisons, Cox model with calculation of hazard ratio (HR) and 95% CI for quantifying the effect. The risk reduction (RR) is reported when significant.

Secondary end-points time-to event were analysed by Kaplan–Meier curves, which accounts for censoring, and rates per 100 person/year for description, log-rank test for comparisons, Cox model with calculation of HR and 95% CI for quantifying the effect. The end-point of the duration of hospitalization for cardiovascular event was analysed using a 0 inflated negative binomial regression.

For non-normally distributed data, median values and inter-quartile ranges are shown except for the duration of hospitalization for which median values and inter-quartile ranges are presented for hospitalization duration >0 day and number (percentage) of patients free from hospitalization is reported.

For categorical data, number and percentage are presented. Safety categorical data were compared with the χ^2 test or Fisher's exact test when appropriate.

All statistical analyses were performed with the SASTM statistical software, version 9.2.

Results

Study population

A total of 650 patients were included in the study at 43 European centres (Austria, France, Germany, Italy, Slovakia, Spain, Switzerland) from 7 December 2007 to 10 March 2010 (83% received a REPLY DR and 17% a Symphony 2550). A total of 632 patients were randomized: 314 to the SafeR group and 318 to the DDD group. A total of 18 patients were not randomized for the following reasons: death ($n = 2$), consent refusal or withdrawal ($n = 6$), did not meet the inclusion criteria ($n = 4$), lost-to-follow-up ($n = 2$), atrial rhythm disorders ($n = 2$), did not attend the M1 visit in due time ($n = 2$). Patient characteristics are shown in Table 1. Approximately half of the population had sick SND (52%) or AVB (48%); 6% had permanent AVB and 42% had intermittent AVB.

The patient flow is shown in Figure 1. A total of 473 patients completed the 36 months follow-up (last visit performed on 17 May 2013). During follow-up, 38 patients (11.9%) out of the DDD group were reprogrammed to SafeR and 13 patients (4.1%) were reprogrammed to VVI; out of the SafeR group 23 patients (7.3%) were reprogrammed to DDD and 8 patients (2.5%) to VVI(R). The average duration of follow-up was 919 ± 342 days from implant. Five hundred and fifty eight patients participated in the analysis of the co-primary end-point of VP, and in 163 out of them the last observation had to be carried forward.

Study outcome

The median (Q1; Q3) prevalence of VP was significantly reduced in the SafeR group vs. DDD at 1 year [4.8%, (Q1–Q3: 0.1–72.0) vs. 95.4%, (Q1–Q3: 53.8–99.4), $P < 0.0001$], which difference remained substantially unaltered at 3 years [11.5%, (Q1–Q3: 0.1–73.8) vs. 93.6%, (Q1–Q3: 62.3–99.2), $P < 0.0001$]. The risk in experiencing a hospitalization for HF, AF, or cardioversion did not significantly differ between randomization groups (HR = 0.78; 95% CI: 0.48–1.25; $P = 0.30$; Figure 2A).

Likewise both individual components of the co-primary composite end-point showed no significant difference between randomization arms, although for the HF component a numerical reduction tended to favour SafeR (hospitalization for HF: HR = 0.58; 95% CI: 0.31–1.09; $P = 0.09$; Figure 2B; hospitalization for AF or cardioversion: HR = 1.09; 95% CI: 0.56–2.09; $P = 0.80$; Figure 2C).

A significant RR of 51% was observed for the combined secondary end-point of cardiac death or HF hospitalization in the SafeR group compared with DDD (HR = 0.49; 95% CI: 0.27–0.90; $P = 0.02$; Figure 3A). Similarly, a 30% RR for the secondary end-point of cardiovascular hospitalization was reported in the SafeR group compared with DDD (HR = 0.70; 95% CI: 0.49–1.00; $P = 0.05$; Figure 3B). The median (Q1; Q3) duration of cardiovascular hospitalization for patients with >0 day of hospitalization was shorter in the SafeR vs. the DDD group [5.0 (2.0; 11.0) vs. 6.0 (2.0; 17.0)]; more patients were free from a cardiovascular hospitalization in SafeR vs. DDD [260 (82.8%) vs. 245 (77.0%)] (0 inflated negative binomial regression, $P = 0.03$).

Safety

No differences in the occurrence of death and device- or procedure-related events were observed between treatment groups (Table 2). None of the syncopal events reported was considered device-related, and no pro-arrhythmic effects of changeover episodes were documented.

Discussion

ANSWER investigated VP prevention and long-term clinical outcomes of an AAI–DDD changeover mode designed to minimize VP (SafeRTM) in a typical patient population indicated to conventional cardiac pacing, as shown by an equal proportion of included patients presenting with either SND and/or AVB. The study met the co-primary technical end-point; it showed that VP was significantly reduced in patients with SND, and—for the first time—it reported that in intermittent AVB VP was reduced as well, whereas the algorithm safely provided mandatory VP in those with permanent AVB. Importantly, the percentage of VP increased over time, which reflects

Table 1 Baseline characteristics of the study population

Clinical characteristics	Enrolled (n = 650)	SafeR group (n = 314)	DDD group (n = 318)
Age, mean ± SD, years	72.4 ± 11.2	71.8 ± 12.2	72.9 ± 9.8
Male gender, n (%)	358 (55.2)	182 (58.0)	169 (53.1)
Heart disease, n (%)			
Coronary artery disease (%)	183 (28.2)	87 (27.7)	91 (28.6)
Dilated cardiomyopathy (%)	31 (4.8)	15 (4.8)	13 (4.1)
Valvular disease (%)	84 (12.9)	37 (11.8)	44 (13.8)
Comorbidities, n (%)			
Arterial hypertension	423 (65.1)	197 (62.7)	215 (67.6)
COPD	32 (4.9)	13 (4.1)	17 (5.3)
Diabetes	140 (21.5)	68 (21.7)	68 (21.4)
Indications for implant, n (%)			
Sinus node disease	336 (52.0)	167 (53.5)	160 (50.5)
AV block	310 (48.0)	145 (46.5)	157 (49.5)
Intermittent AV block	270 (41.8)	127 (40.7)	136 (42.9)
Permanent AV block	40 (6.2)	18 (5.8)	21 (6.6)
Symptoms of HF			
None, n (%)	202 (32.0)	103 (33.7)	91 (29.4)
NYHA I/II/III/IV, %	43.0/50.7/5.8/0.5	41.9/53.7/3.9/0.5	44.5/48.6/6.4/0.5
LVEF, mean ± SD, %	58.3 ± 8.7	58.6 ± 9.1	58.2 ± 8.3
ECG parameters			
LBBB, n (%)	64 (11.1)	29 (10.4)	31 (11.1)
LAHB, n (%)	52 (8.7)	29 (9.9)	23 (7.9)
LPHB, n (%)	1 (0.2)	1 (0.4)	0 (0)
AR, mean ± SD, ms	214.0 ± 58.2	207.1 ± 55.9	219.8 ± 60.2
PR ^a , mean ± SD, ms	191.4 ± 45.2	189.6 ± 47.1	191.8 ± 43.6
Arrhythmias history, n (%)			
Atrial arrhythmias ^b	248 (38.2)	116 (37.1)	125 (39.3)
Ventricular arrhythmias	16 (2.5)	2 (0.6)	13 (4.1)

AR, atrial-paced—ventricle-sensed interval; AV block, atrio-ventricular block; COPD, chronic obstructive pulmonary disease; HF, heart failure; LAHB, left anterior hemi-block; LBBB, left bundle branch block; LPHB, left posterior hemi-block; LVEF, left ventricular ejection fraction determined by echocardiography; NYHA, New York Heart Association; SD, standard deviation; PR, atrial—sensed—ventricle-sensed interval.

^aDetermined on SND and AVBI patients only.

^bAtrial fibrillation, flutter, or tachycardia.

progressive AV conduction disease. In contrast, the co-primary clinical end-point, represented by a combination of hospitalization for HF or AF or cardioversion, did not significantly differ between the randomization groups, nor were the individual end-point components significantly different in the DDD vs. SafeR group.

Dual-chamber pacing implies a trade-off between the paced restoration of a reasonable heart rate and undesired pacing-induced cardiac dyssynchrony. But it is sometimes difficult to decide, when pacing is actually required, and when it is more appropriate to avoid pacing. This is particularly true for patients with intermittent AVB and in those with a prolonged PR interval. In these patients, re-establishing a favourable AV sequence by VP with best possible transmitral LV filling may be offset by pacing-induced LV impairment; and vice versa, preserving prolonged intrinsic AV conduction may prevent pacing-related dyssynchrony, but may in turn produce undesirably fused transmitral filling.

A secondary analysis of a large pacemaker study to compare DDD vs. VVI in SND¹⁴ founded the hypothesis that VP favours clinical HF

despite a fairly preserved LVEF.⁵ Another smaller randomized study² showed that in SND with normal AV conduction DDD with short or long AV delay was associated with more AF compared with AAI. The impairment of LV haemodynamics by right VP¹⁵ was hypothesized to be responsible for the observed adverse effects. Modifiers of right VP adverse effects can likely be seen in the global LV systolic function and the presence of an unpaced bundle branch block (BBB). Patients with depressed LVEF may particularly be harmed by pacing-induced dyssynchrony and require biventricular pacing in case of AVB,^{4,16} whereas those with BBB and already compromised electro-mechanical activation may experience less of a disadvantage by right VP.^{17–19}

Several large studies, conducted in highly selected populations, investigated the effect (AF-related and HF-related outcome) of different device-based pacing strategies to prevent VP.^{6,20–22} The SAVEPACe study,⁶ conducted in patients with SND and preserved intrinsic AV conduction, evaluated a mixture of VP prevention programming compared with DDD with a high percentage of

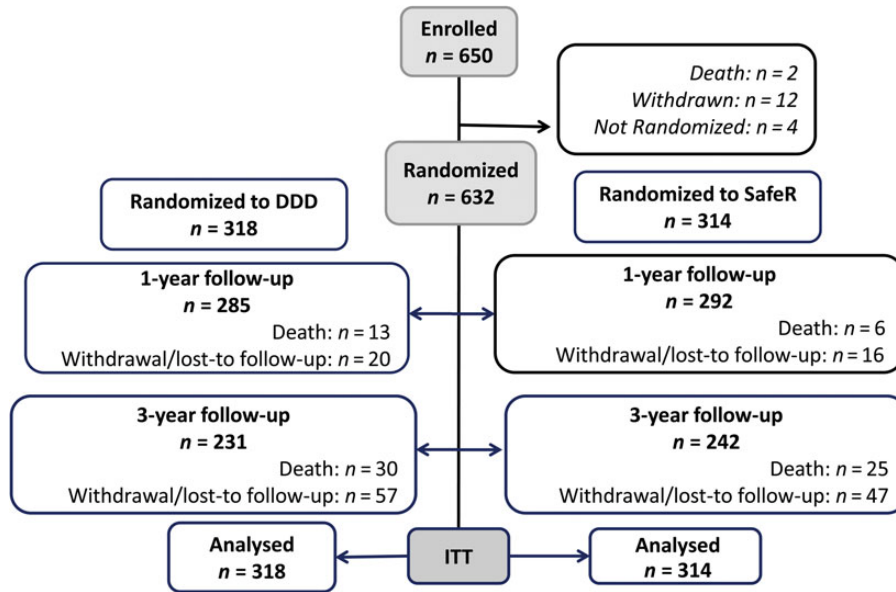


Figure 1 CONSORT flow diagram.

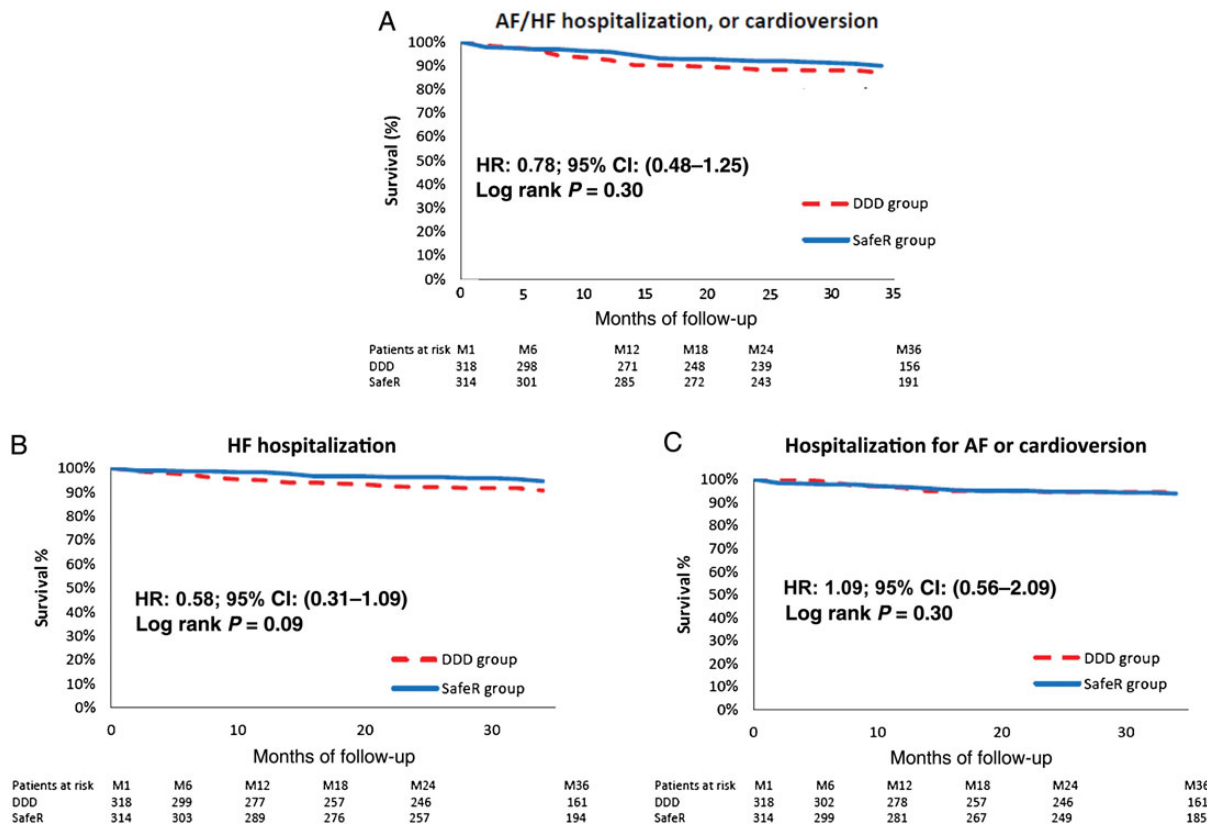


Figure 2 (A) Freedom from hospitalization for heart failure, atrial fibrillation or cardioversion. (B) Freedom from hospitalization for heart failure. (C) Freedom from hospitalization for atrial fibrillation or cardioversion.

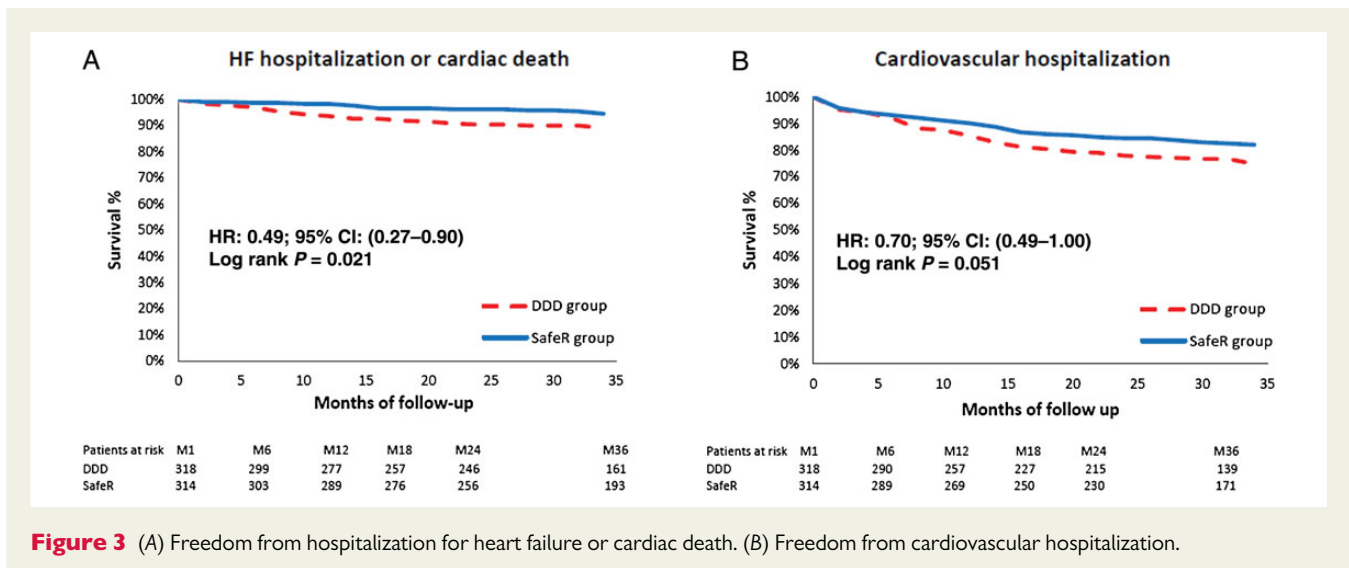


Table 2 Number of patients with death, device, or procedure-related events and syncope

	Overall (n = 650)	BR (n = 18)	SafeR (n = 314)	DDD (n = 318)	P-value
Deaths (%)					
All causes death	58 (8.9)	2 (0.3)	26 (8.3)	30 (9.4)	0.61
Cardiac death	17 (2.6)	1 (0.2)	5 (1.6)	11 (3.5)	0.14
Device or procedure-related adverse events (%)					
All device or procedure-related events	28 (4.3)	14 (2.1)	6 (1.9)	8 (2.5)	0.61
Lead dislodgment	10 (1.5)	6 (0.9)	0	4 (1.3)	0.12
Lead fracture	1 (0.2)	0	0	1 (0.3)	1.00
Pocket hematoma	4 (0.6)	4 (0.6)	0	0	-
Pocket infection	7 (1.1)	3 (0.5)	2 (0.6)	2 (0.6)	1.00
Pocket erosion	1 (0.2)	0	1 (0.3%)	0	0.50
Pacing mode intolerance	5 (0.8)	2 (0.3)	3 (1.0)	1 (0.3)	0.37
Syncope					
Syncope	16 (2.5)	2 (0.3)	5 (1.6)	9 (2.8)	0.42

Results are presented as number of patients (% of patients).

A same patient could experience an event before and after randomization.

BR, before randomization.

VP; it demonstrated a prolonged time to persistent AF by VP prevention. In contrast, three recently published large pacemaker trials^{20–22} fell short of confirming a significant clinical advantage through VP prevention. The DANPACE trial²⁰ randomized 1415 SND patients to AAIR vs. DDDR and adapted the AV programming in the DDDR group to the baseline PR interval. This trial showed no differences in mortality or HF and a disadvantage of AAIR vs. DDDR in paroxysmal AF. The PREFER-MVP study²¹ randomized 605 patients without permanent AVB after pulse generator replacement to VP prevention by the managed ventricular pacing (MVP) mode, vs. DDD. This trial failed to demonstrate a difference in cardiovascular hospitalizations over 2 years. In a similar manner, MINERVA²² study which enrolled patients with bradycardia (mainly with SND and previous atrial tachyarrhythmias) and

compared DDDR with the MVP mode with and without preventive atrial pacing algorithms (DDDRP), demonstrated successful prevention of permanent AF by DDDR in this specific population, but showed no effect of VP prevention on AF progression, death, or cardiovascular hospitalization. Thus, findings of the ANSWER study are well in line with those of most recent trials that appear to collectively contradict the earlier SAVEPACE results⁶ with regard to the AF end-point. It must be kept in mind, however, that SAVEPACE demonstrated a prolonged time to persistent AF by VP prevention, but did not either show a difference in AF-related hospitalizations, HF, or death. When comparing these trials, the heterogeneous end-points, different VP prevention methods, and importantly different study populations must be considered.

The ANSWER study further expands current knowledge because it included AVB patients (6% even with complete permanent AVB) who have not been previously considered. The SafeR changeover mode has safely been applied to a broader pacemaker population indicated for conventional pacing. No pro-arrhythmic adverse effects of SafeR have been observed, whereas the induction of ventricular tachycardia has been described as a rare side-effect of the AAI-to-DDD commutation pattern used by the MVP mode.^{23,24} All-cause mortality, cardiac mortality, and syncope were not significantly different between SafeR and DDD, but deaths and syncopal events occurred numerically less frequently in the SafeR group, which supports the view that this pacemaker mode is safe.

Interestingly, the components of the ANSWER co-primary composite end-point appeared to come out differently, despite both being non-significant. The survival curves for the AF end-point were superimposed, whereas the HF component showed a trend favouring SafeR. The favourable effect of SafeR-mediated VP prevention on HF outcomes, however, warrants further investigation, as the combined clinical secondary outcome of cardiac death or HF hospitalization differed in favour of the SafeR group, and a borderline significant reduction in cardiovascular hospitalizations and shorter duration of hospital stay for these hospitalizations was observed.

Additional favourable effects of the demonstrated VP prevention in AVB patients are the possibly diminished need for biventricular pacing in those with paroxysmal AVB (but otherwise normal PR) and reduced LVEF;²⁵ and improved device longevity by reduced energy consumption.²⁶

Study limitations

The ANSWER study and the co-primary clinical end-point have been designed in 2006–07 based on available knowledge, before the heterogeneous SAVEPACE⁶ and DANPACE²¹ results had been published. The pacemaker memory stores paced and sensed events, but the extent of fused or pseudo-fused pacing, which is likely to be unequal in both randomization groups, cannot be retrieved from the counters. One-fifth of the ANSWER population had LBBB or other types of BBB. This may have extenuated the effects of VP prevention. The occurrence of the primary end-point was lower than predicted by the sample size calculation, which limits the statistical power. Because ANSWER study was a single-blinded study, a possible influence, yet likely marginal, of the investigators' knowledge of the treatment arm on clinical end-point components cannot be ruled out with certainty. Although many of the cardiac deaths in the study occurred in the hospital following an HF hospitalization, it must be said that the classification of causes of death is generally associated with significant uncertainty.

Conclusions

The SafeR pacemaker mode significantly reduced VP compared with DDD in a broad population clinically indicated to dual-chamber pacemaker, regardless of the primary electrical disease (SND or AVB). The risk in experiencing hospitalization for HF or AF or cardioversion was not significantly reduced by SafeR vs. DDD. Secondary end-point results warrant further investigation of SafeR-mediated prevention of HF.

Supplementary material

Supplementary material is available at *European Heart Journal* online.

Acknowledgements

The Steering Committee (M.S., S.B., J.M., and P.D.) was responsible for study planning and design. The authors had full access to and take full responsibility for the integrity of the data. All authors have read and agree to the manuscript as written. The authors want to acknowledge the contribution of Frédérique Maneval and Anne Rousseau-Plasse, scientific writers and Pierre-Henri Siot, bio statistician for the study.

Funding

Sorin Group CRM (Clamart, France) provided financial sponsorship for study conduct and support with the statistical analysis. Funding to pay the Open Access publication charges for this article was provided by Sorin Group CRM, Clamart, France.

Conflict of interest: M.S. received research support and educational grants from Biotronik, Boston Scientific, Medtronic, and Sorin Group; S.B. received grants from Sorin Group, Medtronic and Boston Scientific; J.M. received grants from Sorin Group, Medtronic and Boston Scientific; A.DaC. declares no conflict of interest; R.H. received grants from Sorin, Medtronic and Biotronik; J.B. is a consultant for Biotronik, Medtronic and St Jude Medical; C.B. declares no conflict of interest; J.G.S. received grant from Sorin; M.R. is a Sorin employee; P.D. received grants from Sorin.

Appendix

ANSWER investigators: Austria: Dagmar Burkart-Kuettner, Johann Sipötz, Michael Winkler; France: Frederic Anselme, Serge Boveda, Jean-Pierre Camous, Michel Chauvin, Bertrand Comet, Antoine Da Costa, Pascal Defaye, Benedicte Lauwerier, Antoine Deplagne, Laurent Fauchier, Daniel Gras, Arnaud Lazarus, Philippe Mabo, Jean-Luc Rey, Nicolas Sadoul; Germany: Frank Bode, Johannes Brachmann, Christian Butter, Frank Henschel, Ewald Himmrich, Bernhard Kupper, Bernd Lemke, Ernst Loewe, Jan Noack, Michael Schlegl, Martin Stockburger, Arne Wieckhorst, Uwe Wiegand; Italy: Stefano Nardi, Guido Ranalli, Giovanni Carreras; Spain: Joaquin Alonso, Xulio Beiras-Torrado, Raúl Casariego, Javier García-Seara, José Gutierrez, Juan Martinez, Javier Moreno, Jesús Rodriguez, Julian Pérez-Villacastin; Slovakia: Robert Hatala, Gabriela Kaliska, Jan Kmec, Branislav Stancak; Switzerland: Beat Andreas Schaer.

References

1. Prinzen FW, Cheriex EC, Delhaas T, van Oosterhout MF, Arts T, Wellens HJ, Reneman RS. Asymmetric thickness of the left ventricular wall resulting from asynchronous electric activation: a study in dogs with ventricular pacing and in patients with left bundle branch block. *Am Heart J* 1995;**130**:1045–1053.
2. Nielsen JC, Kristensen L, Andersen HR, Mortensen PT, Pedersen AK. A randomized comparison of atrial and dual-chamber pacing in 177 consecutive patients with sick sinus syndrome: echocardiographic and clinical outcome. *J Am Coll Cardiol* 2003;**42**:614–623.
3. Nahlawi M, Waligora M, Spies SM, Bonow RO, Kadish AH, Goldberger JJ. Left ventricular function during and after right ventricular pacing. *J Am Coll Cardiol* 2004;**44**:1883–1888.
4. Wilkoff BL, Cook JR, Epstein AE, Greene HL, Hallstrom AP, Hsia H, Kutalek SP, Sharma A. Dual-chamber pacing or ventricular backup pacing in patients with an implantable defibrillator: the Dual Chamber and VVI Implantable Defibrillator (DAVID) Trial. *JAMA* 2002;**288**:3115–3123.

5. Sweeney MO, Hellkamp AS, Ellenbogen KA, Greenspon AJ, Freedman RA, Lee KL, Lamas GA; MODe Selection Trial Investigators. Adverse effect of ventricular pacing on heart failure and atrial fibrillation among patients with normal baseline QRS duration in a clinical trial of pacemaker therapy for sinus node dysfunction. *Circulation* 2003;**107**:2932–2937.
6. Sweeney MO, Bank AJ, Nsah E, Koullick M, Zeng QC, Hettrick D, Sheldon T, Lamas GA. Minimizing ventricular pacing to reduce atrial fibrillation in sinus-node disease. *N Engl J Med* 2007;**357**:1000–1008.
7. Veasey RA, Arya A, Silberbauer J, Sharma V, Lloyd GW, Patel NR, Sulke AN. The relationship between right ventricular pacing and atrial fibrillation burden and disease progression in patients with paroxysmal atrial fibrillation: the long-MinVPACE study. *Europace* 2011;**13**:815–820.
8. Savouré A, Fröhlig G, Galley D, Defaye P, Reuter S, Mabo P, Sadoul N, Amblard A, Limousin M, Anselme F. A new dual-chamber pacing mode to minimize ventricular pacing. *Pacing Clin Electrophysiol* 2005;**28**(Suppl. 1):S43–S46.
9. Fröhlig G, Gras D, Victor J, Mabo P, Galley D, Savouré A, Jauvert G, Defaye P, Ducloux P, Amblard A. Use of a new cardiac pacing mode designed to eliminate unnecessary ventricular pacing. *Europace* 2006;**8**:96–101.
10. Pioger G, Leny G, Nitzsché R, Ripart A. AAsafeR limits ventricular pacing in unselected patients. *Pacing Clin Electrophysiol* 2007;**30**(Suppl. 1):S66–S70.
11. Davy J-M, Hoffmann E, Frey A, Jochem K, Rossi S, Dupuis J-M, Frabetti L, Ducloux P, Prades E, Jauvert G. Near elimination of ventricular pacing in SafeR mode compared to DDD modes: a randomized study of 422 patients. *Pacing Clin Electrophysiol* 2012;**35**:392–402.
12. Vardas PE, Auricchio A, Blanc J-J, Daubert J-C, Drexler H, Ector H, Gasparini M, Linde C, Morgado FB, Oto A, Sutton R, Trusz-Gluzka M. Guidelines for cardiac pacing and cardiac resynchronization therapy: The Task Force for Cardiac Pacing and Cardiac Resynchronization Therapy of the European Society of Cardiology. Developed in Collaboration with the European Heart Rhythm Association. *Eur Heart J* 2007;**28**:2256–2295.
13. World Medical Association. WMA Declaration of Helsinki - Ethical Principles for Medical Research Involving Human Subjects, amended by the 59th WMA General Assembly, Seoul, October 2008. 2008. www.wma.net/en/30publications/10policies/b3/index.html.pdf (accessed 8 Jun 2013).
14. Lamas GA, Lee KL, Sweeney MO, Silverman R, Leon A, Yee R, Marinchak RA, Flaker G, Schron E, Orav EJ, Hellkamp AS, Greer S, McAnulty J, Ellenbogen K, Ehlert F, Freedman RA, Estes NA III, Greenspon A, Goldman L; Mode Selection Trial in Sinus-Node Dysfunction. Ventricular pacing or dual-chamber pacing for sinus-node dysfunction. *N Engl J Med* 2002;**346**:1854–1862.
15. Simantirakis EN, Kochiadakis GE, Vardakis KE, Igoumenidis NE, Chrysostomakis SI, Vardas PE. Left ventricular mechanics and myocardial blood flow following restoration of normal activation sequence in paced patients with long-term right ventricular apical stimulation. *Chest* 2003;**124**:233–241.
16. Kindermann M, Hennen B, Jung J, Geisel J, Böhm M, Fröhlig G. Biventricular versus conventional right ventricular stimulation for patients with standard pacing indication and left ventricular dysfunction: the Homburg Biventricular Pacing Evaluation (HOBIPACE). *J Am Coll Cardiol* 2006;**47**:1927–1937.
17. Garrigue S, Barold SS, Valli N, Gencel L, Jais P, Haissaguerre M, Clémenty J. Effect of right ventricular pacing in patients with complete left bundle branch block. *Am J Cardio* 1999;**83**:600–604.
18. Garrigue S, Reuter S, Labeque JN, Jais P, Hocini M, Shah DC, Haissaguerre M, Clémenty J. Usefulness of biventricular pacing in patients with congestive heart failure and right bundle branch block. *Am J Cardiol* 2001;**88**:1436–1441.
19. Varma N. Left ventricular conduction delays induced by right ventricular apical pacing: effect of left ventricular dysfunction and bundle branch block. *J Cardiovasc Electrophysiol* 2008;**19**:144–222.
20. Nielsen JC, Thomsen PEB, Hojberg S, Moller M, Vesterlund T, Dalsgaard D, Mortensen LS, Nielsen T, Asklund M, Friis EV, Christensen PD, Simonsen EH, Eriksen UH, Jensen GV, Svendsen JH, Toff WD, Healey JS, Andersen HR; DANPACE Investigators. A comparison of single-lead atrial pacing with dual-chamber pacing in sick sinus syndrome. *Eur Heart J* 2011;**32**:686–696.
21. Botto GL, Ricci RP, Bénétet JM, Nielsen JC, De Roy L, Piot O, Quesada A, Quaglione R, Vaccari D, Garutti C, Vainer L, Kozák M; PreFER MVP Investigators. Managed ventricular pacing compared with conventional dual-chamber pacing for elective replacement in chronically paced patients: results of the Prefer for Elective Replacement Managed Ventricular Pacing randomized study. *Heart Rhythm* 2014;**11**:992–1000.
22. Boriani G, Tukkie R, Manolis AS, Mont L, Pürerfellner H, Santini M, Inama G, Serra P, de Sousa J, Botto GL, Mangoni L, Grammatico A, Padeletti L; on behalf of the MINERVA Investigators. Atrial antitachycardia pacing and managed ventricular pacing in bradycardia patients with paroxysmal or persistent atrial tachyarrhythmias: the MINERVA randomized multicentre international trial. *Eur Heart J* 2014; (Epub ahead of print).
23. Sekita G, Hayashi H, Nakazato Y, Daida H. Ventricular fibrillation induced by short-long-short sequence during managed ventricular pacing. *J Cardiovasc Electrophysiol* 2011;**22**:1181.
24. Vavasis C, Slotwiner DJ, Goldner BG, Cheung JW. Frequent recurrent polymorphic ventricular tachycardia during sleep due to managed ventricular pacing. *Pacing Clin Electrophysiol* 2010;**33**:641–644.
25. Curtis AB, Worley SJ, Adamson PB, Chung ES, Niazi I, Sherfese L, Shinn T, St. John Sutton M for the Biventricular versus Right Ventricular Pacing in Heart Failure Patients with Atrioventricular Block (BLOCK HF) Trial Investigators. Biventricular Pacing for Atrioventricular Block and Systolic Dysfunction. *N Engl J Med* 2013;**368**:1585–1593.
26. Benkemoun H, Sacrez J, Lagrange P, Amiel A, Prakash A, Himmrich E, Aimè E, Mairese GH, Guénon C, Sbragia P. Optimizing pacemaker longevity with pacing mode and settings programming: results from a pacemaker multicenter registry. *Pacing Clin Electrophysiol* 2012;**35**:403–408.