

Accuracy of the new rapid test for monitoring adalimumab levels

Cátia Rocha, Joana Afonso, Paula Lago, Bruno Arroja, Ana I. Vieira, Claudia C. Dias  and Fernando Magro, on behalf of Portuguese IBD Study Group (GEDII)

Ther Adv Gastroenterol

2019, Vol. 12: 1–11

DOI: 10.1177/
1756284819828238

© The Author(s), 2019.
Article reuse guidelines:
[sagepub.com/journals-](http://sagepub.com/journals-permissions)
[permissions](http://sagepub.com/journals-permissions)

Abstract

Background: The loss of response to adalimumab (ADL) has been related to low serum concentrations at trough. Currently, most methods commercially available for the quantification of ADL are enzyme-linked immunosorbent assay (ELISA) based, with a turnaround time of approximately 8 h, delaying the target dosage adjustment to the subsequent infusion. In this study, we aimed to evaluate the performance of the newly available rapid-test ADL quantification assay by comparing it with three established ELISA methods, using spiked samples and a set of clinical samples.

Methods: Spiked samples from control donors and 120 serum samples from inflammatory bowel disease (IBD) patients undergoing ADL therapy were quantified using lateral flow Quantum Blue® Adalimumab and, the ELISA formats from Immundiagnostik, R-Biopharm and an in-house assay.

Results: The rapid-test assay had intraclass correlation coefficients of 0.590, 0.864 and 0.761 when comparing with the Immundiagnostik, R-Biopharm and in-house assays, respectively. For the five therapeutic windows, the accuracy was high: ADL rapid test compared with the Immundiagnostik (58–88%); R-Biopharm, 68–89%; and in house, 60–88%; and kappa statistics revealed 0.492–0.602, 0.531–0.659 and 0.545–0.682, respectively.

Conclusions: The Quantum Blue® Adalimumab assay can replace the commonly used ELISA-based ADL quantification kits and it is a reliable alternative to these methods. This rapid-test assay enables the quantitative determination of ADL serum trough level in only 15 min. The developed assay allows measurement of ADL over a wide range. Hence, it represents a valuable tool for the clinician to assess the ADL trough level.

Keywords: adalimumab, Quantum Blue® Adalimumab, therapeutic drug monitoring

Received: 17 July 2018; revised manuscript accepted: 19 December 2018.

Introduction

Biological therapies using antitumour necrosis factor alpha (anti-TNF α) monoclonal antibodies (mAbs) are extensively prescribed for inflammatory bowel disease (IBD) patients. Adalimumab (ADL) was the first fully humanized anti-TNF α mAb approved for the treatment of IBD. This mAb is able to bind with a high affinity and specificity to TNF α , thereby blocking its interaction with the p55 and p75 cell-surface TNF receptors.^{1–3} ADL mechanisms of action include the

downregulation of pro-inflammatory cytokines, the induction of T-cell apoptosis and the reduction of leucocyte and lymphocyte migration to the sites of inflammation.^{4,5}

Despite ADL proven efficacy in the treatment of IBD, about 10–30% of all patients fail to respond favourably to the induction phase of the ADL therapy (primary nonresponders) and up to 50% of initial responders lose their clinical response over time (secondary nonresponders).^{6,7} This loss

Correspondence to:

Fernando Magro
Department of
Biomedicine, Unit of
Pharmacology and
Therapeutics, Faculty
of Medicine, University
of Porto, Alameda Prof.
Hernâni Monteiro,
4200-319 Porto,
Portugal

Gastroenterology
Department, Centro
Hospitalar São João,
Porto, Portugal

MedInUP, Centre for Drug
Discovery and Innovative
Medicines, Porto, Portugal
fm@med.up.pt

Cátia Rocha

Department of Biomedicine, University of Porto, Porto, Portugal
University of Lisbon, Faculty of Medicine, Instituto de Saúde Ambiental, Lisbon, Portugal

Joana Afonso

Department of Biomedicine, University of Porto, Porto, Portugal
Centre for Drug Discovery and Innovative Medicines, University of Porto, Porto, Portugal

Paula Lago

Gastroenterology Department, Centro Hospitalar São João, Porto

Bruno Arroja

Gastroenterology Department, Hospital de Braga, Braga, Portugal

A. I. Vieira

Gastroenterology Department, Hospital Garcia de Orta, Almada, Portugal

Claudia C. Dias

Health Information and Decision Sciences Department, University of Porto, Porto, Portugal
Centre for Health Technology and Services Research, University of Porto, Porto, Portugal

of response has been related to low serum trough ADL concentrations; in fact, different studies have reported a clear correlation between serum drug concentrations and clinical response, with IBD patients in clinical remission demonstrating higher median levels of ADL than those with active disease.⁸ Still, an optimal ADL cut-off value, from a therapeutic perspective, remains to be established; whereas some investigators argue that levels above 4.9 µg/ml^{9–11} can predict clinical remission, others suggest that levels above 5.85 µg/ml^{12,13} and above 7.5 µg/ml^{14,15} are able to predict clinical response. In the absence of a specific cut-off, an ADL therapeutic window of 5–12 µg/ml is a generally accepted desirable goal.^{16–18}

Several factors can interfere with the pharmacokinetics and pharmacodynamics of therapeutic mAbs: albumin, body weight, sex, smoking, disease severity and immunogenicity (with formation of antidrug antibodies) are known to alter mAb availability and overall metabolism.^{9,19,20} Therapeutic drug monitoring (TDM) comprises assessment of drug and antidrug antibody levels during mAb therapy. This knowledge allows the optimization of treatment by adjusting drug serum levels in such a way that a minimal efficacious dosage is maintained while adverse effects are minimized. Moreover, TDM can also be used to determine the causes of loss of response to treatment (i.e. low serum levels of the drug or high levels of antidrug antibodies, among other scenarios), allowing informed decision making concerning the patients' therapy. In addition to its therapeutic benefit, TDM can also avoid unnecessary therapeutic interventions, consequently enhancing cost effectiveness of the therapeutic process.^{21–24}

TDM relies on an accurate quantification of the drug and antidrug antibodies from the patients' serum, and several methods have been developed to achieve it. The most common one is the enzyme-linked immunosorbent assay (ELISA), in which the biopharmaceutical is captured on a plate and detected using a secondary antibody; alternative methods include those based on fluid-phase radioimmunoassay, reporter-gene assay, enzyme immunoassay, homogenous mobility shift assay and liquid chromatography–tandem mass spectrometry.^{25–28} However, these techniques require highly trained staff. Moreover, the time from sampling to result reading is often too

long to allow an immediate therapeutic adjustment, which is therefore delayed till the patients' next consultation. Considering this, the development of rapid-test assays is highly useful: these systems allow an on-site and almost immediate reading of the analytical results. The Quantum Blue[®] Adalimumab (BÜHLMANN Laboratories AG, Schönenbuch, Switzerland) test is a new assay for ADL quantification: this rapid test allows quantitative determination of the drug levels from patients' serum in 15 min, allowing an immediate drug dosage adjustment (should it prove necessary).²⁹

In this study, we aim to evaluate the performance of the Quantum Blue[®] Adalimumab quantification assay. To do so, its performance was compared with that of three established ELISA methods in the assessment of exogenously spiked and clinical samples.

Material and methods

Samples and patients

Clinical samples were obtained from IBD patients immediately before an ADL infusion (trough levels): blood samples were collected, centrifuged, and serum samples were kept at –80°C until being processed. Spiked samples of known ADL concentrations (1.5, 4.8, 8.0, 11.3, 14.5, 17.8, 21.0, 24.3, 27.5, 30.8 and 34.0 µg/ml) were generated by diluting the appropriate amount of exogenous ADL (Humira[®], AbbVie Inc., North Chicago, IL, USA) into a pool of serum from control donors.

This study was approved by the Ethics Committees of all involved institutions, and all patients signed a written informed consent prior to their participation.

ADL quantification assays

ADL quantifications using the Quantum Blue[®] Adalimumab assay, hereafter referred to as Quantum Blue[®] Adalimumab, were carried out adhering to the manufacturers' instructions. Briefly, serum samples were diluted 1:20 and 80 µl aliquot was loaded into the port of the test cartridge. After incubation for 15 min, the cartridge was read and the results were shown on the Quantum Blue[®] Adalimumab reader display. The test information and calibration curve for each specific cartridge lot was provided with a chip

card to each test kit. According to the manufacturer, this kit has the following analytical characteristics: the limit of detection is 0.8 µg/ml, and the lower and upper limits of quantification are 1.3 µg/ml and 35 µg/ml, respectively.

The following assays were used as standards in the ADL quantification: the IDKmonitor[®] ADL drug level ELISA kit (Immundiagnostik AG, Bensheim, Germany), hereafter referred to as Immundiagnostik; the RIDASCREEN[®] ADM Monitoring (R-Biopharm AG, Darmstadt, Germany), hereafter referred to as R-Biopharm; and an in-house procedure. The quantifications using Immundiagnostik and R-Biopharm were performed strictly following manufacturers' instructions, whereas the in-house procedure was carried out as previously described by Ben-Horin *et al.*^{30,31} Briefly, serum samples were diluted (1:100) and added to a plate precoated with TNFα (Peprotech, Rocky Hill, NJ, USA). After 60 min of incubation and an appropriate number of washes, a horseradish peroxidase (HRP)-labelled goat antihuman fragment-crystallizable (Fc) antibody (MP Biomedicals, Solon, OH, USA) was added and the plate was incubated for 60 min. Afterwards, tetramethylbenzidine (Millipore, MA, USA) substrate was added, and the reaction was stopped 3 min later with 2 mol/l H₂SO₄. Lastly, the samples' absorbance was read at 450/540 nm, and the ADL concentration was quantified by interpolating the absorbance values in a standard curve built with known concentrations of exogenous ADL. According to the manufacturer, the Immundiagnostik kit has the following analytical characteristics: the lower and upper limits of quantification are the limit of blank × sample dilution factor and the highest concentration of the standard curve × sample dilution factor, respectively. For the R-Biopharm, the lower and upper limits of quantification are 0.5 and 12 µg/ml. For the in-house procedure, the upper limit of quantification was calculated as the highest concentration of the standard curve × the sample dilution factor used. Whenever the results obtained were above these limits of quantification, samples were additionally diluted to obtain linear results within the measuring range of the assays.

Each spiked concentration was repeated between 9 and 13 times and analysed in duplicate. All measurements were carried out by the same researcher.

Statistical analyses

Continuous variables were described using the median, percentile and minimum/maximum value. The reliability between methods was assessed by calculating the intraclass correlation coefficients (ICCs) and the corresponding 95% confidence intervals (CIs). Values less than 0.5 are indicative of poor reliability, values between 0.5 and 0.75 indicate moderate reliability, values between 0.75 and 0.9 indicate good reliability and values greater than 0.90 indicate excellent reliability.³²

Moreover, Bland and Altman plots were used to compare the different techniques. For analysis purposes, the results of all patients' samples measured by the Quantum Blue[®] Adalimumab for which the concentrations were below or above the limits of quantification (1.3 µg/ml and 35 µg/ml, respectively) were considered to be those same limits. The accuracy and kappa statistics were computed based on five different therapeutic windows of ADL (≤3 µg/ml, 3–6.85 µg/ml, >6.85 µg/ml;³³ ≤4.90 µg/ml, >4.90 µg/ml;^{10,11} ≤5.85 µg/ml, >5.85 µg/ml;^{12,13} ≤7.50 µg/ml, >7.50 µg/ml;^{14,15} and ≤5 µg/ml, 5–12 µg/ml, >12 µg/ml^{16–18}). Statistical significance was considered whenever *p* values were below 0.05. All data were arranged, processed, and analysed with SPSS[®] version 24 (Statistical Package for Social Sciences, IBM Corp., Armonk, NY).

Results

Study population

This cohort enrolled 120 samples of 89 IBD patients under ADL therapy whose clinical characteristics are depicted in Table 1. The female proportion of the population was 42%, and 22% of all patients were current smokers. A total of 95.5% of the patients were Crohn's disease patients. All patients were on maintenance phase. A total of 36 patients were medicated with azathioprine (40.4%) and 76 patients (85.4%) were or had been under steroids. Moreover, 35 patients were dependent on steroids and three were steroid resistant.

Quantitative analysis

In order to compare the quantification assays' intravariability and recovery rates, 11 exogenously spiked samples ranging from 1.5 to 34 µg/ml were

Table 1. Cohort characterization.

	<i>n</i>	%
Sex		
Male	47	52.8
Female	42	47.2
Smoking status^a		
Never smoked	44	49.4
Former smoker	18	20.2
Smoker	22	24.7
Disease		
Crohn's disease	85	95.5
Ulcerative colitis disease	4	4.5
Treatment phase		
Induction	0	0.0
Maintenance	89	100.0
Concomitant drugs		
Azathioprine	36	40.4
Steroids	76	85.4
Corticoid dependent	35	39.3
Corticoid resistant	3	3.4
^a Data not available for all subjects. Missing values for smoking status, <i>n</i> = 5.		

quantified using the different methods (Figure 1). The results suggest that the assays yield closer results for lower concentrations, with the standard deviations ranging from 0.3 to 10.6 for the Immundiagnostik, 0.1–7 for the R-Biopharm, 0.74–9.31 for the in-house method, and 0.38–9.66 for the Quantum Blue[®] Adalimumab. Intrasample variability was calculated for each assay showing a mean of intra-assay coefficient of variation (CV) of 24%, 13%, 29% and 24% for Immundiagnostik, R-Biopharm, in house and Quantum Blue[®] Adalimumab, respectively. The average recovery rates were 111% (range 65–163%), 113% (range 84–149%), 110% (range 92–132%) and 85% (range 76–98%) for the Immundiagnostik, R-Biopharm, in house and Quantum Blue[®] Adalimumab methods, respectively.

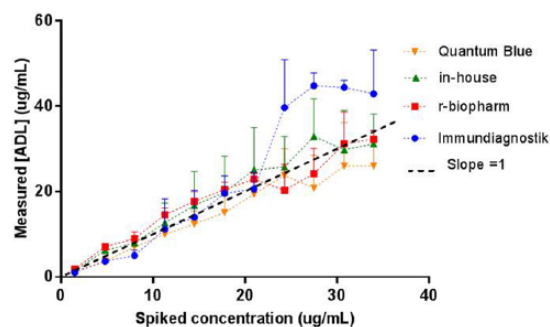
**Figure 1.** ADL quantification of exogenously spiked samples ($\mu\text{g/ml}$). ADL, adalimumab.

Table 2 shows the ICCs between the spiked and the measured ADL concentrations for each method, as well as the average differences. The results show that all assays have a high ICC (above 0.927), which means they have values close to the theoretical concentrations. In accordance with recovery rates, the Immundiagnostik and in-house assays have a negative average difference between the spiked and measured concentrations, and the 95% CI did not include 0, which means that these assays tend to overestimate drug concentration, whereas the opposite is seen for the Quantum Blue[®] Adalimumab, which has a positive average difference and excludes 0, meaning this assay tends to underestimate drug concentration. All assays have the tendency to measure accurate values in the range from 0 to 20 $\mu\text{g/ml}$ and reach a plateau at higher concentrations.

Moreover, in order to test the Quantum Blue[®] Adalimumab assay in a real-life context, both this and the reference assays were used to quantify the ADL amount in 120 serum samples of IBD patients being medicated with this mAb. All patients were in the maintenance phase of ADL therapy. The ICCs and the average differences between the different assays are shown in Table 3. The highest ICCs were found between the R-Biopharm the Quantum Blue[®] Adalimumab (0.864) and the Quantum Blue[®] Adalimumab and in house (0.761), showing a good agreement between these pair of assays. The highest average difference was found between the Immundiagnostik and the R-Biopharm (10.20), in house (13.93), and Quantum Blue[®] Adalimumab assay (13.34), respectively, and the 95% CI did not include 0, showing that the concentrations measured by Immundiagnostik were consistently higher than

Table 2. ICC between the theoretical and measured concentrations of exogenously spiked samples.

	ICC		Difference	
	ICC	CI 95%	Average	CI 95%
Quantum Blue® Adalimumab	0.982	0.933–0.995	2.71	0.95; 4.48
In-house assay	0.989	0.958–0.997	–1.31	–2.84; 0.22
R-Biopharm	0.984	0.940–0.996	–0.60	–2.31; 1.13
Immundiagnostik	0.927	0.727–0.980	–4.67	–9.74; 0.39

ICC, intraclass correlation coefficient; CI, confidence interval.

Table 3. ICC and differences found upon comparing the different ADL quantification assays in clinical samples.

	ICC		Difference	
	ICC	CI 95%	Average	CI 95%
Quantum Blue® Adalimumab				
In-house assay	0.761	0.658–0.834	0.59	–0.48; 1.66
R- Biopharm				
Quantum Blue® Adalimumab	0.864	0.805–0.905	3.13	2.20; 4.06
In-house assay	0.693	0.559–0.786	3.72	2.38; 5.07
Immundiagnostik				
Quantum Blue® Adalimumab	0.590	0.411–0.714	13.34	10.86; 15.81
R-Biopharm	0.530	0.326–0.673	10.20	7.50; 12.90
In-house assay	0.610	0.440–0.728	13.93	11.47; 13.94

ADL, adalimumab; ICC, intraclass correlation coefficient; CI, confidence interval.

those measured by the other assays. Bland–Altman plots were computed to establish whether those differences were related to certain concentration ranges (Supplementary Figure S1). And indeed, these plots suggest that the differences between the methods increase for higher concentrations, although rarely exceed the ± 1.96 SD interval. This is especially evident for the Immundiagnostik ELISA test that shows very good correlations with other tests at concentrations below 20 $\mu\text{g/ml}$, but very poor correlations above this concentration.

Overall, the Quantum Blue® Adalimumab correlates robustly with the R-Biopharm assay over a large concentration range, while this correlation

only holds true for concentrations below 15 $\mu\text{g/ml}$ when compared with the in-house and Immundiagnostik ELISA tests.

Qualitative analysis

To analyse these results from a clinical perspective, ADL levels were stratified according to five possible therapeutic windows: below 3 $\mu\text{g/ml}$, between 3 and 6.85 $\mu\text{g/ml}$, above 6.85 $\mu\text{g/ml}$;³³ below or above 4.90 $\mu\text{g/ml}$;^{9–11} below or above 5.85 $\mu\text{g/ml}$;^{12,13} below or above 7.50 $\mu\text{g/ml}$;^{14,15} below 5 $\mu\text{g/ml}$, between 5 and 12 $\mu\text{g/ml}$, and above 12 $\mu\text{g/ml}$.^{16–18} The agreement analyses for these categories are shown in Table 4.

Table 4. Kappa/accuracy between the different methods using different cut-offs.

	≤3 µg/ml; (3–6.85 µg/ml); >6.85 µg/ml	≤4.90 µg/ml; >4.90 µg/ml	≤5.85 µg/ml; >5.85 µg/ml	≤7.50 µg/ml; >7.50 µg/ml	≤5 µg/ml; (5–12 µg/ml); >12 µg/ml
	Kappa (accuracy)	Kappa (accuracy)	Kappa (accuracy)	Kappa (accuracy)	Kappa (accuracy)
Quantum Blue® Adalimumab					
In-house assay	0.594 (73%)	0.682 (88%)	0.627 (83%)	0.545 (78%)	0.495 (60%)
Immundiagnostik					
Quantum Blue® Adalimumab	0.602 (79%)	0.570 (88%)	0.507 (85%)	0.492 (78%)	0.477 (58%)
R-Biopharm	0.774 (91%)	0.866 (98%)	0.699 (93%)	0.648 (88%)	0.691 (80%)
In-house assay	0.439 (65%)	0.415 (79%)	0.336 (72%)	0.363 (69%)	0.297 (43%)
R-Biopharm					
Quantum Blue® Adalimumab	0.616 (80%)	0.531 (88%)	0.659 (89%)	0.581 (82%)	0.569 (68%)
In-house assay	0.401 (63%)	0.340 (77%)	0.363 (73%)	0.401 (71%)	0.318 (44%)

Comparisons showed that the agreement was higher for the pair Immundiagnostik and the R-Biopharm in the five therapeutic windows, with a substantial to an almost perfect strength of agreement according to the kappa interpretation of Landis and Koch.³⁴ In the case of the Quantum Blue® Adalimumab assay, the kappa statistic revealed that the levels of agreement with the standard assays were moderate to substantial in the five therapeutic windows.

Discussion

The use of TDM for ADL in the treatment of IBD is becoming increasingly common. In cases of nonresponse (primary or secondary), TDM can provide information about the cause of treatment failure. Therefore, TDM is a valuable tool that allows the adjustment of a drug's therapeutic dosage according to the plasma concentrations found in each patient, hence, improving patient care and healthcare resource optimization. The recent development of a rapid ADL quantification assay (Quantum Blue® Adalimumab) holds the promise of revolutionizing the TDM-based therapeutic algorithms, by allowing an immediate adjustment of the ADL dosage. However, and to

ensure accuracy, one has to evaluate whether this assay has a performance comparable with those already in use. This study arises in that context, with the aim of validating the Quantum Blue® Adalimumab by comparing its performance with that of three already-established ELISA assays, using both exogenously spiked and patients' extracted samples.

The results show that all methods have an acceptable performance as assessed by their average recovery percentage and appear to be similar in quantification of ADL. However, and looking at the individual results, the Immundiagnostik assay has a wide variation of recovery, measuring consistently high values for concentrations above 24.3 µg/ml, whereas the Quantum Blue® Adalimumab seems to underestimate ADL concentrations. Regarding the quantitative analysis of the results obtained from the clinical samples, the comparison of the different assays has shown that the R-Biopharm was the closest to the Quantum Blue® Adalimumab, with an ICC of 0.864, but the former kit measures consistently higher values than the latter. This result is supported by the concentrations obtained from the spiked samples, in which in all but the 10 µg/ml sample, higher values were obtained when using

R-Biopharm *versus* Quantum Blue® Adalimumab. The differences found upon comparing the different methods, as well as those between measured and nominal values, are most likely attributable to the ELISA method itself and may include differences at the detection step. Antibodies that bound to the TNF α -drug complex immobilized in the plate differ substantially between the ELISA systems. While the in-house assay uses a HRP-conjugated anti-Fc antibody for the detection step, R-Biopharm uses a HRP-conjugated MA-ADM40D8 antibody generated specifically for ADL.³⁵ Moreover, surface aggregation and denaturation of reagents, which are likely to mask epitopes or show new epitopes, may also interfere with the ELISA system performance. Also, the dilution step may affect results, since serum matrix effects may also interfere with drug level assessments (e.g. presence of complement components, cross-reactive immunoglobulins and rheumatoid factors).³⁶

Bland-Altman plots of measurements of patients' serum locate the differences between the Quantum Blue® Adalimumab and the other assays in different concentration ranges (Supplementary Figure S1). Overall, the lateral flow Quantum Blue® Adalimumab rapid test, and the different ELISAs measure similar levels of ADL at low concentrations but diverge at concentrations above 20 $\mu\text{g/ml}$. This difference is most accentuated in comparison with the Immundiagnostik assay, which systematically measures higher values than other assays at high concentrations. The Bland-Altman plots of the in-house assay show a bimodal distribution compared with other assays, which may explain the poor kappa/accuracy values with all other assays over the various therapeutic cut-off concentration levels (Table 4).

The analysis of results from a qualitative perspective is likely more important in this context, as the placement of a patient within a certain range of ADL concentrations will be reflected in the clinical decisions made if TDM is applied. If the drug concentration is below the therapeutic range in a patient, dose increase, interval shortening, or a combination may be considered. Besides treatment intensification, TDM also includes the possibility of providing insight for reducing the exposure when needed, by re-establishing the standard dosing interval or dose de-escalation.^{37,38}

In this regard, and in the absence of a well-defined therapeutic window for ADL, the samples were

stratified according to five therapeutic windows (≤ 3 $\mu\text{g/ml}$, 3–6.85 $\mu\text{g/ml}$, > 6.85 $\mu\text{g/ml}$;³³ ≤ 4.90 $\mu\text{g/ml}$, > 4.90 $\mu\text{g/ml}$;^{9–11} ≤ 5.85 $\mu\text{g/ml}$, > 5.85 $\mu\text{g/ml}$;^{12,13} ≤ 7.50 $\mu\text{g/ml}$, > 7.50 $\mu\text{g/ml}$;^{14,15} and ≤ 5 $\mu\text{g/ml}$, 5–12 $\mu\text{g/ml}$, > 12 $\mu\text{g/ml}$ ^{16–18}). Considering the range that is used, concentrations below this range are considered infratherapeutic (the patient should escalate the dosage), while concentrations above this range are considered supratherapeutic (the patient can safely de-escalate the dosage). According to our results, the results are substantial to almost perfect for the Immundiagnostik-R-Biopharm comparison, and moderate to substantial for the Quantum Blue® Adalimumab-Immundiagnostik and R-Biopharm-in-house comparisons. However, when in house is involved, results tend to be weaker. These results can be explained by the amplitudes of each method being very different: in the Immundiagnostik, the amplitude varies between 0.2 and 47 $\mu\text{g/ml}$; R-Biopharm varies between 0 and 35 $\mu\text{g/ml}$; and Quantum Blue® Adalimumab varies between 1 and 35 $\mu\text{g/ml}$, while the in-house assay varies between 0.10 and 20 $\mu\text{g/ml}$. Besides, it has been observed that in general the kappa lowers as the cut-off increases, likely as a result of greater dispersion of measurements at higher concentrations.

According to our results, the clinical decision based solely on ADL quantification varies according to the therapeutic window chosen. Thus, considering the different cut-offs: ≤ 3 , 3–6.8, > 6.85 $\mu\text{g/ml}$; ≤ 4.90 , > 4.90 $\mu\text{g/ml}$; ≤ 5.85 , > 5.85 $\mu\text{g/ml}$; ≤ 7.50 , > 7.50 $\mu\text{g/ml}$; and ≤ 5 , 5–12, > 12 $\mu\text{g/ml}$, the clinical decision would be of a similar nature in 79%, 88%, 85%, 78% and 58% of the patients, respectively, using the Quantum Blue® Adalimumab instead of the Immundiagnostik assay; in 80%, 88%, 89%, 82% and 68% of the patients, respectively, using the Quantum Blue® Adalimumab instead of the R-Biopharm; or in 73%, 88%, 83%, 78% and 60% of the patients, respectively, using the Quantum Blue® Adalimumab instead of the in-house assay. Our results show that the specific percentages vary if a different therapeutic range is used. In this sense, it is important to emphasize that the decision making should not only be based on ADL quantification, but these decisions should be integrated into patients' clinical context, considering the presence of symptomatology and other disease markers. More studies are needed to integrate patients'

symptomatology with the performance of the Quantum Blue® Adalimumab in the context of TDM, as well as to define specific therapeutic limits of ADL that should be applied with this method.

The Quantum Blue® Adalimumab for the ADL monitoring in IBD patients is quite advantageous, in the sense that the test response time is 15 min compared with approximately 4 h taken by routine ELISA-based kits (Immundiagnostik, R-Biopharm and in-house assays), allowing the physician to optimize treatment immediately as opposed to delaying possible therapeutic interventions to the next administration. Although the role of TDM assessment during the ADL therapy is not clearly defined, more studies from this perspective are being developed and have been demonstrating the benefits of optimizing the ADL therapy in the treatment of IBD and other inflammatory diseases. In fact, these studies have shown that adjusting ADL doses and administration intervals are a clinically powerful and cost-effective strategy.^{37,39–41} For these reasons, there has been increasing effort by the scientific and medical community in research for the development of novel rapid-test assays and monitoring of IBD patients.

Another important advantage of this commercial rapid test is its user friendliness; in fact, these assays can be operated by any nurse, physician, or researcher, unlike other ELISA kits that require highly trained personnel and specific laboratory facilities. Besides, as a rapid-test method, samples can be analysed upon their collection (i.e. no transportation is needed), and it is designed to be used individually (as opposed to other ELISA kits designed to work in a batch-fashion). Unfortunately, there is no commercially available ADL antibodies Quantum Blue® Adalimumab at the moment. Emerging data increasingly emphasize that the presence of ADL antibodies may lead to ineffective subtherapeutic levels of ADL and contribute to loss of response by increasing drug clearance or blocking the effect of the drug.^{13,41–43} So, monitoring these levels during therapy should be integrated into the management of patients receiving ADL.

For this study, spiked samples and a large number of serum samples obtained from a multicentric and heterogeneous cohort were used and are therefore a representation of reality. However, our study has a few limitations that should be taken into account: the ADL quantification was always

made by the same researcher, which hampers the assessment of the interassay variability; serum matrices often contain components such as rheumatoid factors and other proteins, which could lead to bias during sample analyses, mainly in ligand-binding assays, as well as the presence of ADL antibodies that may differentially interfere with the ADL quantification in each kit (that was unaccounted for). In this study, as the focus was on assessing whether the Quantum Blue® Adalimumab treatment could replace the ELISA-based kits, the analytical performance characteristics of the Quantum Blue® Adalimumab were not considered. However, this performance has been evaluated by the manufacturer and is clearly indicated in the instruction manual accompanying the kit: Quantum Blue® Adalimumab limits of quantification are 1.3–35.5 µg/ml, which may hold a disadvantage when compared with the ELISA-based kits.

In conclusion, the Quantum Blue® Adalimumab is a reliable alternative to the commonly used ELISA-based ADL quantification kit. In fact, the rapid test allows a fast and accurate assessment of ADL levels, which in turn contributes towards proactive and cost-effective therapeutic management of IBD patients. This rapid assay for ADL quantification represents a valuable tool for the fast implementation of tailored therapeutic solutions.

Acknowledgements

The authors would like to thank BÜHLMANN Laboratories AG (Schönenbuch, Switzerland) for kindly providing the Quantum Blue® Adalimumab kits used in this study, and all investigators at the hospitals who provided samples. CCD would like to acknowledge the project NanoSTIMA (NORTE-01-0145-FEDER-000016), which is financed by the North Portugal Regional Operational Programme (NORTE 2020) under the PORTUGAL 2020 Partnership Agreement and through the European Regional Development Fund (ERDF). Moreover, the authors would like to express their gratitude to Sandra Dias for her involvement as the GEDII coordinator and all the help during data collection, as well as to Catarina Santos for medical writing assistance. CR acknowledges “Fundação para a Ciência e Tecnologia (FCT)”, Portugal under grant number PDE/BDE/114583/2016.

FM: study concept and design; analysis and interpretation of data; drafting of the manuscript;

study supervision; critical revision of the manuscript for important intellectual content. CR: drafting of the manuscript; quantification assays; analysis and interpretation of data. JA: drafting of the manuscript, quantification assays; analysis and interpretation of data. CCD: statistical analysis. All the other authors: recruitment of patients and collection of samples.

Funding

This work was supported by the Portuguese IBD Group (GEDII, Grupo de Estudo da Doença Inflamatória Intestinal).

Conflict of interest statement

FM served as speaker and received honoraria from Merck Sharp & Dohme, Abbvie, Vifor, Falk, Laboratorios Vitoria, Ferring, Hospira and Biogen.

Supplemental material

Supplemental material for this article is available online.

ORCID iD

Claudia C. Dias  <https://orcid.org/0000-0001-9356-3272>

References

- Guidi L, Pugliese D and Armuzzi A. Update on the management of inflammatory bowel disease: specific role of adalimumab. *Clin Exp Gastroenterol* 2011; 4: 163–172.
- Plosker GL and Lyseng-Williamson KA. Adalimumab in Crohn's disease. *BioDrugs* 2007; 21: 125–132.
- Hanauer SB, Sandborn WJ, Rutgeerts P, *et al.* Human anti-tumor necrosis factor monoclonal antibody (adalimumab) in Crohn's disease: the CLASSIC-I Trial. *Gastroenterology* 2006; 130: 323–333.
- Baumgart DC and Carding SR. Inflammatory bowel disease: cause and immunobiology. *Lancet* 2007; 369: 1627–1640.
- Weinblatt ME, Keystone EC, Furst DE, *et al.* Adalimumab, a fully human anti-tumor necrosis factor alpha monoclonal antibody, for the treatment of rheumatoid arthritis in patients taking concomitant methotrexate: the ARMADA trial. *Arthritis Rheum* 2003; 48: 35–45.
- Mould DR and Dubinsky MC. Dashboard systems: pharmacokinetic/pharmacodynamic mediated dose optimization for monoclonal antibodies. *J Clin Pharmacol* 2015; 55: S51–S59.
- Stidham RW, Lee TCH, Higgins PDR, *et al.* Systematic review with network meta-analysis: the efficacy of anti-TNF agents for the treatment of Crohn's disease. *Aliment Pharmacol Ther* 2014; 39: 1349–1362.
- Chiu Y, Rubin DT, Vermeire S, *et al.* Serum adalimumab concentration and clinical remission in patients with Crohn's disease. *Inflamm Bowel Dis* 2013; 19: 1112–1122.
- Nakase H, Motoya S, Matsumoto T, *et al.* Significance of measurement of serum trough level and anti-drug antibody of adalimumab as personalised pharmacokinetics in patients with Crohn's disease: a subanalysis of the DIAMOND trial. *Aliment Pharmacol Ther* 2017; 46: 873–882.
- Ward MG, Thwaites PA, Beswick L, *et al.* Intra-patient variability in adalimumab drug levels within and between cycles in Crohn's disease. *Aliment Pharmacol Ther* 2017; 45: 1–11.
- Roblin X, Rinaudo M, Tedesco E Del, *et al.* Development of an algorithm incorporating pharmacokinetics of adalimumab in inflammatory bowel diseases. *Am J Gastroenterol* 2014; 109: 1250–1256.
- Morita Y, Imaeda H, Nishida A, *et al.* Association between serum adalimumab concentrations and endoscopic disease activity in patients with Crohn's disease. *J Gastroenterol Hepatol* 2016; 31: 1831–1836.
- Mazor Y, Almog R, Kopylov U, *et al.* Adalimumab drug and antibody levels as predictors of clinical and laboratory response in patients with Crohn's disease. *Aliment Pharmacol Ther* 2014; 40: 620–628.
- Papamichael K, Baert F, Tops S, *et al.* Post-induction adalimumab concentration is associated with short-term mucosal healing in patients with ulcerative colitis. *J Crohn's Colitis* 2017; 11: 53–59.
- Zittan E, Kabakchiev B, Milgrom R, *et al.* Higher adalimumab drug levels are associated with mucosal healing in patients with Crohn's disease. *J Crohn's Colitis* 2016; 10: 510–515.
- Ungar B, Levy I, Yavne Y, *et al.* Optimizing Anti-TNF- α therapy: serum levels of infliximab and adalimumab are associated with mucosal healing in patients with inflammatory bowel diseases. *Clin Gastroenterol Hepatol* 2016; 14: 550–557.e2.
- Pouw MF, Krieckaert CL, Nurmohamed MT, *et al.* Key findings towards optimising

- adalimumab treatment: the concentration–effect curve. *Ann Rheum Dis*. Epub ahead of print 10 December 2013. DOI: 10.1136/annrheumdis-2013-204172.
18. Mitrev N, Castele N V, Seow CH, *et al*. Review article: consensus statements on therapeutic drug monitoring of anti-tumour necrosis factor therapy in inflammatory bowel diseases. *Aliment Pharmacol Ther* 2017; 46: 1037–1053.
 19. Moss AC. Optimizing the use of biological therapy in patients with inflammatory bowel disease. *Gastroenterol Rep* 2015; 3: 63–68.
 20. Pelletier A and Nicaise-roland P. Adalimumab and pharmacokinetics: impact on the clinical prescription. *World J Pharmacol* 2016; 5: 44–50.
 21. Zandvliet ML, Bezooijen JS Van, Bos MA, *et al*. Monitoring antigen-specific biologics : current knowledge and future prospects. *Ther Drug Monit* 2013; 35: 588–594.
 22. Steenholdt C, Brynskov J, Thomsen OØ, *et al*. Individualised therapy is more cost-effective than dose intensification in patients with Crohn’s disease who lose response to anti-TNF treatment: a randomised, controlled trial. *Gut*. Epub ahead of print 22 June 2013. DOI:10.1136/gutjnl-2013-305279.
 23. Mosli MH, Sandborn WJ, Kim RB, *et al*. Toward a personalized medicine approach to the management of inflammatory bowel disease. *Am J Gastroenterol* 2014; 109: 994–1004.
 24. Krieckaert CLM, Nair SC, Nurmohamed MT, *et al*. Personalised treatment using serum drug levels of adalimumab in patients with rheumatoid arthritis: an evaluation of costs and effects. *Ann Rheum Dis*. Epub ahead of print 21 November 2013. DOI: 10.1136/annrheumdis-2013-204101.
 25. Scott FI and Lichtenstein GR. Therapeutic drug monitoring of anti-TNF therapy in inflammatory bowel disease. *Curr Treat Options Gastroenterol* 2015; 12: 59–75.
 26. Ruiz-argüello B, Ruiz A, Torres N, *et al*. Comparison study of two commercially available methods for the determination of infliximab, adalimumab, etanercept and anti-drug antibody. *Clin Chem Lab Med* 2013; 51: 287–289.
 27. Moss AC and Moss AC. Optimizing the use of biological therapy in patients with inflammatory bowel disease. 2015; 3: 63–68.
 28. Castele N Vande, Buurman DJ, Sturkenboom MGG, *et al*. Detection of infliximab levels and anti-infliximab antibodies: a comparison of three different assays. *Aliment Pharmacol Ther* 2012; 36: 765–771.
 29. Elisa R. Quantum Blue® adalimumab trough level rapid test. BÜHLMANN Laboratories AG, Schönenbuch, Switzerland, <https://www.buhmannlabs.ch/products-solutions/gastroenterology/quantum-blue/quantum-blue-tdm/adalimumab/> (accessed June 2018).
 30. Afonso J, Lopes S, Gonçalves R, *et al*. Proactive therapeutic drug monitoring of infliximab: a comparative study of a new point-of-care quantitative test with two established ELISA assays. *Aliment Pharmacol Ther* 2016; 44: 684–692.
 31. Ben-horin S, Yavzori M, Katz L, *et al*. The immunogenic part of infliximab is the F(ab’)₂, but measuring antibodies to the intact infliximab molecule is more clinically useful. *Gut* 2010; 60: 1–8.
 32. Koo TK and Li MY. A Guideline of selecting and reporting intraclass correlation coefficients for reliability research. *J Chiropr Med* 2016; 15: 155–163.
 33. National Institute for Health and Care Excellence (NICE). Therapeutic monitoring of TNF-alpha inhibitors in Crohn’s disease (LISA-TRACKER ELISA kits, IDKmonitor ELISA kits, and Promonitor ELISA kits). Diagnostics guidance (17 February 2016), <https://www.nice.org.uk/guidance/dg22> (accessed June 2018).
 34. Landis JR and Koch GG. The measurement of observer agreement for categorical data. *Biometrics* 2013; 33: 159–174.
 35. Bian S, Stappen T Van, Baert F, *et al*. Generation and characterization of a unique panel of anti-adalimumab specific antibodies and their application in therapeutic drug monitoring assays. *J Pharm Biomed Anal* 2016; 125: 62–67.
 36. Steenholdt C, Bendtzen K, Brynskov J, *et al*. Optimizing treatment with TNF inhibitors in inflammatory bowel disease by monitoring drug levels and antidrug antibodies. *Inflamm Bowel Dis* 2016; 22: 1999–2015.
 37. Gonczi L, Kurti Z, Rutka M, *et al*. Drug persistence and need for dose intensification to adalimumab therapy; the importance of therapeutic drug monitoring in inflammatory bowel diseases. *Gastroenterology* 2017; 17: 1–7.
 38. Dreesen E, Bossuyt P, Mulleman D, *et al*. Practical recommendations for the use of therapeutic drug monitoring of

- biopharmaceuticals in inflammatory diseases. *Clin Pharmacol Adv Appl* 2017; 9: 101–111.
39. Ward MG, Thwaites PA, Beswick L, *et al.* Intra-patient variability in adalimumab drug levels within and between cycles in Crohn's disease. *Aliment Pharmacol Ther* 2017; 45: 1135–1145.
40. Vande CN, Feagan BG, Gils A, *et al.* Therapeutic drug monitoring in inflammatory bowel disease: current state and future perspectives. *Curr Gastroenterol Rep* 2014; 16: 378.
41. Karmiris K, Paintaud G, Noman M, *et al.* Influence of trough serum levels and immunogenicity on long-term outcome of adalimumab therapy in Crohn's disease. *Gastroenterology* 2009; 137: 1628–1640.
42. Radstake TRDJ, Svenson M, Eijsbouts AM, *et al.* Formation of antibodies against infliximab and adalimumab strongly correlates with functional drug levels and clinical responses in rheumatoid arthritis. *Ann Rheum Dis* 1987; 68: 1739–1746.
43. Bartelds GM, Wijbrandts CA, Nurmohamed MT, *et al.* Clinical response to adalimumab: relationship to anti-adalimumab antibodies and serum adalimumab concentrations in rheumatoid arthritis. *Ann Rheum Dis* 2007; 66: 921–926.

Visit SAGE journals online
[journals.sagepub.com/
home/tag](http://journals.sagepub.com/home/tag)

 SAGE journals