

Effectiveness of the new generation transcatheter aortic valve in the real life studies. Review and meta-analysis

M.C. ACCONCIA¹, Q. CARETTA², L. MONZO¹, G. TANZILLI¹, A. SILI SCAVALLI³, D. SERGI⁴, M. DI LUOZZO⁴, M. MARCHEI⁴, M. CHIOCCHI⁵, F. ROMEO⁴, C. GAUDIO¹

¹Department of Cardiovascular Disease, "La Sapienza" University of Rome, Rome, Italy

²Department of Experimental and Clinical Medicine, University of Florence, Florence, Italy

³Department of Internal Medicine, "La Sapienza" University of Rome, Rome, Italy

⁴Department of Cardiovascular Disease, Tor Vergata University of Rome, Rome, Italy

⁵Department of Diagnostic Imaging, Molecular Imaging, Interventional Radiology and Radiotherapy, Tor Vergata University of Rome, Rome, Italy

Maria Cristina Acconcia and Quintilio Caretta are co-first authors

Abstract. – **OBJECTIVE:** The aim of the meta-analysis was to assess post-procedural outcome of the new generation of transcatheter aortic valve implantation (TAVI) devices, focusing on the transfemoral and balloon-expandable SAPIEN 3 (Edwards Lifesciences Inc., Irvine, CA, USA), the self-expanding CoreValve™ Evolut series R and PRO (R/PRO)™ (Medtronic Inc., Minneapolis, MN, USA) and ACURATE neo™ transcatheter aortic valve (Symetis SA, a Boston Scientific company, Ecublens, Switzerland).

MATERIALS AND METHODS: All observational studies were retrieved through PubMed computerized database from January 2014 until June 30th, 2019. The risk difference (RD) with the 95% confidence interval (CI) was used to assess the effectiveness of the intervention under comparison. The primary end point was 30-day mortality. Safety end points included: (i) stroke, (ii) moderate/severe paravalvular leak, and (iii) the need for new permanent pacemaker implantation.

RESULTS: Meta-analysis demonstrated no significant differences as regards to either 30-day mortality or stroke for all the groups of prostheses under comparison. ACURATE neo was associated with significantly less new permanent pacemaker implantation compared to SAPIEN 3 (RD: -0.06; 95% CI -0.08 to -0.03; $p < 0.0001$; $I^2 = 0\%$) or to EVOLUT R/PRO (RD: -0.06; 95% CI -0.09 to -0.02; $p = 0.0009$; $I^2 = 0\%$). A significant reduction of new permanent pacemaker need was observed in the group of patients implanted with SAPIEN 3 compared to EVOLUT R/PRO (RD: -0.07; 95% CI -0.09 to -0.04; $p < 0.00001$; $I^2 = 7\%$). The occurrence of moderate/severe leak was significantly increased in the group of patients implanted with ACURATE neo vs. SAPIEN 3 (RD:

0.04; 95% CI 0.02 to 0.05; $p < 0.00001$; $I^2 = 0\%$). No significant differences were found between ACURATE neo vs. EVOLUT R/PRO (RD: -0.01; 95% CI -0.04 to 0.02; $p = 0.69$; $I^2 = 0\%$) and between SAPIEN 3 vs. EVOLUT R/PRO (RD: -0.01; 95% CI -0.04 to 0.01; $p = 0.28$; $I^2 = 73\%$).

CONCLUSIONS: The results of the meta-analysis show that: (1) ACURATE neo was associated with significantly less new permanent pacemaker implantation than SAPIEN 3 and EVOLUT R/PRO; (2) SAPIEN 3 had significantly lower occurrence of moderate/severe valvular leak than ACURATE neo.

Key Words:

Transcatheter Aortic Valve Implantation, TAVI, TAVR, Aortic stenosis, Prosthetic aortic valves, Meta-analysis.

Introduction

Transcatheter aortic valve implantation (TAVI) is recognized as an effective therapy for the treatment of aortic stenosis in high, intermediate, and even low-risk operable patients^{1,2}.

Recent randomized trials of TAVI showed that, in patients who were at intermediate or high risk for death with surgery, TAVI was either superior or noninferior to standard therapies, including SAVR³⁻¹⁴.

As a result of continuous TAVI evolution, several new generation transcatheter heart valves have been developed incorporating features (i.e., lower profile, easier positioning, repositionability, and recoverability) addressed to minimize proce-

dural complications such as paravalvular regurgitation, valve malpositioning, vascular complications, and conduction disorders and to improve clinical outcomes¹⁵⁻¹⁷.

The aim of the meta-analysis was to compare the clinical outcome of the new generation transcatheter aortic valves, focusing on real life studies, either as a complement to Randomized Controlled Trials (RCTs), and to provide new insight on the “effectiveness” of the treatments administered in everyday clinical practice in patients with severe aortic stenosis, undergoing transfemoral TAVI.

Materials and Methods

This review and meta-analysis were performed in accordance with the PRISMA (Preferred Reporting Items for Systematic Reviews and Meta-Analyses) statement¹⁸.

Study Definition

We searched through PubMed computerized database for observational studies (Obs.) performing a direct comparison of almost two of the newest heart valves: the balloon-expandable SAPIEN 3 (Edwards Lifesciences Inc., Irvine, CA, USA), the self-expanding CoreValve™ Evolut series R, and PRO (R/PRO)™ (Medtronic Inc., Minneapolis, MN, USA) and ACURATE *neo*™ transcatheter aortic prosthesis (Symetis SA, a Boston Scientific company, Ecublens, Switzerland) in patients with severe aortic stenosis undergoing transfemoral TAVI. The reference lists of the retrieved full-text articles were also examined to identify potentially relevant studies not selected by the electronic search. The search was restricted to English-language journals. Studies on patients undergoing direct aortic or transapical TAVI were excluded. The search was performed from January 2014 to June 30th, 2019. Two investigators independently performed the eligibility screening with the aim to include only studies that report 30-day mortality and/or at least one of the safety endpoints under evaluation. In case of disagreement, consensus was obtained after consulting a third reviewer.

Outcomes

The primary end point was 30-day mortality. Safety end points included: (i) stroke, (ii) moderate/severe paravalvular leak, and (iii) the need for new permanent pacemaker implantation. In-

deed, to avoid risk of bias, due to unobserved or inaccurately measured confounders, we included in the meta-analysis the data related to the overall population of patients from the selected studies.

Statistical Analysis

The meta-analysis was performed using Review Manager (RevMan) [Computer program] Version 5.3. (Copenhagen: The Nordic Cochrane Centre, The Cochrane Collaboration, 2014) using the risk difference (RD) with the 95% Confidence Interval (CI), and the absolute risk reductions were calculated using the Mantel-Haenszel random-effect model to take into account possible heterogeneity among studies. We performed the analysis using the risk difference instead of the relative risk because the differences between the absolute risks give a better representation of the effectiveness of the interventions under comparison.

We evaluated the effectiveness of the prosthetic implanted valves by comparing the following groups of patients: (i) ACURATE *neo* vs. SAPIEN 3, (ii) ACURATE *neo* vs. EVOLUT R/PRO, and (iii) SAPIEN 3 vs. EVOLUT R/PRO.

A Forest plot was used for a graphical presentation of the results. The selected studies were examined to assess the homogeneity/heterogeneity of the results by visually inspecting the CIs of the risk estimates in the different studies and computing the Cochran's Q test and I^2 statistics¹⁹. A bidirectional α error of ≤ 0.05 was defined as statistically significant.

Results

Of 1,686 studies identified for screening, the systematic review selected 15 Obs.²⁰⁻³⁴ that meet the inclusion criteria and were included in the meta-analysis (Figure 1). The selected studies included 9,100 patients. Specifically, ACURATE *neo* was implanted in 2,294 patients, EVOLUT R/PRO in 2,742 patients and SAPIEN 3 in 4,064 patients (Table I). Six studies compared the ACURATE *neo* vs. SAPIEN 3²⁰⁻²⁴ and/or EVOLUT R/PRO^{21,24,25}, and 11 studies SAPIEN 3 vs. EVOLUT R/PRO^{21,24,26-34}. Two studies included all the TAVI valves under evaluation²¹⁻²⁴. The characteristics of the selected studies are reported in Table I.

Meta-analysis demonstrated no significant differences as regards to either 30-day mortality and stroke for all the groups of prostheses under comparison. In particular:

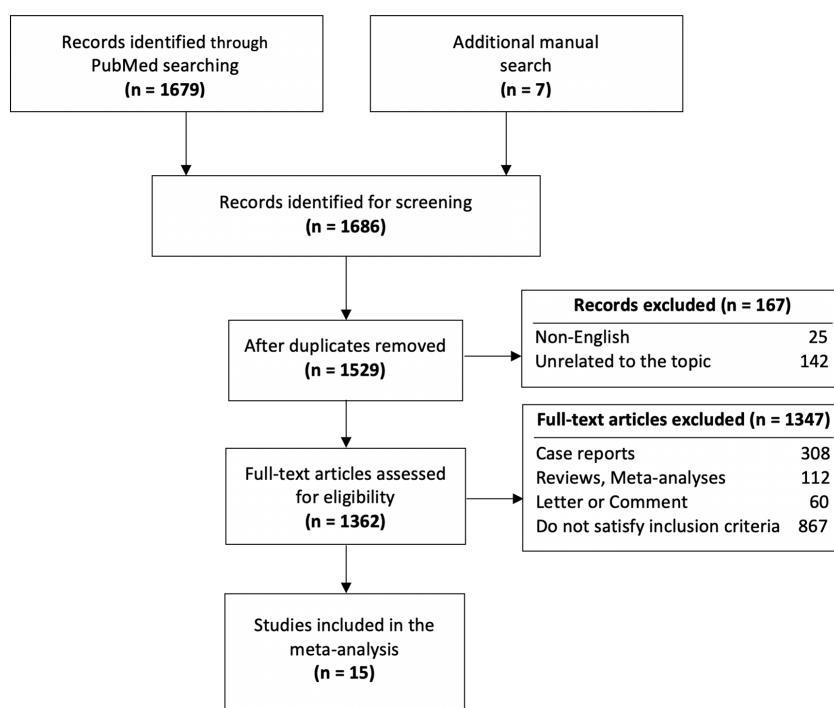


Figure 1. Flow-chart of the study selection process.

- *30-day mortality* was lower, non-significantly, in the comparison between SAPIEN 3 (RD: 0.01; 95% CI -0.01 to 0.02; $p=0.31$; $I^2=0\%$) or EVOLUT R/PRO (RD: 0.01; 95% CI -0.00 to 0.03; $p=0.12$; $I^2=0\%$) vs. the ACURATE *neo* (Figure 2). Again, a lower mortality, not significant, was observed in the comparison between SAPIEN 3 vs. EVOLUT R/PRO (RD -0.00; 95% CI -0.01 to 0.01; $p=0.59$; $I^2=0\%$) (Figure 2).
- *the occurrence of stroke* was similar in all the comparisons (Figure 3).

Indeed, the need for new permanent pacemaker implantation was significantly reduced in the patients implanted with ACURATE *neo* with respect to SAPIEN 3 (RD: -0.06; 95% CI -0.08 to -0.03; $p<0.0001$; $I^2=0\%$) and EVOLUT R/PRO (RD: -0.06; 95% CI -0.09 to -0.02; $p=0.0009$; $I^2=0\%$). A significant lower need for new permanent pacemaker was observed also in patients implanted with SAPIEN 3 compared to EVOLUT R/PRO (RD: -0.07; 95% CI -0.09 to -0.04; $p<0.00001$; $I^2=7\%$) (Figure 4).

On the contrary, the occurrence of moderate/severe postprocedural leak increased significant-

ly in the comparison between ACURATE *neo* vs. SAPIEN 3 (RD: 0.04; 95% CI 0.02 to 0.05; $p<0.00001$; $I^2=0\%$) (Figure 5). While the occurrence of postprocedural leak in the comparison between ACURATE *neo* vs. EVOLUT R/PRO was similar (RD: -0.01; 95% CI -0.04 to 0.02; $p=0.69$; $I^2=0\%$). Also, the comparison between SAPIEN 3 vs. EVOLUT R/PRO, did not show significant differences, but high heterogeneity ($I^2=73\%$) values were observed (Figure 5).

Discussion

The technological progress and the most accurate indications to TAVI have not completely solved the post-procedural adverse events, such as the need for new permanent pacemaker implantation³⁵, the periprosthetic leak^{31,36}, and stroke³⁷. New generation of TAVI devices have been designed to reduce the profile of the delivery catheter, enable repositioning and the ability to recover, facilitate the technical procedure, and reduce TAVI-related complications¹⁷. However, Evidence-Based Medicine and Clinical Research on their safety and

Table 1. Characteristics of the selected studies.

Study	Period	Country	Centre (n)	Design	Transcatheter heart valves				Pts included in the meta-analysis
					Self-expandable		Balloon-expandable		
					ACURATE neo	EVOLUT R	PRO	SAPIEN 3	
Ben-Shoshan et al, 2017 ²⁷	December 2014-April 2016	Israel	Single-centre	Retrospective study comparing short-term outcome of pts undergoing TF-TAVI with SAPIEN 3 and EVOLUT R valves.	108	124	232		
Husser et al, 2017 ²⁸	January 2014-January 2016	Germany	Multicentre	A registry-based study comparing THVs, SE ACURATE neo vs. BE SAPIEN 3, in terms of device failure and early safety at 30 days.	311	810	1121		
Kim et al, 2017 ²¹	January 2011-May 2017	Germany	Single-centre	Retrospective study comparing SE vs. BE THVs according to the degree of aortic valve calcification.	425	379	819		
Schaefer et al, 2017 ²³	2012-2016	Germany	Single-centre	Retrospective study aimed to compare acute 30-day outcomes of ACURATE neo vs. SAPIEN 3 THVs.	104	104	208		
Abdelghani et al, 2018 ²⁶ (CHOICE-Extend registry)	March 2014 - November 2017	Germany	Single-centre	A registry comparing new generation SE and BE THVs in large vs. small aortic valve annulus.	100	334	434		
Eitan et al, 2018 ²⁸	February 2014-August 2017	Germany	Single-centre	Short-term outcome in consecutive pts undergoing TF-TAVI with aortic annulus ≥ 26 mm.	37	55	92		
Enriquez-Rodriguez et al, 2018 ²⁹	Non reported	Spain	Two-centre	A case-matched cohort comparing the hemodynamic performance of SAPIEN 3 vs. EVOLUT R THVs.	64	80	144		
Gonska et al, 2018 ³⁰	February 2014-September 2016	Germany	Single-centre	The influence of new permanent pacemaker implantation on one year outcome in consecutive pts treated with new generation devices.	27	360	387		
Mauri et al, 2018 ²²	February 2014-August 2016	Germany	Multicentre	Retrospective study to identify predictors of paravalvular regurgitation and new permanent pacemaker implantation following TAVI with new generation THVs.	92	92	184		
Costa et al, 2019 ²⁴	June 2007-February 2018	Italy	Single-centre	Retrospective study designed to determine the appropriateness of new permanent pacemaker implantation after TAVI.	269	177	561		
Finkelstein et al, 2019 ³¹	February 2012-December 2016	Israel	Multicentre	A retrospective analysis on a large multicenter registry.	512	223	735		
Pagnesi et al, 2019 ²⁵ (NEOPRO registry)	January 2012-March 2018	Europe, Canada, USA	Multicentre	A retrospective multicenter registry comparing ACURATE neo vs. EVOLUT PRO THVs.	1263	288	1551		
Stundl et al, 2019 ³³	February 2008-September 2016	Germany	Single-centre	The degree of paravalvular aortic regurgitation in consecutive pts treated with "early" vs. "newer generation" of THVs.	114	101	215		
Veulemans et al, 2019 ³³	January 2014-September 2016	Germany	Single-centre	Retrospective analysis comparing quality, success rate, and costs between SAPIEN 3 and EVOLUT R.	101	103	204		
Vlastra et al, 2019 ³⁴	2007-2018	USA, Brazil, Israel, Europe	Multicentre	Data from 10 studies, selected through a systematic search, included in a combined dataset, pooled and analyzed in order to compare BE with SE valves.	1091	1122	2213		
Total number of implanted THVs					2294	2742	9100		

BE: Balloon-expandable; SE: Self-expandable; THVs: Transcatheter Heart Valves; TAVI: Transcatheter Aortic Valve Implantation; TF: Transfemoral; pts: patients.

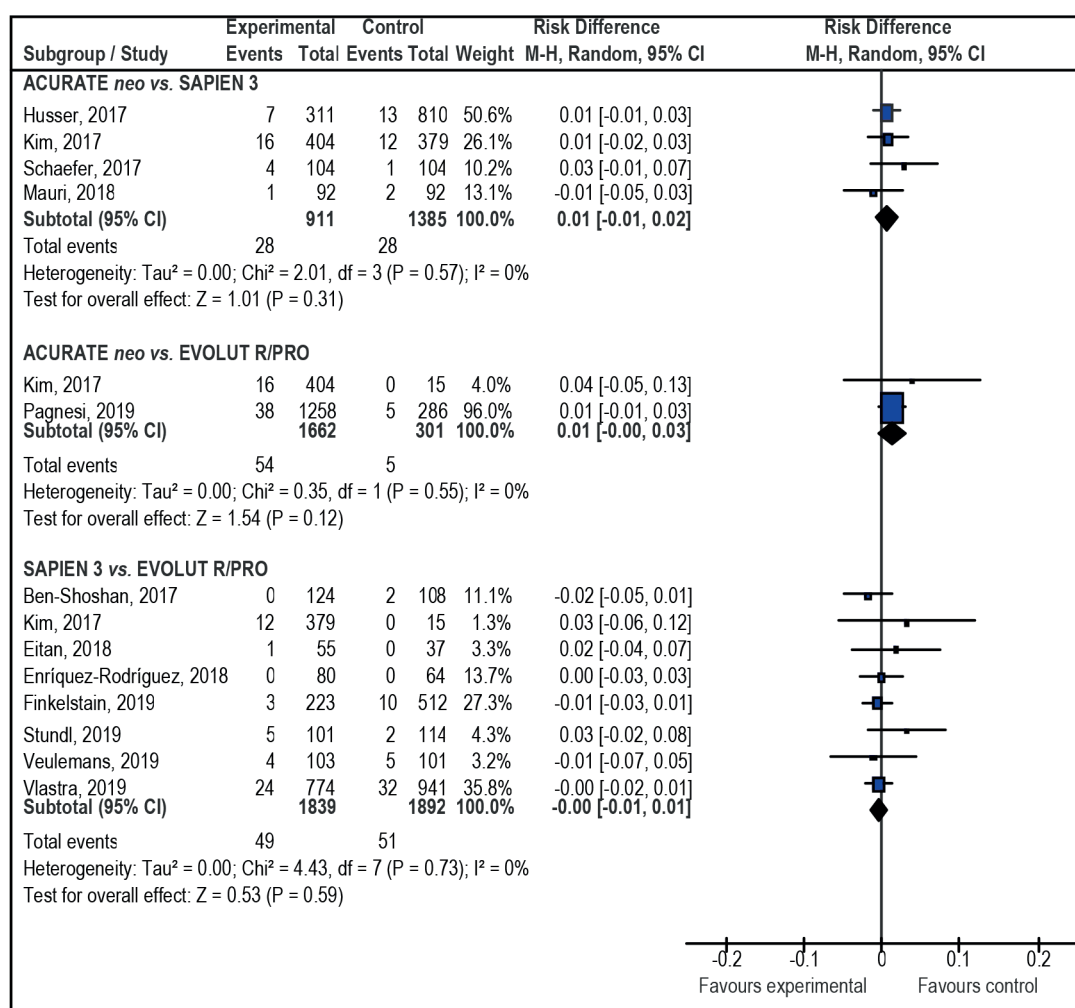


Figure 2. Mortality at 30-day. ACURATE neo vs. (i) SAPIEN 3, (ii) EVOLUT R/PRO. SAPIEN 3 vs. EVOLUT R/PRO.

effectiveness are limited and studies are mainly designed to compare the balloon-expandable vs. self-expandable valves without making a head-to-head comparison of the latest generation of prostheses^{26,34}. Three trials, the SCOPE I (ClinicalTrials.gov Identifier: NCT03011346), SCOPE II (ClinicalTrials.gov Identifier: NCT03192813), designed to perform an head-to-head comparison of the latest valve prostheses (ACURATE neo vs. SAPIEN 3 and ACURATE neo vs. EVOLUT R/PRO, respectively) and the ACURATE IDE (ClinicalTrials.gov Identifier: NCT03735667) designed to compare the ACURATE neo with Edwards SAPIEN 3 and Medtronic CoreValve Evolut R or Evolut PRO are still ongoing (see: <https://clinicaltrials.gov>). Therefore, due to the lack of RCTs, we designed our meta-analysis to evaluate 30-day mortality and postprocedural adverse events in

some new TAVI devices as SAPIEN 3, EVOLUT series (R/PRO) and the ACURATE neo from the real world observational data. Indeed Obs. can provide information on the daily clinical practice in the overall population undergoing transfemoral TAVI without rigorous exclusion criteria.

The main finding from our meta-analysis comes from: (i) a significant lower need for new pacemaker implantation in the group of patients implanted with ACURATE neo compared to SAPIEN 3 ($p < 0.0001$) and EVOLUT R/PRO ($p = 0.0009$) and, (ii) a significant higher postprocedural leak in the group of patients implanted with ACURATE neo compared to SAPIEN 3 ($p < 0.00001$).

SAPIEN 3 and EVOLUT R/PRO heart valves did not show differences in the incidence of leak after TAVI (Figure 5). However, a higher occur-

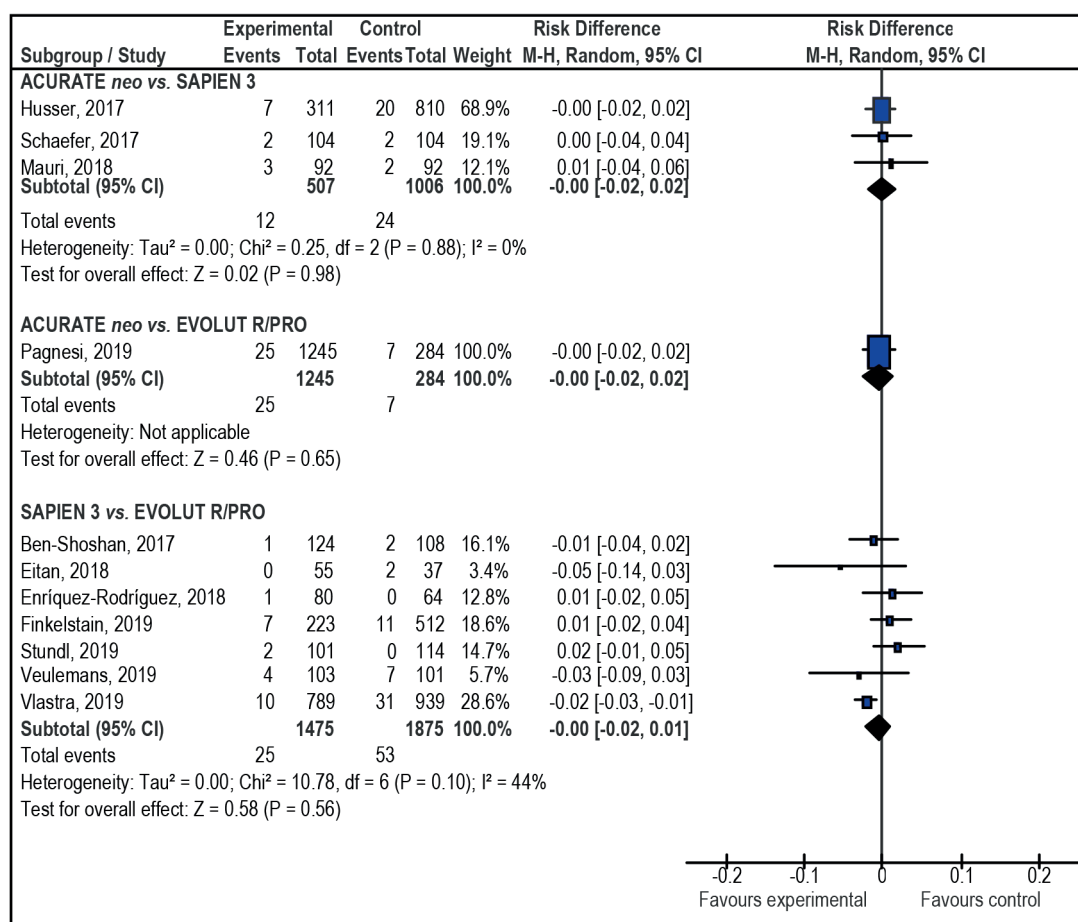


Figure 3. Incidence of stroke.

rence of new permanent pacemaker implantation was observed in the group of patients implanted with the EVOLUT R/PRO valve ($p < 0.00001$) (Figure 4).

Moreover, we have to emphasize that: (i) we included in the meta-analysis all data available from Obs., (ii) patient population were homogeneous each other, as demonstrated by the I² statistics equal to 0 in many comparisons (Figure 2-5).

Indeed, despite the risks of bias due to unmeasured confounders, Obs. often provide the best available evidence of treatment effectiveness³⁸. Anglemeyer et al³⁹, analyzing the impact of the study design, Obs. vs. RCTs, on the estimate of the measure of effect, found that there was increasing evidence that in most cases RCTs and non-randomized studies yielded similar findings, when the studies had homogeneous data.

Furthermore, we can witness the evolution of clinical research every day. Thus, it can be ob-

served that the acceptance of observational data occurs more and more frequently, both through the use of the registry and through the implementation of capillary networks that record the daily clinical practice⁴⁰.

In conclusion our findings, showing adverse outcomes related to the need for new permanent pacemaker implantation and the occurrence of postprocedural moderate/severe aortic insufficiency, could be related to the structural diversity of valve prostheses. However, the issue seems to remain unresolved and warrants further investigations.

Our meta-analysis, based on data from Obs., could overestimate the treatments effect due to the lack of randomization^{41,42}. RCTs on efficacy of the new generation of TAVI devices, considered a key tool for comparative effectiveness research, are still recruiting. Their findings may help provide answers to the limitations of Obs.

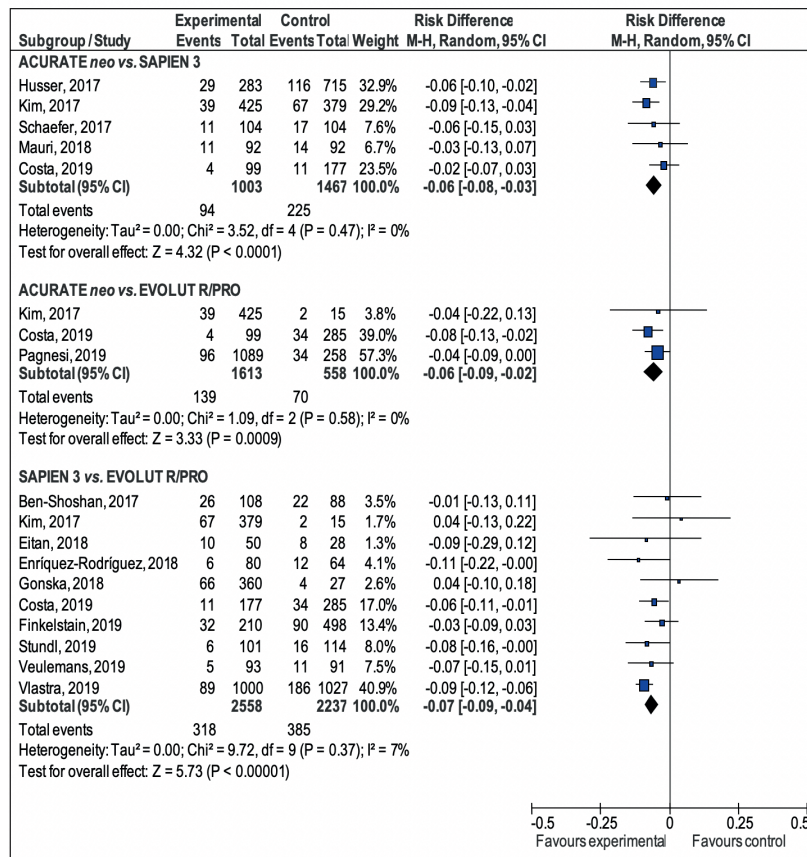


Figure 4. The need for new permanent pacemaker implantation.

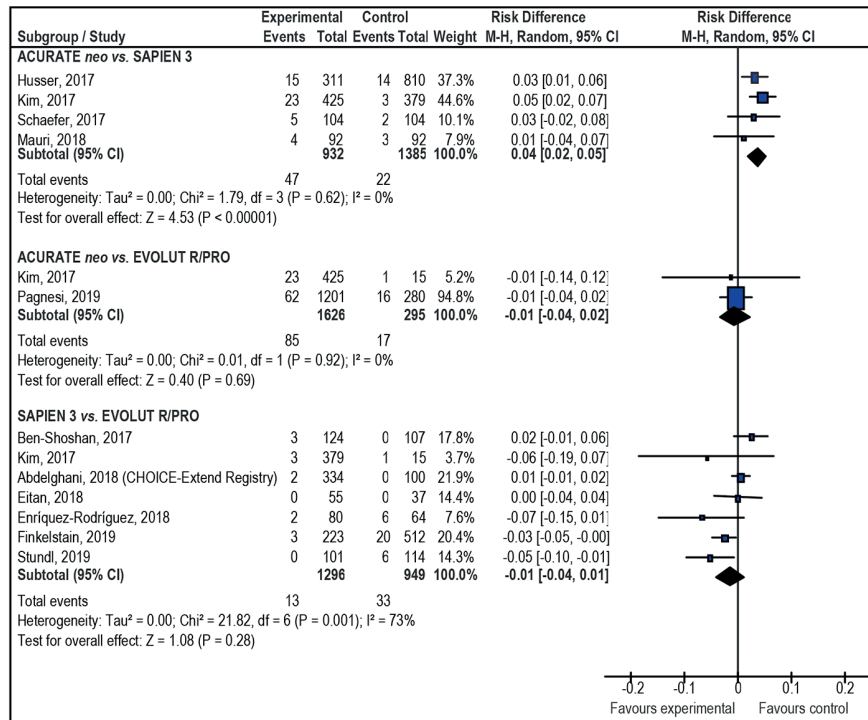


Figure 5. Incidence of moderate/severe paravalvular leak.

Conclusions

The meta-analysis shows that: (i) ACURATE *neo* required significant less new permanent post-procedural pacemaker implantation than SAPIEN 3 and EVOLUT R/PRO, (ii) SAPIEN 3 had significant lower occurrence of moderate/severe valvular leak than ACURATE *neo*.

Conflict of interest

The authors declare no conflicts of interest.

References

- MACK MJ, HOLMES DR, WEBB J, CRIBIER A, KODALI SK, WILLIAMS MR, LEON MB. Patient selection for transcatheter aortic valve replacement. *J Am Coll Cardiol* 2013; 62 (17 Suppl): S1-10.
- SERGI D, ACCONCIA MC, MUSCOLI S, PERRONE MA, CAMMALLERI V, DI LUOZZO M, MARCHEI M, GIANNONI MF, BARILLA F, GAUDIO C, CHIOCCHI M, ROMEO F, CARETTA O. Meta-analysis of the impact on early and late mortality of TAVI compared to surgical aortic valve replacement in high and low-intermediate surgical risk patients. *Eur Rev Med Pharmacol Sci* 2019; 23: 5402-5412.
- LEON MB, SMITH CR, MACK M, MILLER DC, MOSES JW, SVENSSON LG, TUZCU EM, WEBB JG, FONTANA GP, MAK-KAR RR, BROWN DL, BLOCK PC, GUYTON RA, PICHARD AD, BAVARIA JE, HERRMANN HC, DOUGLAS PS, PETERS-EN JL, AKIN JJ, ANDERSON WN, WANG D, POCOCK S; PARTNER Trial Investigators. Transcatheter aortic-valve implantation for aortic stenosis in patients who cannot undergo surgery. *N Engl J Med* 2010; 363: 1597-1607.
- SMITH CR, LEON MB, MACK MJ, MILLER DC, MOSES JW, SVENSSON LG, TUZCU EM, WEBB JG, FONTANA GP, MAK-KAR RR, WILLIAMS M, DEWEY T, KAPADIA S, BABALIAROS V, THOURANI VH, CORSO P, PICHARD AD, BAVARIA JE, HERRMANN HC, AKIN JJ, ANDERSON WN, WANG D, POCOCK SJ; PARTNER Trial Investigators. Transcatheter versus surgical aortic-valve replacement in high-risk patients. *N Engl J Med* 2011; 364: 2187-2198.
- LEON MB, SMITH CR, MACK MJ, MAK-KAR RR, SVENSSON LG, KODALI SK, THOURANI VH, TUZCU EM, MILLER DC, HERRMANN HC, DOSHI D, COHEN DJ, PICHARD AD, KAPADIA S, DEWEY T, BABALIAROS V, SZETO WY, WILLIAMS MR, KEREIAKES D, ZAJARIAS A, GREASON KL, WHISENANT BK, HODSON RW, MOSES JW, TRENTO A, BROWN DL, FEARON WF, PIBAROT P, HAHN RT, JABER WA, ANDERSON WN, ALU MC, WEBB JG; PARTNER 2 Investigators. Transcatheter or surgical aortic-valve replacement in intermediate-risk patients. *N Engl J Med* 2016; 374: 1609-1620.
- KAPADIA SR, LEON MB, MAK-KAR RR, TUZCU EM, SVENSSON LG, KODALI S, WEBB JG, MACK MJ, DOUGLAS PS, THOURANI VH, BABALIAROS VC, HERRMANN HC, SZETO WY, PICHARD AD, WILLIAMS MR, FONTANA GP, MILLER DC, ANDERSON WN, AKIN JJ, DAVIDSON MJ, SMITH CR; PARTNER trial investigators. 5-year outcomes of transcatheter aortic valve replacement compared with standard treatment for patients with inoperable aortic stenosis (PARTNER 1): a randomised controlled trial. *Lancet* 2015; 385: 2485-2491.
- MACK MJ, LEON MB, SMITH CR, MILLER DC, MOSES JW, TUZCU EM, WEBB JG, DOUGLAS PS, ANDERSON WN, BLACKSTONE EH, KODALI SK, MAK-KAR RR, FONTANA GP, KAPADIA S, BAVARIA J, HAHN RT, THOURANI VH, BABALIAROS V, PICHARD A, HERRMANN HC, BROWN DL, WILLIAMS M, AKIN J, DAVIDSON MJ, SVENSSON LG; PARTNER 1 trial investigators. 5-year outcomes of transcatheter aortic valve replacement or surgical aortic valve replacement for high surgical risk patients with aortic stenosis (PARTNER 1): a randomised controlled trial. *Lancet* 2015; 385: 2477-2484.
- WEBB JG, DOSHI D, MACK MJ, MAK-KAR R, SMITH CR, PICHARD AD, KODALI S, KAPADIA S, MILLER DC, BABALIAROS V, THOURANI V, HERRMANN HC, BODENHAMER M, WHISENANT BK, RAMEE S, MANIAR H JR, KEREIAKES D, XU K, JABER WA, MENON V, TUZCU EM, WOOD D, SVENSSON LG, LEON MB. A randomized evaluation of the SAPIEN XT transcatheter heart valve system in patients with aortic stenosis who are not candidates for surgery. *JACC Cardiovasc Interv* 2015; 8: 1797-1806.
- THOURANI VH, KODALI S, MAK-KAR RR, HERRMANN HC, WILLIAMS M, BABALIAROS V, SMALLING R, LIM S, MALAISRIE SC, KAPADIA S, SZETO WY, GREASON KL, KEREIAKES D, AILAWADI G, WHISENANT BK, DEVIREDDY C, LEIPSIK J, HAHN RT, PIBAROT P, WEISSMAN NJ, JABER WA, COHEN DJ, SURI R, TUZCU EM, SVENSSON LG, WEBB JG, MOSES JW, MACK MJ, MILLER DC, SMITH CR, ALU MC, PARVATANENI R, D'AGOSTINO RB JR, LEON MB. Transcatheter aortic valve replacement versus surgical valve replacement in intermediate-risk patients: a propensity score analysis. *Lancet* 2016; 387: 2218-2225.
- POPMA JJ, ADAMS DH, REARDON MJ, YAKUBOV SJ, KLEIMAN NS, HEIMANSOHN D, HERMILLER J JR, HUGHES GC, HARRISON JK, COSELLI J, DIEZ J, KAFI A, SCHREIBER T, GLEASON TG, CONTE J, BUCHBINDER M, DEEB GM, CARABELLO B, SERRUYS PW, CHENOWETH S, OH JK; CoreValve United States Clinical Investigators. Transcatheter aortic valve replacement using a self-expanding bioprosthesis in patients with severe aortic stenosis at extreme risk for surgery. *J Am Coll Cardiol* 2014; 63: 1972-1981.
- ADAMS DH, POPMA JJ, REARDON MJ. Transcatheter aortic-valve replacement with a self-expanding prosthesis. *N Engl J Med* 2014; 371: 967-968.
- REARDON MJ, VAN MIEGHEM NM, POPMA JJ, KLEIMAN NS, SØNDERGAARD L, MUMTAZ M, ADAMS DH, DEEB GM, MAINI B, GADA H, CHETCUTI S, GLEASON T, HEISER J, LANGE R, MERHI W, OH JK, OLSEN PS, PIAZZA N, WILLIAMS M, WINDECKER S, YAKUBOV SJ, GRUBE E, MAK-KAR R, LEE JS, CONTE J, VANG E, NGUYEN H, CHANG Y, MUGGLIN AS, SERRUYS PW, KAPPETEIN AP; SURTAVI Investigators. Surgical or transcatheter aortic-valve replacement in intermediate-risk patients. *N Engl J Med* 2017; 376: 1321-1331.
- GLEASON TG, REARDON MJ, POPMA JJ, DEEB GM, YAKUBOV SJ, LEE JS, KLEIMAN NS, CHETCUTI S, HERMILLER

- ER JB JR, HEISER J, MERHI W, ZORN GL 3RD, TADROS P, ROBINSON N, PETROSSIAN G, HUGHES GC, HARRISON JK, CONTE JV, MUMTAZ M, OH JK, HUANG J, ADAMS DH; CoreValve U.S. Pivotal High Risk Trial Clinical Investigators. 5-Year outcomes of self-expanding transcatheter versus surgical aortic valve replacement in high-risk patients. *J Am Coll Cardiol* 2018; 72: 2687-2696.
- 14) PETRONIO AS, CAPRANZANO P, BARBATO E, PIAZZA N, BAUMBACH A, HAUDE M, WINDECKER S. Current status of transcatheter valve therapy in Europe: results from an EAPCI survey. *EuroIntervention* 2016; 12: 890-895.
 - 15) CAHILL TJ, CHEN M, HAYASHIDA K, LATIB A, MODINE T, PIAZZA N, REDWOOD S, SØNDERGAARD L, PRENDERGAST BD. Transcatheter aortic valve implantation: current status and future perspectives. *Eur Heart J*. 2018; 39: 2625-2634.
 - 16) TCHETCHE D, VAN MIEGHEM NM. New-generation TAVI devices: description and specifications. *EuroIntervention* 2014; 10 Suppl U: U90-U100.
 - 17) VAN GILS L, TCHETCHE D, LATIB A, SGROI C, MANOHARAN G, MÖLLMANN H, VAN MIEGHEM NM. TAVI with current CE-marked devices: strategies for optimal sizing and valve delivery. *EuroIntervention* 2016; 12: Y22-Y27.
 - 18) MOHER D, LIBERATI A, TETZLAFF J, ALTMAN DG; PRISMA group. Preferred reporting items for systematic reviews and meta-analyses: the PRISMA statement. *J Clin Epidemiol* 2009; 62: 1006-1012.
 - 19) HIGGINS JPT, GREEN S (EDITORS). *Cochrane Handbook for Systematic Reviews of Interventions* Version 5.1.0 [updated March 2011]. The Cochrane Collaboration, 2011. Available from www.handbook.cochrane.org.
 - 20) HUSSER O, KIM WK, PELLEGRINI C, HOLZAMER A, WALTHER T, MAYR PN, JONER M, KASEL AM, TRENKWALDER T, MICHEL J, RHEUDE T, KASTRATI A, SCHUNKERT H, BURGDORF C, HILKER M, MÖLLMANN H, HENGSTENBERG C. Multi-center comparison of novel self-expanding versus balloon-expandable transcatheter heart valves. *JACC Cardiovasc Interv* 2017; 10: 2078-2087.
 - 21) KIM WK, BLUMENSTEIN J, LIEBETRAU C, ROLF A, GAEDE L, VAN LINDEN A, ARSALAN M, DOSS M, TUSSEN JGP, HAMM CW, WALTHER T, MÖLLMANN H. Comparison of outcomes using balloon-expandable versus self-expanding transcatheter prostheses according to the extent of aortic valve calcification. *Clin Res Cardiol* 2017; 106: 995-1004.
 - 22) MAURI V, DEUSCHL F, FROHN T, SCHOFFER N, LINDER M, KUHN E, SCHAEFER A, RUDOLPH V, MADERSHAHIAN N, CONRADI L, RUDOLPH TK, SCHÄFER U. Predictors of paravalvular regurgitation and permanent pacemaker implantation after TAVR with a next-generation self-expanding device. *Clin Res Cardiol* 2018; 107: 688-697.
 - 23) SCHAEFER A, LINDER M, SEIFFERT M, SCHOEN G, DEUSCHL F, SCHOFFER N, SCHNEEBERGER Y, BLANKENBERG S, REICHENSPURNER H, SCHAEFER U, CONRADI L. Comparison of latest generation transfemoral self-expandable and balloon-expandable transcatheter heart valves. *Interact Cardiovasc Thorac Surg* 2017; 25: 905-911.
 - 24) COSTA G, ZAPPULLA P, BARBANTI M, CIRASA A, TODARO D, RAPISARDA G, PICCI A, PLATANIA F, TOSTO A, DI GRAZIA A, SGROI C, TAMBURINO C, CALVI V. Pacemaker dependency after transcatheter aortic valve implantation: incidence, predictors and long-term outcomes. *EuroIntervention* 2019 Jun 18. pii: EIJ-D-18-01060. [Epub ahead of print]
 - 25) PAGNESI M, KIM WK, CONRADI L, BARBANTI M, STEFANINI GG, ZEUS T, PILGRIM T, SCHOFFER J, ZWEIKER D, TESTA L, TARAMASSO M, HILDICK-SMITH D, ABIZAID A, WOLF A, VAN MIEGHEM NM, SEDAGHAT A, WÖHRLE J, KHOGALI S, VAN DER HEYDEN JAS, WEBB JG, ESTÉVEZ-LOUREIRO R, MYLOTTE D, MACCARTHY P, BRUGALETTA S, HAMM CW, BHADRA OD, SCHÄFER U, COSTA G, TAMBURINO C, CANNATA F, REIMERS B, VEULEMANS V, ASAMI M, WINDECKER S, EITAN A, SCHMIDT A, BIANCHI G, BEDOGNI F, SACCOCCI M, MAISANO F, ALSANJARI O, SIQUEIRA D, JENSEN CJ, NABER CK, ZIVIELLO F, SINNING JM, SEEGER J, ROTTBAUER W, BROUWER J, ALENEZI A, WOOD DA, TZALAMOURAS V, REGUEIRO A, COLOMBO A, LATIB A. Transcatheter aortic valve replacement with next-generation self-expanding devices: a multicenter, retrospective, propensity-matched comparison of Evolut PRO versus accurate neo transcatheter heart valves. *JACC Cardiovasc Interv* 2019; 12: 433-443.
 - 26) ABDELGHANI M, MANKERIOUS N, ALLALI A, LANDT M, KAUR J, SULIMOV DS, MERTEN C, SACHSE S, MEHILLI J, NEUMANN FJ, FRERKER C, KURZ T, EL-MAWARDY M, RICHARDT G, ABDEL-WAHAB M. Bioprosthetic valve performance after transcatheter aortic valve replacement with self-expanding versus balloon-expandable valves in large versus small aortic valve annuli: insights from the CHOICE trial and the CHOICE-extend registry. *JACC Cardiovasc Interv* 2018; 11: 2507-2518.
 - 27) BEN-SHOSHAN J, KONIGSTEIN M, ZÄHLER D, MARGOLIS G, CHORIN E, STEINVIL A, ARBEL Y, AVIRAM G, GRANOT Y, BARKAGAN M, KEREN G, HALKIN A, BANAI S, FINKELSTEIN A. Comparison of the Edwards SAPIEN S3 versus medtronic Evolut-R devices for transcatheter aortic valve implantation. *Am J Cardiol* 2017; 119: 302-307.
 - 28) EITAN A, WITT J, STRIPLING J, HASELBACH T, RIESS FC, SCHOFFER J. Performance of the Evolut-R 34 mm versus Sapien-3 29 mm in transcatheter aortic valve replacement patients with larger annuli: early outcome results of Evolut-R 34 mm as compared with Sapien-3 29 mm in patients with Annuli ≥ 26 mm. *Catheter Cardiovasc Interv* 2018; 92: 1374-1379.
 - 29) ENRÍQUEZ-RODRÍGUEZ E, AMAT-SANTOS IJ, JIMÉNEZ-QUEVEDO P, MARTÍN-MORQUECHO I, TIRADO-CONTE G, PÉREZ-VIZCAYNO MJ, GÓMEZ DE DIEGO JJ, ARNOLD R, ALDABAL A, ROJAS P, DE AGUSTÍN A, DEL TRIGO M, GUTIÉRREZ H, SAN ROMÁN JA, MACAYA C, NOMBELA-FRANCO L. Comparison of the hemodynamic performance of the balloon-expandable SAPIEN 3 versus self-expandable Evolut R transcatheter valve: a case-matched study. *Rev Esp Cardiol (Engl Ed)* 2018; 71: 735-742.
 - 30) GONSKA B, KESSLER M, WÖHRLE J, ROTTBAUER W, SEEGER J. Influence of permanent pacemaker implantation

- after transcatheter aortic valve implantation with new-generation devices. *Neth Heart J* 2018; 26: 620-627.
- 31) FINKELSTEIN A, STEINVIL A, ROZENBAUM Z, HALKIN A, BANAI S, BARBASH I, GUETTA V, SEGEV A, DANENBERG H, ORVIN K, ASSA HV, ASSALI A, KORNOWSKI R. Efficacy and safety of new-generation transcatheter aortic valves: insights from the Israeli transcatheter aortic valve replacement registry. *Clin Res Cardiol* 2019; 108: 430-437.
 - 32) STUNDL A, LUCHT H, SHAMEKHI J, WEBER M, SEDAGHAT A, MELLERT F, GRUBE E, NICKENIG G, WERNER N, SINNING JM. Early versus newer generation transcatheter heart valves for transcatheter aortic valve implantation: echocardiographic and hemodynamic evaluation of an all-comers study cohort using the dimensionless aortic regurgitation index (AR-index). *PLoS One* 2019; 14: e0217544.
 - 33) VEULEMANS V, PIAYDA K, AFZAL S, POLZIN A, QUAST C, JUNG C, WESTENFELD R, ZEUS T, KELM M, HELLHAMMER K. Cost-comparison of third generation transcatheter aortic valve implantation (TAVI) devices in the German Health Care System. *Int J Cardiol* 2019; 278: 40-45.
 - 34) VLASTRA W, CHANDRASEKHAR J, MUÑOZ-GARCIA AJ, TCHÉTCHÉ D, DE BRITO FS JR, BARBANTI M, KORNOWSKI R, LATIB A, D'ONOFRIO A, RIBICHINI F, BAAN J, TIJSSEN JGP, TRILLO-NOUCHE R, DUMONTEIL N, ABIZAID A, SARTORI S, D'ERRIGO P, TARANTINI G, LUNARDI M, ORVIN K, PAGNESI M, DEL VALLE R, MODINE T, DANGAS G, MEHRAN R, PIEK JJ, DELEWI R. Comparison of balloon-expandable vs. self-expandable valves in patients undergoing transfemoral transcatheter aortic valve implantation: from the CENTER-collaboration. *Eur Heart J* 2019; 40: 456-465.
 - 35) MANGIERI A, MONTALTO C, PAGNESI M, LANZILLO G, DEMIR O, TESTA L, COLOMBO A, LATIB A. TAVI and post procedural cardiac conduction abnormalities. *Front Cardiovasc Med* 2018; 5: 85. doi: 10.3389/fcvm.2018.00085
 - 36) WILCZEK K, BUJAK K, REGUŁA R, CHODÓR P, OSADNIK T. Risk factors for paravalvular leak after transcatheter aortic valve implantation. *Kardiochir Torakochirurgia Pol* 2015; 12: 89-94.
 - 37) VLASTRA W, JIMENEZ-QUEVEDO P, TCHÉTCHÉ D, CHANDRASEKHAR J, DE BRITO FS JR, BARBANTI M, KORNOWSKI R, LATIB A, D'ONOFRIO A, RIBICHINI F, BAAN J, TIJSSEN JGP, DE LA TORRE HERNANDEZ JM, DUMONTEIL N, SARMENTO-LEITE R, SARTORI S, ROSATO S, TARANTINI G, LUNARDI M, ORVIN K, PAGNESI M, HERNANDEZ-ANTOLIN R, MODINE T, DANGAS G, MEHRAN R, PIEK JJ, DELEWI R. Predictors, incidence, and outcomes of patients undergoing transfemoral transcatheter aortic valve implantation complicated by stroke. *Circ Cardiovasc Interv* 2019; 12: e007546.
 - 38) BLONDE L, KHUNTI K, HARRIS SB, MEIZINGER C, SKOLNIK NS. Interpretation and impact of real-world clinical data for the practicing clinician. *Adv Ther* 2018; 35: 1763-1774.
 - 39) ANGLEMYER A, HORVATH HT, BERO L. Healthcare outcomes assessed with observational study designs compared with those assessed in randomized trials. *Cochrane Database Syst Rev* 2014; MR000034. doi: 10.1002/14651858.MR000034.pub2.
 - 40) TAVAZZI L. Big data: is clinical practice changing? *Eur Heart J Suppl* 2019; 21 (Suppl B): B98-B102.
 - 41) SATURNI S, BELLINI F, BRAIDO F, PAGGIARO P, SANDUZZI A, SCICHLONE N, SANTUS PA, MORANDI L, PAPI A. Randomized controlled trials and real life studies. Approaches and methodologies: a clinical point of view. *Pulm Pharmacol Ther* 2014; 27: 129-138.
 - 42) SØRENSEN HT, LASH TL, ROTHMAN KJ. Beyond randomized controlled trials: a critical comparison of trials with nonrandomized studies. *Hepatology* 2006; 44: 1075-1082.