

# Northumbria Research Link

Citation: Nouredanesh, Mina, Godfrey, Alan, Howcroft, Jennifer, Lemaire, Edward and Tung, James (2021) Fall risk assessment in the wild: A critical examination of wearable sensor use in free-living conditions. *Gait & Posture*, 85. pp. 178-190. ISSN 0966-6362

Published by: Elsevier

URL: <https://doi.org/10.1016/j.gaitpost.2020.04.010> <<https://doi.org/10.1016/j.gaitpost.2020.04.010>>

This version was downloaded from Northumbria Research Link:  
<http://nrl.northumbria.ac.uk/id/eprint/42712/>

Northumbria University has developed Northumbria Research Link (NRL) to enable users to access the University's research output. Copyright © and moral rights for items on NRL are retained by the individual author(s) and/or other copyright owners. Single copies of full items can be reproduced, displayed or performed, and given to third parties in any format or medium for personal research or study, educational, or not-for-profit purposes without prior permission or charge, provided the authors, title and full bibliographic details are given, as well as a hyperlink and/or URL to the original metadata page. The content must not be changed in any way. Full items must not be sold commercially in any format or medium without formal permission of the copyright holder. The full policy is available online: <http://nrl.northumbria.ac.uk/policies.html>

This document may differ from the final, published version of the research and has been made available online in accordance with publisher policies. To read and/or cite from the published version of the research, please visit the publisher's website (a subscription may be required.)



UniversityLibrary



**Northumbria**  
**University**  
NEWCASTLE

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

# Fall risk assessment in the wild: A critical examination of wearable sensors use in free-living conditions

Mina Nouredanesh<sup>1\*†</sup>, Alan Godfrey<sup>2†</sup>, Jennifer Howcroft<sup>3</sup>, Edward D Lemaire<sup>4,5</sup> and James Tung<sup>1</sup>

<sup>1</sup> Department of Mechanical and Mechatronics Engineering, University of Waterloo, 200, University Ave. W, Waterloo, Canada

<sup>2</sup> Department of Computer & Information Science, Northumbria University, 2 Ellison Pl, Newcastle upon Tyne, UK.

<sup>3</sup> Department of Systems Design Engineering, University of Waterloo, 200 University Ave., Waterloo, Canada.

<sup>4</sup> Ottawa Hospital Research Institute, Centre for Rehabilitation, Research and Development, Ottawa, Canada.

<sup>5</sup> Faculty of Medicine, University of Ottawa, Ottawa, Canada.

† Equal contributor

**\* Correspondence:**

Mina Nouredanesh

Department of Mechanical and Mechatronics Engineering,

University of Waterloo, 200,

University Ave. W,

Waterloo, Canada

Email: [m2noured@uwaterloo.ca](mailto:m2noured@uwaterloo.ca)

1  
2  
3  
4 **Abstract**  
5  
6

7 **Background:** Despite advances in laboratory-based supervised fall risk assessment  
8 methods (FRAs), falls still remain a major public health problem. This can be due to the  
9 alteration of behavior in laboratory due to the awareness of being observed (i.e., Hawthorne  
10 effect), the multifactorial complex etiology of falls, and our limited understanding of human  
11 behaviour in natural environments, or in the 'wild'. To address these imitations, a growing  
12 body of literature has focused on free-living wearable-sensor-based FRAs. The objective of  
13 this narrative literature review is to discuss papers investigating natural data collected by  
14 wearable sensors for a duration of at least 24 hours to identify fall-prone older adults.  
15  
16  
17  
18  
19  
20  
21

22  
23 **Methods:** Databases (Scopus, PubMed and Google Scholar) were systematically searched for  
24 studies based on a rigorous search strategy.  
25  
26  
27

28 **Results:** The search yielded twenty-four studies, in which inertial sensors were the only  
29 wearable system employed for FRA in the wild. Gait was the most-investigated activity; but  
30 sitting, standing, lying, transitions and gait events, such as turns and missteps, were also  
31 explored. A multitude of free-living fall predictors (FLFPs), e.g., the quantity of daily steps,  
32 were extracted from activity bouts and events. FLFPs were further categorized into discrete  
33 domains (e.g., pace, complexity) defined by conceptual or data-driven models. Heterogeneity  
34 was found within the reviewed studies, which includes variance in: terminology (e.g.,  
35 quantity vs macro), hyperparameters to define/estimate FLFPs, models and domains, and  
36 data processing approaches (e.g., the cut-off thresholds to define an ambulatory bout). These  
37 inconsistencies led to different results for similar FLFPs, limiting the ability to interpret and  
38 compare the evidence.  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49

50 **Conclusion:** Free-living FRA is a promising avenue for fall prevention. Achieving a  
51 harmonized model is necessary to systematically address the inconsistencies in the field and  
52 identify FLFPs with the highest predictive values for falls to eventually address intervention  
53 programs and fall prevention.  
54  
55  
56  
57

58 **Keywords:** Falls in elderly; inertial measurement unit; wearable sensors; ambulatory fall risk assessment;  
59 free-living fall predictors  
60  
61  
62  
63  
64  
65

## 1.0 Introduction

It is estimated that 1 in 3 people globally over the age of 65 fall at least once each year [1], [2]. In addition to physical consequences (e.g., hip fracture, traumatic brain injury), falls can lead to negative mental health outcomes such as fear of falling and depression [3]. Falls among older adults tend to occur from multiple interacting factors [4], generally categorized as intrinsic/biological (e.g., a neurological mechanism or chronic condition such as Parkinson's disease, PD, muscle weakness), and extrinsic/environmental (e.g., slippery floor, obstacles, slopes, poor lighting) [5], [6], [7]. By identifying the various risks specific to an individual, fall risk assessment (FRA) can inform clinical decisions on the most appropriate preventive interventions to reduce the risk for fall events. To date, commonly used FRA methods involve easy-to-implement movement-based tasks with minimal equipment requirements, such as total time to complete a timed-up-and-go (TUG) [8], [9] or Tinetti Test [10]. Based on a meta-analysis, the diagnostic accuracy of TUG was poor to moderate for fall prediction in healthy high-functioning older adults and the cut-off thresholds for TUG-based identification of fallers were highly inconsistent within the included studies [11]. These limitations have led to a methodological shift towards the use of more detailed assessments. As the adopted gold standard, electronic-based tools, such as 3-dimensional motion capture and instrumented walkways, can be used to offer detailed quantitative assessments. Yet, these tools remain resource-intensive and fixed to specialized clinics/locations, offering snapshots during scripted functional tasks. Extrinsic risk factors for falls can be also recorded in (patient) self-reported diaries; however, this often lacks accuracy and adequate descriptions. To systematically investigate the impact of environmental conditions on older adults' tendency to fall, researchers have designed paradigms to mimic challenging natural conditions in a laboratory setting. For example, minimum foot clearance was measured in different lighting conditions in [12] to understand the nature of trips on stairs in older adults, where, in contrast to young adults, the lack of precautionary increase in older adults' foot clearance under reduced lighting contributed to falls on stairs. However, due to the observer effect during controlled gait and balance tests [13], supervised FRA measures may not necessarily reflect naturalistic and multitasking behaviour [14]–[16]. For instance, a weak association ( $r = 0.333$ ,  $p < 0.001$ ) between natural gait speed and in-laboratory gait speed was reported [17]. Similarly, free-living gait speed and step regularity measures were

1  
2  
3  
4 significantly lower compared with in-lab usual walking and tended to be more similar to in-  
5 lab dual-task walking [15]. Thus, novel free-living FRAs to identify fallers based on their free-  
6 living behaviour in their natural daily living environments could provide complementary  
7 information to supervised FRAs.  
8  
9

10  
11  
12 There have been a wide range of methods investigated to measure free-living mobility  
13 behaviour. Ambient sensors, such as radar [18], passive infrared [19], third-person video,  
14 and depth cameras [20]–[23] have been investigated as a means to extract gait parameters,  
15 detect falls, and track longitudinal changes in a person's mobility patterns. However, ambient  
16 sensors have limitations due to visual occlusions (e.g., furniture), inability to extract  
17 spatiotemporal data when full-body view is unavailable, and tracking the same person in  
18 spaces with multiple residents with similar body characteristics [24]. Moreover, they are  
19 restricted to the environments the sensors are installed in. In contrast, wearable sensors and  
20 their data have greater utility beyond the living space where ambient sensor data is recorded  
21 at the expense of additional burden in donning and maintaining devices. These technologies  
22 include wearables inertial sensors (e.g., accelerometers, gyroscopes, magnetometers), in-  
23 shoe plantar pressure sensors [25]–[27] and wearable cameras [28], [29].  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33

34 Recent attention has focused on the identification of free-living fall predictors (FLFPs)  
35 from wearable-based data, such as total time walking/lying, frequency-based (e.g., the  
36 amplitude of dominant frequency) and temporal (e.g., step time) measures extracted from  
37 detected activity bouts (e.g., gait) and events (e.g., turns), towards profiling an individual's  
38 risk for falls. Several studies have shown that wearable-based FLFPs can either outperform  
39 or complement clinical (supervised) FRA tests [30]–[32]. For instance, a machine learning-  
40 based model developed on transition-based FLFPs outperformed its counterpart developed  
41 on clinical test scores (e.g., TUG) in discriminating between older fallers and non-fallers [30].  
42 While this body of evidence has demonstrated promise, there is a high degree of  
43 inconsistency in the literature regarding the relationship between the extracted FLFPs and  
44 falls. Inconsistencies were also observed in data-driven and conceptual models proposed by  
45 the research groups to categorize FLFPs into domains (e.g., pace, asymmetry). At this time,  
46 due to the ongoing novel developments within the field, there are no clear solutions for  
47 transparent deployment of wearables for free-living FRA. Furthermore, the utility of existing  
48 free-living FRA methods to inform interventions remains limited, largely due to challenges  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65


1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

interpreting unconventional metrics of free-living behaviour (e.g., entropy). After summarizing the key aspects of the experimental protocols used to collect free-living data (e.g., sensor placement, duration of free-living data collection, demographics), the current paper reviews sources of inconsistencies between the proposed free-living FRA approaches. At the end, recommendations were provided to inform future work towards achieving a harmonized free-living FRA model.

**2.0 Search criteria**

Three databases, Scopus, PubMed, and Google Scholar, were searched up to and including September 2019 (2010 to 2019). Search terms were ["home" or "unsupervised" or "real-world" or "community" or "ambulatory"] and ["fall" or "fall risk assessment"] and ["elderly" or "senior" or "aged"] and ["wearable sensor" or "accelerometers" or "inertial" or "wearable camera"]. Journal articles were included if they: 1) assessed the relationships between falls and features extracted from free-living data, and 2) collected data from wearables used by older adults (> 65 years) for a duration of at least 24 hours per participant. After the initial title screen, abstracts were reviewed. Twenty six (n=26) papers from databases met the inclusion criteria (Figure 1). Multiple papers from two research groups investigated the same/overlapping datasets or very similar sets of FLFPs: (a) Hausdorff and colleagues examined datasets from healthy older adults [32]–[35] and PD older adults [36], [37], and (b) Pijnappels and colleagues investigated: b-1. fall risk assessment in older adults (FARAO) dataset that was collected from >300 older adults [38]–[40], and b-2. overlapping (but different) subsets of FARAO dataset to address different research questions [16], [31], [41], [42]. Considering the high degree of overlap in b-2, the most relevant, largest sample, and/or highly cited paper examining fall risk was included for the purposes of this review [31] and [42] (see Figure 1). Therefore, the key methodological/demographic information from n=24 papers was extracted and provided in Tables 1-3 (the key aspects of [16] and [41] were highlighted in section 4).

1  
2  
3  
4  
5 ["home" OR "unsupervised" OR "real-world" OR "community" OR "ambulatory"] AND ["fall" OR  
6 "fall risk assessment"] AND ["elderly" OR "senior" OR "aged"] AND ["wearable sensor" OR  
7 "accelerometers" OR "inertial" OR "wearable camera"]

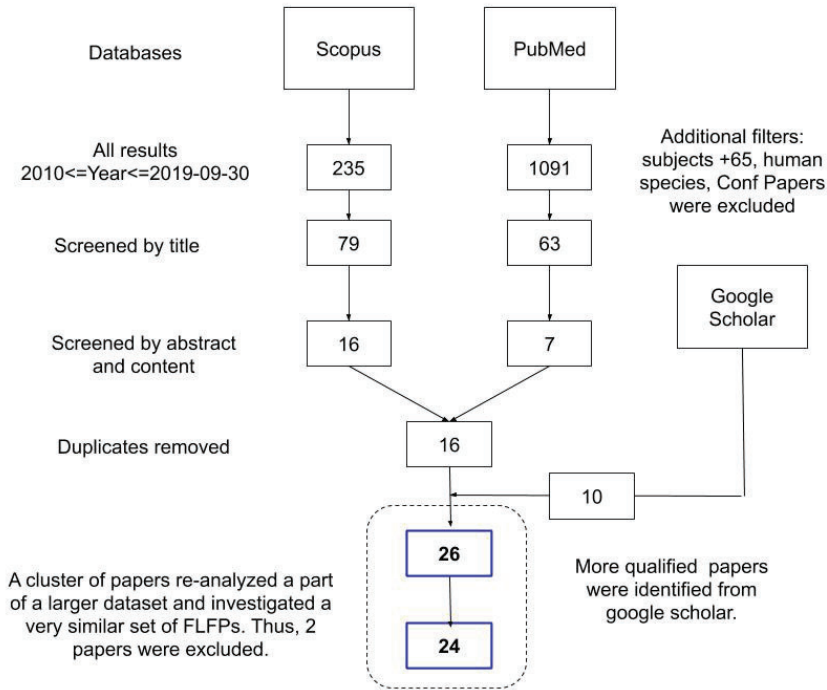

32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

Figure 1: PRISMA flow chart of study design, illustrating search strategy results and filters at each stage of the study selection process.

### 3.0 Results

#### 3.1 Study characteristics


Tables 1-3 show the study designs for capturing free-living data, demographic information, key methodological aspects, types of wearables, sensor anatomical location, general description of outcome measures, and the length of free-living recording for all included papers. The general procedure for wearable-based ambulatory FRA is shown in Figure 2.

In the reviewed studies, a range of inertial-based wearables were employed as described in Table 3. Most studies used a single tri-axial accelerometer-based wearable, with a minority using a uniaxial [43][44] or combined tri-axial accelerometer and tri-axial gyroscope (e.g., [30] [45]). Typically, one inertial-based wearable was worn on the lower back, including the pelvis, sacrum, and L3 to L5 vertebrae [30], [32], [42], [46], [47], [33]-[40], and midsagittal plane of the lower back [45]. Other wearable locations included chest/sternum [48]-[51], middle of the thigh [44], upper-thigh [43] dominant and



1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

nondominant hand/wrist [52]. In one study, multiple wearables were attached, two on shoes and one at L5 [53]. Free-living data were recorded from 24 hours [51] to 58 days (average over participants) in [48]. Most studies monitored community-dwelling older adults without neurological disorders (i.e., OA in Table 2). However, a number of studies also investigated differences between fallers and non-fallers in other populations: PD [36], [37], [43], [44], [46], dementia [51], [54], and varying frailty levels [50]. Additionally, fallers were further categorized as single fallers and recurrent fallers in two papers [43], [53].

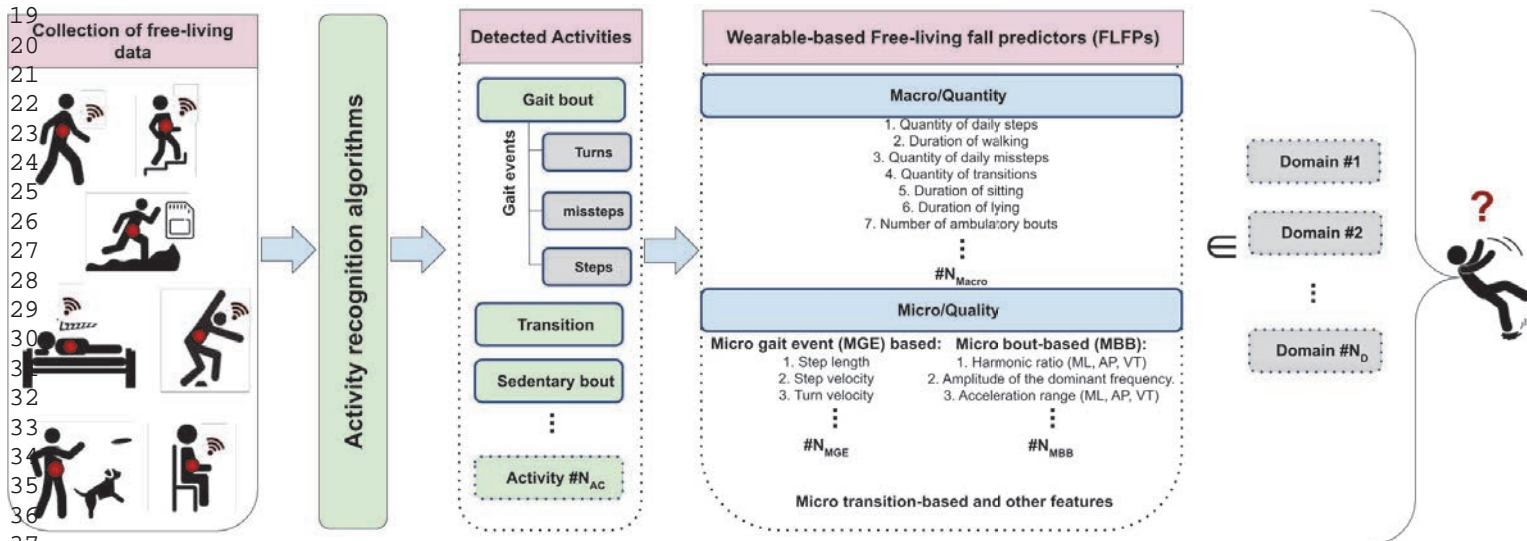

**Figure 2: General process flow to acquire, process, and extract predictors for free-living fall risk assessment. Free-living data are collected using wearable sensors, segmented into bouts of activity types (e.g., gait, sitting), then predictors are extracted from activity bouts. There is a high degree of inconsistency in the literature in the categorization of extracted predictors into free-living FRA domains (dashed boxes).**

Studies performed analysis to understand the relationships between wearable-based FLFPs and prospective falls [38], [39], [43], [50]–[52], [54], retrospective falls [30], [32]–[34], [36], [37], [44], [46], [47], [49], and both [42], [45], [53]. Falls were also categorized with respect to the associated pre-fall events and allocated to one of three categories: 1) transitions during changes of posture (e.g., turning, rising from chair); 2) ambulation (e.g., everyday walking activities, including stair climbing) and 3) advanced activities including complex high-risk motor tasks (e.g., skiing, hill walking) in one study [43]. Multivariate analysis or deep learning techniques were also applied to discriminate between fallers and non-fallers [39], [40], [54] without corresponding univariate analysis to investigate the individual FLFPs with respect to their predictive ability for falls.

1  
2  
3  
4  
5  
6 <Table 1>

7 <Table 2>

8 <Table 3>

### 3.2 Free-living activity/event detection

15  
16  
17 Detecting bouts of activity were critical step in extracting FLFPs. The detection of ambulatory  
18 bouts were most common [30], [32], [44]–[51], [53], [33]–[35], [38]–[40], [42], [43] followed  
19 by, sitting [38], [42], [50], [51], lying [38], [42], [50], [51], sedentary (sitting and lying  
20 together) [44], [45], and standing [38], [42], [44], [50], [51]. Bout of activity detection was  
21 the initial methodological step required for the extraction of FLFPs from inertial sensor data  
22 (Figure 2). Transitions between consecutive ambulatory and sedentary bouts (i.e., walk-to-  
23 sit and sit-to-walk) were also quantified for insights to FRA [30], [38], [42], [50], [52].

24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65  
66  
67  
68  
69  
70  
71  
72  
73  
74  
75  
76  
77  
78  
79  
80  
81  
82  
83  
84  
85  
86  
87  
88  
89  
90  
91  
92  
93  
94  
95  
96  
97  
98  
99  
100  
101  
102  
103  
104  
105  
106  
107  
108  
109  
110  
111  
112  
113  
114  
115  
116  
117  
118  
119  
120  
121  
122  
123  
124  
125  
126  
127  
128  
129  
130  
131  
132  
133  
134  
135  
136  
137  
138  
139  
140  
141  
142  
143  
144  
145  
146  
147  
148  
149  
150  
151  
152  
153  
154  
155  
156  
157  
158  
159  
160  
161  
162  
163  
164  
165  
166  
167  
168  
169  
170  
171  
172  
173  
174  
175  
176  
177  
178  
179  
180  
181  
182  
183  
184  
185  
186  
187  
188  
189  
190  
191  
192  
193  
194  
195  
196  
197  
198  
199  
200  
201  
202  
203  
204  
205  
206  
207  
208  
209  
210  
211  
212  
213  
214  
215  
216  
217  
218  
219  
220  
221  
222  
223  
224  
225  
226  
227  
228  
229  
230  
231  
232  
233  
234  
235  
236  
237  
238  
239  
240  
241  
242  
243  
244  
245  
246  
247  
248  
249  
250  
251  
252  
253  
254  
255  
256  
257  
258  
259  
260  
261  
262  
263  
264  
265  
266  
267  
268  
269  
270  
271  
272  
273  
274  
275  
276  
277  
278  
279  
280  
281  
282  
283  
284  
285  
286  
287  
288  
289  
290  
291  
292  
293  
294  
295  
296  
297  
298  
299  
300  
301  
302  
303  
304  
305  
306  
307  
308  
309  
310  
311  
312  
313  
314  
315  
316  
317  
318  
319  
320  
321  
322  
323  
324  
325  
326  
327  
328  
329  
330  
331  
332  
333  
334  
335  
336  
337  
338  
339  
340  
341  
342  
343  
344  
345  
346  
347  
348  
349  
350  
351  
352  
353  
354  
355  
356  
357  
358  
359  
360  
361  
362  
363  
364  
365  
366  
367  
368  
369  
370  
371  
372  
373  
374  
375  
376  
377  
378  
379  
380  
381  
382  
383  
384  
385  
386  
387  
388  
389  
390  
391  
392  
393  
394  
395  
396  
397  
398  
399  
400  
401  
402  
403  
404  
405  
406  
407  
408  
409  
410  
411  
412  
413  
414  
415  
416  
417  
418  
419  
420  
421  
422  
423  
424  
425  
426  
427  
428  
429  
430  
431  
432  
433  
434  
435  
436  
437  
438  
439  
440  
441  
442  
443  
444  
445  
446  
447  
448  
449  
450  
451  
452  
453  
454  
455  
456  
457  
458  
459  
460  
461  
462  
463  
464  
465  
466  
467  
468  
469  
470  
471  
472  
473  
474  
475  
476  
477  
478  
479  
480  
481  
482  
483  
484  
485  
486  
487  
488  
489  
490  
491  
492  
493  
494  
495  
496  
497  
498  
499  
500  
501  
502  
503  
504  
505  
506  
507  
508  
509  
510  
511  
512  
513  
514  
515  
516  
517  
518  
519  
520  
521  
522  
523  
524  
525  
526  
527  
528  
529  
530  
531  
532  
533  
534  
535  
536  
537  
538  
539  
540  
541  
542  
543  
544  
545  
546  
547  
548  
549  
550  
551  
552  
553  
554  
555  
556  
557  
558  
559  
560  
561  
562  
563  
564  
565  
566  
567  
568  
569  
570  
571  
572  
573  
574  
575  
576  
577  
578  
579  
580  
581  
582  
583  
584  
585  
586  
587  
588  
589  
590  
591  
592  
593  
594  
595  
596  
597  
598  
599  
600  
601  
602  
603  
604  
605  
606  
607  
608  
609  
610  
611  
612  
613  
614  
615  
616  
617  
618  
619  
620  
621  
622  
623  
624  
625  
626  
627  
628  
629  
630  
631  
632  
633  
634  
635  
636  
637  
638  
639  
640  
641  
642  
643  
644  
645  
646  
647  
648  
649  
650  
651  
652  
653  
654  
655  
656  
657  
658  
659  
660  
661  
662  
663  
664  
665  
666  
667  
668  
669  
670  
671  
672  
673  
674  
675  
676  
677  
678  
679  
680  
681  
682  
683  
684  
685  
686  
687  
688  
689  
690  
691  
692  
693  
694  
695  
696  
697  
698  
699  
700  
701  
702  
703  
704  
705  
706  
707  
708  
709  
710  
711  
712  
713  
714  
715  
716  
717  
718  
719  
720  
721  
722  
723  
724  
725  
726  
727  
728  
729  
730  
731  
732  
733  
734  
735  
736  
737  
738  
739  
740  
741  
742  
743  
744  
745  
746  
747  
748  
749  
750  
751  
752  
753  
754  
755  
756  
757  
758  
759  
760  
761  
762  
763  
764  
765  
766  
767  
768  
769  
770  
771  
772  
773  
774  
775  
776  
777  
778  
779  
780  
781  
782  
783  
784  
785  
786  
787  
788  
789  
790  
791  
792  
793  
794  
795  
796  
797  
798  
799  
800  
801  
802  
803  
804  
805  
806  
807  
808  
809  
810  
811  
812  
813  
814  
815  
816  
817  
818  
819  
820  
821  
822  
823  
824  
825  
826  
827  
828  
829  
830  
831  
832  
833  
834  
835  
836  
837  
838  
839  
840  
841  
842  
843  
844  
845  
846  
847  
848  
849  
850  
851  
852  
853  
854  
855  
856  
857  
858  
859  
860  
861  
862  
863  
864  
865  
866  
867  
868  
869  
870  
871  
872  
873  
874  
875  
876  
877  
878  
879  
880  
881  
882  
883  
884  
885  
886  
887  
888  
889  
890  
891  
892  
893  
894  
895  
896  
897  
898  
899  
900  
901  
902  
903  
904  
905  
906  
907  
908  
909  
910  
911  
912  
913  
914  
915  
916  
917  
918  
919  
920  
921  
922  
923  
924  
925  
926  
927  
928  
929  
930  
931  
932  
933  
934  
935  
936  
937  
938  
939  
940  
941  
942  
943  
944  
945  
946  
947  
948  
949  
950  
951  
952  
953  
954  
955  
956  
957  
958  
959  
960  
961  
962  
963  
964  
965  
966  
967  
968  
969  
970  
971  
972  
973  
974  
975  
976  
977  
978  
979  
980  
981  
982  
983  
984  
985  
986  
987  
988  
989  
990  
991  
992  
993  
994  
995  
996  
997  
998  
999  
1000

Ambulatory bouts were further examined for detection of discrete gait events (Figure 2) such as initial and final contact within the gait cycle (e.g., in [32], [38], [42], [47], turns [45], [53], and missteps [37]. Missteps were broadly defined to include compensatory balance reactions (i.e., near-falls) to regain stability following a loss of balance.

#### 3.2.1. Cut-off thresholds for identification of ambulatory bouts and turns

To identify an ambulatory bout, different minimum/maximum cut-off thresholds were defined according to steps, time or a combination of both [46], [48], [49] (Table 3). For example, Del Din et al. [46] referred to an ambulatory bout between 3 steps to 60s, 60-120s, and longer than 120s as 'short', 'medium', and 'long' walks, respectively. Alternatively, Brodie et al. considered short walks as those <7s and <8s and longer than three steps in two different studies [48], [49]. The minimum cut-off thresholds ranged from 1 step [43] to 120s [46] and a minimum of three steps was the most frequent cut-off threshold used within the reviewed studies from distinct datasets [46], [48]–[51]. Discrete angular thresholds were also used to identify turns. For instance, one study [53] examined those greater than 45° but elsewhere different turn resolutions, e.g. small (50 – 100°), medium (100 – 150°), and large (150 – 200°) were taken into account [45], Table 3. The detected activity bouts and

1  
2  
3  
4 events were later used independently for the extraction of FLFPs, which were statistically  
5 analyzed with respect to falls (Figure 2).  
6  
7  
8

### 9 10 **3.3. Conceptual models**

11 As ambulatory bouts were the most investigated free-living activity for FRA, research groups  
12 defined different conceptual FRA models to classify and interpret a range of gait-based  
13 FLFPs. Each model consists of several domains, including a homogeneous group of FLFPs  
14 usually in terms of their mathematical description (Figure 3, models a [46], b [48], c [49], d  
15 [42], and e). Model e represents the merged domains from a set of research papers [32]–  
16 [34], [36] as discussed in section 2. In Figure 3-model e, complexity and local dynamic  
17 stability measures reported in [33], [34] were categorized into the same class because of  
18 their mathematical similarities (e.g., Lyapunov components [55]).  
19  
20  
21  
22  
23  
24  
25

26 Broadly speaking, the reviewed literature examined the following features:

- 27 (1) the ‘quantity’ of gait events or ambulatory bouts and their duration over days/weeks  
28 [32], [36], [48], [49] also termed ‘macro’ (as discussed in 3.3.1) [43], [44], [46] and  
29 ‘amount of gait’ [38], [42],  
30  
31  
32
- 33 (2) FLFPs that are obtained by performing a higher resolution analysis of the inertial  
34 signals or gait events, which include spatial (e.g. step length), temporal (step time),  
35 and frequency-based (e.g. harmonic ratio) features. These features termed as ‘micro’  
36 (referring to more detailed micro-structural characteristics of gait as discussed in  
37 3.3.2) [46] [44] [43] (Figure 3 model a) or ‘quality’ of gait (e.g. in [32], [36], [38], [42],  
38 [48], [49] (Figure 3),  
39  
40  
41  
42  
43  
44
- 45 (3) models of quantity/quality also extended to categorize turns [45], [53] and transition  
46 features [30], [52].  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

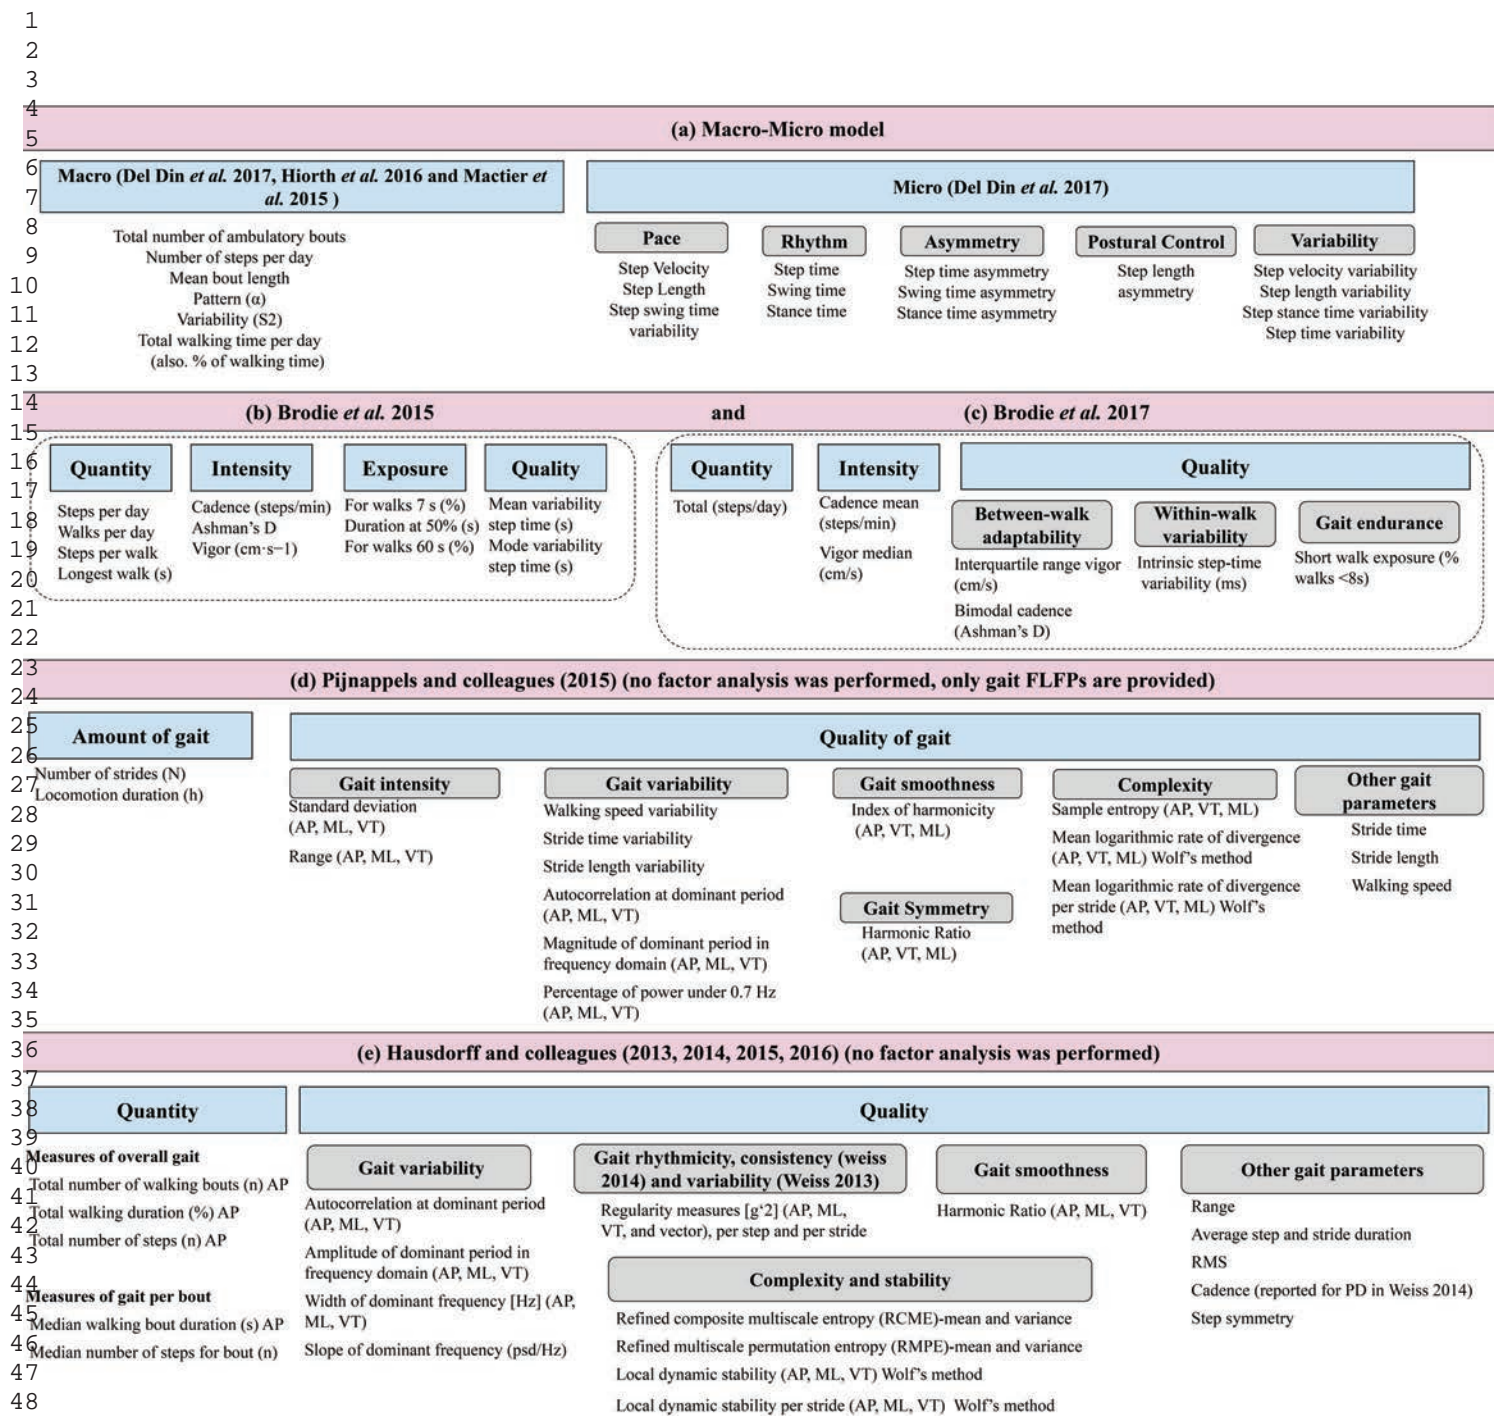


Figure 3: Conceptual models proposed by researchers to categorize gait-related features for fall risk assessment

As depicted in Figure 3-model d [42], gait quality was represented by six domains, each with its own set of FLFPs, such as: intensity (e.g., standard deviation, range); variability (e.g., autocorrelation, slope, magnitude); smoothness (e.g. index of harmonicity) and complexity (sample entropy). Alternatively, quality was presented within quantity-intensity-exposure-quality models (Figure 3, model b) and quantity-intensity-quality

1  
2  
3  
4 (Figure 3-model c) comprising of different predictors within three domains (e.g., between-  
5 walk adaptability). Due to these inconsistencies associated with the use of 'quality', here the  
6 general categorization of FLFPs into macro and micro is used to describe quantity and  
7 quality of activities, respectively.  
8  
9

### 10 11 12 13 **3.3.1 Macro/quantity FLFPs**

14  
15 Macro outcomes were generally described by duration or volume of an activity or the  
16 quantity of daily occurrences. Commonly used macro FLFPs include the number of  
17 ambulatory bouts [38], [42]–[44], [48], total steps within each bout [32], [36], [38], [42],  
18 [48], number of daily turns [45], [53], number of daily compensatory balance reactions [37],  
19 and number of transfers/transitions [30], [38], [42], [50], [52]. In addition to the  
20 aforementioned linear features, macro outcomes were utilized for non-linear analyses [43],  
21 [44], [46] (Figure 3-model a), including: 1. alpha ( $\alpha$ ), which is a unit-less FLFP derived from  
22 the power distribution of ambulatory bouts with respect to the cut-off thresholds and 2.  
23 within subject variability of bout length ( $S_2$ ) obtained from a maximum likelihood technique  
24 as the distribution of bout length.  
25  
26

27  
28 For sedentary (lying and sitting) and standing bouts, only macro features were  
29 investigated within studies [38], [42]–[45], [50], [51], which includes: total standing time  
30 [38], [42], [50], [51], total sedentary time [38], [42], [45], [50], [51], lying, sitting, and  
31 standing bout duration (mean, maximum, and 90th percentile) [50], [51], standing and  
32 sedentary bout duration variability [43], [44], number of sedentary and standing bouts [44],  
33 and alpha measures for sedentary and standing bouts [44].  
34  
35

### 36 37 38 39 40 41 42 43 44 45 46 **3.3.2 Micro/quality FLFPs**

47  
48 Considering micro FLFPs that were investigated in studies, we categorized micro features  
49 into three main classes to aid consistency:  
50

- 51  
52 1. Micro gait event-based (MGE) FLFPs represent features requiring detection of gait  
53 events from ambulatory bouts in order to be quantified. For example, turn duration  
54 [45], [53] and step/stride length (e.g., examined in [38], [42], [46]) require detection  
55 of a gait event, such as turn and foot contacts, respectively. Consequently, established  
56 spatiotemporal gait parameters are generally considered as the MGE features,  
57  
58  
59  
60  
61  
62  
63  
64  
65

1  
2  
3  
4 including stance time, double support, step length. Turn-based MGEs were  
5 investigated in [45], [53], and they included mean turn velocity, peak turn velocity,  
6 turn duration, variability of turn duration, mean turn angle, turn angle variability and  
7 the logarithm of normalized jerk.  
8  
9

- 10  
11  
12  
13 2. Micro ambulatory bout-based (MBB) outcomes include high-level temporal (e.g., root  
14 mean square) and frequency-based (e.g., mean logarithmic rate of divergence) FLFPs  
15 [32], [38], [42], [47] extracted from either the detected ambulatory bouts (based on  
16 the cut-off thresholds discussed in 3.2.1) or the subsequent epochs (discussed later),  
17 regardless of the enclosed gait events. MBB predictors were either direction-  
18 dependent features or based on signal vector magnitude. Directionally-dependent  
19 FLFPs were extracted from antero-posterior (AP), mediolateral (ML), vertical (VT)  
20 accelerations (e.g. regularity measures in [32], [36]). A number of FLFPs were  
21 extracted from the signal vector magnitude associated with the bout or epoch,  
22 including regularity measure [47], phase-dependent generalized multiscale entropy  
23 [40], and phase-dependent local dynamic stability [33]). To avoid possible sample  
24 size-related bias, each axial/signal vector segment attributed to a macro bout was  
25 split into fixed-size epochs for some studies. For example, bouts longer than 10sec  
26 and 60sec were split into the fixed 10 sec [47] and 50 s [34] epochs, respectively, and  
27 each epoch was used separately for the extraction of MBB outcomes.  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40

41 MBB features are less intuitive compared to spatiotemporal gait FLFPs; and  
42 are assumed to be indicative of different aspects of gait based on their mathematical  
43 description. For instance, slope, width, and amplitude of the dominant frequency in  
44 acceleration epochs were linked to variability of gait domain [32], [36], [38], [42], [47]  
45 and entropy measures (e.g., sample entropy [42], multiscale and phase-dependant  
46 entropy [34], [40]), were commonly extracted as potential markers of complexity  
47 domain (in [34] a lower entropy extracted from acceleration signals was linked to  
48 loss of complexity and an increased regularity).  
49  
50  
51  
52  
53  
54  
55

- 56 3. Micro-transitions: similar to MBB predictors, these FLFPs consist of high-level  
57 temporal (e.g., peak velocity, range) or frequency-based (e.g. entropy) outcomes,  
58 which were either direction dependent (i.e., roll, pitch, yaw [30], [52]), or extracted  
59  
60  
61  
62  
63  
64  
65

from the signal vector magnitude (e.g. jerk [52]) attributed to sit-to-walk (or stand) and walk (or stand)-to-sit transitions.

### 3.4 Data-driven models

One study presented a data-driven model by performing factor analysis to systematically categorize FLFPs into independent domains. In [38] principal component analysis (PCA) was performed on 75 outcomes including: *macro* (e.g., median number of strides in one ambulatory bout); MGE (e.g., stride time, stride length variability); MBB (e.g., mean logarithmic rate of divergence), and several questionnaire-based and test outcomes (e.g., inability to use public transportation, ability to ascend/descend stairs). Although PCA revealed 18 domains, wearable-based FLFPs were only loaded into 8 classes (considering their 3 highest weights that exceeded 0.3) as shown in Figure 4-model f.

f. Data-driven model by van Schooten *et al.* 2016

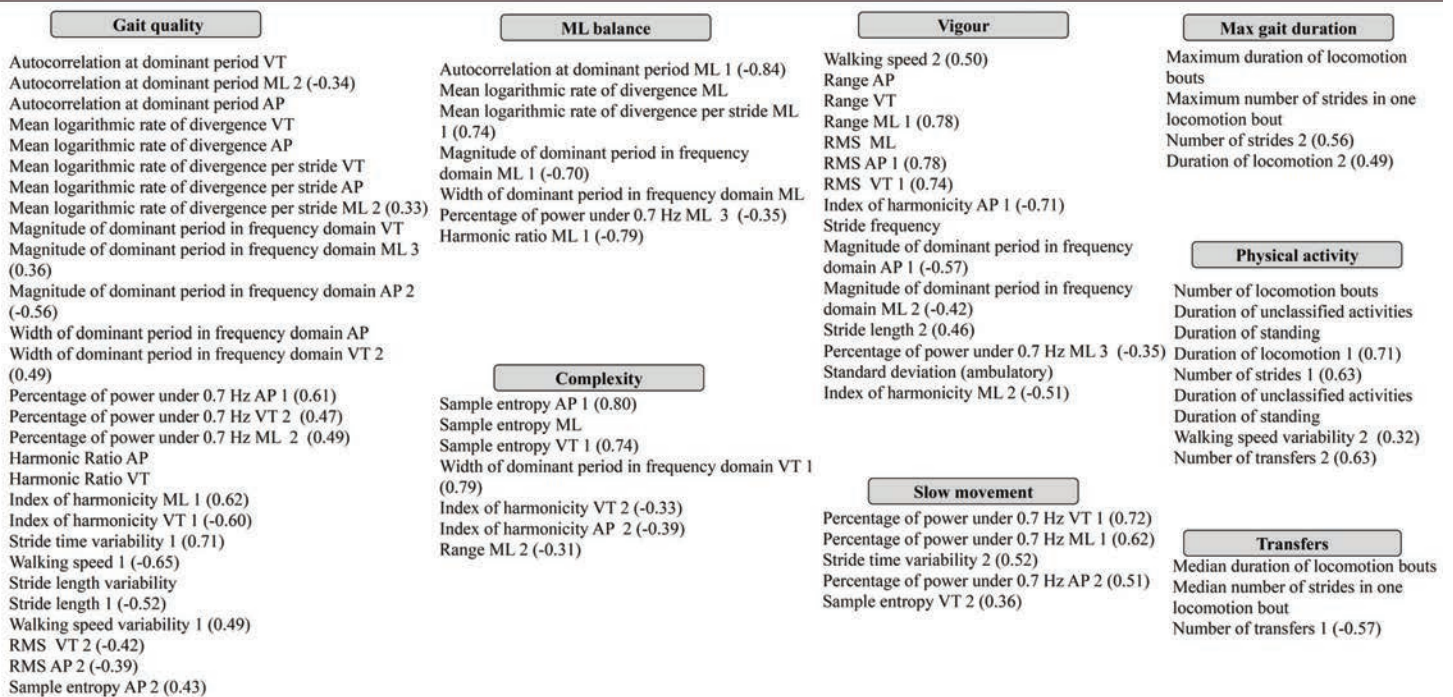


Figure 4: Data-driven model proposed by van Schooten et al, 2016 to categorize FLFPs. Only 8 relevant factors were taken into account (e.g., none of the FLFPs were loaded into domains such as history of falls, so those domains were not taken into account). If the FLFP is loaded into more than one domain (i.e., loading>0.3 in the paper), top three domains to which they indicate highest associations are indicated with integers (1 to 3). The numbers in parenthesis indicate the loading of the variable on varimax-rotated principal components.

## 4.0 Discussion

To date, inertial sensors using primarily acceleration signals, have been the preferred approach used to identify fallers based on their natural free-living behaviour over prolonged periods. These systems have demonstrated adequate capabilities to monitor and detect free-living activities, e.g., gait [30], [32], [44], [46]–[51], [33]–[35], [38]–[40], [42], [43], lying [38], [42], [50], [51] and gait events such as turns [45], [53]. However, it was observed that similar FLFPs that were examined by different studies indicated different levels of fall predictive ability; which can be due to the different experimental protocols used to collect free-living data (e.g. sensor placement, duration of free-living data collection, demographics), different mathematical/statistical methods, and algorithms used to define/detect activities (e.g., different cut-off thresholds). Due to these inconsistencies, developing conclusive interpretations of existing evidence remains limited. In the next subsections, the potential sources of inconsistency in methodology and categorization of FLFPs into domains are discussed. Following the sources of inconsistency, we provide recommendations towards harmonization of free-living FRA methods to advance the field.

### 4.1. Inconsistencies in free-living FRA models

#### 4.1.1. Similar FLFPs, different predictive power for falls

##### a. Inconsistency in ambulatory bout and turn cut-off thresholds

Considering the initial step in processing free-living inertial-based signals is detecting bouts, the observed variability in defining ambulatory bout thresholds is a large source of inconsistency potentially affecting the fall predictive ability of the extracted bout-based FLFPs. For instance, walking duration and the number of ambulatory bouts (two FLFPs) obtained from bouts longer than 3s (i.e., 3s as the minimum cut-off threshold) showed no associations with falls [46]. However, by changing the minimum cut-off threshold to 120s, these same FLFPs (i.e., walking duration, # of bouts) showed a statistically significant predictive ability for falls [46]. Another example of inconsistent results arising from bout definition differences was variability in bout length. Using the definition of bouts >3s yielded significant association with falls; whereas variability in bouts >120 s was not significantly associated [46]. Similarly, while exposure to short duration walks <7s [48] and <8s [49])



1  
2  
3  
4 was significantly associated with falls, exposure from walks shorter than 60 s was not  
5  
6 discriminative ( $p \cong 0.1$ ) [48].  
7

8 It was also observed that discretizing angular cut-off thresholds can impact fall  
9  
10 predictive power of turn-related FLFPs. For instance, although no relationship between the  
11  
12 total number of daily turns (considering turns with different resolutions) and falls was  
13  
14 reported [45], [53], after dividing them into three separate angular levels, the quantity of  
15  
16 turns in each resolution turned out to be significantly lower for prospective fallers [45]. As  
17  
18 only two studies were concerned with turns [45], [53]), the effects of varying cut-off  
19  
20 threshold to determine bouts and/or events and subsequent impact on fall predictive ability  
21  
22 remains underexamined.  
23

#### 24 **b. Central tendency measures to estimate FLFPs**

25  
26 To extract FLFPs from free-living data, measures of central tendency used to calculate  
27  
28 predictors were inconsistent between studies. The different statistical methods resulted in  
29  
30 inter- and intra-study inconsistencies in terms of fall predictive values for similar FLFPs. For  
31  
32 instance, mode of step time variability in [48] was significantly associated with falls; while  
33  
34 the mean estimation did not indicate any relationship. In addition to medians, in [31]  
35  
36 extremes of FLFPs were estimated (i.e., the 10th and 90th percentiles of gait characteristics)  
37  
38 over 10s epochs/bouts; whereas in [38] only the medians of MBB FLFPs (e.g., entropy,  
39  
40 amplitude of the dominant frequency) were reported. For instance, compared to median  
41  
42 values, a stronger association was reported for some of the extreme estimations and falls  
43  
44 [31]. Similarly, macro gait features such as ambulatory bout duration, mean [46], [50], [51],  
45  
46 maximum [32], [38], [42], [48], [51], 90th percentiles [50], and medians [32], [36], [38], [42],  
47  
48 [48] were reported. Overall, the lack of consistency limits the capacity to compare across  
49  
50 studies and synthesize the evidence.  
51

#### 52 **c. Free-living data collection protocols**

53  
54 Across the reviewed studies, inconsistent data collection protocols may play a key role in fall  
55  
56 predictive ability of FLFPs. Specifically, length of data collection, sampling frequency, and  
57  
58 wearable location were inconsistent across studies. Although eight days of free-living data  
59  
60 was reported to be sufficient for the identification of fall-prone individuals [48], only one day  
61  
62  
63  
64  
65

1  
2  
3  
4 of free-living data per participant was investigated in [50], [51]. In [41] up to five days was  
5 reported to be required for the estimation of median duration of locomotion bouts; while a  
6 minimum of two days of free-living data resulted an inter class correlation greater than 0.7  
7  
8 for most activities (sitting, standing and shuffling, except for lying). Sampling frequency was  
9  
10 inconsistently used within the studies, ranging from 10 Hz in [43] to 100 Hz in [52] (see  
11  
12 Table 3). Considering the impact of sampling frequency on the wearable unit battery life [56],  
13  
14 the identification of the optimal sampling frequency requires further investigation.  
15  
16 Moreover, estimates of gait characteristics may suffer from errors due to discrepancies in  
17  
18 accelerometer location [57]. Although lab-based data suggest that inertial-based wearables  
19  
20 mounted on shins can outperform other anatomical locations [58] for detection of fallers, no  
21  
22 study has considered this location for the collection of free-living data with lower back as the  
23  
24 most frequently used location for sensor placement. To date there is no consensus about the  
25  
26 most robust location for free-living FRA, which requires further exploration.  
27  
28

#### 29 30 **4.1.2 Inconsistencies in the proposed free-living FRA models**

31 Efforts to develop an FRA model based on predictors generated from wearables is needed to  
32  
33 interpret FLFPs related to fall risk. These interpretations are critical to understanding the  
34  
35 underlying causes or factors indicating risks and informing interventions for clinicians. In  
36  
37 contrast, black-box models (e.g., deep models) that estimate risk without interpretive value  
38  
39 are less useful. The reviewed studies with models demonstrated considerable inconsistency,  
40  
41 likely reflective of the on-going advancement in the field.  
42

43 As discussed in 3.3, we found quality as the most inconsistently used term with  
44  
45 discrepancies in definition and application. There were many inconsistent terminologies  
46  
47 observed across a range of domains and FLFPs within the examined models. For instance,  
48  
49 harmonic ratio was an indicator of gait smoothness in conceptual model e and but an  
50  
51 indicator of symmetry in model d (instead, index of harmonicity was the measure of  
52  
53 smoothness in model d). In some cases, different terminologies were used to describe the  
54  
55 same FLFP. For example, endurance and exposure were defined by the same calculation in  
56  
57 [48], [49], albeit described in different domains in models b and c, respectively (Figure 3). In  
58  
59 another case, the term 'vigour' was used to describe a domain (Figure 4) [38] and defined as  
60  
61 a FLFP (root mean square of vertical angular velocity) in models b and c [48], [49].  
62  
63  
64  
65

1  
2  
3  
4 In contrast to conceptual models (e.g., Figure 3, models d and e), where all of the AP,  
5 ML, VT, and vector-based components of the same MBB FLFP were considered under the  
6 same domain (e.g., harmonic ratio in ML, AP, and VT were considered under gait  
7 smoothness), different anatomical directions of some of the MBB FLFPs were loaded onto  
8 independent domains in data-driven model f (Figure 4). Many of the FLFPs extracted from  
9 ML acceleration were loaded into a distinct domain called 'ML balance' (e.g., harmonic ratio  
10 in ML direction was loaded into ML balance, while the other two components were  
11 considered under quality). Similarly, index of harmonicity in AP direction was loaded into  
12 vigour; although the other two directions were loaded into quality. It is clear the proposed  
13 models are a work in progress as the field is continually advancing. The existing  
14 inconsistencies highlighted in the current review suggest the need for deeper discussion to  
15 harmonize interpretive models.  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27

## 28 **4.2. Recommendations for harmonization and clinical implications**

### 29 **4.2.1. Precise activity recognition algorithms**

30  
31 One possible reason for inconsistencies in fall predictive power of FLFPs is the use of black-  
32 box thresholds in activity recognition algorithms [59], [60] in some of the studies, resulting  
33 in a low specificity and clarity to analyze free-living activities. For instance, studies included  
34 here were only concerned with general types of activities, such as ambulation, standing,  
35 sitting, and lying. A subset of studies differentiated between patterns of gait, such as  
36 ascending/descending stairs, or fast walking. For instance, [31] excluded locomotion bouts  
37 suspected to contain running episodes as they caused severe outliers in FLFP estimations for  
38 some of the participants. Additionally, turns and compensatory balance reactions were not  
39 excluded from ambulatory bouts before the extraction of MBB features. For instance, the  
40 misstep detection method in [37] revealed a number of suspected missteps from 5-second  
41 ambulatory bouts. However, in a subsequent study [36], MBB features were extracted from  
42 the same dataset without excluding those suspected missteps, which may have affected the  
43 fall predictive values of the MBB features.  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56

57 Multimodal approaches, such as a combination of IMUs, surface electromyography  
58 [61], electroencephalogram [62], heart rate variability and ECG [63] and pressure-sensitive  
59  
60  
61  
62  
63  
64  
65

1  
2  
3  
4 shoe-insoles [25]–[27] may increase the specificity of activity recognition algorithms, and  
5 therefore, to improve the sensitivity of FLFPs to identify fallers. As an example, using a force  
6 sensing insole equipped with an IMU and a barometric sensor, a framework to discriminate  
7 between level walking and stairs patterns of gait was developed and evaluated [64]. State-  
8 of-the-art algorithms, such as long-short term memory and deep convolutional neural  
9 networks have achieved near-human accuracy levels in detection of a broad range of  
10 activities from multimodal public datasets [65], which can be employed as a replacement to  
11 threshold-based methods to detect a broader range of natural activities. Only one study [39]  
12 investigated the use of deep learning models to identify fallers based on their preprocessed  
13 10-second walking patterns; where deep models slightly outperformed the baseline  
14 approach based on the biomechanical FLFPs as discussed in [38].  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25

#### 26 **4.2.2. Interpreting FLFPs by acquiring contextual information**

27  
28 In [66] it was shown that the mobility measures are affected by the environmental features  
29 (e.g., sidewalk slopes and crossings) and it was hypothesized that subjects would adapt to  
30 challenging environments by decreasing gait speed, increasing cadence, and shortening  
31 stride length. Moreover, a higher variability in ML direction, e.g., a lower amplitude of the  
32 dominant frequency, could indicate a higher adaptability to the environment [32]. However,  
33 the intrinsic meaning of these measures and terminologies (e.g., adaptability) in different  
34 anatomical directions and contexts remains unclear, inertial sensors do not provide  
35 sufficient information on human-environment interaction. Although applying cutting-edge  
36 algorithms (as discussed in 4.2.1) can boost the interpretation of context (e.g. stair climbing,  
37 walking downhill), the validity of these algorithms in complicated free-living scenarios needs  
38 to be carefully examined (also refer to the last column in Table 3, which shows the algorithms  
39 used in included studies were not mostly validated in free-living conditions).  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49

50 In [67] time-stamped self-reporting (voice recordings) was along with IMU data to  
51 increase the interpretability of IMU data and to locate compensatory balance reactions (slips,  
52 trips, stumbles) collected in 4 weeks. However, such a tool may also suffer from subjectivity  
53 and under-reporting. On the other hand, egocentric first-person video, acquired via body-  
54 worn cameras have been used as a gold standard [59] for the purpose of validating IMU-  
55 based algorithms or identification of specific events or environmental features [68] [14],  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

1  
2  
3  
4 [69]. First person video captures more contextually relevant information on the properties  
5 of the environment compared to IMU alone. This includes, but is not limited to, varying slope  
6 and surface navigation as well as static and dynamic objects (e.g. obstacles, pedestrians) that  
7 influence mobility behaviour. As an alternative to frame-by-frame investigation (visual  
8 inspection) of first person video data, algorithms are in development to automatically detect  
9 extrinsic risk factors from first person video data. For instance, machine learning (e.g.,  
10 convolutional neural networks) and image processing (e.g., Gabor Barcodes) techniques  
11 have shown promising performance in automatic detection of environmental fall-related  
12 hazards, including slope changes (e.g., stairs, curbs, ramps) and different surfaces (e.g.,  
13 gravel, grass, concrete) [70], [71]. By augmenting IMU approaches with egocentric videos,  
14 more insight can be readily gained from specific motoric activity. For example, gait data  
15 pertaining to micro/quality gait (from an IMU) within a new residential environment under  
16 low-level lighting conditions (video) or within crowded open spaces during daylight offer  
17 different challenges for fallers. Combined IMU and video approaches may allow healthcare  
18 professionals to target individualised approaches for rehabilitation strategies, ensuring  
19 safer navigation and reduced falls.  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33

#### 34 35 **4.2.3. An all-inclusive data-driven model** 36

37 As discussed in 4.1.1, different hyperparameters, such as ambulatory bout length, central  
38 tendency measures, and data collection protocols, such as the length of free-living data and  
39 sampling frequency, can impact fall predictive power of FLFPs. However, there is not  
40 sufficient evidence indicating the optimal values for these hyperparameters to achieve the  
41 highest predictive values specific to each FLFP. Moreover, many features, such as those  
42 quantifying different aspects of compensatory balance reactions, micro-transition- (e.g. jerk,  
43 entropy) and foot clearance-based measures were not investigated in any of the previous  
44 data-driven models (e.g., Figure 4-model f and controlled models such as [72]). Therefore,  
45 debate continues about their real identity in terms of their allocation to free-living domains.  
46 The aforementioned gaps in the literature indicate a need to obtain a standardized model to  
47 define discrete independent domains by performing factor analysis on a comprehensive  
48 range of wearable-based FLFPs derived from a broad range of video-validated activity bouts.  
49 This comprehensive set may also include similar FLFPs but different in terms of  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

hyperparameters (e.g., ambulatory bout lengths, turn cut-off thresholds, and central tendency measures). It is also feasible to simulate shorter/longer collection periods, and sampling rates (by up- and down-sampling signals) and examine FLFPs' sensitivity with respect to these factors. Performing factor analysis on the aforementioned comprehensive set of features altered based on different hyperparameters would permit deeper insights on developing more structured free-living models and provides more information on the differences between laboratory and free-living features in prediction of falls. While a deeper discussion on developing better models by including established lab-based models of fall risk is beyond the scope of the current paper, efforts towards a more comprehensive fall risk model leveraging both laboratory and free-living sources of evidence are on-going. Such efforts will better inform pragmatic efforts for which gait and other functional movements may be useful to identify surrogate markers of incipient pathology, inform diagnostic algorithms, track disease progression, and measure the efficacy of interventions [73].

**5.0 Conclusion**

Overall, free-living FRA using wearables is a promising avenue for fall prevention; however, due to the high level of heterogeneity in the use of wearables; e.g., sensor location, diverse cohorts, stratified employment (e.g., 1 vs 7 days), definition of free-living domains, and the selection of free-living bout resolutions, the evidence for the relationships between FLFPs and falls has remained inconclusive. Moreover, many FLFPs were specific to research groups and were not systematically investigated in an all-inclusive factor analysis. Therefore, achieving a data-driven model is necessary to systematically identify the FLFPs, bout resolutions, and domains with the highest predictive values for falls to eventually address intervention programs and prevent older adults from falling. Publishing well-annotated video-validated free-living datasets to support harmonization efforts is strongly recommended.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

**Acknowledgements**

M Nouredanesh was funded by AGE-WELL Inc. (Canada’s technology and aging network) Graduate Scholarship. A Godfrey holds a grant from the Royal Academy of Engineering: Frontiers of Engineering for Development (FoESF1819T621). The rest of co-authors were supported by National Sciences and Engineering Research Council of Canada (NSERC): E Lemaire (2001-05101), and J Tung (2015-05317). None of the funding sources had a role in the writing of this review.

**Conflict of interest**

The authors declare that they have no conflict of interest.

Table 1: Study designs for capturing free-living data. Dashed lines separate the relevant studies published from the same research group or from overlapping datasets. ACC: accelerometer, Gyro: gyroscope, 3D: three-dimensional, FLFP: free-living fall predictor.

Study	Free-living data-log duration	Type of activities	Modality(ies)	Sensor placement
Weiss (2013) [32]; Ihlen (2015, 2016a, 2016b) [33, 34, 35]	3 days	Gait	DynaPort MoveMonitor	At the L5 level
Ihuz (2014) [37]	3 days	Missteps	DynaPort Hybrid (ACC+Gyro)	Lower back(L4-5)
Weiss (2014) [36]	3 days	Gait	One ACC+Gyro	Lower back
Ihuz (2015) [30]	3 days	Sit-to-walk and walk-to-sit transitions	DynaPort MoveMonitor	Around the waist and set along the lumbar spine
Rispens (2015a) [47]	2 weeks	Amount of physical (in-)activity and quality of daily-life gait	DynaPort MoveMonitor	Dorsally on the trunk at L5
van Schooten (2015a) [42]	8 days	Amount of physical (in-)activity		
Rispens (2015b) [31]	1 week	Amount of physical (in-)activity and quality of daily-life gait		
van Schooten (2016) [38]	1 week	Bouts of locomotion, sitting, lying, standing		
Nait Aicha (2018) [39] and Ihlen (2018) [40]	1 week	only gait in Nait Aicha (2018) [39] and Ihlen (2018) [40]	DynaPort MoveMonitor	At the L5 level
Brodie (2015) [48]	Mean 58 days/participant: Fallers: 44.0(29.0) days, NFs: 67.0(29.0) days	Activities during walking hours were monitored, only gait was investigated	Philips (Senior Mobility Monitor) pendant (ACC+Barometer)	Sternum Level
Brodie (2017) [49]	7 days ( $\geq 6$ hr data per day)	Activities during walking hours were monitored, only gait was investigated	Philips (Senior Mobility Monitor) pendant (ACC+Barometer)	Sternum Level
Mancini (2016) [53]	$\approx 10$ hours/day for 7 days	Turning mobility	3 IMUs(APDM Opal)	One on belt (L5), 2 on shoes
Leach (2018) [45]	5-9 days	Turns and gait	Android smartphone (3DACC+3DGyro) and uFALL app	Midsagittal plane of the lower back
Mohler (2016) [50]	48 hours	Walking, sitting, standing, lying and postural transitions (all time except while showering)	PAMSys BioSensic	Into a T-shirt with a device pocket at sternum level
Pozaic (2016) [52]	7 days	Sit-to-stand transitions (focus of the study)	Bosch sensor tech GmbH (sD ACC, 3D gyro, 3D magnetometer)	One attached to Wrist
Mactier (2015) [43]	7 days	Gait	activPAL (uniaxial ACC)	Upper thigh
Hirth (2016) [44]	7 days (at least 4 days)	1) Volume, 2) pattern, 3) accumulation, 4) variability of sedentary behavior (sitting, lying), standing, and ambulatory bouts	activPAL	Middle of thigh
Del Din (2017) [46]	7 days	Macro- and micro-gait parameters (spatiotemporal)	Axivity AX3	Lower back
Schwenk (2014) [51]	24hours	Walking,sitting,standing,lying	Physlog (2ACC+1Gyro)	Attached to the chest (pocket)
Gietzelt (2014) [54]	7 days after each visit (4 visits in 8 months)		One SHIMMER sensor	



Table 2: Demographic data, Fs: fallers, NFs: non-fallers, OA: community-dwelling older adults, PD: people with Parkinson’s disease, f: female, m: male, FLFP: free-living fall predictor. Dashed lines separate the relevant studies published from the same research group or from overlapping datasets.

Study	Specific disease (Yes/No)	Participants’ Number, Age, female:male	Categorization of fallers and non-fallers based on	
			Prospective falls	Retrospective falls
Weiss (2013) [32]; Ihlen (2015, 2016a, 2016b) [33, 34, 35]	No	NFs: 39, 78.77(4.39)y, Fs:32, 77.86(5.09)y, fs: 64.10%	12 subjects reported $\geq 2$ falls 6 months following the experiment <sup>1</sup>	$\geq 2$ falls one year prior to measurements
Weiss (2014) [36]	All PD	NFs: 67(40 to 85y)	1 year follow-up(each month returned) <sup>2, 14</sup>	$\geq 1$ fall prior year
Ihlu (2014) [37]	All PD	NFs+Fs:40, 62.16(10.02)y, Fs:9, 6m=8.32	NFs turned to Fs, N/A	$\geq 2$ falls in the past 6 months
Ihlu (2015) [30]	No	NFs: 38, 78.65(4.35), f: 66.66%	No	$\geq 2$ falls in the previous year
Rispens (2015a) [47]	No	110 (Fs+NFs), 78.4(7.8)y, fm= 77.33	No	$\geq 2$ falls in the previous year; 1.2(1.6) falls in 12 months prior the measurements
van Schooten (2015a) [42]	No	Retrospective-NFs: 109, Retrospective-Fs: 60, Prospective-NFs: 110, Prospective-Fs: 59, NFs+Fs: 169, 75.4(6.8)y, f: 52.1%	$\geq 1$ Falls in 6 months follow-up	Falls in the preceding 6 months
Rispens (2015b) [31]	No	NFs: 132, 75.1(6.6)y, f: 50%	$\geq 1$ falls 6 months follow-up	Used in models but FLFPs were analyzed with respect to P falls
van Schooten (2016) [38]	No	Complete data for 294/319 participants were analyzed. Total 294 participants: 75.3(6.8)y, f: 50.8%, 48.8% had $\geq 1$ falls in past year, 25.2% had $\geq 2$ falls in past year	Initially 6 months, extended to 12 months if willing to continue)	$\geq 1$ and $\geq 2$ falls in past year
Nait Aicha (2018) [39]		101/296 participants had $\geq 1$ fall (34.1%), m: 74.1%		
Ihlen (2018) [40]		Total NFs: 199; Matched NFs for Single-Fs: 75.9(6.7)y, f: 51%; Matched NFs for Recurrent-Fs: 75.2(6.4)y, f: 48.8%	6 months follow-up	
Brodie (2015) [48]	No	NFs: 11, 84.0(7.9)y, fm=7:0	Fs: 7, 82.2(5.9)y, fm=7:4	$\geq 1$ falls in the past 12 months
Brodie (2017) [49]	No	NFs: 63, 75.8(7.3)y, sex: 0.48(0.50) (considering f=1 and m=0)	Fs: 33, 74.9(8.5)y, sex: 0.81(0.39) (considering f=1 and m=0)	$\geq 1$ fall in prior 12 months

<sup>1</sup>Statistical analysis was done with respect to retrospective falls only

<sup>2</sup>Statistical analysis for single FLFPs was only done with respect to retrospective falls; but separate survival analysis/Cox regression was performed for prospective falls

<sup>3</sup>Fall risk assessment in older adults (FARAO) dataset

Mancini (2016) [53]	No	NFs: 16, f:m=3:13 83.9(7.0)y;	Recurrent-Fs: 7, f:m=2:5 Single-Fs=12, f:m=8:4, 86.0(7.0)y	6 months following the 7 day recording, 7/35 experienced one or more fall	N ≥ 2 falls in the previous year
Leach (2018) [45]	No	Retrospective-NFs: 154 Prospective-NFs = 153	Retrospective-Fs = 6 Prospective-Fs = 7	≥ 2 falls in 12 months	≥ 2 falls in 12 months
Mohler (2016) [50]	Non-frail, pre-frail and frail	Non-frail NFs: 23, 74.7 (6.7)y, fs: 19 Pre-frail NFs: 38, 79.7(8.5)y, fs:28 Frail NFs: 10, 86.6(5.9)y, fs:7	Non-frail Fs: 20, 74.4(6.6)y, fs: 17 Pre-frail Fs: 19, 79.4(8.8)y, fs:15 Frail Fs: 9, 80.9(9.8)y, fs:9	Falls in the 6 months after the initial baseline study visit	N/A
Pozzaic (2016) [52]	No	NFs: 123, 72.4(5.6)y, fs in NFs:57.7%	Fs: 13, 74.2(5.3)y, fs in Fs:69.2%	≥ 1 fall in one month (overall 21 falls, 4 participants ≥ 2 falls)	N/A
Mactier (2015) [43]	All PD (no healthy control)	111 PD, NFs: 70(52), Recurrent-Fs: 24(19), pre-fall event: 14 transition-Fs, 17 ambulation-Fs, 7 advanced-activity-Fs	Single-Fs: 17(12), Fs: 20	12 months	N/A
Hiorth et al. (2016) [44]	All PD	NFs: 28	Fs: 20	N/A	6 months fall history
Del Din (2017) [46]	OA and PD	OA-NFs: 50, PD-NFs:15; For all NFs: 69.05(7.67)y f: 56%	OA-Fs: 122, PD-Fs:155; For all Fs: 73.33(6.78)y, f: 42%	N/A	≥ 2falls past 6 months, NFs: not fallen in at least 18 months
Schwenk (2014) [51]	People with dementia	NFs: 49, 81.8(5.9)y; m: 34.7%	Fs: 28, 82.0(7.1)y; m: 21.4%	3-months follow-up	
Gietzelt (2014) [54]	People with dementia	At the beginning 40 Fs+NFs (fs: 20), Fs=13 (n=8 fell once, n=2 fell 4 times, n=2 fell 5 times)	At the beginning 40 Fs+NFs (fs: 20), Fs=13 (n=8 fell once, n=2 fell 2 times, n=1 fell 4 times, n=2 fell 5 times)	A prospective cohort study with 3 phases: short-term (start to month 2): n=38(2 drop-outs (DOs) , 6 falls, 18 missed, (month 2-4): n=33 (5 DOs), 11 falls, 2 missed, (month4-6): 30 (3 DOs): 8 falls, 5 missed, (month 6-8):n=28 (2 DOs), 1 fall, 11 missed.	

Table 3: Bout of walking and activity definitions. ACC: accelerometer, Gyro: gyroscope, 3D: three-dimensional. Dashed lines separate the relevant studies published from the same research group or from overlapping datasets. FLFP: free-living fall predictor, OA: older adults, VT: vertical, AP: anterior-posterior, F: faller, NF: non-faller.

Study	Bout of activities/walking definition and Specific constraints	signal identifying bout	Sampling rate	Validation
Weiss (2013) [32]; Weiss (2014) [36]; Ihlen(2015, 2016a,2016b) [33, 34, 35]	Ambulatory bouts $\geq 60s$ were taken into account for FLFP extraction (dissected to 60-second intervals, e.g., in [32]). The bouts were identified based on two filters: 1. a signal magnitude area (SMA) threshold-based activity detection monitor, 2. a threshold of the energy in the frequency domain (windows with energy $>0.05$ were excluded). In Ihlen (2016) [34] ambulatory bouts $\geq 60s$ were divided into 50-second epochs for the extraction of entropy/complexity features.	ACC(3D)	100Hz	In Weiss (2013) [32] it was mentioned that the validated methods discussed in papers by Weiss (2011), Moen-Nolssen (2004) and Yack (1993) were used to quantify different aspects of gait. Validation in free-living conditions: N/A.
Ihuz (2014) [37]	5-second windows (running window of 5s) with 2-15 steps were detected and considered for FLFP extraction	ACC(3D), Gyro(3D)	100Hz	To develop the algorithm 29 missteps (negotiating obstacles while walking) were captured in a laboratory setting and more than 60 hours of data were recorded. Their rule-based algorithm achieved a 93.1% hit ratio and 98.6% specificity on this dataset.
Ihuz (2015) [30]	Detection of the subject's gross activity (e.g., gait, sitting) was performed based on the local mean of the acceleration signals (e.g., negative values for local mean of the vertical acceleration signal indicate lying, while positive values may correspond to: gait, standing, or sitting), with additional criteria applied to increase the robustness of the detection. The transitions were identified after detection of sitting and gait episodes	ACC (3D), Gyro (3D)	100 Hz	Validation in free-living conditions: N/A.
Rispens (2015a) [47]	Locomotion episodes $\geq 10s$ , each episode was split into 10-second epochs (to avoid sample-size related bias)	ACC(3D)	100Hz	Validation in free-living conditions: N/A.
van Schooten (2015a) [42] and van Schooten (2016) [38] and Rispens (2015b) [31], Nait Aicha (2018) [39]	Locomotion episodes $\geq 10s$ , each episode was split into 10-second epochs (to avoid sample-size related bias), sufficient quantity of gait bouts ( $\geq 50s$ ) per participants to be included in analysis (18 participants were excluded, 4 excluded in van Schooten (2015), Participants with $\geq 75\%$ wear time. In Rispens(2015b) [31] locomotion bouts with suspected running events were discarded.	ACC(3D)	100Hz	Bouts of non-wearing, locomotion, sitting, lying and standing were identified using manufacturer's algorithm (Dijkstra et al.) Validation in free-living conditions: N/A.
Ihlen (2018) [40]	First, ambulatory bouts $\geq 3s$ were identified by a commercially available activity detection algorithm. Then, 3D ACC signals attributed to ambulatory bouts $\geq 30s$ were included for the analysis. The included ambulatory bouts were split into equal-sized 30-second epochs to provide a consistent sample size to estimate entropy measures. The epochs were further checked (visually) and non-walking activity bouts were excluded. Inclusion criteria for walking epochs were: (a) distinct impact peaks in VT and/or AP component of the ACC signal, (b) distinct cyclical ACC pattern in VT and/or AP component(s), and (c) criteria (a) and (b) were satisfied for at least 80% of the epochs, where max 20% was considered for gait initiation, turning or transitional micro-breaks.	ACC(3D)	50Hz (25Hz barometer not used)	The aforementioned inclusion criteria were based on the visual inspection of fast, normal and slow walking pattern discussed in a 'validation' study for activity detection in OA by Bourke et al., (2017).
Brodie (2015) [48]	Ambulatory bouts were defined by consecutive heel strikes identified by vertical acceleration peaks in the level 4 and 5 Daubechies 5th-order wavelet decomposition. Daily-life gait quantity was quantified by: (a) Steps per day from ambulatory bouts $\geq 3$ steps), (b) Walks per day (of ambulatory bout $>=8$ steps), (c) Steps per walk (mean of walks $>=8$ steps). For intensity and quality analyses: ambulatory bout $>=7$ steps and for exposure analysis ambulatory bout $<7s$ and $<60s$ were taken into account.	ACC(3D)	50Hz (25Hz barometer not used)	Validation in free-living conditions: N/A.
Brodie (2017) [49]	Walks were defined by 3 consecutive heel strike peaks less than 3s apart. Short walk exposure was calculated by the percentage of walking duration $<8s$ .	ACC(3D)	50Hz (25Hz barometer not used)	Validation in free-living conditions: N/A.

Mancini (2016) [53]	10s ≤ ambulatory bouts longer or equal to 10s were first detected using 3D angular velocity signals and then were further investigated for the detection of turns, $0.5s < \text{turn-Duration} < 10s$ $45\text{deg} \leq \text{turn angles}$ . Turn angles were obtained by integrating the angular rate of the lumbar sensor about the V axis.	3D angular velocity signals	128 Hz	In El-Gohary (2013), compared to Motion Analysis and video, the algorithm maintained a sensitivity of 0.90 and 0.76 and a specificity of 0.75 and 0.65, respectively. The turn detection algorithm was further applied to data collected in the home from 12 PD and 18 control subjects and the algorithm successfully detects turn characteristics.
Leach (2018) [45]	Turn type and angular range of turn include $50-100\text{deg}$ , $100-150\text{deg}$ and $150-200\text{deg}$ (analyzed only if happened during gait with 0.5-5s duration). The turn detection algorithm was based on the angular rotational rate of the pelvis about the vertical axis.	ACC(3D) + Gyro(3D)	N/A	The turn detection algorithm was validated in El-Gohary (2013) as above.
Mohler (2016) [50]	Walking bouts $> 5s$ and $> 3$ steps were taken into account (based on Tosizadeh(2015))	ACC(3D)	N/A	Validation in free-living conditions: N/A.
Pozaic (2016) [52]	N/A	ACC(3D)	100Hz	Particular trigger events (such as rotation of the wrist above a predefined threshold), as well as periodical or motionless/dormancy situations after these events. An ACC-based arm swing detector was used for the detection of the walking phase. Methods was validated in a pilot study with 28 OA (65-90y), who performed eight different types of the sit-to-stand transitions in a controlled environment (i.e. camera-supervised lab) as part of the protocol that simulated activities of daily living. The algorithm showed 71.4% precision for the non-dominant hand and 67.9% precision for the dominant hand.
Mactier (2015) [43]	Windows of 15s were used and walking episodes of $\geq 1$ step were taken into account for FLFP extraction.	ACC(1D)	10Hz	Previous work in OA against other accelerometer and video recordings in people with rheumatoid arthritis during simulation of ADL in the laboratory. It was mentioned that the validated activePAL can identify postures (e.g. sitting, lying, standing).
Hiorth (2016) [44]	Ambulatory bouts $< 10$ strides, $10-50$ strides and $> 50$ strides were taken into account.	ACC(1D)	20Hz	Validation in free-living conditions: N/A.
Del Din (2017) [46]	All ambulatory bouts $> 3$ steps (minimum bout length) were taken into account for the analysis. For micro-gait FLFPs, ambulatory bout $> 10s$ were taken into account. For macro-gait FLFPs, ambulatory bouts $> 3$ steps (short), Ambulatory bout $> 60s$ (medium) and Ambulatory bout $> 120s$ (large) were considered. A threshold of 2.5s was set for the maximum resting period between consecutive ambulatory bouts	ACC(3D)	100Hz	The ambulatory bout detection algorithm was validated in a study with wearable cameras (Hickey et al., 2017). Characteristics of gait were selected based upon a model of gait validated both in OA and in people with PD in two distinct studies.
Gietzelt (2014) [54]	Ambulatory bouts of $\geq 20$ s were taken into account.	ACC(3D)	N/A	Validation in free-living conditions: N/A.
Schwenk (2014) [51]	A walking period was defined as an interval with at least 3 successive steps as described in the validation study of the Physilog. Activities with $< 3$ steps were considered as standing (e.g. working in the kitchen and moving $< 3$ steps).	Two ACCs and one Gyro	N/A	It was mentioned that the algorithm was sensitive (87-99%) and specific (87-99.7%) for detection of the physical activity pattern in different samples of OA and patients. Validation in free-living conditions: N/A.

## References

- [1] W. H. Organization, W. H. O. Ageing, and L. C. Unit, *WHO global report on falls prevention in older age*. World Health Organization, 2008.
- [2] H. Hawley-Hague, E. Boulton, A. Hall, K. Pfeiffer, and C. Todd, "Older adults' perceptions of technologies aimed at falls prevention, detection or monitoring: a systematic review," *Int. J. Med. Inform.*, vol. 83, no. 6, pp. 416–426, 2014.
- [3] J. A. Painter, L. Allison, P. Dhingra, J. Daughtery, K. Cogdill, and L. G. Trujillo, "Fear of falling and its relationship with anxiety, depression, and activity engagement among community-dwelling older adults," *Am. J. Occup. Ther.*, vol. 66, no. 2, pp. 169–176, 2012.
- [4] P. Kannus, H. Sievänen, M. Palvanen, T. Järvinen, and J. Parkkari, "Prevention of falls and consequent injuries in elderly people," *Lancet*, vol. 366, no. 9500, pp. 1885–1893, 2005.
- [5] N. Kronfol, "Biological, medical and behavioral risk factors on falls," *World Heal. Organ.* [http://www.who.int/ageing/project/falls\\_prevention\\_older\\_age/en/index.html](http://www.who.int/ageing/project/falls_prevention_older_age/en/index.html), 2012.
- [6] S. E. Carter, E. M. Campbell, R. W. Sanson-Fisher, S. Redman, and W. J. Gillespie, "Environmental hazards in the homes of older people," *Age Ageing*, vol. 26, no. 3, pp. 195–202, 1997.
- [7] T. M. Gill, C. S. Williams, J. T. Robison, and M. E. Tinetti, "A population-based study of environmental hazards in the homes of older persons," *Am. J. Public Health*, vol. 89, no. 4, pp. 553–556, 1999.
- [8] S. Podsiadlo, D. Richardson, "The timed "up & go": A test of basic functional mobility for frail elderly persons," *J. Am. Geriatr. Soc.*, vol. 39, no. 2, pp. 142–148, 1991.
- [9] A. Shumway-Cook, S. Brauer, and M. Woollacott, "Predicting the probability for falls in community-dwelling older adults using the Timed Up & Go Test," *Phys. Ther.*, vol. 80, no. 9, pp. 896–903, 2000.
- [10] M. E. Tinetti, "Performance-Oriented Assessment of Mobility Problems," *J. Am. Geriatr. Soc.*, vol. 34, no. 2, pp. 119–126, 1986.
- [11] D. Schoene *et al.*, "Discriminative ability and predictive validity of the timed Up and Go test in identifying older people who fall: systematic review and meta-analysis," *J. Am. Geriatr. Soc.*, vol. 61, no. 2, pp. 202–208, 2013.
- [12] K. A. Hamel, N. Okita, J. S. Higginson, and P. R. Cavanagh, "Foot clearance during stair descent: effects of age and illumination," *Gait Posture*, vol. 21, no. 2, pp. 135–140, 2005.
- [13] V. Robles-García *et al.*, "Spatiotemporal gait patterns during overt and covert evaluation in patients with Parkinson's disease and healthy subjects: Is there a Hawthorne effect?," *J. Appl. Biomech.*, vol. 31, no. 3, pp. 189–194, 2015.
- [14] S. Del Din, A. Godfrey, B. Galna, S. Lord, and L. Rochester, "Free-living gait characteristics in ageing and Parkinson's disease: impact of environment and ambulatory bout length," *J. Neuroeng. Rehabil.*, vol. 13, no. 1, p. 46, 2016.
- [15] I. Hillel *et al.*, "Is every-day walking in older adults more analogous to dual-task walking or to usual walking? Elucidating the gaps between gait performance in the lab and during 24/7 monitoring," *Eur. Rev. Aging Phys. Act.*, vol. 16, no. 1, pp. 1–12, 2019.
- [16] S. M. Rispens *et al.*, "Fall-related gait characteristics on the treadmill and in daily life," *J. Neuroeng. Rehabil.*, vol. 13, no. 1, p. 12, 2016.
- [17] N. Takayanagi *et al.*, "Relationship between Daily and In-laboratory Gait Speed among Healthy Community-dwelling Older Adults," *Sci. Rep.*, vol. 9, no. 1, pp. 2–3, 2019.
- [18] G. Diraco, A. Leone, and P. Siciliano, "A radar-based smart sensor for unobtrusive elderly monitoring in ambient assisted living applications," *Biosensors*, vol. 7, no. 4, 2017.
- [19] J. Kaye *et al.*, "One walk a year to 1000 within a year: Continuous in-home unobtrusive gait assessment of older adults," *Gait Posture*, vol. 35, no. 2, 2012.
- [20] M. Gabel, R. Gilad-Bachrach, E. Renshaw, and A. Schuster, "Full body gait analysis with

- Kinect.," *Conf. Proc. IEEE Eng. Med. Biol. Soc.*, vol. 2012, 2012.
- [21] E. Cippitelli, S. Gasparrini, S. Spinsante, and E. Gambi, "Kinect as a tool for gait analysis: validation of a real-time joint extraction algorithm working in side view," *Sensors*, vol. 15, no. 1, pp. 1417–1434, 2015.
- [22] L. J. Phillips *et al.*, "Using embedded sensors in independent living to predict gait changes and falls," *West. J. Nurs. Res.*, vol. 39, no. 1, pp. 78–94, 2017.
- [23] E. Auvinet, F. Multon, V. Manning, J. Meunier, and J. P. Cobb, "Validity and sensitivity of the longitudinal asymmetry index to detect gait asymmetry using microsoft kinect data," *Gait Posture*, vol. 51, pp. 162–168, 2017.
- [24] E. E. Stone and M. Skubic, "Unobtrusive, continuous, in-home gait measurement using the microsoft kinect," *IEEE Trans. Biomed. Eng.*, vol. 60, no. 10, 2013.
- [25] M. Di Rosa *et al.*, "Concurrent validation of an index to estimate fall risk in community dwelling seniors through a wireless sensor insole system: A pilot study," *Gait Posture*, vol. 55, no. December 2015, pp. 6–11, 2017.
- [26] C. Moufawad El Achkar, C. Lenoble-Hoskovec, A. Paraschiv-Ionescu, K. Major, C. Büla, and K. Aminian, "Physical behavior in older persons during daily life: Insights from instrumented shoes," *Sensors (Switzerland)*, vol. 16, no. 8, 2016.
- [27] C. M. el Achkar, C. Lenoble-Hoskovec, A. Paraschiv-Ionescu, K. Major, C. Büla, and K. Aminian, "Classification and characterization of postural transitions using instrumented shoes," *Med. Biol. Eng. Comput.*, vol. 56, no. 8, pp. 1403–1412, 2018.
- [28] M. Nouredanesh, A. W. Li, A. Godfrey, J. Hoey, and J. Tung, "Chasing Feet in the Wild: A Proposed Egocentric Motion-Aware Gait Assessment Tool," pp. 176–192, 2019.
- [29] A. Kim, J. Kim, S. Rietdyk, and B. Ziaie, "A wearable smartphone-enabled camera-based system for gait assessment," *Gait Posture*, vol. 42, no. 2, pp. 138–144, 2015.
- [30] T. Iluz *et al.*, "Can a body-fixed sensor reduce Heisenberg's uncertainty when it comes to the evaluation of mobility? Effects of aging and fall risk on transitions in daily living," *Journals Gerontol. Ser. A Biomed. Sci. Med. Sci.*, vol. 71, no. 11, pp. 1459–1465, 2015.
- [31] S. M. Rispens, K. S. van Schooten, M. Pijnappels, A. Daffertshofer, P. J. Beek, and J. H. van Dieën, "Do Extreme Values of Daily-Life Gait Characteristics Provide More Information About Fall Risk Than Median Values?," *JMIR Res. Protoc.*, vol. 4, no. 1, p. e4, 2015.
- [32] A. Weiss *et al.*, "Does the evaluation of gait quality during daily life provide insight into fall risk? A novel approach using 3-day accelerometer recordings," *Neurorehabil. Neural Repair*, vol. 27, no. 8, pp. 742–752, 2013.
- [33] E. A. F. Ihlen, A. Weiss, J. L. Helbostad, and J. M. Hausdorff, "The Discriminant Value of Phase-Dependent Local Dynamic Stability of Daily Life Walking in Older Adult Community-Dwelling Fallers and Nonfallers.," *Biomed Res. Int.*, vol. 2015, p. 402596, 2015.
- [34] E. A. F. Ihlen, A. Weiss, A. Bourke, J. L. Helbostad, and J. M. Hausdorff, "The complexity of daily life walking in older adult community-dwelling fallers and non-fallers," *J. Biomech.*, vol. 49, no. 9, 2016.
- [35] E. A. F. Ihlen, A. Weiss, Y. Beck, J. L. Helbostad, and J. M. Hausdorff, "A comparison study of local dynamic stability measures of daily life walking in older adult community-dwelling fallers and non-fallers," *J. Biomech.*, vol. 49, no. 9, 2016.
- [36] A. Weiss, T. Herman, N. Giladi, and J. M. Hausdorff, "Objective assessment of fall risk in Parkinson's disease using a body-fixed sensor worn for 3 days," *PLoS One*, vol. 9, no. 5, p. e96675, 2014.
- [37] T. Iluz *et al.*, "Automated detection of missteps during community ambulation in patients with Parkinson's disease: A new approach for quantifying fall risk in the community setting," *J. Neuroeng. Rehabil.*, vol. 11, no. 1, 2014.
- [38] K. S. Van Schooten *et al.*, "Daily-life gait quality as predictor of falls in older people: A 1-year prospective cohort study," *PLoS One*, vol. 11, no. 7, 2016.

- 1  
2  
3  
4 [39] A. Nait Aicha, G. Englebienne, K. van Schooten, M. Pijnappels, and B. Kröse, "Deep learning to  
5 predict falls in older adults based on daily-life trunk accelerometry," *Sensors*, vol. 18, no. 5, p.  
6 1654, 2018.  
7  
8 [40] E. A. F. Ihlen *et al.*, "Improved prediction of falls in community-dwelling older adults through  
9 phase-dependent entropy of daily-life walking," *Front. Aging Neurosci.*, vol. 10, p. 44, 2018.  
10 [41] K. S. Van Schooten, S. M. Rispens, P. J. M. Elders, P. Lips, J. H. van Dieën, and M. Pijnappels,  
11 "Assessing physical activity in older adults: required days of trunk accelerometer  
12 measurements for reliable estimation," *J. Aging Phys. Act.*, vol. 23, no. 1, pp. 9–17, 2015.  
13 [42] K. S. van Schooten, M. Pijnappels, S. M. Rispens, P. J. M. Elders, P. Lips, and J. H. van Dieën,  
14 "Ambulatory fall-risk assessment: amount and quality of daily-life gait predict falls in older  
15 adults.," *J. Gerontol. A. Biol. Sci. Med. Sci.*, vol. 70, no. 5, pp. 608–615, May 2015.  
16 [43] K. Mactier, S. Lord, A. Godfrey, D. Burn, and L. Rochester, "The relationship between real  
17 world ambulatory activity and falls in incident Parkinson's disease: influence of classification  
18 scheme," *Parkinsonism Relat. Disord.*, vol. 21, no. 3, pp. 236–242, 2015.  
19 [44] Y. H. Hiorth *et al.*, "Impact of falls on physical activity in people with Parkinson's disease," *J.*  
20 *Parkinsons. Dis.*, vol. 6, no. 1, pp. 175–182, 2016.  
21 [45] J. M. Leach, S. Mellone, P. Palumbo, S. Bandinelli, and L. Chiari, "Natural turn measures  
22 predict recurrent falls in community-dwelling older adults: a longitudinal cohort study," *Sci.*  
23 *Rep.*, vol. 8, no. 1, p. 4316, 2018.  
24 [46] D. Del *et al.*, "Analysis of free-living gait in older adults with and without Parkinson's disease  
25 and with and without a history of falls: identifying generic and disease specific  
26 characteristics.," *Journals Gerontol. Ser. A Med. Sci.*, 2017.  
27 [47] S. M. Rispens, K. S. van Schooten, M. Pijnappels, A. Daffertshofer, P. J. Beek, and J. H. van  
28 Dieën, "Identification of fall risk predictors in daily life measurements: gait characteristics'  
29 reliability and association with self-reported fall history.," *Neurorehabil. Neural Repair*, vol.  
30 29, no. 1, pp. 54–61, Jan. 2015.  
31 [48] M. A. Brodie, S. R. Lord, M. J. Coppens, J. Annegarn, and K. Delbaere, "Eight-Week Remote  
32 Monitoring Using a Freely Worn Device Reveals Unstable Gait Patterns in Older Fallers," vol.  
33 62, no. 11, pp. 2588–2594, 2015.  
34 [49] M. A. Brodie *et al.*, "Comparison between clinical gait and daily-life gait assessments of fall  
35 risk in older people," *Geriatr. Gerontol. Int.*, vol. 17, no. 11, pp. 2274–2282, 2017.  
36 [50] M. J. Mohler, C. S. Wendel, R. E. Taylor-Piliae, N. Toosizadeh, and B. Najafi, "Motor  
37 Performance and Physical Activity as Predictors of Prospective Falls in Community-Dwelling  
38 Older Adults by Frailty Level: Application of Wearable Technology," *Gerontology*, vol. 62, no.  
39 6, 2016.  
40 [51] M. Schwenk, K. Hauer, T. Zieschang, S. Englert, J. Mohler, and B. Najafi, "Sensor-derived  
41 physical activity parameters can predict future falls in people with dementia," *Gerontology*,  
42 vol. 60, no. 6, 2014.  
43 [52] T. Pozaic, U. Lindemann, A.-K. Grebe, and W. Stork, "Sit-to-Stand Transition Reveals Acute  
44 Fall Risk in Activities of Daily Living," *IEEE J. Transl. Eng. Heal. Med.*, vol. 4, 2016.  
45 [53] M. Mancini *et al.*, "Continuous monitoring of turning mobility and its association to falls and  
46 cognitive function: a pilot study," *Journals Gerontol. Ser. A Biomed. Sci. Med. Sci.*, vol. 71, no. 8,  
47 pp. 1102–1108, 2016.  
48 [54] M. Gietzelt, F. Feldwieser, M. Gövercin, E. Steinhagen-Thiessen, and M. Marschollek, "A  
49 prospective field study for sensor-based identification of fall risk in older people with  
50 dementia," *Informatics Heal. Soc. Care*, vol. 39, no. 3–4, 2014.  
51 [55] H. Kantz and T. Schreiber, *Nonlinear time series analysis*, vol. 7. Cambridge university press,  
52 2004.  
53 [56] A. Tobola *et al.*, "Sampling rate impact on energy consumption of biomedical signal  
54 processing systems," *2015 IEEE 12th Int. Conf. Wearable Implant. Body Sens. Networks, BSN*  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

- 2015, 2015.
- [57] S. M. Rispens, M. Pijnappels, K. S. van Schooten, P. J. Beek, A. Daffertshofer, and J. H. van Dieën, "Consistency of gait characteristics as determined from acceleration data collected at different trunk locations," *Gait Posture*, vol. 40, no. 1, pp. 187–192, 2014.
- [58] L. Montesinos, R. Castaldo, and L. Pecchia, "Wearable inertial sensors for fall risk assessment and prediction in older adults: A systematic review and meta-analysis," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 26, no. 3, pp. 573–582, 2018.
- [59] A. Godfrey, "Wearables for independent living in older adults: Gait and falls," *Maturitas*, vol. 100, pp. 16–26, 2017.
- [60] G. Barry, B. Galna, S. Lord, L. Rochester, and A. Godfrey, "Defining ambulatory bouts in free-living activity: Impact of brief stationary periods on bout metrics," *Gait Posture*, vol. 42, no. 4, pp. 594–597, 2015.
- [61] M. Nouredanesh and J. Tung, "IMU, sEMG, or their cross-correlation and temporal similarities: Which features detects lateral compensatory balance reactions more accurately?," *Comput. Methods Programs Biomed.*, p. 105003, Aug. 2019.
- [62] D. De Venuto, V. F. Annese, M. de Tommaso, E. Vecchio, and A. L. S. Vincentelli, "Combining EEG and EMG signals in a wireless system for preventing fall in neurodegenerative diseases," in *Ambient Assisted Living*, Springer, 2015, pp. 317–327.
- [63] R. Castaldo, P. Melillo, R. Izzo, N. De Luca, and L. Pecchia, "Fall prediction in hypertensive patients via short-term HRV Analysis," *IEEE J. Biomed. Heal. Informatics*, vol. 21, no. 2, pp. 399–406, 2017.
- [64] C. M. el Achkar, C. Lenoble-Hoskovec, A. Paraschiv-Ionescu, K. Major, C. Büla, and K. Aminian, "Instrumented shoes for activity classification in the elderly," *Gait Posture*, vol. 44, pp. 12–17, 2016.
- [65] F. J. Ordóñez and D. Roggen, "Deep convolutional and LSTM recurrent neural networks for multimodal wearable activity recognition," *Sensors (Switzerland)*, vol. 16, no. 1, 2016.
- [66] E. Twardzik *et al.*, "What features of the built environment matter most for mobility? Using wearable sensors to capture real-time outdoor environment demand on gait performance," *Gait Posture*, vol. 68, no. November 2018, pp. 437–442, 2019.
- [67] L. V. Ojeda, P. G. Adamczyk, J. R. Rebula, L. V. Nyquist, D. M. Strasburg, and N. B. Alexander, "Reconstruction of body motion during self-reported losses of balance in community-dwelling older adults," *Med. Eng. Phys.*, vol. 64, pp. 86–92, 2019.
- [68] A. Hickey, S. Del Din, L. Rochester, and A. Godfrey, "Detecting free-living steps and walking bouts: validating an algorithm for macro gait analysis," *Physiol. Meas.*, vol. 38, no. 1, p. N1, 2016.
- [69] K. Taylor *et al.*, "Context focused older adult mobility and gait assessment," in *Proceedings of the Annual International Conference of the IEEE Engineering in Medicine and Biology Society, EMBS*, 2015, vol. 2015-Novem.
- [70] M. Nouredanesh, A. McCormick, S. L. Kukreja, and J. Tung, "Wearable vision detection of environmental fall risks using convolutional neural networks," *arXiv Prepr. arXiv1611.00684*, 2016.
- [71] M. Nouredanesh, A. McCormick, S. L. Kukreja, and J. Tung, "Wearable Vision Detection of Environmental Fall Risks using Convolutional Neural Networks," *arXiv Prepr. arXiv1611.00684*, 2016.
- [72] S. Lord, B. Galna, J. Verghese, S. Coleman, D. Burn, and L. Rochester, "Independent domains of gait in older adults and associated motor and nonmotor attributes: validation of a factor analysis approach," *Journals Gerontol. Ser. A Biomed. Sci. Med. Sci.*, vol. 68, no. 7, pp. 820–827, 2012.
- [73] S. Lord, B. Galna, and L. Rochester, "Moving Forward on Gait Measurement : Toward a More Refined Approach," vol. 28, no. 11, pp. 1534–1543, 2013.



**Conflict of interest**

The authors:

Mina Nouredanesh (m2noured@uwaterloo.ca), Alan Godfrey (alan.godfrey@northumbria.ac.uk), Jennifer Howcroft (jenny.howcroft@uwaterloo.ca), Edward D Lemaire (elemaire@ohri.ca), and James Tung (james.tung@uwaterloo.ca)

declare that they have no conflict of interest.