

We are IntechOpen, the world's leading publisher of Open Access books Built by scientists, for scientists

4,800

Open access books available

122,000

International authors and editors

135M

Downloads

Our authors are among the

154

Countries delivered to

TOP 1%

most cited scientists

12.2%

Contributors from top 500 universities



WEB OF SCIENCE™

Selection of our books indexed in the Book Citation Index
in Web of Science™ Core Collection (BKCI)

Interested in publishing with us?
Contact book.department@intechopen.com

Numbers displayed above are based on latest data collected.
For more information visit www.intechopen.com



Augmented Reality Assisted Upper Limb Rehabilitation Following Stroke

Kimberlee Jordan and Marcus King
*Industrial Research Ltd.
New Zealand*

1. Introduction

Stroke is a rapidly developing loss of brain function(s) resulting from lack of blood flow caused by either a blockage, or a hemorrhage (Sims & Muyderman, 2009). Common motor impairments after stroke include muscle weakness, reduced reaction time, loss of joint range of motion and disordered movement organization: hemiparesis or weakness on one side of the body is common. It is widely regarded as a leading cause of disability in the developed world (Adamson et al., 2004). For survivors of stroke, these impairments can severely limit daily activities and participation in social and family environments (Merians et al., 2002; Werner & Kessler, 1996). The upper limb (UL) in particular remains problematic post stroke. Whereas up to 83% of stroke survivors learn to walk again (Skilbeck et al., 1983), it is estimated that only 5 to 20% of stroke survivors attain complete functional recovery of their affected UL (Kwakkel et al., 2003). This may be in part because the high costs of standard therapy mean that treatment frequently ceases once patients are released from acute care and long term outcomes are often poor (Feys et al., 1998; Carter et al., 2006). Another possibility is that it is possible for the patient to learn to use their unaffected arm almost exclusively for most activities of daily living, whereas the patient has no choice but to use both legs for walking (Feys et al., 1998; Kwakkel et al., 1999). Additionally, significant loss of hand function may cause some people to abandon any residual function in that hand through learned non-use (Sterr et al., 2002).

Best practice rehabilitation requires multiple trained personnel up to 30 hours of therapy a week (anon, 2007), but this is seldom achieved and outcomes of conventional therapy are poor (Feys et al., 1998). Evidence suggests that repetitive training of functional UL motor tasks (Van Peppen et al., 2004; Kwakkel et al., 1999; van der Lee, 2001); intensity of practice, and functional relevance of the motor tasks (French et al., 2009; Butefisch et al., 1995) are the critical components of successful UL rehabilitation. Neuroplasticity is the process by which neural circuits in the brain are modified by experience, learning and/or injury (e.g. Nudo, 2003) that allows for motor-relearning and recovery after stroke. A large number of repetitions of the same movement pattern forms the physiological basis of motor learning and is thus an essential component of motor-relearning (Butefisch et al., 1995). Animal studies indicate that as many as 400 to 600 repetitions per day may be required to induce changes in neuroplasticity following stroke (Nudo et al., 1996). But repeated motor activity on its own is not sufficient however to promote recovery: the specificity and functionality of

the repeated task is also an important consideration associated with functional recovery (Butefisch et al., 1995; Nudo et al., 1996; Plautz et al., 2000).

Subjective well-being is reduced one year post stroke and this is mainly attributed to poor arm function (Wyller et al., 1997). However, improvements in outcomes can be seen up to 3 years post stroke (Stinear et al 2007), well past the point at which standard rehabilitation therapy stops (Stein et al., 2009). There is, therefore, a clear need for effective UL rehabilitation tools that provides large repetition of functional movements and can be used in a home setting without the constant supervision of a therapist.

2. Robot assisted rehabilitation therapy

From the stand point of the therapist, the large number of repetitions necessary for effective rehabilitation is very labour intensive. Robot-assisted physiotherapy (e.g. robotic or automated exercise machines) can help in alleviating therapist work load by providing autonomous training where patients can engage in repeated and intense practice of goal-directed tasks (Prange et al., 2006). For example, Krebs et al (2008) describe a 2 DOF robot, the MIT Manus, that trained shoulder and elbow movements in a horizontal plane, although robots can be used for “teaching a trajectory” or “enabling a movement through minimal assistance”, the amount of guidance for maximising recovery is not known (Adamovich, 2009). Robotic-assisted therapy devices can also provide an objective and reliable means of monitoring patient progress, and can be used in conjunction with computer-based augmented or virtual reality environments, leading to improvements in motor function (Fasoli et al., 2003; Krebs et al., 2002; Kwakkel et al., 2008).

Reports indicate that robotic therapy can improve motor control in stroke survivors to a greater extent than conventional therapy and results of clinical trials using these systems to rehabilitate the UL are positive (Prange et al., 2006). However, this is likely to be due primarily to the greater intensity of practice that can be achieved using these devices (Kwakkel et al., 2008).

There is a crucial need to improve the cost-to benefit ratio of robot-assisted therapy and their effectiveness in rehabilitation of the impaired arm (Johnson et al., 2007). The rehabilitation interventions described in Kwakkel et al. (2008) require patient time on the devices of an average of 48 min per day for 8 weeks. A 6-axis robot can be expected to cost about US\$60,000 and deployment (e.g., training, programming, adding tools etc.) may cost another US\$200,000. Such a capital item, with a depreciation rate of say 15%, operating 40 h per week, would need to be charged at US\$19/h, meaning that robotic arm treatment of one patient’s rehabilitation programme will cost US\$800 in capital depreciation alone, regardless of maintenance, running or therapist costs (King et al., 2010). Peattie et al. (2009) describe a reaching training robot, based on an armskate (Fig 1), using a personal computer as the controller. If a low-cost (under US\$1000) peripheral device for a personal computer can supply a beneficial therapy, the cost-effectiveness of such therapies would be significantly improved and clinical uptake will be expedited.

3. Virtual reality rehabilitation

Virtual reality (VR) allows the user to interact with a simulated “real” environment via dedicated computer hardware and software (Holden & Dyer, 2002). It potentially provides a




Fig. 1. Robotic armskate with PC controller for UL rehabilitation.

user with a disability a stimulating experience, engaging and motivating to the practice of UL movements as the user manipulates the interface device (Sviestrup, 2004). VR allows the creation and control of dynamic 3-dimensional, ecologically valid stimulus environments within which behavioral response can be recorded and measured, thereby offering clinical assessment and rehabilitation options not available with traditional methods (Schultheis & Rizzo, 2001).

Studies have reported increased participant motivation, enjoyment or perceived improvement in physical ability following the inclusion of VR into stroke rehabilitation (Broeren et al., 2008; Housman et al., 2009; Yavuzer et al., 2008). Importantly, computer games can improve compliance with prescribed rehabilitation exercises (Kwakkel et al., 2008).

Assistive devices may be combined with virtual reality in order to provide a valuable rehabilitation experience for stroke survivors. For example Pyk et al. (2008) describe a combination of data gloves and virtual reality for UL rehabilitation in children with motor deficits.

3.1 The Able-X

Industrial Research Ltd (IRL) developed the Able-X for UL rehabilitation of stroke survivors who are able to move their arm against gravity, but have minimal strength or control over their actions (Hijmans et al., 2011). It is a light-weight handlebar (Fig 2) which contains a

motion sensitive game controller (CyWee Z, Taiwan) that interfaces with a PC. The Able-X couples the arms so that the unaffected arm can assist movement of the hemiparetic arm.

A suite of computer games provided a graduated series of physical challenges, from target hitting games, to faster sports games, as well as some casual and puzzle games.



Fig. 2. Against-gravity bilateral exercise device that interacts with computer games.

3.2 Able-X pilot study

3.2.1 Able-X participants

To trial the system fourteen participants with post-stroke UL hemiparesis were recruited: their mean age was 71 years (range 47-85); nine were male, five female; time since stroke one to six years; eight had a stroke in their left hemisphere and six in their right and in nine participants the dominant hand was affected while in five it was the non-dominant.

3.2.2 Able-X assessment, outcome measures and Intervention

Assessments were conducted after enrolment in the study (T0). A 2.5 week sham-intervention was provided which consisted of playing mouse based computer games on a personal computer using their unaffected arm for eight to ten sessions, each lasting at least 45 minutes. Following this, participants were re-assessed (T1). There was a 2 ½ week period where no

intervention was provided, after which participants were again re-assessed (T2). The 2.5 week intervention was then performed and consisted of playing computer games with the Able-X for eight to ten therapist supervised sessions lasting 45 to 60 minutes. Game difficulties were adjusted to match the ability of the participant and progressed as participant ability improved. Finally the participants were reassessed (T3). The Fugl Meyer Upper Limb assessment (FMA-UL) (Fugl-Meyer, 1975) was the primary outcome measure. Additional outcome measures were the DASH (Disabilities of the Arm, Shoulder and Hand), a questionnaire for self reported symptoms and abilities in certain activities (Beaton et al., 2001) and the WOLF test (Wolf Motor Function Test for functional movement (Wolf & Catlin, 2001)).

3.2.3 Able-X results

The Able-X intervention resulted in a significant improvement in UL motor performance as measured by the FMA-UL (Table 1). The mean improvement post intervention (T3) ranged from 4.2 (compared to T2) to 5.2 (compared to T1). These results are especially encouraging in light of the fact that the group comprised adults with chronic stroke and the cohort was heterogeneous (FMA-UL ranged from 14 to 65 at inclusion). Post-intervention focus groups showed that participants enjoyed the experience and reported perceived gains in UL movement, concentration and balance.

	T0	T1	T2	T3	F	p
FMA-UL (n=13)	44.2±17.9	44.0±17.2	45.0±16.2	49.2±16.6	10.41	<0.001
WMFT (n=13)	32.7±50.4	32.4±50.6	31.5±50.9	30.5±51.2	2.74	0.06
DASH (n=13)	51.8±21.5	54.5±23.4	55.0±24.4	55.6±23.2	0.66	0.58

Table 1. Means ± standard deviation of the outcome measures pre-control (T0), post-control/pre-washout (T1), post-washout / pre-intervention (T2), and post-intervention (T3).

3.3 Able-X home care pilot study

To test use of the system in an unsupervised home situation, three participants from the above trial were asked to use the system at home for 8 weeks. Participants were assessed prior to the intervention (T1); the systems were left with them for up to 61 days; after which they were reassessed (T2). As patient self-reports are suggested as the best method of evaluating adherence to home-based physiotherapy (Bassett, 2003), participants diaries of usage and the Intrinsic Motivation Inventory (McAuley, 1987) were the outcome measures.

Participant	J	D	W
IMI: average	70%	70.5%	49%
Diary: number of sessions in intervention	44 / 55 days	46 / 58 days	49 / 61 days
Diary: Average session duration (minutes)	46	35	38
Diary: Average sessions per week	5.5	5.5	4.5

Table 2. IMI and diary results for unsupervised homecare therapy using Able-X.

The diaries (Table 2) indicated that all of participants continued therapy at a rate of from 4.5 to 5.5 sessions per week and maintained that throughout the 8 week period. The IMI results

suggest that the therapy successfully motivated the participants. Patient motivation and compliance with prescribed exercise/practice is a key component of successful home-based therapy or telerehabilitation. We have shown this can be provided with a computer game therapy system that did not rely on regular therapist prompting to exercise.

4. Augmented reality rehabilitation

In contrast to VR, Augmented Reality (AR) superimposes a computer-generated image on a user's view of the real world, thus providing a composite view, which has significant advantages over VR for neurorehabilitation. Neurological injuries, such as stroke, cause considerable environmental impoverishment due to the stroke survivor's either limited ability or inability to interact physically with their environment (Stein et al., 1995). There is substantial literature on the negative impact of impoverished environments and their effects on the cortex in rats and primates (Renner & Rosenzweig, 1987). Similarly there is evidence to suggest that enriching an environment has a beneficial effect on both behavioural and cognitive function in brain damaged animals. Although more research on humans is necessary, there is general agreement that this holds for humans too (Rose et al., 1998). There is widespread agreement amongst clinicians that the reduction of interaction with the physical environment resulting from stroke is detrimental to recovery of function (Rose et al., 2005). Thus a key factor in successful stroke rehabilitation is whether the patient's level of interaction with their environment can be dramatically increased.

Augmented environments offer a unique rehabilitation solution for stroke survivors in that the information within the environment and the way in which patients interact with this information can be controlled very specifically (Levin, 2011; Rose et al., 1998). Many of the physical issues giving rise to a stroke-induced impoverished environment can be solved or circumvented using augmented environments. For example, a given sensory aspect or modality can be emphasised or augmented to make up for other sensory loss. If a patient is unable to walk through their physical environment, VR or AR can be combined concurrently with a robotic walking aid, e.g. Hocoma Locomat, therapy to provide visual flow and thus the overall sensation of moving through an environment. In fact the computer technology underlying AR is ideally suited to delivering an enriched environment to humans with disabilities as it is generally possible to cater for whatever motor capability an individual may have. Similarly the particular sensory aspects of an environment may be augmented to offset partial sensory loss.

Because of the above, augmented environments have the potential to be highly engaging for patients undergoing rehabilitation, leading to greater levels of compliance. Approximately 65% of patients are likely to be non-adherent to physical therapy rehabilitation programmes, to varying degrees (Bassett, 2003). Additionally, Tinson (1989) found that stroke patients within a rehabilitation unit spent 30 - 40% of their time in "disengaged and inactive tasks" and only 30-60 minutes per day in formal therapy. It is crucial that a person engaged in rehabilitation following neurological injury is engaged in their therapy and an augmented reality rehabilitation has the potential to fill some of the patient "down-time" with valuable therapeutic activity.

AR environments and the skills practiced or learned within them can be tailored according to a patient's impairment(s) in terms of task complexity, required response(s), sensory

presentation, type and amount of feedback provided (Holden, 2005). Particular elements can be enriched or downplayed as required to exploit principles of motor learning and plasticity (Rose et al., 2005; Levin 2011). Particular elements of a task can be shown selectively to highlight the relevant information. For example, the specifications for reaching movements are determined from observation of the end point trajectory of a moving limb. This can therefore be highlighted to focus the attention of the patient onto the relevant information. Effectively this reduces the complexity of the environment in terms of clutter and unnecessary information that may distract and/or frustrate the patient.

Feedback is a critical component to motor learning which is easily manipulated in an augmented environment and can be delivered in a variety of different ways. Holden (2005) suggests creation of a virtual teacher for demonstration of movements. The virtual teacher has the advantage that they can perform an unlimited number of repetitions (unlike a human therapist). Many studies have investigated the VR environment for stroke rehabilitation, but few have shown effective transfer of training to the real world. Pridmore et al. (2004) discussed how moving VR environments closer to the real world will ease the transfer of rehabilitation activities into daily life. This means moving to the right of the continuum shown in fig 3, i.e. making use of AR. Rand et al. (2005) found that older adults prefer a head-mounted display to seeing an image projected on a screen, which is an example of elderly users requiring the environment to be closer to reality than younger people do.




Fig. 3. Technologies across the virtual divide (Pridmore et al., 2004).

A significant advantage of AR is that it provides for activation of mirror neurons, thought to be the basis of imitative learning. A mirror neuron is one that fires when someone either acts or observes a goal directed action performed by another (Rizzolatti & Craighero, 2004). However, they do not fire when a simple movement is executed or observed, so a task must be associated with the movement (Gallese et al., 1996). Mirror neurons have a direct input to the motor cortex and a role for these neurons in recovery from stroke has been suggested by several authors (Eng et al., 2007; Ramachandran & Altschuler, 2009; Sathian et al., 2000). Human fMRI and TMS studies have shown increased mirror neuron activity and formation of motor memories during learning of new motor tasks by imitation or action-observation (Buccino et al., 2004; Stefan et al., 2005).

Observation of another individual performing a motor training task (action observation) results in increased cortical excitability of the primary motor cortex and can enhance the beneficial effects of motor training on motor memory formation in patients with chronic stroke (Celnik et al., 2008). The mirror system plays the role of 'movement organizer' and is sensitive therefore to observation and thereon action. Preliminary data indicate that the

action / observation approach may produce significant clinical results (Ertelt et al., 2007). The action/observation/execution mechanism requires the stroke survivor to view their hemiparetic arm carrying out the task, even though it may be too weak to function independently and this can stimulate the cortical mirror neurone system.

A related treatment, mirror box therapy has been shown to be effective in UL stroke therapy (Sütbeyaz et al., 2007; Yavuzer et al., 2008). Mirror box therapy, was originally developed to reduce phantom pain in amputees by Ramachandran et al. (1995). The patient places their stump into a box which has mirrors arranged so that the image of the good limb appears to be superimposed onto the stump of the amputated or phantom limb. When the patient moves their good limb, it appears as if their lost limb is also moving and through the use of this artificial visual feedback it becomes possible for the patient to "move" the phantom limb, and to unclench it from potentially painful positions. This demonstrates a real-world attempt to create an AR environment for rehabilitation.

4.1 The Able-B: an AR mirror box for stroke rehabilitation

AR therapy may be utilised to stimulate a similar experience to mirror box therapy and we have developed the Able-B (Figure 3) based on these principles as well as bilateral UL exercise therapy (Caraugh et al., 2005; McCombe-Waller et al., 2008). This device is designed to facilitate re-learning of reaching movements for patients who are either unable or have great difficulty moving their hemiparetic arm. The patient can use the strength of their unaffected arm to assist the hemiparetic arm as required while observing the mirrored movement of the impaired arm through the AR system. The patient sits with both arms in the moulded forearm supports, held in place using padded velcro straps. The hands rest on either a palmar mound or a joy-stick style handle, depending on user preference. The Able-B provides a platform for high repetition, intense bilateral exercise within a relatively low-cost package that decreases therapist supervision requirements and allows persons with more severe UL hemiparesis to exercise independently (Sampson et al., 2011).

4.2 The software

It is necessary to create a specific set of games for rehabilitation of stroke survivors, who are generally over 65 years old. Stroke often results in reduced attention span, short term memory and problem solving skills (anon, 2009) and most computer games are very fast and provide negative feedback when losing (IJsselsteijn, 2007). We have developed a suite of computer games to provide a graduated series of physical challenges, from stationary target hitting games, to strategic target hitting games, to moving target hitting games. These games always provide positive feedback for actions performed and do not have significant memory or problem solving challenges. The graphics are large sized, in high contrast colours and the movements do not require fast reactions. Use of sound is maximised, so that every time an object appears and every time an interaction occurs, a sound is provided.

All games required large cursor movements in both horizontal and vertical directions. The games are presented using a simple AR environment using a web camera and conventional computer monitor as display. The computer game characters were superimposed over the image of the stroke-affected arm and hand (fig 5) to create an action/observation/ execution scenario within an affordable and easy to implement AR environment.




Fig. 4. Able-B to allow an individual to exercise their hemiparetic right arm, using AR to show their hemiparetic arm interacting with a computer game.

A web camera is used to display the hemiparetic arm (Fig 3) on the monitor such that it appears to interact with the computer games. Using color-tracking software, a colored patch attached to the hand acts as a “computer mouse” to play specially designed games.




Fig. 5. The series of computer images of the four AR games used for arm reaching exercises.

4.3 Able-B case study

4.3.1 Able-B participants

To test the efficacy of the Able-B, five post-stroke participants with UL hemiparesis were recruited: their mean age was 61.8 years (range 45 – 76 years); 3 were male, 2 were female; all were right dominant with 3 participants having right hemiparesis and 2 having left hemiparesis. The mean time post stroke that the intervention was started was 45.2 weeks (range 9 – 64 weeks) and participants were free of other neurological deficits.

4.3.2 Able-B assessment, Outcome measures and Intervention

Assessors conducted blinded assessments of the trial participants, in the week prior to the start of intervention (T0) and in the week following the cessation of interventions (T1). The FMA-UL was the primary outcome measure and participant motivation was assessed using the Intrinsic Motivation Inventory (IMI) after the intervention.

Participants completed 6 weeks of Able-B + AR intervention consisting of therapist supervised, 45 minute sessions, 4x/week. Game difficulties were adjusted to match the ability of the participant and progressed as participant ability improved.

4.3.3 Able-B results

Overall the results indicate a positive effect from intervention using the Able-B system (Table 3), with the FMA-UL score increase ranging from 1 to 5 points after 6 weeks of therapy.

Fugl-Meyer Upper extremity scores (/66)			
Participant	T0 (Wk 0)	T1 (Wk 7)	Change
1	16	21	5
2	15	18	3
3	7	11	4
4	19	20	1
5	7	9	2

Table 3. FMA-UE scores before and after Able-B therapy.

The results of the IMI ranged from 80% for participant 4 to 95% for participant 2, indicating that all participants were highly motivated to comply with the Able-B therapy.

4.4 AR rehabilitation using a polished board

Polished board or armskate exercising is designed for patients who have some ability to move their hemiparetic arm, provided they are supported against gravity e.g. by sliding their arm across a polished table top. King et al. (2010) describes an affordable, computerised table-based exercise system using AR in conjunction with such an exercise regime (fig 6).



Fig. 6. AR arm rehabilitation using polished board, showing the virtual butterfly net superimposed on the image of the hand.

4.5 AR and polished board case study

4.5.1 AR and polished board: participants

To test the concept of integrating AR with a simple reaching exercise, four participants with UL hemiparesis as a result of stroke were recruited. The age ranged from 55 to 85; time since stroke ranged from 2 to 12 years; three were male and one female; two were left side hemiparetic, and all were right hand dominant; all participants were free of other neurological deficits.

4.5.2 AR and polished board: assessment, outcome measures and intervention

The FMA-UL was the primary outcome measure, but additional outcome measures were the WOLF and the DASH. Assessors conducted pre- (T0) and post-intervention (T1) assessments.

Participants completed 4 weeks of AR and polished board intervention consisting of 8 supervised sessions which lasted 45 minutes each. An overhead mounted web camera using the computer vision algorithm ARToolkit (HIT Lab, University of Canterbury, NZ), tracked the position of a fiducial marker attached to the user's hand. A computer game showed a butterfly net superimposed over the user's hand. The user placed the marker on a cross marked in the centre of the screen to start the game. Virtual butterflies "flew" from eight

evenly spaced different directions, starting at the outer edge of the screen and traveling towards the centre at a fixed speed. The user's task was to move their hand to the outside of the screen to "catch" the butterfly in the net (Figure 6). After the butterfly was caught, the user moved back to the centre cross and the next butterfly appeared. After all 8 butterflies had been caught, the time taken, and therefore the distance moved in each direction was shown with a graph.

4.5.3 AR and polished board case study results

This study indicated a positive effect of the therapy (Table 4) with two participants increasing their FMA-UL scores and Wolf times significantly. Interestingly their self-reported standard of life as shown by the DASH, showed a decrease for two participants, possibly as a result of the focus of attention on their arm impairment.

No	Fugl-Meyer (/44)			Wolf, average time /task (sec)			DASH (/100)		
	T0	T1	Change	T0	T1	Change	T0	T1	Change
1	33	33	0	34.3	24.5	-9.8	33.3	34.2	0.9
2	10	17	7	84.0	77.0	-7.0	67.5	71.7	3.2
3	31	31	0	43.4	44.4	1.0	-	-	-
4	36	42	6	4.2	4.1	-0.1	21.7	40.0	18.3

Table 4. Results of the outcome measures pre and post ARS intervention for the 4 participants.

5. A computer assisted upper limb rehabilitation system for stroke

We have developed a computer assisted UL rehabilitation system which combines the advantages of both AR and VR with three assistive devices that provide a lower cost alternative to rehabilitation robotics for training of shoulder and elbow reaching. The Able-X and Able-B described above are suitable for people with severe and mild arm movement impairments. A third device, the Able-M has been designed to enable the delivery of the AR with polished board exercises in a rehabilitation setting.

5.1 The able-M

The Able-M is designed for patients who have some ability to move their hemiparetic arm, provided they are supported against gravity. It is based on a traditional arm-skate or sliding board to provide gravity support while practising reaching exercises across a tabletop. The Able-M (Fig 7) interacts with the computer in the same way as a wireless computer mouse, controlling the cursor of the PC. A button, which acts as the mouse clicker switch, is flexibly mounted to position it around the dorsal side of the hand or fingers, hence requiring finger or wrist extension exercises to operate.

5.2 The suite of devices

The assistive devices allow people with hemiparesis to interact with a computer during rehabilitation exercises, providing a system which can be aligned to the degree of



Fig. 7. Able-M, a gravity supported arm exercise device that interacts with computer games.

impairment, or weakness presented by the patient. Fig 8 shows the relationship of the components of the system to the patient’s strength as measured by the Oxford scale of muscle strength (Parkinson, 2000).

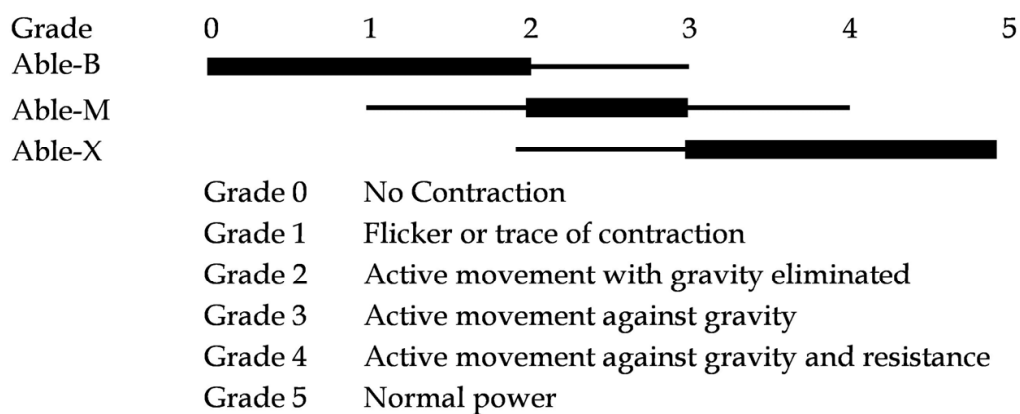


Fig. 8. IRL devices aligned to level of strength.

6. Discussion

There is significant amount of evidence to show that learning in a virtual environment can transfer to the real environment. However, there is also evidence that transfer of rehabilitation training into real world activities of daily living is easier if the training is

carried out in as close to the real environment as possible. Therefore, the AR environment has potential for better rehabilitation outcomes than a VR environment.

Mirror neurons were first described in 1992 so the use of mirror therapy is relatively new. AR seems to be an ideal method for bringing mirror therapy to people with a variety of disabilities or injuries. The development of a suite of devices that can bring this technology into a homecare situation, for people to rehabilitate themselves, with minimal supervision from clinicians, has potential to allow delivery of rehabilitation to a large numbers in a cost effective manner. The operating range of the three IRL devices is wide enough to provide smooth transition and overlap from one to the next, thereby allowing a person to exercise at their own rate until they are able to “graduate” from one to the next. The suite demonstrates the application of a systems approach to the rehabilitation of the UL.

Although the quantity of UL repetitions per session were not recorded, they were estimated (conservatively based on the game parameters set during sessions) to range from 600 to 1000 per 45 min session for each of the 3 devices, depending upon which games were used. Lang et al. (2009) found that in typical stroke rehabilitation units, 32 UL repetitions per session was typical, so this is greater than many conventional UL therapy sessions and would compare favourably with other non-robotic platforms with or without AR or VR. The Able-X results are comparable to more intensive robotic-aided therapies reported previously, with improvements on the FMA-UL of between 3 and 6 (Prange et al., 2006).

Computer game play has been shown to be very motivating for stroke survivors to undertake as part of a rehabilitation programme, even without supervision. However, it is important that the game play actually constitutes task-based movements, because the mirror neuron system is only activated when task are undertaken, rather than when passive movements are made. Further research is required to ensure that AR gameplay activates these neural regions, leading to learning and recovery.

7. Future directions / considerations

Our research has been carried out with small numbers in pilot trial situations. Larger randomised, controlled trials across multiple centres are necessary for clinical validation of these devices. Future clinical research should be aimed at developing protocols for rehabilitation using the range of devices and software or games that may be used with the devices. Additionally, for delivery of a rehabilitation service to stroke survivors, products must meet medical devices standards.

Brain imaging (e.g. fMRI, EEG) should be incorporated into future research programme. This will allow clinicians to determine which patients will benefit most from specific treatments (e.g. bilateral therapy vs. unilateral therapy or AR versus VR environments). The importance of including information on lesion size and location in the planning of stroke treatment trials has also been highlighted. Incorporation of brain imaging can assist with the planning and prescription of rehabilitation (Hamzei et al., 2006). The development of functional imaging promises major advances within neuroscience and there is significant potential for combining these methods with virtual environments. The combination of neuroimaging and activity in virtual environments could be used to investigate the extent to which interaction with virtual and real environments is cognitively equivalent.

A comparison should be made between the use of VR with avatars, versus AR in a stroke affected population. Adamovich et al. (2009) suggested that VR avatars can create an observation condition and hence it may be possible to use avatars, rather than real time images of a person's limbs, to provide positive rehabilitation outcomes. The authors have recorded anecdotal statements from study participants that they do not like viewing their stroke-affected limb, due to its "old look".

The acute phase of stroke recovery is the optimal period for maximum recovery following stroke and so research must move into that area. Currently most researchers work with participants who are in the chronic stage of their stroke recovery, due to their stable baseline and the lack of interference with medical interventions by research protocols.

AR rehabilitation has a large potential for benefit to stroke survivors and the community as it can be delivered in a home environment. But it is necessary to integrate these systems with homecare, using telerehabilitation services, to ensure adherence to the programme and tailoring the service to the individual's requirements. Such systems must be robust for home installation by non-specialised technicians (e.g. physiotherapists) and daily use by the individual who may have a cognitive disability as a result of the injury.

It is not yet clear what mix of cognitive and physical rehabilitation challenges should be provided for optimal recovery following stroke. For example Schimmelpfennig (2000) found that, following orthopaedic or phlebological procedures, patients who underwent mental activation training, showed a greater motivation in rehabilitation and recovered their movement coordination quicker. This area is an ideal research opportunity for AR therapies.

Environmental enrichment, in addition to being beneficial in its own right, can optimise other treatments designed to restore function following brain damage. There is evidence of enrichment induced neuroplastic change in primates and it would be interesting to see how this translates to humans, especially in relation to an AR environment.

8. Conclusions

Neurological injury leads to environmental impoverishment and AR provides the ability to enrich the environment and increase a stroke survivor's interaction / experiences, leading to beneficial effects in terms of engagement and rehabilitation outcomes.

Improvements in UL function and isometric strength were observed during studies of augmented physical therapy utilising a combination of assistive devices and AR that allow people with UL disabilities that range from very severe hemiparesis to almost able-bodied.

Engaging in AR therapy using simple assistive devices seems to be a cost effective alternative to other forms of therapy such as robotic therapy, catering for repetitive self-supported UL exercises. It also can integrate easily with conventional physiotherapy.

Overall these studies suggest that further research on a larger sample size and range of stroke survivors with UL hemiparesis is warranted to provide a greater level of clinical evidence as to the effect of the system for people with UL hemiparesis.

The system has the potential to provide a calibrated range of exercises which can be selected to suit the physical and cognitive abilities of a patient ranging from severe hemiparesis to almost able-bodied or integrated as a systems approach to UL rehabilitation.

9. Acknowledgements

The authors wish to thank the stroke survivors and clinicians who willingly gave their time and thoughts during development of the interventions described here. All studies involving human participants were approved by the University of Otago, NZ Human Ethics Committee or by the NZ Health and Disabilities, Upper South A, Regional Ethic Committee. We thank Im-Able Ltd., New Zealand, for supporting this research through the supply of Able-X and Able-M devices.

10. References


- Adamovich, S.; August, K.; Merians, A. & Tunik, E. (2009). A virtual reality-based system integrated with fmri to study neural mechanisms of action observation-execution: A proof of concept study. *Restorative Neurology and Neuroscience*, Vol.27, No.3, pp. 209-223, ISSN 0922-6028
- Adamovich, S.; Fluet, G.; Merians, A.; Mathai, A. & Qiu, Q. (2009). Incorporating haptic effects into three-dimensional virtual environments to train the hemiparetic upper extremity. *IEEE Transactions on Neural Systems and Rehabilitation Engineering*, Vol.17, No.5, pp. 512-20, ISSN 1534-4320
- Adamson, J.; Beswick, A. & Ebrahim, S. (2004). Is stroke the most common cause of disability? *Journal of Stroke and Cerebrovascular Diseases*, Vol.13, No.4, pp. 171-177, ISSN 1052-3057
- Anon. (2007). *Post-Stroke Rehabilitation Fact Sheet*. National Institute Of Neurological Disorders And Stroke. Available from <http://www.ninds.nih.gov/disorders/stroke/poststrokerehab.htm>
- Anon. (2009). *Recovery After Stroke: Thinking and Cognition*. National Stroke Association. available from http://www.stroke.org/site/DocServer/NSAFactSheet_Cognition.pdf?docID=986
- Bassett, S. (2003). The assessment of patient adherence to physiotherapy rehabilitation. *New Zealand Journal of Physiotherapy*, Vol.31, No.2, pp. 60-66, ISSN 0303-7193
- Beaton, D.; Davis, A., Hudak, P. & McConnell S. (2001). The DASH (Disabilities of the Arm, Shoulder and Hand) outcome measure: what do we know about it now? *British Journal of Hand Therapy*, Vol.6, No.4, pp. 109-117, ISSN 1758-9983
- Broeren, J.; Claesson, L.; Goude, D.; Rydmark, M. & Sunnerhagen, K. (2008). Virtual rehabilitation in an activity centre for community-dwelling persons with stroke: The possibilities of 3-dimensional computer games. *Cerebrovascular Diseases*, Vol.26, No.3, pp. 289-296, ISSN: 1015-9770
- Buccino G.; Vogt, S.; Ritzl, A.; Fink, G.; Zilles, K.; Freund H. & Rizzolatti G. (2004). Neural Circuits Underlying Imitation Learning of Hand Actions: An Event-Related fMRI Study. *Neuron*, Vol.42, pp 323-334, ISSN1748-2968
- Bütefisch, C.; Hummelsheim, H.; Denzler, P.; & Mauritz, K. (1995). Repetitive training of isolated movements improves the outcome of motor rehabilitation of the centrally

- paretic hand. *Journal of the Neurological Sciences*, Vol.130, No.1, pp. 59-68, ISSN 0022-510X
- Carter, K.; Anderson, C.; Hacket, M.; Feigin, V.; Barber, P.; Broad, J. & Bonita, R. (2006). Trends in ethnic disparities in stroke incidence in Auckland, New Zealand, during 1981 to 2003. *Stroke*, Vol.37, No.1, pp. 56-62, ISSN 00392499
- Cauraugh, J. & Summers J. (2005). Neural Plasticity and bilateral movements: A rehabilitation approach for chronic stroke. *Progress in Neurobiology*, Vol.75, pp. 309-320, ISSN: 0301-0082
- Celnik, P.; Webster, B.; Glasser, D. & Cohen, L. (2008). Effects of action observation on physical training after stroke. *Stroke*, Vol.39, No.6, pp. 1814-1820, ISSN 00392499
- Eng, K.; Siekierka, E.; Pyk, P.; Chevrier, E.; Hauser, Y.; Cameirao, M.; Holper, L.; Hägni, K.; Zimmerli, L.; Duff, A.; Schuster, C.; Bassetti, C.; Verschure, P. & Kiper, D. (2007). Interactive visuo-motor therapy system for stroke rehabilitation. *Medical & Biological Engineering & Computing*, Vol.45, No.9, (September), pp. 901-7, ISSN: 0140-0118
- Ertelt, D.; Small, S.; Solodkin, A.; Dettmers, C.; McNamara, A.; Binkofski, F. & Buccino, G. (2007). Action observation has a positive impact on rehabilitation of motor deficits after stroke. *NeuroImage*, Vol.36, No.2, pp. 164-73, ISSN: 1053-8119
- Fasoli, S.; Krebs, H.; Stein, J.; Frontera, W. & Hogan, N. (2003). Effects of robotic therapy on motor impairment and recovery in chronic stroke. *Archives of Physical Medicine and Rehabilitation*, Vol.84, No.4, pp. 477-482, ISSN 0003-9993
- Feys, H.; De Weerd, W.; Selz, B.; Cox Steck, G.; Spichiger, R.; Vereeck, L.; Putman, K. et al. (1998). Effect of a therapeutic intervention for the hemiplegic upper limb in the acute phase after stroke: A single-blind, randomized, controlled multicenter trial. *Stroke*, Vol.29, No.4, pp. 785-792, ISSN 00392499
- French, B.; Thomas, L.; Leathley, M.; Sutton, C.; McAdam, J.; Forster, A.; Langhorne, P. et al. (2009). Repetitive task training for improving functional ability after stroke. *Stroke*, Vol.40, No.4, pp. 98-99, ISSN 00392499
- Fugl-Meyer, A.; Jääskö, L.; Leyman, I.; Olsson, S. & Steglind, S. (1975). The post-stroke patient: 1. A method for evaluation of physical performance. *Scandinavian Journal of Rehabilitation Medicine*, Vol.7, pp. 13-31, ISSN 0036-5505
- Gallese, V.; Fadiga, L.; Fogassi, L. & Rizzolatti, G. (1996). Action recognition in the premotor cortex. *Brain*, Vol.119, pp. 593-609, ISSN 0006-8950
- Hamzei, F., Liepert, J., Dettmers, C., Weiller, C., & Rijntjes, M. (2006). Two different reorganization patterns after rehabilitative therapy: An exploratory study with fMRI and TMS. *NeuroImage*, Vol.31, No.2, pp. 710-720, ISSN: 1053-8119
- Hijmans, J.; Hale, L.; Satherley, J.; McMillan, N. & King, M. (2011). Bilateral upper limb rehabilitation after stroke using a movement based game controller. Accepted for publication in *Journal of Rehabilitation Research and Development*
- Feys, H.; De Weerd, W.; Selz, B.; Cox Steck, G.; Spichiger, R.; Vereeck, L.; Putman, K. & Van Hoydonck, G. (1998). Effect of a Therapeutic Intervention for the Hemiplegic Upper Limb in the Acute Phase After Stroke. *Stroke*, Vol.29, pp. 785-792, ISSN 00392499
- Holden, M. (2005). Virtual environments for motor rehabilitation: review. *Cyberpsychology & Behavior: The Impact of the Internet, Multimedia and Virtual Reality on Behavior and Society*, Vol.8, No.3, pp. 187-211; discussion pp. 212-219, ISSN: 1094-9313

- Housman, S.; Scott, K. & Reinkensmeyer, D. (2009). A randomized controlled trial of gravity-supported, computer-enhanced arm exercise for individuals with severe hemiparesis. *Neurorehabilitation and Neural Repair*, Vol.23, No.5, pp. 505-514, ISSN 1545-9683
- IJsselsteijn, W.; Nap, H.; de Kort, Y.; & Poels, K. (2007). Digital Game Design for Elderly Users, In *Proceedings of Futureplay 2007*. (Toronto, Canada, 14-18 November 2007), pp. 17-22, ISBN 978-1-59593-943-2
- Johnson, M.; Feng, X.; Johnson, L. & Winters, J. (2007). Potential of a suite of robot/computer-assisted motivating systems for personalized, home-based, stroke rehabilitation. *Journal of NeuroEngineering and Rehabilitation*, Vol.4, pp. 6, ISSN: 17430003
- King, M.; Hale, L.; Pekkari, A.; Persson, M.; Gregorsson, M. & Nilsson, M. (2010). An affordable, computerized, table-based exercise system for stroke survivors. *Disability and Rehabilitation Assistive Technology*, Vol.5, No.4, (July), pp. 288-93, ISSN: 1748-3107
- Krebs, H. I., Volpe, B. T., Ferraro, M., Fasoli, S., Palazzolo, J., Rohrer, B., Edelstein, L., et al. (2002). Robot-aided neuro-rehabilitation: From evidence-based to science-based rehabilitation. *Topics in Stroke Rehabilitation*, Vol.8, No.4, pp. 54-70, ISSN: 1074-9357
- Krebs, H.; Mernoff, S.; Fasoli, S.; Hughes, R.; Stein, J. & Hogan, N. (2008). A comparison of functional and impairment-based robotic training in severe to moderate chronic stroke: a pilot study. *NeuroRehabilitation*, Vol.23, No.1, pp. 81-87, ISSN 1053-8135
- Kwakkel, G.; Wagenaar, R.; Twisk, J.; Lankhorst, G. & Koetsier, J. (1999). Intensity of leg and arm training after primary middle-cerebral-artery stroke: A randomised trial. *Lancet*, Vol.354, No.9174, pp. 191-196, ISSN: 0140-6736
- Kwakkel, G.; Kollen, B.; Van der Grond, J. & Prevo, A. (2003). Probability of regaining dexterity in the flaccid upper limb: Impact of severity of paresis and time since onset in acute stroke. *Stroke*, 34(9), 2181-2186, ISSN 00392499
- Kwakkel, G.; Kollen, B. & Krebs, H. (2008). Effects of Robot-assisted therapy on upper limb recovery after stroke: A Systematic Review. *Neurorehabilitation and neural repair*, Vol.22, No.2, pp. 111-121, ISSN: 1545-9683
- Lang, C.; MacDonald, J.; Reisman, D.; Boyd, L.; Kimberley, T.; Schindler-Ivens, S.; Hornby, G.; Ross, S. & Scheets, P. (2009). Observation of amounts of movement practice provided during stroke rehabilitation. *Archives of Physical Medicine and Rehabilitation*, Vol.90, No.10, (October), pp. 1692-1698, ISSN 0003-9993
- Levin, M. (2011). Can virtual reality offer enriched environments for rehabilitation? *Expert Review of Neurotherapeutics*, Vol.11, No.2, (February), pp.153-5, ISSN: 1473-7175
- Merians, A.; Jack, D.; Boian, R.; Tremaine, M.; Burdea, G.; Adamovich, S.; Recce, M. et al. (2002). Virtual reality-augmented rehabilitation for patients following stroke. *Physical Therapy*, Vol.82, No.9, pp. 898-915, ISSN 0031-9023
- McAuley, E.; Duncan, T. & Tammem, V. (1987). Psychometric properties of the Intrinsic Motivation Inventory in a competitive sport setting: A confirmatory analysis. *Research Quarterly for Exercise & Sport*, Vol.60, pp. 48-58, ISSN 0270-1367
- McCombe-Waller, S. & Whittall, J. (2008). Bilateral arm training: Why and who benefits? *NeuroRehabilitation*, Vol.23, pp. 29-41, ISSN 1053-8135
- Parkinson, M. (ed.) (2000). *Aids to examination of the peripheral nervous system*. 4th ed. W. B. Saunders, ISBN0-7020-2512-7, Edinburgh, United Kingdom

- Peattie, A.; Korevaar, A.; Wilson, J.; Sandilands, B.; Chen, X. & King, M. (2009). Automated Variable Resistance System for Upper Limb Rehabilitation, *Proceedings of Australasian Conference on Robotics and Automation 2009*, ISBN 978-0-9807404-0-0 Sydney, Australia, December 2-4, 2009
- Prange, G.; Jannink, M.; Groothuis-Oudshoorn, C.; Hermens, H. & Ijzerman, M. (2006). Systematic review of the effect of robot-aided therapy on recovery of the hemiparetic arm after stroke. *Journal of Rehabilitation Research and Development*, Vol.43, No.2, pp. 171-183, ISSN 0748-7711
- Pridmore, T.; Hilton, D.; Green, J.; Eastgate, R. & Cobb, S. (2004). Mixed reality environments in stroke rehabilitation: interfaces across the real/virtual divide. *Proceedings of International Conference on Virtual Reality, Disability and Associated Technologies*. ISBN-10: 0704911426 Oxford, United Kingdom, September 20-22, 2004
- Pyk, P.; Wille, D.; Chevrier, E.; Hauser, Y.; Holper, L.; Fatton, I.; Greipl, R.; Schlegel, S.; Ottiger, L.; Rückreim, B.; Pescatore, A.; Meyer-Heim, A.; Kiper, D. & Eng, K. (2008). A Paediatric Interactive Therapy System for Arm and Hand Rehabilitation. *Virtual Rehabilitation 2008*, pp. 127-132, ISBN 978-1-4244-2700-0 Vancouver, Canada August 25-27, 2008.
- Ramachandran, V.; Rogers-Ramachandran, D. & Cobb, S. (1995). Touching the phantom., *Nature*, Vol.377, pp. 489-490, ISSN 0028-0836
- Ramachandran, V. & Altschuler, E. (2009). The use of visual feedback, in particular mirror visual feedback, in restoring brain function. *Brain*, Vol.132, No.7, pp. 1693-1710, ISSN 0006-8950
- Rand, D.; Kizony, R.; Feintuch, U.; Katz, N.; Josman, N.; Rizzo, A. & Weiss, P. (2005). Comparison of Two VR Platforms for Rehabilitation: Video Capture versus HMD. *Presence Teleoperators and Virtual Environments*, Vol.14, No.2, pp. 147-160, ISSN 1054-7460
- Renner, M. & Rosenzweig, M. (1987). *Enriched and Impoverished Environments. Effects on Brain and Behavior*. Springer-Verlag, New York, ISBN 978-3540965237
- Rizzolatti, G. & Craighero, L. (2004). The mirror-neuron system. *Annual Review of Neuroscience*, Vol.27, pp. 169-192, ISSN 0147-006X
- Rose, F.; Attree, E.; Brooks, B. & Johnson, D. (1998). Virtual Environments In Brain Damage Rehabilitation: A Rationale From Basic Neuroscience, In *Virtual Environments in Clinical Psychology and Neuroscience*. Riva, G.; Wiederhold, B. & Molinari, E. (Eds.) Ios Press: Amsterdam, Netherlands, ISBN-10 905199429X
- Rose, F.; Brooks, B. & Rizzo, A. (2005). Virtual Reality in Brain Damage Rehabilitation: Review. *CyberPsychology & Behavior*, Vol.8, No.3, pp. 241-262, ISSN 1094-9313
- Sampson, M.; Shau, Y. & King, M. (2011). Bilateral Upper Limb Trainer with Virtual Reality for poststroke rehabilitation: case series report. *Disability and Rehabilitation: Assistive Technology*. (doi:10.3109/17483107.2011.562959), ISSN 1748-3107
- Sathian, K. Greenspan, A. & Wolf, S. (2000). Doing it with mirrors: a case study of a novel approach to neurorehabilitation. *Neurorehabilitation and Neural Repair*, Vol.14, pp. 73-76, ISSN 1545-9683
- Schimmelpfennig, L. (2000) Ohne Kopf geht's nicht. *Geistig Fit*. Vol.2, pp. 6-9, ISBN 3211836756
- Schultheis, M. & Rizzo, A. (2001). The application of virtual reality technology in rehabilitation. *Rehabilitation Psychology*, Vol.46, No.3, pp. 296-311, ISSN 0090-5550

- Sims, N. & Muyderman, H. (2009). Mitochondria, oxidative metabolism and cell death in stroke. *Biochimica et Biophysica Acta*, Vol.1802, No.1, pp. 80–91, ISSN 0006-3002
- Stefan, K.; Cohen, L.; Duque, J.; Mazzocchio, R.; Celnik, P.; Sawaki, L.; Ungerleider, L. & Classen, J. (2005). Formation of a motor memory by action observation. *Journal of Neuroscience*, Vol.25, pp. 9339–9346, ISSN 0270-6474
- Stein, D.; Brailowski, S. & Will, B. (1995). *Brain Repair*, Oxford University Press, ISBN 0195076427, New York
- Stein, J.; Harvey, R.; Macko, R.; Winstein, C. & Zorowitz, R. (2009). *Stroke recovery and rehabilitation*, Demos Medical Publishing. ISBN 978-1933864129, New York
- Sterr, A.; Freivogel, S. & Schmalohr, D. (2002). Neurobehavioral aspects of recovery: Assessment of the learned nonuse phenomenon in hemiparetic adolescents. *Archives of Physical Medicine and Rehabilitation*, Vol.83, No.12, pp. 1726-1731, ISSN 0003-9993
- Stinear, C.; Barber, P.; Smale, P.; Coxon, J.; Fleming, M. & Byblow, W. (2007). Functional potential in chronic stroke patients depends on corticospinal tract integrity. *Brain*, Vol.130, pp. 170–180, ISSN 0006-8950
- Sütbeyaz, S.; Yavuzer, G.; Sezer, N. & Koseoglu B. (2007). Mirror Therapy Enhances Lower-Extremity Motor Recovery and Motor Functioning After Stroke: A Randomized Controlled Trial. *Archives of Physical Medicine and Rehabilitation*, Vol.88, pp. 555-559, ISSN 0003-9993
- Sveistrup, H. (2004). Motor rehabilitation using virtual reality. *Journal of NeuroEngineering and Rehabilitation*, Vol.1, pp. 10, ISSN 17430003
- Tinson, D. (1989). How stroke patients spend their days: An observational study of the treatment regime offered to patients with movement disorders in hospitals following stroke. *International Disability Studies*, Vol.11, pp. 45-49, ISSN:0259-9147
- van der Lee, J.; Snels, I; Beckerman, H.; Lankhorst, G.; Wagenaar, R. & Bouter, L. (2001). Exercise therapy for arm function in stroke patients: A systematic review of randomized controlled trials. *Clinical Rehabilitation*, Vol.15, No.1, pp. 20-31, ISSN 0269-2155
- Van Peppen, R.; Kwakkel, G.; Wood-Dauphinee, S.; Hendriks, H.; Van der Wees, P. & Dekker, J. (2004). The impact of physical therapy on functional outcomes after stroke: What's the evidence? *Clinical Rehabilitation*, Vol.18, No.8, pp. 833-862, ISSN 0269-2155
- Werner, R. & Kessler, S. (1996). Effectiveness of an intensive outpatient rehabilitation program for postacute stroke patients. *American Journal of Physical Medicine and Rehabilitation*, Vol.75, No.2, pp. 114-120, ISSN 08949115
- Wolf, S. & Catlin, P. (2001). Assessing Wolf Motor function Test as outcome measure for research in patients after stroke. *Stroke*, Vol.32, pp. 1635-1639, ISSN 00392499
- Wyller, T.; Sveen, U.; Sedring, K.; Pettersen, A. & Bautz-Holter, E. (1997). Subjective well-being one year after stroke. *Clinical Rehabilitation*, Vol.11, No.2, pp. 139-145, ISSN 0269-2155
- Yavuzer, G.; Selles, R.; Sezer, N.; Sutbeyaz, S.; Bussmann, J.; Koseoglu, F.; Atay, M. et al. (2008). Mirror therapy improves hand function in subacute stroke: a randomized controlled trial. *Archives of Physical Medicine and Rehabilitation*, Vol.89, No.3, pp. 393–398, ISSN 0003-9993



Augmented Reality - Some Emerging Application Areas

Edited by Dr. Andrew Yeh Ching Nee

ISBN 978-953-307-422-1

Hard cover, 266 pages

Publisher InTech

Published online 09, December, 2011

Published in print edition December, 2011

Augmented Reality (AR) is a natural development from virtual reality (VR), which was developed several decades earlier. AR complements VR in many ways. Due to the advantages of the user being able to see both the real and virtual objects simultaneously, AR is far more intuitive, but it's not completely detached from human factors and other restrictions. AR doesn't consume as much time and effort in the applications because it's not required to construct the entire virtual scene and the environment. In this book, several new and emerging application areas of AR are presented and divided into three sections. The first section contains applications in outdoor and mobile AR, such as construction, restoration, security and surveillance. The second section deals with AR in medical, biological, and human bodies. The third and final section contains a number of new and useful applications in daily living and learning.

How to reference

In order to correctly reference this scholarly work, feel free to copy and paste the following:

Kimberlee Jordan and Marcus King (2011). Augmented Reality Assisted Upper Limb Rehabilitation Following Stroke, Augmented Reality - Some Emerging Application Areas, Dr. Andrew Yeh Ching Nee (Ed.), ISBN: 978-953-307-422-1, InTech, Available from: <http://www.intechopen.com/books/augmented-reality-some-emerging-application-areas/augmented-reality-assisted-upper-limb-rehabilitation-following-stroke>

INTECH
open science | open minds

InTech Europe

University Campus STeP Ri
Slavka Krautzeka 83/A
51000 Rijeka, Croatia
Phone: +385 (51) 770 447
Fax: +385 (51) 686 166
www.intechopen.com

InTech China

Unit 405, Office Block, Hotel Equatorial Shanghai
No.65, Yan An Road (West), Shanghai, 200040, China
中国上海市延安西路65号上海国际贵都大饭店办公楼405单元
Phone: +86-21-62489820
Fax: +86-21-62489821

© 2011 The Author(s). Licensee IntechOpen. This is an open access article distributed under the terms of the [Creative Commons Attribution 3.0 License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

IntechOpen

IntechOpen