

# Analytical Methods

Accepted Manuscript



This article can be cited before page numbers have been issued, to do this please use: M. Á. Aguirre Pastor, H. Nikolova, M. Hidalgo Núñez and A. Canals, *Anal. Methods*, 2014, DOI: 10.1039/C4AY02218A.




This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

*Accepted Manuscripts* are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

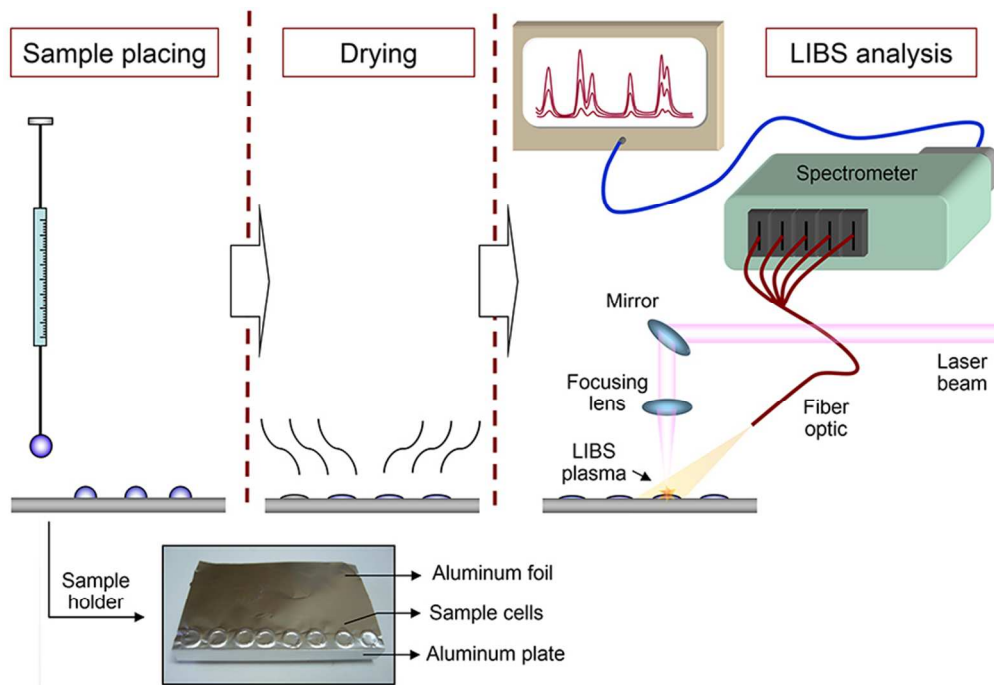

SDME-LIBS as a synergistic association for overcoming LIBS drawback in liquid analysis.  
80x55mm (300 x 300 DPI)

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26

1 **HYPHENATION OF SINGLE-DROP MICROEXTRACTION WITH**  
2 **LASER-INDUCED BREAKDOWN SPECTROMETRY FOR TRACE**  
3 **ANALYSIS IN LIQUID SAMPLES: A VIABILITY STUDY<sup>†</sup>**

View Article Online  
DOI: 10.1039/C4AY02218A

5 **M.A. Aguirre,<sup>a</sup> H. Nikolova,<sup>b</sup> M. Hidalgo<sup>a,\*</sup> and A. Canals<sup>a</sup>**

7 <sup>a</sup> Department of Analytical Chemistry and Food Sciences and University Institute of  
8 Materials, University of Alicante, P.O. Box 99 - 03080, Alicante, Spain.

9 <sup>b</sup> Department of Analytical Chemistry and Computer Chemistry, University of Plovdiv, 24  
10 Tzar Asen St., 4000 Plovdiv, Bulgaria.

11 \* Corresponding author: Tel.: +34 965903400 (Ext. 2224). Fax: +34 965903697. E-mail  
12 address: montserrat.hidalgo@ua.es (M. Hidalgo).

13 <sup>†</sup> Electronic supplementary information (ESI) available: Further experimental results.

15 **Abstract**

16 In this work, an analytical methodology based on Single Drop Microextraction (SDME)  
17 followed by Laser-Induced Breakdown Spectrometry (LIBS) has been tested for trace metals  
18 determination in liquid samples. By this method, analytes in the samples were extracted into a  
19 small volume of toluene as ammonium pyrroldinedithiocarbamate (APDC) chelates. After  
20 that, the analyte-enriched toluene was dried on a solid substrate and, finally, the resulting  
21 solid residue was analyzed by LIBS. Analyte extraction by SDME procedure was firstly  
22 optimized by using a multivariate optimization approach. Under optimum SDME conditions,  
23 analytical figures of merit of the proposed SDME-LIBS methodology were compared to  
24 those of the direct LIBS analysis method (i.e., without SDME procedure). An estuarine water  
25 certified reference material was analyzed for method trueness evaluation. The results  
26 obtained in this study indicate that SDME-LIBS methodology leads to a sensitivity increase

1 of about 2.0-2.6 times the ones obtained with LIBS. Detection limits of SDME-LIBS  
2 decreases accordingly to the obtained sensitivity improvement, reaching values in the range  
3 21-301  $\mu\text{g kg}^{-1}$  for the analytes tested. Measurement repeatability was similar in both SDME-  
4 LIBS (13-20% RSD) and LIBS (16-20% RSD) methodologies, being mainly limited by the  
5 LIBS experimental setup used in this work for LIBS analysis of liquid samples. The SDME-  
6 LIBS analysis of the certified reference material led to recovery values in the range of 96% to  
7 112%.

## 9 1 Introduction

10 Laser-Induced Breakdown Spectrometry (LIBS) is perhaps one of the most versatile  
11 techniques for elemental analysis, since it can be applied to a great variety of real-world  
12 analytical problems.<sup>1-6</sup> However, in spite of its potential for the analysis of practically any  
13 kind of sample, most LIBS applications have been focused on solid samples analysis whereas  
14 its applicability to liquid samples has been, in comparison, poorly exploited. The minor  
15 interest in LIBS analysis of liquids can be mainly attributed to its inherent experimental  
16 drawbacks,<sup>2,7,8</sup> which lead to low sensitivity and precision compared to LIBS analysis of  
17 solids or to the analysis of liquids with most conventional spectrometric techniques. Even if  
18 numerous LIBS experimental strategies have been developed to solve, or at least to reduce,  
19 the experimental drawbacks of LIBS analysis of liquid samples,<sup>9-18</sup> these methodologies still  
20 provide analytical results that are, in general, worst than those provided by other well  
21 established spectrometric techniques such as ICP-OES.<sup>19</sup>  
22 In spite of its comparatively lower sensitivity, there is still an inherent advantage that could  
23 turn LIBS into a very attractive technique for liquid samples analysis compared to the use of  
24 conventional techniques; that is the possibility for *in situ* and on-line analysis offered by this  
25 technique due to its field-operable and easily automated instrumentation.

1 A possible way to improve sensitivity and decrease limits of detection in LIBS analysis of  
2 liquid samples could be the use of a previous step for analyte enrichment. Liquid Phase  
3 Microextraction (LPME) procedures are nowadays extensively used for separation and  
4 concentration of both organic and inorganic analytes.<sup>20-22</sup> These novel microextraction  
5 methodologies are faster and more easily automatable than conventional extraction  
6 procedures and use negligible volume of extraction solvents, which are often hazardous and  
7 expensive. Among the different LPME modalities, Single Drop Microextraction (SDME),  
8 Dispersive Liquid Liquid Microextraction (DLLME) and Hollow Fibre Liquid Phase  
9 Microextraction (HF-LPME) methodologies have been applied to the concentration of  
10 inorganic analytes for trace elemental analysis with excellent results.<sup>23-30</sup> The combination of  
11 LPME with LIBS could be a promising alternative for trace elemental analysis due to the  
12 complementarity of both extraction and detection procedures; LPME usually results in a  
13 microvolume of analyte-enriched extraction solvent, which sometimes needs to be  
14 subsequently diluted to adequate it (i.e., quantity, chemical or physical properties) to the  
15 requirements of the instrumental system used for analysis (e.g., ICP-OES or FAAS). LIBS,  
16 however, has proved to be useful for the direct analysis of microvolumes of liquid samples,  
17 owing to its ability to interrogate extremely low quantities of material.<sup>31</sup> Therefore,  
18 microvolumes of solvent resulting from microextraction procedures could be easily analyzed  
19 without the need of previous dilution. An added advantage of this combination could arise  
20 from the small dimensions and possibility of automation of both LPME and LIBS  
21 instrumentation, which could make LPME-LIBS hyphenation suitable for the future  
22 development of portable systems for *in situ* and on-line analysis of liquid samples.

23 In this work, combination of LIBS with SDME modality has been tested as an analytical  
24 methodology aimed to extend the applicability of LIBS to trace elemental analysis of liquid  
25 samples, opening a new way of research on LPME-LIBS hyphenation. Here, Single Drop

1 Microextraction was applied to water samples prior to analyte determination by LIBS, in  
2 order to improve the sensitivity of the method. Toluene was used in SDME as extracting  
3 solvent of several metals as ammonium pyrrolidinedithiocarbamate (APDC) complexes.  
4 SDME procedure was previously optimized by using multivariate analysis. The resulting  
5 microvolumes of analyte-enriched solvent were analyzed by LIBS after being dried on an  
6 aluminum substrate, as a method for overcoming the experimental difficulties of LIBS  
7 analysis of liquids. Analytical figures of merit obtained with both SDME-LIBS and direct  
8 LIBS methodologies (*i.e.*, analysis of the water samples by LIBS, after being dried on the  
9 aluminum substrate but without previous SDME procedure) are presented and discussed. The  
10 proposed methodology was finally tested for determination of several metals in a certified  
11 reference material (Estuarine Water, LGC6016).

## 12 13 **2 Experimental**

### 14 **2.1 LIBS experimental setup**

15 Fig. 1 shows the LIBS experimental setup used throughout this work for liquid samples  
16 analysis. The laser-induced plasmas were generated by focusing a 10 Hz pulsed Nd-YAG  
17 laser (model HYL Handy-YAG, Q-switched, Quanta System S.P.A., Varese, Italy), emitting  
18 a pulse of energy 180 mJ (pulse width 10 ns FWHM) at 1064 nm, on the sample to analyze.  
19 The laser was focused on the sample by a N-BK7 plano-convex lens with 100 mm focal  
20 length (model KPX094AR.33, Newport Corporation, Irvine, United States). Plasma emission  
21 was collected directly with a five-furcated fiber optic (5x400  $\mu\text{m}$  fiber optic cable, model  
22 FC5-UV400-2, Avantes, Apeldoorn, The Netherlands) and was imaged on the entrance slits  
23 of a five channel spectrometer with full spectral coverage from 200 nm to 844 nm (model  
24 AVS-Rackmount-USB2 housing equipped with five preconfigured AvaSpec-ULS2048-  
25 USB2-RM channels, Avantes, Apeldoorn, The Netherlands). A delay system consisting in

1 two pulse generators (Digital delay/pulse generator, model DG 535, Stanford Research  
2 Systems Inc., Sunnyvale, USA and 1 Hz-50 MHz pulse generator, model PM-5715, Philips  
3 Export B.V., Eindhoven, The Netherlands) was used for synchronization of laser firing and  
4 data acquisition. Spectra were collected 1.3  $\mu$ s after the plasma generation (optimum  
5 condition), with 1 ms acquisition time (minimum time setting available on the spectrometer).

## 6 7 **2.2 Sample preparation**

8 Water samples containing Cr, Mn, Ni, Cu and Zn as target analytes were analyzed by LIBS in  
9 two different ways: (i) without applying any previous sample treatment for analyte  
10 concentration (*i.e.*, direct LIBS) and (ii) after a microextraction procedure with SDME  
11 methodology to separate and concentrate analytes present in the samples (*i.e.*, SDME-LIBS).  
12 In both cases, and in order to avoid liquid splashing during LIBS analysis and to enhance  
13 LIBS sensitivity and reproducibility, the corresponding liquids (*i.e.*, water sample or analyte-  
14 enriched toluene) were converted into solid by drying on an aluminum surface prior to LIBS  
15 measurement (*i.e.*, SENLIBS), as already described elsewhere.<sup>31</sup> In direct LIBS, few  $\mu$ L of  
16 the water samples were confined into a small cell shaped in an aluminum foil (see Fig. 1).  
17 The aluminum foil, placed on an 8 mm thick aluminum plate, was heated by a hot plate to  
18 completely evaporate the water. The solid residue was then irradiated with the laser for LIBS  
19 analysis.

20 In SDME-LIBS, metal ions were extracted from the water samples as ammonium  
21 pyrrolidinedithiocarbamate (APDC) complexes, using toluene as extraction solvent for  
22 SDME. After extraction, few  $\mu$ L of the analyte-enriched toluene were placed on the  
23 aluminum foil, were heated by the hot plate to completely evaporate the toluene and, as  
24 described above for direct LIBS analysis, were irradiated by the laser for LIBS measurement.



1 In both methodologies, the result of the LIBS analysis was the mean of three replicate  
2 measurements (*i.e.*, three single laser shots) made on different positions of the same solid  
3 residue.

#### 5 2.2.1 Single Drop Microextraction procedure

6 For metals extraction by SDME, approximately 9 g of sample was placed in a 20 mL glass  
7 vial containing a magnetic stir bar. Solid APDC reagent was added to the vial up to a  
8 concentration well in excess of that required to chelate all metals in the solution. Then, the  
9 solution pH was adjusted with diluted NH<sub>3</sub> and HCl solutions and, finally, the sample weight  
10 was brought to 10 g with deionized water. A microsyringe, containing a known volume of  
11 toluene, was clamped above the vial and its needle was immersed into the sample. The  
12 plunger was depressed and a microdrop of toluene was exposed to the sample at room  
13 temperature for a certain period of time, to allow partition of the analytes between the  
14 aqueous phase and the organic droplet. During this time, the solution was continuously stirred  
15 with a magnetic stirrer to accelerate the mass transfer process. After extraction, the toluene  
16 drop was retracted into the microsyringe and a microvolume of this analyte-enriched solvent  
17 was placed on the aluminum foil for LIBS analysis (Figure 1).

#### 19 2.3 Reagents and solutions

20 Aqueous calibration standards were prepared by appropriate dilution of a 1000 mg L<sup>-1</sup> mono-  
21 element standard solutions of Cr, Mn, Ni, Cu and Zn (High-purity mono-element standard  
22 solutions, Charleston, United Kingdom) in distilled deionized water (18 MΩ cm resistivity).  
23 Ammonium pyrrolidinedithiocarbamate (APDC) (Fluka, Buchs, Switzerland) was used as  
24 chelating agent. Diluted hydrochloric acid solution, prepared from a Suprapur 30% (w w<sup>-1</sup>)  
25 HCl solution (Merck, Darmstadt, Germany) and diluted ammonia solution, prepared from a



1 Reagent Grade 32% (w w<sup>-1</sup>) (in NH<sub>3</sub>) solution (Scharlau, Barcelona, Spain) were used for pH  
2 adjustment. HPLC grade toluene (Scharlau, Barcelona, Spain) was used as extraction solvent  
3 in the microextraction procedure. Estuarine water certified reference material (LGC6016,  
4 LGC Deselaeres S.L., Middlesex, United Kingdom) was used for evaluation of method  
5 trueness.

## 6

### 7 **2.4 Apparatus**

8 A 25  $\mu$ L syringe (model 1702, Hamilton, Bonaduz, Switzerland) was used to suspend the  
9 toluene microdrop inside the standard/sample solutions in the SDME procedure and to place  
10 a microvolume of water sample/extraction solvent on the metallic substrate (*i.e.*, aluminum  
11 foil) for LIBS analysis. pH measurements were performed with a pH meter (model micropH  
12 2000, Crison, Alella, Spain). The solutions were stirred with a magnetic stirrer (model 501,  
13 Darlab Egara S.L., Barcelona, Spain). A hot plate (model 500 Darlab Egara S.L., Barcelona,  
14 Spain) was used to dry the droplets before LIBS analysis.

## 15

### 16 **3 Results and discussion.**

#### 17 **3.1 Optimization of SDME experimental parameters**

18 A multivariate approach was employed to optimize the main experimental factors affecting  
19 metals extraction. Several factors including pH, APDC concentration, drop volume,  
20 extraction time and stirring speed were studied in order to maximize the extraction yield of  
21 the SDME procedure. In order to identify the most important experimental factors affecting  
22 SDME, among the ones initially considered, a previous screening study (Plackett-Burman  
23 design) was carried out. After that, significant factors were optimized by means of a  
24 Circumscribed Central Composite Design (CCCD). In the screening and optimization studies,  
25 the experiments were randomly carried out in order to nullify the effect of extraneous or

1 nuisance variables. In both cases, emission signal obtained from LIBS analysis of the  
2 resulting extractions was used as the output variable (response) of interest. Statistical  
3 software (NemrodW<sup>®</sup> version 2007, LPRAI, Marseille, France) was used for generation of  
4 the experimental design matrices and for data processing.

### 5 3.1.1 Screening study

6 A Plackett-Burman design was used for identification of the significant factors affecting  
7 SDME (screening). In this particular type of experimental design, interactions between the  
8 different factors are considered to be negligible and, therefore, significant factors can be  
9 identified using a limited number of experiments. In this study, a five-factor 12-experiments  
10 Plackett–Burman screening design was used. Each factor was represented at two levels,  
11 defining the upper and lower limits of the range covered by each factor (see Table 1). Levels  
12 chosen for the different factors were based on literature data and preliminary experiments.  
13 Synthetic aqueous solutions containing 1  $\mu\text{g g}^{-1}$  of the analytes were used as samples in all  
14 the screening experiments. After the extractions, the resulting analyte-enriched solvents were  
15 analyzed by LIBS, evaluating the emission signal obtained for the different analytes.  
16 Fig. S1 in ESI<sup>†</sup> shows the main effects Pareto charts obtained from the screening  
17 experiments. Since microextraction conditions are usually analyte-dependent, a separate  
18 screening evaluation was performed for each analyte in order to identify the common  
19 significant factors affecting the overall extraction process. Pareto charts in Fig. S1 in ESI<sup>†</sup>  
20 illustrate the order of significance of the variables affecting SDME for the different emission  
21 lines evaluated. As can be seen, these charts contain a bar for each factor, with the length of  
22 the bar being proportional to the relative influence of that factor on the metal extraction.  
23 Those bars that extend over the dashed vertical line indicate factors that are statistically  
24 significant at 95% probability. The direction of the bar is related to the “sign” of the effect  
25

1 produced by that factor. That is, those bars to the right of the origin indicate positive effect in  
2 the response when increasing the value of the factor and, on the contrary, those bars to the  
3 left indicate negative effect.

4 As observed from Fig. S1 in ESI,<sup>†</sup> the screening study provides similar results for all the  
5 emission lines evaluated. Drop volume, extraction time and pH can be considered significant  
6 factors affecting the extraction with a positive effect, with pH being the most critical  
7 parameter. On the other hand, APDC concentration and stirring speed, even if having a  
8 slightly positive effect on the response, do not produce any significant impact on extraction.  
9 These two factors were, therefore, fixed at their higher level for subsequent extractions (*i.e.*,  
10 1% (w v<sup>-1</sup>) APDC concentration; 1700 rpm stirring speed), and only drop volume, extraction  
11 time and pH were considered for optimization in the following study.

### 13 3.1.2 Optimization study

14 The three main factors identified in the previous screening study were optimized by using a  
15 Circumscribed Central Composite Design (CCCD). This experimental design requires 5  
16 levels for each factor: a central level (0), a low level (-1), a high level (+1) and two star points  
17 located at  $\pm\alpha$  ( $\alpha = 1.682$ ) from the centre of the experimental domain (0). The levels chosen  
18 for the three factors considered (*i.e.*, drop volume, extraction time and pH), as well as the  
19 location of their start points, are given in Table 2. The design matrix for this CCCD design  
20 involved a total of 18 runs. As in the previous screening study, all the experiments were  
21 carried out using synthetic solutions containing 1  $\mu\text{g g}^{-1}$  of the target analytes. LIBS signals  
22 of the different emission lines were evaluated in order to compare the optimum conditions for  
23 extraction of the different analytes and to decide, accordingly, a common optimum conditions  
24 for extraction of all of them.

1 The results obtained in this study are given in Figs. S2 to S6 in ESI<sup>†</sup> as response surfaces and  
2 contour plots. Each figure shows the results obtained for a different analyte. Graphics (a), (b)  
3 and (c) in these figures show the variation of LIBS emission signal as a function of each pair  
4 of factors, while keeping fixed the third one at its optimum value. As can be observed from  
5 the plots, all response surfaces show maximum points which are, in general, similar for all the  
6 analytes evaluated.

7 Emission signal increases with drop volume to reach a maximum at approximately 7.5  $\mu\text{L}$ . In  
8 any case, the use of larger volumes was difficult to handle since the droplet became unstable  
9 and easily fell off from the tip of the syringe needle.

10 Similar behavior was observed for pH, with signal increasing up to pH of approximately 10  
11 and decreasing thereafter. For metal cations extraction, pH plays a crucial role in the  
12 formation of the neutral chelates which can be efficiently transferred to the organic phase.

13 Low pH values favor the protonated form of the complexing reagent, therefore limiting  
14 chelates formation and, consequently, metals extraction. On the other hand, insoluble  
15 hydroxides or soluble ammonia complexes are preferentially formed at high pH values,  
16 avoiding the neutral chelates to form and leading also to a decrease in metals extraction.

17 As expected, increasing the extraction time results in an increase in the total amount of  
18 analyte extracted, reaching a maximum at around 10 minutes. Mass transfer is, indeed, a  
19 time-dependent process in which transfer rate decreases as the system approach equilibrium.

20 Due to the similarity between the optima obtained for the different analytes, average values  
21 were chosen as the common optimum condition for SDME of all of them. Thus, experimental  
22 conditions for extraction were set at pH, 10; drop volume, 7.5  $\mu\text{L}$ ; extraction time, 10 min.;  
23 APDC concentration, 1% ( $\text{w v}^{-1}$ ) and stirring speed, 1700 rpm.

24

25

### 3.2 LIBS and SDME-LIBS: analytical figures of merit

In order to assess the analytical capability of SDME-LIBS procedure versus LIBS for the analysis of trace metals in liquid samples, analytical figures of merit (*i.e.*, sensitivity, repeatability and LOD) of both analytical procedures were evaluated and compared. To this end, calibration standards were analyzed by both methods in order to obtain the corresponding calibration graphs: (i) without a previous extraction procedure (direct LIBS analysis of the standards) and (ii) after extraction of the analytes by SDME at optimum conditions. In the former method, calibration was performed by directly analyzing five calibration standards with concentrations of Zn, Mn, Cu and Cr increasing up to 2500  $\mu\text{g kg}^{-1}$  and Ni increasing up to 8000  $\mu\text{g kg}^{-1}$ . In the latter, analytes were extracted from the same number of calibration standard solutions, but with concentrations of Ni, Mn, Cu and Cr increasing up to 1000  $\mu\text{g kg}^{-1}$  and Zn increasing up to 800  $\mu\text{g kg}^{-1}$ . Afterward, the resulting analyte-enriched toluene microdroplets were analyzed by LIBS. In both cases, the experimental procedure for LIBS analysis of the liquids was that described in the experimental section (section 2.2.). That is, 7.5  $\mu\text{L}$  of the calibration standard (direct LIBS analysis) or 7.5  $\mu\text{L}$  of the resulting analyte-enriched toluene (SDME-LIBS analysis) were placed on the aluminum foil, heated to dryness and analyzed by LIBS. In all cases, LIBS analysis was carried out by averaging the LIBS signal obtained from three single laser shots in different positions on the same dried residue. Even if more laser firings could have been possibly performed on the dried residue, this number was chosen in order to completely avoid a possible overlapping of the ablated zones created in the residue by previous laser shots. Table 3 summarizes the analytical figures of merit obtained by both methods. Here, sensitivity was derived from the slope of the calibration graphs. Repeatability, expressed as RSD, was estimated from the analysis of eight aliquots taken from the same vial of 1  $\mu\text{g g}^{-1}$  calibration standard. For SDME-LIBS procedure, this means from eight extractions, one per

1 aliquot. LOD calculation was based on 3 times the standard deviation of 10 blank  
2 determinations (*i.e.*, deionized water for LIBS and toluene for SDME-LIBS). LIBS signal  
3 was found to be linear in the concentration range evaluated for each method.

4 As expected, the use of a microextraction procedure leads to sensitivity improvement for all  
5 the emission lines evaluated. The extent of this improvement can be easily assessed by  
6 looking at the enhancement factor in Table 3, which was calculated as the ratio of  
7 sensitivities obtained with and without SDME. As can be seen, all enhancement factors were  
8 in the range 2.0-2.6, without any appreciable analyte-dependence. Since sensitivity  
9 improvement for a given analyte can be directly associated with its extraction efficiency into  
10 the organic phase, this result probably indicates that all metal-APDC chelates were similarly  
11 extracted by the applied SDME procedure. As a matter of example, Figs. 2a and 2b show the  
12 signal increase observed for ZnII (202.548 nm) and NiI (352.454 nm) emission lines,  
13 respectively, when a 1  $\mu\text{g g}^{-1}$  calibration standard is analyzed by SDME-LIBS. In general  
14 terms, it seems that SDME-LIBS procedure results in analytical sensitivities that are  
15 approximately 2.3 times the ones obtained with LIBS (mean value over the five emission  
16 lines evaluated).

17 Repeatability was found to be in the range 13% - 20% RSD, without any clear trend with  
18 respect to analyte or analytical procedure. Repeatability of both analytical procedures was  
19 observed to be mainly limited by the current LIBS experimental setup for liquid samples  
20 analysis. It could be seen, by visual inspection, that the solid residue resulting from the liquid  
21 sample drying was not homogeneously distributed over the aluminum foil, thus leading to  
22 low repeatability even from replicate measurements performed on different positions on the  
23 same sample residue.

24 Detection limits were all below 0.5  $\text{mg kg}^{-1}$  for both LIBS and SDME-LIBS methodologies.

25 Without the use of SDME, LOD values ranged from 463  $\mu\text{g kg}^{-1}$  for NiI (352.454nm) to 49

1  $\mu\text{g kg}^{-1}$  for ZnII (202.548 nm). These values were reduced to  $189 \mu\text{g kg}^{-1}$  and  $21 \mu\text{g kg}^{-1}$   
2 respectively, with the use of SDME. As can be observed from Table 3, relative LODs  
3 obtained for the different emission lines were in good agreement with the corresponding  
4 enhancement factor, with the exception of Mn. This fact, as well as the comparatively high  
5 limit of detection obtained for this element, can be probably due to the presence of Mn as an  
6 impurity in the aluminum foil used as solid substrate, which leads to poor reproducibility of  
7 the blank measurements. Without considering this element, it can be seen from Table 3 that  
8 the use of SDME-LIBS results in LOD values that are approximately 2.5 times lower than  
9 those obtained with direct LIBS.

### 11 3.3 Analysis of a certified reference material

12 Method trueness was evaluated from the analysis of a certified reference material (estuarine  
13 water). Trueness test was only carried out with the proposed SDME-LIBS procedure, since  
14 certified concentrations were all below the quantification limits obtained for direct LIBS  
15 analysis. Table 4 shows the results of the estuarine water analysis. Here, percent recovery  
16 was used as estimation of method trueness. As observed, the results obtained with SDME-  
17 LIBS methodology were in good agreement with the certified values, with recovery values  
18 ranging from 96% to 112%.

## 20 4 Conclusions

21 The results obtained in this preliminary study demonstrate that LIBS detection preceded by a  
22 single drop microextraction procedure for analyte enrichment allows performing liquid  
23 samples analysis with higher sensitivity than direct LIBS. Therefore, SDME-LIBS could be  
24 considered a synergistic association for improving LIBS sensitivity drawback in liquid  
25 analysis. With the proposed SDME-LIBS analytical methodology, approximately 2.3 fold



1 sensitivity enhancement and 2.5 fold LOD improvement were obtained, compared to the  
2 direct LIBS analysis of the liquid samples (i.e., without SDME procedure). Under optimum  
3 SDME conditions, SDME-LIBS methodology lead to LOD values in the range of 21-301  $\mu\text{g}$   
4  $\text{kg}^{-1}$  for the analytes tested, being LIBS analysis performed in almost single pulse mode.  
5 However, even if the use of SDME, as LPME modality chosen in this work, has been proved  
6 to improve sensitivity of direct LIBS analysis, the obtained results can not be considered  
7 completely satisfactory for the proposed goal and should be only considered as a starting  
8 point for exploring the potentialities of this hyphenated techniques for trace elemental  
9 analysis of liquid samples. Therefore, much more research work in this field should be done  
10 in the future, aimed to improve the capability of the method.

11 On one hand, sensitivity could be further improved with the use of different reagents for  
12 metal chelation and extraction, with the use of different microextraction methodologies such  
13 as DLLME or HF-LPME, which could lead to enrichment factors higher than those obtained  
14 with SDME, or even with the application of double pulse LIBS configuration for LIBS  
15 analysis instead of single pulse LIBS, which has been demonstrated to be an efficient strategy  
16 for LIBS signal enhancement.<sup>18</sup> On the other hand, the precision of the method, currently  
17 limited by the low repeatability of LIBS measurements, could be also improved by using  
18 alternative strategies for deposition of the microdroplets on the aluminum substrate, leading  
19 to predictable and homogeneous deposits morphology, or by optimizing the LIBS system  
20 optical setup, allowing the integration of a higher number of laser shots on the solid residue  
21 without the risk of overlapping between the several ablated zones. Last but not least, future  
22 studies should also be focused on the possibility to convert the three currently separated, but  
23 independently automatable processes (i.e., microextraction, sample deposition/drying and  
24 LIBS analysis) in a fully automated SDME-LIBS analytical procedure for stand-alone  
25 operation, useful for in-situ trace metals analysis of liquid samples.

## 5 Acknowledgements

The authors are grateful to the Spanish Government (projects CTQ2011-23968) and the Regional Government of Valencia (Spain) (ACOMP/2013/072) for the financial support. M.A.A. is grateful to the University of Alicante for his PhD fellowship. This work is part of the PhD. degree of M.A.A.


## 6. References

- 1 D. A. Cremers and J. L. Radziemski, Handbook of laser-induced breakdown spectroscopy, John Wiley & Sons, Ltd., West Sussex, 2006.
- 2 J. P. Singh and S. N. Thakur, Laser-induced breakdown spectroscopy, Elsevier, Amsterdam, 2007.
- 3 R. Noll, Laser-induced breakdown spectroscopy fundamentals and applications, Springer-Verlag, Berlin Heidelberg, 2012.
- 4 D. A. Cremers and R. C. Chinni, *Appl. Spectrosc. Rev.*, 2009, **44**, 457-506.
- 5 D. W. Hahn and N. Omenetto, *Appl. Spectrosc.*, 2012, **66**, 347-419.
- 6 F. J. Fortes, J. Moros, P. Lucena, L. M. Cabalín and J. J. Laserna, *Anal. Chem.*, 2013, **85**, 640-669.
- 7 D. A. Cremers, L. J. Radziemski and T. R. Loree, *Appl. Spectrosc.*, 1984, **38**, 721-729.
- 8 A. De Giacomo, M. Dell'Aglio and O. De Pascale, *Appl. Phys. A*, 2004, **79**, 1035-1038.
- 9 B. Charfi and M. A. Harith, *Spectrochim. Acta Part B*, 2002, **57**, 1141-1153.
- 10 L. St-Onge, E. Kwong, M. Sabsabi and E. B. Vadas, *J. Pharm. Biomed. Anal.*, 2004, **36**, 277-284.
- 11 O. Samek, D. C. S. Beddows, J. Kaiser, S. V. Kukhlevsky, M. Liška, H. H. Telle and J. Young, *Opt. Eng.*, 2000, **39**, 2248-2262.

- 1  
2  
3  
4 1 12 Y. Feng, J. Yang, J. Fan, G. Yao, X. Ji, X. Zhang, X. Zheng and Z. Cui, *Appl. Opt.*, Article Online  
5  
6 2 49, C70-C74. DOI: 10.1039/C4AY02218A
- 7  
8 3 13 C. Janzen, R. Fleige, R. Noll, H. Schwenke, W. Lahmann, J. Knoth, P. Beaven, E.  
9  
10 4 Jantzen, A. Oest and P. Koke, *Spectrochim. Acta Part B*, 2005, **60**, 993-1001.
- 11  
12 5 14 Y. Godwal, G. Kaigala, V. Hoang, S. L. Lui, C. Backhouse, Y. Tsui and R.  
13  
14 6 Fedosejevs, *Opt. Express*, 2008, **16**, 12435-12445.
- 15  
16 7 15 A. Sarkar, S. K. Aggarwal, K. Sasibhusan and D. Alamelu, *Microchim. Acta*, 2010,  
17  
18 8 **168**, 65-69.
- 19  
20 9 16 D. Alamelu, A. Sarkar and S. K. Aggarwal, *Talanta*, 2008, **77**, 256-261.
- 21  
22 10 17 V. Lazic, S. Jovicevic, R. Fantoni and F. Colao, *Spectrochim. Acta Part B*, 2007, **62**,  
23  
24 11 1433-1442.
- 25  
26 12 18 V. N. Rai, F. Y. Yueh and J. P. Singh, *Appl. Opt.*, 2008, **47**, G21-G29.
- 27  
28 13 19 P. Fichet, M. Tabarant, B. Salle and C. Gautier, *Anal. Bioanal. Chem.*, 2006, **385**, 338-  
29  
30 14 344.
- 31  
32 15 20 A. Spietelun, Ł. Marcinkowski, M. de la Guardia and J. Namieśnik, *Talanta*, 2014,  
33  
34 16 **119**, 34-45.
- 35  
36 17 21 F. Pena-Pereira, I. Lavilla and C. Bendicho, *Spectrochim. Acta Part B*, 2009, **64**, 1-15.
- 37  
38 18 22 B. Hu, M. He, B. Chen and L. Xia, *Spectrochim. Acta Part B*, 2013, **86**, 14-30.
- 39  
40 19 23 A. N. Anthemidis and I. S. I. Adam, *Anal. Chim. Acta*, 2009, **632**, 216-220.
- 41  
42 20 24 N. Goudarzi, *J. Agric. Food Chem.*, 2009, **57**, 1099-1104.
- 43  
44 21 25 M. A. Jeannot, A. Przyjazny and J. M. Kokosa, *J. Chromatogr. A*, 2010, **1217**, 2326-  
45  
46 22 2336.
- 47  
48 23 26 M. Kaykhaii and S. Noorinejad, *J. Anal. At. Spectrom.*, 2014, **29**, 875-879.
- 49  
50 24 27 R. Sitko, K. Kocot, B. Zawisza, B. Feist and K. Pytlakowska, *J. Anal. At. Spectrom.*,  
51  
52 25 2011, **26**, 1979-1985.


- 1  
2  
3  
4 1 28 H. Sereshti, V. Khojeh and S. Samadi, *Talanta*, 2011, **83**, 885-890.  
5  
6 2 29 L. Li and B. Hu, *Talanta*, 2007, **72**, 472-479.  
7  
8 3 30 K. Shrivastava and D. K. Patel, *Food Chem.*, 2011, **124**, 1673–1677.  
9  
10 4 31 M. A. Aguirre, S. Legnaioli, F. Almodóvar, M. Hidalgo, V. Palleschi and A. Canals,  
11  
12 *Spectrochim. Acta Part B*, 2013, **79-80**, 88-93.  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

# Figures

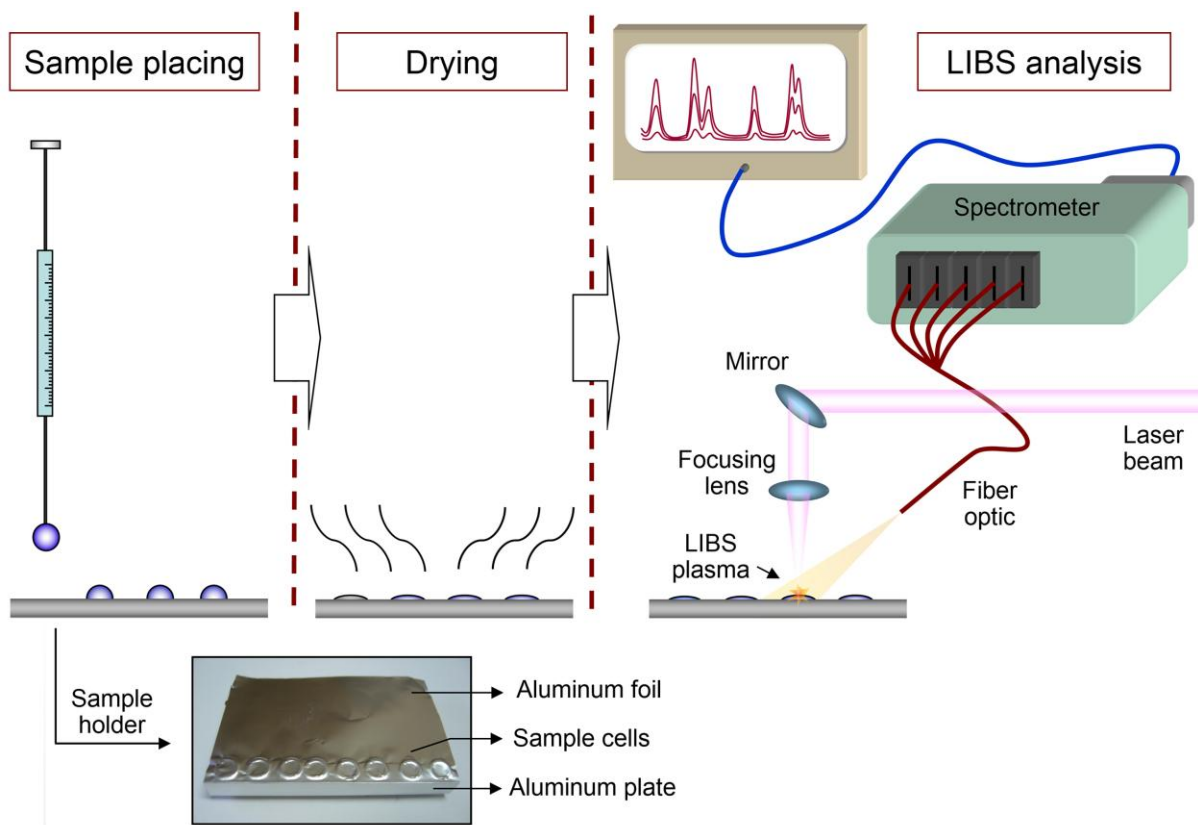

**Fig. 1** LIBS experimental setup used in the analysis of liquid samples.

Analytical Methods Accepted Manuscript

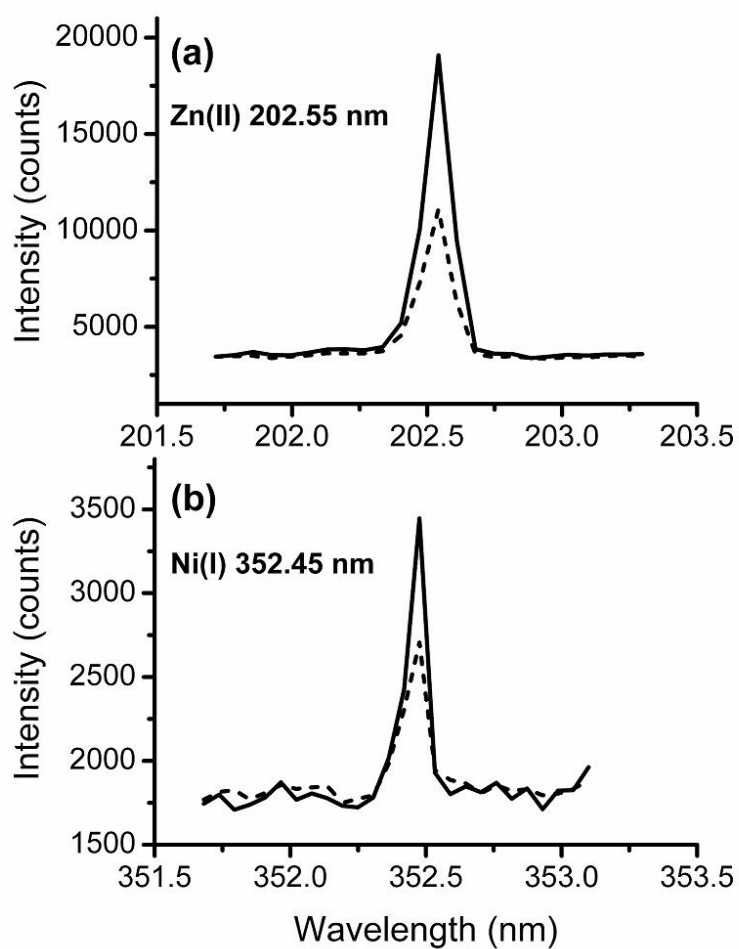

**Fig. 2** LIBS signals obtained for (a) ZnII (202.548 nm) and (b) NiI (352.454 nm) emission lines when a  $1 \mu\text{g g}^{-1}$  standard solution is analyzed by LIBS (dash line) and SDME-LIBS (solid line) methodologies.

# Tables

**Table 1** Experimental factors and levels of the Plackett-Burman design.

Experimental factor	Level	
	Low (-1)	High (+1)
[APDC] (% w v <sup>-1</sup> )	0.5	1
Drop volume (μL)	5	7.5
pH	5	10
Stirring speed (r.p.m.)	850	1700
Extraction time (min)	5	10



**Table 2** Experimental factors and levels of the Circumscribed Central Composite design (CCCD).

Experimental factor	Level			Star points ( $\alpha=1.682$ )	
	Low (-1)	Central (0)	High (+1)	$-\alpha$	$+\alpha$
Drop volume ( $\mu\text{L}$ )	2.5	5	7.5	0.8	9.2
pH	6	8	10	4.6	11.4
Extraction time (min)	4	7	10	1.9	12.1

1  
2 **Table 3** Analytical figures of merit obtained with LIBS and SDME-LIBS analytical methodologies.

Emission line (nm)	LIBS			SDME-LIBS			Enhancement Factor <sup>c</sup>	LOD Ratio <sup>d</sup>
	Sensitivity <sup>a</sup> (cts kg $\mu\text{g}^{-1}$ )	RSD <sup>b</sup> (%)	LOD ( $\mu\text{g kg}^{-1}$ )	Sensitivity <sup>a</sup> (cts kg $\mu\text{g}^{-1}$ )	RSD <sup>b</sup> (%)	LOD ( $\mu\text{g kg}^{-1}$ )		
ZnII (202.548)	19.5±1.1	17	49	51±2	13	21	2.6	2.3
MnII (259.373)	29±4	16	427	59±4	15	301	2.1	1.4
CuI (324.754)	26±5	20	141	55±5	18	54	2.2	2.6
NiI (352.454)	1.64±0.10	16	463	3.3±0.3	20	189	2.0	2.4
CrI (357.869)	7.0±1.0	19	143	17.6±1.2	16	50	2.5	2.9

3 <sup>a</sup> Uncertainty expressed as standard deviation.

4 <sup>b</sup> Evaluated from the analysis of eight aliquots taken from the same vial of 1  $\mu\text{g g}^{-1}$  calibration standard.

5 <sup>c</sup> Calculated as the ratio of sensitivities obtained with SDME-LIBS and LIBS.

6 <sup>d</sup> Calculated as the ratio of LODs obtained with LIBS and SDME-LIBS.

7  
8  
9  
10  
11  
12  
13  
14  
15

**Table 4** Analysis of LGC6016 certified reference material (estuarine water) by SDME-LIBS. View Article Online  
DOI: 10.1039/C4AY02218A

Emission line (nm)	Certified value <sup>a</sup>	SDME-LIBS	
		Found value <sup>a</sup>	Recovery value (%)
ZnII (202.548)	75±2	84±21	112±25
MnII (259.373)	976±31	1026±215	105±21
CuI (324.754)	190±4	183±35	96±19
NiII (352.454)	186±3	n.q. <sup>b</sup>	n.q. <sup>b</sup>

<sup>a</sup> In  $\mu\text{g L}^{-1}$   $\pm$  confidence interval at 95%. <sup>b</sup> not quantified.