

Biomaterials Science

Accepted Manuscript

This article can be cited before page numbers have been issued, to do this please use: L. Burroughs, S. Singh, W. Ashraf, L. Martinez-Pomares, R. Bayston and A. Hook, *Biomater. Sci.*, 2020, DOI: 10.1039/D0BM00709A.



This is an Accepted Manuscript, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this Accepted Manuscript with the edited and formatted Advance Article as soon as it is available.

You can find more information about Accepted Manuscripts in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this Accepted Manuscript or any consequences arising from the use of any information it contains.

ARTICLE

Received 00th January 20xx,
Accepted 00th January 20xx
DOI: 10.1039/x0xx00000x

Development of Dual Anti-biofilm and Anti-bacterial Medical Devices

Laurence Burroughs, a Waheed Ashraf, b Sonali Singh, c Luisa Martinez-Pomares, c Roger Bayston, b Andrew L. Hook *a

The rising occurrence of antimicrobial resistance demands new strategies for delivering antibiotics to ensure their effective use. In this study, a multi-functional strategy to address medical device associated infections is explored whereby an anti-attachment and an antibacterial mechanism have been combined. Silicone catheters impregnated with multiple antibiotics are coated with polyacrylate coatings previously shown to reduce bacterial attachment and biofilm formation. Antibiotics are delivered through the applied coating and the delivery rate depends on the coating thickness and chemistry. Coated devices achieve a zone of inhibition and TK100 to gram-negative *Escherichia coli* and gram-positive *Staphylococcus aureus* similar to those of uncoated devices, whilst maintaining anti-attachment properties. No adverse immunological responses of the coatings were observed. The multi-functional nature of the device developed in the study represents an important approach to combatting medical device associated infections.

Introduction

Antibiotic resistance is rising to dangerous levels in all areas of the world, decreasing the effectiveness of disease treatments and placing increasing pressure on the global health system.¹ One issue reducing the efficacy of antibiotic treatments is biofilm formation; after adhering to a surface, planktonic bacteria form biofilms, which are up to 1000 times less susceptible to antimicrobial treatments and host defences.² Around 80% of healthcare-acquired infections are believed to be associated with biofilm formation, with catheter-associated urinary tract infections (CAUTIs) one of the most common infections found in patients.²⁻³ The duration of catheterisation has a direct influence on the likelihood and type of infection, with treatment considerations often varying between long-term (> 28 days) and short-term catheter infections.^{3b} Long-term, indwelling catheterisation can be required in cases of chronic debilitating illness with loss of mobility, such as multiple sclerosis, or in patients with a condition affecting nerves that control the bladder, such as spinal injury. The daily risk of bacterial colonisation when an indwelling catheter is in place is 3-7%; patients requiring extended catheter use are therefore at high risk of bacterial infection and those with chronic indwelling catheters are assumed to be bacteriuric.^{3b}

Development and implementation of novel biomaterials able to resist biofilm formation is an attractive target for use in a variety of biomedical applications including urinary catheters. A range of synthetic polymeric materials able to resist bacterial attachment have been reported including zwitterionic polymers and polymeric ammonium salts,⁴ poly(ethylene glycol)⁵ and polyglycerols,⁶ and polyacrylates and polymethacrylates.⁷ In particular, polyacrylates with molecular stiff hydrophobic pendant groups offer broad spectrum resistance to biofilm

formation,⁸ which has also been demonstrated *in vivo*.^{7b} The mechanism by which these materials prevent bacterial biofilm has not yet been established, however, the polymers do not kill bacteria and the importance of a bulky hydrophobic moiety suggests possible interactions with the lipophilic cell wall or preferential adsorption of hydrophobic biomolecules that mediate the biological response.⁷⁻⁸ These materials can be engineered as flexible coatings adhered to silicone such that they are suitable for use with urinary catheters.⁹ However, these materials have yet to be shown to resist biofilm formation for long-term periods of 28 days or more.

An alternative approach to developing anti-biofilm coatings involves the release of antimicrobials from impregnated materials. Antiseptics such as chlorhexidine¹⁰ and silver containing compounds have been employed;¹¹ however, toxicity issues and limited evidence of efficacy question the viability of these approaches.¹² McCoy *et al.* developed a pH-responsive antimicrobial release system using polymerised drug conjugates in an effort to extend the therapeutic release time beyond that often observed with diffusion-controlled release.¹³ However, such an approach restricts use to a narrow range of infections, and efficacy may be decreased in complex cases. Bayston *et al.* developed a method to impregnate silicone catheters with multiple antimicrobials. This methodology successfully prevented colonisation by a wide range of pathogens for over 12 weeks.^{3a, 14}

We hypothesised that this approach, used in conjunction with polyacrylate coatings resistant to biofilm formation, would allow for the development of infection-resistant devices with reduced dependence on antimicrobials and optimised antimicrobial release profiles suitable for long-term use. Hence, the coating would both prevent biofilm formation and control the release of antimicrobials. Here, the coating would be intended to prevent formation of biofilm on a urinary catheter rather than for the treatment of established urinary tract infections.

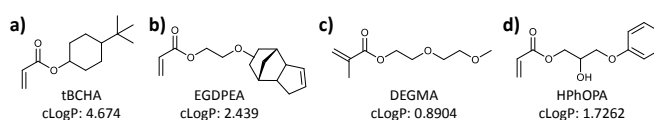


Figure 1. a-d) Monomers used in the study (cLogP calculated using

^a School of Pharmacy, University of Nottingham, Nottingham NG7 2RD, UK.

^b School of Medicine, Queen's Medical Centre, Nottingham NG7 2UH, UK.

^c School of Life Sciences, Faculty of Medicine and Health Sciences, Queen's Medical Centre, Nottingham NG7 2UH, UK.

Electronic Supplementary Information (ESI) available: Supporting Information is available from the RSC Online Library or from the author. See DOI: 10.1039/x0xx00000x



ChemDraw 16.0 software.

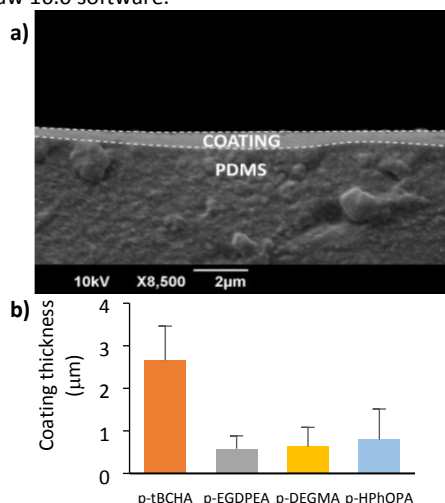


Figure 2. a) Representative SEM image of the cross-sectional view of a coated catheter showing coating thickness. b) Measured coating thickness for all four polymers using a polymer solution concentration of 1% (w/v). Scale bars equal one standard deviation, $n = 5$.

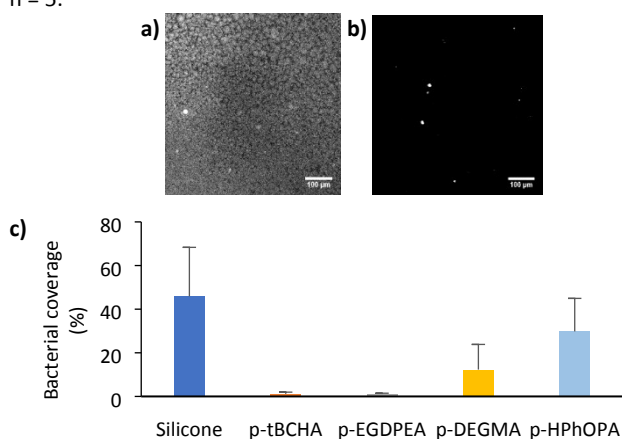


Figure 3. a-b) Representative fluorescence images of bacterial coverage measured on a) uncoated PDMS and b) p-tBCHA coated samples. c) *S. aureus* coverage after 72 h culture with uncoated and polymer coated catheters. Bacteria were stained with SYTO64 (Ex = 599 nm, Em = 619 nm) and imaged by confocal microscopy. Average of 4 technical replicates taken from two biological replicates, $N = 2$. Error bars equal ± 1 standard deviation unit.

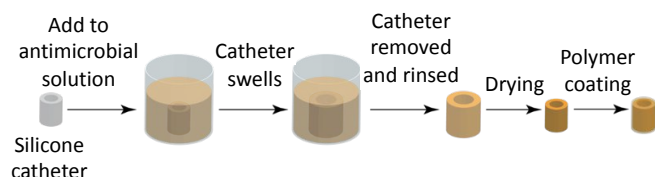


Figure 4. Schematic depiction of the production of coated and impregnated catheters.

Results and Discussion

Validation of anti-biofilm performance

Four monomers of varying hydrophobicity were polymerised using thermally-initiated free-radical polymerisation to provide a homopolymer library of coatings (Figure 1); two of these polymers, poly-*tert*-butyl cyclohexyl acrylate (p-tBCHA, Figure 1a) and poly-ethylene glycol dicyclopentyl ether acrylate (p-EGDPEA, Figure 1b),

have been previously shown to resist biofilm formation, whilst poly-di(ethylene glycol) methyl ether methacrylate (p-DEGMA, Figure 1c) and poly-2-hydroxy-3-phenoxypropyl acrylate (p-HPhOPA, Figure 1d) both supported biofilm formation.^{7b} The four polymers were selected due to their range in hydrophobicity, with calculated logP (cLogP) values varying from 0.89 to 4.7 (Figure 1). Successful polymerisation of the monomers was confirmed by NMR (Figure S11-3)

Initially the anti-biofilm nature of the silicone sections coated with 1 wt% solutions of each polymer was assessed. Coating thickness was measured by SEM to be 0.5-3 μm (Figure 2). Variations in coating thickness are likely due to viscosity differences between the different polymer solutions.¹⁵ Samples were incubated with *S. aureus* for 72 h before staining with SYTO64 and imaging by confocal microscopy. Samples were assessed with *S. aureus* as this species produced higher surface coverages of bacterial biofilm on uncoated plain catheters ($45.9 \pm 22.5\%$) compared with *E. coli* ($3.6 \pm 3.1\%$). The bacterial biofilm coverages measured on each coating are shown in Figure 3. A statistically significant ($p < 0.0001$) reduction in bacterial coverage of $> 97\%$ was observed on the coatings of p-tBCHA and p-EGDPEA compared with the uncoated catheters. This was consistent with previous observations for these coatings,⁷ suggesting that the coating methodology maintained the anti-biofilm properties. The p-DEGMA coating also significantly ($p=0.002$) reduced the bacterial coverage by 73% compared with the uncoated sample, whilst the bacterial coverage on the p-HPhOPA coating was not statistically different from the uncoated catheter samples.

Antimicrobial Delivery Experiments

Next, the delivery of antimicrobials through a polymer coating and how polymer hydrophobicity influenced antimicrobial release was investigated. Silicone catheter sections were impregnated with the antimicrobials rifampicin, sparfloxacin and triclosan according to a previously published procedure.¹⁶ Improved prevention of biofilm formation and emergence of resistant strains has previously been demonstrated when using multiple antimicrobials compared with a single drug.^{3a, 14c} These compounds were chosen due to their activity against CAUTI pathogens and chemical compatibility with the impregnation procedure.^{14b} Rifampicin was included because of its activity alone and in combination against staphylococci and its synergistic activity against many multidrug-resistant gram negative bacteria.¹⁷ Sparfloxacin has been withdrawn from the market as it has been overtaken by other quinolone antimicrobials, but it is still available for medical applications, is active against CAUTI pathogens and is safe for use in the lower and upper urinary tracts.¹⁸ Triclosan is approved for use in medicinal products within the EU and by the FDA and is a component of Vicryl Plus surgical sutures.¹⁹ The impregnated catheter sections were dip-coated 3 times in a 1-5 wt% polymer in toluene solution and dried for 24 h under vacuum (Figure 4). Non-impregnated plain silicone catheter controls were also dip-coated similarly using the four polymer solutions.

Serial plate transfer tests were carried out for 10 days on the coated, impregnated catheters using plates inoculated with *Staphylococcus aureus* (*S. aureus*) and *Escherichia coli* (*E. coli*) and compared to the uncoated impregnated control (Figure 5). All four polymer coatings showed zones of inhibition for both bacterial species indicating that antimicrobials could be successfully delivered through a poly(meth)acrylate coating. However, the zones of inhibition were reduced relative to that of the impregnated catheters without a polymer coating. No correlation between the cLogP of the monomer, as a measure of hydrophobicity,^{8a, 8c} and zone of inhibition size could be seen (see Figure S14). Coatings of p-tBCHA prepared using a 5 wt%



solution did not achieve a zone of inhibition with *E. coli*, however,

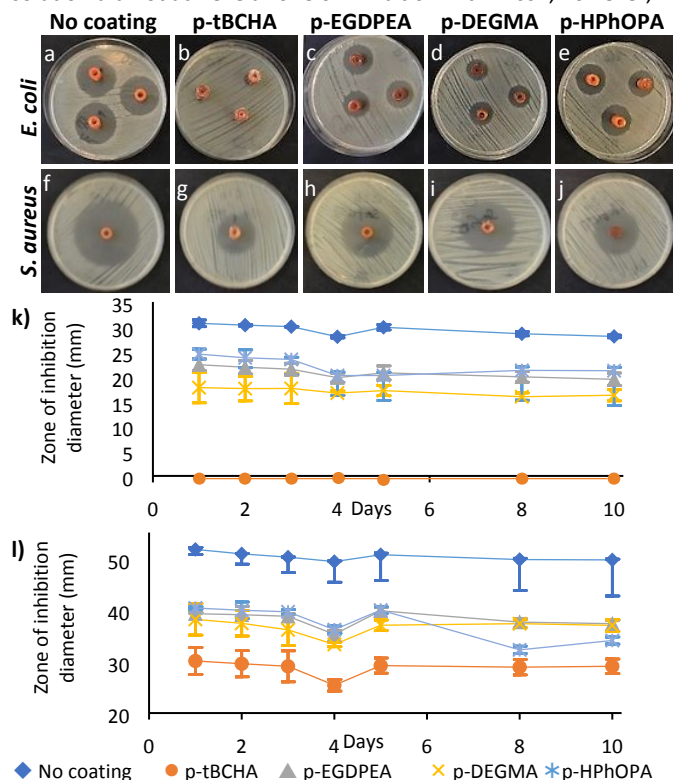


Figure 5. Assessment of the zone of inhibition for antimicrobial impregnated catheters with **a-e)** *E. coli* and **f-j)** *S. aureus* for **a and f)** no coating, **b and g)** p-tBCHA, **c and h)** p-EGDPEA, **d and i)** p-DEGMA, and **e and j)** p-HPhOPA. Photographs after 1 day. Samples located in 90 mm petri dishes. **k)** 10 day serial plate transfer, *E. Coli* **l)** 10 day serial plate transfer, *S. aureus*. Error bars equal \pm one standard deviation unit, N = 3.

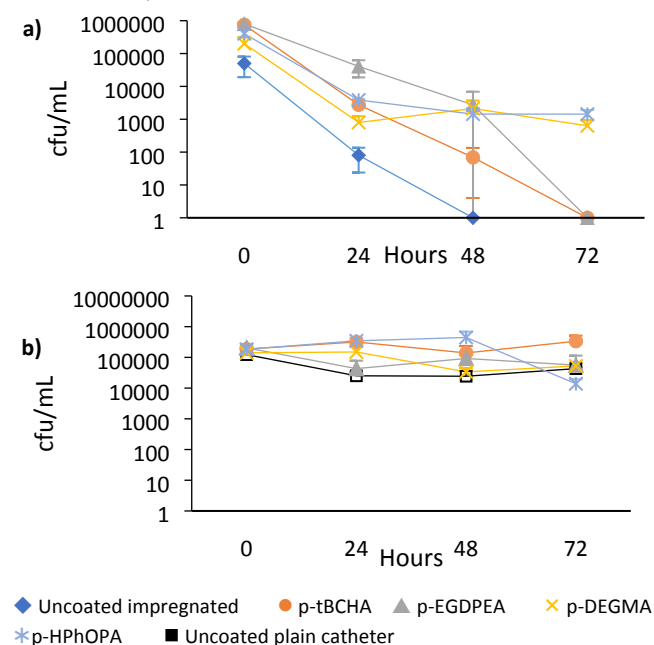


Figure 6. Assessment of the ability of catheters impregnated with antimicrobials and coated with different polymers to kill associated bacteria. **a)** tk100 for impregnated catheters **b)** tk100 for catheters without impregnated antimicrobials. Error bars equal \pm one standard deviation unit, N = 3.

reducing the solution concentration to 1 wt% achieved a zone of inhibition of \approx 90% of an uncoated catheter (Figure S15).

Next, a series of assays of the time taken to kill 100% of attached *E. coli* (tk100) were carried out on the coated catheters to determine whether the coatings were still able to kill all attached bacteria (Figure 6a). The attached bacteria on the catheters coated with p-DEGMA or p-HPhOPA were reduced after 24 h but could not be taken to $< 1 \text{ Log}_{10} \text{ cfu/mL}$ after 72 h, suggesting that antimicrobial permeability through these coatings was reduced. Catheters coated with p-EGDPEA and p-tBCHA were both able to reach $< 1 \text{ Log}_{10} \text{ cfu/mL}$ after 72 h. In comparison, the uncoated impregnated catheter reached $< 1 \text{ Log}_{10} \text{ cfu/mL}$ viability at 48 h. There was no difference in viability between plain silicone catheter and plain silicone catheter coated with the polymers (Figure 6b). Thus, the coatings that were more hydrophobic showed increased permeation of the antimicrobials compared with the more hydrophilic coatings despite an increased or similar thickness (Figure 2b). No significant difference in the amount of bacteria on the different coatings was observed in the absence of impregnated anti-microbials, despite the different chemistries producing significantly different amounts of biofilm formation.⁷ Thus, the polyacrylate coatings did not prevent association with planktonic bacteria, which is consistent with the mode of action of these polymers acting specifically on biofilm formation and not involving a killing mechanism.

Quantification of Antimicrobial Release

With the initial bacterial studies indicating a reduction in antimicrobial release through the polymer coatings, we next quantified drug elution from the catheters. The catheter sections were immersed in deionised water for 48 h at 37°C and the solution analysed by liquid chromatography mass spectrometry (LC-MS). The percentage of drug elution (Figure S17-13) was normalised relative to the uncoated impregnated catheter set at 100% and plotted against cLogP (Figure 7). No monomer or coating oligomers were detected in the analysed solutions suggesting that the coating was stable in the aqueous environment over 48 h. Antimicrobial release was achieved through all four polymer coatings although at a reduced quantity as compared with the uncoated impregnated catheter. The smallest reduction for all three antibiotics was observed for the coating of tBCHA, where 43%, 97% and 90% of sparfloxacin, triclosan and rifampicin was released, respectively, compared with the uncoated catheter (Figure 7a-c). p-HPhOPA exhibited the greatest reduction in sparfloxacin release, with 15 $\mu\text{g/mL}$ detected compared to 91 $\mu\text{g/mL}$ for the uncoated sample (Figure 7a). For the other coated samples a range of 24-39 $\mu\text{g/mL}$ detected concentration was observed. p-DEGMA showed the greatest reduction in triclosan release, with 50 $\mu\text{g/mL}$ detected compared to 78 $\mu\text{g/mL}$ detected for the uncoated catheter (Figure 7b). A correlation between cLogP and percentage elution of triclosan was seen, suggesting that intermolecular interactions between the antibiotic and the polymers may play a role in the drug elution (Figure 7b and d). Rifampicin release was most affected by the p-DEGMA coating; in 2 out of 3 repeats, the level of rifampicin was shown to be below the limit of detection on the LC-MS system, making the detected level statistically non-significant (Figure 7c). The other 3 coatings exhibited a reduced effect on rifampicin release, delivering around 1.3 $\mu\text{g/mL}$ versus the uncoated sample at 1.5 $\mu\text{g/mL}$.

These results were consistent with the tk100 tests, where only p-tBCHA and p-EGDPEA coatings were able to reach $< 1 \text{ Log}_{10} \text{ cfu/mL}$ after 72 h (Figure 6a). p-tBCHA showed the greatest level of detected drug elution using LC-MS with all 3 antimicrobials, possibly due to



reduced intermolecular interactions between the antibiotics

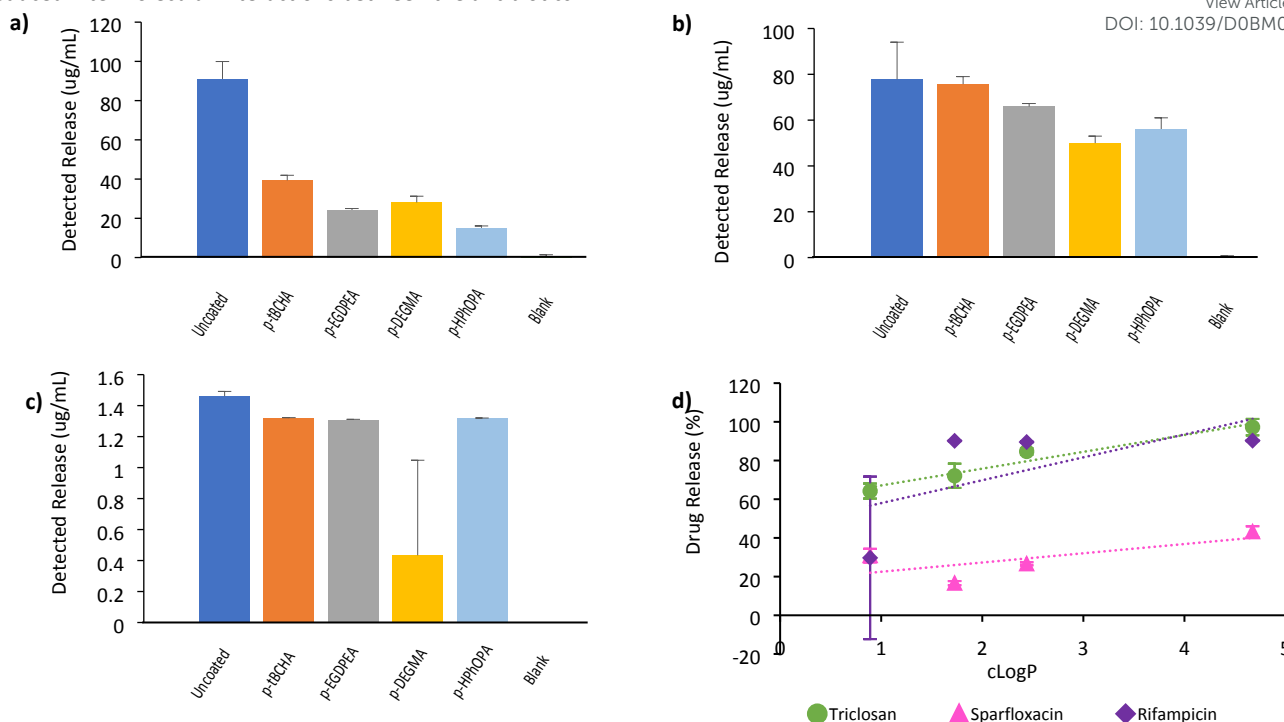


Figure 7. LC-MS assessment of the antimicrobial release from impregnated catheters through different polymer coatings. **a)** Sparfloxacin drug elution, **b)** triclosan drug elution, **c)** rifampicin drug elution, **d)** Percentage of drugs eluted through coatings relative to uncoated catheter against cLogP. The line of best fit and associated coefficient of determination (R^2) is shown for each antibiotic: triclosan (green), sparfloxacin (yellow) and rifampicin (orange). Error bars equal ± 1 standard deviation unit, $n = 3$.

and the polymer. The p-tBCHA coating was thicker than the other samples (Figure 2b), which was anticipated to impede antimicrobial release. Counter to this, relatively high drug release was observed through the p-tBCHA coating compared with the other samples (Figure 7), thus, it was likely that intermolecular interactions rather than coating thickness played the key role in determining drug elution through the samples studied. It is important to note that the zone of inhibition and tk100 tests were not carried out with the catheter sections fully immersed in solution, which may result in less coating swelling and consequently more restricted drug elution. There was no strong correlation between cLogP and elution of rifampicin or sparfloxacin ($R^2 = 0.41$ and $R^2 = 0.50$ respectively, Figure 7d); in contrast, triclosan elution showed a strong correlation to cLogP ($R^2 = 0.95$, $R^2(adj) = 0.92$, $p = 0.03$, Figure 7d) It is possible that the bulkier molecules are more affected by the polymer network than triclosan, making hydrophobicity of the coating less of a factor determining release.

Coating Characterisation

Time of flight secondary ion mass spectrometry (ToF-SIMS) depth profiling analysis, using an Ar-cluster sputter beam at 10 keV with Bi_3^+ primary beam at 25 keV over a random raster area, was then used to assess the depth distribution of the coating and antimicrobials within the coated, impregnated devices. Molecular ions for all 3 antimicrobials could be detected; rifampicin ($\text{M}+\text{H}^+ = \text{C}_{43}\text{H}_{59}\text{N}_4\text{O}_{12}$) at 823.4, sparfloxacin ($\text{M}+\text{H}^+ = \text{C}_{19}\text{H}_{23}\text{F}_2\text{N}_4\text{O}_3$) at 393.2 and triclosan ($\text{M}+\text{H}^+ = \text{C}_{12}\text{H}_8\text{Cl}_3\text{O}_2$) at 289.0, whilst characteristic ions for p-tBCHA (C_4H_9^+), p-EGDPEA (C_5H_7^+), p-DEGMA ($\text{C}_3\text{H}_7\text{O}^+$) and p-HPhOPA (C_6H_5^+) were also identified.²⁰ Both the p-tBCHA and p-EGDPEA coatings appeared to have a lower intensity of antimicrobial ions in the polymer coating, which increased to a maximum at the interface between the coating and silicone catheter before decreasing again

(Figure 8a-b). The more hydrophilic polymer coatings p-DEGMA and p-HPhOPA appeared to have greatest intensity of antimicrobial peaks in the coating, which then decreased in line with the coating ion intensities (Figure 8c-d). It is possible that during the coating procedure more of the impregnated antimicrobials leach out into the polymers p-DEGMA and p-HPhOPA than p-tBCHA and p-EGDPEA. This may also account for the observed discrepancy between the zone of inhibition and tk100 tests and the detected drug elution in the LC-MS studies; if the rate of drug elution through the polymers differs between samples, then an increased initial concentration of drug in the coating may produce a greater biological response. The uncoated impregnated sample showed uniform antimicrobial distribution through the profiled area (see Figure S14-16).

Biocompatibility Studies

The components of the dual anti-biofilm anti-microbial device have previously been demonstrated to not be cytotoxic.¹⁷⁻²⁰ To further assess the biocompatibility of polymer coatings, primary human monocyte-derived macrophages were incubated with the coated or uncoated plain or antibiotic-impregnated catheters for 24 h. The effect of polymer coatings on macrophage function was assessed by stimulating these cells with lipopolysaccharide (LPS) for a further 24 h. Cell viability before and after LPS addition was determined by measuring the amount of lactate dehydrogenase in the cell supernatants (Supporting Information). None of the coatings tested appeared to increase cell death appreciably compared to a macrophage only control (no catheter condition).

To determine the effect of the coatings on immune cell function, the production of two pro-inflammatory cytokines: tumour necrosis factor alpha (TNF- α) and interleukin 6 (IL-6), by macrophages was also measured before and after addition of LPS (Figure 9a). Macrophages did not produce the pro-inflammatory cytokines TNF-



α or IL-6 when incubated with coated or uncoated plain catheters

alone, i.e. in "unstimulated samples" (Figure 9b-c). Thus the

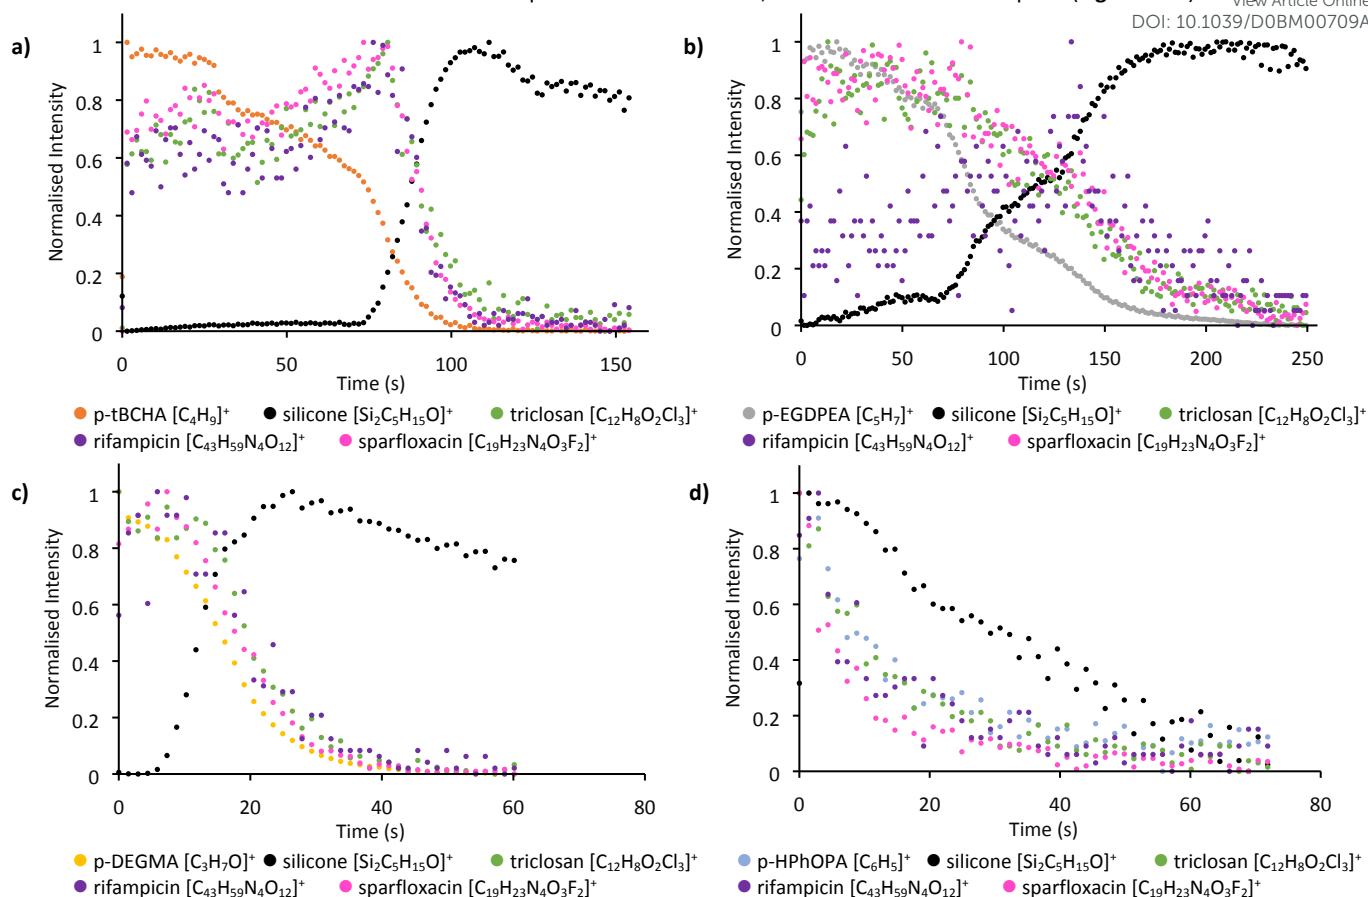


Figure 8. Normalised ToF-SIMS depth profile analysis for **a)** p-tBCHA coated impregnated catheter, **b)** p-EGDPEA coated impregnated catheter, **c)** p-DEGMA coated impregnated catheter, and **d)** p-HPhOPA coated impregnated catheter. Normalised ion intensities for ions characteristic of the polymer coatings, the antimicrobials and silicone are shown.

catheters or coating polymers did not cause inappropriate macrophage activation.

Upon LPS stimulation, macrophages alone (i.e. in the absence of catheters) produced TNF- α and IL-6 (Figure 9b-c), as expected. Significantly lower TNF- α and IL-6 production was seen by LPS-stimulated macrophages in all catheter samples (uncoated and coated) (Figure 9b-c and Figure S117), indicating that these samples were suppressing the normal inflammatory response. Further work would be necessary to determine the cause of this effect.

Materials and Methods

General information. All polymerisation reactions were carried out under an atmosphere of argon using degassed monomer solutions. Degassing was carried out by bubbling argon through the monomer solution for 40 minutes immediately before use. Monomers and 2,2'-Azobis(2-methylpropionitrile) (AIBN) were purchased from Sigma-Aldrich and were used as received. All temperatures are referred to the temperatures of the oil baths used. Nuclear magnetic resonance (NMR) spectra were recorded on a Bruker AV400 (400.3 MHz) spectrometer at ambient temperature; chemical shifts are quoted in parts per million (ppm) and were referenced as follows: chloroform-d, 7.26 ppm; benzene-d₆ 7.16 ppm for ¹H NMR data.²² Coupling constants (*J*) are quoted in Hertz. Gel Permeation Chromatography (GPC) was carried out on a Polymer Labs GPC 50 with 2 × PLgel Mixed-D columns and *N,N*-

dimethylformamide containing 0.1 wt% LiBr eluent. GPC calibration was carried out using poly(methyl methacrylate).

Polymerisation Reactions. All polymerisation reactions were carried out under an atmosphere of argon using degassed monomer solutions. Degassing was carried out by bubbling argon through the monomer solution for 40 minutes immediately before use. Monomers and 2,2'-Azobis(2-methylpropionitrile) (AIBN) were purchased from Sigma-Aldrich and were used as received. All temperatures are referred to the temperatures of the oil baths used. Nuclear magnetic resonance (NMR) spectra were recorded on a Bruker AV400 (400.3 MHz) spectrometer at ambient temperature; chemical shifts are quoted in parts per million (ppm) and were referenced as follows: chloroform-d, 7.26 ppm; benzene-d₆ 7.16 ppm for ¹H NMR data.²² Coupling constants (*J*) are quoted in Hertz. Gel Permeation Chromatography (GPC) was carried out on a Polymer Labs GPC 50 with 2 × PLgel Mixed-D columns and *N,N*-dimethylformamide containing 0.1 wt% LiBr eluent. GPC calibration was carried out using poly(methyl methacrylate).

Antimicrobial Impregnation of Catheters. Silicone catheter tubing with a lumen diameter of 3.2 mm (Appleton Woods) was impregnated with sparfloxacin (SIGMA), triclosan (CIBA) and rifampicin (SIGMA) dissolved in chloroform to give concentrations of 1%, 1% and 0.2% respectively (Figure 4), as described previously.¹⁶

Coating of Catheters. Catheters were cut into sections



measuring 1 cm in length. These were then attached to a 21 gauge needle by piercing the catheter wall with the needle and

DOI: 10.1039/D0BM00709A

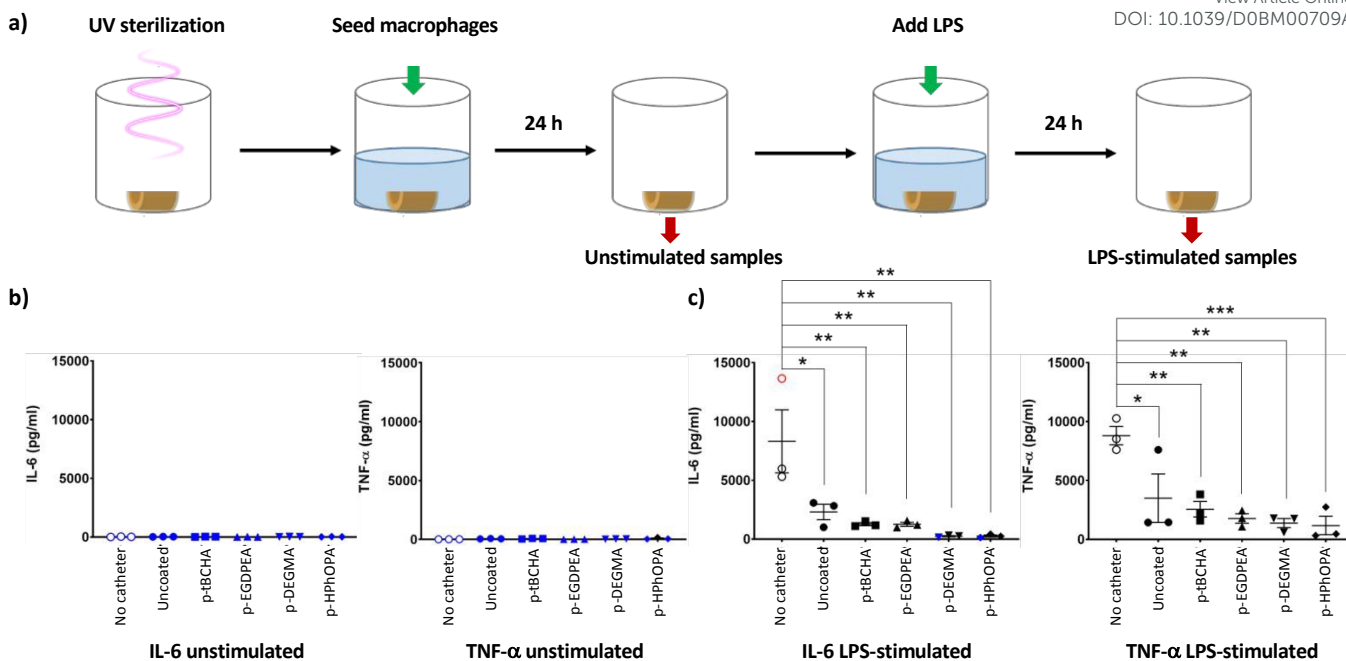


Figure 9. Effect of catheter coatings on primary human monocyte-derived macrophages. **a)** Schematic representation of experimental procedure for macrophage-catheter assays for cytokine determination. **b-c)** TNF- α and IL-6 production from macrophages that had been incubated with coated and uncoated plain catheters for **b)** 24 h (unstimulated) and **c)** followed by stimulation with 100 ng/ml LPS for 24 h (LPS-stimulated). Graphs represent mean \pm SEM for $n=3$ (3 independent experiments using 3 separate donors). ANOVA with Tukey's multiple comparison post-test conducted, *, $p \leq 0.05$, **, $p \leq 0.01$, and ***, $p \leq 0.001$. Blue symbols denote values that were below the standard range of the assay. Red symbols denote values that were above the standard range of the assay.

immersed by hand into a monomer solution of desired concentration (5 wt% or 1 wt%) in toluene for 1 s before being removed and left to dry under ambient conditions for 15 minutes. This procedure was repeated twice before the catheter sections were placed under vacuum (<1 mbar) for 24 h. Coating thickness was determined using a JEOL JSM-6490LV SEM using an accelerator voltage of 10 kV. Prior to analysis, coated samples were fractured after immersion in liquid nitrogen to expose the sample cross-section. Samples were mounted on carbon tape and gold coated using a Polaron SC7640 sputter coater, sputter time was 90 s, plasma current was 18-19 mA and a base chamber pressure of 0.6 mbar was achieved prior to coating.

Liquid chromatography mass spectrometry. Liquid chromatography mass spectrometry (LC-MS) was carried out on a ThermoFisher Exactive using a Sunfire C18 column stationary phase. Mobile phase was gradient elution from 95:5 0.1% NH_3 in $\text{H}_2\text{O}:\text{CH}_3\text{CN}$ to 5:95 0.1% NH_3 in $\text{H}_2\text{O}:\text{CH}_3\text{CN}$ with a flow rate of 0.800 mL/min. Experiment stop time was 10.00 min

Time-of-flight secondary ion mass spectrometry. Dual beam depth profiling Time-of-flight secondary ion mass spectrometry (ToF-SIMS) measurements were conducted using a ToF-SIMS IV (IONTOF GmbH) instrument operated using a 25 kV Bi_3^+ primary ion source in combination with a 10 kV Ar_n^+ sputter beam. Samples were scanned with a random raster over an area of $200 \times 200 \mu\text{m}$. Positive secondary ion spectra were collected. Owing to the non-conductive nature of the samples, a low energy (20 eV) electron flood gun was applied to provide charge compensation.

Serial Plate Transfer Test Assay. Test bacteria, methicillin resistant *Staphylococcus aureus* (MRSA) and extended

spectrum beta-lactamases producing *E. coli*, were isolated from patients with CAUTI. MRSA was sensitive to rifampicin and triclosan, but resistant to sparflloxacin. *E. coli* was resistant to both rifampicin and sparflloxacin but susceptible to triclosan. Minimum inhibitory concentrations were determined by agar incorporation or in the case of rifampicin, by Etest (AB Biodisk, Solna, Sweden). A serial transfer of the material to fresh plates will show how long the material produces a zone of inhibition (Serial Plate Transfer Test, SPTT).²³ Mueller Hinton agar (Oxoid) plates were seeded with the test bacteria ($A630$ 0.6, $\sim 1 \times 10^7$ cfu/mL) and impregnated silicone catheters with and without a coating were placed in triplicate on their surfaces and incubated overnight. Zones of inhibition were measured with calipers and the catheters were transferred to a fresh seeded plate and incubated at 37°C for 24 h. The process was repeated for up to 10 days.

tk100 Assay. The plain and test catheters were immersed in a suspension (approximately 1×10^8 cfu/mL) of early log phase test bacteria and incubated at 37 °C for 1 h for attachment to take place. After rinsing to remove unattached bacteria, triplicates of discs were placed in diluted Tryptone Soya Broth (Oxoid) for up to 72 h, the dilution necessary for survival of attached bacteria to controls without planktonic multiplication, being found by experiment for each test isolate. At intervals of 0, 24, 48 and 72 h, after rinsing and medium replacement each day, triplicates of catheters were removed and sonicated (50 Hz for 20 min) and surviving colonies plate - counted.

Generation of Monocyte-derived Macrophages. Monocyte-derived macrophages were generated from buffy coats (Blood Transfusion Service, Sheffield, UK). Peripheral blood mononuclear cells (PBMCs) were isolated by density gradient



centrifugation using Histopaque-1077 (Sigma-Aldrich, UK). The PBMC layer was collected, washed and the monocyte fraction (CD14+ cells) was obtained by positive selection using human CD14 MicroBeads and LS MACS columns (Miltenyi Biotec, UK), following the manufacturer's instructions. Purified monocytes were re-suspended in RPMI complete medium RPMI 1640 (Sigma-Aldrich, UK) containing 15% human AB serum (Sigma-Aldrich, UK), 2 mM GlutaMAX (Gibco, UK), 10 mM HEPES (Invitrogen, UK) and 50 ng/mL recombinant human macrophage colony stimulating factor (rhM-CSF, premium grade, Miltenyi Biotec, UK) and plated on ultra-low attachment 24-well flat bottom plates (Corning incorporated, USA) at a density of 1×10^6 monocytes/500 μ L. On Day 3, 500 μ L per well of fresh RPMI complete medium containing 50 ng/mL rhM-CSF was added. Macrophages were harvested on Day 6 and used for assays with catheters.

Macrophage Response to Catheters. Catheters were placed in a 24-well tissue culture-treated (TC) plate (Costar, UK) and UV-sterilised for 30 min. Day 6 macrophages were harvested, washed once with RPMI complete medium, counted, and seeded in the 24-well TC plate containing sterilised catheters at 2.5×10^5 cells/750 μ L/well in RPMI complete medium containing 50 ng/mL rhM-CSF. The volume of culture medium was sufficient to completely submerge the catheters. Cells were incubated with catheters for 24 h at 37°C, 5% CO₂ in a humidified incubator. The following day, supernatants were removed from each well and stored at -20°C for cytokine determination (referred to in the text as "unstimulated samples"). 100 ng/mL ultrapure LPS from *E. coli* (Invivogen, UK) in fresh RPMI complete medium containing 50 ng/mL rhM-CSF was then added and the cells were re-incubated for a further 24 h at 37°C, 5% CO₂ in a humidified incubator. Supernatants from each well were collected the following day and stored at -20°C for cytokine analysis (referred to in the text as "LPS-stimulated samples"). Macrophage supernatants (appropriately diluted) were tested for presence of the cytokines TNF- α and IL-6 using DuoSet ELISA kits (R&D Systems, Inc., UK) following the manufacturer's instructions. To assess macrophage viability, uncoated or coated antibiotic-impregnated catheters were placed in a 24-well tissue culture-treated (TC) plate (Eppendorf) and UV-sterilised for 30 min. Day 6 macrophages were harvested, washed 3 times with X-Vivo 15 serum-free medium (Lonza, UK), counted, and seeded in the 24-well TC plate containing sterilised catheters at 2.5×10^5 cells/1.5 mL/well in X-Vivo 15 medium containing 50 ng/mL rhM-CSF. The volume of culture medium was sufficient to completely submerge the catheters. Cells were incubated with catheters for 24 h at 37°C, 5% CO₂ in a humidified incubator. The following day, 750 μ L of cell supernatants were removed from each well and stored at -20°C for lactate dehydrogenase (LDH) determination (referred to in the text as "unstimulated samples"). 100 ng/mL ultrapure LPS from *E. coli* (Invivogen, UK) was then added and the cells with catheters were re-incubated for a further 24 h. The remaining 750 μ L of cell supernatants from each well were collected the following day and stored at -20°C for LDH analysis (referred to in the text as "LPS-stimulated samples"). LDH in the supernatants was measured using the Cytotoxicity Detection Kit (LDH) kit (Roche, UK) as per the manufacturer's instructions.

Statistical analysis. Linear regression analysis was carried out using the built-in linear model function in R version 3.6.1. Statistical analysis for macrophage cytokine responses was carried out in Prism v8.2.1, a repeated measures ANOVA with

Tukey's multiple comparison post-test was used. [View Article Online](#)
DOI: 10.1039/D0BM00709A

Conclusions

In summary, two different strategies for preventing bacterial biofilm formation on catheters have been combined. We have shown that multiple antimicrobials can be delivered through polyacrylate coatings on impregnated silicone catheters. The rate of delivery through the coating was modulated by the coating chemistry and thickness. The zone of inhibition and prevention of biofilm formation was not adversely affected on the optimised device after application of the anti-biofilm coating. Surface characterisation and depth profiling by ToF-SIMS confirmed the presence of the polymer coatings on the devices and demonstrated the ability of the antibiotics to permeate through the polyacrylate layer. No adverse immunological response was observed to the coatings. The multi-functional nature of the device developed in the study makes it an important approach to combatting medical device associated infections.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

This work was supported by the Bridging the Gaps project at The University of Nottingham, funded by the Engineering and Physical Sciences Research Council grant reference EP/M027333/1. Assistance with ToF-SIMS measurements by David Scurr and with the macrophage assays by Georgina Taylor is kindly acknowledged. Andrew Hook kindly acknowledges the University of Nottingham for funding his Nottingham Research Fellowship.

Notes and references

- 1 *Antimicrobial Resistance: Global Report on Surveillance*, World Health Organisation, 2014.
- 2 R. D. Monds and G. A. O'Toole, *Trends Microbiol.*, 2009, **17**, 73-87.
- 3 a) L. E. Fisher, A. L. Hook, W. Ashraf, A. Yousef, D. A. Barrett, D. J. Scurr, X. Chen, E. F. Smith, M. Fay, C. D. J. Parmenter, R. Parkinson and R. Bayston, *J. Controlled Release*, 2015, **202**, 57-64; b) L. E. Nicolle, *Antimicrobial Resistance and Infection Control*, 2014, **3**.
- 4 a) G. Cheng, Z. Zhang, S. F. Chen, J. D. Bryers and S. Y. Jiang, *Biomaterials*, 2007, **28**, 4192-4199; b) X. Xie, J. C. Doloff, V. Yesilyurt, A. Sadraei, J. J. McGarrigle, M. Commis, O. Veisoh, S. Farah, D. Isa, S. Ghanis, I. Joshis, A. Vegas, J. Li, W. Wang, A. Bader, H. H. Tam, J. Tao, H.-j. Chen, B. Yang, K. A. Williamson, J. Oberholzers, R. Langer and D. G. Anderson, *Nature Biomedical Engineering*, 2018, **2**, 894-906; c) C. Zhou, Y. Wu, K. R. V. Thappeta, J. T. L. Subramanian, D. Pranantyo, E. T. Kang, H. W. Duan, K. Kline and M. B. Chan-Park, *Acs Applied Materials & Interfaces*, 2017, **9**, 36269-36280.
- 5 a) I. Banerjee, R. C. Pangule and R. S. Kane, *Adv. Mater.*, 2011, **23**, 690-718; b) M. Li, K. G. Neoh, L. Q. Xu, R. Wang, E. T. Kang, T. Lau, D. P. Olszyna and E. Chiong, *Langmuir*, 2012, **28**, 16408-16422.
- 6 Q. Wei, T. Becherer, P. L. M. Noeske, I. Grunwald and R. Haag, *Adv. Mater.*, 2014, **26**, 2688-2693.
- 7 a) A. L. Hook, C. Chang, J. Yang, S. Atkinson, R. Langer, D. G. Anderson, M. C. Davies, P. Williams and M. R. Alexander, *Adv. Mater.*, 2013, **25**, 2542-2547; b) A. L. Hook, C. Chang, J. Yang,



- J. Lockett, A. Cockrayne, S. Atkinson, Y. Mei, R. Bayston, D. J. Irvine, R. Langer, D. G. Anderson, P. Williams, M. C. Davies and M. R. Alexander, *Nat. Biotechnol.*, 2012, **30**, 868-875.
- 8 a) A. A. Dundas, O. Sanni, J. Dubern, G. Dimitrakis, A. L. Hook, D. J. Irvine, P. Williams and M. R. Alexander, *Adv. Mater.*, 2019, **1903513**; b) P. Mikulskis, A. L. Hook, A. Dundas, D. J. Irvine, O. Sanni, D. G. Anderson, R. Langer, M. R. Alexander, P. Williams and D. A. Winkler, *ACS Applied Materials & Interfaces*, 2018, **10**, 139-149; c) O. Sanni, C. Chang, D. G. Anderson, R. Langer, M. C. Davies, P. M. Williams, P. Williams, M. R. Alexander and A. L. Hook, *Advanced Healthcare Materials*, 2015, **4**, 695-701.
- 9 a) K. Adlington, N. T. Nguyen, E. Eaves, J. Yang, C.-Y. Chang, J. Li, A. L. Gower, A. Stimpson, D. G. Anderson, R. Langer, M. C. Davies, A. L. Hook, P. Williams, M. R. Alexander and D. J. Irvine, *Biomacromolecules*, 2016, **17**, 2830-2838; b) E. P. Magennis, A. L. Hook, P. Williams and M. R. Alexander, *ACS Applied Materials & Interfaces*, 2016, **8**, 30780-30787; c) B. J. Tyler, A. Hook, A. Pelster, P. Williams, M. Alexander and H. F. Arlinghaus, *Biointerphases*, 2017, **12**, 02C412.
- 10 R. Hachem, R. Reitzel, A. Borne, Y. Jiang, P. Tinkey, R. Uthamantil, J. Chandra, M. Ghannoum and I. Raad, *Antimicrob. Agents Chemother.*, 2009, **53**, 5145-5149.
- 11 a) R. Pickard, T. Lam, G. MacLennan, K. Starr, M. Kilonzo, G. McPherson, K. Gillies, A. McDonald, K. Walton, B. Buckley, C. Glazener, C. Boachie, J. Burr, J. Norrie, L. Vale, A. Grant and J. N'Dow, *Lancet*, 2012, **380**, 1927-1935; b) D. M. Riley, D. C. Classen, L. E. Stevens and J. P. Burke, *Am. J. Med.*, 1995, **98**, 349-356.
- 12 T. B. L. Lam, M. I. Omar, E. Fisher, K. Gillies and S. MacLennan, *Cochrane Database of Systematic Reviews*, 2014, DOI: 10.1002/14651858.CD004013.pub4.
- 13 C. P. McCoy, N. J. Irwin, C. Brady, D. S. Jones, L. Carson, G. P. Andrews and S. P. Gorman, *Mol. Pharm.*, 2016, **13**, 2817-2822.
- 14 a) R. Bayston, W. Ashraf and C. Bhundia, *J. Antimicrob. Chemother.*, 2004, **53**, 778-782; b) R. Bayston, W. Ashraf and C. Ortori, *J. Neurosurg.*, 2016, **124**, 375-381; c) R. Bayston, L. E. Fisher and K. Weber, *Biomaterials*, 2009, **30**, 3167-3173; d) R. Bayston, G. Ullas and W. Ashraf, *Antimicrob. Agents Chemother.*, 2012, **56**, 2842-2845.
- 15 L. E. Scriven, *MRS Proceedings*, 1988, **121**, 717.
- 16 R. Bayston, N. Grove, J. Siegel, D. Lawellin and S. Barsham, *Journal of Neurology Neurosurgery and Psychiatry*, 1989, **52**, 605-609.
- 17 a) M. Bassetti, E. Repetto, E. Righi, S. Boni, M. Diverio, M. P. Molinari, M. Mussap, S. Artioli, F. Ansaldi, P. Durando, G. Orengo, F. B. Pallavicini and C. Viscoli, *J. Antimicrob. Chemother.*, 2008, **61**, 417-420; b) D. J. Hong, J. O. Kim, H. Lee, E. J. Yoon, S. H. Jeong, D. Yong and K. Lee, *Diagn. Microbiol. Infect. Dis.*, 2016, **86**, 184-189.
- 18 D. Kowalczyk, G. Ginalska and A. Przekora, *Journal of Biomedical Materials Research Part A*, 2011, **98A**, 222-228.
- 19 a) *Opinion on triclosan: antimicrobial resistance*, Scientific Committee on Consumer Safety, Directorate-General for Health and Consumers, European Commission, Brussels, 2010; b) Food-and-Drug-Administration, *Federal Register*, 2016, **81**, 61106-61130.
- 20 N. Jeffery, K. Kalenderski, J. Dubern, A. Lomiteng, M. Dragova, A. Frost, B. Macrae, A. Mundy, M. Alexander, P. Williams and D. Andrich, *European Urology Supplements*, 2019, **18**, e377.
- 21 H. E. Gottlieb, V. Kotlyar and A. Nudelman, *J. Org. Chem.*, 1997, **62**, 7512-7515.
- 22 R. Bayston and R. D. G. Milner, *J. Clin. Pathol.*, 1981, **34**, 1057-1062.
 View Article Online
DOI: 10.1039/D08M00709A



TOC

View Article Online
DOI: 10.1039/D0BM00709A

Silicone catheters impregnated with antibiotics and coated with an anti-attachment polyacrylate produce a device with dual anti-biofilm and anti-bacterial properties.

