

NOTE • OPEN ACCESS

The effect of magnetic field strength on the response of Gafchromic EBT-3 film

To cite this article: Ilias Billas *et al* 2019 *Phys. Med. Biol.* **64** 06NT03

View the [article online](#) for updates and enhancements.

Recent citations

- [Borna Maraghechi *et al*](#)
- [Impact of transverse magnetic fields on dose response of a radiophotoluminescent glass dosimeter in megavoltage photon beams](#)
Shotaro Ito *et al*
- [Dosimetric performance of the Elekta Unity MR-linac system: 2D and 3D dosimetry in anthropomorphic inhomogeneous geometry](#)
E Pappas *et al*



SMARTSCAN™

**Consistently the Best Commissioning Outcome.
Automated.**

- Data Quality. Automated.
- Scanning Efficiency. Automated.
- Commissioning Excellence. Automated.



OPEN ACCESS



NOTE

The effect of magnetic field strength on the response of Gafchromic EBT-3 film

RECEIVED

25 October 2018

REVISED

23 January 2019

ACCEPTED FOR PUBLICATION

7 February 2019

PUBLISHED

14 March 2019

Original content from this work may be used under the terms of the [Creative Commons Attribution 3.0 licence](https://creativecommons.org/licenses/by/3.0/).

Any further distribution of this work must maintain attribution to the author(s) and the title of the work, journal citation and DOI.

Ilias Billas^{1,3,4}, Hugo Bouchard², Uwe Oelfke³ and Simon Duane¹¹ National Physical Laboratory, Chemical, Medical and Environmental Science Department, Teddington, United Kingdom² Département de Physique, Université de Montréal, Montréal, Canada³ Joint Department of Physics, The Institute of Cancer Research and The Royal Marsden NHS Foundation Trust, London, United Kingdom⁴ Author to whom correspondence should be addressed.E-mail: ilias.billas@npl.co.uk

Keywords: MRI-Linac, MRI-guided radiotherapy, film dosimetry, magnetic field

Abstract

With the advent of MRI-guided radiotherapy, the suitability of commercially available radiation dose detectors needs to be assessed. The aim of this study was to investigate the effect of the magnetic field (B-field) on the response of the Gafchromic EBT-3 films. Moreover, as an independent study, we contribute to clarifying the inconsistency of the results of recent published studies, on the effect of B-field on the sensitivity of Gafchromic films.

A ⁶⁰Co beam was used to irradiate film samples in an electromagnet. An in-house PMMA phantom was designed to fit in the 5 cm gap between the two poles of the magnet. The phantom consists of two symmetrical plates where a film can be inserted. The absorbed dose rate of the ⁶⁰Co beam for zero B-field was measured using alanine pellets in a Farmer-type holder. A 12-point response curve was created, representing netOD as a function of dose, for each of five different B-field strengths (0 T to 2 T).

This study finds that there is at most a small effect of the magnetic field on the response of EBT-3 film. In terms of netOD (red channel) the change in response varied from -0.0011 at 0.5 T to 0.0045 at 2.0 T, with a standard uncertainty of 0.0030. If uncorrected, this would lead to an error in film-measured dose, for the red channel, of 2.4% at 2 T, with a standard uncertainty on dose of 1.4%. Results are also presented for B-field strengths of 0.5 T, 1 T and 1.5 T, which are all zero within the measurement uncertainty. Comparison between other studies is also presented.

Considering the small change on dose determined with EBT-3 when irradiated under the presence of B-field and taking into account the overall uncertainty in dosimetry using EBT-3 film achieved in this work, EBT-3 is assessed to be a suitable detector for relative and absolute dosimetry, with appropriate corrections, in MRI-guided radiotherapy. The results of the current work also elucidate the inconsistency on the reports from previous studies and demonstrate the necessity of similar investigations by independent teams, especially if the existing results may be in conflict.

1. Introduction

Recent progress in MRI-guided radiotherapy includes the integration of a linear accelerator (Linac) with a magnetic resonance imaging (MRI) scanner. MRI-Linacs provide real-time imaging during patient treatment and greatly enhanced soft-tissue image contrast, while completely avoiding radiation dose associated with x-ray imaging (Lagendijk *et al* 2008, Raaymakers *et al* 2009).

While great benefits for cancer treatment are anticipated using this new technology, the external magnetic field (B-field) affects conventional dosimeters and dose distributions. Currently, there are no available protocols that can provide traceability for reference dosimetry and there is no guidance available for performing measurements of the radiation field characteristics. Furthermore, experimental techniques to measure the commissioning data required for treatment planning systems (TPS) need to be adapted for the context of MRI-guided

radiotherapy (MRIgRT). Indeed, detector specifications are crucial to correctly measure input data for TPS, such as beam profiles and depth doses, since the presence of a B-field is known to perturb the detector dose response (Meijsing *et al* 2009, Reynolds *et al* 2013, Smit *et al* 2013, O'Brien 2016). In this context, the performance of suitable detectors under the influence of a B-field needs to be characterised. Detector suitability will then be defined by the ability to capture electrons affected by the Lorentz force in a medium and consequently the distorted lateral beam profiles and depth dose curves. Among available detectors that could fulfil such conditions, radiochromic film is a promising candidate.

Radiochromic film is a useful tool for relative dosimetry (measurements of the radiation field characteristics) and reference dosimetry (Girard *et al* 2012, Devic *et al* 2016, Billas *et al* 2017). It has high spatial resolution and a large measurement area suitable for validation of 2D dose maps. It is known to be almost water equivalent (Niroomand-Rad *et al* 1998) and shows small energy dependence (Devic *et al* 2004, Arjomandy *et al* 2010). Radiochromic film is used in advanced radiotherapy modalities (such as stereotactic radiosurgery (SRS) (Palmer *et al* 2015b, Dimitriadis *et al* 2017), intensity modulated radiotherapy (IMRT) (Sankar *et al* 2006, Low *et al* 2011), etc) that require complex quality assurance (QA) and verification methods for radiation dosimetry. It is also used for end-to-end dosimetry audits where the whole treatment chain as experienced by a patient is considered (Clark *et al* 2015, Palmer *et al* 2015a). Radiochromic film has shown that it is a promising candidate for the detection of the affected lateral profiles and depth dose curves due to the B-field in MRIgRT systems (Crijs *et al* 2011, 2012, Smit *et al* 2014). It has also been demonstrated that radiochromic film is a good detector for capturing the electron return effect (Raaijmakers *et al* 2005, 2007), which increases the dose at tissue-air boundaries.

Recent studies (Reynoso *et al* 2016, Roed *et al* 2017, Barten *et al* 2018, Delfs *et al* 2018) have investigated the performance of EBT-2 and EBT-3 films in different B-field strengths, at different orientation of the reference film edge with respect to the B-field, with and without real-time MR imaging and using different beam energies. Contradicting data were published by various authors and these will be covered in more detail in discussion. Briefly, the peer reviewed work by Reynoso *et al* (2016) investigated the effect of a 0.35 T B-field strength on EBT-2 film, using a ^{60}Co energy beam, and they found that the dose was changed by up to 15%. A study by Roed *et al* (2017) examined the effect of a 1.5 T B-field strength on EBT-3 film using the same energy beam as Reynoso *et al* (2016) (^{60}Co) and their results show a change on dose ranging from 1% to 3%. Delfs *et al* (2018) studied the effect of B-field strength (0.35 T and 1.42 T) on EBT-3 film. Although they used a different energy beam (6 MV) from Reynoso *et al* (2016) and Roed *et al* (2017), they report a dose change of 2.1%. A recent study by Barten *et al* (2018) investigated the response of EBT-3 film sheets at different angles to a B-field in a ^{60}Co unit with an integrated 0.35 T MRI system by VIEWRAY (MRI-dian). They compared to equivalent measurements at a 6 MV conventional linac (0 T) and they found a change of 0.9%.

The Gafchromic EBT-2 production has been discontinued and its next generation, EBT-3, differs in its structure (symmetrical polyester layers in order to eliminate errors on the scanning orientation) and the surface (matt surface to prevent Newton rings). However, both EBT-2 and EBT-3 films feature the same composition in the sensitive layer (Reinhardt *et al* 2012, Moylan *et al* 2013) and any change due to the B-field is expected to be similar.

Considering the need for a suitable detector to perform relative and absolute dosimetry in MRI-linac systems and the apparent inconsistencies between results from some recent publications (specifically between Reynoso *et al* (2016) and Roed *et al* (2017) that used same energy beam) on the effect of the B-field on radiochromic film signal, the aim of this study is to independently investigate the effect of the B-field on the response of the Gafchromic EBT-3 films at different magnetic strengths and clarify the contradiction between the findings of different published studies.


2. Materials and methods

2.1. Experimental setup

The experimental setup (figure 1) involved irradiation of Gafchromic EBT-3 film in an electromagnet (GMW type 3474-140) using a ^{60}Co beam (Theratronics, Theratron 780c). The distance from the ^{60}Co source to the centre of the magnetic poles (measurement point) was 162 cm. An in-house polymethyl methacrylate (PMMA) phantom, 5 cm width and 26 cm height, was designed to fit inside the 5 cm gap between the two poles of the magnet (as shown in figure 1), which provide a maximum B-field strength of 2 T. The phantom consisted of two symmetrical PMMA plates, each at a water equivalent depth of 1 cm, placed in front of and behind the film, and located so that the central axis of the film is placed in the centre of the two magnetic poles. The edge of the film was orientated parallel to B-field, along the x -axis, and perpendicular to radiation beam, in direction of the z -axis (figure 1). The B-field uniformity in an area of $3 \times 3 \text{ cm}^2$ along the centre of the two magnetic poles (in z and y direction) was found to be within $\pm 0.5 \text{ mT}$.

2.2. Output measurements

Output measurements were made using alanine/EPR dosimetry, calibrated in terms of absorbed dose to water and traceable to the NPL primary standard, to determine the absorbed dose rate of the ^{60}Co beam at zero B-field.

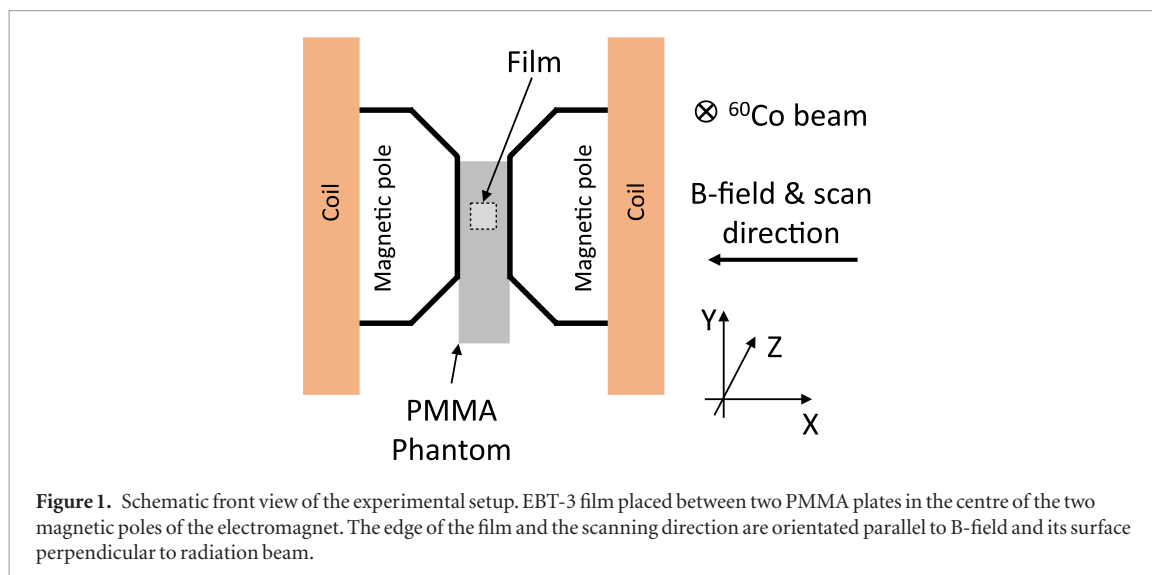

Nine alanine pellets, 2.5 mm height and 5 mm diameter, placed in a Farmer type (F-type) holder were used in a similar phantom to the one adopted for film dosimetry. Alanine was chosen due to non-standard condition of our experimental setup (such as field size and scatter conditions in the restricted space between the poles of the electromagnet). The phantom was built from a PMMA block, 2 cm × 5 cm × 26 cm, with a hole drilled into the insert to take an alanine F-type holder which could be fitted perpendicular to the direction of the radiation beam. The film and alanine phantoms were constructed to place the film and alanine reference points at the same measurement point.

2.3. Effect of B-field on absorbed dose to water at ^{60}Co beam quality

Although the effect of a B-field is more pronounced in air cavities, it also modifies the distribution of dose in water. A study by O'Brien *et al* (2016), including Monte Carlo calculation of depth-dose curves at 0 T and 1.5 T with an ELEKTA MR-linac beam quality (7 MV), has shown that the 1.5 T field systematically decreases the dose by 0.5% at depths beyond d_{max} . The effect of a B-field on dose to water, needs to be taken into account and corrected for.

In the current work, ^{60}Co absorb dose to water was calculated in B-field strengths up to 2 T using the usercode cavity that forms part of the EGSnrc Monte Carlo system (Kawrakow *et al* 2011) (development version: GitHub: Aug 2017). The simulation used a water phantom to represent the PMMA phantom, with water equivalence defined by scaling depth inversely with electron density. Dose was scored in slabs of 0.05 cm thick and 1 cm wide up to a depth of 2 cm.


2.4. Film response curve

Films were prepared, scanned and analysed by using the method developed by Bouchard *et al* (2009). Briefly, 12 pieces of EBT3 films (3.5 cm × 3.5 cm), cut from one sheet of film, were used to generate a calibration curve. Each piece maintained the same orientation as the original short dimension of the film (landscape orientation) and placed parallel to the B-field during irradiation and parallel to scanning direction during digitisation. The film orientation and alignment was kept consistent throughout the measurements.

The radiation field filled the gap between the two magnetic poles and the source-to-surface distance was set at 161 cm. Films were irradiated at a depth of 1 cm (a sufficient amount of PMMA was used to provide charged particle equilibrium) and the maximum dose given at each B-field was approximately 825 cGy. A region of interest of 2.5 cm × 2.5 cm was analysed for each film in order to obtain the netOD, where netOD is the difference between the optical density (OD) after and before irradiation. The film response curve is defined as netOD as a function of dose.

2.5. Film digitisation

The films were digitised with an EPSON Expression 10000XL Pro flat-bed colour scanner in transmission mode. Coloured images were acquired with a spatial resolution of 150 dpi with 48 bit RGB and all scanner colour corrections turned off. A frame was used to position the films at an area of the scanner bed which could correct OD readings for scanner light non-uniformity (Saur and Frengen 2008). The orientation of all films was kept constant and aligned within $\pm 5^\circ$ to avoid any effect due to polarised light. A 3.5 mm PMMA sheet was placed on top of the films during digitisation in order to position the films flat on the scanner bed. The scanner warming-up effect was diminished by using ten repeated scans. Films were scanned before, to account for background correction, and 48 h after irradiation in order to allow the film optical density to stabilise (Cheung *et al* 2005).

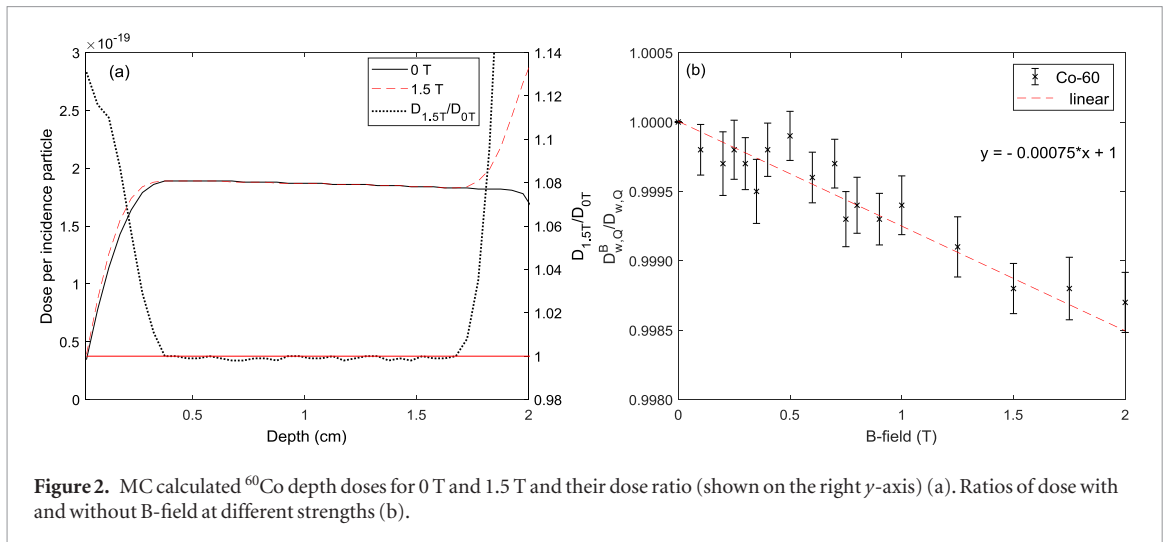

2.6. Film uncertainty

In a measurement of absorbed dose, the additional uncertainty⁵ introduced by using film arises from two sources: (i) the variations in film response from pixel to pixel within each ROI, which was determined using the method of Bouchard *et al* (2009), and (ii) the variations in response between ROIs on different pieces of film (in particular, the film used for measurement, compared with the films used for calibration), which was determined from a statistical analysis of repeated film measurements with 40 degrees of freedom.

3. Results

3.1. Effect of B-field on absorbed dose to water at ^{60}Co beam quality

Figure 2(a) shows the MC calculated ^{60}Co depth-doses for 0 T and 1.5 T B-field strengths and the ratio, dose from B-field of 1.5 T ($D_{w,Q}^{B1.5}$) divided by the dose in zero B-field ($D_{w,Q}$), on the right y -axis. It can be observed that for a B-field of 1.5 T the surface dose is enhanced by 13% and the d_{max} position is shifted closer to the surface by 0.05 cm. No effect was observed on the dose of d_{max} between the two B-field strengths. Figure 2(b) shows the ratios of calculated dose in water with and without B-field as a function of a B-field strength. The ratios were determined from the average ratios between the depths of 0.5 cm and 1.7 cm and it was found to change by -0.08% per T when a linear model is fitted. Based on this change, the dose values of the EBT-3 calibration curve at each B-field strength were adjusted to account for the effect of the B-field on dose to water. The electron return effect could also be visible after a depth of approximately 1.7 cm.

3.2. Effect of B-field on EBT-3 signal

In this work we have analysed the red, green and blue channel. However, we present selected results in graphical form, but mostly for the red channel only, as this is the channel which is usually used for single channel film dosimetry.

The EBT-3 film response curves (expressed in terms of netOD as a function of dose) for the red channel for all B-field strengths considered in this study are shown in figure 3. The maximum spread between all the B-fields for the red channel is also presented on the right y -axis of the same figure. For dose values greater than 75 cGy the maximum spread is 2.6% for the red channel, 3.5% for the green channel and 4.2% for the blue channel.

Table 1 shows the average absolute difference (in percent) of all dose levels between the response curves irradiated with and without a B-field. The difference is presented for each B-field and each colour channel.

We define ΔnetOD_B to be the difference between the netOD with and without a B-field:

$$\Delta\text{netOD}_B = \text{netOD}_{B \neq 0} - \text{netOD}_{B=0}. \quad (1)$$

Figure 4 shows ΔnetOD_B as a function of dose, for each B-field and for the red channel only. The error bars denote the standard uncertainty in netOD. The maximum ΔnetOD_B was found to be 0.006 for the red and green channels and -0.003 for the blue channel. Figure 4 shows that ΔnetOD_B does not have a strong dependence on dose. Similar results were observed for the green and blue channels.

It appears that ΔnetOD_B does depend on the B-field strength, being typically negative at 0.5 T and positive at 1 T and above. This effect is shown more clearly in figure 5, which depicts the average ΔnetOD_B over all dose levels, $\langle \Delta\text{netOD}_B \rangle_{D_{\text{all}}}$, as a function of B-field strength, for each channel.

⁵That is, in addition to the uncertainty of the dosimeter against which the film is calibrated.


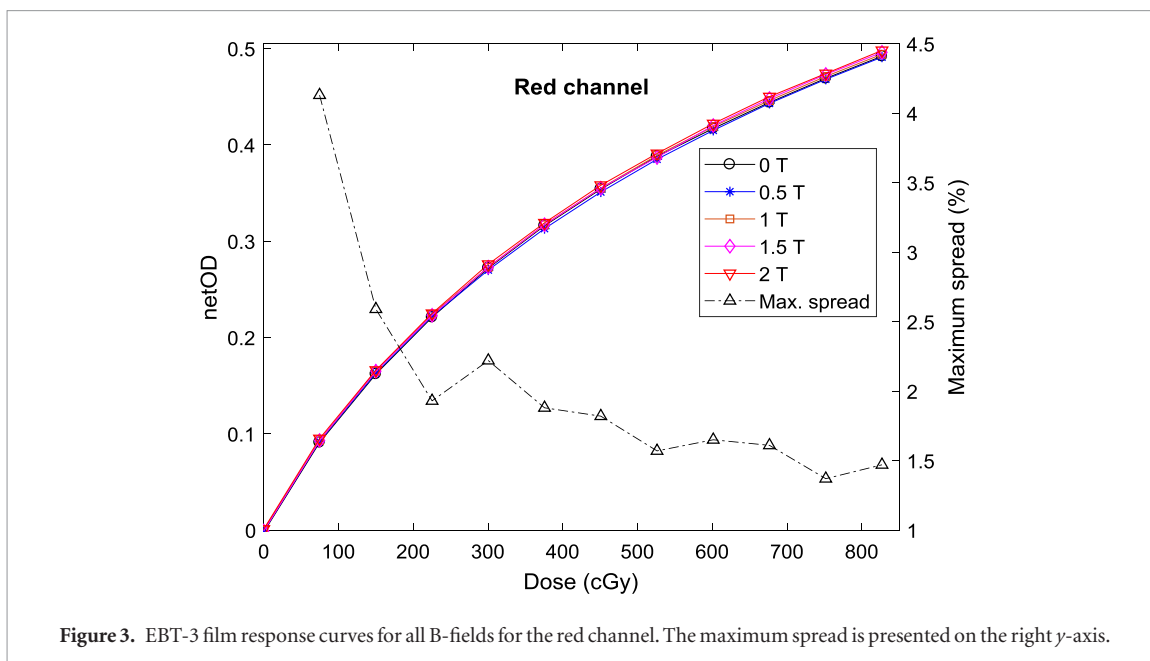



Table 1. Average absolute difference for red, green and blue channel. $\left(\left| \frac{\text{netOD}_{B \neq 0}}{\text{netOD}_{B=0}} - 1 \right| \right) \cdot 100$.

Channel	0.5 T (%)	1.0 T (%)	1.5 T (%)	2.0 T (%)
Red	0.5	0.9	0.8	1.6
Green	0.8	1.2	1.2	2.1
Blue	1.2	1.6	0.8	0.7

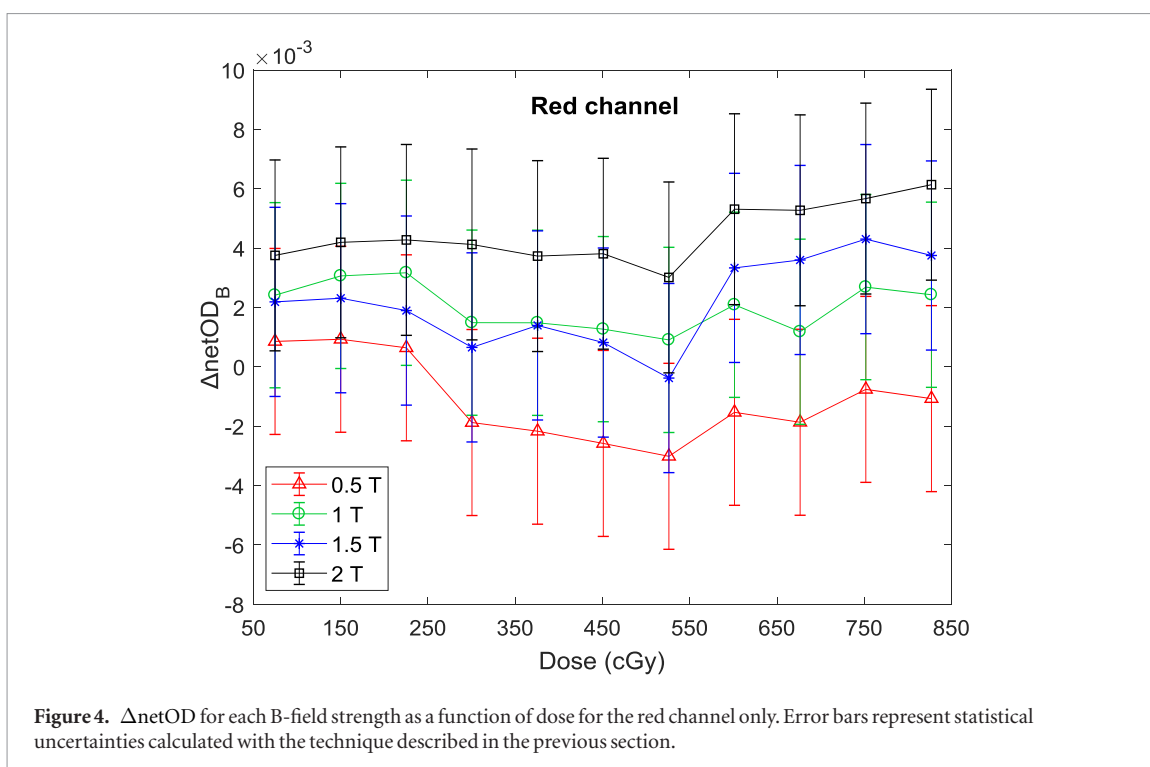

3.3. Effect of B-field on dose determined with EBT-3 film

The effect of the B-field on dose measured using EBT-3 films is shown in figure 6. The calibration curve, based on films irradiated at zero B-field, was used to obtain absorbed dose from films irradiated at non-zero B-field, which would be valid if the B-field has no effect on film response. Figure 6 shows the ratios, dose obtained from non-zero B-field films (using red channel) divided by the dose actually delivered. The delivered dose value takes account of the small effect of the B-field on dose to water, which was calculated by MC. The extent to which these ratios are significantly different from unity indicates the effect of the B-field on the film response. For all B-field

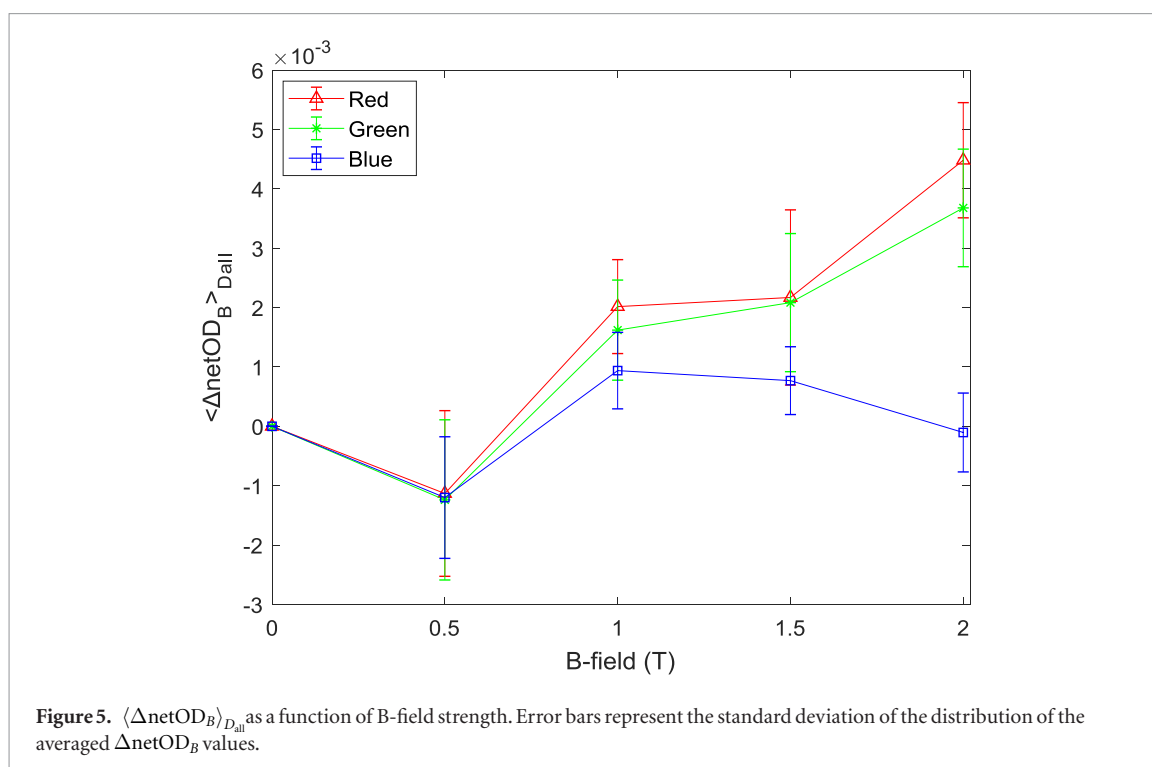

strengths the ratios decrease with dose, up to 225 cGy. Such behaviour would be accounted for by the inability of a fourth order polynomial to adequately represent film response at low dose. For values above 225 cGy, the ratios as a function of dose do not follow a simple trend and are somewhat scattered. Indeed, all ratios below 2 T are unity within the uncertainties.

Taking averages over all dose values above 75 cGy, the mean ratios are 0.994 ± 0.024 (0.5 T), 1.011 ± 0.023 (1 T), 1.012 ± 0.028 (1.5 T) and 1.024 ± 0.026 (2 T).

4. Discussion


The performance of the EBT-3 film in the presence of a B-field, has been investigated at different dose levels and over a range of B-field strengths. A ^{60}Co unit was used to irradiate film pieces placed between the poles of an electromagnet and the film response as a function of dose was obtained at five different field strengths. MC simulations were performed to determine the effect of a B-field on dose to water at the position of the film, and this effect was included in the analysis. The results show that there is at most a weak dependence of film sensitivity on magnetic field strength. At the smallest field strength (0.5 T), the film was found to under respond, while for field strengths of 1 T and above there was an over response. In terms of netOD (red channel) the under response was -0.0011 and the over response was up to 0.0045 at 2.0 T, with a standard uncertainty of ± 0.0030 . Similar results were observed for the green and blue channels. If this effect remains uncorrected, the error in a film measurement of absorbed dose (using the red channel) would vary from -0.6% at 0.5 T up to 2.4% at 2 T. The error at 1.5 T would be 1.2% . The standard uncertainty on this dose error is $\pm 1.4\%$, which is the contribution to a measurement of absorbed dose to water which arises from the use of film.

For the dose levels typically measured with EBT-3 film, and for the magnetic field strengths considered here, the actual values measured at different dose levels do not differ significantly from a magnetic field-dependent (but dose-independent) constant value.

Several studies have investigated the various sources of uncertainties on film dosimetry (Martiskova *et al* 2008, Saur and Frengen 2008, Bouchard *et al* 2009, Garcia and Azorin 2013), including film manufacturing, film manipulation, the irradiation and digitisation processes and film characterisation, leading to estimates of best uncertainty that range from 1% to 2%. The measurement uncertainties in the present work with EBT-3 (as explained in section 2.6) are consistent with this, ranging from 1.1% to 2.2% for dose levels above 75 cGy. This includes the small uncertainty related to the effect of the B-field on dose to water (0.05%). The magnitude of the effect of B-fields on EBT-3 film dosimetry observed in this study is comparable to the best achievable measurement uncertainty.

4.1. Comparison with different studies

The development of dosimetry in MRIGRT is still at a fairly early stage and it is essential that the performance of detectors used is well characterised. In the current literature on film dosimetry in B-fields, there remains some

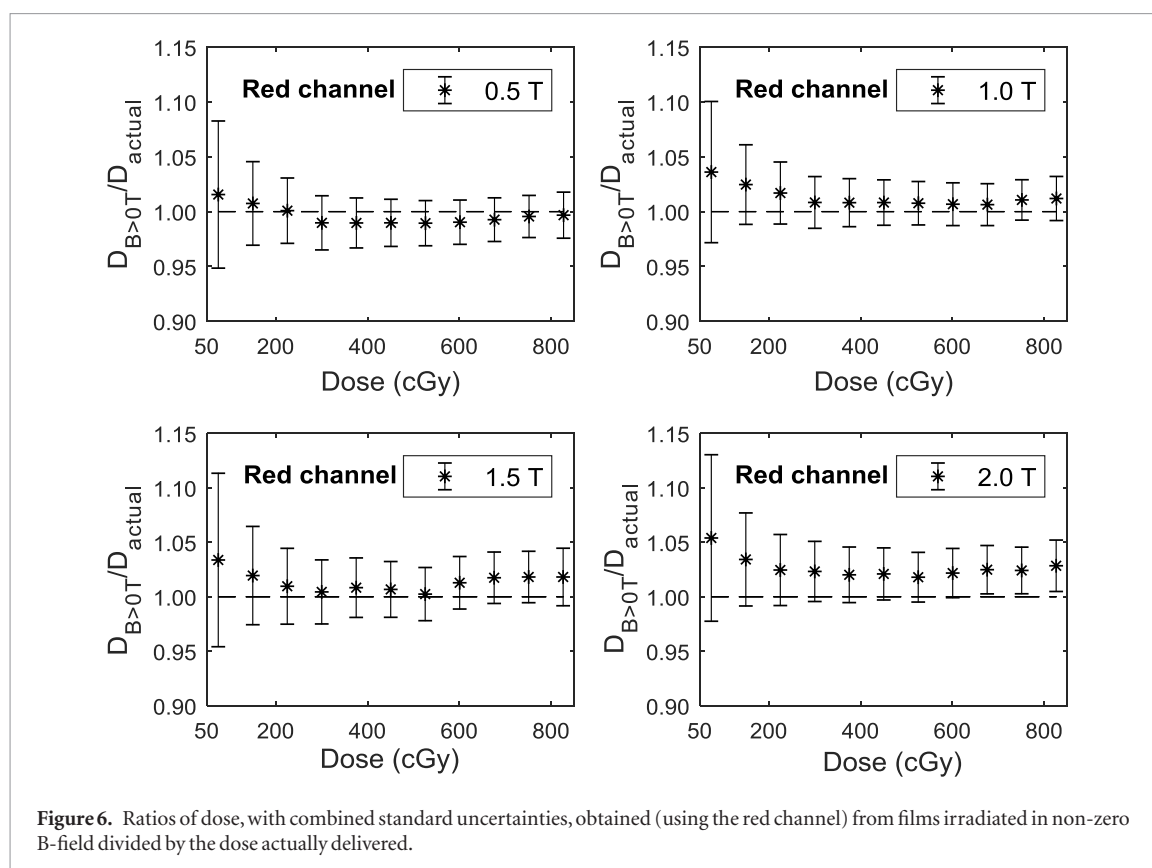

apparent inconsistency in the results reported from different studies. With the aim of resolving any consequent confusion we compare, where possible, the results reported here with those already published.

Roed *et al* (2017) examined the effect of a B-field (0 T and 1.5 T) on the response of EBT-3 film signal exposed in a ^{60}Co radiation beam. Their experiment involved two different orientations of the reference film edge with respect to (a) the B-field and (b) to scanning direction: either parallel or perpendicular in both cases. In all possible combinations, when film analysed using red channel, they found an under-response (ranging from approximately 1% to 3%) on all examined dose levels with B-field strength of 1.5 T compared to zero B-field dose. However, they also state that when the film is left in the B-field for a duration of (a) 6 min and 30 min the dose is over responding by less than 1% and (b) 7 min and 10 min the dose is under responding by less than 1%. The relationship between the dose change and the time of the film left in B-field they do not follow a simple pattern. In our study, the irradiation time of the films was ranging between 4 min to 15 min and the dose was found to over respond by an average of 1.2% at 1.5 T.

Reynoso *et al* (2016) used a ^{60}Co 0.35 T MRIdian system to irradiate EBT-2 films. Their results indicate that the netOD of the red, green and blue channel is decreased by an average of 8.7%, 8% and 4.3%, respectively. This study concludes that B-fields affect crystal orientation and polymerization during irradiation, judging from films scanned with an electron microscope. Although that study evaluated a different type of film, they specifically state that similar behaviour can be expected for EBT-3 because of the identical composition of the active layer. In the present work, the effect of a B-field on the netOD response of EBT-3 was found to be small. In the Reynoso *et al* (2016) study they show an average under response of netOD of approximately 7% for data up to 8 Gy (figure 2(b) in Reynoso *et al* (2016)). The reason for the difference between the results of these two studies is unclear.

A publication by Delfs *et al* (2018) assessed the effect of the B-field on EBT-3 using a 6 MV conventional linac and irradiating films in an electromagnet at two different magnetic strengths (0.35 T and 1.42 T). They report a decrease in the OD of up to 2.5% with an average, over all channels and over a range of dose values, of -0.8% . This effect was described by the authors as 2.1% increase in the dose values needed to produce a given OD at a B-field of 1.42 T. Our study found that there is indeed a change on film sensitivity however in the opposite direction of Delfs findings: the net OD is increased by $+0.8\%$ (red channel, 1.5 T). The dose required to produce a given optical density is smaller by 1.2%. Part of this difference might be explained due to energy dependence of EBT-3 film.

A recent study by Barten *et al* (2018) investigated the suitability of EBT-3 film for QA use in a 0.35 T ^{60}Co MRIdian system. Their measurements involved irradiation of EBT-3 film with and without MR imaging and at different angles with respect to B-field. They also performed equivalent measurements at 0 T, but this time using

a 6 MV conventional linac. Comparing calibration curves generated in ^{60}Co , with B-field, and in 6 MV, without B-field, they found a maximum difference of 0.9%. In our study the difference on dose measured using EBT-3 film with and without B-field in a ^{60}Co beam and at 0.5 T (the closest strength to 0.35 T) was found to be 0.7%, which agrees with the findings from Barten *et al* (2018).

The observed differences between the current study and the study by Roed *et al* (2017) show to be consistent within film uncertainties. Due to the nature of the film technique, any deviation can be explained because of the film perturbations influencing measurements uncertainties. However, this cannot explain the difference with the findings from Reynoso *et al* (2016) as it exceeds uncertainty margins. Although different type of EBT film generations were used, we anticipated consistency of published data and that EBT-2 to have a similar behaviour to EBT-3 under the strength of B-field.

It is essential to take measurement uncertainty into account when assessing the degree of agreement between two investigations. The field strength used by Delfs *et al* (2018) was 1.42 T. Assuming that it is fair to compare their result with our result for 1.5 T, and assuming that no correction is made for the possible effect of B-field on a film measurement of absorbed dose, then Delfs *et al* (2018) would estimate the uncorrected error as +2.1%, and we would estimate the uncorrected error as -1.2%. We quantify our standard uncertainty on this error as 1.4%, while Delfs *et al* (2018) merely assert that their 2.1% value 'exceeds the uncertainty margin of the experiment' but without quantifying the uncertainty on dose measured by film in their paper. We would note, however, that the difference between our results could only be significant at the level of two sigma if their standard uncertainty on dose is smaller than 0.8%, which is not plausible.

A good agreement was found between our study and the study of Barten *et al* (2018). Each of these studies (Barten *et al* 2018, Delfs *et al* 2018), however, used different beam quality, or a combination of beam qualities, to examine the effect of B-field on EBT-3 film response, compared to our work.

5. Conclusion

For the strongest B-field considered here (2 T), the sensitivity of Gafchromic EBT-3 film may be affected by the presence of a magnetic field at the time of irradiation. However, for MRI-linacs currently in use or under development, for which the field strength is at most 1.5 T, the effect of the B-field on EBT-3 film response was found to be zero within the best achievable measurement uncertainty. Results from this work agrees well with results presented by Roed *et al* (2017), but significantly deviates from the results shown by Reynoso *et al* (2016). A 3.3% difference was found from Delfs *et al* (2018) and a good agreement was observed with the findings by Barten *et al* (2018). The outcome of the current work contributes on settling the contradiction of these studies and conclude that EBT-3 film is a suitable dosimeter for absolute and relative dosimetry, with appropriate corrections, in MRI-guided radiotherapy.

Acknowledgments

The authors wish to thank Hugo Palmans from the Chemical, Medical and Environmental Science Department at NPL for his useful comments on the manuscript. The work was supported by the UK government's Department for Business, Innovation and Skills and the European Metrology Programme for Innovation and Research (EMPIR) project 15HLT08 MRIGRT. The EMPIR initiative is co-funded by the European Union's Horizon 2020 research and innovation programme and the EMPIR participating states. Research at The Institute of Cancer Research is supported by Cancer Research UK under Programme C33589/A19727 and NHS funding to the NIHR Biomedical Research Centre at The Royal Marsden Hospital and The Institute of Cancer Research.

ORCID iDs

Ilias Billas  <https://orcid.org/0000-0002-0446-1723>

References

- Arjomandy B, Taylor R, Anand A, Sahoo N, Gillin M, Prado K and Vico M 2010 Energy dependence and dose response of Gafchromic EBT2 film over a wide range of photon, electron, and proton beam energies *Med. Phys.* **37** 1942–7
- Barten D L J, Hoffmans D, Palacios M A, Heukelom S and van Battum L J 2018 Suitability of EBT3 GafChromic film for quality assurance in MR-guided radiotherapy at 0.35 T with and without real-time MR imaging *Phys. Med. Biol.* **63** 165014
- Billas I, Bouchard H, Subiel A, Silvestre I and Duane S 2017 A characterisation of EBT3 Gafchromic film for relative and absolute dosimetry (PO-0781) *ESTRO 36 (Vienna, Austria)*
- Bouchard H, Lacroix F, Beaudoin G, Carrier J F and Kawrakow I 2009 On the characterization and uncertainty analysis of radiochromic film dosimetry *Med. Phys.* **36** 1931–46
- Cheung T, Butson M J and Yu P K N 2005 Post-irradiation colouration of Gafchromic EBT radiochromic film *Phys. Med. Biol.* **50** N281–5

- Clark C H, Aird E G A, Bolton S, Miles E A, Nisbet A, Snaith J A D, Thomas R A S, Venables K and Thwaites D I 2015 Radiotherapy dosimetry audit: three decades of improving standards and accuracy in UK clinical practice and trials *Br. J. Radiol.* **88** 20150251
- Crijns S P M, Kok J G M, Lagendijk J J W and Raaymakers B W 2011 Towards MRI-guided linear accelerator control: gating on an MRI accelerator *Phys. Med. Biol.* **56** 4815–25
- Crijns S P M, Raaymakers B W and Lagendijk J J W 2012 Proof of concept of MRI-guided tracked radiation delivery: tracking one-dimensional motion *Phys. Med. Biol.* **57** 7863–72
- Delfs B, Schoenfeld A A, Popping D, Kapsch R P, Jiang P, Harder D, Poppe B and Looe H K 2018 Magnetic fields are causing small, but significant changes of the radiochromic EBT3 film response to 6 MV photons *Phys. Med. Biol.* **63** 035028
- Devic S, Seuntjens J, Hegyi G, Podgorsak E B, Soares C G, Kirov A S, Ali I, Williamson J F and Elizondo A 2004 Dosimetric properties of improved GafChromic films for seven different digitizers *Med. Phys.* **31** 2392–401
- Devic S, Tomic N and Lewis D 2016 Reference radiochromic film dosimetry: Review of technical aspects *Phys. Med.* **32** 541–56
- Dimitriadis A, Palmer A, Thomas R, Nisbet A and Clark C 2017 Adaptation and validation of a commercial head phantom for cranial radiosurgery dosimetry end-to-end audit *Br. J. Radiol.* **90** 20170053
- Garcia L I R and Azorin J F P 2013 Improving the calibration of radiochromic films by the use of uncertainties in optical density and dose *Med. Phys.* **40** 7
- Girard F, Bouchard H and Lacroix F 2012 Reference dosimetry using radiochromic film *J. Appl. Clin. Med. Phys.* **13** 339–53
- Kawrakow I, Mainegra-Hing E, Rogers D W O, Tessier F and Walters W B R 2011 The EGSnrc code system: Monte Carlo simulation of electron and photon transport *Report PIRS-701*, National Research Council of Canada (NRCC)
- Lagendijk J J W, Raaymakers B W, Raaijmakers A J E, Overweg J, Brown K J, Kerkhof E M, van der Put R W, Hardemark B, van Vutpen M and van der Heide U A 2008 MRI/linac integration *Radiother. Oncol.* **86** 25–9
- Low D A, Moran J M, Dempsey J F, Dong L and Oldham M 2011 Dosimetry tools and techniques for IMRT *Med. Phys.* **38** 1313–38
- Martiskova M, Ackermann B and Jakel O 2008 Analysis of uncertainties in Gafchromic (R) EBT film dosimetry of photon beams *Phys. Med. Biol.* **53** 7013–27
- Meijsing I, Raaymakers B W, Raaijmakers A J E, Kok J G M, Hogeweg L, Liu B and Lagendijk J J W 2009 Dosimetry for the MRI accelerator: the impact of a magnetic field on the response of a Farmer NE2571 ionization chamber *Phys. Med. Biol.* **54** 2993–3002
- Moylan R, Aland T and Kairn T 2013 Dosimetric accuracy of Gafchromic EBT2 and EBT3 film for *in vivo* dosimetry *Australas. Phys. Eng. Sci. Med.* **36** 331–7
- Niroomand-Rad A, Blackwell C R, Coursey B M, Gall K P, Galvin J M, McLaughlin W L, Meigooni A S, Nath R, Rodgers J E and Soares C G 1998 Radiochromic film dosimetry: recommendations of AAPM radiation therapy committee task group 55 *Med. Phys.* **25** 2093–115
- O'Brien D J, Roberts D A, Ibbott G S and Sawakuchi G O 2016 Reference dosimetry in magnetic fields: formalism and ionization chamber correction factors *Med. Phys.* **43** 4915–27
- Palmer A L et al 2015a A multicentre 'end to end' dosimetry audit for cervix HDR brachytherapy treatment *Radiother. Oncol.* **114** 264–71
- Palmer A L, Dimitriadis A, Nisbet A and Clark C H 2015b Evaluation of Gafchromic EBT-XD film, with comparison to EBT3 film, and application in high dose radiotherapy verification *Phys. Med. Biol.* **60** 8741–52
- Raaijmakers A J E, Raaymakers B W and Lagendijk J J W 2005 Integrating a MRI scanner with a 6 MV radiotherapy accelerator: dose increase at tissue-air interfaces in a lateral magnetic field due to returning electrons *Phys. Med. Biol.* **50** 1363–76
- Raaijmakers A J E, Raaymakers B W and Lagendijk J J W 2007 Experimental verification of magnetic field dose effects for the MRI-accelerator *Phys. Med. Biol.* **52** 4283–91
- Raaymakers B W et al 2009 Integrating a 1.5 T MRI scanner with a 6 MV accelerator: proof of concept *Phys. Med. Biol.* **54** N229–37
- Reinhardt S, Hillbrand M, Wilkens J J and Assmann W 2012 Comparison of Gafchromic EBT2 and EBT3 films for clinical photon and proton beams *Med. Phys.* **39** 5257–62
- Reynolds M, Fallone B G and Rathee S 2013 Dose response of selected ion chambers in applied homogeneous transverse and longitudinal magnetic fields *Med. Phys.* **40** 042102
- Reynoso F J, Curcuru A, Green O, Mutic S, Das I J and Santanam L 2016 Technical Note: Magnetic field effects on Gafchromic-film response in MR-IGRT *Med. Phys.* **43** 6552–6
- Roed Y, Lee H, Pinsky L and Ibbott G 2017 Characterizing the response of Gafchromic EBT3 film in a 1.5 T magnetic field (PO-0763) *ESTRO 36 (Vienna, Austria)*
- Sankar A, Kurup P, Murali V, Ayyangar K, Nehru R and Velmurugan J 2006 Evaluation of gafchromic EBT film for intensity modulated radiation therapy dose distribution verification *J. Med. Phys.* **31** 78–82
- Saur S and Frengen J 2008 GafChromic EBT film dosimetry with flatbed CCD scanner: A novel background correction method and full dose uncertainty analysis *Med. Phys.* **35** 3094–101
- Smit K, Kok J G M, Lagendijk J J W and Raaymakers B W 2014 Performance of a multi-axis ionization chamber array in a 1.5 T magnetic field *Phys. Med. Biol.* **59** 1845–55
- Smit K, van Asselen B, Kok J G M, Aalbers A H L, Lagendijk J J W and Raaymakers B W 2013 Towards reference dosimetry for the MR-linac: magnetic field correction of the ionization chamber reading *Phys. Med. Biol.* **58** 5945–57