

Decreasing the Polymerization Potential Improves the Selectivity of PPD Coated Disc Biosensors for Glutamate

Journal:	<i>Analytical Letters</i>
Manuscript ID:	draft
Manuscript Type:	Manuscript
Date Submitted by the Author:	n/a
Complete List of Authors:	Govindarajan, Sridhar; Newcastle University McNeil, Calum; Newcastle University, Diagnostic and Therapeutic Technologies
Keywords:	Glutamate Biosensor, selectivity, poly(o-phenylenediamine)



Decreasing the Polymerization Potential Improves the Selectivity of PPD Coated Disc Biosensors for Glutamate

Sridhar Govindarajan*^a and Calum J. McNeil^a

^a *Diagnostic and Therapeutic Technologies, The Medical School, Newcastle University, Newcastle upon Tyne, NE2 4HH, UK.*

E-mail: Sridhar.Govindarajan@ncl.ac.uk

Abstract

Selectivity of glutamate microdisc biosensors coated with poly(*o*-phenylenediamine) (PPD) as the interference rejecting layer against ascorbic acid was observed to be very low. Enhancement in the selectivity was noticed when the electropolymerization potential for the polymerization of the *o*-phenylenediamine monomer was decreased from 0.65V to 0.40V vs. Ag/AgCl. The selectivity coefficient increased from $-34.93 \pm 3.75 \% (n = 5)$ to $53.05 \pm 4.33 \% (n = 3)$. Decreasing the polymerization potential decreases the rate of formation of the polymer and therefore improves the compactness of the polymer layer formed, thereby increasing the selectivity of the electrodes.

Introduction

Biosensors to monitor the levels of glutamate with applications towards food industry and health have been developed since the early 1990s. Biosensors utilize a biological element such as an enzyme or an antibody to detect electro-inactive or poorly electroactive substances (O'Neill and Lowry 2006; O'Neill, Lowry, and Mas 1998). Biosensors prepared from different electrode materials and enzymes have been used to detect a variety of analytes, with glucose getting considerable attention due to its importance in diabetes care. More recently, neurochemical monitoring has gained considerable attention and in particular, the excitatory amino acid neurotransmitter glutamate due to its abundant

1
2
3
4 presence in the brain and its association to pathophysiological conditions such as
5 neuronal synaptic plasticity, learning and memory, ischaemia, secondary brain injury,
6
7 schizophrenia and epilepsy amongst others (Budd 1998; Danbolt 2001; Dingledine and
8
9 McBain 1999; Lancelot and Beal 1998). *In vivo* monitoring of glutamate by
10
11 electrochemical methods has been mentioned to be a difficult process due to the presence
12
13 of several electro-active species in the brain extracellular fluid that could be oxidised at
14
15 the electrodes, influencing the measured current (O'Neill and Lowry 2006); of particular
16
17 importance is ascorbic acid which has been found to be present in approximately 50 times
18
19 larger concentration than glutamate in the normal brain (O'Neill 1994). Therefore,
20
21 particularly for *in vivo* applications, the selectivity of the biosensor is of utmost
22
23 importance. First generation biosensor methods of H₂O₂ detection utilizing potentials of
24
25 0.65V or 0.70V vs. Ag/AgCl reference electrode are more prone to interferences due to
26
27 higher recording potentials. To improve the selectivity of the first generation glutamate
28
29 biosensors, several techniques have been used such as polymer coatings on platinum,
30
31 gold, palladium or glassified carbon electrodes (O'Neill et al. 2004) (*e.g.*, over oxidised
32
33 polypyrrole (Hamdi et al. 2006), polyphenylenediamines (O'Neill, Lowry, and Ryan
34
35 1997), polyurethanes (Yu, Moussy, and Moussy 2005), polynaphthalenes (Murphy 1998),
36
37 Nafion (Gerhardt et al. 2002)).
38
39
40
41
42
43
44

45
46 Electropolymerization of *o*-phenylenediamine (*o*-PD) at platinum electrodes have been
47
48 shown to provide a high level of selectivity at platinum cylinders while maintaining a
49
50 high sensitivity to the target analyte (O'Neill, Lowry, and Ryan 1997). Recently,
51
52 McMahon and co-workers showed that platinum microdiscs showed increased oxygen
53
54 tolerance when compared to platinum cylinders (McMahon et al. 2006). In addition, in
55
56 our own study, it was found that the temporal stability of the glutamate response was
57
58 higher for microdiscs than cylinders (results not shown). But the selectivity of poly(*o*-
59
60

1
2
3 phenylenediamine) (PPD) covered microdiscs have been shown to be quite low when
4 compared to 1mm cylinders and that the efficiency of the polymer formation decreases
5 with decrease in the surface area of the electrode (McMahon et al. 2004). Therefore, in
6 this study, we investigate the impact of decreasing the potential required for the
7 electropolymerization of the monomer on the selectivity of the PPD coated disc
8 electrodes.

9
10 Teflon[®] coated platinum wire of 125 μ m diameter was used for the experiments.
11 Microdiscs of 125 μ m diameter were obtained by cutting the insulated platinum wire
12 transversely and leaving the Teflon[®] coating intact. The solutions for glutamate (Glut),
13 ascorbic acid (AA) and H₂O₂ were prepared in distilled water, while the monomer
14 solution (300mM *o*-PD + 0.5% (w/v) BSA) was prepared in PBS at pH 7.4.

15
16 To determine the effects of polymerization potential on the selectivity of PPD covered
17 disc electrodes, different polymerization potentials were examined; 0.40V, 0.45V, 0.50V
18 and 0.65V *vs.* Ag/AgCl for 20 minutes. The polymerization was performed at bare
19 platinum disc electrodes by applying a potential against Ag/AgCl electrode in a 3
20 electrode cell with a stainless steel needle acting as the auxilliary electrode immersed in
21 the monomer solution mentioned above. All calibrations were performed in a two
22 electrode cell with the reference electrode acting as both reference and counter at 0.65V
23 *vs.* Ag/AgCl in PBS at pH 7.4.

24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 **Results and Discussion**

52 Poly(*o*-phenylenediamine) electropolymerized at neutral pH has been shown to form a
53 insulating, self-sealing polymer layer on Pt and other electrode materials (O'Neill et al.
54 2004; O'Neill et al. 1994; O'Neill, Lowry, and Ryan 1997; McMahon et al. 2004). The
55 selectivity of disc electrodes immobilized with glutamate oxidase (GluOx) and
56
57
58
59
60

1
2
3 electropolymerized with PPD-BSA (Pt_D/GluOx/PPD-BSA) at 0.65V vs. Ag/AgCl
4 provided a mean selectivity of $-34.93 \pm 3.75 \%$ ($n = 5$) against ascorbic acid calculated as
5
6
7
8 $S_{\text{Glut(AA)}} = (I_{\text{Glut}} - I_{\text{AA}}) * 100 / I_{\text{Glut}}$ (O'Neill, Lowry, and Ryan 1997). I_{Glut} and I_{AA}
9 represent the absolute steady-state currents obtained for $10 \mu\text{mol l}^{-1}$ glutamate and 500
10 $\mu\text{mol l}^{-1}$ AA respectively, as they correspond to the physiological levels of the substances
11 in the brain ECF. A negative selectivity value meant that the response for $500 \mu\text{mol l}^{-1}$
12 AA was greater than the response for $10 \mu\text{mol l}^{-1}$ Glut. A biosensor with a negative
13 selectivity value would be unusable and therefore further investigation was necessary in
14 order to attempt to enhance the selectivity of PPD coated discs towards glutamate.

15
16
17
18
19
20
21
22
23
24
25 As it had been speculated by McMahan et al. that the decreased selectivity at disc
26 electrodes could be due to the highly efficient hemispherical transport of monomer
27 molecules resulting in a very rapid but non-compact polymer formation on the electrode
28 (McMahan et al. 2004), it was necessary to decrease the rate of polymer formation in
29 order to increase the selectivity. As it is well known that the rate of polymer formation is
30 affected by variations in monomer concentration, polymerization potential and the
31 polymerization time, amongst others, the effect of polymerization potential on the
32 selectivity of the PPD coated discs were considered.

33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
The effect of polymerization potential on the selectivity of the electrodes was studied by
performing electropolymerization at a series of different potentials on bare platinum
discs. The results showed a drastic improvement in the selectivity of the electrodes with
decreasing potential. Since the electrodes were devoid of the enzyme, H₂O₂ was used to
determine their selectivity. The selectivity of the PPD coated discs (Pt_D/PPD-BSA) were
calculated using the formula $S_{\text{AA(H}_2\text{O}_2)}} = I(\text{AA}) * 100 / I(\text{H}_2\text{O}_2)$, with $I(\text{AA})$ and $I(\text{H}_2\text{O}_2)$
representing the currents obtained at 1mM concentrations respectively (McMahan et al.
2004). As $I(\text{AA})$ should ideally be very small when compared to $I(\text{H}_2\text{O}_2)$, the electrode

1
2
3 with a $S_{AA(H_2O_2)}$ value closer to zero would a lower relative permeability to AA compared
4
5 to H_2O_2 and hence have a higher selectivity towards H_2O_2 and glutamate. By performing
6
7 cyclic voltammetric experiments it was determined that a polymerization potential lower
8
9 than 0.4V (vs. Ag/AgCl) would result in a non-compact polymer layer as the threshold
10
11 potential was identified to be close to 0.35V. Performing H_2O_2 and AA calibrations at
12
13 PPD coated electrodes electropolymerized at 0.40V, 0.45V, 0.50V and 0.65V vs.
14
15 Ag/AgCl, selectivity values of 0.16%, 0.18%, 0.37% and 0.72% were obtained
16
17 respectively; a 400% increase in selectivity could be seen when the electrode was
18
19 polymerized at 0.40V (vs. Ag/AgCl) when compared to 0.65V (vs. Ag/AgCl) which was
20
21 common until now. A graphical representation of the AA calibration at electrodes
22
23 polymerized at different potentials along with the respective selectivity coefficients have
24
25 been shown in Figure 1.
26
27
28
29
30

31
32 By closer observation of the currents obtained during polymerization at different
33
34 potentials reveals the nature of polymer of formed. From Figure 2, the magnitude of the
35
36 initial spike currents obtained immediately following the start of the polymerization
37
38 process can be seen to decrease with decrease in the polymerization potential. This results
39
40 in a slower self-sealing polymer formation leading to a more compact polymer layer,
41
42 thereby increasing the electrode selectivity.
43
44

45
46 Following the observation of improvement in selectivity with decrease in polymerization
47
48 potential, enzyme incorporated disc electrodes were prepared with the polymerization
49
50 performed at 0.45V (vs. Ag/AgCl). The selectivity $S_{Glut(AA)}$ could be seen to have
51
52 improved to $53.05 \pm 4.33 \%$ ($n = 3$) from $-34.93 \pm 3.75 \%$ ($n = 5$) obtained for electrodes
53
54 polymerized at 0.65V (vs. Ag/AgCl). Figure 3 shows the selectivities obtained for
55
56 glutamate against ascorbic acid with the electropolymerization potential maintained at
57
58 0.65V and 0.45V (vs. Ag/AgCl) respectively. Since all the other measurement parameters
59
60

1
2
3 were similar during the experiments, the improvement in selectivity for glutamate can be
4
5 directly attributed to the decreased electropolymerization potential.
6
7
8
9

10 **Conclusion**

11
12 In this study we observed that decreasing the polymerization potential for the formation
13
14 of PPD at platinum microdiscs, increases the compactness of the polymer structure due to
15
16 slower diffusion of the monomer towards the electrode, thereby increasing the selectivity
17
18 of the disc electrodes to glutamate and H₂O₂. Additional lipid coatings incorporated into
19
20 the biosensor matrix enhanced the selectivity of glutamate microdiscs above 85% (results
21
22 not shown).
23
24
25
26
27
28
29

30 **Acknowledgement**

31
32 We thank Prof. R.D. O'Neill (Department of Chemistry, University College Dublin,
33
34 Ireland) for his guidance and support.
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

References

- Budd, Samantha L. 1998. Mechanisms of Neuronal Damage in Brain Hypoxia/Ischemia: Focus on the Role of Mitochondrial Calcium Accumulation. *Pharmacol. Ther.* 80 (2):203 - 229.
- Danbolt, Niels C. 2001. Glutamate uptake. *Progress in Neurobiology* 65 (1):1-75.
- Dingledine, Raymond, and Chris L. McBain. 1999. Glutamate and Aspartate. In *Basic Neurochemistry: Molecular, cellular and medical aspects*, edited by G. J. Siegel, B. W. Agranoff, R. W. Albers, S. K. Fisher and M. D. Uhler. Philadelphia: Lippincott Williams & Wilkins.
- Gerhardt, Greg A., Jason J. Burmeister, Francois Pomerleau, Michael Palmer, Brian K. Day, and Peter Huettl. 2002. Improved ceramic-based multisite microelectrode for rapid measurements of L-glutamate in the CNS. *Journal of Neuroscience Methods* 119:163 - 171.
- Hamdi, Naser, Jianjun Wang, Eric Walker, Nigel T. Maidment, and Harold G. Monbouquette. 2006. An electroenzymatic l-glutamate microbiosensor selective against dopamine. *Journal of Electroanalytical Chemistry* 591 (1):33-40.
- Lancelot, Eric, and M. Flint Beal. 1998. Glutamate toxicity in chronic neurodegenerative diseases. In *The Glutamate Synapse as a Therapeutic Target: Molecular Organization and Pathology of the Glutamate Synapse*, edited by O. P. Ottersen, I. A. Langmoen and L. Gjerstad. Amsterdam: Elsevier Science.
- McMahon, C. P., S. J. Killoran, S. M. Kirwan, and D. O'Neill R. 2004. The selectivity of electrosynthesised polymer membranes depends on the electrode dimensions: implications for biosensor applications. *Chemical Communication*:2128-2130.
- McMahon, C. P., G. Rocchitta, P. A. Serra, S. M. Kirwan, J. P. Lowry, and R. D. O'Neill. 2006. Control of the oxygen dependence of an implantable polymer/enzyme composite biosensor for glutamate. *Analytical Chemistry* 78 (7):2352-9.
- Murphy, L. J. 1998. Reduction of Interference Response at a Hydrogen Peroxide Detecting Electrode Using Electropolymerized Films of Substituted Naphthalenes. *Analytical Chemistry* 70 (14):2928-2935.
- O'Neill, R. D. 1994. Microvoltammetric techniques and sensors for monitoring neurochemical dynamics in vivo. A review. *Analyst* 119 (5):767-79.

- 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
- O'Neill, R. D., and J. P. Lowry. 2006. Neuroanalytical Chemistry In Vivo Using Electrochemical Sensors. In *Encyclopedia of Sensors*, edited by C. A. Grimes, E. C. Dickey and M. V. Pishko: American Scientific Publishers.
- O'Neill, Robert D., Seung-Cheol Chang, John P. Lowry, and Calum J. McNeil. 2004. Comparisons of platinum, gold, palladium and glassy carbon as electrode materials in the design of biosensors for glutamate. *Biosensors and Bioelectronics* 19 (11):1521-1528.
- O'Neill, Robert D., John P. Lowry, and Manuel Mas. 1998. Monitoring Brain Chemistry In Vivo: Voltammetric Techniques, Sensors and Behavioral Applications. *Critical Reviews in Neurobiology* 12 (1&2):69-127.
- O'Neill, Robert D., John P. Lowry, Karl McAleer, Adrienne Duff, and Satea S. El Atrash. 1994. Characterization of Glucose Oxidase-Modified Poly(phenylenediamine)-Coated Electrodes in Vitro and in Vivo: Homogeneous Interference by Ascorbic Acid in Hydrogen Peroxide Detection. *Analytical Chemistry* 66:1754 - 1761.
- O'Neill, Robert D., John P. Lowry, and Michael R. Ryan. 1997. Biosensor for Neurotransmitter L-Glutamic Acid Designed for Efficient Use of L-Glutamate Oxidase and Effective Rejection of Interference. *The Analyst* 122:1419 - 1424.
- Yu, Bazhang, Yvonne Moussy, and Francis Moussy. 2005. Coil-type Implantable Glucose Biosensor with Excess Enzyme Loading. *Frontiers in Bioscience* 10:512-520.

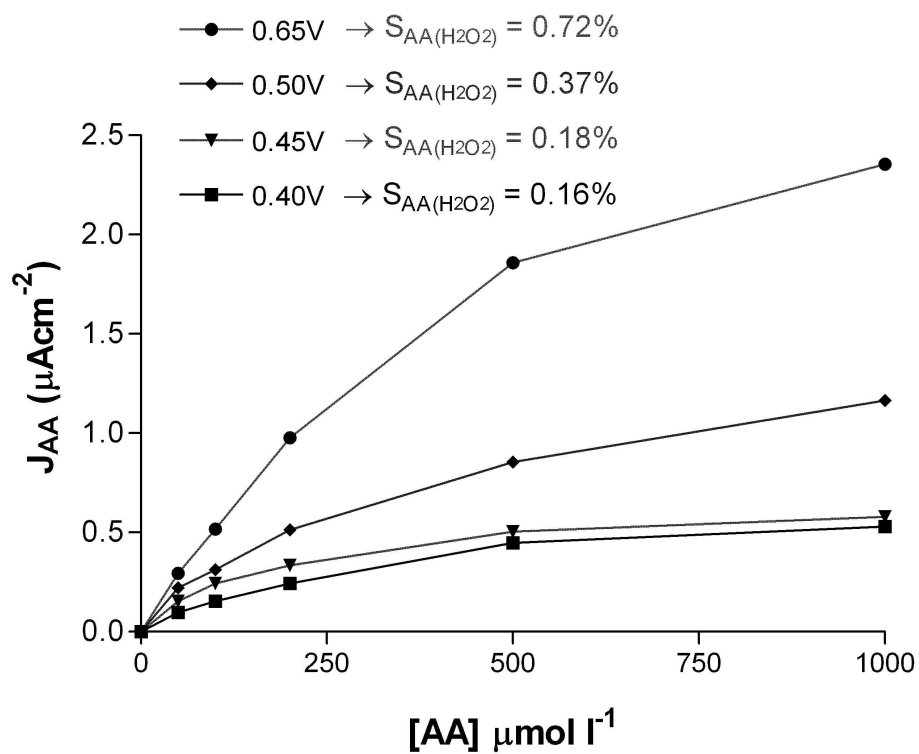


Figure 1: Ascorbic acid calibrations obtained at Pt_D/PPD-BSA electrodes polymerized at different potentials. The values are represented as current densities. The selectivity values for AA obtained against H_2O_2 at the different polymerization potentials are shown in the legend.

116x93mm (600 x 600 DPI)


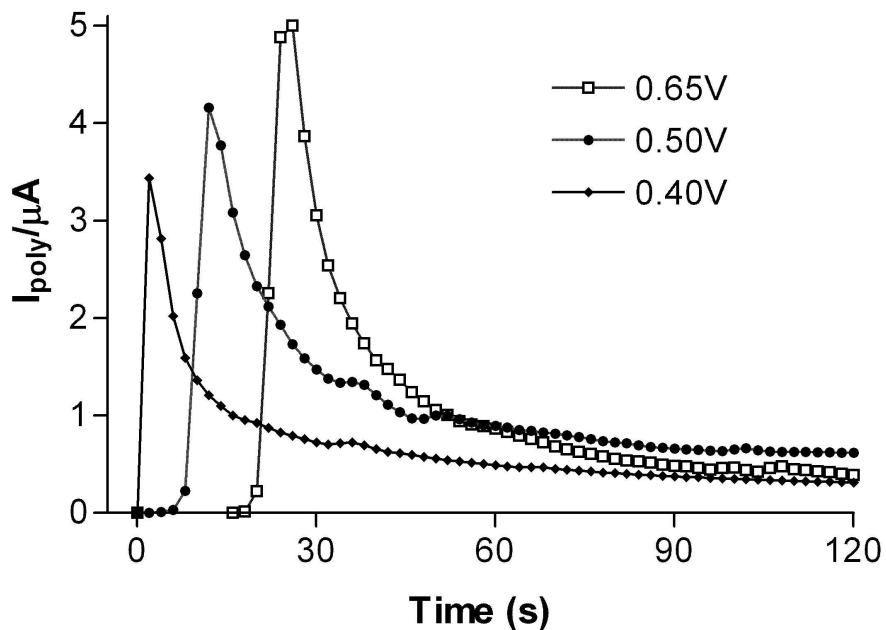


Figure 2: Currents obtained during the first 2 minutes after the initiation of electropolymerization of bare platinum discs at 0.40V, 0.50V and 0.65V (vs. Ag/AgCl). The currents have been shown with a 5 second time shift for better readability. The lower the polymerization potential, the lower the initial spike, leading to slower and more compact polymer deposition.
102x73mm (600 x 600 DPI)

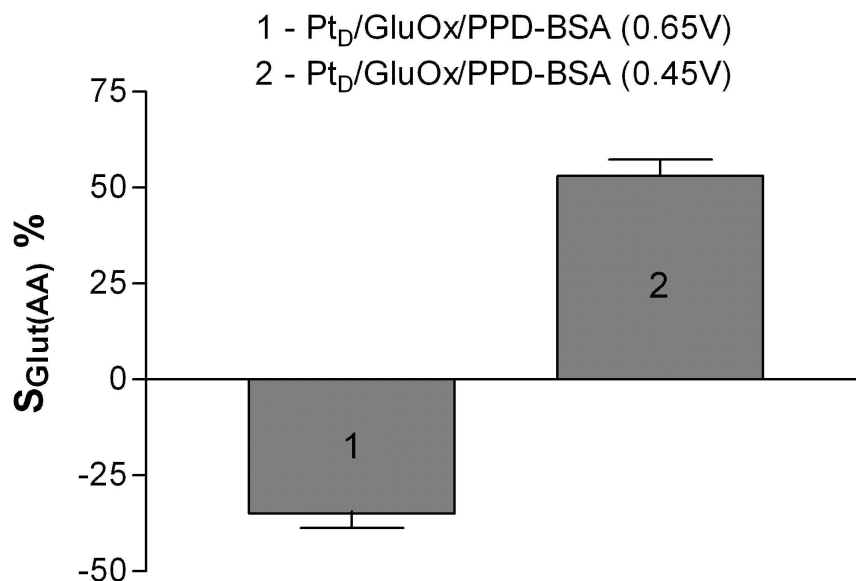

29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Figure 3: Selectivity values obtained for Pt_D/GluOx/PPD-BSA biosensor with the PPD-BSA polymerization performed at 0.65V and 0.45V vs. Ag/AgCl respectively have been shown. 1 - Pt_D/GluOx/PPD-BSA (0.65V) with a S_{Glut(AA)} value of -34.93 ± 3.75 % (n = 5) and 2 - Pt_D/GluOx/PPD-BSA (0.45V) with a S_{Glut(AA)} value of 53.05 ± 4.33 % (n = 3). The bars indicate Mean ± SEM values.
105x65mm (600 x 600 DPI)