



CHEMOMETRIC – ASSISTED UV SPECTROPHOTOMETRIC METHOD FOR DETERMINATION OF ANTIHYPERLIPIDEMIC AGENTS IN PHARMACEUTICAL FORMULATION

Santosh V. Gandhi*, Amit S. Mutha

AISSMS College of Pharmacy, Kennedy Road, Pune- 411001, Maharashtra, India

Article Information

Received: 15th March 2017

Revised: 26th March 2017

Accepted: 04th April 2017

Keywords

Atorvastatin calcium, Ezetimibe, PLS, PCR, Validation

ABSTRACT

This presented work is based on application of two multivariate calibration methods for simultaneous UV-VIS spectrophotometric determination of active substances in combined pharmaceutical formulation composed of Atorvastatin calcium (ATV) and Ezetimibe (EZT). The methods used were Principal Component Regression (PCR) and Partial Least Square (PLS). The Spectra of ATV and EZT were recorded at concentrations within their linear range 5.0-30.0 µg/ml for both drugs. 28 set of mixtures were used for calibration and 08 set of mixtures were used for validation in the wavelength range of 230 to 260 nm with the wavelength intervals $\lambda=0.5$ nm in methanol. The methods were validated as per International Conference on Harmonization Q2 (R1) (ICH) guidelines. These methods were successfully applied for determination of drugs in pharmaceutical formulation (tablet) with no interference of the excipient as indicated by the recovery study results. The proposed methods are simple, rapid and can be easily used as an alternative analysis tool in the quality control as well as in process control of drugs and formulation.

INTRODUCTION

Atorvastatin calcium is [R-(R, R*)]-2-(4-fluorophenyl)- β , δ -dihydroxy-5(1-methylethyl)-3-phenyl-4-[phenylamino carbonyl]-1H-pyrrole-1-heptanoic acid, calcium salt [Fig. 1(a)] is well-known member of the drug class known as statins, which are used primarily as a lipid-lowering agent that inhibits HMG-CoA reductase enzyme which is found in liver tissue for production of cholesterol [1]. It is official in Indian Pharmacopeia [2]. Ezetimibe is 1-(-4-fluorophenyl)-(3S)-hydroxypropyl)-(4S)-(4-hydroxyphenyl)-2azeti-dinone [Fig. 1(b)] is a selective cholesterol absorption inhibitor, which potentially inhibits the absorption of biliary and dietary cholesterol [3]. It is official in Indian Pharmacopeia [4]. Several methods are reported for quantitative determination of ATV and EZT in single and in combination such as UV, HPTLC, and RP-HPLC [5-14]. Chemometric is the science of extracting information from chemical systems. Multivariate calibration

method (e.g., multiple linear regression (MLR), principle component regression (PCR) and partial least squares (PLS) utilizing spectrophotometric data are the important chemometric approach for determination of mixtures including drugs combination [15]. While working on development of simple, accurate and precise method for this combination we came across one recent report for analysis of these drugs by chemometric analysis using MATLAB software [16]. We have developed method using Unscrambler X (10.3) software. Compared with reported method the results were found promising.

MATERIALS AND METHODS

Instrumentation

Double beam UV- Vis spectrophotometer (Jasco V-730) with matched pair of 1cm quartz cells were used to record spectra of all solutions. The spectra were recorded at spectral band width

*For Correspondence: santoshvgandhi@rediffmail.com

©2017 The authors. This is an Open Access article distributed under the terms of the Creative Commons Attribution (CC BY NC), which permits unrestricted use, distribution, and reproduction in any medium, as long as the original authors and source are cited. No permission is required from the authors or the publishers.

of 2.0 nm, scanning speed 100 nm/min and data pitch 0.5 nm. Unscrambler X (10.3) (64-bit) trial version and Microsoft Excel 2013 were used for model generation and application of chemometric.




Figure 1: Structure of a) Atorvastatin calcium (ATV) and b) Ezetimibe (EZT)

Material and Reagents

Reference standard of ATV and EZT were obtained from Wockhardt Research Centre, Aurangabad as gift samples and methanol (AR grade) purchased from LOBA Chemie, India. Atorsave EZ tablets manufactured by Eris Life Sciences Pvt. Ltd. containing Atorvastatin calcium IP 10 mg and Ezetimibe IP 10 mg were procured from local pharmacy shop.

One component calibration

To find linear concentration of each drug, one component calibration was performed. Linear dynamic ranges were studied in the concentration range of 5.0-30.0 $\mu\text{g/ml}$ for both ATV and EZT. Absorbance values were recorded at λ_{max} of each drug (247 nm for ATV and 233 nm for EZT) against methanol as blank. Linear dynamic range for each compound was determined by least-square linear regression of concentration and the corresponding absorbance. Fig. 2 represents Individual spectra, mixtures and sum of the spectra for ATV and EZT. According to the figures, there is no interaction between analytes as the signals appear with additive properties.




Figure 2: Individual spectra, mixtures and sum of the spectra for ATV and EZT

Preparation of standard stock solution

Stock solution of ATV and EZT were prepared by dissolving accurately weighed 10 mg of standard drug in 10 ml of methanol, separately. The concentration of ATV and EZT were 1000 $\mu\text{g/ml}$ from which further 5 ml was pipetted and diluted to 50 ml to achieve final concentration of 100 $\mu\text{g/ml}$ of ATV and EZT, separately.

Preparation of working stock solution

Working standard solutions were prepared from standard stock solution of 100 $\mu\text{g/ml}$ by appropriate dilution with methanol to obtain final concentration of 5, 10, 15, 20, 25 and 30 $\mu\text{g/ml}$ for both ATV and EZT respectively.

Construction of calibration and validation set

A total set of 36 mixtures were prepared by combining working standard of ATV and EZT in their linear concentration range of 5.0-30.0 $\mu\text{g/ml}$. (Table I). From these 28 mixtures were used for calibration set and 08 mixtures were used for validation set by random selection. The absorbance spectra were recorded in range of 230- 260 nm with 0.5 nm interval. The spectra were saved as ASCII (.txt) format which were further extracted in MS-Excel as required by Unscrambler software for model generation. The PCR and PLS models were developed utilizing absorption data using Unscrambler software. Selection of proper number of latent variables for development of model was necessary to obtain good prediction. Leave-one-out (LOO)

cross validation method was used to obtain necessary number of latent variables (LVs), as shown in Fig. 3 and calculated using formula [17],

$$RMSECV = \sqrt{\sum \frac{(C_{act} - C_{pre})^2}{I_c}}$$

Where,

RMSECV= Root mean square error of cross validation

C_{act}= actual concentration of calibration set

C_{pre}= predicted concentration of validation set

I_c= Total number of samples in calibration set

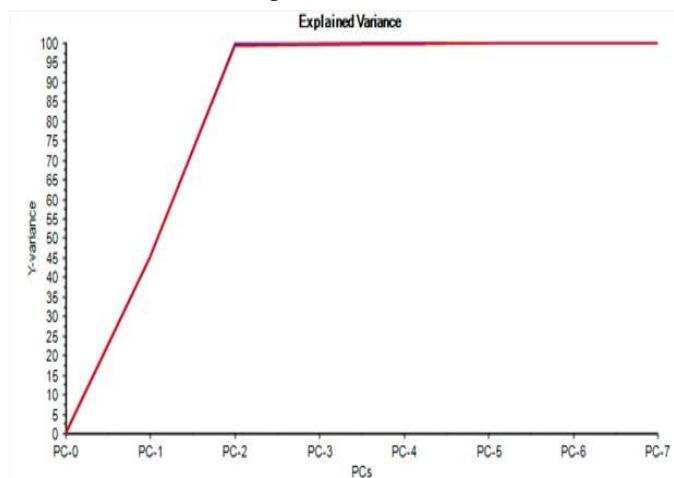


Figure 3: Explained Variance describing number of optimum PCs (Principle Components)

After the PCR and PLS models have been constructed, it was found that the optimum number of LVs were two factors for both PCR and PLS. For validation of generated models, concentration in validation set was predicted by using proposed PCR and PLS models (Table II). The validation of developed methods was performed as per ICH Q2 (R1) [18].

Assay of marketed preparation

20 tablets of AtorsaveEZ were accurately weighed and finely powdered. Tablet powder equivalent to 10 mg of ATV (10 mg of EZT) was taken and transferred to 10 ml volumetric flask and was diluted to 10 ml with methanol. The solution was sonicated for 10 minutes. This solution was then filtered with help of whatman filter paper no. 41. 1 ml of filtrate solution was diluted to 10 ml with methanol. Further 1 ml of this solution was diluted to 10 ml with methanol to get final concentration of 10 µg/ml of ATV and EZT each. The procedure was repeated 6 times for tablet formulation. The assay results are presented in Table III.

Accuracy study

The accuracy study was carried out at three levels 50 %, 100 % and 150 % of assay concentration. Calculated amount of ATV and EZT from standard solutions were spiked into sample solution and scanned in range of 230-260 nm. Concentrations were predicted by using developed PCR and PLS models. Accuracy data is presented in Table IV and Table V.

Table I: Composition of calibration and validation sets.

MIX. NO	ATV (µg/ml)	EZT (µg/ml)	MIX. NO	ATV (µg/ml)	EZT (µg/ml)
1	5	15	19	25	10
2	5	20	20	25	15
3	5	25	21	25	20
4	5	30	22	25	25
5	10	5	23	25	30
6	10	10	24	30	5
7	10	15	25	30	15
8	10	20	26	30	20
9	10	25	27	30	25
10	10	30	28	30	30
11	15	15	29	5	5
12	15	20	30	5	10
13	15	25	31	15	5
14	20	5	32	15	10
15	20	10	33	15	30
16	20	15	34	20	20
17	20	25	35	20	30
18	25	5	36	30	10

*Calibration set - Mix No. 1-28

*Validation set - Mix No. 29-36

Precision

Precision was carried at three concentration levels (10, 15, 20 µg/ml for both ATV and EZT) in three replicates at each level. The results of intraday and interday precision studies which are presented in Table VI and Table VII.

LOD and LOQ

LOD and LOQ were calculated as 3.3 σ/S and 10 σ/S, respectively; where σ is the standard deviation of the response (y-intercept) and S is the slope of the calibration plot.

Table II: Predicted results for validation set by PCR and PLS method.

METHOD		PCR				PLS			
ATV	EZT	ATV		EZT		ATV		EZT	
Actual ($\mu\text{g/ml}$)		Predicted	% R*	Predicted	% R*	Predicted	% R*	Predicted	% R*
5	5	5.046	100.9	5.013	100.2	5.046	100.9	5.016	100.3
5	10	5.070	101.4	10.129	101.2	5.077	101.5	10.122	101.2
15	5	15.108	100.7	4.902	98.0	15.108	100.7	4.903	98.0
15	10	15.560	103.7	9.882	98.8	15.559	103.7	9.884	98.8
15	30	15.106	100.7	29.127	97.0	15.105	100.7	29.128	97.0
20	20	19.942	99.7	21.488	107.4	19.946	99.7	21.484	107.4
20	30	19.626	98.1	30.412	101.3	19.627	98.1	30.411	101.3
30	10	29.965	99.8	9.895	98.9	29.966	99.8	9.894	98.9

* % R - % Recovery

Table III: Assay result for ATV and EZT in tablet (AtorsaveEZ) by proposed methods

METHOD		PCR				PLS			
ATV	EZT	ATV		EZT		ATV		EZT	
Actual ($\mu\text{g/ml}$)		Predicted ($\mu\text{g/ml}$)	% R	Predicted ($\mu\text{g/ml}$)	% R	Predicted ($\mu\text{g/ml}$)	% R	Predicted ($\mu\text{g/ml}$)	% R
10	10	9.716	97.1	9.877	98.7	9.700	97.0	9.878	98.7
10	10	9.969	99.6	9.922	99.2	9.968	99.6	9.927	99.2
10	10	9.959	99.5	9.975	99.7	9.954	99.5	9.975	99.7
10	10	10.004	100.0	10.162	101.6	10.001	100.0	10.164	101.6
10	10	9.979	99.7	9.892	98.9	9.975	99.7	9.899	98.9
10	10	9.995	99.9	9.916	99.1	9.994	99.9	9.917	99.1
MEAN		9.937	99.3	9.957	99.5	9.932	99.3	9.960	99.6
SD		0.109	1.095	0.105	1.057	0.114	1.148	0.105	1.050

* % R - % Recovery

Table IV: Accuracy data of ATV by PCR and PLS models.

Level %	Sample Conc. $\mu\text{g/ml}$	Amount added $\mu\text{g/ml}$	Total Conc. $\mu\text{g/ml}$	Predicted Conc. $\mu\text{g/ml}$		% Recovery		% RSD	
				PCR	PLS	PCR	PLS	PCR	PLS
50 %	10	5	15	14.88	14.88	99.2	99.2	0.389	0.953
				14.97	14.97	99.8	99.8		
				14.99	14.69	99.9	97.9		
100 %	10	10	20	20.08	20.07	100.4	100.3	0.774	0.773
				20.15	20.14	100.7	100.7		
				19.85	19.85	99.2	99.2		
150 %	10	15	25	24.64	24.64	98.5	98.5	1.466	1.466
				25.37	25.37	101.5	101.5		
				24.98	24.97	99.9	99.9		

Table V: Accuracy data of EZT by PCR and PLS models.

LEVEL %	Sample Conc. µg/ml	Amount added µg/ml	Total Conc. µg/ml	PREDICTED CONC. µg/ml		% Recovery		% RSD	
				PCR	PLS	PCR	PLS	PCR	PLS
50 %	10	5	15	14.912	14.919	99.4	99.4	0.651	0.563
				15.093	15.080	100.6	100.5		
				14.939	14.954	99.5	99.6		
100 %	10	10	20	20.285	20.297	101.4	101.4	0.557	0.558
				20.281	20.292	101.4	101.4		
				20.088	20.099	100.4	100.4		
150 %	10	15	25	24.824	24.839	99.2	99.3	0.433	0.433
				25.020	25.035	100.0	100.1		
				24.843	24.858	99.3	99.4		

Table VI: Precision results obtained using developed PCR and PLS models (Intraday Precision)

Amount taken µg/ml		Predicted Conc. µg/ml				% Recovery				% RSD			
ATV	EZT	PCR		PLS		PCR		PLS		PCR		PLS	
		ATV	EZT	ATV	EZT	ATV	EZT	ATV	EZT	ATV	EZT	ATV	EZT
10	10	9.99	9.93	9.99	9.91	99.9	99.3	99.9	99.1	1.504	1.568	1.500	1.574
10	10	10.04	10.23	10.04	10.21	100.4	102.3	100.4	102.1				
10	10	10.27	10.16	10.27	10.15	102.7	101.6	102.7	101.5				
15	15	14.78	14.87	14.76	14.87	98.4	99.19	98.4	99.1	1.326	1.381	1.324	1.389
15	15	14.86	14.99	14.86	14.99	99.1	99.9	99.1	99.9				
15	15	15.14	15.27	15.14	15.28	100.9	101.8	100.9	101.8				
20	20	20.26	20.22	20.26	20.23	101.3	101.1	101.3	101.1	1.145	1.122	1.144	1.121
20	20	19.84	19.94	19.84	19.94	99.2	99.7	99.2	99.7				
20	20	19.88	19.78	19.88	19.78	99.4	98.9	99.4	98.9				

Table VII: Precision results obtained using developed PCR and PLS models (Interday Precision)

Amount Taken µg/ml		Predicted Conc. µg/ml				% Recovery				% RSD			
ATV	EZT	PCR		PLS		PCR		PLS		PCR		PLS	
		ATV	EZT	ATV	EZT	ATV	EZT	ATV	EZT	ATV	EZT	ATV	EZT
10	10	10.01	10.04	10.00	10.03	100.1	100.4	100.0	100.3	1.614	1.245	1.616	1.242
10	10	10.29	10.25	10.28	10.25	102.9	102.5	102.8	102.5				
10	10	10.30	10.26	10.29	10.26	103.0	102.6	102.9	102.6				
15	15	15.58	15.33	15.57	15.32	103.9	102.2	103.8	102.1	1.123	0.881	1.124	0.881
15	15	15.91	15.58	15.90	15.57	106.0	103.8	106.0	103.8				
15	15	15.87	15.55	15.86	15.54	105.8	103.6	105.7	103.6				
20	20	21.22	20.66	21.21	20.65	106.1	103.3	106.0	103.2	0.355	0.281	0.355	0.281
20	20	21.36	20.77	21.35	20.76	106.8	103.8	106.7	103.8				
20	20	21.33	20.75	21.32	20.74	106.6	103.7	106.6	103.7				

RESULTS AND DISCUSSION

Out of 36 mixtures, 28 set of mixtures were used for calibration and 08 set of mixtures were used for validation. The models were tried to develop with varying $\Delta \lambda$. The best results were obtained with the wavelengths intervals $\lambda = 0.5$ nm in methanol. The developed method found to be accurate as results are close to 100 % and precise with % RSD less than 2. Summary of results is presented in Table VIII. The limitations of the reported method [16] found to narrower range (8-14 $\mu\text{g/ml}$), less accuracy (94.1 - 108.9 %) and large scanning range (210-300 nm) as compare our developed methods.

CONCLUSION

A study of the use of UV spectrophotometric in combination with PLS and PCR for the simultaneous determination of Atorvastatin calcium (ATV) and Ezetimibe (EZT) in a binary mixture has been accomplished. The results obtained confirmed the suitability of the proposed method for simple, accurate and precise analysis of ATV and EZT in pharmaceutical preparations. The proposed methods do not need separation of ATV and EZT before analysis. In addition, the proposed methods can be applied for analysis of drugs in quality control lab as well as for in process quality control.

Table VIII: Summary of results

Parameters	Atorvastatin calcium (ATV)		Ezetimibe (EZT)	
	PCR	PLS	PCR	PLS
Range ($\mu\text{g/ml}$)	5.0-30.0	5.0-30.0	5.0-30.0	5.0-30.0
Wavelength, nm	230- 260	230- 260	230- 260	230- 260
Data interval , $\Delta\lambda$	0.5	0.5	0.5	0.5
Factors/ PC's	2	2	2	2
% Recovery	99.3	99.3	99.5	99.6
LOD	0.53	0.53	0.18	0.18
LOQ	1.61	1.61	0.57	0.57
Correlation Coefficient (r^2)	0.9968	0.9968	0.9922	0.9922
Intercept	0.0564	0.0563	0.1415	0.1415
Slope	0.9968	0.9968	0.9922	0.9922
RMSECV	0.42649	0.48623	0.7097	0.7089
RMSEP	0.4864	0.4862	0.7089	0.7089

ACKNOWLEDGMENT

Authors are thankful to the Principal, AISSMS college of Pharmacy for providing necessary facilities to carry out the experiment. Authors are also thankful to Wockhardt Research Centre, Aurangabad for providing a Reference standard of Atorvastatin calcium and Ezetimibe.

REFERENCES

- [1] Salt/ester/formulation Atorvastatin Calcium for DB01076 (Atorvastatin): <https://www.drugbank.ca/salts/DBSALT000011> cited 21st December 2016.
- [2] The Indian Pharmacopoeia. Vol. I, 1099-1100, (2014)
- [3] Ezetimibe for DB00973: <https://www.drugbank.ca/drugs/DB00973> cited 21st December 2016
- [4] The Indian Pharmacopoeia. Vol. I, 1727-1728, (2014)
- [5] Baldha R, Patel V and Bapna M. Simultaneous Spectrophotometric Determination of Atorvastatin Calcium and Ezetimibe in Tablet Dosage Form. *International Journal of ChemTech Research*, **1**(2), 233-236 (2009)
- [6] Kumar P, Ghosh A and Chaudhary M. Stability Indicating Method Development for Simultaneous Estimation of Ezetimibe and Atorvastatin in Pharmaceutical Formulations by RP-HPLC. *Pharmaceut Anal Acta*, **3**(6), 1-6 (2012)
- [7] Kumar S A, Debnath M, Seshagiri Rao JV and Sankar G D. Stability indicating RP-HPLC analytical method development and Validation for simultaneous estimation of Atorvastatin and Ezetimibe in bulk as well in pharmaceutical dosages form by using PDA detector. *Scholar Research Library*, **6**(5), 37-55, (2014)
- [8] V Rajamanickam, Rajasekaran, Stephen Rathinaraj and K Anandarajagopal. Development and Validation of Analytical Methods for Simultaneous Estimation of Atorvastatin Calcium and Ezetimibe in Combined Dosage Form. *World Applied Sciences Journal*, **9**(12), 1424-1429, (2010)
- [9] Kumar S A, Debnath M, Seshagiri Rao JV. New Validated RP – HPLC Analytical Method for Simultaneous Estimation of Atorvastatin and Ezetimibe in

- Bulk Samples as well in Tablet Dosage Forms by Using PDA Detector. *Bentham Sciences*, **11**(4), 259-70, (2014)
- [10] Miriam F A and N Magdy. Application of New Spectrofluometric Determination Techniques for Determination of Atorvastatin and Ezetimibe Combined Tablet Dosage Form. *Chem. Pharm. Bull.*, **63**(6), 443-449, (2015)
- [11] Dhaneshwar S S, Dhaneshwar S R, Deshpande P, and Patil M. Development and Validation of a Method for Simultaneous Densitometric Estimation of Atorvastatin Calcium and Ezetimibe as the Bulk Drug and in Tablet Dosage Forms. *Acta Chromatographica*, **19**, 141-148, (2007)
- [12] Sonawane S S, Shirkhedkar A A, Fursule R A, Surana S J. Application of UV-Spectrophotometry and RP-HPLC for Simultaneous Determination of Atorvastatin Calcium and Ezetimibe in Pharmaceutical Dosage Form. *Eurasian Journal of Analytical Chemistry*, **1**(1), 32-41, (2006)
- [13] Saroj Kumar Raul, Atna Bhaskar Aravelli, Durgasi Jhansi. RP-Hplc Method Development and Validation for the Simultaneous Estimation of Atorvastatin and Ezetimibe in Pharmaceutical Dosage Form. *Asian J Pharm Clin Res*, **8**, 178-181, (2015)
- [14] Kumar S A, Debnath M, Seshagiri Rao JV and Sankar G D. New Validated Stability-Indicating RP-HPLC Method for Simultaneous Estimation of Atorvastatin and Ezetimibe in Human Plasma by Using PDA Detector. *Advanced Pharmaceutical Bulletin*, **5**(3), 385-391, (2015)
- [15] Dinc E, Baleanu D. Spectrophotometric quantitative determination of cilazapril and hydrochlorothiazide in tablets by chemometric methods. *Journal of Pharmaceutical and Biomedical Analysis*, **30**, 715-723, (2002)
- [16] Azin Jahangiri, Khosro Adibkia, Karim Asadpour-Zeynali, Yousef Javadzadeh, Hamed Hamishehkar, Mohammad Barzegar-Jalali. Application of Multivariate Calibration Methods, in Dissolution Testing and Simultaneous Determination of Atorvastatin and Ezetimibe in Their Combined Solid Dosage Form. *Pharmaceutical Sciences*, **22**, 105-111, (2016)
- [17] Bhaskar R, Sagar M, Saini V, Bhat M. UV-spectrophotometric-assisted chemometric methods for the simultaneous determination of metformin hydrochloride and gliclazide in pharmaceutical formulations. *Pharmaceut Anal Acta*, **3**, 1-5, (2012)
- [18] International Conference on Harmonization. ICH harmonized tripartite guideline validation of analytical procedures text and methodology Q2 (R1) ICH, Geneva, 1-17, (2005)