

Barrow Neurological Institute at St. Joseph's Hospital and Medical Center

Barrow - St. Joseph's Scholarly Commons

Neurosurgery

12-1-2019

A Biomechanical Evaluation of a Next-Generation Integrated and Modular ACDF Device Possessing Full-Plate, Half-Plate, and No-Profile Fixation Iterations.

Ripul Panchal

Anup Gandhi

Chris Ferry

Sam Farmer

Jeremy Hansmann

See next page for additional authors

Follow this and additional works at: <https://scholar.barrowneuro.org/neurosurgery>

Authors

Ripul Panchal, Anup Gandhi, Chris Ferry, Sam Farmer, Jeremy Hansmann, and John E Wanebo

A Biomechanical Evaluation of a Next-Generation Integrated and Modular ACDF Device Possessing Full-Plate, Half-Plate, and No-Profile Fixation Iterations

Ripul Panchal, DO, FACOS, FACS¹, Anup Gandhi, PhD²,
Chris Ferry, MS³ , Sam Farmer, BS², Jeremy Hansmann, BS²,
and John Wanebo, MD, FAANS⁴

Global Spine Journal
2019, Vol. 9(8) 826-833
© The Author(s) 2019
Article reuse guidelines:
sagepub.com/journals-permissions
DOI: 10.1177/2192568219834252
journals.sagepub.com/home/gsj



Abstract

Study Design: In vitro biomechanical study.

Objectives: The objective of this in vitro biomechanical range-of-motion (ROM) study was to evaluate spinal segmental stability following fixation with a novel anterior cervical discectomy and fusion (ACDF) device (“novel device”) that possesses integrated and modular no-profile, half-plate, and full-plate fixation capabilities.

Methods: Human cadaveric (n = 18, C3-T1) specimens were divided into 3 groups (n = 6/group). Each group would receive one novel device iteration. Specimen terminal ends were potted. Each specimen was first tested in an intact state, followed by anterior discectomy (C5/C6) and iterative instrumentation. Testing order: (1) novel device (group 1, no-profile; group 2, half-plate; group 3, full-plate); (2) novel device (all groups) with lateral mass screws (LMS); (3) traditional ACDF plate + cage; (4) traditional ACDF plate + cage + LMS. A 2 N·m moment was applied in flexion/extension (FE), lateral bending (LB), and axial rotation (AR) via a kinematic testing machine. Segmental ROM was tracked and normalized to intact conditions. Comparative statistical analyses were performed.

Results: Key findings: (1) the novel half- and full-plate constructs provided comparable reduction in FE and LB ROM to that of traditional plated ACDF ($P \geq .05$); (2) the novel full-plate construct significantly exceeded all other anterior-only constructs ($P \leq .05$) in AR ROM reduction; and (3) the novel half-plate construct significantly exceeded the no-profile construct in FE ($P < .05$).

Conclusions: The novel ACDF device may be a versatile alternative to traditional no-profile and independent plating techniques, as it provides comparable ROM reduction in all principle motion directions, across all device iterations.

Keywords

cervical, ACDF, degenerative disc disease, biomechanics, anterior cervical discectomy and fusion, modular, integrated, zero-profile, standalone, range-of-motion

Introduction

Anterior cervical discectomy and fusion (ACDF) is a common surgical technique in treating symptomatic disc degeneration, segmental instability, and trauma of the cervical spine. Characterized by acute segmental motion reduction, ACDF has demonstrated robust fusion capabilities and subsequent clinical improvement.^{1,2} While the placement of an intervertebral graft alone aides in anterior fusion by stretching the annulus, breach of the anterior and posterior longitudinal ligaments diminishes

¹ American Neurospine Institute, Plano, TX, USA

² Zimmer Biomet Spine Research & Development, Westminster, CO, USA

³ Cooper Medical School of Rowan University, Camden, NJ, USA

⁴ Barrow Brain and Spine, Scottsdale, AZ, USA

Corresponding Author:

Chris Ferry, Cooper Medical School of Rowan University, 401 Broadway, Camden, NJ 08103, USA.
Email: ferryc2@rowan.edu





Figure 1. Modular anterior cervical discectomy and fusion (ACDF) construct with integrated fixation: no-profile (left), half-plate (middle), full-plate (right).

stability in flexion and extension. Accordingly, an anterior cervical plate is readily used in ACDF and has been documented to further improve sagittal stability and rate of fusion.^{3,4} However, both surgical exposure and plate profile/footprint have been shown to play a role in subsequent adjacent soft tissue injury (dysphagia and dysphasia) and contiguous level pathology (heterotopic ossification).⁵⁻⁷

Consequently, the ACDF paradigm has seen a considerable shift toward techniques possessing a decreased access window and a minimal anterior device footprint/profile. Next-generation short stature plates and integrated “low-profile” or “no-profile” anchored devices have emerged.⁸⁻¹¹ While a number of biomechanical studies have documented good mechanical stability with such devices, the majority have suggested that the integrated design provides less stability in flexion and extension than traditional cage and plate constructs.¹⁰⁻¹⁷ Moreover, when considering the limitations of instrument angulation, presence of adjacent and/or previous hardware, and the degree of sagittal correction desired, it remains apparent that a “one size fits all” approach to ACDF is not possible.

More recently, a novel ACDF construct capable of both integrated screw and modular plate fixation (MPF) was developed to provide greater device versatility beyond the current spectrum of ACDF constructs (Figures 1 and 2). The device

supports in situ transitioning between no-profile, half-plate, and full-plate fixation. This provides a more comprehensive ACDF strategy that may better accommodate pathological and anatomical variables on a patient-specific level. Furthermore, the connected MPF design, which creates a singular and continuous body about the index level, facilitates optimal plate orientation/alignment, significantly diminishes potential for cage migration and/or subsidence, and promotes physiological compression of the cage/graft.

While these features present with an array of perceived biomechanical, ergonomic, and clinical benefits, no data exists yet in the literature. The objective of this study was to assess the segmental stability achieved with the novel ACDF (“novel”) construct, across all iterations, utilizing traditional plated ACDF and anteroposterior cervical fusion constructs as controls.

Materials and Methods

Specimen Preparation and Instrumentation Technique

Eighteen ($n = 18$) fresh-frozen human cadaveric spine specimens (C3-T1) were tested (7 females, 11 males; mean age 59.1 ± 11.1 years). Each spine was thawed at room temperature, the cervicothoracic specimens were resected, the ligamentous structures were maintained, and the residual musculature and adipose tissue was removed. Structural integrity was confirmed via standard anteroposterior and lateral radiographs. Any specimens exhibiting previous surgery or anatomical discrepancy were excluded. Bone mineral density (BMD) evaluations were performed by dual-energy X-ray absorptiometry (DEXA) scans. The terminal ends of each specimen were potted for test apparatus attachment using standard wood screws placed in the vertebral bodies and anchored within high-strength resin (Bondo Body Filler; 3M, St Paul, MN, USA). The potted specimens were sealed in plastic bags and maintained frozen



Figure 2. Anatomical renderings of modular anterior cervical discectomy and fusion (ACDF) construct with integrated fixation: no-profile (left), half-plate (middle), full-plate (right).

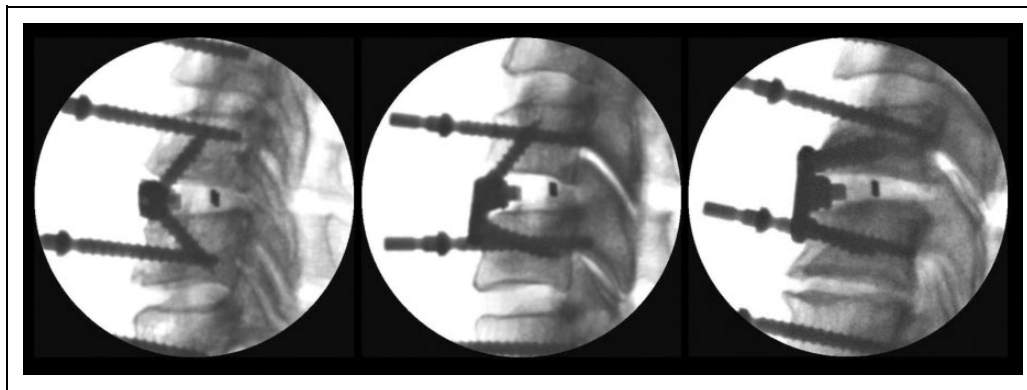


Figure 3. Lateral fluoroscopic images of modular anterior cervical discectomy and fusion (ACDF) construct with integrated fixation, taken prior to range-of-motion (ROM) testing: no-profile (left), half-plate (middle), full-plate (right).

Table 1. Summary of Implant Sizes Used.

Implant Type	Interbody Size Height × Width × Length (mm × mm × mm)	Plate Height (mm)	Number of Screws	Screw Diameter (mm)	Screw Length (mm)
Integrated modular device	6-7 × 12-13 × 14-15	Matched to Interbody Height (6-7)	2 3 4	3.5	14-16
Cervical interbody cage	6-7 × 12-13 × 14-15	—	0	—	—
Anterior cervical plate	—	12-13	4	4	14
Lateral mass screws	—	—	4	3.5, 4	12, 14, 16

at -20°C until approximately 10 hours before testing, at which time they were thawed at room temperature ($\sim 25^{\circ}\text{C}$).

Specimens were divided into 3 groups such that the mean BMD values for each group were comparable. The 3-group protocol was used such that each specimen group received a single iteration of the novel ACDF device (full-plate, $n = 6$; half-plate, $n = 6$; or no-profile, $n = 6$) (Alta ACDF System; Zimmer Biomet Spine, Westminister, CO, USA) in addition to the traditional (control) plate (MaxAn Anterior Cervical Plate System; Zimmer Biomet Spine, Westminister, CO, USA) and cage (C-THRU Anterior Spinal System; Zimmer Biomet Spine, Westminister, CO, USA) construct. It should be noted that the novel ACDF device is a commercially available (non-prototype) ACDF device, approved by the US Food and Drug Administration for indication as a stand-alone cervical fusion device in skeletally mature patients with degenerative disc disease of the cervical spine (C3-T1) at one level. Additionally, in all 3 modular iterations, the device is composed of a PEEK-OPTIMA LT1 (Invivo Inc, West Conshohocken, PA, USA) intervertebral spacer, with titanium plate and screws (Figures 1 and 2).

Separate grouping allowed for greater bone preservation during iterative testing, as single specimen instrumentation with all 3 modular device conditions would greatly compromise bone quality for each subsequent construct. Mean BMD values for each group were as follows: group 1 (novel no-profile), $0.79 \pm 0.14 \text{ g/cm}^2$; group 2 (novel half-plate),

$0.73 \pm 0.11 \text{ g/cm}^2$; and group 3 (novel full-plate), $0.75 \pm 0.15 \text{ g/cm}^2$; respectively. Mean T -score values for each group were as follows: group 1, -1.92 ± 1.05 ; group 2, -2.43 ± 0.62 ; and group 3, -2.40 ± 1.81 , respectively. No significant differences in bone quality existed between groups. Prior to device instrumentation and testing, marker screws to hold optoelectronic triad markers were affixed to each rigid vertebral body (C3-T1), and marker screw placement was performed such that construct screw trajectories would be uninhibited.

All procedures and instrumentation were performed under fluoroscopic guidance by a board certified, fellowship-trained, spine surgeon in a clinically representative manor (Figure 3A-C; Table 1). Lateral mass screws (LMS) were placed bilaterally (Lineum OCT Spine System; Zimmer Biomet Spine, Westminister, CO, USA) (screw diameters, 3.5, 4 mm; screw lengths, 12, 14, 16 mm). Range of interbody cage (all iterations) height, width, and length were 6-7 mm, 12-13 mm, and 14-15 mm, respectively, and the size of the corresponding modular plate was matched to that of the interbody cage. Traditional anterior plates were either 12 or 13 mm in height and received 4.0 mm (diameter) by 14 mm (length) screws. All novel device iterations received 3.5 mm (diameter) by 14 or 16 mm (length) screws. All novel device half-plate constructs were placed with the plate oriented caudally. It is emphasized that the half-plate construct can be oriented cranially or caudally, however, for sake of consistency, only the caudal orientation was chosen in

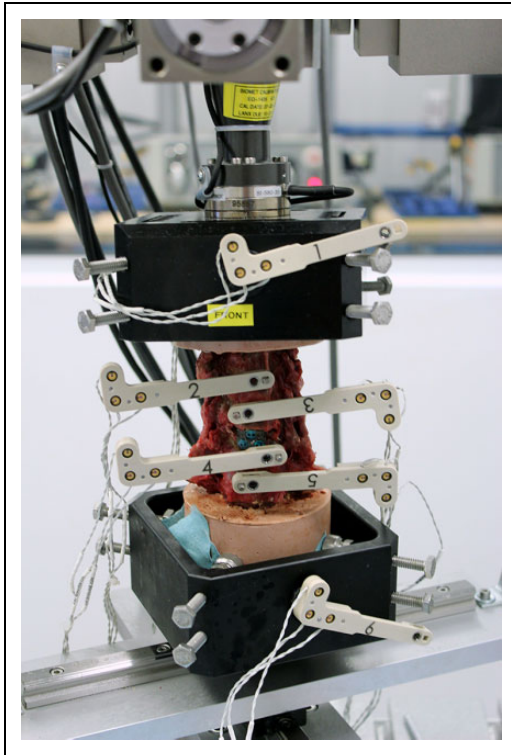


Figure 4. Potted C3-T1 specimen affixed with optical markers within the kinematic testing system (Bionix Spine Kinematics System, MTS Corporation, Eden Prairie, MN, USA).

the present study. This rationale was based on evidence showing a greater risk for adjacent level ossification at the cranial level when using a traditional plate.^{5,18} Furthermore, given the inherent lordosis of the cervical spine, less bony work is necessary to position a plate over the caudal body.

Testing and Motion Analysis Protocol

A 6 degree-of-freedom (6-DOF) kinematic testing machine (Bionix Spine Kinematics System, MTS Corporation, Eden Prairie, MN, USA) was used to apply nonconstraining, non-destructive, pure-moment loading in the 3 principal motion directions. Specimens were affixed with optoelectronic markers and mounted within the test apparatus at the C3 and T1 pots (Figure 4). The caudal pot attachment afforded translation in the *X-Y* plane via a translating table. A maximum loading moment of ± 2.0 N·m was applied in flexion/extension (FE), left/right lateral bending (LB), and axial rotation (AR) at a rate of 1 deg/s for 3 cycles. Each specimen was subjected to pure moment loading; first in its native intact condition, then following a C5/6 anterior discectomy and iterative C5/6 fixation. The testing sequence across groups is summarized in Figure 5. The authors do acknowledge that a randomized testing sequence was not used. However, while randomizing or alternating the order of fixation was appealing, the benefit of always placing the novel device first allowed for the same interbody cage to be used in subsequent fixation (traditional plate)

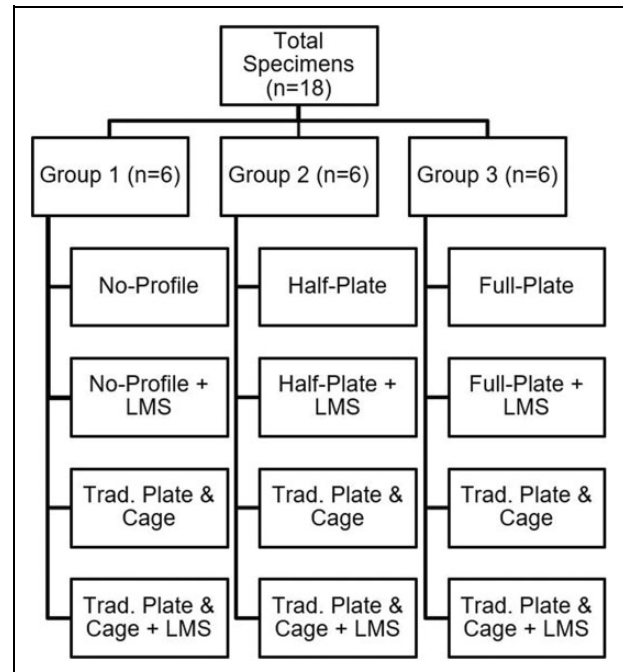


Figure 5. Specimen distribution and testing order. LMS = lateral mass screws

without additional cage manipulation and risk of segmental compromise. Furthermore, the authors believe that the good quality of specimen bone, as well as a small loading moment, minimized the risk of segment compromise and bias during subsequent testing. Specimens were covered in saline-soaked gauze in between testing periods. The authors acknowledge that a compressive follower load was not used; this was done to assess device performance within a “worst-case” environment, as described by Patwardhan et al.¹⁹ Furthermore, as demonstrated by Dreischarf et al,²⁰ nonoptimized follower load paths and poorly defined starting conditions can diminish the comparability of studies and make drawing conclusions more challenging.

Three-dimensional motion of each vertebral body was recorded, in all cycles, relative to their adjacent caudal level (C3-C4, C4-C5, C5-C6, C6-C7, C7-T1), as well as the 3-dimensional motion of the cumulative specimen (C3-T1) using an optoelectronic motion measurement system (Optotrak Certus Motion Capture System; Northern Digital Inc, Waterloo, Ontario, Canada). Each optoelectronic triad maker was coupled to its respective level to establish a local coordinate system. Additionally, two optoelectronic markers were rigidly attached to the static test frame to define the *+X* and *+Y* axes, and subsequently the *+Z* axis. Data acquired during the third test cycle was used for statistical analyses, as recommended by Wilke et al.²¹ ROM reduction relative to intact conditions was subsequently determined.

Statistical Analysis

Intact data outcomes for each ROM within each group were compared using 3 one-way analyses of variance. The natural

Table 2. Summary of Mean Range-of-Motion (ROM) Outcomes.^a

Construct	ROM as % Intact Condition		
	FE	LB	AR
No-profile	69 ± 39	48 ± 14	76 ± 19
Half-plate	42 ± 34	25 ± 14	67 ± 26
Full-plate	32 ± 26	29 ± 12	40 ± 15
Traditional plate and cage	37 ± 26	39 ± 18	61 ± 20
No-profile + LMS	14 ± 6	13 ± 6	31 ± 11
Half-plate + LMS	18 ± 15	10 ± 6	31 ± 19
Full-plate + LMS	12 ± 10	10 ± 3	16 ± 4
Traditional plate and cage + LMS	12 ± 7	11 ± 7	22 ± 11

Abbreviations: AR, axial rotation; FE, flexion/extension; LB, lateral bending; LMS, lateral mass screws.

^a All data represent the mean ± standard deviation (%).

log of the ROM outcome data was taken to force a normal distribution within the data sets. Next, a linear mixed model framework was used to model the natural log of each ROM outcome (flexion-extension, lateral bending, and axial rotation) as a function of the 9 interventions, using intact ROM as a reference category. A random intercept was included in the model to account for correlation due to multiple measurements taken on each sample. All pairwise comparisons of the change from the intact state were made between the interventions. To maintain a .05 type 1 error rate, a Bonferroni correction was made to the *P* values for each model.

Ethics Approval

No medical ethics committee approval or institutional review board was required for this cadaveric study. All specimens were obtained from an accredited tissue bank service (Science Care, Inc, Phoenix, AZ, USA). All donors and the next of kin were fully legally competent and consented to use for research. Written informed consent from the donor or the next of kin was obtained.

Results

Mean ROM outcomes are summarized in Table 2, and in Figures 6, 7, and 8, respectively. No significant differences existed within a ROM outcome and between groups for the intact data sets ($P \leq .05$). Therefore, ROM outcomes from each group were combined and analyzed via linear mixed models to draw conclusions regarding the effects of the plate profile on segmental ROM.

Flexion/Extension

All plated constructs (+/- LMS) achieved significance reduction in ROM over the novel no-profile device ($P \leq .05$). No significant reduction in ROM were observed between the novel half-, full-plate, and traditional plated constructs ($P \geq .05$). No significant differences existed between circumferential constructs (+LMS, $P \geq .05$), but ROM reduction of the novel

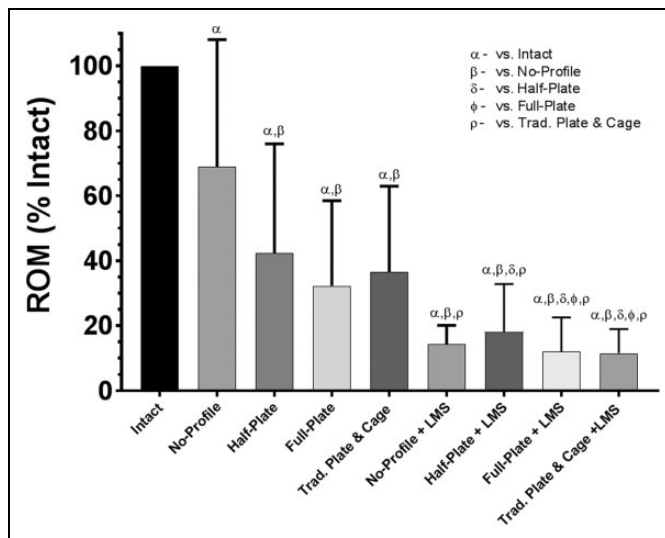


Figure 6. Range of motion (ROM), relative to intact conditions, when loaded in flexion-extension under a pure moment of ± 2.0 Ncm. Bars represent the mean and error bars are standard deviation. Symbols denote significant differences between groups according to a repeated-measures analysis of variance with Bonferroni's correction for multiple comparisons.

full-plate +LMS and traditional plate + LMS significantly exceeded those of anterior-only constructs ($P \leq .05$).

Lateral Bending

Anterior-only constructs significantly reduced ROM from that of intact ($P \leq .05$), and no significant differences were observed between anterior-only constructs ($P \geq .05$). All circumferential (+LMS) constructs significantly exceeded the anterior-only constructs ($P \leq .05$). No significant differences were observed between circumferential (+LMS) constructs ($P \geq .05$).

Axial Rotation

No significant differences in ROM reduction were observed between the novel no-profile, half-plate, or traditional plate constructs ($P \geq .05$); however, the novel full-plate construct significantly exceeded all other anterior-only constructs ($P \leq .05$). All circumferential constructs exceeded the anterior-only constructs ($P \leq .05$) except for the novel full-plate when compared to the novel no-profile + LMS and novel half-plate + LMS constructs ($P \geq .05$).

Discussion

The present biomechanical study assessed a novel integrated and modular ("novel") ACDF device, possessing multiple face-plate fixation options (no-profile, half-plate, and full-plate), using a traditional ACDF (plate + cage) as a control. While integrated fixation features have become prevalent in ACDF, no device has been studied in which multiple face-plate

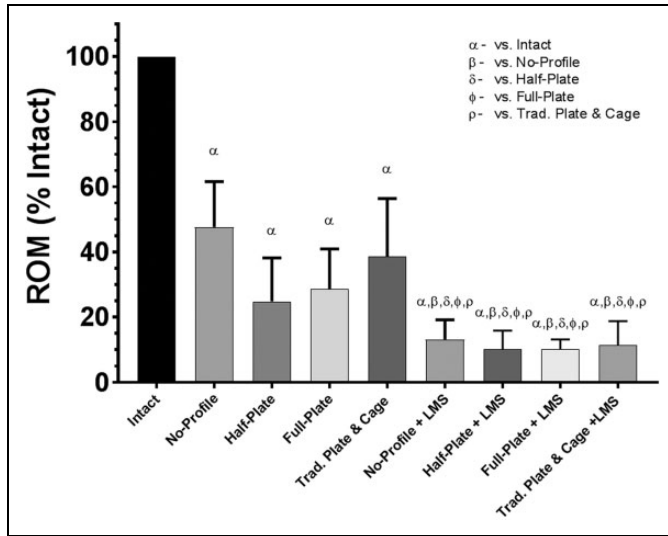


Figure 7. Range of motion (ROM), relative to intact conditions, when loaded in lateral bending under a pure moment of ± 2.0 Ncm. Bars represent the mean and error bars are standard deviation. Symbols denote significant differences between groups according to a repeated-measures analysis of variance with Bonferonni's correction for multiple comparisons.

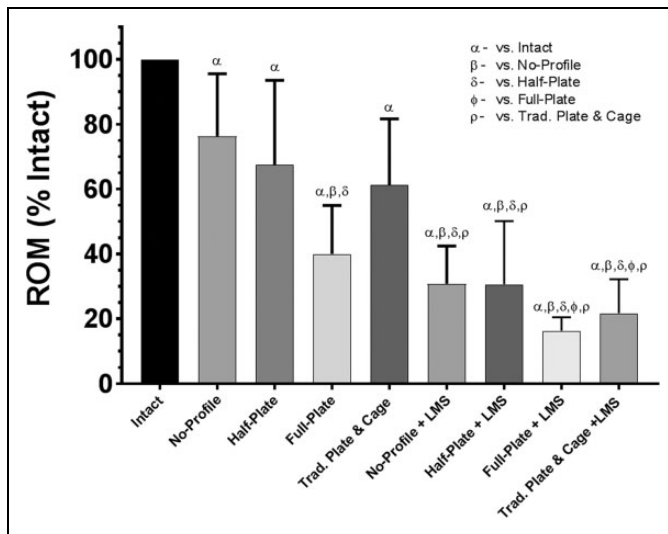


Figure 8. Range of motion (ROM), relative to intact conditions, when loaded in axial rotation under a pure moment of ± 2.0 Ncm. Bars represent the mean and error bars are standard deviation. Symbols denote significant differences between groups according to a repeated measures analysis of variance with Bonferonni's correction for multiple comparisons.

fixation mechanisms can be leveraged and further adapted in situ.^{9-13,15-17,22-24} It was postulated that such a design may improve the ease and safety of implantation, while also improving mechanical stability.

Pertaining to the latter, the current study found that the novel full-plate construct provided comparable stability to traditional plated ACDF in all motion planes, reaching significance in AR ($P < .05$). While the comparable stability of the novel full-plate

construct is not insignificant, it has already been well substantiated in the literature that traditional plated ACDF supports robust fusion outcomes, with single-level fusion rates as high as 97.1%.^{1,2} Furthermore, while the ROM values of the novel full-plate device (FE, $32\% \pm 26\%$; LB, $29\% \pm 12\%$; AR, $40\% \pm 15\%$) trend comparably within the context of historical biomechanical data for ACDF plate and cage constructs, they are not markedly different. Majid et al²⁵ reported approximate mean ROM values for a traditional ACDF plate and cage of 50%/25% (F/E), 29.1% (LB), and 43.2% (AR), respectively. Similarly, Stein et al,²⁶ also assessing biomechanical stability of a traditional ACDF plate and cage construct, reported approximate mean ROM values of 36%/40% (F/E), 33% (LB), and 41% (AR), respectively.

However, the comparable stability of the novel full-plate construct, considered in the context of a consolidated insertion/implantation technique and streamlined cage/plate orientation, may still be of unique clinically utility. Given that emerging evidence suggests that both retraction time and end-stage sagittal alignment play a role in subsequent pathology following ACDF, future clinical assessment of potential ergonomic and biomechanical benefits resultant from the integrated half-plate design is warranted.²⁷⁻²⁹

The novel half-plate construct may also help in avoiding the limitations introduced by preexisting adjacent level instrumentation. Means to achieving secondary adjacent level instrumentation have traditionally involved the removal, replacement and/or extension of the existing plate, use of axillary posterior instrumentation, and/or selection of a no-profile construct. These techniques often require additional and/or lengthier surgical interventions, leading to longer operative time and possibly compromising segmental stability. In the current study, the novel half-plate construct supported lower mean ROM (greater reduction) in comparison to the no-profile construct in all principle directions (FE ROM, $42\% \pm 34\%$ vs $69\% \pm 39\%$; LB, $25\% \pm 14\%$ vs $48\% \pm 14\%$; AR $67\% \pm 26\%$ vs $76\% \pm 19\%$), achieving significance in FE. However, it should be noted that the no-profile construct in the current study possessed 2 screws, while many commercially available no-profile/zero-profile devices often possess 3 or 4 screws. Scholz et al,¹⁰ assessing a 4-screw no-profile ACDF device, found that device ROM reduction was comparable to that of traditional ACDF plate and cage constructs ($P \geq .325$). Similarly, Stein et al,²⁶ assessing a 3-screw no-profile ACDF device, reported no significant differences in ROM reduction in comparison with a traditional ACDF plate and cage ($P \geq .90$). Majid et al,²⁵ evaluating both 2-screw and 3-screw no-profile constructs, found that neither construct demonstrated significantly different ROM reductions in comparison with each other, or a traditional ACDF cage and plate construct. Collectively, these historical data suggest that no-profile devices, despite variation in number of screws, typically support ROM reduction comparable to that of a traditional ACDF plate and cage construct. While the significant difference observed in the current study between the novel no-profile and half-plate constructs in FE appears as an advantageous anomaly, additional evaluation is

needed to determine how the half-plate design compares against no-profile/zero-profile devices with greater points of screw fixation.

Moreover, when used in a primary index procedure, the comparable stability of the novel half-plate construct (vs no-profile) may be of value in the high and low cervical segments when the mandible and sternum/clavicle can obstruct high-angled screw instrumentation. Additionally, given its comparable stability to traditional/full-plate constructs, the novel half-plate construct may be an effective alternative when preservation of cranial vertebral face is desired, avoiding a potential etiology for adjacent level ossification.^{5,19,28}

Finally, while the outcomes demonstrated by the novel no-profile construct appear of less novelty than those of the half- and full-plate constructs, the no-profile technology remains a powerful option within ACDF. As previously noted, the continued development of no- or low-profile anchored cages has been fueled by the desire to simplify surgical technique and reduce implant prominence.⁸⁻¹⁰ While biomechanical studies have demonstrated that the stability of no-profile constructs may be comparable to traditional plated ACDF, diminished stability is still typically observed in flexion and extension.^{10-14,22,24} Outcomes of the current study are consistent with this trend, as the novel no-profile construct was markedly less stable in flexion/extension. However, despite these biomechanical discrepancies with no-profile devices, several clinical studies have demonstrated excellent efficacy with the technology.^{12,15-17,22,23} These findings further support the assertion that ACDF is far from a “one size fits all” technique and that more versatile technologies, and subsequent characterization, is needed to support this paradigm and delineate standards of care.

The authors acknowledge several limitations in this study that are consistent with those previously reported in the literature.^{10-14,22,24} Limitations include use of cadaveric specimens, use of a non-diseased state model, no accounting for fatigue behavior, and no accounting for the presence of bony fusion. Given the already intrinsic variability across specimens, further introduction of anatomical and/or biomechanical variables can result in significant irregularities. Accordingly, the aforementioned design parameters were deemed confounding for the purpose of the present evaluation. An additional study limitation is that of the no-profile device design, which leveraged 2-point screw fixation. No-profile ACDF devices possessing 3- or 4-point screw fixation are commercially available, which can have implications on the amount of segmental stability afforded by this technique. The authors emphasize that the novelty of the data presented here pertains primarily to the performance of the integrated half- and full-plate iterations in comparison to traditional plate ACDF, irrespective of the no-profile iteration.

Conclusion

Use of an integrated and modular ACDF device, particularly in half- and full-plate fixation, can provide comparable ROM reduction to that of a traditional ACDF plate and cage. Given

this finding, future clinical evaluation is warranted to better understand device design implications on perioperative and patient outcomes.

Acknowledgments

The authors would like thank Amy Claeson, PhD, and Vijay Permeswaran, PhD for their help in editing the article.


Declaration of Conflicting Interests

The author(s) declared the following potential conflicts of interest with respect to the research, authorship, and/or publication of this article: Anup Gandhi, Sam Farmer, and Jeremy Hansmann are employees (salary) of the funding source. Ripul Panchal and John Wanebo have received consulting fees (hourly) from the funding source. John Wanebo is a design surgeon (royalty bearing) of the device examined in this study (Alta ACDF System).

Funding

The author(s) disclosed receipt of the following financial support for the research, authorship, and/or publication of this article: This study was funded by Zimmer Biomet Spine.

ORCID iD

Chris Ferry, MS  <https://orcid.org/0000-0002-5594-088X>

References

- Fraser JF, Härtl R. Anterior approaches to fusion of the cervical spine: a metaanalysis of fusion rates. *J Neurosurg Spine*. 2007;6:298-303.
- Kaiser MG, Haid RW Jr, Subach BR, Barnes B, Rodts GE Jr. Anterior cervical plating enhances arthrodesis after cervical discectomy and fusion with cortical allograft. *Neurosurgery*. 2002;50:229-238.
- Wang JC, McDonough PW, Endow KK, Delamarter RB. Increased fusion rates with cervical plating for two-level anterior cervical discectomy and fusion. *Spine (Phila Pa 1976)*. 2000;25:41-45.
- Wang JC, McDonough PW, Kanim LE, Endow KK, Delamarter RB. Increased fusion rates with cervical plating for three-level anterior cervical discectomy and fusion. *Spine (Phila Pa 1976)*. 2001;26:643-647.
- Park JB, Watthanaaphisit T, Riew KD. Timing of development of adjacent-level ossification after anterior cervical arthrodesis with plates. *Spine J*. 2007;7:633-636.
- Sahjpaul RL. Esophageal perforation from anterior cervical screw migration. *Surg Neurol*. 2007;68:205-210.
- Xiao S, Liang Z, Wei W, Ning J. Zero-profile anchored cage reduces risk of postoperative dysphagia compared with cage with plate fixation after anterior cervical discectomy and fusion. *Eur Spine J*. 2017;26:975-984.
- Chen F, He W, Mahaney K, et al. Alternative grafts in anterior cervical fusion. *Clin Neurol Neurosurg*. 2013;115:2049-2055.
- Chong E, Pelletier MH, Mobbs RJ, Walsh WR. The design evolution of interbody cages in anterior cervical discectomy and fusion: a systematic review. *BMC Musculoskelet Disord*. 2015;16:99.
- Scholz M, Reyes PM, Schleicher P, et al. A new stand-alone cervical anterior interbody fusion device. *Biomechanical*

- comparison with established anterior cervical fixation devices. *Spine (Phila Pa 1976)*. 2009;34:156-160.
11. Scholz M, Schleicher P, Pabst S, Kandziora F. A zero-profile anchored spacer in multilevel cervical anterior interbody fusion: biomechanical comparison to established fixation techniques. *Spine (Phila Pa 1976)*. 2015;40:E375-E380.
 12. Barbagallo GM, Romano D, Certo F, Milone P, Albanese V. Zero-P: a new zero-profile cage-plate device for single and multi-level ACDF. A single institution series with four years maximum follow-up and review of the literature on zero-profile devices. *Eur Spine J*. 2013;22(suppl 6): S868-S878.
 13. Healy AT, Sundar SJ, Cardenas RJ, et al. Zero-profile hybrid fusion construct versus 2-level plate fixation to treat adjacent-level disease in the cervical spine. *J Neurosurg Spine*. 2014;21:753-760.
 14. Lee YS, Kim YB, Park SW. Does a zero-profile anchored cage add additional stabilization as an anterior cervical plate? *Spine (Phila Pa 1976)*. 2015;40:E563-E570.
 15. Miao J, Shen Y, Kuang Y, et al. Early follow-up outcomes of a new zero-profile implant used in anterior cervical discectomy and fusion. *J Spinal Disord Tech*. 2013;26:E193-E197.
 16. Njoku I Jr, Alimi M, Leng LZ, et al. Anterior cervical discectomy and fusion with a zero-profile integrated plate and spacer device: a clinical and radiological study: Clinical article. *J Neurosurg Spine*. 2014;21:529-537.
 17. Vanek P, Bradac O, Delacy P, Lacman J, Benes V. Anterior interbody fusion of the cervical spine with Zero-P spacer: prospective comparative study-clinical and radiological results at a minimum 2 years after surgery. *Spine (Phila Pa 1976)*. 2013;38:E792-E797.
 18. Kim HJ, Kelly MP, Ely CG, Dettori JR, Riew KD. The risk of adjacent-level ossification development after surgery in the cervical spine: are there factors that affect the risk? A systematic review. *Spine (Phila Pa 1976)*. 2012;37(22 suppl):S65-S74.
 19. Patwardhan AG, Havey RM, Meade KP, Lee B, Dunlap B. A follower load increases the load-carrying capacity of the lumbar spine in compression. *Spine (Phila Pa 1976)*. 1999;24:1003-1009.
 20. Dreischarf M, Zander T, Bergmann G, Rohlmann A. A non-optimized follower load path may cause considerable intervertebral rotations. *J Biomech*. 2010;43:2625-2628.
 21. Wilke HJ, Wenger K, Claes L. Testing criteria for spinal implants: recommendations for the standardization of in vitro stability testing of spinal implants. *Eur Spine J*. 1998;7:148-154.
 22. Li Y, Hao D, He B, Wang X, Yan L. The efficiency of zero-profile implant in anterior cervical discectomy fusion: a prospective controlled long-term follow-up study. *J Spinal Disord Tech*. 2015;28: 398-403.
 23. Wang C, Zhang Y, Yuan W. Early clinical outcomes and radiographic features after treatment of cervical degenerative disk disease with the new zero-profile implant: a 1-year follow-up retrospective study. *Clin Spine Surg*. 2016;29:E73-E79.
 24. Wang ZD, Zhu RF, Yang HL, et al. The application of a zero-profile implant in anterior cervical discectomy and fusion. *J Clin Neurosci*. 2014;21:462-466.
 25. Majid K, Chinthakunta S, Muzumdar A, Khalil S. A comparative biomechanical study of a novel integrated plate spacer for stabilization of cervical spine: an in vitro human cadaveric model. *Clin Biomech (Bristol, Avon)*. 2012;27:532-536.
 26. Stein MI, Nayak AN, Gaskins RB 3rd, Cabezas AF, Santoni BG, Castellvi AE. Biomechanics of an integrated interbody device versus ACDF anterior locking plate in a single-level cervical spine fusion construct. *Spine J*. 2014;14:128-136.
 27. Anderson KK, Arnold PM. Oropharyngeal dysphagia after anterior cervical spine surgery: a review. *Global Spine J*. 2013;3: 273-286.
 28. Chung JY, Park JB, Seo HY, Kim SK. Adjacent segment pathology after anterior cervical fusion. *Asian Spine J*. 2016;10: 582-592.
 29. Lee MJ, Bazaz R, Furey CG, Yoo J. Influence of anterior cervical plate design on dysphagia: a 2-year prospective cohort study. *J Spinal Disord Tech*. 2005;18:406-409.