



ELSEVIER

The Spine Journal 13 (2013) 1563–1570

**THE
SPINE
JOURNAL**

Basic Science

Rough titanium alloys regulate osteoblast production of angiogenic factors

Rene Olivares-Navarrete, DDS, PhD^a, Sharon L. Hyzy, MS^{a,b}, Rolando A. Gittens, I, PhD^c, Jennifer M. Schneider, MS^d, David A. Haithcock, BS^a, Peter F. Ullrich, MD^e, Paul J. Slosar, MD^f, Zvi Schwartz, DMD, PhD^{a,g}, Barbara D. Boyan, PhD^{a,*}

^aWallace H. Coulter Department of Biomedical Engineering at Georgia Tech and Emory University, Georgia Institute of Technology, 315 Ferst Drive NW, Atlanta, GA 30332-0363, USA

^bSchool of Biology, Georgia Institute of Technology, 315 Ferst Drive NW, Atlanta, GA 30332, USA

^cSchool of Materials Science and Engineering, Georgia Institute of Technology, 711 Ferst Drive NW, Atlanta, GA 30332, USA

^dTitan Spine, LLC, 6140 W. Executive Drive, Suite A, Mequon, WI 53092, USA

^eNeuroSpine Center of Wisconsin, 5320 W. Michaels Drive, Appleton, WI 54913, USA

^fSpineCare Medical Group, San Francisco Spine Institute, 1199 Bush St, San Francisco, CA 94109, USA

^gDepartment of Periodontics, University of Texas Health Science Center at San Antonio, 7703 Floyd Curl Drive, San Antonio, TX 78229, USA

Received 3 March 2012; revised 28 November 2012; accepted 20 March 2013

Abstract

BACKGROUND CONTEXT: Polyether-ether-ketone (PEEK) and titanium-aluminum-vanadium (titanium alloy) are used frequently in lumbar spine interbody fusion. Osteoblasts cultured on microstructured titanium generate an environment characterized by increased angiogenic factors and factors that inhibit osteoclast activity mediated by integrin $\alpha 2\beta 1$ signaling. It is not known if this is also true of osteoblasts on titanium alloy or PEEK.

PURPOSE: The purpose of this study was to determine if osteoblasts generate an environment that supports angiogenesis and reduces osteoclastic activity when grown on smooth titanium alloy, rough titanium alloy, or PEEK.

STUDY DESIGN: This in vitro study compared angiogenic factor production and integrin gene expression of human osteoblast-like MG63 cells cultured on PEEK or titanium-aluminum-vanadium (titanium alloy).

METHODS: MG63 cells were grown on PEEK, smooth titanium alloy, or rough titanium alloy. Osteogenic microenvironment was characterized by secretion of osteoprotegerin and transforming growth factor beta-1 (TGF- $\beta 1$), which inhibit osteoclast activity and angiogenic factors including vascular endothelial growth factor A (VEGF-A), fibroblast growth factor 2 (FGF-2), and angiopoietin-1 (ANG-1). Expression of integrins, transmembrane extracellular matrix recognition proteins, was measured by real-time polymerase chain reaction.

RESULTS: Culture on titanium alloy stimulated osteoprotegerin, TGF- $\beta 1$, VEGF-A, FGF-2, and angiopoietin-1 production, and levels were greater on rough titanium alloy than on smooth titanium alloy. All factors measured were significantly lower on PEEK than on smooth or rough titanium

FDA device/drug status: Not applicable.

Author disclosures: **RO-N:** Grant: Titan Spine (D, Paid directly to institution/employer); Consulting fee or honorarium: Titan Spine (A). **SLH:** Grant: Titan Spine (D, Paid directly to institution/employer); Support for travel to meetings for the study or other purposes: Titan Spine (A). **RAG:** Royalties: Patent application (A). **JMS:** Stock Ownership: Titan Spine, LLC (<1%); Trips/Travel: Titan Spine, LLC (C); Other: Employee of Titan Spine. **DAH:** Nothing to disclose. **PFU:** Royalties: Titan Spine, LLC (F); Stock Ownership: Titan Spine, LLC (33%); Trips/Travel: Titan Spine, LLC (B). **PJS:** Royalties: Titan Spine (B); Stock Ownership: Titan Spine (<1%); Scientific Advisory Board: Titan Spine (E); Other Office: Titan Spine (E); Fellowship Support: NuVasive/OREF (D). **ZS:** Grant: Titan Spine (D, Paid directly to institution/employer); Support for travel to meetings for the study or other purposes: Titan Spine (travel to Eurospine

meeting) (\$1500 in travel expenses). **BDB:** Grant: Titan Spine (D, Paid directly to institution/employer); Consulting fee or honorarium: Titan Spine (B); Support for travel to meetings for the study or other purposes: Titan Spine (B).

The disclosure key can be found on the Table of Contents and at www.TheSpineJournalOnline.com.

Funding: This research was supported by US PHS grant NIH AR052102. Titan Spine, LLC, provided the Ti6Al4V and polyether-ether-ketone substrates as a gift.

* Corresponding author. Wallace H. Coulter Department of Biomedical Engineering, Georgia Institute of Technology, 315 Ferst Drive NW, Atlanta, GA 30332-0363, USA. Tel.: +1 (404) 385-4108; fax: +1 (404) 894-2291.

E-mail address: barbara.boyan@bme.gatech.edu (B.D. Boyan)

alloy. Culture on titanium alloy stimulated expression of messenger RNA for integrins that recognize Type I collagen in comparison with PEEK.

CONCLUSIONS: Rough titanium alloy stimulated cells to create an osteogenic-angiogenic microenvironment. The osteogenic-angiogenic responses to titanium alloy were greater than PEEK and greater on rough titanium alloy than on smooth titanium alloy. Surface features regulated expression of integrins important in collagen recognition. These factors may increase bone formation, enhance integration, and improve implant stability in interbody spinal fusions. © 2013 Elsevier Inc. All rights reserved.

Keywords: Titanium-aluminum-vanadium alloy; Polyether-ether-ketone; PEEK; Osteoblast; Angiogenesis

Introduction

An aging population has increased the demand for orthopedic implants to restore function. Lumbar and cervical interbody fusion surgeries are commonly used procedures for many types of spine pathology. Advantages to fusing the disc space anteriorly include the fact that the graft has compression loads applied to it (Wolff law), has excellent vascularity, and can hold large quantities of bone graft. Another advantage is that there is ready access to mesenchymal stem cells and osteoprogenitor cells, which help in the healing and osseointegration of the implant. Although many factors contribute to the success of a spinal fusion procedure, including surgical technique, biologics or bone grafting materials, and the mechanical and structural properties of an interbody device, contributions of the implant material to intervertebral bone formation are not well known.

Currently, there are multiple material choices for an interbody implant. Of these, two of the most popular synthetic implant materials are titanium (typically titanium-aluminum-vanadium alloy [Ti6Al4V]) and polyether-ether-ketone (PEEK) [1–3]. In addition to acting as a spacer between vertebrae, interbody implants provide surfaces that may have impacts on peri-implant bone formation. Studies examining bone formation adjacent to dental and total joint implant surfaces indicate that lack of bone apposition may lead to implant micromotion and loosening with clinical failure [4,5]. Whereas implants fabricated from Ti6Al4V result in good bone-to-implant contact and are osseointegrated into the surrounding bone [6–8], PEEK does not integrate well with the surrounding bone and instead may form a fibrous connective interface [3,9,10].

Development of a fusion mass is required for spine fusion, and one role of an interbody device is to support osteogenesis across the interbody space. Bone graft materials and biologics facilitate this process by providing a surface and bioactive factors that promote migration of osteoblast progenitor cells and osteoblast differentiation. Macroscale properties, such as implant geometry, are important with respect to vascular ingrowth, but implant topography at the microscale is important for osteoblastic differentiation, osteoid synthesis, and mineralization. In vivo success of titanium alloy implants may be in part

because of a stimulatory effect of the device surface on osteoblastic differentiation. In vitro studies show that this effect is greater in osteoblasts cultured on titanium alloy with a micron-scale rough surface texture in comparison with smooth or machined titanium alloy [11,12]. In vivo observations support these in vitro results. Grit-blasted titanium alloy pedicle screws showed a 100% increase in pullout force in sheep spines compared with smooth screws [12].

Surface texture is also an important factor in normal bone formation. During healing and remodeling of bone, osteoblasts mature and mineralize their extracellular matrix in areas of the bone that have been preconditioned by osteoclasts. The action of the osteoclasts creates micron- and submicron-scale roughness [13]. Most importantly, cells on rough surfaces produce increased levels of factors that increase osteogenesis in comparison with cells on smooth surfaces; these factors include transforming growth factor beta-1 (TGF- β 1) and bone morphogenetic proteins [14,15]. This suggests that surface texture is an important factor in bone formation.

Bone formation is a result of several processes that work in concert to achieve net new bone. Osteoclast number and/or activity need to decrease to achieve less bone remodeling than new bone formation. When osteoblasts grow on microtextured titanium surfaces, they increase production of local factors that reduce osteoclastic bone remodeling in comparison with osteoblasts grown on smooth surfaces [16]. These factors include osteoprotegerin, a decoy receptor for receptor activator of nuclear factor κ B ligand, which modulates osteoclast activity. It is not known if either titanium alloy or PEEK elicits a similar outcome.

Angiogenesis, new blood vessel formation stemming from existing vasculature, is important in bone formation, fracture healing, bone regeneration, and osseointegration [17–19]. Angiogenic factors must create the vascularity needed to support bone creation. Angiogenesis is promoted by several growth factors including vascular endothelial growth factor A (VEGF-A), fibroblast growth factor 2 (FGF-2), and angiopoietin-1 (ANG-1) [20–22]. Studies examining the role of surface microarchitecture on osteoblast production of these factors showed that cells cultured on rough microtextured titanium substrates produce higher levels of VEGF-A and FGF-2 [23]. The results of these

studies demonstrate that chemistry and microtexture of surfaces affect cell response, bringing into question how biomaterials used in interbody fusion, PEEK, and titanium alloy differ.

Osteoblasts interact with proteins adsorbed on implant surfaces through integrins, heterodimeric transmembrane receptors that bind specific extracellular matrix components. As cells adopt a more differentiated phenotype, complex interactions between cells and extracellular matrix occur, strengthening cell adhesion and possibly leading to improved biomaterial osseointegration [24,25]. Whereas less differentiated osteoblasts express the integrin pair $\alpha 5\beta 1$, the more differentiated cells on titanium and titanium alloy express $\alpha 2\beta 1$, which recognizes collagen [26–28]. Several studies show that levels of integrin subunits $\alpha 2$ and $\beta 1$ increase on rough titanium surfaces compared with smooth titanium and are required for enhanced osteoblast maturation on these surfaces [26–28]. It is not known if osteoblasts on PEEK behave in a similar manner.

The aim of this study was to compare the production of osteogenic and angiogenic factors by human osteoblast-like cells cultured on smooth or microtextured (rough) titanium alloy substrates with cells cultured on PEEK, factors that regulate the cells via autocrine and paracrine pathways and contribute to peri-implant bone formation [16,29,30], and correlate these results to expression of specific integrin extracellular matrix receptors. To determine this, we assessed whether cells on these surfaces presented a mature osteoblast phenotype and whether secretion of local factors and angiogenic factors were affected by the chemistry and topography of the substrate. In addition, we investigated the types of integrins expressed by the cells as a first step in understanding why osteoblasts respond differentially to these two materials used in interbody fusions.

Methods

Disc preparation

Surgical grade titanium alloy (Ti6Al4V) and PEEK discs were provided by Titan Spine, LLC (Mequon, WI, USA). Titanium alloy discs (15 mm diameter) were machined, yielding a smooth surface texture (sTiAlV). Alternatively, the machined titanium alloy discs were etched with a proprietary process to create titanium alloy discs with a rough microtexture (rTiAlV). Polyether-ether-ketone substrates were machined. All discs were ultrasonically cleaned, sonicated in ultrapure water (Millipore, Billerica, MA, USA), and sterilized by autoclave (Tuttnauer, Hauppauge, NY, USA) for 20 minutes at 121°C and 15 psi before use in cell culture studies.

Disc characterization

Scanning electron microscopy and laser confocal microscopy were used to characterize the surface topographies of

the titanium alloy and PEEK discs. In addition, the chemistry of the surface was determined using energy-dispersive X-ray spectroscopy and sessile-drop contact angle. The detailed description of the methods used and the results have been published previously [31]. Briefly, the PEEK discs had a machined surface finish with parallel grooves because of processing and no other distinctive features; sTiAlV discs also had a machined surface finish with shallower grooves than were seen on PEEK surfaces; and rTiAlV discs were characterized by 100 to 300 μm craters with superimposed micron-scale features. The roughness of each surface was determined by laser confocal microscopy ($S_a=0.09\pm 0.01\ \mu\text{m}$ for sTiAlV, $S_a=0.43\pm 0.07\ \mu\text{m}$ for PEEK, and $S_a=1.81\pm 0.51\ \mu\text{m}$ for rTiAlV). Energy-dispersive X-ray spectroscopy measurements confirmed that PEEK and the titanium alloy substrates had different chemistries. As expected, PEEK samples were comprised of C and O. Both sTiAlV and rTiAlV were comprised of Ti, Al, and V with no significant compositional differences between the two. Surface wettability assessed by contact angle measurements showed that all three substrates presented similar contact angles.

Cell culture

Human MG63 cells (American Type Culture Collection, Manassas, VA, USA) were used as a model for these studies. They have been well studied in cell response to titanium [32], and results correlate well with the results obtained from in vitro studies using normal human osteoblasts, fetal and adult rat calvarial osteoblasts, and neonatal mouse calvarial osteoblasts [33–37] and also with in vivo osseointegration of dental and orthopedic implants [11,12,25]. Cells were cultured at an initial density of 10,000 cells/cm² on tissue culture polystyrene (TCPS, the surface of the cell culture plate wells), PEEK, sTiAlV, and rTiAlV. Medium (Dulbecco modification of Eagle medium [Cellgro; MediaTech, Manassas, VA, USA] containing 10% fetal bovine serum [Hyclone; Thermo Scientific, Pittsburg, PA, USA] and 1% penicillin-streptomycin [Gibco; Invitrogen, Carlsbad, CA, USA]) was changed 24 hours after plating and then every 48 hours thereafter. When cultures reached confluence on TCPS, the cells on all surfaces were treated for an additional 24 hours with fresh medium. To ensure that cells were removed completely from the surfaces, the cells were released with two sequential 10-minute incubations in 0.25% trypsin-EDTA (Invitrogen) at 37°C and counted (Z2 Counter; Beckman Coulter, Fullerton, CA, USA).

The cell culture model was validated by assessing cell number, alkaline phosphatase-specific activity of isolated cells, and levels of osteocalcin in the conditioned medium as reported previously [31]. Briefly, in comparison with growth on TCPS, cell number was reduced on the test substrates (TCPS>PEEK>sTiAlV>rTiAlV). Alkaline phosphatase-specific activity was increased on the titanium alloy surfaces compared with TCPS and PEEK

(TCPS=PEEK<sTiAlV<rTiAlV). Similarly, osteocalcin was elevated on the titanium alloy substrates in comparison with TCPS and PEEK, but there was no additional effect of roughness (TCPS=PEEK<sTiAlV, rTiAlV).

Analysis of secreted factors

Conditioned media were collected and assayed for secreted proteins and factors as described previously [33]. Osteoprotegerin, VEGF-A, FGF-2, and ANG-1 were assayed using commercially available enzyme-linked immunosorbent assays (R&D Systems, Minneapolis, MN, USA) following manufacturer's instructions. Active TGF- β 1 was measured before acidification of the conditioned media using a commercially available ELISA (R&D Systems). Total TGF- β 1 was measured after acidifying the media, and latent TGF- β 1 was defined as total TGF- β 1 minus active TGF- β 1. Results of immunoassays were normalized to total cell number.

Integrin expression

Changes in integrin messenger RNA (mRNA) expression were measured using real-time polymerase chain reaction. When MG63 cells reached confluence on TCPS, all cultures were incubated for an additional 12 hours with fresh medium. RNA was isolated using TRIzol (Invitrogen) and quantified using a Nanodrop spectrophotometer (Thermo Scientific, Waltham, MA, USA). Two hundred fifty nanograms of RNA was reverse transcribed to complementary DNA templates using High Capacity Reverse Transcription cDNA kit (Applied Biosystems, Carlsbad, CA, USA). Gene-specific primers and Power SYBR Green Master Mix (Applied Biosystems) were used to quantify mRNA expression using the StepOnePlus Real-time PCR System (Applied Biosystems). Starting mRNA quantities were quantified using a standard curve of mRNA created from known dilutions of MG63 cells cultured on TCPS and related to threshold cycle values. Genes are presented as normalized to glyceraldehyde 3-phosphate dehydrogenase (GAPDH, forward 5'-GCTCTCCAGAACATCATCC-3' and reverse 5'-TGCTTACCACCTTCTTG-3'). Primers for integrin α 1 (ITGA1, forward 5'-CACTCGTA

AATGCCAAGAAAAG-3' and reverse 5'-TAGAACCCAA-CACAAAGATGC-3'), integrin α 2 (ITGA2, forward 5'-ACTGTTCAAGGAGAGAC-3' and reverse 5'-GGTCA AAGGCTTGTTTAGG-3'), integrin α 5 (ITGA5, forward 5'-ATCTGTGTGCCTGACCTG-3' and reverse 5'-AAGTTC CCTGGGTGTCTG-3'), integrin α v (ITGAV, forward 5'-GTTGCTACTGGCTGTTTTGG-3' and reverse 5'-CTGCTC CCTTTCTTGTCTTC-3'), integrin β 1 (ITGB1, forward 5'-ATTACTCAGATCCAACCAC-3' and reverse 5'-TCCTCCT CATTTCATTCATC-3'), and integrin β 3 (ITGB3, forward 5'-AATGCCACCTGCCTCAAC-3' and reverse 5'-GCTCA CCGTGTCTCCAATC-3') were designed using Beacon Designer (Premier Biosoft, Palo Alto, CA, USA) and synthesized by Eurofins MWG Operon (Huntsville, AL, USA).

Statistical analysis

For each experiment, there were six independent cultures per type of surface. Experiments were repeated to ensure validity of the results. Data presented are from one representative experiment. Data were analyzed by analysis of variance; when statistical differences were detected, Student *t* test was used with post hoc correction for multiple comparisons using Tukey's method, and $p < .05$ was considered significant.

Results

Effects on factors modulating osteoclast activity

Osteoprotegerin production was sensitive to surface properties. Levels were increased in cultures grown on PEEK and smooth titanium alloy (sTiAlV) compared with TCPS ($p < .05$). However, when cells were grown on rough titanium alloy (rTiAlV), production increased by 100% in comparison with TCPS and PEEK and by 30% in comparison with sTiAlV (Fig. 1, Left, $p < .05$). Active TGF- β 1 was more than 100% higher on titanium alloy surfaces compared with either TCPS or PEEK (Fig. 1, Middle, $p < .05$). Latent TGF- β 1 was higher on sTiAlV than PEEK and further increased in cells on rTiAlV (Fig. 1, Right, $p < .05$).

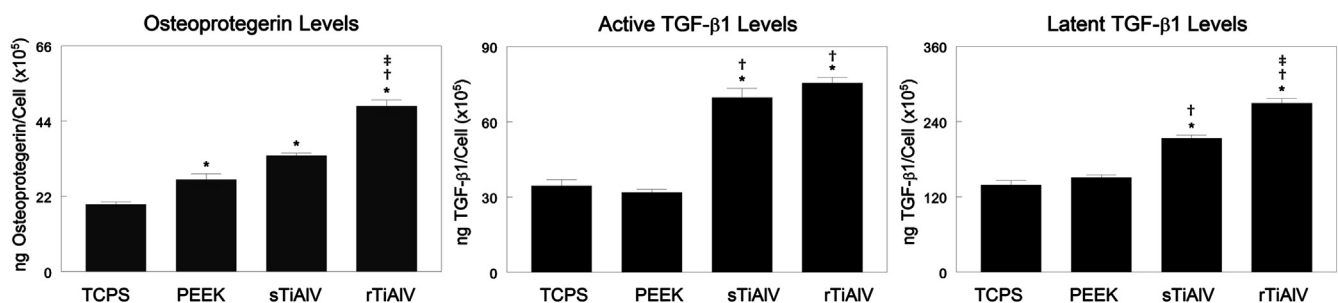


Fig. 1. Secreted osteoprotegerin (Left), active TGF- β 1 (Middle), and latent TGF- β 1 (Right) were measured in the conditioned media of cells cultured on TCPS, PEEK, smooth titanium alloy (sTiAlV), or rough titanium alloy (rTiAlV). Levels were normalized to total cell number. * $p < .05$, versus TCPS; † $p < .05$, versus PEEK; ‡ $p < .05$, versus sTiAlV. TGF- β 1, transforming growth factor beta-1; TCPS, tissue culture polystyrene; PEEK, polyether-ether-ketone; sTiAlV, smooth Ti6Al4V; rTiAlV, rough Ti6Al4V.

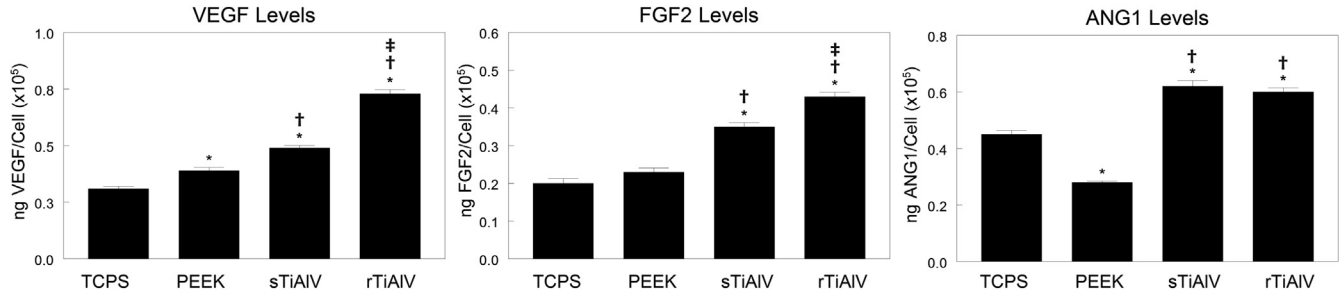


Fig. 2. Secreted VEGF-A (Left), FGF-2 (Middle), and ANG-1 (Right) were measured in the conditioned media of cells cultured on TCPS, PEEK, smooth titanium alloy (sTiAlV), or rough titanium alloy (rTiAlV). Levels were normalized to total cell number. * $p < .05$, versus TCPS; † $p < .05$, versus PEEK; ‡ $p < .05$, versus sTiAlV. VEGF-A, vascular endothelial growth factor A; FGF-2, fibroblast growth factor 2; ANG-1, angiopoietin-1; TCPS, tissue culture polystyrene; PEEK, polyether-ether-ketone; sTiAlV, smooth Ti6Al4V; rTiAlV, rough Ti6Al4V.

Angiogenic factor production

All experimental surfaces supported higher levels of VEGF than cells cultured on TCPS (Fig. 2, Left). However, cells on sTiAlV produced higher levels of VEGF than cells on PEEK, and rTiAlV enhanced this effect ($p < .05$). Culture on TCPS and PEEK produced similar levels of FGF-2, but levels were 75% higher on sTiAlV and 100% higher on rTiAlV than on PEEK (Fig. 2, Middle, $p < .05$). Levels of ANG-1 decreased on PEEK in comparison with TCPS, but culture on titanium alloy, both smooth and rough, increased ANG-1 50% over cells on TCPS (Fig. 2, Right, $p < .05$). The results show that cells cultured on titanium alloy produce higher levels of angiogenic factors than cells on PEEK, but the effect on VEGF and FGF-2 was enhanced on rough titanium alloy substrates.

Integrin expression

Culture on sTiAlV and rTiAlV substrates stimulated higher expression of ITGA1 mRNA (Table), ITGA2 (Fig. 3, Left), ITGAV (Table), and ITGB1 (Fig. 3, Right) than on TCPS or PEEK ($p < .05$). Moreover, ITGA2 expression was greater on rTiAlV than on sTiAlV (Fig. 3, Left, $p < .05$). Expression of ITGA5 was higher on PEEK than on TCPS, reduced on titanium alloy surfaces in comparison with TCPS, and further reduced on rTiAlV in comparison

with sTiAlV (Table, $p < .05$). Expression of ITGB3 was lower on PEEK than on TCPS, sTiAlV, or rTiAlV (Table, $p < .05$).

Discussion

Studies using both commercially available pure titanium and titanium alloys (ie, Ti6Al4V) have demonstrated in vitro that increased surface roughness enhances osteoblast maturation and production of local factors associated with osteogenesis and in vivo that the same topographies increase bone-to-implant contact and torque removal forces [12,23,38]. We previously showed that osteoblasts on rough titanium substrates produce angiogenic factors [23]. The present study indicates that osteoblasts also produced significantly higher VEGF-A and FGF-2 levels on smooth and rough titanium alloys than on PEEK, an effect significantly more robust on rough titanium alloy. These results suggest that peri-implant osteoblasts may create an environment that modulates angiogenesis around the implant and in the adjacent tissue, indicating that the chemistry of the implant plays an important role in determining the nature of the angiogenic milieu. Interestingly, cells grown on PEEK surfaces did not stimulate production of angiogenic factors.

The importance of angiogenesis in bone homeostasis is well appreciated. Vasculature is required for delivery of

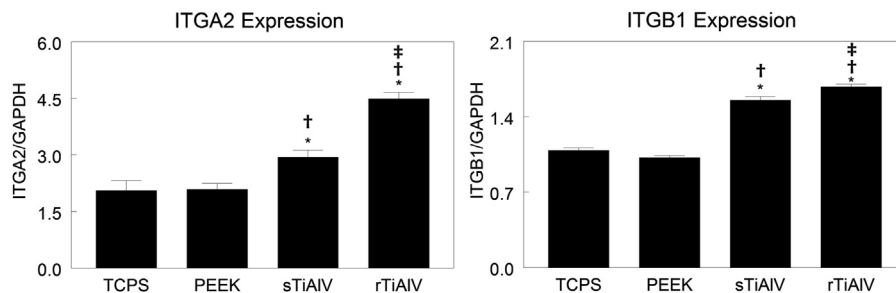


Fig. 3. Expression of messenger RNA for ITGA2 (Left) and ITGB1 (Right) were measured by real-time qPCR of cells cultured on TCPS, PEEK, smooth titanium alloy (sTiAlV), or rough titanium alloy (rTiAlV). Expression is normalized to GAPDH. * $p < .05$, versus TCPS; † $p < .05$, versus PEEK; ‡ $p < .05$, versus sTiAlV. ITGA2, integrin $\alpha 2$; ITGB1, integrin $\beta 1$; TCPS, tissue culture polystyrene; qPCR, quantitative polymerase chain reaction; GAPDH, glyceraldehyde 3-phosphate dehydrogenase; PEEK, polyether-ether-ketone; sTiAlV, smooth Ti6Al4V; rTiAlV, rough Ti6Al4V.

Table
Expression of mRNA for ITGA1, ITGA5, ITGAV, and ITGB3

Surface	Gene expression (mean±SEM)			
	ITGA1	ITGA5	ITGAV	ITGB3
TCPS	0.935±0.057	1.403±0.026	1.008±0.030	1.211±0.040
PEEK	0.875±0.128	1.686±0.022*	0.829±0.020	0.862±0.102*
sTiAIV	1.407±0.114 ^{*,†}	1.115±0.023 ^{*,†}	1.402±0.079 ^{*,†}	1.301±0.091 [†]
rTiAIV	1.577±0.108 ^{*,†}	0.892±0.023 ^{*,†,‡}	1.569±0.037 ^{*,†}	1.161±0.059

mRNA, messenger RNA; SEM, standard error of the mean; TCPS, tissue culture polystyrene; PEEK, polyether-ether-ketone; sTiAIV, smooth titanium alloy; rTiAIV, rough titanium alloy; ITGA1, integrin $\alpha 1$; ITGA5, integrin $\alpha 5$; ITGAV, integrin αv ; ITGB3, integrin $\beta 3$; PCR, polymerase chain reaction; GAPDH, glyceraldehyde 3-phosphate dehydrogenase.

Note: Human MG63 osteoblast-like cells were harvested 12 hours after confluence on TCPS. Expression of mRNA for ITGA1, ITGA5, ITGAV, and ITGB3 was measured by real-time quantitative PCR of cells cultured on TCPS, PEEK, sTiAIV, or rTiAIV. Expression is normalized to GAPDH. * $p < .05$, versus TCPS; [†] $p < .05$, versus PEEK; [‡] $p < .05$, versus sTiAIV.

nutrients and removal of wastes and provides a source of multipotent cells for tissue regeneration and remodeling [39]. The factors measured in this study play distinct but cooperative roles in the process. VEGF-A is produced by diverse cells, including osteoblasts, and is one of the most important initiators of the signaling cascade during neo-vascularization in endothelial cells [40]. FGF-2, a soluble factor with autocrine and paracrine functions, induces proliferation and migration of endothelial cells and is considered a key factor in angiogenesis [41]. Angiopoietin-1 is known to control late stages of blood vessel formation, such as stabilization of the endothelial sprout and endothelial interaction with pericytes [42]. Our results suggest that failure of osseointegration observed with PEEK implants is associated with reduced ability of cells on the implant surface to generate an environment rich in these factors.

Our results suggest that angiogenic factor production is associated with osteoblast maturation state. As we have noted previously, MG63 cells exhibit a more differentiated phenotype on rough titanium alloy, characterized by reduced cell number and increased osteocalcin production [31]. This suggests that osteoblast differentiation is sensitive to general micron-scale elements. Polyether-ether-ketone surfaces differ both chemically and physically from titanium alloy; so it is difficult to ascribe a specific parameter or feature of the surface to the lack of an angiogenic response. Cellular response studies of PEEK have been limited to cell attachment and proliferation, but we previously showed that MG63 cells and normal human osteoblasts on PEEK do not exhibit increased alkaline phosphatase or osteocalcin production typical of differentiated osteoblast [31]. Moreover, studies have attempted to modify PEEK using coatings of hydroxyapatite [43], titanium [44], or diamond-like carbon [45] to improve cellular response, supporting our findings that PEEK does not induce an osteogenic response.

In this experimental in vitro study, MG63 cells grown on rough titanium alloy increased levels of active and latent TGF- $\beta 1$ and osteoprotegerin in their media, both of which are associated with bone formation. Osteoblasts produce TGF- $\beta 1$ in latent form and store it in the extracellular

matrix. In its active form, TGF- $\beta 1$ stimulates osteoblast differentiation and matrix synthesis [46] whereas inhibiting osteoclast activity [47]. Osteoprotegerin is produced by osteoblasts as a decoy receptor for receptor activator of nuclear factor κB ligand, thereby reducing osteoblast-dependent osteoclast activation [48]. Together these factors result in net new bone formation. This microenvironment may enhance bone formation while regulating bone remodeling in areas adjacent to the implant.

We previously showed that osteoblast differentiation and production of VEGF-A and FGF-2 on microtextured titanium are mediated by $\alpha 2 \beta 1$ integrin signaling [23]. Here, we show that mRNAs for integrins $\alpha 1$, $\alpha 2$, αv , and $\beta 1$ were upregulated in cells grown on titanium alloy surfaces. Interestingly, ITGA2 and ITGB1 expressions were higher on rough titanium alloy surfaces than smooth surfaces, as was noted in cells grown on titanium [26]. MG63 cells grown on PEEK express similar integrin subunits as seen on TCPS, specifically $\alpha 5$, which is associated with cell attachment and proliferation but not with differentiation [27]. These results may explain why PEEK failed to induce osteoblast maturation or yield an osteogenic environment.

Conclusions

This experimental study demonstrates that rough titanium alloy stimulates an angiogenic-osteogenic environment with factors important in bone formation and remodeling. This osteogenic environment may enhance bone formation, implant stability, and fusion. Clinically, these findings point to the possibility that surface texture and material composition of spinal interbody implants can be manipulated to maximize the endogenous production of bone growth and angiogenic factors.

References

- [1] Toth JM, Wang M, Estes BT, et al. Polyetheretherketone as a biomaterial for spinal applications. *Biomaterials* 2006;27:324–34.
- [2] Bruner HJ, Guan Y, Yoganandan N, et al. Biomechanics of polyaryletherketone rod composites and titanium rods for posterior

- lumbosacral instrumentation. Presented at the 2010 Joint Spine Section Meeting. Laboratory investigation. *J Neurosurg Spine* 2010;13:766–72.
- [3] Kurtz SM, Devine JN. PEEK biomaterials in trauma, orthopedic, and spinal implants. *Biomaterials* 2007;28:4845–69.
 - [4] Bauer TW, Schils J. The pathology of total joint arthroplasty. II. Mechanisms of implant failure. *Skeletal Radiol* 1999;28:483–97.
 - [5] Brunski JB. In vivo bone response to biomechanical loading at the bone/dental-implant interface. *Adv Dent Res* 1999;13:99–119.
 - [6] Stenport VF, Johansson CB. Evaluations of bone tissue integration to pure and alloyed titanium implants. *Clin Implant Dent Relat Res* 2008;10:191–9.
 - [7] De Leonardi D, Garg AK, Pecora GE. Osseointegration of rough acid-etched titanium implants: 5-year follow-up of 100 minimatic implants. *Int J Oral Maxillofac Implants* 1999;14:384–91.
 - [8] Linder L. Osseointegration of metallic implants. I. Light microscopy in the rabbit. *Acta Orthop Scand* 1989;60:129–34.
 - [9] Santos ER, Goss DG, Morcom RK, Fraser RD. Radiologic assessment of interbody fusion using carbon fiber cages. *Spine* 2003;28:997–1001.
 - [10] Anjarwalla NK, Morcom RK, Fraser RD. Supplementary stabilization with anterior lumbar intervertebral fusion—a radiologic review. *Spine* 2006;31:1281–7.
 - [11] Lincks J, Boyan BD, Blanchard CR, et al. Response of MG63 osteoblast-like cells to titanium and titanium alloy is dependent on surface roughness and composition. *Biomaterials* 1998;19:2219–32.
 - [12] Schwartz Z, Raz P, Zhao G, et al. Effect of micrometer-scale roughness of the surface of Ti6Al4V pedicle screws in vitro and in vivo. *J Bone Joint Surg Am* 2008;90:2485–98.
 - [13] Boyan BD, Schwartz Z, Lohmann CH, et al. Pretreatment of bone with osteoclasts affects phenotypic expression of osteoblast-like cells. *J Orthop Res* 2003;21:638–47.
 - [14] Vlacic-Zischke J, Hamlet SM, Friis T, et al. The influence of surface microroughness and hydrophilicity of titanium on the up-regulation of TGFbeta/BMP signalling in osteoblasts. *Biomaterials* 2011;32:665–71.
 - [15] Kieswetter K, Schwartz Z, Hummert TW, et al. Surface roughness modulates the local production of growth factors and cytokines by osteoblast-like MG-63 cells. *J Biomed Mater Res* 1996;32:55–63.
 - [16] Schwartz Z, Olivares-Navarrete R, Wieland M, et al. Mechanisms regulating increased production of osteoprotegerin by osteoblasts cultured on microstructured titanium surfaces. *Biomaterials* 2009;30:3390–6.
 - [17] Geris L, Gerisch A, Sloten JV, et al. Angiogenesis in bone fracture healing: a bioregulatory model. *J Theor Biol* 2008;251:137–58.
 - [18] Duvall CL, Taylor WR, Weiss D, et al. Impaired angiogenesis, early callus formation, and late stage remodeling in fracture healing of osteopontin-deficient mice. *J Bone Miner Res* 2007;22:286–97.
 - [19] Abshagen K, Schrodli I, Gerber T, Vollmar B. In vivo analysis of biocompatibility and vascularization of the synthetic bone grafting substitute NanoBone. *J Biomed Mater Res A* 2009;91:557–66.
 - [20] Schweigerer L, Neufeld G, Friedman J, et al. Capillary endothelial cells express basic fibroblast growth factor, a mitogen that promotes their own growth. *Nature* 1987;325:257–9.
 - [21] Connolly DT, Heuvelman DM, Nelson R, et al. Tumor vascular permeability factor stimulates endothelial cell growth and angiogenesis. *J Clin Invest* 1989;84:1470–8.
 - [22] Mehta VB, Besner GE. HB-EGF promotes angiogenesis in endothelial cells via PI3-kinase and MAPK signaling pathways. *Growth Factors* 2007;25:253–63.
 - [23] Raines AL, Olivares-Navarrete R, Wieland M, et al. Regulation of angiogenesis during osseointegration by titanium surface microstructure and energy. *Biomaterials* 2010;31:4909–17.
 - [24] Anselme K, Bigerelle M. Topography effects of pure titanium substrates on human osteoblast long-term adhesion. *Acta Biomater* 2005;1:211–22.
 - [25] Anselme K, Bigerelle M, Noel B, et al. Qualitative and quantitative study of human osteoblast adhesion on materials with various surface roughnesses. *J Biomed Mater Res* 2000;49:155–66.
 - [26] Olivares-Navarrete R, Raz P, Zhao G, et al. Integrin alpha2beta1 plays a critical role in osteoblast response to micron-scale surface structure and surface energy of titanium substrates. *Proc Natl Acad Sci U S A* 2008;105:15767–72.
 - [27] Raz P, Lohmann CH, Turner J, et al. 1Alpha,25(OH)2D3 regulation of integrin expression is substrate dependent. *J Biomed Mater Res A* 2004;71:217–25.
 - [28] Siebers MC, ter Brugge PJ, Walboomers XF, Jansen JA. Integrins as linker proteins between osteoblasts and bone replacing materials. A critical review. *Biomaterials* 2005;26:137–46.
 - [29] Boyan BD, Lohmann CH, Sisk M, et al. Both cyclooxygenase-1 and cyclooxygenase-2 mediate osteoblast response to titanium surface roughness. *J Biomed Mater Res* 2001;55:350–9.
 - [30] Bessho K, Carnes DL, Cavin R, et al. BMP stimulation of bone response adjacent to titanium implants in vivo. *Clin Oral Implants Res* 1999;10:212–8.
 - [31] Olivares-Navarrete R, Gittens RA, Schneider JM, et al. Osteoblasts exhibit a more differentiated phenotype and increased BMP production on titanium alloy substrates than on PEEK. *Spine J* 2012;22:265–72.
 - [32] Schwartz Z, Nasazky E, Boyan BD. Surface microtopography regulates osteointegration: the role of implant surface microtopography in osteointegration. *Alpha Omega* 2005;98:9–19.
 - [33] Olivares-Navarrete R, Hyzy SL, Chaudhri RA, et al. Sex dependent regulation of osteoblast response to implant surface properties by systemic hormones. *Biol Sex Differ* 2010;1:4.
 - [34] Lohmann CH, Tandy EM, Sylvia VL, et al. Response of normal female human osteoblasts (NHOst) to 17beta-estradiol is modulated by implant surface morphology. *J Biomed Mater Res* 2002;62:204–13.
 - [35] Schneider GB, Perinpanayagam H, Clegg M, et al. Implant surface roughness affects osteoblast gene expression. *J Dent Res* 2003;82:372–6.
 - [36] Dekker RJ, van Blitterswijk CA, Hofland I, et al. Studying the effect of different macrostructures on in vitro cell behaviour and in vivo bone formation using a tissue engineering approach. *Novartis Found Symp* 2003;249:148–67; discussion 67–69, 70–74, 239–241.
 - [37] Martin JY, Schwartz Z, Hummert TW, et al. Effect of titanium surface roughness on proliferation, differentiation, and protein synthesis of human osteoblast-like cells (MG63). *J Biomed Mater Res* 1995;29:389–401.
 - [38] Cochran DL, Nummikoski PV, Higginbottom FL, et al. Evaluation of an endosseous titanium implant with a sandblasted and acid-etched surface in the canine mandible: radiographic results. *Clin Oral Implants Res* 1996;7:240–52.
 - [39] Heino TJ, Hentunen TA. Differentiation of osteoblasts and osteocytes from mesenchymal stem cells. *Curr Stem Cell Res Ther* 2008;3:131–45.
 - [40] Eilken HM, Adams RH. Dynamics of endothelial cell behavior in sprouting angiogenesis. *Curr Opin Cell Biol* 2010;22:617–25.
 - [41] Chen CH, Poucher SM, Lu J, Henry PD. Fibroblast growth factor 2: from laboratory evidence to clinical application. *Curr Vasc Pharmacol* 2004;2:33–43.
 - [42] Saharinen P, Bry M, Alitalo K. How do angiopoietins tie in with vascular endothelial growth factors? *Curr Opin Hematol* 2010;17:198–205.
 - [43] Tan KH, Chua CK, Leong KF, et al. Fabrication and characterization of three-dimensional poly(ether- ether- ketone)/-hydroxyapatite bio-composite scaffolds using laser sintering. *Proc Inst Mech Eng H* 2005;219:183–94.
 - [44] Han CM, Lee EJ, Kim HE, et al. The electron beam deposition of titanium on polyetheretherketone (PEEK) and the resulting enhanced biological properties. *Biomaterials* 2010;31:3465–70.

- [45] Wang H, Xu M, Zhang W, et al. Mechanical and biological characteristics of diamond-like carbon coated poly aryl-ether-ether-ketone. *Biomaterials* 2010;31:8181–7.
- [46] Bonewald LF, Dallas SL. Role of active and latent transforming growth factor beta in bone formation. *J Cell Biochem* 1994;55:350–7.
- [47] Janssens K, ten Dijke P, Janssens S, Van Hul W. Transforming growth factor-beta1 to the bone. *Endocrine Rev* 2005;26:743–74.
- [48] Kobayashi Y, Udagawa N, Takahashi N. Action of RANKL and OPG for osteoclastogenesis. *Crit Rev Eukaryot Gene Expr* 2009;19:61–72.