

Advances in transdermal insulin delivery

Yuqi Zhang^{a,b}, Jicheng Yu^b, Anna R. Kahkoska^c, Jinqiang Wang^{a,b}, John B. Buse^c, Zhen Gu^{a,b,d,*}

^a Department of Bioengineering, University of California, Los Angeles, CA 90095, USA

^b Joint Department of Biomedical Engineering, University of North Carolina at Chapel Hill and North Carolina State University, Raleigh, NC 27695, USA

^c Department of Medicine, University of North Carolina School of Medicine, Chapel Hill, NC 27599, USA

^d California NanoSystems Institute, Jonsson Comprehensive Cancer Center, Center for Minimally Invasive Therapeutics, University of California, Los Angeles, CA 90095, USA

ARTICLE INFO

Article history:

Received 29 June 2018

Received in revised form 6 November 2018

Accepted 5 December 2018

Available online 8 December 2018

Keywords:

Drug delivery

Transdermal delivery

Insulin

Diabetes

Iontophoresis

Electroporation

Ultrasound

Jet injection

Microneedle

ABSTRACT

Insulin therapy is necessary to regulate blood glucose levels for people with type 1 diabetes and commonly used in advanced type 2 diabetes. Although subcutaneous insulin administration via hypodermic injection or pump-mediated infusion is the standard route of insulin delivery, it may be associated with pain, needle phobia, and decreased adherence, as well as the risk of infection. Therefore, transdermal insulin delivery has been widely investigated as an attractive alternative to subcutaneous approaches for diabetes management in recent years. Transdermal systems designed to prevent insulin degradation and offer controlled, sustained release of insulin may be desirable for patients and lead to increased adherence and glycemic outcomes. A challenge for transdermal insulin delivery is the inefficient passive insulin absorption through the skin due to the large molecular weight of the protein drug. In this review, we focus on the different transdermal insulin delivery techniques and their respective advantages and limitations, including chemical enhancers-promoted, electrically enhanced, mechanical force-triggered, and microneedle-assisted methods.

Contents

1. Introduction	51
2. Chemical enhancers-promoted transdermal delivery	52
3. Electrically facilitated transdermal delivery	53
3.1. Iontophoresis	54
3.2. Electroporation	54
4. Mechanical force-triggered insulin delivery	55
4.1. Ultrasound	55
4.2. Jet injection	56
5. Microneedle-assisted transdermal delivery	57
5.1. Solid microneedles	57
5.2. Hollow microneedles	58
5.3. Dissolving microneedles	58
5.4. Degradable microneedles	63
5.5. Bioresponsive microneedles	63
6. Conclusion and outlook	66
Acknowledgement	66
References	66

* Corresponding author at: Department of Bioengineering, University of California, Los Angeles, CA 90095, USA.

E-mail address: guzhen@ucla.edu (Z. Gu).

1. Introduction

Diabetes mellitus is a group of metabolic diseases characterized by increased production of glucose by the liver and decreased clearance of glucose into muscle and fat resulting in abnormal accumulation of glucose in the blood, all driven by inadequate insulin levels [1]. Approximately 425 million adults suffer from diabetes according to 2018 reports from The International Diabetes Federation [2]. Moreover, the prevalence of diabetes is increasing and expected to rise across the world in the coming decades [3]. Diabetes is usually caused by the failure of insulin secretion by the pancreas (type 1 diabetes) or the defective responsiveness of the body to insulin (type 2 diabetes) [4,5].

Exogenous insulin administration is essential in the management of type 1 diabetes and advanced type 2 diabetes [6,7]. Typically, people with diabetes are instructed to self-inject insulin subcutaneously several times per day, which requires both training and intensive self-management with frequent dose adjustments by patients based on glucose monitoring [8]. The need for frequent injections may be associated with poor adherence, and also carries the risk of microbial contamination, local tissue necrosis, and nerve damage [9–11]. Alternatively, patients may use continuous subcutaneous insulin infusions, also known as insulin pump therapy, which also carries limitations including technological difficulties [12]. To address these limitations, a broad range of delivery methods have been investigated as needle-free alternatives for daily insulin therapy, including oral, pulmonary, nasal, and transdermal approaches [13–20]. However, the poor permeability of insulin across the tissue barriers hinders bioavailability, which poses a major limitation in the clinical applications of these approaches [21–23].

A transdermal delivery strategy that transports insulin across the skin barrier represents a minimally invasive and attractive method for insulin delivery in contrast to painful hypodermic injections [24,25]. It also has several advantages over oral, pulmonary, and nasal administration techniques. For example, insulin delivered *via* a transdermal system is able to avoid the chemical and enzymatic degradation in the digestive tract [26]. This approach can also provide a sustained release to maintain therapeutic concentrations for prolonged time [27]. Finally, the convenience of this administration may increase patient adherence, leading to improved glycemic control [27].

However, effective insulin delivery *via* the skin remains challenging due to the intrinsic, protective properties of the intact skin. Therapeutics with low molecular weight (<500 Da) can easily penetrate the skin, while the passive transport of protein drugs with higher molecular weight, such as insulin, is significantly restricted [28]. To overcome skin barriers in transdermal insulin delivery, various approaches have been explored to physically or chemically enhance the transport efficiency of the insulin molecule across the skin. This review presents the recent advances in transdermal insulin delivery systems, including chemical enhancers-promoted, electrically facilitated, mechanical force-triggered and microneedle-assisted delivery systems.

force-triggered, and microneedle (MN)-assisted approaches (Fig. 1). The challenges for potential clinical applications are also discussed.

2. Chemical enhancers-promoted transdermal delivery

In order to improve skin permeability, chemical penetration enhancers that can disrupt the skin barrier and provide an adding driving force for transporting therapeutics have been intensively investigated [29–31]. There are various effective chemical enhancers, including conventional chemical molecules as well as membrane-permeable peptides and vehicles. Chemical enhancers can insert into the highly ordered lipid bilayer in stratum corneum to disorganize molecular packing or extract lipids to create lipid-packing defects of nanometer dimensions, thus leading higher transport efficiency of insulin [32,33].

The Gasem group has previously examined the permeation enhancement properties of 43 different chemical enhancers that have been used in insulin delivery [34]. The authors also discussed the potential criteria for further screening of enhancers. Sintov et al. reported that iodine facilitated insulin delivery across the skin as iodine could inactivate endogenous sulfhydryls, such as glutathione and gamma-glutamylcysteine, thereby reducing the formation of disulfide bonds and retaining the potency of insulin during its flux through the skin into the circulation [35]. The ability of trypsin to react with the stratum corneum was also assessed for enhanced transdermal insulin delivery, where it was shown that trypsin altered the protein structure of stratum corneum from the alpha- to the beta-form and decreased the electrical resistance of the skin, reflecting a 5.2-fold increase in insulin absorption (insulin at pH 3) [36].

Wen and coworkers identified a class of membrane-permeable peptides that can promote delivery of cargo into the systemic circulation by *in vivo* phage display, in addition to previously characterized peptides (such as protein transduction domains (PTDs) that could only locally transport drugs [37]. The synthetic peptide, ACSSSPSKHCG (TD-1), was suggested to be capable of creating transient opening in the skin to enable penetration of insulin into hair follicles beyond a depth of 600 μm . An obvious suppression in blood glucose levels (BGLs) (~40% of initial values) was observed in diabetic rats, which was sustained over 11 h compared to <5 h with subcutaneously injected insulin. This research spurred development of an alternative series of peptide-based enhancers designed to transcutaneously deliver hydrophilic macromolecular therapeutics. For example, Chang et al. screened a number of TD-1-derived cationic cyclopeptides in Caco-2 cell monolayers-based *in vitro* model and assessed *in vivo* performance in diabetic rats [38]. The results indicated that TD-34 (ACSSKSKHCG) with bis-substituted lysine in N-5 and N-6 sites displayed the best transdermal enhancement activity, where administration of 2.1 IU insulin with 0.5 μmol of TD-34 led to an approximately 26% reduction in BGLs of rats that was sustained for 8 h.

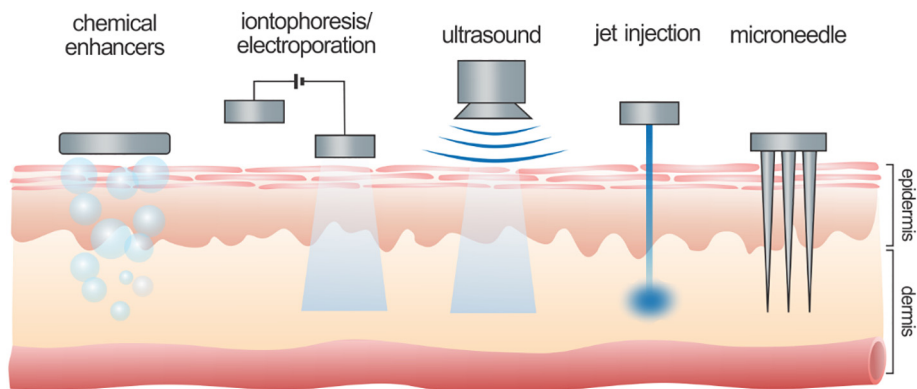


Fig. 1. Representative transdermal strategies for insulin delivery based on diverse mechanisms, including chemical enhancers-promoted, electrically facilitated, mechanical force-triggered and microneedle-assisted delivery systems.

Nano/micro vesicles, such as liposomes and nano/microemulsions, have also been explored as chemical enhancers [39–43]. They can not only improve skin permeability but also act as the vehicles for drug solubilization and drug transport through the skin [39,44]. A variety of nanocarriers have been demonstrated the ability to encapsulate and transdermally deliver insulin into the dermis, such as lipid-based vesicles [45–47], CaCO₃ nanoparticles [48] and nanoemulsions [49,50]. For example, King et al. reported lipid-based biphasic vesicles as skin penetration enhancers for insulin delivery [46]. These researchers incorporated insulin-encapsulated biphasic vesicles in a transdermal patch and applied the patch on the abdominal skin of diabetic mice for 48 h. The mice showed response to the patch loading 50 mg vesicle-entrapped insulin for over 51 h with a decrease in blood glucose of ~43%. Further analysis of the topical administration of biphasic vesicles demonstrated that the transport and absorption of insulin was primarily mediated by the lymphatic pathway in a diabetic rat model [47].

Goto and coworkers proposed an alternative formulation based on solid-in-oil (S/O) nanodispersion for protein delivery [49,51,52]. They prepared the S/O nanodispersions were approximately 250 nm and integrated with isopropyl myristate (IPM), an oil with a penetration-enhancing effect, along with insulin and R9 peptides loaded at a molar ratio of 1:3 [49]. The R9 peptides, a type of arginine-rich peptides, was involved as PTDs to enhance the skin permeability to insulin. A synergistic effect of isopropyl myristate and PTDS to disrupt the barrier property of the skin and improve insulin penetration across the skin *in vitro* was demonstrated. Nose, Pissuwan and colleagues formed a different S/O formulation by introducing gold nanorods into an oil phase for transdermal delivery under irradiation of near-infrared light [50,53]. Individually, the gold nanorods (27 nm in width and 66 nm in length) were

coated with methoxy(polyethylene glycol)-thiol and formed a complex with surfactant (L-195) and insulin, followed by dispersing in the oil phase, IPM (Fig. 2) [50]. Under near-infrared light (0.4 W/cm² for 10 min), the photothermal effect caused by gold nanorods might break the skin barrier by disrupting skin lipids or changing the size and density of the skin barrier, thus allowing insulin to permeate through the skin. Additionally, the surfactant L-195 and IPM acted as enhancers to promote transdermal transport of insulin. After treatment of nanodispersion and light irradiation, the BGLs of diabetic mice significantly decreased to approximately 58% of pre-treatment values at 4 h.

Chemical penetration enhancers can disrupt the skin structure to promote permeability and improve drug solubility to provide the drug concentration-gradient driving force. Despite this, many chemical enhancers still show limited transdermal delivery efficiency of insulin. For the most effective chemical enhancers, strategies to prevent their diffuse out of the stratum corneum and the relevant irritation to the deeper tissue should be further addressed.

3. Electrically facilitated transdermal delivery

In addition to the chemical penetration enhancers, electrical instruments that facilitate insulin transport through the skin have also received considerable attention [54–57]. Unlike chemical penetration enhancers, these electrical instruments improve the insulin delivery efficiency through the skin by providing additional driving force *via* electrical interactions or introducing transient perturbation of the stratum corneum *via* high-voltage electrical pulse.

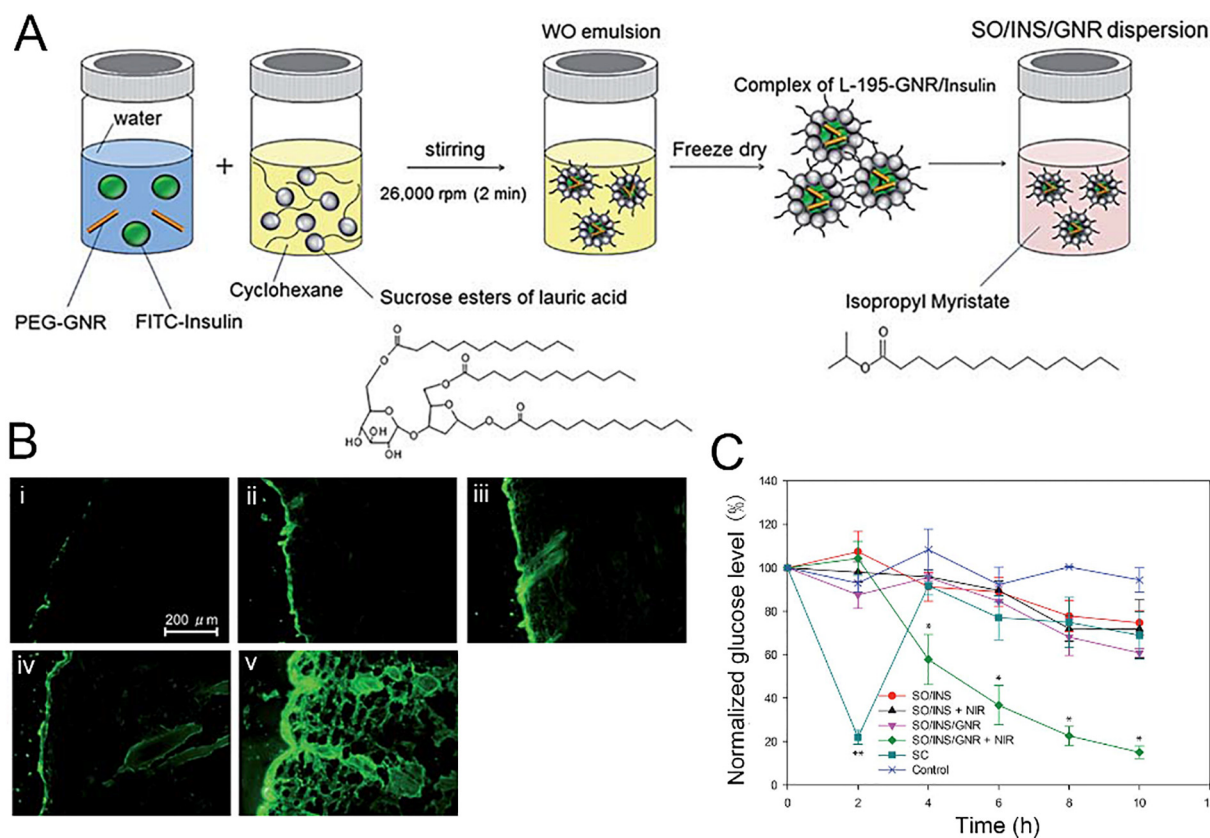


Fig. 2. A representative solid-in-oil nanoformulation for insulin transdermal delivery. A) Scheme of the preparation of gold nanorod-insulin complexes/oil formulation (SO-INS-GNR) (SO: solid-in-oil; INS: insulin; PEG-GNR: mPEG coated gold nanorod; FITC: fluorescein isothiocyanate; WO: water in oil). B) Fluorescent images showing transdermal delivery of FITC-labeled insulin after the treatment of various insulin formulations, with or without near infrared (NIR) light irradiation: insulin in water (W-INS) treatment (i), SO-INS treatment alone (ii), SO-INS treatment with NIR irradiation (iii), SO-INS-GNR treatment alone (iv), and SO-INS-GNR treatment with NIR irradiation (v). C) Blood glucose levels of diabetic mice after administration of SO-INS and SO-INS-GNR with and without NIR light irradiation, and subcutaneous injection (SCI) of insulin (*P < 0.05, **P < 0.01). Adapted with permission from Ref [50].

3.1. Iontophoresis

Iontophoresis emerged as a transdermal enhancement technique in the early 20th century. This technique uses a mild electric current for the delivery of large and/or charged molecules [54,58]. This technology relies on a pair of electrodes that is placed on the skin to generate an electrical potential between the skin surface and the capillaries below (Fig. 3). Positively charged therapeutic molecules are driven toward the capillaries from the skin surface at the positive electrode, while negatively charged molecules transport through the skin toward the negative electrode. Extensive studies have identified that electromigration and electroosmosis are two of the predominant driving forces to affect the transport of drug ions across the skin into systemic circulation [59], and the amount of transported charge depends on the intensity of the electric field and the treatment duration [60,61]. Nonetheless, the skin is permselective to cations under an electric current since it is negatively charged at the physiological condition [62]. Therefore, the transdermal delivery of insulin to give therapeutic levels is challenged by the negative charge of human insulin (~5800 Da) under physiological conditions [63–67].

Siddiqui et al. found that adjusting the aqueous solution of concentrated insulin (500 IU/mL) to a pH of 3.7 was the most effective condition for regular insulin iontophoresis [68]. Similarly, Pillai et al. revealed that anodal iontophoresis of insulin at pH 3.6 resulted in better stability and permeation of insulin [69,70]. Kajimoto et al. also attempted to raise the transport efficiency of insulin by utilizing charged liposomes as carriers during iontophoresis [71]. The *in vivo* performance in a diabetic rat model showed that the transdermal iontophoresis (0.45 mA/cm² for 1 h) of cationic liposome-encapsulated insulin through the transfollicular pathway led to a gradual decrease of 20% in BGLs at 18 h after administration which was maintained for up to 24 h. A corresponding increase in plasma insulin levels was also detected (~1.4 ng/mL 18 h post-treatment) that exceeded levels detected in rats treated with intraperitoneally injected insulin.

Pretreatment of skin such as stripping skin [72,73], using penetration enhancers [74–77] and depilatory cream [75,78,79] has been reported to enhance the transport of insulin through the skin under iontophoresis. An investigation on the effect of diverse chemical enhancers including ethanol (EtOH), propylene glycol (PG), dimethylacetamide (DMA), ethyl acetate (EtOAc) and IPM demonstrated that skin permeability was severely improved with DMA, followed by EtOH and EtOAc, while IPM and PG exhibited relatively insignificant skin barrier altering potential [77]. By acting on the lipid bilayer, these chemicals led to lipid extraction (EtOH, DMA, EtOAc), changes in skin proteins (EtOH, DMA), or increased lipid fluidity (IPM), thus produced a synergistic enhancement with iontophoresis.

Furthermore, hydrogel formulations are considered to be desirable for iontophoresis, as they can act as an electroconductive base and adapt to the contours of the skin; these formulations can also be easily integrated with the iontophoresis delivery systems [80]. Kagatani et al. reported a pulsatile insulin delivery system with an electro-responsive poly(dimethylaminopropylacrylamide) (PDMAPAA) gel [81]. The insulin-loaded PDMAPAA gel was subcutaneously injected into the skin of rats as a depot. Upon stimulation with a constant current of 1.0 mA (0.36 mA/cm²), a pulsatile plasma glucose decrease was detected in the animals. Both insulin and PDMAPAA gel in this system might be positively charged at the pH of 2.3. When an electrical field is applied, the cross-linked PDMAPAA network undergoes slight expansion at the cathode side, allowing solvated insulin to quickly diffusing out the gel with the outflow of the solution, caused by the electrokinetic flow of solvated insulin with water. In another study, Pillai et al. used poloxamer 407 to prepare the insulin gel that was further integrated with chemical enhancers for the *ex vivo* and *in vivo* skin permeation analysis [82]. Application of iontophoresis, either alone or in combination with linoleic acid, resulted in a 36–40% reduction in BGLs of diabetic rats.

To mitigate the potential electrochemical damage caused during iontophoresis, such as burns and skin irritation [83], alternating current iontophoresis was investigated over conventional direct current iontophoresis; this approach showed reduced side effects [84]. Feasibility studies showed that alternating current iontophoresis-activated transdermal insulin delivery systems were associated with an average delivery of 57% of the initial insulin amount (2.85 mg in 500 μ L sample) [85].

Unlike chemical penetration enhancers, iontophoresis does not disrupt the skin structure that may affect its barrier ability. Nonetheless, the low-level current of such technique limits the transport efficiency of insulin through the stratum corneum. Although increasing current intensity can lead to a higher delivery rate, the potential risk of skin irritation and pain also limits the maximum current intensity.

3.2. Electroporation

Electroporation has evolved as another attractive technique for electrically assisted transdermal drug delivery [55,86,87]. Different from the continuous application (hours) of low-level current in iontophoresis, the procedure of electroporation involves using short, high-voltage pulses to induce transient perturbation in the stratum corneum by creating micro-pathways across its lipid bilayers [88]. The stratum corneum forms the major barrier and contributes the major portion of the electric resistance in the skin (5–25 k Ω /cm²) [88]. In electroporation, the application of high voltage pulses that are higher than the breakdown potential of the stratum corneum (75–100 V) and thus results in the formation of temporary pores in the lipid bilayers of the

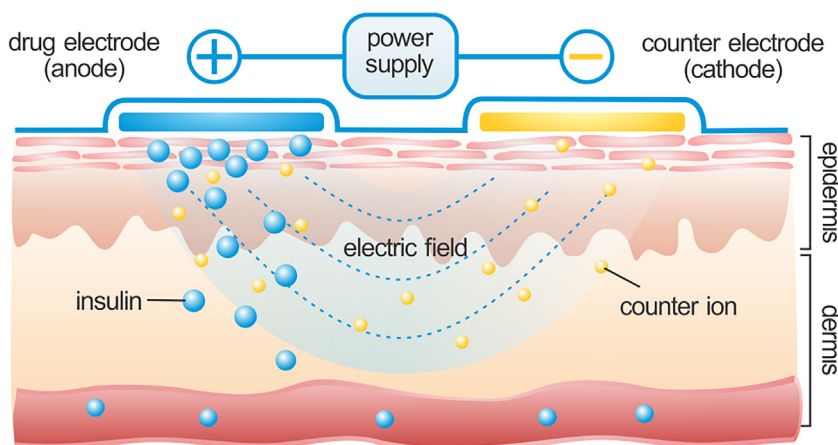


Fig. 3. Illustration of iontophoresis-assisted insulin delivery through the skin.

stratum corneum which facilitates the transport of the drugs across skin [89,90].

Several studies have been investigated to validate the enhanced transdermal delivery of insulin by electroporation. Mohammad and colleagues examined the effect of different electroporation parameters (number of pulses, insulin concentrations, and field strengths) and chemical enhancers (castor oil, iodine, and oleic acid) on transdermal insulin delivery in rabbits [91]. In another work, Rastogi et al. explored electroporation of polymeric nanoparticles encapsulated insulin, demonstrating a 4-fold enhancement in insulin deposition in rat skin compared to electroporation using free insulin, as well as an extended therapeutic effect from 24 h to 36 h [92]. Sen et al. reported an alternative transdermal enhancement method by mixing the anionic lipids with target molecules that were associated with enhancing the electroporative transport of negatively charged permeants up to 10 kDa in size [93]. The resultant enhancing effect was attributed to the increased number and size, as well as prolonged lifetime, of the electropores created during the electroporation in the presence of the lipid dispersion. Specifically, the anionic lipids were shown to have a positive effect in dropping the skin resistance and retard the recovery of resistance after the cessation of pulse application, thereby expanding the potential of lipid-enhanced electroporation for delivering large biomolecules. More recently, these researchers examined the impact of another anionic lipid, 1,2-dimyristoyl-3-phosphatidylserine (DMPS), on the transdermal transport of insulin using porcine epidermis model and observed a 20-fold enhancement of insulin with dispersion in DMPS electroporation for 10 min (100–105 V, 1 ms pulse width at 1 Hz) compared to that without DMPS [94]. Sen and coworkers also demonstrated a synergistic effect of coupling DMPS and anodal iontophoresis (electroosmosis) with electroporation on the transport of insulin both *ex vivo* and *in vivo*, where the combination treatment of DMPS (in 0.2% sodium dodecyl sulfate) and electroosmosis resulted in a ~10-fold increase in plasma insulin level in a Sprague-Dawley rat model [95,96]. This *in vivo* synergistic treatment of electroporation and iontophoresis was also validated by Sugibayashi and colleagues using human insulin [97]. Interestingly, this group suggested that insulin had different aggregation properties under different pH conditions in their study: insulin at pH 10 had a higher ratio of nonassociation formulation, whereas most of the insulin associated into hexamers at pH 7. Therefore, a much higher plasma level of insulin was detected with pH at 10 than at 7.

Considering the clinical application of electroporation, Wong et al. developed a painless electroporation technique using a microelectrode array block to mitigate the potential painful sensation induced by electrodes on the human skin while maintaining the delivery efficacy of insulin (Fig. 4) [98]. Studies in diabetic mice indicated a 100-fold increase in transdermal insulin delivery by electroporation using the electrodes array (150 V, 120 pulses at 0.2 ms, 1 Hz) compared to passive diffusion.

The associated human studies suggested that the microelectrodes array design provided a feasible electroporation condition that was both painless and harmless to humans. Of note, the combination of mild hyperthermia (40 °C for 20 min) with electroporation resulted in an even higher delivery efficiency in mice, which is 237-fold more than the control values by passive diffusion. The delivery efficiency is consistent with pharmacodynamic studies of insulin: a significant hypoglycemic effect was observed immediately after the electroporation actuation and heating treatment that continued up to 10 h. For translation purpose, Ching et al. developed a compact, low-cost and programmable electroporation device that could easily adjust high-voltage (2–300 V) electrical waveforms including both pulsed and pulsed-biphasic forms for precise regulation of the magnitude and waveform of electroporation [99]. They also evaluated the potency of this device *in vitro* for transdermal delivery of medications including insulin.

Since the involvement of high-intensity electrical field, electroporation leads to an enhanced delivery efficiency for insulin compared to iontophoresis. However, the high-voltage pulses inevitably affect the deeper tissues, causing potential pain and muscle stimulation. Further studies on device design to minimize the side effect should be performed to facilitate clinical translation.

4. Mechanical force-triggered insulin delivery

Besides electrical field, mechanical force is another alternative to produce transient channels on the surface of the skin for transdermal drug delivery [100]. Ultrasound and jet injection are two representative mechanical force-triggered methods for insulin delivery. Ultrasound can enhance the permeability of drugs across the skin by hyperthermia or cavitation effect. Jet injection applies the high-speed liquid to disrupt the surface of the skin to dispense insulin solution within the skin tissue.

4.1. Ultrasound

Ultrasound, a longitudinal sound wave with a frequency above 20 kHz, has long been used for biomedical purposes since the beginning of the 20th century for imaging as well as to ablate tissue, shatter kidney stones, and to facilitate transdermal drug delivery [101–106]. The mechanical force produced by ultrasound has been shown to enhance skin permeability to therapeutics compounds *via* ultrasound-induced hyperthermia or cavitation [107,108]. The application of ultrasound for drug delivery through the skin is generally termed as sonophoresis, and the range of frequencies used varies between 20 kHz and 16 MHz [56,109]. Early on, high-frequency sonophoresis (HFS) (≥ 700 kHz) was mostly investigated for transdermal drug delivery, with typical skin penetration enhancements between 1 and 10 folds comparing to passive diffusion [110,111]. In the early to mid-1990s, scientists developed a better understanding of the cavitation effects for sonophoresis

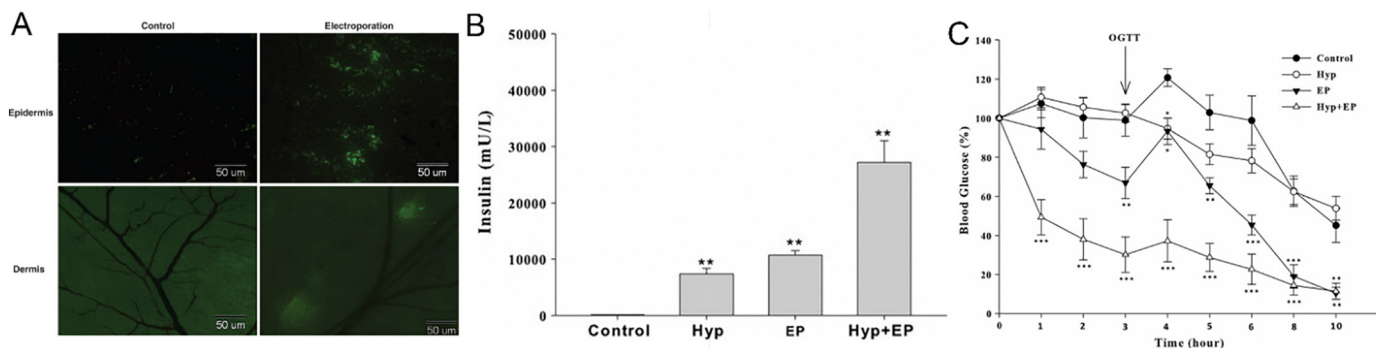


Fig. 4. Transdermal insulin delivery based on electroporation technique. A) Fluorescence image of skin treated with electroporation of FITC-insulin. B) Transport amount of insulin in mouse skin. Control: insulin occlusion only; Hyp: hyperthermia at 40 °C for 5 min before and during the 15-min insulin occlusion; EP: electroporation. C) Blood glucose levels of mice after treatment. EP (▼) (150 V, 120 pulses at 0.2 ms, 1 Hz); Hyp + EP (△) (40 ± 0.5 °C 5 min before EP and during 15-min post-pulsing); Hyp alone (○); control group (●) (insulin application only). Oral glucose tolerance test (OGTT) was performed 3 h-post EP. * $P < 0.05$, ** $P < 0.01$, *** $P < 0.001$. Adapted with permission from Ref [98].

[112] and found low-frequency sonophoresis (LFS) (20–100 kHz) was more effective than HFS in enhancing skin permeability [113,114]. Tachibana and coworkers used ultrasound with a frequency of 48 kHz or 105 kHz to yield greater transport of insulin through the skin than passive diffusion that resulted in significant decrease of BGLs in mice and rabbits [113,115]. Mitragotri et al. also showed effective LFS-mediated transdermal transport of proteins, including insulin, interferon- γ , and erythropoietin (Fig. 5) [114]. Their experiments in a diabetic rat model showed sufficient insulin delivery by LFS, with a reduction of the BGLs from ~400 to ~200 mg/dL in 30 min. A subsequent investigation demonstrated that LFS at 20 kHz was up to three orders of magnitude more effective than HFS at 1 MHz for enhancing skin permeability [116]. Since then, LFS-mediated transdermal insulin delivery has been extensively investigated [117,118]. Studies conducted by Boucaud et al. in rats and newborn pigs illustrated that the use of LFS (20 Hz) could facilitate rapid, reproducible, and reversible transdermal delivery of insulin [119,120]. They also demonstrated that the amount of insulin transported through the skin of rats was significantly associated with the energy dose and length of an ultrasound pulse, consistent with the cavitation-related mechanism [121].

Aside from using commercial, large, and heavy ultrasound equipment to deliver insulin across the skin, Smith et al. developed a portable and energy efficient transducer array for LFS-aided transdermal insulin delivery [122–128]. Specifically, this lightweight (<38 g) and compact ($56 \times 56 \times 8 \text{ mm}^3$) transducer array consisted of individual cymbal-shaped transducers, which were arranged into a multi-element array design (3×3). It also had an adjustable resonance frequency between 1 and 100 kHz, depending on the geometry. The efficacy of the portable transducer was evaluated by comparing the LFS-based insulin delivery route with subcutaneous injection route in rats [129]. The transducer was placed on top of an insulin reservoir (4 mL of 50 U/mL) that adhered to the skin of rats. Ultrasound irradiation treatment at 20 kHz with an intensity of 100 mW/cm² for 60 min resulted in a reduction of BGLs by $262 \pm 40 \text{ mg/dL}$ within 90 min; little change or less decrease ($-190 \pm 96 \text{ mg/dL}$) was observed in BGLs of rats administered with subcutaneously injected insulin (0.15, 0.2 and 0.25 U/kg). In another study, researchers assessed the effect of the cymbal transducer on Yorkshire pigs (45–64 kg) (Fig. 6) [128]. The group treated with the insulin and LFS for 60 min (20 kHz, 100 mW/cm², 20% duty cycle) showed a decrease in BGLs of $72 \pm 5 \text{ mg/dL}$ at 60 min post-treatment and a decrease of $91 \pm 23 \text{ mg/dL}$ at 90 min, indicating the feasibility of the cymbal transducer for clinical applications. In an attempt to improve the accuracy of delivered insulin doses, this team further designed a closed-loop system that allowed for on-demand delivery of insulin by coupling ultrasound-assisted insulin delivery with glucose sensing *via* a feedback controller [130]. The *in vivo* experiments were performed on 200-pound pigs, to which two ultrasound arrays were applied: one for insulin delivery (3×3 , 30 kHz, 100 mW/cm²) and the other for glucose

sensing (2×2 , 20 kHz, 100 mW/cm²). BGLs were assessed every 20 min for 2 h and the level of automatically delivered insulin was determined according to the BGLs by a proportional feedback controller. The results suggested the feasibility of using the combined cymbal ultrasound array system for noninvasive glucose sensing and insulin delivery.

Aside from stimulating insulin delivery from aqueous solution, Di et al. applied focused ultrasound (FUS) with an injectable nano-network for long-term regulation of BGLs [131]. The injectable polymeric nano-network was cross-linked by oppositely charged nanoparticles, which were prepared by coating chitosan (positively-charged) and alginate (negatively-charged) on insulin-loaded poly(lactic-co-glycolic acid) (PLGA) nanoparticles. The *in vivo* study in diabetic mice showed that after injection of the 3D nano-network, insulin was effectively released upon FUS-administration for 30 s (950 kHz, 4.31 W) with a corresponding decrease of BGLs in 10 min that reached the normoglycemic range (<200 mg/dL) in 1 h. Moreover, similar changes in BGLs were also detected under the same ultrasound treatment condition 4-day and 7-day post the injection of the nano-network, suggesting that the capability of this strategy for a long-term and pulsatile regulation of BGLs. In another study, the researchers employed chitosan microgels as the carriers to achieve the ultrasound-mediated insulin delivery [132].

More recently, Castellanos and coworkers investigated the effects of ultrasound on evoking secretory responses in pancreatic β -cells [133]. After exposure to unfocused ultrasound for 5 min at a peak intensity of 1 W/cm² and frequencies of 400 kHz or 600 kHz, a marked release of insulin was observed from β -cells (approximately $150 \text{ ng}/10^6 \text{ cells}$). Moreover, application of ultrasound at frequencies of 800 kHz resulted in $24 \text{ ng}/10^6 \text{ cells}$ releasing insulin, while retaining the cell viability. In their further study, researchers sought to elucidate the mechanism by which ultrasound stimulated secretion and described the role of calcium in the process [134]. These findings implicate the potential of ultrasound to augment insulin release from pancreatic cells for diabetes treatment.

Ultrasound-mediated transdermal drug delivery has been extensively investigated in *in vivo* animal studies and demonstrated clinical potential in small macromolecule delivery including insulin. However, HFS may lead to damage to deep skin tissue, and LFS often needs a corresponding medium or scaffold, such as hydrogel, nano-network, and cells which is invasively injected into skin tissue. Moreover, the requirement of sophisticated devices also limits the usage for people with diabetes.

4.2. Jet injection

Jet injection is another needle-free administration for transdermal insulin delivery. Instead of solid syringes, the jet injector applies a high-speed narrow stream containing insulin to create a tiny hole for

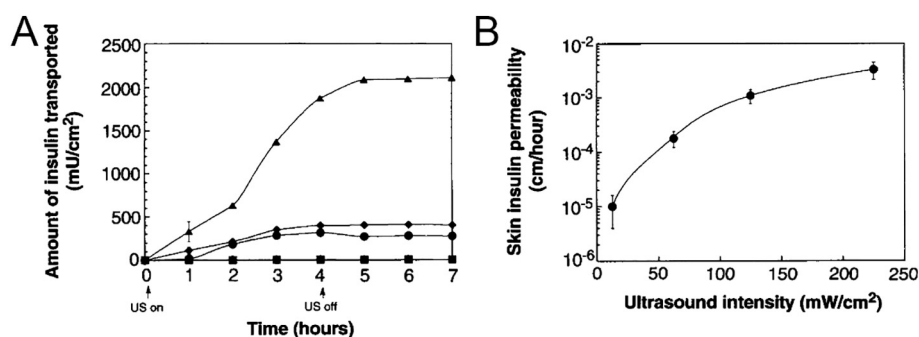


Fig. 5. Ultrasound-mediated transdermal insulin delivery. A) *In vitro* transport profile of insulin across human skin in the presence of ultrasound (20 kHz, 100-ms pulses applied every second) at 12.5 (■), 62.5 (◆), 125 (●), and 225 mW/cm² (▲) (n = 3 or 4). B) *In vitro* transdermal insulin permeability with different ultrasound intensity (20 kHz, 100-ms pulses applied every second) (n = 3 or 4). Adapted with permission from Ref [114].

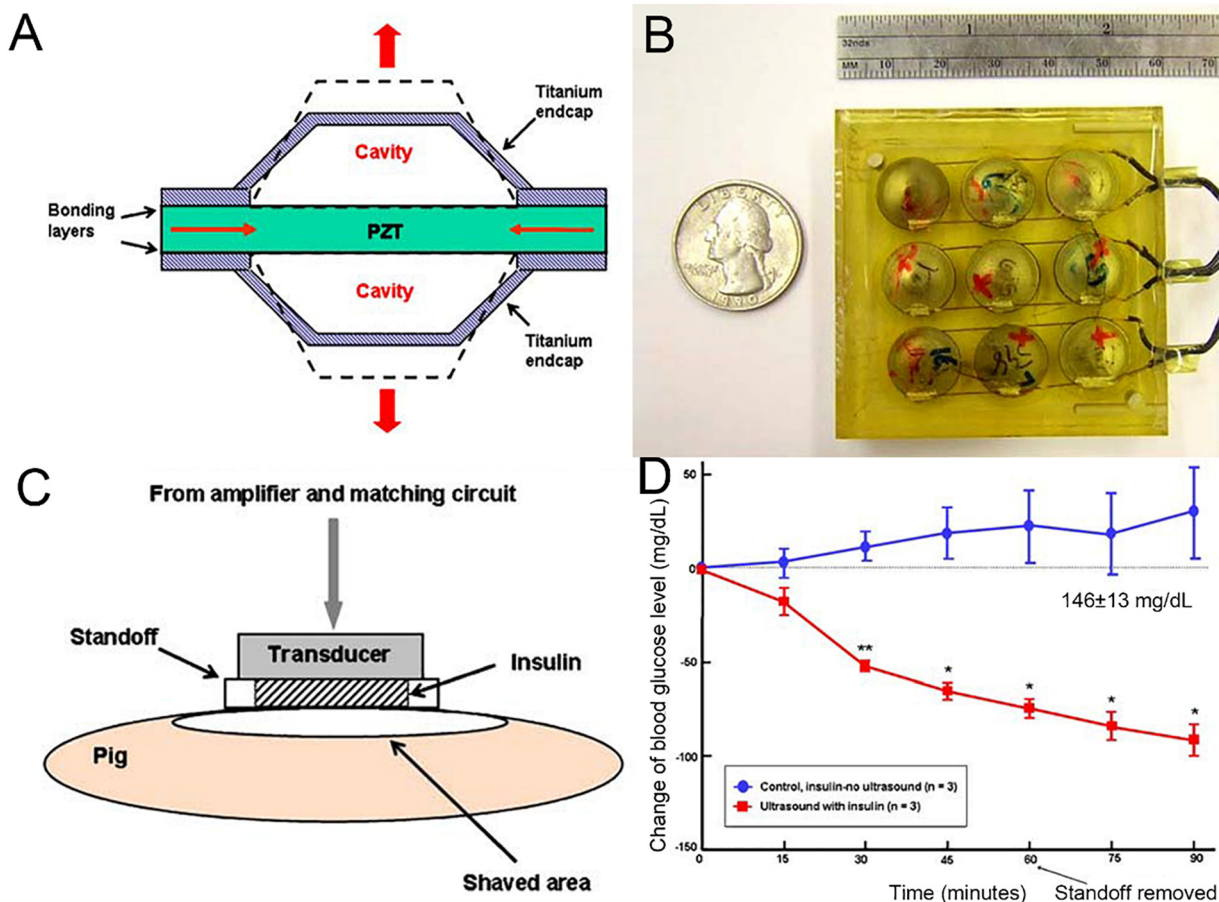


Fig. 6. Transdermal insulin triggered by a cymbal transducer. A) Schematic of the cymbal transducer and the motion of the cymbal disk. B) Photo of a 3×3 cymbal transducers array. C) Schematic of a cymbal transducers array on pig skin for transdermal insulin delivery. D) The blood glucose levels of pig treated with pure insulin or ultrasound-mediated transdermal insulin delivery ($n = 3$, $*P < 0.05$, $**P < 0.01$). Adapted with permission from Ref [128].

insulin transport through the skin [135–137]. Jet injection has been associated with high delivery efficiency exceeding 90%, similar to hypodermic injection [135,138,139]. Moreover, insulin administration by jet injectors leads to a faster on-set of plasma insulin [140,141]. Wit et al. demonstrated rapid correction of marked hyperglycemia using jet injection in overweight and obese patients with diabetes [142]. In addition, because jet injection dispenses insulin over a larger area of skin tissue than conventional injection, the pharmacokinetics of this route of insulin administration are more similar to endogenous insulin secretion by pancreas [143]. Guo et al. compared postprandial glucose control obtained using a jet injector and an insulin pen and found that the improved insulin absorption by the jet injector is beneficial for postprandial blood glucose regulation [144].

Despite the advantages mentioned above, several concerns limit the current use of jet injection technology. Although liquid jet injection technology is a needle-free route, the large volume of high-pressure spray may also lead to adverse reactions including bruising, bleeding, and pain [135,145–147]. Studies have reported that jet injectors actually cause no less pain than hypodermic needles [145,148]. To minimize the adverse reactions, Mitragotri and coworkers designed a microjet injection device that only injects solution volumes within the nanoliter range [149]. Using pulsed microjets, they reported that insulin was injected into the skin without deep penetration in a rat model, which may potentially reduce pain and bleeding. Besides, the sustained and controlled release of insulin realized by integration with biodegradable particles may also improve the application of jet injection. When Mitragotri and coworkers assessed the capability of jet injectors to deliver polymeric nanoparticles through the skin, they found the nanoparticles did not penetrate the skin deeply but could release cargoes for

prolonged periods [150]. Several jet injectors are commercially available though they have not been widely adopted. In the future, the cost, size, and performance of jet injectors may be optimized to facilitate routine usage.

5. Microneedle-assisted transdermal delivery

Recently, the emergence of microneedle (MN) techniques has provided an alternative method for transdermal protein delivery [151–156]. The micro-scaled needles are able to painlessly disrupt the stratum corneum and reach the epidermal and dermal layer for drug release [157,158]. The micro-channels caused by MN exist temporarily for drug transport but quickly recover after removal of MN to prevent long-term damage to the skin tissue [159,160]. Based on the material of the MN and the mechanism of drug delivery, the MN device is classified into different types (Fig. 7). Generally, solid MNs are designed to pierce the skin to improve the drug transport; hollow MNs are used for injection of a fluid drug formulation through the opening on the skin caused by needles, and dissolving or degradable MNs are made from polymers with encapsulated drugs. Below, we also describe recently-developed bioresponsive MNs that can respond to physiological glucose levels for on-demand delivery of insulin.

5.1. Solid microneedles

The early generation of MN-aided insulin delivery was often based on skin perforations from solid MNs, which is also termed as “poke with patch” [151]. In this approach, the MNs pierce the skin to create microchannels where insulin can be transported during the subsequent

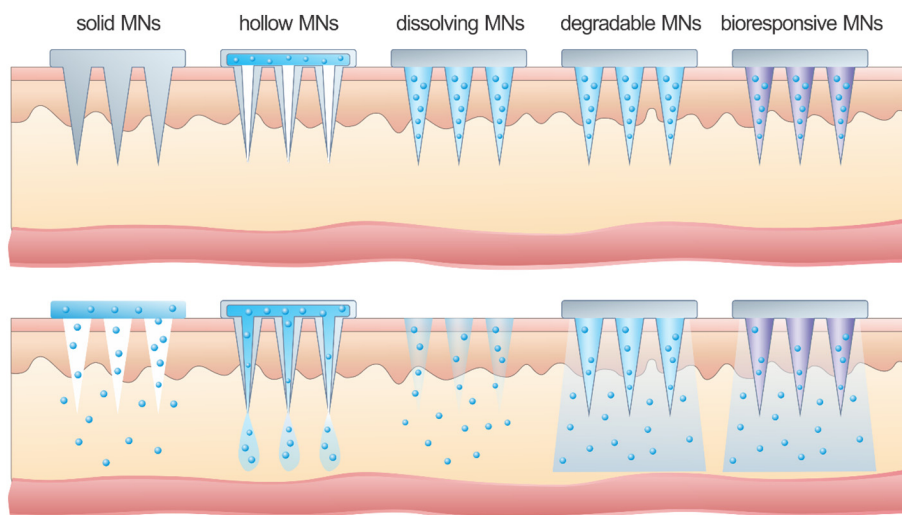


Fig. 7. Schematic illustration of delivery mechanisms through different types of MNs.

administration of a patch or topical formulation. A plethora of studies have been reported demonstrating effective delivery of insulin through the skin during the past decades.

For example, Prausnitz and coworkers demonstrated the hypoglycemic effect of insulin in diabetic rats using MNs [161]. An array of 105 microneedles was prepared by laser-cut from stainless steel sheet and inserted into the skin of diabetic rats, after which insulin solution was administered in contact of the skin for 4 h. These solid metal MNs displayed increased transdermal delivery of insulin and reduction of BGLs *in vivo* as much as 80%.

Zhou et al. evaluated the potential of using a commercially available MN roller for the transdermal delivery of insulin in a rat model, testing three different lengths (250, 500, and 1000 μm) of the stainless steel MNs [162]. Rapid reduction in BGLs was observed in 1 h after application of the MN rollers, while the glycemic effect diminished with the recovery of the skin holes that were created by MNs. MN rollers with a length of 500 μm or shorter were demonstrated to be safe and able to enhance the transdermal delivery of insulin *in vivo*. It was also reported that the reduction of BGLs could be extended by adjusting the treating area of MNs [163].

Furthermore, a combination of microneedle and iontophoresis was studied to allow a larger range of delivered drugs for transdermal delivery [164]. Chen et al. presented a 700-fold higher absorbance rate of insulin from nanovesicles driven by iontophoresis through the microchannels induced by MNs than that by passive diffusion [165]. The positively charged nanovesicles showed significant permeation ability with the assistance of MNs and iontophoresis and reduced the BGLs of diabetic rats by 33.3% and 28.3% of the initial levels at 4 and 6 h, respectively.

To control and maximize the delivered insulin dose, solid MNs were recently modified by coating payloads directly onto the surface of MNs. Al-Qallaf et al. studied the insulin concentration profiles in blood using drug-coated microneedles with different shapes and dimensions in theoretical models [166]. The simulating results indicated a maximum insulin concentration was achieved by rocket-shaped MNs.

5.2. Hollow microneedles

Hollow MNs are designed to facilitate drugs delivery into the skin through the interior of needles (Fig. 5). Prausnitz and coworkers injected insulin into the diabetic rat skin through hollow glass MNs by microinfusion, resulting in a steady drop of up to 70% of preinfusion BGLs over a 5-h period [167]. They also designed and fabricated hollow metal MN arrays for transdermal insulin delivery [168]. The mechanical study showed that these MNs were strong enough to pierce the entire

skin without breaking. In addition, silicon hollow MNs have also been explored for insulin delivery [169,170].

Nordquist, Roxhed, and coworkers developed a “controlled release”-designed MN patch integrated with an active dispensing functionality capable of controlled release of insulin in the microliter range at low flow-rates [171,172]. The electrically controlled dispenser consisted of a heater layer, an expandable composite, and a liquid reservoir. When current passed through the heater, the composite was heated up and then acted as the liquid reservoir, which could consequently eject the insulin solution through the hollow silicone MNs. In a diabetic rat model, this system was associated with a 5-times higher plasma insulin concentration compared to passive diffusion with a significant decrease in BGLs.

The delivery efficacy of hollow MNs has also been investigated in human studies. Gupta et al. first examined the transdermal delivery of insulin by hollow metal MNs on two type 1 diabetic adults [173]. An insulin pump was connected to the MNs and then applied on the abdominal skin to control the insulin infusion rate. Results demonstrated rapid insulin absorption and decline in BGLs with the insertion of MN in depth of 1 mm within the skin. Further clinical trials have also been conducting to evaluate the safety and efficiency of hollow MNs for insulin delivery in humans [174].

5.3. Dissolving microneedles

In addition to insoluble metal and silicon MNs, recent studies on biocompatible polymeric MNs have attracted significant attention, such as dissolving MNs [175]. Dissolving MNs are prepared by the soluble polymers to encapsulate the drug in the matrix, and upon inserted into the skin, can fully dissolve to release the drug. The therapeutic duration is dependent on the dissolution rate of the polymer material, which can be adjusted from minutes to hours to meet the goals of treatment [176]. Furthermore, the use of the biocompatible polymers could avoid any production of sharp biohazardous waste. [177,178].

To date, various dissolving MNs made of sugar glass polymers have been reported, such as maltose [179–182], trehalose [183–186] and sucrose [187,188]. Sugar glass MNs typically dissolve quickly in human skin after insertion [189,190]. However, the fabrication of these MNs requires a high temperature that over 100 °C to induce rubber to glass transitions of sugar glasses, which may damage the bioactivity of biomolecules including insulin [191]. New fabrication techniques have been developed to address the thermal challenges of melting fabrication process. For example, Martin et al. used a low-temperature processing method to fabricate dissolving MNs [187].

Another strategy could be using other polymers with high solubility to form MNs, such as hyaluronic acid (HA) [192–196], carboxymethylcellulose (CMC) [183,197], chitosan [198,199], alginate [200,201], polyvinylpyrrolidone (PVP) [202–205], and polyvinyl alcohol (PVA) [206–208]. The associated fabrication process can avoid high-temperatures, thereby enhancing the storage ability of drug-containing MNs. Liu et al. fabricated HA MNs *via* micromolding technology and characterized their application in the transdermal delivery of insulin [209]. >90% of the loaded insulin retained bioactivity, even after one month-storage at different temperatures (–40, 4, 20 and 40 °C). Moreover, the HA MNs exhibited higher resistance to deformation against humidity than sugar glass MNs. *In vivo* studies in diabetic rats demonstrated a dose-dependent hypoglycemic effect after administration with insulin-loaded HA MNs. Furthermore, the transient microchannel caused by the insertion of MNs disappeared within 24 h.

Chen and coworkers developed a dissolving MN patch composed of starch and gelatin for transdermal insulin delivery [210]. Here, gelation was blended with starch to produce tough and strong composited MNs that was suitable for skin penetration due to its film-forming ability. *In vitro* and *in vivo* penetration tests verified the sufficient mechanical strength of MNs to be inserted into porcine or rat skin with a depth of approximately 200 μm . The mild solvent casting process for MN fabrication preserved the activity of encapsulated insulin which was able to induce a significant decline in BGLs of diabetic rats upon insertion.

Furthermore, the relative availability and bioactivity of insulin were still higher than 90% after one-month storage at 25 or 37 °C, suggesting that these dissolving starch/gelatin MNs could be a promising device for delivery of biomolecules.

Although many formulations of dissolving MNs have been shown to successfully delivery insulin and reduce BGLs *in vivo*, incomplete insertion of polymeric MNs due to skin elasticity limits their delivery efficiency and also causes wastage of valuable medication [211]. To this end, researchers designed fully insertable MNs with a supporting structure that provided an extended length for counteracting skin compressive deformation during administration [212]. In this study, insulin was first loaded on tips of 600 μm -high MNs made of poly- γ -glutamic acid, while the second layer of PVA/PVP was filled in the MN molds to form the 600 μm -high supporting structures (Fig. 8). When inserted into the skin, both the MNs and supporting layer dissolved within 4 min to fully release the drug load. A comparable hypoglycemic effect was detected in diabetic mice treated the same dose of insulin (0.2 IU) *via* MN patches *versus* subcutaneous injection, indicating the feasibility and accuracy of using this proposed MN design for insulin delivery.

Based on a similar mechanism, Liu and coworkers developed multi-layered dissolving MN patches composed of stiff silk fibroin MN tips supported on flexible PVA pedestals [213]. The tips had a robust mechanical strength and were able to penetrate the skin and rapidly dissolve to release encapsulated insulin. *In vivo* tests in an obese mouse

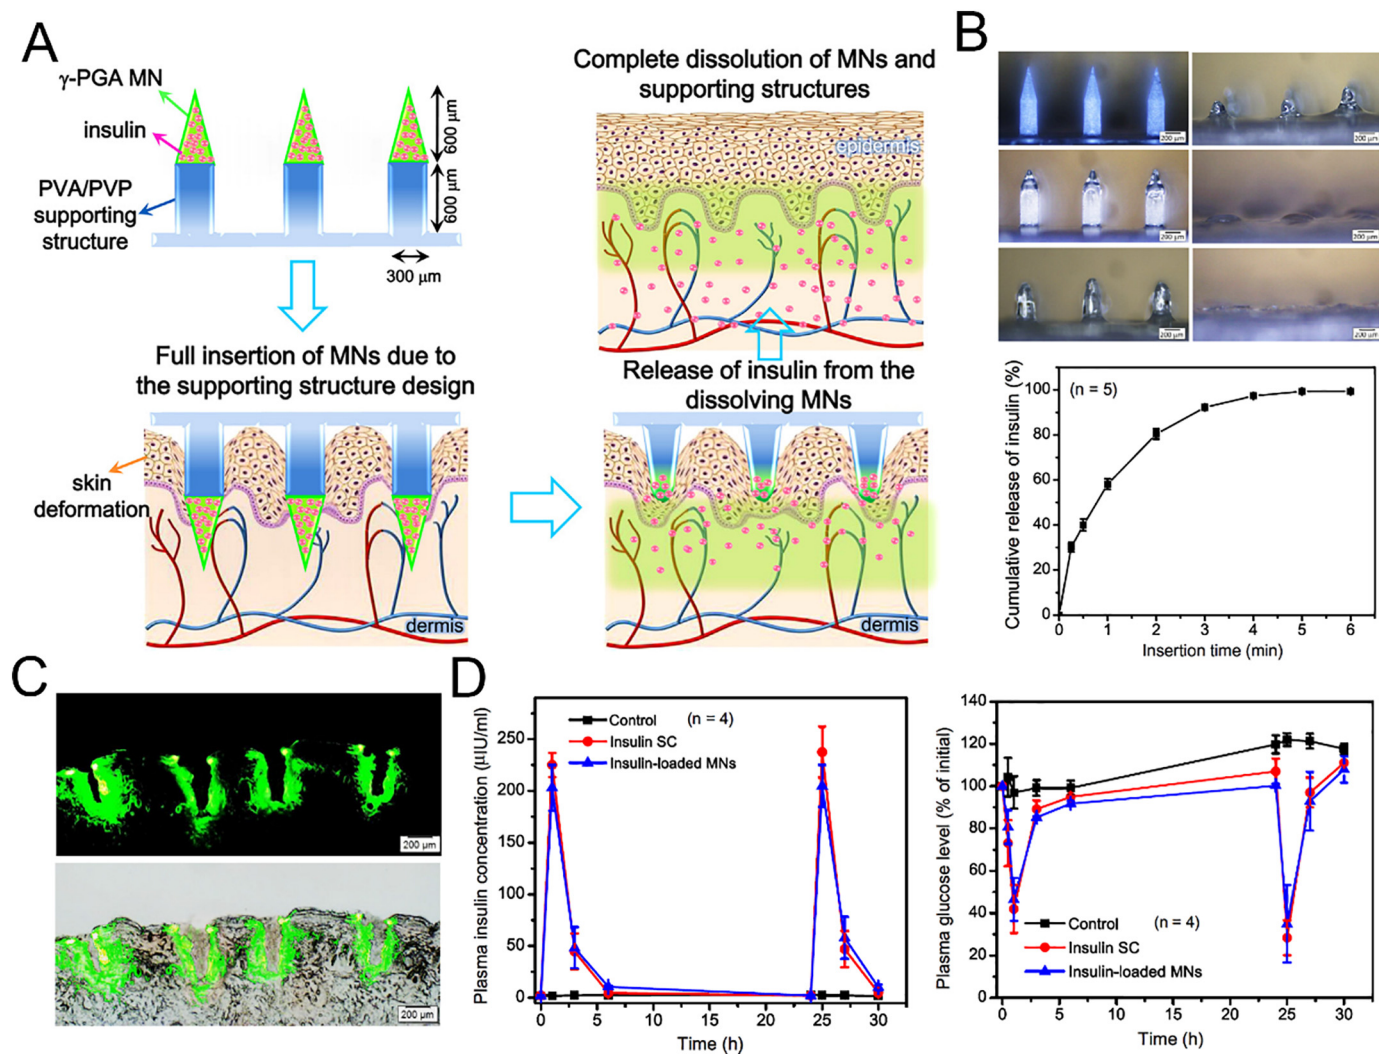


Fig. 8. Transdermal delivery of insulin using a fully insertable MN system. A) Schematic of MNs composed of poly- γ -glutamic acid (γ -PGA) MNs and PVA/PVP supporting structures. B) *In vitro* release profile of insulin from MNs (n = 5). C) Fluorescence images of skin puncture sites. D) Plasma insulin concentrations (left) and plasma glucose levels (right) of diabetic rats treated with unloaded (control) and insulin-loaded MNs and subcutaneous injection of insulin (insulin SC) (n = 4). Adapted with permission from Ref [212].

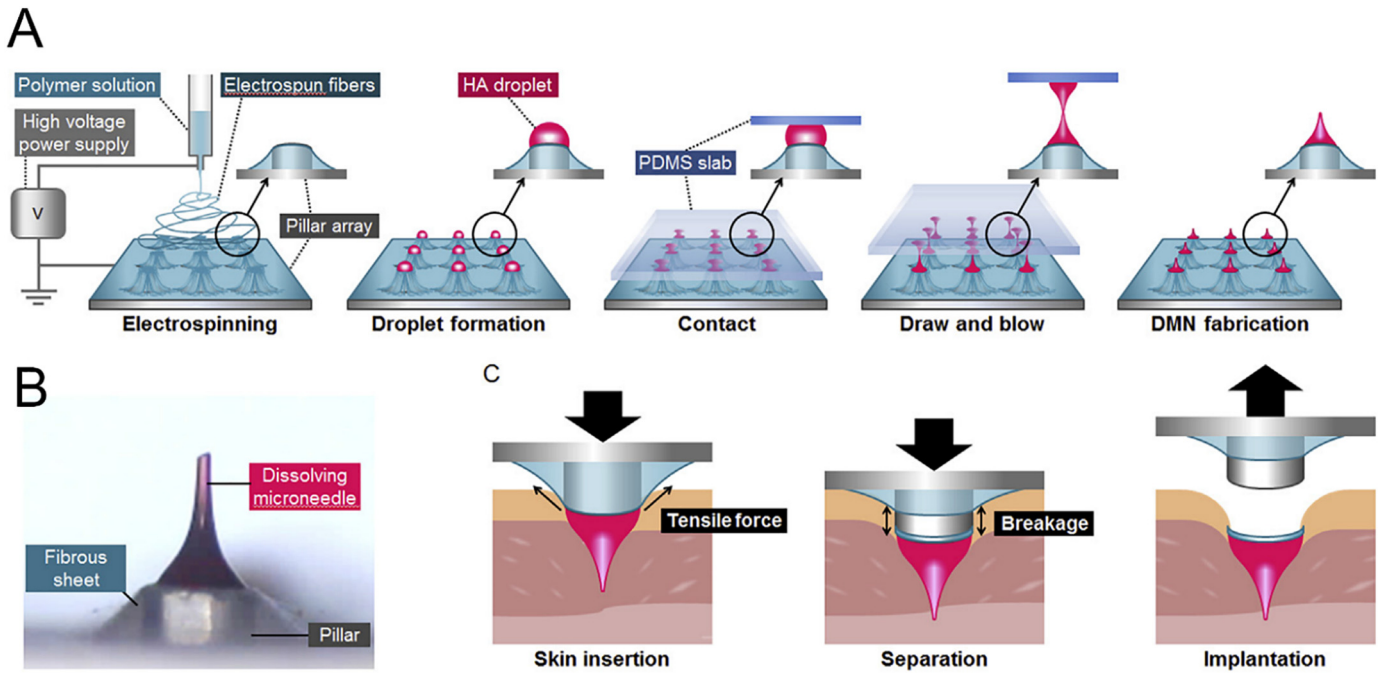


Fig. 9. Transdermal MN based on droplet-born air blowing (DAB) technique. A) Schematic of MN fabrication. B) Rapid implantation of MN in the skin including insertion, separation, implantation steps. Adapted with permission from Ref [217].

model indicated rapid insulin absorption through the skin into the systemic circulation, where maximum serum insulin concentrations were reached 2 h-post MN administration. The MN patch could also be stored at room temperature for 20 days, with >99.4% of insulin remained in the

MNs. In this MN design, the multilayered fabrication process may condense therapeutics to reduce wastage, as well as satisfy different mechanical performance requirements for tips and pedestals. Following this rationale, two-layered MNs made from diverse materials with

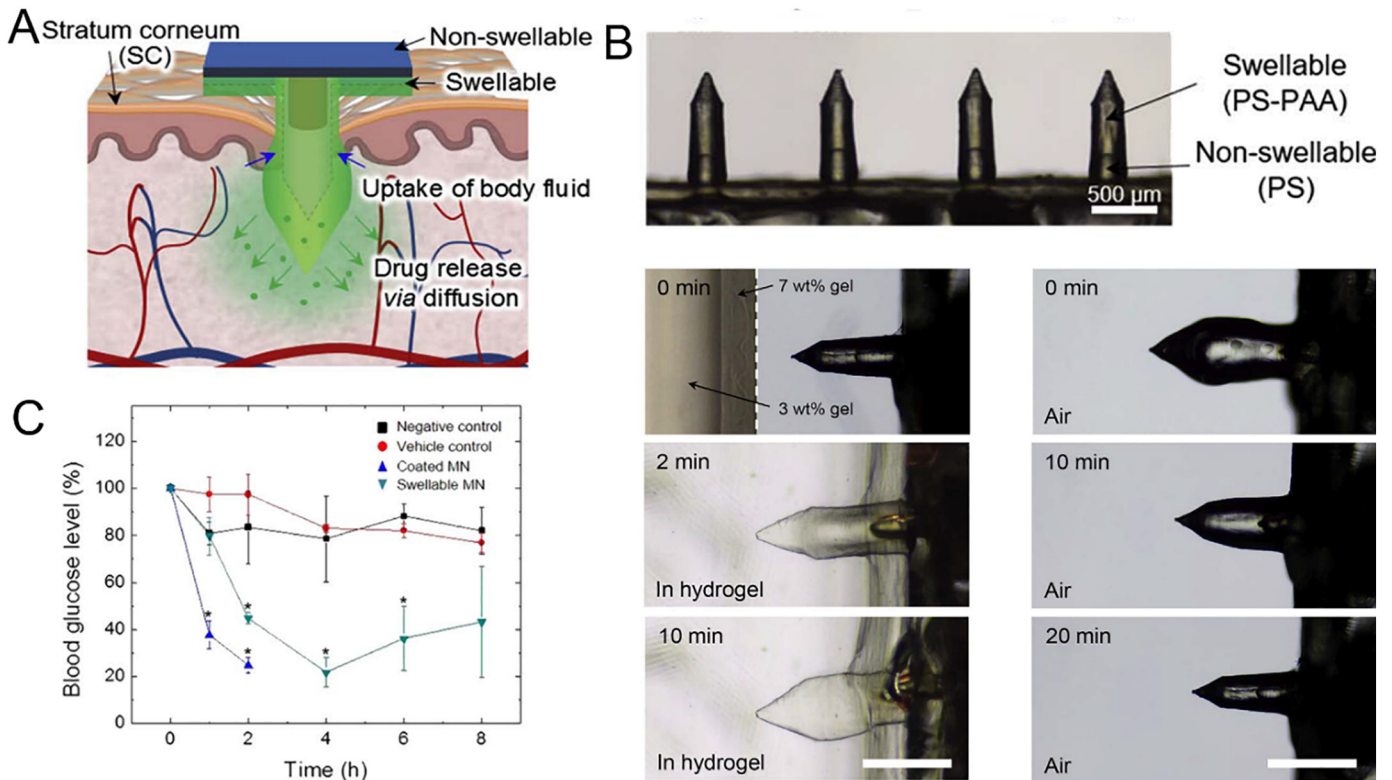


Fig. 10. Swellaible MN for transdermal insulin delivery. A) Schematic of a water-swellaible MN for mechanical interlocking with skin and drug release through passive diffusion. B) Swelling/deswelling behavior of the MN in gel and air respectively. Scale bar: 500 μm . C) Blood glucose levels of normal mice treated with (▼) 10 U insulin-loaded swellaible MN patches (swellaible MN), (▲) 10 U insulin-coated MN patches (coated MN), and (●) non-insulin-loaded swellaible MN (vehicle control) ($n = 3$). Normal untreated mice (■) were used as a negative control ($*P < 0.01$). Adapted with permission from Ref [222].

different ratios have been assessed for optimized insulin delivery efficiency [214,215]. Lee et al. analyzed the penetration ability of MNs consisting of several ratios of PVP with two molecular weights (PVP10/PVP360) and found the ratio of 1:3 was the best for *in vivo* insulin delivery [214]. The backing layer prepared from PVP360/CMC was selected for better flexibility for skin fitting other than pure PVP360 supporting. To further strengthen the mechanical property of MNs, Liu et al. fabricated composite MNs integrating PVP matrix with insulin-loaded CaCO₃ microparticles [216]. The prepared MNs exhibited enhanced stiffness and slower solubility compared to pure PVP MNs.

Traditionally, dissolving MNs are mostly fabricated using micro-sieve molds through a stepwise casting method. Kim et al. developed an alternative fabrication technique by applying droplet-born air blowing

(DAB) to directly shape the polymer droplets to solidified the MNs, thereby providing benign (4–25 °C) and fast (<10 min) fabrication conditions without drug loss [218]. In this method, biopolymer droplets were first dispensed on the flat surface for MN base fabrication, and a second layer of drug-containing droplets was additionally dispensed for MN tip fabrication. Thereafter, an upper plate was used to elongate the droplets by drawing. Throughout this process, the MNs were solidified using air blowing, where the size of the MNs and the amount of loaded insulin could be tailored by the pressure and time of droplet dispenser. A decrease in BGLs in diabetic mice and quantitative bioavailability (96.6 ± 2.4%) data confirmed the efficacy of insulin delivery associated with this fabrication method. This technology may also provide multiple options with regards to the materials for fabrication of

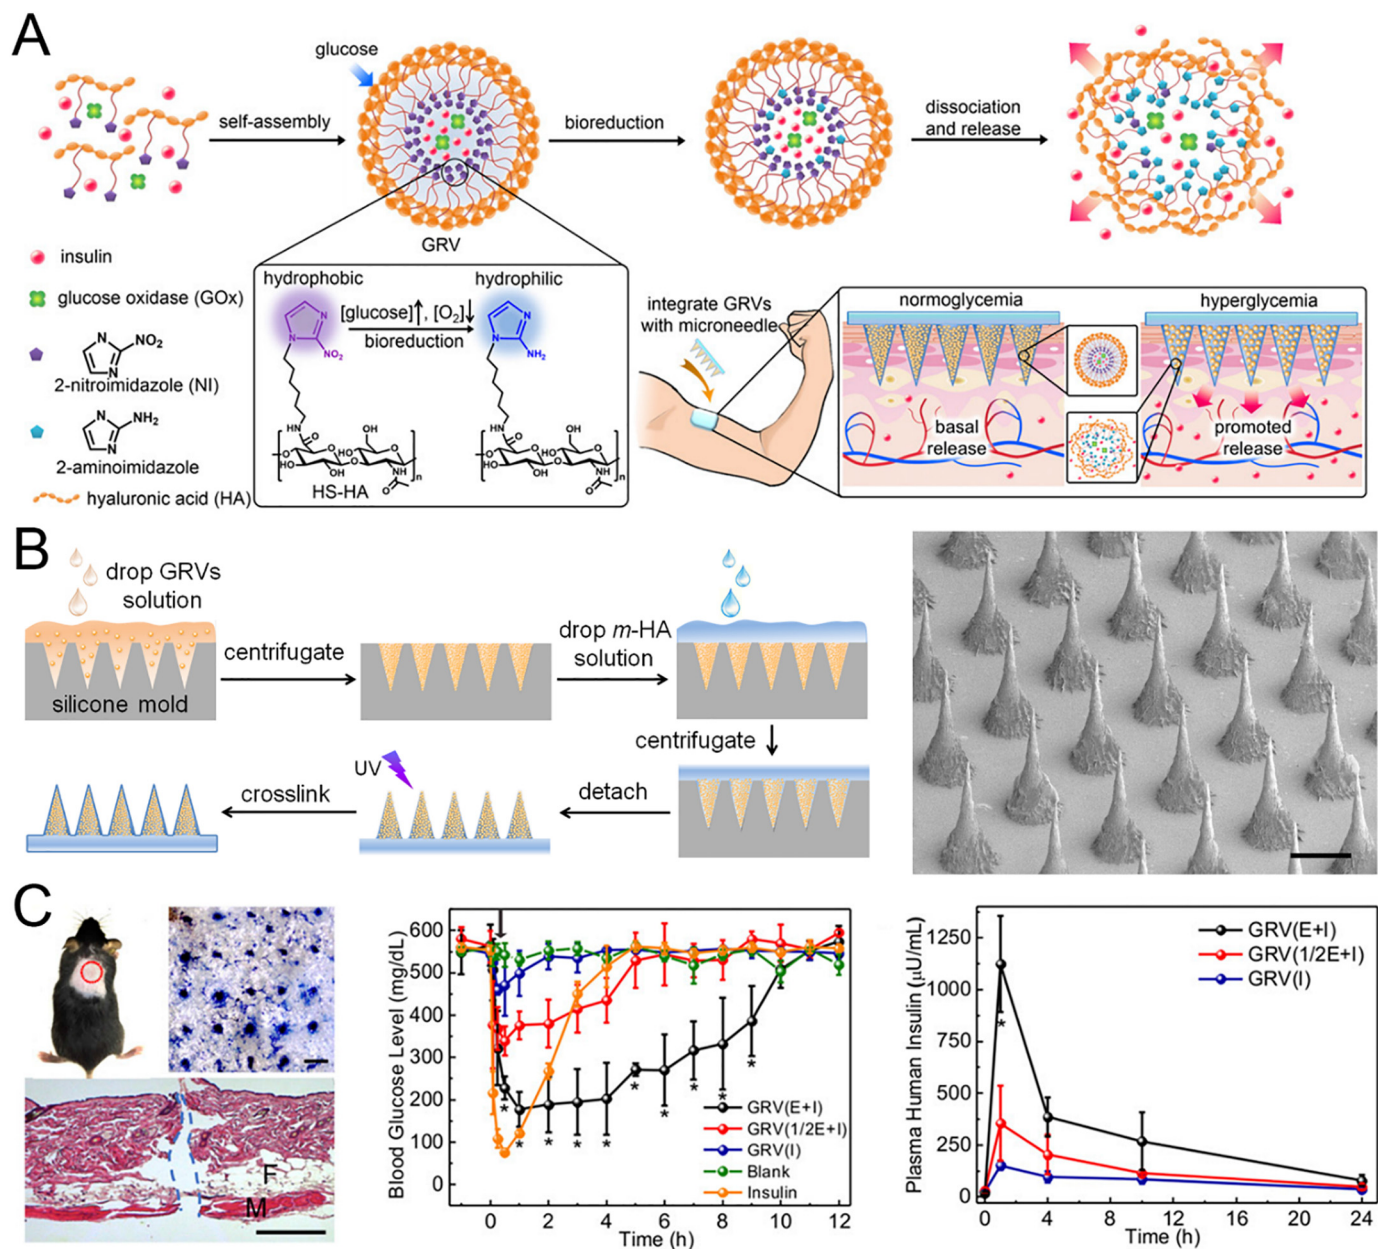


Fig. 11. A representative transcutaneous MN patch loaded with glucose-responsive nanoformulations. A) Schematic showing the formation and mechanism of GRV-containing MN-array patch for *in vivo* fast insulin delivery triggered by a high blood glucose level. B) Fabrication process (left) and SEM image (right) of the MN patch. C) *In vivo* administration of MN-array patch in STZ-induced type 1 diabetic mice: Photograph showing penetration of mouse skin by MNs Scale bar: 500 μm (Left); BGLs (middle) and plasma insulin levels (right) of diabetic mice after treatment with blank MNs containing only cross-linked HA, MNs loaded with human recombinant insulin, MNs loaded with GRV(E + I), MNs loaded with GRV(1/2E + I), or MNs loaded with GRV(I). *P < 0.05 for administration with GRV(E + I)-loaded MNs compared with GRV(1/2E + I)-loaded MNs or GRV(I)-loaded MNs. Adapted with permission from Ref [234].

dissolving MNs, including HA, CMC, and PVP, while the layered structure enabled minimized wastage of therapeutics. To further overcome incomplete drug delivery, Yang et al. recently reported an electrospun pillar array-assisted MN delivery which allowed rapid implantation of MNs into the skin [217]. The pillar array was first coated with an electrospun fibrous PLGA sheet, after which dissolving HA droplets were dispensed on each pillar to shape MNs *via* DAB (Fig. 9). The resulting MNs on the electrospun pillar array was quickly separated from the porous fibrous substrate within 10 s once completely inserted into the porcine skin due to the tensile breakage of the fibrous sheet during the compression. The

hypoglycemic effect of insulin-loaded MN device was demonstrated *in vivo* using a healthy mouse model.

Besides employing multilayered MNs to enhance delivery efficiency, Garland et al. investigated the incorporation of polymeric MNs with iontophoresis to improve the bioavailability of insulin and showed that a synergistic enhancement of insulin release was achieved when iontophoresis was applied in combination of the soluble poly(methyl vinyl ether-*co*-maleic acid) (PMVE/MA) MN arrays [219]. Furthermore, their results revealed that the incorporation of electric current could facilitate the permeation of protein within the entire MN patch rather than the MN alone, thus increasing the delivery efficiency.

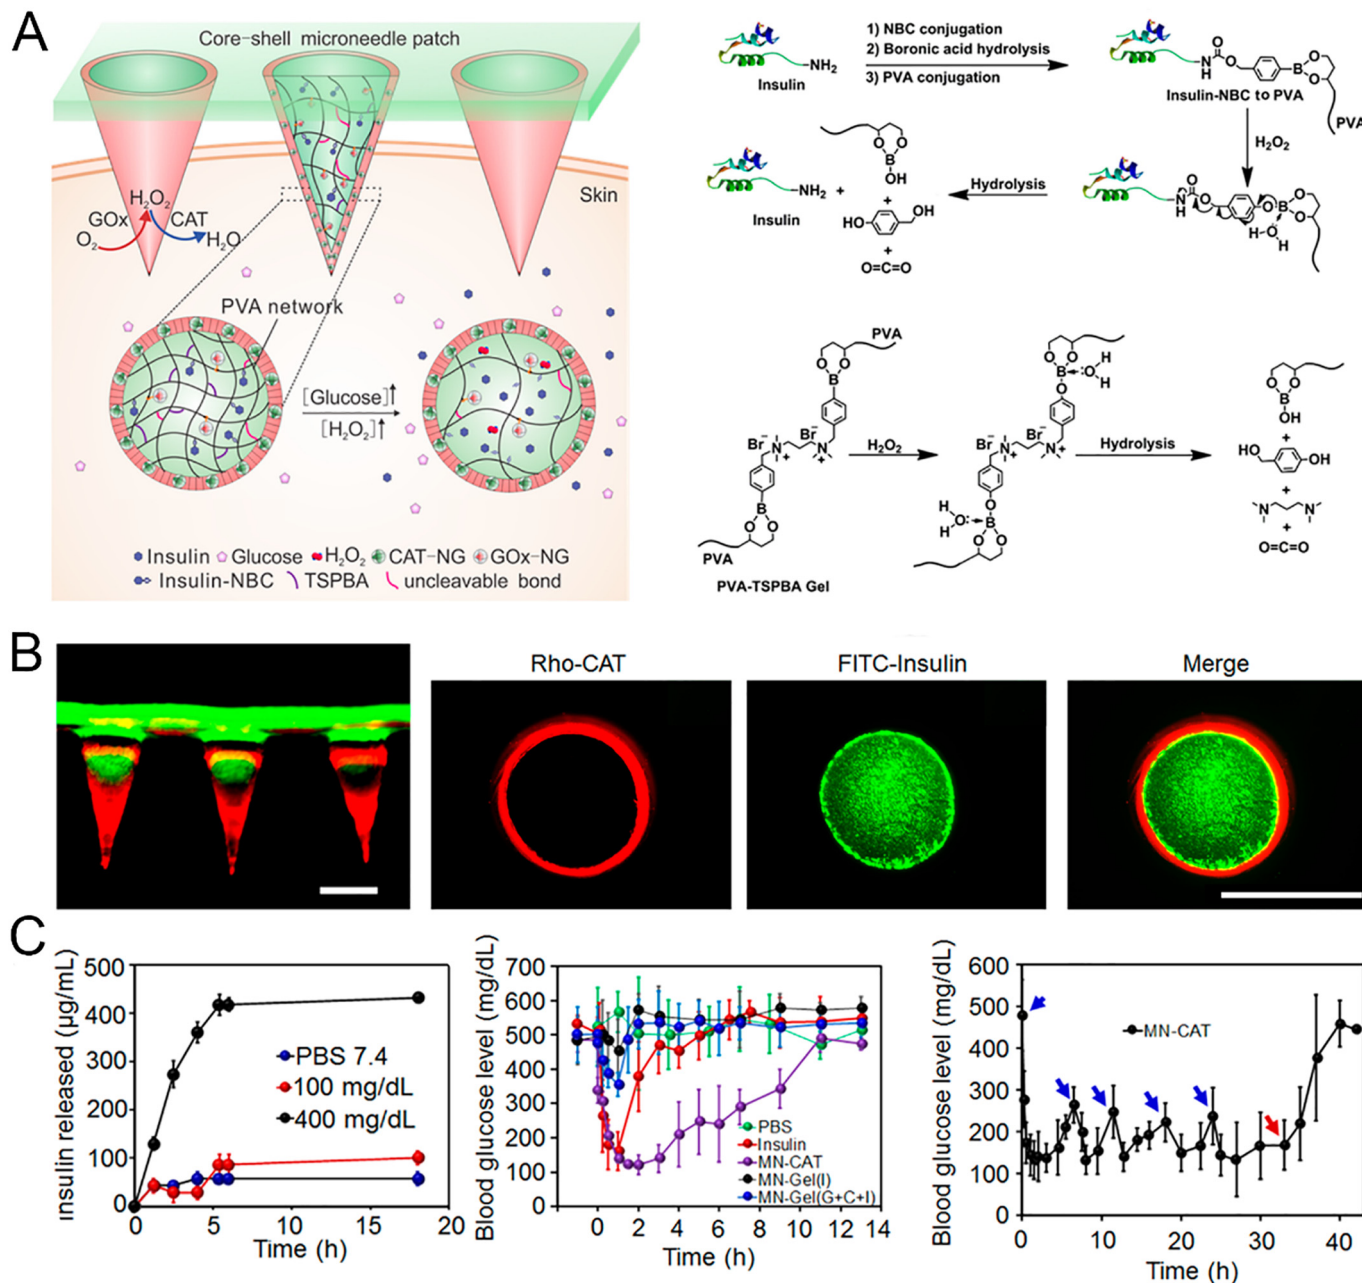


Fig. 12. Glucose-responsive matrix-loaded MN for controllable insulin delivery. A) Schematic of the glucose-responsive insulin delivery system using H₂O₂ responsive PVA-TSPBA gel. B) Fluorescence images of rhodamine B-labeled insulin-loaded MN arrays with FITC-labeled HA base (left) and a cross-section of MN containing rhodamine B-labeled CAT shell and FITC-labeled insulin core (right). Scale bar: 300 μm. D) *In vitro* release profile of insulin from gels in PBS 7.4 in the presence of GOx (0.2 mg/mL). *n* = 3 (left); Blood glucose levels of diabetic mice treated with different kinds of MN array patches, *n* = 5 (middle); Blood glucose levels of diabetic mice treated with multiple MN array patches. The administration of MN-CAT is indicated by blue arrows. MNs were removed as indicated by red arrows, *n* = 5 (right). Adapted with permission from Ref [243].

5.4. Degradable microneedles

The release dynamics of payloads from dissolving MNs is closely associated with the dissolution rate of polymers, which is usually fast. For protein drugs that require continuous delivery to maintain a constant therapeutic dose, MNs with a longer degradation period are preferred as the delivery device [177]. Polymers with a higher molecular weight and crosslinking density have been shown to provide extended release of insulin as well as mechanical properties of MNs [175,220]. Drug is gradually released from biodegradable MNs through passive diffusion during the degradation process, while swelling of MNs may also accelerate drug diffusion. For instance, calcium ion cross-linked alginate/maltose composite MNs were explored for insulin delivery, where maltose was included to improve the mechanical strength of the MN [221]. The resultant biodegradable MNs exhibited a mechanical strength around 0.41 N/needle and rapidly swelled in 5 min with eventual dissolution in 40 min. The insulin-loaded MNs revealed a sustained decline in BGLs of diabetic rats and maintained the pharmacological activity of insulin with a longer period compared to the group subcutaneously injected the same dose of insulin. Yang and coworkers designed a swellable MN patch that could self-adhered in the skin for prolonged release of insulin (Fig. 10) [222]. The double-layered MN patch consisted of swellable PS-PAA MN tips that could swell by absorbing body fluids after insertion into skin and a non-swellable PS layer. The *in vitro* insulin released from the MNs presented a more sustained manner over 12 h without burst release. In contrast, >90% of the insulin was released from the coated MNs. Consistent with the release behavior, this swellable MN platform provided an extended hypoglycemic effect in normal mice that lasted up to 8 h. The Jin group developed a phase-transition MN patch from PVA for transdermal insulin delivery [223]. The microcrystalline crosslinking allowed the MN to swell, but not dissolve, upon insertion into the skin, thus leading to a sustained insulin release from the patch. *In vivo* studies in a diabetic pig model demonstrated transdermal bioavailability that exceeded 20%. Meanwhile, the glycated hemoglobin of pigs treated with the patches continuously for 2 months was lower than those treated with the insulin pen, indicating the insulin patches provided a better blood glucose

regulation capability. In another recent study, Di et al. integrated a stretchable MN patch for tensile strain-triggered transdermal delivery of insulin [224]. The elastomer patch embedded insulin-loaded microgel depots inside deformed under mechanical stretch to promote the release of payloads, which further diffused into the cross-linked HA microneedle for transdermal delivery. *In vivo* studies demonstrated effective reduction of BGLs in diabetic mice administered with this stretchable device.

Lately, bioceramics have attracted increasing interest in the field of transdermal drug delivery due to their attractive biocompatibility and strong mechanical properties. For example, the flexible porous structure of bioceramics and the electrostatic interaction between the ceramic surface and the biotherapeutics suggest promise for bioceramics to transporting biomolecules. Yu et al. prepared organic-inorganic bioceramic composite microneedles MNs made from gelatin and hydroxyapatite for extended transdermal insulin delivery [225]. Hydroxyapatite, which has a similar chemical composition as human hard tissues, is considered as a biodegradable ceramic that has been widely used in the biomedical application. The MNs composed of cross-linked gelatin and incorporated with hydroxyapatite provided sufficient mechanical strength to penetrate human skin and exhibited an effective hypoglycemic effect and extended plasma insulin release compared with that of subcutaneous injection in diabetic rats. The researchers also characterized calcium sulfate and gelatin composite MNs, which also presented similar behaviors in transdermal delivery of insulin [226].

5.5. Bioresponsive microneedles

Recently, extensive efforts have been devoted to achieving glucose-responsive smart insulin delivery [15,17,18,227–230]. Bioresponsive MNs that can respond to the physiological signals have been spotlighted as a promising approach for glucose-regulated insulin delivery [231–233]. This platform generally integrates glucose-responsive components with polymeric MN matrix.

In 2015, Yu et al. reported a glucose-responsive MN patch composed of cross-linked HA matrix and hypoxia-responsive vesicles (GRVs) as a

Table 1
Representative transdermal strategies for insulin delivery.

Strategies	Approaches	Advantages	Limitations
Chemical Enhancers	Disrupt the skin structure to increase permeability and improve drug solubility to provide the drug concentration-gradient driving force	<ul style="list-style-type: none"> Increased skin permeability and insulin absorption Improved patient satisfaction over injection 	<ul style="list-style-type: none"> Limited transdermal delivery efficiency of macromolecule drug-insulin Potential skin irradiation Lack of robust controlled drug dosage
Iontophoresis/Electroporation	Alter permeation of cell walls	<ul style="list-style-type: none"> Enhanced insulin penetration over passive transport Improved patient satisfaction over injection Allowing strict control of delivery period 	<ul style="list-style-type: none"> Iontophoresis could be time-consuming to administer Potential cell damage or rupture after membrane discharge by electroporation Lack of robust controlled drug dosage
Ultrasound	Generate hyperthermia or cavitation effect to increase permeability of cell membrane	<ul style="list-style-type: none"> Enhanced insulin penetration over passive transport Allowing strict control of delivery period Reduced immunization reaction Improved patient satisfaction over injection 	<ul style="list-style-type: none"> Requirement of sophisticated devices Potential physical damage to skin tissue Lack of robust controlled drug dosage
Jet injection	Deliver solution of insulin into skin powered by high-pressure gas	<ul style="list-style-type: none"> Improved insulin absorption over injection as jet injection dispenses insulin over a larger area of skin tissue Reduced immunization reaction 	<ul style="list-style-type: none"> Potential bruising, bleeding, and pain due to high-pressure spray
Microneedle	Insert into skin to enhance skin permeability or directly deliver drug by micro-scaled needles	<ul style="list-style-type: none"> Relative higher transport efficiency than other strategies by directly carrying insulin into the dermis layer Home friendly administration method Improved patient satisfaction over injection Controllable drug release rates 	<ul style="list-style-type: none"> Potential breakage of needle Toxicity concern of needle materials Potential skin irradiation or/and infection

Table 2
Representative clinical trials of transdermal insulin delivery.

Formulation	Study	Subjects	Primary Outcome Measures	Status	Phase	Related publication
Microporation	Transdermal Basal Insulin Patch Study in Type 1 Diabetes • (NCT00519623)	<ul style="list-style-type: none"> • T1D >10 years • Age 18–65 years • BMI 18.5–32 kg/m² • HbA1c ≤9.0% • C-peptide negative 	PK and PD of the PassPort(R) Transdermal Insulin Delivery System in Type 1 Diabetes Patients	Completed	Phase 1/2	[250]
A stable anhydrous insulin solution	Transdermally Delivered Human Insulin Product • (NCT03544996)	<ul style="list-style-type: none"> • 1 male, brittle T1D patient with poor insulin sensitivity requiring >3000 IUs on insulin a day 	Measurement of down modulation of serum glucose not otherwise attributable to injected insulin	Completed		
Jet injection	Insulin by Jet-injection for Hyperglycemia in Diabetes • (NCT01947556)	<ul style="list-style-type: none"> • Age 60–61 • T1D or T2D • Age 18–75 years • BMI 25–40 kg/m² • HbA1c 6.5–10% 	The time in minutes until plasma glucose concentration has dropped with ≥10 mmol/L	Completed		[142]
	Reliability of Insulin by Jet Injection • (NCT02272296)	30 participants	The variability in time until maximal glucose lowering effect to maintain normoglycemia, after insulin injection; Time to maximal exogenous glucose infusion rate (GIR, in mL/min) required to maintain euglycaemia.	Completed	Phase 4	[251]
	Pharmacology of Insulin Injected With Jet-Injection • (NCT00983775)	<ul style="list-style-type: none"> • Age 18–50 years • BMI 18–32 kg/m² • Blood pressure < 160/90 mmHg 	Maximal glucose infusion rate: 0–8 h after insulin injection	Completed		[252]
	Pharmacokinetic and Pharmacodynamic Profile of Insulin Lispro Using Needle-Free Jet Injection Technology • (NCT02443714)	<ul style="list-style-type: none"> • T1D >1 year • Age 18–50 years • BMI 18–28 kg/m² • HbA1c 6.5–9.0% • Blood pressure < 160/90 mmHg 	Early insulin exposure: AUC 0(of insulin from 0 to 30 min	Completed	Phase 4	[141]
	Pharmacology of Insulin Injected With Jet-injection in Diabetes • (NCT01438632)	<ul style="list-style-type: none"> • Age 18–40 years • Height 170 ± 10 cm. • Weight ± 10%kg • Liver and renal function should be normal • Health subjects with no chronic diseases or medications 	AUC from time 0 to 2 h after insulin injection and meal ingestion	Completed	Phase 4	[140]
		24 participants				
		<ul style="list-style-type: none"> • Duration of diabetes >1 year • Age 18–70 years • BMI 18–32 kg/m² • HbA1c 6.0–9.0% • Insulin use at least once daily or with subcutaneous pump • Blood pressure < 160/90 mmHg 				
Microneedle	A Pilot Study to Assess the Safety, PK and PD of Insulin Injected Via MicronJet or Conventional Needle (MicronJet) • (NCT00602914)	<ul style="list-style-type: none"> • 23 males • Healthy: • Age 18–40 years • BMI <30 kg/m² 	Blood samples for PK and PD	Completed	Early Phase 1	[174]
	Pharmacokinetics/Dynamics of Basal (Continuous) Insulin Infusion Administered Either Intradermally or Subcutaneously • (NCT01061216)	<ul style="list-style-type: none"> • Age 30–70 years • BMI <35 kg/m² • HA1c 6.5–10% • 20 T1D males • Age 18–55 years • BMI ≤32 kg/m² 	Insulin measurements will be used to compute PK model parameters	Completed	Phase 1/2	
	Multi-day (3) In-patient Evaluation of Intradermal Versus Subcutaneous Basal and Bolus Insulin Infusion • (NCT01557907)	<ul style="list-style-type: none"> • 23 participants • T1D for at least 1 year • Ages 18–55 years • BMI ≤ 32 kg/m² • HbA1c ≤ 8.0% 	t _{max} of insulin delivered intradermally as compared to subcutaneously after a meal bolus.	Completed	Phase 1/2	


Table 2 (continued)

Formulation	Study	Subjects	Primary Outcome Measures	Status	Phase	Related publication
	Study	20 participants	Aggregate mean difference in t_{\max}	Completed	Phase 1/2	
	Transdermal Basal Insulin Patch Study in Type 1 Diabetes	30 males	AUC of the blood glucose profile after the meal	Completed	Phase 2	[253]
	• (NCT00519623)	• T1D > 1 year • Age \geq 18 years				
	Transdermally Delivered Human Insulin Product	16 participants	Average t_{\max}	Completed	Phase 2/3	[254]
	• (NCT03544996)	• T1D 1–15 year • Ages 18–55 years • BMI < 32 kg/m ² • HbA1c \leq 9.0%				
		• T1D > 2 year • Age 8–18 years • BMI \leq 85% for age • HbA1c \leq 8.5%				

T1D: type 1 diabetes; T2D: type 2 diabetes; BMI: body mass index; HbA1c: hemoglobin A1c; PK: pharmacokinetic; PD: pharmacodynamic; AUC: area under curve; t_{\max} : time to peak insulin concentration.

Data obtained from <https://clinicaltrials.gov/>.

“smart insulin patch”, representing a painless and self-regulated modality (Fig. 11) [234]. The GRVs were self-assembled by the hypoxia-sensitive hyaluronic acid derivative (HS-HA), which contained a hypoxia-sensitive group, 2-nitroimidazole (NI). Under reductive conditions, the hydrophobic NI on HS-HA is reduced to hydrophilic 2-aminoimidazole, inducing the disassembly of the nanovesicles. The GRVs encapsulating insulin and glucose oxidase (GOx) were then deposited in the MNs to sense the elevated blood glucose level in the dermis. GOx, an enzyme that can convert glucose to gluconic acid, has been widely applied as a glucose-sensing element [227,235].



During the GOx-catalyzed oxidation of glucose, oxygen in the body fluid was consumed, leading a localized hypoxic environment [236]. The enzyme-induced hypoxic microenvironment further actuated the dissociation of GRVs as a result of bioreduction of HS-HA and led to subsequent insulin release. The hypoxia-responsive GRVs were able to rapidly release insulin in the presence of glucose and quickly reduced the BGLs of type 1 diabetic mice to around 200 mg/dL within 0.5 h with maintenance in a normal range for up to 4 h. Moreover, the administration of an additional patch was able to prolong the treatment period, while avoiding the risk of hypoglycemia.

In addition to an enzymatically-generated hypoxic or the acid environment, the generation of H_2O_2 during the reaction can also act as a trigger to promote insulin release from MNs [237]. Hu et al. reported bioresponsive MNs incorporated with polymeric vesicles (PVs) [238]. The PVs were prepared by self-assembly of a block copolymer composed of polyethylene glycol (PEG) and phenylboronic ester (PBE)-conjugated polyserine and further loaded into MN patch. In the presence of high glucose levels, the enzymatically-produced H_2O_2 oxidized the PBE pendant, leading to the disassociation of PVs and delivery of insulin through polymeric MN matrix. In this system, the release profiles responding to glucose could be modulated by adjusting the amount of GOx. The integration of H_2O_2 -responsive PVs with MNs displayed the capability of self-regulating BGLs in a type 1 diabetic mouse model. In another example, Tong et al. synthesized glucose- and H_2O_2 -responsive PVs by engineering phenylboronic acid (glucose-sensitive) and 4-(4,4,5,5-tetramethyl-1,3,2-dioxaborolan-2-yl)benzyl acrylate (H_2O_2 -sensitive) functional groups in the triblock copolymer [239]. The resultant PVs-loaded MNs presented an effective hypoglycemic effect in a diabetic rat model compared to that of subcutaneous injection or only insulin-loaded MNs. Xu et al. built H_2O_2 -responsive mesoporous silica

nanoparticles (MSNs), which were then loaded with insulin and entrapped into MNs for transdermal delivery [240]. The porous MSNs acted as the reservoir of insulin together with GOx for H_2O_2 generation in hyperglycemic states. Here, the MSNs were modified with 4-(imidazolyl carbamate)phenylboronic acid pinacol ester to form host-guest complexation with α -cyclodextrin, thereby keeping insulin within the MSNs. Upon exposure to H_2O_2 , the phenylboronic ester on the surface of the MSNs was oxidized, resulting in the destruction of the host-guest complexation and subsequent release of the preloaded insulin. Recently, mesoporous bioactive glasses was employed as the insulin carrier and integrated with MN device for glucose-responsive insulin delivery [241]. In this design, the porous bioactive glasses loaded with insulin and two enzymes (GOx/CAT) were capped with pH-sensitive ZnO quantum dots as “gatekeepers”. These ZnO quantum dots dissolved in the enzyme-mediated acid environment under hyperglycemic conditions, opening the pores on the bioactive glasses and releasing the encapsulated insulin.

However, the undesirable byproduct H_2O_2 produced during the enzymatic oxidation of glucose could reduce the activity of GOx thus hamper the response rate. The generation of H_2O_2 may also lead to free radical-induced damage to skin tissue during the long-term usage. Therefore, to further enhance the glucose-responsive capacity, Yu et al. designed a hypoxia and H_2O_2 dual-sensitive system based on polymersome-incorporated MNs for optimized insulin delivery [242]. An amphiphilic diblock copolymer consisting of PEG and polyserine was utilized to prepare the dual-sensitive polymersomes (*d*-GRPs), on which hypoxia-sensitive NI group was modified via H_2O_2 -responsive thioether moiety. Rapid oxygen consumption and H_2O_2 generation by enzymatic reactions under high glucose levels contributed to the increased water-solubility of the copolymer, triggering the dissociation and release of the insulin from the *d*-GRPs. *In vivo* results in diabetic mice showed that this patch effectively regulated BGLs for 10 h after administration with minimal skin inflammation. In another design, Wang et al. prepared core-shell structured MNs directly from H_2O_2 -degradable polymeric gel (Fig. 12) [243]. The core of MNs consisted of PVA network cross-linked by a H_2O_2 -cleavable linker (TSPBA), with insulin chemically anchored on PVA via a H_2O_2 -sensitive linkage. GOx was encapsulated into the acrylated nanogel (GOx-NG) to form a large size for covalent immobilization on PVA, restricting the leakage of GOx while maintaining the ease of insulin release. Under hyperglycemic conditions, H_2O_2 was locally generated by GOx, resulting in oxidation and hydrolyzation of both the PVA crosslinkers and insulin conjugates, facilitating the rapid release of free insulin from the MNs. Researchers demonstrated that this H_2O_2 -

responsive insulin patch presented rapid glucose-responsiveness and, with a consecutive administration of MNs, was able to control BGLs for 40-h without severe hypoglycemia. Of note, the MNs were further coated with a thin-layer of nanogel embedding H₂O₂-scavenging enzymes (catalase), thus facilitate elimination of H₂O₂ to mitigate its injury toward normal tissues by oxidative stress. *In vivo* performance of this core-shell gelled MN patch effectively improved inflammation in skin tissue treated with coated MNs compared to non-coated MNs *in vivo*. More recently, the same research group developed an H₂O₂ and pH cascade-triggered insulin delivery system based on sheath-structured MNs [244]. Insulin was entrapped by H₂O₂-sensitive and positively charged diblock copolymers to form nano-size complex micelles. Upon incubation in hyperglycemic conditions, this highly positively charged polymer can be oxidized by H₂O₂ and subsequently hydrolyzed to be weakly positive-charged materials. The reduction in pH during the oxidation of glucose also reduced the density of negative charges on insulin to weaken the interaction between insulin and polymers, further promoting its release. The trigger mechanism based on both pH and H₂O₂ ensured that insulin was only released in both the oxidative and acidic environment created by oxidation of glucose in the presence of GOx. By embedding catalase-nanogels in the sheath covering the insulin complex micelles-loaded MN core, this patch could regulate the glucose levels in diabetic mice within the normal range with effective mitigation of H₂O₂.

Outside of synthetic insulin carriers, Ye et al. described an innovative transdermal insulin delivery strategy incorporating insulin-secreted pancreatic β -cells with MN array patch for diabetes treatment [245]. Transplantation of insulin-secreting cells has been intensively investigated in type 1 diabetes treatment. However, this method may be hampered by the host immune response and issues with biocompatibility of cell grafts. In this approach, the insulin secretion from exogenous β -cells are not implanted and instead are modulated by BGLs through MNs containing glucose-signal amplifiers (GSAs). The GSAs were glucose-sensitive polymeric nanovesicles entrapping GOx, α -amylase (AM) and glucoamylase (GA). GOx was selected to induce the dissociation of nanovesicles in hyperglycemic conditions. The released AM hydrolyzed α -amylose embedded in the MNs to give disaccharides and trisaccharides, which were further converted to glucose by GA. The "amplified" local-concentrated glucose effectively diffused into the externally positioned β -cell capsules, where it promoting secretion and diffusion of insulin through MNs into the skin. This design showed extended therapeutic efficacy compared to the MNs without GSAs, where one such MN patch was shown to rapidly reduce BGLs of type 1 diabetic mice and maintain the reduction in glucose levels for over 6 h.

As microneedles do not only penetrate stratum corneum to increase skin permeability, but also directly carry insulin into the dermis layer, the microneedle-based technique demonstrated a relatively higher transport efficiency compared to other strategies. Due to the convenient, easy, and painless administration, it is considered to be suitable for people with diabetes to utilize by themselves at home. With the glucose-responsive moieties, it further shows great promising for continuous effective regulation of blood glucose. However, the potential breakage, irritation, and infection should be thoroughly investigated before clinical usage.

6. Conclusion and outlook

In this review, we have surveyed the technological advances in the development of transdermal insulin delivery systems for blood glucose regulation. Compared to passive transport through the skin, the use of chemical enhancers, external instruments, and microneedle devices have exhibited great potential to enhance the permeation of insulin by disrupting the skin barrier (Table 1). Unlike the traditional hypodermic injection, the transdermal insulin delivery demonstrates a more patient-friendly and minimally invasive method for daily diabetes management (Table 2). In addition, researchers also took the advantages of laser and another microdermabrasion device to facilitate insulin

transport through the skin [246–248]. Besides, transdermal strategies such as power jet, heat or magnetophoresis-assisted administration routes could also be investigated for needless delivery of insulin [137,249].

Despite great successes in transdermal insulin delivery, there are several limitations associated with long-term use, delivery efficiency, and reliability that warrant further research. Further experiments should be performed to evaluate the short- and long-term side effects associated with chemical enhancers and different microneedle materials. The potential risk of irradiation and inflammation must also be assessed in clinical studies. In addition, correct dosage relies on an understanding of how to guarantee consistent insulin delivery in different patients or in different skin sites within the same patient. To this end, pharmacokinetics should also be characterized to determine the transport efficiency. More extensive investigation on transdermal insulin delivery with a closed-loop control is required to prevent the risk of hypoglycemia, which represents a severe complication of any insulin therapy method. For approaches that rely on electrical instruments, a reusable and low-cost handheld device would be beneficial for self-administration at home. Finally, innovative technologies to improve the stability, enhance bioavailability, and maintain bioactivity of insulin are critical to enable the ultimate development of effective, low-cost, and convenient transdermal insulin delivery systems.

Acknowledgement

This work was supported by the grants from the National Science Foundation (Grant No. 1708620), American Diabetes Association (ADA) (Grant No. 1-15-ACE-21), the JDRF (Grant No. 2-SRA-2016-269-A-N) to Z.G. ARK is supported by funding from the National Institute of Diabetes and Digestive and Kidney Disease of the National Institutes of Health under Award Number F30DK113728.

References

- [1] E.R.F. Collaboration, Diabetes mellitus, fasting blood glucose concentration, and risk of vascular disease: a collaborative meta-analysis of 102 prospective studies, *Lancet* 375 (2010) 2215–2222.
- [2] International Diabetes Federation, <http://www.idf.org/diabetesatlas>.
- [3] L. Guariguata, D.R. Whiting, I. Hambleton, J. Beagley, U. Linnenkamp, J.E. Shaw, Global estimates of diabetes prevalence for 2013 and projections for 2035, *Diabetes Res. Clin. Pract.* 103 (2014) 137–149.
- [4] M.A. Atkinson, G.S. Eisenbarth, Type 1 diabetes: new perspectives on disease pathogenesis and treatment, *Lancet* 358 (2001) 221–229.
- [5] M. Stumvoll, B.J. Goldstein, T.W. van Haefen, Type 2 diabetes: principles of pathogenesis and therapy, *Lancet* 365 (2005) 1333–1346.
- [6] D.R. Owens, B. Zinman, G.B. Bolli, Insulins today and beyond, *Lancet* 358 (2001) 739–746.
- [7] A.N. Zaykov, J.P. Mayer, R.D. Dimarchi, Pursuit of a perfect insulin, *Nat. Rev. Drug Discov.* 15 (2016) 425.
- [8] M.L. Misso, K.J. Egberts, M. Page, D. O'Connor, J. Shaw, Cochrane review: continuous subcutaneous insulin infusion (CSII) versus multiple insulin injections for type 1 diabetes mellitus, *Evid. Based Child Health* 5 (2010) 1726–1867.
- [9] Y. Ohkubo, H. Kishikawa, E. Araki, T. Miyata, S. Isami, S. Motoyoshi, Y. Kojima, N. Furuyoshi, M. Shichiri, Intensive insulin therapy prevents the progression of diabetic microvascular complications in Japanese patients with non-insulin-dependent diabetes mellitus: a randomized prospective 6-year study, *Diabetes Res. Clin. Pract.* 28 (1995) 103–117.
- [10] A.D. Morris, D.I. Boyle, A.D. McMahon, S.A. Greene, T.M. MacDonald, R.W. Newton, D.M. Collaboration, Adherence to insulin treatment, glycaemic control, and ketoacidosis in insulin-dependent diabetes mellitus, *Lancet* 350 (1997) 1505–1510.
- [11] J. Pickup, H. Keen, Continuous subcutaneous insulin infusion at 25 years: evidence base for the expanding use of insulin pump therapy in type 1 diabetes, *Diabetes Care* 25 (2002) 593–598.
- [12] J. Weissberg-Benchell, J. Antisdell-Lomaglio, R. Seshadri, Insulin pump therapy: a meta-analysis, *Diabetes Care* 26 (2003) 1079–1087.
- [13] D.R. Owens, New horizons-alternative routes for insulin therapy, *Nat. Rev. Drug Discov.* 1 (2002) 529.
- [14] D.R. Owens, B. Zinman, G. Bolli, Alternative routes of insulin delivery, *Diabet. Med.* 20 (2003) 886–898.
- [15] V. Ravaine, C. Ancla, B. Catargi, Chemically controlled closed-loop insulin delivery, *J. Control. Release* 132 (2008) 2–11.
- [16] H. Iyer, A. Khedkar, M. Verma, Oral insulin—a review of current status, *Diabetes Obes. Metab.* 12 (2010) 179–185.

- [17] R. Hovorka, Closed-loop insulin delivery: from bench to clinical practice, *Nat. Rev. Endocrinol.* 7 (2011) 385.
- [18] R. Mo, T. Jiang, J. Di, W. Tai, Z. Gu, Emerging micro-and nanotechnology based synthetic approaches for insulin delivery, *Chem. Soc. Rev.* 43 (2014) 3595–3629.
- [19] O. Veisoh, B.C. Tang, K.A. Whitehead, D.G. Anderson, R. Langer, Managing diabetes with nanomedicine: challenges and opportunities, *Nat. Rev. Drug Discov.* 14 (2015) 45.
- [20] N.A. Bakh, A.B. Cortinas, M.A. Weiss, R.S. Langer, D.G. Anderson, Z. Gu, S. Dutta, M.S. Strano, Glucose-responsive insulin by molecular and physical design, *Nat. Chem.* 9 (2017) 937.
- [21] E.-S. Khafagy, M. Morishita, Y. Onuki, K. Takayama, Current challenges in non-invasive insulin delivery systems: a comparative review, *Adv. Drug Deliv. Rev.* 59 (2007) 1521–1546.
- [22] S. Mitragotri, P.A. Burke, R. Langer, Overcoming the challenges in administering biopharmaceuticals: formulation and delivery strategies, *Nat. Rev. Drug Discov.* 13 (2014) 655.
- [23] R. Yang, T. Wei, H. Goldberg, W. Wang, K. Cullion, D.S. Kohane, Getting drugs across biological barriers, *Adv. Mater.* 29 (2017) 1606596.
- [24] M.R. Prausnitz, S. Mitragotri, R. Langer, Current status and future potential of transdermal drug delivery, *Nat. Rev. Drug Discov.* 3 (2004) 115.
- [25] M.R. Prausnitz, R. Langer, Transdermal drug delivery, *Nat. Biotechnol.* 26 (2008) 1261.
- [26] E.L. Giudice, J.D. Campbell, Needle-free vaccine delivery, *Adv. Drug Deliv. Rev.* 58 (2006) 68–89.
- [27] B. Godin, E. Toutou, Transdermal skin delivery: predictions for humans from in vivo, ex vivo and animal models, *Adv. Drug Deliv. Rev.* 59 (2007) 1152–1161.
- [28] J.D. Bos, M.M. Meinardi, The 500 Dalton rule for the skin penetration of chemical compounds and drugs, *Exp. Dermatol.* 9 (2000) 165–169.
- [29] R.B. Walker, E.W. Smith, The role of percutaneous penetration enhancers, *Adv. Drug Deliv. Rev.* 18 (1996) 295–301.
- [30] B.C. Finnin, T.M. Morgan, Transdermal penetration enhancers: applications, limitations, and potential, *J. Pharm. Sci.* 88 (1999) 955–958.
- [31] A.C. Williams, B.W. Barry, Penetration enhancers, *Adv. Drug Deliv. Rev.* 56 (2004) 603–618.
- [32] P. Karande, A. Jain, K. Ergun, V. Kispersky, S. Mitragotri, Design principles of chemical penetration enhancers for transdermal drug delivery, *Proc. Natl. Acad. Sci. U. S. A.* 102 (2005) 4688–4693.
- [33] M.E. Lane, Skin penetration enhancers, *Int. J. Pharm.* 447 (2013) 12–21.
- [34] K.M. Yerramsetty, V.K. Rachakonda, B.J. Neely, S.V. Madihally, K.A. Gasem, Effect of different enhancers on the transdermal permeation of insulin analog, *Int. J. Pharm.* 398 (2010) 83–92.
- [35] A.C. Sintov, U. Wormser, Topical iodine facilitates transdermal delivery of insulin, *J. Control. Release* 118 (2007) 185–188.
- [36] Y.-z. Li, Y.-s. Quan, L. Zang, M.-n. Jin, F. Kamiyama, H. Katsumi, A. Yamamoto, S. Tsutsumi, Transdermal delivery of insulin using trypsin as a biochemical enhancer, *Biol. Pharm. Bull.* 31 (2008) 1574–1579.
- [37] Y. Chen, Y. Shen, X. Guo, C. Zhang, W. Yang, M. Ma, S. Liu, M. Zhang, L.P. Wen, Transdermal protein delivery by a coadministered peptide identified via phage display, *Nat. Biotechnol.* 24 (2006) 455–460.
- [38] M. Chang, X. Li, Y. Sun, F. Cheng, Q. Wang, X. Xie, W. Zhao, X. Tian, Effect of cationic cyclopeptides on transdermal and transmembrane delivery of insulin, *Mol. Pharm.* 10 (2013) 951–957.
- [39] A. Kogan, N. Garti, Microemulsions as transdermal drug delivery vehicles, *Adv. Colloid Interf. Sci.* 123 (2006) 369–385.
- [40] E. Toutou, B. Godin, Vesicular carriers for enhanced delivery through the skin, in: E. Toutou, B.W. Barry (Eds.), *Enhancement in Drug Delivery*, CRC Press, Florida 2006, pp. 255–278.
- [41] C. Pegoraro, S. MacNeil, G. Battaglia, Transdermal drug delivery: from micro to nano, *Nanoscale* 4 (2012) 1881–1894.
- [42] Y. Yang, J. Bugno, S. Hong, Nanoscale polymeric penetration enhancers in topical drug delivery, *Polym. Chem.* 4 (2013) 2651–2657.
- [43] C.M. Nastiti, T. Ponto, E. Abd, J.E. Grice, H.A. Benson, M.S. Roberts, Topical nano and microemulsions for skin delivery, *Pharmaceutics* 9 (2017) 37.
- [44] T.W. Prow, J.E. Grice, L.L. Lin, R. Faye, M. Butler, W. Becker, E.M. Wurm, C. Yoong, T.A. Robertson, H.P. Soyer, Nanoparticles and microparticles for skin drug delivery, *Adv. Drug Deliv. Rev.* 63 (2011) 470–491.
- [45] J. Guo, Q. Ping, L. Zhang, Transdermal delivery of insulin in mice by using lecithin vesicles as a carrier, *Drug Deliv. Rev.* 7 (2000) 113–116.
- [46] M.J. King, I. Badea, J. Solomon, P. Kumar, K.J. Gaspar, M. Foldvari, Transdermal delivery of insulin from a novel biphasic lipid system in diabetic rats, *Diabetes Technol. Ther.* 4 (2002) 479–488.
- [47] M.J. King, D. Michel, M. Foldvari, Evidence for lymphatic transport of insulin by topically applied biphasic vesicles, *J. Pharm. Pharmacol.* 55 (2003) 1339–1344.
- [48] M. Higaki, M. Kameyama, M. Udagawa, Y. Ueno, Y. Yamaguchi, R. Igarashi, T. Ishihara, Y. Mizushima, Transdermal delivery of CaCO₃-nanoparticles containing insulin, *Diabetes Technol. Ther.* 8 (2006) 369–374.
- [49] Y. Tahara, S. Honda, N. Kamiya, M. Goto, Transdermal delivery of insulin using a solid-in-oil nanodispersion enhanced by arginine-rich peptides, *Med. Chem. Commun.* 3 (2012) 1496.
- [50] K. Nose, D. Pissuwan, M. Goto, Y. Katayama, T. Niidome, Gold nanorods in an oil-base formulation for transdermal treatment of type 1 diabetes in mice, *Nanoscale* 4 (2012) 3776–3780.
- [51] Y. Tahara, S. Honda, N. Kamiya, H. Piao, A. Hirata, E. Hayakawa, T. Fujii, M. Goto, A solid-in-oil nanodispersion for transcutaneous protein delivery, *J. Control. Release* 131 (2008) 14–18.
- [52] Y. Tahara, K. Namatsu, N. Kamiya, M. Hagimori, S. Kamiya, M. Arakawa, M. Goto, Transcutaneous immunization by a solid-in-oil nanodispersion, *Chem. Commun.* 46 (2010) 9200–9202.
- [53] D. Pissuwan, K. Nose, R. Kurihara, K. Kaneko, Y. Tahara, N. Kamiya, M. Goto, Y. Katayama, T. Niidome, A solid-in-oil dispersion of gold nanorods can enhance transdermal protein delivery and skin vaccination, *Small* 7 (2011) 215–220.
- [54] Y.N. Kalia, A. Naik, J. Garrison, R.H. Guy, Iontophoretic drug delivery, *Adv. Drug Deliv. Rev.* 56 (2004) 619–658.
- [55] A.-R. Denet, R. Vanbever, V. Pr at, Skin electroporation for transdermal and topical delivery, *Adv. Drug Deliv. Rev.* 56 (2004) 659–674.
- [56] A. Azagury, L. Khoury, G. Ender, J. Kost, Ultrasound mediated transdermal drug delivery, *Adv. Drug Deliv. Rev.* 72 (2014) 127–143.
- [57] R. Vadlapatla, E.Y. Wong, S.G. Gayakwad, Electronic drug delivery systems: an overview, *J. Drug Deliv. Sci. Technol.* 41 (2017) 359–366.
- [58] A.K. Banga, Y.W. Chien, Iontophoretic delivery of drugs: fundamentals, developments and biomedical applications, *J. Control. Release* 7 (1988) 1–24.
- [59] M.J. Pikal, The role of electroosmotic flow in transdermal iontophoresis, *Adv. Drug Deliv. Rev.* 46 (2001) 281–305.
- [60] D.T.-W. Lau, J.W. Sharkey, L. Petryk, F.A. Mancuso, Z. Yu, L. Francis, Effect of current magnitude and drug concentration on iontophoretic delivery of octreotide acetate (Sandostatin®) in the rabbit, *Pharm. Res.* 11 (1994) 1742–1746.
- [61] A. Sieg, F. Jeanneret, M. Fathi, D. Hochstrasser, S. Rudaz, J.-L. Veuthey, R.H. Guy, M.B. Delgado-Charro, Extraction of amino acids by reverse iontophoresis in vivo, *Eur. J. Pharm. Biopharm.* 72 (2009) 226–231.
- [62] A. Naik, Y.N. Kalia, R.H. Guy, Transdermal drug delivery: overcoming the skin's barrier function, *Pharm. Sci. Technol. Today* 3 (2000) 318–326.
- [63] B.H. Sage Jr., Insulin iontophoresis, in: L.M. Sanders, R.W. Hendren (Eds.), *Protein Delivery-Physical Systems*, Plenum Publishing Corp., New York, NY 1997, pp. 319–341.
- [64] R. Stephen, T. Petelenz, S. Jacobsen, Potential novel methods for insulin administration: I. Iontophoresis, *Biomed. Biochim. Acta* 43 (1984) 553–558.
- [65] Y. Chien, O. Siddiqui, Y. Sun, W. Shi, J. Liu, Transdermal iontophoretic delivery of therapeutic peptides/proteins I: insulin, *Ann. N. Y. Acad. Sci.* 507 (1987) 32–51.
- [66] L. Jue-Chen, S. Ying, O. Siddiqui, S. Wei-Min, L. John, Blood glucose control in diabetic rats by transdermal iontophoretic delivery of insulin, *Int. J. Pharm.* 44 (1988) 197–204.
- [67] A.K. Banga, Y.W. Chien, Characterization of in vitro transdermal iontophoretic delivery of insulin, *Drug Dev. Ind. Pharm.* 19 (1993) 2069–2087.
- [68] O. Siddiqui, Y. Sun, J.C. Liu, Y.W. Chien, Facilitated transdermal transport of insulin, *J. Pharm. Sci.* 76 (1987) 341–345.
- [69] O. Pillai, N. Kumar, C.S. Dey, S. Borkute, S. Nagalingam, R. Panchagnula, Transdermal iontophoresis of insulin. Part 1: a study on the issues associated with the use of platinum electrodes on rat skin, *J. Pharm. Pharmacol.* 55 (2003) 1505–1513.
- [70] R. Panchagnula, P. Bindra, N. Kumar, C. Shanker Dey, O. Pillai, Stability of insulin under iontophoretic conditions, *Pharmazie* 61 (2006) 1014–1018.
- [71] K. Kajimoto, M. Yamamoto, M. Watanabe, K. Kigasawa, K. Kanamura, H. Harashima, K. Kogure, Noninvasive and persistent transfollicular drug delivery system using a combination of liposomes and iontophoresis, *Int. J. Pharm.* 403 (2011) 57–65.
- [72] B. Kari, Control of blood glucose levels in alloxan-diabetic rabbits by iontophoresis of insulin, *Diabetes* 35 (1986) 217–221.
- [73] L. Langkj er, J. Brange, G.M. Grodsky, R.H. Guy, Iontophoresis of monomeric insulin analogues in vitro: effects of insulin charge and skin pretreatment, *J. Control. Release* 51 (1998) 47–56.
- [74] E.H. Choi, S.H. Lee, S.K. Ahn, S.M. Hwang, The pretreatment effect of chemical skin penetration enhancers in transdermal drug delivery using iontophoresis, *Skin Pharmacol. Physiol.* 12 (1999) 326–335.
- [75] S.K. Rastogi, J. Singh, Transepidermal transport enhancement of insulin by lipid extraction and iontophoresis, *Pharm. Res.* 19 (2002) 427–433.
- [76] O. Pillai, R. Panchagnula, Transdermal iontophoresis of insulin, *J. Control. Release* 88 (2003) 287–296.
- [77] O. Pillai, V. Nair, R. Panchagnula, Transdermal iontophoresis of insulin: IV. Influence of chemical enhancers, *Int. J. Pharm.* 269 (2004) 109–120.
- [78] C.A. Zakzewski, J. Wasilewski, P. Cawley, W. Ford, Transdermal delivery of regular insulin to chronic diabetic rats: effect of skin preparation and electrical enhancement, *J. Control. Release* 50 (1998) 267–272.
- [79] N. Kanikkannan, J. Singh, P. Ramarao, Transdermal iontophoretic delivery of bovine insulin and monomeric human insulin analogue, *J. Control. Release* 59 (1999) 99–105.
- [80] S. Murdan, Electro-responsive drug delivery from hydrogels, *J. Control. Release* 92 (2003) 1–17.
- [81] S. Katagami, T. Shinoda, Y. Konno, M. Fukui, T. Ohmura, Y. Osada, Electroresponsive pulsatile depot delivery of insulin from poly(dimethylaminopropylacrylamide) gel in rats, *J. Pharm. Sci.* 86 (1997) 1273–1277.
- [82] O. Pillai, Transdermal delivery of insulin from poloxamer gel: ex vivo and in vivo skin permeation studies in rat using iontophoresis and chemical enhancers, *J. Control. Release* 89 (2003) 127–140.
- [83] H. Inada, A.-H. Ghanem, W.I. Higuchi, Studies on the effects of applied voltage and duration on human epidermal membrane alteration/recovery and the resultant effects upon iontophoresis, *Pharm. Res.* 11 (1994) 687–697.
- [84] G. Yan, K.D. Peck, H. Zhu, W.I. Higuchi, S.K. Li, Effects of electrophoresis and electroosmosis during alternating current iontophoresis across human epidermal membrane, *J. Pharm. Sci.* 94 (2005) 547–558.
- [85] V.F. Lvovich, E. Matthews, A.T. Riga, L. Kaza, AC electrokinetic platform for iontophoretic transdermal drug delivery, *J. Control. Release* 145 (2010) 134–140.

- [86] J.J. Escobar-Chávez, D. Bonilla-Martínez, M.A. Villegas-González, A.L. Revilla-Vázquez, Electroporation as an efficient physical enhancer for skin drug delivery, *J. Clin. Pharmacol.* 49 (2009) 1262–1283.
- [87] M.L. Yarmush, A. Golberg, G. Serša, T. Kotnik, D. Miklavčič, Electroporation-based technologies for medicine: principles, applications, and challenges, *Annu. Rev. Biomed. Eng.* 16 (2014).
- [88] J.D. Denuzio, B. Berner, Electrochemical and iontophoretic studies of human skin, *J. Control. Release* 11 (1990) 105–112.
- [89] M.R. Prausnitz, V.G. Bose, R. Langer, J.C. Weaver, Electroporation of mammalian skin: a mechanism to enhance transdermal drug delivery, *Proc. Natl. Acad. Sci. U. S. A.* 90 (1993) 10504–10508.
- [90] D.A. Edwards, M.R. Prausnitz, R. Langer, J.C. Weaver, Analysis of enhanced transdermal transport by skin electroporation, *J. Control. Release* 34 (1995) 211–221.
- [91] E.A. Mohammad, W.M. Elshemy, A.A. Elsayed, A.A. Abd-Elghany, Electroporation parameters for successful transdermal delivery of insulin, *Am. J. Ther.* 23 (2016) e1560–e1567.
- [92] R. Rastogi, S. Anand, V. Koul, Electroporation of polymeric nanoparticles: an alternative technique for transdermal delivery of insulin, *Drug Dev. Ind. Pharm.* 36 (2010) 1303–1311.
- [93] A. Sen, Y. Zhao, L. Zhang, S.W. Hui, Enhanced transdermal transport by electroporation using anionic lipids, *J. Control. Release* 82 (2002) 399–405.
- [94] A. Sen, M.E. Daly, S.W. Hui, Transdermal insulin delivery using lipid enhanced electroporation, *Biochim. Biophys. Acta-Biomembr.* 1564 (2002) 5–8.
- [95] S.N. Murthy, Y.L. Zhao, K. Marlan, S.W. Hui, A.L. Kazim, A. Sen, Lipid and electroosmosis enhanced transdermal delivery of insulin by electroporation, *J. Pharm. Sci.* 95 (2006) 2041–2050.
- [96] S.N. Murthy, Y.-L. Zhao, S.-W. Hui, A. Sen, Synergistic effect of anionic lipid enhancer and electroosmosis for transcutaneous delivery of insulin, *Int. J. Pharm.* 326 (2006) 1–6.
- [97] S. Tokumoto, N. Higo, K. Sugibayashi, Effect of electroporation and pH on the iontophoretic transdermal delivery of human insulin, *Int. J. Pharm.* 326 (2006) 13–19.
- [98] T.W. Wong, T.Y. Chen, C.C. Huang, J.C. Tsai, S.W. Hui, Painless skin electroporation as a novel way for insulin delivery, *Diabetes Technol. Ther.* 13 (2011) 929–935.
- [99] C.T.-S. Ching, T.-P. Sun, W.-T. Huang, S.-H. Huang, C.-S. Hsiao, K.-M. Chang, A circuit design of a low-cost, portable and programmable electroporation device for biomedical applications, *Sensors Actuators B Chem.* 166–167 (2012) 292–300.
- [100] Y. Zhang, J. Yu, H.N. Bomba, Y. Zhu, Z. Gu, Mechanical force-triggered drug delivery, *Chem. Rev.* 116 (2016) 12536–12563.
- [101] K.S. Suslick, G.J. Price, Applications of ultrasound to materials chemistry, *Annu. Rev. Mater. Sci.* 29 (1999) 295–326.
- [102] S. Mitragotri, J. Kost, Low-frequency sonophoresis: a review, *Adv. Drug Del. Rev.* 56 (2004) 589–601.
- [103] K. Ferrara, R. Pollard, M. Borden, Ultrasound microbubble contrast agents: fundamentals and application to gene and drug delivery, *Annu. Rev. Biomed. Eng.* 9 (2007).
- [104] P.N. Wells, H.-D. Liang, Medical ultrasound: imaging of soft tissue strain and elasticity, *J. R. Soc. Interface* 8 (2011) 1521–1549.
- [105] F.A. Jolesz, MRI-guided focused ultrasound surgery, *Annu. Rev. Med.* 60 (2009).
- [106] C.C. Coussios, R.A. Roy, Applications of acoustics and cavitation to noninvasive therapy and drug delivery, *Annu. Rev. Fluid Mech.* 40 (2008) 395–420.
- [107] S. Miyazaki, C. Yokouchi, M. Takada, External control of drug release: controlled release of insulin from a hydrophilic polymer implant by ultrasound irradiation in diabetic rats, *J. Pharm. Pharmacol.* 40 (1988) 716–717.
- [108] B.E. Polat, D. Hart, R. Langer, D. Blankschtein, Ultrasound-mediated transdermal drug delivery: mechanisms, scope, and emerging trends, *J. Control. Release* 152 (2011) 330–348.
- [109] S. Mitragotri, Sonophoresis: a 50-year journey, *Drug Discov. Today* 9 (2004) 735–736.
- [110] P. Tyle, P. Agrawala, Drug delivery by phonophoresis, *Pharm. Res.* 6 (1989) 355–361.
- [111] N.N. Byl, The use of ultrasound as an enhancer for transcutaneous drug delivery: phonophoresis, *Phys. Ther.* 75 (1995) 539–553.
- [112] W. Gaertner, Frequency dependence of ultrasonic cavitation, *J. Acoust. Soc. Am.* 26 (1954) 977–980.
- [113] K. Tachibana, S. Tachibana, Transdermal delivery of insulin by ultrasonic vibration, *J. Pharm. Pharmacol.* 43 (1991) 270–271.
- [114] S. Mitragotri, D. Blankschtein, R. Langer, Ultrasound-mediated transdermal protein delivery, *Science* 269 (1995) 850–853.
- [115] K. Tachibana, Transdermal delivery of insulin to alloxan-diabetic rabbits by ultrasound exposure, *Pharm. Res.* 9 (1992) 952–954.
- [116] S. Mitragotri, D. Blankschtein, R. Langer, Transdermal drug delivery using low-frequency sonophoresis, *Pharm. Res.* 13 (1996) 411–420.
- [117] O.M. Al-Bataineh, K. Lweesy, L. Fraiwan, Noninvasive transdermal insulin delivery using piston-shaped PZT transducers: in vivo rabbits evaluation, *JMIME* (2012) 6.
- [118] H. Feiszthuber, S. Bhatnagar, M. Gyongy, C.C. Coussios, Cavitation-enhanced delivery of insulin in agar and porcine models of human skin, *Phys. Med. Biol.* 60 (2015) 2421–2434.
- [119] A. Boucaud, L. Tessier, L. Machet, L. Vaillant, F. Patat, Transdermal delivery of insulin using low frequency ultrasound, *Ultrasonics Symposium, IEEE* 2000, pp. 1453–1456.
- [120] A. Boucaud, L. Machet, M. Garrigue, L. Vaillant, F. Patat, A practical use of low frequency ultrasound for rapid and reproducible transdermal delivery of insulin, *Ultrasonics Symposium, IEEE* 2001, pp. 1327–1330.
- [121] A. Boucaud, M.A. Garrigue, L. Machet, L.C. Vaillant, F. Patat, Effect of sonication parameters on transdermal delivery of insulin to hairless rats, *J. Control. Release* 81 (2002) 113–119.
- [122] N.B. Smith, S. Lee, E. Maione, R.B. Roy, S. McElligott, K.K. Shung, Ultrasound-mediated transdermal transport of insulin in vitro through human skin using novel transducer designs, *Ultrasound Med. Biol.* 29 (2003) 311–317.
- [123] N.B. Smith, S. Lee, K.K. Shung, Ultrasound-mediated transdermal in vivo transport of insulin with low-profile cymbal arrays, *Ultrasound Med. Biol.* 29 (2003) 1205–1210.
- [124] S. Lee, R.E. Newnham, N.B. Smith, Short ultrasound exposure times for noninvasive insulin delivery in rats using the lightweight cymbal array, *IEEE Trans. Ultrason. Ferroelectr. Freq. Control* 51 (2004) 176–180.
- [125] S. Lee, B. Snyder, R.E. Newnham, N. Barrie Smith, Noninvasive ultrasonic transdermal insulin delivery in rabbits using the light-weight cymbal array, *Diabetes Technol. Ther.* 6 (2004) 808–815.
- [126] S. Lee, N. Smith, D. Markley, B. Snyder, A. Uzgu, M. Pishko, R. Newnham, Composite transducer arrays for the treatment of diabetes, *Int. J. Appl. Ceram. Technol.* 2 (2005) 308–316.
- [127] J. Luis, E.J. Park, R.J. Meyer Jr., N.B. Smith, Rectangular cymbal arrays for improved ultrasonic transdermal insulin delivery, *J. Acoust. Soc. Am.* 122 (2007) 2022–2030.
- [128] E.J. Park, J. Werner, N.B. Smith, Ultrasound mediated transdermal insulin delivery in pigs using a lightweight transducer, *Pharm. Res.* 24 (2007) 1396–1401.
- [129] E. Park, J. Dodds, N. Smith, Dose comparison of ultrasonic transdermal insulin delivery to subcutaneous insulin injection, *Int. J. Nanomedicine* 3 (2008) 335.
- [130] E.J. Park, J. Werner, D. Jaiswal, N.B. Smith, Closed-loop controlled noninvasive ultrasonic glucose sensing and insulin delivery, *AIP Conf. Proc.*, AIP 2010, pp. 157–160.
- [131] J. Di, J. Price, X. Gu, X. Jiang, Y. Jing, Z. Gu, Ultrasound-triggered regulation of blood glucose levels using injectable nano-network, *Adv. Healthc. Mater.* 3 (2014) 811–816.
- [132] J. Di, J. Yu, Q. Wang, S. Yao, D. Suo, Y. Ye, M. Pless, Y. Zhu, Y. Jing, Z. Gu, Ultrasound-triggered noninvasive regulation of blood glucose levels using microgels integrated with insulin nanocapsules, *Nano Res.* 10 (2017) 1393–1402.
- [133] I. Suarez Castellanos, A. Jeremic, J. Cohen, V. Zderic, Ultrasound stimulation of insulin release from pancreatic beta cells as a potential novel treatment for Type 2 diabetes, *Ultrasound Med. Biol.* 43 (2017) 1210–1222.
- [134] I. Suarez Castellanos, T. Singh, B. Balteanu, D.C. Bhowmick, A. Jeremic, V. Zderic, Calcium-dependent ultrasound stimulation of secretory events from pancreatic beta cells, *J. Ther. Ultrasound* 5 (2017) 30.
- [135] K. Sonoki, M. Yoshinari, M. Iwase, K. Tashiro, K. Iino, M. Wakisaka, M. Fujishima, Regurgitation of blood into insulin cartridges in the pen-like injectors, *Diabetes Care* 24 (2001) 603–604.
- [136] J. Baxter, S. Mitragotri, Needle-free liquid jet injections: mechanisms and applications, *Expert Rev. Med. Dev.* 3 (2006) 565–574.
- [137] S. Mitragotri, Immunization without needles, *Nat. Rev. Immunol.* 5 (2005) 905.
- [138] C. Weller, M. Linder, Jet injection of insulin vs the syringe-and-needle method, *JAMA* 195 (1966) 844–847.
- [139] E. Katoulis, E. Drosinos, G. Dimitriadis, D. Hadjidakis, P. Mavrokefalos, S. Raptis, Efficacy of a new needleless insulin delivery system monitoring of blood glucose fluctuations and free insulin levels, *Int. J. Artif. Organs* 12 (1989) 333–338.
- [140] E.E. Engwerda, C.J. Tack, B.E. De Galan, Needle-free jet injection of rapid-acting insulin improves early postprandial glucose control in patients with diabetes, *Diabetes Care* 36 (2013) 3436–3441.
- [141] J. Hu, H. Shi, C. Zhao, X. Li, Y. Wang, Q. Cheng, R. Goswami, Q. Zhen, M. Mei, Y. Song, Lispro administered by the QS-M Needle-Free Jet Injector generates an earlier insulin exposure, *Expert Opin. Drug Deliv.* 13 (2016) 1203–1207.
- [142] H. de Wit, E. Engwerda, C. Tack, B. de Galan, Insulin administered by needle-free jet injection corrects marked hyperglycaemia faster in overweight or obese patients with diabetes, *Diabetes Obes. Metab.* 17 (2015) 1093–1099.
- [143] J. Malone, S. Lowitt, N. Grove, S. Shah, Comparison of insulin levels after injection by jet stream and disposable insulin syringe, *Diabetes Care* 9 (1986) 637–640.
- [144] L. Guo, X. Xiao, X. Sun, C. Qi, Comparison of jet injector and insulin pen in controlling plasma glucose and insulin concentrations in type 2 diabetic patients, *Medicine* 96 (2017).
- [145] S. Shahani, L. Shahani, Use of insulin in diabetes: a century of treatment, *Hong Kong Med. J.* 21 (2015) 553–559.
- [146] C. Houtzagers, A.P. Visser, P. Berntzen, R. Heine, E. Veen, The medi-jector II: efficacy and acceptability in insulin-dependent diabetic patients with and without needle phobia, *Diabet. Med.* 5 (1988) 135–138.
- [147] D.L.B. Pharm. D. F. Pass, Delivery of insulin by jet injection: recent observations, *Diabetes Technol. Ther.* 3 (2001) 225–232.
- [148] U. Schneider, R. Birnbacher, E. Schober, Painfulness of needle and jet injection in children with diabetes mellitus, *Eur. J. Pediatr.* 153 (1994) 409–410.
- [149] A. Arora, I. Hakim, J. Baxter, R. Rathasingham, R. Srinivasan, D.A. Fletcher, S. Mitragotri, Needle-free delivery of macromolecules across the skin by nanoliter-volume pulsed microjets, *Proc. Natl. Acad. Sci. U. S. A.* 104 (2007) 4255–4260.
- [150] A.M. Römgens, D. Rem-Bronneberg, R. Kassies, M. Hijlkema, D.L. Bader, C.W. Oomens, M.P. van Bruggen, Penetration and delivery characteristics of repetitive microjet injection into the skin, *J. Control. Release* 234 (2016) 98–103.
- [151] M.R. Prausnitz, Microneedles for transdermal drug delivery, *Adv. Drug Deliv. Rev.* 56 (2004) 581–587.
- [152] Y.-C. Kim, J.-H. Park, M.R. Prausnitz, Microneedles for drug and vaccine delivery, *Adv. Drug Deliv. Rev.* 64 (2012) 1547–1568.
- [153] S. Bhatnagar, K. Dave, V.V.K. Venuganti, Microneedles in the clinic, *J. Control. Release* 260 (2017) 164–182.
- [154] X. Jin, D.D. Zhu, B.Z. Chen, M. Ashfaq, X.D. Guo, Insulin delivery systems combined with microneedle technology, *Adv. Drug Deliv. Rev.* 127 (2018) 119–137.
- [155] A.S. Rzhnevskiy, T.R.R. Singh, R.F. Donnelly, Y.G. Anissimov, Microneedles as the technique of drug delivery enhancement in diverse organs and tissues, *J. Control. Release* 270 (2017) 184–202.

- [156] R.F. Donnelly, E. Larrañeta, Microarray patches: potentially useful delivery systems for long-acting nanosuspensions, *Drug Discov. Today* 23 (2017) 1026–1033.
- [157] S. Henry, D.V. McAllister, M.G. Allen, M.R. Prausnitz, Microfabricated microneedles: a novel approach to transdermal drug delivery, *J. Pharm. Sci.* 87 (1998) 922–925.
- [158] E. Larrañeta, M.T.C. McCrudden, A.J. Courtenay, R.F. Donnelly, Microneedles: a new frontier in nanomedicine delivery, *Pharm. Res.* 33 (2016) 1055–1073.
- [159] R.J. Narayan, Transdermal delivery of insulin via microneedles, *J. Biomed. Nanotechnol.* 10 (2014) 2244–2260.
- [160] M.R. Prausnitz, Engineering microneedle patches for vaccination and drug delivery to skin, *Annu. Rev. Chem. Biomol. Eng.* 8 (2017) 177–200.
- [161] W. Martanto, S.P. Davis, N.R. Holiday, J. Wang, H.S. Gill, M.R. Prausnitz, Transdermal delivery of insulin using microneedles in vivo, *Pharm. Res.* 21 (2004) 947–952.
- [162] C.P. Zhou, Y.L. Liu, H.L. Wang, P.X. Zhang, J.L. Zhang, Transdermal delivery of insulin using microneedle rollers in vivo, *Int. J. Pharm.* 392 (2010) 127–133.
- [163] Y. Wu, Y. Gao, G. Qin, S. Zhang, Y. Qiu, F. Li, B. Xu, Sustained release of insulin through skin by intradermal microdelivery system, *Biomed. Microdevices* 12 (2010) 665–671.
- [164] X.-M. Wu, H. Todo, K. Sugibayashi, Enhancement of skin permeation of high molecular compounds by a combination of microneedle pretreatment and iontophoresis, *J. Control. Release* 118 (2007) 189–195.
- [165] H. Chen, H. Zhu, J. Zheng, D. Mou, J. Wan, J. Zhang, T. Shi, Y. Zhao, H. Xu, X. Yang, Iontophoresis-driven penetration of nanovesicles through microneedle-induced skin microchannels for enhancing transdermal delivery of insulin, *J. Control. Release* 139 (2009) 63–72.
- [166] B. Al-Qallaf, D.B. Das, A. Davidson, Transdermal drug delivery by coated microneedles: geometry effects on drug concentration in blood, *Asia Pac. J. Chem. Eng.* 4 (2009) 845–857.
- [167] D.V. McAllister, P.M. Wang, S.P. Davis, J.H. Park, P.J. Canatella, M.G. Allen, M.R. Prausnitz, Microfabricated needles for transdermal delivery of macromolecules and nanoparticles: fabrication methods and transport studies, *Proc. Natl. Acad. Sci. U. S. A.* 100 (2003) 13755–13760.
- [168] S.P. Davis, W. Martanto, M.G. Allen, M.R. Prausnitz, Hollow metal microneedles for insulin delivery to diabetic rats, *IEEE Trans. Biomed. Eng.* 52 (2005) 909–915.
- [169] H.J. Gardeniers, R. Lutjtte, E.J. Berenschot, M.J. De Boer, S.Y. Yeshurun, M. Hefetz, R. Van T Oever, A. van den Berg, Silicon micromachined hollow microneedles for transdermal liquid transport, *J. Microelectromech. Syst.* 12 (2003) 855–862.
- [170] D. Resnik, M. Možek, B. Pečar, A. Janež, V. Urbančič, C. Iliescu, D. Vrtačnik, In vivo experimental study of noninvasive insulin microinjection through hollow si microneedle array, *Micromachines* 9 (2018) 40.
- [171] L. Nordquist, N. Roxhed, P. Griss, G. Stemme, Novel microneedle patches for active insulin delivery are efficient in maintaining glycaemic control: an initial comparison with subcutaneous administration, *Pharm. Res.* 24 (2007) 1381–1388.
- [172] N. Roxhed, B. Sameł, L. Nordquist, P. Griss, G. Stemme, Painless drug delivery through microneedle-based transdermal patches featuring active infusion, *IEEE Trans. Biomed. Eng.* 55 (2008) 1063–1071.
- [173] J. Gupta, E.I. Felner, M.R. Prausnitz, Minimally invasive insulin delivery in subjects with type 1 diabetes using hollow microneedles, *Diabetes Technol. Ther.* 11 (2009) 329–337.
- [174] E. Kochba, Y. Levin, I. Raz, A. Cahn, Improved insulin pharmacokinetics using a novel microneedle device for intradermal delivery in patients with type 2 diabetes, *Diabetes Technol. Ther.* 18 (2016) 525–531.
- [175] Y. Ye, J. Yu, D. Wen, A.R. Kahkoska, Z. Gu, Polymeric microneedles for transdermal protein delivery, *Adv. Drug Deliv. Rev.* 127 (2018) 106–118.
- [176] H.L. Quinn, E. Larrañeta, R.F. Donnelly, Dissolving microneedles: safety considerations and future perspectives, *Ther. Deliv.* 7 (2016) 283–285.
- [177] X. Hong, L. Wei, F. Wu, Z. Wu, L. Chen, Z. Liu, W. Yuan, Dissolving and biodegradable microneedle technologies for transdermal sustained delivery of drug and vaccine, *Drug Des. Devel. Ther.* 7 (2013) 945.
- [178] M. An, H. Liu, Dissolving microneedle arrays for transdermal delivery of amphiphilic vaccines, *Small* 13 (2017).
- [179] G. Li, A. Badkar, S. Nema, C.S. Koli, A.K. Banga, In vitro transdermal delivery of therapeutic antibodies using maltose microneedles, *Int. J. Pharm.* 368 (2009) 109–115.
- [180] K. Lee, C.Y. Lee, H. Jung, Dissolving microneedles for transdermal drug administration prepared by stepwise controlled drawing of maltose, *Biomaterials* 32 (2011) 3134–3140.
- [181] H. Kalluri, A.K. Banga, Formation and closure of microchannels in skin following microporation, *Pharm. Res.* 28 (2011) 82–94.
- [182] G. Li, A. Badkar, H. Kalluri, A.K. Banga, Microchannels created by sugar and metal microneedles: characterization by microscopy, macromolecular flux and other techniques, *J. Pharm. Sci.* 99 (2010) 1931–1941.
- [183] J.W. Lee, S.O. Choi, E.I. Felner, M.R. Prausnitz, Dissolving microneedle patch for transdermal delivery of human growth hormone, *Small* 7 (2011) 531–539.
- [184] F.-S. Quan, Y.-C. Kim, A. Vunna, D.-G. Yoo, J.-M. Song, M.R. Prausnitz, R.W. Compans, S.-M. Kang, Intradermal vaccination with influenza virus-like particles by using microneedles induces protection superior to that with intramuscular immunization, *J. Virol.* 84 (2010) 7760–7769.
- [185] S. Kommarreddy, B.C. Baudner, S. Oh, S.-y. Kwon, M. Singh, D.T. O'Hagan, Dissolvable microneedle patches for the delivery of cell-culture-derived influenza vaccine antigens, *J. Pharm. Sci.* 101 (2012) 1021–1027.
- [186] M.J. Mistilis, J.C. Joyce, E.S. Esser, I. Skountzou, R.W. Compans, A.S. Bommaris, M.R. Prausnitz, Long-term stability of influenza vaccine in a dissolving microneedle patch, *Drug Deliv. Transl. Res.* 7 (2017) 195–205.
- [187] C. Martin, C.J. Allender, K.R. Brain, A. Morrissey, J.C. Birchall, Low temperature fabrication of biodegradable sugar glass microneedles for transdermal drug delivery applications, *J. Control. Release* 158 (2012) 93–101.
- [188] A.P. Raphael, M.L. Crichton, R.J. Falconer, S. Meliga, X. Chen, G.J. Fernando, H. Huang, M.A. Kendall, Formulations for microprojection/microneedle vaccine delivery: Structure, strength and release profiles, *J. Control. Release* 225 (2016) 40–52.
- [189] Y. Ito, E. Hagiwara, A. Saeki, N. Sugioka, K. Takada, Feasibility of microneedles for percutaneous absorption of insulin, *Eur. J. Pharm. Sci.* 29 (2006) 82–88.
- [190] Y. Ito, T. Nakahigashi, N. Yoshimoto, Y. Ueda, N. Hamasaki, K. Takada, Transdermal insulin application system with dissolving microneedles, *Diabetes Technol. Ther.* 14 (2012) 891–899.
- [191] T. Miyano, Y. Tobinaga, T. Kanno, Y. Matsuzaki, H. Takeda, M. Wakui, K. Hanada, Sugar micro needles as transdermic drug delivery system, *Biomed. Microdevices* 7 (2005) 185–188.
- [192] S. Hirobe, H. Azukizawa, T. Hanafusa, K. Matsuo, Y.-S. Quan, F. Kamiyama, I. Katayama, N. Okada, S. Nakagawa, Clinical study and stability assessment of a novel transcutaneous influenza vaccination using a dissolving microneedle patch, *Biomaterials* 57 (2015) 50–58.
- [193] Y. Ye, J. Wang, Q. Hu, G.M. Hochu, H. Xin, C. Wang, Z. Gu, Synergistic transcutaneous immunotherapy enhances antitumor immune responses through delivery of checkpoint inhibitors, *ACS Nano* 10 (2016) 8956–8963.
- [194] C. Wang, Y. Ye, G.M. Hochu, H. Sadeghifar, Z. Gu, Enhanced cancer immunotherapy by microneedle patch-assisted delivery of anti-PD1 antibody, *Nano Lett.* 16 (2016) 2334–2340.
- [195] Y. Ye, C. Wang, X. Zhang, Q. Hu, Y. Zhang, Q. Liu, D. Wen, J. Milligan, A. Bellotti, L. Huang, A melanin-mediated cancer immunotherapy patch, *Sci. Immunol.* 2 (2017) eaan5692–5692.
- [196] Y. Zhang, Q. Liu, J. Yu, S. Yu, J. Wang, L. Qiang, Z. Gu, Locally induced adipose tissue browning by microneedle patch for obesity treatment, *ACS Nano* 11 (2017) 9223–9230.
- [197] J.W. Lee, J.-H. Park, M.R. Prausnitz, Dissolving microneedles for transdermal drug delivery, *Biomaterials* 29 (2008) 2113–2124.
- [198] M.-C. Chen, M.-H. Ling, K.-Y. Lai, E. Pramudityo, Chitosan microneedle patches for sustained transdermal delivery of macromolecules, *Biomacromolecules* 13 (2012) 4022–4031.
- [199] M.-C. Chen, S.-F. Huang, K.-Y. Lai, M.-H. Ling, Fully embeddable chitosan microneedles as a sustained release depot for intradermal vaccination, *Biomaterials* 34 (2013) 3077–3086.
- [200] W. Chen, R. Tian, C. Xu, B.C. Yung, G. Wang, Y. Liu, Q. Ni, F. Zhang, Z. Zhou, J. Wang, Microneedle-array patches loaded with dual mineralized protein/peptide particles for type 2 diabetes therapy, *Nat. Commun.* 8 (2017) 1777.
- [201] W. Yu, G. Jiang, Y. Zhang, D. Liu, B. Xu, J. Zhou, Polymer microneedles fabricated from alginate and hyaluronate for transdermal delivery of insulin, *Mater. Sci. Eng. C* 80 (2017) 187–196.
- [202] C.-J. Ke, Y.-J. Lin, Y.-C. Hu, W.-L. Chiang, K.-J. Chen, W.-C. Yang, H.-L. Liu, C.-C. Fu, H.-W. Sung, Multidrug release based on microneedle arrays filled with pH-responsive PLGA hollow microspheres, *Biomaterials* 33 (2012) 5156–5165.
- [203] L. Guo, J. Chen, Y. Qiu, S. Zhang, B. Xu, Y. Gao, Enhanced transcutaneous immunization via dissolving microneedle array loaded with liposome encapsulated antigen and adjuvant, *Int. J. Pharm.* 447 (2013) 22–30.
- [204] M.-C. Chen, Z.-W. Lin, M.-H. Ling, Near-infrared light-activatable microneedle system for treating superficial tumors by combination of chemotherapy and photothermal therapy, *ACS Nano* 10 (2015) 93–101.
- [205] W. Sun, Z. Araci, M. Inayathullah, S. Manickam, X. Zhang, M.A. Bruce, M.P. Marinkovich, A.T. Lane, C. Milla, J. Rajadas, Polyvinylpyrrolidone microneedles enable delivery of intact proteins for diagnostic and therapeutic applications, *Acta Biomater.* 9 (2013) 7767–7774.
- [206] F. Perennes, B. Marmiroli, M. Matteucci, M. Tormen, L. Vaccari, E. Di Fabrizio, Sharp beveled tip hollow microneedle arrays fabricated by LIGA and 3D soft lithography with polyvinyl alcohol, *J. Micromech. Microeng.* 16 (2006) 473.
- [207] I.-C. Lee, J.-S. He, M.-T. Tsai, K.-C. Lin, Fabrication of a novel partially dissolving polymer microneedle patch for transdermal drug delivery, *J. Mater. Chem. B* 3 (2015) 276–285.
- [208] Y. Zhang, P. Feng, J. Yu, J. Yang, J. Zhao, J. Wang, Q. Shen, Z. Gu, ROS-responsive microneedle patch for acne vulgaris treatment, *Adv. Therap.* 1 (2018) 1800035.
- [209] S. Liu, M.N. Jin, Y.S. Quan, F. Kamiyama, H. Katsumi, T. Sakane, A. Yamamoto, The development and characteristics of novel microneedle arrays fabricated from hyaluronic acid, and their application in the transdermal delivery of insulin, *J. Control. Release* 161 (2012) 933–941.
- [210] M.H. Ling, M.C. Chen, Dissolving polymer microneedle patches for rapid and efficient transdermal delivery of insulin to diabetic rats, *Acta Biomater.* 9 (2013) 8952–8961.
- [211] M. Leone, J. Mönkäre, J. Bouwstra, G. Kersten, Dissolving microneedle patches for dermal vaccination, *Pharm. Res.* 34 (2017) 2223–2240.
- [212] M.C. Chen, M.H. Ling, S.J. Kusuma, Poly-gamma-glutamic acid microneedles with a supporting structure design as a potential tool for transdermal delivery of insulin, *Acta Biomater.* 24 (2015) 106–116.
- [213] S. Lau, J. Fei, H. Liu, W. Chen, R. Liu, Multilayered pyramidal dissolving microneedle patches with flexible pedestals for improving effective drug delivery, *J. Control. Release* 265 (2017) 113–119.
- [214] I.C. Lee, Y.-C. Wu, S.-W. Tsai, C.-H. Chen, M.-H. Wu, Fabrication of two-layer dissolving polyvinylpyrrolidone microneedles with different molecular weights for in vivo insulin transdermal delivery, *RSC Adv.* 7 (2017) 5067–5075.
- [215] I.C. Lee, W.M. Lin, J.C. Shu, S.W. Tsai, C.H. Chen, M.T. Tsai, Formulation of two-layer dissolving polymeric microneedle patches for insulin transdermal delivery in diabetic mice, *J. Biomed. Mater. Res. A* 105 (2017) 84–93.
- [216] D. Liu, B. Yu, G. Jiang, W. Yu, Y. Zhang, B. Xu, Fabrication of composite microneedles integrated with insulin-loaded CaCO₃ microparticles and PVP for transdermal delivery in diabetic rats, *Mater. Sci. Eng. C* 90 (2018) 180–188.

- [217] H. Yang, S. Kim, I. Huh, S. Kim, S.F. Lahiji, M. Kim, H. Jung, Rapid implantation of dissolving microneedles on an electrospun pillar array, *Biomaterials* 64 (2015) 70–77.
- [218] J.D. Kim, M. Kim, H. Yang, K. Lee, H. Jung, Droplet-born air blowing: Novel dissolving microneedle fabrication, *J. Control. Release* 170 (2013) 430–436.
- [219] M.J. Garland, E. Caffarel-Salvador, K. Migalska, A.D. Woolfson, R.F. Donnelly, Dissolving polymeric microneedle arrays for electrically assisted transdermal drug delivery, *J. Control. Release* 159 (2012) 52–59.
- [220] J.-H. Park, M.G. Allen, M.R. Prausnitz, Polymer microneedles for controlled-release drug delivery, *Pharm. Res.* 23 (2006) 1008–1019.
- [221] Y. Zhang, G. Jiang, W. Yu, D. Liu, B. Xu, Microneedles fabricated from alginate and maltose for transdermal delivery of insulin on diabetic rats, *Mater. Sci. Eng. C* 85 (2018) 18–26.
- [222] K.Y. Seong, M.S. Seo, D.Y. Hwang, E.D. O’Cearbhaill, S. Sreenan, J.M. Karp, S.Y. Yang, A self-adherent, bullet-shaped microneedle patch for controlled transdermal delivery of insulin, *J. Control. Release* 265 (2017) 48–56.
- [223] S. Yang, F. Wu, J. Liu, G. Fan, W. Welsh, H. Zhu, T. Jin, Phase-transition microneedle patches for efficient and accurate transdermal delivery of insulin, *Adv. Funct. Mater.* 25 (2015) 4633–4641.
- [224] J. Di, S. Yao, Y. Ye, Z. Cui, J. Yu, T.K. Ghosh, Y. Zhu, Z. Gu, Stretch-triggered drug delivery from wearable elastomer films containing therapeutic depots, *ACS Nano* 9 (2015) 9407–9415.
- [225] W. Yu, G. Jiang, D. Liu, L. Li, Z. Tong, J. Yao, X. Kong, Transdermal delivery of insulin with bioceramic composite microneedles fabricated by gelatin and hydroxyapatite, *Mater. Sci. Eng. C* 73 (2017) 425–428.
- [226] W. Yu, G. Jiang, D. Liu, L. Li, H. Chen, Y. Liu, Q. Huang, Z. Tong, J. Yao, X. Kong, Fabrication of biodegradable composite microneedles based on calcium sulfate and gelatin for transdermal delivery of insulin, *Mater. Sci. Eng. C* 71 (2017) 725–734.
- [227] Q. Wu, L. Wang, H. Yu, J. Wang, Z. Chen, Organization of glucose-responsive systems and their properties, *Chem. Rev.* 111 (2011) 7855–7875.
- [228] J. Yu, Y. Zhang, H. Bomba, Z. Gu, Stimuli-responsive delivery of therapeutics for diabetes treatment, *Bioeng. Transl. Med.* 1 (2016) 323–337.
- [229] Y. Lu, A.A. Aimetti, R. Langer, Z. Gu, Bioresponsive materials, *Nat. Rev. Mater.* 2 (2017), 16075.
- [230] W. Sun, Q. Hu, W. Ji, G. Wright, Z. Gu, Leveraging physiology for precision drug delivery, *Physiol. Rev.* 97 (2016) 189–225.
- [231] J. Yu, Y. Zhang, A.R. Kahkoska, Z. Gu, Bioresponsive transcutaneous patches, *Curr. Opin. Biotechnol.* 48 (2017) 28–32.
- [232] G. Ma, C. Wu, Microneedle, bio-microneedle and bio-inspired microneedle: a review, *J. Control. Release* 251 (2017) 11–23.
- [233] G. Chen, J. Yu, Z. Gu, Glucose-responsive microneedle patches for diabetes treatment, *J. Diabetes Sci. Technol.* (2018) (1932296818778607).
- [234] J. Yu, Y. Zhang, Y. Ye, R. Disanto, W. Sun, D. Ranson, F.S. Ligler, J.B. Buse, Z. Gu, Microneedle-array patches loaded with hypoxia-sensitive vesicles provide fast glucose-responsive insulin delivery, *Proc. Natl. Acad. Sci. U. S. A.* 112 (2015) 8260–8265.
- [235] S.B. Bankar, M.V. Bule, R.S. Singhal, L. Ananthanarayan, Glucose oxidase—an overview, *Biotechnol. Adv.* 27 (2009) 489–501.
- [236] J. Yu, Y. Zhang, X. Hu, G. Wright, Z. Gu, Hypoxia-sensitive materials for biomedical applications, *Ann. Biomed. Eng.* 44 (2016) 1931–1945.
- [237] J. Wang, Y. Zhang, E. Archibong, F.S. Ligler, Z. Gu, Leveraging H₂O₂ levels for biomedical applications, *Adv. Biosys.* 1 (2017), 1700084.
- [238] X. Hu, J. Yu, C. Qian, Y. Lu, A.R. Kahkoska, Z. Xie, X. Jing, J.B. Buse, Z. Gu, H₂O₂-responsive vesicles integrated with transcutaneous patches for glucose-mediated insulin delivery, *ACS Nano* 11 (2017) 613–620.
- [239] Z. Tong, J. Zhou, J. Zhong, Q. Tang, Z. Lei, H. Luo, P. Ma, X. Liu, Glucose-and H₂O₂-responsive polymeric vesicles integrated with microneedle patches for glucose-sensitive transcutaneous delivery of insulin in diabetic rats, *ACS Appl. Mater. Interfaces* 10 (2018) 20014–20024.
- [240] B. Xu, G. Jiang, W. Yu, D. Liu, Y. Zhang, J. Zhou, S. Sun, Y. Liu, H₂O₂-Responsive mesoporous silica nanoparticles integrated with microneedle patches for the glucose-monitored transdermal delivery of insulin, *J. Mater. Chem. B* 5 (2017) 8200–8208.
- [241] B. Xu, Q. Cao, Y. Zhang, W. Yu, J. Zhu, D. Liu, G. Jiang, Microneedles integrated with ZnO quantum dots capped mesoporous bioactive glasses for glucose-mediated insulin delivery, *CS Biomater. Sci. Eng.* 4 (2018) 2473–2483.
- [242] J. Yu, C. Qian, Y. Zhang, Z. Cui, Y. Zhu, Q. Shen, F.S. Ligler, J.B. Buse, Z. Gu, Hypoxia and H₂O₂ dual-sensitive vesicles for enhanced glucose-responsive insulin delivery, *Nano Lett.* 17 (2017) 733–739.
- [243] J. Wang, Y. Ye, J. Yu, A.R. Kahkoska, X. Zhang, C. Wang, W. Sun, R.D. Corder, Z. Chen, S.A. Khan, J.B. Buse, Z. Gu, Core-shell microneedle gel for self-regulated insulin delivery, *ACS Nano* 12 (2018) 2466–2473.
- [244] Y. Zhang, J. Wang, J. Yu, D. Wen, A.R. Kahkoska, Y. Lu, X. Zhang, J.B. Buse, Z. Gu, Bioresponsive microneedles with a sheath structure for H₂O₂ and pH cascade-triggered insulin delivery, *Small* 14 (2018) 1704181.
- [245] Y. Ye, J. Yu, C. Wang, N.Y. Nguyen, G.M. Walker, J.B. Buse, Z. Gu, Microneedles integrated with pancreatic cells and synthetic glucose-signal amplifiers for smart insulin delivery, *Adv. Mater.* 28 (2016) 3115–3121.
- [246] S. Lee, D.J. McAuliffe, S.E. Mulholland, A.G. Doukas, Photomechanical transdermal delivery of insulin in vivo, *Lasers Surg. Med.* 28 (2001) 282–285.
- [247] S. Andrews, J.W. Lee, S.-O. Choi, M.R. Prausnitz, Transdermal insulin delivery using microdermabrasion, *Pharm. Res.* 28 (2011) 2110–2118.
- [248] S. Giannos, Skin microporation: strategies to enhance and expand transdermal drug delivery, *J. Drug Deliv. Sci. Technol.* 24 (2014) 293–299.
- [249] X. Chen, Current and future technological advances in transdermal gene delivery, *Adv. Drug Deliv. Rev.* 127 (2017) 85–105.
- [250] A. Smith, K. Zerke, P.-L. Roerig, S. Mills, C. Humphries, R. Durland, V. Spratlin, Transdermal Delivery of Insulin in Patients With Type 1 Diabetes, *Diabetes*, Virginia, 2008 A88.
- [251] E.E. Engwerda, C.J. Tack, B.E. de Galan, Pharmacokinetic and pharmacodynamic variability of insulin when administered by jet injection, *J. Diabetes Sci. Technol.* 11 (2017) 947–952.
- [252] E.E. Engwerda, E.J. Abbink, C.J. Tack, B.E. De Galan, Improved pharmacokinetic and pharmacodynamic profile of rapid-acting insulin using needle-free jet injection technology, *Diabetes Care* 34 (2011) 1804–1808.
- [253] R.J. Pettis, L. Hirsch, C. Kapitza, L. Nosek, U. Hövelmann, H.-J. Kurth, D.E. Sutter, N.G. Harvey, L. Heinemann, Microneedle-based intradermal versus subcutaneous administration of regular human insulin or insulin lispro: pharmacokinetics and postprandial glycemic excursions in patients with type 1 diabetes, *Diabetes Technol. Ther.* 13 (2011) 443–450.
- [254] J.J. Norman, M.R. Brown, N.A. Raviele, M.R. Prausnitz, E.I. Felner, Faster pharmacokinetics and increased patient acceptance of intradermal insulin delivery using a single hollow microneedle in children and adolescents with type 1 diabetes, *Pediatr. Diabetes* 14 (2013) 459–465.