



You have downloaded a document from
RE-BUŚ
repository of the University of Silesia in Katowice

Title: Cellulose mini-membranes modified with TiO₂ for separation, determination, and speciation of arsenates and selenites

Author: Beata Zawisza, Rafał Sitko, Ignasi Queralt, Eva Margui, Anna Gagor

Citation style: Zawisza Beata, Sitko Rafał, Queralt Ignasi, Margui Eva, Gagor Anna. (2020). Cellulose mini-membranes modified with TiO₂ for separation, determination, and speciation of arsenates and selenites. "Microchimica Acta" (Vol. 187 (2020), Art. No 430), doi 10.1007/s00604-020-04387-4



Uznanie autorstwa - Licencja ta pozwala na kopiowanie, zmienianie, rozprowadzanie, przedstawianie i wykonywanie utworu jedynie pod warunkiem oznaczenia autorstwa.



UNIwersYTET ŚLĄSKI
W KATOWICACH



Biblioteka
Uniwersytetu Śląskiego



Ministerstwo Nauki
i Szkolnictwa Wyższego



Cellulose mini-membranes modified with TiO₂ for separation, determination, and speciation of arsenates and selenites

Beata Zawisza¹ · Rafal Sitko¹ · Ignasi Queralt² · Eva Margui³ · Anna Gagor⁴

Received: 12 March 2020 / Accepted: 13 June 2020
© The Author(s) 2020

Abstract

Sorptive and selective mini-membranes based on TiO₂ directly synthesized onto cellulose filters (TiO₂@cellulose) have been developed. The in situ synthesis of TiO₂@cellulose applied is simple and economically advantageous. The obtained membranes can be useful for (1) separating arsenic(V) and selenium(IV) from other ions and organic matter, (2) speciation of arsenic and selenium, and (3) determining ultratraces of these ions in water samples. The membranes exhibit good stability and high maximum adsorption capacities for Se(IV) (71 mg g⁻¹) and As(V) (41 mg g⁻¹). A monolayer chemical adsorption of analytes on the membranes was confirmed. The structure of membranes was examined with scanning electron microscopy, x-ray diffraction, and micro energy-dispersive x-ray fluorescence spectrometry (μ-EDXRF). The membranes were characterized by homogenous distribution of TiO₂ onto cellulose. The TiO₂@cellulose was used as a new sorbent in micro-solid phase extraction for determination of Se(IV) and As(V) by EDXRF. Using direct analysis of mini-membranes after sorption of analytes avoids the elution step. Thus, the proposed procedure is an attractive and solvent-free option for quantitative monitoring of Se(IV) and As(V) in different materials. Both analytes were quantitatively and simultaneously separated/determined from samples at pH 2 with very good recovery (close to 100%), precision (4.5%), and detection limits (0.4 ng mL⁻¹ Se and 0.25 ng mL⁻¹ As). TiO₂@cellulose membranes were applied to water analysis.

Keywords Arsenate · Selenite · Preconcentration · Complexes · Titanium dioxide

Introduction

Many sorbents included nanosorbents are mainly oriented towards cationic species of metal but in fact, the sorption of

anionic forms is an analytical challenge. Thus, the development of new sorbents dedicated to anionic species of elements is a strategically important and current issue, especially when they are toxic and hazardous for people and natural environment. Arsenic and selenium species can have negative influence on environment. Moreover, arsenic and selenium of various oxidation states have different chemical toxicity. The arsenites and selenates (AsO₃³⁻, SeO₄²⁻) are more toxic than the arsenates and selenites (AsO₄³⁻, SeO₃²⁻). Therefore, the development of the reliable analytical procedures enabling speciation analysis is very important. References regarding the regulations for water as well as toxicity of arsenic and selenium are given in Electronic Supplementary Material (ESM). Various analytical techniques such as inductively coupled plasma optical emission spectrometry (ICP-OES) [1], graphite furnace atomic absorption spectrometry (GF-AAS) [2, 3] and hydride generation atomic absorption spectrometry (HG-AAS) [4], hydride generation atomic fluorescence spectrometry (HG-AFS) [5, 6], inductively coupled plasma mass spectrometry (ICP-MS) [7, 8], total reflection x-ray fluorescence spectrometry (TXRF) [9], and energy-dispersive x-ray fluorescence spectrometry (EDXRF) [10] were

Electronic supplementary material The online version of this article (<https://doi.org/10.1007/s00604-020-04387-4>) contains supplementary material, which is available to authorized users.

✉ Beata Zawisza
beata.zawisza@us.edu.pl

- ¹ Institute of Chemistry, University of Silesia, Szkolna 9, 40-006 Katowice, Poland
- ² Department of Geosciences, Institute of Environmental Assessment and Water Research, IDAEA-CSIC, Jordi Girona St., 18-26, 08034 Barcelona, Spain
- ³ Department of Chemistry, Faculty of Sciences, University of Girona, C/M. Aurèlia Campmany 69, Girona, Spain
- ⁴ Institute of Low Temperature and Structure Research, Polish Academy of Sciences, P.O. Box 1410, 50-950 Wrocław, Poland

used for the quantification of As and Se at ultra-trace level in different samples. The preconcentration was an important step before determination of these elements. Dispersive liquid-liquid microextraction (DLLME), hollow fiber liquid phase microextraction (HF-LPME), cloud point extraction (CPE), capillary microextraction, and solid phase extraction (SPE) were used for the extraction of As and Se species from various matrices. Numerous adsorbents have been successfully used in both solid-phase extraction (SPE) and micro-SPE (μ SPE) for metal ion preconcentration such as modified nanocomposites [11], different types of nanoparticles (carbon, metals, and metal oxides) [12], and cellulose and its derivatives [13]. Extensive studies on new sorbents are still demanded to investigate the sorption of metalloid ions and then determination when different anions are present simultaneously in the solution.

Up to now, not many detailed studies on cellulose modified with metal oxides as sorbents have been described. Certain studies prove that some oxides are characterized by a very high adsorption capacity. The surface of amphoteric titania (TiO_2) contains hydroxyl groups, and it is a promising material for SPE studies. Determining the nature of active sites susceptible to adsorption of analytes is crucial. In general, the surface hydroxyl groups are prone to the ions adsorption on oxide surfaces [14]. Nevertheless, TiO_2 is among the few oxides, which after calcined, that has a very low coverage by hydroxyl groups [15]. There are not the systematic data and research relating to the absorption properties as well as using cellulose with titania in the analysis of trace elements. The use of cellulose as a host for TiO_2 particles is particularly preferred because of its cross-linking character.

In this work, an effective sorbet cellulose-based is developed. The treatment of cellulose fibers is extremely important when using metal oxide particles as a coating, since the properties of the coated substrate varies. TiO_2 is easy to be synthesized and grafted to cellulose backbone. In this paper, we developed a novel, simple surface treatment method. The cellulose filters were pipetted with $\text{Ti}(\text{OC}_3\text{H}_7)_4$ and then immersed in ammonia to coat/impregnate cellulose surface with TiO_2 . In this way, using in situ method, new stable filters (TiO_2 @cellulose) of excellent sorptive properties have been obtained. Next, TiO_2 @cellulose was applied as a solid adsorbent in μ SPE for preconcentration of metalloid species from an aqueous solution. After sorption, the filters were directly analyzed by an energy-dispersive x-ray fluorescence spectrometry (EDXRF) for determination of preconcentrated trace amount of selenium and arsenic. Direct analysis of filters by EDXRF does not allow the sample to be contaminated and analytes to be lost. The problems mentioned above usually accompany the more complex treatment of the sample. Moreover, as long as analytes are problematic to elute from adsorbents, a great superiority is direct sample analysis. In addition, due to the high selectivity of membranes, they can be used to separate arsenic(V) and selenium(IV) from other ions present in waters.

Experimental

Reagents, materials, and apparatus

Propanolan titanium ($\text{Ti}(\text{OCH}_2\text{CH}_2\text{CH}_3)_4$) 98%, sodium selenite (Na_2SeO_3) 99%, and sodium selenate (Na_2SeO_4) 98% were purchased from Sigma-Aldrich (Germany); propan-2-ol ($\text{C}_3\text{H}_7\text{OH}$) was purchased from Chempur (Poland); nitric acid (HNO_3) 65% and ammonia solution ($\text{NH}_3\cdot\text{H}_2\text{O}$) 30% p.a. were purchased from POCH (Poland); standard solutions (1 mg mL^{-1}): Se(IV), As(III), and As(V) were purchased from Sigma-Aldrich (Germany), and Cr(III), Cr(VI), Cu(II), Pb(II), Zn(II), and Fe(III) were purchased from Merck (Germany); redistilled water was from Milli-Q System of Millipore (France); filters Whatman 3MM were purchased from GE Healthcare Life Sciences (United Kingdom); Certified Reference Material (CRM) of natural water, NIST 1640a, was purchased from Sigma-Aldrich (Germany).

The following equipment were used for the research: FEI Nova NanoSEM 230 microscope (FEI Company, Hillsboro, Oregon, USA), x-ray powder diffractometer (XRD) (PANalytical, The Netherlands), energy-dispersive x-ray fluorescence spectrometer (EDXRF) XDV-SD model (Helmut Fischer GmbH, Sindelfingen, Germany), energy-dispersive x-ray fluorescence spectrometer (EDXRF) Epsilon 3 model (PANalytical, Almelo, The Netherlands), and inductively coupled plasma optical emission spectrometer (ICP-OES) SpectroBlue FMS16a model (Spectro Analytical Instruments GmbH, Germany). The apparatus is described in detail in [ESM](#).

Synthesis of TiO_2 @cellulose membranes

Two hundred microliters of 4% $\text{Ti}(\text{OC}_3\text{H}_7)_4$ solution in propan-2-ol [16] was pipetted onto a warm cellulose filter (about 60°C) of diameter 25 mm, in order to cover the whole surface. Then, the filters were dried into the oven at 60°C (around 30 min), and they were introduced into beakers with $\text{NH}_3\cdot\text{H}_2\text{O}$ solution (pH 9–10) and agitated for 1 h. After agitation, the filters were put in an oven for 3 h (60°C). Then, the filters were cut into smaller ones, thus obtaining 10 mini-filters (5 mm diameter). The mini-filters with this diameter are well matched to spot size of primary x-ray beam emitted by x-ray tube. Consequently, a large part of the adsorbed ions is excited, and therefore, a high analytical signal is obtained.

Batch adsorption and sample preparation

Experiments aimed at determining adsorption isotherms and developing a preconcentration procedure were preceded by determination of the optimal pH for sorption of analytes. For this purpose, 25 mL single-element aqueous solutions were prepared. Next, obtained mini- TiO_2 @cellulose filters were

immersed in these solutions of the desired concentration and pH. The mini-filters were shaken (250 rpm) to reach the equilibrium of adsorption. After this procedure, dried mini-filters at 60 °C were analyzed by EDXRF, and remaining solutions were analyzed by ICP-OES.

Results and discussion

Preparation of TiO₂@cellulose membranes

The proposed in situ method for developing new cellulose-based sorbents is a simpler method in comparison with the ex situ procedures, in which the metal oxide particles must be synthesized separately and then incorporated in cellulose matrix. Moreover, when using the ex situ methods, the use of retention/covering aids, flocculants, and binders is required. In the in situ methods, metal particles are synthesized on the cellulose matrix directly. The in situ method of sorbent preparation is based on the creation of covalent bonds between TiO₂ molecules and cellulose. As a result, we obtain a high coverage and homogenous distribution of metal particles on the cellulose surface, as well as high availability of metal particles for sorption. Considering the above facts, as well as the simplicity of filter preparation, the proposed method is more favorable than ex situ methods [17]. The in situ formation of TiO₂ particles on the cellulose surface (permanent covalent bonds between TiO₂ and cellulose fibers as result of dehydration reactions between the hydroxyl groups of cellulose and the hydroxyl groups of titania) is demonstrated in Fig. 1. The developed method results in a high covering percent of titania particles into the cellulose fibers, which in turn lead to the formation of available active sites for the sorption. Hydrogen bonds can also be formed between hydroxyl groups presented on the surface of cellulose fibers and TiO₂ particles [18].

The stability of the membranes as well as homogenous distribution of TiO₂ in membranes is very important in the point of view of effective sorption process as well as XRF analysis. Thus, the influence of the following parameters was examined: temperature of cellulose treatment, application

of propan-2-ol, and way of contact ammonia (pipetting, agitating) with membranes covered by Ti(OC₃H₇)₄ solution.

Summarizing this study, the best results we obtained when the preparation of membranes were performed pipetting Ti(OC₃H₇)₄ solution into warm cellulose filter and then agitating the filter with Ti(OC₃H₇)₄ into a beaker with NH₃·H₂O solution (pH 9–10). Agitating the filters with the NH₃·H₂O solution provides the good contact of entire filter surface with the solution, and, in consequence, homogenous distribution of TiO₂ on the membranes is observed. After that, the membranes must stay in the oven for 3 h. The longer time (12 h) the filter was left in the oven did not affect the results.

Considering the above facts, filter characteristics as well as the simplicity of filter preparation, the proposed method is interesting and more advantageous than ex situ methods.

Characterization of TiO₂@cellulose

The TiO₂@cellulose mini-filters were examined with SEM, XRD, and micro-EDXRF. Figure 2 a, b presents the SEM images of the cellulose@TiO₂ membrane. The amorphous fraction of TiO₂ coats cellulose fibers. The spaces between the fibers are also partially filled by the modifier. The results of powder diffraction of pristine and modified cellulose (Fig. 2c) confirm the amorphous form of TiO₂. Both diffractograms exhibit the two characteristic broad peaks of cellulose. However, in the modified sample, the diffracted background is significantly higher compared with the pure cellulose, especially for the low diffraction angles. This is an indicator of the additional, amorphous phase present in the diffracted volume of the TiO₂@cellulose membrane.

Micro-EDXRF mapping is a helpful technique in showing the distribution of the TiO₂ on the cellulose surface as well as analytes on the TiO₂@cellulose. The real image of the sorbent surface with actual distribution of analytes was created by analyzing small areas of mini-filters using a suitably small collimator. In Fig. S1, 2D-mapping pictures of TiO₂@cellulose are presented. As can be seen (see Fig. S1), titanium is distributed over the whole cellulose surface, and the mass per unit area is homogenous. For titanium, the mean mass per unit area is 108.2 ± 8.8 μg cm⁻².

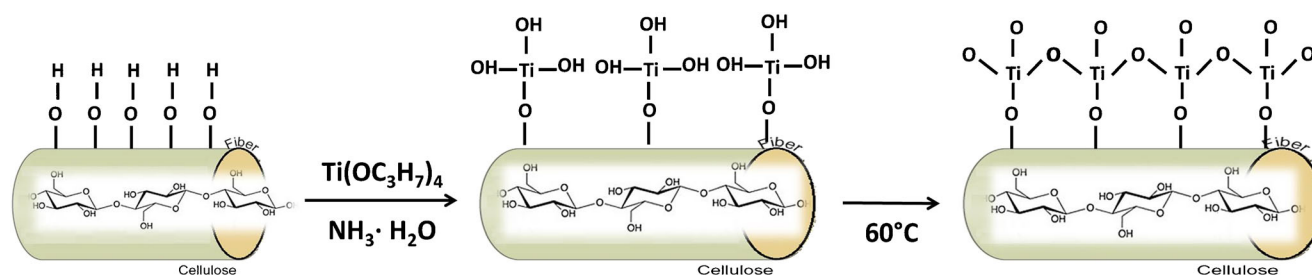


Fig. 1 In situ formation of TiO₂ particles on cellulose filters



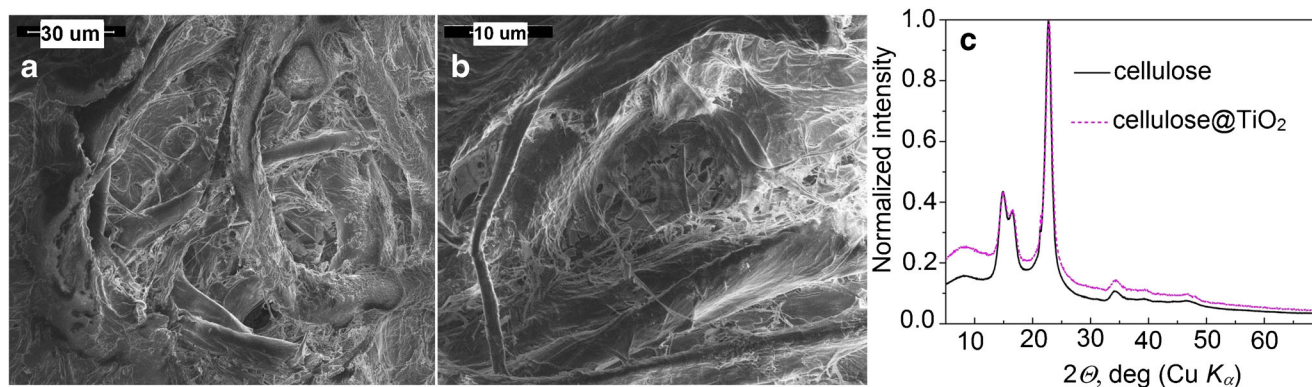


Fig. 2. **a, b** SEM images of cellulose@TiO₂. **c** XRD of pure cellulose membrane and modified cellulose @TiO₂

Adsorption study

The goal of the pH study is to know which ions are absorbed and which is the best pH for the adsorption of selected oxyanions. According to the results in Fig. S2, both Se(IV) as well as As(V) are adsorbed on TiO₂@cellulose with the highest recovery (near 100%) at pH = 2. Se(VI) and As(III) are adsorbed with maximum recovery about 10% and 20%, respectively. The Se(VI) is included in the group of oxyanions with moderate or weak affinity, among others, for Al₂O₃ and FeOOH [19]. The results of XPS and electrophoretic mobility clearly showed that the bond between selenium(VI) and TiO₂ is mainly weak electrostatic attraction [20]. Our research also confirms that Se(VI) ions are weakly adsorbed ions on TiO₂@cellulose in comparison to Se(IV). At pH < 3, Se(IV) is probably adsorbed as H₂SeO₃(aq) and HSeO₃⁻ [21] and As(V) as H₃AsO₄ and H₂AsO₄⁻ ions [22]. The species for Se(VI), Se(IV), As(V), and As(III) in aqueous solutions at varied pH are presented in Fig. S2.


The surface charge of the adsorbent also depends on the pH. The surface charge is related to what ions (H⁺ or OH⁻) are released during the adsorption process. As(V) adsorption is accompanied by the release of OH⁻ ions, while As(III) adsorption at acidic pH is accompanied by H⁺ release [23]. As long as anion adsorption is associated with the release of OH⁻ ions, better adsorption occurs at a lower pH. The formation of arsenic ion complexes with titanium dioxide is another option. Given the above considerations, As(V) can only form Ti₂AsO₄⁻. The interactions between TiO₂ and H₂AsO₄⁻ can be as follows:




With bidentate ligands (mono nuclear or binuclear), surface chelates are formed.

The maximum uptake of As(V) occurred at approximately pH 2 (Fig. S2), and it is convergent with the first dissociation constant of H₃AsO₄ (pK_{a1} = 2.25). The same situation is observed in case of H₂SeO₃ (pK_{a1} = 2.46). This fact confirms statement that pK_{a1} of weak acid adsorbed by metal oxides is close to the pH at which the highest adsorption of this acid is observed [24]. The pK_{a1} of H₃AsO₃ is 9.22, and consistently, the growing the adsorption of the As(III) at pH 9 is observed. Thus, the sorption of As(V) and Se(IV) can be explained by similar acidic strength of arsenic acid and selenous acid.



The adsorption of arsenic acid and selenous acid can occur via complexation reactions onto sorbent surface [25]:



and analogously



Surface complexation of HSeO₃⁻ can be illustrated by the following reactions:



The adsorption of Se(IV) and As(V) on TiO₂@cellulose at pH 2 was simulated using Langmuir and Freundlich isotherm models (for details, see Adsorption isotherms in [ESM](#) and [Table S1](#)).

The maximum adsorption capacities (q_{max}) of our mini-filters determined in this work as well as other single and mixed oxides as adsorbents described in the literature in relation to selenium and arsenic are presented in [Table 1](#).

As can be seen in [Table 1](#), iron, manganese, cerium, and aluminum oxides, usually as mixed oxides or composites, have been evaluated for selenium and arsenic species

Table 1 Maximum adsorption capacities (q_{\max}) for selenium(IV) and arsenic(V) by single and mixed oxides

Adsorbent	Species	pH	q_{\max} , mg g ⁻¹	Ref.
Fe–Mn hydrous oxides	Se(IV)	4	41.02	[26]
MGO composites	Se(IV)	6–9	23.81	[27]
Mn ₃ O ₄ nanomaterial	Se(IV)	4	0.8	[28]
MnFe ₂ O ₄ nanomaterial	Se(IV)	4	6.57	[29]
Ce–Mn binary oxide	As(V)	7	63.6	[30]
Zr-doped TiO ₂	As(V)	3	32.4	[31]
Cu doped Fe ₃ O ₄	As(V)	5	42.9	[32]
Al ₂ O ₃ /GO	As(V)	5	43.9	[33]
G/CeO ₂	Se(IV) As(V)	3 4	14.1 8.4	[34]
GO/CeO ₂	Se(IV) As(V)	3 5	10.7 5.8	[35]
TiO ₂ @cellulose	Se(IV) As(V)	2 2	71.1 49.2	This work

adsorption. Maximum adsorption capacities for selenium (IV) are in range of 0.8–64 mg g⁻¹. In the light of these results, the obtained maximum sorption capacity of the developed mini-TiO₂@cellulose is impressively high, i.e., almost twice as high as the highest literature value. In case of arsenic, the maximum sorption capacity of the obtained material is comparable to the others shown in the Table 1, with the exception of composites with cerium oxides, for which the maximum sorption capacities are about 7 times lower than for TiO₂@cellulose. Comparing the maximum sorption capacity of the obtained membranes with the composite of zirconium ions incorporated into crystal structure of titanium dioxide, we conclude that they are comparable. However, TiO₂@cellulose also gives the possibility of adsorption of Se (IV) at the same pH. Thus, its use is wider, because at the same time, we can absorb and then determine both As(V) as well as Se(IV). In this way, we save time, the amount of sorbent and analyzed sample, and we do not generate additional wastes. This aspect of the developed method is therefore extremely important from the point of view of environmental protection, as well as compliance with the principles of green analytical chemistry.

The contact time of membrane with analyte solution can significantly affect the adsorption of analytes percentage, particularly when high sample volume is used. The influence of contact time and the sample volume on the adsorption of Se(IV) and As(V) were studied in the range of time, 5–180 min and sample volume, 20–100 mL. Figure S3 shows that quantitative adsorption of both Se(IV) as well as As(V) is achieved then the shaking time was at least 120 min. It should be also emphasized that even when the membranes were vigorously shaken (250 rpm) in an aqueous solution for 180 min, no damage was noted. This indicates a high durability and stability of the obtained membranes. When considering sorption time of

developed method, it can get the impression that it is quite long and may be considered a slight drawback. However, since the method involves only shaking the filters in the analyte solution, nothing stands in the way to prepare many samples at one time using an orbital platform shaker. Simultaneous sample preparation is therefore very beneficial, especially if the method is not labor intensive.

Interferent study

Considering the coexisting cations, anions and natural organic matter (NOM) included humic acid (HA) in real water samples, and the influence of Na⁺, K⁺, Mg²⁺, Ca²⁺, Al³⁺, Fe³⁺, SO₄²⁻, PO₄³⁻, Cl⁻, NO₃⁻, and HA on the recovery of Se(IV) and As(V) adsorbed on TiO₂@cellulose was investigated. The obtained results are shown in Table S2 and Fig. S4. The high tolerance of TiO₂@cellulose for foreign ions is observed. Therefore, it can be concluded that the obtained mini-membranes can be used to quantify trace amounts of arsenic and selenium, in presence of many another ions in water, by EDXRF in a simple and straightforward manner.

Validation parameters

The analytical figures of merit of developed μ SPE/EDXRF are presented in Table 2 and Fig. 3. The calibration plot is reflected in a correlation coefficient R of 0.999 and 0.999 for Se(IV) and As(V), respectively. The limit of detection (LOD) and limit of quantification (LOQ) were calculated from the following equations: $LOD = (3 \cdot k^{-1}) \cdot (R_B \cdot t^{-1})^{1/2}$, where k is the sensitivity of the method, R_B is the background count rate in counts·s⁻¹, and t is the counting time, and $LOQ = 3 \cdot LOD$. The good LODs mean 0.4 ng mL⁻¹ and 0.25 ng mL⁻¹ for selenium and arsenic, respectively, characterized developed method.

Please note that the LODs are 125 and 40 times lower for selenium and arsenic, respectively, than the acceptable maximum contaminant levels (MCL) of these elements. MCL of

Table 2 Analytical figures of merit of the μ SPE/EDXRF using TiO₂@cellulose as solid adsorbent. Measurement conditions: Rh x-ray tube operated at 30 kV and 300 μ A, 300 s counting time, air atmosphere, and Ag primary beam filter

Parameter	Se(IV)	As(V)
Linearity, ng mL ⁻¹	2–50	2–50
Correlation coefficient R	0.999	0.999
Sensitivity, mL ng ⁻¹ s ⁻¹	0.479	0.379
LOD, ng mL ⁻¹	0.4	0.25
LOQ, ng mL ⁻¹	1.2	0.75
RSD, %	4.5	4.5

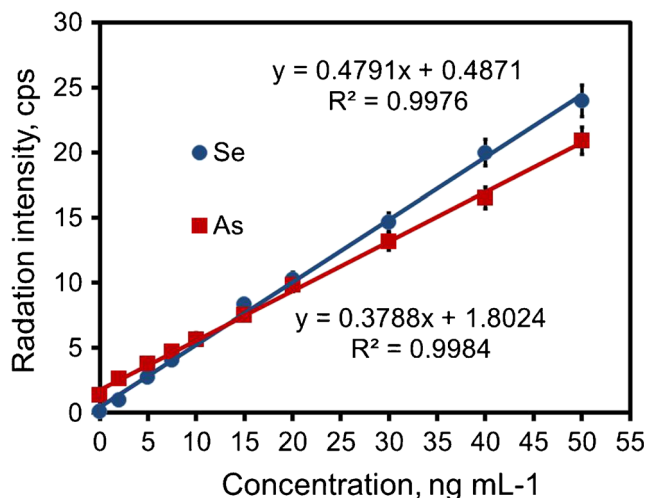


Fig. 3 Calibration curves of the signal intensities vs the concentrations of Se and As

50 ng mL⁻¹ (for Se) and 10 ng mL⁻¹ (for As) is established by US EPA.

The method precision expressed by the relative standard deviation (RSD) is 4.5% for both analytes. In case of trace analysis, this value should be considered as very good. Good precision results *inter alia* from the high homogeneity of the surface of the analyzed samples. As illustrated in Fig. 4, the mapping of TiO₂@cellulose with analytes confirms that the distribution of selenium as well as arsenic is homogenous in

the whole TiO₂@cellulose surface. The mappings in Fig. 4 clearly show that the distribution of titanium and selenium or titanium and arsenic is overlapping. The distribution of elements expressed as the mass per unit area for Ti is higher than for Se and As. This fact resulted from the differences in concentration of Ti and Se or As in the analyzed samples. Titanium as TiO₂ beside cellulose is the main component of analyzed membranes. The high titanium concentration allows covering whole cellulose surface. Although the concentration of selenium and arsenic is at trace level, the distribution of selenium as well as arsenic is homogeneous. This fact shows that the metalloids sorption occurs evenly over the entire membrane surface.

In Tables 3 and 4, the methods of determination of Se(IV) and As(V) using various adsorbents based on cellulose membranes are compared, respectively.

Three basic advantages of the developed method should be emphasized, looking at the others presented in the Tables 3 and 4, i.e., (1) a very low mass of the sorbent used, which is the smallest one among masses used in all other methods; (2) no need to elute the analytes after sorption and before the determination; and also (3) the possibility of simultaneous determination of both selenium and arsenic in one sample. In case of method using graphene membrane and cellulose/SiO₂/MPTMS, the analytes did not have to be also eluted, but the mass of sorbents was about 2 and 15 times bigger, and additionally, in case of

Fig. 4 Mapping of TiO₂@cellulose with adsorbed Se(IV) or As(V). **a** Distribution patterns of Ti and Se(IV) on TiO₂@cellulose. **b** Distribution patterns of Ti and As(V) on TiO₂@cellulose

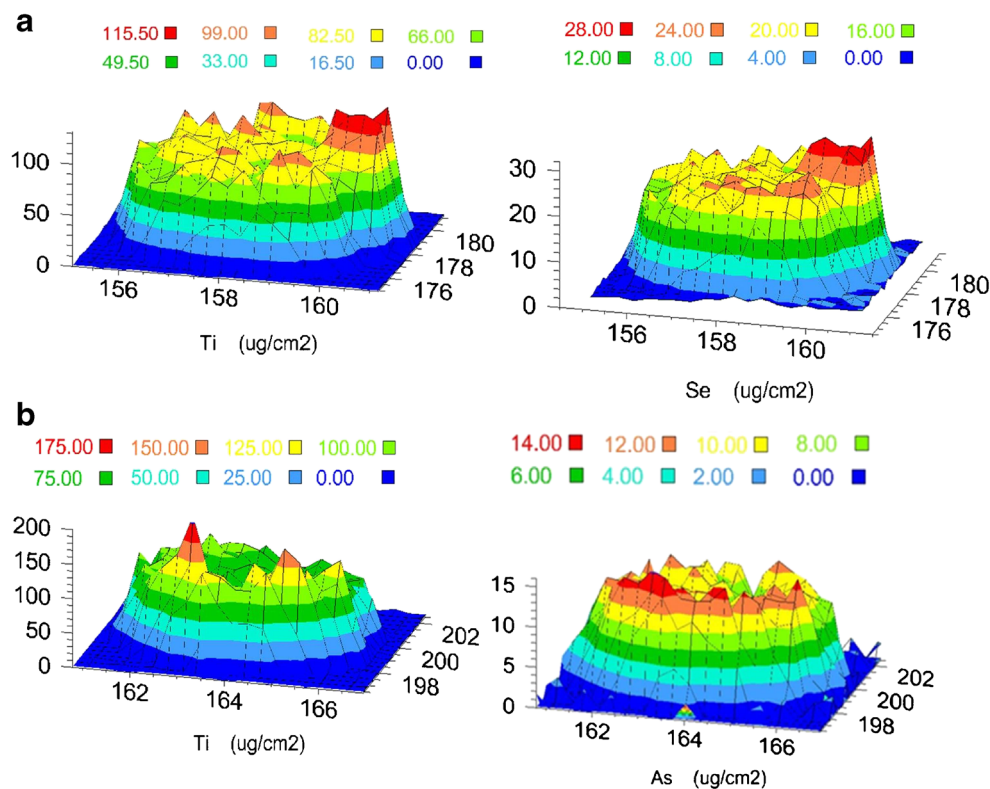


Table 3 The determination of selenium species with various adsorbents based on cellulose membranes

Analyte	pH	Sorbent	Mass of sorbent, mg	Eluent	LOD, ng·mL ⁻¹	RSD, %	Technique detection	Ref.
Se(IV)	3	Graphene membrane /APDC ^a	0.45	–	0.15	2.3	TXRF ^c	[9]
Se(IV)	4.5	TMA-C ^b	20	3.0 mol/L HCl-2% KClO ₃	–	2	ICP-OES ^d	[1]
Se(IV)	6	La(OH) ₃ coated on cellulose fiber	5	1.0% NaBH ₄ (in 1.0% NaOH)	0.009	1.7	HG-AFS ^e	[5]
Se(IV)		Cellulose TLC plate	–	–	3.2	3.3	DLTV-ICP-MS ^f	[8]
Se(VI)								
Se(IV)	2.0	TiO ₂ @ cellulose	0.25*	Solvent-free	0.4	4.5	EDXRF	This work

*mass of TiO₂^aAmmonium pyrrolidinedithiocarbamate^bCellulose grafted thiomalic acid^cTotal reflection x-ray fluorescence spectrometry^dInductively coupled plasma-optical emission spectrometry^eHydride generation atomic fluorescence spectrometry^fDiode laser thermal vaporization inductively coupled plasma mass spectrometry

the first mentioned sorbent, it was necessary to use a chelating agent (APDC) for sorption of analytes. The method with cellulose TLC plate and DLTV-ICP-MS detection was performed without elution of analytes, but LODs obtained then were about 10 times worse in comparison with developed method. As can be seen in Tables 3 and 4, the value of LOD depends on detection technique. The lowest LODs were achieved using HG-AFS. However, in case of EDXRF with very low-power x-ray tube (9 W) without gas consumption, LODs obtained for analytes should be considered as very good. Therefore, taking all this into account, the developed method coupled with EDXRF analysis can be considered as new, promising, and competitive compared with previous ones and also environmentally friendly, lying in the green principles of analytical chemistry.

Application

The trustworthiness of the developed procedure was established on the basis of the analysis of various types of drinking waters. The studies were performed using waters spiked with analytes at two concentration levels (7.5 and 10 ng·mL⁻¹). As demonstrated in Table S3, for all the studied water matrices, recoveries near 100% were assessed. Since TiO₂@cellulose is highly selective towards Se(IV) and As(V) at pH 2, the speciation analysis can also be performed (see Table S4). The total concentration of Se was calculated after reduction of Se(VI) to Se(IV) with H₂SO₄ and C₂H₅OH. The total concentration of As was calculated after oxidation of As(III) to As(V) with KMnO₄. Then, the Se(VI) and As(III) content was calculated as the difference between total Se and Se(III) or

Table 4 The determination of arsenic species with various adsorbents based on cellulose membranes

Analyte	pH	Sorbent	Mass of sorbent, mg	Eluent	LOD, ng·mL ⁻¹	RSD, %	Technique detection	Ref
As(III)	3	Graphene membrane/APDC ^a	0.45	–	0.2	4.1	TXRF ^d	[9]
As(V)	6	MESM ^b	10	1.5 mol L ⁻¹ HCl	0.015	3.5	HG-AFS ^e	[6]
As(III)	1	cellulose/SiO ₂ /MPTMS ^c	4.4	–	0.045	5.6	EDXRF ^f	[10]
As(V)	2.0	TiO ₂ @ cellulose	0.25*	Solvent-free	0.25	4.5	EDXRF	This work

*mass of TiO₂^aAmmonium pyrrolidinedithiocarbamate^bMethyl esterified egg-shell membrane^cSilica coating cellulose fibers modified with (3-mercaptopropyl)-trimethoxysilane^dTotal reflection x-ray fluorescence spectrometry^eHydride generation atomic fluorescence spectrometry^fEnergy-dispersive x-ray fluorescence spectrometry

Table 5 Analysis of CRM (NIST 1640a) (\pm std.; $n = 3$)

Analyte	Certified concentration, $\mu\text{g L}^{-1}$	Obtained concentration, $\mu\text{g L}^{-1}$	Error, %	Recovery, %	t test ($t_{0.05} = 2.92$)
As	8.075 ± 0.070	8.5 ± 0.52	5.2	105	1.42
Se	20.13 ± 0.17	18.9 ± 0.83	6.1	94	2.57

Concentration of minor elements in mg L^{-1} : Ca (5.615 ± 0.021), Mg (1.0586 ± 0.0041), K (0.5799 ± 0.0023), Si (5.210 ± 0.021), and Na (3.137 ± 0.031); concentration of trace element in $\mu\text{g L}^{-1}$: Al (53.0 ± 1.8), Ba (151.80 ± 0.83), B (303.1 ± 3.1), Cr (40.54 ± 0.30), Co (20.24 ± 0.24), Cu (85.75 ± 0.51), Fe (36.8 ± 1.8), Mn (40.39 ± 0.36), Mo (45.60 ± 0.61), Ni (25.32 ± 0.14), Pb (12.101 ± 0.050), Sr (126.03 ± 0.27), U (25.35 ± 0.27), V (15.05 ± 0.25), and Zn (55.64 ± 0.35)

As(V) concentration, respectively. The results presented in Table S4 indicate that method can be successfully applied for speciation of selenium and arsenic species in real water samples with good recovery and precision.

The developed method was used to determine selenium and arsenic in the CRM of natural water (NIST 1640a) to assess its accuracy. The results of this analysis are shown in Table 5. The high compatibility of certified values with determined analyte concentrations supports the suitability of the TiO_2 @cellulose membrane in routine ultratrace analysis. The error of determination of analytes with developed method is about 5.5%, and recovery is near 100%.

Conclusion

This research was focused on the development eco-friendly cellulose-based membrane (TiO_2 @cellulose). The incorporation of TiO_2 particles into raw cellulose filter by developed in situ method is more beneficial than ex situ procedures. TiO_2 @cellulose membranes obtained in this way are characterized by high maximum adsorption capacity, excellent stability in aqueous solutions, and high homogeneity. The selectivity of TiO_2 @cellulose membranes towards Se(IV) and As(V) indicates their potential application in speciation of these metalloids. Taking advantage of the excellent properties of membranes, a simple method for determining trace amounts of selenium and arsenic in water, was developed. The simultaneous adsorption/determination of Se(IV) and As(V) at the same pH using very low mass of adsorbent and without the need for using additional reagents, such as a chelating agent, is profitable. Even though the adsorption time can be considered as not very short, still as long as the orbital platform shaker is applied, the procedure is not labor-intensive and demanding since many samples are prepared at once. Because the ultratrace amounts of metalloid species are simultaneously and directly determined onto the mini-membranes without the need for eluting analytes, the quantitative analysis is not only easy and cost-effective, but also fulfilling the green analytical chemistry principles.

Compliance with ethical standards

Competing interests The authors declare that they have no conflicts of interest.

Conflict of interest The authors declare that they have no competing of interests.

Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

References

1. Min M, Shen C, Fang L, Zhu B, Li J, Yao L, Jiang Y, Xiong C (2017) Design of a selective regenerable cellulose microcolumn for selenium efficient recovery and economic determination. *Chem Eng Res Des* 117:773–783. <https://doi.org/10.1016/j.cherd.2016.11.032>
2. Tuzen M, Saygi KO, Soylak M (2007) Separation and speciation of selenium in food and water samples by the combination of magnesium hydroxide coprecipitation-graphite furnace atomic absorption spectrometric determination. *Talanta* 71:424–429. <https://doi.org/10.1016/j.talanta.2006.04.016>
3. Saygi KO, Melek E, Tuzen M, Soylak M (2007) Speciation of selenium(IV) and selenium(VI) in environmental samples by the combination of graphite furnace atomic absorption spectrometric determination and solid phase extraction on Diaion HP-2MG. *Talanta* 71:1375–1381. <https://doi.org/10.1016/j.talanta.2006.07.008>
4. Tuzen M, Saygi KO, Karaman I, Soylak M (2010) Selective speciation and determination of inorganic arsenic in water, food and biological samples. *Food Chem Toxicol* 48:41–46. <https://doi.org/10.1016/j.fct.2009.09.012>
5. Chen M, Yang T, Wang J (2009) Precipitate coating on cellulose fibre as sorption medium for selenium preconcentration and speciation with hydride generation atomic fluorescence spectrometry. *Anal Chim Acta* 631:74–79. <https://doi.org/10.1016/j.aca.2008.10.019>

6. Chen M-L, Gu C-B, Yang T, Sun Y, Wang J-H (2013) A green sorbent of esterified egg-shell membrane for highly selective uptake of arsenate and speciation of inorganic arsenic. *Talanta* 116:688–694. <https://doi.org/10.1016/j.talanta.2013.07.061>
7. Su CK, Chen WC (2018) 3D-printed, TiO₂ NP-incorporated minicolumn coupled with ICP-MS for speciation of inorganic arsenic and selenium in high-salt-content samples. *Microchim Acta* 185:268–276. <https://doi.org/10.1007/s00604-018-2812-8>
8. Bednarik A, Kuta J, Vu DL, Ranglová K, Hrouzek P, Kanicky V, Preisler J (2018) Thin-layer chromatography combined with diode laser thermal vaporization inductively coupled plasma mass spectrometry for the determination of selenomethionine and selenocysteine in algae and yeast. *J Chromatogr A* 1533:199–207. <https://doi.org/10.1016/j.chroma.2017.12.017>
9. de la Calle I, Ruibal T, Lavilla I, Bendicho C (2019) Direct immersion thin-film microextraction method based on the sorption of pyrrolidine dithiocarbamate metal chelates onto graphene membranes followed by total reflection x-ray fluorescence analysis. *Spectrochim Acta Part B* 152:14–24. <https://doi.org/10.1016/j.sab.2018.12.005>
10. Lukojko E, Talik E, Gagor A, Sitko R (2018) Highly selective determination of ultratrace inorganic arsenic species using novel functionalized miniaturized membranes. *Anal Chim Acta* 1008: 57–65. <https://doi.org/10.1016/j.aca.2017.12.038>
11. Kalantari H, Manoochehri M (2018) A nanocomposite consisting of MIL-101(Cr) and functionalized magnetite nanoparticles for extraction and determination of selenium(IV) and selenium(VI). *Microchim Acta* 185:196–204. <https://doi.org/10.1007/s00604-018-2731-8>
12. Hashemi B, Rezaei S (2019) Carbon-based sorbents and their nanocomposites for the enrichment of heavy metal ions: a review. *Microchim Acta* 186:578–598. <https://doi.org/10.1007/s00604-019-3668-2>
13. Musielak M, Gagor A, Zawisza B, Talik E, Sitko R (2019) Graphene oxide/carbon nanotube membranes for highly efficient removal of metal ions from water. *ACS Appl Mater Interfaces* 11: 28582–28590. <https://doi.org/10.1021/acsami.9b11214>
14. Fuerstenau DW, Osseo-Asare K (1987) Adsorption of copper, nickel, and cobalt by oxide adsorbents from aqueous ammoniacal solutions. *J Colloid Interf Sci* 118:524–542. [https://doi.org/10.1016/0021-9797\(87\)90487-5](https://doi.org/10.1016/0021-9797(87)90487-5)
15. Morterra C (1988) An infrared spectroscopic study of anatase properties. *J Chem Soc Faraday Trans I* 84:1617–1637. <https://doi.org/10.1039/F19888401617>
16. Yan Y, Liu Q, Du X, Qian J, Mao H, Wang K (2015) Visible light photoelectrochemical sensor for ultrasensitive determination of dopamine based on synergistic effect of praphene quantum dots and TiO₂ nanoparticles. *Anal Chim Acta* 853:258–264. <https://doi.org/10.1016/j.aca.2014.10.021>
17. Adel AM (2016) Incorporation of nano-metal particles with paper matrices. *Interdiscip J Chem* 1:36–46. <https://doi.org/10.15761/IJC.1000107>
18. Chauhan I, Mohanty P (2015) In situ decoration of TiO₂ nanoparticles on the surface of cellulose fibers and study of their photocatalytic and antibacterial activities. *Cellulose* 22:507–519. <https://doi.org/10.1007/s10570-014-0480-3>
19. Sposito G (1984) *The surface chemistry of soils*. University Press Inc, Oxford
20. Jordan N, Foerstendorf H, Weiß S, Heim K, Schild D, Brendler V (2011) Sorption of selenium(VI) onto anatase: macroscopic and microscopic characterization. *Geochim Cosmochim Acta* 75: 1519–1530. <https://doi.org/10.1016/j.gca.2011.01.012>
21. Awwal MR, Hasan MM, Khaleque MA (2015) Efficient selenium (IV) detection and removal from water by tailor-made novel conjugate adsorbent. *Sens Actuat B Chem* 209:194–202. <https://doi.org/10.1016/j.snb.2014.11.010>
22. Veličković Z, Vuković GD, Marinković AD, Moldovand M-S, Perić-Grujić AA, Uskoković PS, Ristić MD (2012) Adsorption of arsenate on iron(III) oxide coated ethylenediamine functionalized multiwall carbon nanotube. *Chem Eng J* 181:174–181. <https://doi.org/10.1016/j.cej.2011.11.052>
23. Dutta PK, Ray AK, Sharma VK, Millero FJ (2004) Adsorption of arsenate and arsenite on titanium dioxide suspensions. *J Colloid Interf Sci* 278:270–275. <https://doi.org/10.1016/j.jcis.2004.06.015>
24. Stumm W (1992) *Chemistry of the solid-water interface: processes at the mineral-water and particle-water interface in natural systems*. Wiley Inc, New York
25. Pena ME, Korfiatis GP, Patel M, Lippincott L, Meng X (2005) Adsorption of as(V) and as(III) by nanocrystalline titanium dioxide. *Water Res* 39:2327–2337. <https://doi.org/10.1016/j.watres.2005.04.006>
26. Szlachta M, Chubar N (2013) The application of Fe–Mn hydrous oxides based adsorbent for removing selenium species from water. *Chem Eng J* 217:159–168. <https://doi.org/10.1016/j.cej.2012.11.100>
27. Fu Y, Wang J, Liu Q, Zeng H (2014) Water-dispersible magnetic nanoparticle–graphene oxide composites for selenium removal. *Carbon* 77:710–721. <https://doi.org/10.1016/j.carbon.2014.05.076>
28. Gonzalez CM, Hernandez J, Parsons JG, Gardea-Torresdey JL (2011) Adsorption of selenite and selenate by a high- and low-pressure aged manganese oxide nanomaterial. *Instrum Sci Technol* 39:1–19. <https://doi.org/10.1080/10739149.2010.537721>
29. Gonzalez CM, Hernandez J, Parsons JG, Gardea-Torresdey JL (2010) A study of the removal of selenite and selenate from aqueous solutions using a magnetic iron/manganese oxide nanomaterial and ICP-MS. *Microchem J* 96:324–329. <https://doi.org/10.1016/j.microc.2010.05.005>
30. Chen J, Wang J, Zhang G, Wu Q, Wang D (2018) Facile fabrication of nanostructured cerium-manganese binary oxide for enhanced arsenite removal from water. *Chem Eng J* 334:1518–1526. <https://doi.org/10.1016/j.cej.2017.11.062>
31. Andjelkovic I, Jovic B, Jovic M, Markovic M, Stankovic D, Manojlovic D, Roglic G (2016) Microwave-hydrothermal method for the synthesis of composite materials for removal of arsenic from water. *Environ Sci Pollut Res* 23:469–476. <https://doi.org/10.1007/s11356-015-5283-z>
32. Wang T, Yang W, Song T, Li C, Zhang L, Wang H, Chai L (2015) Cu doped Fe₃O₄ magnetic adsorbent for arsenic: synthesis, property, and sorption application. *RSC Adv* 5:50011–50018. <https://doi.org/10.1039/C5RA03951G>
33. Baranik A, Gagor A, Queralt I, Marguí E, Sitko R, Zawisza B (2018) Determination and speciation of ultratrace arsenic and chromium species using aluminium oxide supported on graphene oxide. *Talanta* 185:264–274. <https://doi.org/10.1016/j.talanta.2018.03.090>
34. Baranik A, Gagor A, Queralt I, Marguí E, Sitko R, Zawisza B (2018) Ceria nanoparticles deposited on graphene nanosheets for adsorption of copper(II) and lead(II) ions and of anionic species of arsenic and selenium. *Microchim Acta* 185:264–272. <https://doi.org/10.1007/s00604-018-2806-6>
35. Baranik A, Sitko R, Gagor A, Queralt I, Marguí E, Zawisza B (2018) Graphene oxide decorated with cerium(IV) oxide in determination of ultratrace metal ions and speciation of selenium. *Anal Chem* 90:4150–4159. <https://doi.org/10.1021/acs.analchem.8b00137>

Publisher's note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.