

7

3 **A new method for the determination of low-level actinium-227**
4 **in geological samples**5 **Henrieta Dulaiova · Kenneth W. W. Sims ·**
6 **Matthew A. Charette · Julie Prytulak ·**
7 **Jerzy S. Blusztajn**8 Received: 31 July 2012
9 © Akadémiai Kiadó, Budapest, Hungary 2012

10 **Abstract** We developed a new method for the determi-
11 nation of ^{227}Ac in geological samples. The method
12 uses extraction chromatographic techniques and alpha-
13 spectrometry and is applicable for a range of natural matri-
14 ces. Here we report on the procedure and results of the
15 analysis of water (fresh and seawater) and rock samples.
16 Water samples were acidified and rock samples underwent
17 total dissolution via acid leaching. A DGA (N,N,N',N' -tetra-
18 n -octyldiglycolamide) extraction chromatographic column
19 was used for the separation of actinium. The actinium frac-
20 tion was prepared for alpha spectrometric measurement via
21 cerium fluoride micro-precipitation. Recoveries of actinium
22 in water samples were $80 \pm 8 \%$ (number of analyses
23 $n = 14$) and in rock samples $70 \pm 12 \%$ ($n = 30$). The
24 minimum detectable activities (MDA) were 0.017 –
25 0.5 Bq kg^{-1} for both matrices. Rock sample ^{227}Ac activities
26 ranged from 0.17 to 8.3 Bq kg^{-1} and water sample activities

ranged from below MDA values to 14 Bq kg^{-1} of ^{227}Ac . 27
From the analysis of several standard rock and water samples 28
with the method we found very good agreement between our 29
results and certified values. 30
31

Keywords Actinium-227 · Extraction chromatography · 32
Water · Rock · Alpha-spectrometry 33

Introduction 34

Actinium-227 is a member of the naturally occurring ^{235}U 35
decay series (Fig. 1). It is a beta-emitter with a half-life of 36
 $T_{1/2} = 21.77$ years. The concentration of ^{227}Ac in natural 37
samples is extremely low, in seawater the reported activities 38
range from 0.83 to 90 mBq m^{-3} [1], in some basalts, 39
assuming equilibrium with ^{231}Pa , the expected range can be 40
as low as <0.1 – 5 Bq kg^{-1} [2]. Actinium-227 is used as an 41
oceanographic tracer for studies of deep-ocean mixing and 42
upwelling [1, 3], and it has the potential to be used as a tracer 43
for geochemical characterization of rocks and other geo- 44
logical material. Some already existing techniques for ^{227}Ac 45
analysis include separation on ion exchange columns fol- 46
lowed by measurement of its daughters ^{227}Th and ^{223}Ra by 47
alpha-spectrometry [4, 5]. The disadvantage of the ion 48
exchange columns is that chemical recoveries tend to be 49
lower (~ 50 – 60%) and may not be well suited for actinium 50
separation from complex matrices. Another popular method 51
uses a radium delayed coincidence counting (RaDeCC) 52
system [6]. Actinium-227 in water samples is quantitatively 53
sorbed on a MnO_2 -coated acrylic fiber and allowed to sit for 54
 90 days for ^{223}Ra ingrowth. The fiber is then measured by the 55
RaDeCC system in which the ^{219}Rn – ^{215}Po pair is counted. 56
This technique works well for seawater analysis for example 57
[6], but is impractical for rock samples. 58

A1 H. Dulaiova (✉)
A2 Department of Geology and Geophysics, University of Hawaii,
A3 1680 East-West Road, POST 707, Honolulu, HI 96822, USA
A4 e-mail: hdulaiov@hawaii.edu

A5 K. W. W. Sims
A6 Department of Geology and Geophysics, University
A7 of Wyoming, Laramie, WY 82071, USA

A8 M. A. Charette
A9 Department of Marine Chemistry and Geochemistry, Woods
A10 Hole Oceanographic Institution, Woods Hole, MA 02543, USA

A11 J. Prytulak
A12 Department of Earth Science and Engineering, Imperial College,
A13 London SW7 2AZ, UK

A14 J. S. Blusztajn
A15 Department of Geology and Geophysics, Woods Hole
A16 Oceanographic Institution, Woods Hole, MA 02543, USA

We adapted a single-column extraction chromatographic technique (DGA column), which simplifies the separation step, reduces analysis time and the amount of reagents needed. The use of this technique assures clean separation of actinium from other elements and leads to close to quantitative chemical recoveries from diverse geological matrices. Here we report on its use for ^{227}Ac separation from freshwater, seawater, and rock samples.

Experimental

Experimental design


A commercially available extraction chromatographic resin containing N,N,N',N' -tetra- n -octyldiglycolamide sorbed on 50–100 μm particle size Amberchrom^R CG-71 (DGA column manufactured by Eichrom Technologies, Inc [7]) was chosen for separation of actinium from other actinides and the sample matrix. This resin has high adsorption capacity for rare earth elements and actinides (0.086 mmol/mL of Eu) and various concentrations of acidic solutions allow a sequential elution of individual elements. The separation sequence for Ac was selected based on distribution coefficients of actinides and common ions on DGA derived by Horwitz et al. [7] using batch experiments for 1-h contact time of solutes with DGA at 22 °C. Figure 2 illustrates k' for Ac, Th, Fe and alkaline earth cations in each separation and rinsing step on the column. K' is defined as the volume distribution ratio of the element between the stationary extractant phase and the mobile aqueous phase times the ratio of the volumes of the stationary and mobile phases in a

slurry packed column. We used 4 M HCl as load solution for which the k' of Ac is 20, of Th, U and Am is $>1,000$, of Ba, Sr, Ca and Ra is 1–5, and of Fe is 1,000. Based on these k' values, actinides and iron are well retained on the column with a 4 M HCl load solution while radium and other alkaline earth elements have no affinity and pass through the column without retention. We used 3 M HNO_3 to rinse any leftover alkaline earth elements and iron from the column. In 3 M HNO_3 the k' of iron drops to <2 , while all actinides including Ac have $k' >1,000$. In the next step we eluted actinium with 2 M HCl, which is efficient for Ac but leaves Th and other actinides retained on the DGA column. If needed for further analysis, thorium (^{228}Th for ^{228}Ac or ^{227}Th analysis) can be stripped from the column using dilute nitric acid [7]. We tested the procedure using an aliquot of NIST certified $^{229}\text{Th}/^{225}\text{Ac}$ standard solution (Fig. 1), which offered an ideal opportunity to demonstrate good separation between actinium and thorium on the DGA column. Consistent with the findings of Horwitz et al. [7] we observed that the presence of iron in the load solution positively affects the actinium uptake on DGA due to the salting out effect. Therefore, each load solution was spiked with 1 mg of iron as FeCl_3 .

Chemical procedure

Rock samples were crushed to <1 mm and then dissolved completely by a series of digestions using HF and HNO_3 , followed by $\text{HNO}_3 + \text{H}_3\text{BO}_3$ and HClO_4 to decompose fluorides [8]. In the final stage they were dissolved and stored in 4 M or higher HCl + sat. H_3BO_3 until analysis. Freshwater and seawater samples were acidified to pH 1.

Fig. 1 Decay schemes of **a** ^{235}U including ^{227}Ac and its daughters ^{227}Th – ^{223}Ra , and **b** the ^{229}Th – ^{225}Ac pair used as a yield tracer. The vertical arrows indicate alpha decays and the tilted arrows represent transformations via beta decay. Half-lives are indicated below each isotope

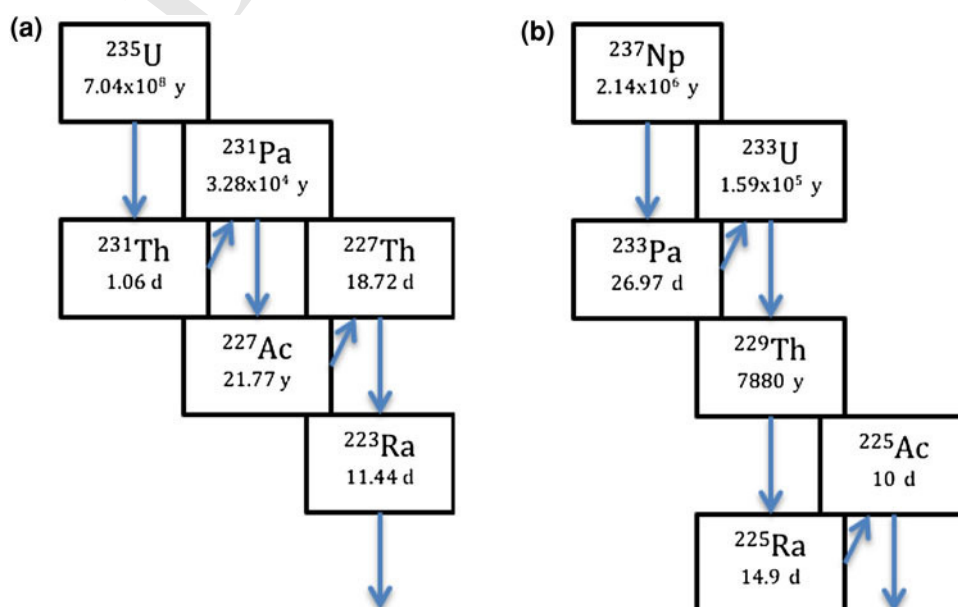




Fig. 2 Resin capacity factor k' for Ac, Th, Fe and alkaline earth cations in each separation and rinsing step on the DGA column derived using batch experiments for 1-hour contact time of solutes with DGA at 22 °C [7]. The higher the k' the higher the fraction of the element in the stationary extractant phase

All samples were spiked using a NIST certified $^{229}\text{Th}/^{225}\text{Ac}$ tracer.

While it is possible for water samples to be evaporated, dissolved in 4 M HCl and loaded to the column directly, the high amount of salts in dissolved rock samples required a pre-concentration step. We used a PbSO_4 co-precipitation technique after Martin et al. [4]. All sample volumes were reduced to 100 mL. We added 1 mL of 98 % H_2SO_4 to each sample after which 2 g of K_2SO_4 were added and dissolved. While stirring, 1 mL of 0.24 M $\text{Pb}(\text{NO}_3)_2$ solution was added to the sample drop-wise. The sample was then heated and the precipitation was allowed to settle. The supernatant was decanted and the precipitate was washed using 20 mL of 0.1 M $\text{K}_2\text{SO}_4 + 0.2$ M H_2SO_4 . The precipitate was then easily dissolved in 20 mL of 4 M HCl. Some precipitates required heating and the addition of higher volumes of 4 M HCl; we tested the method with up to 50 mL of load solution for which we still achieved quantitative recoveries. A 1 mg Fe in solution was added to the solution prior to loading on the DGA column. The column was attached to a vacuum box (Eichrom Technologies, Inc.), which was used to achieve flow rates of 1 mL/min. The beaker was rinsed with 2×5 mL of 4 M HCl, which was loaded on the column. The DGA was then rinsed using 10 mL of 3 M HNO_3 and the eluate, which contained iron and any leftover alkaline earth elements was discarded. Actinium was eluted using 20 mL 2 M HCl while Th and other actinides were retained on the DGA column.

The Ac fraction was saved and an alpha-source was prepared using CeF_3 micro-precipitation [9]. 100 μg of Ce carrier in solution was added to the Ac fraction, stirred and 2 mL of concentrated HF were added while stirring. The solution rested for 30 min and then the precipitate was filtered using 0.1 μm polypropylene, 25 mm diameter 0.1 μm polypropylene ResolveTM filters (Eichrom Technologies, Inc.). The filters were dried and mounted on steel planchets.

Alpha-spectroscopy

The samples were counted using silicon surface barrier alpha detectors (Ortec, 450 mm) that were calibrated by a NIST certified ^{241}Am solution prepared in the same geometry as the samples. The source detector distance was 10 mm and in this geometry the detector efficiencies ranged from 19.3 to 20.9 %. After source preparation the samples were stored for 15–20 min for the ingrowth of the ^{225}Ac daughters ^{221}Fr ($T_{1/2} = 4.8$ min) and ^{217}At (0.3 s). The sample was then counted immediately to obtain the highest count rate due to the 10-day half-life of ^{225}Ac . From this measurement, counts from the region of ^{217}At at 7.06 MeV (Fig. 3a) were used to calculate the chemical recovery of ^{225}Ac and therefore also ^{227}Ac . A second measurement was performed after 90 days of sample preparation, which allowed for the decay of ^{225}Ac and the ingrowth of ^{227}Th and ^{223}Ra from ^{227}Ac (Fig. 3b). Counts from the energy region of 5.38–6.10 MeV originating from ^{227}Th and ^{223}Ra (99.4 %) were used to calculate ^{227}Ac . Any leftover ^{225}Ac still present was subtracted from this region.

The ^{227}Ac activity was calculated using the count-rate in the 7.06 MeV peak of ^{217}At for yield determination and in the 5.38–6.10 MeV originating from ^{227}Th and ^{223}Ra minus any decay corrected leftover counts from the ^{225}Ac spike [4]. Actinium-227 at the time of separation $A_{227\text{Ac}}$ was then calculated using the branching ratios for ^{227}Ac of




Fig. 3 Alpha-spectrum of the actinium fraction of a seawater sample **a** counted immediately after source preparation showing peaks of ^{225}Ac , ^{221}Fr and ^{217}At , and **b** the same source counted 90-days after preparation when ^{225}Ac has mostly decayed and daughters ^{227}Th and ^{223}Ra are almost in equilibrium with ^{227}Ac

180 98.2 % by beta-decay to ^{227}Th and 1.38 % by alpha-
 181 particle emission to ^{223}Fr , while 100 % of ^{227}Th and
 182 99.4 % of ^{223}Ra decay via alpha-particle emission:

$$A_{^{227}\text{Ac}} = \frac{A_{^{227}\text{Th}+^{223}\text{Ra}}}{0.9862I_{^{227}\text{Th}} + 0.994I_{^{223}\text{Ra}}},$$

184 where $A_{^{227}\text{Th}+^{223}\text{Ra}}$ is the measured $^{227}\text{Th} + ^{223}\text{Ra}$ activity,
 185 and $I_{^{227}\text{Th}}$ and $I_{^{223}\text{Ra}}$ are the calculated ingrowth fractions of
 186 ^{227}Th and ^{223}Ra at the time of separation [4].

187 Minimum detectable activities (MDA) were calculated
 188 for a confidence limit of $\alpha = 0.05$, 3-day counting times
 189 and one sigma standard deviation of the counts from the
 190 $^{227}\text{Th} + ^{223}\text{Ra}$ region of background spectra according to
 191 the method described by Currie [10].

192 Results and discussion

193 We tested the procedure with $^{229}\text{Th}/^{225}\text{Ac}$ spike in de-
 194 ionized water. As suggested by Horwitz et al. [7], in our
 195 test solutions the chemical recovery increased from 70 %
 196 ($^{229}\text{Th}/^{225}\text{Ac}$ solution in de-ionized water) to 100 % with
 197 the addition of Fe ($^{229}\text{Th}/^{225}\text{Ac}$ in de-ionized water with
 198 50 mg Fe). Increasing Fe concentrations did not have fur-
 199 ther beneficial effects on the Ac sorption, the chemical
 200 recovery dropped to 70 % when we added up to 1 g of iron
 201 (Fig. 4). During these test runs we observed good separa-
 202 tion of ^{229}Th from the ^{225}Ac fraction. One way to check the
 203 performance of our chemical separation was to evaluate the
 204 alpha-spectra for radium, polonium and thorium. Radium-
 205 226 (4.8 MeV), ^{222}Rn (5.49 MeV) and ^{218}Po (6.00 MeV)
 206 counts in the spectrum would be an indication of ^{226}Ra
 207 impurity, ^{210}Po has a peak at 5.30 MeV and finally ^{228}Th
 208 and its daughters can be detected via the ^{212}Po peak at
 209 8.78 MeV. All our spectra including seawater and rock
 210 samples were free of these or only had minor interferences
 211 indicating that the extraction chromatography procedure
 212 reliably removes any interferences and impurities from the
 213 Ac fraction.




Fig. 4 Actinium recoveries from a $^{229}\text{Th}/^{225}\text{Ac}$ spiked de-ionized water solution without and with the addition of variable amounts of iron

The analyzed water samples included de-ionized water, seawater and tap water spiked with ^{227}Ac . The analysis of the de-ionized water sample was considered as blank and resulted in zero net counts in the $^{227}\text{Th} + ^{223}\text{Ra}$ region after background correction. Our analysis of a certified ^{227}Ac standard (AEA Technology supplied by the IAEA [11]) resulted in $(333 \pm 16) \text{ Bq kg}^{-1}$ and was in good agreement with the IAEA value of $(329 \pm 16) \text{ Bq kg}^{-1}$ [11]. Actinium recoveries of water samples were $80 \pm 8 \%$ (number of analyses $n = 14$; where the standard deviation of the average of the 14 analyses is 8 %). The average minimum detectable activity for water samples for ~ 4 day counting time was 0.017 Bq kg^{-1} . The sample activities ranged from below MDA values to 14 Bq kg^{-1} of ^{227}Ac .

The weights of analyzed rock samples were between 0.3 and 5.4 g and we analyzed various basalts and USGS and U-series community rock standards (BCR-2 [12], BHVO-1 [13], Hawaiian basalt (HK) [2], Samoan basalt (SAV) [14]). No certified value for ^{227}Ac exists for these standards but assuming equilibrium through the decay chain (all basalts were over 100 years old) and a closed system we can compare ^{227}Ac to ^{231}Pa [2] (Table 1). There is a good agreement for ^{227}Ac and ^{231}Pa , for all samples the $^{227}\text{Ac}/^{231}\text{Pa}$ ratio is within 5 % of secular equilibrium. For the 24 rock analyses the chemical recoveries were $70 \pm 12 \%$ ($n = 24$). The lower recoveries were the results of (1) an incomplete PbSO_4 precipitation because some rock samples could not be held dissolved unless kept in high acidity solution, (2) a high iron

Table 1 ^{227}Ac activities in selected standard water and basalt samples (BCR-2 [12], BHVO-1 [13], Hawaiian basalt (HK) [2], Samoan basalt (SAV) [14]) analyzed by DGA-column followed by alpha-spectrometry

| Standard | ^{227}Ac by DGA Bq/kg | Certified ^{227}Ac Bq/kg | $^{227}\text{Ac}_{\text{DGA}}/^{227}\text{Ac}_{\text{cert}}$ | Chemical recovery (%) |
|---------------------|--------------------------------|-----------------------------------|--|-----------------------|
| Water | | | | |
| AEA technology-IAEA | 333 ± 16 | 329 ± 16 | 1.01 | 75 |
| | | $^{231}\text{Pa}^*$ | $^{227}\text{Ac}_{\text{DGA}}/^{231}\text{Pa}$ | |
| Rocks (basalts) | | | | |
| BCR-2 | 0.955 ± 0.083 | 0.967 | 0.99 | 83 |
| BHVO-1 | 0.299 ± 0.017 | 0.283 | 1.05 | 71 |
| HK-018 | 0.965 ± 0.009 | 0.948 | 1.02 | 86 |
| HK-019 | 0.962 ± 0.073 | 0.966 | 0.99 | 91 |
| HK-021 | 0.559 ± 0.055 | 0.572 | 0.98 | 80 |
| HK-022 | 0.887 ± 0.080 | 0.862 | 1.03 | 68 |
| SAV B6 | 0.677 ± 0.067 | 0.680 | 1.00 | 66 |

All of the basalt rock samples analyzed are older than 100 years and ^{231}Pa and ^{227}Ac are expected to be in secular radioactive equilibrium

* 2σ uncertainty of $^{231}\text{Pa} < 0.8 \%$

242 content (>1 g) remaining in the samples even after the
 243 PbSO₄ precipitation negatively affects the Ac sorption on
 244 DGA (Figs. 3, 4) the presence of significant amount of lan-
 245 thanides which negatively affects the co-precipitation of
 246 actinium by PbSO₄ [4].

247 The minimum detectable activities for rock samples
 248 averaged 0.05 Bq kg⁻¹ for 3-day counting and MDAs for
 249 individual sample measurements were in the range of
 250 0.017–0.5 Bq kg⁻¹. Sample activities ranged from 0.17 to
 251 8.3 Bq kg⁻¹.

252 Uncertainties were derived from counting statistics of
 253 the ²¹⁷At (usually 3 % error) and ²²⁷Th + ²²³Ra (ranged
 254 from 3 to 10 %) region peaks and error propagation.
 255 Uncertainties of all analysis were <10 %. Overall the DGA
 256 separation method performed well, providing actinium
 257 fractions without interferences in alpha-spectrometry and
 258 resulting in high chemical recoveries. Our results agree
 259 well with certified values for water and ²³¹Pa values for
 260 rock samples.

261 Conclusions

262 The advantages of extraction chromatographic techniques
 263 over ion exchange columns in general are a shorter analysis
 264 time and less acid waste produced. The method developed
 265 here has a high sensitivity due to the low backgrounds on
 266 the alpha-detectors and because of the use of the double-
 267 peak of ²²⁷Th and ²²³Ra, which doubles the counts and
 268 lowers the counting error [15]. Additional advantage of the
 269 DGA method is its possible extension to the analysis of
 270 thorium isotopes. Our typical 2 σ errors were 5 % which
 271 are much higher than those usually obtained for example
 272 by mass spectrometric analysis (ICP-MS, TIMS) of other
 273 isotopes, however due to the low abundance of ²²⁷Ac MS
 274 methods are currently not sensitive enough for its analysis.
 275 For comparison, in units of fg g⁻¹ used for MS techniques,
 276 our method has a limit of detection of 0.02 fg g⁻¹.

277 **Acknowledgments** We would like to acknowledge Phil Horwitz
 278 and William Burnett for their advice on the extraction chromato-
 279 graphic techniques. Ken Sims' lab at the Woods Hole Oceanographic
 280 Institution performed the rock dissolution procedures and Ken
 281 Buesseler (WHOI) provided the counting equipment for the alpha-
 282 spec analysis. Jan Scholten from the IAEA provided the actinium
 283 standard and spiked seawater samples.

References

1. Geibert W, Rutgers van der Loeff MM, Hanfland C, Dauelsberg H-J (2002) Actinium-227 as a deep-sea tracer: sources, distribution and applications. *Earth Planet Sci Lett* 198(1–2):147–165 285
2. Sims KWW, Murrell MT, DePaolo DJ, Baldrige WS, Goldstein SJ, Clague D, Jull M (1999) Porosity of the melting zone and variations in the solid mantle upwelling rate beneath Hawaii: inferences from 238U–230Th–226Ra and 235U–231Pa disequilibria. *Geochim Cosmochim Acta* 63(23):4119–4138 286
3. Nozaki Y (1984) Excess ²²⁷Ac in deep ocean water. *Nature* 310:486–488 287
4. Martin P, Hancock GJ, Paulka S, Akber RA (1995) Determination of ²²⁷Ac by α-particle spectrometry. *Appl Radiat Isot* 46(10):1065–1070 288
5. Geibert W, Vöge I (2008) Progress in the determination of ²²⁷Ac in sea water. *Mar Chem* 109(3–4):238–249 289
6. Moore WS, Arnold R (1996) Measurement of ²²³Ra and ²²⁴Ra in coastal waters using a delayed coincidence counter. *J Geophys Res (Oceans)* 101(1):1321–1329 290
7. Horwitz EP, McAlister DR, Bond AH, Barrans RE (2005) Novel extraction chromatographic resins based on tetraalkyldiglycolamides: characterization and potential applications. *Solvent Extr Ion Exch* 23:219 291
8. Ball LA, Sims KWW, Schwieters J (2008) Measurement of ²³⁴U/²³⁸U and ²³⁰Th/²³²Th in volcanic rocks using the Neptune MC-ICP-MS. *J Anal At Spectrom* 23:173–180 292
9. Dulaiova H, Kim G, Burnett WC, Horwitz EP (2001) Separation and analysis of Am and Pu from large soil and sediment samples. *Radioact Radiochem* 12(3):4–15 293
10. Currie LA (1968) Limits for qualitative detection and quantitative determination. Application to radiochemistry. *Anal Chem* 40(3):586–593 294
11. Scholten JC, Pham MK, Blinova O, Charette MA, Dulaiova H, Eriksson M (2010) Preparation of Mn-fibers standards for the efficiency calibration of the delayed coincidence counting system (RaDeCC). *Mar Chem* 121(1–4):206–214 295
12. Prytulak J, Elliott T, Hoffmann DL, Coath CD (2008) Measurement of USGS BCR-2 as a reference material for silicate rock U-Pa disequilibrium measurements. *Geostand Geoanal Res* 32(1):55–63 296
13. Pichat S, Sims KWW, Francois R, McManus JF, Brown Leger S, Albarede F (2004) Lower export production during glacial periods in the equatorial Pacific derived from (²³¹Pa/²³⁰Th)_{xs,0} measurements in deep-sea sediments. *Paleoceanography* 19 PA4023. doi:10.1029/2003PA000994 297
14. Sims KWW, Hart SR, Reagan MK, Blusztajn J, Staudigel H, Sohn RA, Layne GD, Ball LA, Andrews J (2008) ²³⁸U–²³⁰Th–²²⁶Ra–²¹⁰Pb–²¹⁰Po, ²³²Th–²²⁸Ra, and ²³⁵U–²³¹Pa constraints on the ages and petrogenesis of Vaialulu'u and Malumalu lavas, Samoa. *Geochem Geophys Geosyst* 9:Q04003 298
15. Bojanowski R, Holm E, Whitehead NE (1987) Determination of ²²⁷Ac in environmental samples by ion-exchange and alpha-spectrometry. *J Radioanal Nucl Chem* 115(1):23–37 299