

# JRC Scientific and Technical Reports



## Project HORIZONTAL Validation Report on linear alkylbenzene sulphonates

Validation of a horizontal standard for the determination of linear alkylbenzene sulphonates (LAS) by liquid chromatography with fluorescence detection (LC-FLD) and liquid chromatography with mass selective detection (LC-MS) in a European Intercomparison Exercise

**E. Sobiecka, H. van der Sloot, N. Hansen, B. M. Gawlik**



EUR 22998 EN - 2007

The mission of the Institute for Environment and Sustainability is to provide scientific-technical support to the European Union's Policies for the protection and sustainable development of the European and global environment.

European Commission  
Joint Research Centre  
Institute for Environment and Sustainability

**Contact information**

Address: Via Enrico Fermi 2749, 21027 Ispra (VA), Italy

E-mail: [bernd.gawlik@jrc.it](mailto:bernd.gawlik@jrc.it)

Tel.: +39 0332 789487

Fax: +39 0332 789158

<http://ies.jrc.ec.europa.eu>

<http://www.jrc.ec.europa.eu>

**Legal Notice**

Neither the European Commission nor any person acting on behalf of the Commission is responsible for the use which might be made of this publication.

A great deal of additional information on the European Union is available on the Internet.

It can be accessed through the Europa server

<http://europa.eu/>

JRC 40176

EUR 22998 EN

ISBN 978-92-79-07094-5

ISSN 1018-5593

DOI 10.2788/44441

Luxembourg: Office for Official Publications of the European Communities

© European Communities, 2007

Reproduction is authorised provided the source is acknowledged

*Printed in Luxembourg*

# Project HORIZONTAL Validation Report

## Validation of a horizontal standard for the determination of linear alkylbenzene sulphonates (LAS) by liquid chromatography with fluorescence detection (LC-FLD) and liquid chromatography with mass selective detection (LC-MS) in a European Intercomparison Exercise

*Authors:*

*E. Sobiecka, H. Van der Sloot, N. Hansen, B. M. Gawlik<sup>✉</sup>*

---

**Elzbieta Sobiecka, Bernd Manfred Gawlik**

*European Commission, Joint Research Centre  
Institute for Environment and Sustainability  
Via Enrico Fermi  
21020 Ispra - Italy*

**Hans van der Sloot**

*ECN  
Emission Characterisation and Reduction  
Westerduinweg 3, P.O. Box 1  
1755 ZG Petten  
The Netherlands*

**Nis Hansen**

*Eurofins  
Strandesplanaden 110  
2665 Vallensbaek Strand  
Denmark*

---

✉ to whom correspondence should be sent  
by email to [bernd.gawlik@jrc.it](mailto:bernd.gawlik@jrc.it)



## **Summary**

Project HORIZONTAL is interdisciplinary aiming at a harmonisation and horizontal standardisation of test procedures, in particular for sludge, soils and biowastes. In the context of this standardization project, a series of draft technical specifications were designed upon an extensive desk study, fine-tuned after expert consultations and finally validated in international intercomparisons exercise.

This report summarises the work performed within the validation study of the draft standard for the determination of linear alkylbenzene sulphonates (LAS) in soils, sludge and treated bio-waste using liquid chromatography with fluorescence detection (LC-FLD) and liquid chromatography with mass selective detection (LC-MS). It further explains the underlying statistical concept for the calculation of reproducibility and repeatability from intercomparisons data. In addition all single values, results of the statistical evaluation as well as background information on the validation materials used are described and explained.

## Abbreviations

Throughout this report the following abbreviations are used:

ANOVA	Analysis of variances	LC-FLD	liquid chromatography with fluorescence detection
CAS	Chemical Abstracts System	LC-MS	liquid chromatography with mass selective detection
CEN	Comité Européen de Normalisation	MILC	Measure Interlaboratory Comparison
DG	Directorate General	p	Number of labs
ECN	Energy Research Centre for the Netherlands	r	Repeatability limit
EU	European Union	R	Reproducibility limit
IES	Institute for Environment and Sustainability	s <sub>r</sub>	Repeatability standard deviation
IT	Information Technology	s <sub>R</sub>	Reproducibility standard deviation
ISO	International Organization for Standardisation	TC	Technical Committee
JRC	Joint Research Centre		
LAS	linear alkylbenzene sulphonates		

# Table of Contents

Summary.....	2
Abbreviations .....	3
Table of Contents .....	4
Introduction to the validation project .....	5
1.1 Statistical concept underlying the validation.....	6
1.1.1 Introduction to the statistical model .....	6
1.1.2 Requirements for precision experiment.....	7
Layout of the experiment.....	7
Recruitment of the laboratories .....	7
Preparation and use of the materials.....	7
Reporting of results .....	7
1.1.3 Statistical analysis .....	8
1.2 Validation exercise for Linear Alkylbenzene Sulphonates .....	8
1.2.1 Compounds to be measured.....	8
1.2.2 Samples dispatched for the validation of LAS .....	8
1.2.3 Draft standards to be followed .....	8
1.2.4 Analytical program.....	8
1.2.5 Timing and Submission of data.....	9
1.2.6 Participants .....	10
1.3 Summary results and derived performance characteristics .....	11
1.4 Annexes .....	13





## ***Introduction to the validation project***

Project HORIZONTAL is interdisciplinary aiming at a harmonisation and horizontal standardisation of test procedures, in particular for sludges, soils and biowastes. It was created as in response to the European Commission Mandate M 330 given to CEN, asking for the

development and validation of those standards in support of forthcoming EU Directives, such as:

- The revision of the Sewage Sludge Directive 86/278/EEC.
- The Directive on the biological treatment of biodegradable waste.
- The initiative on a legal framework for soil monitoring in Europe.

This mandate explicitly considers standards for the entire analytical procedure (i.e., sampling, pre-treatment and analytical measurement methods for inorganic, organic, hygiene and biological parameters). These are grouped into classes according to their physical/chemical

properties, which in turn determine the methods needed to quantify the potential impact on human and animal health, plant uptake, soil function and groundwater quality. As the materials generally feature a mixture of different types of contaminants, it is important to provide an integrated answer covering evaluation of all relevant pollutants.

In order to fulfil the requirements of the aforementioned mandate, the European Commissions Joint Research Centre (JRC) and its Directorate-General for Environment (DG ENV) together with the Technical Committees of the European Standardisation Committee (CEN TCs) concerned designed a pre-normative research initiative called Project HORIZONTAL and presented it to the Commission and the Environmental Authorities in the Member States.

After an extensive literature research and careful evaluation of the feasibility of a given horizontal standard, the standards were drafted and finally validated in an European laboratory intercomparison.

The underlying statistical concept, information about the materials used, details about the participants, measurement results obtained as well as the derived performance characteristics obtained for the determination of alkylbenzene sulphonates (LAS) are described hereafter.

## 1.1 Statistical concept underlying the validation

According to the requirements of the work package concerning data handling & interpretation of the project HORIZONTAL-ORG the respective validation intercomparisons have to be evaluated according to the principles laid down in ISO standard 5725-2:1994. In particular repeatability and reproducibility of the draft standard methods have to be determined. The determination of trueness would require the availability of independent reference values for the materials investigated. This, however, is not possible and was not requested in the frame of this work. In the following, the approach chosen is explained.

### 1.1.1 Introduction to the statistical model

The statistical model used in ISO 5725 for estimation of accuracy of a measurement method assumes that every test result is the sum of three components:

$$y = m + B + e$$

*y*: test result

*m*: general mean

*B*: laboratory component of bias under repeatability conditions

*e*: random error occurring in every measurement under repeatability conditions

In the workprogram the quantification of term *e* is explicitly asked for (i.e. repeatability and reproducibility). The repeatability variance is measured directly as the variance of the error term *e*, but the reproducibility depends on the sum of the repeatability variance and the between-laboratory variance:

$$\sigma_r = \sqrt{\text{var}(e)}$$

$$\sigma_R = \sqrt{\sigma_L^2 + \sigma_r^2} \quad \text{with} \quad \sigma_L = \sqrt{\text{var}(B)}$$

However, soil, biowaste and sludge are multi-phase materials, i.e. they contain two or more distinct types of particles which are fundamentally different in their properties and composition. As a consequence, this introduces an important source of variation for the intercomparison exercise which needs to be considered, i.e. the inherent heterogeneity of the materials.

Thus, a contribution of variation between samples *H* is introduced to the general statistical model:

$$y = m + B + e + H$$

Using ANOVA techniques the different variances are calculated and separated for the evaluation.

## 1.1.2 Requirements for precision experiment

### Layout of the experiment

A suite of 10 to 12 different materials (soil, sludge and biowaste) has been made available for the intercomparison exercise. For each parameter investigated, at least 10 laboratories should be nominated to participate. The same laboratories should be used for different parameters as far as possible. Due to the complexity of analysis and the respective workload to the laboratories, it was decided to propose three materials for the validation of the LAS draft standard.

Each laboratory received two bottles of each material and was requested to perform 4 independent analyses per material<sup>1</sup> (2 per bottle) using the respective draft standard methods. The 4 analyses per material should be carried out under repeatability conditions (i.e. same operator<sup>2</sup>, same equipment, within a short period of time). As far as possible, also the different materials should be measured under repeatability conditions; however, changes of e.g. operator or equipment are permitted, but must be reported. Likewise, different materials can be analysed on different days if necessary.

Equipment used in the experiment needed to be checked prior to the experiment according to the requirements of the draft standard, The results of these checks have to be documented. Similarly, date and time of each measurement had to be recorded for verification of repeatability conditions.

An appropriate timeframe for the entire exercise has been set and was to be respected.

### Recruitment of the laboratories

Each sub-workpackage leader of HORIZONTAL was asked to select the laboratories using the information from section 5.2 of ISO 5725-2:1994 and provide the signed questionnaires (see also Annex 1). The workpackage leaders were responsible for providing the laboratories with the draft standard method and explaining the context of this exercise.

### Preparation and use of the materials

Materials used for the exercise were prepared according to the general requirements for reference materials as laid down in ISO Guide 34. Materials were accompanied by instructions for use.

### Reporting of results

Online submissions of results using an internet-based IT platform as well as XLS-Spreadsheets were used. In case of online data submission, the participating laboratories received a unique and confidential login and password in due time, enabling them to

---

<sup>1</sup> Independent analysis means analysis of independent test portions, applying the entire analytical scheme to this test portion, from e.g. extraction to quantification. For instance it does not mean replicate injections of aliquots into a GC-MS instrument.

<sup>2</sup> Operator in this context may also consist of a fixed team of persons, e.g. one person performing extraction, one clean-up, one quantification.

enter their data in a structured form. For authentication purposes a signed printout had to be submitted by mail.

The online data submission included a detailed questionnaire for additional information on the measurements.

### **1.1.3 Statistical analysis**

Statistical analysis of data followed the requirements of ISO 5725-2:1994 and ISO 5725-5:1998. Appropriate tests for the homogeneity of variance, detection of outliers and normal distribution were applied. Statistical evaluation was done using an Excel Macro, developed, tested and successfully applied in other occasion by ECN. Evaluation was executed jointly by JRC and ECN.

## **1.2 Validation exercise for Linear Alkylbenzene Sulphonates**

### **1.2.1 Compounds to be measured**

Linear Alkylbenzene Sulphonates (LAS) were measured for the validation exercise. According to the method studied LAS was determined as the sum of C10-LAS, C11-LAS, C12-LAS, C13-LAS and C14-LAS.

### **1.2.2 Samples dispatched for the validation of LAS**

After a preliminary rough screening, the following materials were used for the validation round of LAS:

- Compost 1                      A pollutant loaded compost material from Vienna
- Sewage Sludge 1              A mixed sewage sludge from Essen
- Soil 3                             A sludge amended soil from Barcelona

A more detailed description of background concentrations can be found in Annex 2 to this report. The samples were dispatched simultaneously to all participants using a private courier service.

### **1.2.3 Draft standards to be followed**

The draft standards to be followed could be downloaded following this link, which is situated on the website of the Project HORIZONTAL:

[http://www.ecn.nl/docs/society/horizontal/LAS\\_Standard\\_for\\_validation.pdf](http://www.ecn.nl/docs/society/horizontal/LAS_Standard_for_validation.pdf)

### **1.2.4 Analytical program**

Of each of the three materials 2 bottles had to be analysed and each bottle had to analyse independently twice. As mentioned above analysis was to be done under repeatability conditions. Results were to be reported referring to DRY MATTER content. The choice, how to apply d.m. correction was free for each participant.

### **1.2.5 Timing and Submission of data**

Dispatch of samples was done on the 18<sup>th</sup> of October 2006. For users of the Online data submission system (MILC), User Registration was possible from 14<sup>th</sup> of November 2006 with opening of the MILC Data Submission on 1<sup>st</sup> of December 2006. The deadline for submission of results has been set for LAS to the 12th of January 2007, but was extended to the end of the same months. After that no further submission was possible.

Alternatively the participants were allowed to submit data electronically as Excel sheet using simply Email.

All data were treated in a confidential way. Any presentation hereafter will refer only to numerical data and it will not be possible to identify the originating laboratory. Lab Codes displayed are NOT related to the order of laboratories hereafter.

In addition to the information provide a Helpdesk was implemented in order to give quick and individual response to the participants during and immediately after the validation study. In case of doubt and suspected transcription errors, further enquires were conducted by JRC.

### 1.2.6 Participants

The following table lists the participating organisations and entities in the validation exercise for the horizontal LAS standard;

- Austria
  - Umweltbundesamt
- Denmark
  - Eurofins A/S
- France
  - INERIS
- Germany
  - Bundesanstalt fuer Materialforschung und -pruefung (BAM)
  - Federal Environmental Agency, Section III 3.4, Laboratory Methods for the Surveillance of Waste and Wastewater (UBA)
- Spain
  - Consejo Superior de Investigaciones Cientificas (CSIC)

### **1.3 Summary results and derived performance characteristics**

The result of the various statistical evaluation including outlier tests, calculation of repeatability and reproducibility standard deviation for the congeners of interest can be found in Annex 3 of this report. In addition, all data submitted by the participants as well as those considered for the calculation of the performance characteristics are listed in Annex 3 to this report.

Based on these calculations the following results were obtained in the validation round upon statistical evaluation according to ISO 5725-2. The average values, the repeatability standard deviation ( $s_r$ ) and the reproducibility standard deviation ( $s_R$ ) were obtained (Table1).

The repeatability is determined as an interval around a measurement result (i.e. "repeatability limit"). This interval corresponds to the maximum difference that can be expected (with a 95% statistical confidence) between one test result and another, both test results being obtained under the following conditions: The tests are performed in accordance with all the requirements of the present standard by the same laboratory using its own facilities and testing laboratory samples obtained from the same primary field sample and prepared under identical procedures. The repeatability limit was calculated using the relationship:  $r_{\text{test}} = f \cdot \sqrt{2} \cdot s_{r,\text{test}}$  with the critical range factor  $f = 2$ .

The reproducibility, like repeatability is also determined as an interval around a measurement result (i.e. "reproducibility limit"). This interval corresponds to the maximum difference that can be expected (with a 95% statistical confidence) between one test result and another test result obtained by another laboratory, both test results being obtained under the following conditions : The tests are performed in accordance with all the requirements of the present standard by two different laboratories using their own facilities and testing laboratory samples obtained from the same primary field sample and prepared under identical procedures. The reproducibility limit was calculated using the relationship:  $R = f \cdot \sqrt{2} \cdot s_R$  with the critical range factor  $f = 2$ .

**Table 1 - Results of the interlaboratory comparison studies of the Determination of LAS by HPLC with fluorescence detection (LC\_FLD) and mass selective detection (LCMSD) in soil, sludge and treated biowaste. All concentrations are expressed in mg/kg dm.**

<i>Matrix</i>	<i>Parameter</i>	<i>Mean</i>	<i>sr</i>	<i>sR</i>	<i>r</i>	<i>R</i>	<i>p</i>	<i>Outliers</i>	<i>Total number of data</i>	<i>No of LOD</i>	<i>Avg</i>	<i>Std</i>	<i>Var %</i>
Sludge 1	LAS Total	1769	3.07%	46.5%	151.9	2302	5	1	20	0	2432	1780	73
Compost 1	LAS Total	2.8	12.4%	55.4%	0.98	4.38	4	0	16	4	2.82	1.53	54
Soil 3	LAS Total	24.5	1.85%	78.6%	1.26	53.80	4	2	13	0	29.0	24.2	83

Abbreviations: sr Repeatability standard deviation; SR Reproducibility standard deviation; r Repeatability limit (comparing two measurements); R Reproducibility limit (comparing two measurements); p Number of labs; \*/\* determination not possible.



## **1.4 Annexes**

Annex 1: Model questionnaire to be filled by the participating laboratories

Annex 2: Report on the validation materials used

Annex 3: Statistical calculations

Annex 4: Data submitted



**Annex 1:**

**Model questionnaire to be filled by the participating laboratories**







## **Annex 2:**

### **Report on the validation materials used**





## **Abstract**

This report gives an overview on the available analytical information on the following raw materials to be used for the production of validation materials of the so-called Project HORIZONTAL:

- Four sludge materials from Düsseldorf, Germany,
- An agricultural soil material from Reading, United Kingdom;
- A compost material from Vienna, Austria;
- A compost material from Korschenbroich, Germany;
- A sludge-amended, agricultural soil from Pavia Province, Italy;
- A sludge-amended soil from Barcelona, Spain
- A sludge-amended soil from Essen, Germany
- A long-term sludge exposed soil from Hohenheim, Germany

## List of Abbreviations

Throughout this report the following abbreviations are used.

AOX	absorbable organic halogens	LoD	limit of detection
C <sub>org</sub>	organic carbon content	LUA	Landesumweltamt
C <sub>total</sub>	total carbon content	N <sub>total</sub>	total nitrogen content
CAT	cation exchangeable	NH <sub>4</sub> -N	Ammonium nitrogen
CDD	chlorinated dibenzodioxin	NO <sub>3</sub> -N	Nitrate nitrogen
CDF	chlorinated dibenzofuran	NP	nonylphenol
DEHP	di(2-ethylhexyl)phthalate	NRW	North Rhine Westphalia
DM	dry matter	O	octa
EPA	Environment Protection Agency	P	poly
EU	European Union	PAH	polycyclic aromatic hydrocarbon
FM	fresh matter	PCB	polychlorinated biphenyl
Hp	hepta	Pe	penta
Hx	hexa	T	tetra
IES	Institute for Environment and Sustainability	TEQ	toxicity equivalent
IRMM	Institute for Reference Materials and Measurements	UBA	Umweltbundesamt
JRC	Joint Research Centre	WHO	World Health Organization
LAS	linear alkylsulfonates	WWTP	waste water treatment plant

## 1 Introduction

This report gives an overview on the available analytical information on the following raw materials to be used for the production of validation materials of the so-called Project HORIZONTAL:

- Four sludge materials from Düsseldorf, Germany,
- An agricultural soil material from Reading, United Kingdom;
- A compost material from Vienna, Austria;
- A compost material from Korschenbroich, Germany;
- A sludge-amended, agricultural soil from Pavia Province, Italy;
- A sludge-amended soil from Barcelona, Spain
- A sludge-amended soil from Essen, Germany
- A long-term sludge exposed soil from Hohenheim, Germany

The following analytical information was gathered partly before and during the sampling of the raw materials, to be used for the production of the HORIZONTAL validation materials. The material were sampled by IES and shipped to IRMM in the course of the year 2005. The information gathered was then completed by various analytical screenings for PAHs and PCBs done by the Institute for Reference Materials and Measurements, Geel, Belgium, for phthalates done by UBA, Berlin, Germany, for PBDE done by IIQAB-CSIC, Barcelona, Spain, for trace elements and some selected major and minor elements by the Institute for Environment and Sustainability, Ispra, Italy.

The work compiled hereafter is based on the numerous additional efforts of the scientists working at various members of the consortium Project HORIZONTAL-Org and contributing organisations.

This work is gratefully acknowledged.

## 2 Overview on property values

### 2.1 *Sludge materials from Düsseldorf, Germany*

The various sewage sludge materials originate from various installations in the North Rhine Westphalia and were produced and sampled by staff from the Landesumweltamt (LUA) NRW under the responsibility from Dr. K. Furtmann.

In total, four sludge materials (Sludge A and D from a major municipal WWTP, Sludge B from a municipal WWTP with industrial input, and Sludge C from a municipal WWTP with high PCB-Content,) were obtained and will be blended to two final materials. Before sampling the following analytical data for a typical sample were received.

Table 1 – Analytical data obtained on an average sludge sample in LUA NRW (with courtesy of K. Furtmann, LUA, Düsseldorf)

<i>Parameter</i>	<i>Concentration</i>
PCB	120 ug/kg
DEHP	110 mg/kg
PAH	5 mg/kg (EPA)
PCDD/F	15 ng TE/kg
PBDE	400 ug/kg
NP	40 mg/kg
LAS	3 g/kg
AOX	300 mg/kg

Subsequent screening led to the information displayed hereafter. It should be stressed that the data were obtained as SCREENING information on the UNTREATED or partially treated raw materials. Therefore, the final target values, which are relevant for the validation intercomparison can be different.

Table 2 – Analytical data obtained on a first screening on the sludge samples from LUA NRW

	<i>Sewage sludge A Dusseldorf</i>	<i>sewage sludge D Dusseldorf</i>
<b>PCB (ng/g)</b>		
28	62	35
52	101	65
101	31	38
118	49	40
153	30	33
105	24	11
138	46	38
156	<1	<1
180	34	23
170	23	19
<b>PAH (ng/g)</b>		
Naphtalene	34	381
Acenaphtylene	15	43
Acenaphthene	81	108
Fluorene	94	1167
Phenantrene		3440
Anthracene	22	344
Flouranthene	316	4817
Pyrene	235	3011
Benz(a)anthracene	473	791
Chrysene	691	1078
Benz(b)fluoranthene	538	1688
Benz(k)fluoranthene	228	635
Benz(a)pyrene	383	1114
Indeno(1,2,3-c,d)pyrene	92	229
Dibenzo(a,h)anthracene	71	70
Benzo(g,h,i)perylene	80	185

Table 3 – Data on phthalate contents (with courtesy of S. Heise, UBA, Germany)

	<i>DiBP</i>	<i>DBP</i>	<i>DCHP</i>	<i>DEHP</i>	<i>Water</i>
	µg/g dm	µg/g dm	µg/g dm	µg/g dm	Wgt. %
Sludge D (1)		0.135		41.474	3.85
Sludge B (2)	0.538	0.034		30.634	5.47
Sludge A (3)	0.184	0.037		31.399	1.46
Sludge C (4)		0.354	1.528	6.678	2.29

Table 4 – Data on PDBE contents (with courtesy of D. Barceló and co-workers, IIQAB-CSIC, Barcelona, Spain)

	<i>Sludge 2</i> <i>(B)</i>
Tetra-BDE-47	55.4
Penta-BDE-100	9.59
Penta-BDE-99	69.4
Hexa-BDE-154	5.91
Hexa-BDE-153	7.72
Hepta-BDE-183	5.09
Octa-BDE-196	nq
Octa-BDE-197	nq
Octa-BDE-203	9.70
Deca-BDE-209	2216
TOTAL	2379

Table 5 – Screening data on some selected trace elements by ICP-AES after micro-wave assisted digestion using aqua regia (with courtesy of F. Sena, IES, Ispra, Spain). Note that these data are based on single measurements!

	<i>Cd</i>	<i>Co</i>	<i>Cr</i>	<i>Cu</i>	<i>Mn</i>	<i>Ni</i>	<i>Pb</i>	<i>Sb</i>	<i>Tl</i>	<i>V</i>	<i>Zn</i>
	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g
Sludge 1 (D)	2.65	29.0	53.3	359	1231	33.8	78.4	4.38	< 0.05	23.2	786
Sludge 2 (B)	1.19	31.1	62.6	202	278	29.9	72.2	2.51	< 0.05	11.8	625
Sludge 3 (A)	1.68	36.0	62.1	332	847	41.6	119	4.51	< 0.05	11.6	1237
Sludge 4 (C)	5.63	19.8	116	273	726	51.1	473	6.18	< 0.05	44.4	2015

Table 6 – Screening data on some selected matrix constituents and elements by WDXRF (with courtesy of S. Vaccaro).

<i>Sample</i>	<i>SiO2 (%)</i>	<i>Al2O3 (%)</i>	<i>CaO (%)</i>	<i>K2O (%)</i>	<i>Fe2O3 (%)</i>	<i>MgO (%)</i>	<i>TiO2 (PPM)</i>	<i>S (PPM)</i>	<i>P2O5 (PPM)</i>
Sludge 1 (D)	21.54	5.8	8.44	0.99	10.3	1.01	4367	<15	50448
Sludge 2 (B)	10.67	3.66	6.92	0.46	14.91	0.77	5217	<15	57633
Sludge 3 (A)	7.31	6.63	6.84	0.35	12.87	0.68	3733	<15	60369
Sludge 4 (C)	43.79	9.65	5.27	1.63	5.22	1.07	5628	<15	23945

<i>Sample</i>	<i>Na2O (%)</i>	<i>Cl (PPM)</i>	<i>Pb (PPM)</i>	<i>Zn (PPM)</i>	<i>Cu (PPM)</i>	<i>Ni (PPM)</i>	<i>Mn (PPM)</i>	<i>Cr (PPM)</i>
Sludge 1 (D)	0.3	2403	101	1002	350	15	1944	132
Sludge 2 (B)	0.31	315	97	879	172	12	514	180
Sludge 3 (A)	0.31	1281	153	1567	265	16	1440	168
Sludge 4 (C)	0.55	231	628	2625	371	81	1101	244

## 2.2 Agricultural soil material from Reading, United Kingdom

The material was proposed by the University of Reading (S. Nortcliff) and was sampled from a site called “Frogmore Farm” which was featured in the “Metals” Report for HORIZONTAL. This site is close to Reading with soils developed on flintyloamy periglacial materials over Chalk, has a long and well documented history of sludge application. The focus of the work of Nortcliff *et al.* undertook at this site and the monitoring and control at the site (by Thames Water and the subsequent subsidiary bodies dealing with sludge application to soil) was on metals (and metal loads), with no analysis or indeed any form of investigation in to organics in the broadest sense.

The analytical information produced in the context of the screening of the raw material is displayed below.

Table 7 – Data on phthalate contents (with courtesy of S. Heise, UBA, Germany)

	<i>DiBP</i>	<i>DBP</i>	<i>DCHP</i>	<i>DEHP</i>	<i>Water</i>
	µg/g dm	µg/g dm	µg/g dm	µg/g dm	Wgt. %
Soil 3 (Reading)		0.032		0.119	6.69

Table 8 – Screening data on some selected trace elements by ICP-AES after micro-wave assisted digestion using aqua regia (with courtesy of F. Sena). Note that these data are based on single measurements!

	<i>Cd</i>	<i>Co</i>	<i>Cr</i>	<i>Cu</i>	<i>Mn</i>	<i>Ni</i>	<i>Pb</i>	<i>Sb</i>	<i>Tl</i>	<i>V</i>	<i>Zn</i>
	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g
Soil 3 (Reading)	0.15	7.06	27.9	13.8	152	9.01	26.7	3.00	< 0.05	25.8	93.1

Table 9 – Analytical data obtained on a first screening on the sludge-amended soil from Reading (courtesy of IRMM)

<i>Parameter</i>	<i>Concentration</i>
<b>PCB</b>	<b>ng/g</b>
28	<1
52	<1
101	<1
118	<1
153	<1
105	<1
138	<1
156	<1
180	<1
170	<1
<b>PAH</b>	<b>ng/g</b>
Naphtalene	<10
Acenaphtylene	21
Acenaphthene	<10
Fluorene	<10
Phenantrene	<10
Anthracene	<10
Flouranthene	818
Pyrene	776
Benz(a)anthracene	565

<i>Parameter</i>	<i>Concentration</i>
Chrysene	608
Benz(b)fluoranthene	824
Benz(k)fluoranthene	329
Benz(a)pyrene	799
Indeno(1,2,3-c,d)pyrene	779
Dibenzo(a,h)anthracene	118
Benzo(g,h,i)perylene	394

*Table 10 – Data on PDBE contents (with courtesy of D. Barceló and co-workers, IIQAB-CSIC, Barcelona, Spain)*

	<i>Soil 3 (Reading)</i>
Tetra-BDE-47	nq
Penta-BDE-100	nq
Penta-BDE-99	1.03
Hexa-BDE-154	0.03
Hexa-BDE-153	nq
Hepta-BDE-183	nq
Octa-BDE-196	nq
Octa-BDE-197	nd
Octa-BDE-203	nd
Deca-BDE-209	272
TOTAL	273

*Table 11 – Screening data on some selected trace elements by ICP-AES after micro-wave assisted digestion using aqua regia (with courtesy of F. Sena). Note that these data are based on single measurements!*

	<i>Cd</i>	<i>Co</i>	<i>Cr</i>	<i>Cu</i>	<i>Mn</i>	<i>Ni</i>	<i>Pb</i>	<i>Sb</i>	<i>Tl</i>	<i>V</i>	<i>Zn</i>
Soil 3 (Reading)	0.15	7.06	27.9	13.8	152	9.01	26.7	3.00	< 0.05	25.8	93.1

*Table 12 – Screening data on some selected matrix constituents and elements by WDXRF (with courtesy of S. Vaccaro).*

<i>Sample</i>	<i>SiO2 (%)</i>	<i>Al2O3 (%)</i>	<i>CaO (%)</i>	<i>K2O (%)</i>	<i>Fe2O3 (%)</i>	<i>MgO (%)</i>	<i>TiO2 (PPM)</i>	<i>S (PPM)</i>	<i>P2O5 (PPM)</i>
Soil 3 (Reading)	79.36	4.77	1.12	0.96	1.94	0.17	4107	443	2102

<i>Sample</i>	<i>Na2O (%)</i>	<i>Cl (PPM)</i>	<i>Pb (PPM)</i>	<i>Zn (PPM)</i>	<i>Cu (PPM)</i>	<i>Ni (PPM)</i>	<i>Mn (PPM)</i>	<i>Cr (PPM)</i>
Soil 3 (Reading)	0.42	13	45	69	69	69	216	92

*Table 13 – Screening data on mercury by solid-sampling cold-vapour AAS using amalgamation enrichment (with courtesy of G. Locoro).*

<i>Sample</i>	<i>Hg µg/g</i>
Soil 3 (Reading)	0.12

### 2.3 Compost from Vienna, Austria

The fresh compost material was obtained from the Austrian Federal Environment Agency (UBA, Vienna), which had used a sub-batch of the raw material for national intercomparison. The remainder of the material was stored at 4°C until shipment to IRMM for further processing. The following analytical information was provided by UBA Austria and completed with various screenings.

Table 14 – Analytical data on compost material received from UBA Austria  
Inorganic and sum parameters

Parameter	Unit	Sample fraction used	Observed mean
B CAT	mg/l F.M.	Fresh sample, <10mm	6.1
K CAT	mg/l F.M.	Fresh sample, <10mm	2624
Mg CAT	mg/l F.M.	Fresh sample, <10mm	242
P CAT	mg/l F.M.	Fresh sample, <10mm	49
B CAT	% D.M.	Fresh sample, <10mm	0.0017
K CAT	% D.M.	Fresh sample, <10mm	0.72
Mg CAT	% D.M.	Fresh sample, <10mm	0.07
P CAT	% D.M.	Fresh sample, <10mm	0.01
NO3-N	mg/kg F.M.	Fresh sample, <10mm	3.5
NH4-N	mg/kg F.M.	Fresh sample, <10mm	230
Ctotal	% D.M.	<45° dry, milled	29
Corg	% D.M.	<45° dry, milled	27
Ntotal	% D.M.	<45° dry, milled	1.7
P	mg/kg D.M.	<45° dry, milled	2596
K	mg/kg D.M.	<45° dry, milled	11019
K	% D.M.	<45° dry, milled	1.10
B	mg/kg D.M.	<45° dry, milled	60
Cd	mg/kg D.M.	<45° dry, milled	0.46
Cr	mg/kg D.M.	<45° dry, milled	25
Cu	mg/kg D.M.	<45° dry, milled	46
Hg	mg/kg D.M.	<45° dry, milled	0.20
Ni	mg/kg D.M.	<45° dry, milled	18
Pb	mg/kg D.M.	<45° dry, milled	45
Zn	mg/kg D.M.	<45° dry, milled	198
Ca	mg/kg D.M.	<45° dry, milled	68776
Ca	% D.M.	<45° dry, milled	6.9
Mo	mg/kg D.M.	<45° dry, milled	0.8
S	mg/kg D.M.	<45° dry, milled	2137
Fe	mg/kg D.M.	<45° dry, milled	9959
Mn	mg/kg D.M.	<45° dry, milled	418
Na	mg/kg D.M.	<45° dry, milled	742
Co	mg/kg D.M.	<45° dry, milled	4.1
AOX	mg/kg D.M.	<30° dry, milled	62

Table 15 – Analytical data on compost material received from UBA Austria  
Polycyclic aromatic hydrocarbons

PAH	Unit	Result
Naphthaline	µg/kg DM	9.3
Acenaphthylene	µg/kg DM	8.6
Acenaphthene	µg/kg DM	5
Fluorene	µg/kg DM	8.0
Phenanthrene	µg/kg DM	89
Anthracene	µg/kg DM	27
Fluoranthene	µg/kg DM	487
Pyrene	µg/kg DM	380



<i>PAH</i>	<i>Unit</i>	<i>Result</i>
Benzo(a)anthracene	µg/kg DM	278
Chrysene	µg/kg DM	317
Benzo(b)fluoranthene	µg/kg DM	365
Benzo(k)fluoranthene	µg/kg DM	193
Benz(a)pyrene	µg/kg DM	320
Indeno(1,2,3-c,d)pyrene	µg/kg DM	233
Dibenz(a,h)anthracene	µg/kg DM	67
Benzo(g,h,i)perylene	µg/kg DM	225
Sum EPA	µg/kg DM	3013
Sum EPA	mg/kg DM	3.0

Table 16 – Analytical data on compost material received from UBA Austria  
Sum PCDDs and PCBs

<i>Parameter</i>			
Dioxine	TEQ (ITEF)	ng/kg DM	7.3
PCB	TEQ (WHO)	ng/kg DM	3.5
	Σ Ballschmiter	mg/kg DM	0.05

Table 17 – Analytical data on compost material obtained by screening in IRMM

<i>Parameter</i>	<i>Result in ng/g</i>
<b>PCB</b>	
28	2
52	2
101	4
118	3
153	10
105	1
138	8
156	1
180	5
170	<1
<b>PAH</b>	
Naphtalene	<10
Acenaphthylene	<10
Acenaphthene	<10
Fluorene	<10
Phenantrene	<10
Anthracene	26
Fluoranthene	611
Pyrene	510
Benzo(a)anthracene	888
Chrysene	957
Benzo(b)fluoranthene	1531
Benzo(k)fluoranthene	547
Benzo(a)pyrene	1101
Indeno(1,2,3-c,d)pyrene	416
Dibenzo(a,h)anthracene	81
Benzo(g,h,i)perylene	295

Table 18 – Data on PDBE contents (with courtesy of D. Barceló and co-workers, IIQAB-CSIC, Barcelona, Spain)

	Compost 1 (Vienna)
Tetra-BDE-47	4.02
Penta-BDE-100	0.19
Penta-BDE-99	2.59
Hexa-BDE-154	nq
Hexa-BDE-153	0.23
Hepta-BDE-183	0.04
Octa-BDE-196	nq
Octa-BDE-197	nq
Octa-BDE-203	1.44
Deca-BDE-209	17.4
TOTAL	25.9

Table 19 – Data on phthalate contents (with courtesy of S. Heise, UBA, Germany)

	DiBP	DBP	DCHP	DEHP	Water
	µg/g dm	µg/g dm	µg/g dm	µg/g dm	Wgt. %
Compost 1 (Vienna)		0.058		1.426	5.57

Table 20 – Screening data on some selected trace elements by ICP-AES after micro-wave assisted digestion using aqua regia (with courtesy of F. Sena). Note that these data are based on single measurements!

	Cd	Co	Cr	Cu	Mn	Ni	Pb	Sb	Tl	V	Zn
	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g
Compost 1 (Vienna)	0.39	7.36	31.9	41.0	365	12.7	49.5	0.04	0.79	0.13	208

Table 21 – Screening data on some selected matrix constituents and elements by WDXRF (with courtesy of S. Vaccaro).

Sample	SiO2 (%)	Al2O3 (%)	CaO (%)	K2O (%)	Fe2O3 (%)	MgO (%)	TiO2 (PPM)	S (PPM)	P2O5 (PPM)
Compost 1 (Vienna)	20.63	4.31	6.17	4.26	1.99	2.49	1602	<15	10521

Sample	Na2O (%)	Cl (PPM)	Pb (PPM)	Zn (PPM)	Cu (PPM)	Ni (PPM)	Mn (PPM)	Cr (PPM)
Compost 1 (Vienna)	0.35	3496	81	375	79	55	653	60

Table 22 – Screening data on mercury by solid-sampling cold-vapour AAS using amalgamation enrichment (with courtesy of G. Locoro).

Sample	Hg µg/g
Compost 1 (Vienna)	0.17

## 2.4 Agricultural soil, sludge amended soil from Pavia, Italy

This sludge-amended soil material was obtained during a monitoring campaign, which aimed at a generic description of the over-all soil quality in Pavia Province, Italy. The material, which was collected from the upper horizon, originates from a small farm called “*Cascina Novello*”. During the characterisation of the site, the following analytical information was obtained on a pooled sample of a sub-area of the farm of 20 X 20 m<sup>2</sup>.

Table 23 – Analytical data on Pavia soil

<i>Parameter</i>	<i>Result</i>
Al	7.13 Wgt%
As	22.4 mg/kg
Cd	0.79 mg/kg
Cr	59 mg/kg
Cu	30.8 mg/kg
Hg	0.08 mg/kg
Ni	34.4 mg/kg
Pb	24.6 mg/kg
Zn	95 mg/kg
C	0.91 Wgt %
2,3,7,8-TCDD	0.047 pg/g
1,2,3,7,8-PeCDD	0.15 pg/g
1,2,3,4,7,8-HxCDD	0.19 pg/g
1,2,3,6,7,8-HxCDD	1.5 pg/g
1,2,3,7,8,9-HxCDD	0.74 pg/g
1,2,3,4,6,7,8-HpCDD	26 pg/g
OCDD	382 pg/g
2,3,7,8-TCDF	0.68 pg/g
1,2,3,7,8-PeCDF	0.53 pg/g
2,3,4,7,8-PeCDF	0.71 pg/g
1,2,3,4,7,8-HxDF	1.00 pg/g
1,2,3,6,7,8-HxDF	0.66 pg/g
2,3,4,6,7,8-HxDF	1.6 pg/g
1,2,3,7,8,9-HxDF	0.27 pg/g
1,2,3,4,6,7,8-HpDF	12 pg/g
1,2,3,4,7,8,9-HpDF	0.68 pg/g
OCDF	33 pg/g
I-TEQ	2.0 pg/g
WHO-TEQ	1.7 pg/g

In addition, the screening performed at IRMM did not reveal significant quantities of PCBs and PAHs, which were all below the LoDs (1 ng/g for PCBs and 10 ng/g for PAHs, respectively).

Table 24 – Data on phthalate contents (with courtesy of S. Heise, UBA, Germany)

	<i>DiBP</i>	<i>DBP</i>	<i>DCHP</i>	<i>DEHP</i>	<i>Water</i>
	µg/g TM	µg/g TM	µg/g TM	µg/g TM	Wgt. %
Soil 5 (Pavia)		0.005		0.011	1.54

Table 25 – Data on PDBE contents (with courtesy of D. Barceló and co-workers, IIQAB-CSIC, Barcelona, Spain)

	Soil 5 (Pavia)
Tetra-BDE-47	nq
Penta-BDE-100	nq
Penta-BDE-99	0.39
Hexa-BDE-154	nq
Hexa-BDE-153	nq
Hepta-BDE-183	0.08
Octa-BDE-196	nq
Octa-BDE-197	nd
Octa-BDE-203	nd
Deca-BDE-209	670
TOTAL	671

Table 26 – Screening data on some selected trace elements by ICP-AES after microwave assisted digestion using aqua regia (with courtesy of F. Sena). Note that these data are based on single measurements!

	Cd	Co	Cr	Cu	Mn	Ni	Pb	Sb	Tl	V	Zn
	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g
Soil 5 (Pavia)	0.33	18.4	57.3	22.5	426	30.5	20.6	2.00	< 0.05	38.1	87.8

Table 27 – Screening data on some selected matrix constituents and elements by WDXRF (with courtesy of S. Vaccaro).

Sample	SiO <sub>2</sub> (%)	Al <sub>2</sub> O <sub>3</sub> (%)	CaO (%)	K <sub>2</sub> O (%)	Fe <sub>2</sub> O <sub>3</sub> (%)	MgO (%)	TiO <sub>2</sub> (PPM)	S (PPM)	P <sub>2</sub> O <sub>5</sub> (PPM)
Soil 5 (Pavia)	69.39	12.9	1.45	2.24	4.25	1.16	6118	255	1789

Sample	Na <sub>2</sub> O (%)	Cl (PPM)	Pb (PPM)	Zn (PPM)	Cu (PPM)	Ni (PPM)	Mn (PPM)	Cr (PPM)
Soil 5 (Pavia)	1.84	62	38	108	55	66	597	110

Table 28 – Screening data on mercury by solid-sampling cold-vapour AAS using amalgamation enrichment (with courtesy of G. Locoro).

Sample	Hg µg/g
Soil 5 (Pavia)	0.06

## 2.5 Sludge-amended-soil from Barcelona, Spain

The sludge-amended soil material from Barcelona sampled upon indication from the Barcelo'- Group in Barcelona.

Table 29 – Data on phthalate contents (with courtesy of S. Heise, UBA, Germany)

	<i>DiBP</i>	<i>DBP</i>	<i>DCHP</i>	<i>DEHP</i>	<i>Water</i>
	µg/g dm	µg/g dm	µg/g dm	µg/g dm	Wgt. %
Soil 2 (Lleida T.)		0.015		0.183	11.38

Table 30 – Data on PDBE contents (with courtesy of D. Barceló and co-workers, IIQAB-CSIC, Barcelona, Spain)

	<i>Soil 2</i> ( <i>Lleida T.</i> )
Tetra-BDE-47	nq
Penta-BDE-100	nq
Penta-BDE-99	1.59
Hexa-BDE-154	0.45
Hexa-BDE-153	nq
Hepta-BDE-183	0.48
Octa-BDE-196	1.60
Octa-BDE-197	nq
Octa-BDE-203	nq
Deca-BDE-209	1000
TOTAL	1004

Table 31 – Screening data on some selected trace elements by ICP-AES after micro-wave assisted digestion using aqua regia (with courtesy of F. Sena). Note that these data are based on single measurements!

	<i>Cd</i>	<i>Co</i>	<i>Cr</i>	<i>Cu</i>	<i>Mn</i>	<i>Ni</i>	<i>Pb</i>	<i>Sb</i>	<i>Tl</i>	<i>V</i>	<i>Zn</i>
	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g
Soil 2 (Lleida T.)	0.59	14.1	32.7	53.6	405	18.6	18.4	2.24	< 0.05	31.8	111

Table 32 – Screening data on some selected matrix constituents and elements by WDXRF (with courtesy of S. Vaccaro).

<i>Sample</i>	<i>SiO2 (%)</i>	<i>Al2O3 (%)</i>	<i>CaO (%)</i>	<i>K2O (%)</i>	<i>Fe2O3 (%)</i>	<i>MgO (%)</i>	<i>TiO2 (PPM)</i>	<i>S (PPM)</i>	<i>P2O5 (PPM)</i>
Soil 2 (Lleida T.)	44.43	10.67	14.29	2.53	3.44	2.04	4116	780	3396

<i>Sample</i>	<i>Na2O (%)</i>	<i>Cl (PPM)</i>	<i>Pb (PPM)</i>	<i>Zn (PPM)</i>	<i>Cu (PPM)</i>	<i>Ni (PPM)</i>	<i>Mn (PPM)</i>	<i>Cr (PPM)</i>
Soil 2 (Lleida T.)	0.64	65	26	125	59	17	547	65

Table 33 – Screening data on mercury by solid-sampling cold-vapour AAS using amalgamation enrichment (with courtesy of G. Locoro).

<i>Sample</i>	<i>Hg µg/g</i>
Soil 2 (Lleida T.)	0.10

## 2.6 Sludge amended soil from Essen, Germany

The German sludge-amended soil from Essen, which was provided as the three sludge materials by LUA NRW, did not feature significant concentrations of the PCB congeners 28, 52, 101, 118, 153, 105, 138, 156, 180, 170, but had detectable amounts of some PAHs.

Table 34 – Analytical screening data on the German sludge-amended soil.

Parameter	Concentration (ng/g)
Naphtalene	<10
Acenaphtylene	<10
Acenaphthene	<10
Fluorene	<10
Phenantrene	<10
Anthracene	<10
Fluoranthene	28
Pyrene	20
Benz(a)anthracene	24
Chrysene	47
Benz(b)fluoranthene	76
Benz(k)fluoranthene	20
Benz(a)pyrene	35
Indeno(1,2,3-c,d)pyrene	35
Dibenzo(a,h)anthracene	10
Benzo(g,h,i)perylene	26

Table 35 – Data on phthalate contents (with courtesy of S. Heise, UBA, Germany)

	DiBP	DBP	DCHP	DEHP	Water
	µg/g dm	µg/g dm	µg/g dm	µg/g dm	Wgt. %
Soil 4 (Essen)		0.011		0.302	0.55

Table 36 – Data on PDBE contents (with courtesy of D. Barceló and co-workers, IIQAB-CSIC, Barcelona, Spain)

	Soil 4 (Essen)
Tetra-BDE-47	nq
Penta-BDE-100	nq
Penta-BDE-99	nq
Hexa-BDE-154	nq
Hexa-BDE-153	nq
Hepta-BDE-183	nq
Octa-BDE-196	nq
Octa-BDE-197	nq
Octa-BDE-203	1.28
Deca-BDE-209	19.1
TOTAL	20.3

Table 37 – Screening data on some selected trace elements by ICP-AES after micro-wave assisted digestion using aqua regia (with courtesy of F. Sena). Note that these data are based on single measurements!

	<i>Cd</i>	<i>Co</i>	<i>Cr</i>	<i>Cu</i>	<i>Mn</i>	<i>Ni</i>	<i>Pb</i>	<i>Sb</i>	<i>Tl</i>	<i>V</i>	<i>Zn</i>
	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g
Soil 4 (Essen)	0.52	5.45	26.1	8.05	320	4.03	27.3	2.73	< 0.05	29.5	78.1

Table 38 – Screening data on some selected matrix constituents and elements by WDXRF (with courtesy of S. Vaccaro).

<i>Sample</i>	<i>SiO2 (%)</i>	<i>Al2O3 (%)</i>	<i>CaO (%)</i>	<i>K2O (%)</i>	<i>Fe2O3 (%)</i>	<i>MgO (%)</i>	<i>TiO2 (PPM)</i>	<i>S (PPM)</i>	<i>P2O5 (PPM)</i>
Soil 4 (Essen)	79.47	4.42	0.85	0.6	0.86	0.07	2163	189	2019

<i>Sample</i>	<i>Na2O (%)</i>	<i>Cl (PPM)</i>	<i>Pb (PPM)</i>	<i>Zn (PPM)</i>	<i>Cu (PPM)</i>	<i>Ni (PPM)</i>	<i>Mn (PPM)</i>	<i>Cr (PPM)</i>
Soil 4 (Essen)	0.45	19	42	87	683	60	462	61

Table 39 – Screening data on mercury by solid-sampling cold-vapour AAS using amalgamation enrichment (with courtesy of G. Locoro).

<i>Sample</i>	<i>Hg µg/g</i>
Soil 4 (Essen)	0.04

## 2.7 Long-term sludge exposed soil from Hohenheim-Stuttgart, Germany

Similarly, an additional sludge exposed soil was sampled at the University of Hohenheim, Stuttgart, where a test soil was long-term exposed to elevated concentrations of sewage sludge.

Table 40 – Data on phthalate contents (with courtesy of S. Heise, UBA, Germany)

	<i>DiBP</i>	<i>DBP</i>	<i>DCHP</i>	<i>DEHP</i>	<i>Water</i>
	µg/g TM	µg/g TM	µg/g TM	µg/g TM	Wgt. %
Soil 1 (Stuttgart)		0.045		0.263	17.65

Table 41 – Data on PDBE contents (with courtesy of D. Barceló and co-workers, IIQAB-CSIC, Barcelona, Spain)

	<i>Soil 1</i> ( <i>Stuttgart</i> )
Tetra-BDE-47	nq
Penta-BDE-100	nq
Penta-BDE-99	2.30
Hexa-BDE-154	0.06
Hexa-BDE-153	0.04
Hepta-BDE-183	0.04
Octa-BDE-196	nq
Octa-BDE-197	nd
Octa-BDE-203	nd
Deca-BDE-209	498
TOTAL	500

Table 42 – Screening data on some selected trace elements by ICP-AES after micro-wave assisted digestion using aqua regia (with courtesy of F. Sena). Note that these data are based on single measurements!

	<i>Cd</i>	<i>Co</i>	<i>Cr</i>	<i>Cu</i>	<i>Mn</i>	<i>Ni</i>	<i>Pb</i>	<i>Sb</i>	<i>Tl</i>	<i>V</i>	<i>Zn</i>
	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g	µg/g
Soil 1 (Stuttgart)	0.69	12.7	36.1	26.2	504	18.3	25.2	2.62	<0.05	26.6	142

Table 43 – Screening data on some selected matrix constituents and elements by WDXRF (with courtesy of S. Vaccaro).

<i>Sample</i>	<i>SiO2 (%)</i>	<i>Al2O3 (%)</i>	<i>CaO (%)</i>	<i>K2O (%)</i>	<i>Fe2O3 (%)</i>	<i>MgO (%)</i>	<i>TiO2 (PPM)</i>	<i>S (PPM)</i>	<i>P2O5 (PPM)</i>
Soil 1 (Stuttgart)	71.94	10.06	1.33	1.86	3.66	0.88	7874	275	3571

<i>Sample</i>	<i>Na2O (%)</i>	<i>Cl (PPM)</i>	<i>Pb (PPM)</i>	<i>Zn (PPM)</i>	<i>Cu (PPM)</i>	<i>Ni (PPM)</i>	<i>Mn (PPM)</i>	<i>Cr (PPM)</i>
Soil 1 (Stuttgart)	1.23	50	47	212	85	69	991	129

Table 44 – Screening data on mercury by solid-sampling cold-vapour AAS using amalgamation enrichment (with courtesy of G. Locoro).

<i>Sample</i>	<i>Hg µg/g</i>
Soil 1 (Stuttgart)	1.77




**Annex 3:**  
**Statistical calculations**




Sample: Soil 3  
 Element: LAS total

Mandel's h statistics  
 (Soil 3 - LAS total)

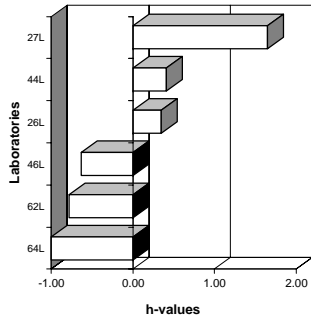

Mandel's k statistics  
 (Soil 3 - LAS total)

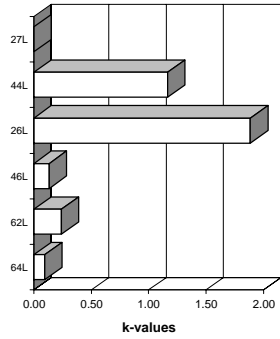

Unit: mg/kg

Mandel's k statistics (Soil 3 - LAS total)  
 Mandel's h statistics (Soil 3 - LAS total)

Soil 3 - LAS total -- Mean PARM = 24.46 [mg/kg]


General calc.parm.  
 T1= 1.84515E+02  
 T2= 6.02589E+03  
 T3= 13  
 T4= 49  
 T5= 1.8329E+00  
 n= variabel  
 p= 4  
 N-table= 4

LAB	PARM-gem	Stdev	N	h-mark	Mandel's statistics		k-mark $\sqrt{X} > AvST+2std$	AvX < AvST-2std	End Result:					
					h	k			PARM	Stdev	Rej.labs	N	N-1	dev_mean
64L	4.9100	0.255	4	-1.00	-1.00	0.10		Fail	4.9100	0.2546		4	3	-19.55
62L	10.1600	0.646	4	-0.78	-0.78	0.24		Fail	10.1600	0.6458		4	3	-14.30
46L	13.8250	0.359	4	-0.63	-0.63	0.13		Fail	13.8250	0.3594		4	3	-10.63
26L	37.5441	5.033	4	0.35	0.35	1.89	!!	Fail	-	-	,26L	-	-	13.09
44L	38.9250	3.112	4	0.41	0.41	1.17		Fail	-	-	,44L	-	-	14.47
27L	68.9350	-	1	1.65	1.65	-		Fail	68.9350	-		1	-	44.48
Tot.gem	29.050	1.881 mg/kg		1%-level:	1.87	(1.73)			4	24.4575	(44L,26L)	4	3	
Tot.std=	24.215	2.117		5%-level:	1.66	(1.53)			2					


RESULTS: Mean = 24.45750 mg/kg

Repeatability variance S2r = 0.20366  
 Repeatability std. Sr = 0.45128 --> 1.85% r = 1.2636  
 Between lab variance S2L = 369.02385  
 Reproducibility var. S2R = 369.22751  
 Reproducibility std. SR = 19.21529 --> 78.57% R = 53.8028

Remarks: 2 Labs rejected! (44L,26L)

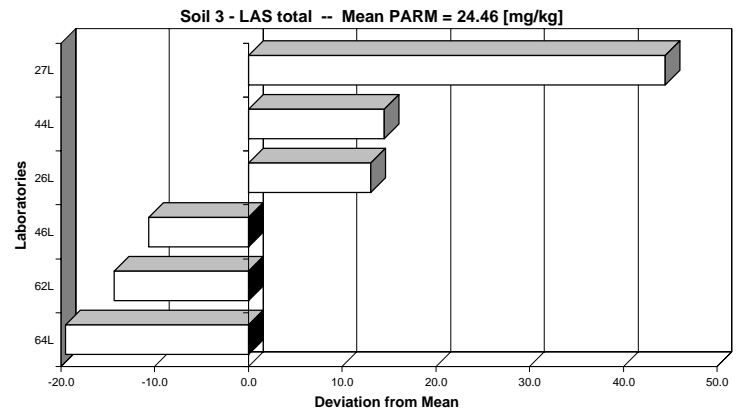

Sample: **Sludge 1**  
 Element: **LAS Total**

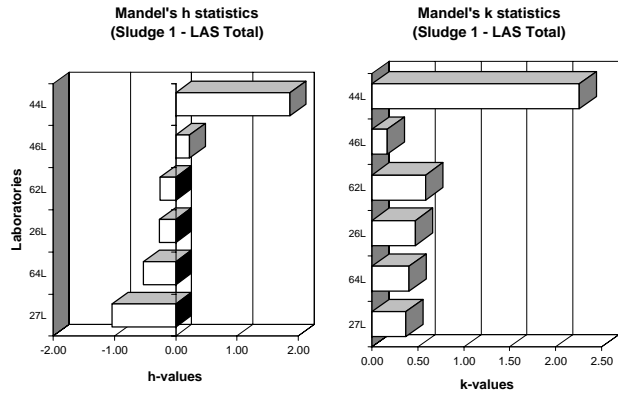

Unit: mg/kg

Mandel's k statistics (Sludge 1 - LAS Total)  
 Mandel's h statistics (Sludge 1 - LAS Total)  
 Sludge 1 - LAS Total -- Mean PARM = 1770 [mg/kg]

```

General calc.parm.
T1= 3.53916E+04
T2= 7.34080E+07
T3= 20
T4= 80
T5= 4.4175E+04
n= variabel
p= 5
N-table= 4
  
```


Mandel's statistics										End Result:				
LAB	PARM-gem	Stdev	N	h-mark	h	k	k-mark $\sqrt{X} > AvST+2std$	AvX < AvST-2std	PARM	Stdev	Rej.labs	N	N-1	dev_mean
27L	583.6424	46.964	4		-1.04	0.37		Fail	583.6424	46.9642		4	3	-1185.94
64L	1486.2550	51.561	4		-0.53	0.40		Fail	1486.2550	51.5613		4	3	-283.32
26L	1964.9959	61.036	4		-0.26	0.48		Fail	1964.9959	61.0357		4	3	195.42
62L	1983.0000	75.291	4		-0.25	0.59		Fail	1983.0000	75.2905		4	3	213.42
46L	2830.0000	21.602	4		0.22	0.17		Fail	2830.0000	21.6025		4	3	1060.42
44L	5742.7500	289.026	4	I	1.86	2.26	II	Fail	-	-	,44L	-	-	3973.17
Tot.gem	2431.774	90.913 mg/kg			1%level:	1.87			5	1769.5787		5	4	
Tot.std=	1780.451	98.661			5%level:	1.66			1					

**RESULTS:** Mean = 1769.57866 mg/kg


Repeatability variance S2r = 2944.97994  
 Repeatability std. Sr = 54.26767 --> 3.07% r = 151.9495

Between lab variance S2L = 673000.53054  
 Reproducibility var. S2R = 675945.51048  
 Reproducibility std. SR = 822.15905 --> 46.46% R = 2302.0454

Remarks: 1 Lab rejected! (44L)

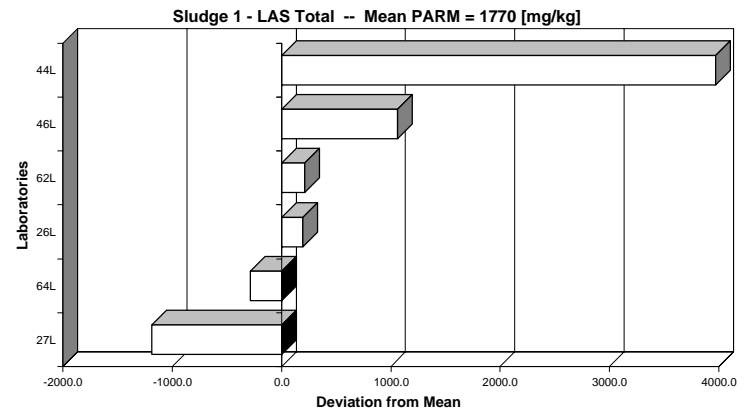

Sample: **Compost 1**  
 Element: **LAS total**

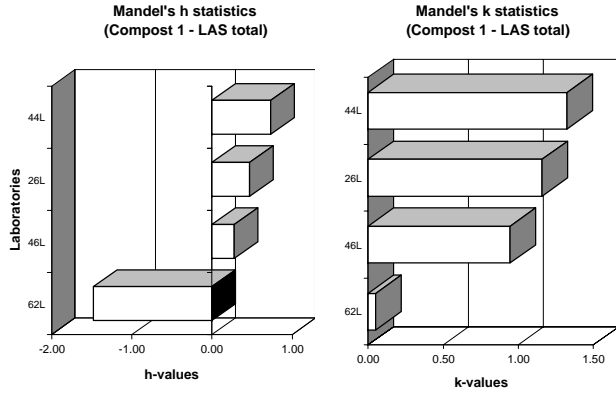

Unit: mg/kg

Mandel's k statistics (Compost 1 - LAS total)  
 Mandel's h statistics (Compost 1 - LAS total)  
 Compost 1 - LAS total -- Mean PARM = 2.82 [mg/kg]


General calc.parm.  
 T1= 4.51856E+01  
 T2= 1.55855E+02  
 T3= 16  
 T4= 64  
 T5= 1.4708E+00  
 n= variabel  
 p= 4  
 N-table= 4

LAB	PARM-gem	Stdev	N	Mandel's statistics				End Result:						
				h-mark	h	k	k-mark	AvX > AvST+2std	AvX < AvST-2std	PARM	Stdev	Rej.labs	N	
62L	0.5625	0.017	4	I	-1.47	0.05			0.5625	0.0171		4	3	-2.26
46L	3.2500	0.332	4		0.28	0.95	Fail	Fail	3.2500	0.3317		4	3	0.43
26L	3.5414	0.406	4		0.47	1.16	Fail		3.5414	0.4058		4	3	0.72
44L	3.9425	0.464	4		0.73	1.33	Fail		3.9425	0.4640		4	3	1.12
Tot.gem	2.824	0.305 mg/kg			1.49	(1.67)			4	2.8241	0	4	3	
Tot.std=	1.534	0.199			5%-level:	(1.5)								

**RESULTS:** Mean = 2.82410 mg/kg

Repeatability variance S2r = 0.12257  
 Repeatability std. Sr = 0.35010 --> 12.40% r = 0.9803  
 Between lab variance S2L = 2.32321  
 Reproducibility var. S2R = 2.44578  
 Reproducibility std. SR = 1.56390 --> 55.38% R = 4.3789

Remarks: none

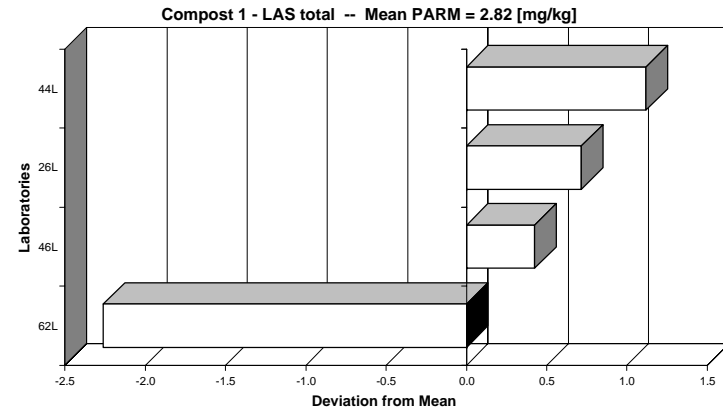



## **Annex 4:**

### **Raw data submitted**





Sample:	<i>Compost 1</i>		[mg/kg]
Element:	<i>LAS total</i>		
	<i>LAB</i>	<i>PARM</i>	
62L	0.58		
62L	0.54		
62L	0.57		
62L	0.56		
44L	3.59		
44L	3.71		
44L	4.62		
44L	3.85		
46L	2.80		
46L	3.50		
46L	3.20		
46L	3.50		
26L	3.25		
26L	3.81		
26L	3.14		
26L	3.96		

Sample:	<i>Sludge 1</i>		[mg/kg]
Element:	<i>LAS Total</i>		
	<i>LAB</i>	<i>PARM</i>	
64L	1510		
64L	1546		
64L	1457		
64L	1432		
62L	2037		
62L	2003		
62L	1872		
62L	2020		
44L	6033		
44L	5930		
44L	5597		
44L	5411		
46L	2810		
46L	2830		
46L	2820		
46L	2860		
27L	649		
27L	567		
27L	580		
27L	539		
26L	1952		
26L	2052		
26L	1909		
26L	1947		

Sample:	<i>Soil 3</i>		[mg/kg]
Element:	<i>LAS total</i>		
	<i>LAB</i>	<i>PARM</i>	
64L	5.2		
64L	4.7		
64L	4.7		
64L	5.0		
62L	10.9		
62L	9.6		
62L	10.6		
62L	9.6		
44L	40.9		
44L	37.3		
44L	42.1		
44L	35.4		
46L	13.3		
46L	14.0		
46L	14.1		
46L	13.9		
26L	32.4		
26L	43.2		
26L	34.3		
26L	40.3		
27L	68.9		



European Commission

**EUR 22998 EN – Joint Research Centre – Institute for Environment and Sustainability**

Title: Project HORIZONTAL Validation Report on linear alkylbenzene sulphonates

Author(s): E. Sobiecka, H. van der Sloot, N. Hansen, B. M. Gawlik

Luxembourg: Office for Official Publications of the European Communities

2007 – 47 pp. – 21.00 x 29.7 cm

EUR – Scientific and Technical Research series – ISSN 1018-5593

ISBN 978-92-79-07094-5

**Abstract**

Project HORIZONTAL is interdisciplinary aiming at a harmonisation and horizontal standardisation of test procedures, in particular for sludge, soils and biowastes. In the context of this standardization project, a series of draft technical specifications were designed upon an extensive desk study, fine-tuned after expert consultations and finally validated in international intercomparisons exercise.

This report summarises the work performed within the validation study of the draft standard for the determination of linear alkylbenzene sulphonates (LAS) in soils, sludge and treated bio-waste using liquid chromatography with fluorescence detection (LC-FLD) and liquid chromatography with mass selective detection (LC-MS). It further explains the underlying statistical concept for the calculation of reproducibility and repeatability from intercomparisons data. In addition all single values, results of the statistical evaluation as well as background information on the validation materials used are described and explained.



The mission of the JRC is to provide customer-driven scientific and technical support for the conception, development, implementation and monitoring of EU policies. As a service of the European Commission, the JRC functions as a reference centre of science and technology for the Union. Close to the policy-making process, it serves the common interest of the Member States, while being independent of special interests, whether private or national.

LB-NA-22998-EN-C



ISBN 978-92-79-07094-5



9 789279 070945