



EC Harmonization Programme for Air Quality Measurements:

The evaluation of the Intercomparison Exercise for SO₂, CO, O₃, NO and NO₂ 6.- 9. October 2008

Matej Kapus Dukarić, Annette Borowiak and Fritz Lagler



EUR 23806 EN - 2009

The mission of the JRC-IES is to provide scientific-technical support to the European Union's policies for the protection and sustainable development of the European and global environment.

European Commission
Joint Research Centre
Institute for Environment and Sustainability

Contact information

Address: T.P. 441, Via E. Fermi, 21027 Ispra (VA), Italy
E-mail: annette.borowiak@jrc.ec.europa.eu
Tel.: +39 0332 789956
Fax: +39 0332 785236

<http://ies.jrc.ec.europa.eu/>
<http://www.jrc.ec.europa.eu/>

Legal Notice

Neither the European Commission nor any person acting on behalf of the Commission is responsible for the use which might be made of this publication.

***Europe Direct is a service to help you find answers
to your questions about the European Union***

Freephone number (*):

00 800 6 7 8 9 10 11

(*) Certain mobile telephone operators do not allow access to 00 800 numbers or these calls may be billed.

A great deal of additional information on the European Union is available on the Internet.
It can be accessed through the Europa server <http://europa.eu/>

JRC50630

EUR 23806 EN
ISBN 978-92-79-12170-8
ISSN 1018-5593

Luxembourg: Office for Official Publications of the European Communities

© European Communities, 2009

Reproduction is authorised provided the source is acknowledged

Printed in Italy

In collaboration with:

Adjanski-Spasic, L.; Assel, J.; Filipovic, A.; Gaizutis, T.; Giusto, M.; Grozdanovski, L.;
Hadjikyriacou, T.; Molis, J.; Montagnoli, M.; Panayotov, N.; Papadopoulos, C.; Parolin, M.;
Parvanova, M.; Pólay, G.; Seewoester, J.; Solagna, S.; Van der Laan, J.; Viktor, D.; Wallast, P.



WHO COLLABORATING CENTRE FOR AIR QUALITY
MANAGEMENT AND AIR POLLUTION CONTROL

at the

FEDERAL ENVIRONMENTAL AGENCY



Executive Summary

From the 6th to the 9th of October 2008 in Ispra (IT), 7 AQUILA (Network of European Air Quality Reference Laboratories) and 2 laboratories of the World Health Organisations (WHO) Euro-Region met at an intercomparison exercise to evaluate their proficiency in the analysis of inorganic gaseous pollutants covered by European Air Quality Directives (SO₂, CO, NO, NO₂ and O₃).

The proficiency evaluation, where each participant's bias was compared to two criteria, provides information on the current situation and capabilities to the European Commission and can be used by participants in their quality control system.

In terms of criteria imposed by the European Commission, 36% of the results reported by AQUILA laboratories were good both in terms of measured values and reported uncertainties. Another 56% of the results had good measured values, but the reported uncertainties were either too small (21%) or too high (35%).

The comparability of results among AQUILA participants is satisfactory for O₃, SO₂, CO and NO measurement method, but the pollutant NO₂ needs further improvements and harmonization programmes.

Contents

1.	Introduction	1
2.	Communication and time schedule	3
3.	Participants	3
4.	Preparation of test mixtures.....	4
5.	Evaluation of laboratory's measurement proficiency	5
	z' - score	5
	E _n - number.....	9
6.	Performance characteristics of individual laboratories	15
	The efficiency of NO ₂ -to-NO converters of NO _x analyzers	15
7.	Discussion	17
8.	Conclusions	19
9.	References	20
Annex A.	Assigned values	22
Annex B.	Results of the IE	24
	Reported values for SO ₂	24
	Reported values for CO	27
	Reported values for O ₃	30
	Reported values for NO.....	33
	Reported values for NO ₂	39
Annex C.	Precision of standardized measurement methods.....	45
Annex D.	Scrutiny of results for consistency and outliers.....	51

List of tables

Table 1: The list of participating organizations.	3
Table 2: The sequence program of generated test gases	4
Table 3: The standard deviation for proficiency assessment	5
Table 4: The efficiency of NO ₂ -to-NO converters.	16
Table 5: The general assessment of proficiency results.	18
Table 6: The validation of assigned values (X)	23
Table 7: Reported values for SO ₂ concentration level 0.	24
Table 8: Reported values for SO ₂ concentration level 1.	25
Table 9: Reported values for SO ₂ concentration level 2.	25
Table 10: Reported values for SO ₂ concentration level 3.	26
Table 11: Reported values for SO ₂ concentration level 4.	26
Table 12: Reported values for SO ₂ concentration level 5.	27
Table 13: Reported values for CO concentration level 0.	27
Table 14: Reported values for CO concentration level 1.	28
Table 15: Reported values for CO concentration level 2.	28
Table 16: Reported values for CO concentration level 3.	29
Table 17: Reported values for CO concentration level 4.	29
Table 18: Reported values for CO concentration level 5.	30
Table 19: Reported values for O ₃ concentration level 0.	30
Table 20: Reported values for O ₃ concentration level 1.	31
Table 21: Reported values for O ₃ concentration level 2.	31
Table 22: Reported values for O ₃ concentration level 3.	32
Table 23: Reported values for O ₃ concentration level 4.	32
Table 24: Reported values for O ₃ concentration level 5.	33
Table 25: Reported values for NO concentration level 0.	33
Table 26: Reported values for NO concentration level 1.	34
Table 27: Reported values for NO concentration level 2.	34
Table 28: Reported values for NO concentration level 3.	35
Table 29: Reported values for NO concentration level 4.	35
Table 30: Reported values for NO concentration level 5.	36
Table 31: Reported values for NO concentration level 6.	36
Table 32: Reported values for NO concentration level 7.	37
Table 33: Reported values for NO concentration level 8.	37
Table 34: Reported values for NO concentration level 9.	38
Table 35: Reported values for NO concentration level 10.	38
Table 36: Reported values for NO ₂ concentration level 0.	39
Table 37: Reported values for NO ₂ concentration level 1.	39
Table 38: Reported values for NO ₂ concentration level 2.	40
Table 39: Reported values for NO ₂ concentration level 3.	40
Table 40: Reported values for NO ₂ concentration level 4.	41
Table 41: Reported values for NO ₂ concentration level 5.	41
Table 42: Reported values for NO ₂ concentration level 6.	42
Table 43: Reported values for NO ₂ concentration level 7.	42
Table 44: Reported values for NO ₂ concentration level 8.	43
Table 45: Reported values for NO ₂ concentration level 9.	43
Table 46: Reported values for NO ₂ concentration level 10.	44
Table 47: The degrees of freedom (v) and critical student factors ($t_{\alpha,v}$) of r and R evaluations.	45
Table 48: The R and r of CO standard measurement method.	46
Table 49: The R and r of O ₃ standard measurement method.	47
Table 50: The R and r of SO ₂ standard measurement method.	48
Table 51: The R and r of NO standard measurement method.	49
Table 52: The R and r of NO ₂ standard measurement method.	50
Table 53: "Genuine" statistical outliers.	51

List of figures

Figure 1: The z'-score evaluations of SO ₂ measurements	6
Figure 2: The z'-score evaluations of CO measurements	7
Figure 3: The z'-score evaluations of O ₃ measurements	7
Figure 4: The z'-score evaluations of NO measurements	8
Figure 5: The z'-score evaluations of NO ₂ measurements	8
Figure 6: Bias of participant's SO ₂ measurement results	10
Figure 7: Bias of participant's CO measurement results	11
Figure 8: Bias of participant's O ₃ measurement results	12
Figure 9: Bias of participant's NO measurement results	13
Figure 10: Bias of participant's NO ₂ measurement results	14
Figure 11: Bias of participant's NO ₂ measurements for run numbers 1, 3, 5, 7 and 9	15
Figure 12: The decision diagram for general assessment of proficiency results.	17
Figure 13: Reported values for SO ₂ concentration level 0.	24
Figure 14: Reported values for SO ₂ concentration level 1.	25
Figure 15: Reported values for SO ₂ concentration level 2.	25
Figure 16: Reported values for SO ₂ concentration level 3.	26
Figure 17: Reported values for SO ₂ concentration level 4.	26
Figure 18: Reported values for SO ₂ concentration level 5.	27
Figure 19: Reported values for CO concentration level 0.	27
Figure 20: Reported values for CO concentration level 1.	28
Figure 21: Reported values for CO concentration level 2.	28
Figure 22: Reported values for CO concentration level 3.	29
Figure 23: Reported values for CO concentration level 4.	29
Figure 24: Reported values for CO concentration level 5.	30
Figure 25: Reported values for O ₃ concentration level 0.	30
Figure 26: Reported values for O ₃ concentration level 1.	31
Figure 27: Reported values for O ₃ concentration level 2.	31
Figure 28: Reported values for O ₃ concentration level 3.	32
Figure 29: Reported values for O ₃ concentration level 4.	32
Figure 30: Reported values for O ₃ concentration level 5.	33
Figure 31: Reported values for NO concentration level 0.	33
Figure 32: Reported values for NO concentration level 1.	34
Figure 33: Reported values for NO concentration level 2.	34
Figure 34: Reported values for NO concentration level 3.	35
Figure 35: Reported values for NO concentration level 4.	35
Figure 36: Reported values for NO concentration level 5.	36
Figure 37: Reported values for NO concentration level 6.	36
Figure 38: Reported values for NO concentration level 7.	37
Figure 39: Reported values for NO concentration level 8.	37
Figure 40: Reported values for NO concentration level 9.	38
Figure 41: Reported values for NO concentration level 10.	38
Figure 42: Reported values for NO ₂ concentration level 0.	39
Figure 43: Reported values for NO ₂ concentration level 1.	39
Figure 44: Reported values for NO ₂ concentration level 2.	40
Figure 45: Reported values for NO ₂ concentration level 3.	40
Figure 46: Reported values for NO ₂ concentration level 4.	41
Figure 47: Reported values for NO ₂ concentration level 5.	41
Figure 48: Reported values for NO ₂ concentration level 6.	42
Figure 49: Reported values for NO ₂ concentration level 7.	42
Figure 50: Reported values for NO ₂ concentration level 8.	43
Figure 51: Reported values for NO ₂ concentration level 9.	43
Figure 52: Reported values for NO ₂ concentration level 10.	44
Figure 53: The R and r of CO standard measurement method as a function of concentration.	46
Figure 54: The R and r of O ₃ standard measurement method as a function of concentration.	47
Figure 55: The R and r of SO ₂ standard measurement method as a function of concentration.	48
Figure 56: The R and r of NO standard measurement method as a function of concentration.	49
Figure 57: The R and r of NO ₂ standard measurement method as a function of concentration.	50
Figure 58: Grubb's one outlying observation test statistics for SO ₂ runs.	52
Figure 59: Grubb's one outlying observation test statistics for CO runs.	52
Figure 60: Grubb's one outlying observation test statistics for O ₃ runs.	53
Figure 61: Grubb's one outlying observation test statistics for NO runs.	53
Figure 62: Grubb's one outlying observation test statistics for NO ₂ runs.	54
Figure 63: Grubb's two outlying observations test statistics for SO ₂ runs	55
Figure 64: Grubb's two outlying observations test statistics for CO runs	55
Figure 65: Grubb's two outlying observations test statistics for O ₃ runs	56
Figure 66: Grubb's two outlying observations test statistics for NO runs	56

Figure 67: Grubb's two outlying observations test statistics for NO₂ runs

Abbreviations:

AQUILA	Network of National Reference Laboratories for Air Quality
CO	Carbon monoxide
DQO	Data Quality Objective
ERLAP	European Reference Laboratory of Air Pollution
EC	European Commission
GPT	Gas phase titration
IE	Intercomparison Exercise
IES	Institute for Environment and Sustainability
ISO	International Organization for Standardization
JRC	Joint Research Centre
NO	Nitrogen monoxide
NO ₂	Nitrogen dioxide
NO _x	the oxides of nitrogen, the sum of NO and NO ₂
NRL	National Reference Laboratory
O ₃	Ozone
SO ₂	Sulphur dioxide
WHO CC	World Health Organization Collaborating Centre for Air Quality Management and Air Pollution Control, Berlin

Mathematical Symbols:

<i>symbol</i>	<i>explanation</i>
E_n	E_n – number statistic (ISO 13528; [18])
X	Assigned/reference value (ISO 13528; [18])
u_x	The standard uncertainty of the assigned/reference value (ISO 13528; [18])
U_x	The expanded uncertainty of the assigned/reference value (ISO 13528; [18])
x_i	the average of three values reported by the participant i (for particular parameter and concentration level) (ISO 5725; [19])
$x_{i,j}$	j -th reported value of participant i (for particular parameter and concentration level) (ISO 5725; [19])
U_{x_i}	The expanded uncertainty of the participant's value
z'	z' -score statistic (ISO 13528; [18])
σ_p	the standard deviation for proficiency assessment (ISO 13528; [18])
x^*	robust average (Annex C ISO 13528; [18])
s^*	robust standard deviation (Annex C ISO 13528; [18])
α	converter efficiency (EN 14211; [9])
s_r	repeatability standard deviation (ISO 5725; [19])
s_R	reproducibility standard deviation (ISO 5725; [19])
r	repeatability limit (ISO 5725; [19])
R	reproducibility limit (ISO 5725; [19])

1. Introduction

As the old “Framework Directive” [1] and its “Daughter Directives” [2], [3], [4] and [5], the new Directive 2008/50/EC [6] on ambient air quality and cleaner air for Europe sets a framework for a harmonized air quality assessment in Europe. One important objective of the Directive is that the ambient air quality shall be assessed on the basis of common methods and criteria. It deals with the air pollutants sulphur dioxide (SO₂), nitrogen dioxide (NO₂) and monoxide (NO), particulate matter, lead, benzene, carbon monoxide (CO) and ozone (O₃). Among others it specifies the reference methods for measurements and Data Quality Objectives (DQO) for the accuracy of measurements.

The European Commission (EC) has supported the development and publication of reference measurement methods [7], [8], [9] and [10] as European standards. Appropriate calibration methods [11], [12] and [13] have been standardised by the International Organization for Standardization (ISO).

As foreseen in the Framework Directive, the European Reference Laboratory of Air Pollution (ERLAP) of the Institute for Environment and Sustainability (IES) at the Joint Research Centre (JRC) organizes intercomparison exercises (IE) to assess and improve the status of comparability of measurements of National Reference Laboratories (NRL) of each Member State of the European Union.

The World Health Organization Collaborating Centre for Air Quality Management and Air Pollution Control, Berlin (WHO CC) is carrying out similar activities since 1994 [14] [15], but with a view to obtaining harmonized air quality data for health related studies. Their program integrates within the WHO EURO region, which includes public health institutes and other national institutes - especially from the Central Eastern Europe, Caucasus and countries from Central Asia.

Starting in 2004, it has been decided to bring together the efforts of both the JRC-ERLAP and WHO CC and to coordinate activities as far as possible, with a view to optimize resources and have better international harmonization. The following report deals with the IE that took place from the 6th to the 9th of October 2008 in Ispra (IT) in joint cooperation of EC/ JRC/IES/ERLAP and WHO CC.

ERLAP has been organizing IEs since 1990 aiming at evaluating the comparability of measurements carried out by NRLs and promoting information exchange among the expert laboratories. Nowadays the main objective, in accordance with the Network of National Reference Laboratories for Air Quality (AQUILA) [16], comprises a more systematic approach that offers alert mechanism for the purposes of the EC and is also useful to NRLs in quality assurance of their implemented quality systems. The methodology of organization of IEs was developed by ERLAP and is described in a position paper on the organization of intercomparison exercises for gaseous air pollutants [17]. This position paper is currently a proposal to the AQUILA and the final agreement of position paper is foreseen to take place during 2008. Then it will be applied throughout all future IEs.

The evaluation scheme applied to this IE is described in detail in the position paper [17] and it reflects the inputs given by AQUILA. Firstly, it was acknowledged that the evaluation scheme should have common criteria, to alert the EC on the possible performance failure, and not to base these alerts on claimed uncertainty of participants. For that purpose the common criterion was proposed to AQUILA and the z'-score method [18] was implemented in to the evaluation scheme. The common criterion is derived from the uncertainty requirements for calibration gases stated in the European standards [6], [8], [9] and [10], which are consistent with the DQOs of European Directives. In view of AQUILA, NRLs with overall unsatisfactory results of the z'-score evaluation (one unsatisfactory or two questionable results per parameter) are required to repeat their participation to the next IE in order to demonstrate remediation measures [17]. Secondly, it was acknowledged that the evaluation scheme

should be useful to participants accredited according to ISO 17025 and thus should include measurement uncertainty of participants. For that purpose, participants measurement results (measurement values and uncertainties) are compared to assigned values applying the E_n – number method [18].

Beside the proficiency of participating laboratories the repeatability and reproducibility of standardized measurement methods [19], [20] and [21] are evaluated as well. These group evaluations will be used in a separate communication as the indicators of trends of quality of measurements over different IEs undertaken by ERLAP.

2. Communication and time schedule

The IE was announced in November 2007 to the members of the AQUILA network and the WHO CC representative. A registration letter was sent to interested parties and the registration was closed in June 2008 with the list of 9 participating laboratories. The participants were required to bring their own measurement instruments, data acquisition equipment and travelling standards (to be used for calibrations or checks during the IE).

The participants were invited to arrive on Monday, 6th October 2008, for the installation of their equipment. The calibration of NO_x and O₃ analysers was carried out on Tuesday morning and the generation of NO_x and O₃ gas mixtures started at 11:00. The calibration of SO₂ and CO analysers was carried out on Wednesday 18:00 and the generation of CO and SO₂ gas mixtures started at 20:00. The test gases generation finished on Thursday at 7:00 a.m..

3. Participants

All participants were organizations dealing with the routine ambient air monitoring or health related studies. The national representatives came from EU member states, Bulgaria, Cyprus, Hungary, Italy, Lithuania and Luxembourg, and from The former Yugoslav Republic of Macedonia. Regional representatives came from Belgrade (Serbia) and Amsterdam (The Netherlands).

Table 1: The list of participating organizations.

Country	Name of Organization	IE code
Bulgaria	Executive Environmental Agency	A
Cyprus	Ministry of Labour and Social Insurance	B
Hungary	Environmental Protection & Water Management Research Institute	C
Italy	Institute for Atmospheric Pollution CNR	D
Lithuania	Environmental Protection Agency	E
Luxembourg	Administration of Environment	F
European Commission	European Reference Laboratory of Air Pollution	G
The former Yugoslav Republic of Macedonia	Ministry of Environment and Physical Planning	H
The Netherlands	GGD Amsterdam	I
Serbia	Institute for Public Health, Belgrade	J

4. Preparation of test mixtures

The ERLAP IE facility has been described in several reports [22] and [23]. During this IE, gas mixtures were prepared for SO₂, CO, O₃, NO and NO₂ at concentration levels around European Air Quality limit values, critical levels and assessment thresholds.

The test mixtures were prepared by the dilution of gases from cylinders containing high concentration of NO, SO₂ or CO using thermal mass flow controllers [13]. O₃ was added using an ozone generator and NO₂ was produced applying the gas phase titration method [24] in the conditions of excess NO.

The participants were required to report three half-hour-mean measurements for each concentration level in order to evaluate the repeatabilities of standardized measurement methods. Zero concentration levels were generated for one hour and one half-hour-mean measurements were reported. The sequence program of generated test gases is given in Table 2.

Table 2: The sequence program of generated test gases

day	start time	duration	operation or run number	zero air	NO	NO ₂	O ₃	CO	SO ₂
		(h)		(nmol/mol)	(nmol/mol)	(nmol/mol)	(nmol/mol)	(μmol/mol)	(nmol/mol)
06-Oct	12:00	6	installation						
07-Oct	08:00	3	calibration						
07-Oct	11:00	1	NO & NO ₂ & O ₃ run 0	0					
07-Oct	12:00	2	NO & NO ₂ run 1		500	0			
07-Oct	14:00	2	NO & NO ₂ run 2		380	120			
07-Oct	16:00	2	O ₃ run 1				120		
07-Oct	18:00	2	NO & NO ₂ run 3		250	0			
07-Oct	20:00	2	NO & NO ₂ run 4		146	104			
07-Oct	22:00	2	O ₃ run 2				104		
08-Oct	00:00	2	NO & NO ₂ run 5		150	0			
08-Oct	02:00	2	NO & NO ₂ run 6		90	60			
08-Oct	04:00	2	O ₃ run 3				60		
08-Oct	06:00	2	NO & NO ₂ run 7		50	0			
08-Oct	08:00	2	NO & NO ₂ run 8		29.1	20.9			
08-Oct	10:00	2	O ₃ run 4				20.9		
08-Oct	12:00	2	NO & NO ₂ run 9		15.7	0			
08-Oct	14:00	2	NO & NO ₂ run 10		2.1	13.6			
08-Oct	16:00	2	O ₃ run 5				13.6		
08-Oct	< 18:00	2	calibration						
08-Oct	20:00	1	CO & SO ₂ run 0	0					
08-Oct	21:00	2:30	CO & SO ₂ run 1					8.6	132
08-Oct	23:30	2	CO & SO ₂ run 2					6	47
09-Oct	01:30	2	CO & SO ₂ run 3					4.3	18.8
09-Oct	03:30	2	CO & SO ₂ run 4					2	7.5
09-Oct	05:30	2	CO & SO ₂ run 5					1	3
09-Oct	07:30	1		0					
09-Oct	08:30								

5. Evaluation of laboratory's measurement proficiency

To evaluate the participants measurement proficiency the methodology described in ISO 13528 [18] was applied. It has been agreed among the members of the AQUILA to take the measurement results of ERLAP as the assigned/reference values for the whole IE [17]. The traceability of ERLAP's measurement results and the method applied to validate them are presented in Annex A. In the following proficiency evaluations, the uncertainty of test gas homogeneity (Annex A) was added to the uncertainties of ERLAP's measurement results.

All data reported by participating laboratories are presented in Annex B.

As it is described in the position paper [17], the proficiency of the participants was assessed by calculating two performance indicators. The first performance indicator (z'-score) tests if the difference between the participants measured value and the assigned/reference value remains within the limits of a common criterion, while the second performance indicator (E_n-number) tests if the difference between the participants measured values and assigned/reference value remains within the limits of a criterion, that is calculated individually for each participant, from the uncertainty of the participants measurement result and the uncertainty of the assigned/reference value.

z' - score

The z' - score statistic is calculated according to ISO 13528 [18] as:

$$z' = \frac{x_i - X}{\sqrt{\sigma_p^2 + u_x^2}} = \frac{x_i - X}{\sqrt{(a \cdot X + b)^2 + u_x^2}} \quad (1)$$

where 'x_i' is a participant's run average value, 'X' is the assigned/reference value, 'σ_p' is the 'standard deviation for proficiency assessment' and 'u_x' is the standard uncertainty of assigned value. For 'a' and 'b' see Table 3.

In the European standards [6], [8], [9] and [10] the uncertainties for calibration gases used in ongoing quality control are prescribed. In fact, it is stated that the maximum permitted expanded uncertainty for calibration gases is 5% and that 'zero gas' shall not give instrument reading higher than the detection limit. As one of the tasks of NRLs is to verify the accuracy of above mentioned 'zero gas' and calibration gas mixtures, the 'standard deviation for proficiency assessment' (σ_p) [18] is calculated in fitness-for-purpose manner from requirements given in European standards.

Over the whole measurement range σ_p is calculated by linear interpolation between 2.5% at the calibration point (75% of calibration range) and the limit of detection at zero concentration level. The limits of detection of studied measurement methods were evaluated from the data of previous IEs [25]. The linear function parameters of σ_p are given in Table 3.

Table 3: The standard deviation for proficiency assessment as a linear function of concentration (c) with linear function parameters: slope (a) and intercept (b).

	σ _p =a·c+b	
	a	b
		nmol/mol
SO ₂	0.024	0.4
CO	0.023	100
O ₃	0.022	0.5
NO	0.025	0.35
NO ₂	0.023	0.46

During the November 2008 AQUILA meeting, σ_p was enlarged, to 1 ppb at zero concentration of SO₂, O₃, NO, NO₂, and approved. It has been agreed that this change is noted in all relevant and not yet published IE reports and applied to all future IEs.

The z'-score evaluation allows the following criteria to be used for the assessment of results:

- $|z'| \leq 2$ are designated satisfactory.
- $2 < |z'| \leq 3$ are designated questionable.
- $|z'| > 3$ are designated unsatisfactory. Scores falling in this range are very unusual and are taken to indicate that the cause of the event should be investigated and remedied.

The results of z'-score evaluation are presented in bar plots (Figure 1 to Figure 5) in which the z'-scores of each participant are grouped together, and assessment criteria are presented as $z'=\pm 2$ and $z'=\pm 3$ lines.

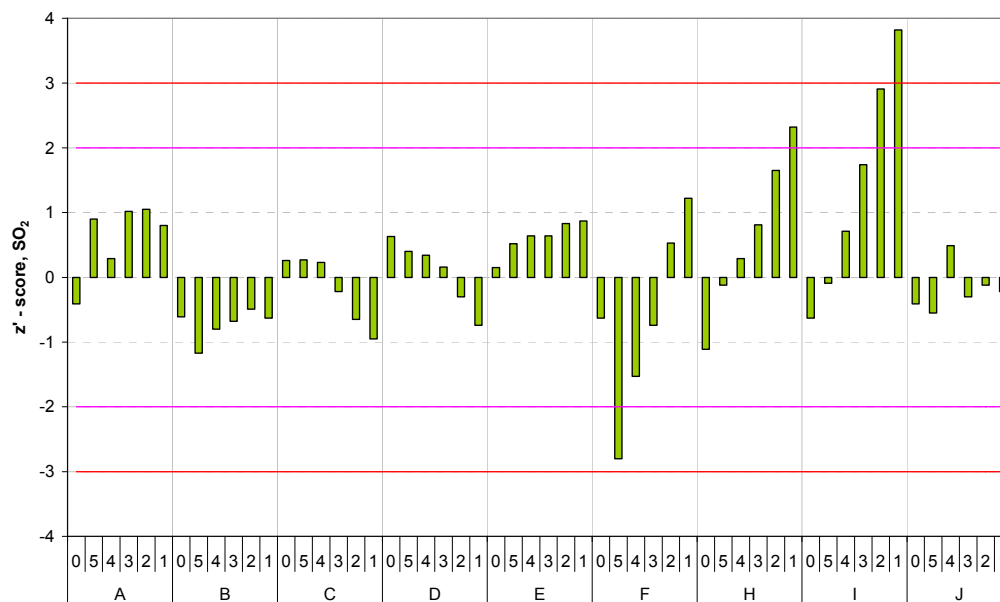


Figure 1: The z'-score evaluations of SO₂ measurements are given for each participant and each tested concentration level. The evaluations are in the order of increasing concentrations (run number order (with nominal concentration) is: 0 (0 nmol/mol), 5 (3 nmol/mol), 4 (7 nmol/mol), 3 (19 nmol/mol), 2 (47 nmol/mol), 1 (132 nmol/mol)). The assessment criteria are presented as $z'=\pm 2$ and $z'=\pm 3$ lines. They represent the limits for the questionable and unsatisfactory results.

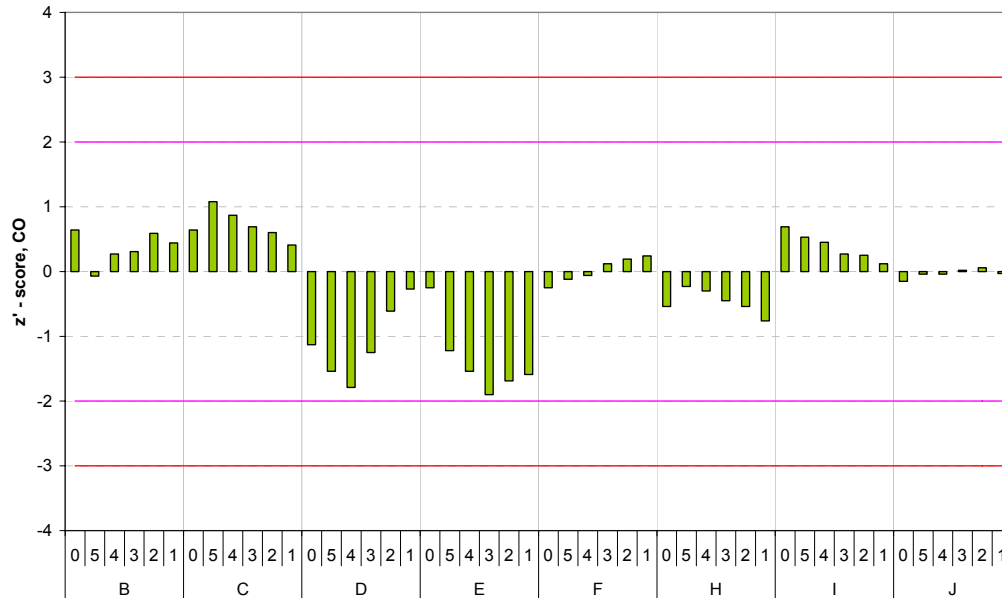


Figure 2: The z'-score evaluations of CO measurements are given for each participant and each tested concentration level. The evaluations are in the order of increasing concentrations (run number order (with nominal concentration) is: 0 (0 µmol/mol), 5 (1 µmol/mol), 4 (2 µmol/mol), 3 (4 µmol/mol), 2 (6 µmol/mol), 1 (9 µmol/mol)). The assessment criteria are presented as $z'=\pm 2$ and $z'=\pm 3$ lines. They represent the limits for the questionable and unsatisfactory results.

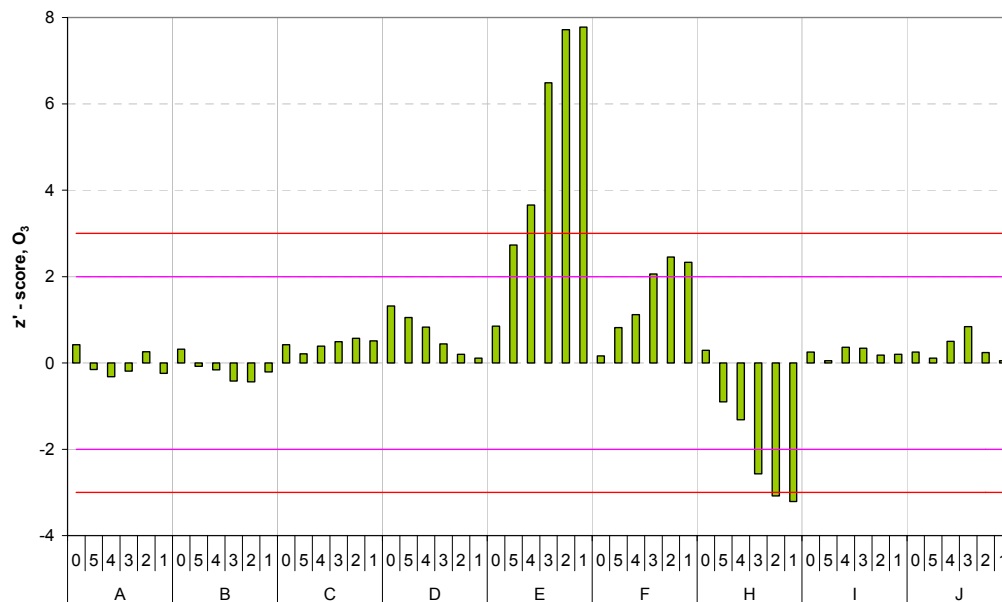


Figure 3: The z'-score evaluations of O₃ measurements are given for each participant and each tested concentration level. The evaluations are in the order of increasing concentrations (run number order (with nominal concentration) is: 0 (0 nmol/mol), 5 (14 nmol/mol), 4 (21 nmol/mol), 3 (60 nmol/mol), 2 (104 nmol/mol), 1 (120 nmol/mol)). The assessment criteria are presented as $z'=\pm 2$ and $z'=\pm 3$ lines. They represent the limits for the questionable and unsatisfactory results.

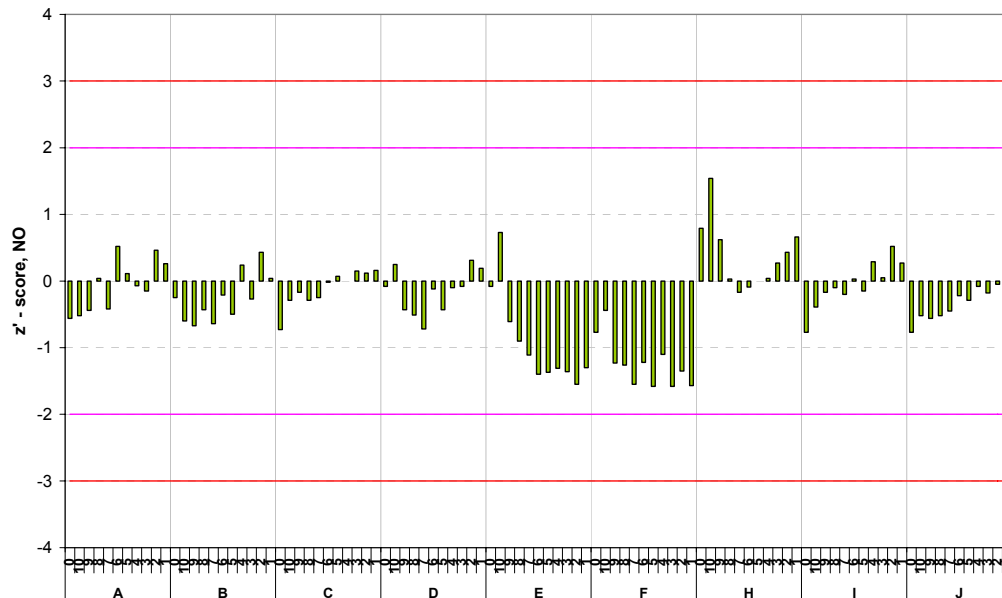


Figure 4: The z'-score evaluations of NO measurements are given for each participant and each tested concentration level. The evaluations are in the order of increasing concentrations (run number order (with nominal concentration) is: 0 (0 nmol/mol), 10 (2 nmol/mol), 9 (16 nmol/mol), 8 (30 nmol/mol), 7 (50 nmol/mol) , 6 (90 nmol/mol) , 5 (150 nmol/mol) , 4 (150 nmol/mol) , 3 (250 nmol/mol) , 2 (380 nmol/mol), 1 (500 nmol/mol)). The assessment criteria are presented as $z'=\pm 2$ and $z'=\pm 3$ lines. They represent the limits for the questionable and unsatisfactory results.

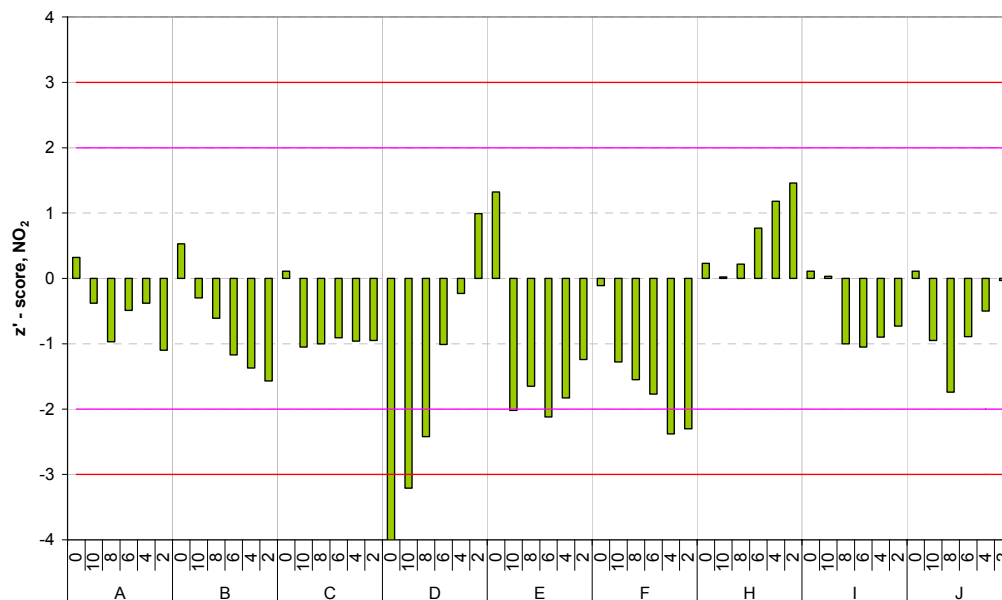


Figure 5: The z'-score evaluations of NO₂ measurements are given for each participant and each tested concentration level. The evaluations are in the order of increasing concentrations (run number order (with nominal concentration) is: 0 (0 nmol/mol), 10 (14 nmol/mol), 8 (21 nmol/mol), 6 (60 nmol/mol), 4 (104 nmol/mol), 2 (120 nmol/mol)). The assessment criteria are presented as $z'=\pm 2$ and $z'=\pm 3$ lines. They represent the limits for the questionable and unsatisfactory results.

E_n - number

The normalised deviations [18] (E_n) were calculated according to:

$$E_n = \frac{x_i - X}{\sqrt{U_{x_i}^2 + U_X^2}} \quad (2)$$

where 'X' is the assigned/reference value with an expanded uncertainty 'U_X' and 'x_i' is the participant's average value with an expanded uncertainty 'U_{x_i}'. Satisfactory results are the ones for which $|E_n| \leq 1$.

In Figure 6 to Figure 10 the biases of each participant (x_i-X) are plotted and error bars are used to denote the value of denominator of equation 2 ($\sqrt{U_{x_i}^2 + U_X^2}$). These plots represent also the E_n-number evaluations where, considering the E_n criteria ($|E_n| \leq 1$), all results with error bars touching or crossing x-axis are satisfactory. Reported standard uncertainties (Annex B) that are bigger than "standard deviation for proficiency assessments" (σ_p, Table 3) are considered not fit-for-purpose and are denoted with "*" in the x-axis of each figure.

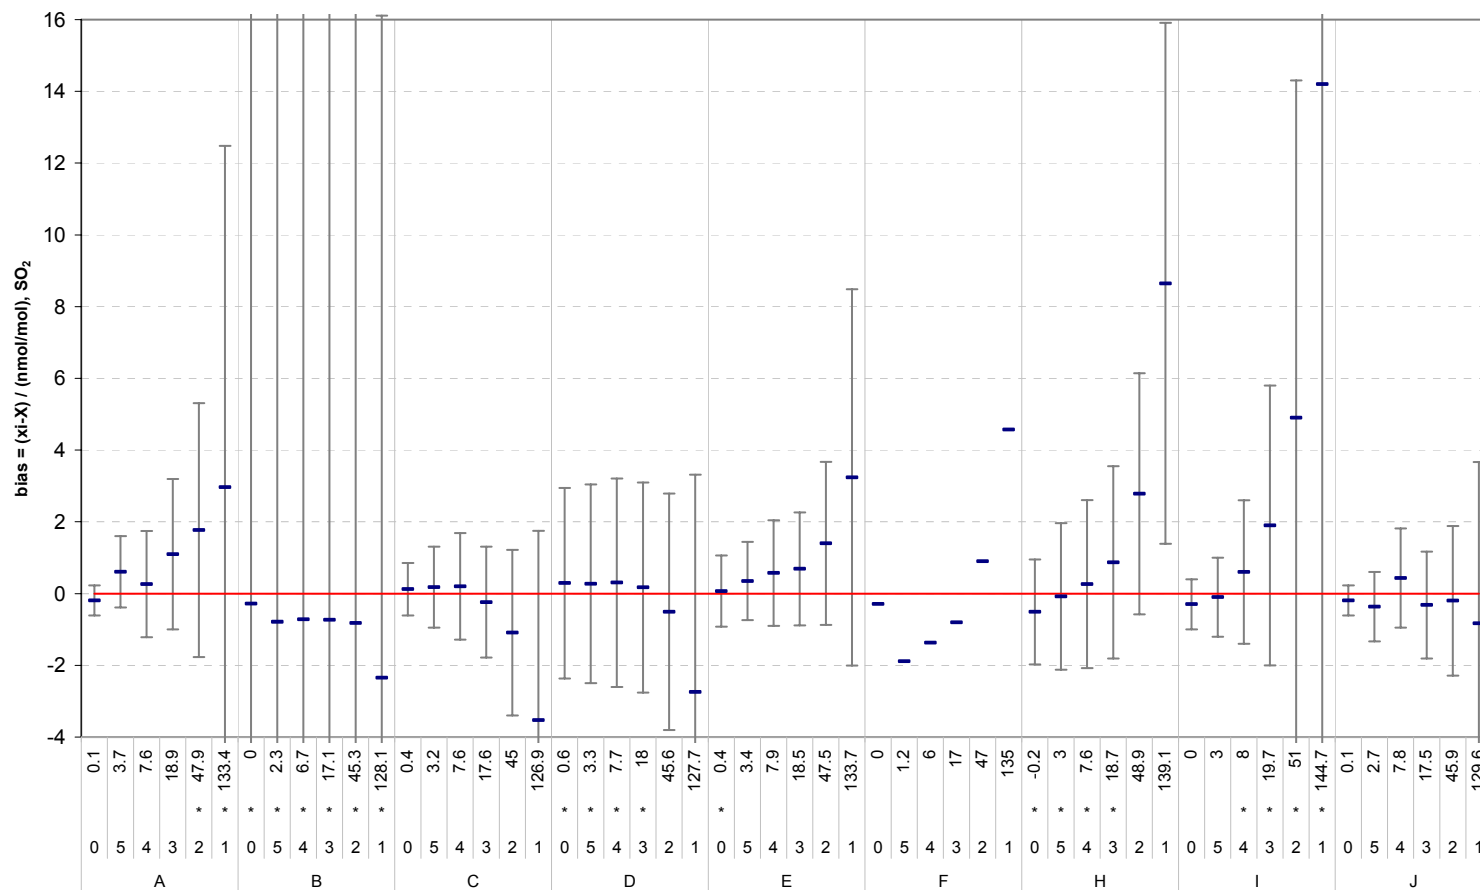


Figure 6: Bias of participant's SO₂ measurement results together with the expanded uncertainty of bias presented with error bar are given for each tested concentration level. The results with error bars touching or crossing the x-axis are satisfactory. For each evaluation the run number (numbers 0 to 5) together with the participants rounded run average (nmol/mol) is given. The '*' mark indicates reported standard uncertainties bigger then σ_p .

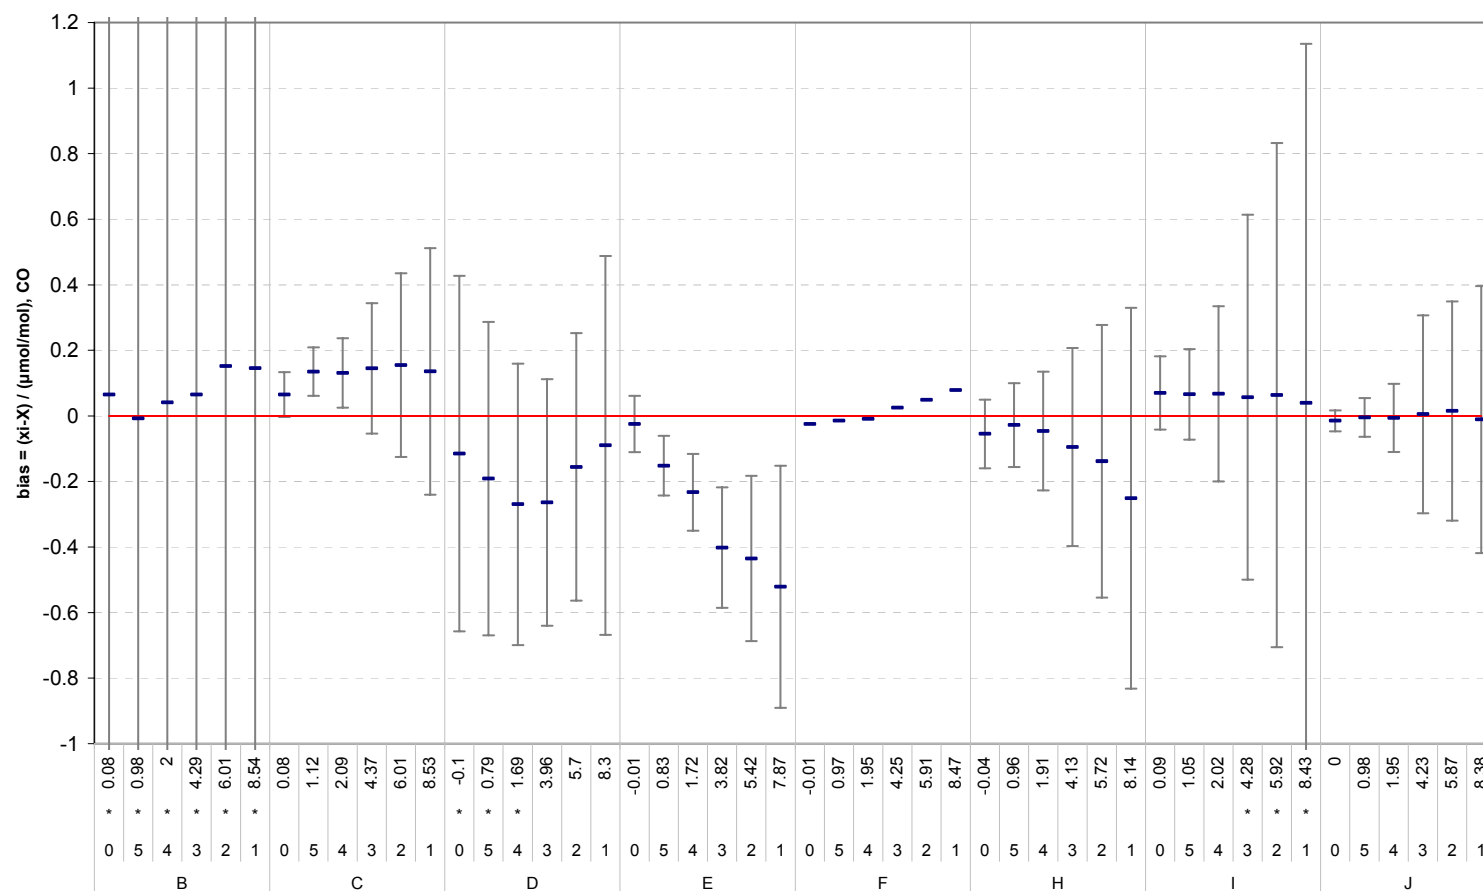


Figure 7: Bias of participant's CO measurement results together with the expanded uncertainty of bias presented with error bar are given for each tested concentration level. Results with error bars touching or crossing the x-axis are satisfactory. For each evaluation the run number (numbers 0 to 5) together with the participants rounded run average (μmol/mol) is given. The '*' mark indicates reported standard uncertainties bigger then σ_p .

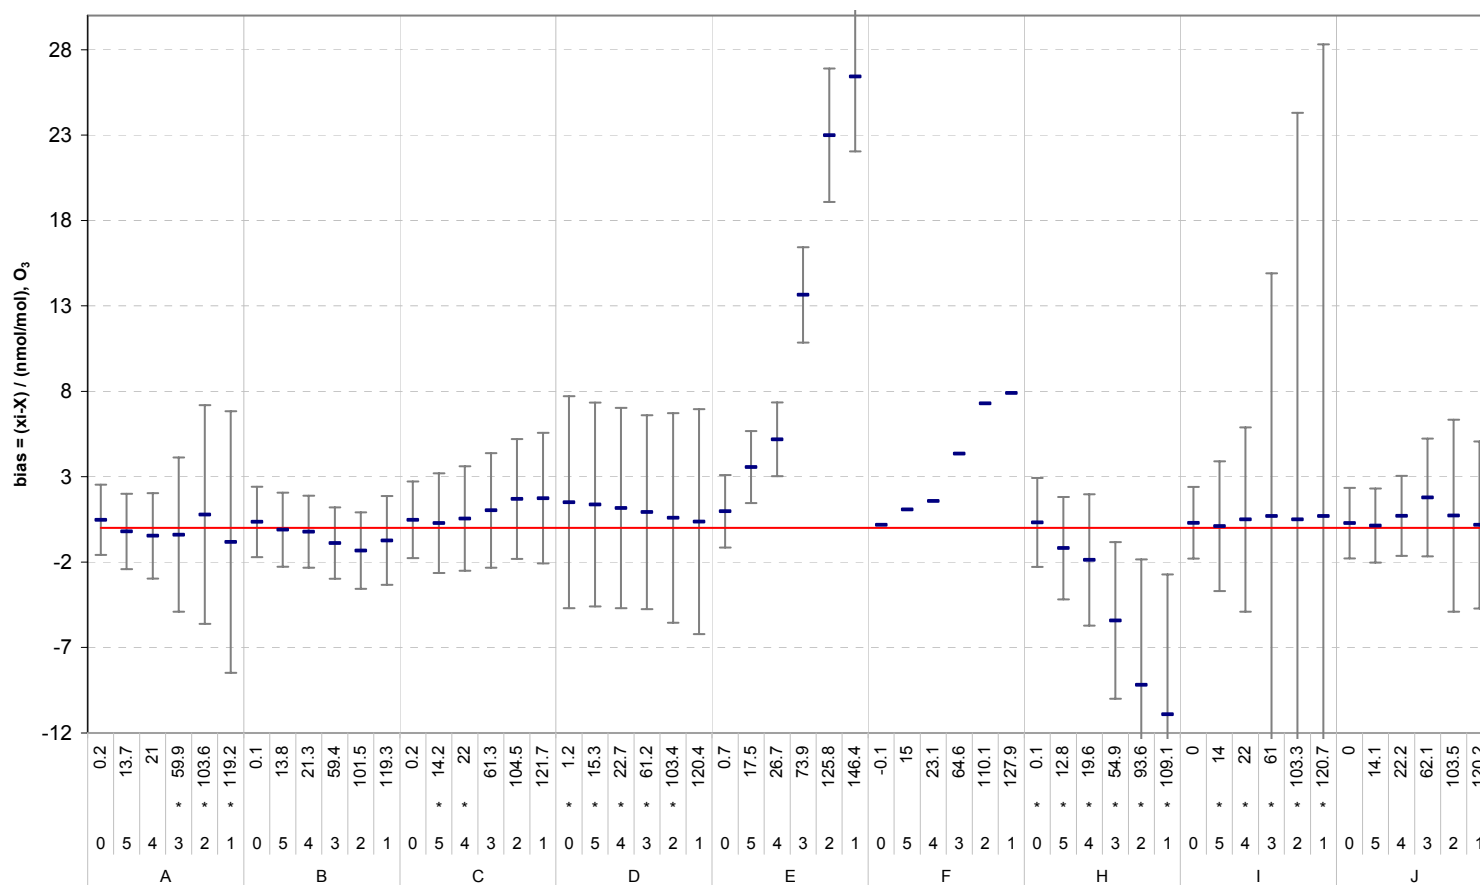


Figure 8: Bias of participant's O₃ measurement results together with the expanded uncertainty of bias presented with error bar are given for each tested concentration level. Results with error bars touching or crossing the x-axis are satisfactory. For each evaluation the run number (numbers 0 to 5) together with the participants rounded run average (nmol/mol) is given. The '*' mark indicates reported standard uncertainties bigger then σ_p .

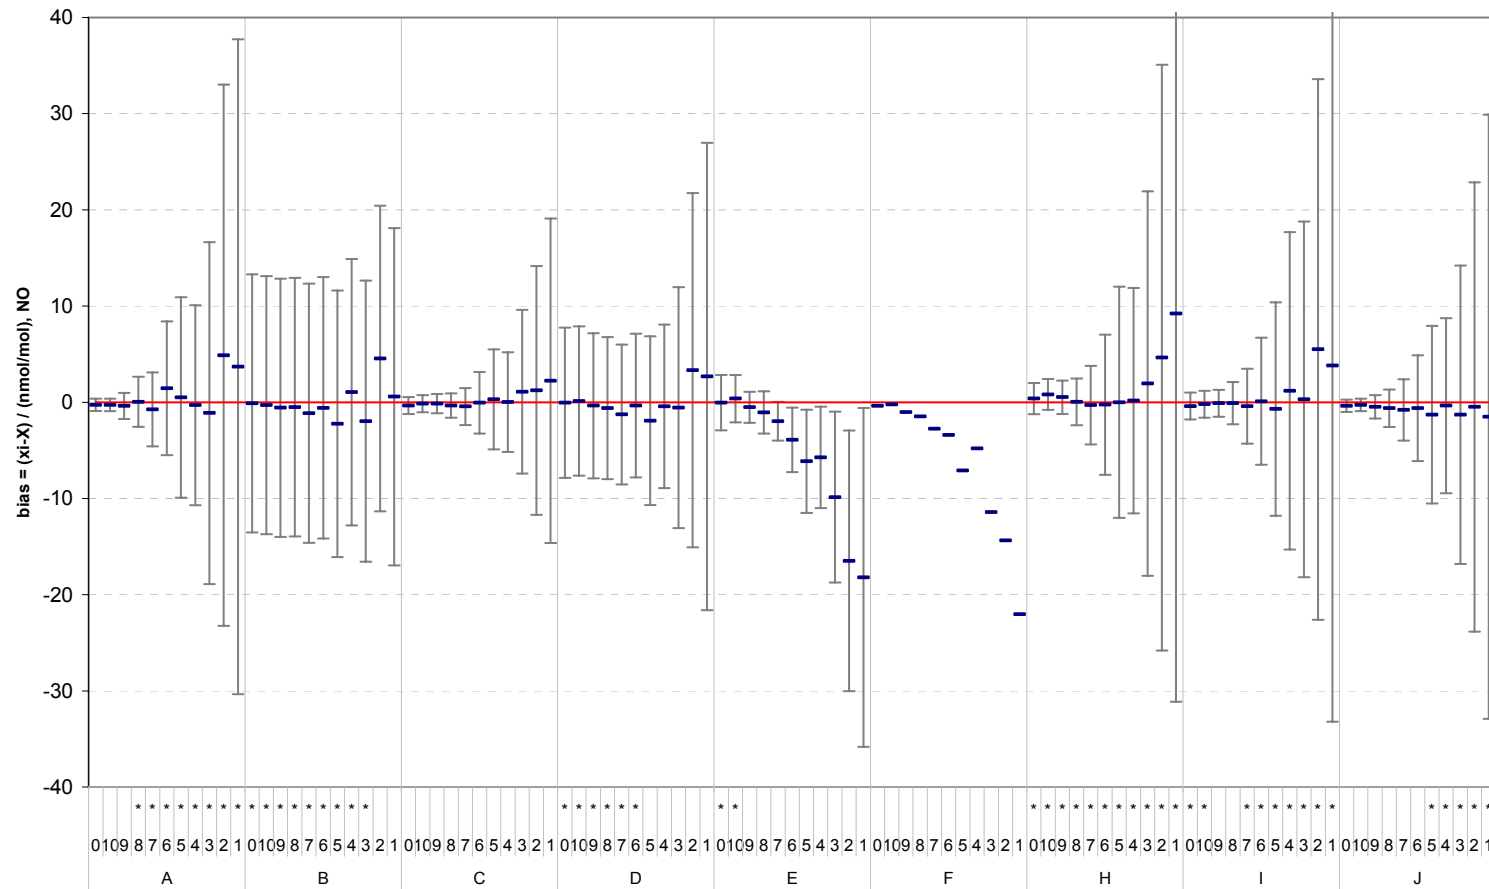


Figure 9: Bias of participant's NO measurement results together with the expanded uncertainty of bias presented with error bar are given for each tested concentration level. Results with error bars touching or crossing the x-axis are satisfactory. Evaluations are in the order of increasing concentrations (run number order (with nominal concentration) is: 0 (0 nmol/mol), 10 (2 nmol/mol), 9 (16 nmol/mol), 8 (30 nmol/mol), 7 (50 nmol/mol), 6 (90 nmol/mol), 5 (150 nmol/mol), 4 (150 nmol/mol), 3 (250 nmol/mol), 2 (380 nmol/mol), 1 (500 nmol/mol)). The '*' mark indicates reported standard uncertainties bigger then σ_p .

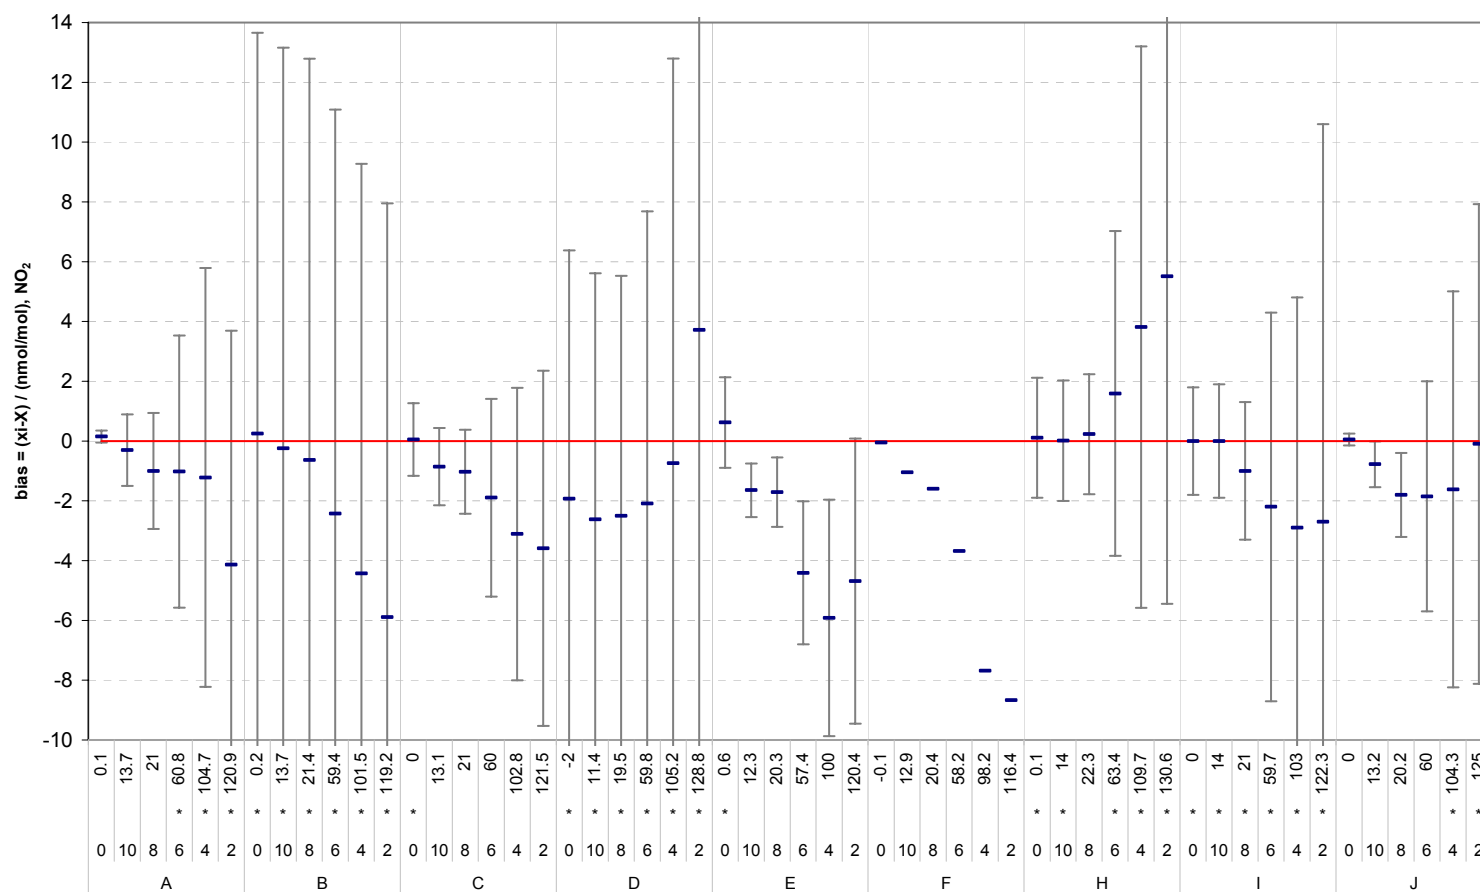


Figure 10: Bias of participant's NO₂ measurement results together with the expanded uncertainty of bias presented with error bar are given for tested concentration levels with NO₂ run numbers 0, 2, 4, 6, 8 and 10 (see Table 2). Results with error bars touching or crossing the x-axis are satisfactory. For each evaluation the run number together with the participants rounded run average (nmol/mol) is given. The '**' mark indicates reported standard uncertainties bigger then σ_p.

6. Performance characteristics of individual laboratories

Individual participants' biases were evaluated and are presented in chapter 5 (Figure 6-Figure 10). Since the results of NO₂ runs 1,3,5,7 and 9 were not treated in the proficiency evaluation the biases of these runs are presented in Figure 11.

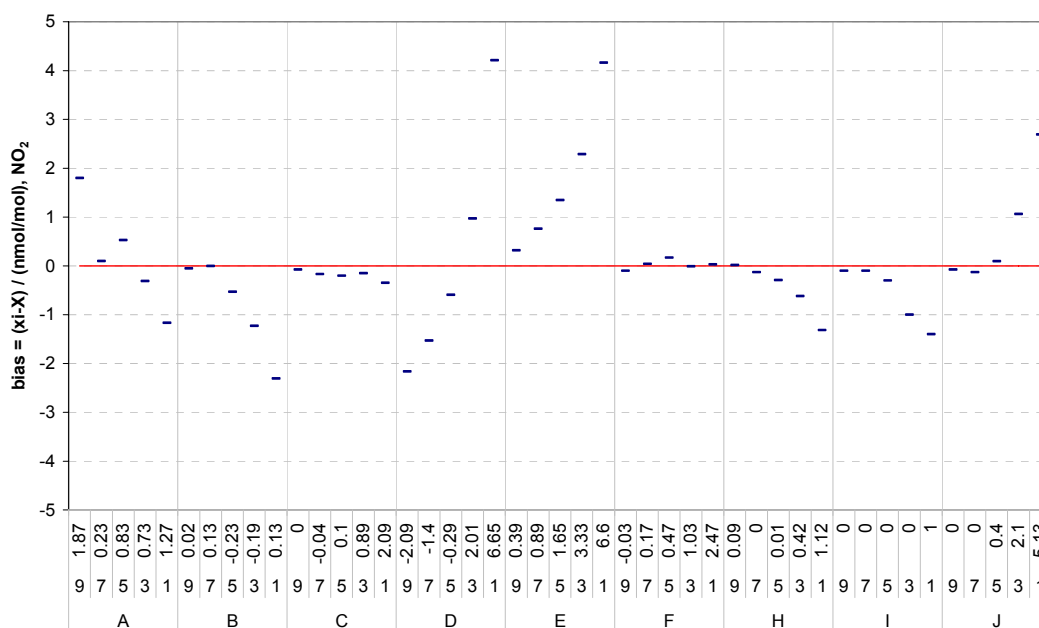


Figure 11: Bias of participant's NO₂ measurements for run numbers 1, 3, 5, 7 and 9
 At these test gas mixtures the concentration levels of NO₂ were zero and the concentration levels of NO were not zero (see Table 2). In that perspective the figure shows the effect of NO concentration on NO₂ measurements. For each evaluation the run number together with the participants rounded run average (nmol/mol) is given.

The efficiency of NO₂-to-NO converters of NO_x analyzers

Since NO and NO₂ test gases were produced by gas phase titration it is possible to evaluate the efficiency of NO₂-to-NO converter of each participant's NO_x analyser. The evaluation takes each participants NO and NO₂ measurements before and after oxidation by O₃. The converter efficiency (α) is calculated using equation 3 [9]:

$$\alpha = \frac{[NO2]_i - [NO2]_{i-1}}{[NO]_{i-1} - [NO]_i} \cdot 100\% \quad (3)$$

The O₃ measurements of each participant can also be compared to either NO or NO₂ change by calculating Δ^{NO} or Δ^{NO2} using equation 4 and 5 respectively:

$$\Delta^{NO} = [O3]_{i+1} - ([NO]_{i-1} - [NO]_i) \quad (4)$$

$$\Delta^{NO2} = [O3]_{i+1} - ([NO2]_i - [NO2]_{i-1}) \quad (5)$$

Ideal value for α is 100% while for Δ^{NO} and Δ^{NO2} it is 0 nmol/mol.

The evaluations of equation 4 and 5 can not be made for the fourth GPT test (at 14 ppb of NO₂), because O₃ was not completely reduced due to insufficient excess of NO. The evaluations of equations 3, 4 and 5 for each participant at different concentration levels are given in Table 4.

Table 4: The efficiency of NO₂-to-NO converters.

IE	NO ₂	α	Δ^{NO}	Δ^{NO_2}
code	nmol/mol	%	nmol/mol	nmol/mol
A	14	85.3		
A	22	98.6	-0.1	0.2
A	60	98.7	-0.9	-0.1
A	100	99.9	-0.5	-0.4
A	120	98.5	-2.3	-0.5
B	14	100.3		
B	22	100.0	0.0	0.0
B	60	99.2	-0.7	-0.2
B	100	99.8	-0.4	-0.2
B	120	100.3	0.6	0.2
C	14	94.1		
C	22	96.6	0.2	1.0
C	60	96.4	-0.8	1.5
C	100	96.2	-1.5	2.6
C	120	96.5	-1.9	2.3
D	14	100.0		
D	22	98.6	1.4	1.7
D	60	99.8	1.0	1.2
D	100	98.5	-1.4	0.2
D	120	100.1	-1.6	-1.8
E	14	91.6		
E	22	92.5	5.7	7.3
E	60	93.7	14.4	18.2
E	100	95.9	25.0	29.1
E	120	94.1	25.5	32.6
F	14	98.7		
F	22	98.2	2.4	2.8
F	60	99.4	6.6	6.9
F	100	98.9	11.8	12.9
F	120	99.1	12.9	14.0
G	14	99.7		
G	22	100.0	-0.4	-0.4
G	60	99.7	-1.5	-1.3
G	100	100.0	-2.1	-2.1
G	120	100.0	-2.7	-2.6
H	14	101.7		
H	22	103.2	-2.0	-2.6
H	60	102.3	-7.1	-8.6
H	100	102.5	-13.1	-15.7
H	120	101.7	-18.2	-20.4
I	14	100.0		
I	22	96.8	0.3	1.0
I	60	97.9	0.0	1.3
I	100	99.0	-0.7	0.3
I	120	100.2	-0.3	-0.6
J	14	96.1		
J	22	93.1	0.5	2.0
J	60	97.6	1.0	2.5
J	100	98.3	-0.5	1.3
J	120	98.5	-1.5	0.3

The uncertainty of converter efficiency evaluation at higher NO₂ concentration is smaller than at lower NO₂ concentration. For the general feeling, the average standard uncertainty of the converter efficiency is calculated, by taking standard deviations of repeatable measurements of quantities in equation 3, and is evaluated to approximately 1%, at 120 nmol/mol of NO₂, and 1.5%, at 14 nmol/mol of NO₂.

7. Discussion

For a general assessment of the quality of each result a decision diagram was developed (Figure 12) that categorises results in seven categories (a1 to a7). The general comments for each category are:

- a1: measurement result is completely satisfactory
- a2: measurement result is satisfactory (z'-score satisfactory and En-number ok) but the reported uncertainty is too high
- a3: measured value is satisfactory (z'-score satisfactory) but the reported uncertainty is underestimated (En-number not ok)
- a4: measurement result is questionable (z'-score questionable) but due to a high reported uncertainty can be considered valid (En-number ok)
- a5: measurement result is questionable (z'-score questionable and En-number not ok)
- a6: measurement result is unsatisfactory (z'-score unsatisfactory) but due to a high reported uncertainty can be considered valid (En-number ok)
- a7: measurement result is unsatisfactory (z'-score unsatisfactory and En-number not ok)

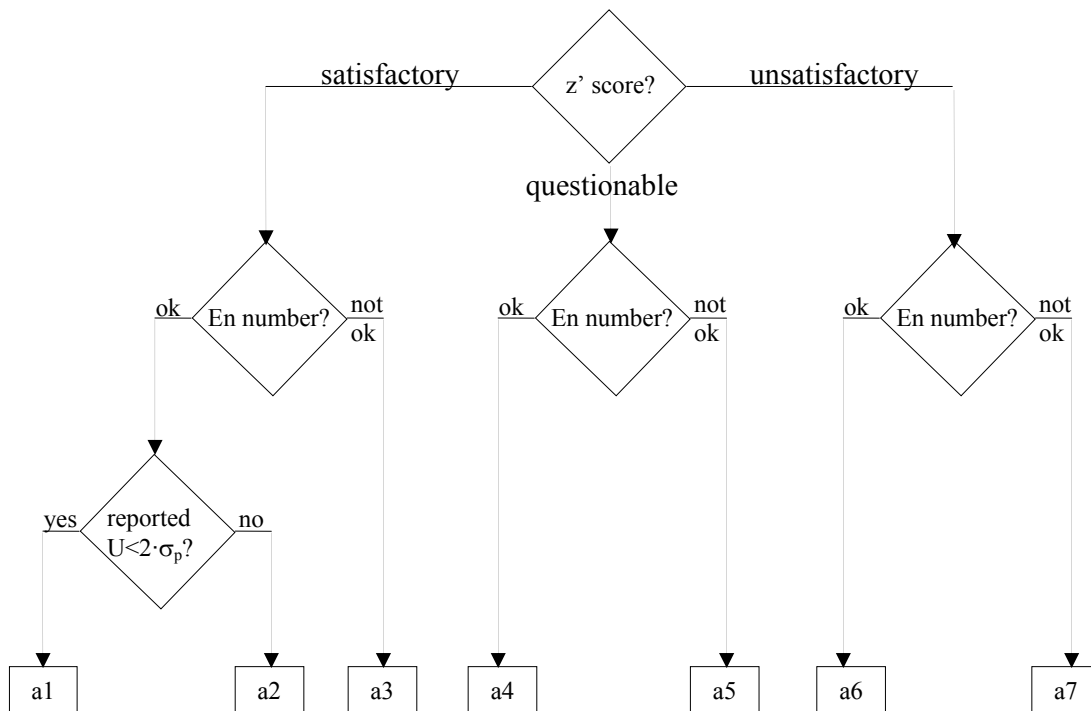


Figure 12: The decision diagram for general assessment of proficiency results.

The results of the IE were assigned to categories according to the diagram given in Figure 12 and are presented in Table 5. For clarity reasons, notation 'a1' is not inserted in Table 5 and all empty spaces represent 'a1' results.

Table 5: The general assessment of proficiency results.
 Empty spaces represent ‘a1’ results while results not reported are represented by ‘nv’ (no value).

	run number	conc. level	IE code									
			A	B	C	D	E	F	H	I	J	
SO ₂ (nmol/mol)	0	0.3		a2		a2	a2	a3	a2			
	5	3.1		a2		a2		a5	a2			
	4	7.4		a2		a2		a3	a2	a2		
	3	17.8		a2		a2		a3	a2	a2		
	2	46.1	a2	a2				a3		a4		
	1	130.4	a2	a2				a3	a5	a6		
CO (µmol/mol)	0	0.015	nv	a2		a2		a3				
	5	0.985	nv	a2	a3	a2	a3	a3				
	4	1.956	nv	a2	a3	a2	a3	a3				
	3	4.225	nv	a2			a3	a3		a2		
	2	5.858	nv	a2			a3	a3		a2		
	1	8.394	nv	a2			a3	a3		a2		
O ₃ (nmol/mol)	0	-0.3				a2		a3	a2			
	5	13.9			a2	a2	a5	a3	a2	a2		
	4	21.5			a2	a2	a7	a3	a2	a2		
	3	60.3	a2			a2	a7	a5	a5	a2		
	2	102.8	a2			a2	a7	a5	a7	a2		
	1	120	a2				a7	a5	a7	a2		
NO (nmol/mol)	0	0.4		a2		a2	a2	a3	a2	a2		
	10	2.2		a2		a2	a2	a3	a2	a2		
	9	16.1		a2		a2		a3	a2			
	8	29.1	a2	a2		a2		a3	a2			
	7	51	a2	a2		a2		a3	a2	a2		
	6	88.9	a2	a2		a2	a3	a3	a2	a2		
	4	147.1	a2	a2			a3	a3	a2	a2	a2	
	5	150.7	a2	a2			a3	a3	a2	a2	a2	
	3	252	a2	a2			a3	a3	a2	a2	a2	
	2	376.5	a2				a3	a3	a2	a2	a2	
1	499.2	a2					a3	a2	a2	a2		
NO ₂ (nmol/mol)	0	-0.1		a2	a2	a6	a2	a3	a2	a2		
	10	14		a2		a6	a5	a3	a2	a2		
	8	22		a2		a4	a3	a3		a2	a3	
	6	61.9	a2	a2		a2	a5	a3	a2	a2		
	4	105.9	a2	a2		a2	a3	a5	a2	a2	a2	
	2	125.1	a2	a2		a2		a5	a2	a2	a2	

Comparability of NO₂ and ozone measurements via GPT was investigated in studies [26] [27], where O₃ was traceable to international standards implementing ultraviolet photometry method and NO concentration change was traceable to NO international standards and GPT method was applied, and a significant difference of about 2% was confirmed. At this IE, this difference can not be confirmed by individual participants, due to significant uncertainties attributed to O₃ and NO concentration change measurements, but in the general evaluation a difference of 1% is observed between group average NO concentration change and average O₃.

8. Conclusions

The proficiency evaluation scheme has provided an assessment of the participants measured values and their evaluated uncertainties. In terms of the criteria imposed by the European Commission (σ_p) 36% of the results reported by AQUILA laboratories fall into 'a1' category and are good both in terms of measured values and evaluated uncertainties. In residual 56% of the results have good measured values but the evaluated uncertainties were either too high, category 'a2' (35%), or too small, category 'a3' (21%). The relative high number of 'a2' cases, where participant's evaluated uncertainty is higher than the common IE criterion, needs further investigation. The common IE criterion is confirmed to be realistic by comparison to reproducibility standard deviation obtained at this (Annex C) and other IEs [25], and is derived from the European standards' uncertainty requirements, which are explicit at high concentrations. Since the uncertainty requirements at zero concentration are not quantitatively stated in the European standards, the IE criteria at zero concentration had to be set within AQUILA. The initially proposed values were in use for IEs since June 2007 to October 2008 but at the November 2008 AQUILA meeting the IE criteria at zero concentration were enlarged and approved. The final values were also communicated to relevant CEN working group for potential future amendments of European standards. With that in mind especially 'a2' results at high concentration levels should be further investigated by the NRLs.

Three NRLs (participants D, E and F) have overall unsatisfactory results of the z'-score evaluation (one unsatisfactory, categories 'a6' or 'a7', or two questionable, categories 'a4' or 'a5', result per parameter) which in the view of AQUILA requires participation to the next IE in order to demonstrate remediation measures.

The comparability of results among AQUILA participants is best for NO and worst for NO₂ measurement method. The relative reproducibility limits, at the highest studied concentration levels, are 8.7% for SO₂, 11% for CO, 3.5% for O₃ and 1.2% for NO which are all below the objective derived from criteria imposed by the European Commission (σ_p). This is not the case for NO₂ where the relative reproducibility limit is 11.7% and the objective is 9.3% and is therefore generally considered as unsatisfactory. The NO₂ reproducibility limit was evaluated for the test mixture where beside NO₂ also NO was present. To achieve objective in such conditions, investigations should focus on converter efficiency and traceability of gas standards. For the latter case the uncertainties of both NO and NO₂ amount in the gas standard should be reduced.

9. References

- [1] Council Directive 1996/62/EC of 27 September 1996 on ambient air quality assessment and management, [Official Journal L 296 of 21.11.1996]
- [2] Council Directive 1999/30/EC of 22 April 1999 relating to limit values for sulphur dioxide, nitrogen dioxide and oxides of nitrogen, particulate matter and lead in ambient air, [Official Journal L 163 of 29.06.1999]
- [3] Council Directive 2000/69/EC Directive of the European Parliament and of the Council of 16 November 2000 relating to limit values for benzene and carbon monoxide in ambient air, [Official Journal L 313 of 13.12.2000]
- [4] Council Directive 2002/3/EC Directive of the European Parliament and of the Council of 12 February 2002 relating to ozone in ambient air, [Official Journal L 67 of 09.03.2002]
- [5] Directive 2004/107/EC of the European Parliament and of the Council of 15 December 2004 relating to arsenic, cadmium, mercury, nickel and polycyclic aromatic hydrocarbons in ambient air. Official Journal L 023 , 26/01/2005 P. 0003 - 0016
- [6] Directive 2008/50/EC of the European Parliament and of the Council of 21 May 2008 on ambient air quality and cleaner air for Europe, L 152, 11.06.2008
- [7] EN 14626:2005, Ambient air quality - Standard method for the measurement of the concentration of carbon monoxide by non-dispersive infrared spectroscopy
- [8] EN 14212:2005, Ambient air quality - Standard method for the measurement of the concentration of sulphur dioxide by ultraviolet fluorescence
- [9] EN 14211:2005, Ambient air quality - Standard method for the measurement of the concentration of nitrogen dioxide and nitrogen monoxide by chemiluminescence
- [10] EN 14625:2005, Ambient air quality - Standard method for the measurement of the concentration of ozone by ultraviolet photometry
- [11] ISO 6143:2001, Gas analysis - Comparison methods for determining and checking the composition of calibration gas mixtures
- [12] ISO 6144:2003, Gas analysis - Preparation of calibration gas mixtures - Static volumetric method
- [13] ISO 6145-7:2001, Gas analysis - Preparation of calibration gas mixtures using dynamic volumetric methods - Part 7: Thermal mass-flow controllers
- [14] Mücke H.-G., (2008), Air quality management in the WHO European Region – Results of a quality assurance and control programme on air quality monitoring (1994-2004), Environment International, EI-01718

- [15] Mücke H.-G., et al. (2000), European Intercomparison workshop on air quality monitoring vol.4 – Measuring NO, NO₂, O₃ and SO₂ – Air Hygiene Report 13, WHO Collaboration Centre for Air Quality Management and Air Pollution Control, ISSN 0938 - 9822
- [16] <http://ies.jrc.ec.europa.eu/aquila-homepage.html>
- [17] Organization of intercomparison exercises for gaseous air pollution for EU national air quality reference laboratories and laboratories of the WHO EURO region; <http://ies.jrc.ec.europa.eu/aquila-project/role-and-tasks-of-national-reference-laboratories.html>
- [18] ISO 13528:2005, Statistical methods for use in proficiency testing by interlaboratory comparisons
- [19] ISO 5725-1:1994, Accuracy (trueness and precision) of measurement methods and results – Part 1: General principles and definitions
- [20] ISO 5725-2:1994, Accuracy (trueness and precision) of measurement methods and results – Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method
- [21] ISO 5725-6:1994, Accuracy (trueness and precision) of measurement methods and results - Part 6: Use in practice of accuracy values
- [22] Harmonisation of Directive 92/72/EEC on air pollution by ozone, E. De Saeger et al., EUR 17662, 1997
- [23] European comparison of Nitrogen Dioxide calibration methods, E. De Saeger et al., EUR 17661, 1997
- [24] ISO/DIS:15337, Ambient air - Gas phase titration - Calibration of analysers for ozone
- [25] Draft report: The evaluation of the Intercomparison Exercise for SO₂, CO, O₃, NO and NO₂ carried out in June 2007 in Ispra
- [26] Viallon, J., et al. (2006), International comparison CCQM-P28: Ozone at ambient level, Metrologia, 43, Tech. Suppl., 08010, doi:10.1088/0026-1394/43/1A/08010
- [27] Tanimoto, H., et al. (2006), Intercomparison of ultraviolet photometry and gas-phase titration techniques for ozone reference standards at ambient levels, Journal of Geophysical Research, vol. 111, D16313, doi:10.1029/2005JD006983
- [28] GUM Workbench, The Tool for Expression of Uncertainty of Measurements
- [29] VDI 2449 Part3: 2001, Measurement methods test criteria- General method for the determination of the uncertainty of calibratable measurement methods

Annex A. Assigned values

The assigned values of tested concentration levels were derived from ERLAPs measurements which are calibrated against the certified reference values of CRMs and are traceable to international standards. In this perspective the assigned values are reference values as defined in the ISO 13528 [18].

ERLAPs SO₂, CO and NO analysers were calibrated according to the methodology described in the ISO 6143 [11]. A different number (4 for SO₂, 7 for CO and 5 for NO) of reference gas mixtures were produced from the primary reference materials (produced and certified by NMi Van Swinden Laboratorium) by dynamic dilution method using mass flow controllers [13]. All flows were measured with a certified volumeter. For the evaluation of concentration values and the uncertainties of reference gas mixtures and the evaluation of calibrations two computer applications were used, the “GUM WORKBENCH” [28] and “B-least” [29] respectively. For extending calibration from the NO to NO₂ channel of NO_x analyser the GPT test was performed to establish the efficiency of NO₂-converter. For O₃ measurements, the primary standard was used.

ERLAP’s measurement results were validated by comparison to the group statistics (x^* and s^*) for every parameter and concentration level of the IE. These statistics are calculated from all participants, applying the robust method described in the Annex C of ISO 13528 [18]. The validation is taking in account ERLAP’s value (X) and its standard uncertainty (u_X) as given in expression 6 [18]:

$$\frac{|x^* - X|}{\sqrt{\frac{(1,25 \cdot s^*)^2}{p} + u_X^2}} < 2 \quad (6)$$

Where ‘ x^* ’ and ‘ s^* ’ represent robust average and robust standard deviation respectively and ‘ p ’ is the number of participants.

In Table 6 all inputs for expression 6 are given and all ERLAP’s measurement results are confirmed to be valid.

Table 6: The validation of assigned values (X) by comparison to the robust averages (x*) with taking into the account the standard uncertainties of assigned values (uX'), and robust standard deviations (s*) as denoted by expression 6.

run	unit	X	uX'	x*	s*	p	val.	run	unit	X	uX'	x*	s*	p	val.
CO_0	µmol/mol	0.015	0.016	0.012	0.068	9	OK	NO_0	nmol/mol	0.4	0.4	0.2	0.3	10	OK
CO_1	µmol/mol	8.394	0.148	8.383	0.147	9	OK	NO_1	nmol/mol	499.2	5.7	500.2	3.9	10	OK
CO_2	µmol/mol	5.858	0.104	5.845	0.161	9	OK	NO_2	nmol/mol	376.5	4.3	378.2	3.8	10	OK
CO_3	µmol/mol	4.225	0.077	4.218	0.106	9	OK	NO_3	nmol/mol	252	2.9	251.1	2	10	OK
CO_4	µmol/mol	1.956	0.042	1.948	0.083	9	OK	NO_4	nmol/mol	147.1	1.8	146.9	0.6	10	OK
CO_5	µmol/mol	0.985	0.022	0.975	0.037	9	OK	NO_5	nmol/mol	150.7	1.8	149.4	1.7	10	OK
O3_0	nmol/mol	-0.3	1.1	0.1	0.3	10	OK	NO_6	nmol/mol	88.9	1.1	88.6	0.6	10	OK
O3_1	nmol/mol	120	1.3	120.5	1.8	10	OK	NO_7	nmol/mol	51	0.8	50.2	0.8	10	OK
O3_2	nmol/mol	102.8	1.2	103.5	1.5	10	OK	NO_8	nmol/mol	29.1	0.5	28.7	0.6	10	OK
O3_3	nmol/mol	60.3	1.1	61.1	1.9	10	OK	NO_9	nmol/mol	16.1	0.4	15.8	0.4	10	OK
O3_4	nmol/mol	21.5	1.1	22	1.1	10	OK	NO_10	nmol/mol	2.2	0.4	2.1	0.2	10	OK
O3_5	nmol/mol	13.9	1.1	14.1	0.5	10	OK	NO2_0	nmol/mol	-0.1	0.1	0	0.1	9	OK
SO2_0	nmol/mol	0.3	0.3	0.1	0.3	10	OK	NO2_1	nmol/mol	2.4	0.9	2.1	1.7	9	OK
SO2_1	nmol/mol	130.4	1.2	132.3	5.2	10	OK	NO2_2	nmol/mol	125.1	1.8	121.9	3.7	9	OK
SO2_2	nmol/mol	46.1	0.8	46.8	1.7	10	OK	NO2_3	nmol/mol	1	0.7	0.9	0.9	9	OK
SO2_3	nmol/mol	17.8	0.7	18	1	10	OK	NO2_4	nmol/mol	105.9	1.5	103.1	3	9	OK
SO2_4	nmol/mol	7.4	0.7	7.6	0.4	10	OK	NO2_5	nmol/mol	0.3	0.5	0.3	0.5	9	OK
SO2_5	nmol/mol	3.1	0.5	3	0.6	10	OK	NO2_6	nmol/mol	61.9	0.9	60	1.6	9	OK
								NO2_7	nmol/mol	0.1	0.3	0.1	0.2	9	OK
								NO2_8	nmol/mol	22	0.4	21.1	0.9	9	OK
								NO2_9	nmol/mol	0.1	0.2	0	0.1	9	OK

The homogeneity of test gas was evaluated from measurements at the beginning and end of the distribution line. From the relative differences between beginning and end measurements, average and standard deviation were calculated, and the uncertainty of test gas due to lack of homogeneity was calculated as the sum of squares of these average and standard deviation. The upper and lower limits of bias due to homogeneity was evaluated to be smaller than 0.5% which constitutes the relative standard uncertainty of 0,3% ($u_{\text{homogeneity}}$) of tested concentration level. The standard uncertainties of assigned/reference values (u_X) were calculated with equation 7 and used in the proficiency evaluations of chapter 5.

$$u_X^2 = u_{X'}^2 + (X \cdot u_{\text{homogeneity}})^2 \quad (7)$$

Annex B. Results of the IE

The reported values, presented also in graphs, are given in this annex. The participants were asked to report results (x_{ij} , $u(x_i)$ and $U(x_i)$) expressed in mol/mol units. For all the runs except concentration levels 0, also each participant's average (x_i) and standard deviation (s_i) are presented. As a group evaluation robust average (x^*) and robust standard deviation (s^*) were calculated (applying the procedure described in Annex C of ISO 13528) for each run, and are presented in the following tables. The assigned value is indicated on the graphs with the red line and the individual laboratories expanded uncertainties ($U(x_i)$) are indicated with error bars.

Reported values for SO₂

Table 7: Reported values for SO₂ concentration level 0.

parameter: SO2		all units are nmol/mol									
level: 0		x*: 0.15		s*: 0.24							
	A	B	C	D	E	F	G	H	I	J	
$x_{i,1}$	0.10	0.01	0.41	0.58	0.36	0.0	0.29	-0.22	0	0.10	
$u(x_i)$	0.005	9.15	0.30	1.31	0.45		0.21	0.70	0.3	0.01	
$U(x_i)$	0.010	18.30	0.60	2.62	0.90		0.42	1.40	0.6	0.01	

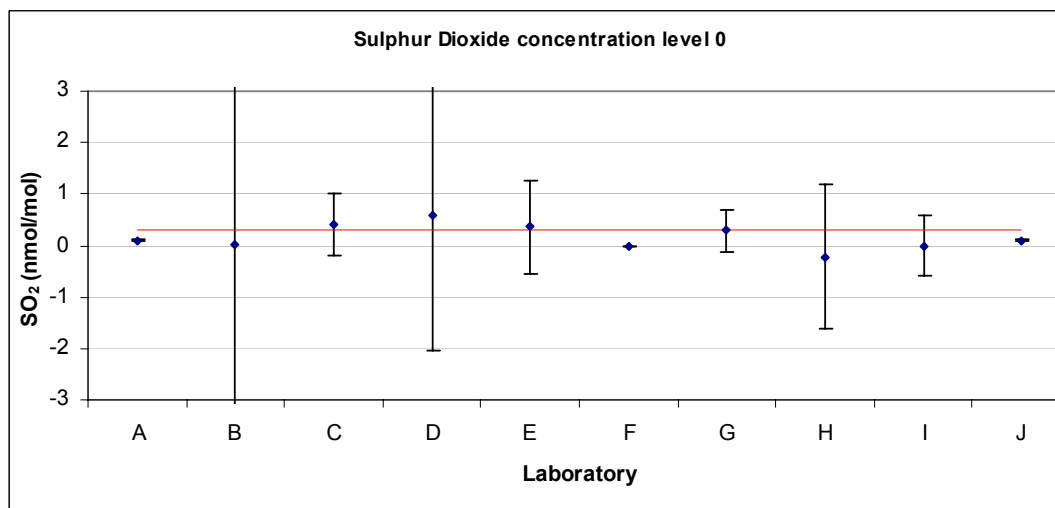


Figure 13: Reported values for SO₂ concentration level 0.

Table 8: Reported values for SO₂ concentration level 1.

parameter: SO ₂		all units are nmol/mol									
level: 1		x*: 132.35					s*: 5.19				
	A	B	C	D	E	F	G	H	I	J	
xi,1	133.30	128.02	126.70	127.41	133.41	135.0	130.47	138.93	144	129.30	
xi,2	133.40	128.15	127.05	127.76	133.82	135.0	130.47	139.12	145	129.60	
xi,3	133.50	128.10	126.96	127.91	133.79	135.0	130.36	139.18	145	129.90	
xi	133.400	128.090	126.903	127.693	133.673	135.00	130.433	139.077	144.7	129.600	
si	0.100	0.066	0.182	0.257	0.229	0.00	0.064	0.131	0.6	0.300	
u(xi)	4.60	9.15	2.35	2.78	2.33		1.14	3.43	13.2	1.90	
U(xi)	9.20	18.30	4.70	5.56	4.66		2.28	6.85	26.4	3.80	

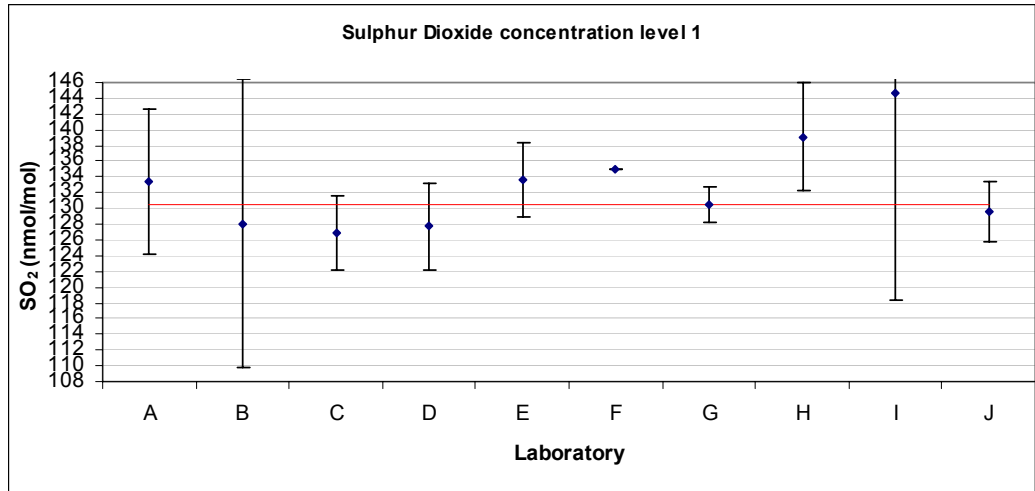


Figure 14: Reported values for SO₂ concentration level 1.

Table 9: Reported values for SO₂ concentration level 2.

parameter: SO ₂		all units are nmol/mol									
level: 2		x*: 46.82					s*: 1.66				
	A	B	C	D	E	F	G	H	I	J	
xi,1	47.80	45.32	45.12	45.68	47.54	46.5	46.10	48.85	51	45.93	
xi,2	47.90	45.22	45.01	45.53	47.48	47.5	45.99	48.83	51	45.91	
xi,3	47.90	45.30	44.91	45.56	47.49	47.0	46.21	48.95	51	45.87	
xi	47.867	45.280	45.013	45.590	47.503	47.00	46.100	48.877	51.0	45.903	
si	0.058	0.053	0.105	0.079	0.032	0.50	0.110	0.064	0.0	0.031	
u(xi)	1.60	9.15	0.87	1.46	0.85		0.74	1.50	4.6	0.72	
U(xi)	3.20	18.30	1.74	2.93	1.70		1.48	3.00	9.3	1.44	

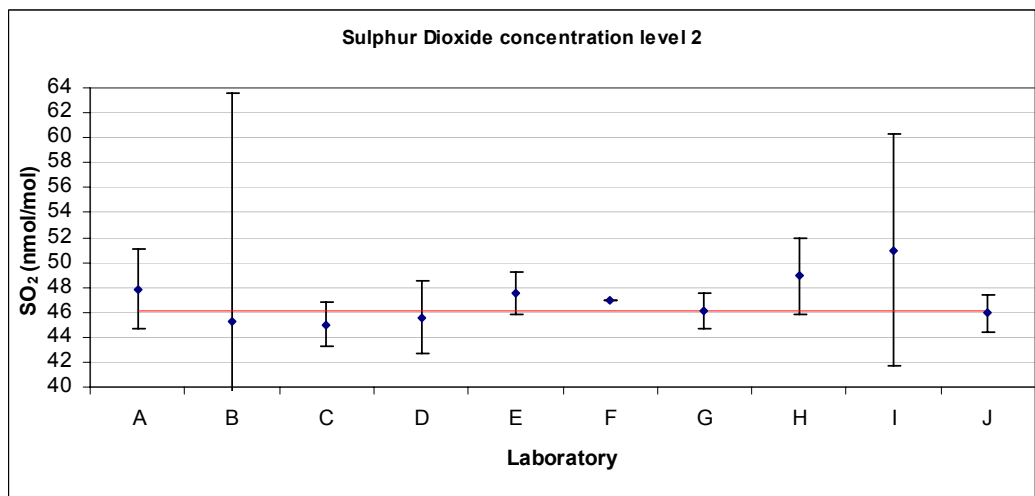


Figure 15: Reported values for SO₂ concentration level 2.

Table 10: Reported values for SO₂ concentration level 3.

parameter: SO ₂		all units are nmol/mol									
level: 3		x*: 18.03 s*: 0.91									
	A	B	C	D	E	F	G	H	I	J	
xi,1	18.90	17.14	17.62	18.06	18.51	17.0	17.91	18.65	20	17.56	
xi,2	18.90	17.01	17.38	18.01	18.48	17.0	17.69	18.63	20	17.46	
xi,3	18.90	17.06	17.68	17.84	18.48	17.0	17.80	18.74	19	17.41	
xi	18.900	17.070	17.560	17.970	18.490	17.00	17.800	18.673	19.7	17.477	
si	0.000	0.066	0.159	0.115	0.017	0.00	0.110	0.059	0.6	0.076	
u(xi)	0.79	9.15	0.35	1.29	0.38		0.69	1.15	1.8	0.28	
U(xi)	1.58	18.30	0.70	2.58	0.76		1.38	2.30	3.6	0.56	

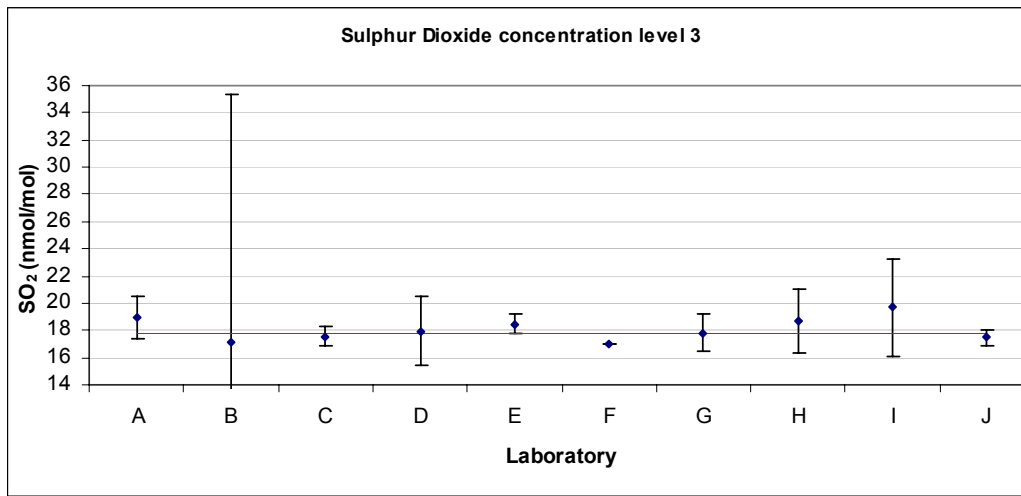


Figure 16: Reported values for SO₂ concentration level 3.

Table 11: Reported values for SO₂ concentration level 4.

parameter: SO ₂		all units are nmol/mol									
level: 4		x*: 7.59 s*: 0.34									
	A	B	C	D	E	F	G	H	I	J	
xi,1	7.70	6.67	7.68	7.47	7.93	6.0	7.33	7.61	8	7.79	
xi,2	7.60	6.63	7.50	7.74	7.94	6.0	7.44	7.63	8	7.81	
xi,3	7.60	6.64	7.54	7.79	7.94	6.0	7.33	7.64	8	7.81	
xi	7.633	6.647	7.573	7.667	7.937	6.00	7.367	7.627	8.0	7.803	
si	0.058	0.021	0.095	0.172	0.006	0.00	0.064	0.015	0.0	0.012	
u(xi)	0.29	9.15	0.30	1.29	0.28		0.68	0.96	0.8	0.12	
U(xi)	0.58	18.30	0.60	2.57	0.56		1.36	1.91	1.5	0.24	

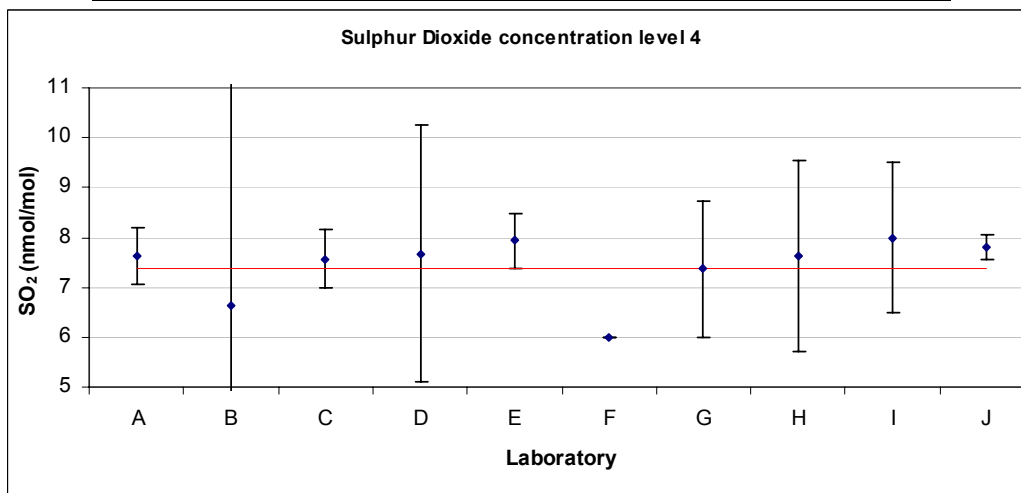


Figure 17: Reported values for SO₂ concentration level 4.

Table 12: Reported values for SO₂ concentration level 5.

parameter: SO ₂ level: 5		all units are nmol/mol									
		x*: 3.00					s*: 0.51				
	A	B	C	D	E	F	G	H	I	J	
xi,1	3.60	2.27	3.21	3.37	3.42	1.5	3.06	3.06	3	2.71	
xi,2	3.70	2.27	3.32	3.27	3.42	1.0	3.06	2.92	3	2.69	
xi,3	3.70	2.27	3.19	3.35	3.38	1.0	3.06	2.97	3	2.68	
xi	3.667	2.270	3.240	3.330	3.407	1.17	3.060	2.983	3.0	2.693	
si	0.058	0.000	0.070	0.053	0.023	0.29	0.000	0.071	0.0	0.015	
u(xi)	0.13	9.15	0.30	1.30	0.26		0.48	0.90	0.3	0.06	
U(xi)	0.26	18.30	0.60	2.60	0.52		0.96	1.80	0.6	0.12	

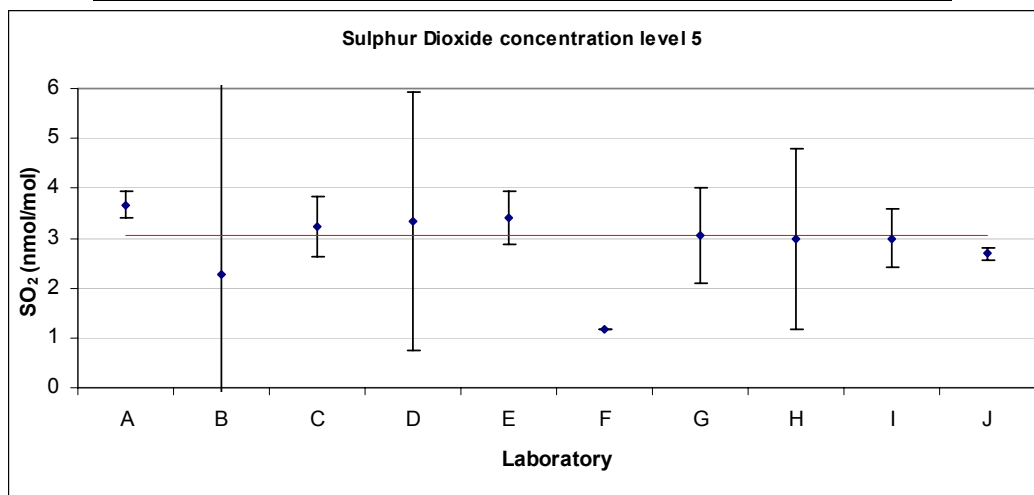


Figure 18: Reported values for SO₂ concentration level 5.

Reported values for CO

Table 13: Reported values for CO concentration level 0.

parameter: CO level: 0		all units are µmol/mol									
		x*: 0.01					s*: 0.07				
	B	C	D	E	F	G	H	I	J		
xi,1	0.08	0.08	-0.100	-0.01	-0.01	0.015	-0.04	0.085	0.00		
u(xi)	0.86	0.030	0.270	0.04		0.016	0.05	0.053	0.00		
U(xi)	1.72	0.060	0.541	0.080		0.032	0.10	0.107	0.00		

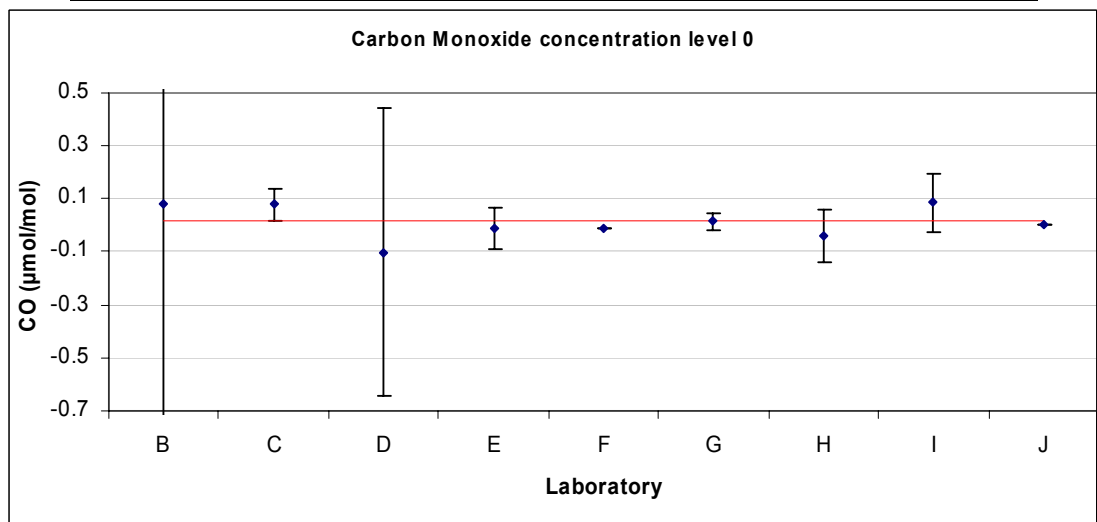


Figure 19: Reported values for CO concentration level 0.

Table 14: Reported values for CO concentration level 1.

parameter: CO level: 1		all units are $\mu\text{mol/mol}$								
		x*: 8.38			s*: 0.15					
	B	C	D	E	F	G	H	I	J	
xi,1	8.54	8.53	8.307	7.94	8.47	8.389	8.14	8.428	8.38	
xi,2	8.54	8.53	8.303	7.81	8.47	8.397	8.14	8.437	8.38	
xi,3	8.54	8.53	8.303	7.87	8.48	8.396	8.15	8.437	8.39	
xi	8.540	8.530	8.3043	7.873	8.473	8.3940	8.143	8.4340	8.383	
si	0.000	0.000	0.0023	0.065	0.006	0.0044	0.006	0.0052	0.006	
u(xi)	0.86	0.116	0.248	0.11		0.146	0.25	0.527	0.14	
U(xi)	1.72	0.232	0.496	0.220		0.292	0.50	1.054	0.28	

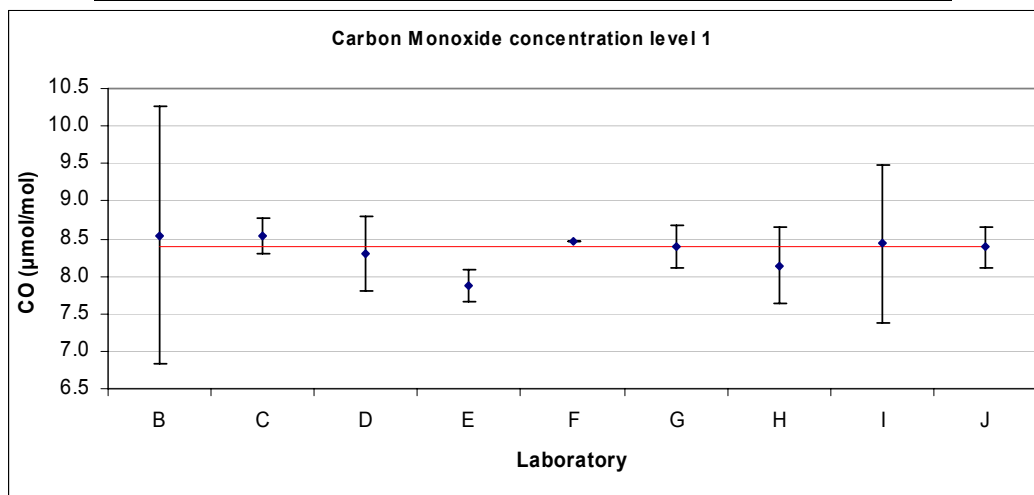


Figure 20: Reported values for CO concentration level 1.

Table 15: Reported values for CO concentration level 2.

parameter: CO level: 2		all units are $\mu\text{mol/mol}$								
		x*: 5.85			s*: 0.16					
	B	C	D	E	F	G	H	I	J	
xi,1	6.01	6.01	5.707	5.42	5.87	5.856	5.72	5.920	5.87	
xi,2	6.01	6.01	5.697	5.43	5.92	5.858	5.72	5.921	5.87	
xi,3	6.01	6.02	5.703	5.42	5.93	5.859	5.72	5.921	5.88	
xi	6.010	6.013	5.7023	5.423	5.907	5.8577	5.720	5.9207	5.873	
si	0.000	0.006	0.0050	0.006	0.032	0.0015	0.000	0.0006	0.006	
u(xi)	0.85	0.093	0.175	0.07		0.103	0.18	0.370	0.13	
U(xi)	1.70	0.187	0.350	0.140		0.206	0.36	0.740	0.26	

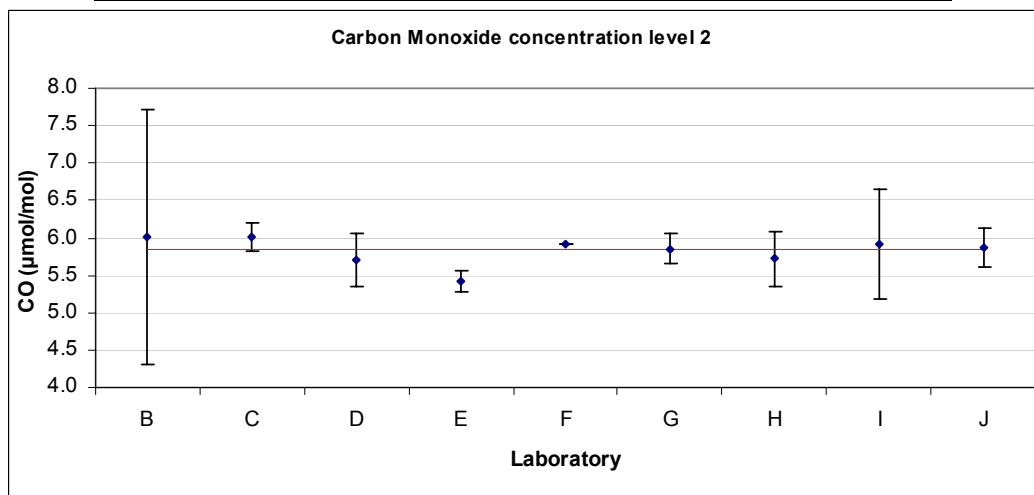


Figure 21: Reported values for CO concentration level 2.

Table 16: Reported values for CO concentration level 3.

parameter: CO level: 3		all units are $\mu\text{mol/mol}$							
		x*: 4.22				s*: 0.11			
	B	C	D	E	F	G	H	I	J
xi,1	4.29	4.37	3.967	3.83	4.25	4.225	4.13	4.284	4.23
xi,2	4.29	4.37	3.963	3.82	4.25	4.228	4.13	4.282	4.23
xi,3	4.29	4.37	3.953	3.82	4.25	4.222	4.13	4.280	4.23
xi	4.290	4.370	3.9610	3.823	4.250	4.2250	4.130	4.2820	4.230
si	0.000	0.000	0.0072	0.006	0.000	0.0030	0.000	0.0020	0.000
u(xi)	0.85	0.063	0.171	0.05		0.076	0.13	0.268	0.13
U(xi)	1.70	0.126	0.343	0.100		0.152	0.26	0.535	0.26

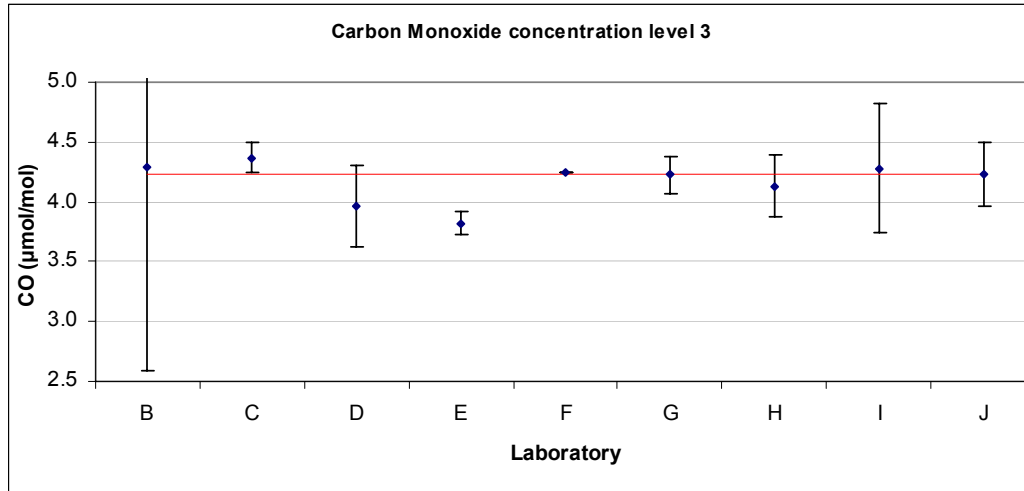


Figure 22: Reported values for CO concentration level 3.

Table 17: Reported values for CO concentration level 4.

parameter: CO level: 4		all units are $\mu\text{mol/mol}$							
		x*: 1.95				s*: 0.08			
	B	C	D	E	F	G	H	I	J
xi,1	2.00	2.09	1.697	1.72	1.95	1.959	1.91	2.024	1.95
xi,2	2.00	2.08	1.670	1.73	1.95	1.955	1.91	2.024	1.95
xi,3	1.99	2.09	1.690	1.72	1.94	1.953	1.91	2.022	1.95
xi	1.997	2.087	1.6857	1.723	1.947	1.9557	1.910	2.0233	1.950
si	0.006	0.006	0.0140	0.006	0.006	0.0031	0.000	0.0012	0.000
u(xi)	0.89	0.032	0.210	0.04		0.042	0.08	0.127	0.03
U(xi)	1.78	0.064	0.421	0.080		0.084	0.16	0.253	0.06

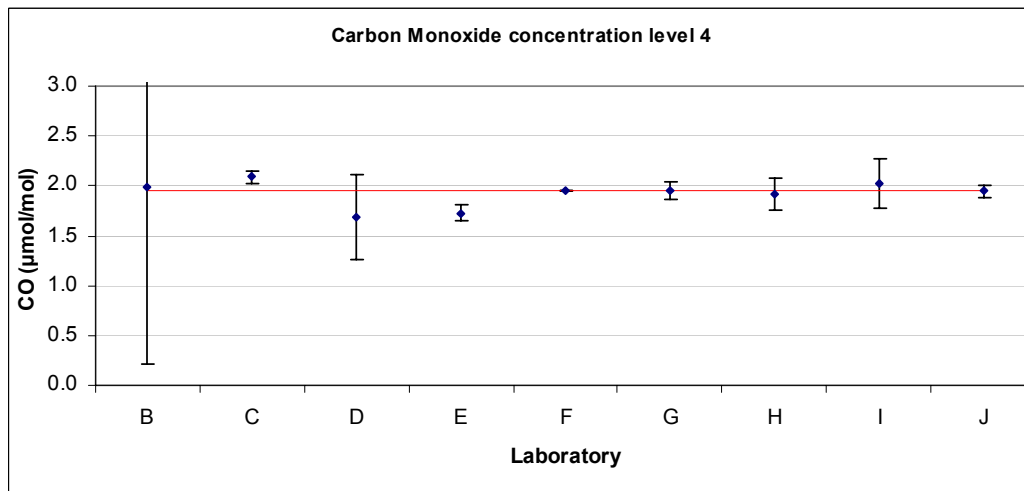


Figure 23: Reported values for CO concentration level 4.

Table 18: Reported values for CO concentration level 5.

parameter: CO level: 5		all units are $\mu\text{mol/mol}$								
		x*: 0.98			s*: 0.04					
	B	C	D	E	F	G	H	I	J	
xi,1	0.98	1.12	0.793	0.83	0.97	0.986	0.96	1.054	0.98	
xi,2	0.98	1.12	0.797	0.83	0.97	0.986	0.95	1.050	0.98	
xi,3	0.97	1.12	0.793	0.84	0.97	0.984	0.96	1.048	0.98	
xi	0.977	1.120	0.7943	0.833	0.970	0.9853	0.957	1.0507	0.980	
si	0.006	0.000	0.0023	0.006	0.000	0.0012	0.006	0.0031	0.000	
u(xi)	0.89	0.030	0.238	0.04		0.022	0.06	0.066	0.02	
U(xi)	1.78	0.060	0.476	0.080		0.044	0.12	0.131	0.04	

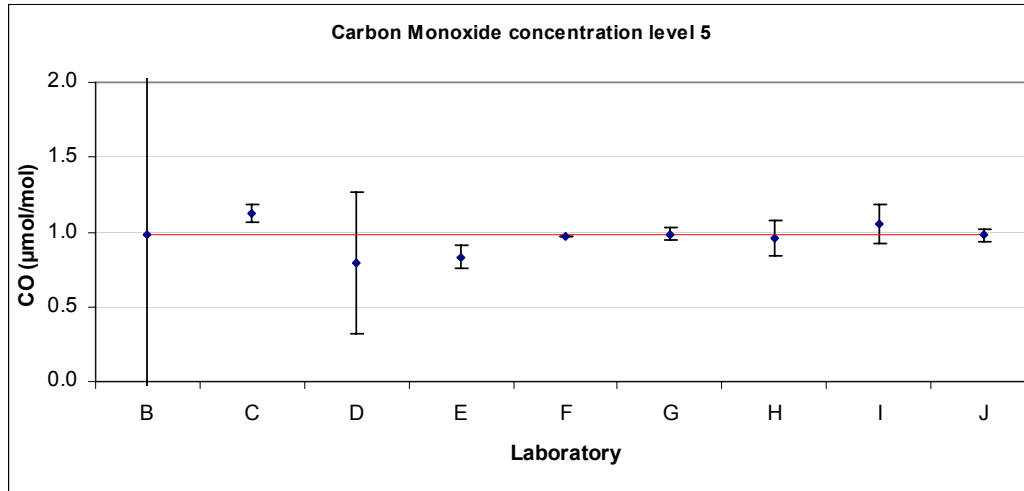


Figure 24: Reported values for CO concentration level 5.

Reported values for O₃

Table 19: Reported values for O₃ concentration level 0.

parameter: O3 level: 0		all units are nmol/mol								
		x*: 0.09			s*: 0.22					
	A	B	C	D	E	F	G	H	I	J
xi,1	0.20	0.08	0.20	1.23	0.69	-0.1	-0.28	0.05	0	0.00
u(xi)	0.01	0.04	0.45	2.93	0.25		1.03	0.80	0.3	0.00
U(xi)	0.02	0.08	0.90	5.85	0.50		2.06	1.60	0.6	0.00

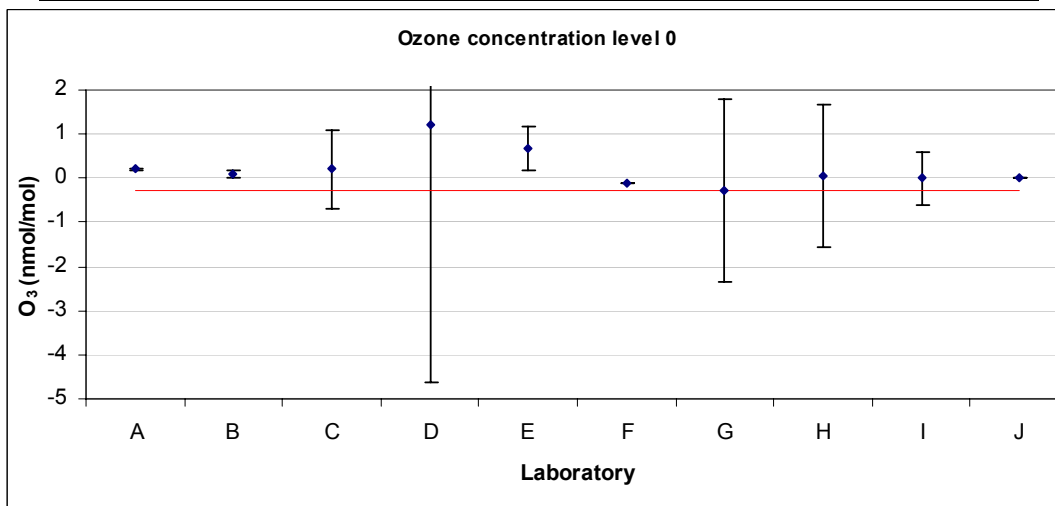


Figure 25: Reported values for O₃ concentration level 0.

Table 20: Reported values for O₃ concentration level 1.

parameter: O ₃ level: 1		all units are nmol/mol									
		x*: 120.46					s*: 1.72				
	A	B	C	D	E	F	G	H	I	J	
xi,1	119.10	119.10	121.28	120.02	145.78	127.3	119.72	108.61	120	122.10	
xi,2	119.20	119.22	121.88	120.59	146.58	128.0	120.04	109.24	121	122.60	
xi,3	119.20	119.50	122.05	120.50	146.89	128.4	120.23	109.42	121	115.80	
xi	119.167	119.273	121.737	120.370	146.417	127.90	119.997	109.090	120.7	120.167	
si	0.058	0.205	0.405	0.306	0.573	0.56	0.258	0.425	0.6	3.790	
u(xi)	3.60	0.04	1.40	3.02	1.76		1.25	3.88	13.8	2.07	
U(xi)	7.20	0.08	2.80	6.05	3.52		2.50	7.76	27.5	4.14	

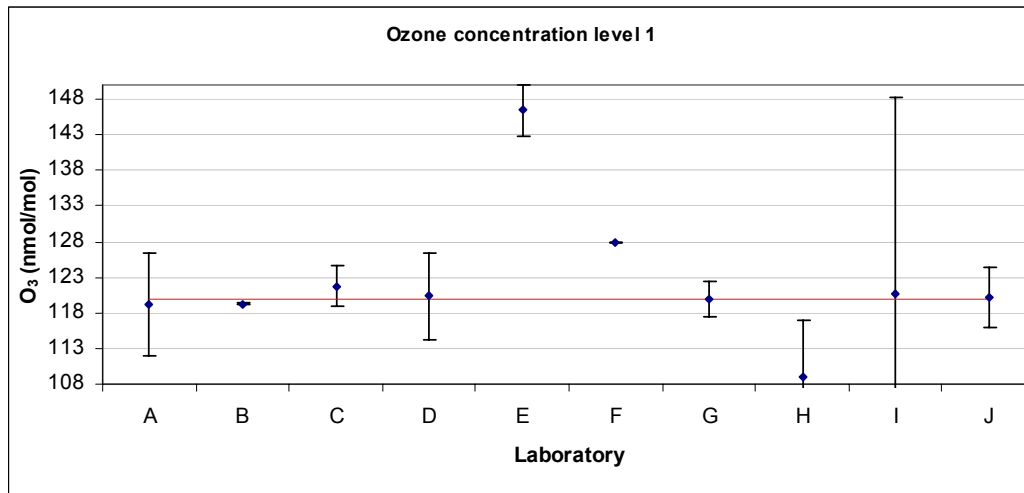


Figure 26: Reported values for O₃ concentration level 1.

Table 21: Reported values for O₃ concentration level 2.

parameter: O ₃ level: 2		all units are nmol/mol									
		x*: 103.48					s*: 1.50				
	A	B	C	D	E	F	G	H	I	J	
xi,1	103.50	101.30	104.20	102.93	125.22	109.6	102.44	93.16	103	100.60	
xi,2	103.50	101.44	104.57	103.50	125.90	110.2	102.87	93.70	103	104.70	
xi,3	103.70	101.65	104.66	103.69	126.18	110.4	103.04	93.94	104	105.20	
xi	103.567	101.463	104.477	103.373	125.767	110.07	102.783	93.600	103.3	103.500	
si	0.115	0.176	0.244	0.396	0.494	0.42	0.309	0.399	0.6	2.524	
u(xi)	3.00	0.05	1.34	2.85	1.60		1.07	3.50	11.8	2.58	
U(xi)	6.00	0.10	2.70	5.71	3.20		2.14	6.99	23.7	5.16	

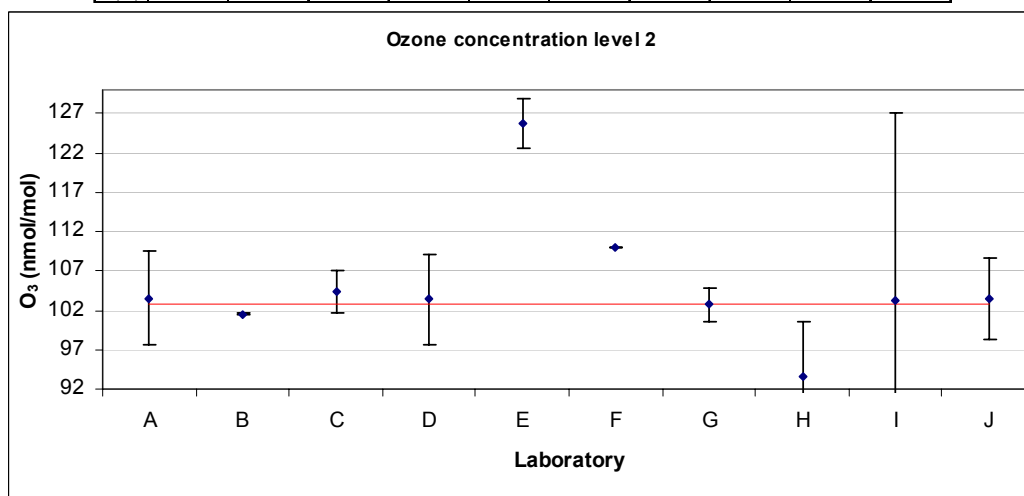


Figure 27: Reported values for O₃ concentration level 2.

Table 22: Reported values for O₃ concentration level 3.

parameter: O ₃ level: 3		all units are nmol/mol									
		x*: 61.09 s*: 1.83									
	A	B	C	D	E	F	G	H	I	J	
xi,1	60.00	59.40	61.48	61.24	73.93	64.7	60.36	54.92	61	61.20	
xi,2	59.90	59.42	61.38	61.06	73.95	64.6	60.30	54.87	61	62.40	
xi,3	59.80	59.40	61.10	61.35	73.95	64.6	60.22	54.85	61	62.60	
xi	59.900	59.407	61.320	61.217	73.943	64.63	60.293	54.880	61.0	62.067	
si	0.100	0.012	0.197	0.146	0.012	0.06	0.070	0.036	0.0	0.757	
u(xi)	2.00	0.08	1.31	2.64	0.92		1.03	2.04	7.0	1.37	
U(xi)	4.00	0.16	2.62	5.28	1.84		2.06	4.08	14.0	2.74	

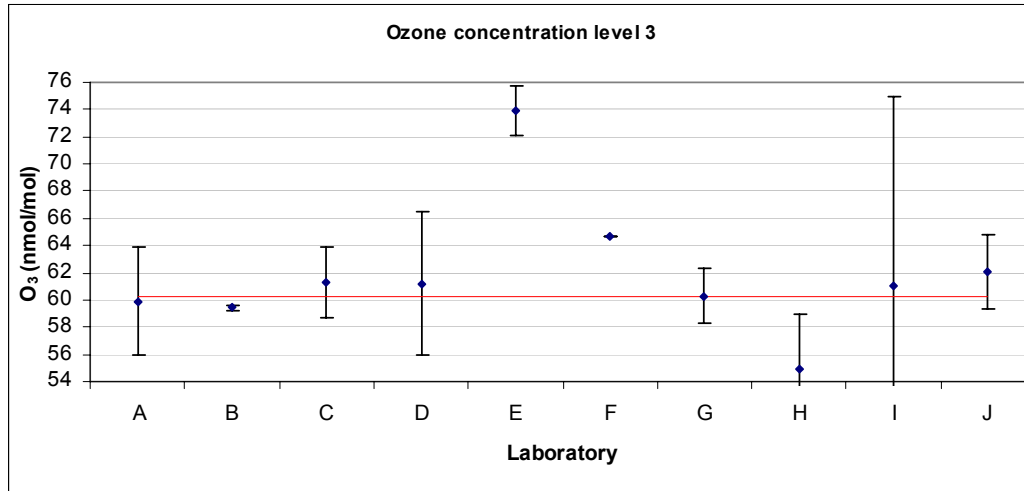


Figure 28: Reported values for O₃ concentration level 3.

Table 23: Reported values for O₃ concentration level 4.

parameter: O ₃ level: 4		all units are nmol/mol									
		x*: 21.98 s*: 1.07									
	A	B	C	D	E	F	G	H	I	J	
xi,1	21.10	21.25	21.87	22.64	26.61	23.0	21.46	19.60	22	21.90	
xi,2	21.00	21.28	22.10	22.67	26.69	23.1	21.52	19.63	22	22.10	
xi,3	21.00	21.29	22.15	22.66	26.74	23.1	21.49	19.62	22	22.60	
xi	21.033	21.273	22.040	22.657	26.680	23.07	21.490	19.617	22.0	22.200	
si	0.058	0.021	0.149	0.015	0.066	0.06	0.030	0.015	0.0	0.361	
u(xi)	0.70	0.22	1.13	2.75	0.32		1.03	1.62	2.5	0.56	
U(xi)	1.40	0.44	2.26	5.49	0.64		2.06	3.24	5.0	1.12	

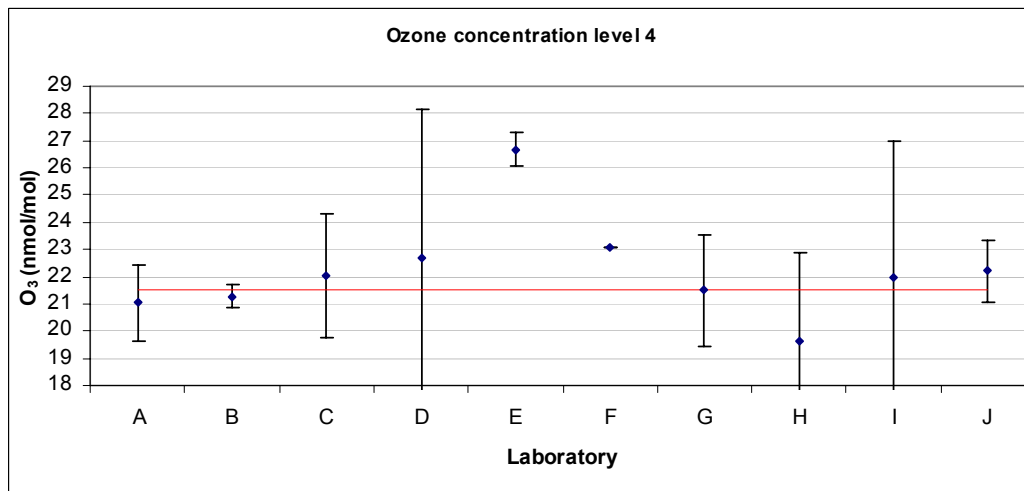


Figure 29: Reported values for O₃ concentration level 4.

Table 24: Reported values for O₃ concentration level 5.

parameter: O ₃ level: 5		all units are nmol/mol									
		x*: 14.10					s*: 0.44				
	A	B	C	D	E	F	G	H	I	J	
xi,1	13.80	13.80	14.25	15.26	17.44	15.0	13.91	12.75	14	13.60	
xi,2	13.70	13.85	14.20	15.33	17.49	15.0	13.94	12.73	14	14.10	
xi,3	13.70	13.85	14.19	15.32	17.56	15.0	13.94	12.76	14	14.50	
xi	13.733	13.833	14.213	15.303	17.497	15.00	13.930	12.747	14.0	14.067	
si	0.058	0.029	0.032	0.038	0.060	0.00	0.017	0.015	0.0	0.451	
u(xi)	0.40	0.34	1.03	2.80	0.22		1.03	1.09	1.6	0.35	
U(xi)	0.80	0.68	2.06	5.60	0.44		2.06	2.18	3.2	0.70	

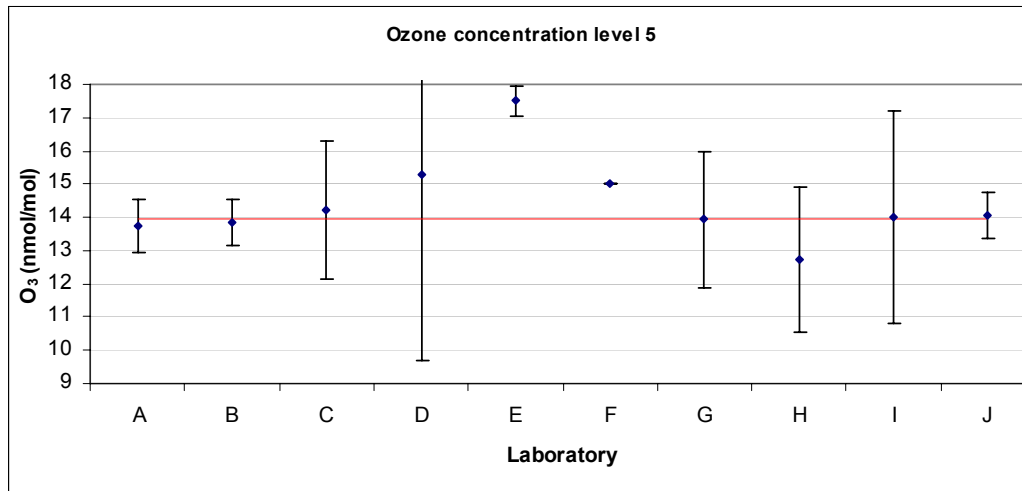


Figure 30: Reported values for O₃ concentration level 5.

Reported values for NO

Table 25: Reported values for NO concentration level 0.

parameter: NO level: 0		all units are nmol/mol									
		x*: 0.19					s*: 0.22				
	A	B	C	D	E	F	G	H	I	J	
xi,1	0.10	0.25	0.02	0.33	0.33	0.0	0.37	0.75	0	0.00	
u(xi)	0.01	6.97	0.30	3.89	1.40		0.32	0.75	0.6	0.00	
U(xi)	0.02	13.40	0.60	7.78	2.80		0.64	1.50	1.2	0.00	

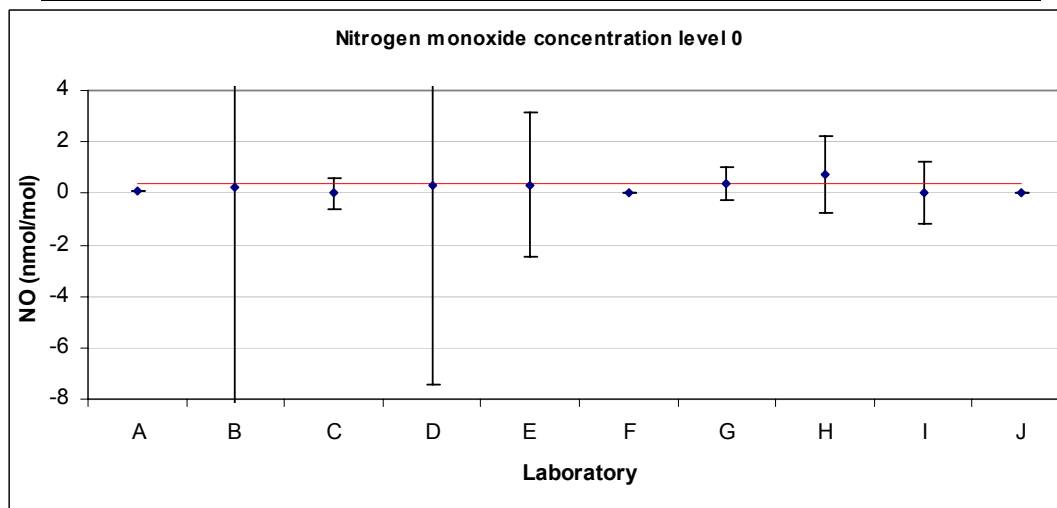


Figure 31: Reported values for NO concentration level 0.

Table 26: Reported values for NO concentration level 1.

parameter: NO level: 1		all units are nmol/mol									
		x*: 500.22 s*: 3.88									
	A	B	C	D	E	F	G	H	I	J	
xi,1	502.30	500.10	501.11	501.17	480.10	476.9	498.87	508.41	502	497.60	
xi,2	503.50	499.68	501.22	502.10	481.70	477.4	499.29	508.34	502	497.80	
xi,3	502.80	499.47	501.89	502.28	481.10	477.1	499.36	508.39	505	497.60	
xi	502.867	499.750	501.407	501.850	480.967	477.13	499.173	508.380	503.0	497.667	
si	0.603	0.321	0.422	0.596	0.808	0.25	0.265	0.036	1.7	0.115	
u(xi)	16.05	6.97	6.23	10.75	6.73		5.46	19.36	17.6	14.65	
U(xi)	32.10	13.40	12.50	21.50	13.48		10.92	38.71	35.2	29.30	

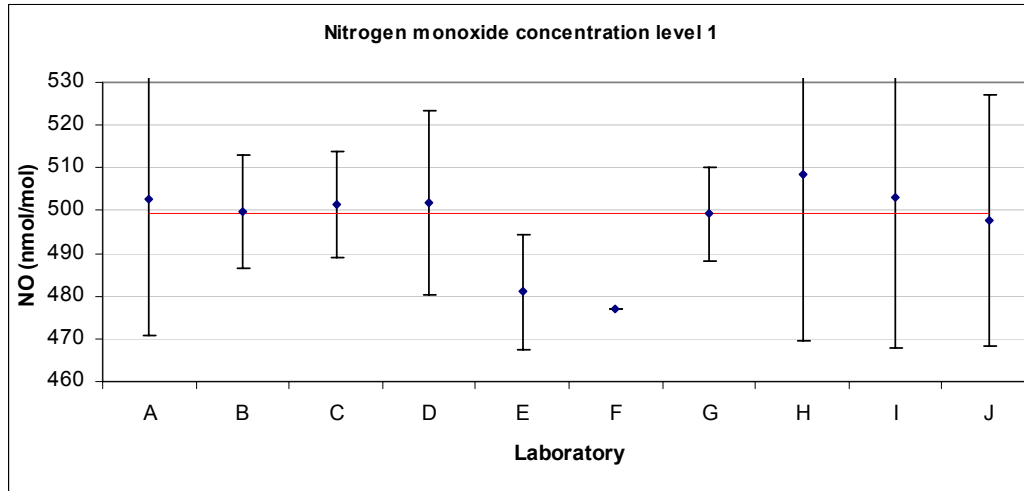


Figure 32: Reported values for NO concentration level 1.

Table 27: Reported values for NO concentration level 2.

parameter: NO level: 2		all units are nmol/mol									
		x*: 378.23 s*: 3.79									
	A	B	C	D	E	F	G	H	I	J	
xi,1	381.10	380.49	377.33	379.65	359.90	361.5	376.16	381.02	382	375.70	
xi,2	381.50	381.05	377.72	379.42	359.20	362.4	376.45	380.97	383	376.20	
xi,3	381.60	381.62	378.17	380.46	361.00	362.5	376.92	381.43	381	376.20	
xi	381.400	381.053	377.740	379.843	360.033	362.13	376.510	381.140	382.0	376.033	
si	0.265	0.565	0.420	0.546	0.907	0.55	0.384	0.252	1.0	0.289	
u(xi)	13.20	6.98	4.85	8.16	5.26		4.12	14.61	13.4	10.87	
U(xi)	26.80	13.40	9.70	16.32	10.52		8.24	29.22	26.8	21.74	

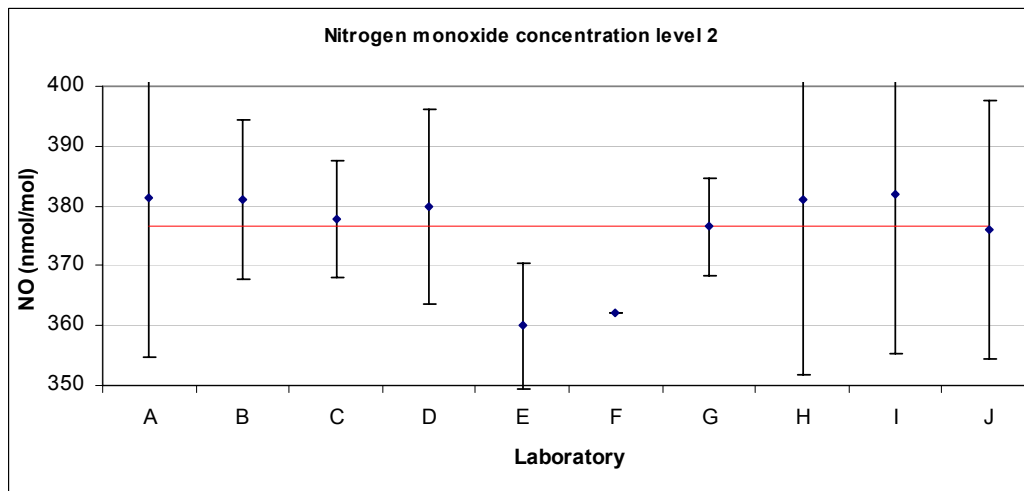


Figure 33: Reported values for NO concentration level 2.

Table 28: Reported values for NO concentration level 3.

parameter: NO level: 3		all units are nmol/mol									
		x*: 251.13 s*: 1.95									
	A	B	C	D	E	F	G	H	I	J	
xi,1	250.80	249.98	253.01	252.06	241.60	240.5	251.62	253.71	252	250.70	
xi,2	250.90	250.01	252.91	251.67	242.40	240.6	252.06	253.98	252	250.70	
xi,3	250.90	250.10	253.33	250.52	242.39	240.6	252.30	254.15	253	250.70	
xi	250.867	250.030	253.083	251.417	242.130	240.57	251.993	253.947	252.3	250.700	
si	0.058	0.062	0.219	0.801	0.459	0.06	0.345	0.222	0.6	0.000	
u(xi)	8.40	6.97	3.12	5.56	3.36		2.80	9.56	8.8	7.19	
U(xi)	16.80	13.40	6.24	11.11	6.72		5.59	19.12	17.6	14.38	

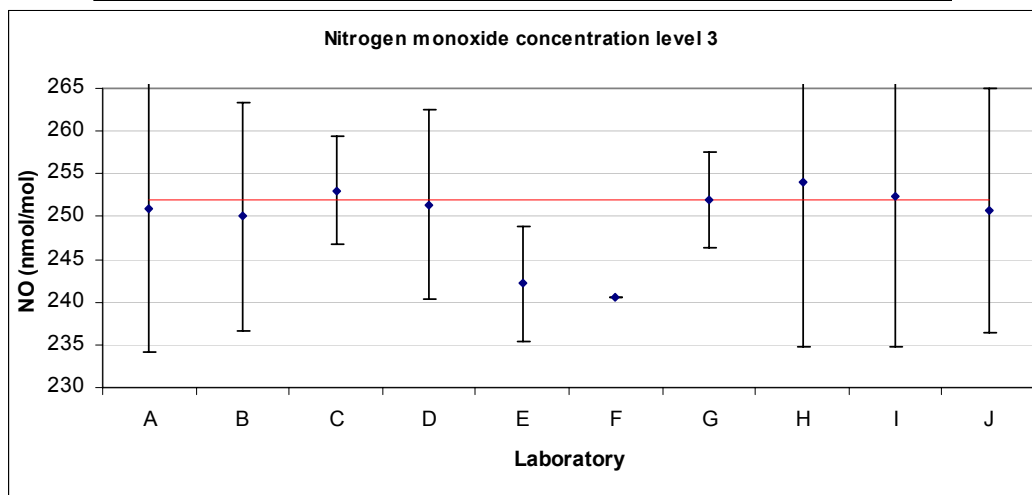


Figure 34: Reported values for NO concentration level 3.

Table 29: Reported values for NO concentration level 4.

parameter: NO level: 4		all units are nmol/mol									
		x*: 146.93 s*: 0.54									
	A	B	C	D	E	F	G	H	I	J	
xi,1	146.60	148.03	146.93	146.51	141.46	141.8	146.78	146.93	148	146.40	
xi,2	146.80	148.10	147.16	146.44	140.20	142.5	147.15	147.31	148	146.80	
xi,3	146.90	148.25	147.20	147.01	142.40	142.5	147.31	147.51	149	147.00	
xi	146.767	148.127	147.097	146.653	141.353	142.27	147.080	147.250	148.3	146.733	
si	0.153	0.112	0.146	0.311	1.104	0.40	0.272	0.295	0.6	0.306	
u(xi)	4.90	6.97	1.92	3.98	1.99		1.68	5.60	8.1	4.20	
U(xi)	9.80	13.40	3.84	7.75	3.98		3.36	11.19	16.1	8.41	

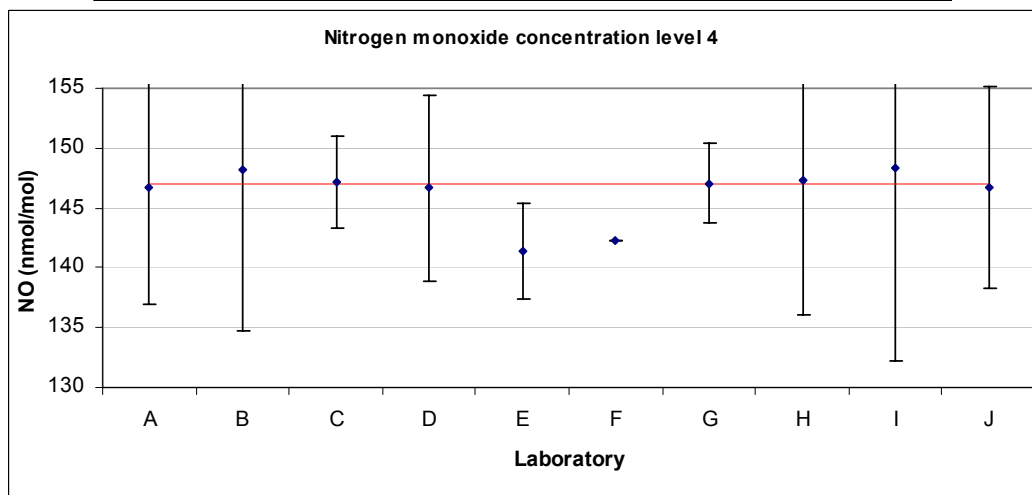


Figure 35: Reported values for NO concentration level 4.

Table 30: Reported values for NO concentration level 5.

parameter: NO		all units are nmol/mol									
level: 5		x*: 149.44 s*: 1.70									
	A	B	C	D	E	F	G	H	I	J	
xi,1	151.20	148.50	150.86	148.90	144.50	143.6	150.63	150.63	150	149.30	
xi,2	151.30	148.30	150.96	148.98	144.70	143.6	150.68	150.63	150	149.40	
xi,3	151.00	148.50	151.09	148.36	144.40	143.5	150.69	150.73	150	149.40	
xi	151.167	148.433	150.970	148.747	144.533	143.57	150.667	150.663	150.0	149.367	
si	0.153	0.115	0.115	0.337	0.153	0.06	0.032	0.058	0.0	0.058	
u(xi)	4.90	6.97	1.88	4.01	2.00		1.72	5.74	5.3	4.26	
U(xi)	9.80	13.40	3.80	8.02	4.00		3.44	11.48	10.5	8.52	

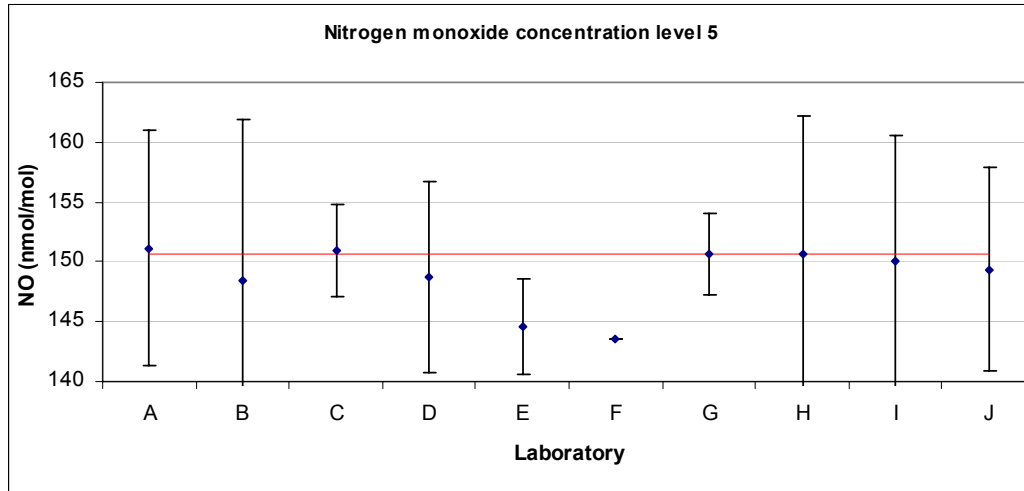


Figure 36: Reported values for NO concentration level 5.

Table 31: Reported values for NO concentration level 6.

parameter: NO		all units are nmol/mol									
level: 6		x*: 88.58 s*: 0.51									
	A	B	C	D	E	F	G	H	I	J	
xi,1	90.50	88.42	89.00	88.74	85.10	85.6	89.08	88.82	89	88.40	
xi,2	90.30	88.30	88.80	88.47	84.31	85.5	88.90	88.65	89	88.30	
xi,3	90.30	88.27	88.77	88.51	85.60	85.4	88.75	88.48	89	88.20	
xi	90.367	88.330	88.857	88.573	85.003	85.50	88.910	88.650	89.0	88.300	
si	0.115	0.079	0.125	0.146	0.650	0.10	0.165	0.170	0.0	0.100	
u(xi)	3.30	6.97	1.16	3.56	1.27		1.07	3.47	3.1	2.52	
U(xi)	6.60	13.40	2.32	7.13	2.54		2.14	6.94	6.2	5.04	

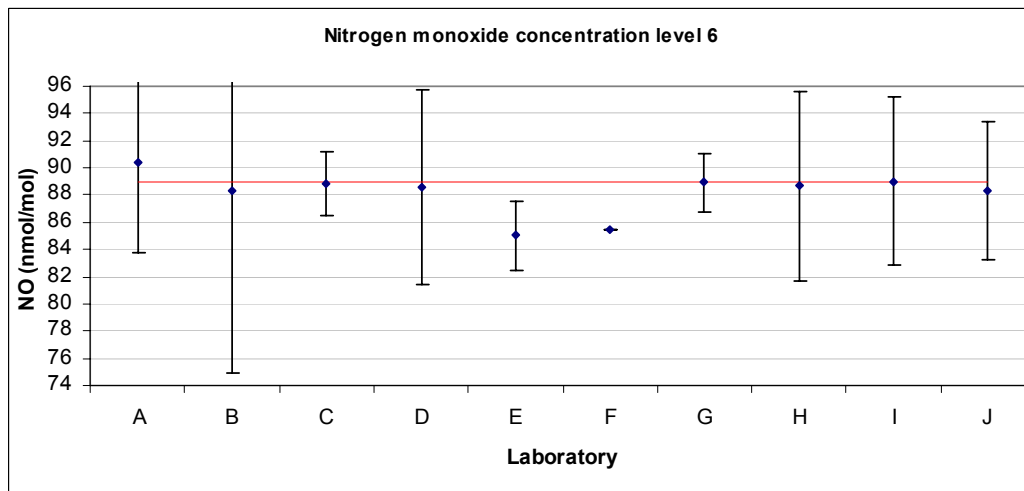


Figure 37: Reported values for NO concentration level 6.

Table 32: Reported values for NO concentration level 7.

parameter: NO level: 7		all units are nmol/mol									
		x*: 50.16					s*: 0.71				
	A	B	C	D	E	F	G	H	I	J	
xi,1	50.20	49.70	50.53	49.43	49.10	48.3	50.97	50.54	51	50.20	
xi,2	50.30	49.93	50.49	50.05	48.95	48.3	51.03	50.75	50	50.30	
xi,3	50.30	50.01	50.72	49.73	49.10	48.2	51.06	50.88	51	50.20	
xi	50.267	49.880	50.580	49.737	49.050	48.27	51.020	50.723	50.7	50.233	
si	0.058	0.161	0.123	0.310	0.087	0.06	0.046	0.172	0.6	0.058	
u(xi)	1.79	6.97	0.63	3.57	0.72		0.70	1.92	1.8	1.43	
U(xi)	3.58	13.40	1.30	7.13	1.44		1.39	3.83	3.6	2.86	

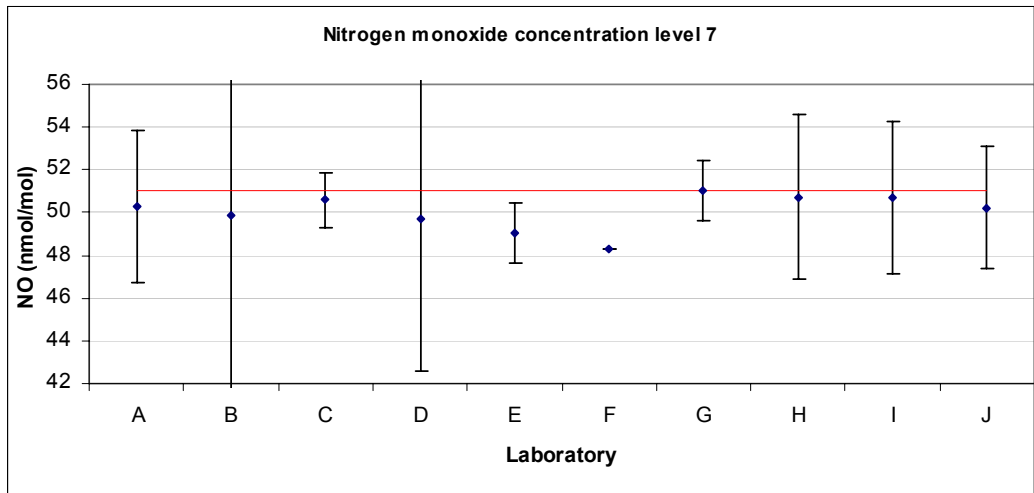


Figure 38: Reported values for NO concentration level 7.

Table 33: Reported values for NO concentration level 8.

parameter: NO level: 8		all units are nmol/mol									
		x*: 28.68					s*: 0.51				
	A	B	C	D	E	F	G	H	I	J	
xi,1	29.20	28.66	28.89	28.37	28.13	27.7	29.19	29.38	29	28.60	
xi,2	29.20	28.61	28.88	28.72	27.82	27.6	29.11	29.22	29	28.50	
xi,3	29.10	28.55	28.58	28.45	28.20	27.6	29.06	28.85	29	28.40	
xi	29.167	28.607	28.783	28.513	28.050	27.63	29.120	29.150	29.0	28.500	
si	0.058	0.055	0.176	0.183	0.202	0.06	0.066	0.272	0.0	0.100	
u(xi)	1.20	6.98	0.40	3.66	0.98		0.49	1.11	1.0	0.84	
U(xi)	2.40	13.40	0.80	7.32	1.96		0.98	2.22	2.0	1.68	

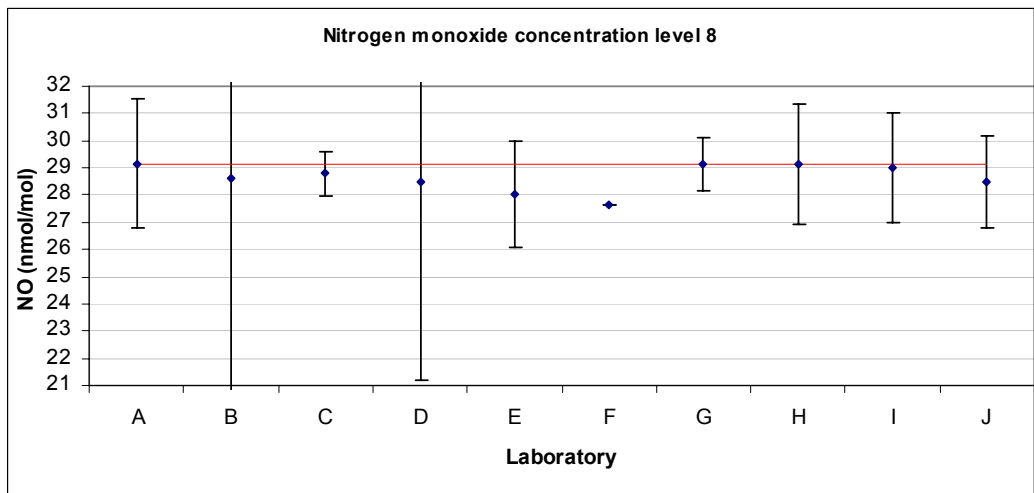


Figure 39: Reported values for NO concentration level 8.

Table 34: Reported values for NO concentration level 9.

parameter: NO		all units are nmol/mol									
level: 9		x*: 15.81					s*: 0.32				
	A	B	C	D	E	F	G	H	I	J	
xi,1	15.70	15.61	16.04	15.51	15.49	15.1	16.14	16.49	16	15.60	
xi,2	15.80	15.47	16.03	15.85	15.58	15.1	16.15	16.69	16	15.70	
xi,3	15.80	15.63	15.92	15.99	15.80	15.1	16.14	16.84	16	15.70	
xi	15.767	15.570	15.997	15.783	15.623	15.10	16.143	16.673	16.0	15.667	
si	0.058	0.087	0.067	0.247	0.159	0.00	0.006	0.176	0.0	0.058	
u(xi)	0.55	6.97	0.30	3.75	0.70		0.39	0.77	0.6	0.46	
U(xi)	1.10	13.40	0.60	7.50	1.40		0.78	1.54	1.2	0.92	

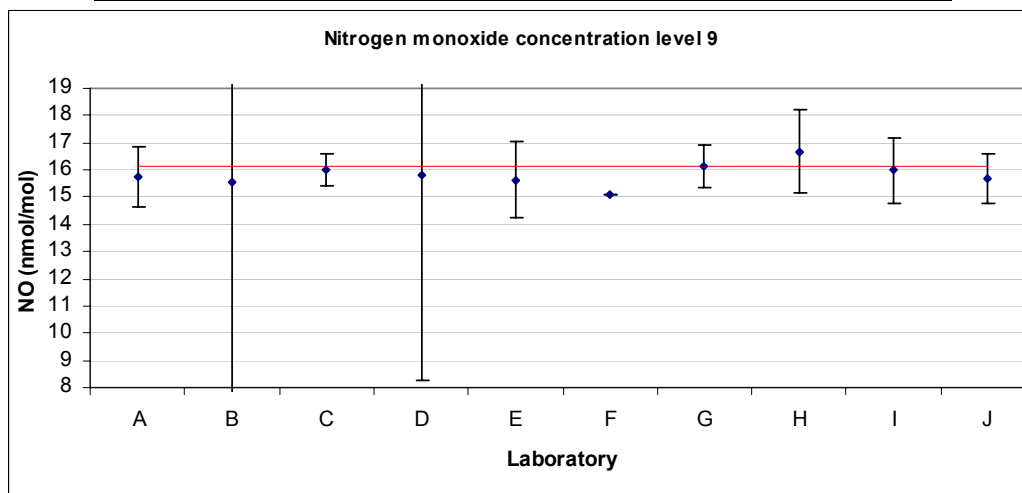


Figure 40: Reported values for NO concentration level 9.

Table 35: Reported values for NO concentration level 10.

parameter: NO		all units are nmol/mol									
level: 10		x*: 2.08					s*: 0.18				
	A	B	C	D	E	F	G	H	I	J	
xi,1	1.90	1.87	2.03	2.40	2.52	2.0	2.23	3.13	2	1.90	
xi,2	1.90	1.98	2.07	2.48	2.42	2.0	2.20	3.05	2	2.00	
xi,3	2.00	1.83	2.05	2.11	2.80	1.9	2.17	2.82	2	1.90	
xi	1.933	1.893	2.050	2.330	2.580	1.97	2.200	3.000	2.0	1.933	
si	0.058	0.078	0.020	0.195	0.197	0.06	0.030	0.161	0.0	0.058	
u(xi)	0.04	6.97	0.30	3.86	1.18		0.33	0.74	0.6	0.05	
U(xi)	0.08	13.40	0.60	7.72	2.36		0.65	1.47	1.2	0.10	

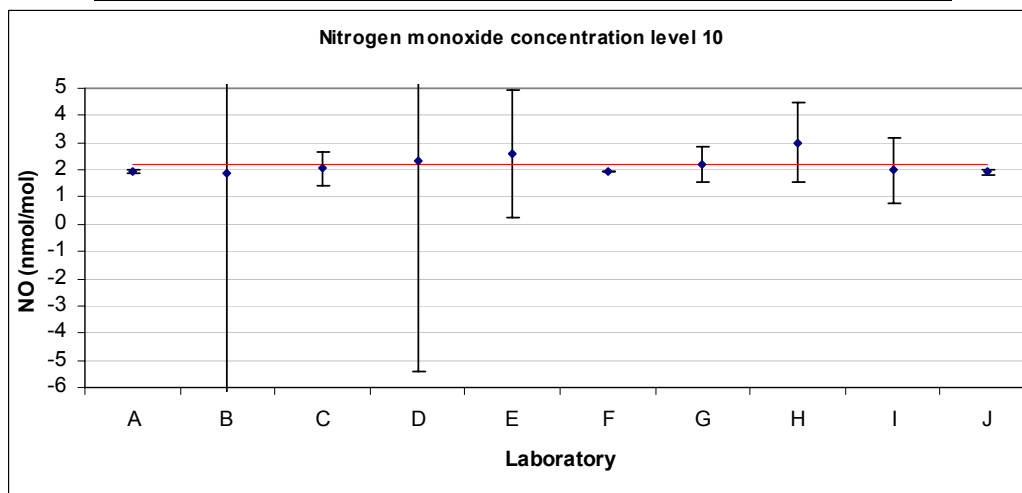


Figure 41: Reported values for NO concentration level 10.

Reported values for NO₂

Table 36: Reported values for NO₂ concentration level 0.

parameter: NO2		all units are nmol/mol									
level: 0		x*: 0.03		s*: 0.09							
	A	B	C	D	E	F	G	H	I	J	
xi,1	0.10	0.20	0.00	-1.98	0.57	-0.1	-0.05	0.06	0	0.00	
u(xi)	0.01	6.97	0.60	4.15	0.75		0.10	1.00	0.9	0.00	
U(xi)	0.02	13.40	1.20	8.30	1.50		0.20	2.00	1.8	0.00	

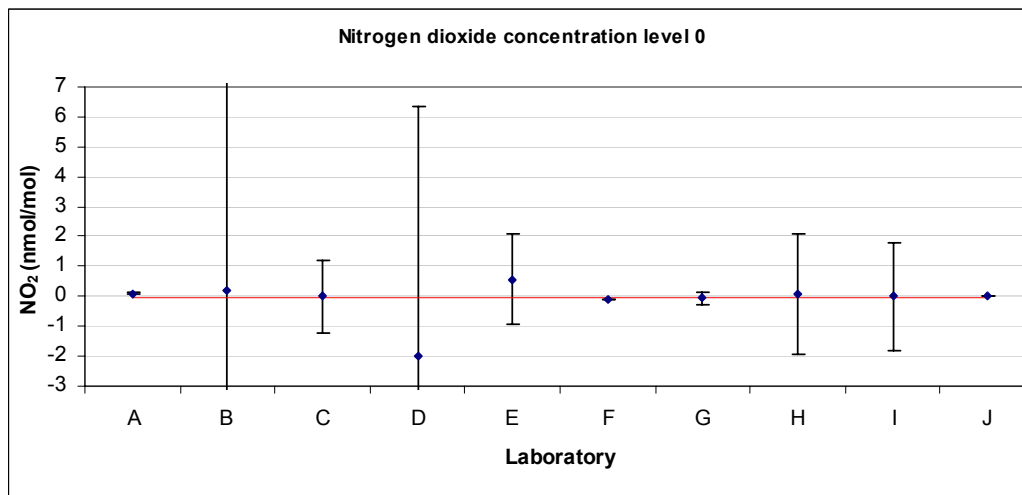


Figure 42: Reported values for NO₂ concentration level 0.

Table 37: Reported values for NO₂ concentration level 1.

parameter: NO2		all units are nmol/mol									
level: 1		x*: 2.12		s*: 1.62							
	A	B	C	D	E	F	G	H	I	J	
xi,1	1.10	0.20	2.10	7.30	6.39	3.5	2.46	1.11	1	4.90	
xi,2	1.50	0.12	2.08	6.73	6.60	2.0	2.31	1.08	1	5.10	
xi,3	1.20	0.08	2.10	5.91	6.80	1.9	2.54	1.17	1	5.40	
xi	1.267	0.133	2.093	6.647	6.597	2.47	2.437	1.120	1.0	5.133	
si	0.208	0.061	0.012	0.699	0.205	0.90	0.117	0.046	0.0	0.252	
u(xi)	0.03	6.97	0.60	15.10	0.38		0.89	1.00	0.6	0.15	
U(xi)	0.06	13.40	1.20	30.20	0.76		1.78	2.00	1.2	0.30	

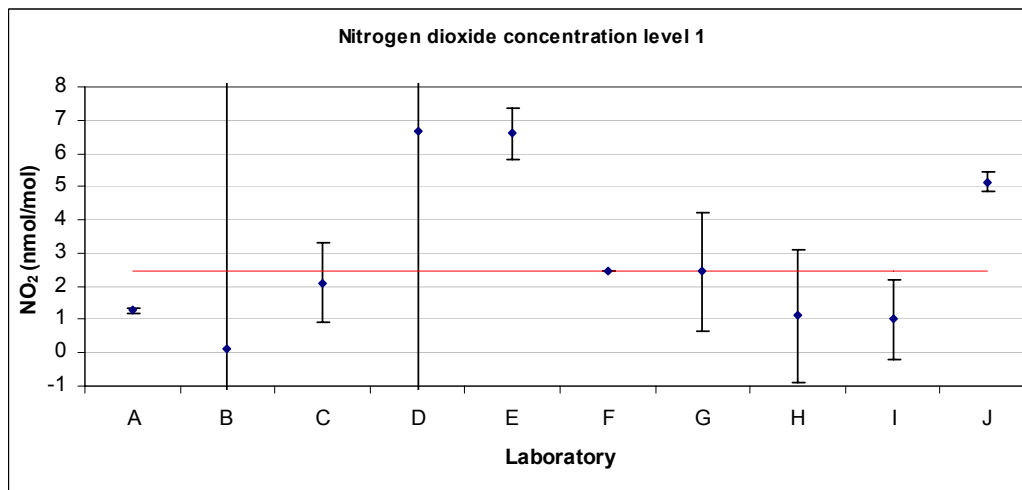


Figure 43: Reported values for NO₂ concentration level 1.

Table 38: Reported values for NO₂ concentration level 2.

parameter: NO2		all units are nmol/mol									
level: 2		x*: 121.94					s*: 3.63				
	A	B	C	D	E	F	G	H	I	J	
xi,1	120.80	118.85	121.88	128.87	120.40	117.1	125.40	131.02	124	125.20	
xi,2	121.10	119.21	121.52	129.11	120.14	114.9	125.14	130.50	122	124.90	
xi,3	120.90	119.45	121.05	128.36	120.60	117.2	124.66	130.22	121	124.80	
xi	120.933	119.170	121.483	128.780	120.380	116.40	125.067	130.580	122.3	124.967	
si	0.153	0.302	0.416	0.383	0.231	1.30	0.375	0.406	1.5	0.208	
u(xi)	3.50	6.97	2.40	13.38	1.62		1.71	5.20	6.4	3.61	
U(xi)	7.00	13.40	4.80	26.76	3.24		3.42	10.39	12.8	7.22	

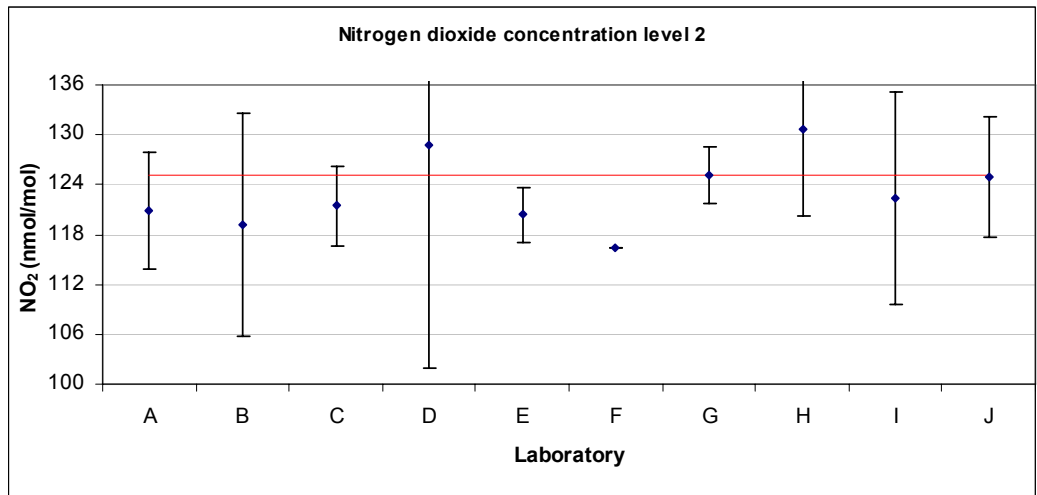


Figure 44: Reported values for NO₂ concentration level 2.

Table 39: Reported values for NO₂ concentration level 3.

parameter: NO2		all units are nmol/mol									
level: 3		x*: 0.87					s*: 0.84				
	A	B	C	D	E	F	G	H	I	J	
xi,1	0.80	-0.10	0.94	1.53	3.30	0.7	1.20	0.49	0	2.00	
xi,2	0.90	-0.21	0.99	2.06	3.20	1.0	1.05	0.47	0	2.10	
xi,3	0.50	-0.25	0.74	2.45	3.50	1.4	0.87	0.29	0	2.20	
xi	0.733	-0.187	0.890	2.013	3.333	1.03	1.040	0.417	0.0	2.100	
si	0.208	0.078	0.132	0.462	0.153	0.35	0.165	0.110	0.0	0.100	
u(xi)	0.02	6.97	0.60	7.69	0.38		0.63	1.00	0.9	0.07	
U(xi)	0.04	13.40	1.20	15.39	0.76		1.26	2.00	1.8	0.14	

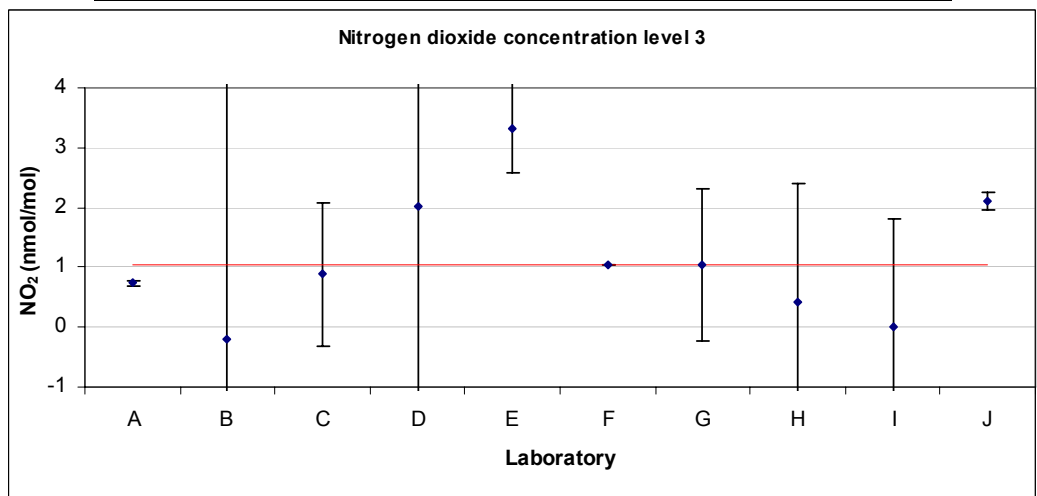


Figure 45: Reported values for NO₂ concentration level 3.

Table 40: Reported values for NO₂ concentration level 4.

parameter: NO2 level: 4		all units are nmol/mol									
		x*: 103.14 s*: 2.92									
	A	B	C	D	E	F	G	H	I	J	
xi,1	104.70	101.55	103.13	105.37	100.60	98.9	106.24	110.15	104	104.50	
xi,2	104.80	101.50	102.80	105.44	99.20	97.9	105.86	109.60	103	104.20	
xi,3	104.60	101.43	102.49	104.74	100.20	97.9	105.66	109.45	102	104.20	
xi	104.700	101.493	102.807	105.183	100.000	98.23	105.920	109.733	103.0	104.300	
si	0.100	0.060	0.320	0.386	0.721	0.58	0.295	0.369	1.0	0.173	
u(xi)	3.20	6.97	1.99	6.62	1.37		1.39	4.48	3.6	2.99	
U(xi)	6.40	13.40	3.98	13.23	2.74		2.78	8.95	7.2	5.98	

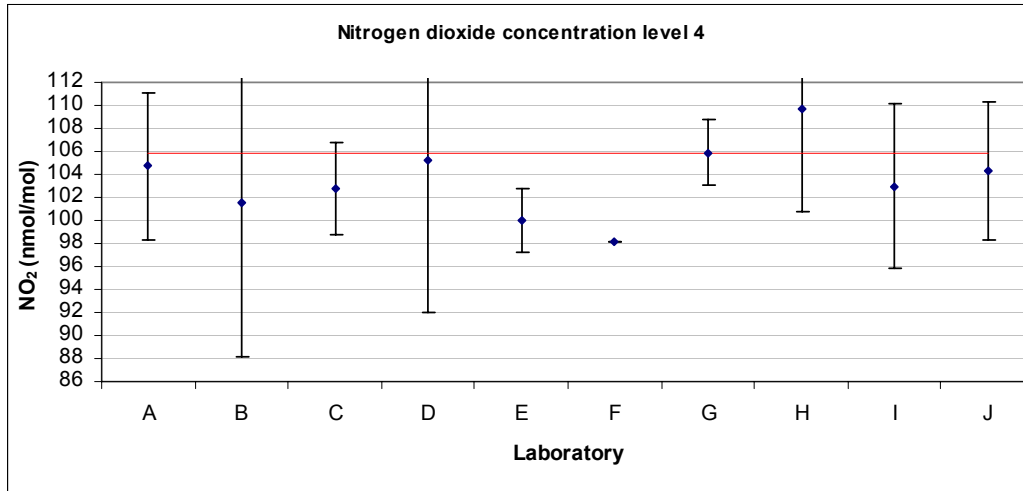


Figure 46: Reported values for NO₂ concentration level 4.

Table 41: Reported values for NO₂ concentration level 5.

parameter: NO2 level: 5		all units are nmol/mol									
		x*: 0.32 s*: 0.45									
	A	B	C	D	E	F	G	H	I	J	
xi,1	0.80	-0.25	0.19	-0.54	1.59	0.5	0.35	0.07	0	0.40	
xi,2	1.00	-0.21	0.12	-0.33	1.62	0.0	0.25	0.08	0	0.40	
xi,3	0.70	-0.24	-0.01	-0.01	1.75	0.9	0.31	-0.13	0	0.40	
xi	0.833	-0.233	0.100	-0.293	1.653	0.47	0.303	0.007	0.0	0.400	
si	0.153	0.021	0.101	0.267	0.085	0.45	0.050	0.118	0.0	0.000	
u(xi)	0.025	6.97	0.60	5.16	0.85		0.46	1.00	0.9	0.07	
U(xi)	0.05	13.40	1.20	10.32	1.70		0.92	2.00	1.8	0.14	

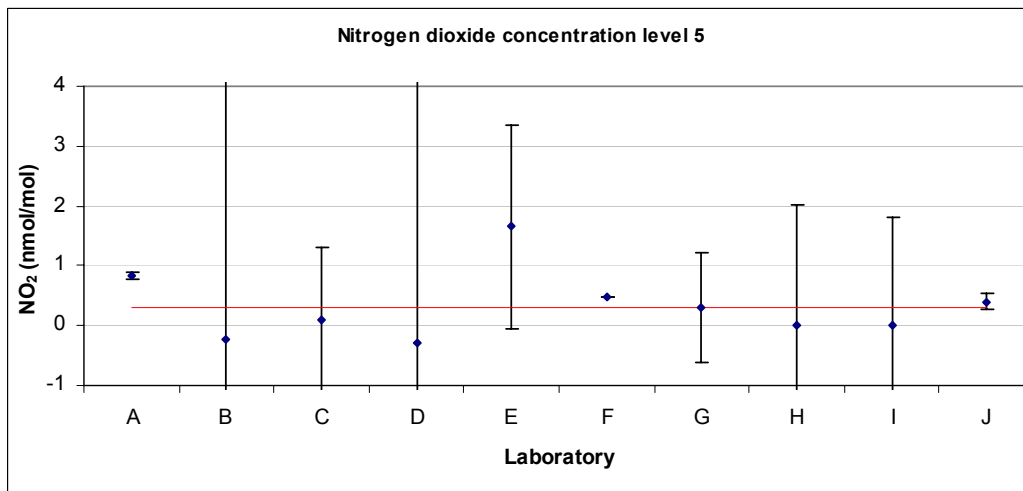


Figure 47: Reported values for NO₂ concentration level 5.

Table 42: Reported values for NO₂ concentration level 6.

parameter: NO2 level: 6		all units are nmol/mol									
		x*: 59.98					s*: 1.59				
	A	B	C	D	E	F	G	H	I	J	
xi,1	60.80	59.30	59.81	60.19	57.60	58.2	61.62	63.33	59	59.80	
xi,2	61.00	59.47	59.98	59.79	56.62	58.1	61.93	63.43	60	60.00	
xi,3	60.70	59.48	60.05	59.29	58.10	58.2	62.00	63.56	60	60.20	
xi	60.833	59.417	59.947	59.757	57.440	58.17	61.850	63.440	59.7	60.000	
si	0.153	0.101	0.123	0.451	0.753	0.06	0.202	0.115	0.6	0.200	
u(xi)	2.10	6.97	1.40	4.81	0.81		0.86	2.57	3.2	1.71	
U(xi)	4.20	13.40	2.80	9.61	1.62		1.72	5.14	6.3	3.42	

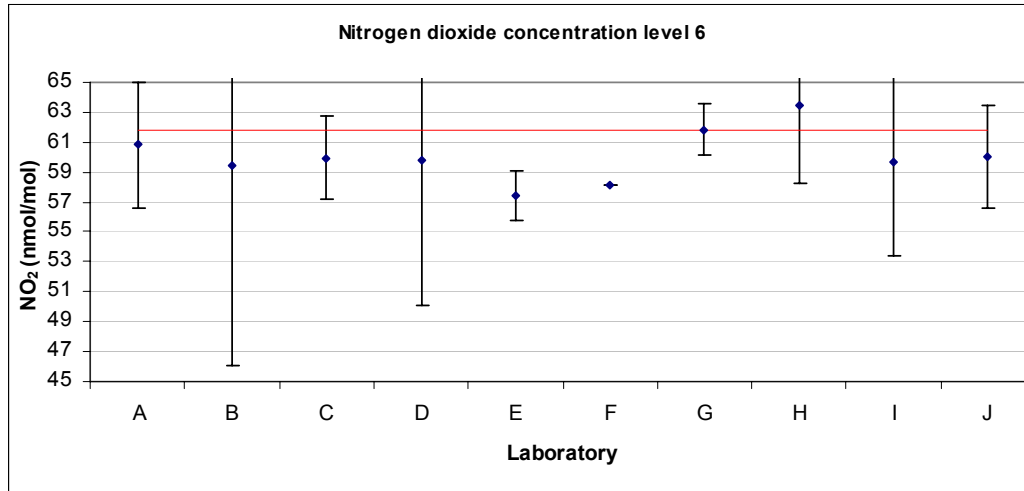


Figure 48: Reported values for NO₂ concentration level 6.

Table 43: Reported values for NO₂ concentration level 7.

parameter: NO2 level: 7		all units are nmol/mol									
		x*: 0.10					s*: 0.14				
	A	B	C	D	E	F	G	H	I	J	
xi,1	0.30	0.32	-0.05	-1.24	0.67	0.1	0.22	0.09	0	0.00	
xi,2	0.20	0.12	-0.04	-1.61	1.00	0.2	0.10	-0.07	0	0.00	
xi,3	0.20	-0.05	-0.04	-1.34	1.00	0.2	0.07	-0.01	0	0.00	
xi	0.233	0.130	-0.043	-1.397	0.890	0.17	0.130	0.003	0.0	0.000	
si	0.058	0.185	0.006	0.191	0.191	0.06	0.079	0.081	0.0	0.000	
u(xi)	0.012	6.97	0.60	3.92	0.85		0.29	1.00	0.9	0.00	
U(xi)	0.024	13.40	1.20	7.83	1.70		0.58	2.00	1.8	0.00	

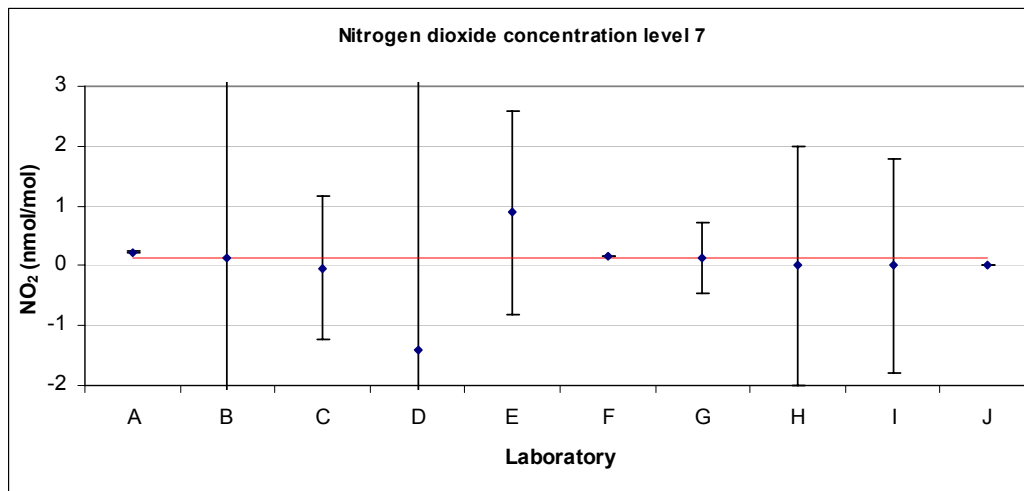


Figure 49: Reported values for NO₂ concentration level 7.

Table 44: Reported values for NO₂ concentration level 8.

parameter: NO2 level: 8		all units are nmol/mol									
		x*: 21.08					s*: 0.82				
	A	B	C	D	E	F	G	H	I	J	
xi,1	21.00	21.35	21.00	19.41	20.39	20.6	21.95	22.20	21	20.10	
xi,2	21.10	21.40	21.00	19.55	19.89	20.4	22.03	22.23	21	20.20	
xi,3	21.00	21.46	21.01	19.64	20.68	20.3	22.11	22.36	21	20.40	
xi	21.033	21.403	21.003	19.533	20.320	20.43	22.030	22.263	21.0	20.233	
si	0.058	0.055	0.006	0.116	0.400	0.15	0.080	0.085	0.0	0.153	
u(xi)	0.90	6.98	0.60	3.99	0.45		0.36	0.94	1.1	0.60	
U(xi)	1.80	13.40	1.20	7.99	0.90		0.72	1.87	2.2	1.20	

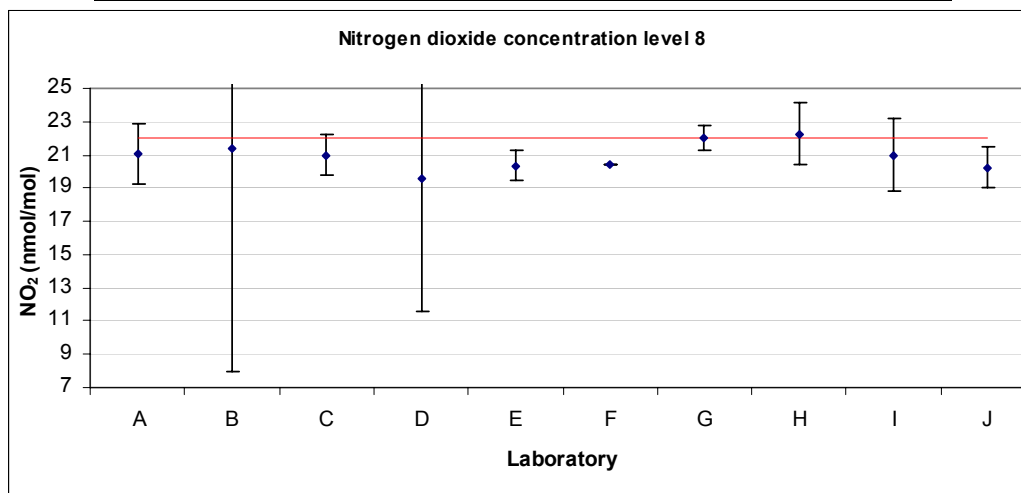


Figure 50: Reported values for NO₂ concentration level 8.

Table 45: Reported values for NO₂ concentration level 9.

parameter: NO2 level: 9		all units are nmol/mol									
		x*: 0.05					s*: 0.07				
	A	B	C	D	E	F	G	H	I	J	
xi,1	1.80	-0.02	0.00	-1.93	0.39	0.0	0.11	0.14	0	0.00	
xi,2	1.90	0.10	0.00	-2.03	0.38	0.0	0.02	0.05	0	0.00	
xi,3	1.90	-0.02	0.00	-2.32	0.40	-0.1	0.09	0.07	0	0.00	
xi	1.867	0.020	0.000	-2.093	0.390	-0.03	0.073	0.087	0.0	0.000	
si	0.058	0.069	0.000	0.203	0.010	0.06	0.047	0.047	0.0	0.000	
u(xi)	0.012	6.98	0.60	4.00	0.85		0.17	1.00	0.9	0.00	
U(xi)	0.024	13.40	1.20	8.01	1.70		0.34	2.00	1.8	0.00	

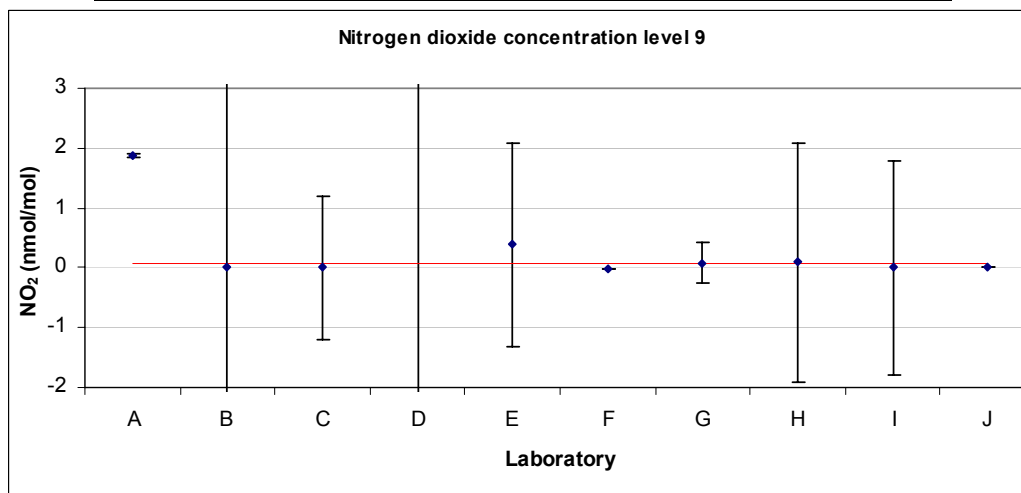


Figure 51: Reported values for NO₂ concentration level 9.

Table 46: Reported values for NO₂ concentration level 10.

parameter: NO2 level: 10		all units are nmol/mol									
		x*: 13.51					s*: 0.52				
	A	B	C	D	E	F	G	H	I	J	
xi,1	13.60	13.76	13.10	11.20	12.40	13.0	13.98	13.97	14	13.20	
xi,2	13.70	13.64	13.12	11.34	11.90	12.9	13.99	14.01	14	13.20	
xi,3	13.70	13.80	13.14	11.53	12.70	12.9	13.96	14.00	14	13.20	
xi	13.667	13.733	13.120	11.357	12.333	12.93	13.977	13.993	14.0	13.200	
si	0.058	0.083	0.020	0.166	0.404	0.06	0.015	0.021	0.0	0.000	
u(xi)	0.55	6.99	0.60	4.11	0.38		0.23	0.98	0.9	0.30	
U(xi)	1.10	13.40	1.20	8.21	0.76		0.46	1.96	1.8	0.60	

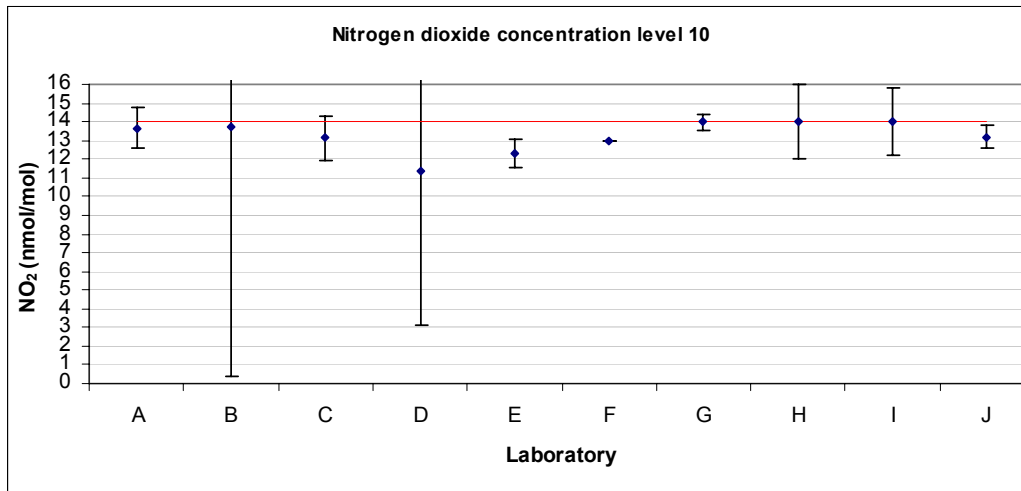


Figure 52: Reported values for NO₂ concentration level 10.

Annex C. Precision of standardized measurement methods

For the main purpose of monitoring trends between different IEs undertaken by ERLAP the precision of standardized SO₂, CO, O₃ and NO_x measurement methods [7], [8], [9] and [10] as implemented by NRLs was evaluated. Applied methodology is described in ISO 5725-1, -2 and -6 [19], [20] and [21]. The precision experiment has involved seven laboratories, for NO_x, O₃ and SO₂ measurement methods, and six laboratories, for CO measurement method. Six concentration levels were tested, for O₃, CO, SO₂ and NO₂, and eleven for NO. Data consistency and outlier tests have been performed (Annex D).

The repeatability standard deviation (s_r) was calculated in accordance with ISO 5725-2 as the square root of average within laboratory variance. The repeatability limit (r) is calculated using equation 8 [21]. It represents the biggest difference between two test results found on an identical test gas by one laboratory using the same apparatus within the shortest feasible time interval, that should not be exceeded on average more than once in 20 cases in the normal and correct operation of method.

$$r = t_{95\%,v} \cdot \sqrt{2} \cdot s_r \tag{8}$$

The reproducibility standard deviation (s_R) was calculated in accordance with ISO 5725-2 as the square root of sum of repeatability and between laboratory variance. The reproducibility limit (R) is calculated using equation 9 [21]. It represents the biggest difference between two measurements on an identical test gas reported by two laboratories, that should not occur on average more than once in 20 cases in the normal and correct operation of method.

$$R = t_{95\%,v} \cdot \sqrt{2} \cdot s_R \tag{9}$$

The number of degrees of freedom (v), which depend on the number of participating NRLs (p) and number of repetitions (n) after removal of outliers, with which the repeatability standard deviation and reproducibility standard deviation are evaluated and the relevant critical range student factors ($t_{\alpha,v}$) are given in Table 47.

Table 47: The degrees of freedom (v) and critical student factors ($t_{\alpha,v}$) of r and R evaluations.

parameter	run numbers	p	n	$t_{95\%,v=p \cdot (n-1)}$	$t_{95\%,v=p-1}$
CO	0	6	1		2.571
CO	1 to 5	6	3	2.179	2.571
NO	0	5	1		2.776
NO	1 to 10	5	3	2.228	2.776
NO ₂	0	6	1		2.571
NO ₂	1 to 10	7	3	2.145	2.447
O ₃	0	5	1		2.776
O ₃	1 to 5	5	3	2.228	2.776
SO ₂	0	7	1		2.447
SO ₂	1 to 3	7	3	2.145	2.447
SO ₂	4 to 5	5	3	2.228	2.776

The reproducibility and repeatability of NO₂ measurements are dependant on both NO and NO₂ concentrations. In Table 52 both concentrations are given and in Figure 57, R and r are plotted as functions of NO₂ concentration.

Table 52 and Figure 53-Figure 57 the repeatability and reproducibility limits of measurement methods are presented with (r, R) and without (r*, R*) outliers. Also presented is ‘reproducibility from common criteria (R(from σ_p))’ calculated by substituting s_R in equation 9 with a ‘standard deviation for proficiency assessment’ (Table 3). Comparison between R and R(from σ_p) serves to indicate that σ_p is realistic ([18] 6.3.1) or from the other point of view, that the general methodology implemented by NRLs is fit for σ_p.

Table 48: The R and r of CO standard measurement method.

CO data (µmol/mol)			
all data			
group average	repeatability limit : r	reproducibility limit : R	reproducibility limit (relative)
0.01		0.25	
0.95	0.01	0.43	
1.90	0.02	0.58	
4.15	0.01	0.77	
5.82	0.04	0.82	
8.35	0.08	0.92	11.0%

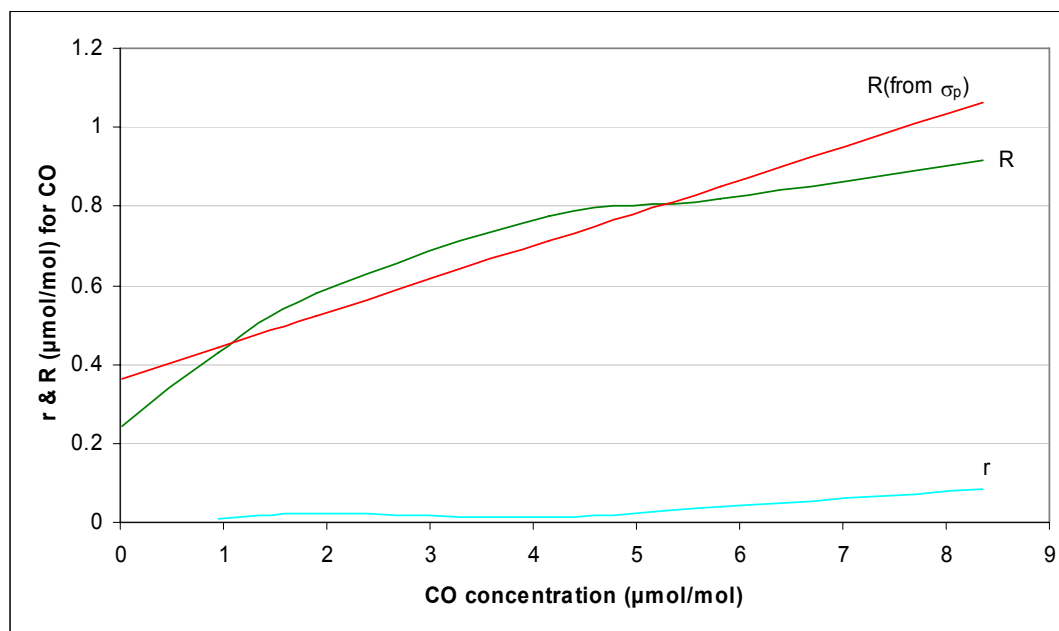


Figure 53: The R and r of CO standard measurement method as a function of concentration.

Table 49: The R and r of O₃ standard measurement method.

O ₃ data (nmol/mol)						
all data			without outliers			
group average	repeatability limit : r	reproducibility limit : R	group average	repeatability limit : r*	reproducibility limit : R*	reproducibility limit (relative)
0.3		1.8	0.3		2.3	
14.8	0.2	4.7	14.2	0.2	2.6	
22.6	0.3	6.8	21.7	0.3	2.6	
63.0	0.4	17.8	60.4	0.4	3.3	
107.4	1.1	29.7	103.1	0.9	4.5	
125.0	1.2	34.4	120.1	0.9	4.2	3.5%

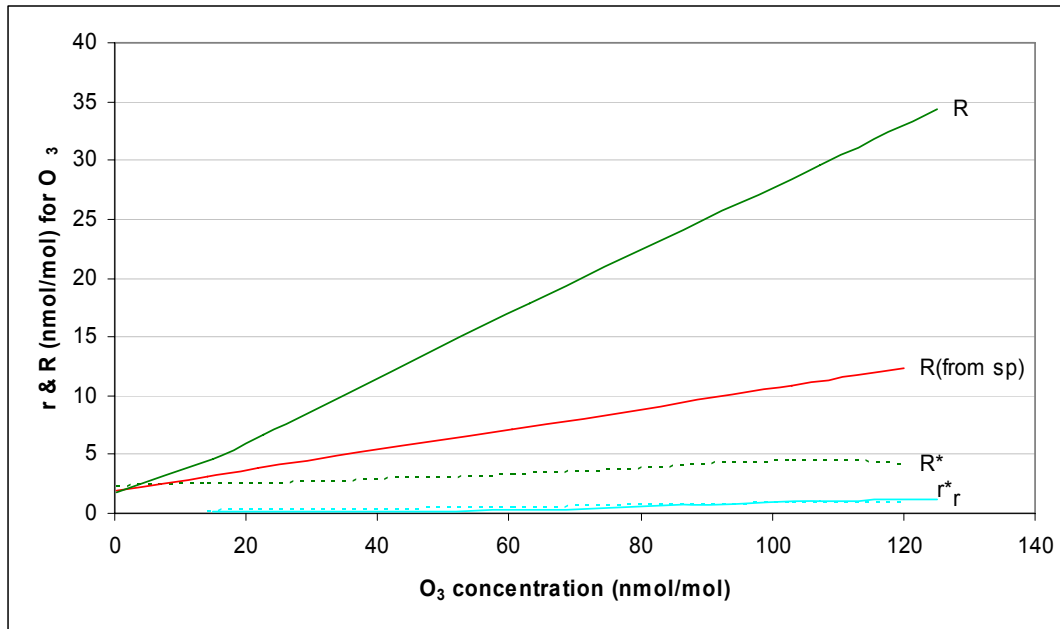


Figure 54: The R and r of O₃ standard measurement method as a function of concentration.

Table 50: The R and r of SO₂ standard measurement method.

SO ₂ data (nmol/mol)						
all data			without outliers			
group average	repeatability limit : r	reproducibility limit : R	group average	repeatability limit : r*	reproducibility limit : R*	reproducibility limit (relative)
0.3		0.8	0.3		0.8	
2.9	0.4	3.1	3.3	0.2	0.9	
7.3	0.3	2.4	7.6	0.4	0.9	
17.8	0.3	2.5	17.8	0.3	2.5	
46.3	0.7	4.0	46.3	0.7	4.0	
130.7	0.5	11.4	130.7	0.5	11.4	8.7%

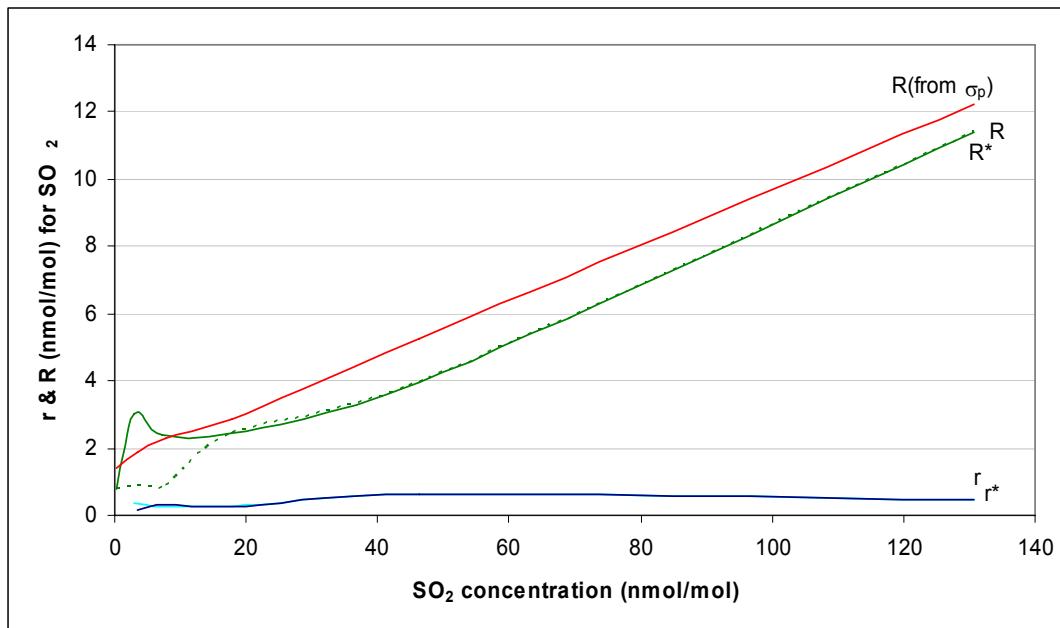


Figure 55: The R and r of SO₂ standard measurement method as a function of concentration.

Table 51: The R and r of NO standard measurement method.

NO data (nmol/mol)						
all data			without outliers			
group average	repeatability limit : r	reproducibility limit : R	group average	repeatability limit : r*	reproducibility limit : R*	reproducibility limit (relative)
0.2		0.6	0.2		0.6	
2.1	0.4	1.0	2.1	0.4	0.8	
15.7	0.4	1.3	15.9	0.4	1.0	
28.6	0.4	2.0	28.8	0.4	1.3	
49.8	0.5	3.3	50.3	0.6	2.2	
87.9	0.9	6.8	89.0	0.5	3.2	
145.6	1.5	9.3	147.1	0.7	2.4	
148.3	0.6	10.8	150.0	0.6	5.2	
248.6	1.2	17.6	251.5	1.3	4.8	
374.1	1.7	31.5	379.3	1.5	8.5	
494.7	1.6	37.6	501.0	1.5	6.2	1.2%

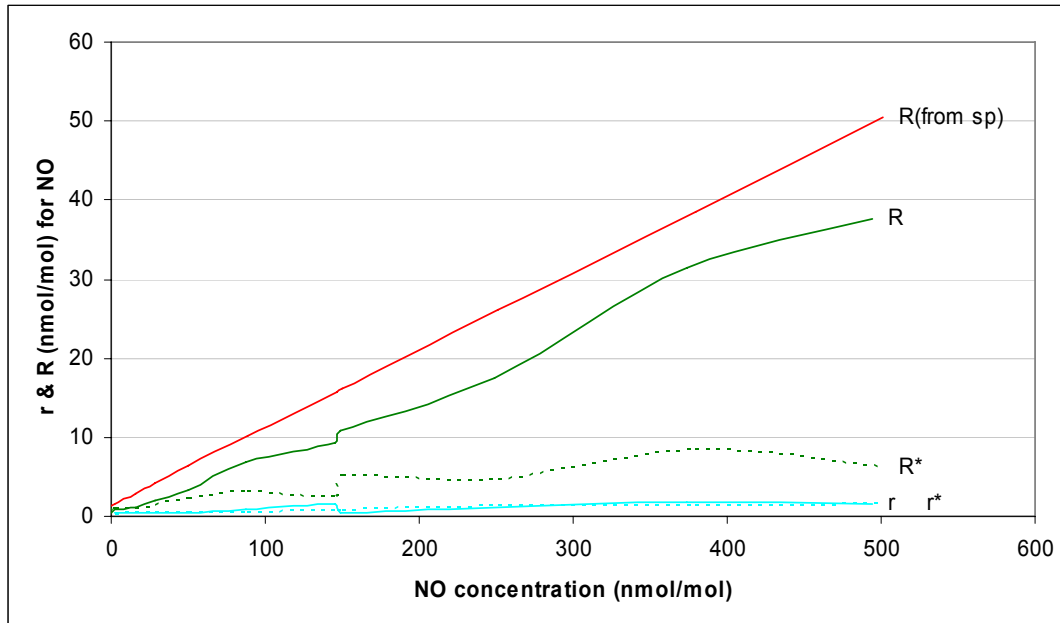


Figure 56: The R and r of NO standard measurement method as a function of concentration.

The reproducibility and repeatability of NO₂ measurements are dependant on both NO and NO₂ concentrations. In Table 52 both concentrations are given and in Figure 57, R and r are plotted as functions of NO₂ concentration.

Table 52: The R and r of NO₂ standard measurement method.

NO ₂ data (nmol/mol)								
all data				without outliers				
NO	NO ₂	NO ₂		NO	NO ₂	NO ₂		
group average	group average	repeatability limit : r	reproducibility limit : R	group average	group average	repeatability limit : r*	reproducibility limit : R*	reproducibility limit (relative)
0.2	-0.2		2.9	0.2	0.1		0.9	
2.1	13.0	0.6	3.3	2.1	13.0	0.6	3.3	
15.7	0.0	0.3	4.1	15.9	0.0	0.3	4.1	
28.6	20.8	0.6	2.9	28.8	20.8	0.6	2.9	
49.8	0.0	0.4	2.5	50.3	0.0	0.4	2.5	
87.9	59.6	1.1	5.3	89.0	59.6	1.1	5.3	
148.3	0.4	0.7	2.5	150.0	0.4	0.7	2.5	
145.6	102.6	1.3	10.0	147.1	102.6	1.3	10.0	
248.6	1.3	0.8	4.0	251.5	1.3	0.8	4.0	
374.1	121.7	1.8	14.2	379.3	121.7	1.8	14.2	11.7%
494.7	3.1	1.4	8.9	501.0	3.1	1.4	8.9	

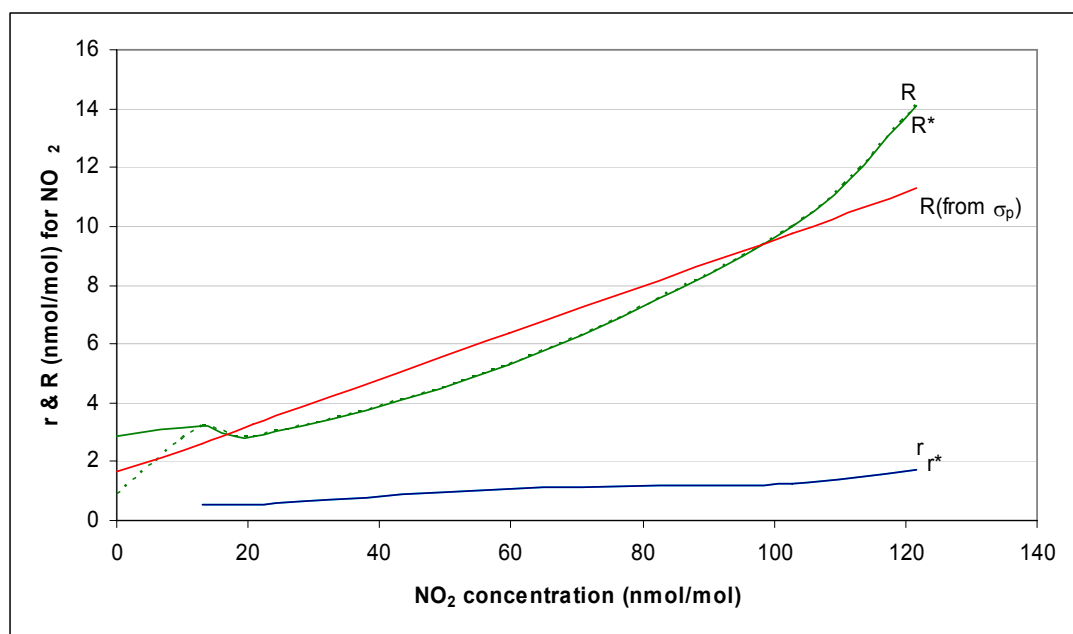


Figure 57: The R and r of NO₂ standard measurement method as a function of concentration.

Annex D. Scrutiny of results for consistency and outliers

The precision evaluation (Annex C) focuses on data that are as much as possible the reflection of every day work of NRLs and thus represents the comparability of participant’s standard operating procedures. For that reason a procedure for the detection of exceptional errors (error during typing, slip in performing the measurement or calculation, the bad averaging interval, malfunction of instrumentation, etc.) was applied. In this procedure the IE data first underwent the scrutiny for its consistency and the detection of statistical outliers as described in ISO 5725-2. Then the three laboratories showing some form of statistical inconsistency were contacted to try to ascertain the cause of discrepancies. Laboratories were allowed to correct their results. After that data was considered of appropriate quality and the final tests of statistical outliers were performed.

In this final test “Grubb’s one outlying observation test” was performed Figure 58 to Figure 62. For runs:

- a.) where outliers were detected outliers were removed and “Grubb’s one outlying observation test” was repeated. After this one repetition there were no more outliers in these runs.
- b.) where no outliers were detected the “Grubb’s two outlying observations test” was performed (Figure 63 to Figure 67).

Statistical outliers obtained at this stage are not considered as due to extraordinary errors but due to significant difference in participant’s standard operating procedure. These “genuine” statistical outliers are presented in table below:

Table 53: “Genuine” statistical outliers.

Parameter	Run	Participant	Failing test
O3	1, 2, 3	E, F	“Grubb’s two outlying observation test” Figure 65
SO2	4, 5	B, F	“Grubb’s two outlying observation test” (Figure 63)
NO	1, 2, 3, 4	E, F	“Grubb’s two outlying observation test” (Figure 66)
NO2	0	D	“Grubb’s one outlying observation test” (Figure 62)

Not to have unrealistic jumps in the evaluation of precision of standardized method all NO and O₃ results of participants E and F were removed from this evaluation.

Presented in the following figures are Grubb's one outlying observation test statistics for the minimum (blue) and maximum (orange with pattern) values of each run. Values between the two lines are considered strugglers and values over violet line are considered outliers.

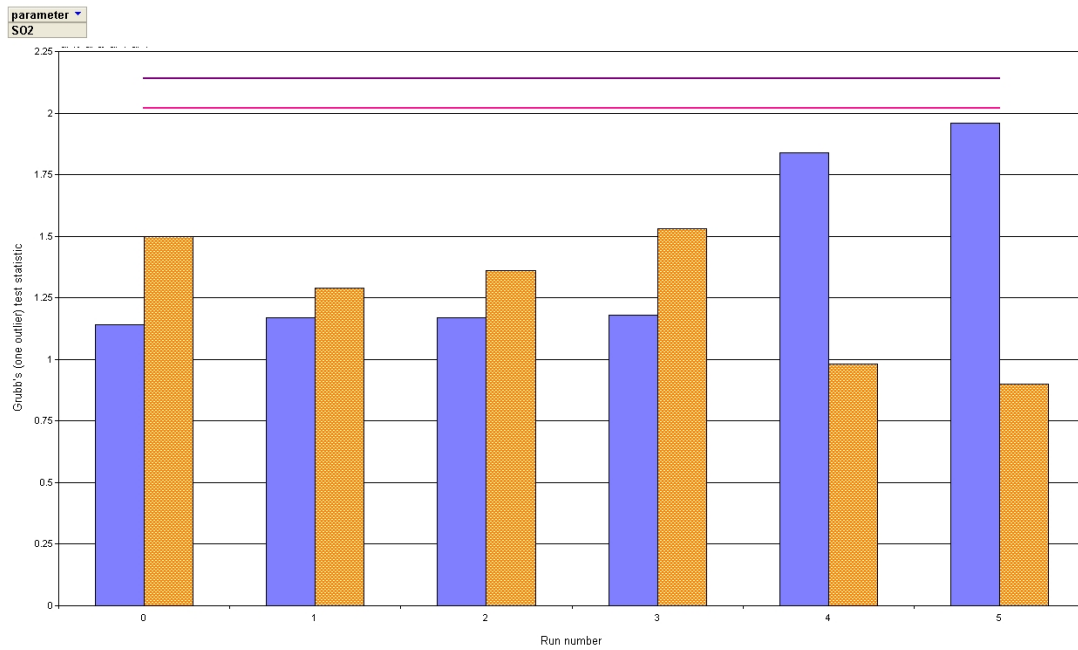


Figure 58: Grubb's one outlying observation test statistics for SO₂ runs.

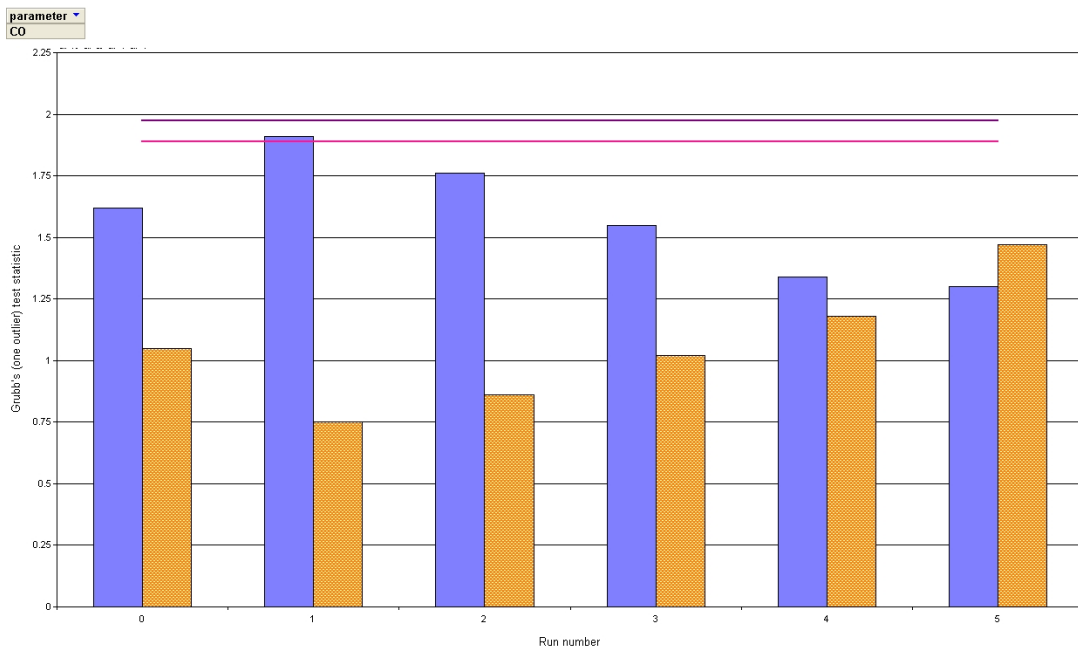


Figure 59: Grubb's one outlying observation test statistics for CO runs.

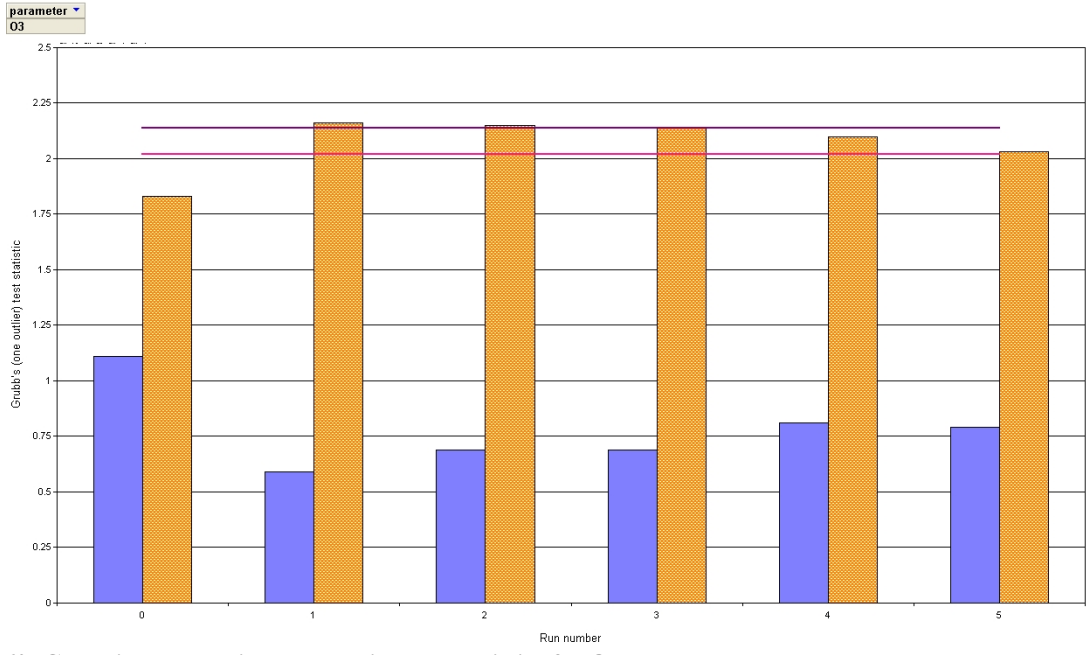


Figure 60: Grubb's one outlying observation test statistics for O₃ runs.

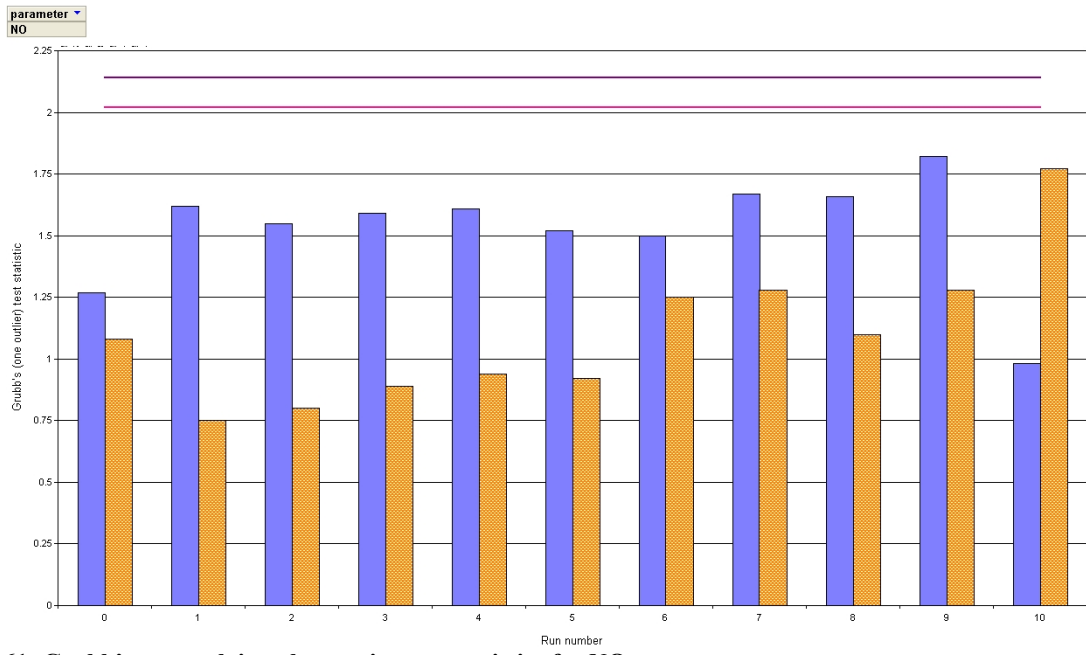


Figure 61: Grubb's one outlying observation test statistics for NO runs.

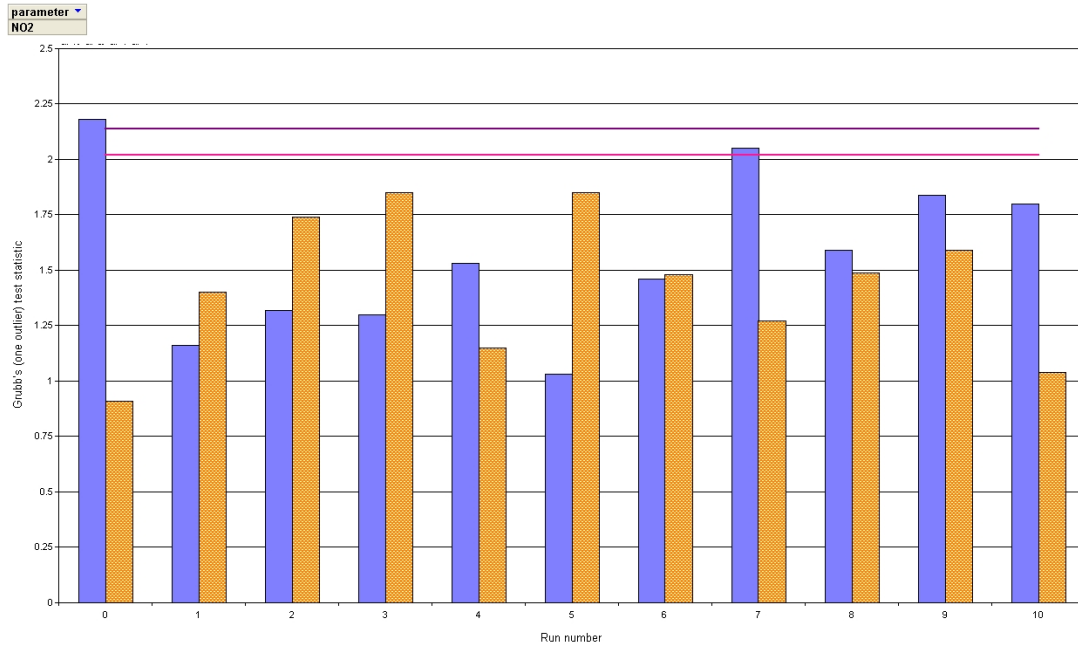


Figure 62: Grubb's one outlying observation test statistics for NO₂ runs.

Grubb's two outlying observations test statistics for the minimum (blue) and maximum (orange with pattern) values of all runs that passed "Grubb's one outlying observation" test. Values between the two lines are considered strugglers and values under red line are considered outliers.

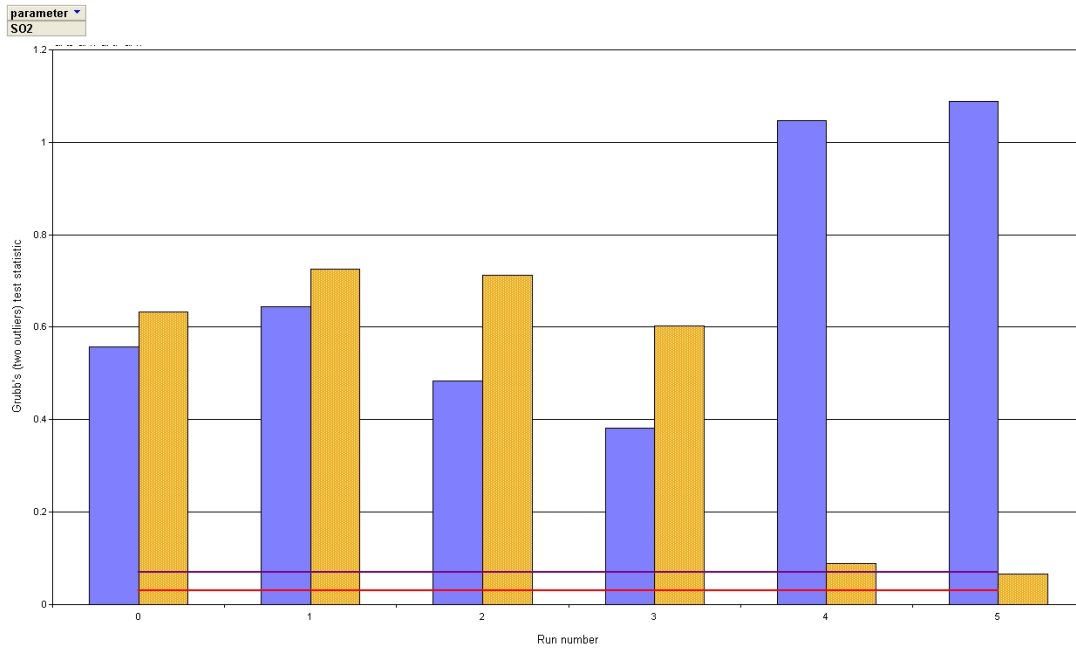


Figure 63: Grubb's two outlying observations test statistics for SO₂ runs

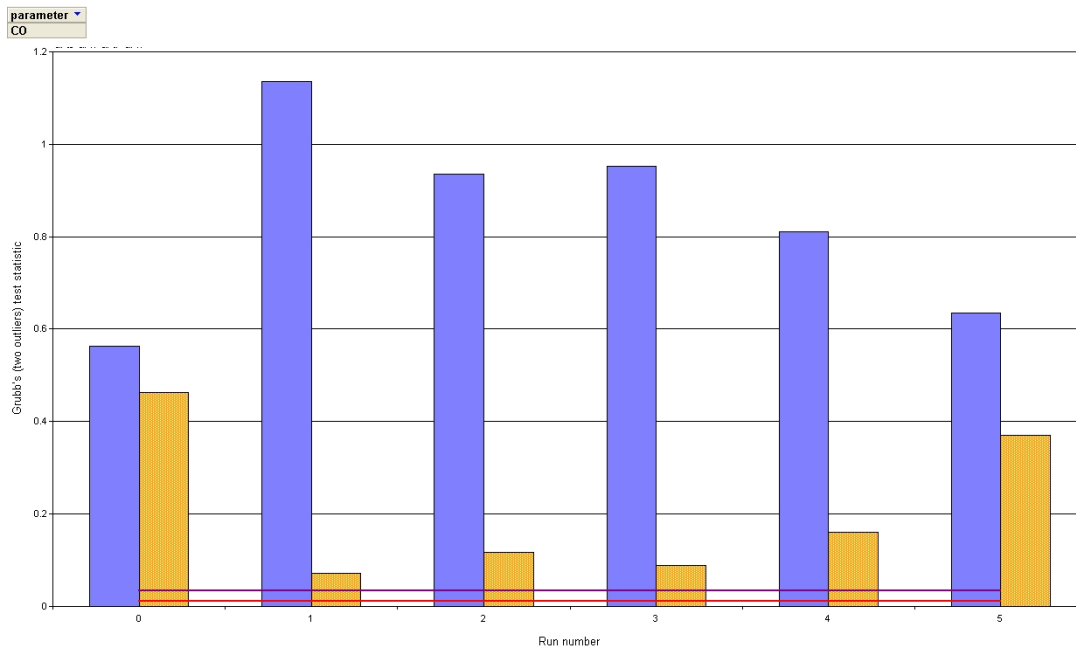


Figure 64: Grubb's two outlying observations test statistics for CO runs

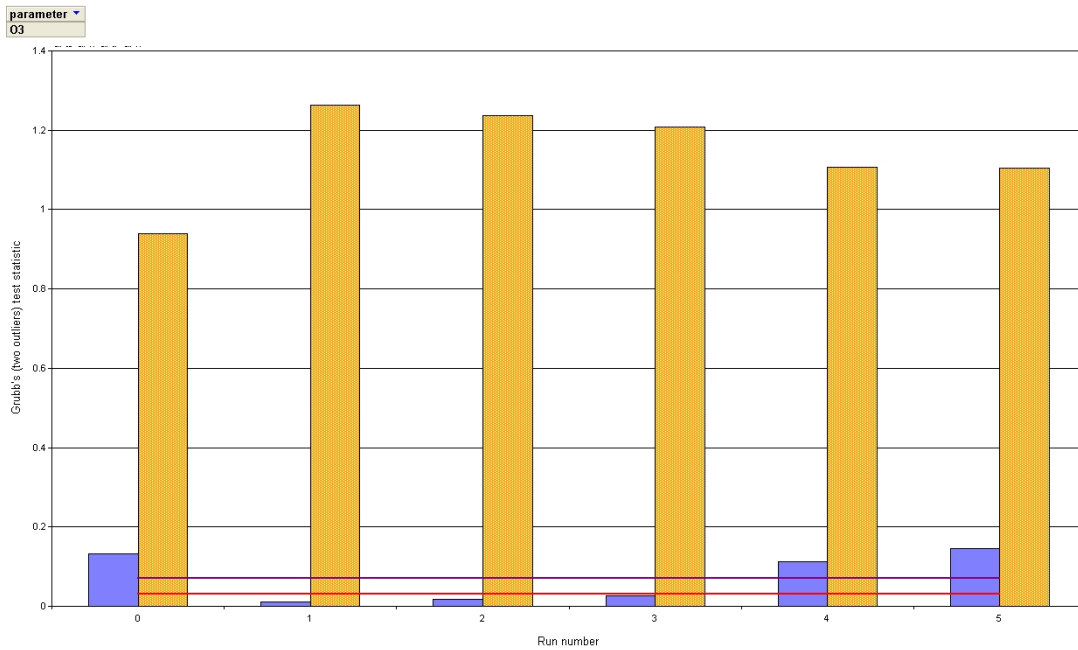


Figure 65: Grubb's two outlying observations test statistics for O₃ runs

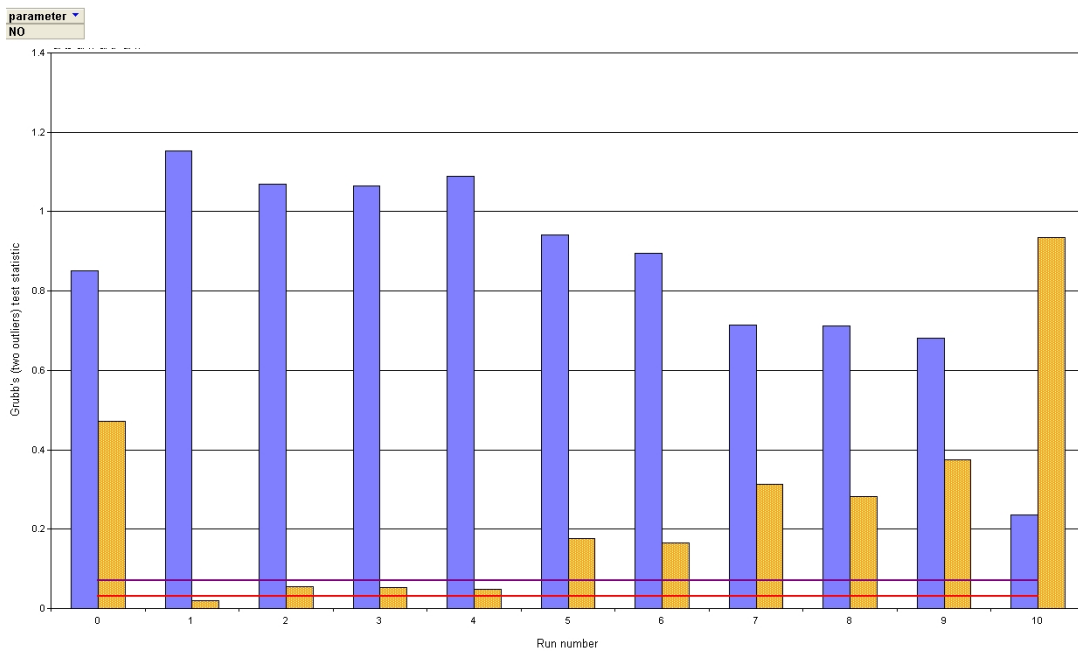


Figure 66: Grubb's two outlying observations test statistics for NO runs

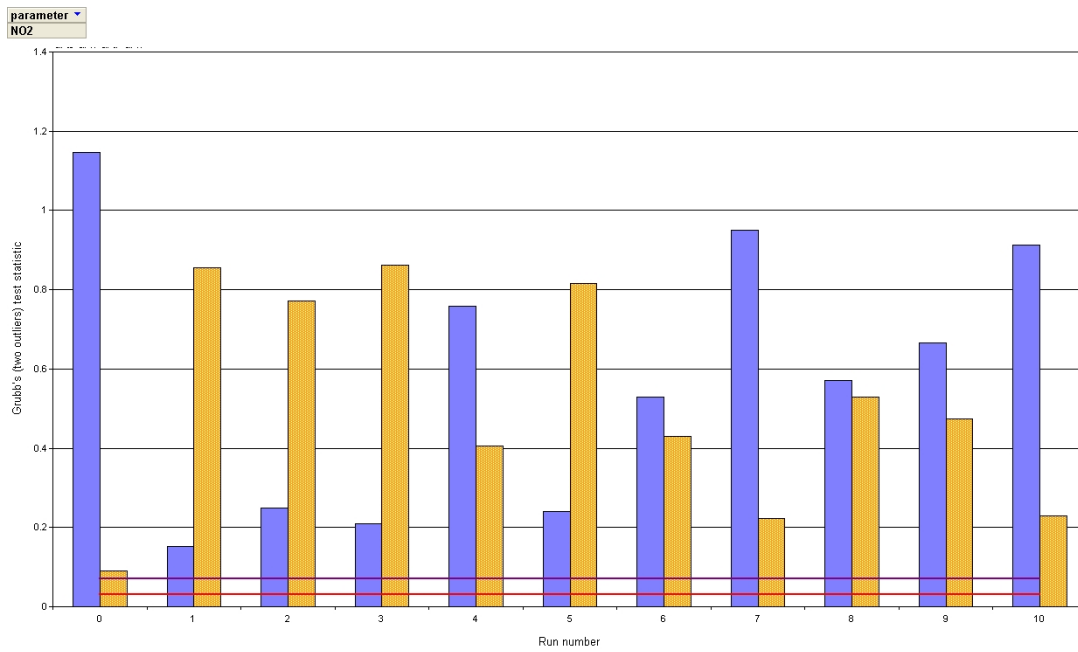


Figure 67: Grubb's two outlying observations test statistics for NO₂ runs

European Commission

EUR 23806 EN – Joint Research Centre – Institute for Environment and Sustainability

Title: The Evaluation of the Intercomparison Exercise for SO₂, CO, O₃, NO and NO₂ - 6 - 9 October 2008

Author(s): Matej Kapus Dukarić, Annette Borowiak and Fritz Lagler

Luxembourg: Office for Official Publications of the European Communities

2009 – 60 pp. – 29.7 x 21.0 cm

EUR – Scientific and Technical Research series – ISSN 1018-5593

ISBN 978-92-79-12170-8

Abstract

From the 6th to the 9th of October 2008 in Ispra (IT), 7 AQUILA (Network of European Air Quality Reference Laboratories) and 2 laboratories of the World Health Organisations (WHO) Euro-Region met at an intercomparison exercise to evaluate their proficiency in the analysis of inorganic gaseous pollutants covered by European Air Quality Directives (SO₂, CO, NO, NO₂ and O₃).

The proficiency evaluation, where each participant's bias was compared to two criteria, provides information on the current situation and capabilities to the European Commission and can be used by participants in their quality control system.

In terms of criteria imposed by the European Commission, 36% of the results reported by AQUILA laboratories were good both in terms of measured values and reported uncertainties. Another 56% of the results had good measured values, but the reported uncertainties were either too small (21%) or too high (35%).

The comparability of results among AQUILA participants is satisfactory for O₃, SO₂, CO and NO measurement method, but the pollutant NO₂ needs further improvements and harmonization programmes.

How to obtain EU publications

Our priced publications are available from EU Bookshop (<http://bookshop.europa.eu>), where you can place an order with the sales agent of your choice.

The Publications Office has a worldwide network of sales agents. You can obtain their contact details by sending a fax to (352) 29 29-42758.

The mission of the JRC is to provide customer-driven scientific and technical support for the conception, development, implementation and monitoring of EU policies. As a service of the European Commission, the JRC functions as a reference centre of science and technology for the Union. Close to the policy-making process, it serves the common interest of the Member States, while being independent of special interests, whether private or national.

LB-NA-23806-EN-C

